



US00D902431S

(12) **United States Design Patent** (10) **Patent No.:** **US D902,431 S**  
**Sims et al.** (45) **Date of Patent:** **\*\* Nov. 17, 2020**

(54) **TUBE STRIP WITH CAPS**  
(71) Applicant: **ABGENE UK LTD.**, Ashford (GB)  
(72) Inventors: **Daniel Sims**, Ashford (GB); **Clive Harrison**, Ashford (GB); **Nicola Burbidge**, Carlsbad, CA (US)  
(73) Assignee: **ABGENE UK LTD**, Ashford (GB)

D703,345 S \* 4/2014 Tajima ..... D24/224  
D709,625 S \* 7/2014 Baum ..... D24/224  
D717,468 S \* 11/2014 Tsai ..... B01L 3/50855  
D24/224  
D718,465 S \* 11/2014 Tajima ..... D24/224  
D742,027 S \* 10/2015 Lentz ..... D24/224  
D759,835 S \* 6/2016 Baum ..... D24/224  
D778,459 S \* 2/2017 Tajima ..... D24/224  
D792,981 S \* 7/2017 Tajima ..... D24/224

(Continued)

(\*\*) Term: **15 Years**

**OTHER PUBLICATIONS**

(21) Appl. No.: **29/703,313**

<https://www.southernlabware.com/pure-amptm-pcr-tubes-strips-0-2ml-qpcr-8-strip-with-separate-optical-strip-caps-natural-clear-120-pkg.html?gclid=> (Mar. 2, 2020).\*

(22) Filed: **Aug. 26, 2019**

(Continued)

**Related U.S. Application Data**

(62) Division of application No. 29/565,448, filed on May 20, 2016, now Pat. No. Des. 862,724.

*Primary Examiner* — Janice Hallmark  
*Assistant Examiner* — Rebecca Tsehaye

(51) **LOC (12) Cl.** ..... **24-02**

(57) **CLAIM**

(52) **U.S. Cl.**

The ornamental design for a tube strip with caps, as shown and described.

USPC ..... **D24/224**

(58) **Field of Classification Search**

**DESCRIPTION**

USPC ..... D24/224–230, 216; 422/562, 561, 560, 422/568, 500; 435/288.1, 288.4, 305.2

CPC ..... B01L 3/00; B01L 3/02; B01L 3/14; B01L 3/50; B01L 3/50825; B01L 3/5085; B01L 3/50853

FIG. 1 is a perspective view of a tube strip with caps showing our new design.  
FIG. 2 is a front side view thereof;  
FIG. 3 is a back side view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a top view thereof;  
FIG. 7 is a bottom view thereof;  
FIG. 8 is a top view thereof;  
FIG. 9 is a bottom view thereof; and,  
FIG. 10 is a top view thereof.  
The broken lines shown in the drawings depict portions of the tube strip with caps that form no part of the claimed design.


See application file for complete search history.

(56) **References Cited**

**1 Claim, 9 Drawing Sheets**

**U.S. PATENT DOCUMENTS**

6,001,310 A \* 12/1999 Shaffer ..... B01L 3/5085  
422/548  
D439,673 S \* 3/2001 Brophy ..... D24/226  
D445,907 S \* 7/2001 Monks ..... D24/216  
D453,573 S \* 2/2002 Lafond ..... D24/216  
6,601,725 B2 \* 8/2003 Lafond ..... B01L 3/50853  
220/23.4  
D608,013 S \* 1/2010 Coulling ..... D24/224  
D679,830 S \* 4/2013 May ..... D24/224  
D687,567 S \* 8/2013 Jungheim ..... D24/224

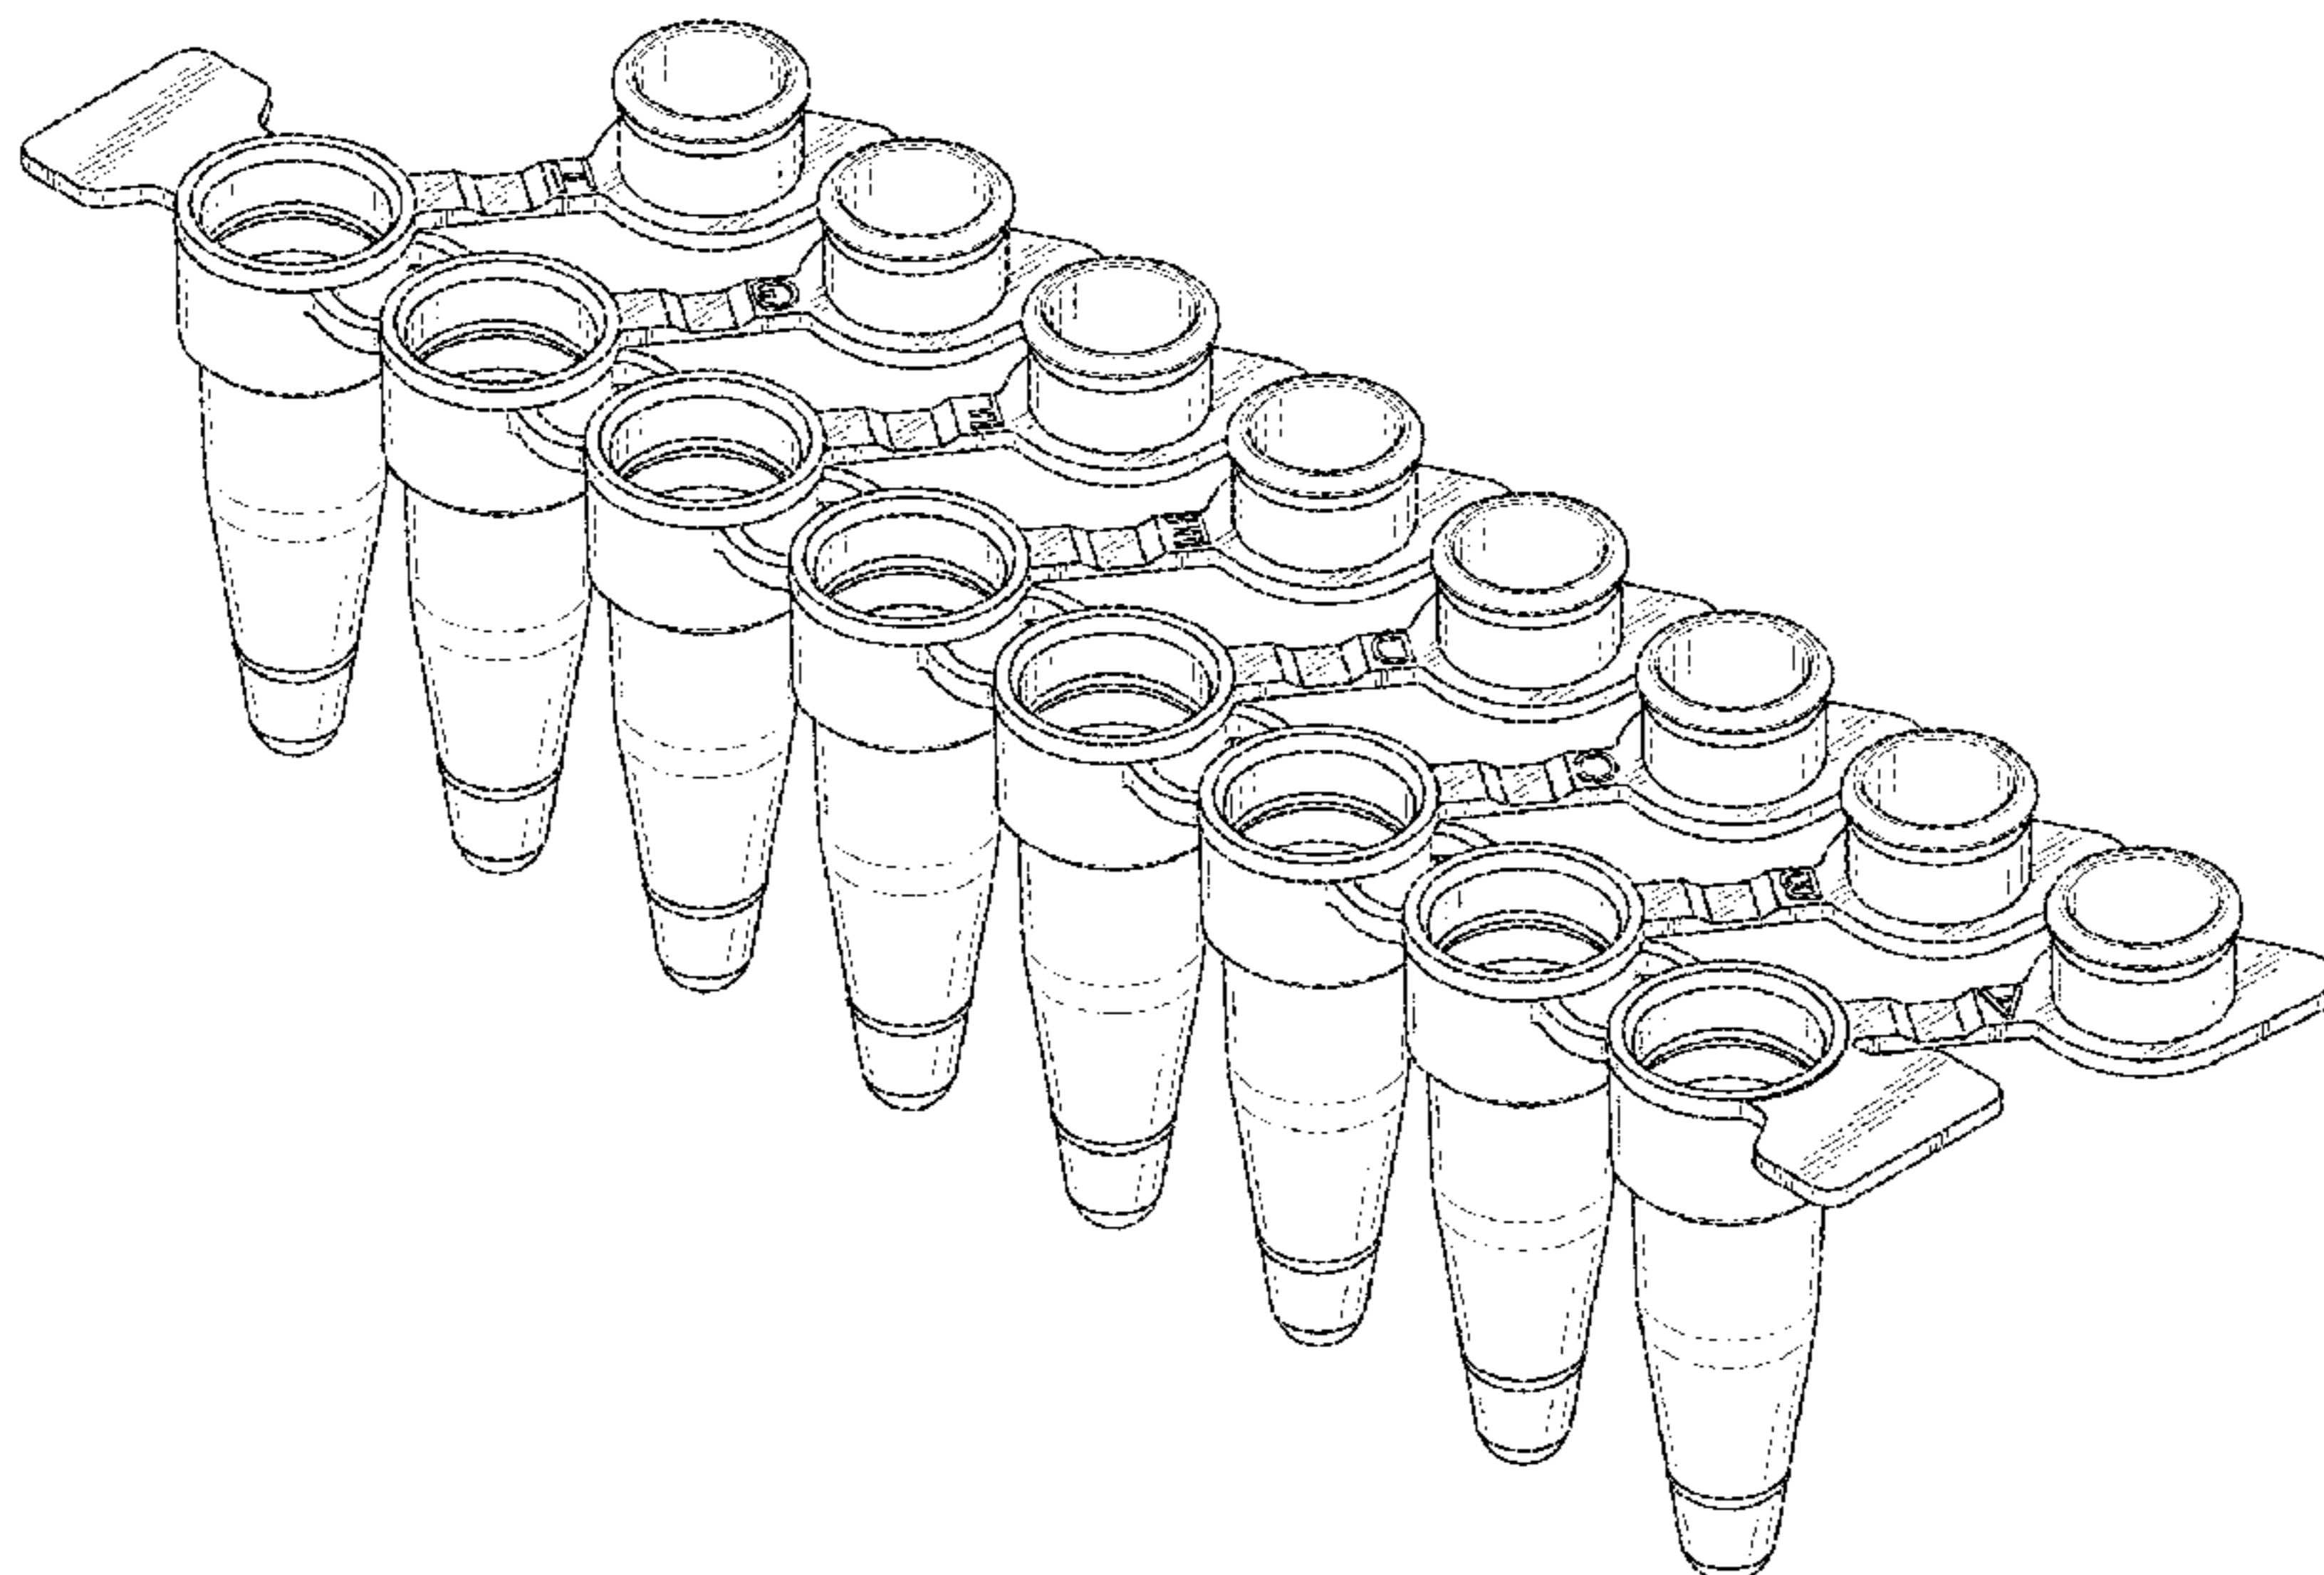

(56)

**References Cited**

U.S. PATENT DOCUMENTS

9,802,196 B2 \* 10/2017 Taunk ..... B01L 3/50825  
D862,724 S \* 10/2019 Sims ..... D24/224

OTHER PUBLICATIONS

<https://dnalandsci.com/product/0-2ml-thin-wall-pcr-strip-with-individual-flat-cap-8-tube/> (Mar. 2, 2020).\*

\* cited by examiner

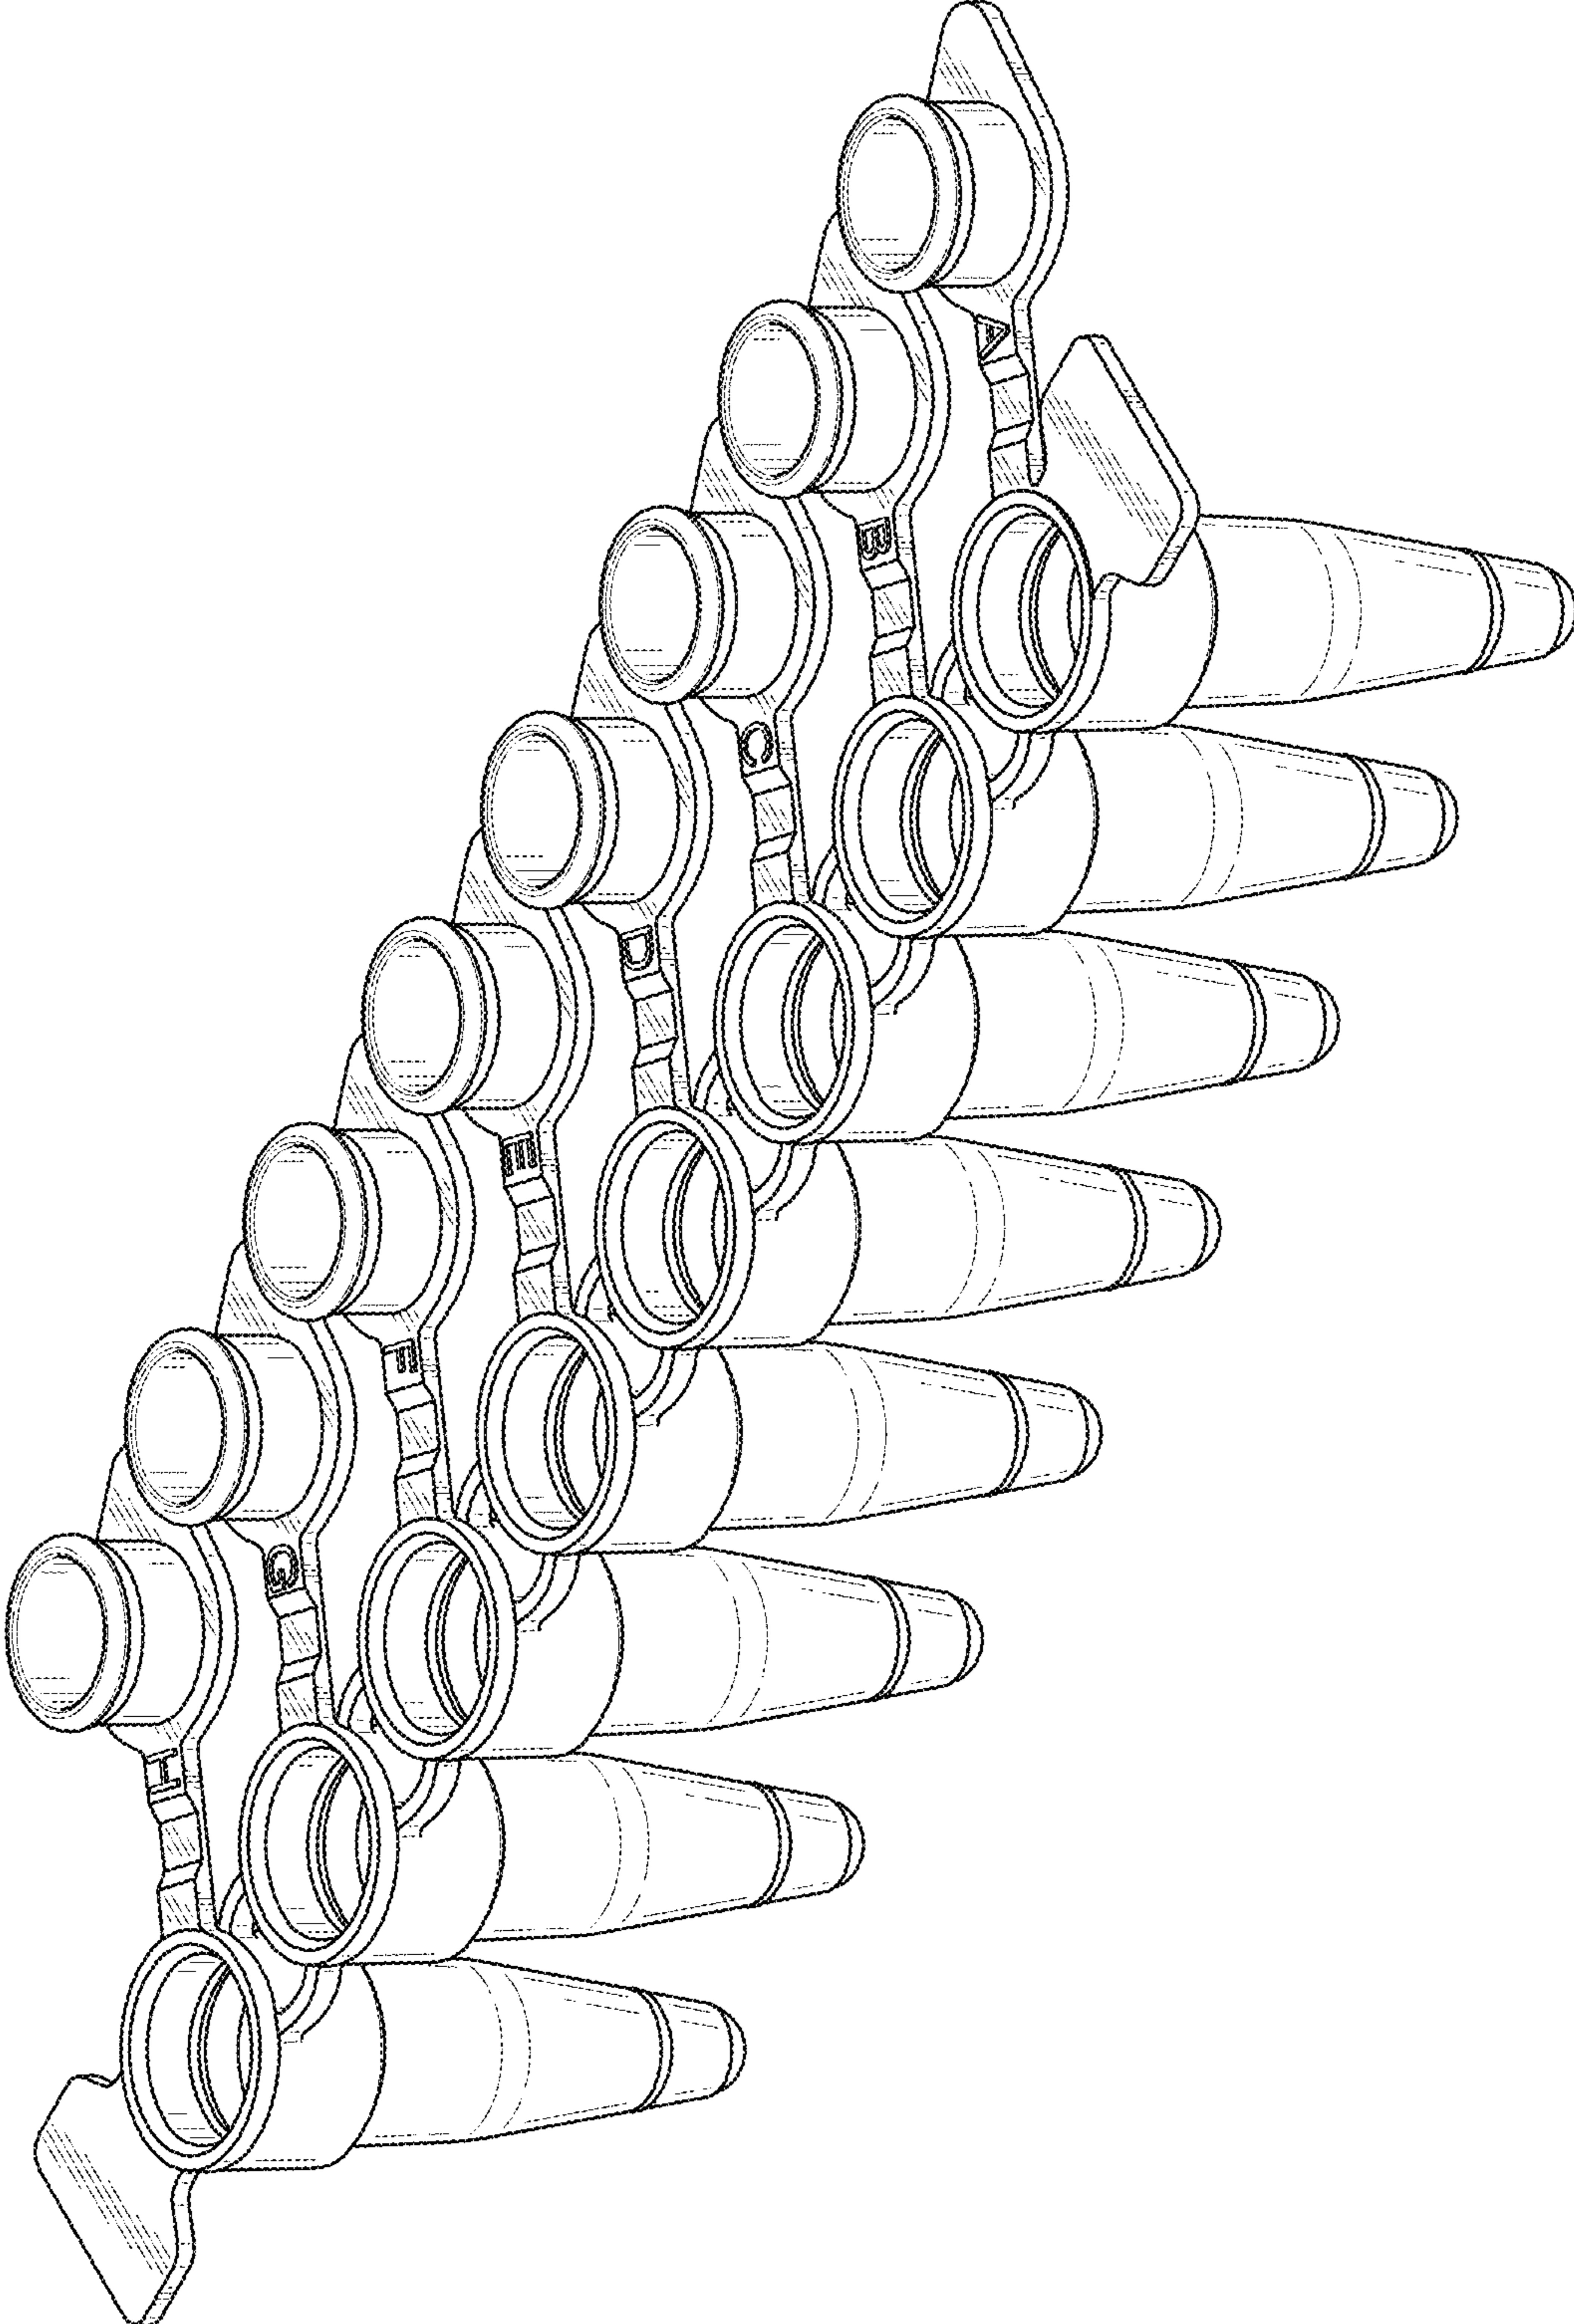


FIG. 1



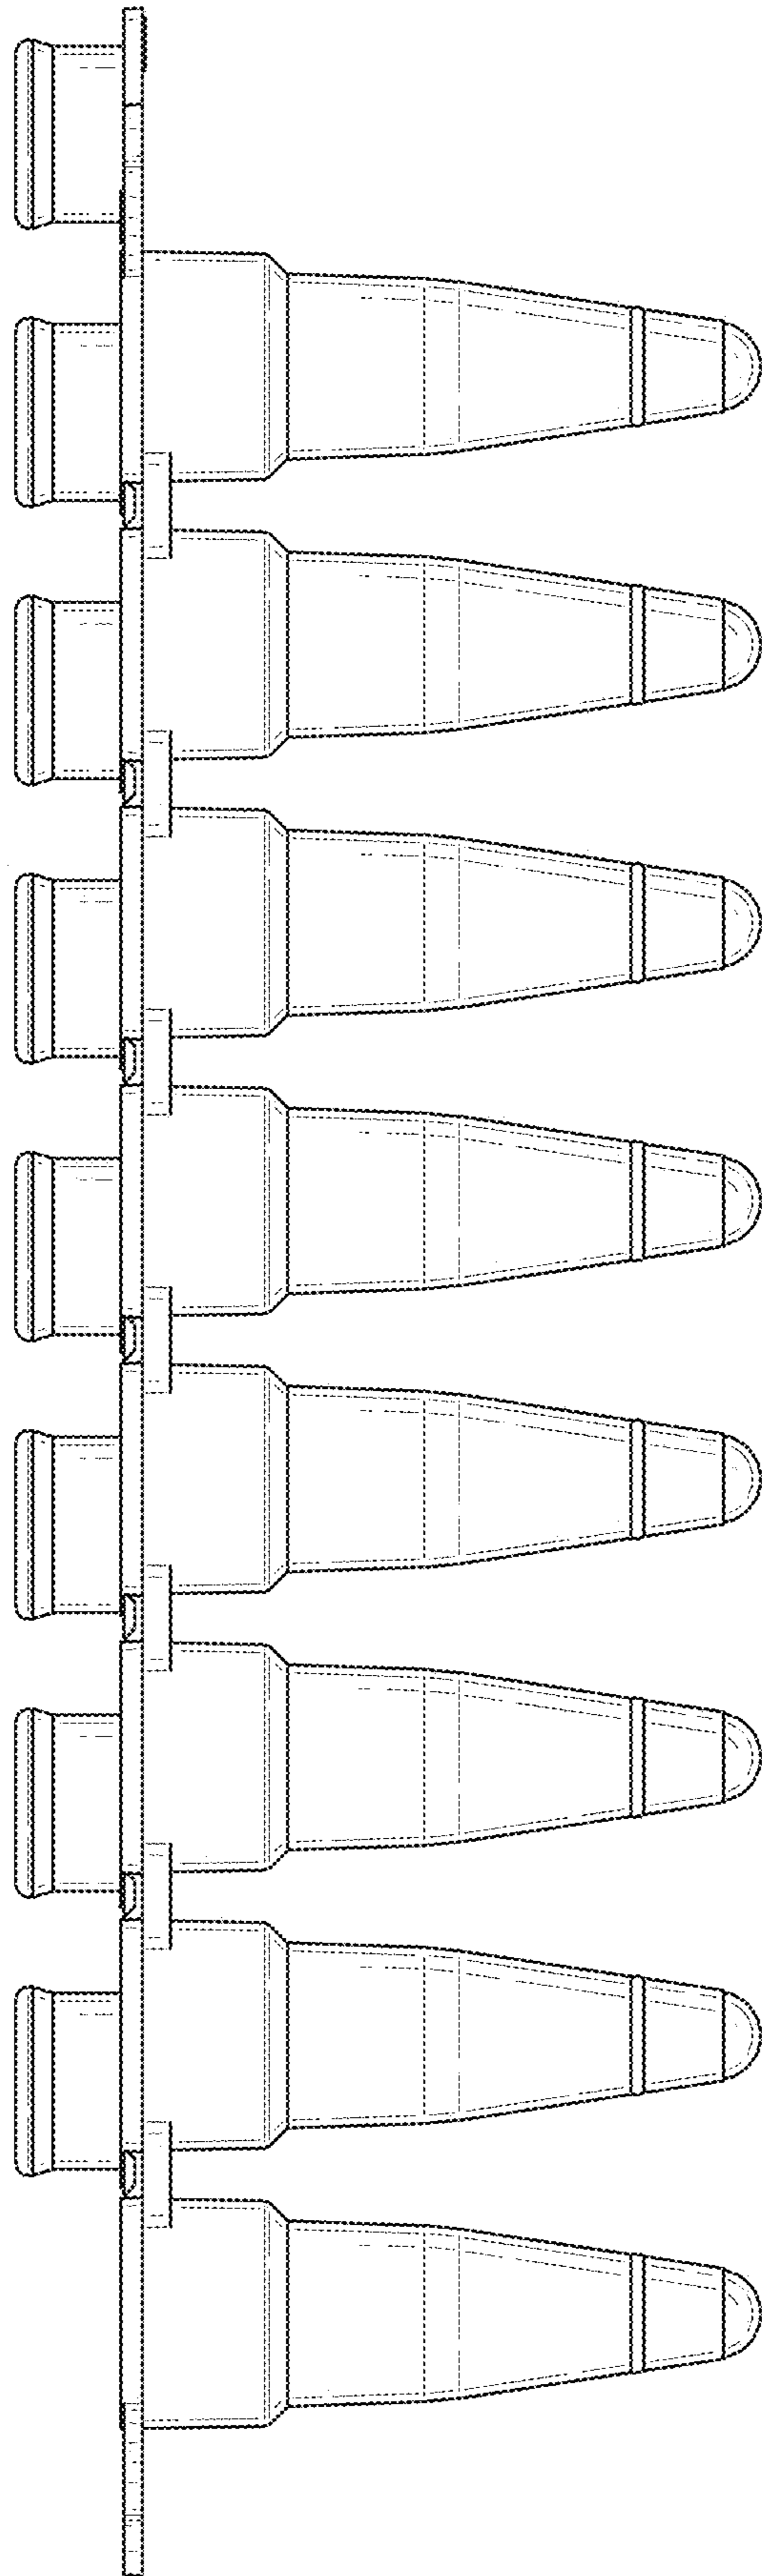


FIG. 2

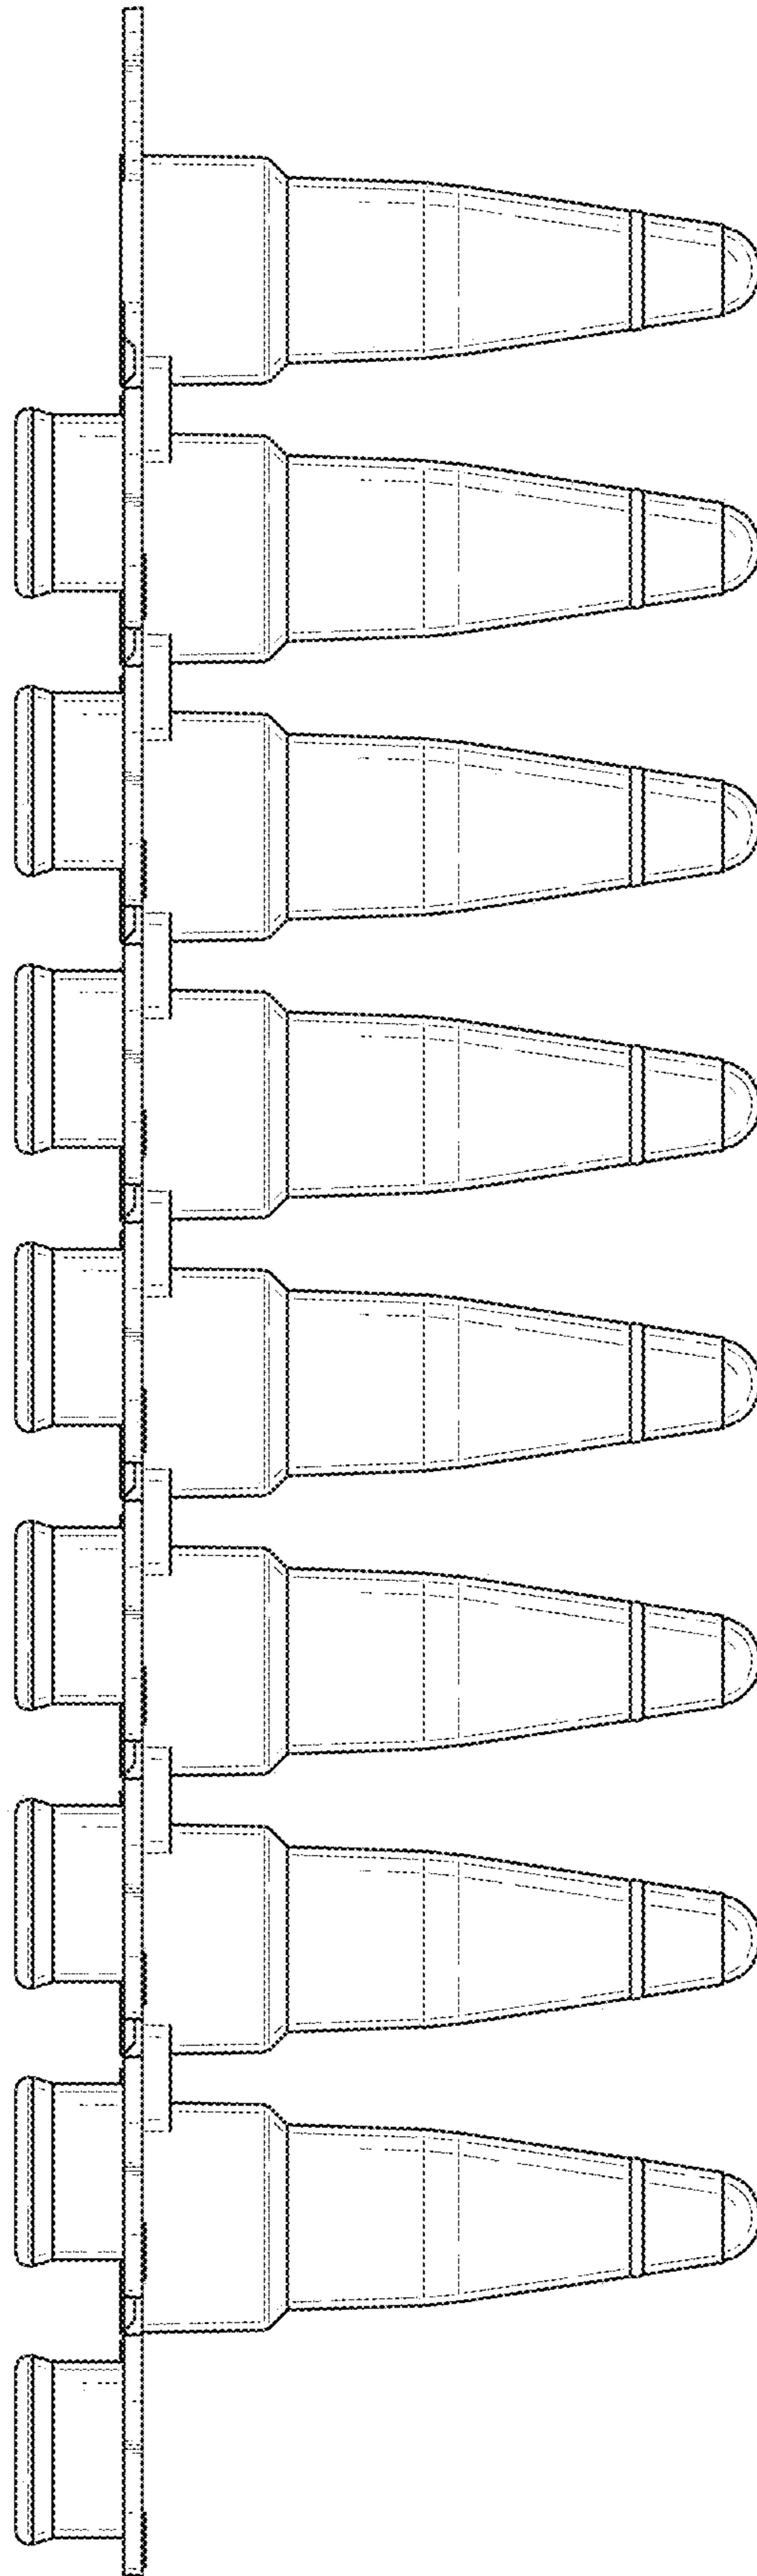


FIG. 3

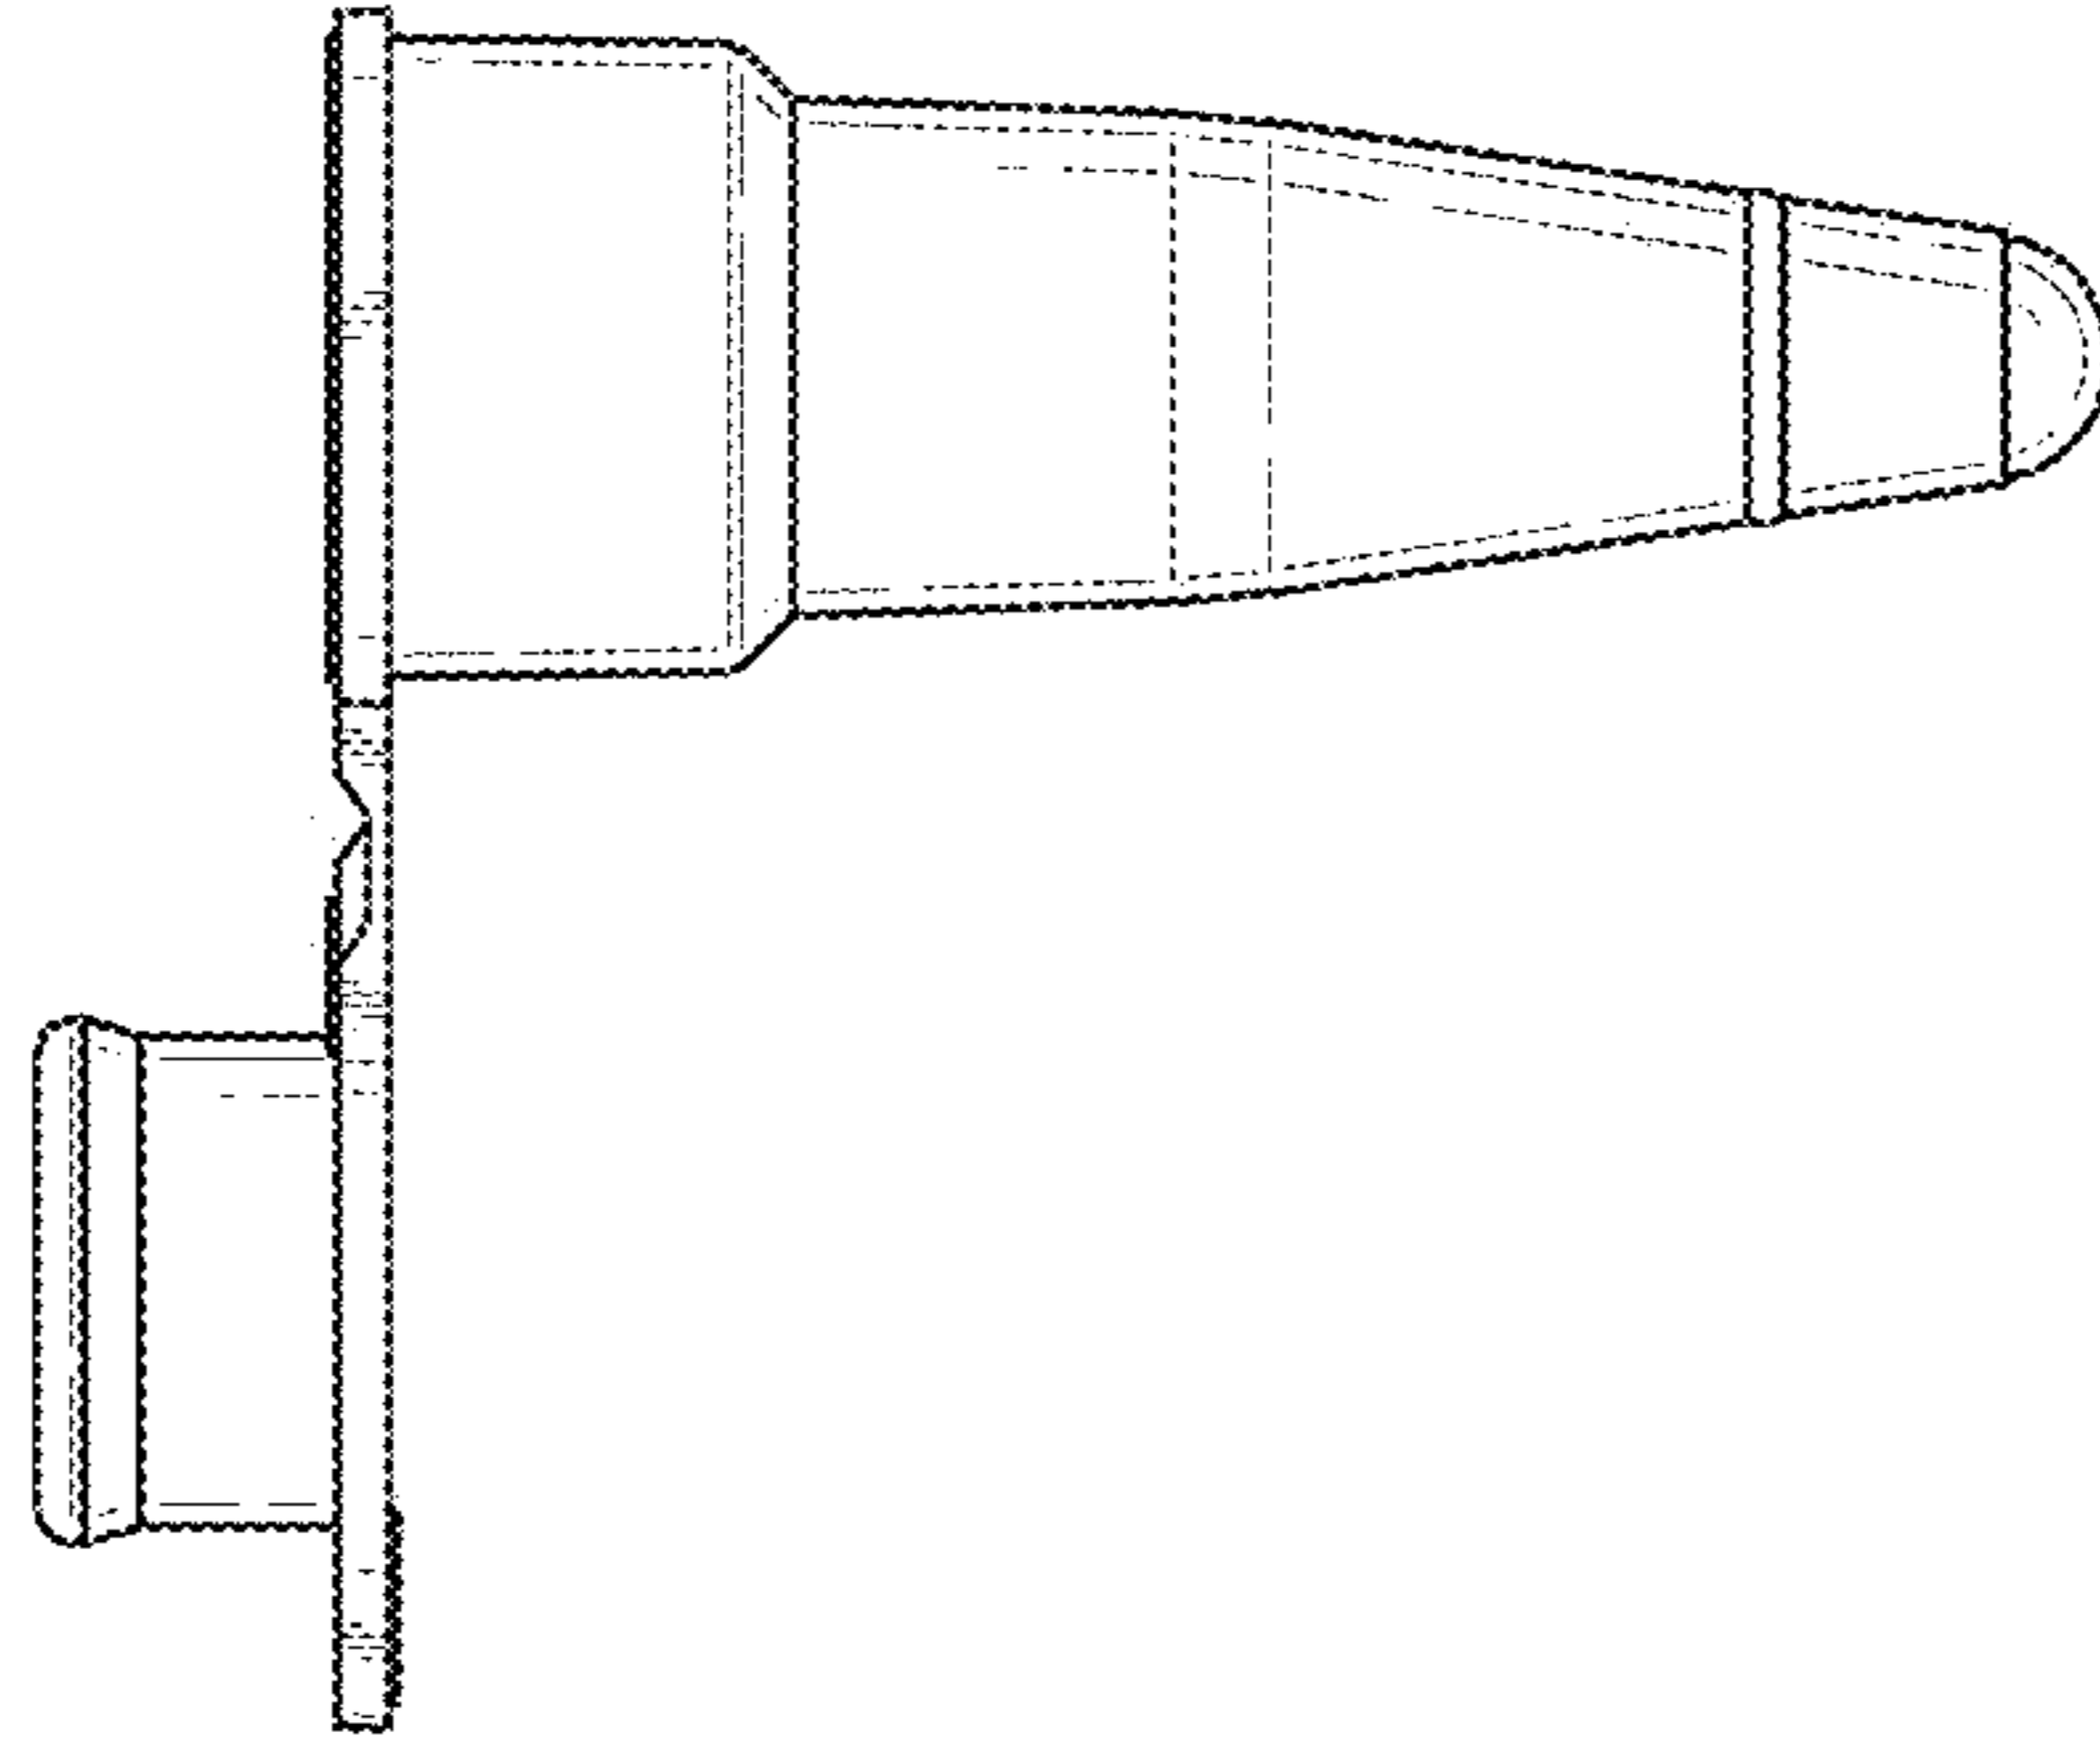


FIG. 4

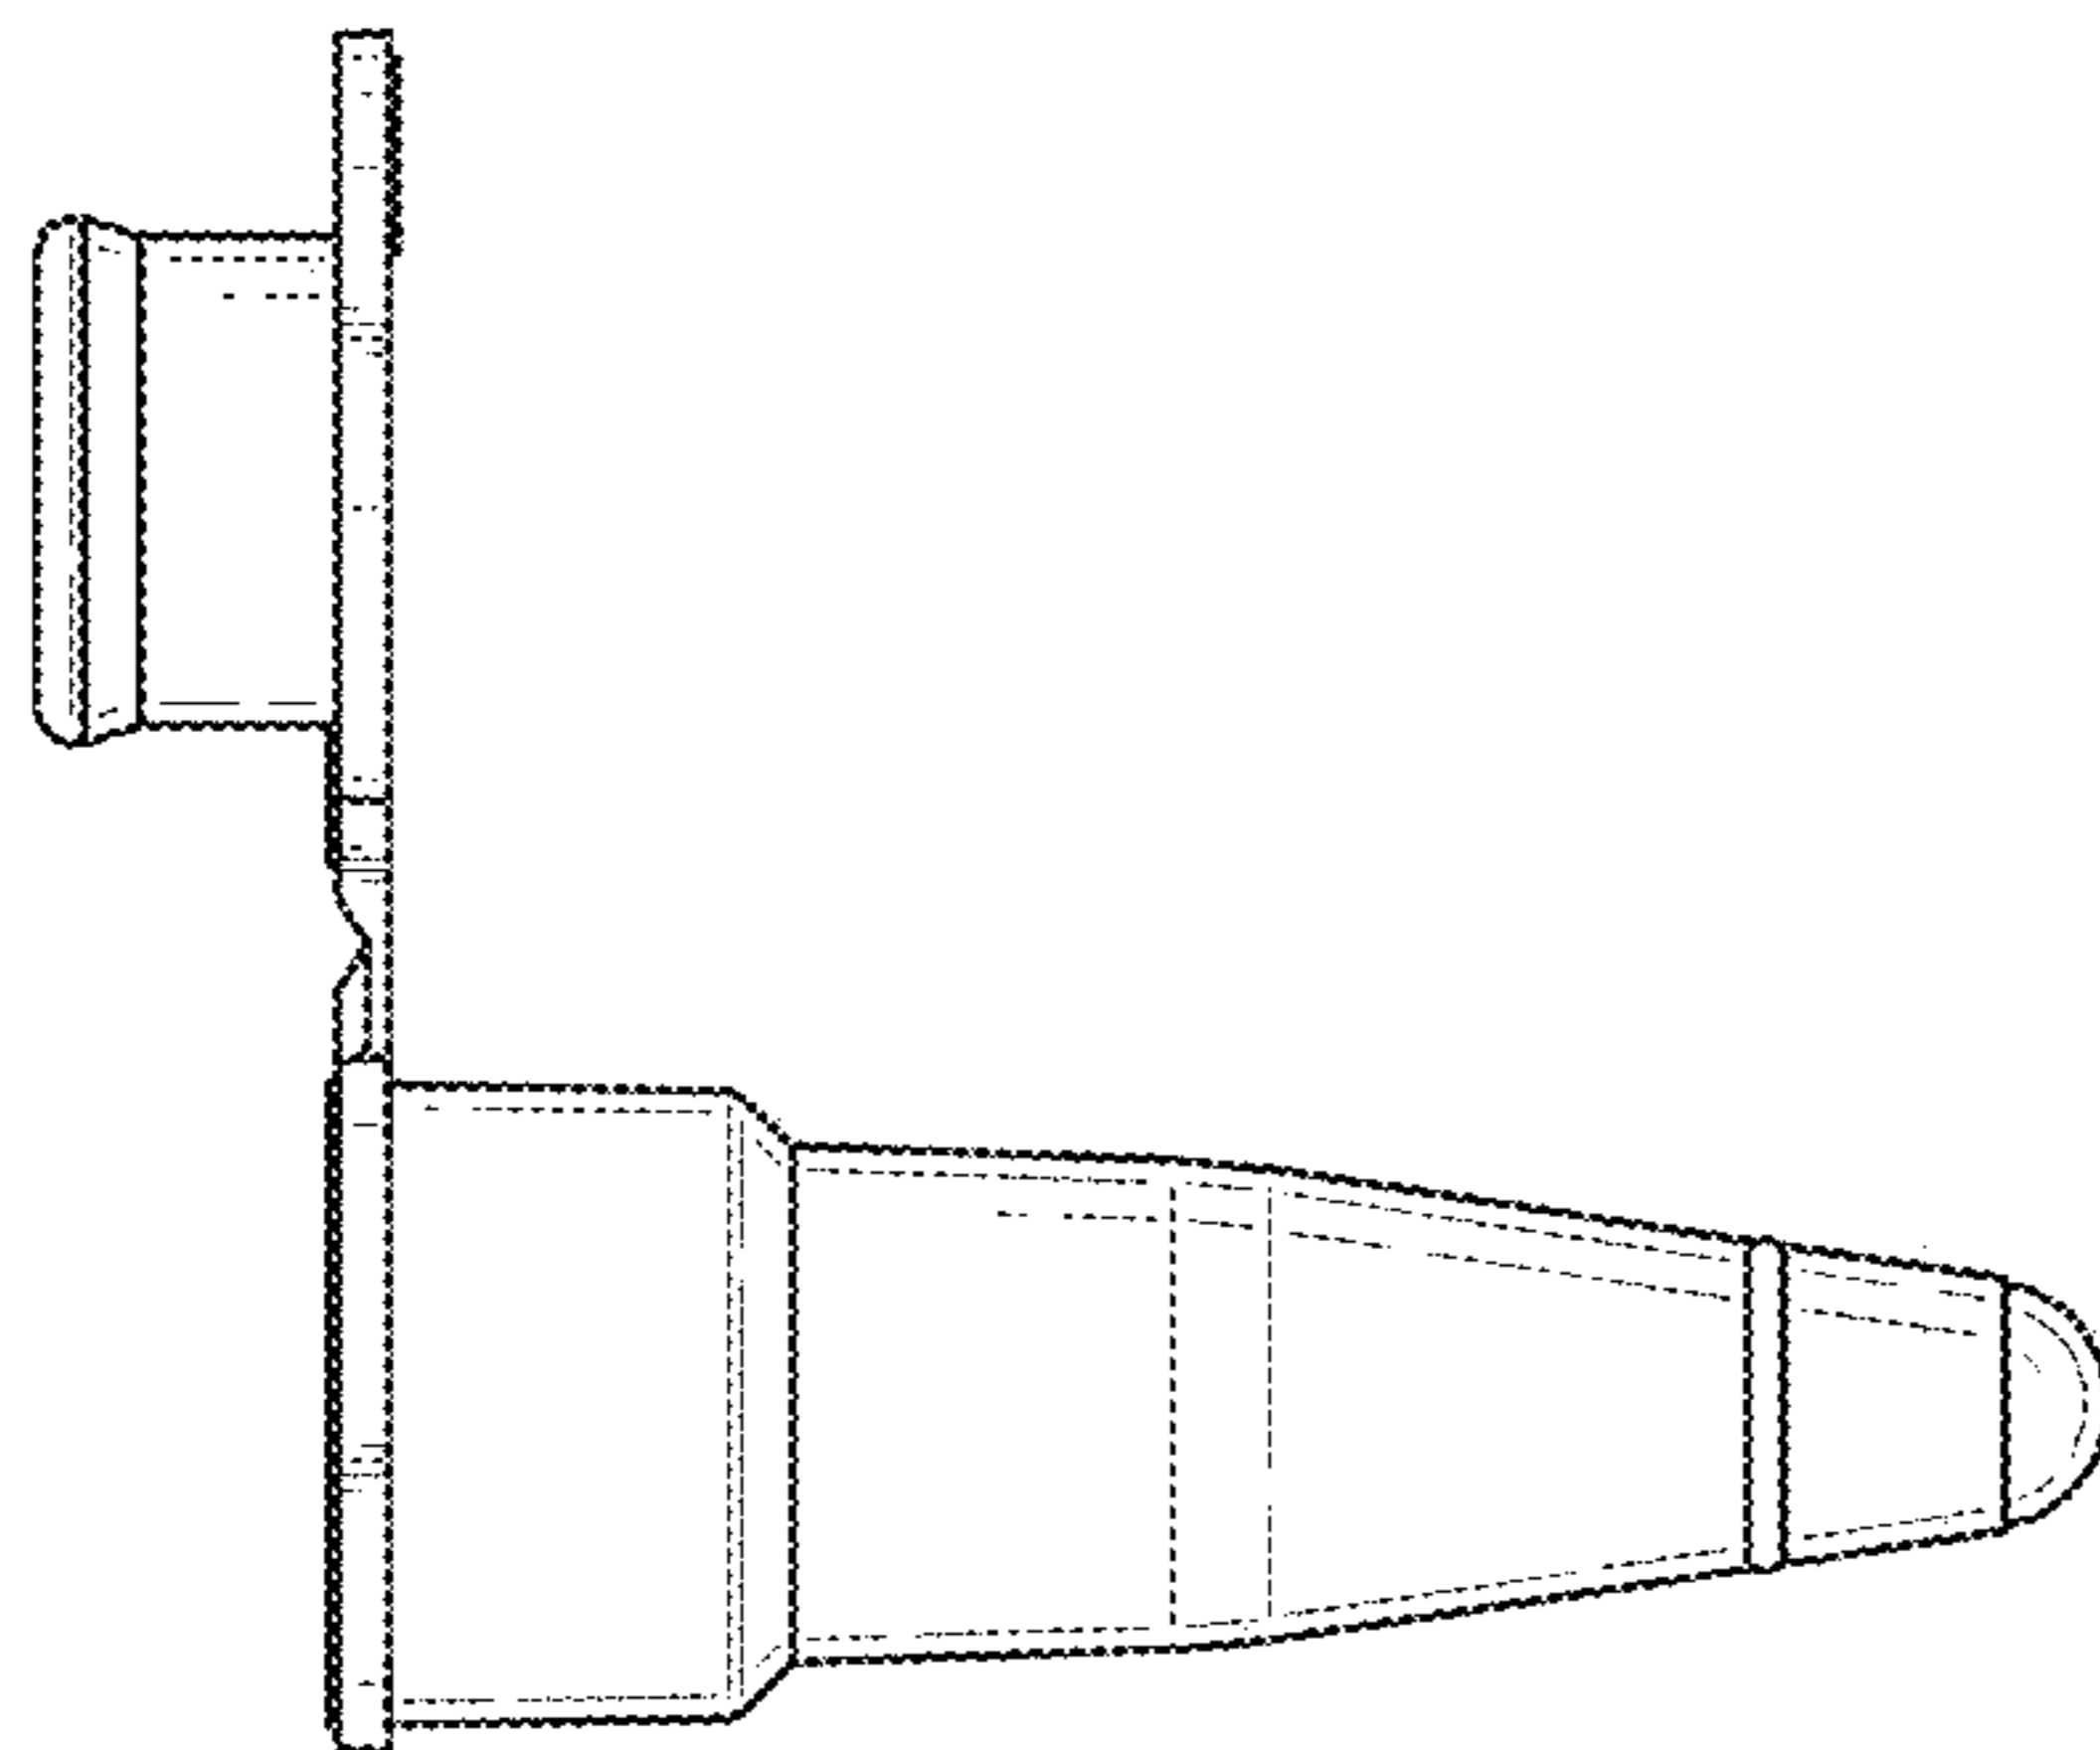


FIG. 5

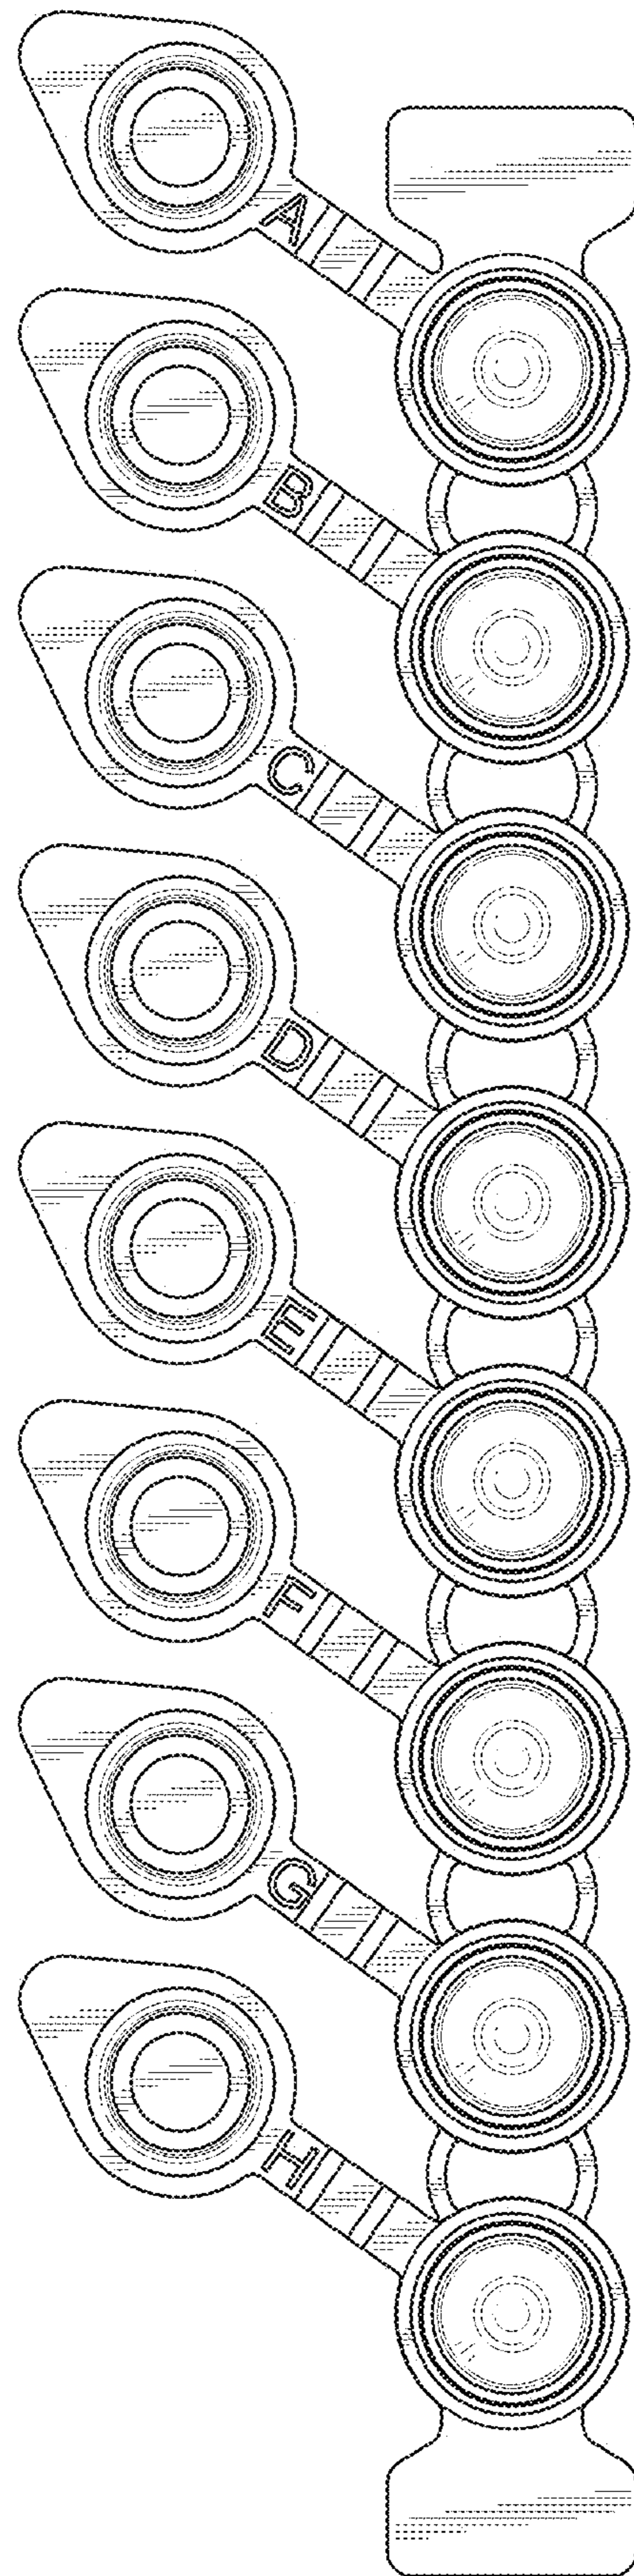


FIG. 6



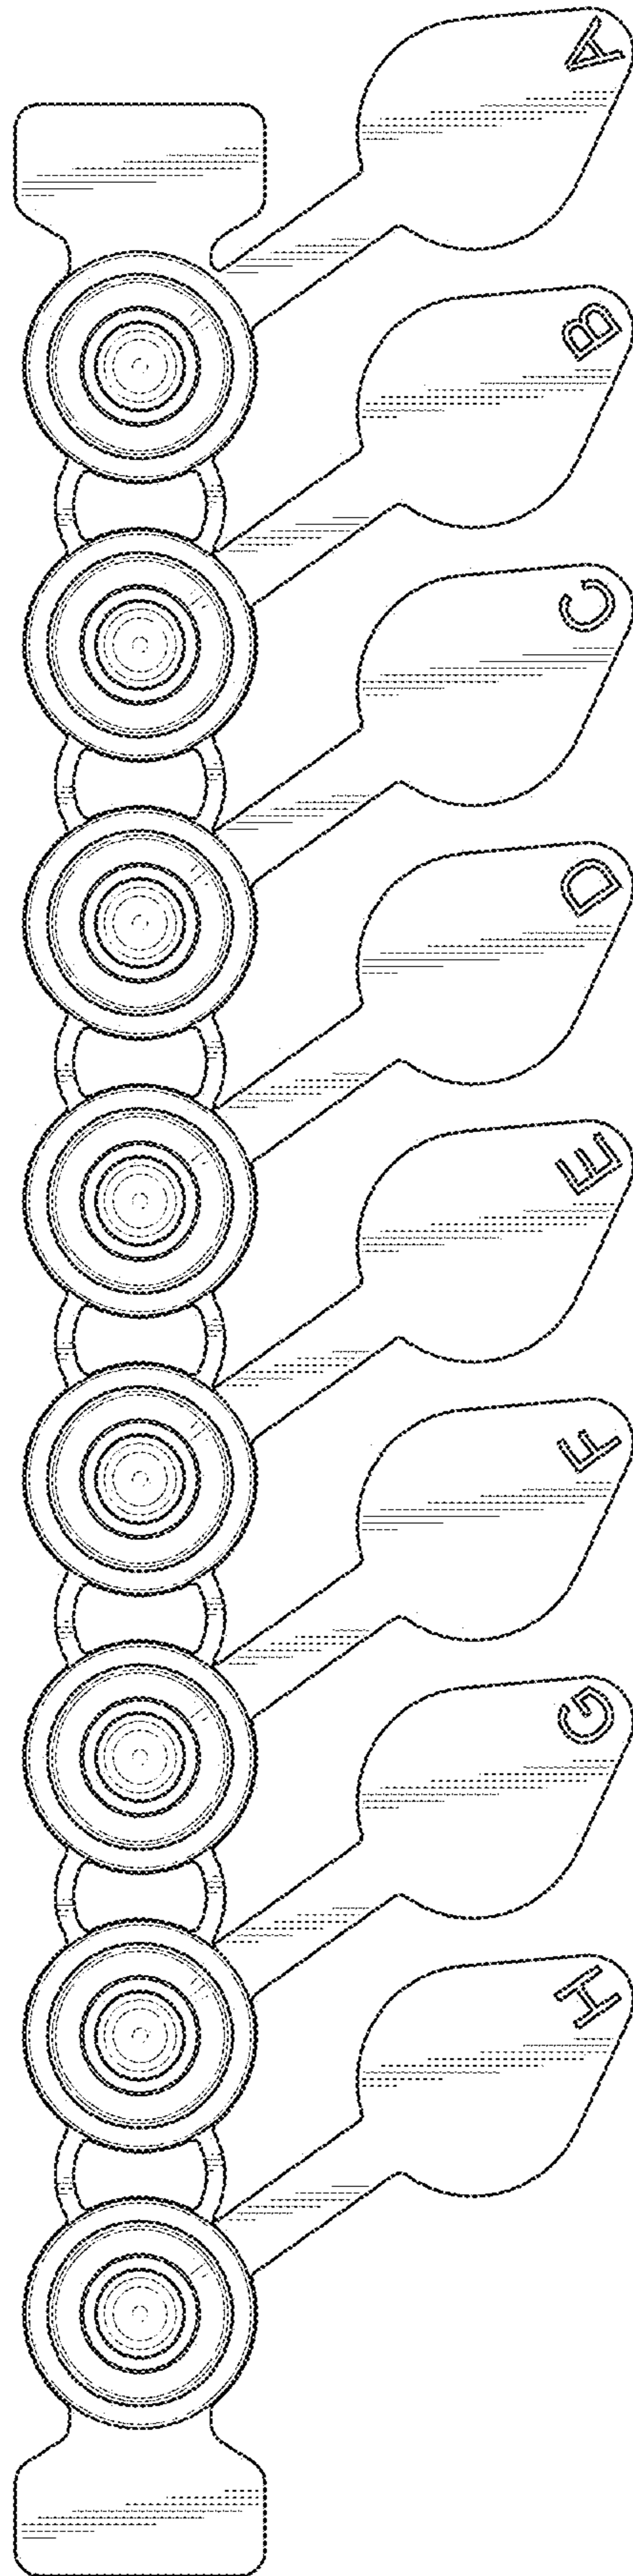


FIG. 7



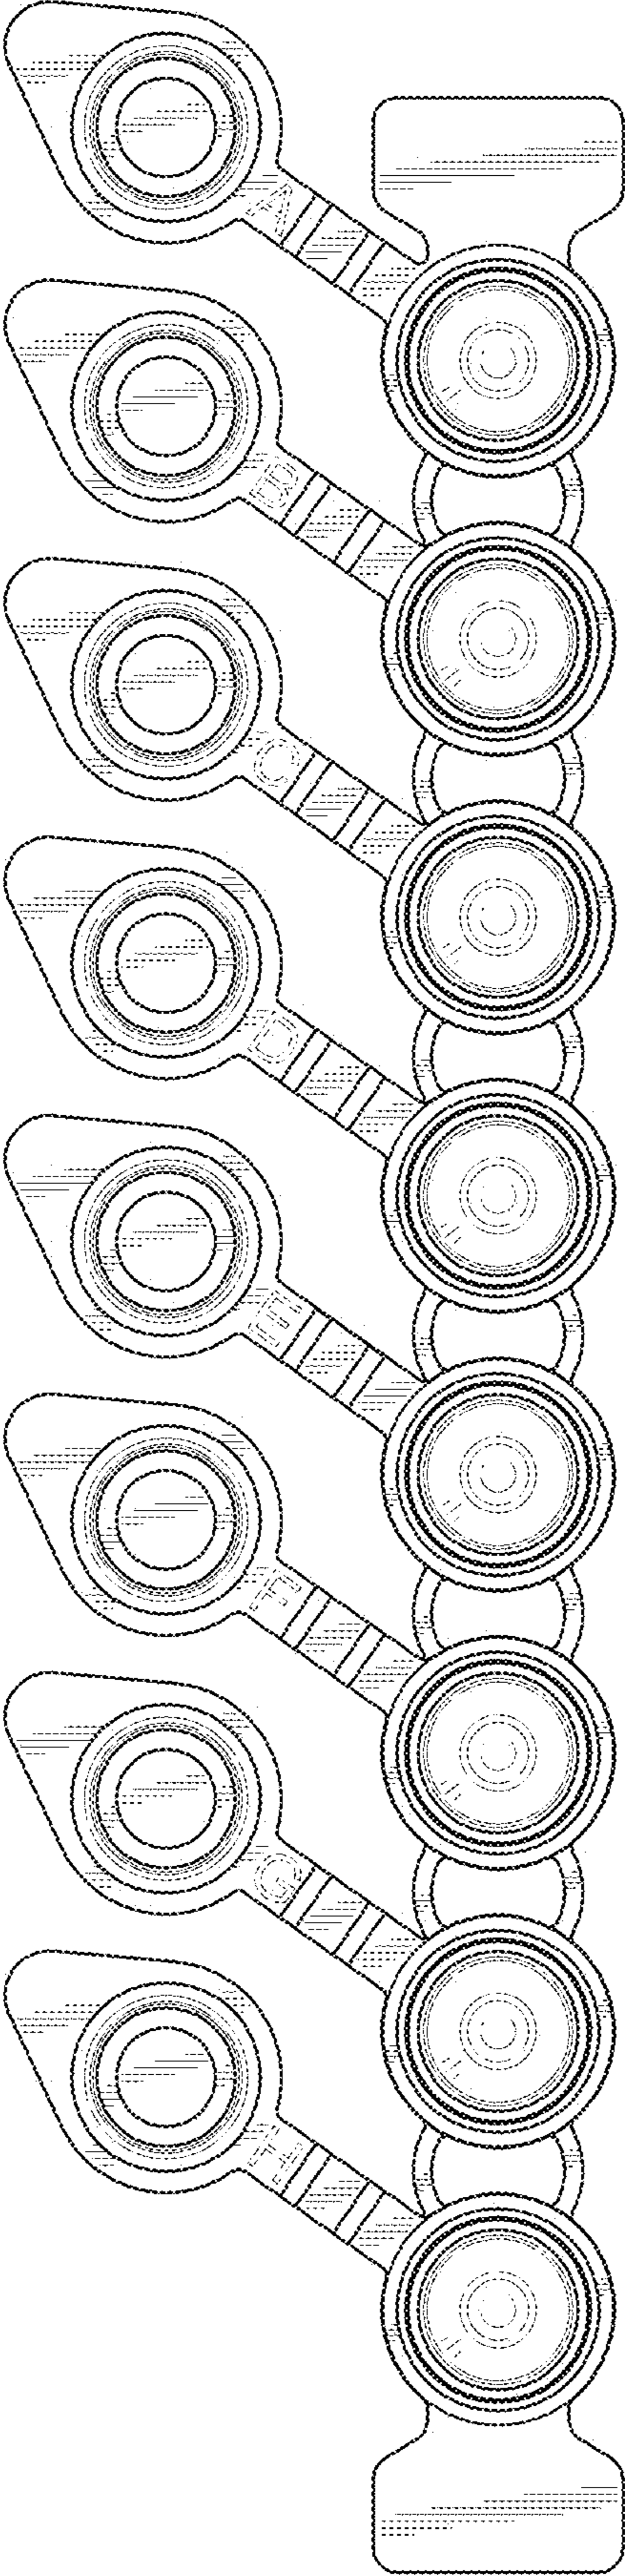


FIG. 8

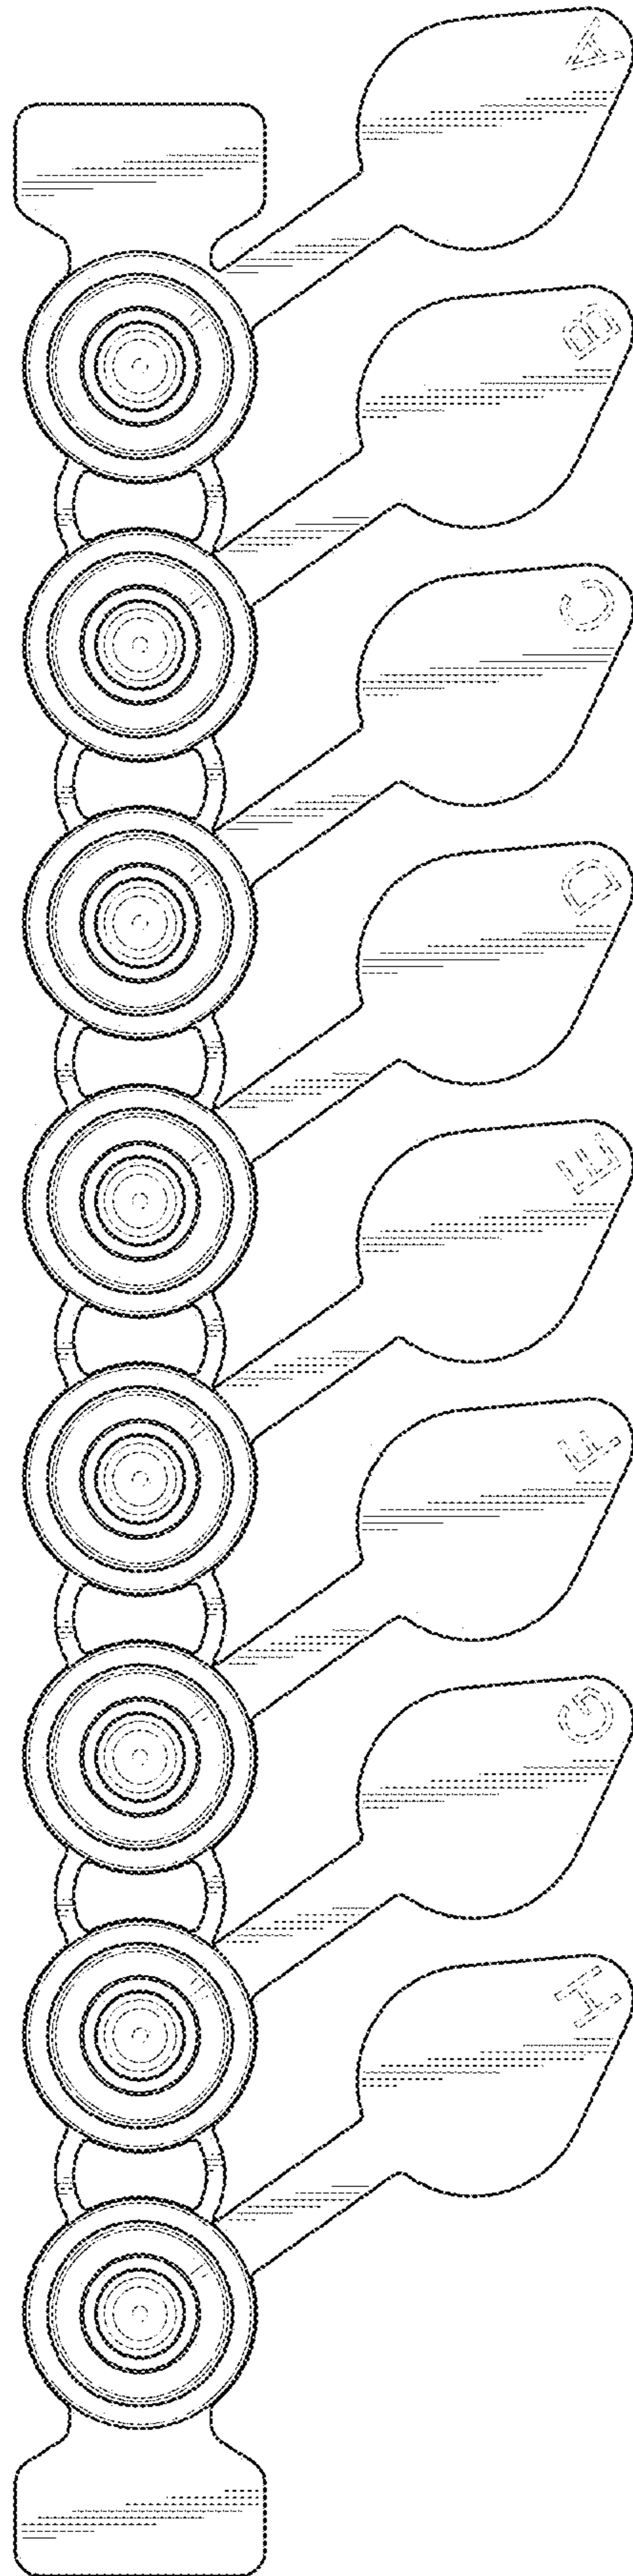


FIG. 9



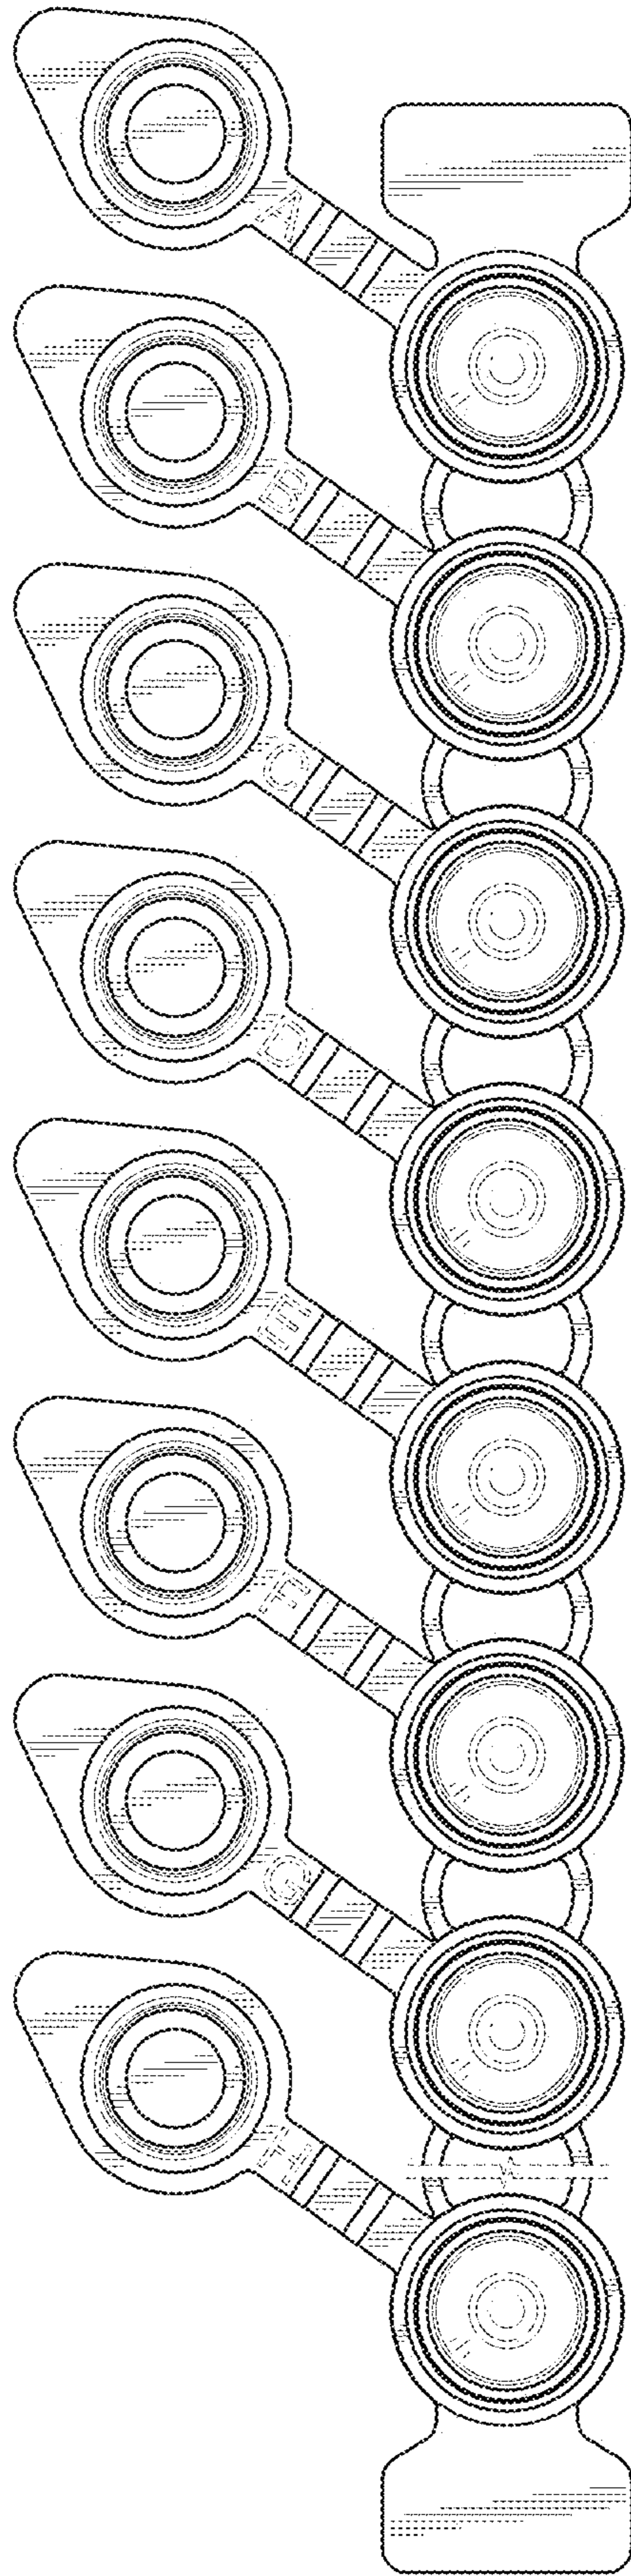


FIG. 10