



US00D903112S

(12) **United States Design Patent**  
**Keating**

(10) **Patent No.:** **US D903,112 S**

(45) **Date of Patent:** **\*\* Nov. 24, 2020**

- (54) **PLUNGER FASTENING DEVICE**
- (71) Applicant: **Kellida Inc.**, Atlanta, GA (US)
- (72) Inventor: **Virginia Souris Keating**, Atlanta, GA (US)
- (73) Assignee: **Kellida Inc.**, Atlanta, GA (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/688,668**
- (22) Filed: **Apr. 23, 2019**
- (51) **LOC (12) Cl.** ..... **24-02**
- (52) **U.S. Cl.**  
USPC ..... **D24/130; D24/114**
- (58) **Field of Classification Search**  
USPC ..... D8/34, 40, 349, 352, 354; D11/26, 27,  
D11/86; D29/113, 114, 122  
CPC ..... A61M 5/158; A61M 2005/1585  
See application file for complete search history.

6,944,914 B2 9/2005 Tillim  
 D543,625 S \* 5/2007 Numata ..... D24/114  
 7,364,570 B2 4/2008 Gerondale et al.  
 (Continued)

**FOREIGN PATENT DOCUMENTS**

WO 9822166 A1 5/1998

**OTHER PUBLICATIONS**

EP 20170359.2, European Search Report dated Jun. 3, 2020, 8 pages.

(Continued)

*Primary Examiner* — Michael C Stout  
*Assistant Examiner* — Fritzgerald L Butac

(57) **CLAIM**

The ornamental design for a plunger fastening device, as shown and described.

**DESCRIPTION**


FIG. 1 is a perspective view of a plunger fastening device, showing my new design;  
 FIG. 2 is front view thereof;  
 FIG. 3 is a back view thereof;  
 FIG. 4 is a side view thereof;  
 FIG. 5 is another side view thereof;  
 FIG. 6 is a top view thereof;  
 FIG. 7 is a bottom view thereof; and,  
 FIG. 8 is another view thereof showing a plunger fastening device of the present invention in an environment in which it may be used, with a plunger of a syringe (shown in phantom) fastened to a user's hand (shown in phantom).  
 Any broken lines showing portions of the plunger fastening device, the environment (which includes a syringe and a hand), or features thereof form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- 2,346,607 A \* 4/1944 Raiman ..... A44C 9/02  
63/15
- 2,842,128 A 7/1958 Hein, Jr.
- 3,758,006 A 9/1973 Gravlee
- D248,598 S \* 7/1978 Bahmer ..... D11/27
- 4,217,896 A 8/1980 Behnke
- 4,324,241 A 4/1982 Reese
- 4,351,334 A 9/1982 Inglefield, Jr.
- 4,687,472 A 8/1987 Gross
- 5,046,381 A 9/1991 Mueller
- D335,196 S \* 4/1993 Lamb ..... D11/3
- 5,554,132 A 9/1996 Straits et al.
- D397,790 S \* 9/1998 Naganuma ..... D24/127
- 5,833,668 A 11/1998 Aguilar
- 6,068,616 A 5/2000 Janus
- D434,850 S \* 12/2000 Balestracci ..... D24/112
- D465,306 S \* 11/2002 Price ..... D29/114
- D504,635 S \* 5/2005 Jones ..... D11/26

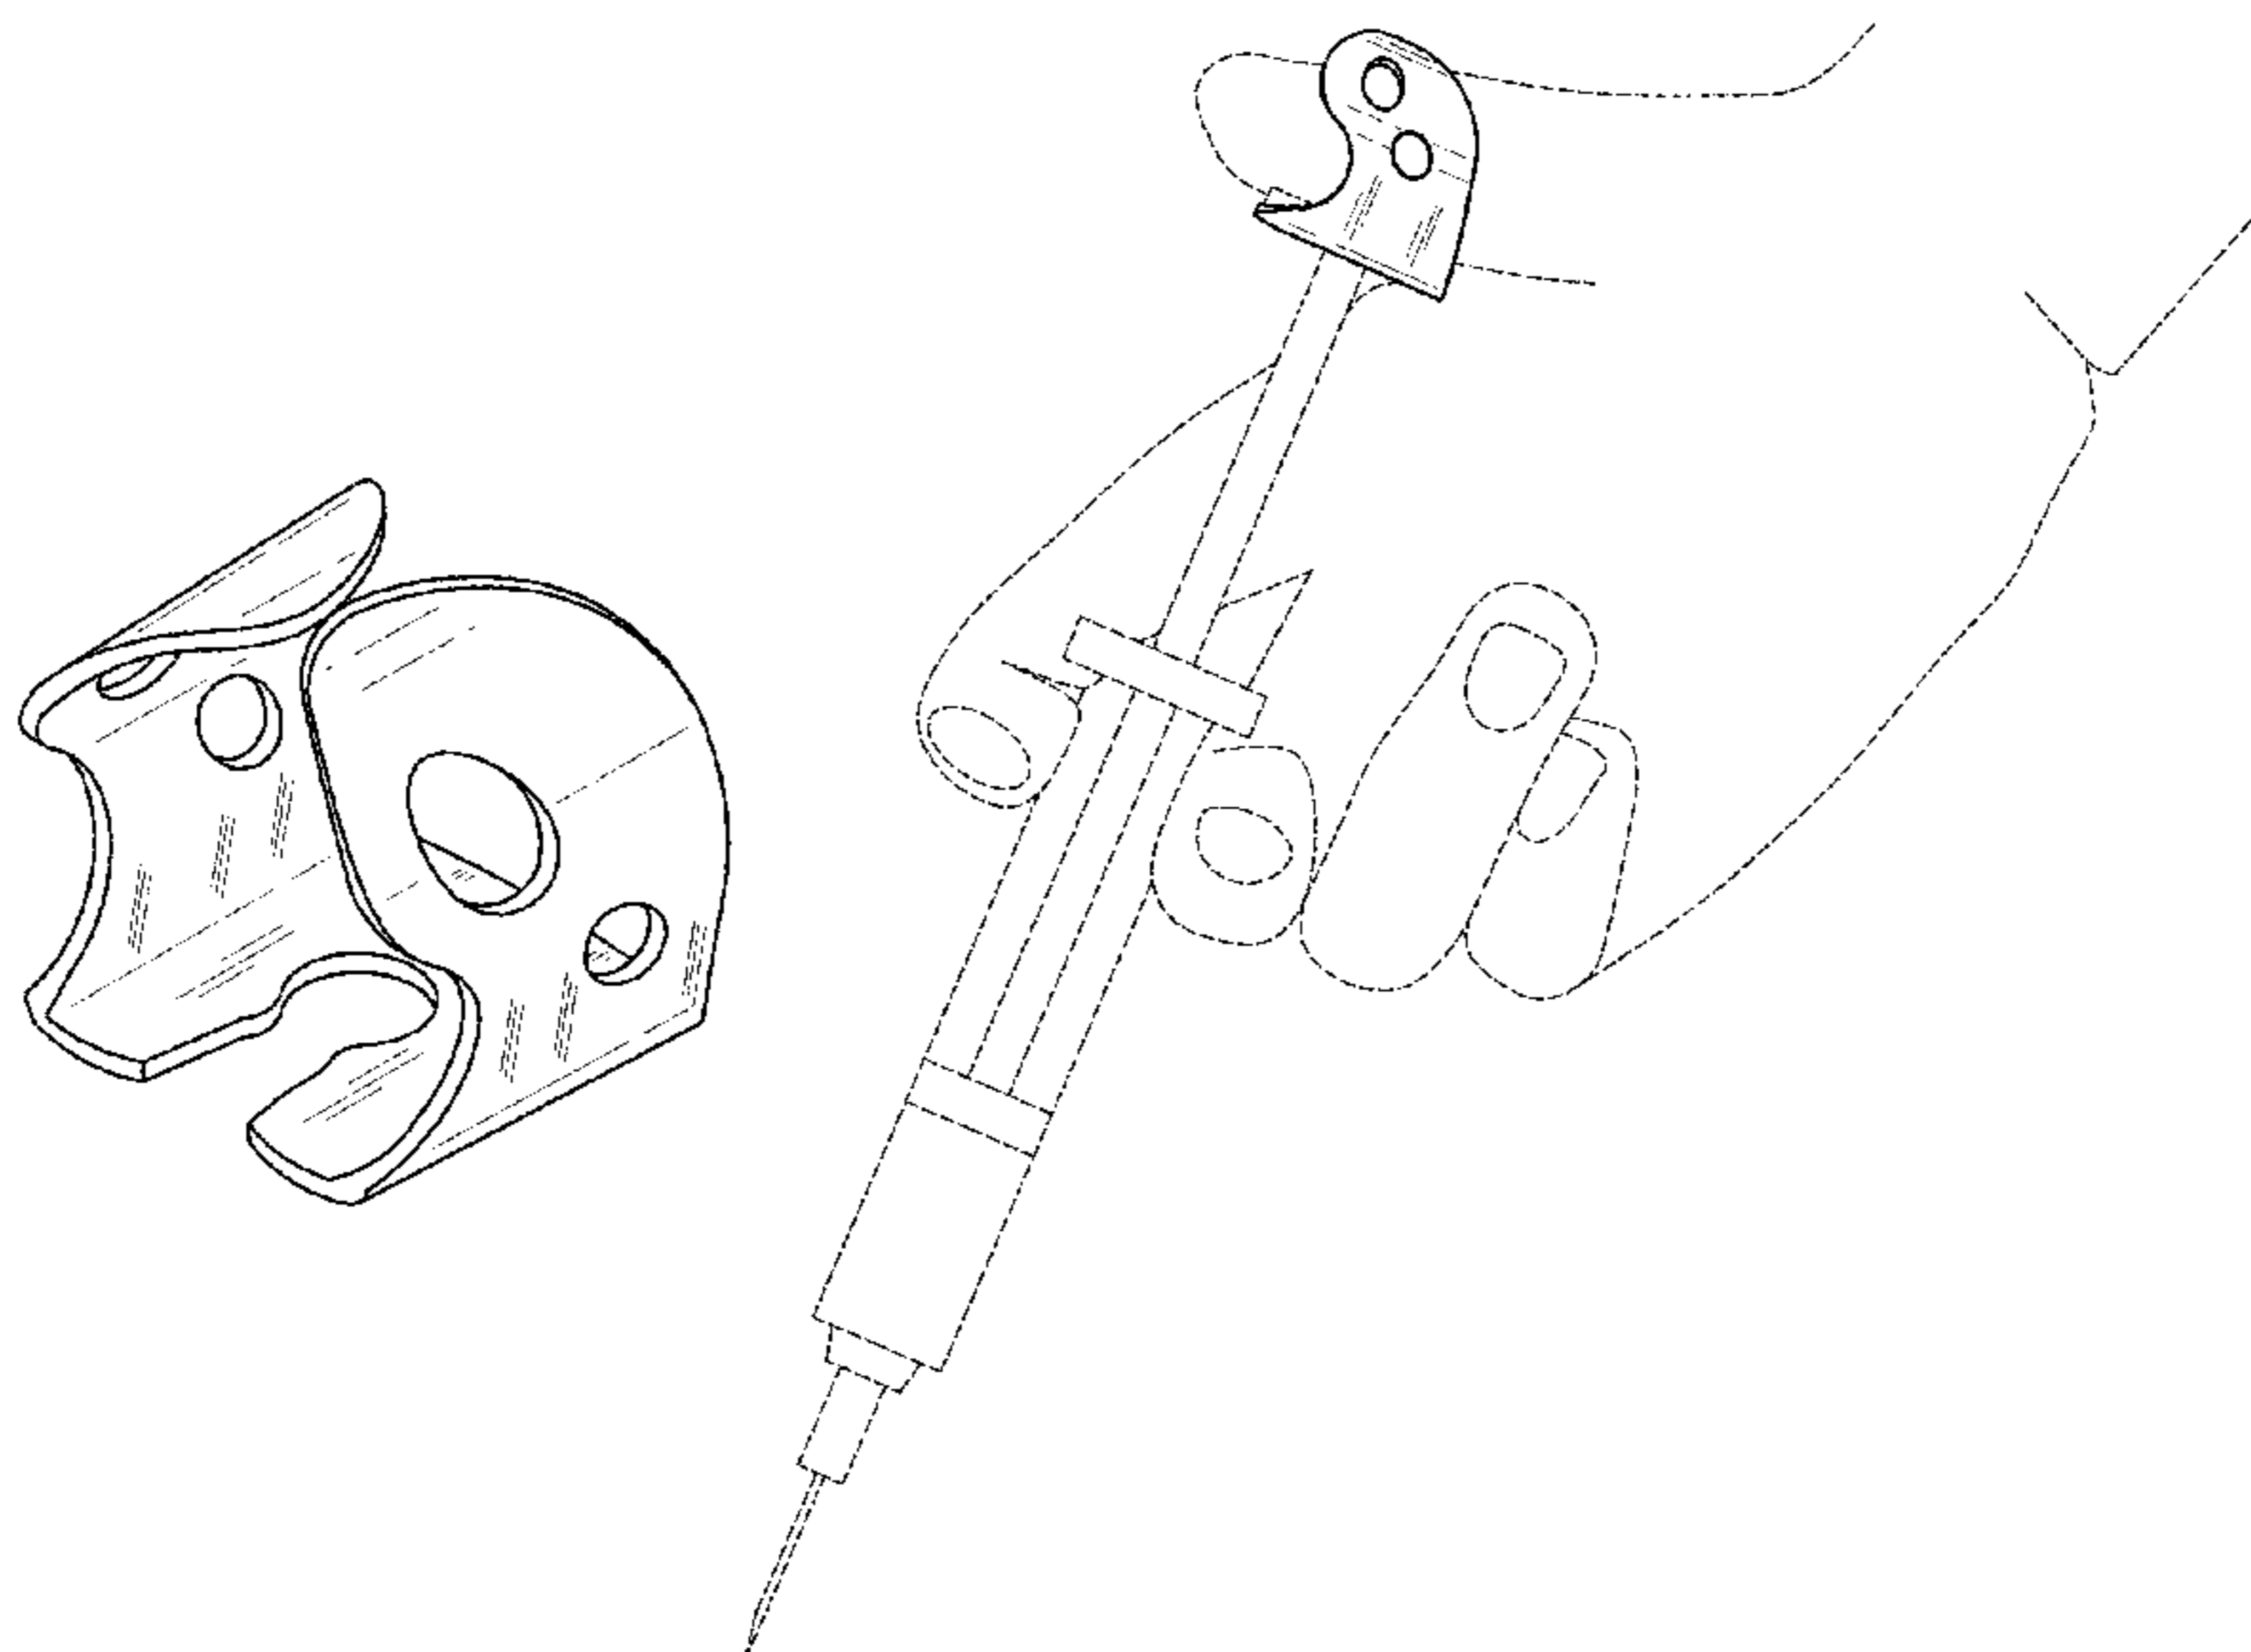

(56)

References Cited

U.S. PATENT DOCUMENTS


D620,384 S \* 7/2010 Crovetti ..... D11/27  
D675,317 S \* 1/2013 Baxter ..... D24/130  
D702,402 S \* 4/2014 Pew ..... D29/113  
D750,768 S \* 3/2016 Davidian ..... D24/114  
D790,691 S \* 6/2017 Davis ..... D24/130  
D794,185 S \* 8/2017 Dolk ..... D24/130  
D794,187 S \* 8/2017 Dolk ..... D24/130  
D797,282 S \* 9/2017 Dolk ..... D24/130  
D811,589 S \* 2/2018 Finke ..... A61M 5/24  
D812,223 S \* 3/2018 Evans ..... D24/130  
D814,630 S \* 4/2018 Finke ..... D24/114  
D823,836 S \* 7/2018 Eaton ..... D14/229  
D830,220 S \* 10/2018 Hardy ..... D11/26  
10,124,238 B2 11/2018 McCrane  
D842,751 S \* 3/2019 Hardy ..... D11/26  
D844,776 S \* 4/2019 Combes ..... D24/114  
D865,950 S \* 11/2019 Mandaroux ..... D24/114  
D869,775 S \* 12/2019 Voosen ..... D29/114  
2003/0028146 A1 2/2003 Ayes  
2006/0205526 A1 9/2006 Whitehead et al.  
2009/0093787 A1 4/2009 Barbour  
2012/0220948 A1 8/2012 Barbour

2015/0238698 A1 8/2015 Perry et al.  
2019/0030253 A1 1/2019 Barbour  
2020/0206425 A1\* 7/2020 Keating ..... A61M 5/3137


OTHER PUBLICATIONS

Miltex, Dental Syringes and Accessories, 2010, 6 pages, Integra LifeSciences Corporation (brochure).  
Medestheticsmag.com, Jan. 12, 2017, 1 page.  
Angiographic Control Syringes, Namic Fluid Management, 2014, 4 pages, AngioDynamics, Inc.  
Lee, Preventing Catastrophes—While Injecting Facial Wrinkles, Oct. 21, 2016, 2 pages, Press Advantage.  
ProSystem Bionic Oxygen Recovery, Prime-Journal.com, Jul./Aug. 2017, 2 pages.  
Jireis, The Best Guitar Finger Picks by Dunlop—Thumbpicks Included! Jan. 7, 2017, 2 pages.  
Sibbitt et al., Thyroid Biopsy with the Reciprocating Procedure Device (RPD), 2006, 2007, 114 pages, University of New Mexico Health Sciences Center.  
Non-Final Office Action issued in U.S. Appl. No. 16/827,433, dated Jun. 23, 2020, 39 pages.  
Non-Final Office Action issued in U.S. Appl. No. 16/827,433, dated Sep. 8, 2020, 24 pages.


\* cited by examiner

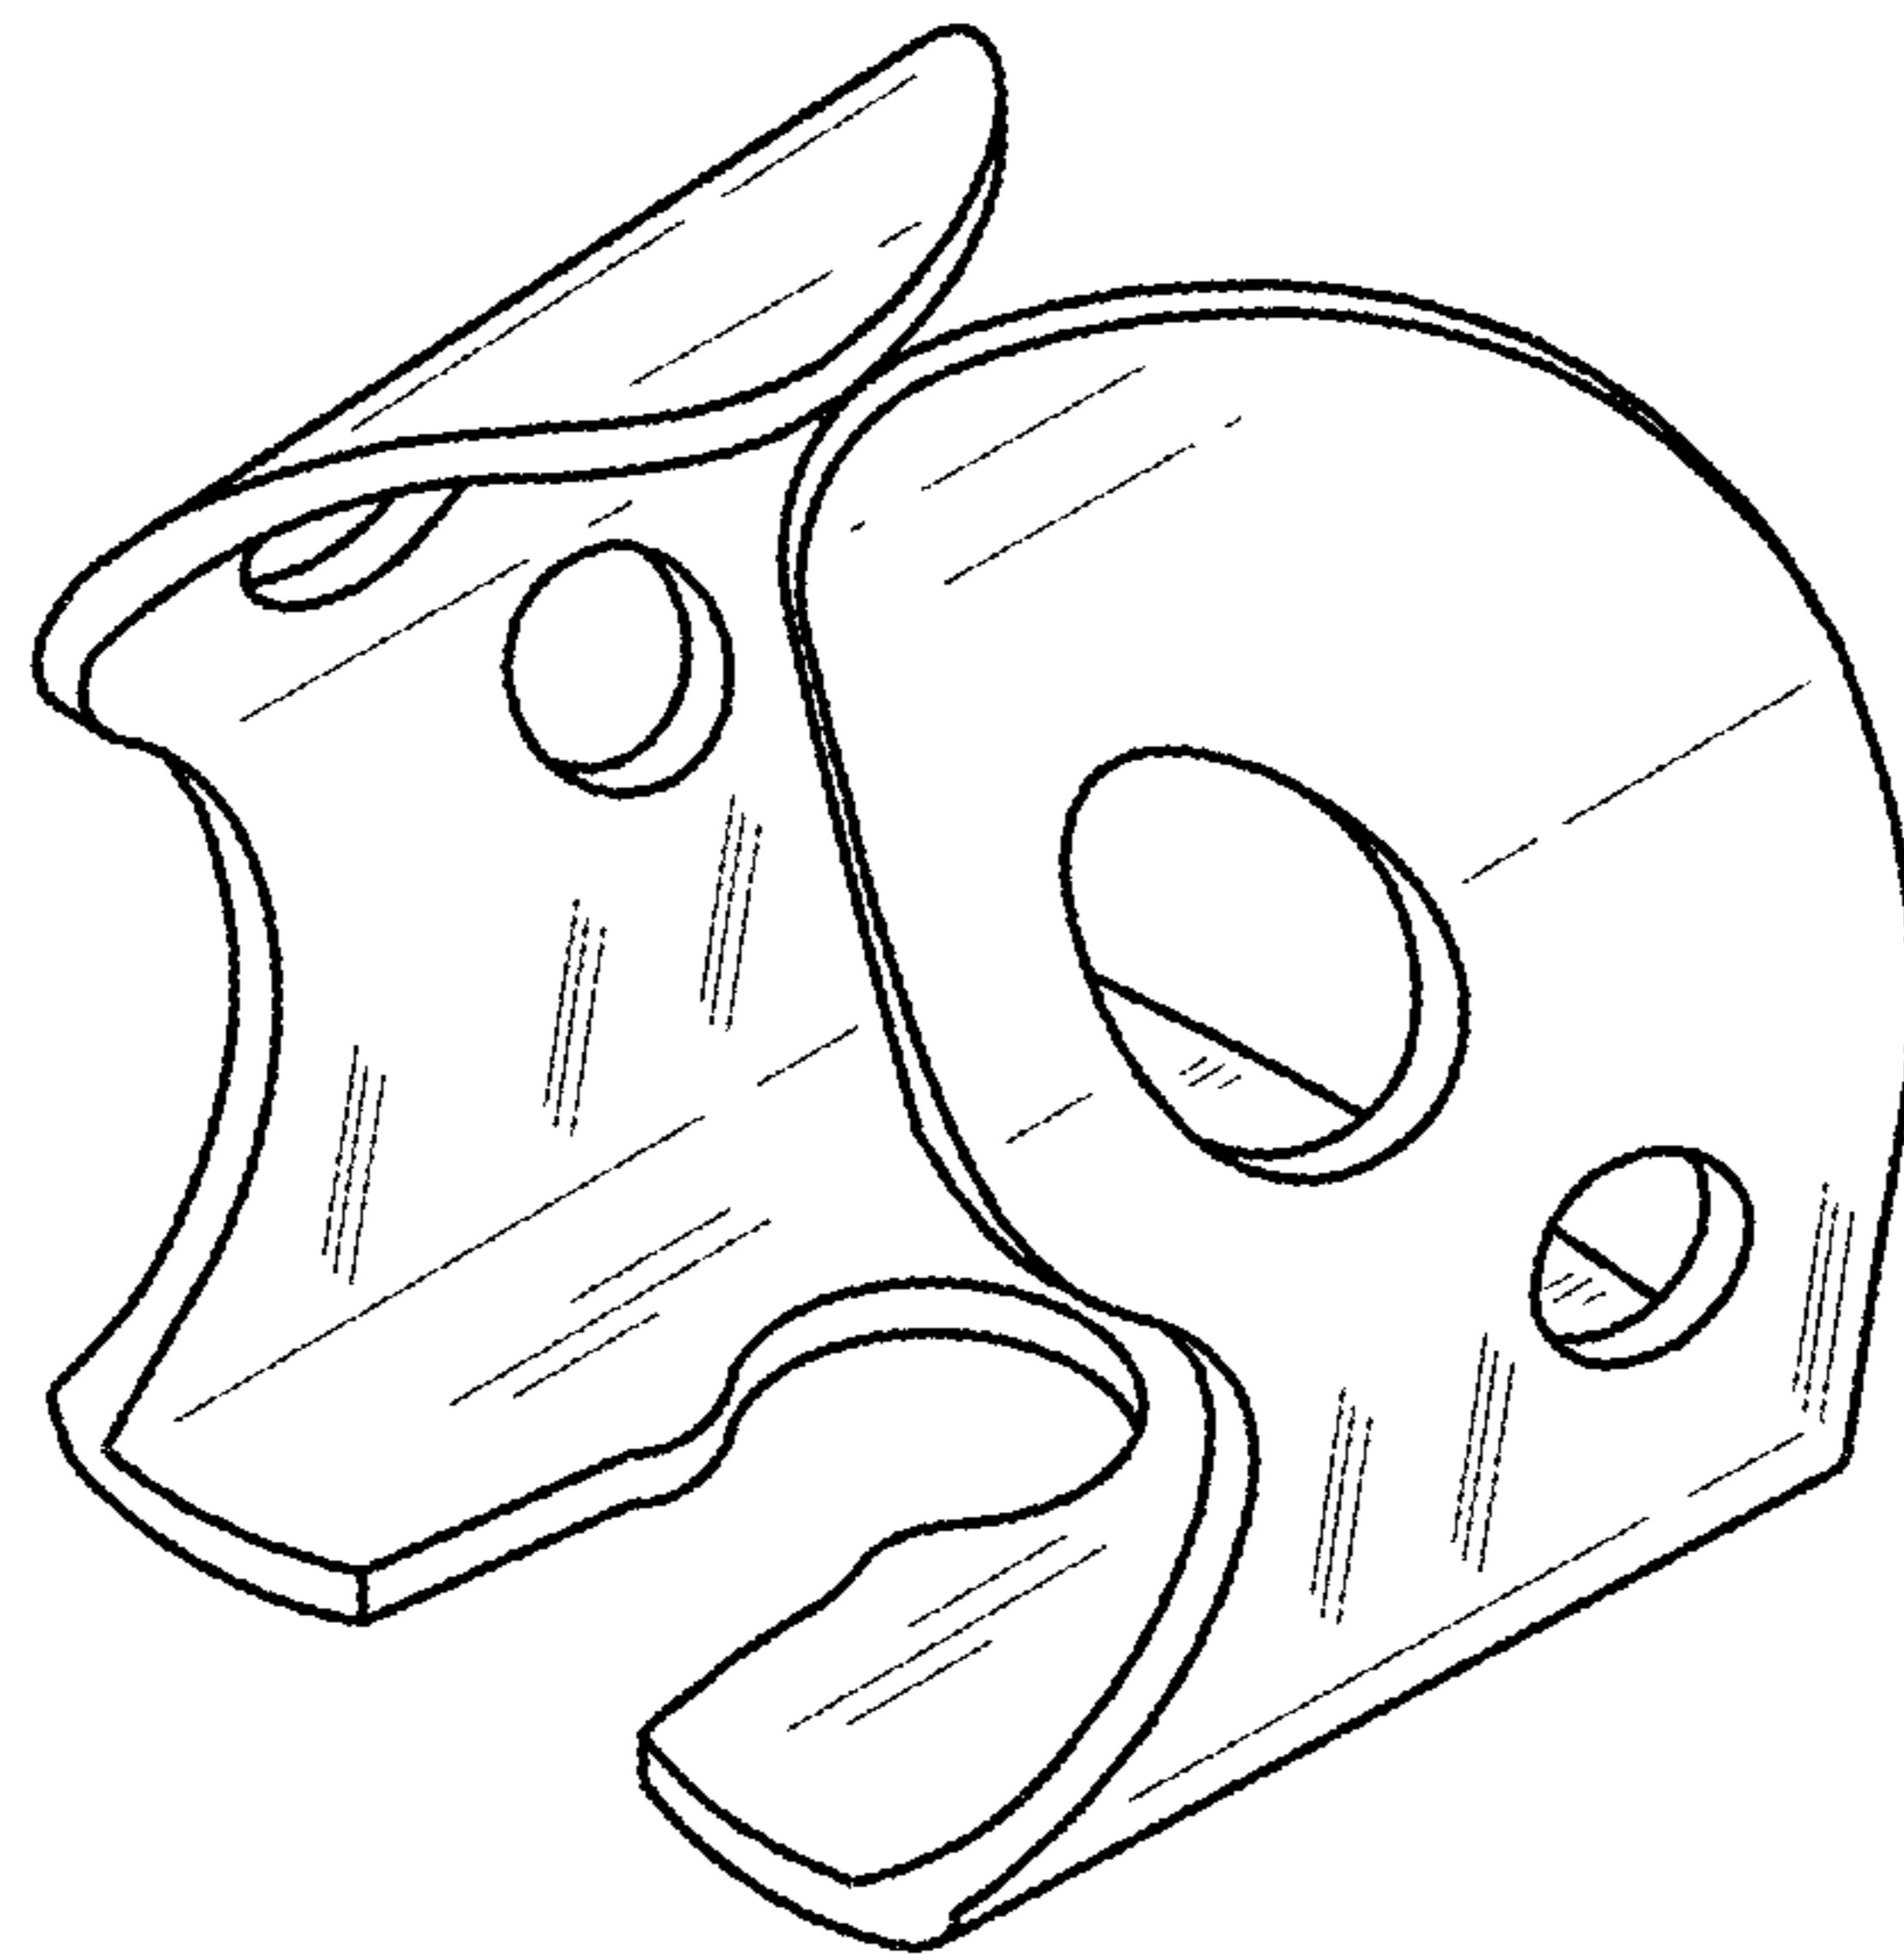


**FIG. 1**

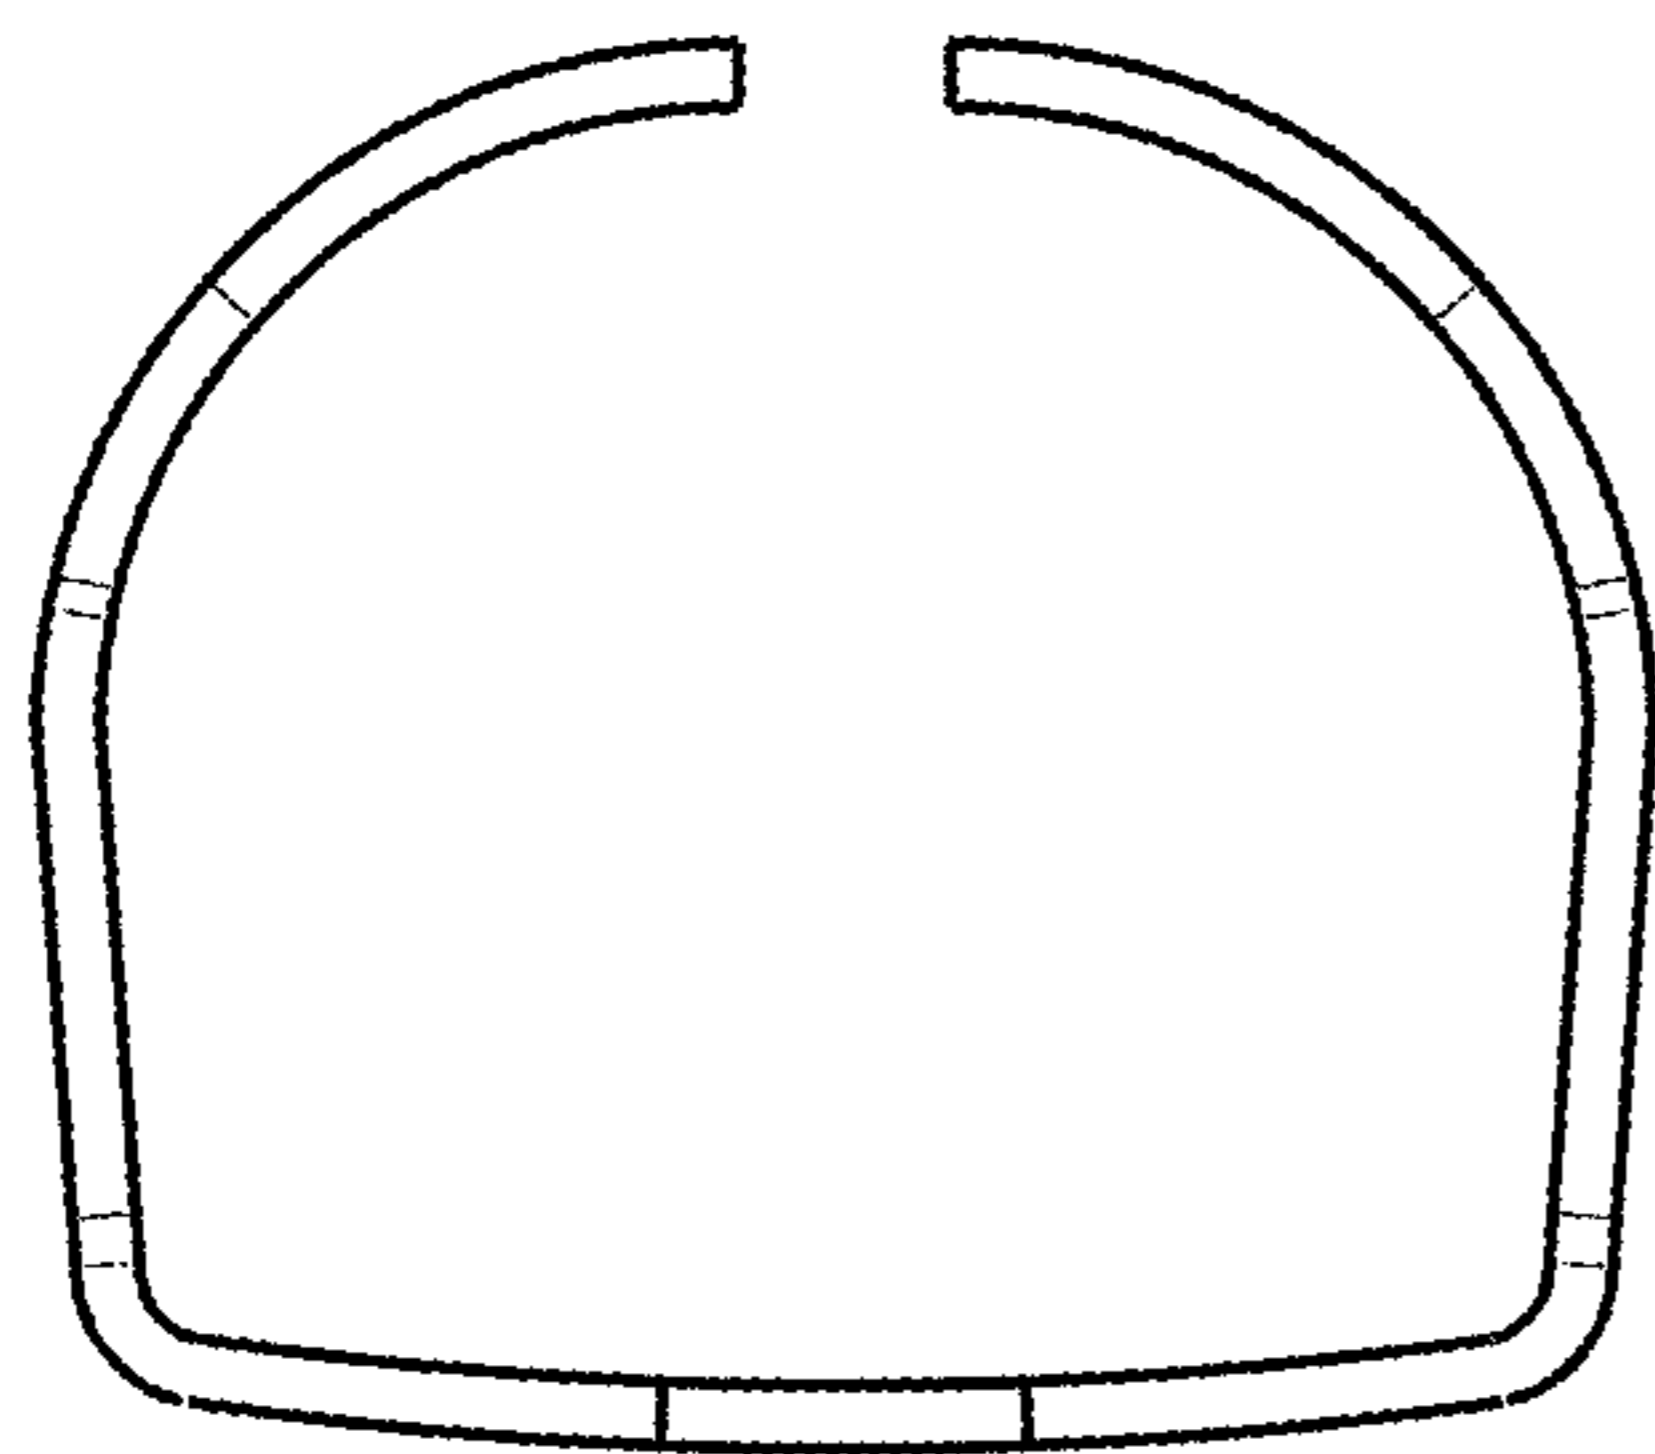


**FIG. 2**

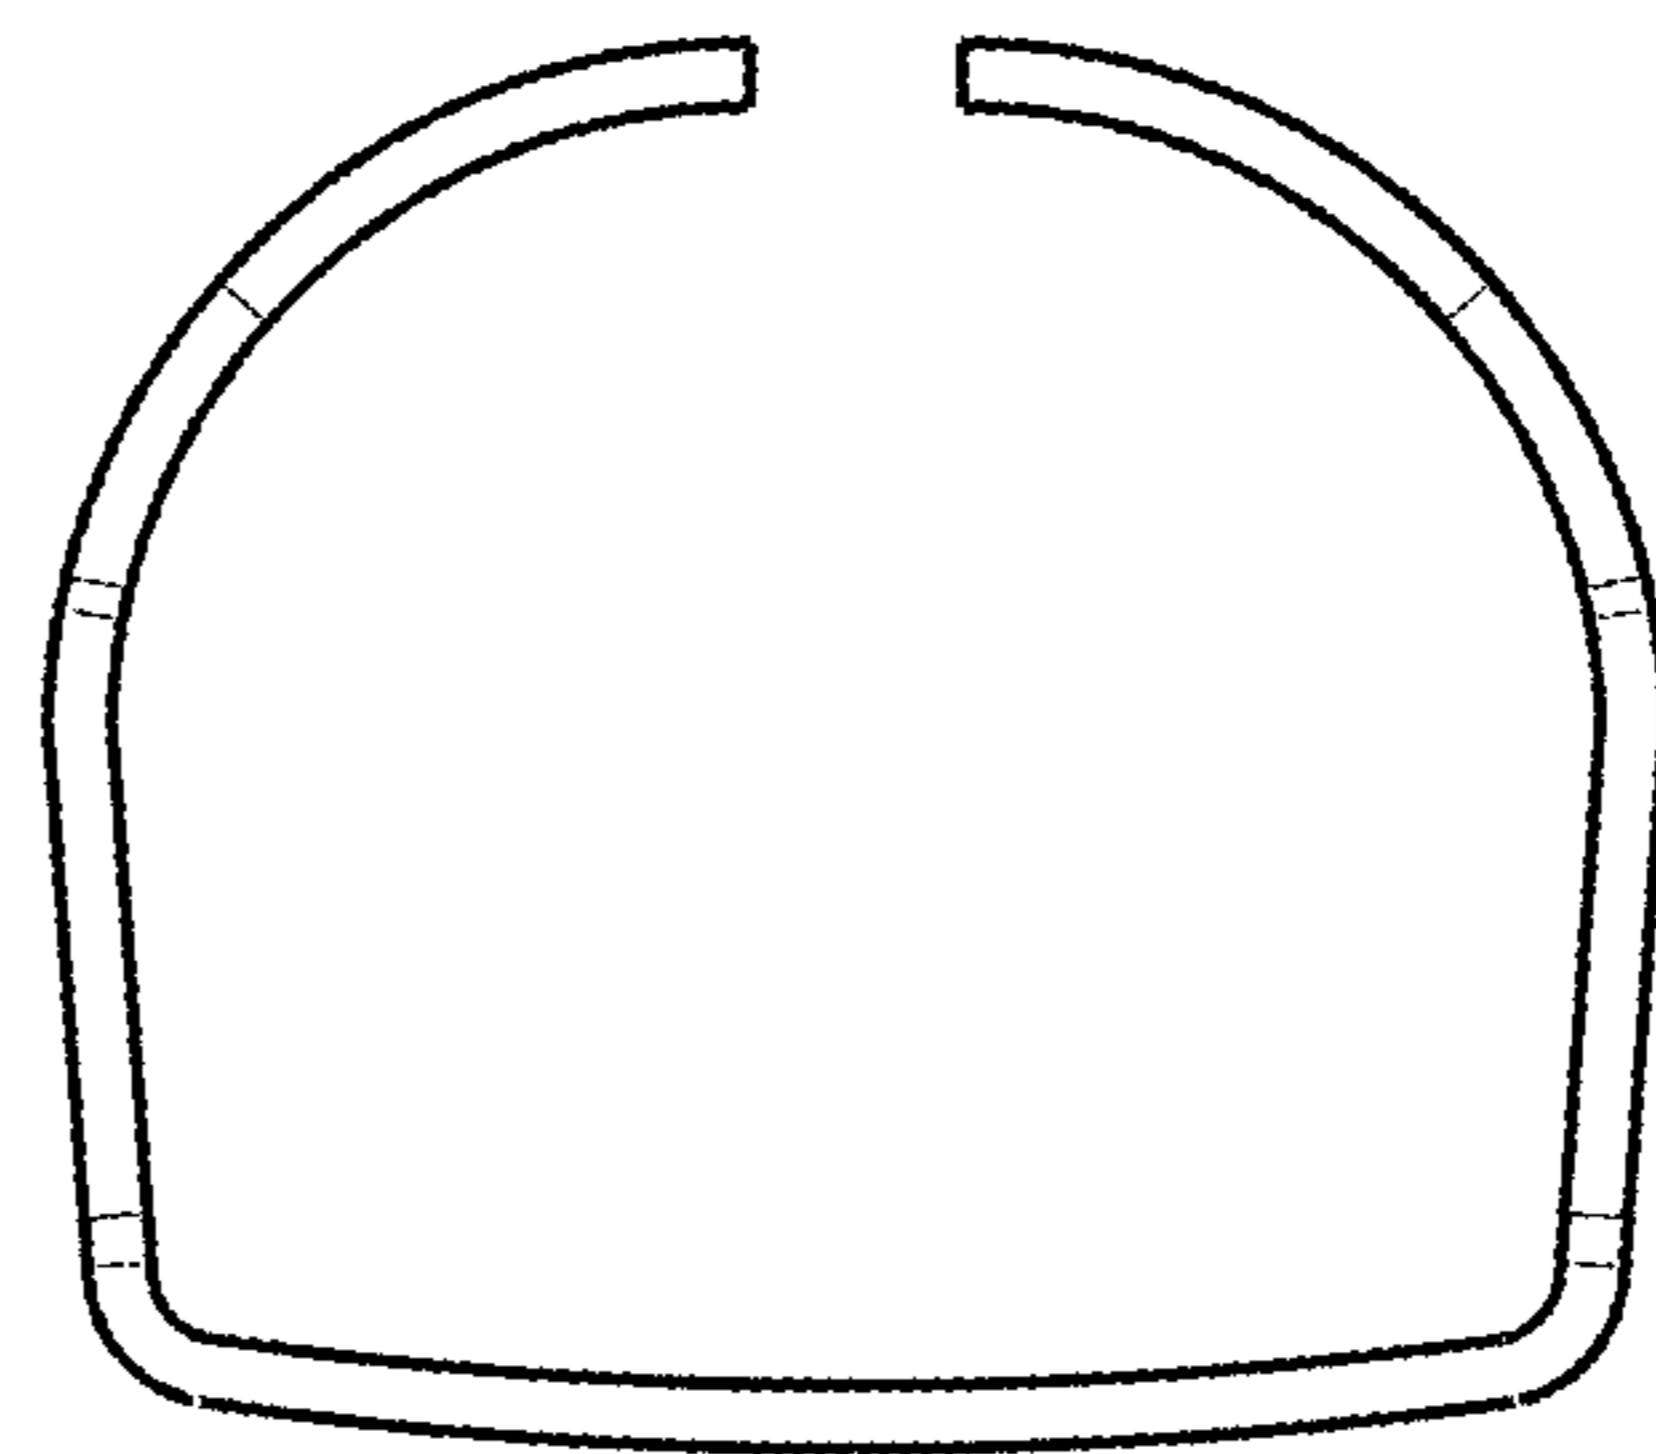


**FIG. 3**

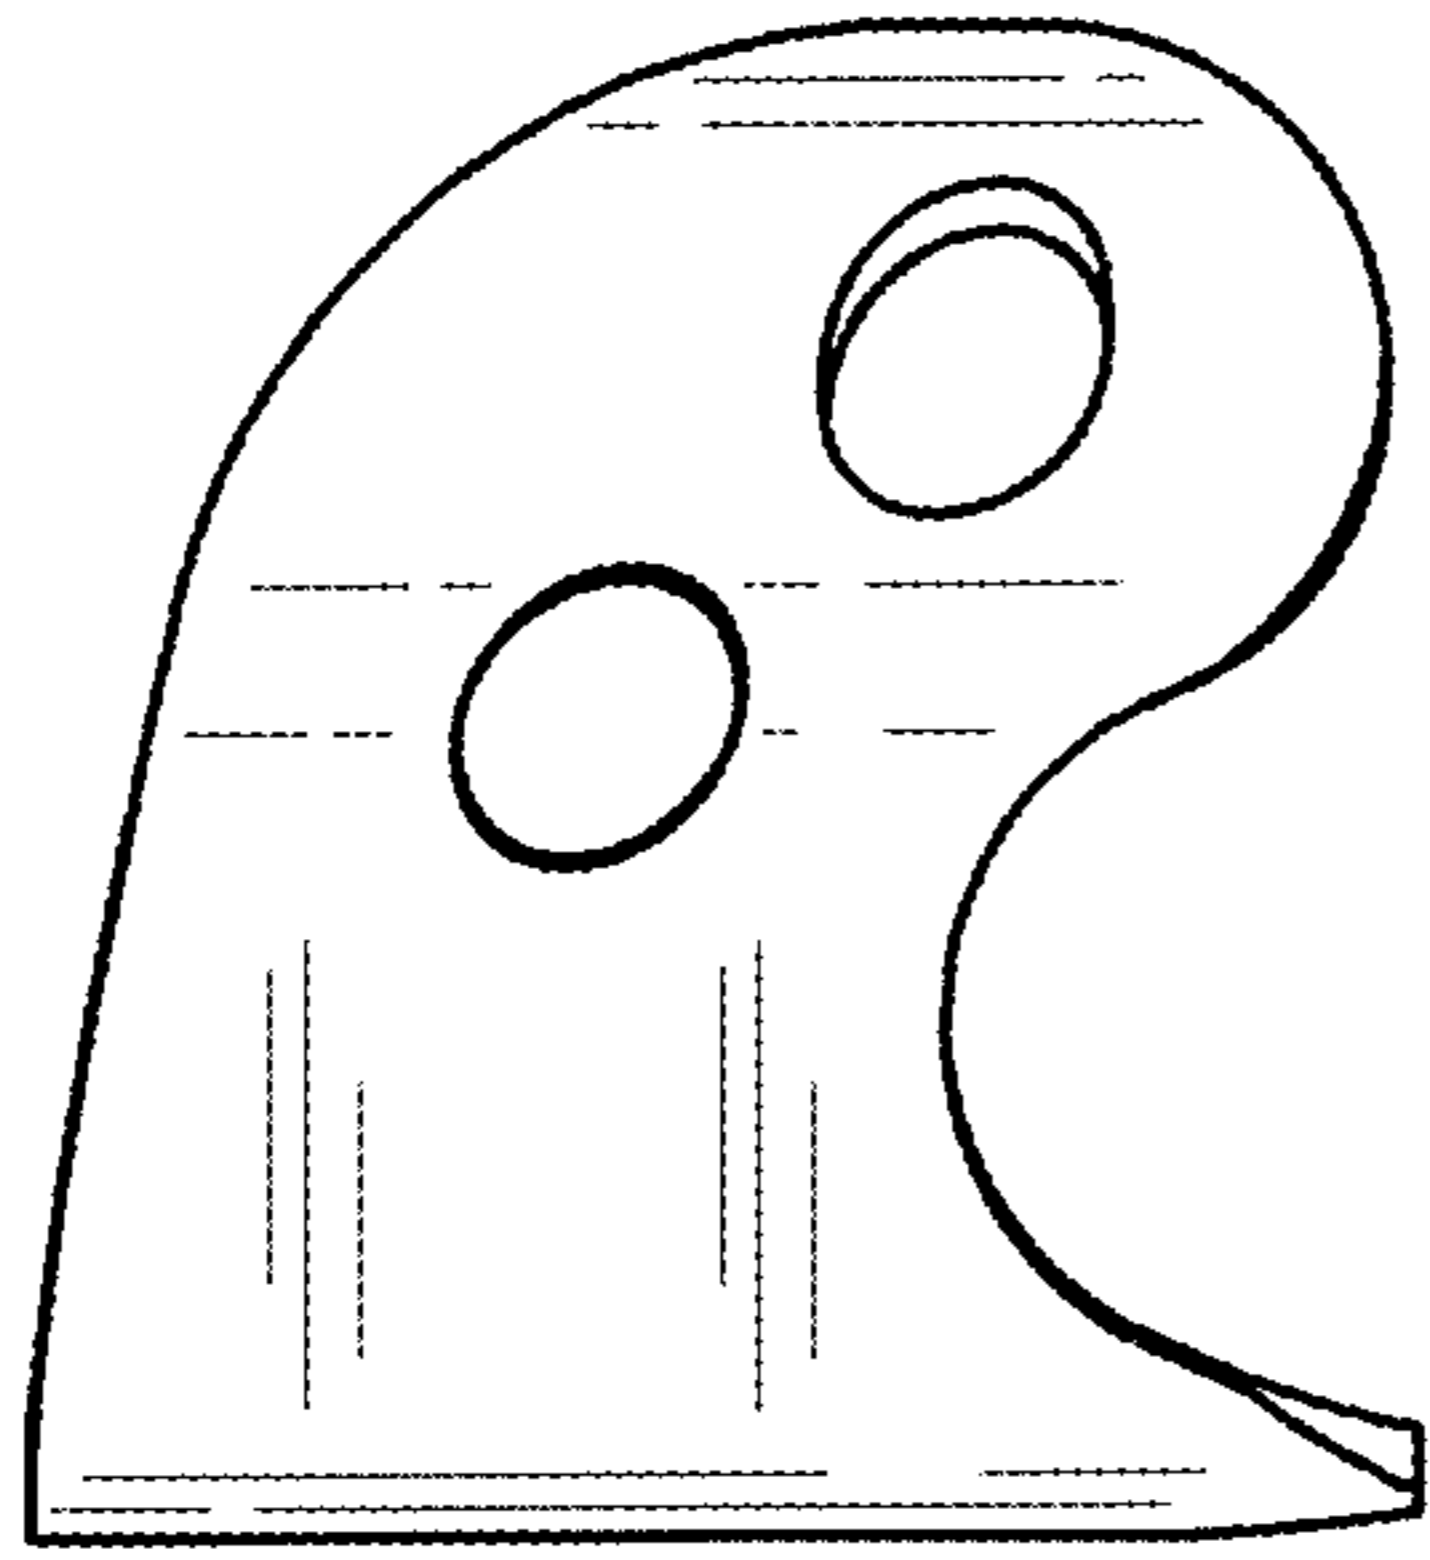


**FIG. 4**

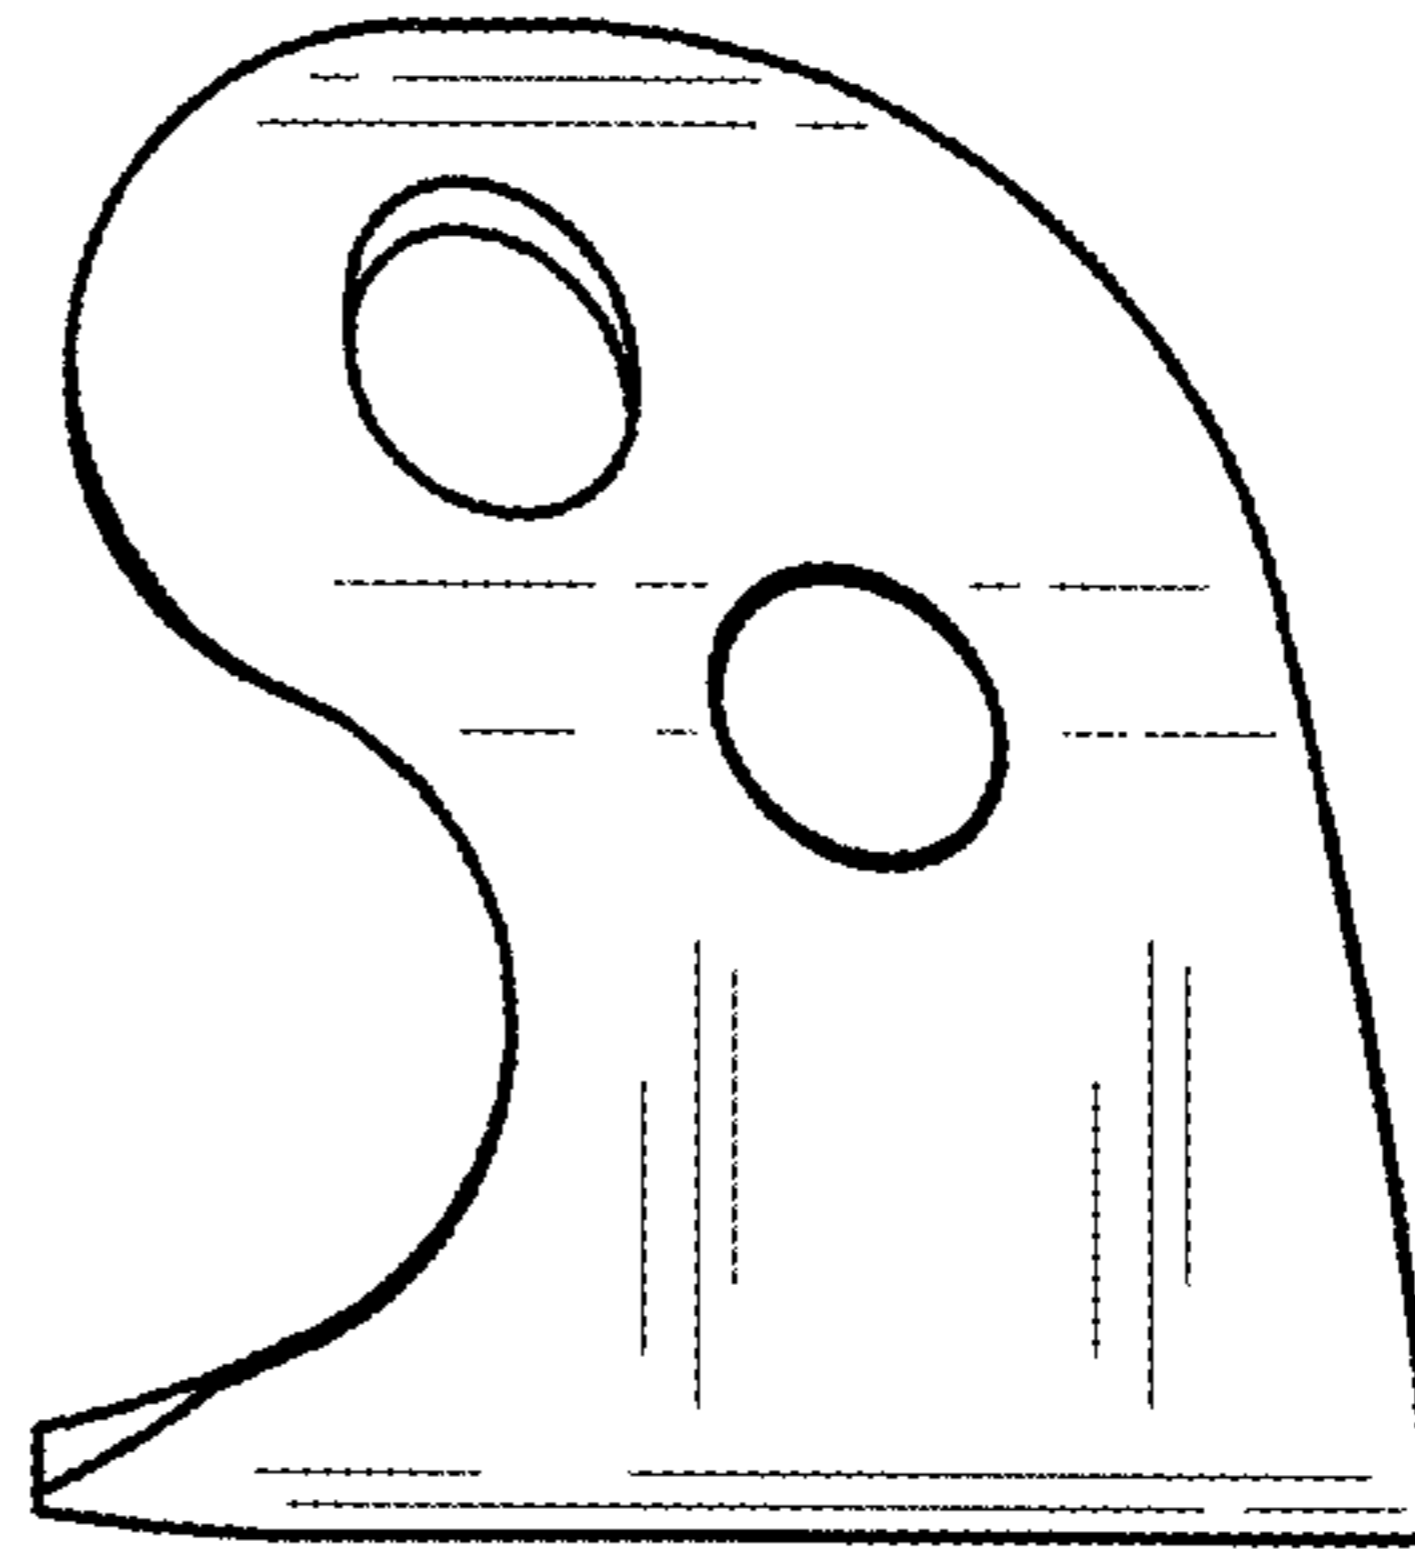

**FIG. 5**

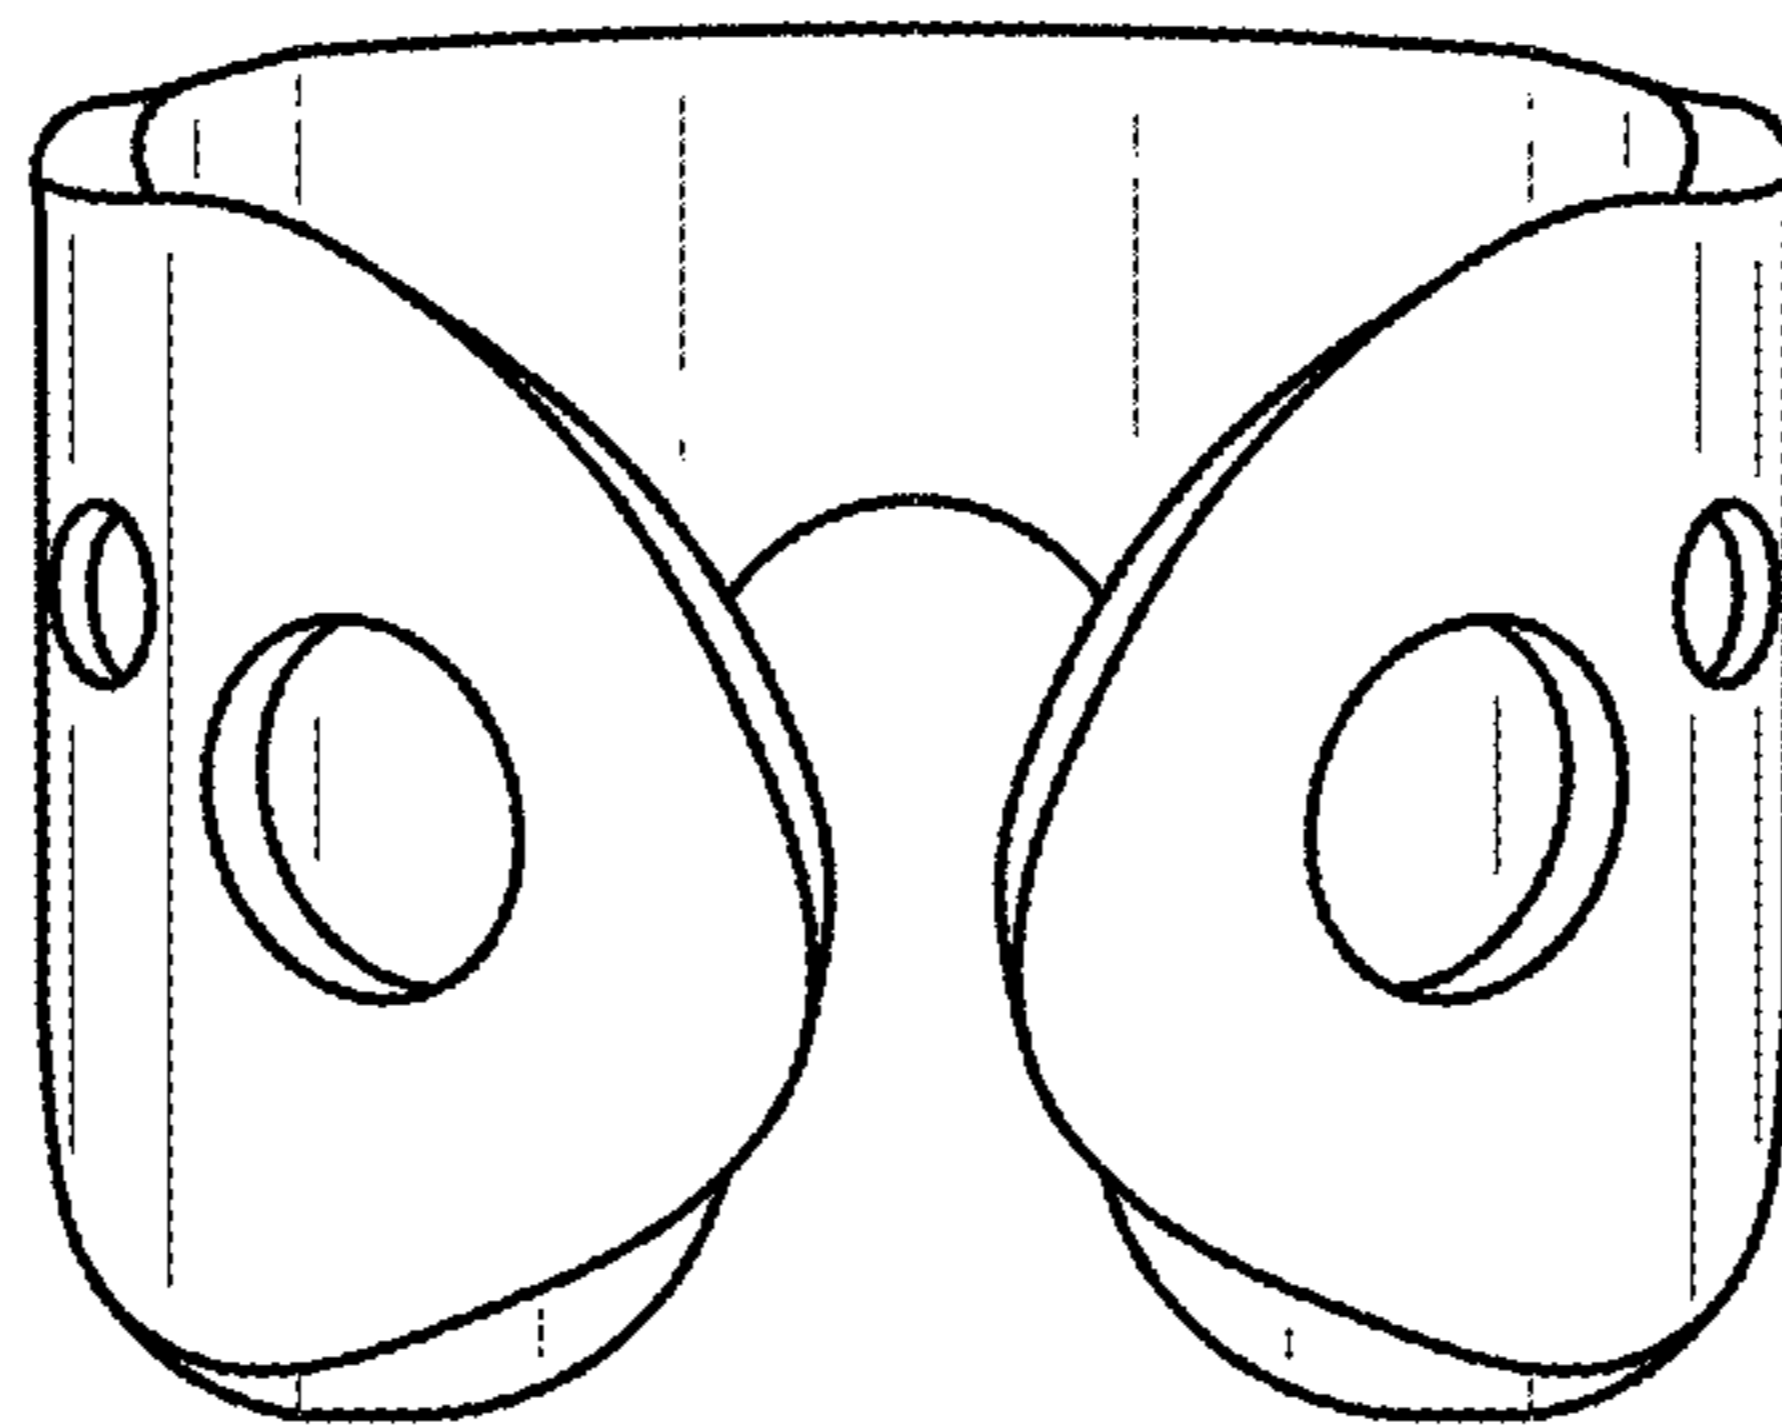

**FIG. 6**

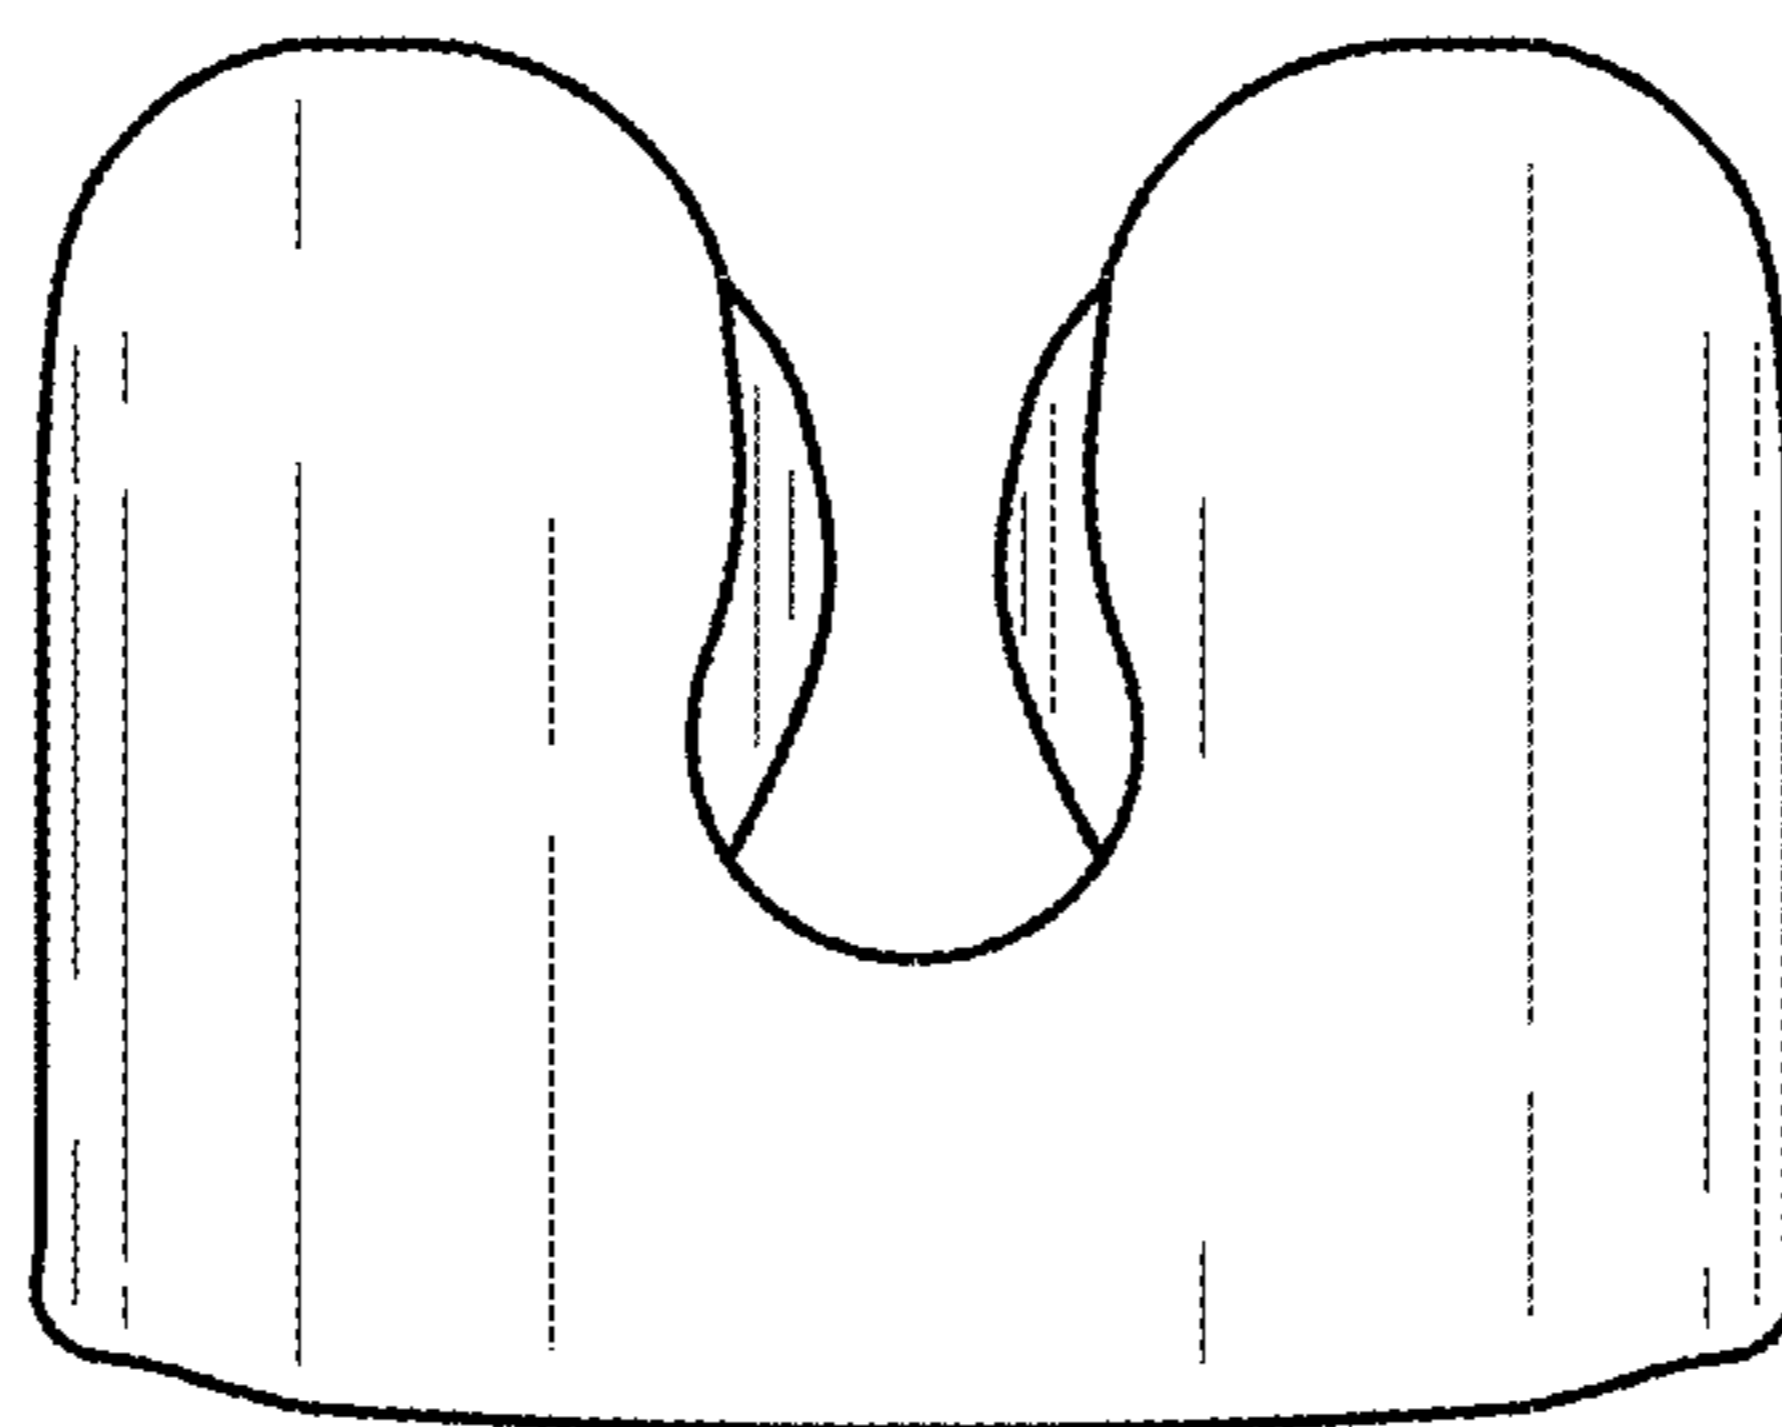

**FIG. 7**

