



US00D905080S

(12) **United States Design Patent** (10) **Patent No.:** **US D905,080 S**  
**Ebler et al.** (45) **Date of Patent:** **\*\* Dec. 15, 2020**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE FOR A MEDICAL DEVICE**

(71) Applicant: **Maquet Cardiopulmonary GmbH**, Rastatt (DE)

(72) Inventors: **Ralph J. Ebler**, Warwick, NY (US); **Daniel Medart**, Stahnsdorf (DE)

(73) Assignee: **MAQUET CARDIOPULMONARY GMBH**, Rastatt (DE)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/645,640**

(22) Filed: **Apr. 27, 2018**

**Related U.S. Application Data**

(62) Division of application No. 29/541,759, filed on Oct. 7, 2015, now Pat. No. Des. 819,042.

(51) **LOC (12) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/486**

(58) **Field of Classification Search**  
USPC ..... D14/485-495  
CPC ..... G06F 3/048; G06F 3/0481; G06F 3/0482; G06F 3/04842; G06F 3/04817  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,791,907 A	8/1998	Ramshaw et al.	
D415,134 S	10/1999	Culp et al.	
D419,543 S	1/2000	Warren et al.	
D422,986 S	4/2000	Williams, Jr. et al.	
D427,574 S *	7/2000	Sawada	D14/486
D468,748 S *	1/2003	Inagaki	D14/486
D474,198 S *	5/2003	Barnes	D14/486

D479,720 S	9/2003	Ohashi et al.	
D503,178 S	3/2005	Choi	
D510,582 S	10/2005	Hoang et al.	
D545,829 S *	7/2007	Fletcher	D14/485
D548,238 S	8/2007	Fletcher	
D548,242 S *	8/2007	Viegers	D14/487
D548,732 S	8/2007	Fletcher	
D548,742 S	8/2007	Fletcher	
D548,743 S *	8/2007	Takahashi	D14/486
D554,663 S	11/2007	Van Dongen et al.	

(Continued)

**FOREIGN PATENT DOCUMENTS**

JP	1294399	1/2007
JP	1437253	3/2012

(Continued)

**OTHER PUBLICATIONS**

Stockert S5 (an article of design: a cardiopulmonary device), S5 Perfusion System, Sorin Group Deutschland GmbH, 2010.

(Continued)

*Primary Examiner* — Philip S Hyder  
*Assistant Examiner* — Cary M Robinson

(74) *Attorney, Agent, or Firm* — Wesley Scott Ashton


(57) **CLAIM**

The ornamental design for a display screen or portion thereof with graphical user interface for a medical device, as shown and described.

**DESCRIPTION**

The FIGURE is a front view of a display screen or portion thereof with graphical user interface for a medical device. The set of broken lines at the periphery of the figure illustrates the display screen and the remaining broken lines illustrate portions of the graphical user interface. None of the broken lines form part of the claimed design.

**1 Claim, 1 Drawing Sheet**

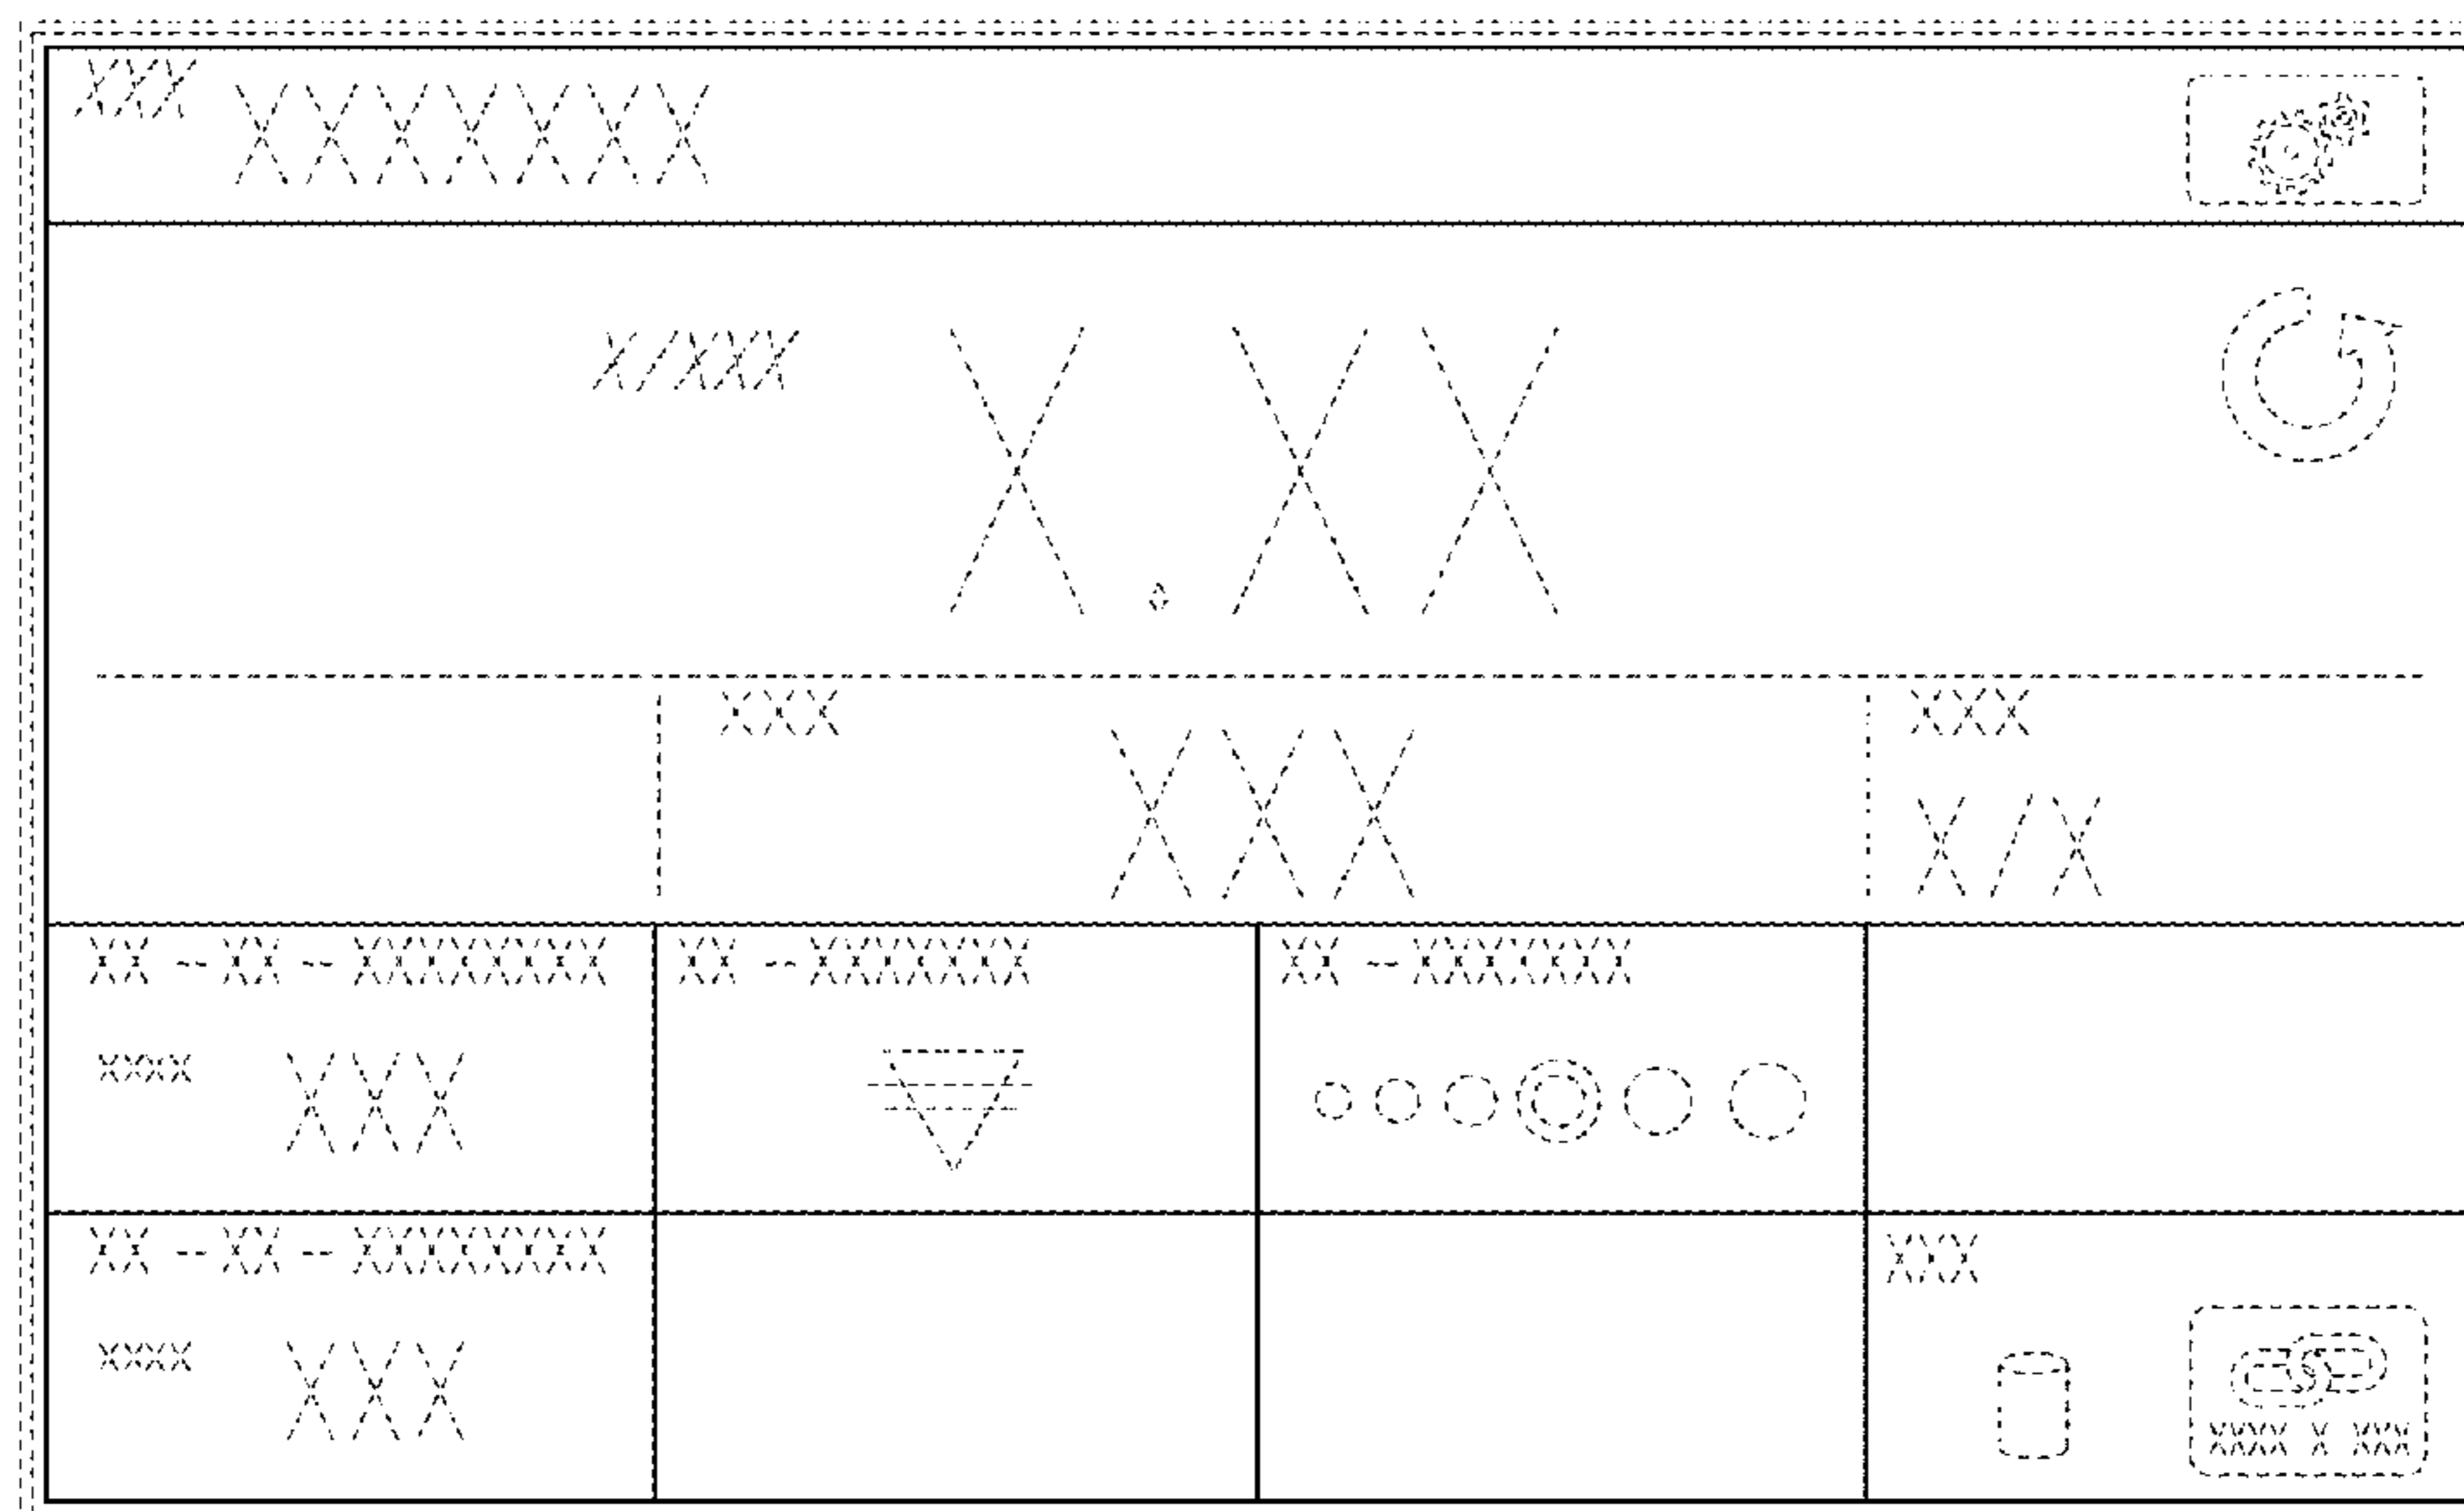



(56)

**References Cited**

U.S. PATENT DOCUMENTS

2004/0268413 A1\* 12/2004 Reid ..... H04N 21/25891  
725/131  
2005/0044485 A1\* 2/2005 Mondry ..... G06Q 10/043  
715/247  
2005/0229110 A1\* 10/2005 Gegner ..... G06F 3/0481  
715/800  
2006/0053384 A1\* 3/2006 La Fetra, Jr. .... G06F 3/048  
715/765  
2007/0011702 A1 1/2007 Vaysman ..... H04N 21/84  
725/45  
2007/0199022 A1\* 8/2007 Moshiri ..... H04N 5/44513  
725/39  
2007/0288868 A1 12/2007 Rhee ..... G06F 3/04817  
715/840  
2008/0082938 A1\* 4/2008 Buczek ..... G06F 40/18  
715/784  
2012/0005607 A1\* 1/2012 Tofinetti ..... G06F 3/0481  
715/769  
2012/0079429 A1\* 3/2012 Stathacopoulos .. H04N 5/44543  
715/830  
2012/0089914 A1\* 4/2012 Holt ..... G06F 3/0485  
715/728  
2013/0055167 A1\* 2/2013 Leong ..... G06F 16/9038  
715/854  
2013/0127870 A1\* 5/2013 Baudel ..... G06F 9/451  
345/441  
2013/0187780 A1 7/2013 Angelides ..... A61B 5/0002  
340/573.1  
2014/0127063 A1 5/2014 Petersen et al.  
2014/0149942 A1\* 5/2014 Wood-Salomon .... G06F 3/0482  
715/840  
2014/0192229 A1\* 7/2014 Kim ..... G06K 9/00302  
348/231.3  
2015/0067611 A1\* 3/2015 Spohr ..... G06Q 10/10  
715/844  
2015/0169581 A1\* 6/2015 Pusateri ..... G06F 16/35  
707/737  
2015/0213211 A1\* 7/2015 Zaleski ..... G06F 16/9535  
715/753  
2015/0248534 A1\* 9/2015 Krzywicki ..... G06F 3/04847  
715/771  
2015/0362927 A1 12/2015 Giorgi  
2017/0013147 A1\* 1/2017 Umezawa ..... G06F 9/451  
2017/0102846 A1 4/2017 Ebler et al.  
2019/0302981 A1\* 10/2019 Storr ..... G06F 3/0486

FOREIGN PATENT DOCUMENTS

JP 1458638 1/2013  
JP 1484744 10/2013  
JP 1584029 S 7/2017  
JP 1585836 S 8/2017

OTHER PUBLICATIONS

“We introduced “Stockert artificial cardiopulmonary device S5” in 2013” in an item “an artificial cardiopulmonary device”, and it is recognized that this “Stockert artificial cardiopulmonary device S5” is same as the above “Stockert S5”, downloaded from <https://web.archive.org/web/20140321232731/www.nho-kumamoto.jp/about/hardwares.html> on Nov. 20, 2018.

Official Action issued in JP Application No. 2017-12102, dated Oct. 30, 2018.  
Final Official Action issued in JP Application No. 2018-284, dated Nov. 15, 2018.  
Non-Final Office Action—dated Jan. 26, 2018—for U.S. Appl. No. 29/601,895, which corresponds to this pending application.  
Product Brochure—CS300 IABP—Product Features—2009 Publication—Maquet Cardiovascular LLC. U.S.A.  
Product Brochure—CS100 IABP—Intelligent Counterpulsation—2010 Publication—Maquet Cardiovascular LLC. U.S.A.  
Operators Guide—The CS100/CS100i Abbreviated Operator’s Guide—2009 Publication—Maquet Cardiovascular LLC. U.S.A.  
Operators Guide—Datascope Abbreviated Operator’s Guide for the System 97 Intra-Aortic Balloon Pump—Published prior to 2009—Datascope Corp. U.S.A.  
Brochure—Sensation and CS300 IABP System Smaller Meets Faster—Published in 2009—Maquet Cardiovascular LLC. U.S.A.  
Brochure—CS300 IABP Product Features—Published in 2009—Maquet Cardiovascular LLC. U.S.A.  
Sorin | S5 Brochure, Sorin Group USA, Inc., 2010.  
MetaVision Perfusion™, a point-of-care clinical information system for perfusionists, Maquet Getinge Group 2015 <<http://www.maquet.com/int/products/metavision-perfusion/>>.  
Heart-Lung Machine HL20 Brochure, Maquet Cardiopulmonary AG 2012.  
“Heart Lung Machine Fundraising.” Aug. 18, 2015. Web. Nov. 6, 2015. <<http://www.heartcentreforchildren.com.au/heart-lung-machine-fundraising.html>>.  
Heart-lung machines. surgeryencyclopedia.com. Advameg, Inc. 2015. Web. Nov. 5, 2015. <<http://www.surgeryencyclopedia.com/Fi-La/Heart-Lung-Machines.html>>.  
Machine coeur-poumon HL30. Feb. 21, 2013. Web. Nov. 18, 2015. <<file:///C:/Users/u2002449/Downloads/mes-130225-MachineCoeurPoumonHL30-Maquet.pdf>>.  
Terumo Advanced Perfusion System 1. Terumo Cardiovascular Group. Nov. 2014. Web. Nov. 18, 2015. <[http://www.terumo-cvs.com/doc/848594\\_Terumo-System1\\_Brochure%20\\_Nov2013\\_LowRes\\_Pgs.pdf](http://www.terumo-cvs.com/doc/848594_Terumo-System1_Brochure%20_Nov2013_LowRes_Pgs.pdf)>.  
Product Catalog Jostra HL 20. Maquet Cardiopulmonary AG. Web. Nov. 18, 2015. <[http://glavm.ru/upload/information\\_system\\_18/2/8/7/item\\_287/information\\_items\\_property\\_343\\_pdf](http://glavm.ru/upload/information_system_18/2/8/7/item_287/information_items_property_343_pdf)>.  
Sorin | S5 System Operating Instructions, Sorin Group Deutschland GmbH, 2006, 2007.  
Hessel, Eugene A., “Circuitry and Cannulation Techniques”, Chapter 5, Cardiopulmonary Bypass: Principles and Practices, edited by Glenn P. Gravlee, 3rd edition, 2008, pp. 63-65.  
Sorin article, <http://www.sorin.com/products/cardiac-surgery/perfusion/hlm/s5>, printed on Jun. 13, 2015, 11 pages.  
Non-Final Office Action dated Dec. 14, 2018 issued for related U.S. Appl. No. 29/646,368, 7 pages.  
Japanese Office Action dated Feb. 22, 2019 during the prosecution of Japanese Design Patent Application No. 2018-000284, 5 pages.  
Japanese Decision on Appeal dated Mar. 6, 2019 during the prosecution of Japanese Design Patent Application No. 2017-012102, 59 pages.  
EP Office Action dated May 8, 2019 during the prosecution of EP Patent Application No. 16722661.2, 6 pages.

\* cited by examiner

