



US00D905080S

(12) **United States Design Patent** (10) **Patent No.:** **US D905,080 S**
Ebler et al. (45) **Date of Patent:** **** Dec. 15, 2020**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE FOR A MEDICAL DEVICE**

(71) Applicant: **Maquet Cardiopulmonary GmbH**, Rastatt (DE)

(72) Inventors: **Ralph J. Ebler**, Warwick, NY (US); **Daniel Medart**, Stahnsdorf (DE)

(73) Assignee: **MAQUET CARDIOPULMONARY GMBH**, Rastatt (DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/645,640**

(22) Filed: **Apr. 27, 2018**

Related U.S. Application Data

(62) Division of application No. 29/541,759, filed on Oct. 7, 2015, now Pat. No. Des. 819,042.

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048; G06F 3/0481; G06F 3/0482; G06F 3/04842; G06F 3/04817
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,791,907 A	8/1998	Ramshaw et al.	
D415,134 S	10/1999	Culp et al.	
D419,543 S	1/2000	Warren et al.	
D422,986 S	4/2000	Williams, Jr. et al.	
D427,574 S *	7/2000	Sawada	D14/486
D468,748 S *	1/2003	Inagaki	D14/486
D474,198 S *	5/2003	Barnes	D14/486

D479,720 S	9/2003	Ohashi et al.	
D503,178 S	3/2005	Choi	
D510,582 S	10/2005	Hoang et al.	
D545,829 S *	7/2007	Fletcher	D14/485
D548,238 S	8/2007	Fletcher	
D548,242 S *	8/2007	Viegers	D14/487
D548,732 S	8/2007	Fletcher	
D548,742 S	8/2007	Fletcher	
D548,743 S *	8/2007	Takahashi	D14/486
D554,663 S	11/2007	Van Dongen et al.	

(Continued)

FOREIGN PATENT DOCUMENTS

JP	1294399	1/2007
JP	1437253	3/2012

(Continued)

OTHER PUBLICATIONS

Stockert S5 (an article of design: a cardiopulmonary device), S5 Perfusion System, Sorin Group Deutschland GmbH, 2010.

(Continued)

Primary Examiner — Philip S Hyder
Assistant Examiner — Cary M Robinson
(74) *Attorney, Agent, or Firm* — Wesley Scott Ashton


(57) **CLAIM**

The ornamental design for a display screen or portion thereof with graphical user interface for a medical device, as shown and described.

DESCRIPTION

The FIGURE is a front view of a display screen or portion thereof with graphical user interface for a medical device. The set of broken lines at the periphery of the figure illustrates the display screen and the remaining broken lines illustrate portions of the graphical user interface. None of the broken lines form part of the claimed design.

1 Claim, 1 Drawing Sheet

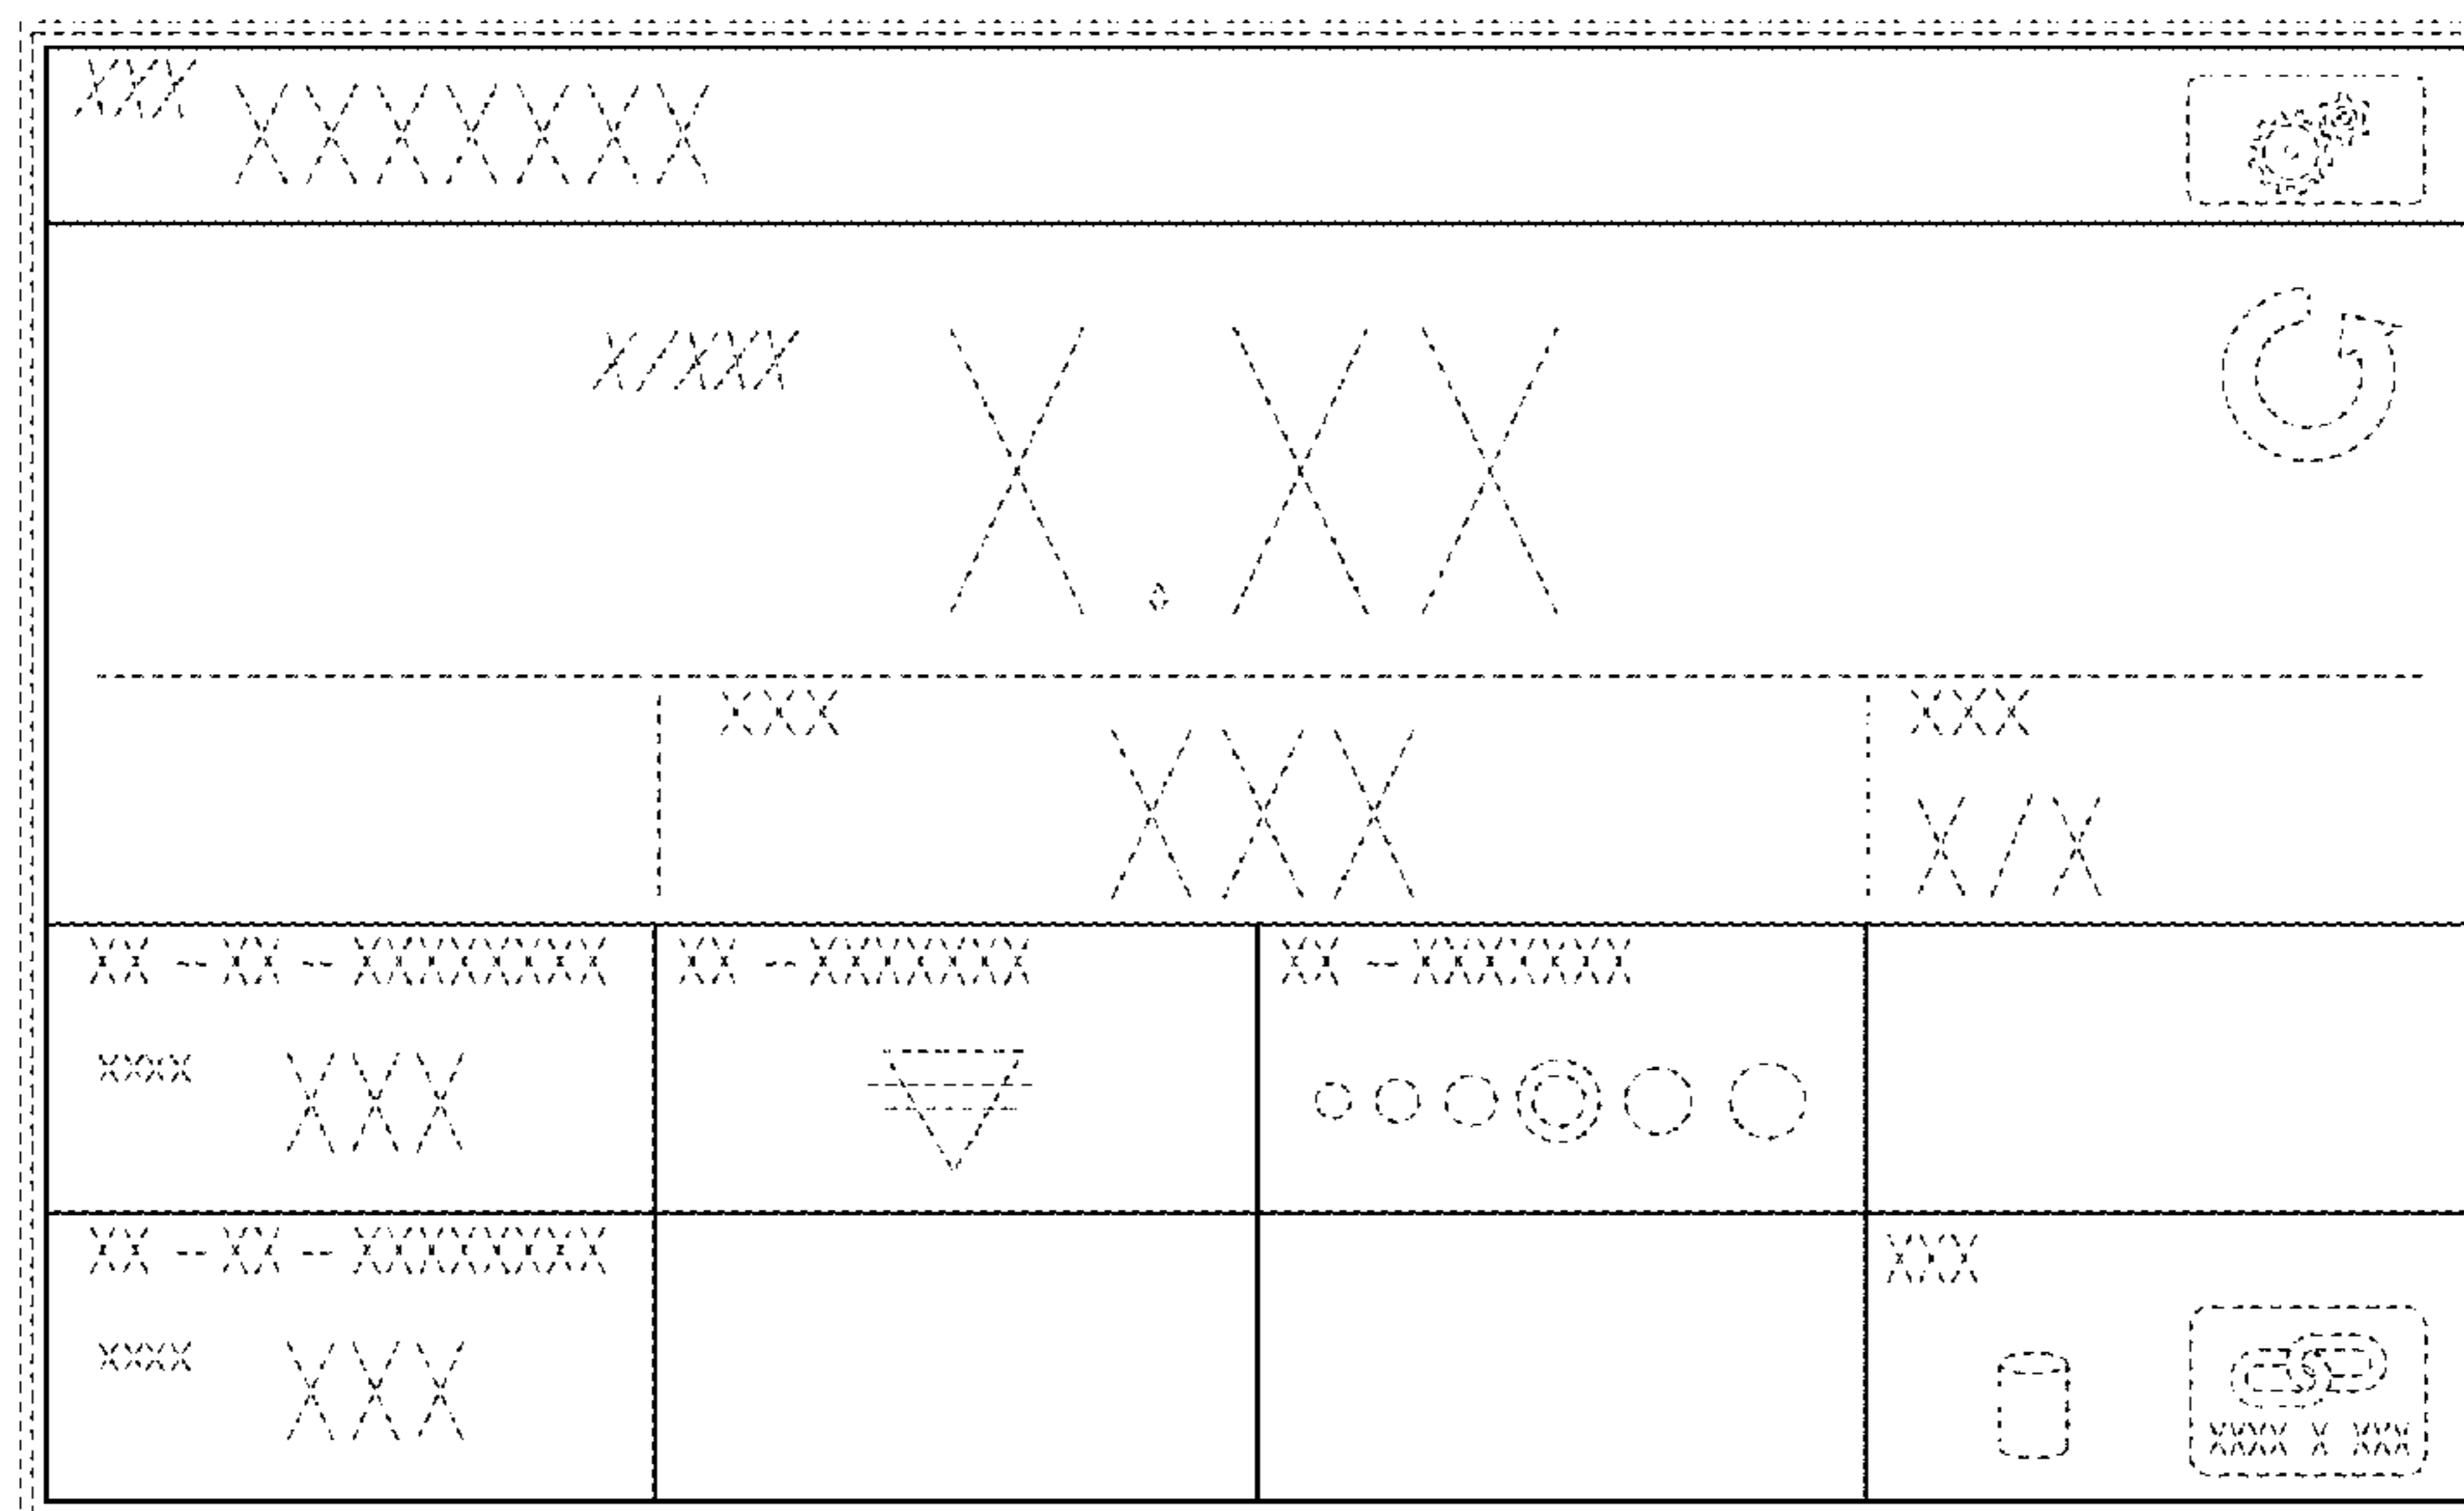

(56)

References Cited

U.S. PATENT DOCUMENTS

D565,627 S	4/2008	Kase	D14/486	D745,026 S	*	12/2015	Bae	D14/486
D570,363 S	6/2008	Ulm et al.		D746,310 S		12/2015	Ta	D14/485
D574,010 S	7/2008	Borovsky et al.		D746,851 S	*	1/2016	Richelson	D14/486
D575,792 S	8/2008	Benson		D750,099 S		2/2016	Seo	D14/485
D586,818 S	* 2/2009	Luck	D14/485	D750,132 S		2/2016	Kim et al.	
D593,117 S	5/2009	Lettau		D751,088 S		3/2016	Seo	D14/485
D594,018 S	6/2009	Ball et al.		D751,100 S	*	3/2016	Linden	D14/486
D611,055 S	3/2010	Jonasson		D752,076 S		3/2016	Guesnon	
D614,191 S	* 4/2010	Takano	D14/486	D752,085 S	*	3/2016	Staiano	D14/487
D626,140 S	10/2010	McLaughlin	D14/486	D753,169 S		4/2016	Kim	D14/486
D629,005 S	12/2010	Jewitt	D14/485	D753,173 S	*	4/2016	Cojuangco	D14/486
D632,698 S	2/2011	Judy et al.		D753,174 S	*	4/2016	Cojuangco	D14/486
D632,699 S	2/2011	Judy et al.		D753,177 S	*	4/2016	Mierau	D14/488
D633,919 S	3/2011	Chen		D753,685 S	*	4/2016	Zimmerman	D14/486
D640,264 S	6/2011	Fujii et al.		D754,143 S		4/2016	Sugimoto	D14/485
D653,672 S	2/2012	Friedlander		D754,161 S		4/2016	Wilder	D14/486
D655,301 S	3/2012	Ray	D14/486	D754,163 S		4/2016	Park	D14/486
D655,710 S	3/2012	Inada	D14/485	D754,172 S		4/2016	Ferreira	D14/486
D656,946 S	4/2012	Judy	D14/486	D754,181 S	*	4/2016	Dong	D14/487
D657,369 S	4/2012	Hecht et al.		D754,679 S	*	4/2016	Gobinski	D14/485
D658,196 S	4/2012	Wood et al.		D754,680 S		4/2016	Lee	D14/485
D660,864 S	5/2012	Anzures et al.		D754,692 S	*	4/2016	Hurst	D14/486
D662,507 S	6/2012	Mori	D14/486	D754,695 S	*	4/2016	Moon	D14/486
D664,152 S	7/2012	Ray	D14/486	D754,700 S	*	4/2016	Lee	D14/486
D665,414 S	8/2012	Lee	D14/488	D754,701 S		4/2016	Seo	D14/486
D667,419 S	9/2012	Rai	D14/486	D754,703 S		4/2016	Moon et al.	
D675,224 S	1/2013	Lee	D14/488	D754,710 S	*	4/2016	Dong	D14/487
D678,895 S	3/2013	Ebler et al.		D755,242 S	*	5/2016	Rajeswaran	D14/495
D681,650 S	* 5/2013	Fletcher	D14/485	D755,821 S		5/2016	Lee	D14/486
D682,288 S	5/2013	Donahue	D14/486	D757,059 S		5/2016	Gray	D14/486
D684,177 S	* 6/2013	Winther	D14/486	D759,100 S		6/2016	Pal et al.	
D685,814 S	* 7/2013	Bork	D14/486	D760,756 S	*	7/2016	Koeten	D14/486
D689,085 S	9/2013	Pasceri et al.		9,389,234 B2	*	7/2016	Von Hoff	G16B 25/00
D691,164 S	* 10/2013	Lim	D14/486	D763,274 S		8/2016	Edwards	D14/485
D698,800 S	* 2/2014	Jung	D14/486	D763,295 S	*	8/2016	Zuckerberg	D14/486
D701,236 S	3/2014	Hatta	D14/486	D764,488 S		8/2016	Bae	D14/485
D701,526 S	* 3/2014	Poston	D14/486	D765,111 S		8/2016	Cole	
D702,247 S	4/2014	d'Amore	D14/485	D765,698 S		9/2016	Kwon	
D703,681 S	4/2014	d'Amore	D14/485	D766,960 S	*	9/2016	Kim	D14/486
D704,206 S	* 5/2014	Jung	D14/486	D768,166 S	*	10/2016	Kim	D14/486
D708,210 S	* 7/2014	Capua	D14/488	D768,174 S	*	10/2016	Kim	D14/486
D709,901 S	7/2014	Landis	D14/486	D768,686 S	*	10/2016	Cho	D14/486
D709,906 S	7/2014	Jonasson		D769,290 S		10/2016	Choi	D14/486
D710,377 S	8/2014	Rydenhag		D769,291 S		10/2016	Kim	D14/486
D712,908 S	9/2014	Rodenhouse	D14/485	D772,887 S		11/2016	Frew	D14/485
D714,336 S	* 9/2014	Cojuangco	D14/486	D773,512 S	*	12/2016	Miura	D14/486
D714,822 S	* 10/2014	Capua	D14/488	D774,077 S	*	12/2016	Donnelly	D14/488
D715,815 S	* 10/2014	Bortman	G06F 3/04817	D776,701 S		1/2017	Huang	D14/486
D716,825 S	* 11/2014	Bachman	D14/486	D780,189 S		2/2017	Yang	D14/485
D721,092 S	* 1/2015	Walkin	D14/488	D781,308 S		3/2017	Austin	D14/485
D722,318 S	2/2015	Moore	D14/486	D782,496 S		3/2017	Contreras et al.	
D722,319 S	2/2015	Moore	D14/486	D783,039 S		4/2017	Park	D14/486
D722,322 S	2/2015	Strayle	D14/486	D786,279 S		5/2017	McKim	
D722,611 S	2/2015	Moore	D14/486	D786,910 S		5/2017	Higuchi	D14/486
D727,342 S	* 4/2015	Omiya	D14/486	D787,543 S		5/2017	Qiu	D14/486
D728,586 S	5/2015	Konno	D14/485	D788,134 S	*	5/2017	Wong	D14/486
D728,601 S	5/2015	Angelides	D14/486	D791,153 S	*	7/2017	Rice	D14/486
D729,267 S	5/2015	Yoo et al.		D791,810 S		7/2017	Hatzikostas	D14/486
D729,837 S	* 5/2015	Kang	D14/487	9,847,044 B1		12/2017	Foster	
9,039,635 B2	5/2015	Burdorff et al.		D810,108 S		2/2018	Tuthill	
D730,929 S	6/2015	Yu et al.		D812,628 S	*	3/2018	Okado	D14/486
D731,507 S	6/2015	Kyakuno	D14/485	D819,042 S		5/2018	Ebler	
D732,549 S	6/2015	Kim	D14/485	D824,941 S	*	8/2018	Cooperman	D14/486
D733,172 S	6/2015	Angelides	D14/486	D829,234 S	*	9/2018	Yuguchi	D14/486
D735,220 S	* 7/2015	Seo	D14/486	D829,736 S		10/2018	Jochetz	
D735,743 S	8/2015	Kanenari	D14/486	D834,050 S	*	11/2018	Yuguchi	D14/486
D737,304 S	8/2015	Urdan	D14/486	D837,820 S	*	1/2019	Itano	D14/486
D737,308 S	* 8/2015	Zuckerberg	D14/486	D839,279 S	*	1/2019	Dudey	D14/485
D739,429 S	* 9/2015	Veilleux	D14/488	D843,387 S	*	3/2019	Yuguchi	D14/485
D740,310 S	10/2015	Drozd et al.		D848,468 S	*	5/2019	Ng	D14/486
D740,311 S	10/2015	Drozd et al.		D851,114 S	*	6/2019	Schulz	D14/486
D742,892 S	11/2015	Mitchell	D14/485	D852,828 S	*	7/2019	Guesnon, Jr.	D14/486
D743,443 S	* 11/2015	Miura	D14/491	D866,578 S	*	11/2019	Ang	D14/486
D745,025 S	* 12/2015	Bae	D14/486	D867,378 S	*	11/2019	Ang	D14/486
				D867,379 S	*	11/2019	Ang	D14/486
				D869,489 S	*	12/2019	Farh	D14/486
				D879,122 S		3/2020	Ebler et al.	
				D886,142 S	*	6/2020	Lynne	D14/486
				2003/0135087 A1		7/2003	Hickle et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0268413 A1* 12/2004 Reid H04N 21/25891
725/131
2005/0044485 A1* 2/2005 Mondry G06Q 10/043
715/247
2005/0229110 A1* 10/2005 Gegner G06F 3/0481
715/800
2006/0053384 A1* 3/2006 La Fetra, Jr. G06F 3/048
715/765
2007/0011702 A1 1/2007 Vaysman H04N 21/84
725/45
2007/0199022 A1* 8/2007 Moshiri H04N 5/44513
725/39
2007/0288868 A1 12/2007 Rhee G06F 3/04817
715/840
2008/0082938 A1* 4/2008 Buczek G06F 40/18
715/784
2012/0005607 A1* 1/2012 Tofinetti G06F 3/0481
715/769
2012/0079429 A1* 3/2012 Stathacopoulos .. H04N 5/44543
715/830
2012/0089914 A1* 4/2012 Holt G06F 3/0485
715/728
2013/0055167 A1* 2/2013 Leong G06F 16/9038
715/854
2013/0127870 A1* 5/2013 Baudel G06F 9/451
345/441
2013/0187780 A1 7/2013 Angelides A61B 5/0002
340/573.1
2014/0127063 A1 5/2014 Petersen et al.
2014/0149942 A1* 5/2014 Wood-Salomon G06F 3/0482
715/840
2014/0192229 A1* 7/2014 Kim G06K 9/00302
348/231.3
2015/0067611 A1* 3/2015 Spohr G06Q 10/10
715/844
2015/0169581 A1* 6/2015 Pusateri G06F 16/35
707/737
2015/0213211 A1* 7/2015 Zaleski G06F 16/9535
715/753
2015/0248534 A1* 9/2015 Krzywicki G06F 3/04847
715/771
2015/0362927 A1 12/2015 Giorgi
2017/0013147 A1* 1/2017 Umezawa G06F 9/451
2017/0102846 A1 4/2017 Ebler et al.
2019/0302981 A1* 10/2019 Storr G06F 3/0486

FOREIGN PATENT DOCUMENTS

JP 1458638 1/2013
JP 1484744 10/2013
JP 1584029 S 7/2017
JP 1585836 S 8/2017

OTHER PUBLICATIONS

“We introduced “Stockert artificial cardiopulmonary device S5” in 2013” in an item “an artificial cardiopulmonary device”, and it is recognized that this “Stockert artificial cardiopulmonary device S5” is same as the above “Stockert S5”, downloaded from <https://web.archive.org/web/20140321232731/www.nho-kumamoto.jp/about/hardwares.html> on Nov. 20, 2018.

Official Action issued in JP Application No. 2017-12102, dated Oct. 30, 2018.
Final Official Action issued in JP Application No. 2018-284, dated Nov. 15, 2018.
Non-Final Office Action—dated Jan. 26, 2018—for U.S. Appl. No. 29/601,895, which corresponds to this pending application.
Product Brochure—CS300 IABP—Product Features—2009 Publication—Maquet Cardiovascular LLC. U.S.A.
Product Brochure—CS100 IABP—Intelligent Counterpulsation—2010 Publication—Maquet Cardiovascular LLC. U.S.A.
Operators Guide—The CS100/CS100i Abbreviated Operator’s Guide—2009 Publication—Maquet Cardiovascular LLC. U.S.A.
Operators Guide—Datascope Abbreviated Operator’s Guide for the System 97 Intra-Aortic Balloon Pump—Published prior to 2009—Datascope Corp. U.S.A.
Brochure—Sensation and CS300 IABP System Smaller Meets Faster—Published in 2009—Maquet Cardiovascular LLC. U.S.A.
Brochure—CS300 IABP Product Features—Published in 2009—Maquet Cardiovascular LLC. U.S.A.
Sorin | S5 Brochure, Sorin Group USA, Inc., 2010.
MetaVision Perfusion™, a point-of-care clinical information system for perfusionists, Maquet Getinge Group 2015 <<http://www.maquet.com/int/products/metavision-perfusion/>>.
Heart-Lung Machine HL20 Brochure, Maquet Cardiopulmonary AG 2012.
“Heart Lung Machine Fundraising.” Aug. 18, 2015. Web. Nov. 6, 2015. <<http://www.heartcentreforchildren.com.au/heart-lung-machine-fundraising.html>>.
Heart-lung machines. surgeryencyclopedia.com. Advameg, Inc. 2015. Web. Nov. 5, 2015. <<http://www.surgeryencyclopedia.com/Fi-La/Heart-Lung-Machines.html>>.
Machine coeur-poumon HL30. Feb. 21, 2013. Web. Nov. 18, 2015. <<file:///C:/Users/u2002449/Downloads/mes-130225-MachineCoeurPoumonHL30-Maquet.pdf>>.
Terumo Advanced Perfusion System 1. Terumo Cardiovascular Group. Nov. 2014. Web. Nov. 18, 2015. <http://www.terumo-cvs.com/doc/848594_Terumo-System1_Brochure%20_Nov2013_LowRes_Pgs.pdf>.
Product Catalog Jostra HL 20. Maquet Cardiopulmonary AG. Web. Nov. 18, 2015. <http://glavm.ru/upload/information_system_18/2/8/7/item_287/information_items_property_343_pdf>.
Sorin | S5 System Operating Instructions, Sorin Group Deutschland GmbH, 2006, 2007.
Hessel, Eugene A., “Circuitry and Cannulation Techniques”, Chapter 5, *Cardiopulmonary Bypass: Principles and Practices*, edited by Glenn P. Gravlee, 3rd edition, 2008, pp. 63-65.
Sorin article, <http://www.sorin.com/products/cardiac-surgery/perfusion/hlm/s5>, printed on Jun. 13, 2015, 11 pages.
Non-Final Office Action dated Dec. 14, 2018 issued for related U.S. Appl. No. 29/646,368, 7 pages.
Japanese Office Action dated Feb. 22, 2019 during the prosecution of Japanese Design Patent Application No. 2018-000284, 5 pages.
Japanese Decision on Appeal dated Mar. 6, 2019 during the prosecution of Japanese Design Patent Application No. 2017-012102, 59 pages.
EP Office Action dated May 8, 2019 during the prosecution of EP Patent Application No. 16722661.2, 6 pages.

* cited by examiner

