



US00D907214S

(12) **United States Design Patent**
Wu et al.

(10) **Patent No.:** **US D907,214 S**
(45) **Date of Patent:** **** Jan. 5, 2021**

(54) **ECG MEASUREMENT AND DATA
COLLECTION CUSHION PAD COVER**

D643,309 S * 8/2011 Birchmeier D9/425
D733,915 S * 7/2015 Stuyfzand D24/231
D818,129 S * 5/2018 Heine D24/165

(71) Applicant: **Shenzhen Novocare Medical Devices
Co., Inc, Shenzhen (CN)**

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Zhengyu Wu, Shenzhen (CN);
Xuefang Yang, Shenzhen (CN)**

JP D2008-29270 * 11/2018

* cited by examiner

(73) Assignee: **SHENZHEN NOVOCARE
MEDICAL DEVICES CO., INC,
Shenzhen (CN)**

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Treasure IP Group, LLC

(**) Term: **15 Years**

(57) **CLAIM**

(21) Appl. No.: **29/622,340**

The ornamental design for an ECG measurement and data collection cushion pad cover, as shown and described.

(22) Filed: **Oct. 17, 2017**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/187**

(58) **Field of Classification Search**

USPC D24/107, 165–168, 186, 187, 189, 200,
D24/231; D10/70, 75, 98

CPC A61B 5/02411; A61B 5/02427; A61B
5/02438; A61B 5/002; A61B 5/04325

See application file for complete search history.

DESCRIPTION

FIG. 1 is a perspective view of an ECG measurement and data collection cushion pad cover showing our new design; FIG. 2 is a front view thereof, wherein in this elevation view, the straps of the cushion pad are hanging; FIG. 3 is a rear view thereof, wherein in this elevation view, the straps of the cushion pad are hanging; FIG. 4 is a left side view thereof, wherein in this elevation view, the straps of the cushion pad are hanging; FIG. 5 is a right side view thereof, wherein in this elevation view, the straps of the cushion pad are hanging; FIG. 6 is a top view thereof; FIG. 7 is a bottom view thereof showing the straps of the cushion laid flat on the bottom surface; and, FIG. 8 is a bottom view thereof showing the straps of the cushion hanging.


The broken lines depict portions of the ECG measurement and data collection cushion pad cover that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D258,155 S * 2/1981 Mathews 8/160
D264,755 S * 6/1982 Olson D24/189
4,524,087 A * 6/1985 Engel A61B 5/04087
252/519.33
D297,460 S * 8/1988 Inoue D24/168
D297,461 S * 8/1988 Inoue D24/168
5,566,672 A * 10/1996 Faasse, Jr. A61B 5/0408
600/372
D492,248 S * 6/2004 Gregory D13/103
D499,488 S * 12/2004 Chastain D24/187

1 Claim, 8 Drawing Sheets

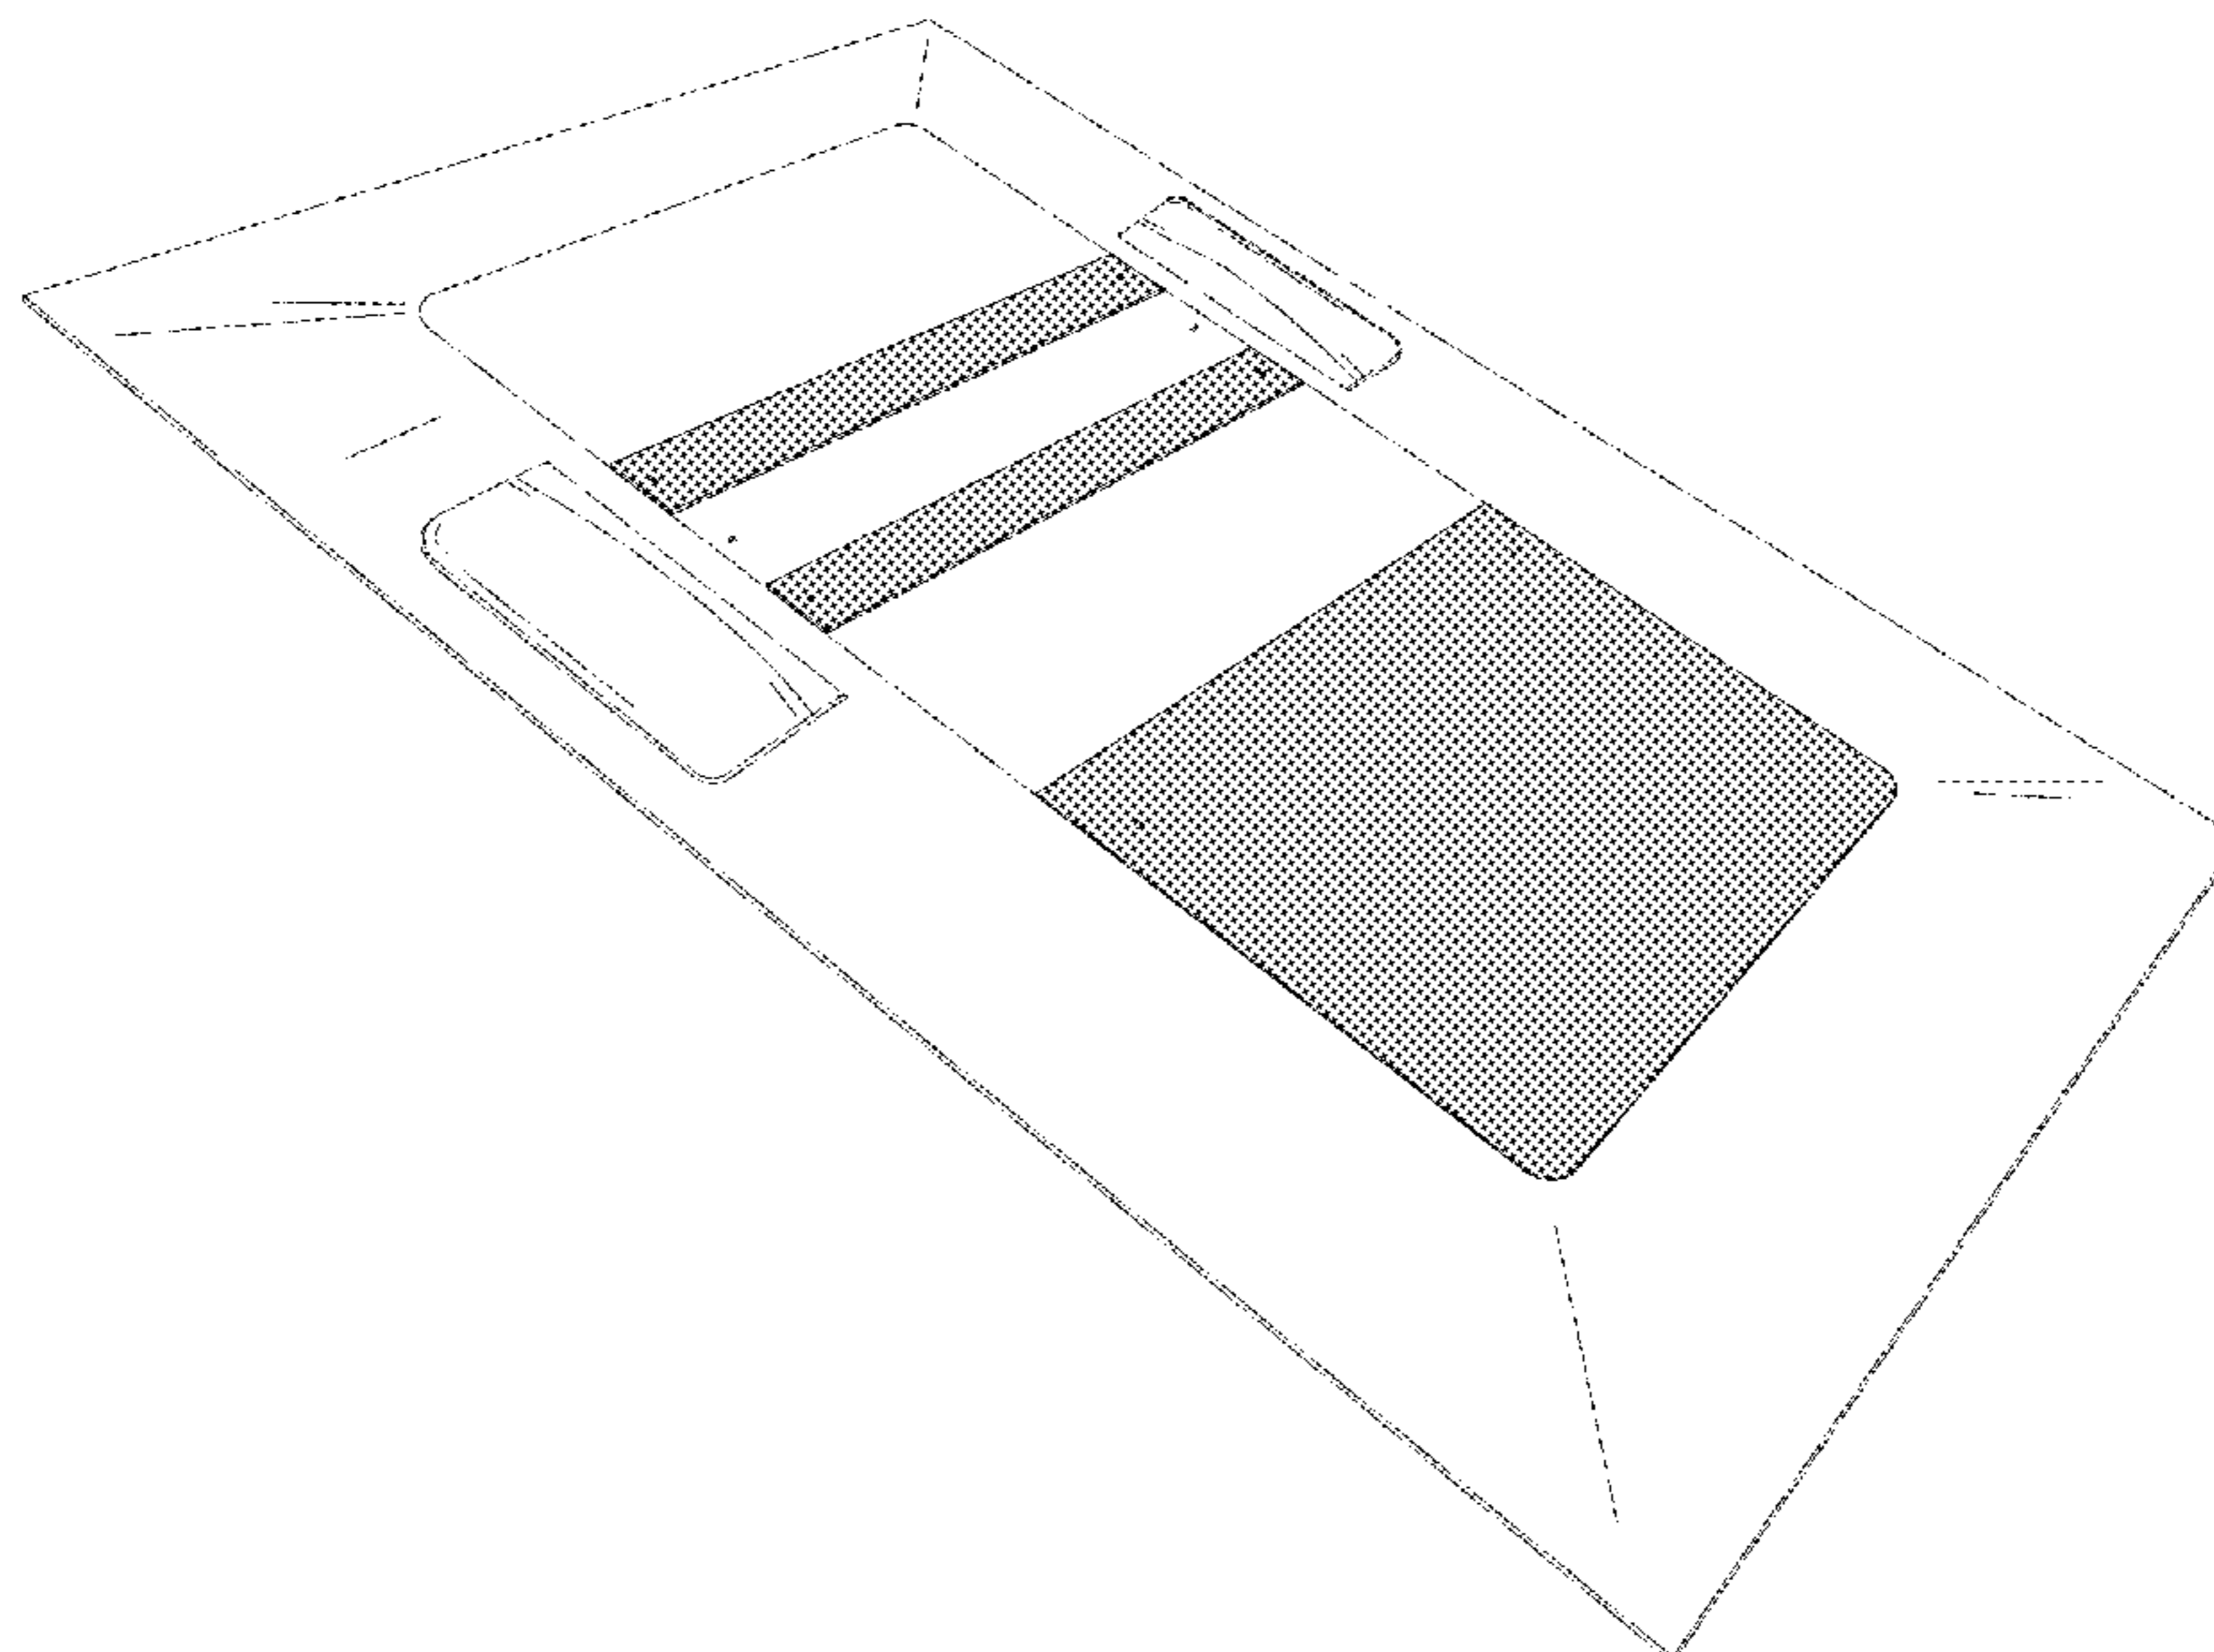

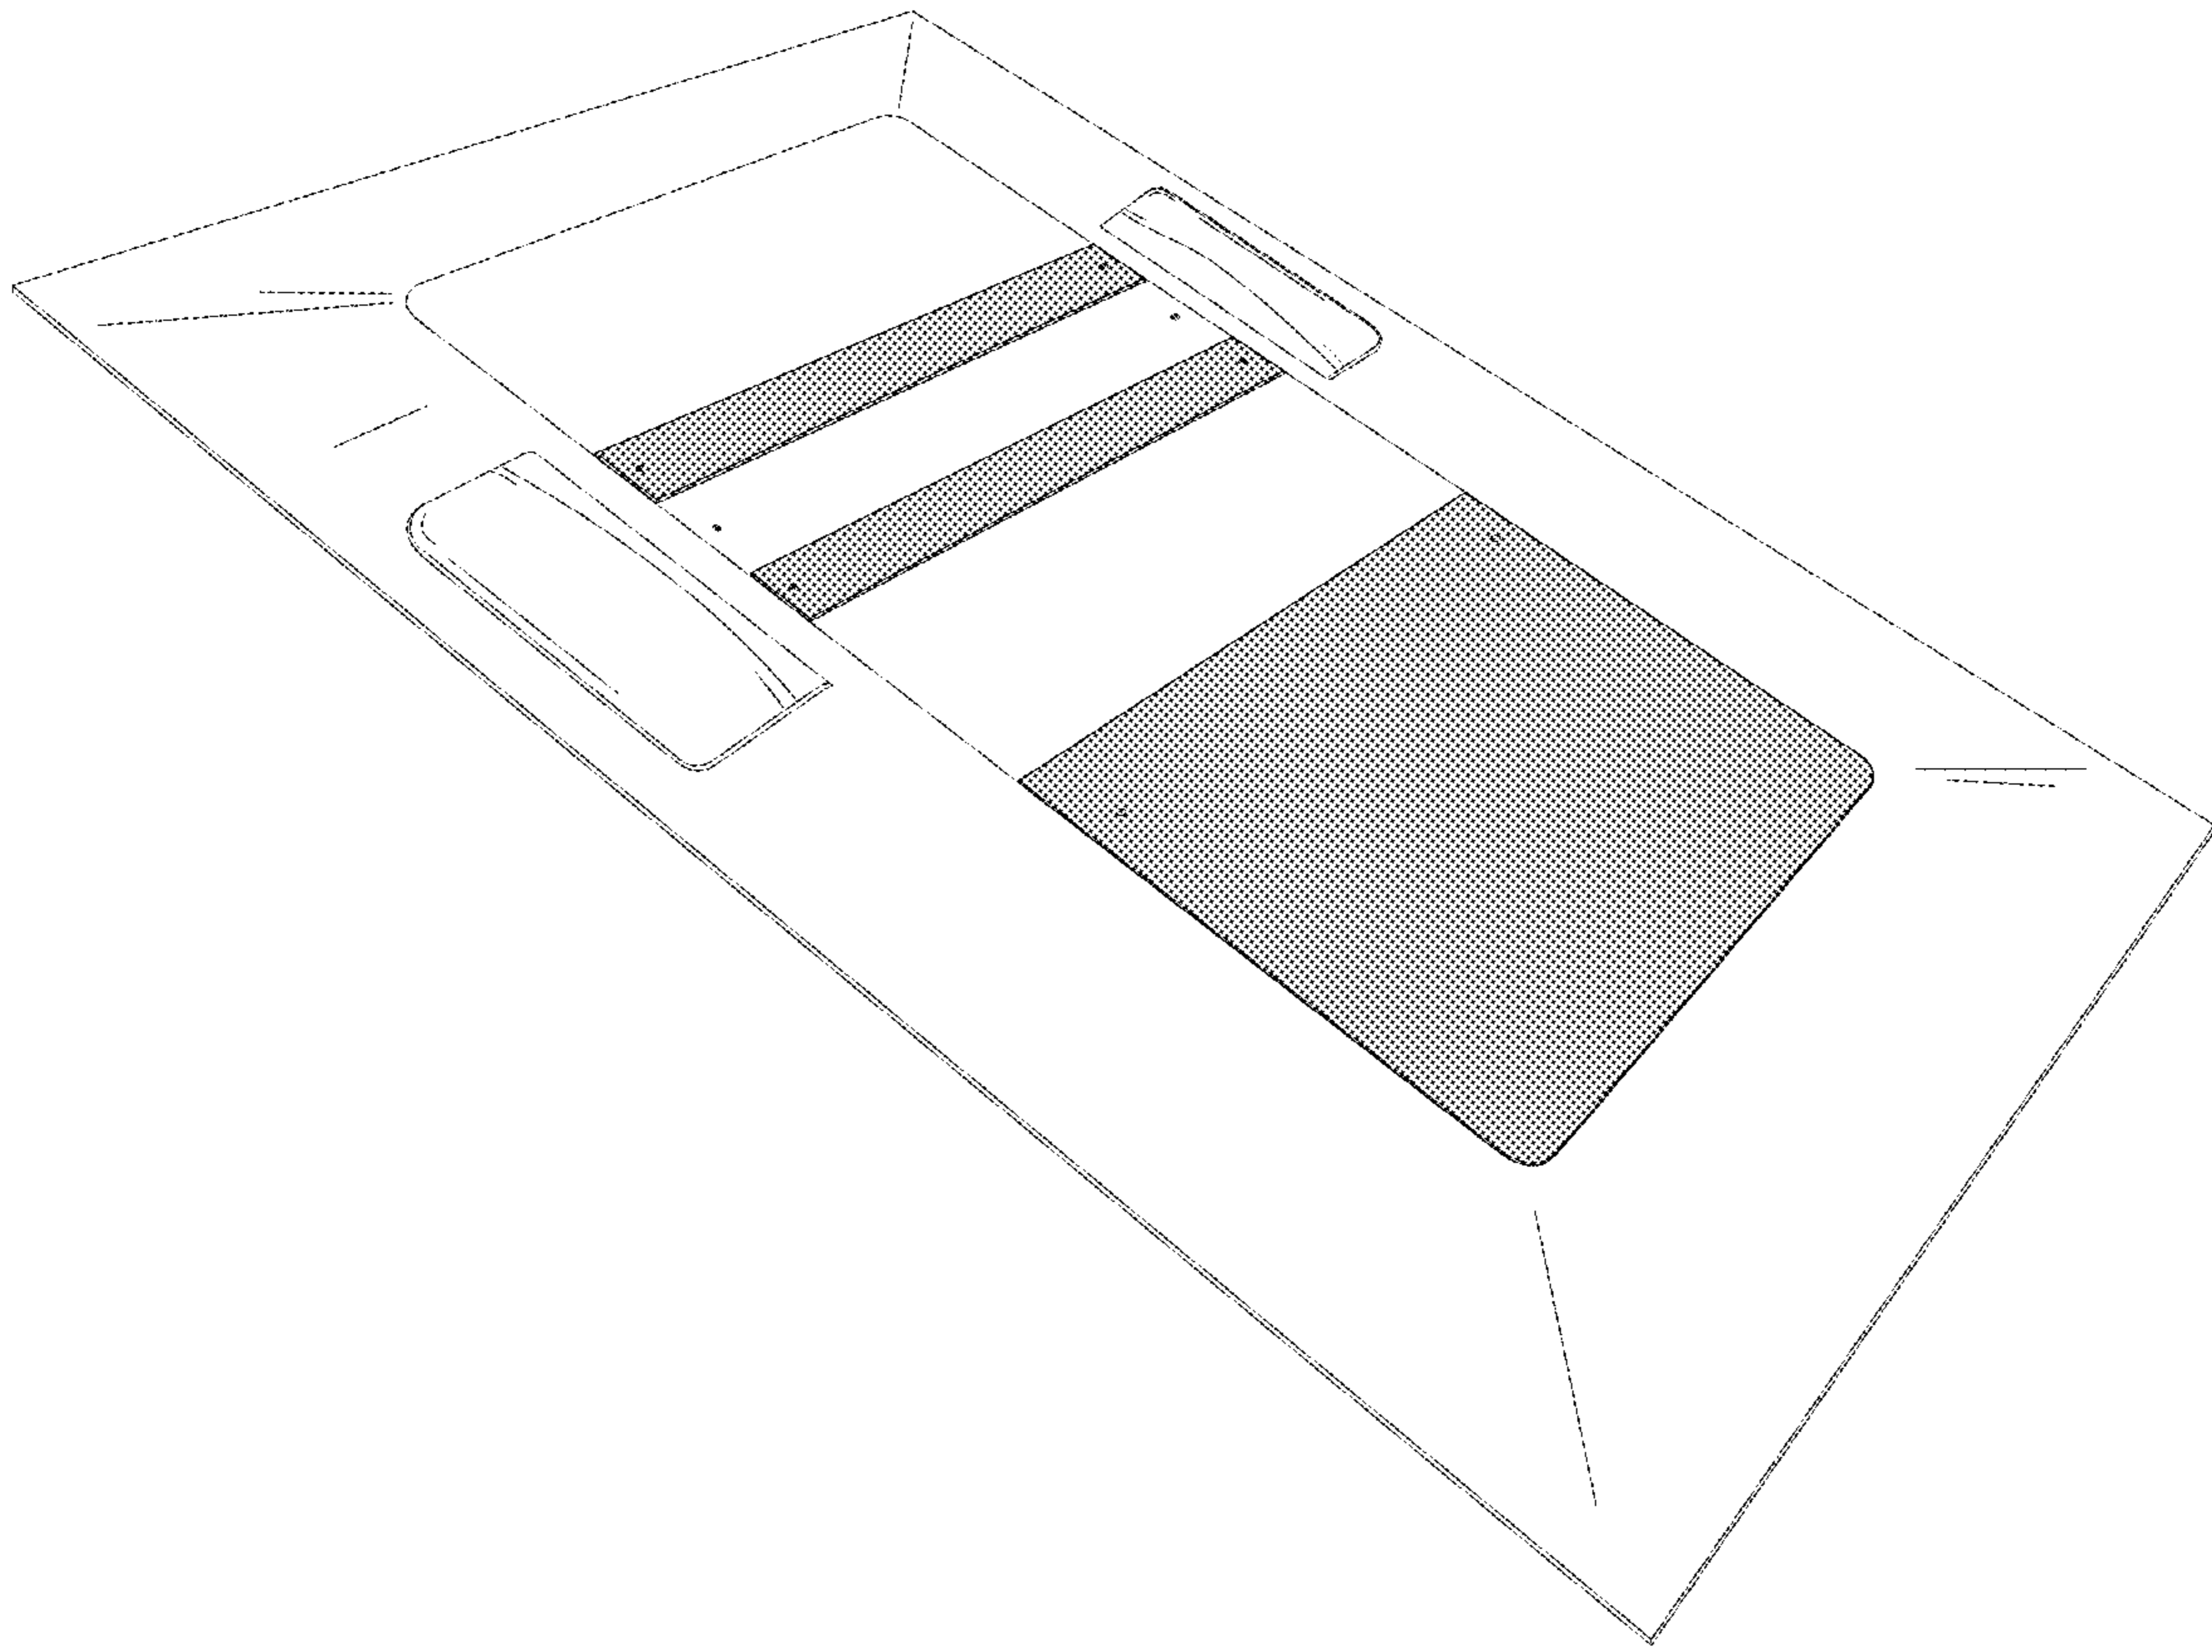


FIG. 1

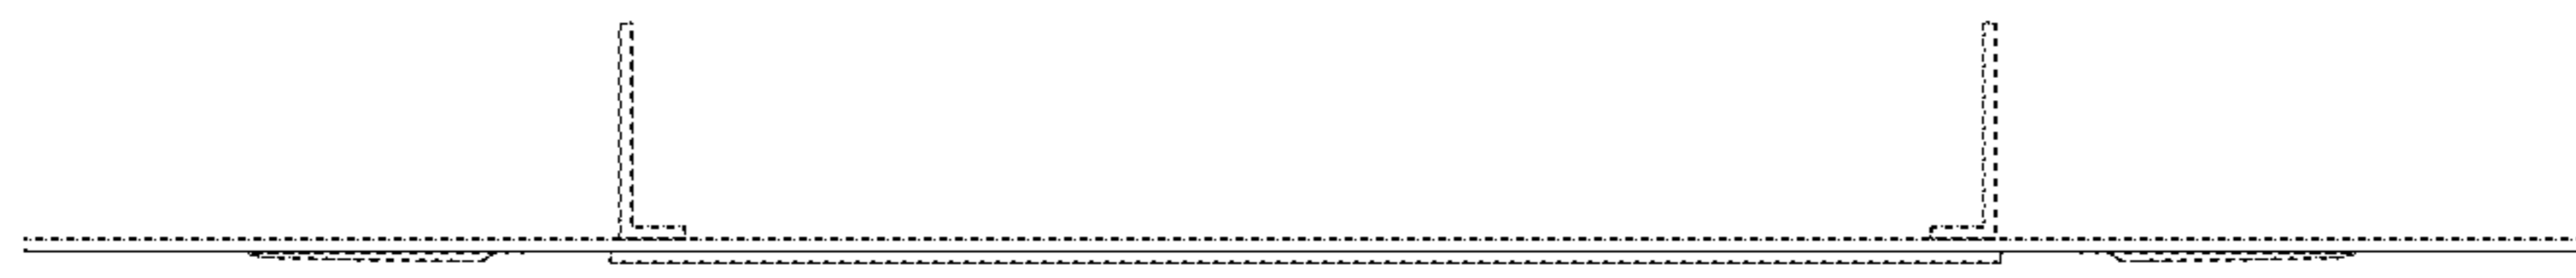


FIG.2

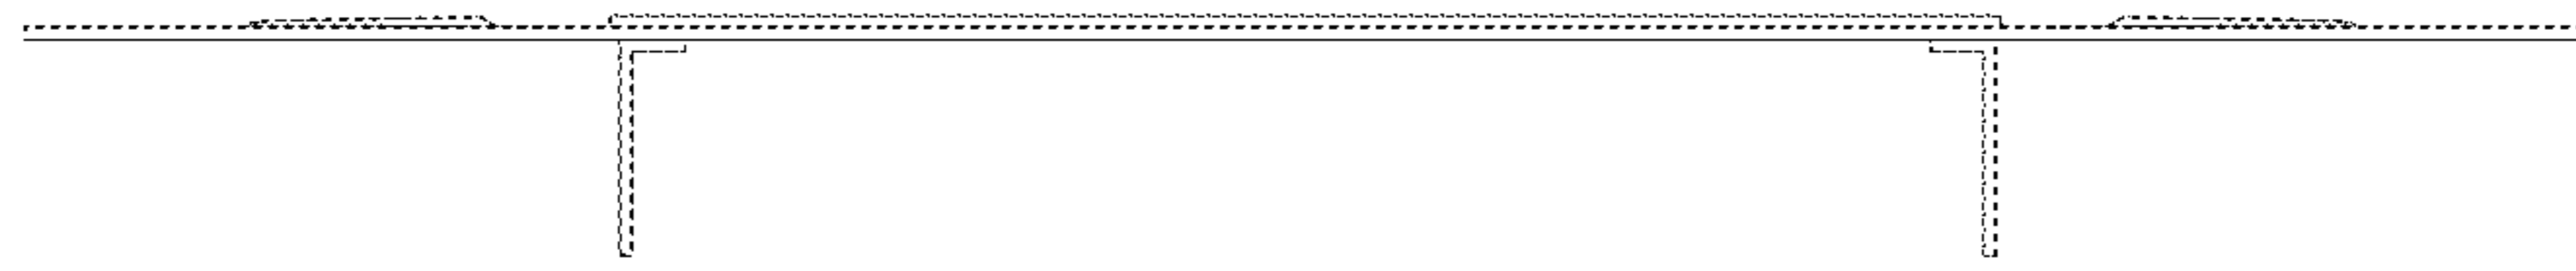


FIG.3

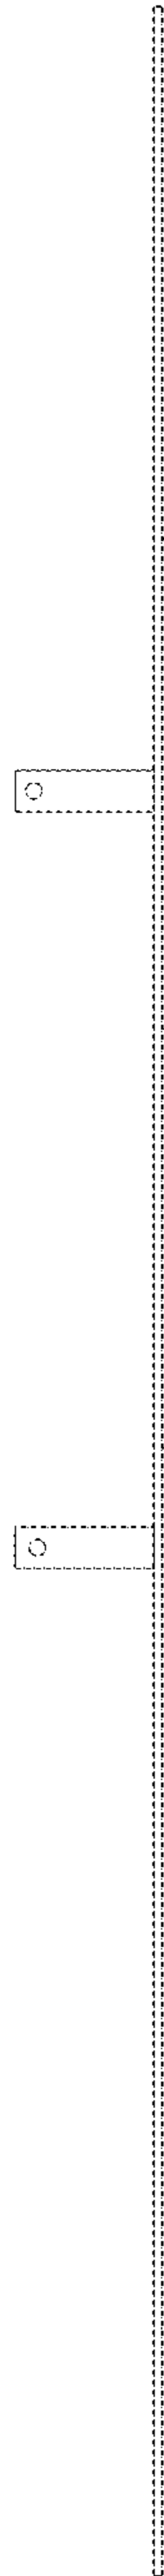


FIG.4

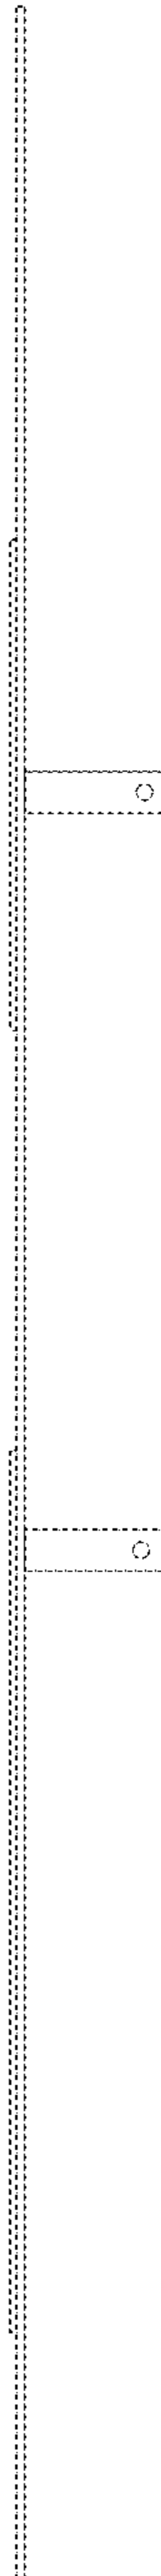


FIG.5

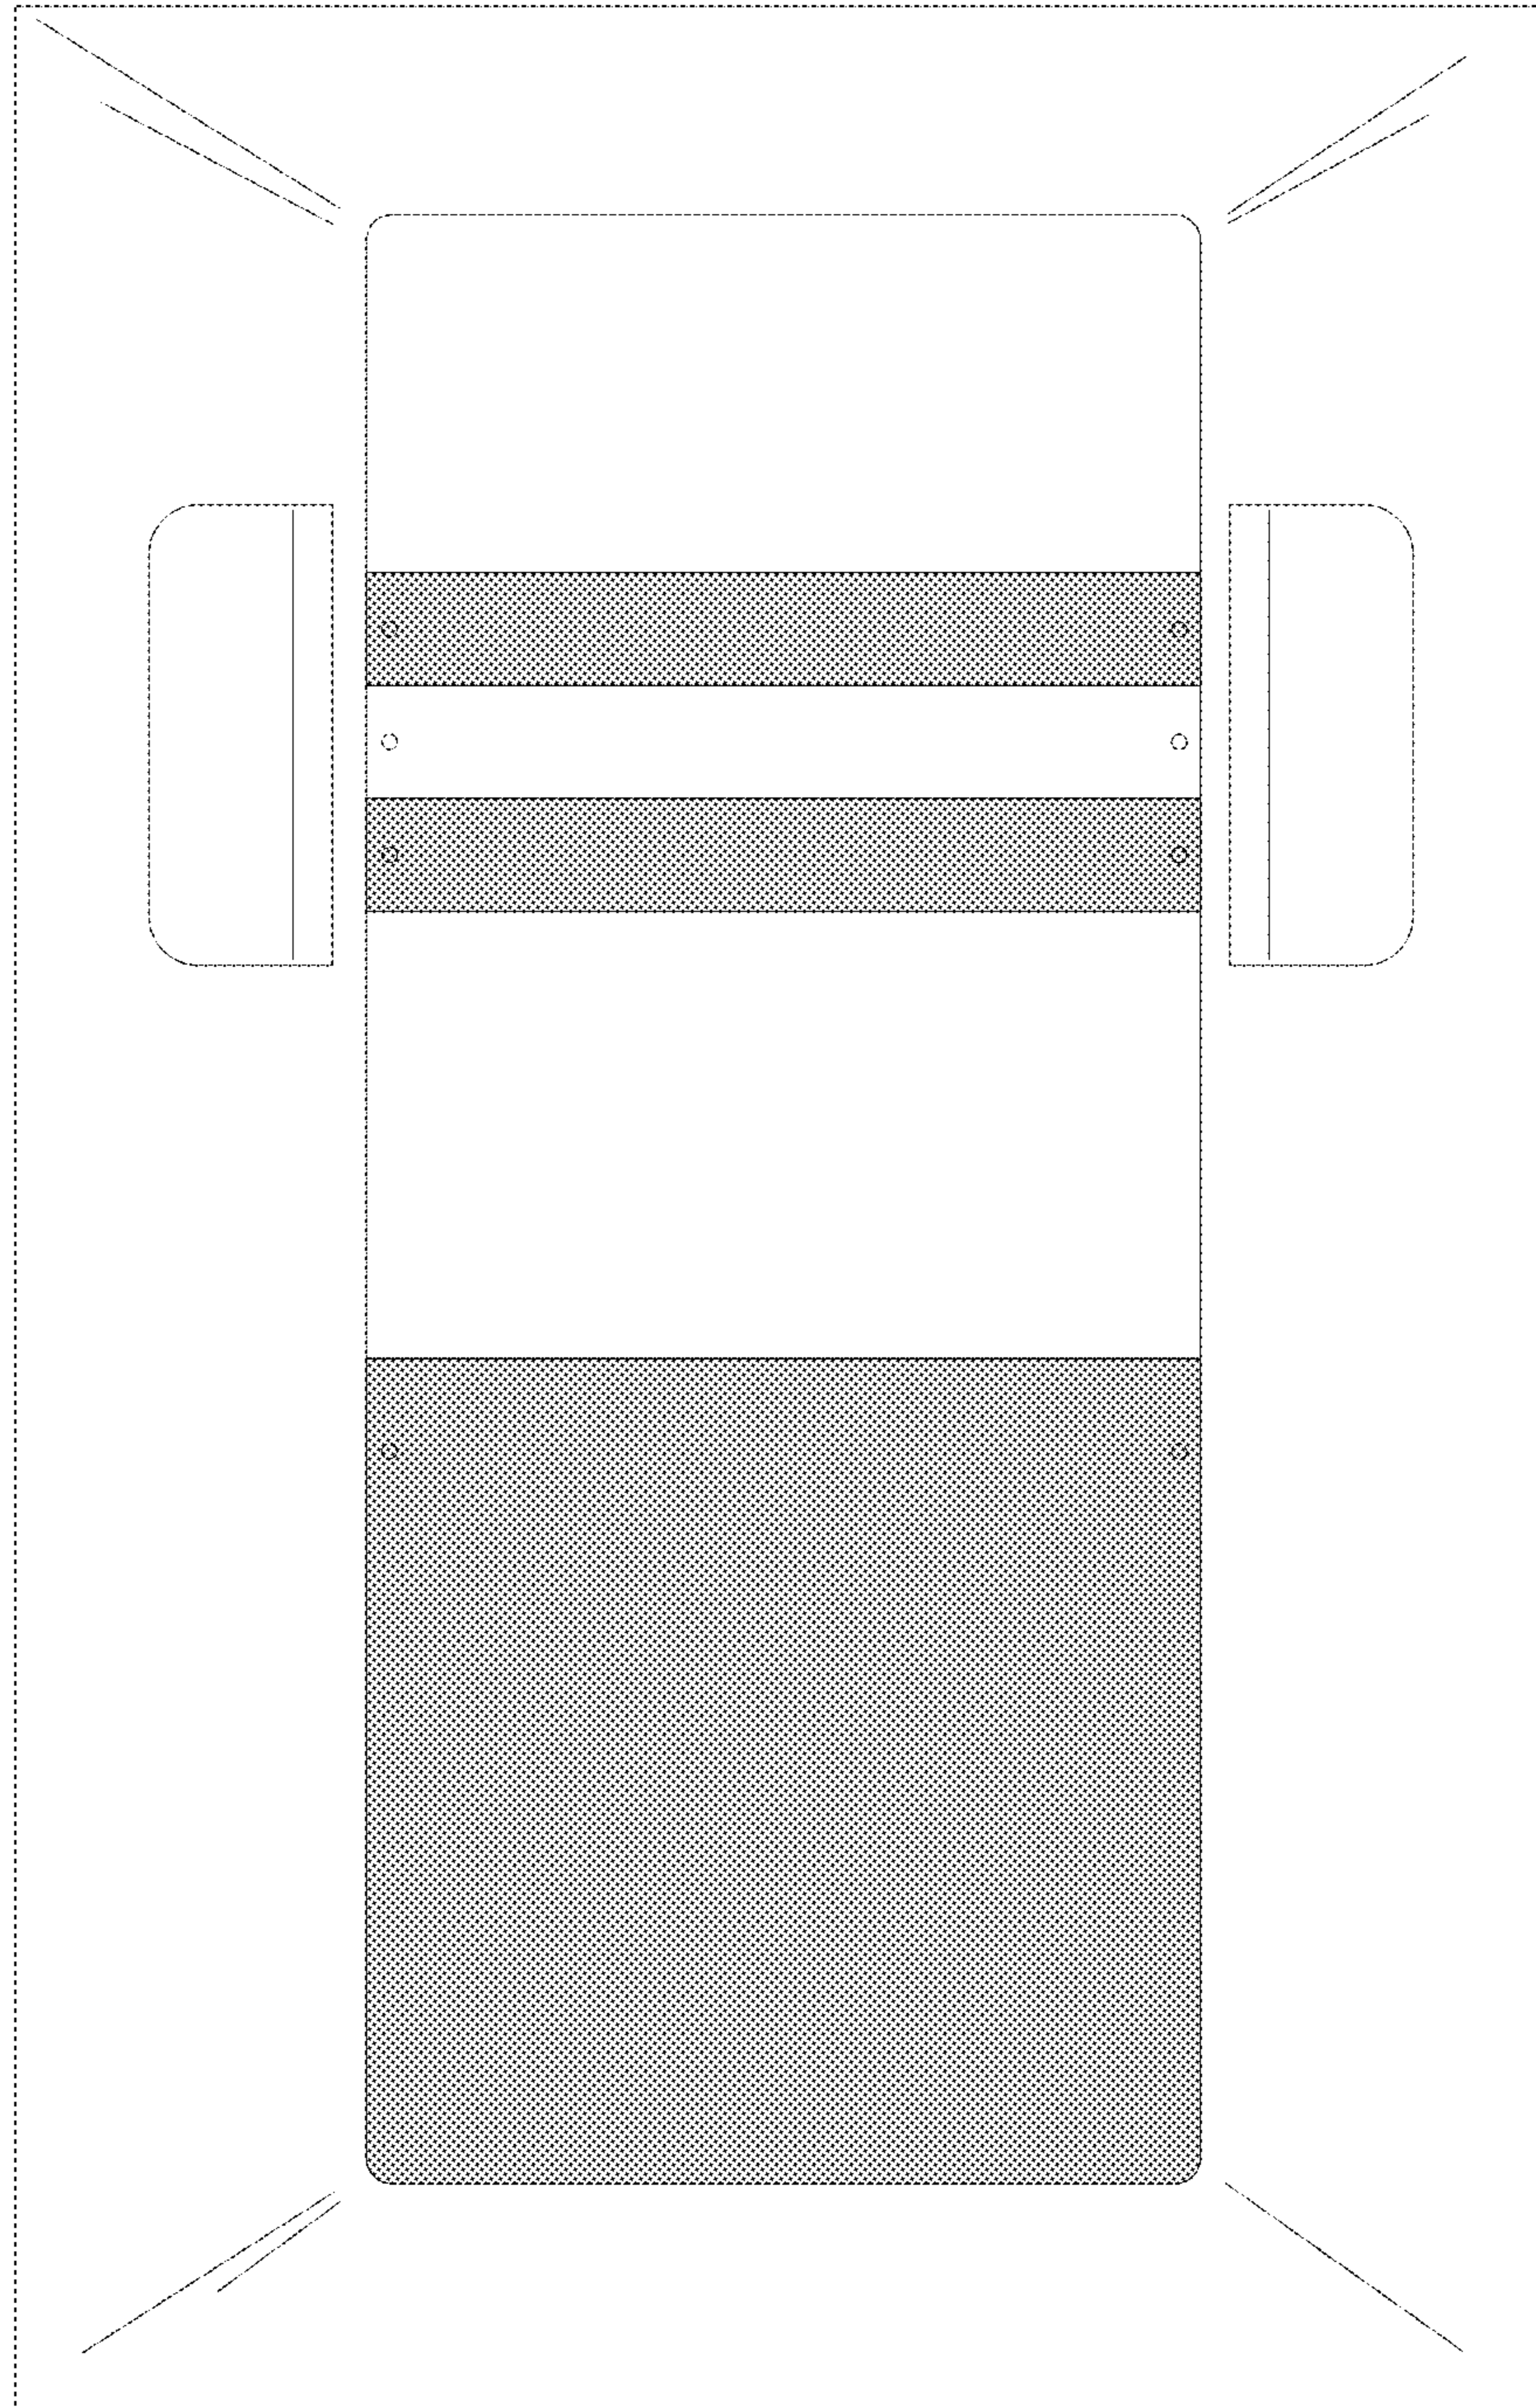


FIG. 6

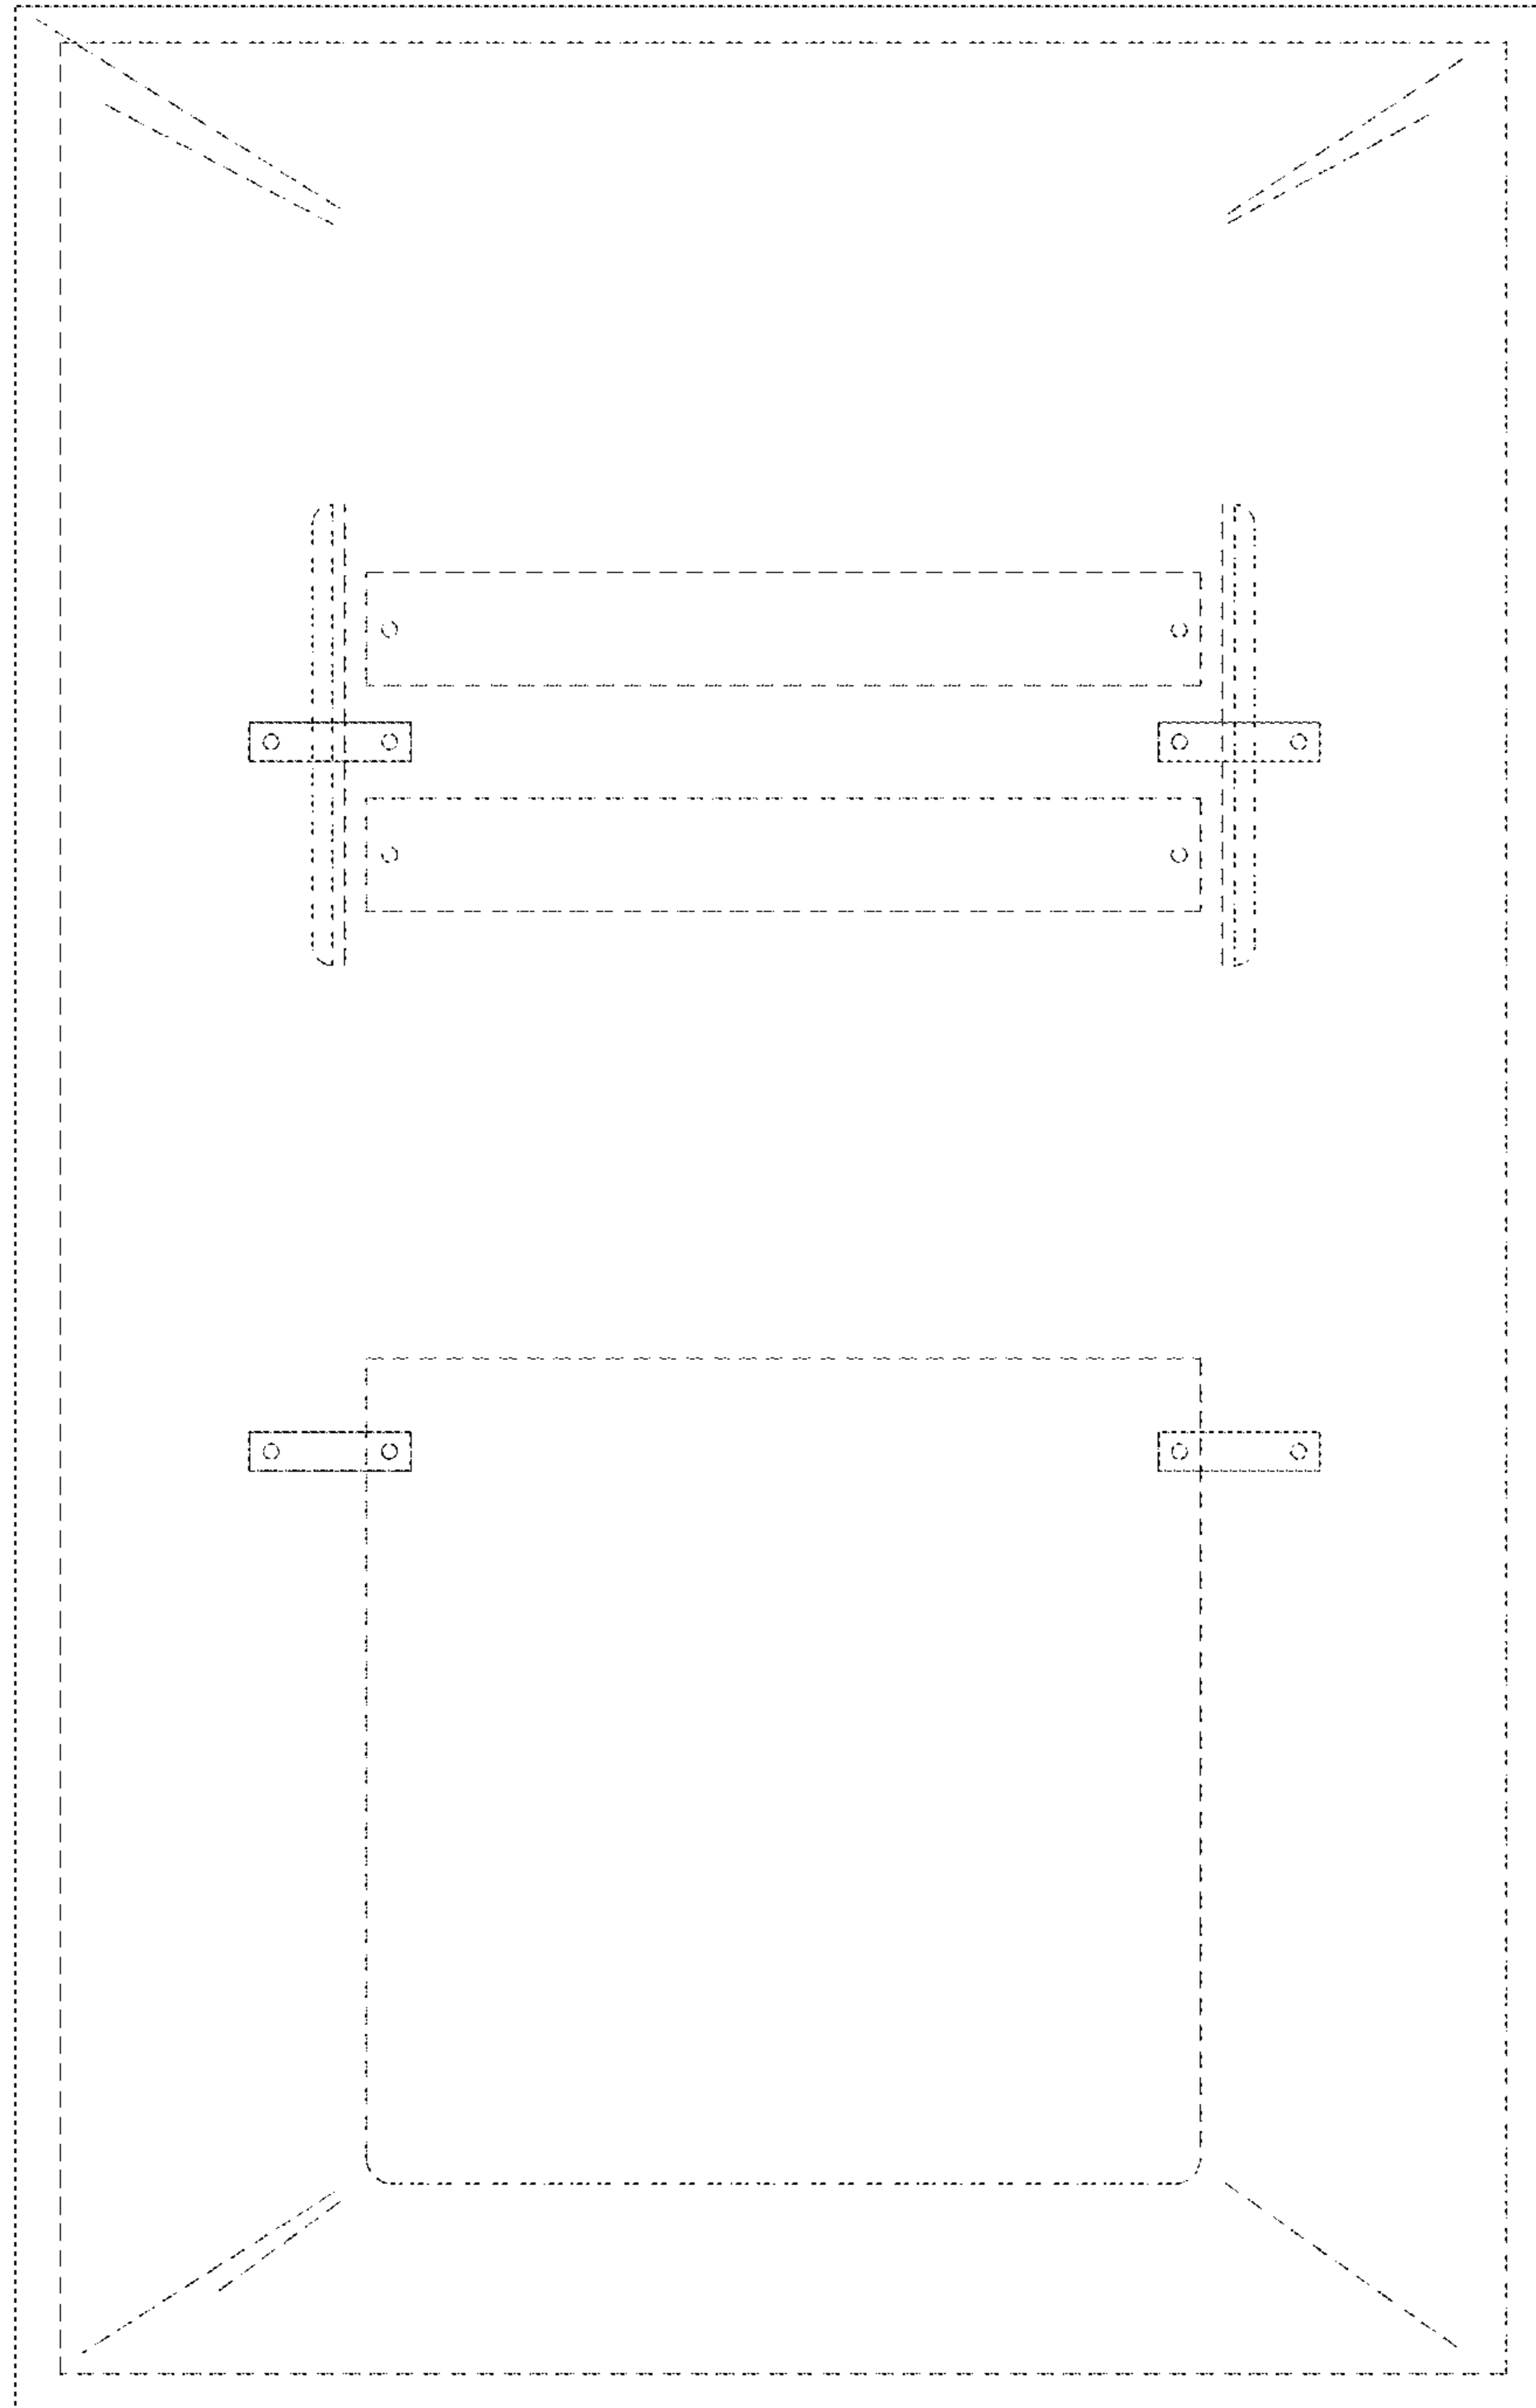


FIG.7

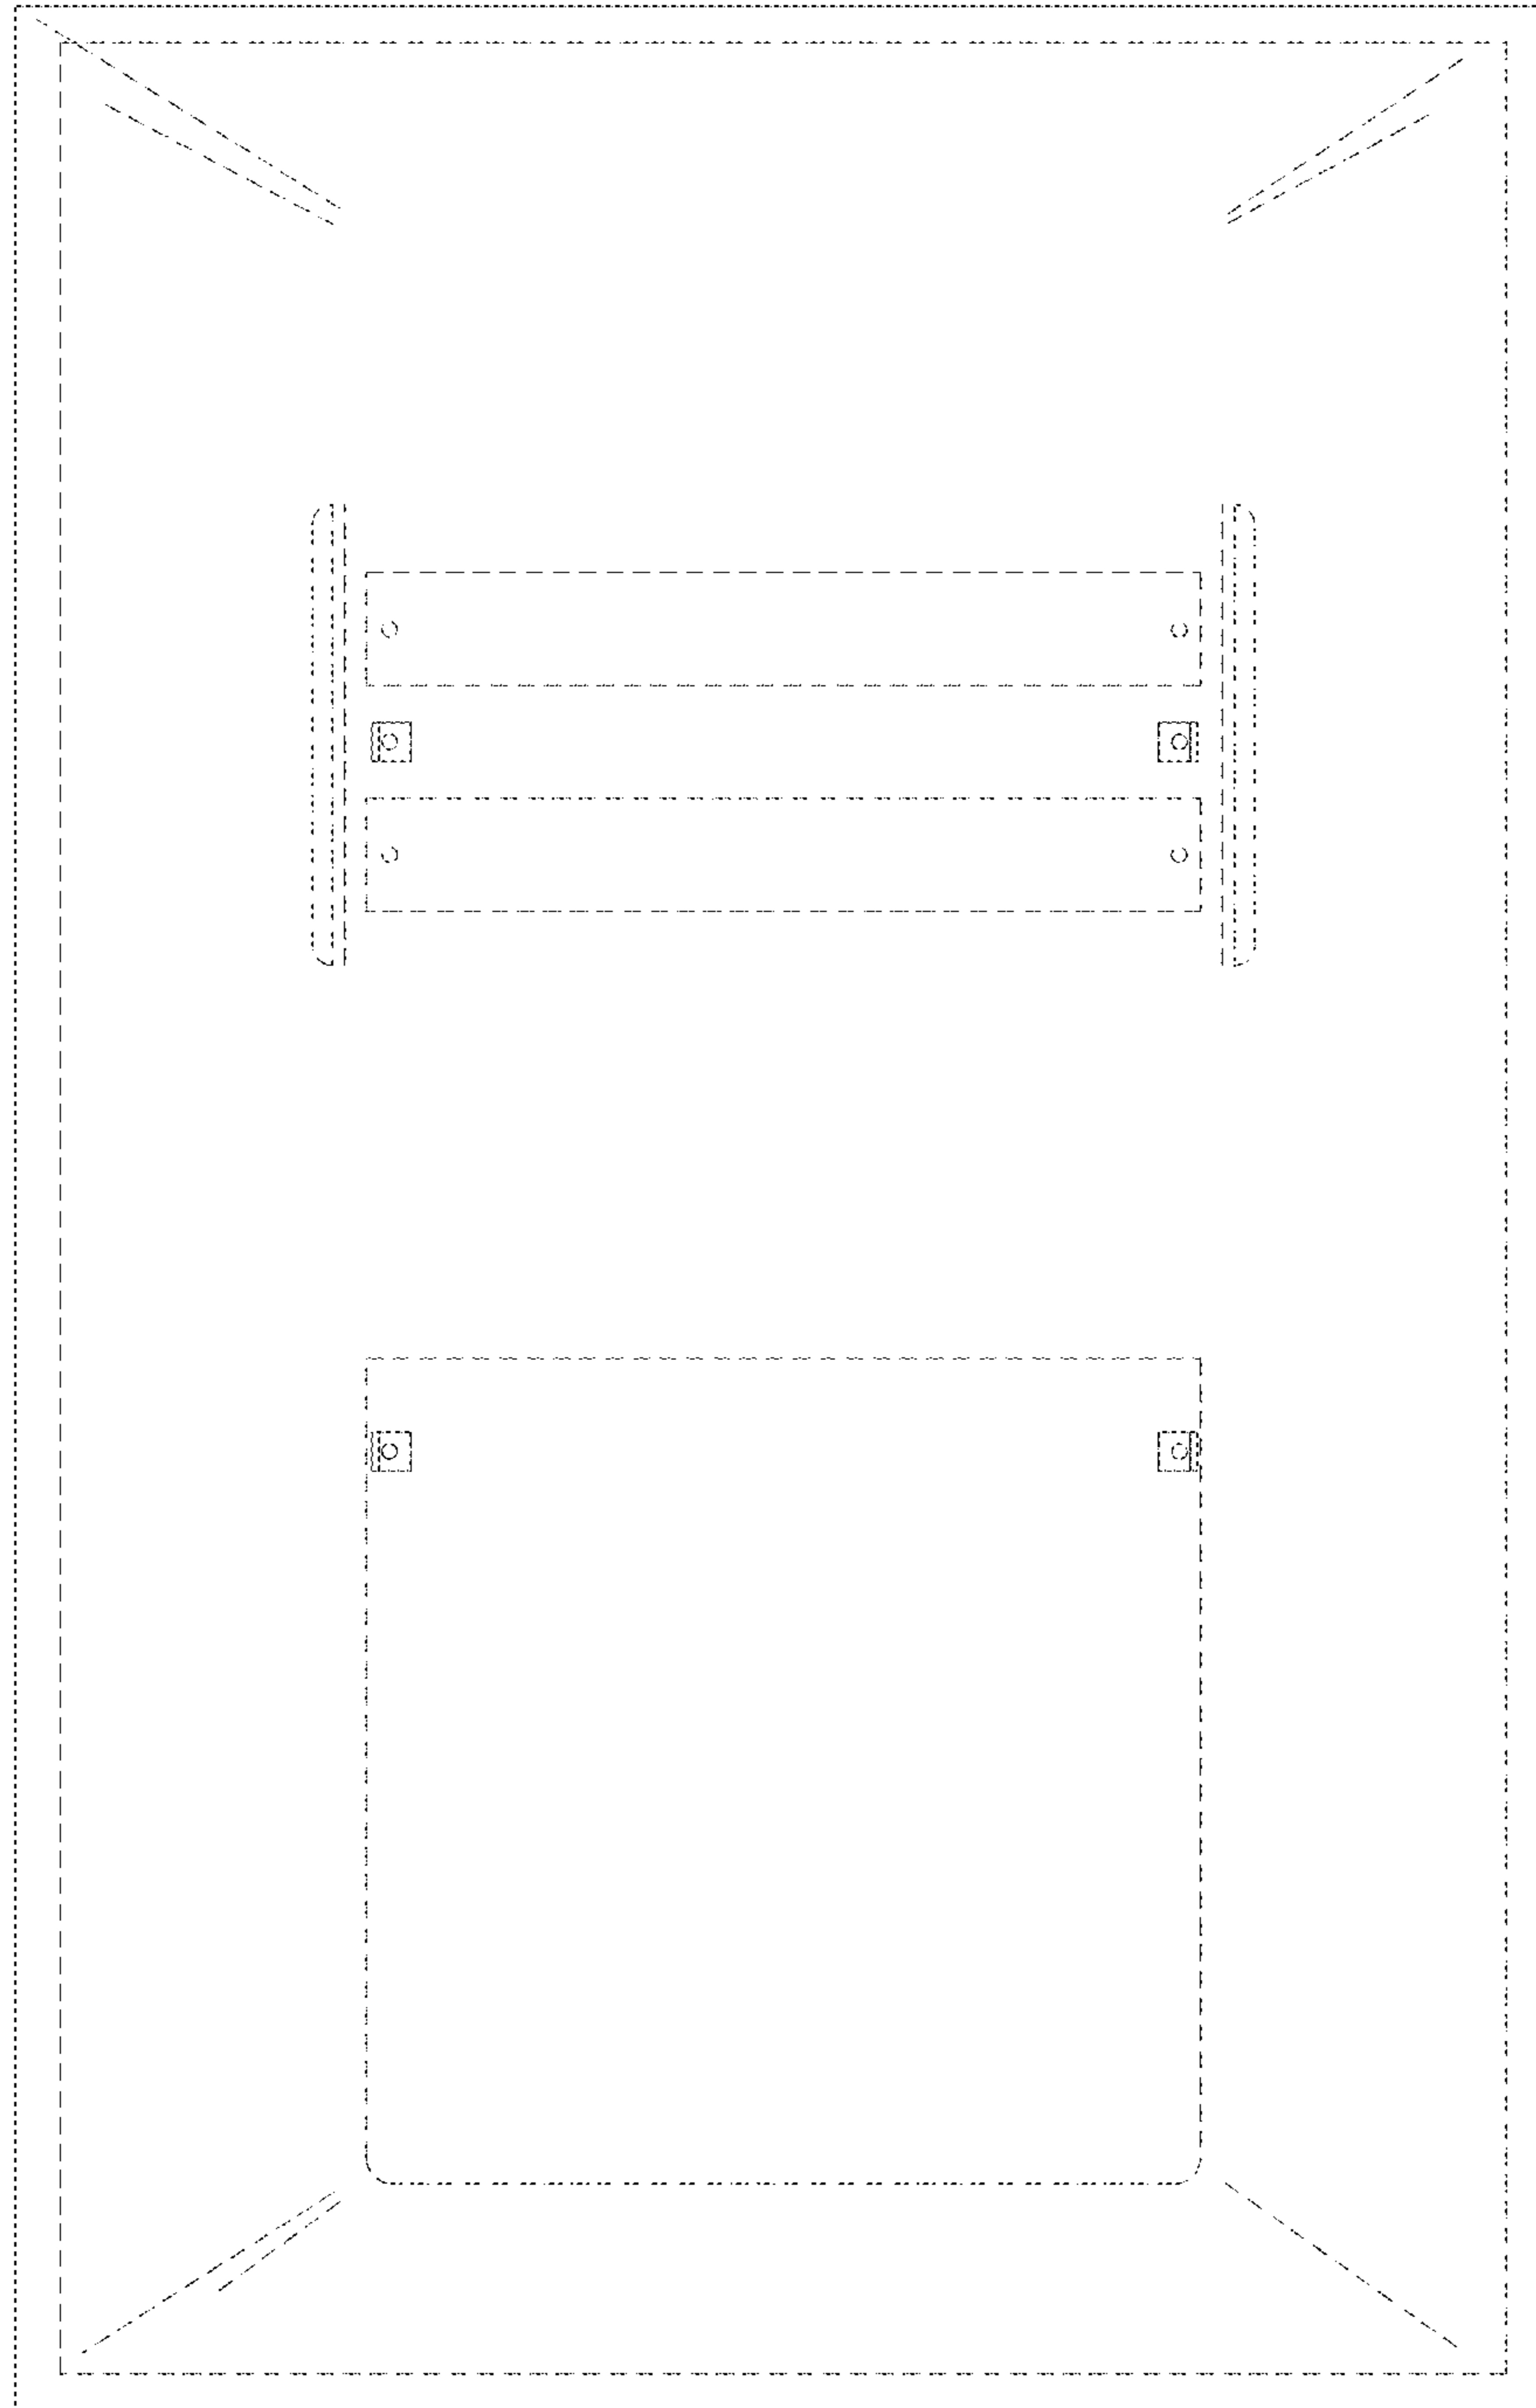


FIG.8