



US00D907234S

(12) **United States Design Patent** (10) **Patent No.:** **US D907,234 S**
Rosin et al. (45) **Date of Patent:** **** Jan. 5, 2021**

(54) **SUPPORT ASSEMBLY FOR MEDICAL INSTRUMENTS**

(71) Applicant: **Aesculap AG**, Tuttlingen (DE)

(72) Inventors: **Bianca Rosin**, Tuttlingen (DE);
Mariana Jakob, Tuttlingen (DE)

(73) Assignee: **Aesculap AG**, Tuttlingen (DE)

(**) Term: **15 Years**

(21) Appl. No.: **35/507,783**

(22) Filed: **Apr. 18, 2019**

(80) **Hague Agreement Data**

Int. Filing Date: **Apr. 18, 2019**

Int. Reg. No.: **DM/203910**

Int. Reg. Date: **Apr. 18, 2019**

Int. Reg. Pub. Date: **Nov. 15, 2019**

(30) **Foreign Application Priority Data**

Nov. 9, 2018 (EM) 005821717

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/217**

(58) **Field of Classification Search**

USPC D24/107, 108, 186, 200, 209–213, 217,
D24/218, 219, 224–232; D9/456;
D14/217; D12/167, 172; D34/19, 38

CPC .. A61L 2202/24; A61L 2/26; A61L 2202/182;
A61L 2202/10; A61B 50/33; A61B
2090/701; A61B 1/00144; A61B 1/121;
A61B 2050/005; A61B 2050/007; A61B
50/00; A61B 50/20

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D374,936 S *	10/1996	Jakab	D24/217
6,331,280 B1 *	12/2001	Wood	A61L 2/26 206/268
D458,448 S *	6/2002	Jakab	D24/217
D531,734 S *	11/2006	Haunschild	D24/217
D557,814 S *	12/2007	Glenn	D24/217
D668,348 S *	10/2012	Murphy	D24/217
D721,441 S *	1/2015	Tipton	D24/217
D867,610 S *	11/2019	Ohata	D24/217
D873,408 S *	1/2020	Li	D24/108
D877,927 S *	3/2020	Nathan	D24/217
D878,620 S *	3/2020	Nathan	D24/217

* cited by examiner

Primary Examiner — Samantha Q Lawrence

(57) **CLAIM**

The ornamental design for a support assembly for medical instruments, as shown and described.

DESCRIPTION

Fig. 1.1 is a perspective view of a support assembly for medical instruments;

Fig. 1.2 is a front view thereof;

Fig. 1.3 is a rear view thereof;

Fig. 1.4 is a left side view thereof;


Fig. 1.5 is a right side view thereof;


Fig. 1.6 is a top view thereof; and

Fig. 1.7 is a bottom view thereof.

The broken lines shown in Figures 1.1-1.3 and Figures 1.6-1.7 illustrate portions of the bearing system for sterilization tray for medical instruments and form no part of the claimed design.


1 Claim, 7 Drawing Sheets

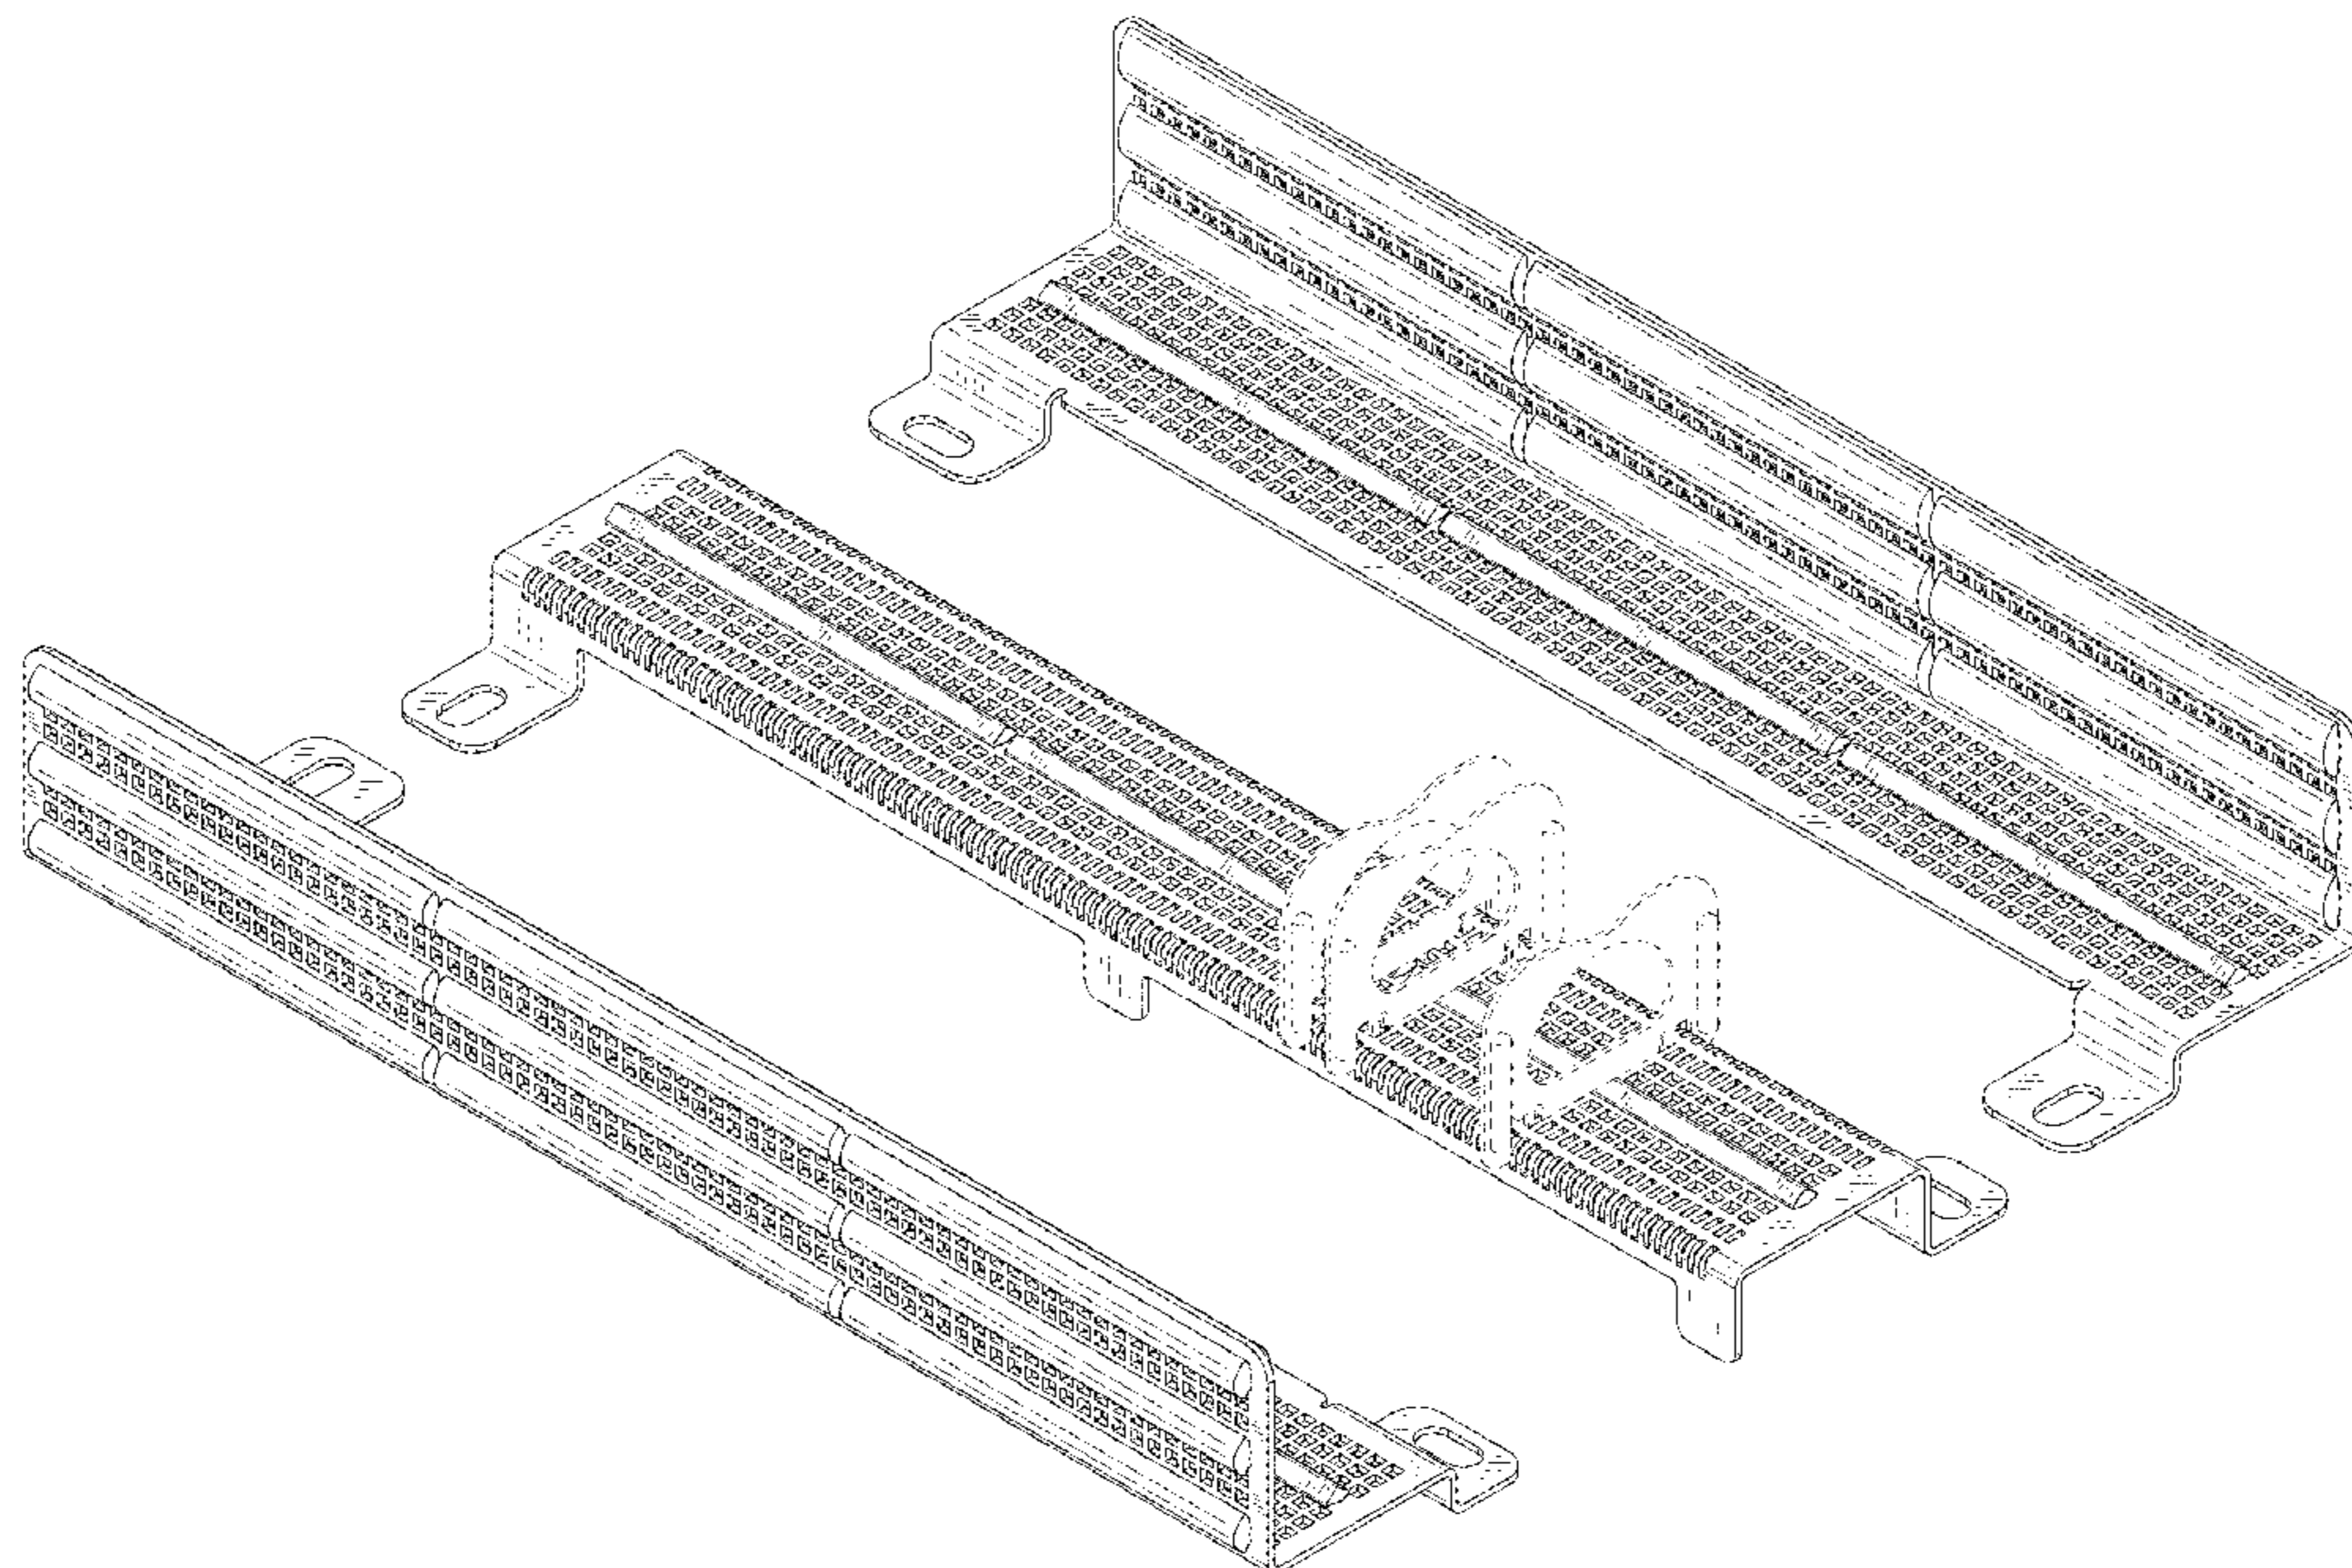

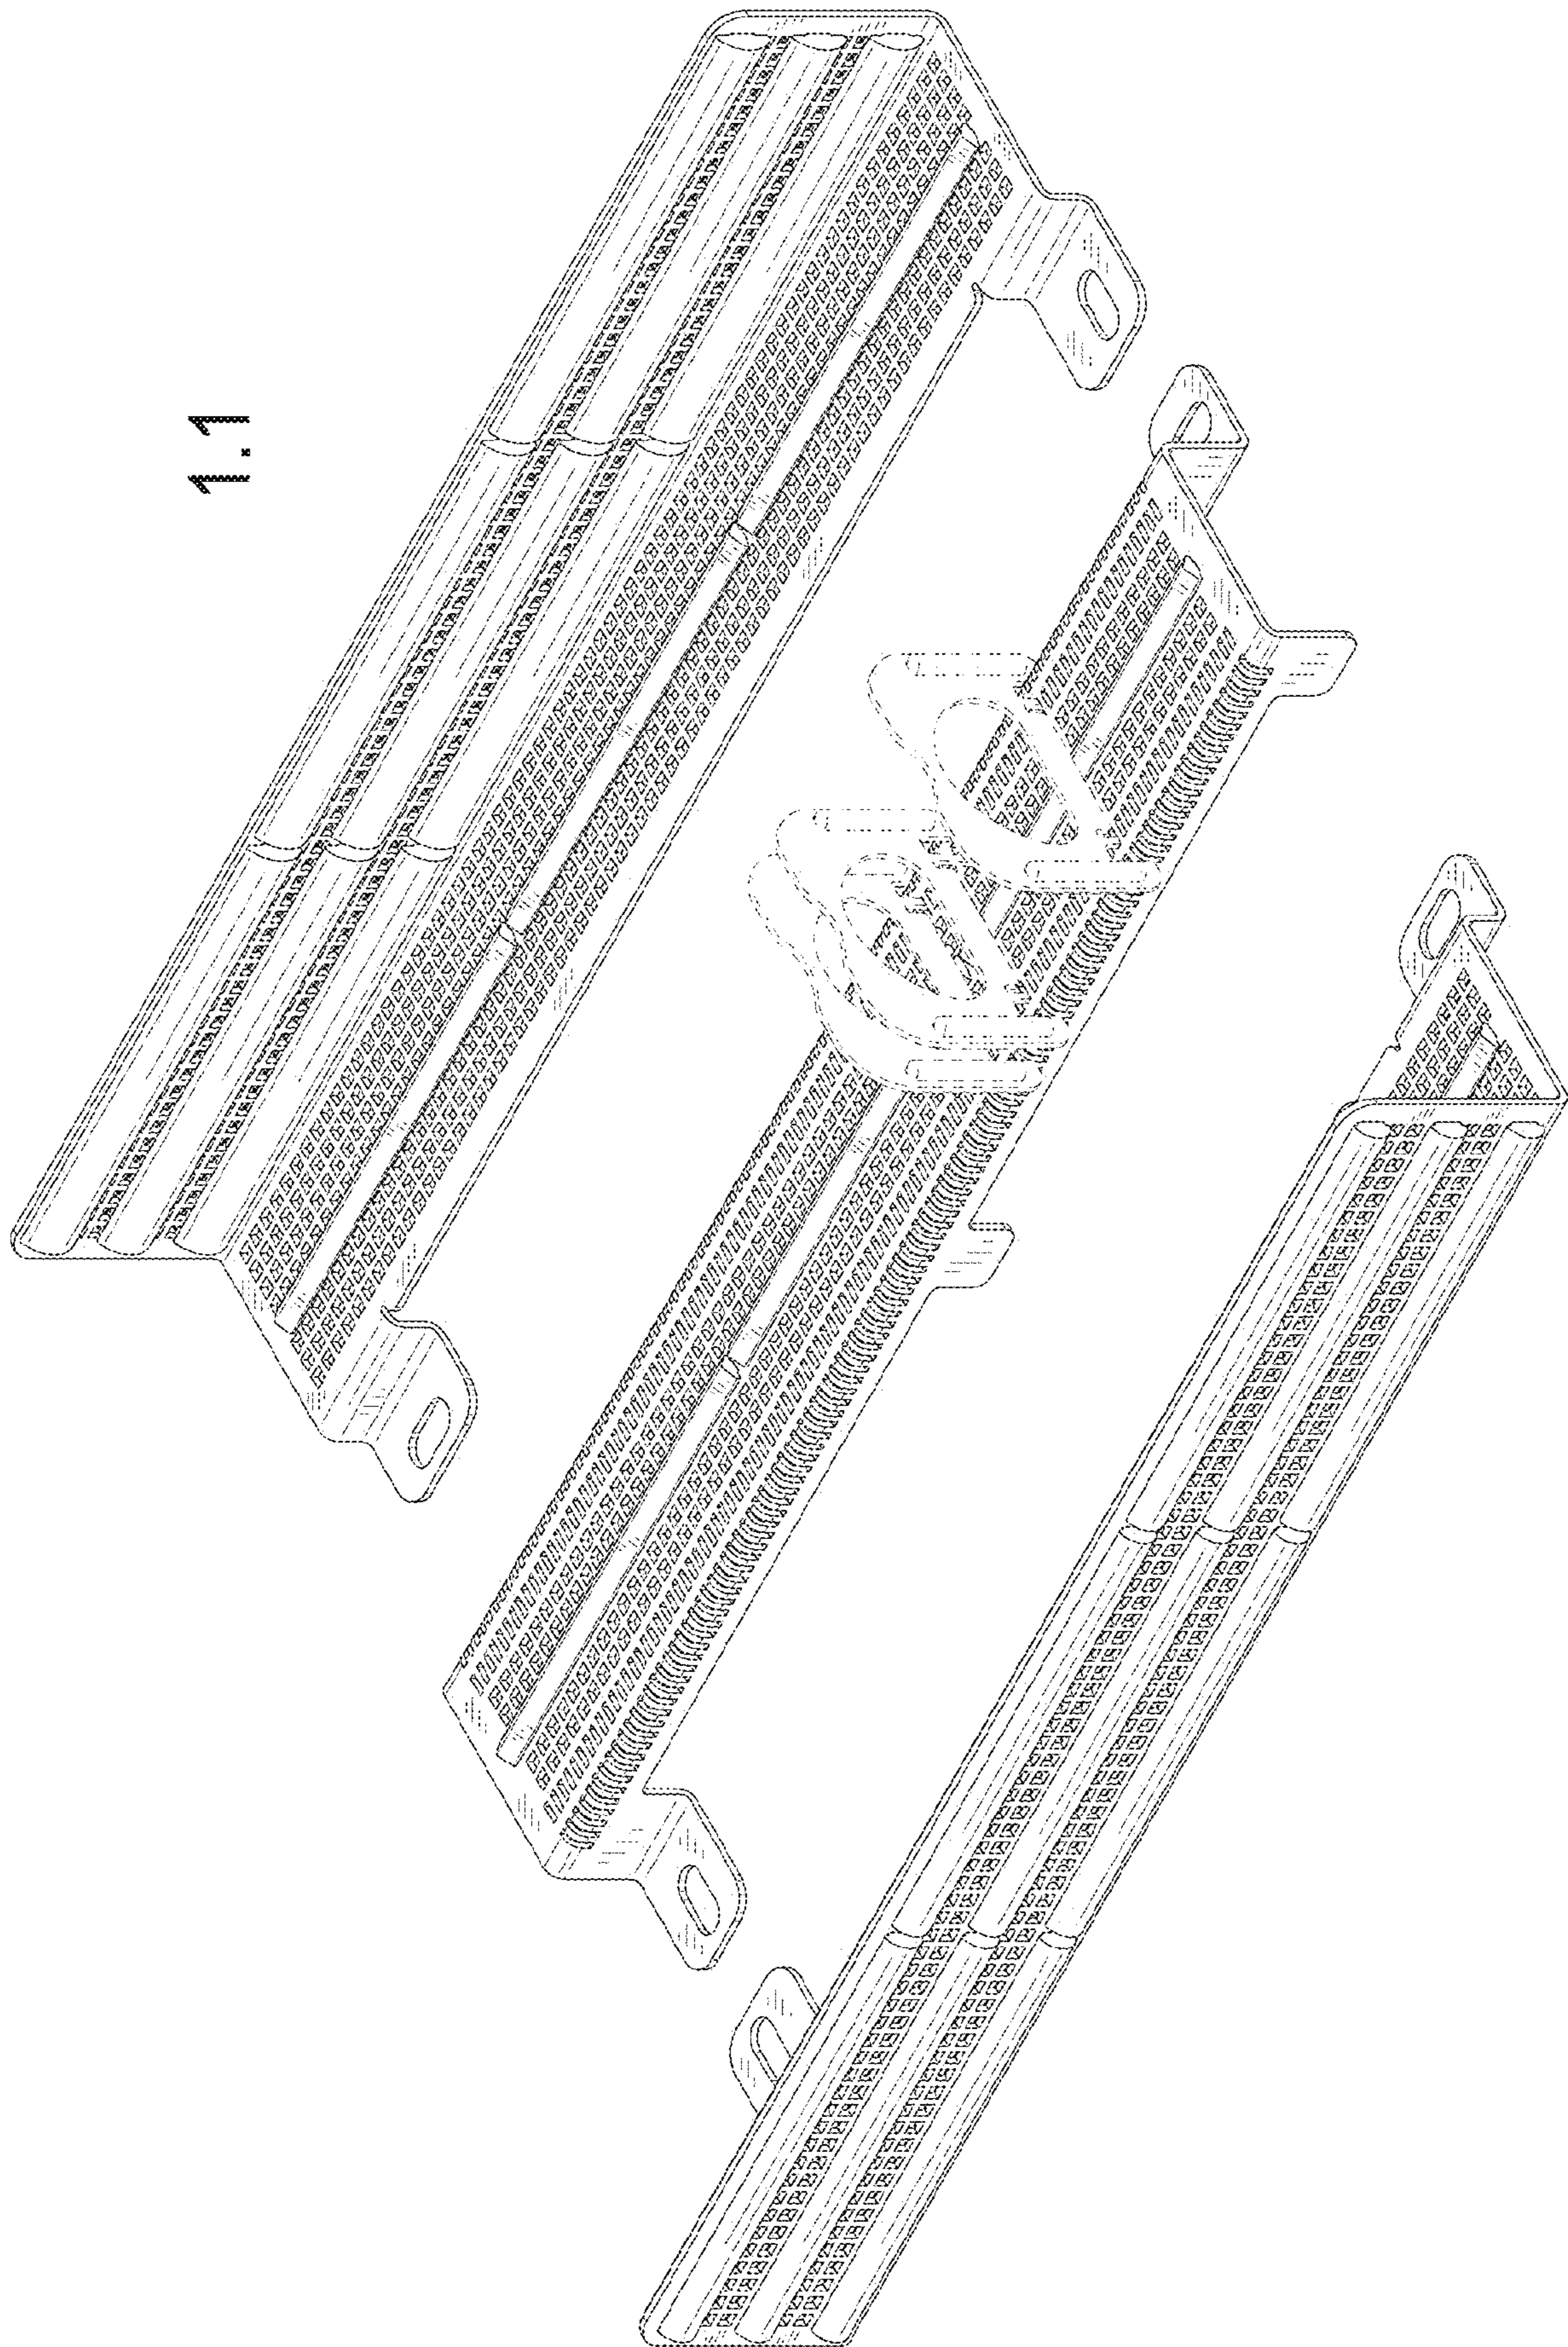


1.1


1.2

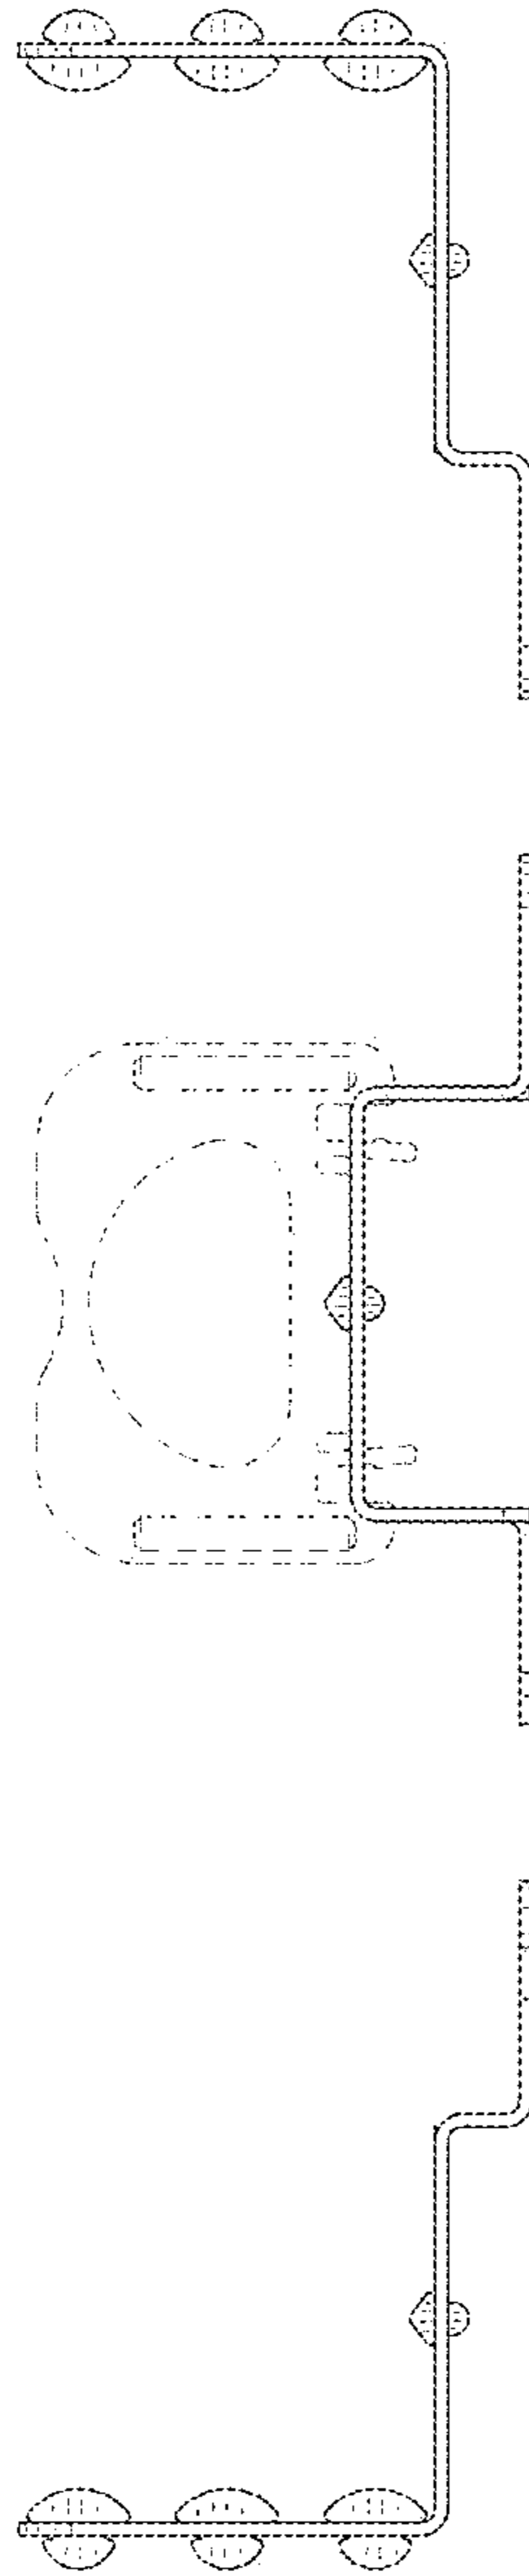


1.3

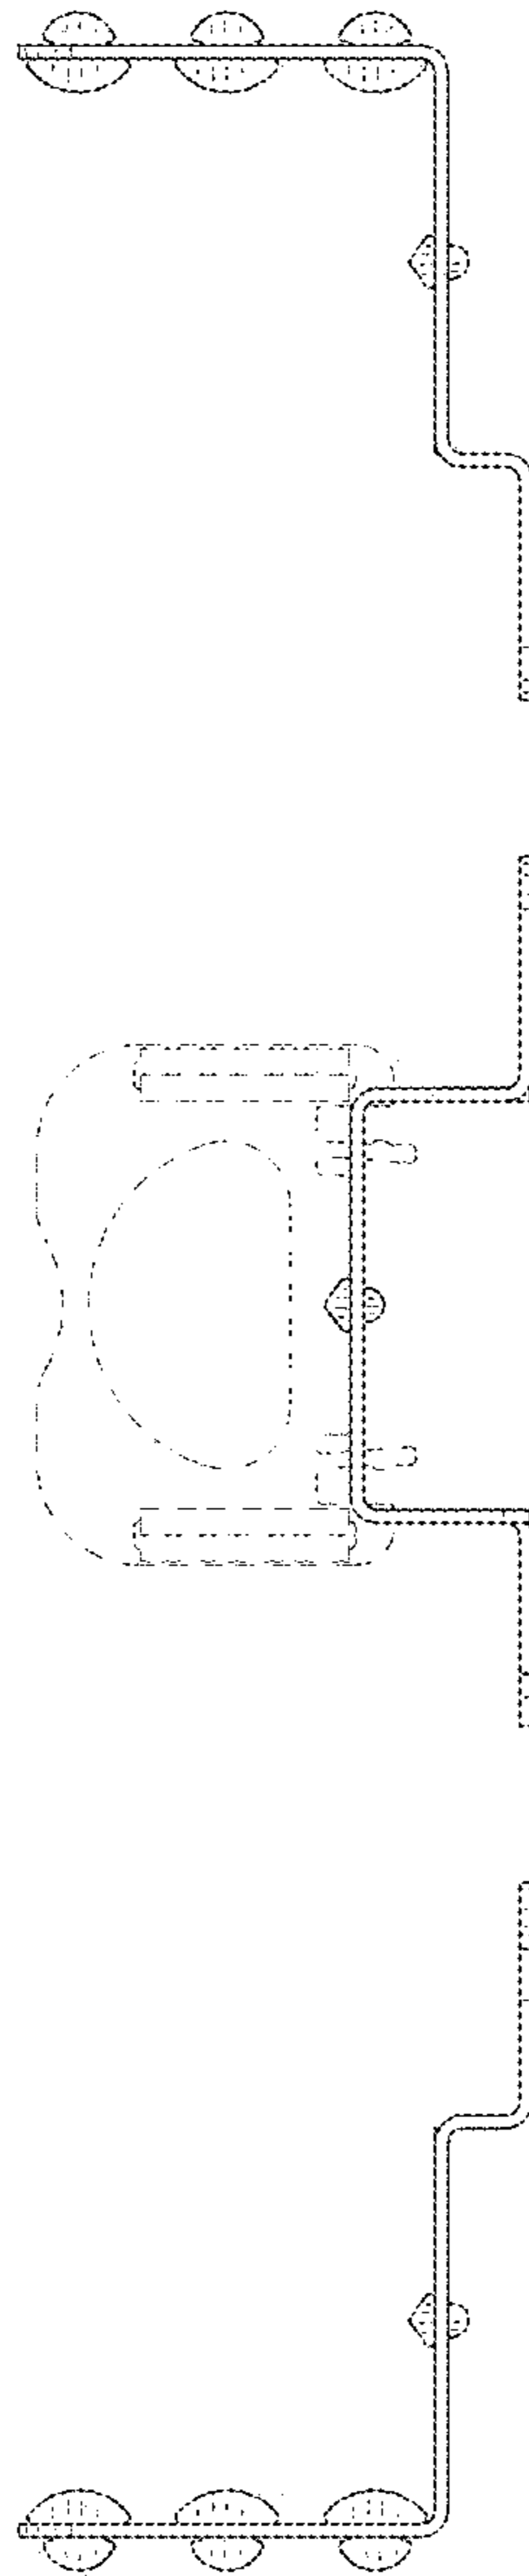




1.4

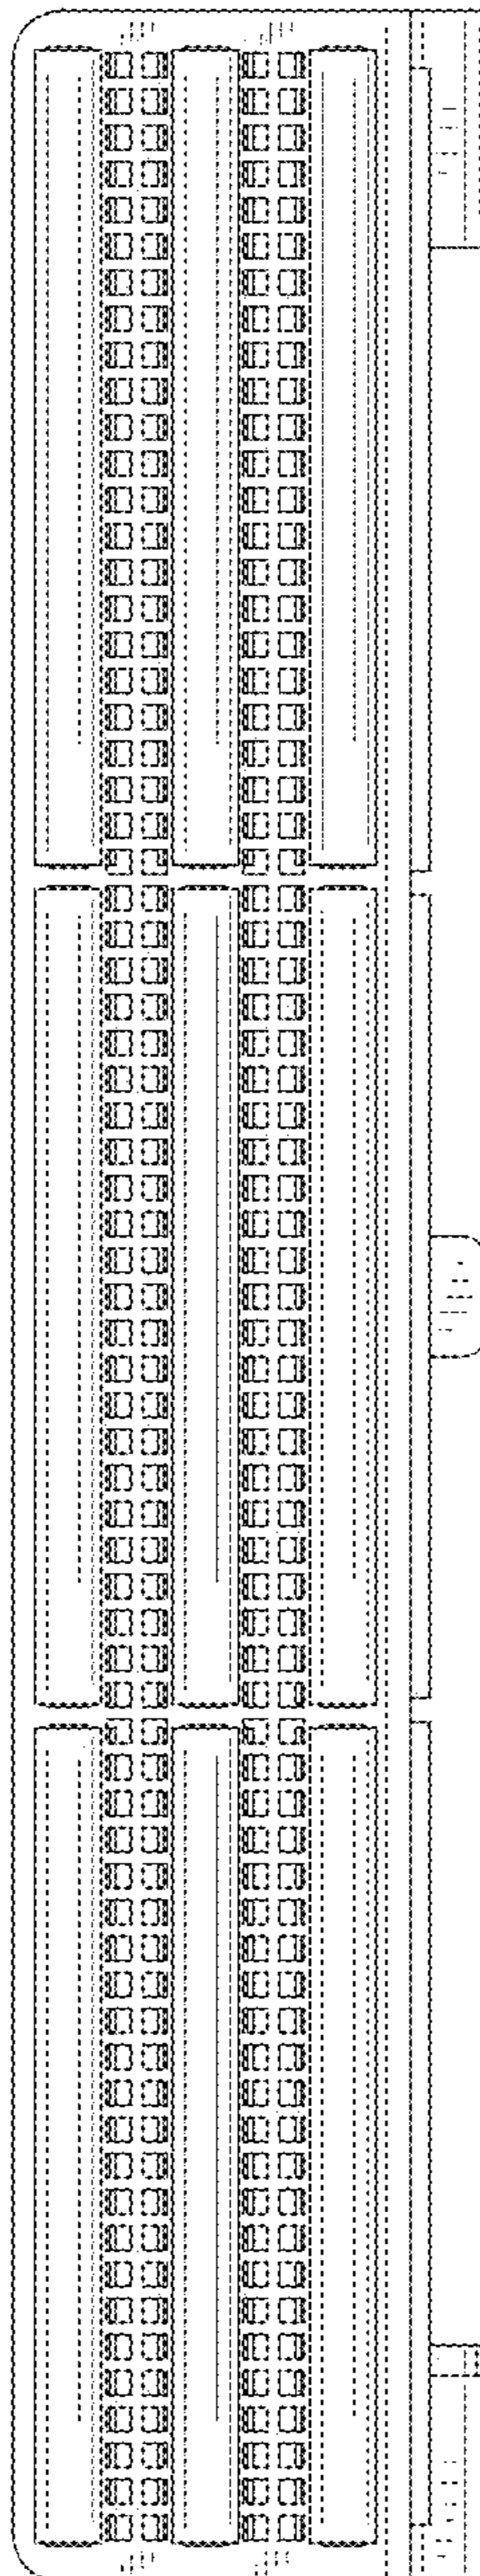

1.5

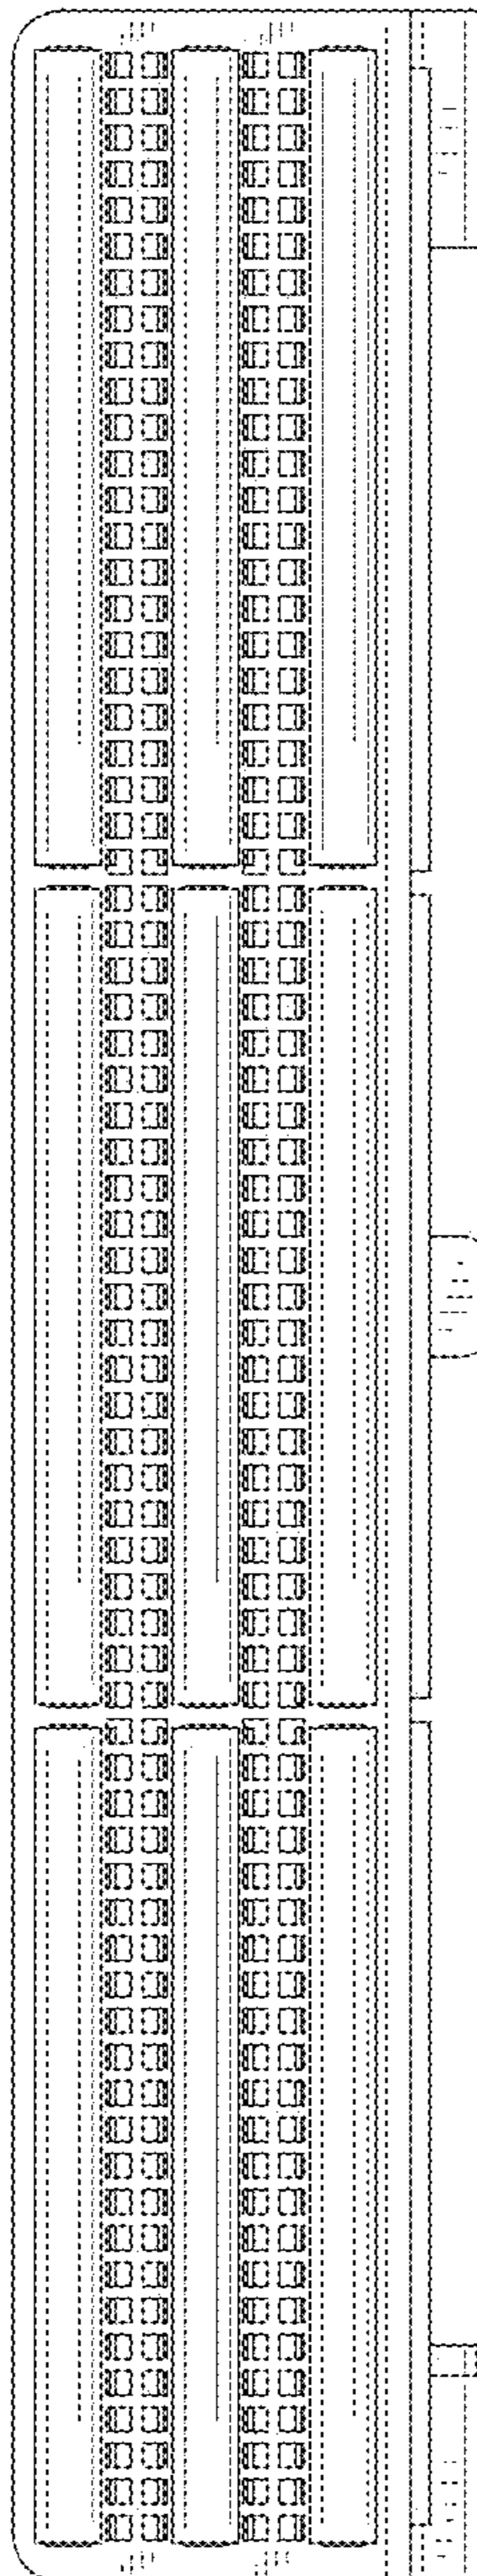

1.6

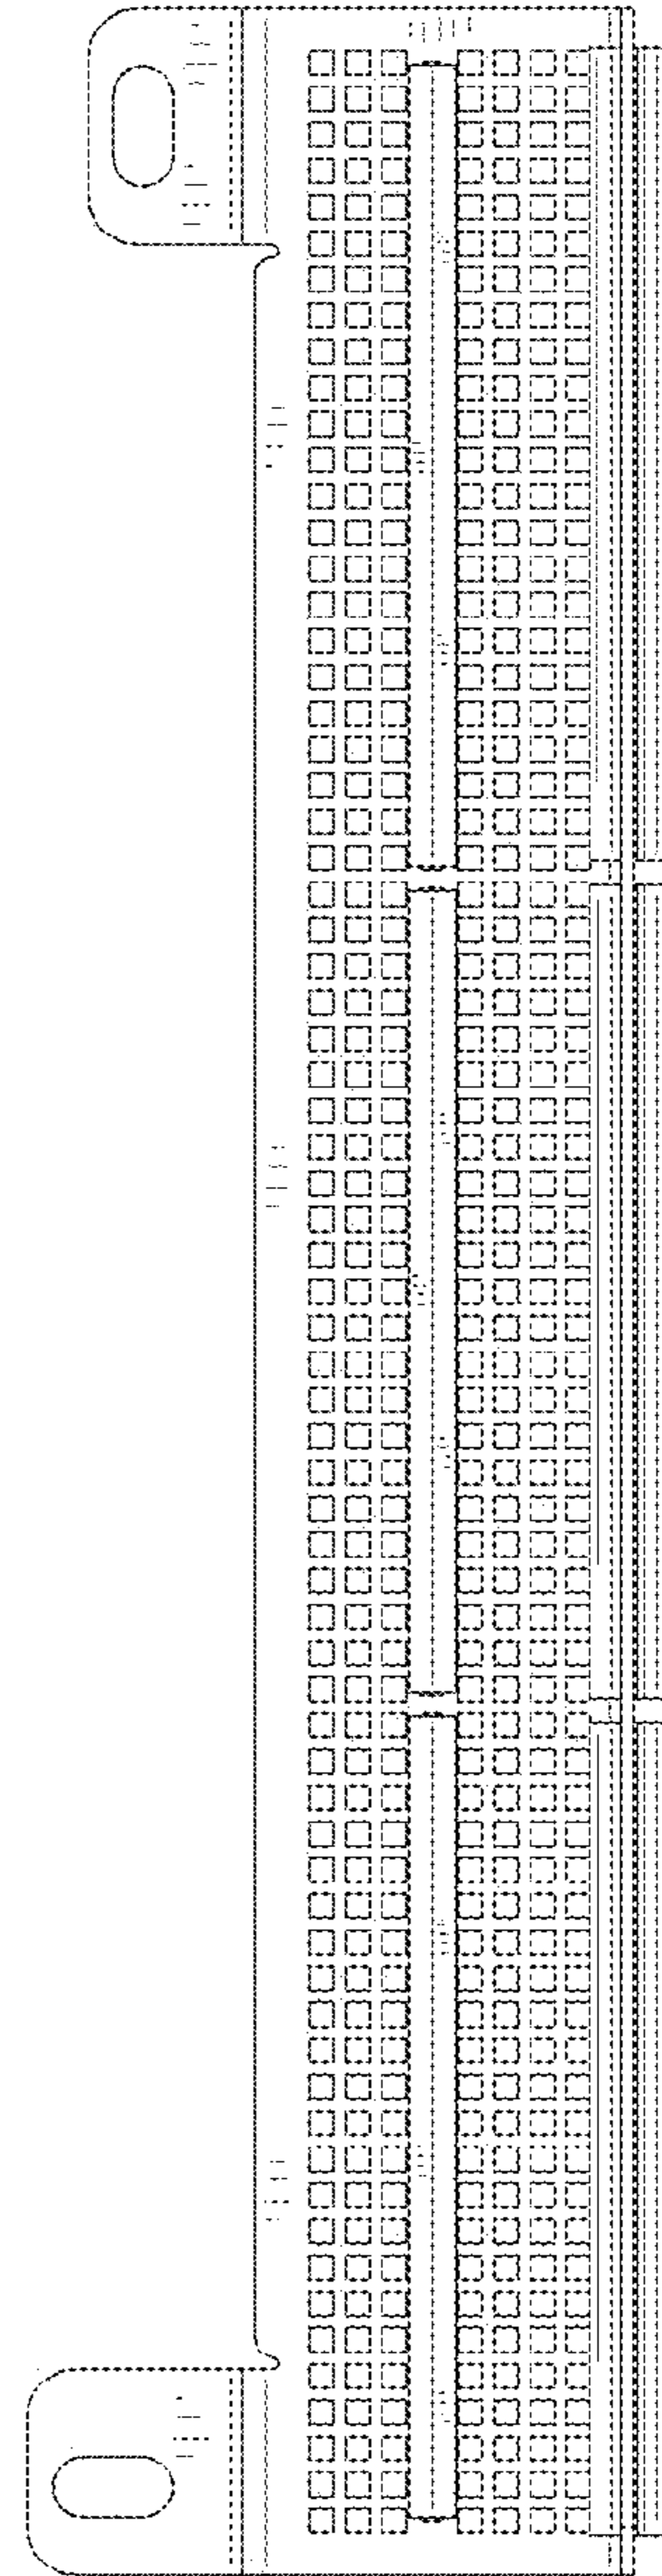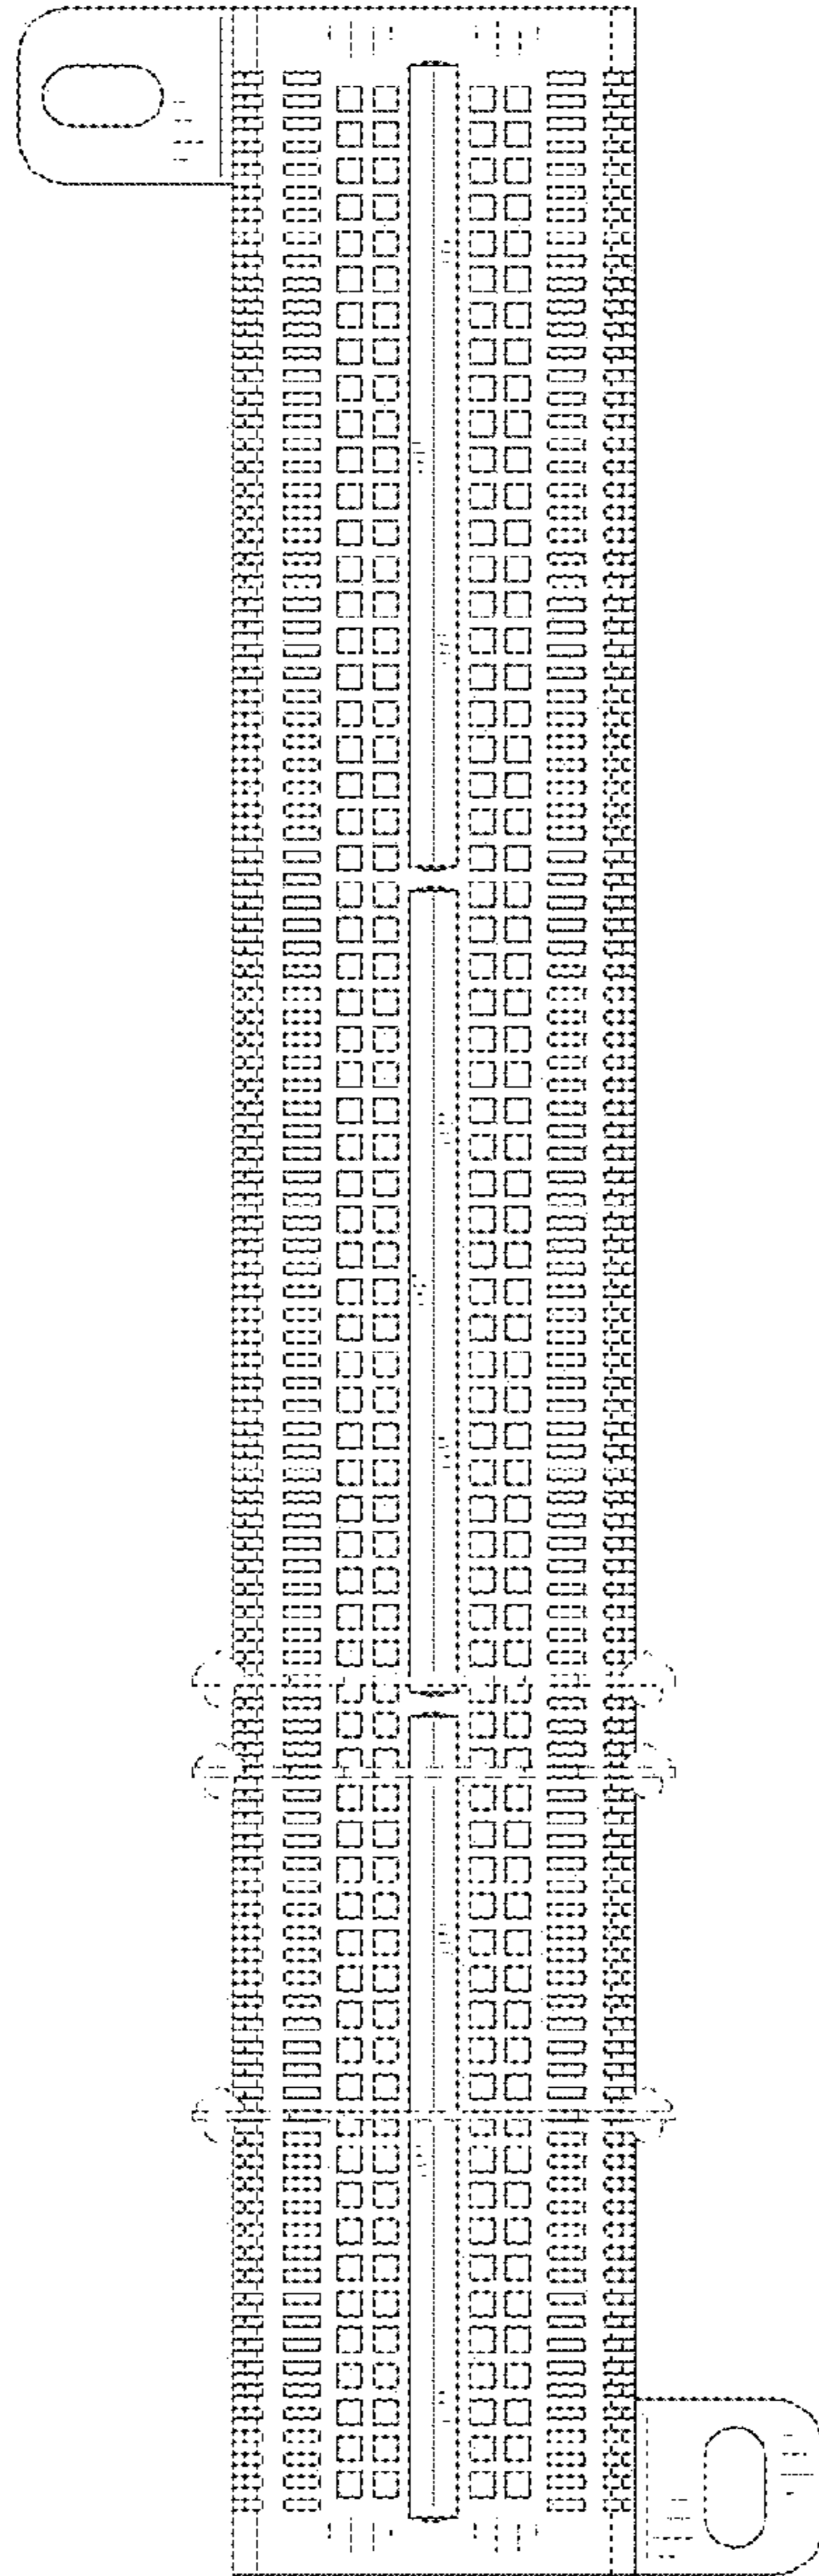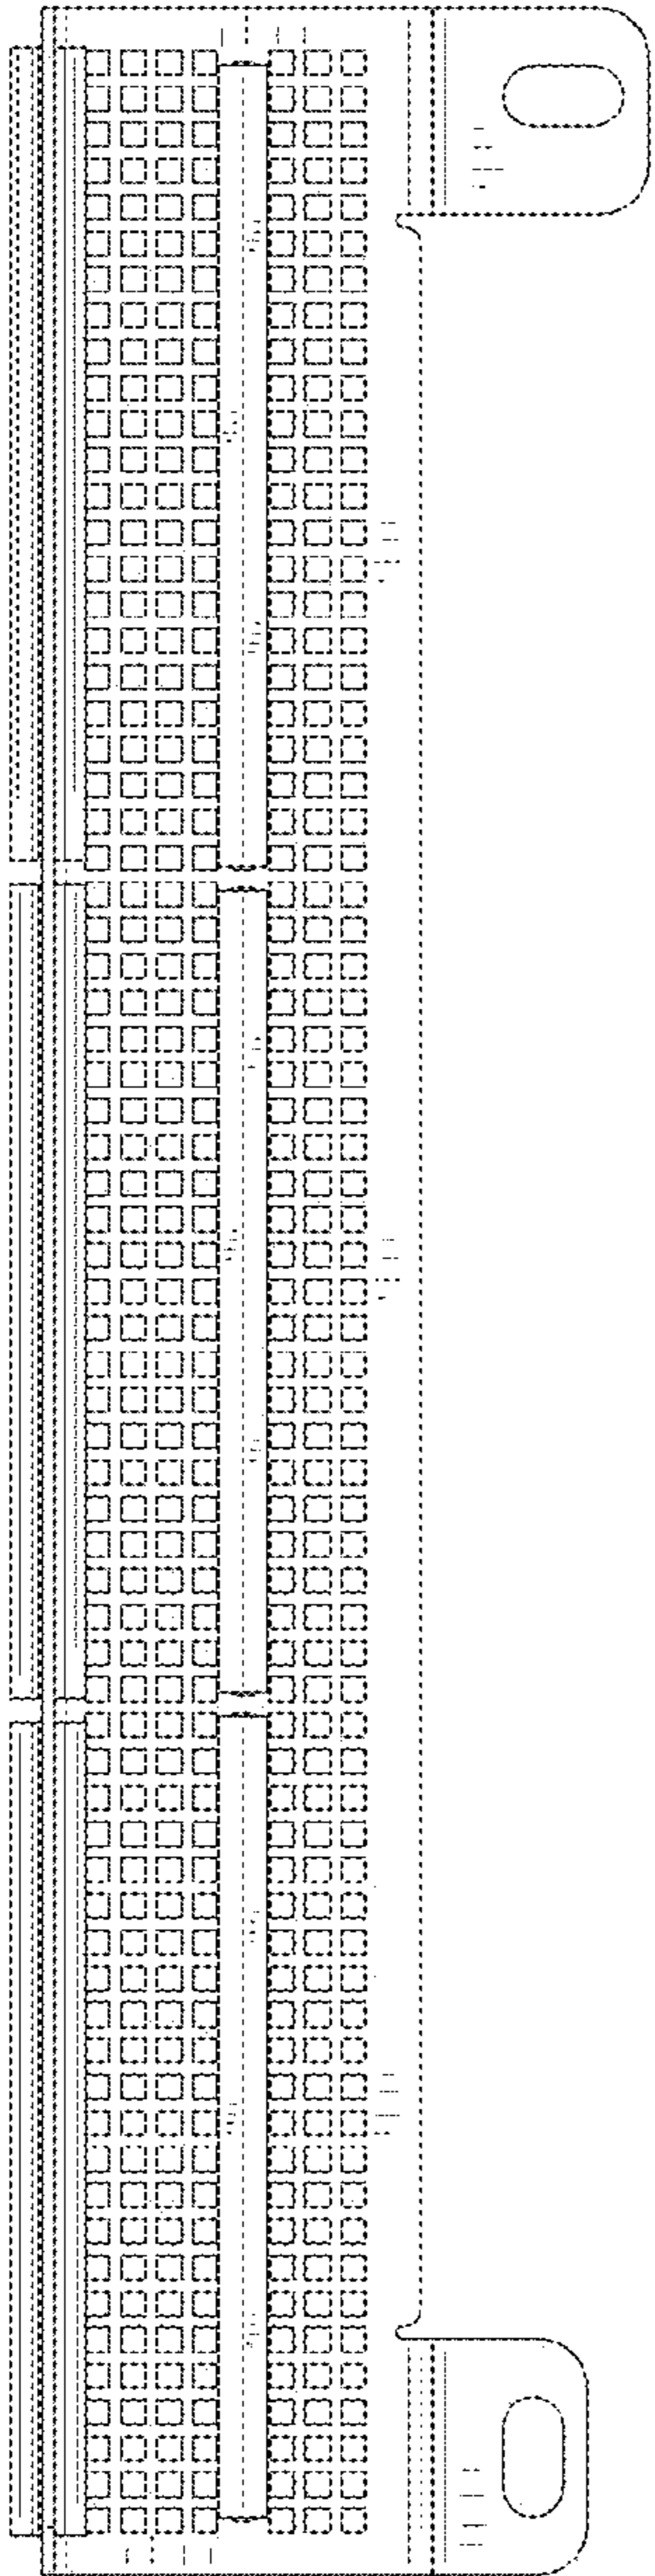

1.7

