

US00D907782S

(12) **United States Design Patent** (10) **Patent No.:** **US D907,782 S**  
**Bailey et al.** (45) **Date of Patent:** **\*\* Jan. 12, 2021**

(54) **SURGICAL CONTROL APPARATUS**

8,286,977 B2 \* 10/2012 Butler ..... A61G 12/001  
280/47.35

(71) Applicant: **Intuitive Surgical Operations, Inc.**,  
Sunnyvale, CA (US)

D687,147 S \* 7/2013 Yoshida ..... D24/185  
D695,898 S \* 12/2013 Chung ..... D24/158  
D699,852 S \* 2/2014 Chung ..... D24/158  
D702,840 S \* 4/2014 Blomquist ..... D24/164  
D702,842 S \* 4/2014 Hyde ..... D24/185  
D711,539 S \* 8/2014 Hunt ..... D24/158  
D712,042 S \* 8/2014 Chung ..... D24/185

(72) Inventors: **David W. Bailey**, Portola Valley, CA  
(US); **Robert B. Hubler**, Sunnyvale,  
CA (US); **Timothy B. Hulford**, San  
Jose, CA (US); **Nicholas W. Oakley**,  
Portland, OR (US)

(Continued)

(73) Assignee: **INTUITIVE SURGICAL  
OPERATIONS, INC.**, Sunnyvale, CA  
(US)

**OTHER PUBLICATIONS**

(\*\*) Term: **15 Years**

Vertut, Jean and Phillipe Coiffet, Robot Technology: Teleoperation  
and Robotics Evolution and Development, English translation,  
Prentice-Hall, Inc., Inglewood Cliffs, NJ, USA 1986, vol. 3A, 332  
pages.

(21) Appl. No.: **29/718,922**

*Primary Examiner* — Rhea Shields

(22) Filed: **Dec. 30, 2019**

(74) *Attorney, Agent, or Firm* — Haynes and Boone, LLP

**Related U.S. Application Data**

(57) **CLAIM**

(63) Continuation of application No. 29/648,249, filed on  
May 18, 2018, now Pat. No. Des. 874,657.

The ornamental design for a surgical control apparatus, as  
shown and described.

(51) **LOC (13) Cl.** ..... **24-02**

**DESCRIPTION**

(52) **U.S. Cl.**

USPC ..... **D24/185**

(58) **Field of Classification Search**

USPC ..... D24/185, 186, 176, 158, 167, 164;  
D14/307; D15/199; D34/14

CPC ..... A61B 90/04; A61B 34/32; A61B 50/30;  
A61B 8/463; A61G 12/001

See application file for complete search history.

FIG. 1 is a perspective view of a surgical control apparatus  
showing our new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a rear elevational view thereof;  
FIG. 4 is a right side elevational view thereof;  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a top plan view thereof;  
FIG. 7 is a bottom plan view thereof; and,  
FIGS. 8 and 9 are additional perspective views thereof.

(56) **References Cited**


**U.S. PATENT DOCUMENTS**

D486,915 S \* 2/2004 Warschewske ..... D24/185  
D550,362 S \* 9/2007 Olivera ..... D24/185  
D561,342 S \* 2/2008 Zimmer ..... D24/185  
D621,513 S \* 8/2010 Cinqualbre ..... D24/185  
D626,235 S \* 10/2010 Smith ..... D24/158

The surgical control apparatus illustrated in FIGS. 1-9 may  
be, for example, a surgical control apparatus for lung sur-  
gery.

The broken lines in FIGS. 1-9 illustrate unclaimed portions  
of the surgical control apparatus and form no part of the  
claimed design.

**1 Claim, 8 Drawing Sheets**

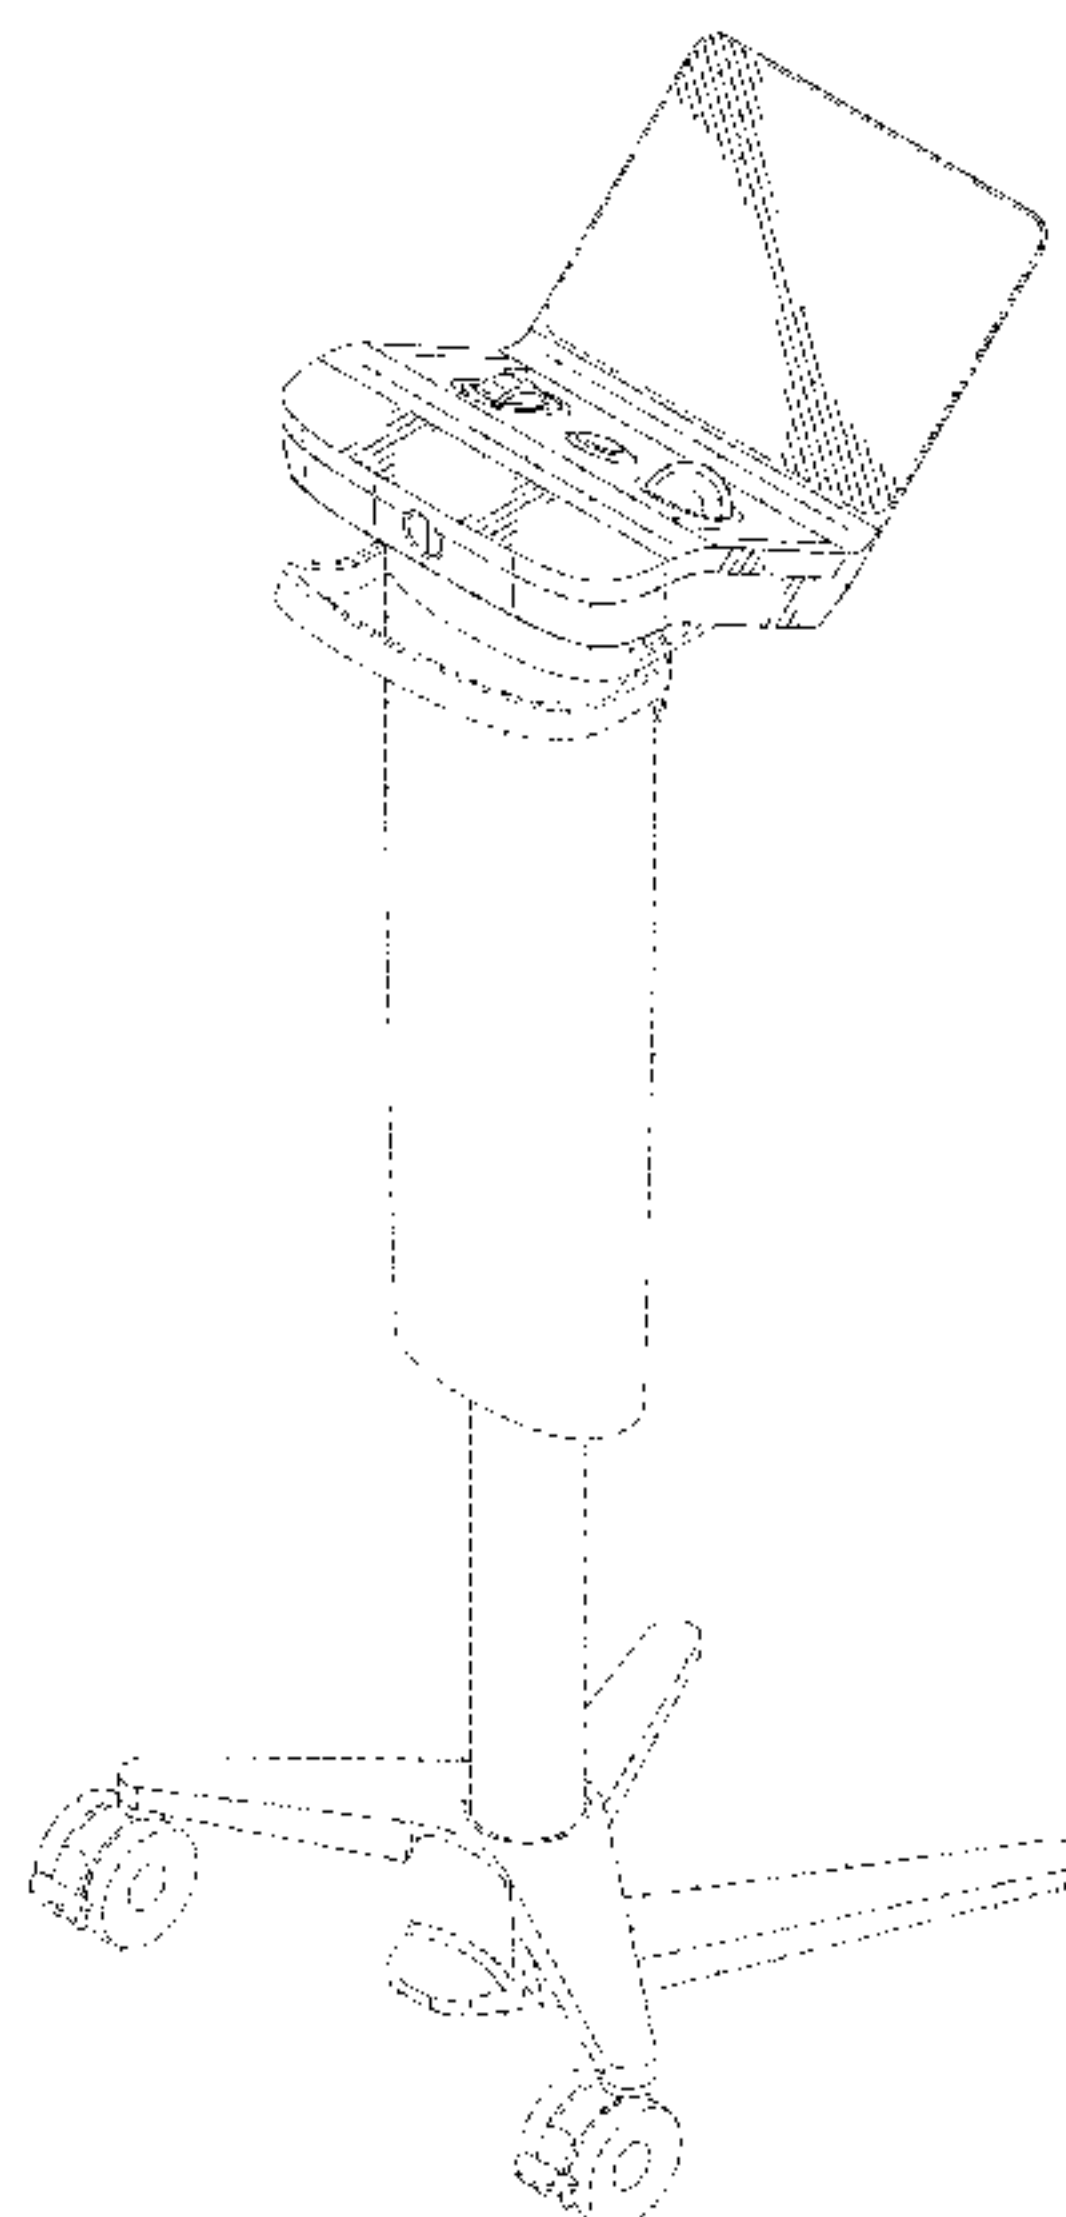

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

D721,696 S \* 1/2015 Birgeoglu ..... D14/307  
D724,737 S \* 3/2015 Kawamura ..... D24/158  
D725,274 S \* 3/2015 Kawamura ..... D24/158  
D730,011 S \* 5/2015 McRorie ..... D34/14  
9,055,910 B2 \* 6/2015 Nakajima ..... A61B 8/463  
D735,866 S \* 8/2015 Assa ..... D24/185  
D739,538 S \* 9/2015 Bernal ..... D24/185  
D753,310 S \* 4/2016 Thakar ..... D24/185  
D768,861 S \* 10/2016 Barak ..... D24/176  
9,463,069 B2 \* 10/2016 Dunworth ..... A61B 50/30  
D771,817 S \* 11/2016 Barak ..... D24/160  
D776,279 S \* 1/2017 Newman ..... D24/164  
D777,927 S \* 1/2017 Choudhary ..... D24/167  
D787,065 S \* 5/2017 Yanase ..... D24/160  
D790,066 S \* 6/2017 Lei ..... D24/158  
D796,679 S \* 9/2017 Dekock ..... D24/158  
D827,139 S \* 8/2018 Henderson ..... D24/160  
D836,781 S \* 12/2018 Meurer ..... D24/185  
D844,792 S \* 4/2019 Choe ..... D24/186  
10,350,015 B2 \* 7/2019 Toth ..... A61B 34/32  
10,376,331 B2 \* 8/2019 Cooper ..... A61B 90/04  
D865,182 S \* 10/2019 Richter ..... D24/186  
D865,972 S \* 11/2019 Jeanjean ..... D24/186  
D868,055 S \* 11/2019 Benic ..... D14/307  
D874,657 S \* 2/2020 Bailey ..... D24/185  
D879,303 S \* 3/2020 Engler ..... D24/185  
D893,570 S \* 8/2020 Zheng ..... D15/199  
D894,403 S \* 8/2020 Couch ..... D24/185

\* cited by examiner

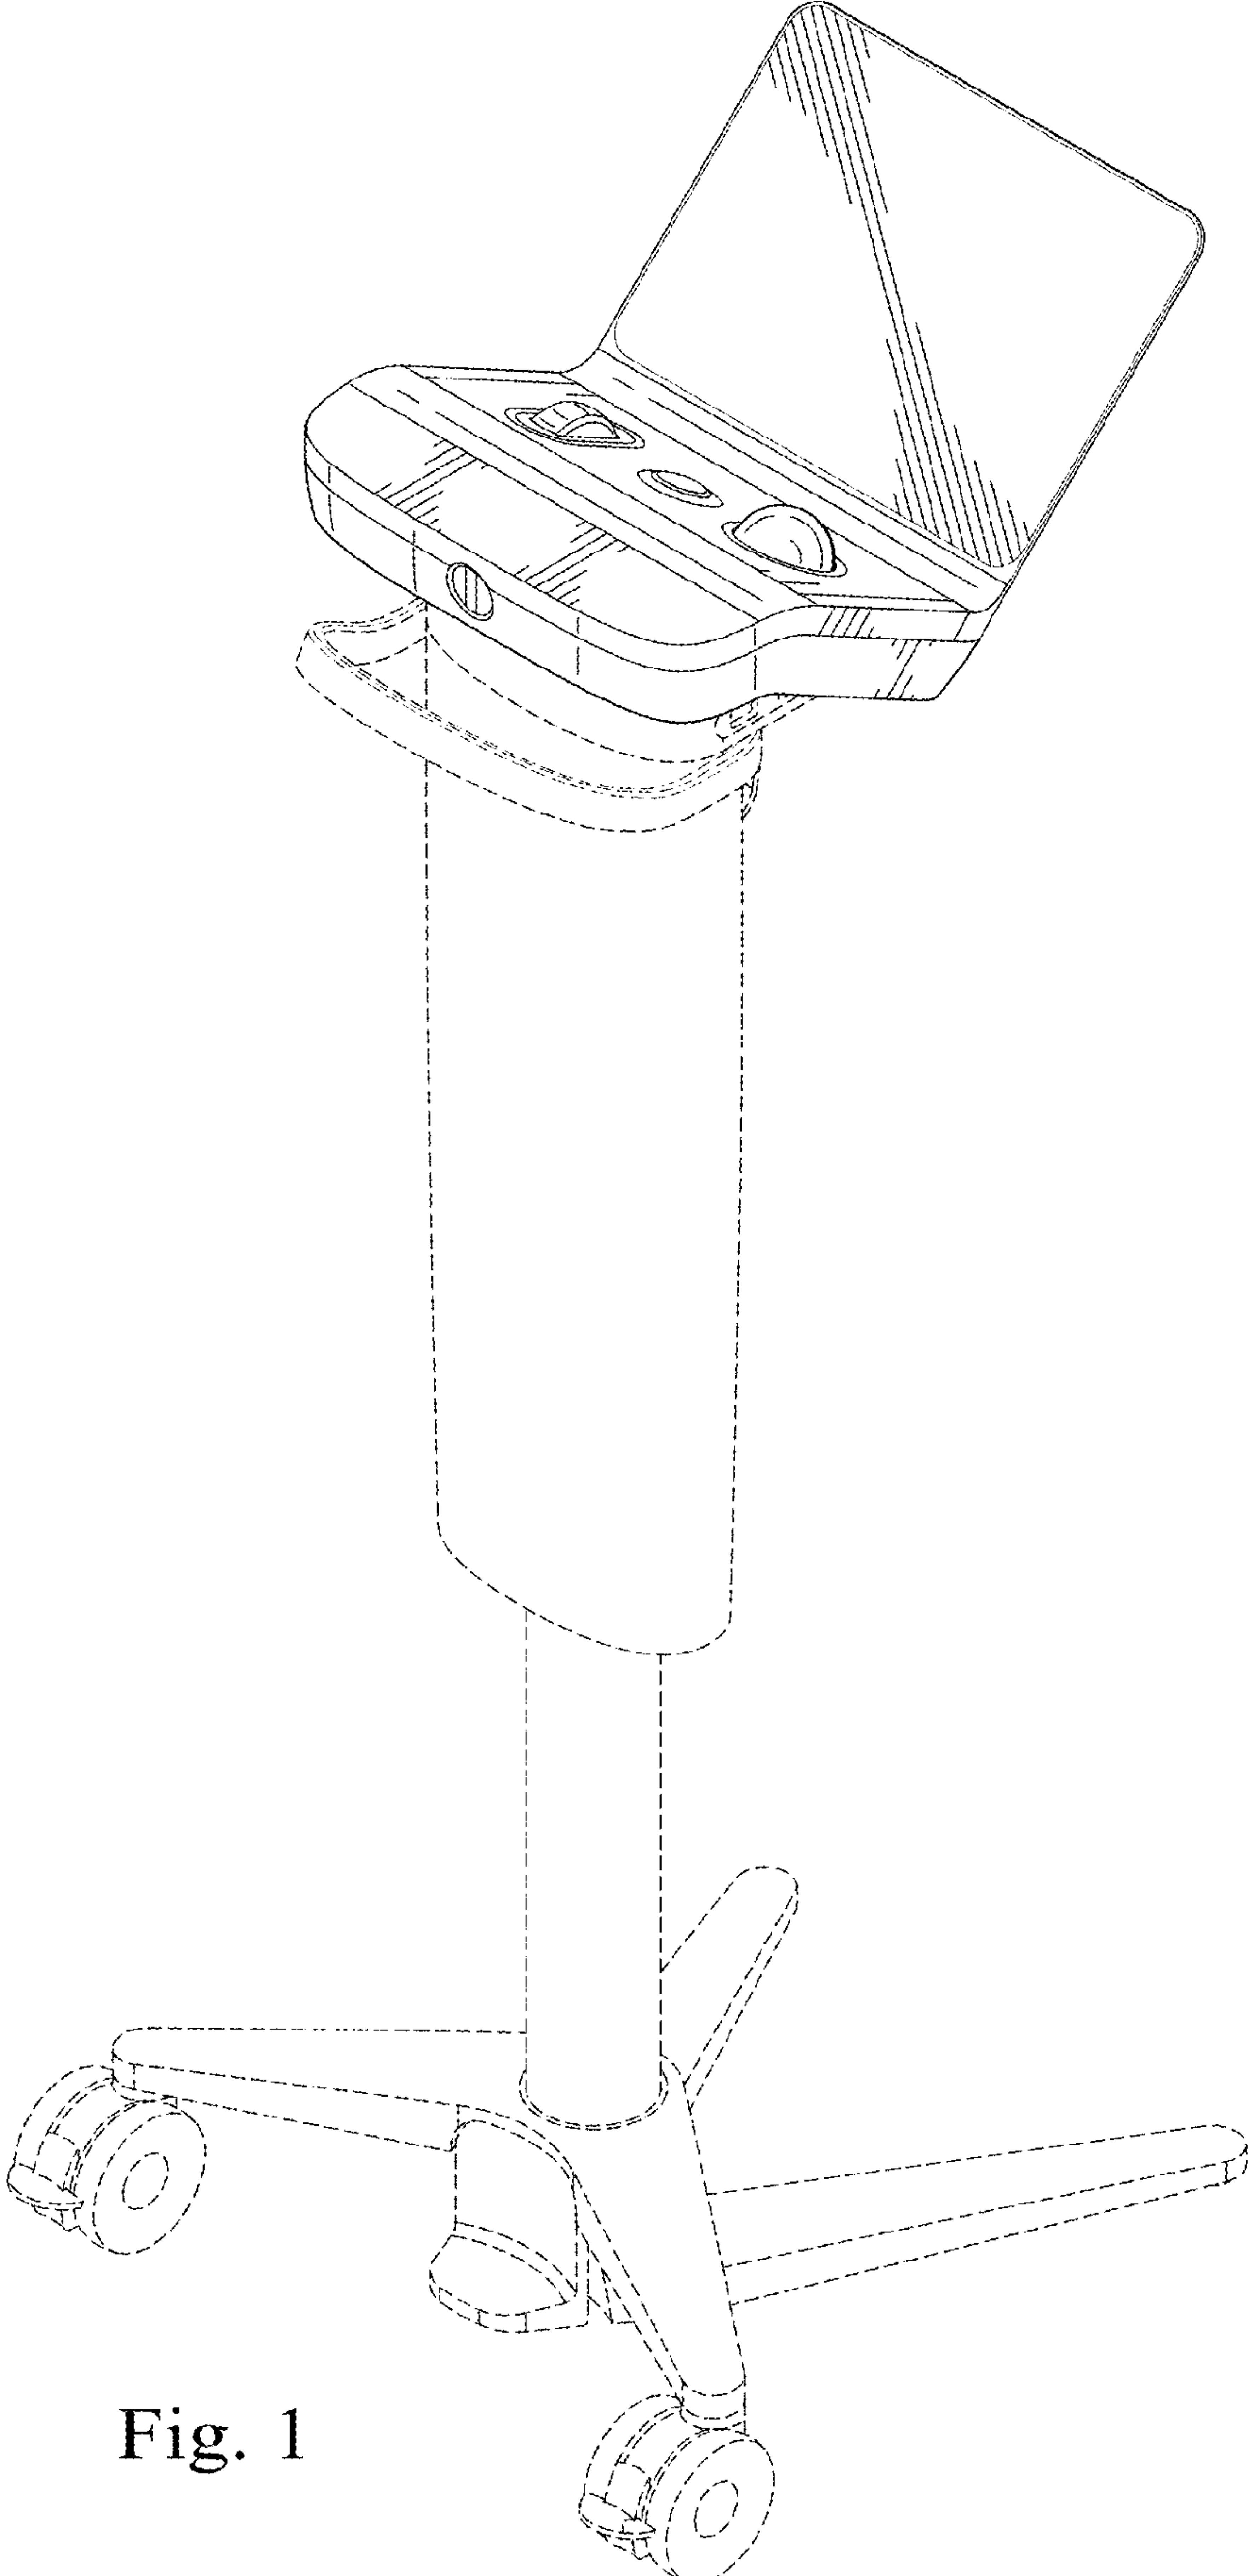


Fig. 1

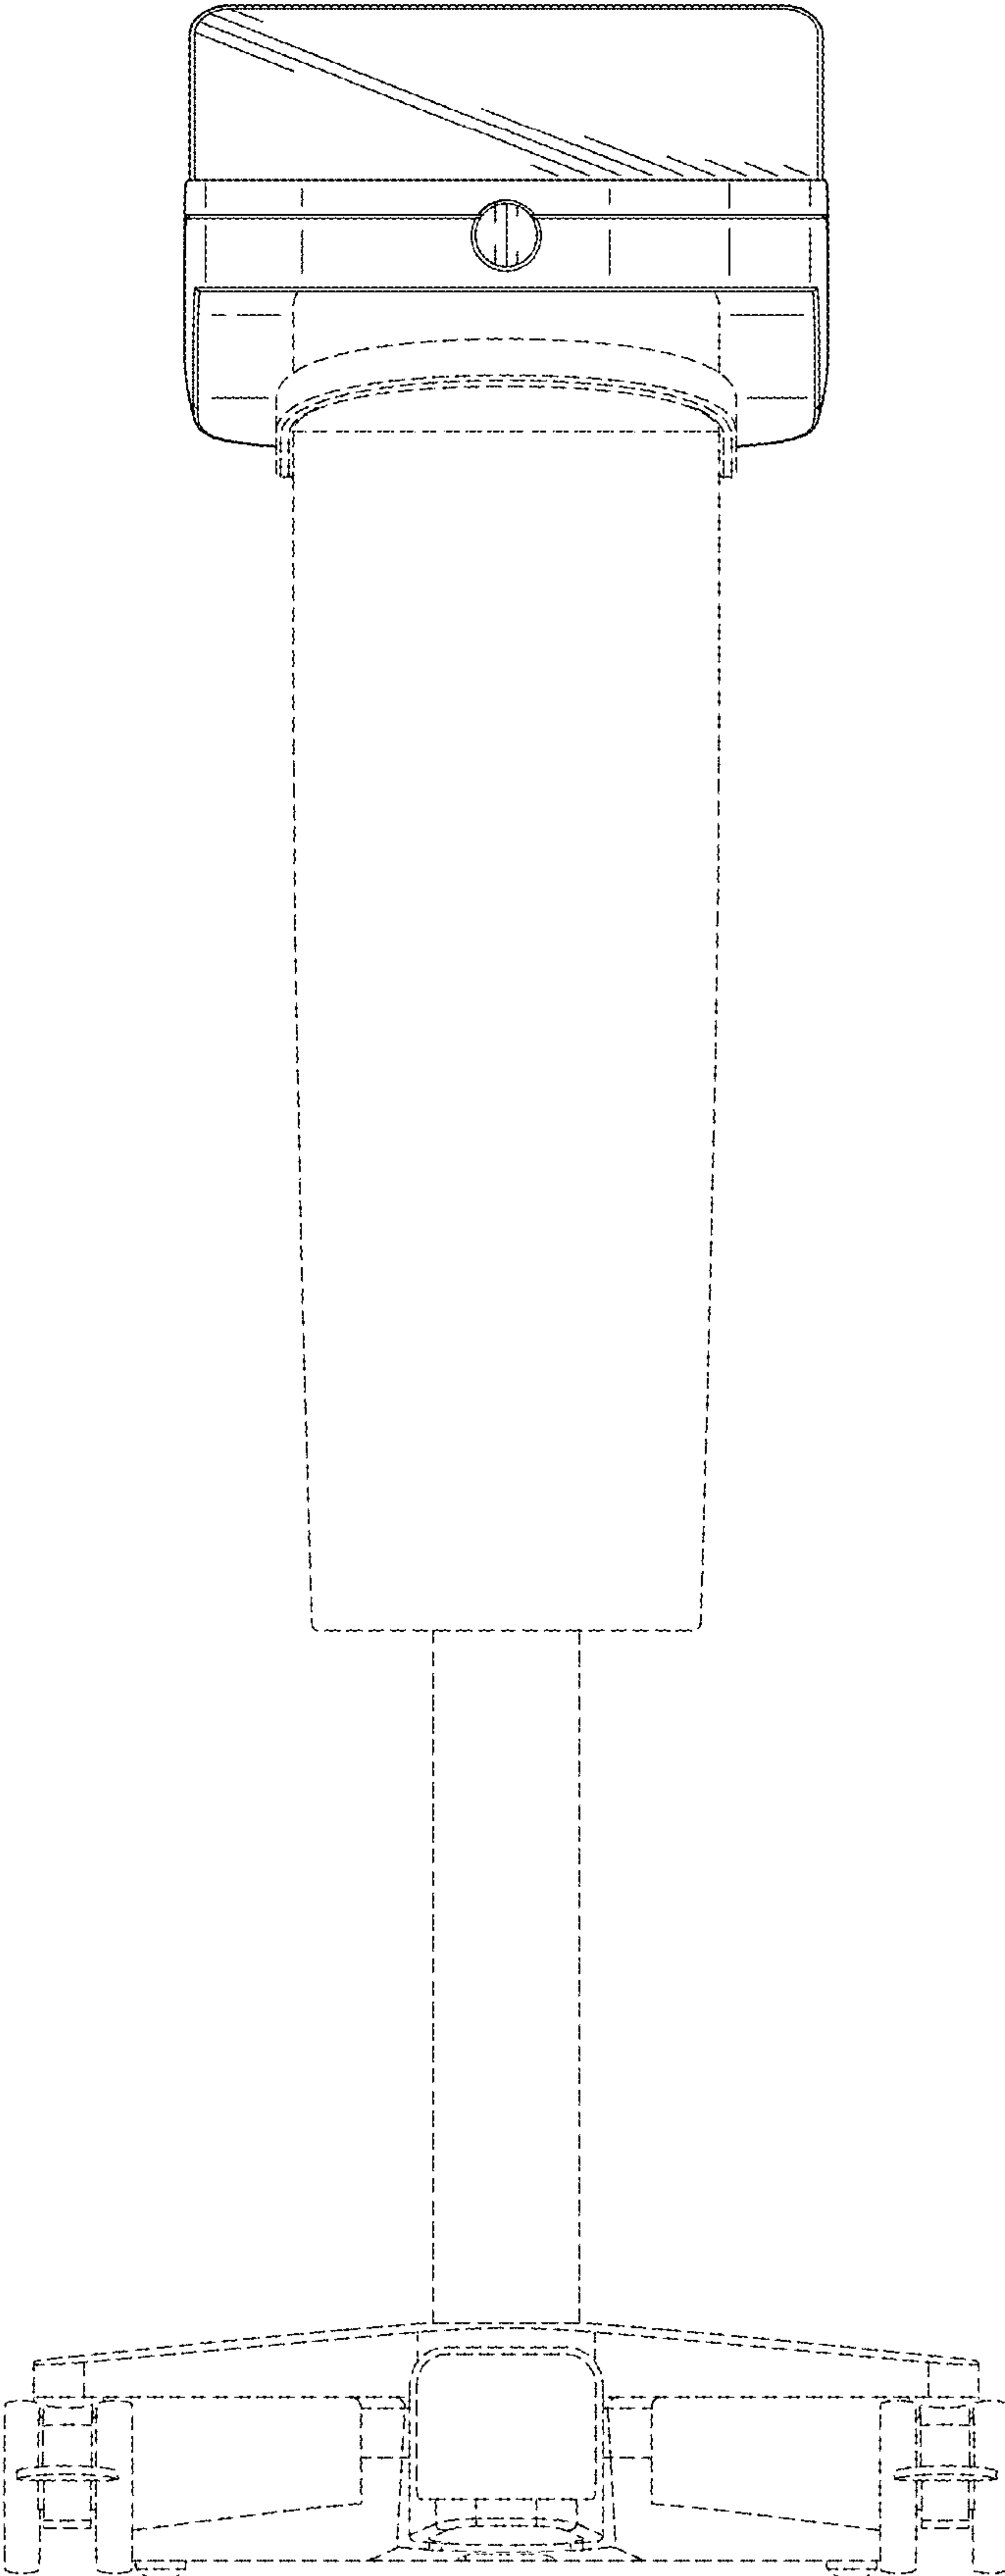


Fig. 2

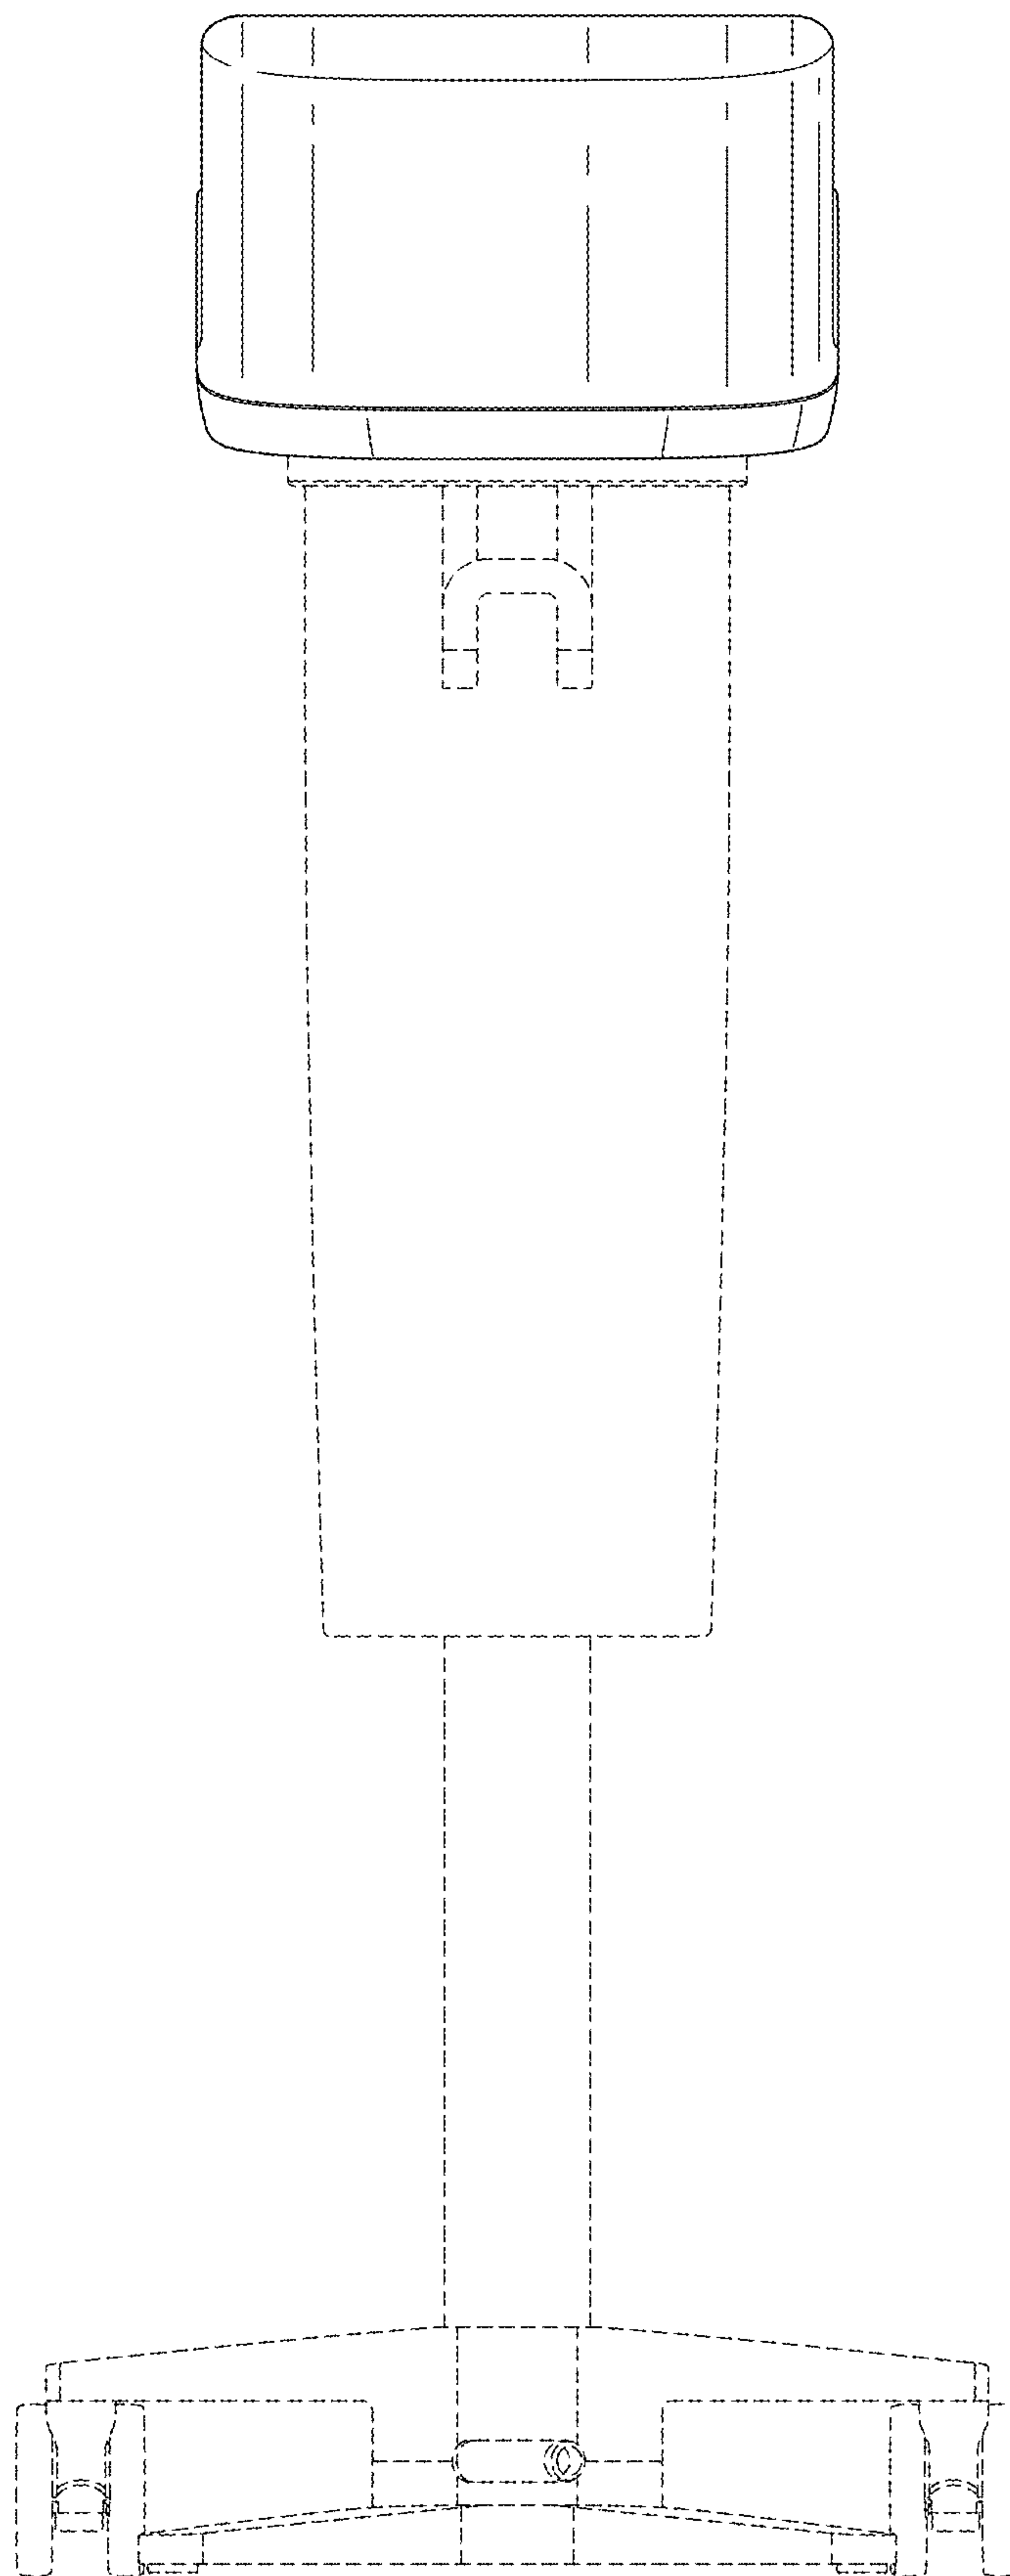


Fig. 3

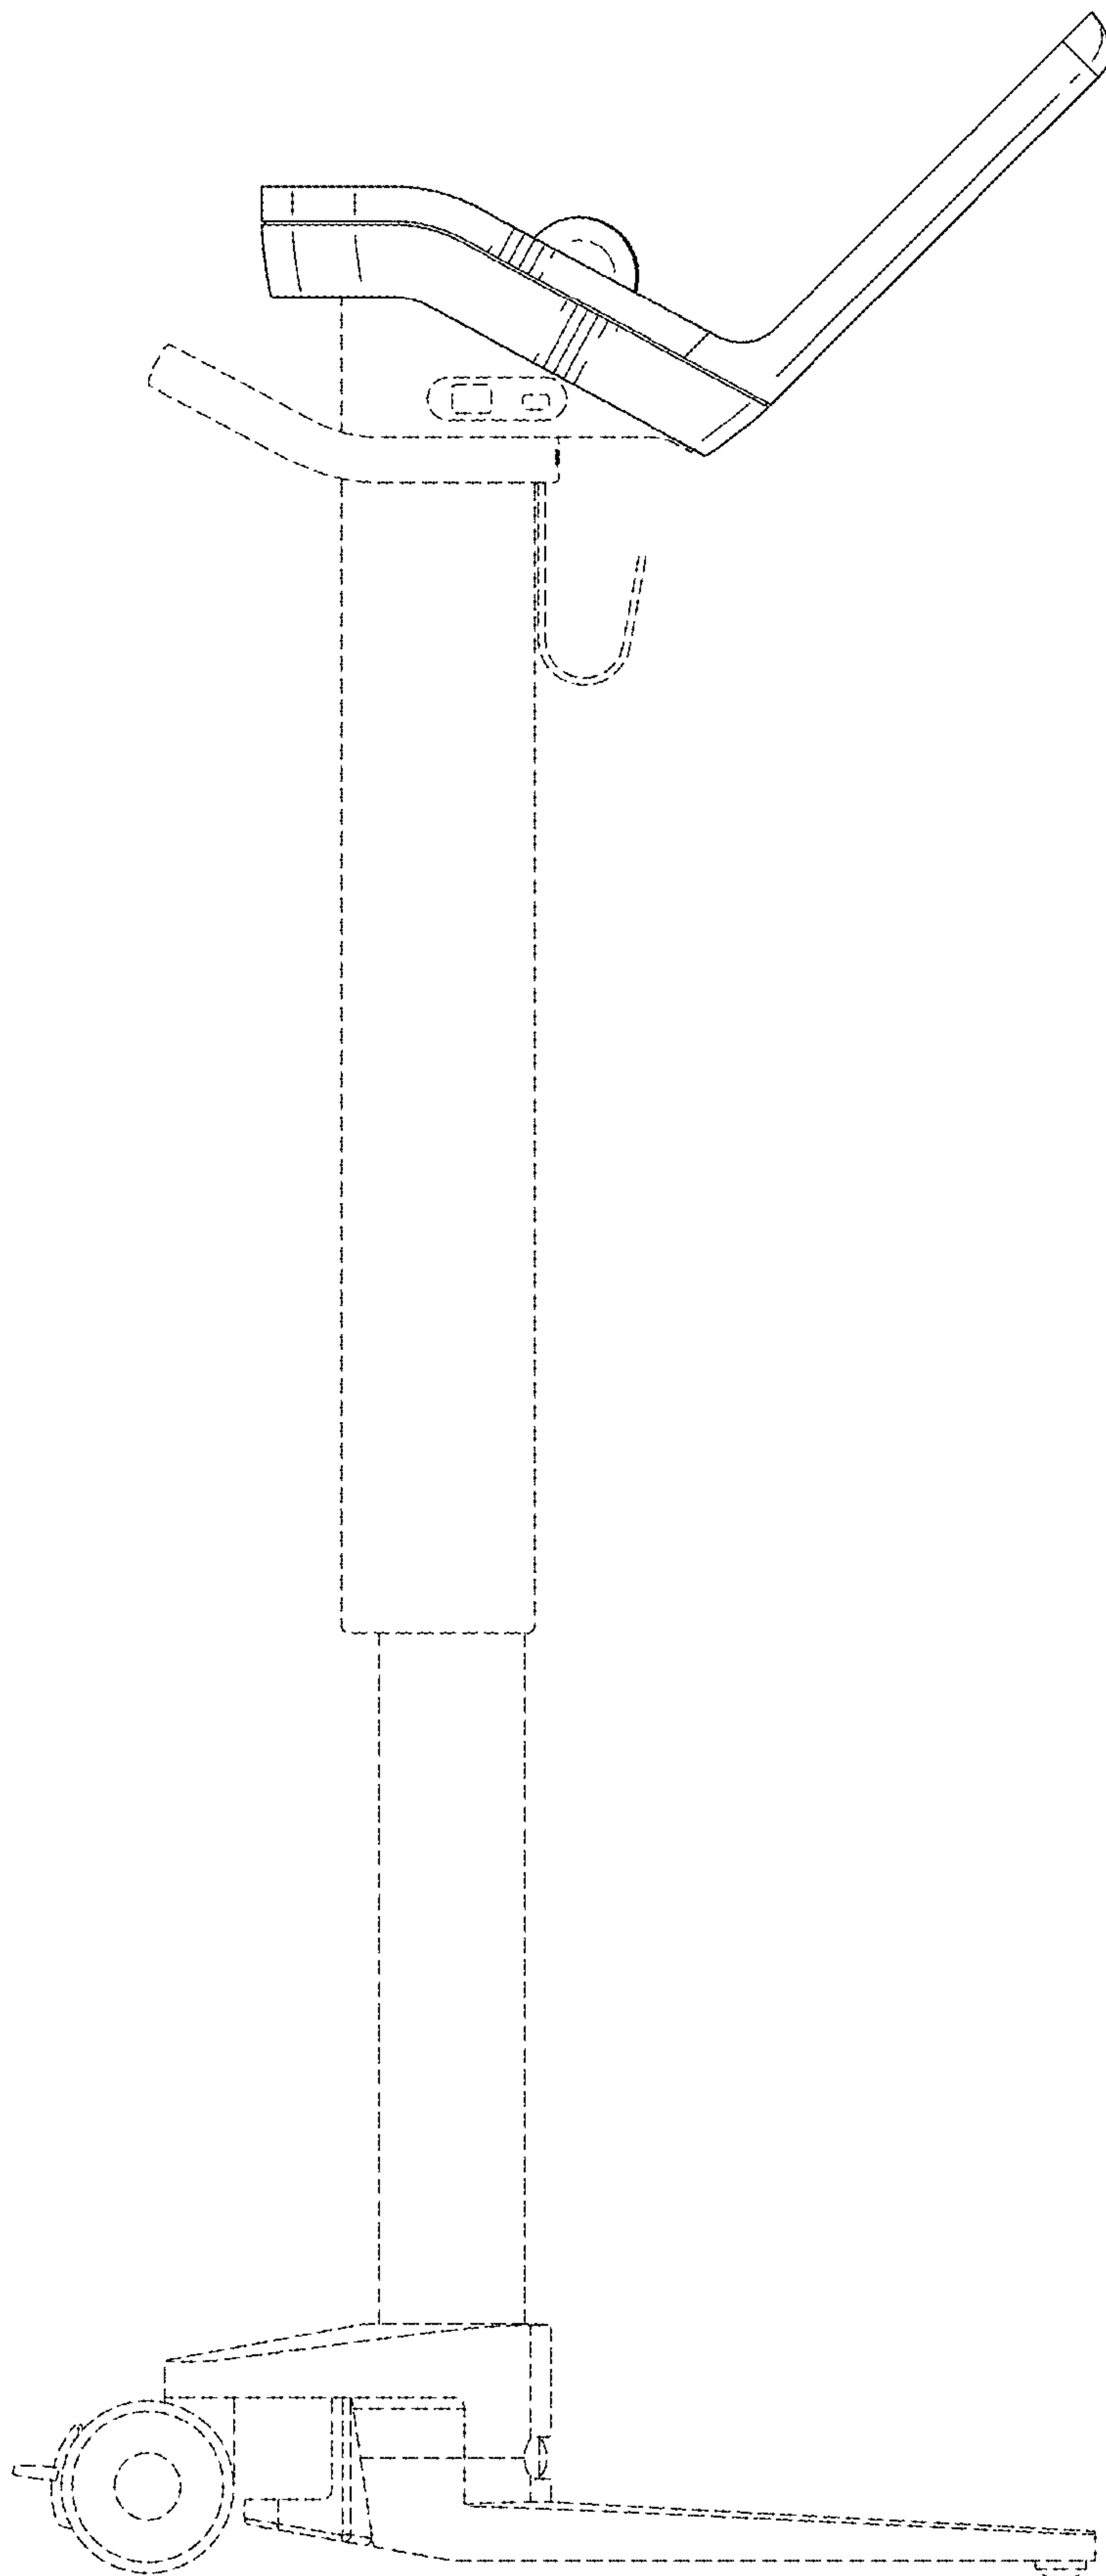


Fig. 4



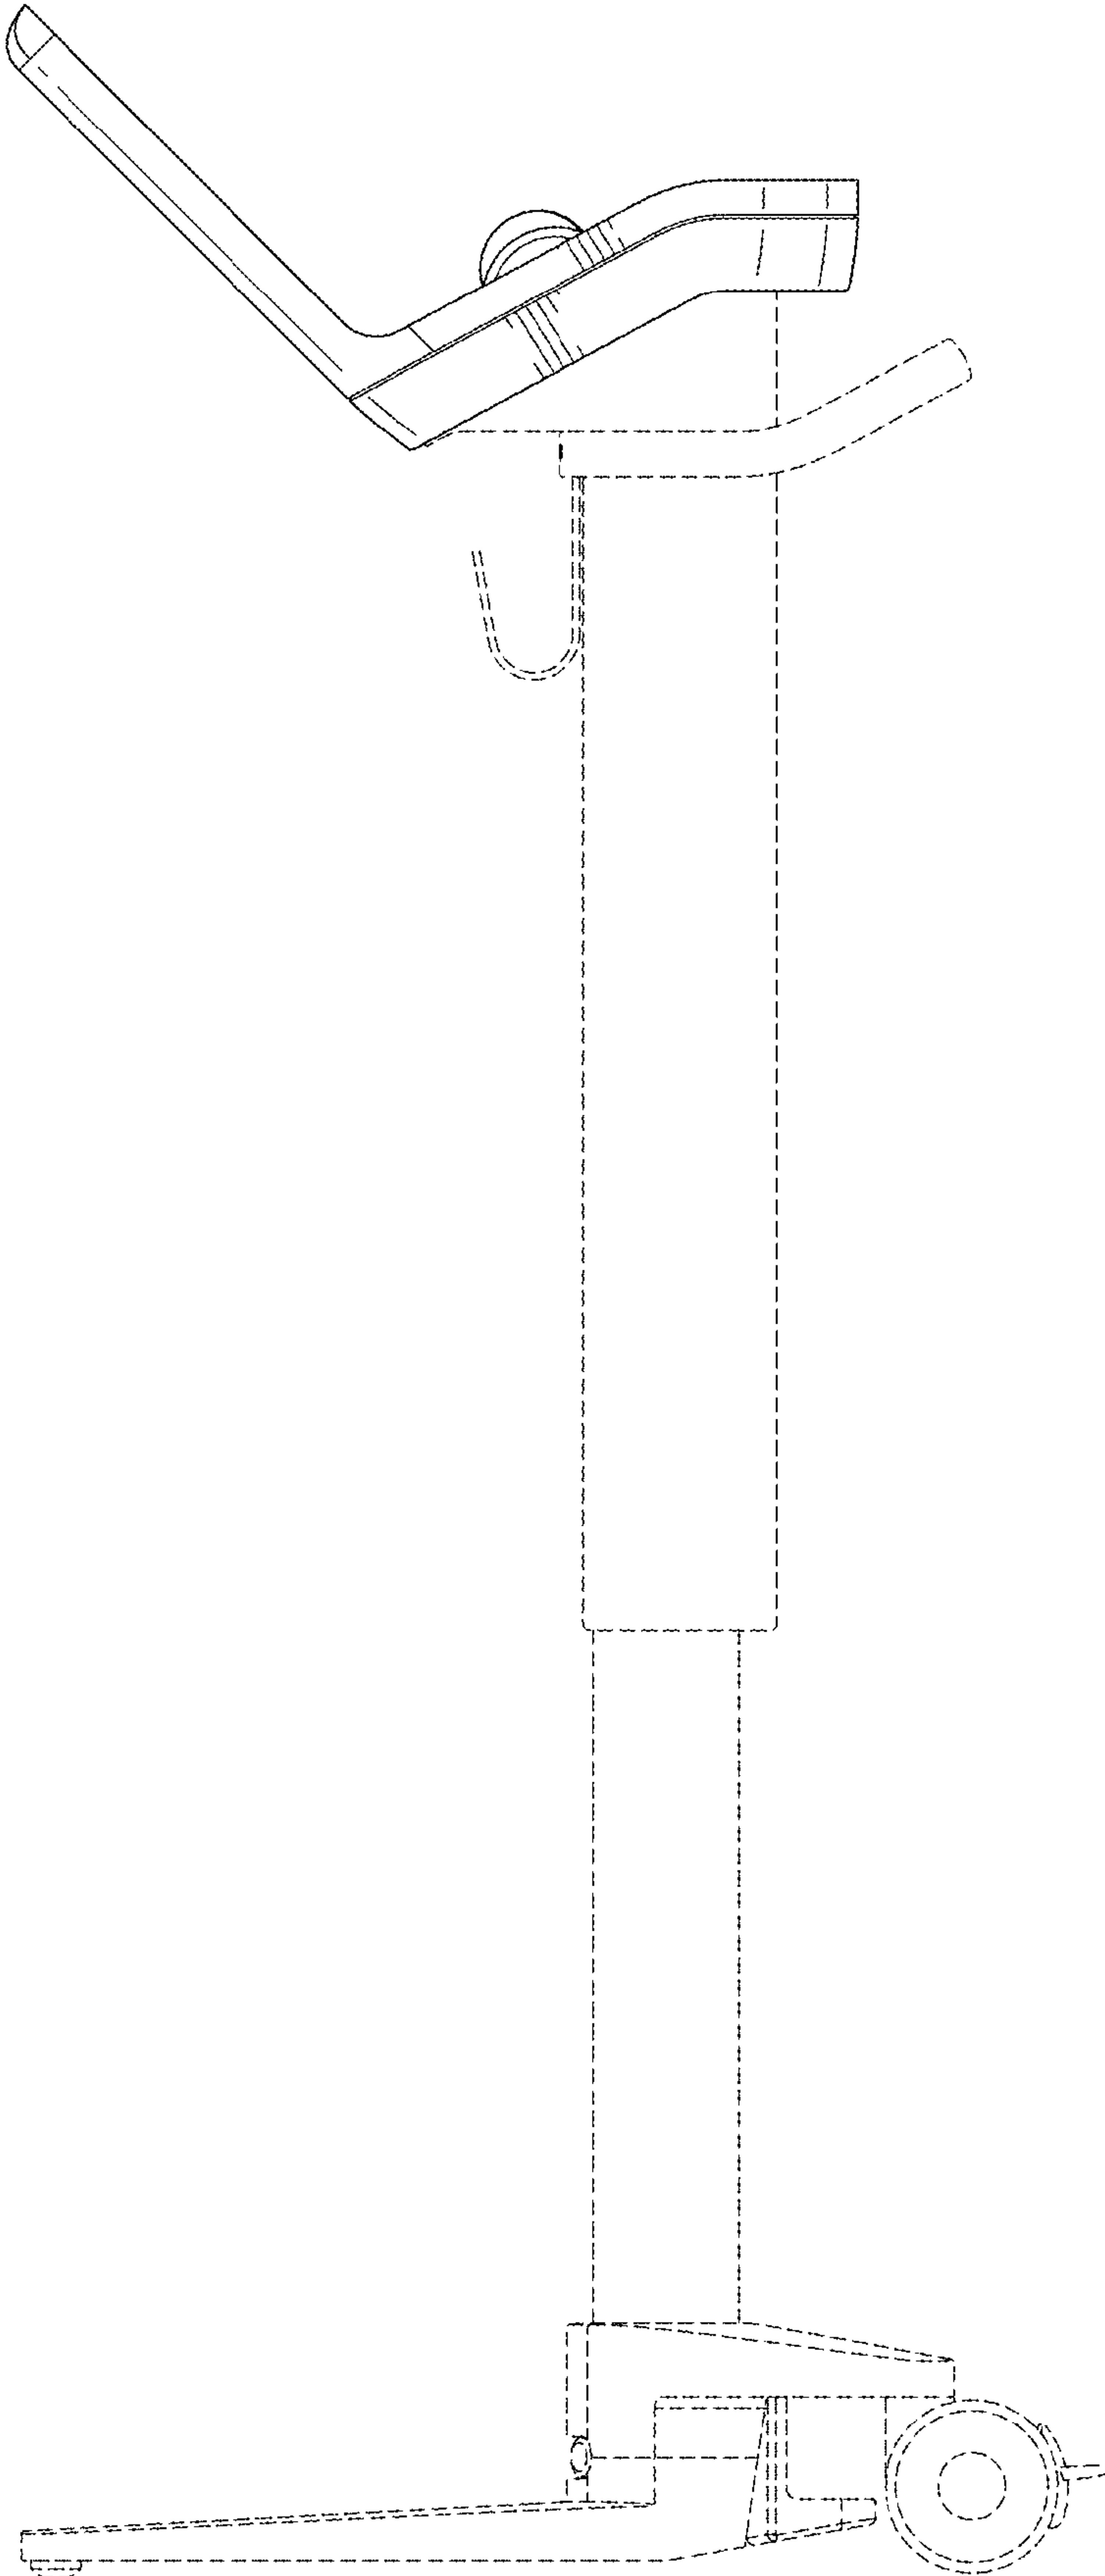


Fig. 5

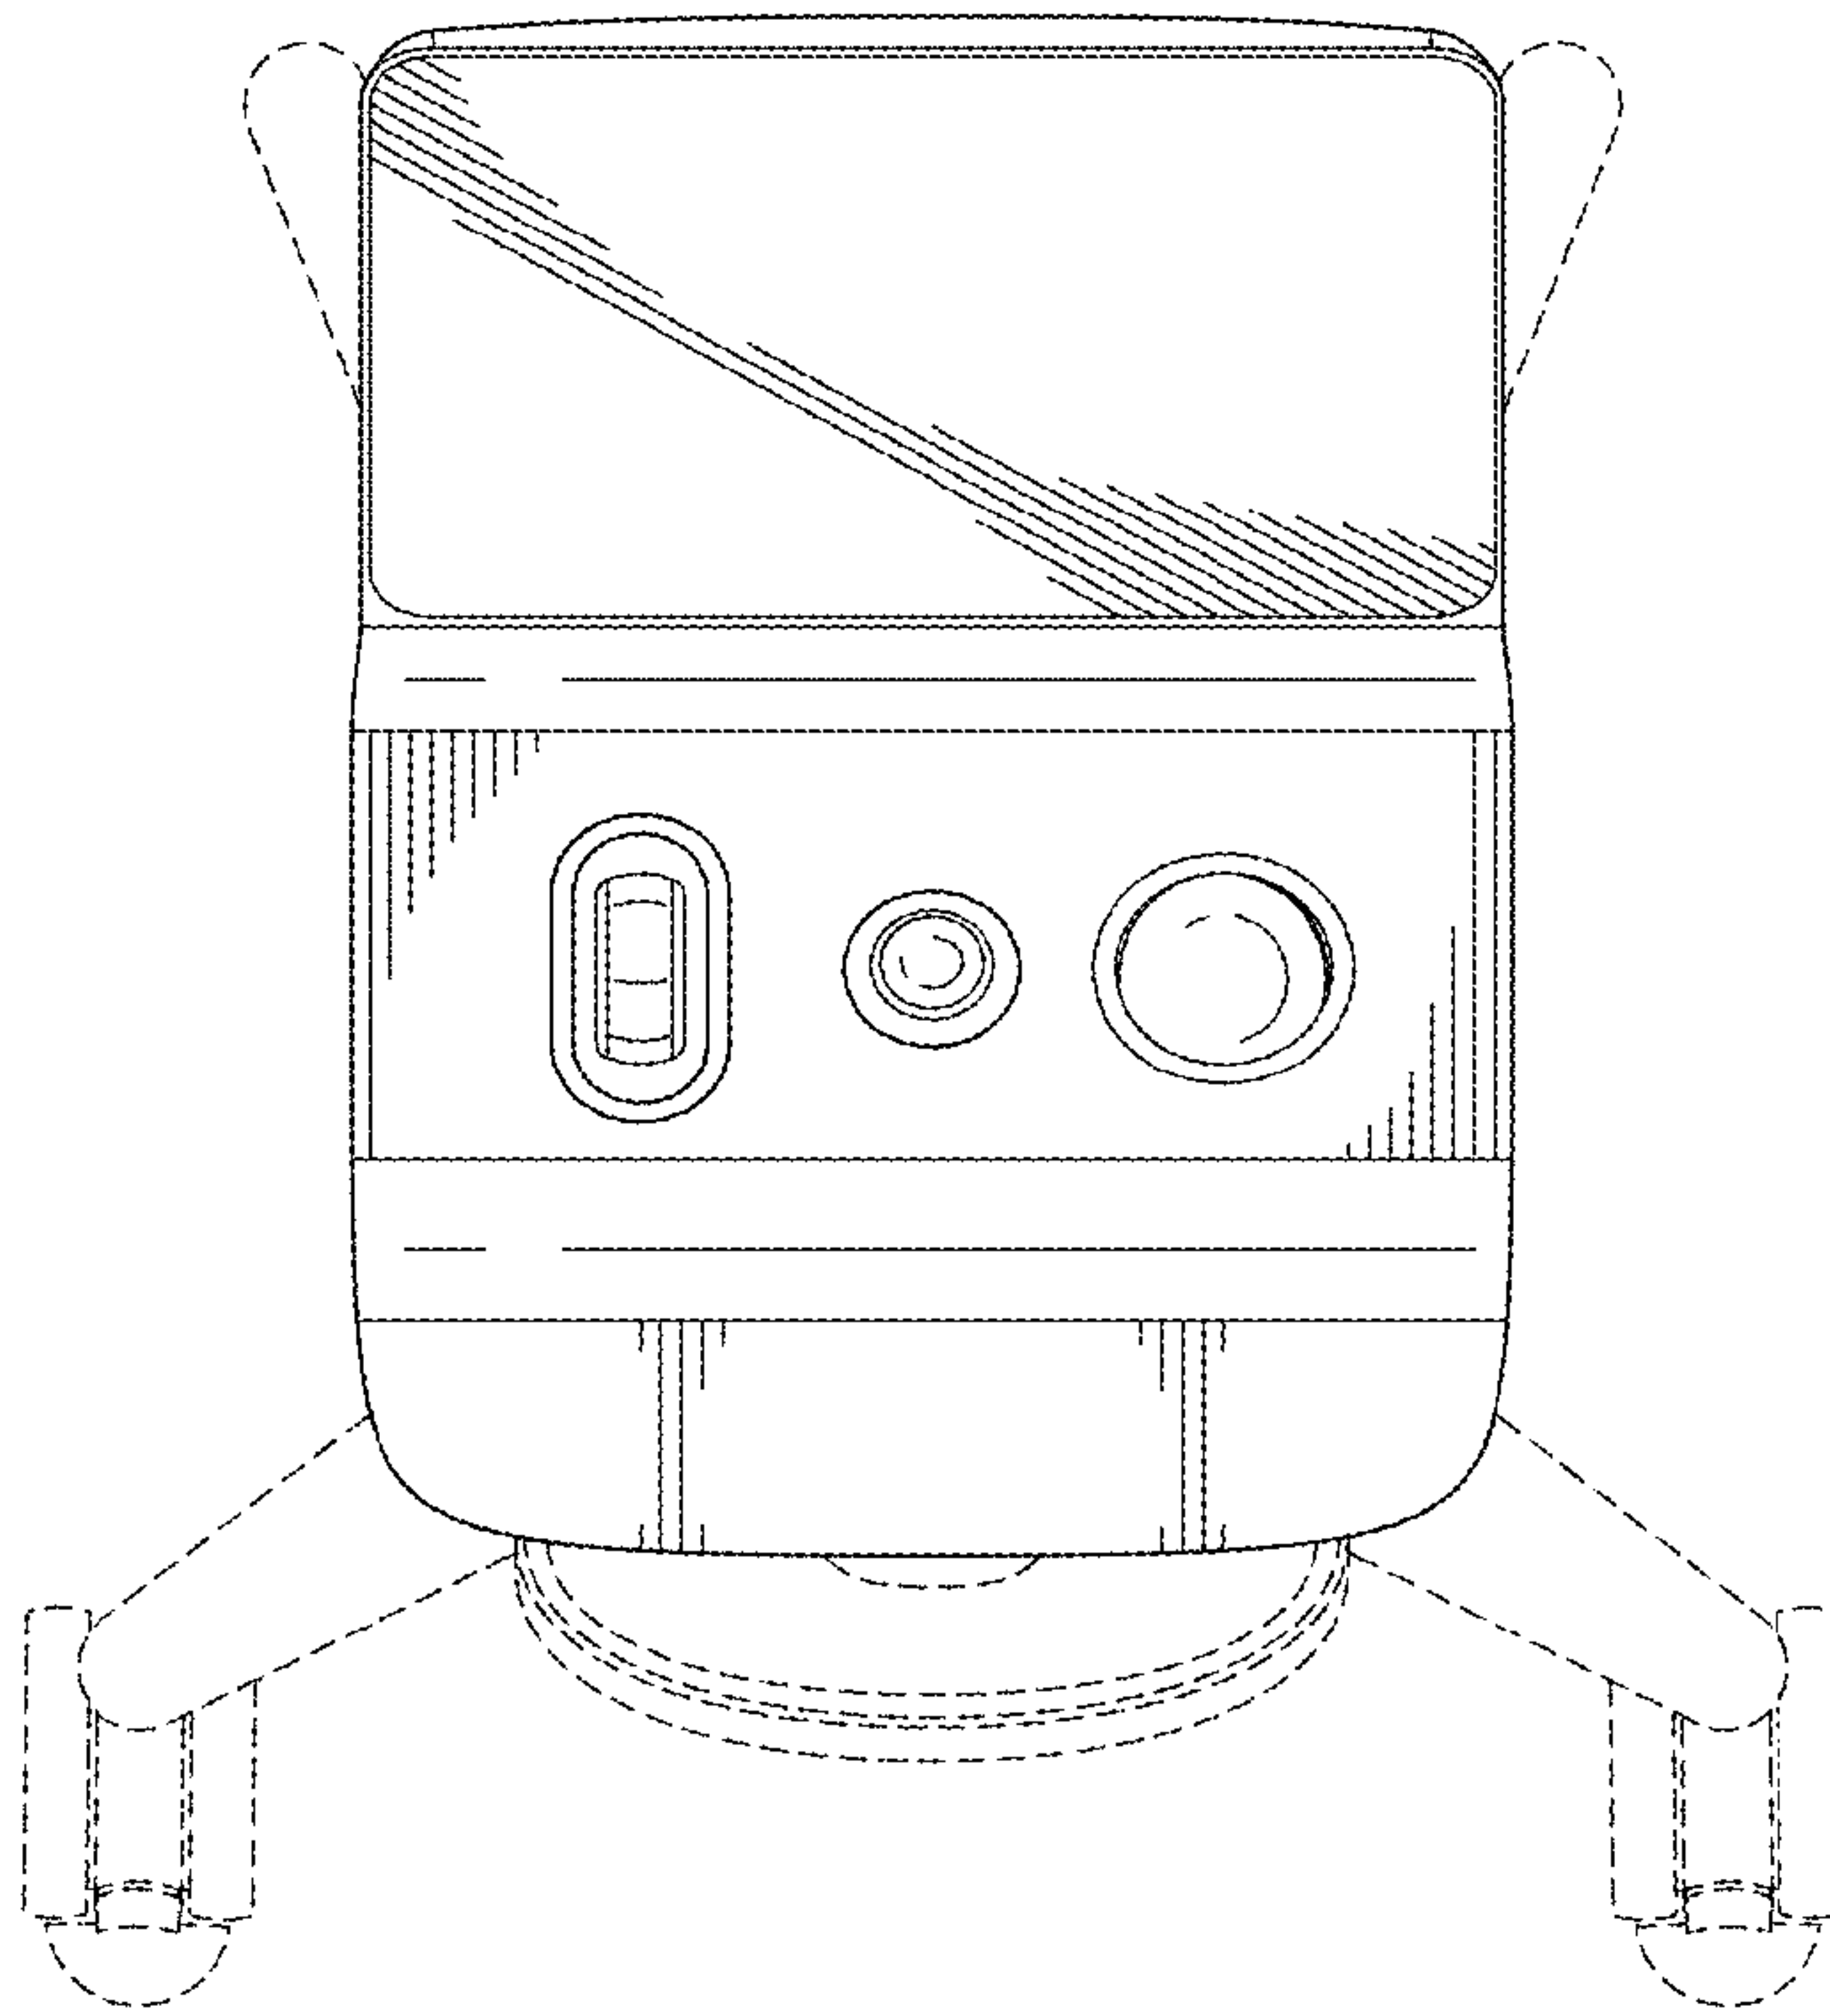


Fig. 6

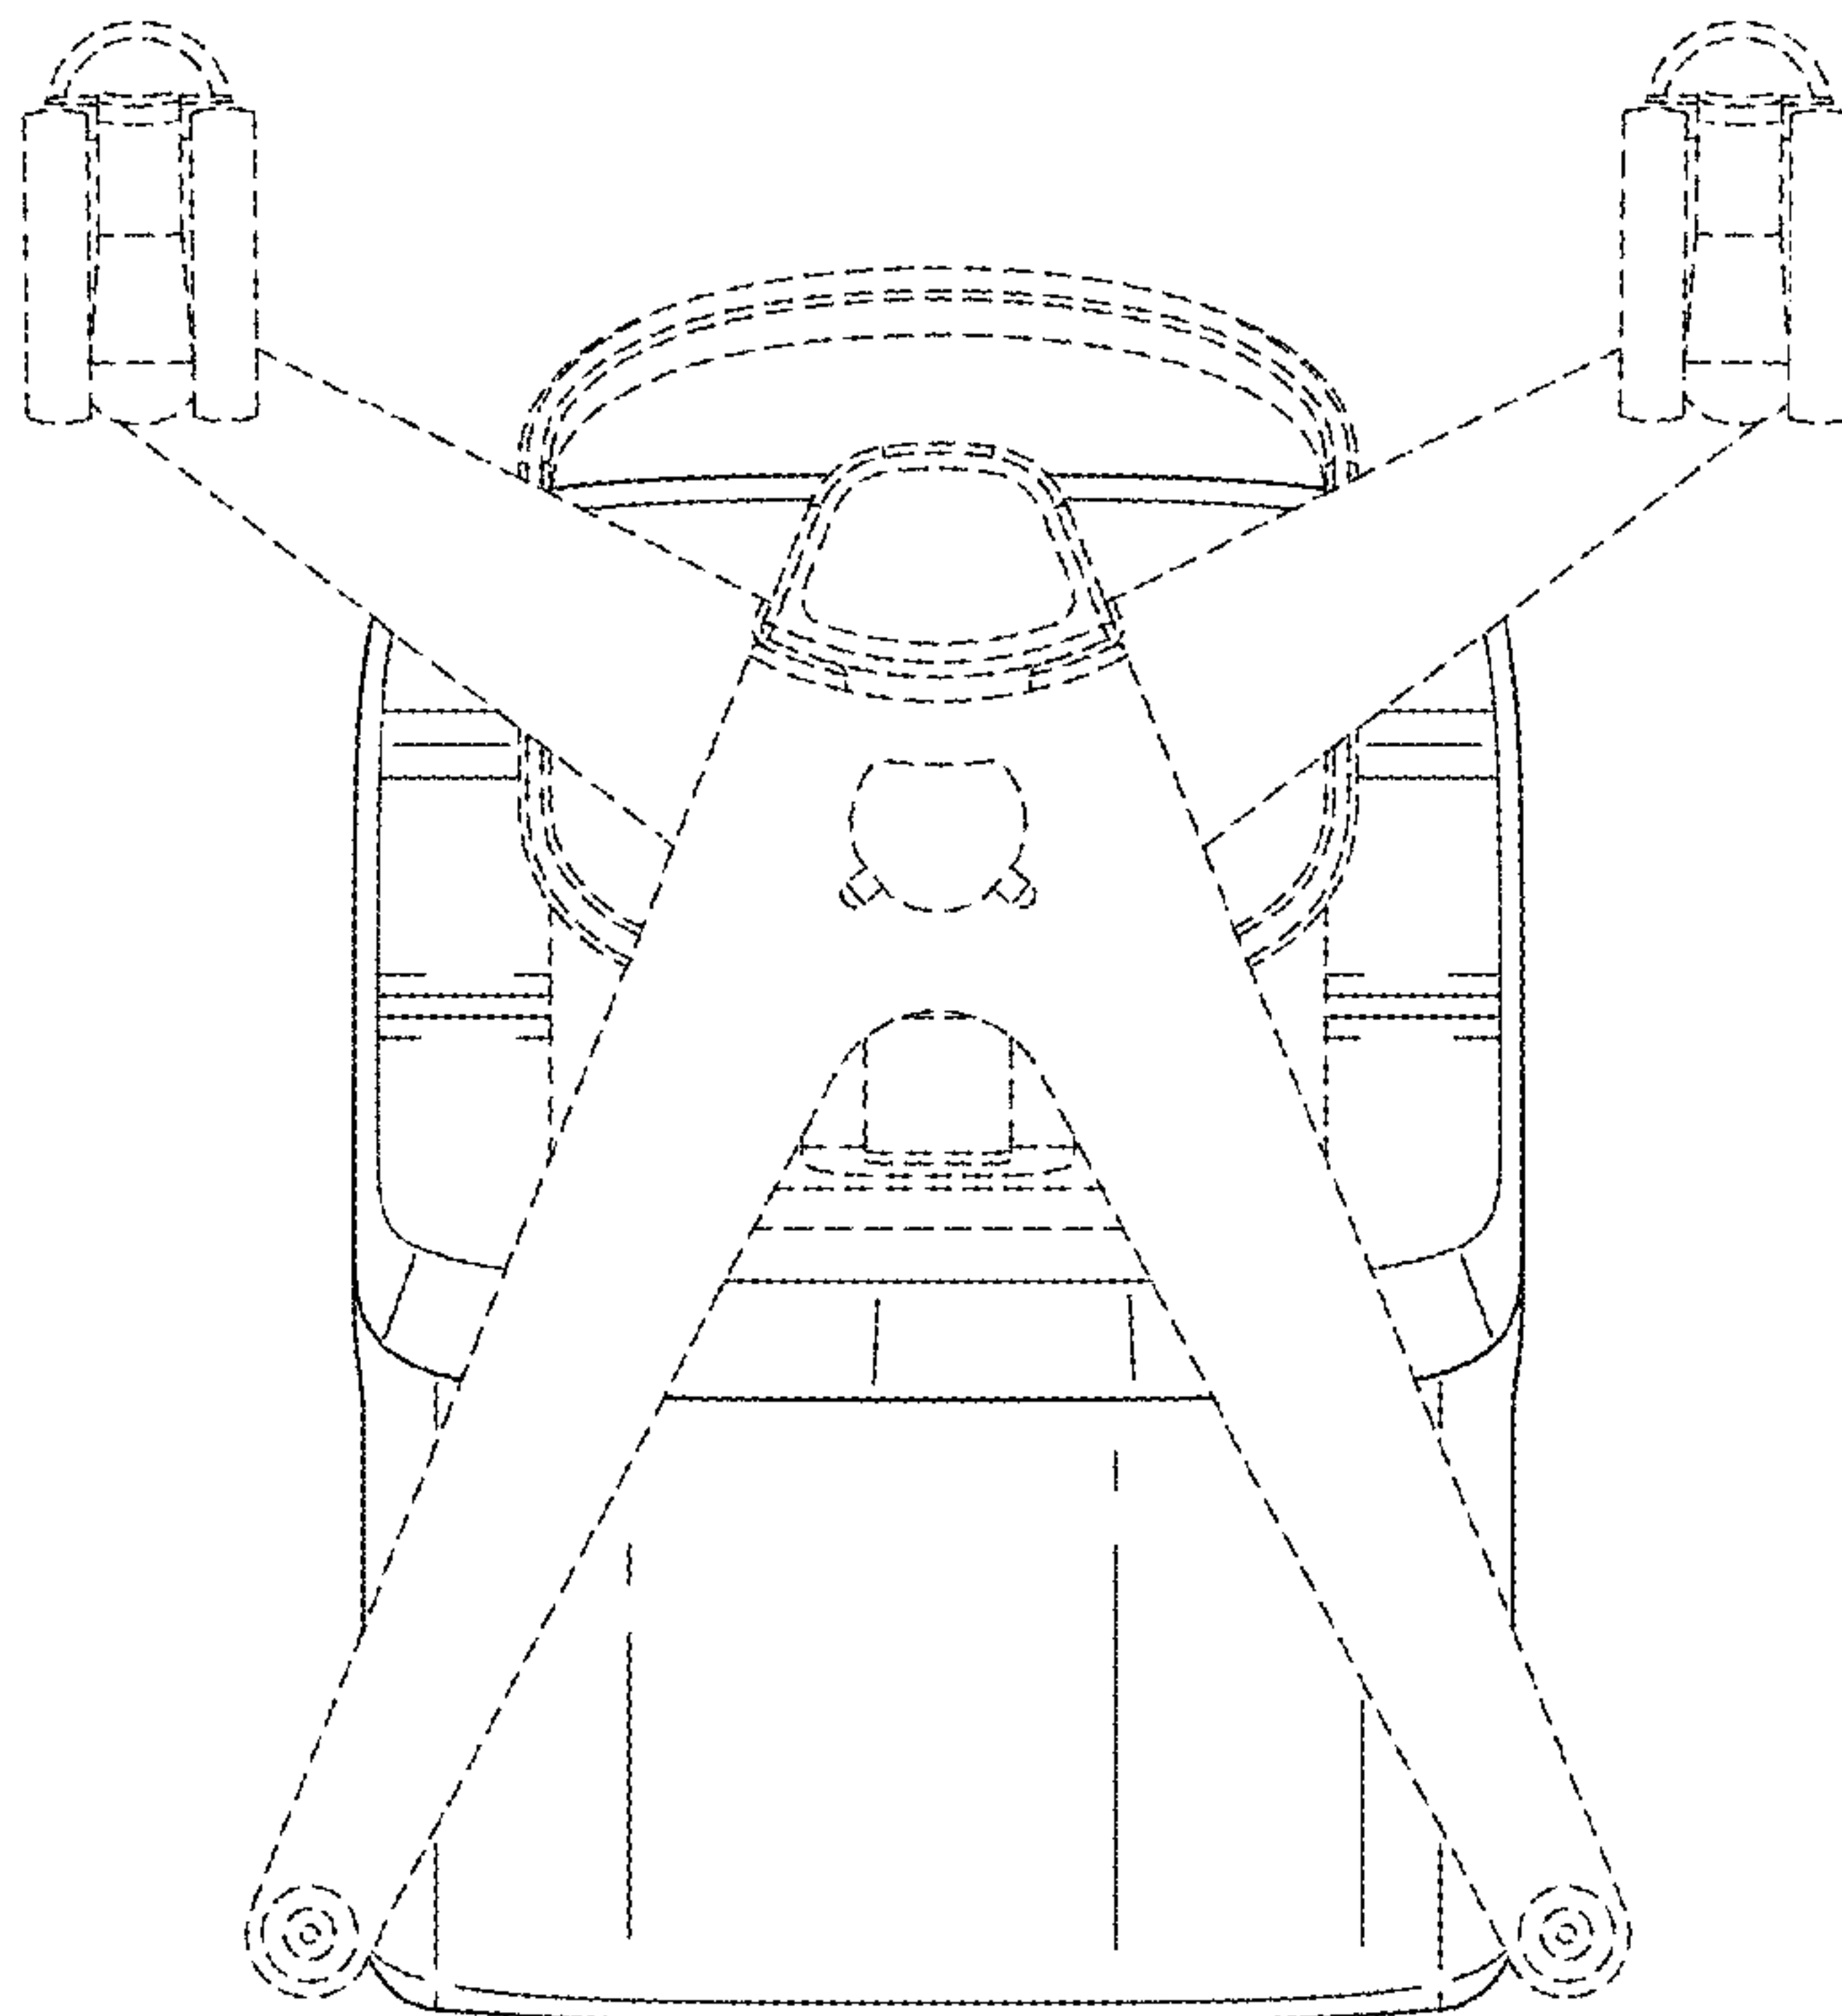


Fig. 7



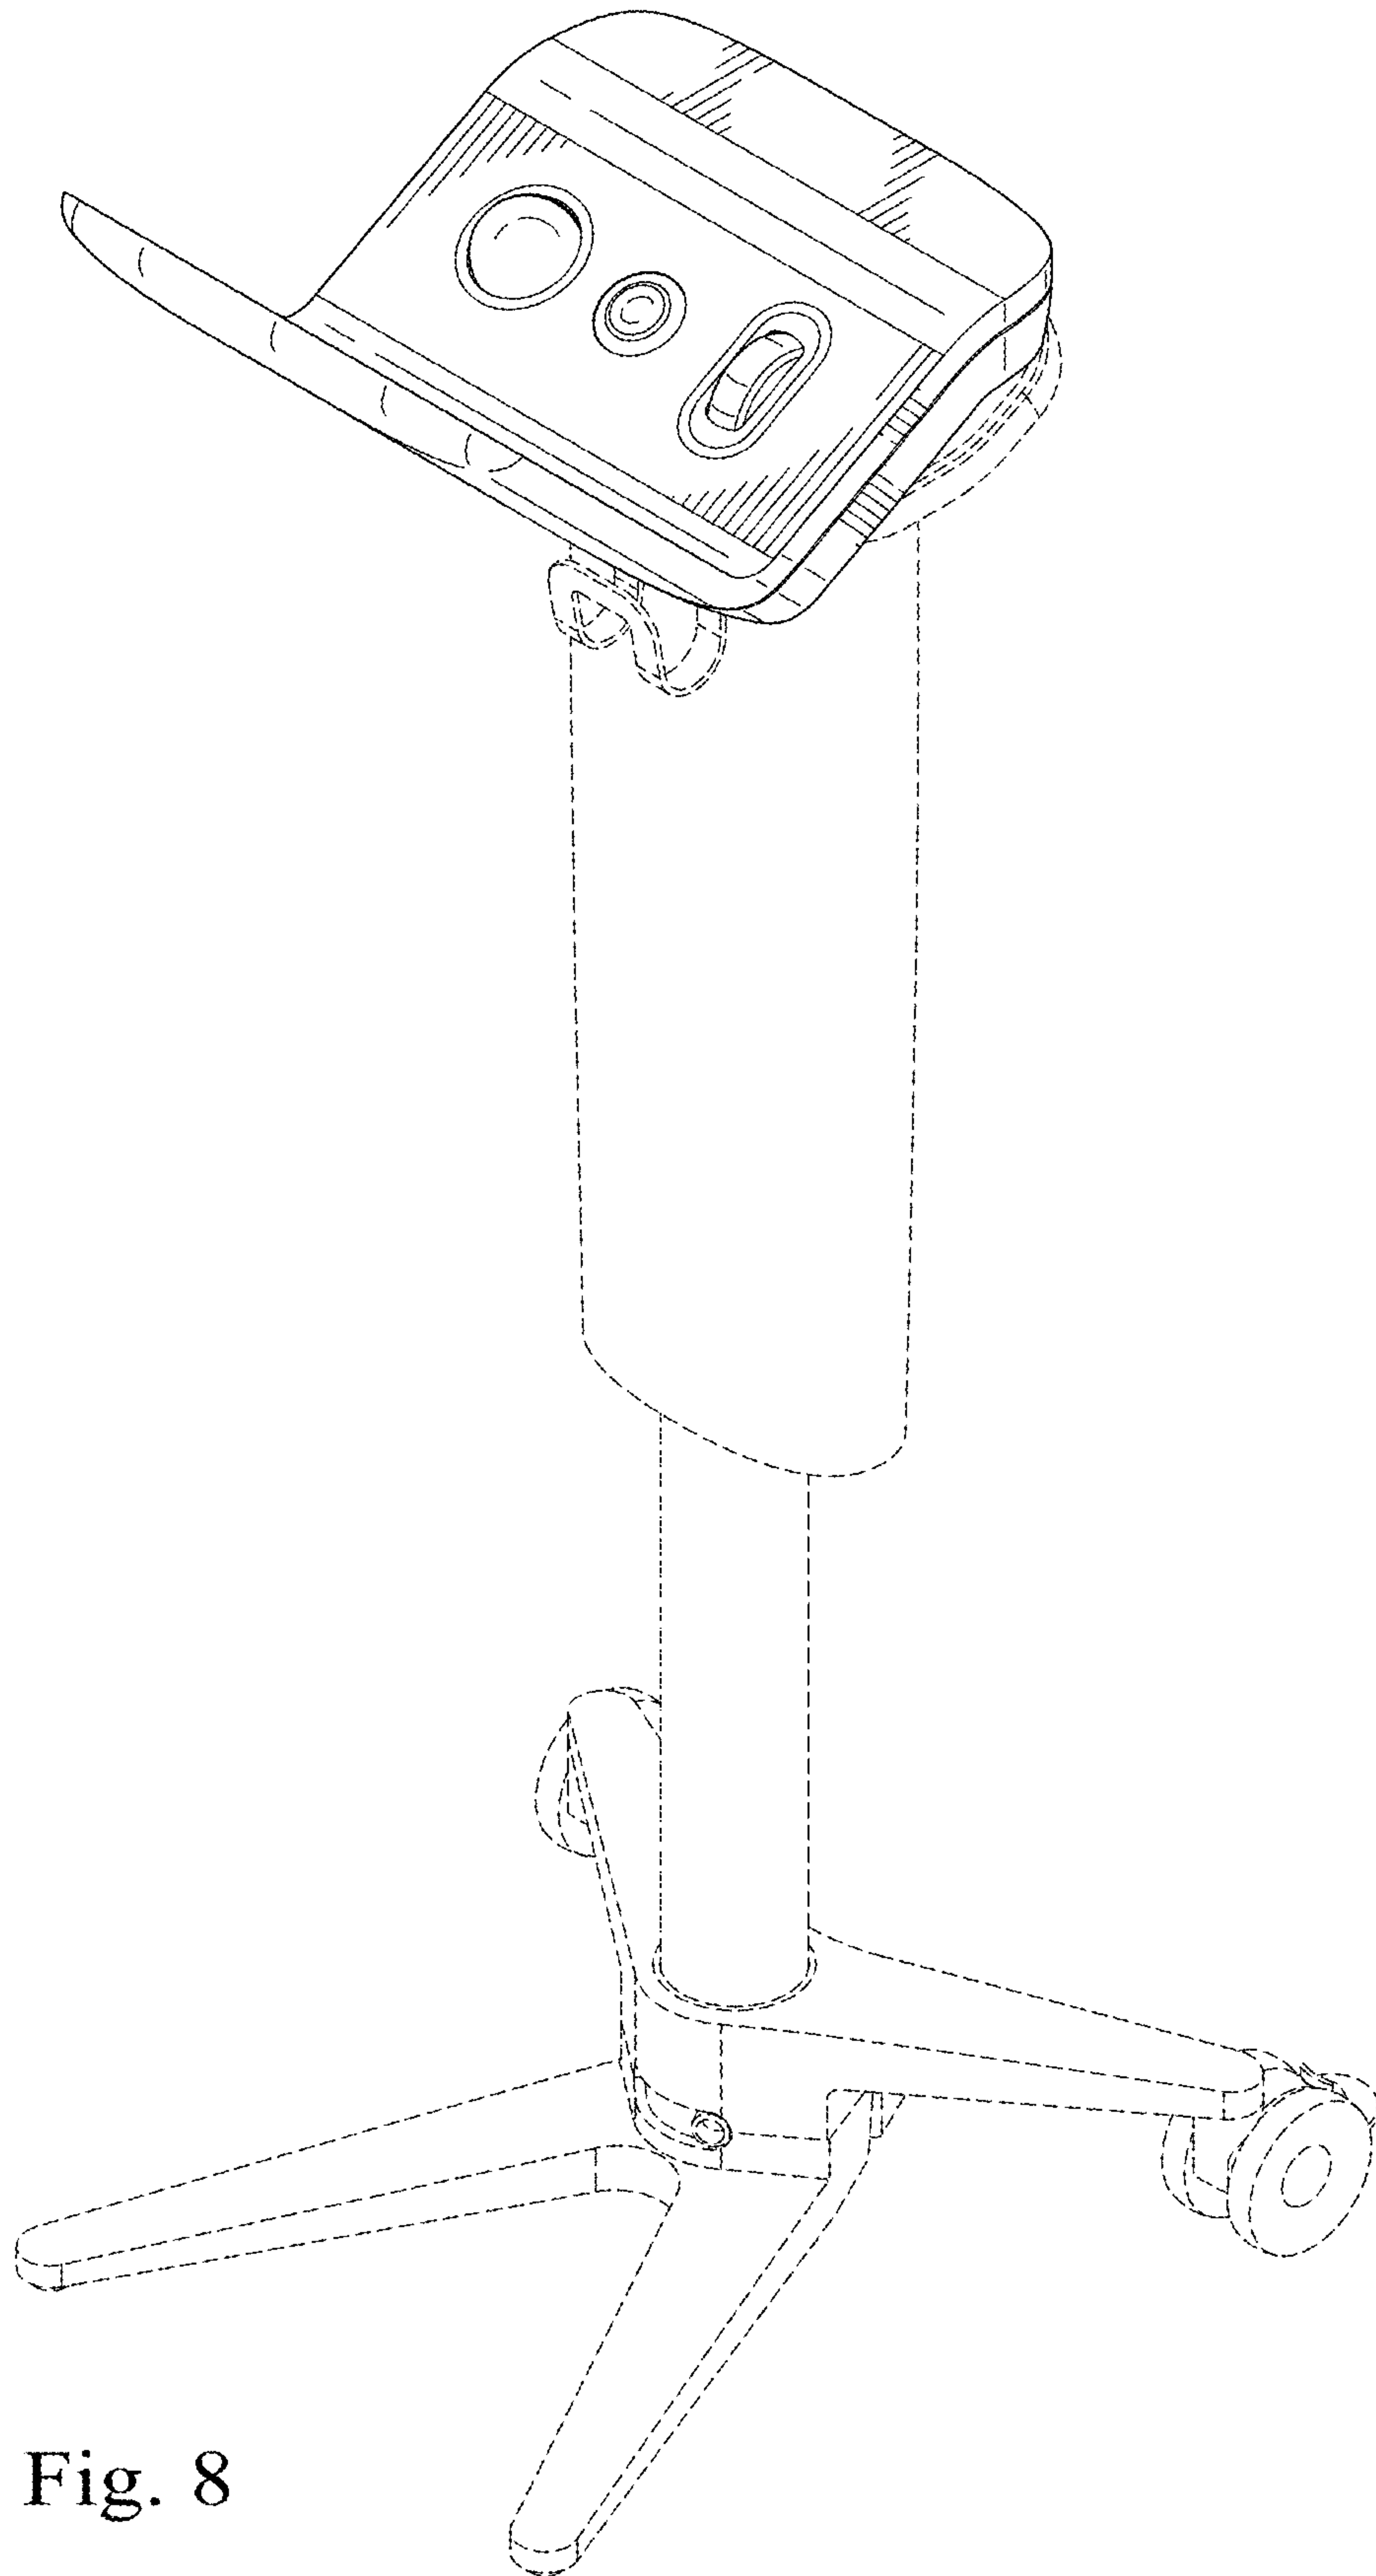


Fig. 8

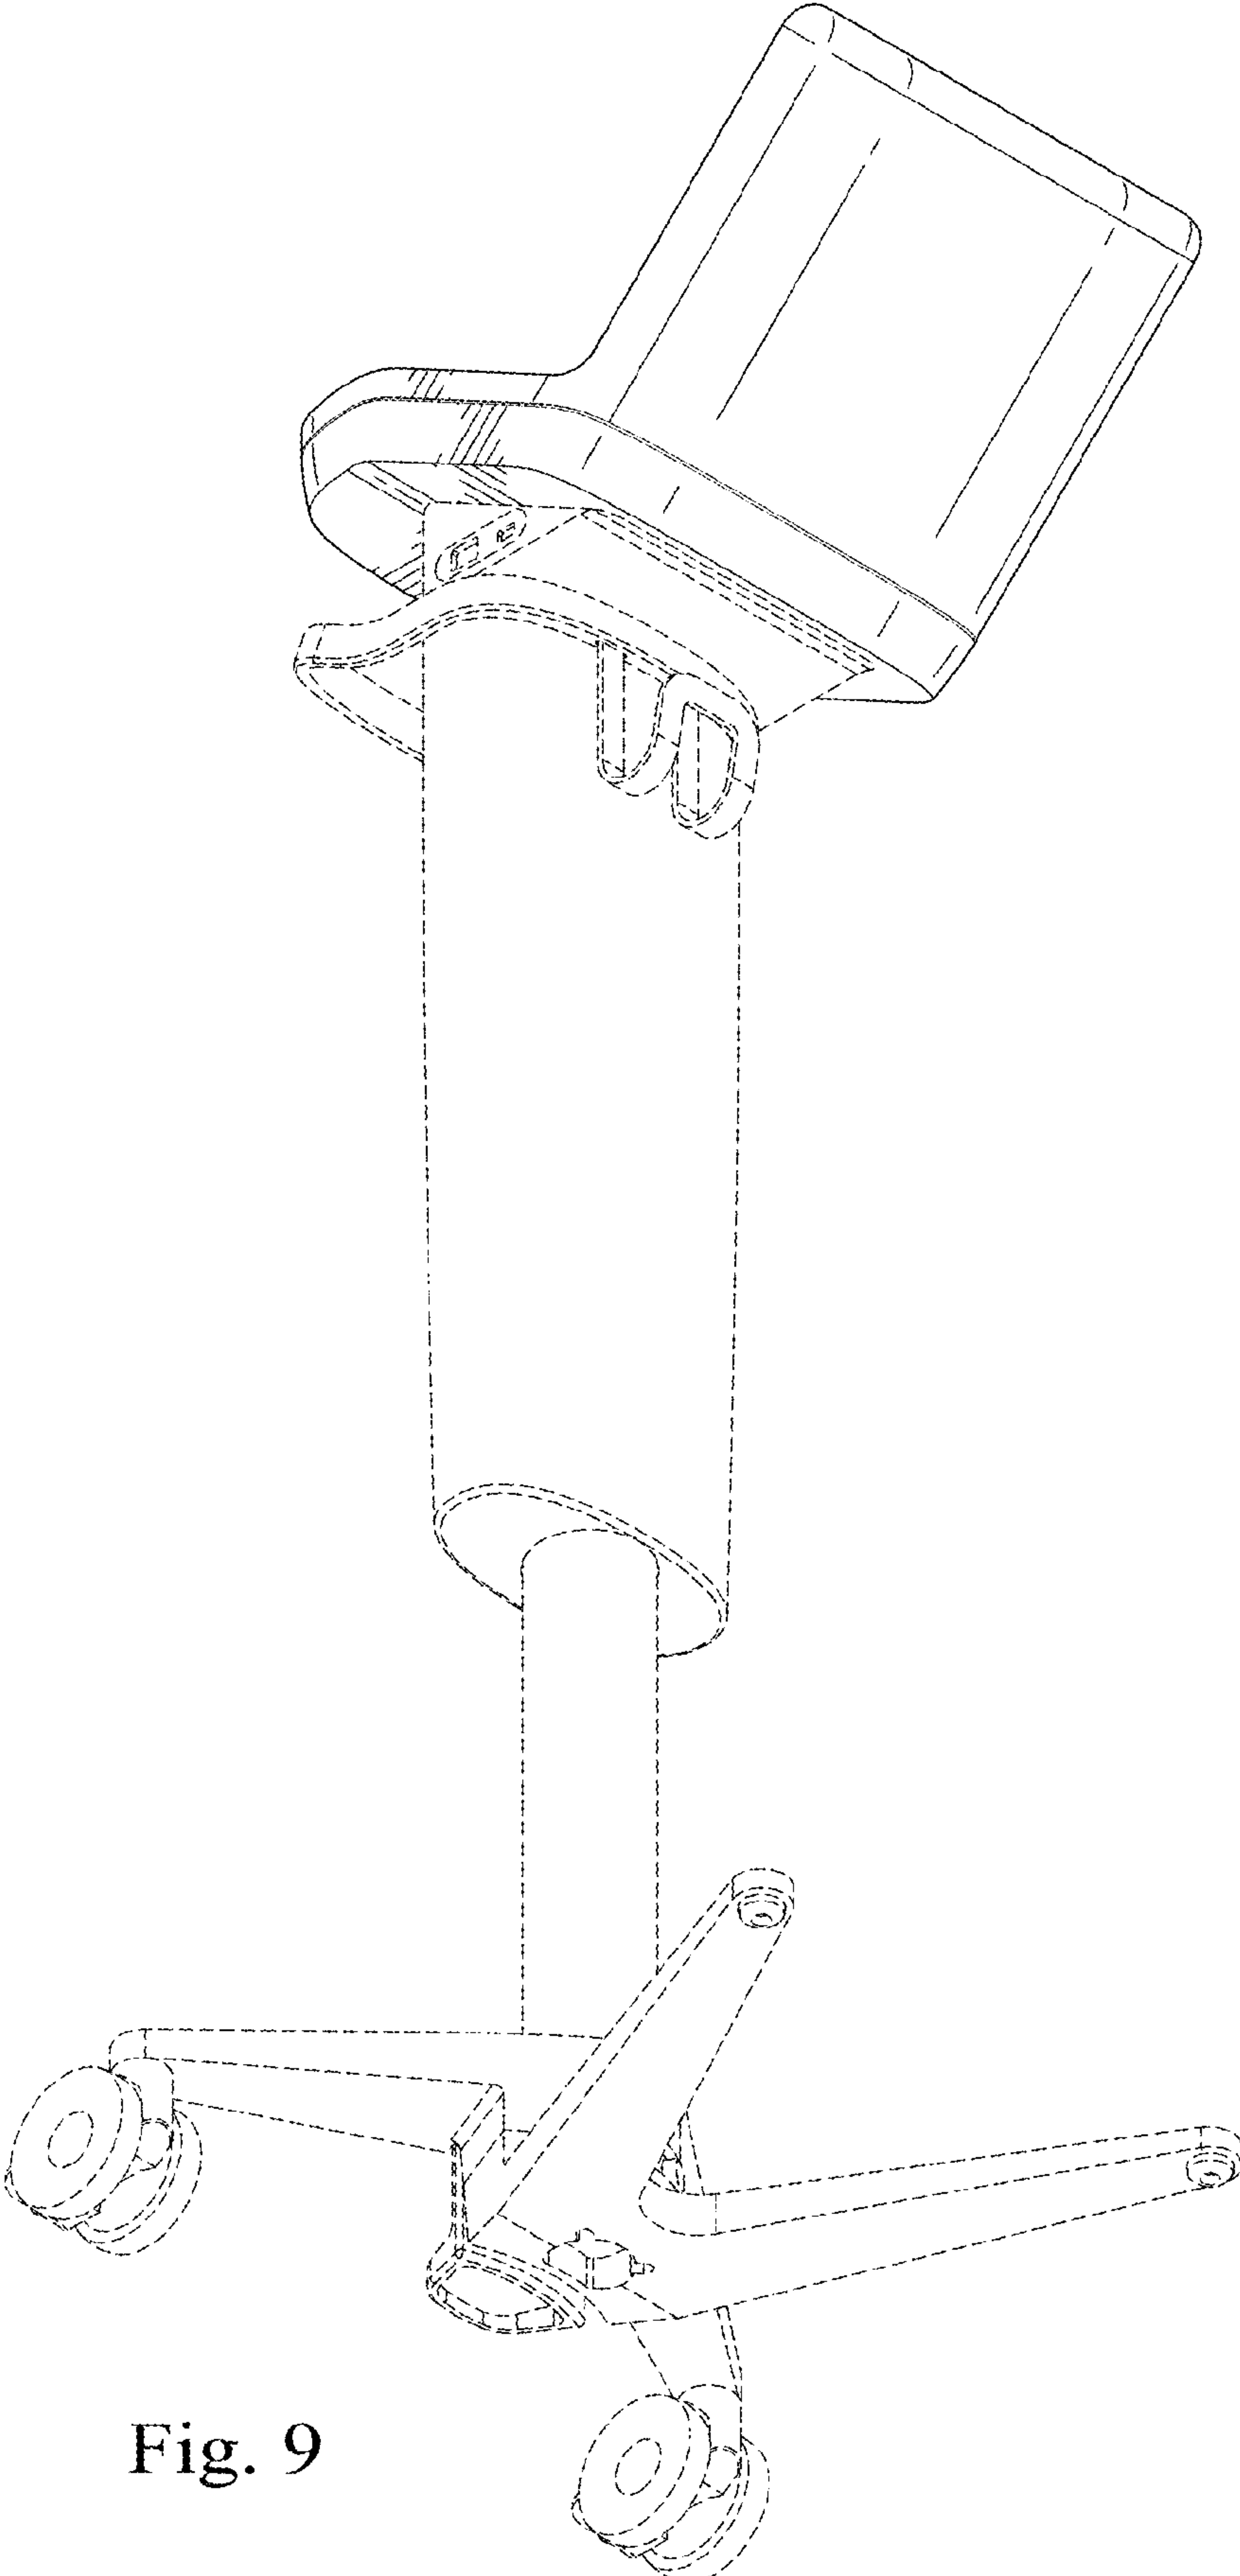


Fig. 9