



US00D908911S

(12) **United States Design Patent** (10) **Patent No.:** **US D908,911 S**
Reavis, Jr. et al. (45) **Date of Patent:** **** Jan. 26, 2021**

(54) **ANALYZING INSTRUMENT AND DISPLAY MONITOR IN COMBINATION**

(71) Applicant: **Siemens Healthcare Diagnostics Inc.**,
Tarrytown, NY (US)

(72) Inventors: **Philip Reavis, Jr.**, Somerville, MA
(US); **William Chura**, Newton, MA
(US); **Prabhu Ramachandran**,
Newton, MA (US)

(73) Assignee: **Siemens Healthcare Diagnostics Inc.**,
Tarrytown, NY (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/692,063**

(22) Filed: **May 22, 2019**

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/107, 169, 186, 216, 219, 231, 232;
D10/81

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D609,350 S * 2/2010 Hickey D24/186
D617,461 S * 6/2010 Kaushal D24/169

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dunlap Coddling P.C.

(57) **CLAIM**

The ornamental design for an analyzing instrument and display monitor in combination, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or application with

color drawings will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is an exploded, front perspective view of a first embodiment of an analyzing instrument and display monitor in combination showing our new design, with the display monitor shown detached from the analyzing instrument.

FIG. 2 is a front perspective view of the analyzing instrument and display monitor in combination of FIG. 1, with the display monitor shown attached to the analyzing instrument.

FIG. 3 is a front elevational view thereof.

FIG. 4 is a rear elevational view thereof.

FIG. 5 is a left side elevational view thereof.

FIG. 6 is a right side elevational view thereof.

FIG. 7 is a top plan view thereof.

FIG. 8 is a bottom plan view thereof.

FIG. 9 is an exploded, front perspective view of a second embodiment of an analyzing instrument and display monitor in combination showing our new design, with the display monitor shown detached from the analyzing instrument.

FIG. 10 is a front perspective view of the analyzing instrument and display monitor in combination of FIG. 9, with the display monitor shown attached to the analyzing instrument.

FIG. 11 is a front elevational view thereof.

FIG. 12 is a rear elevational view thereof.

FIG. 13 is a left side elevational view thereof.

FIG. 14 is a right side elevational view thereof.

FIG. 15 is a top plan view thereof.

FIG. 16 is a bottom plan view thereof.

FIG. 17 is an exploded, front perspective view of a third embodiment of an analyzing instrument and display monitor in combination showing our new design, with the display monitor shown detached from the analyzing instrument.

FIG. 18 is a front perspective view of the analyzing instrument and display monitor in combination of FIG. 17, with the display monitor shown attached to the analyzing instrument.

FIG. 19 is a front elevational view thereof.

FIG. 20 is a rear elevational view thereof.

FIG. 21 is a left side elevational view thereof.


FIG. 22 is a right side elevational view thereof.

FIG. 23 is a top plan view thereof; and,

FIG. 24 is a bottom plan view thereof.

The broken lines depict portions of the analyzing instrument and display monitor in combination that form no part of the

(Continued)

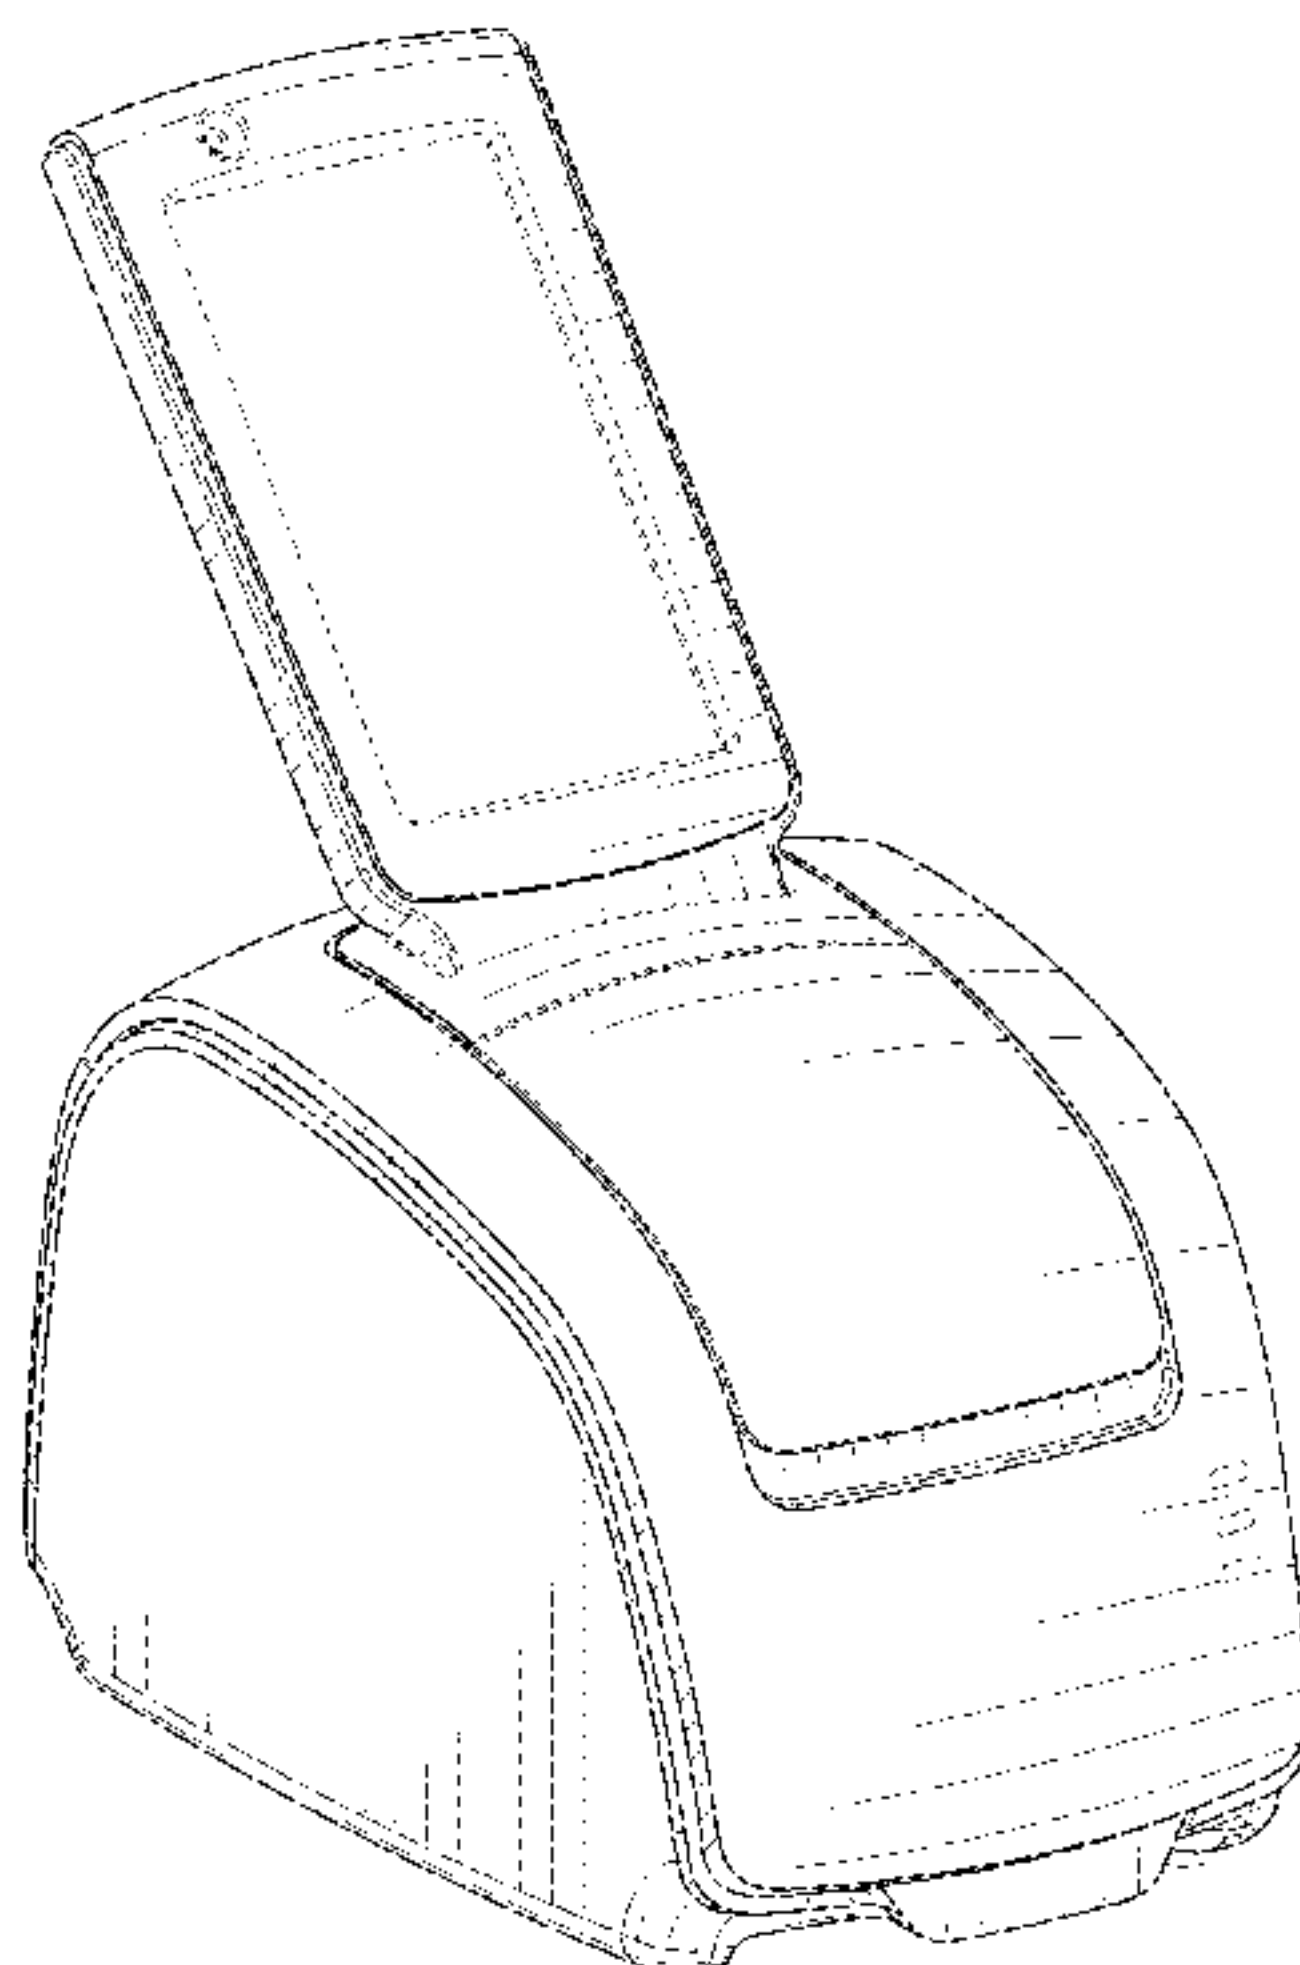

claimed design; the broken lines and the unshaded surfaces form no part of the claimed design. In the drawings, the stippled shading represents surfaces having the contrast in appearance shown.

1 Claim, 24 Drawing Sheets
(8 of 24 Drawing Sheet(s) Filed in Color)

(58) Field of Classification Search

CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76; G01N 33/50; G01N 35/025
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D629,907	S	*	12/2010	Boessneck		D24/169
D647,209	S	*	10/2011	Muller		D24/216
D665,917	S	*	8/2012	TerMaat		D24/216
D729,661	S	*	5/2015	Dickinson		D10/81
D759,519	S	*	6/2016	Apotheloz		D24/232
D843,005	S	*	3/2019	Kobeli		D24/216
D848,020	S	*	5/2019	Kobeli		D24/216
2016/0018426	A1	*	1/2016	Moriya		G01N 35/026 422/65
2016/0030613	A1	*	2/2016	Paul		A61L 2/10 422/24

* cited by examiner

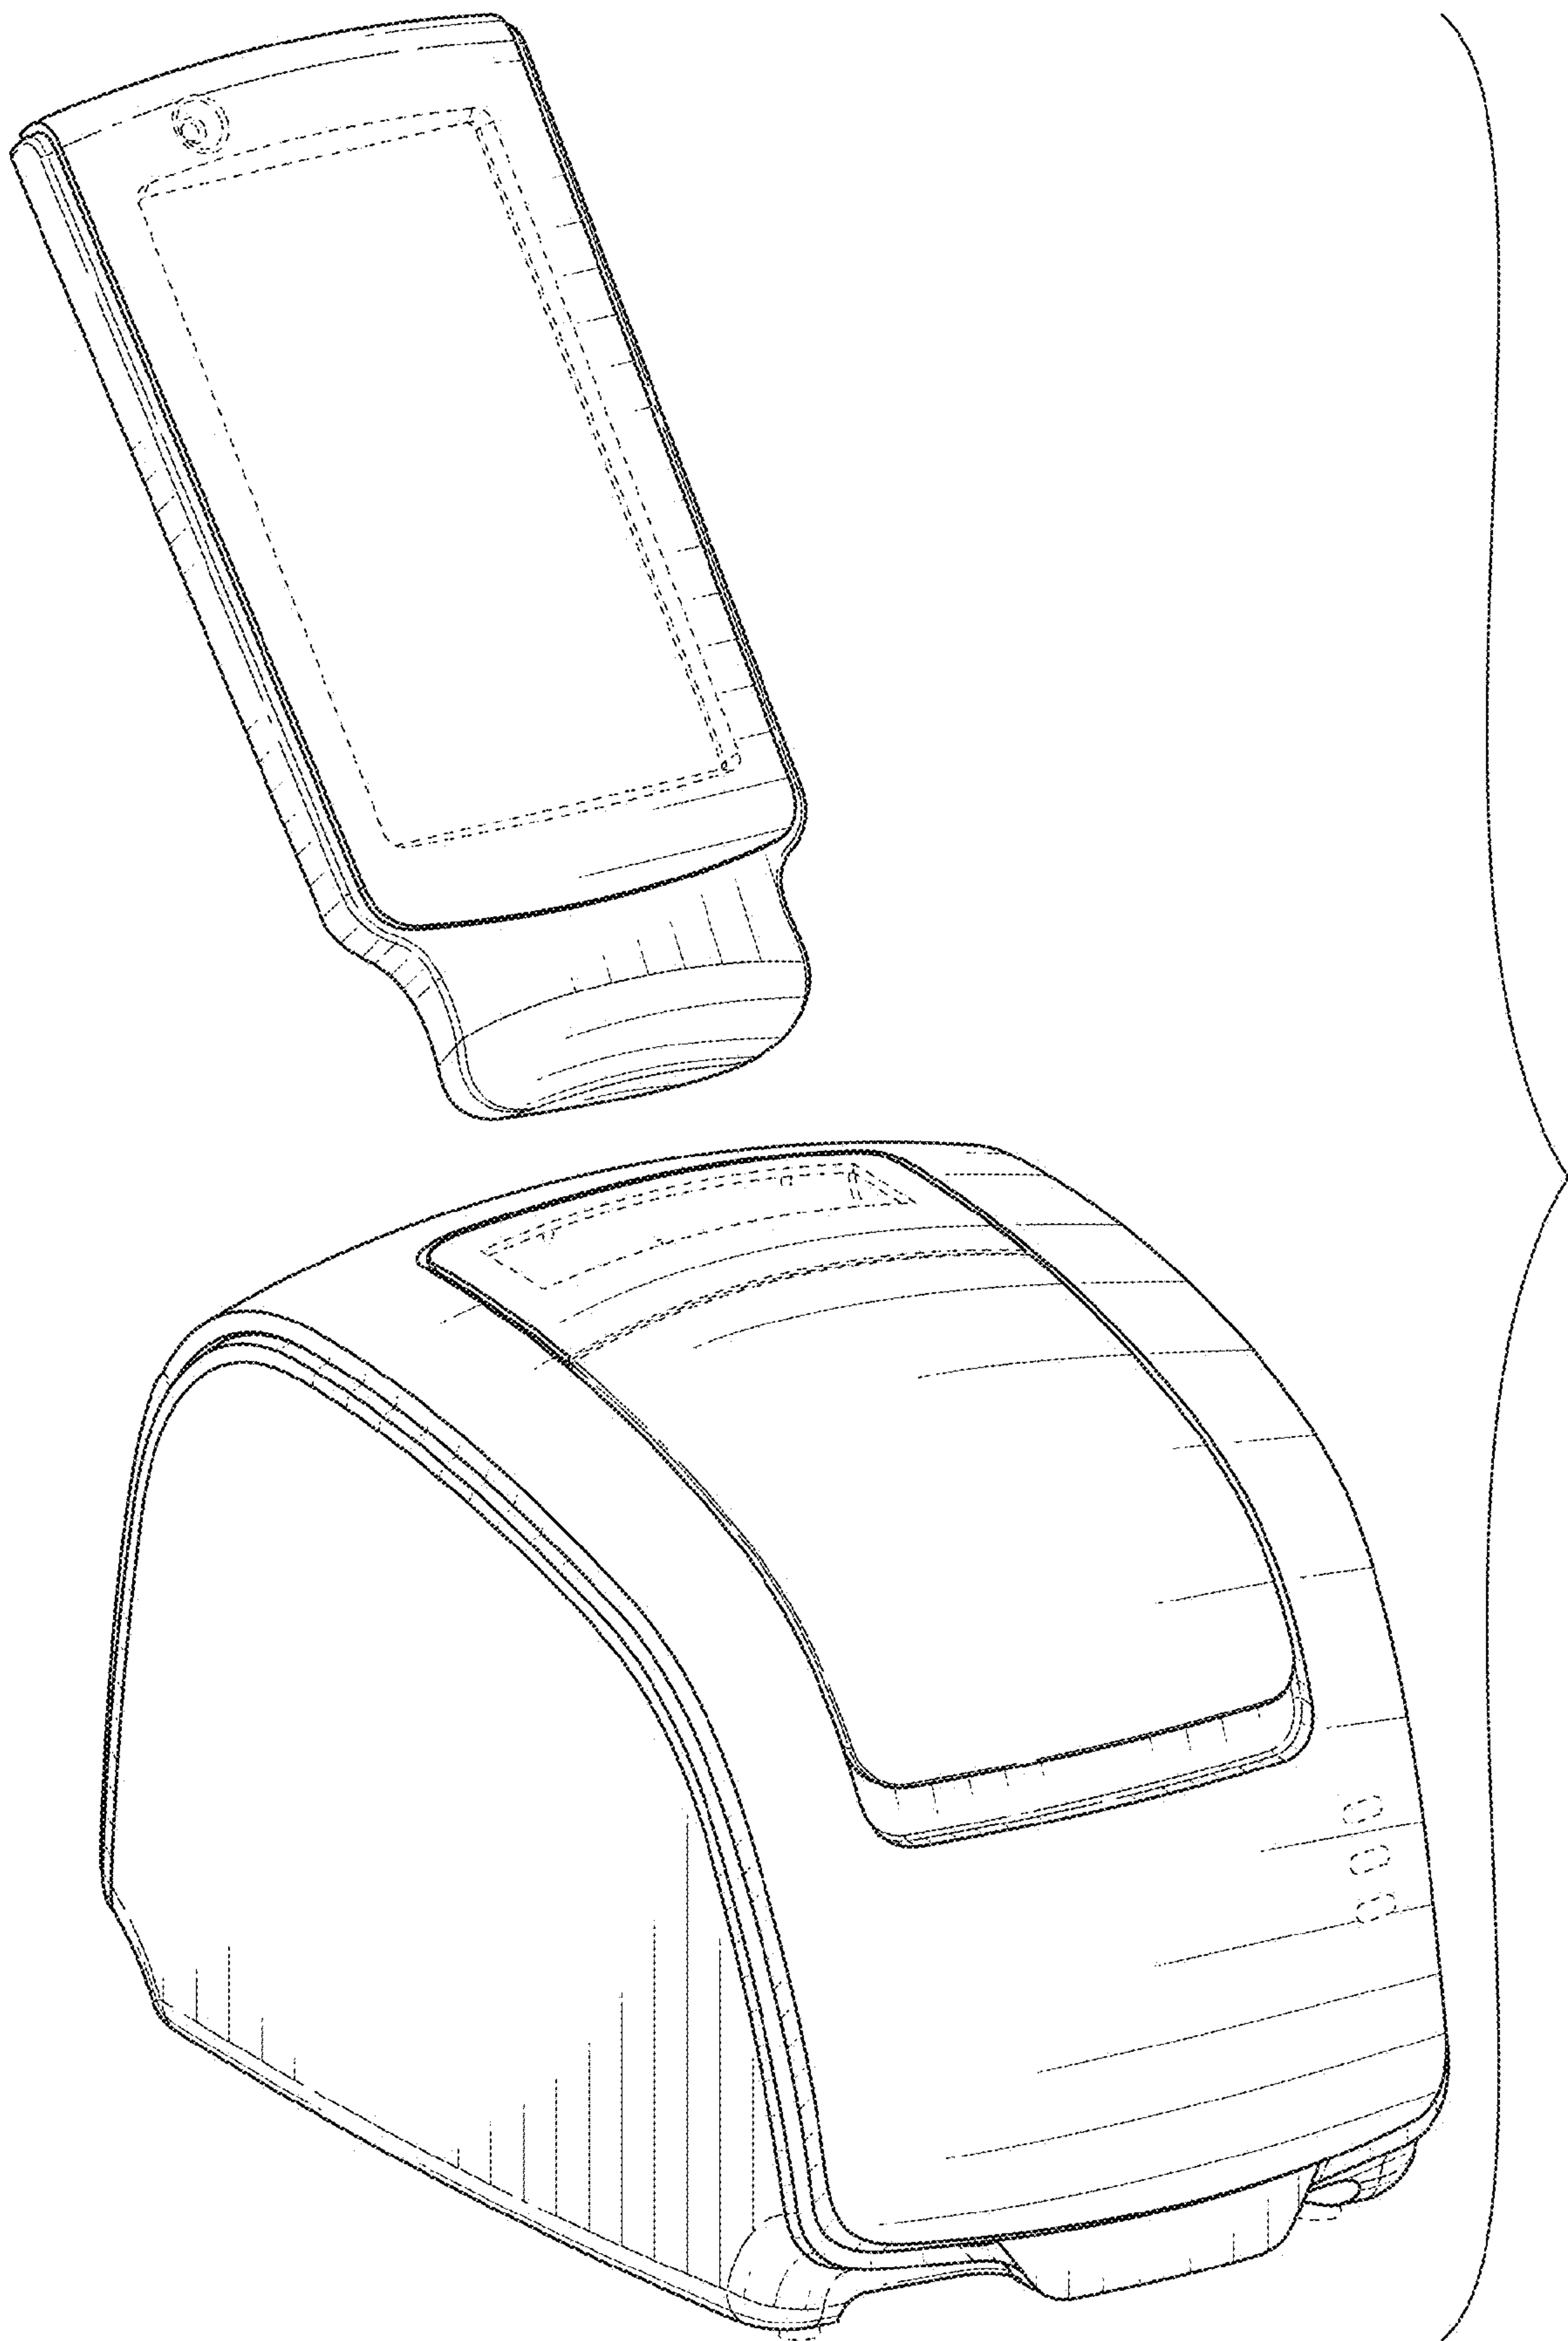


FIG. 1

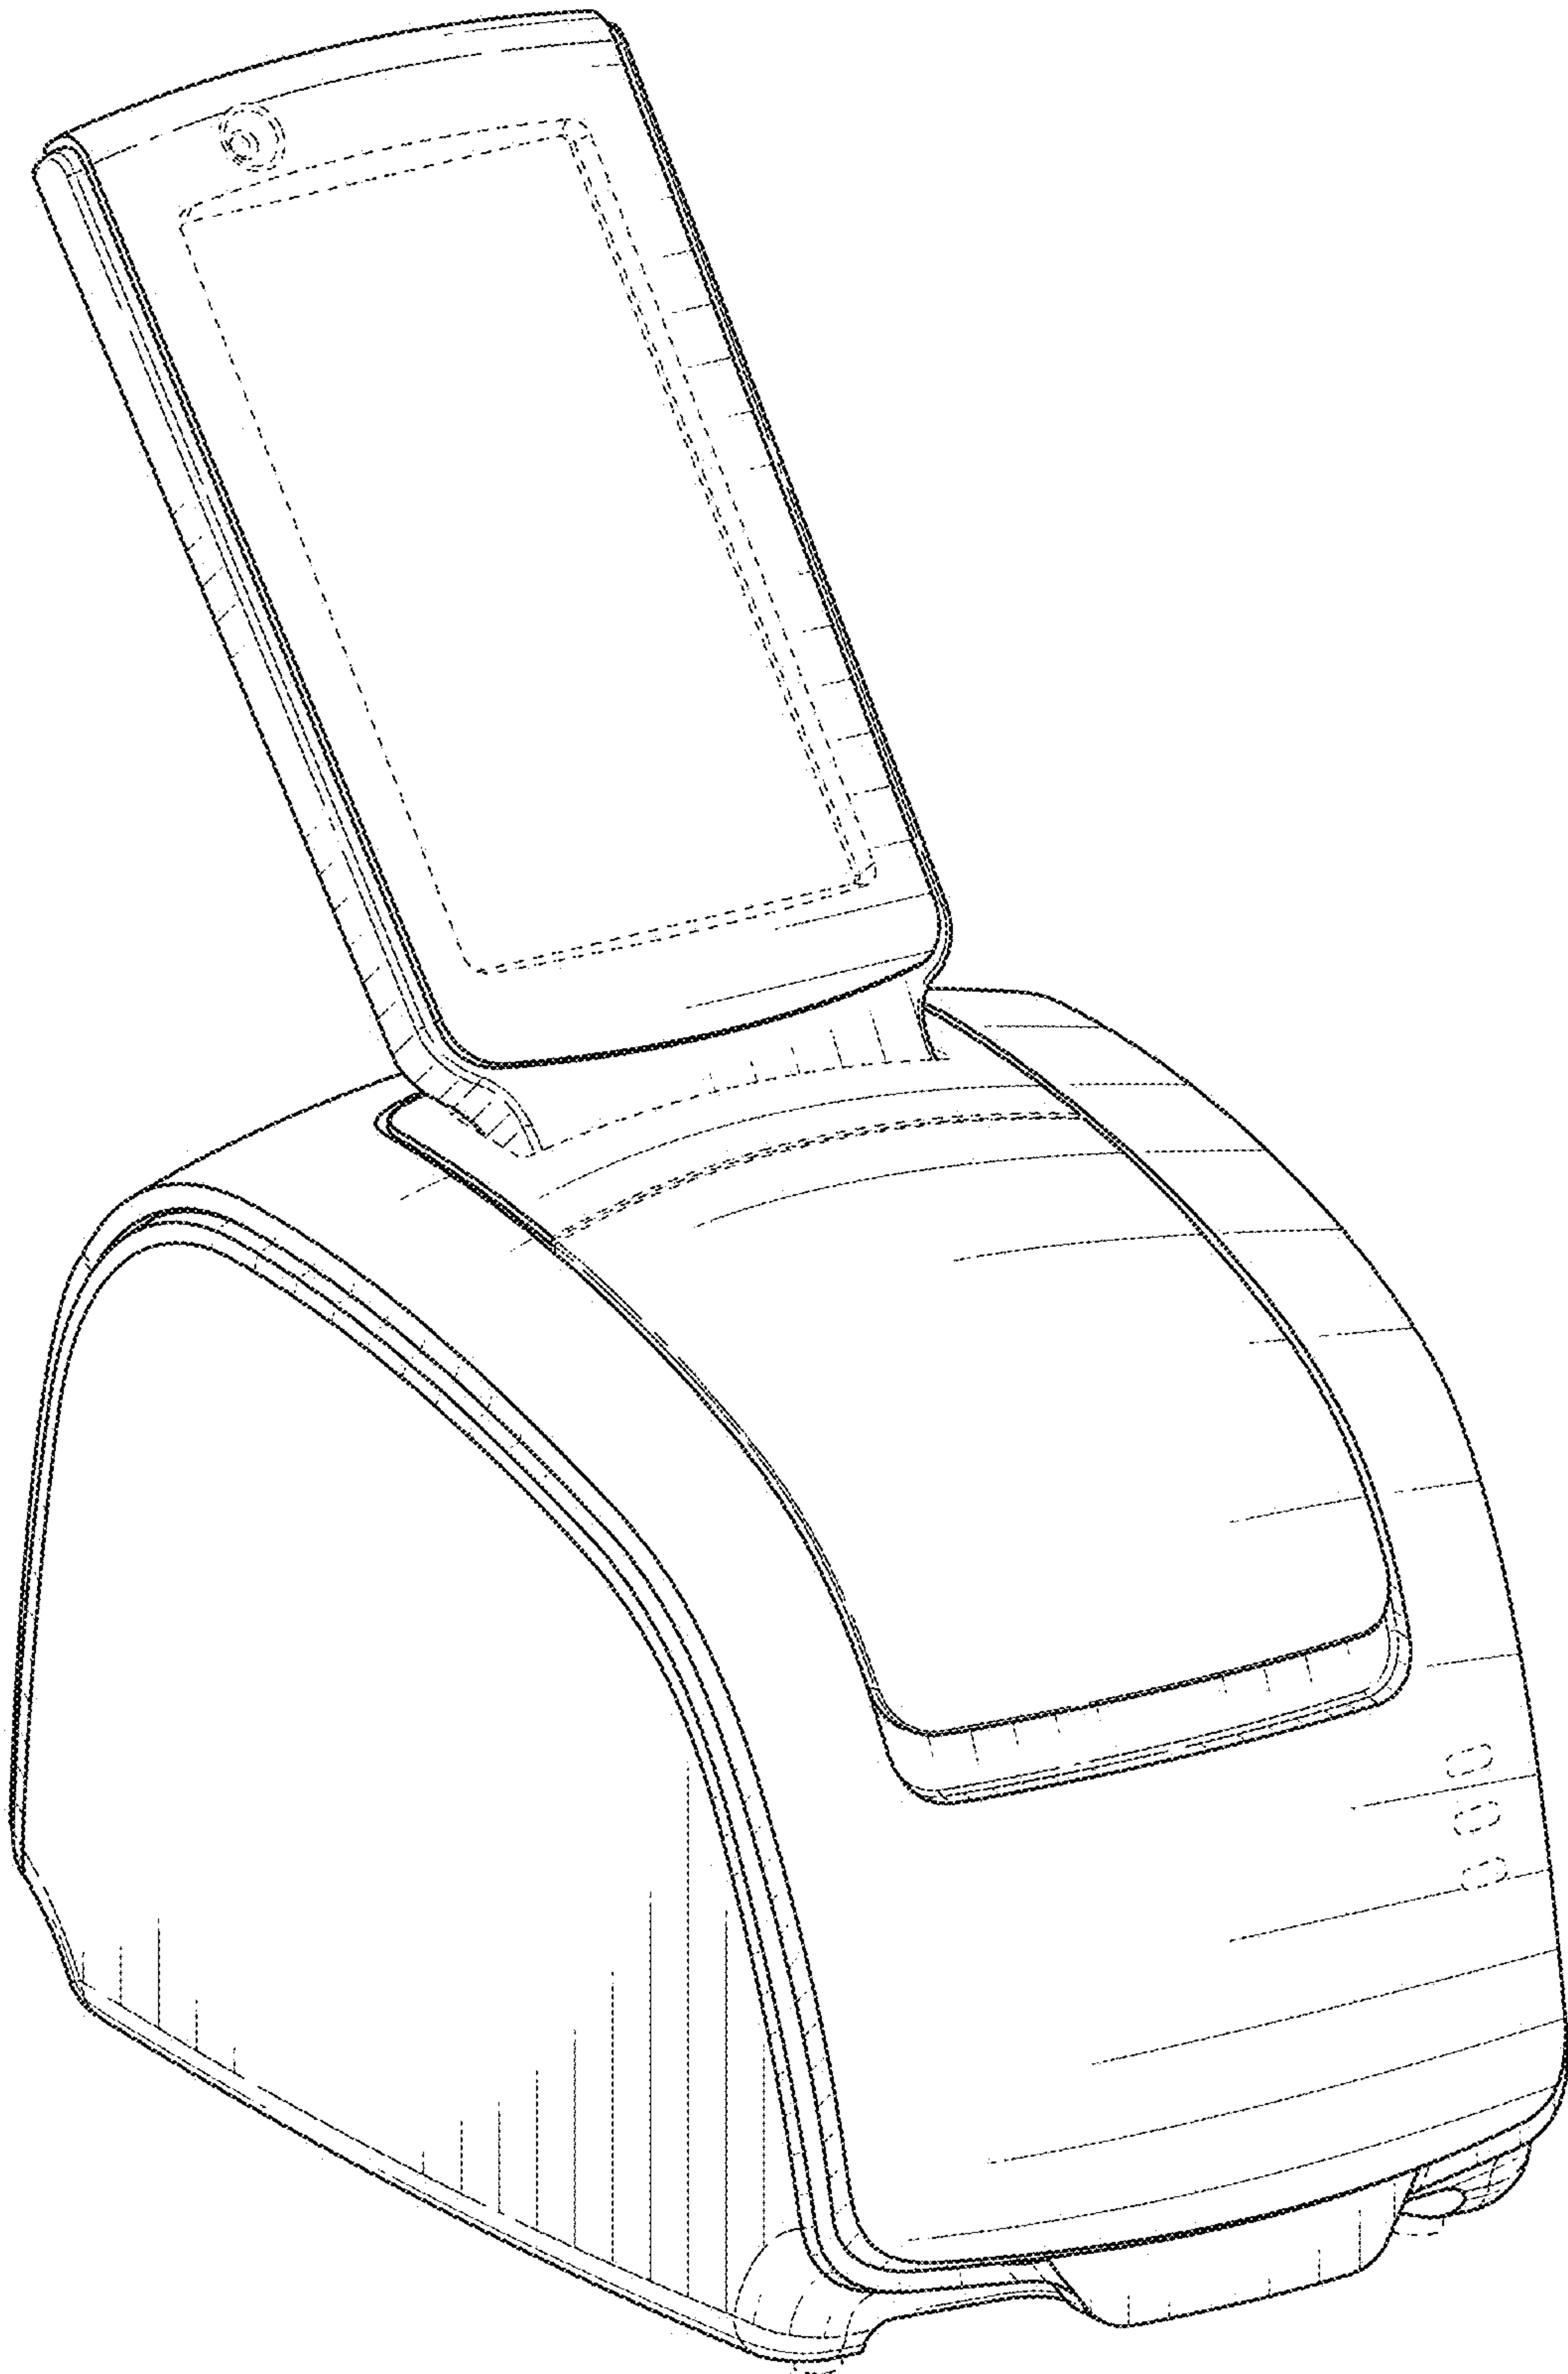


FIG. 2

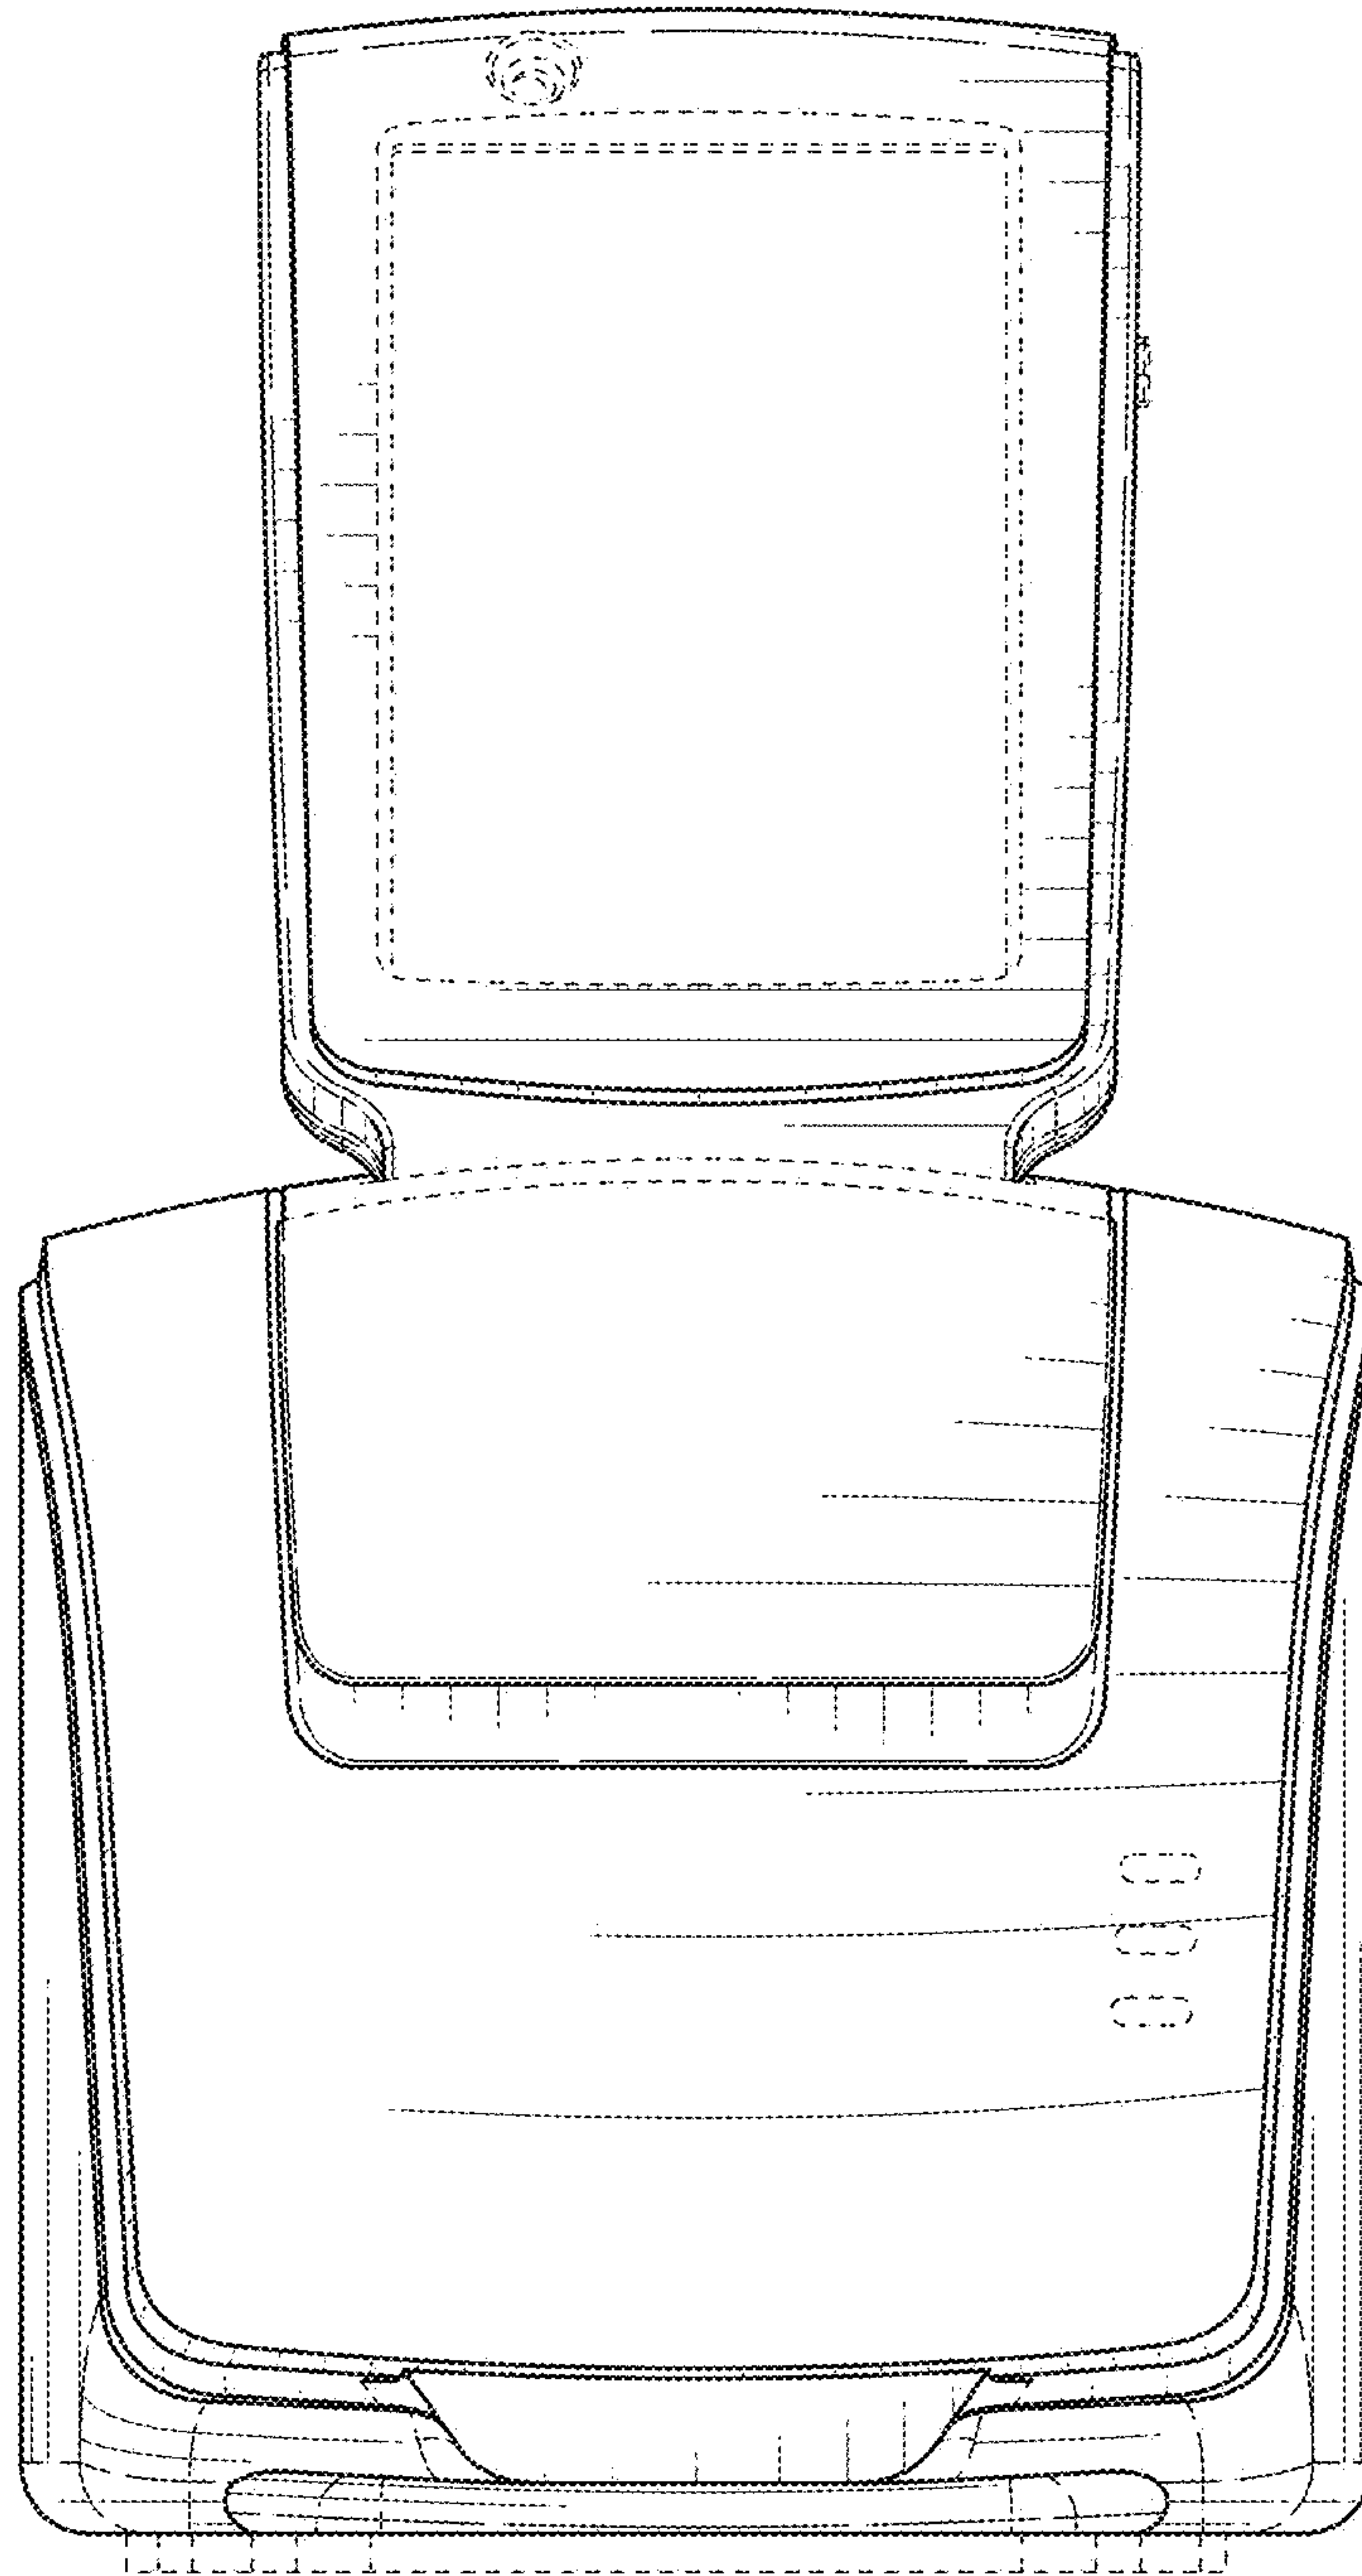


FIG. 3

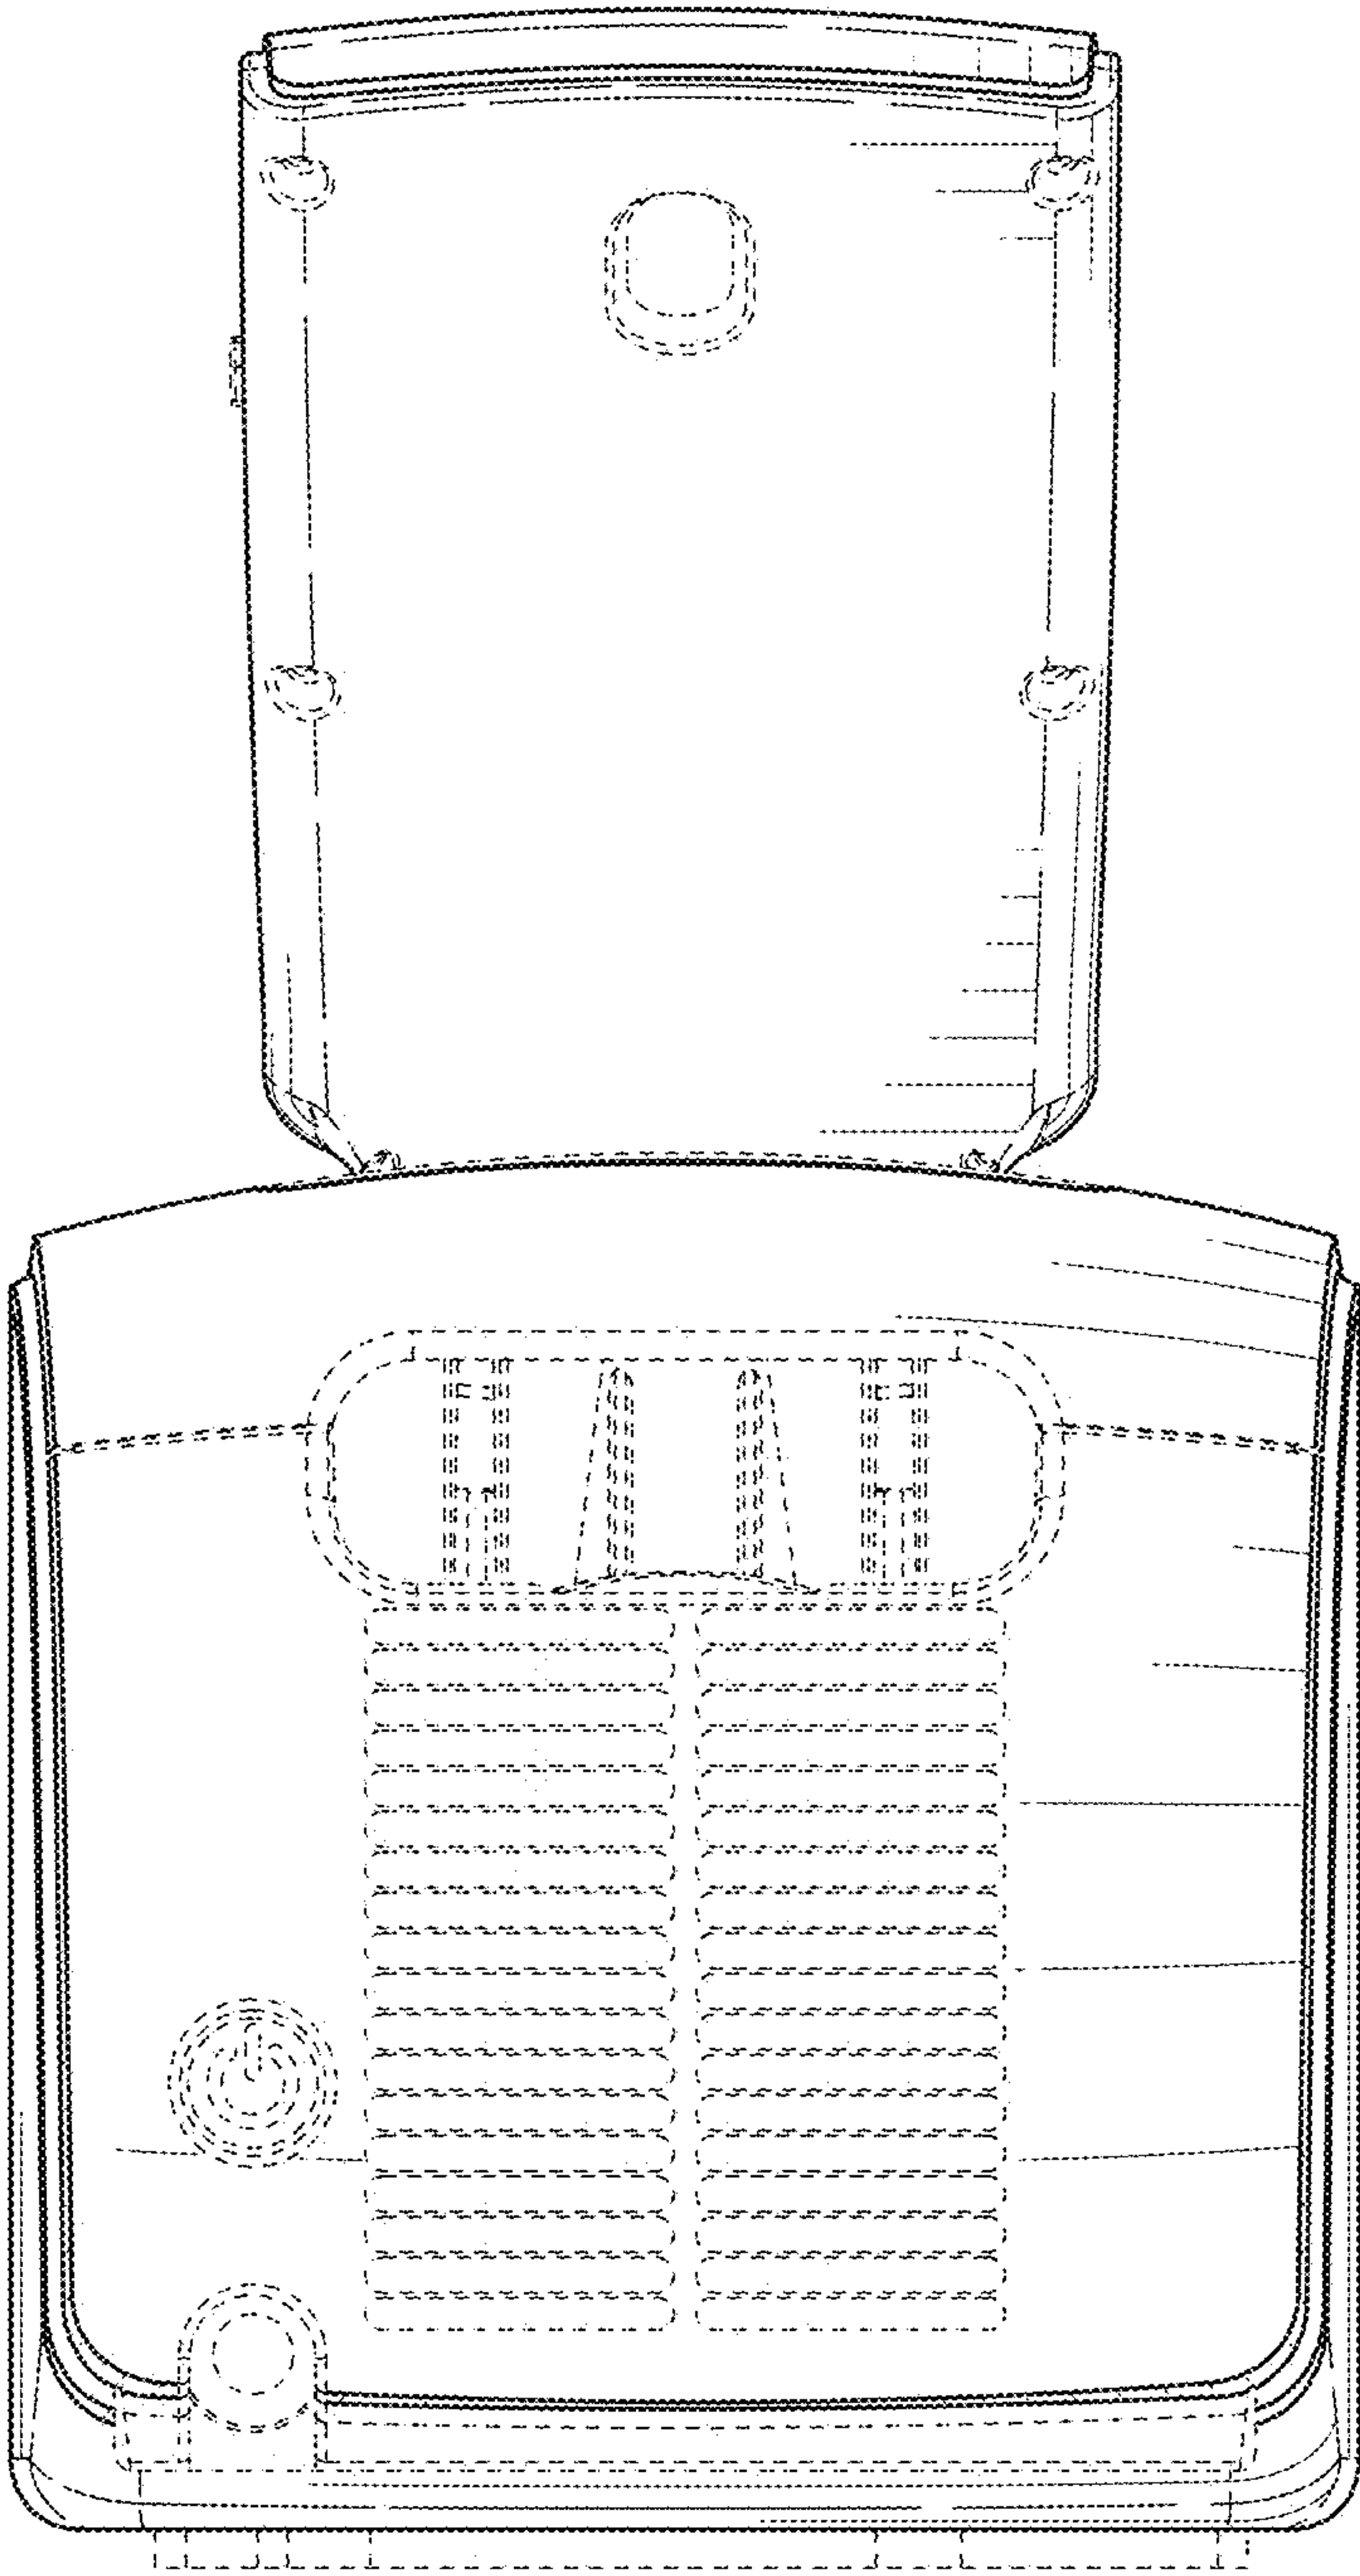


FIG. 4

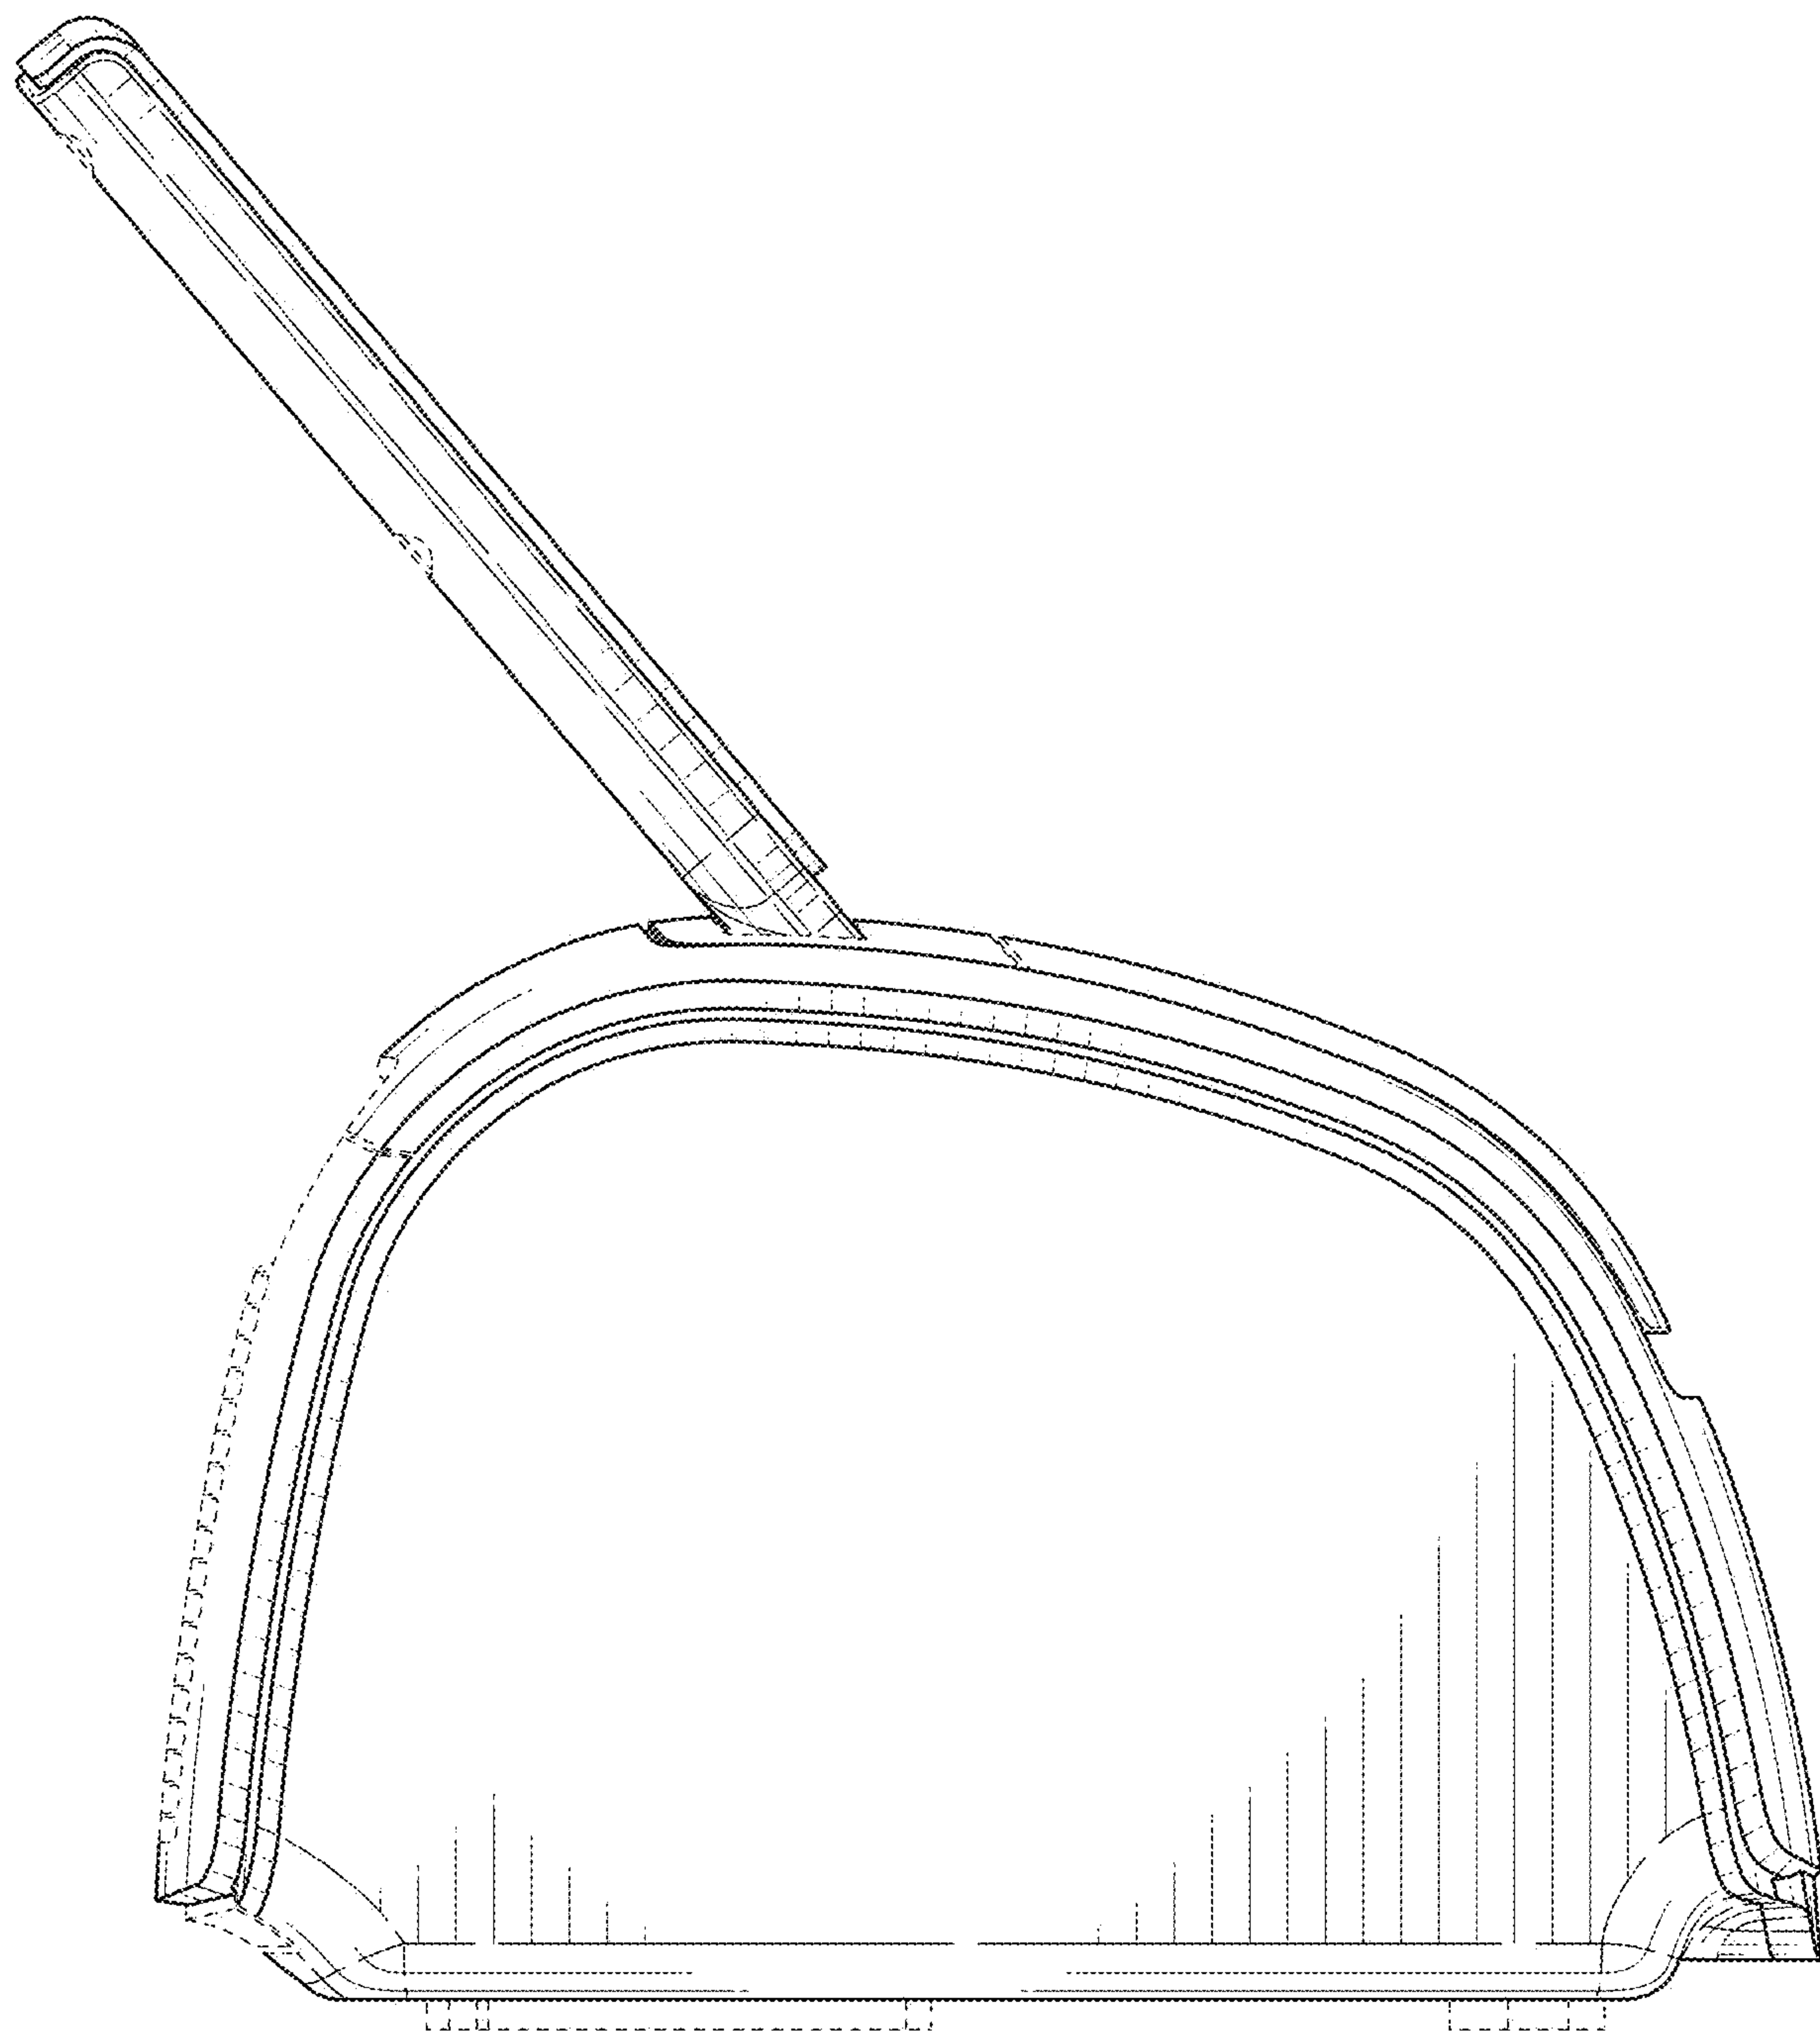


FIG. 5

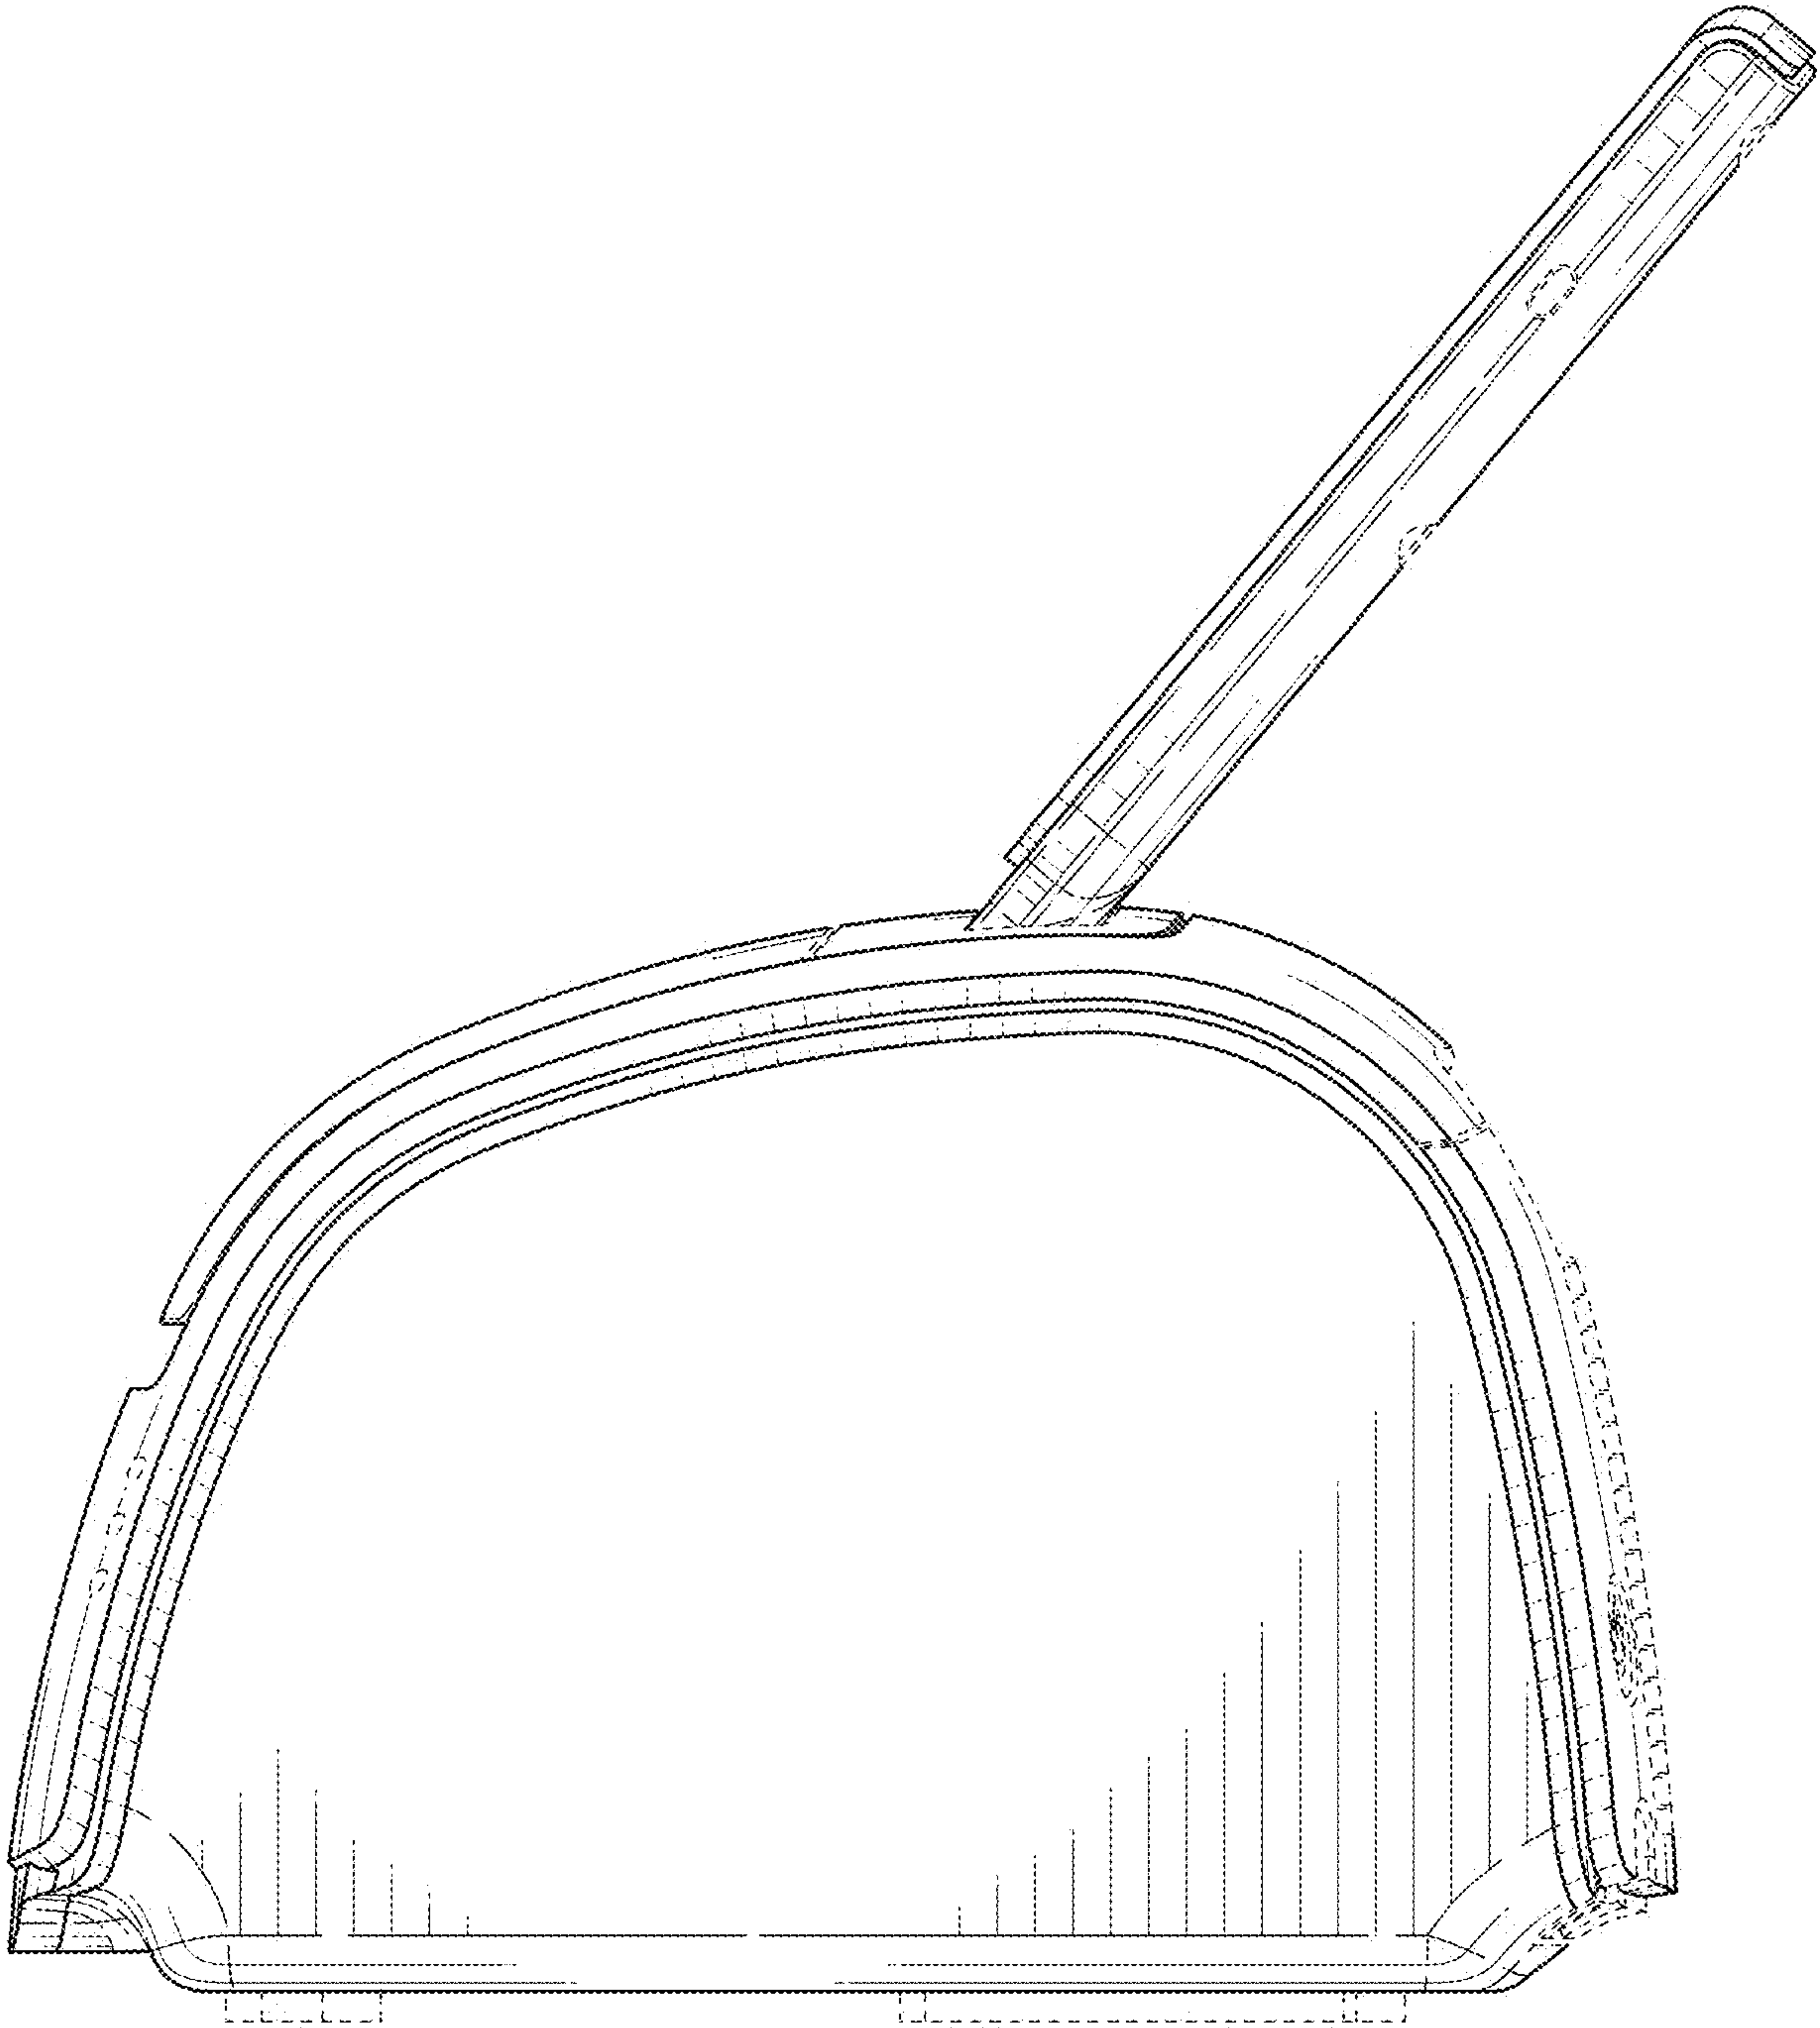


FIG. 6

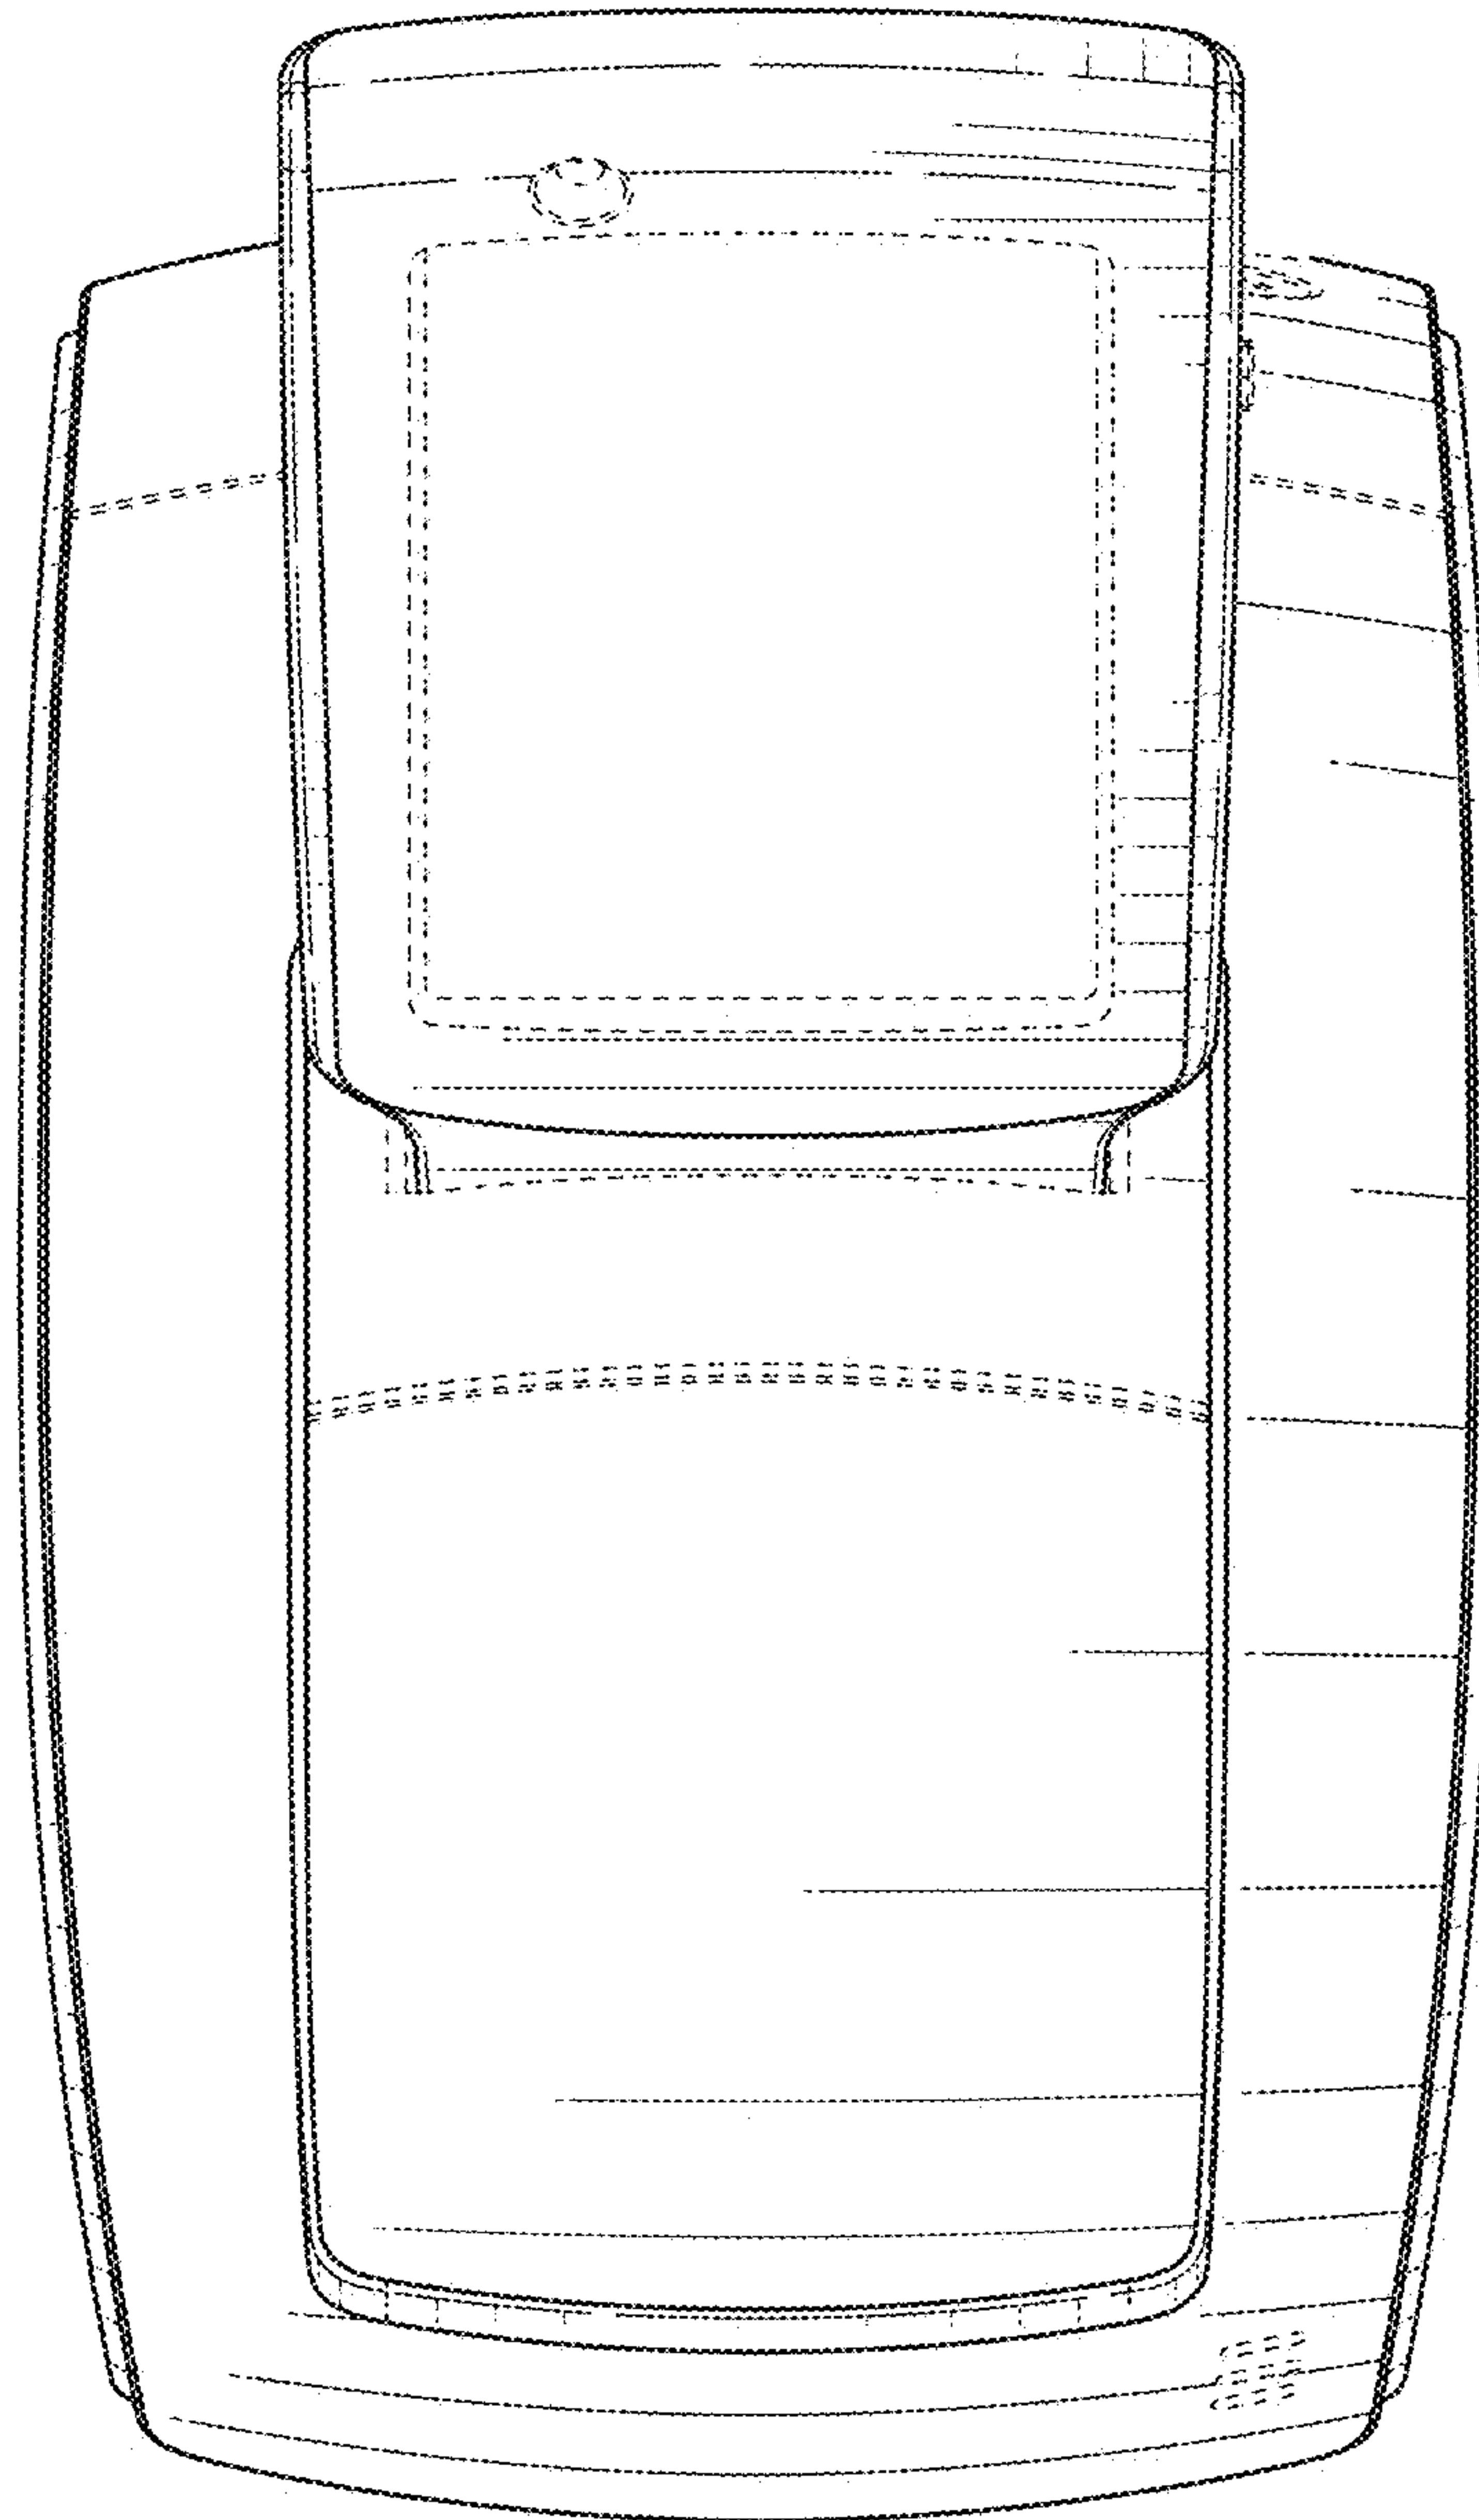


FIG. 7

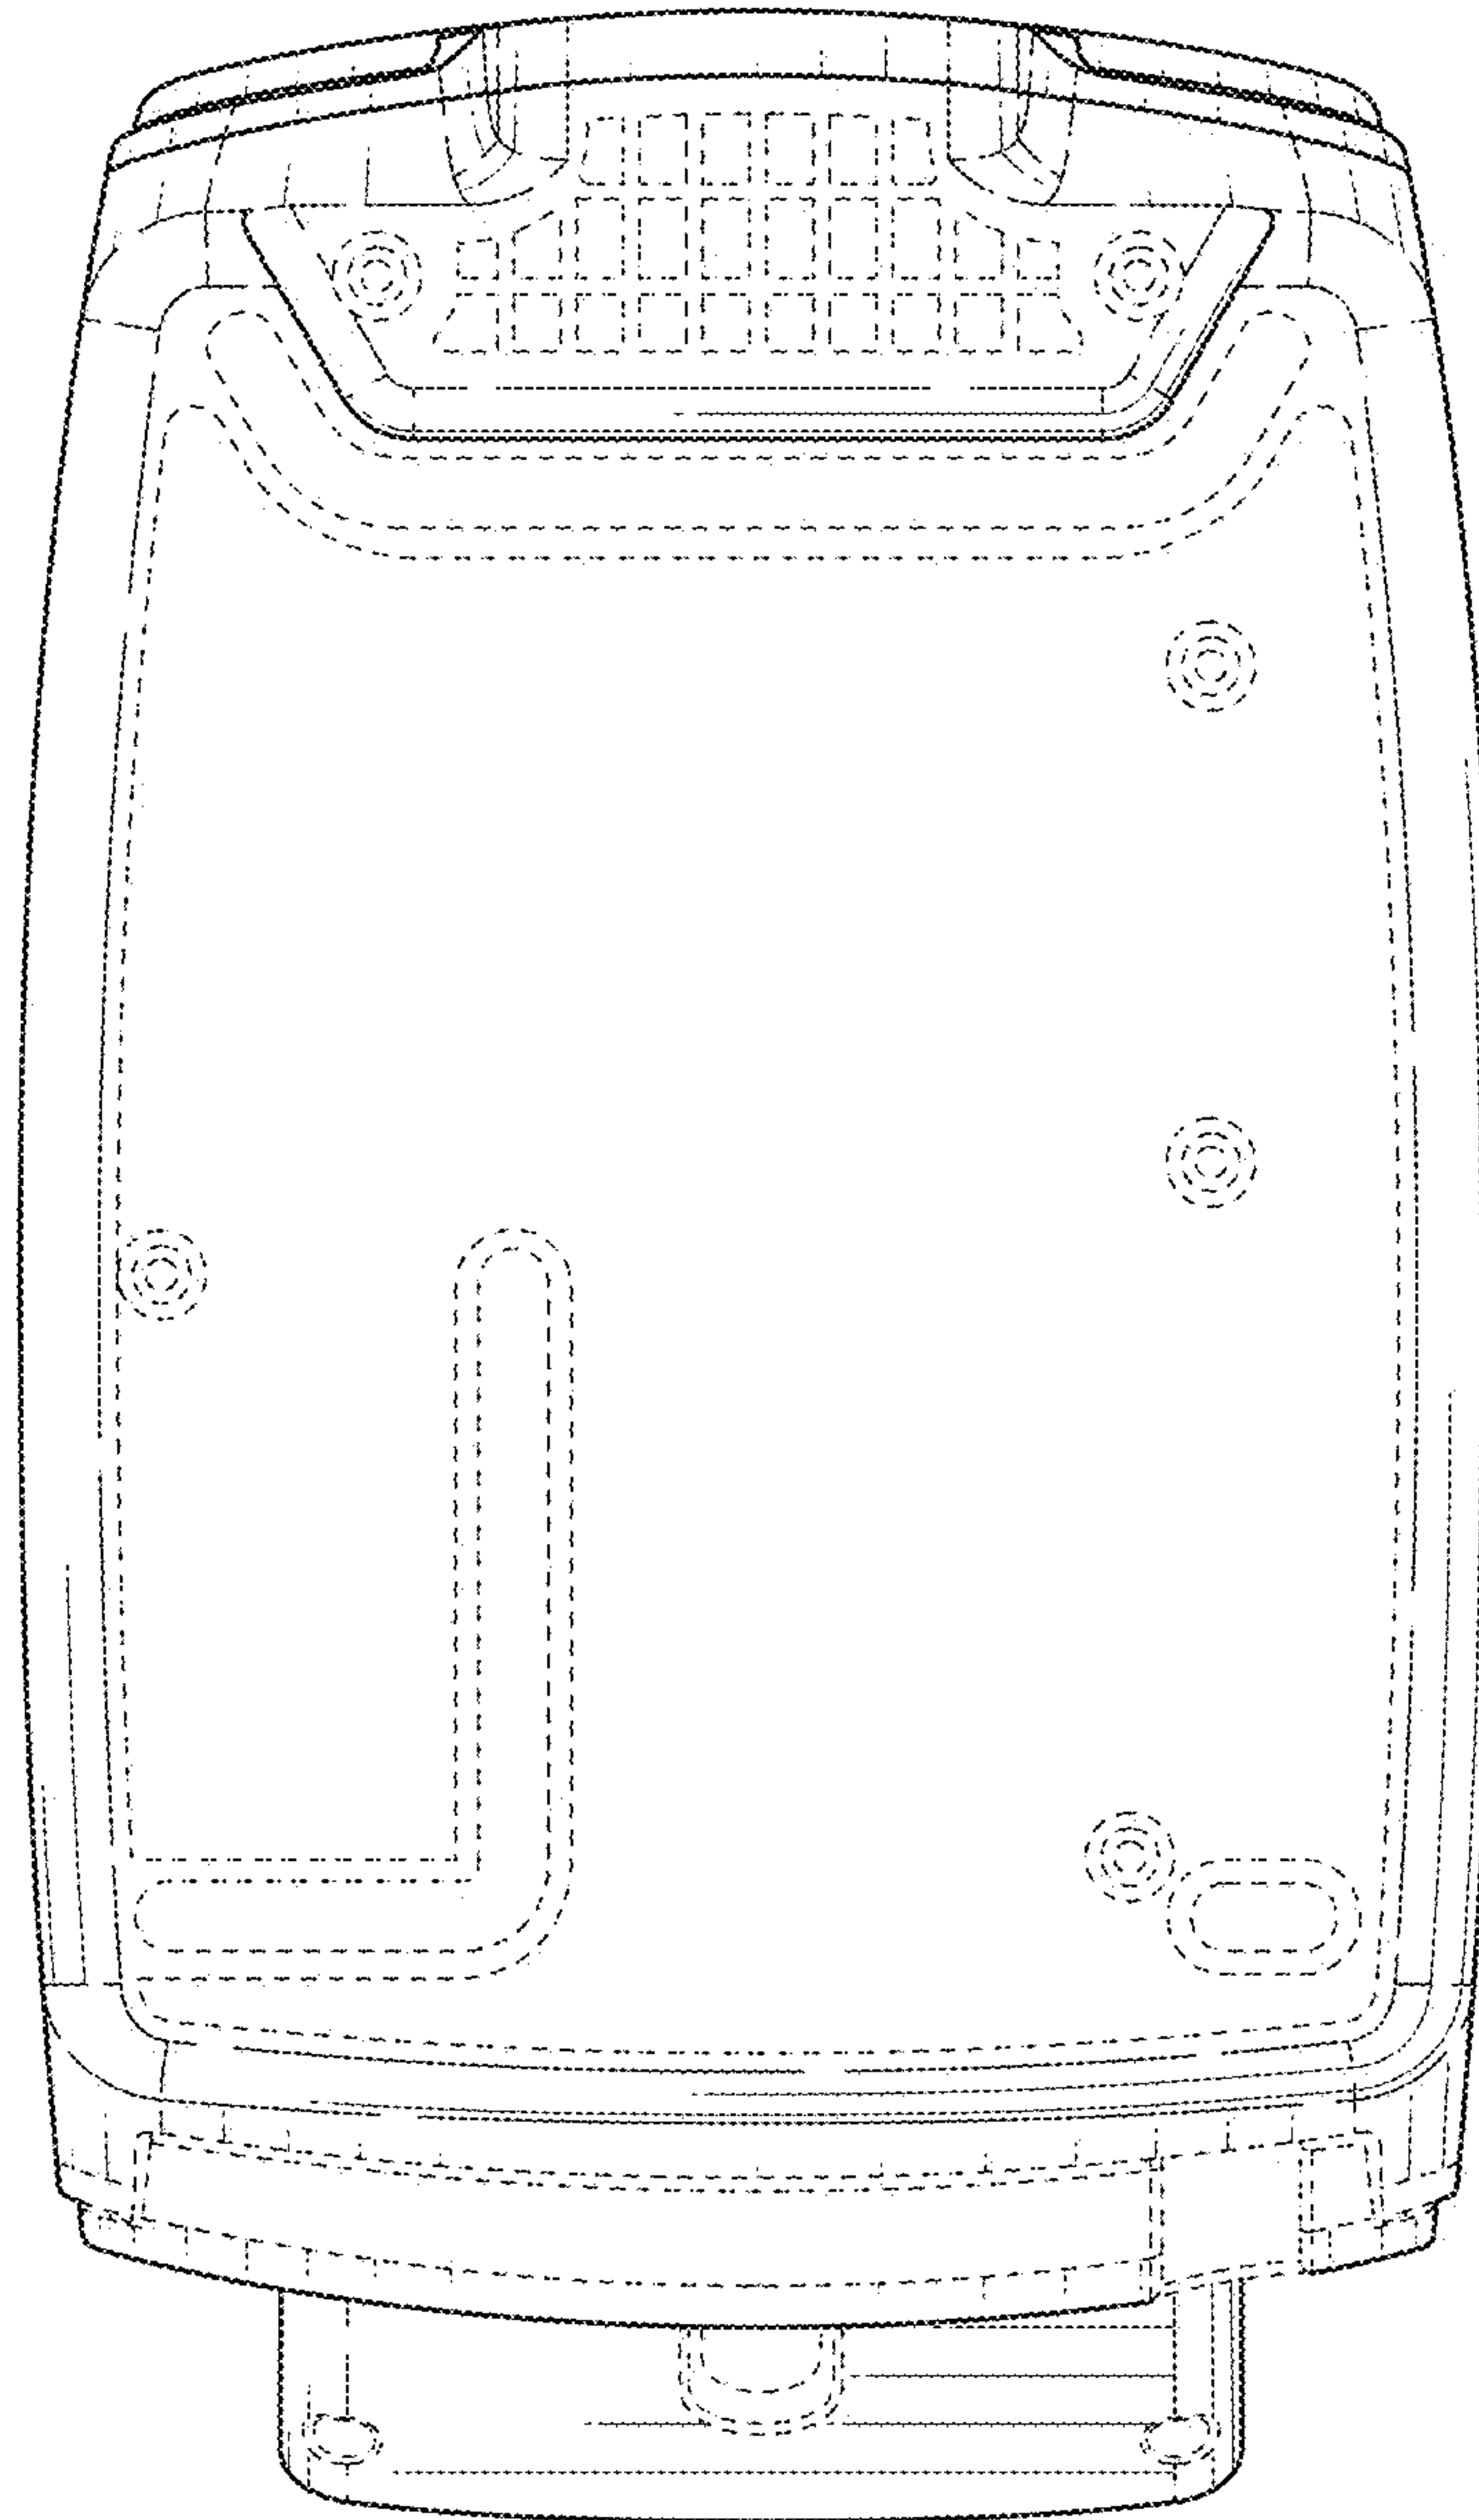


FIG. 8

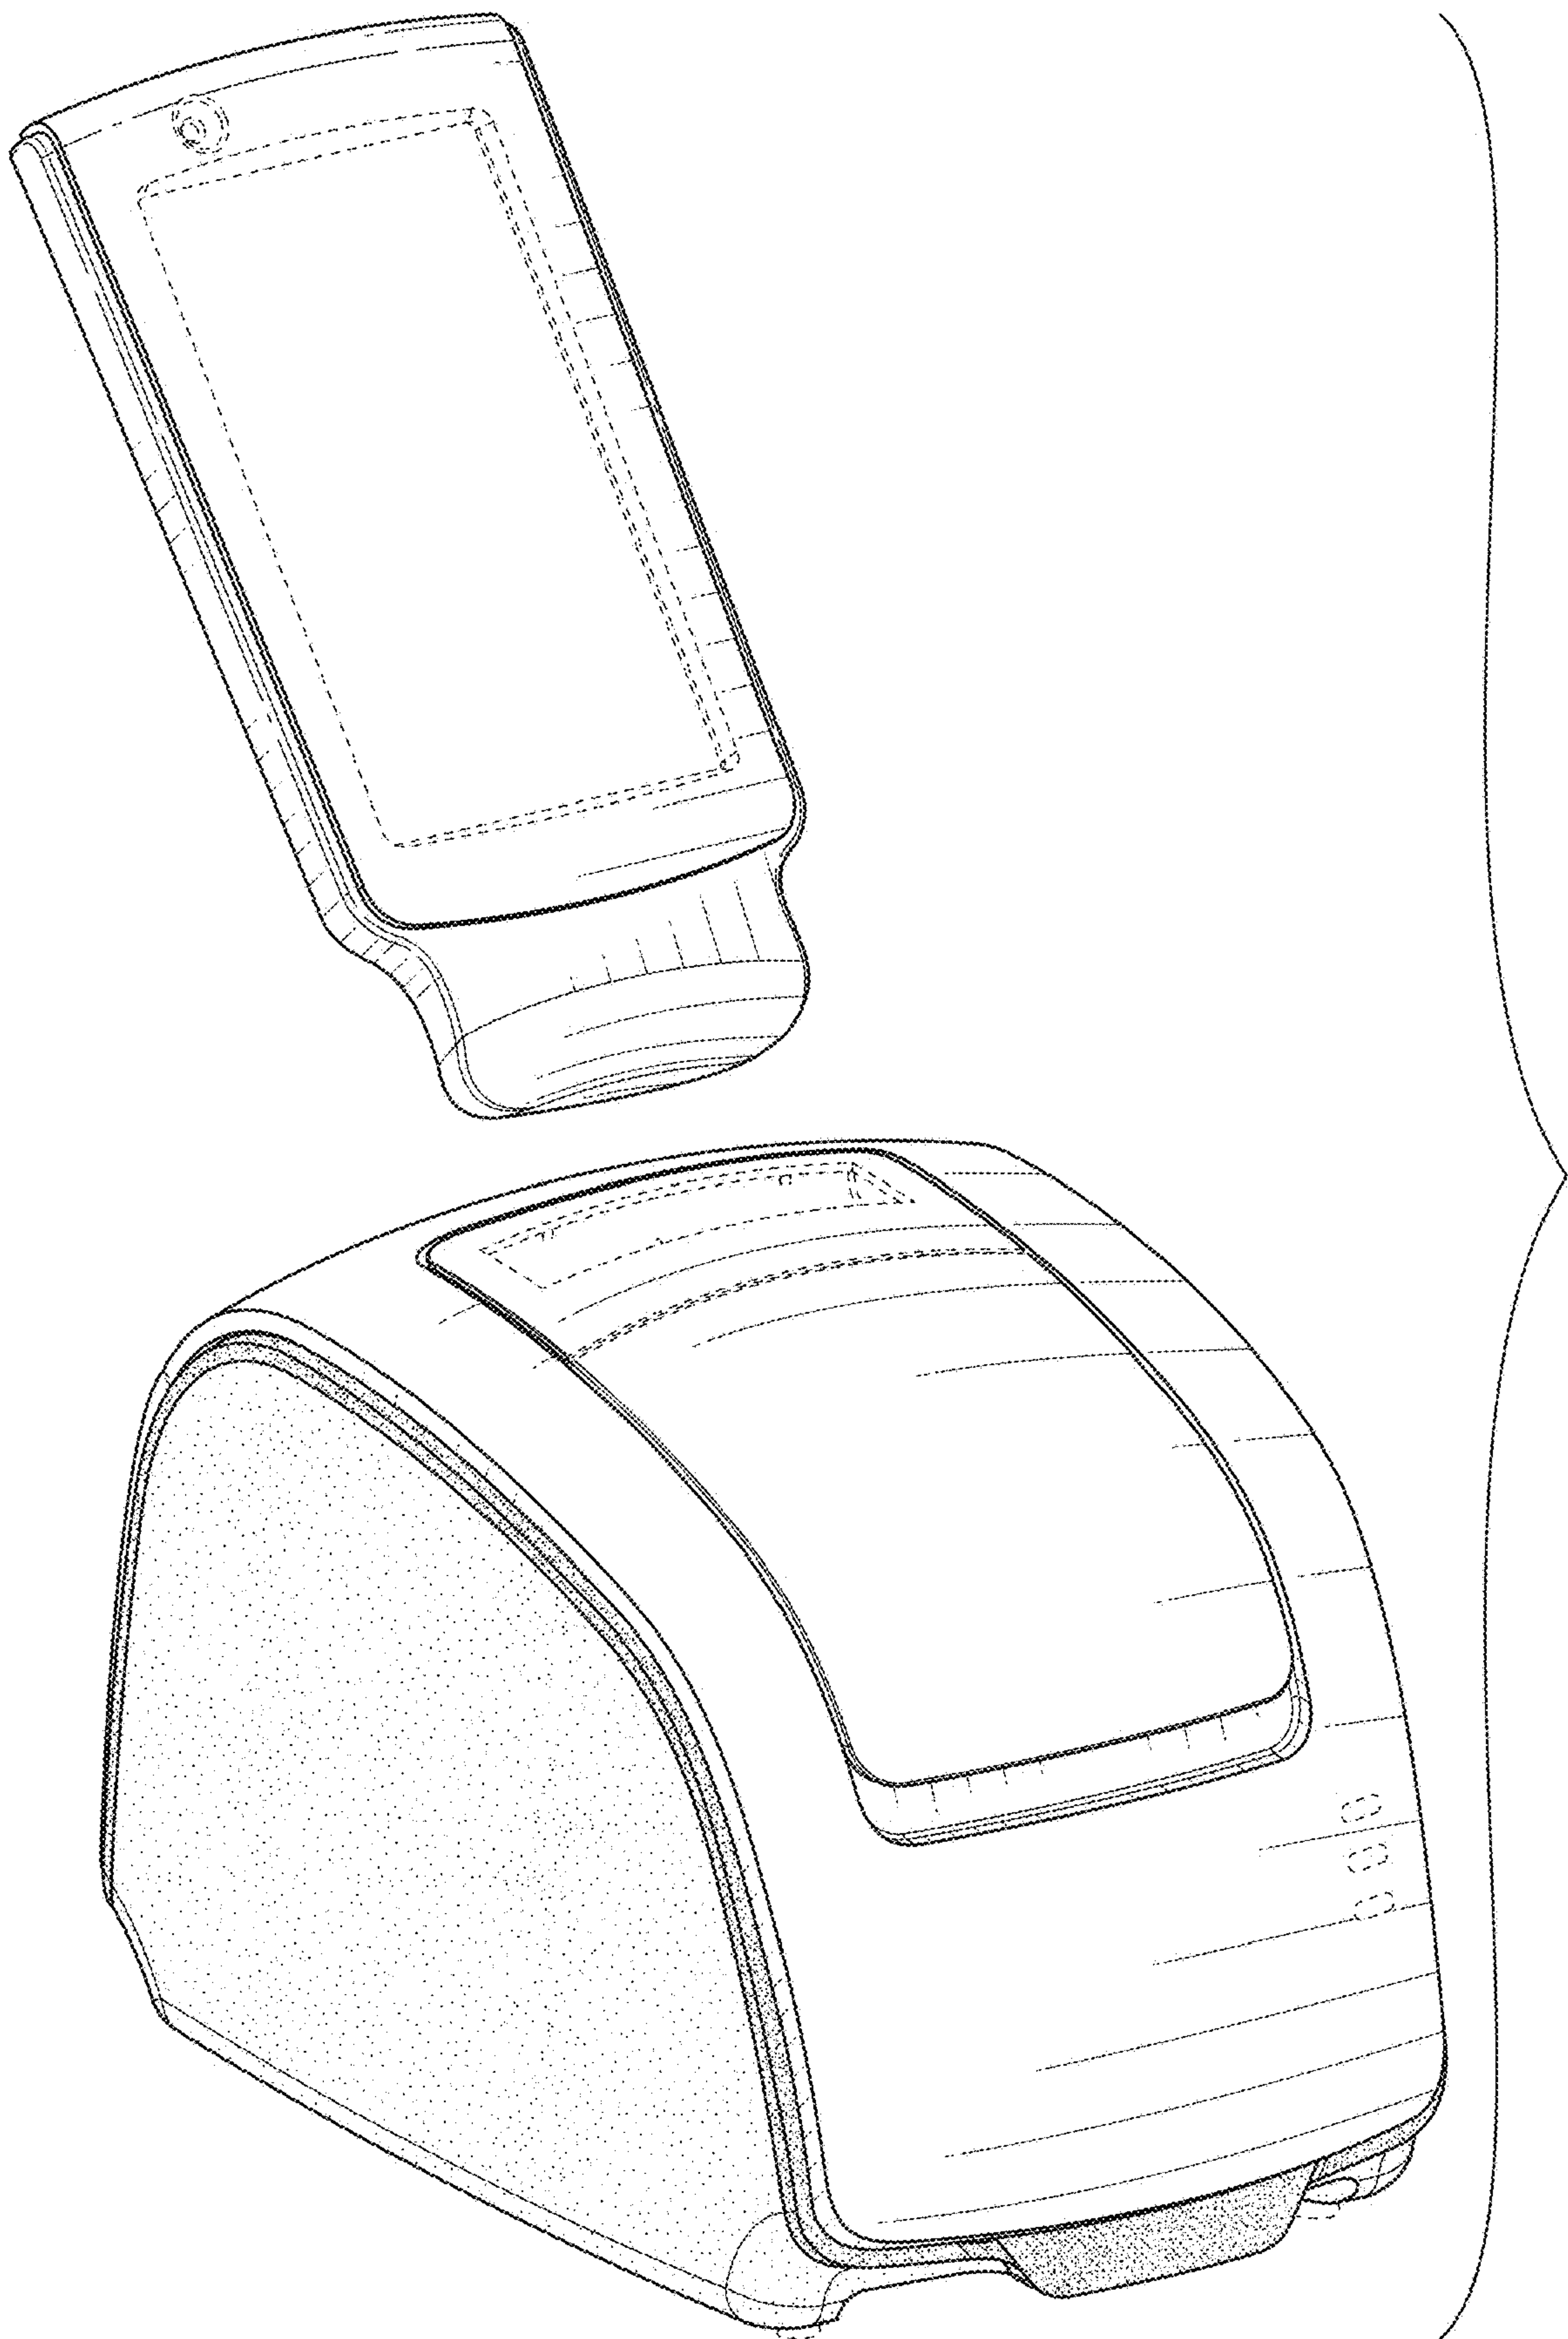


FIG. 9

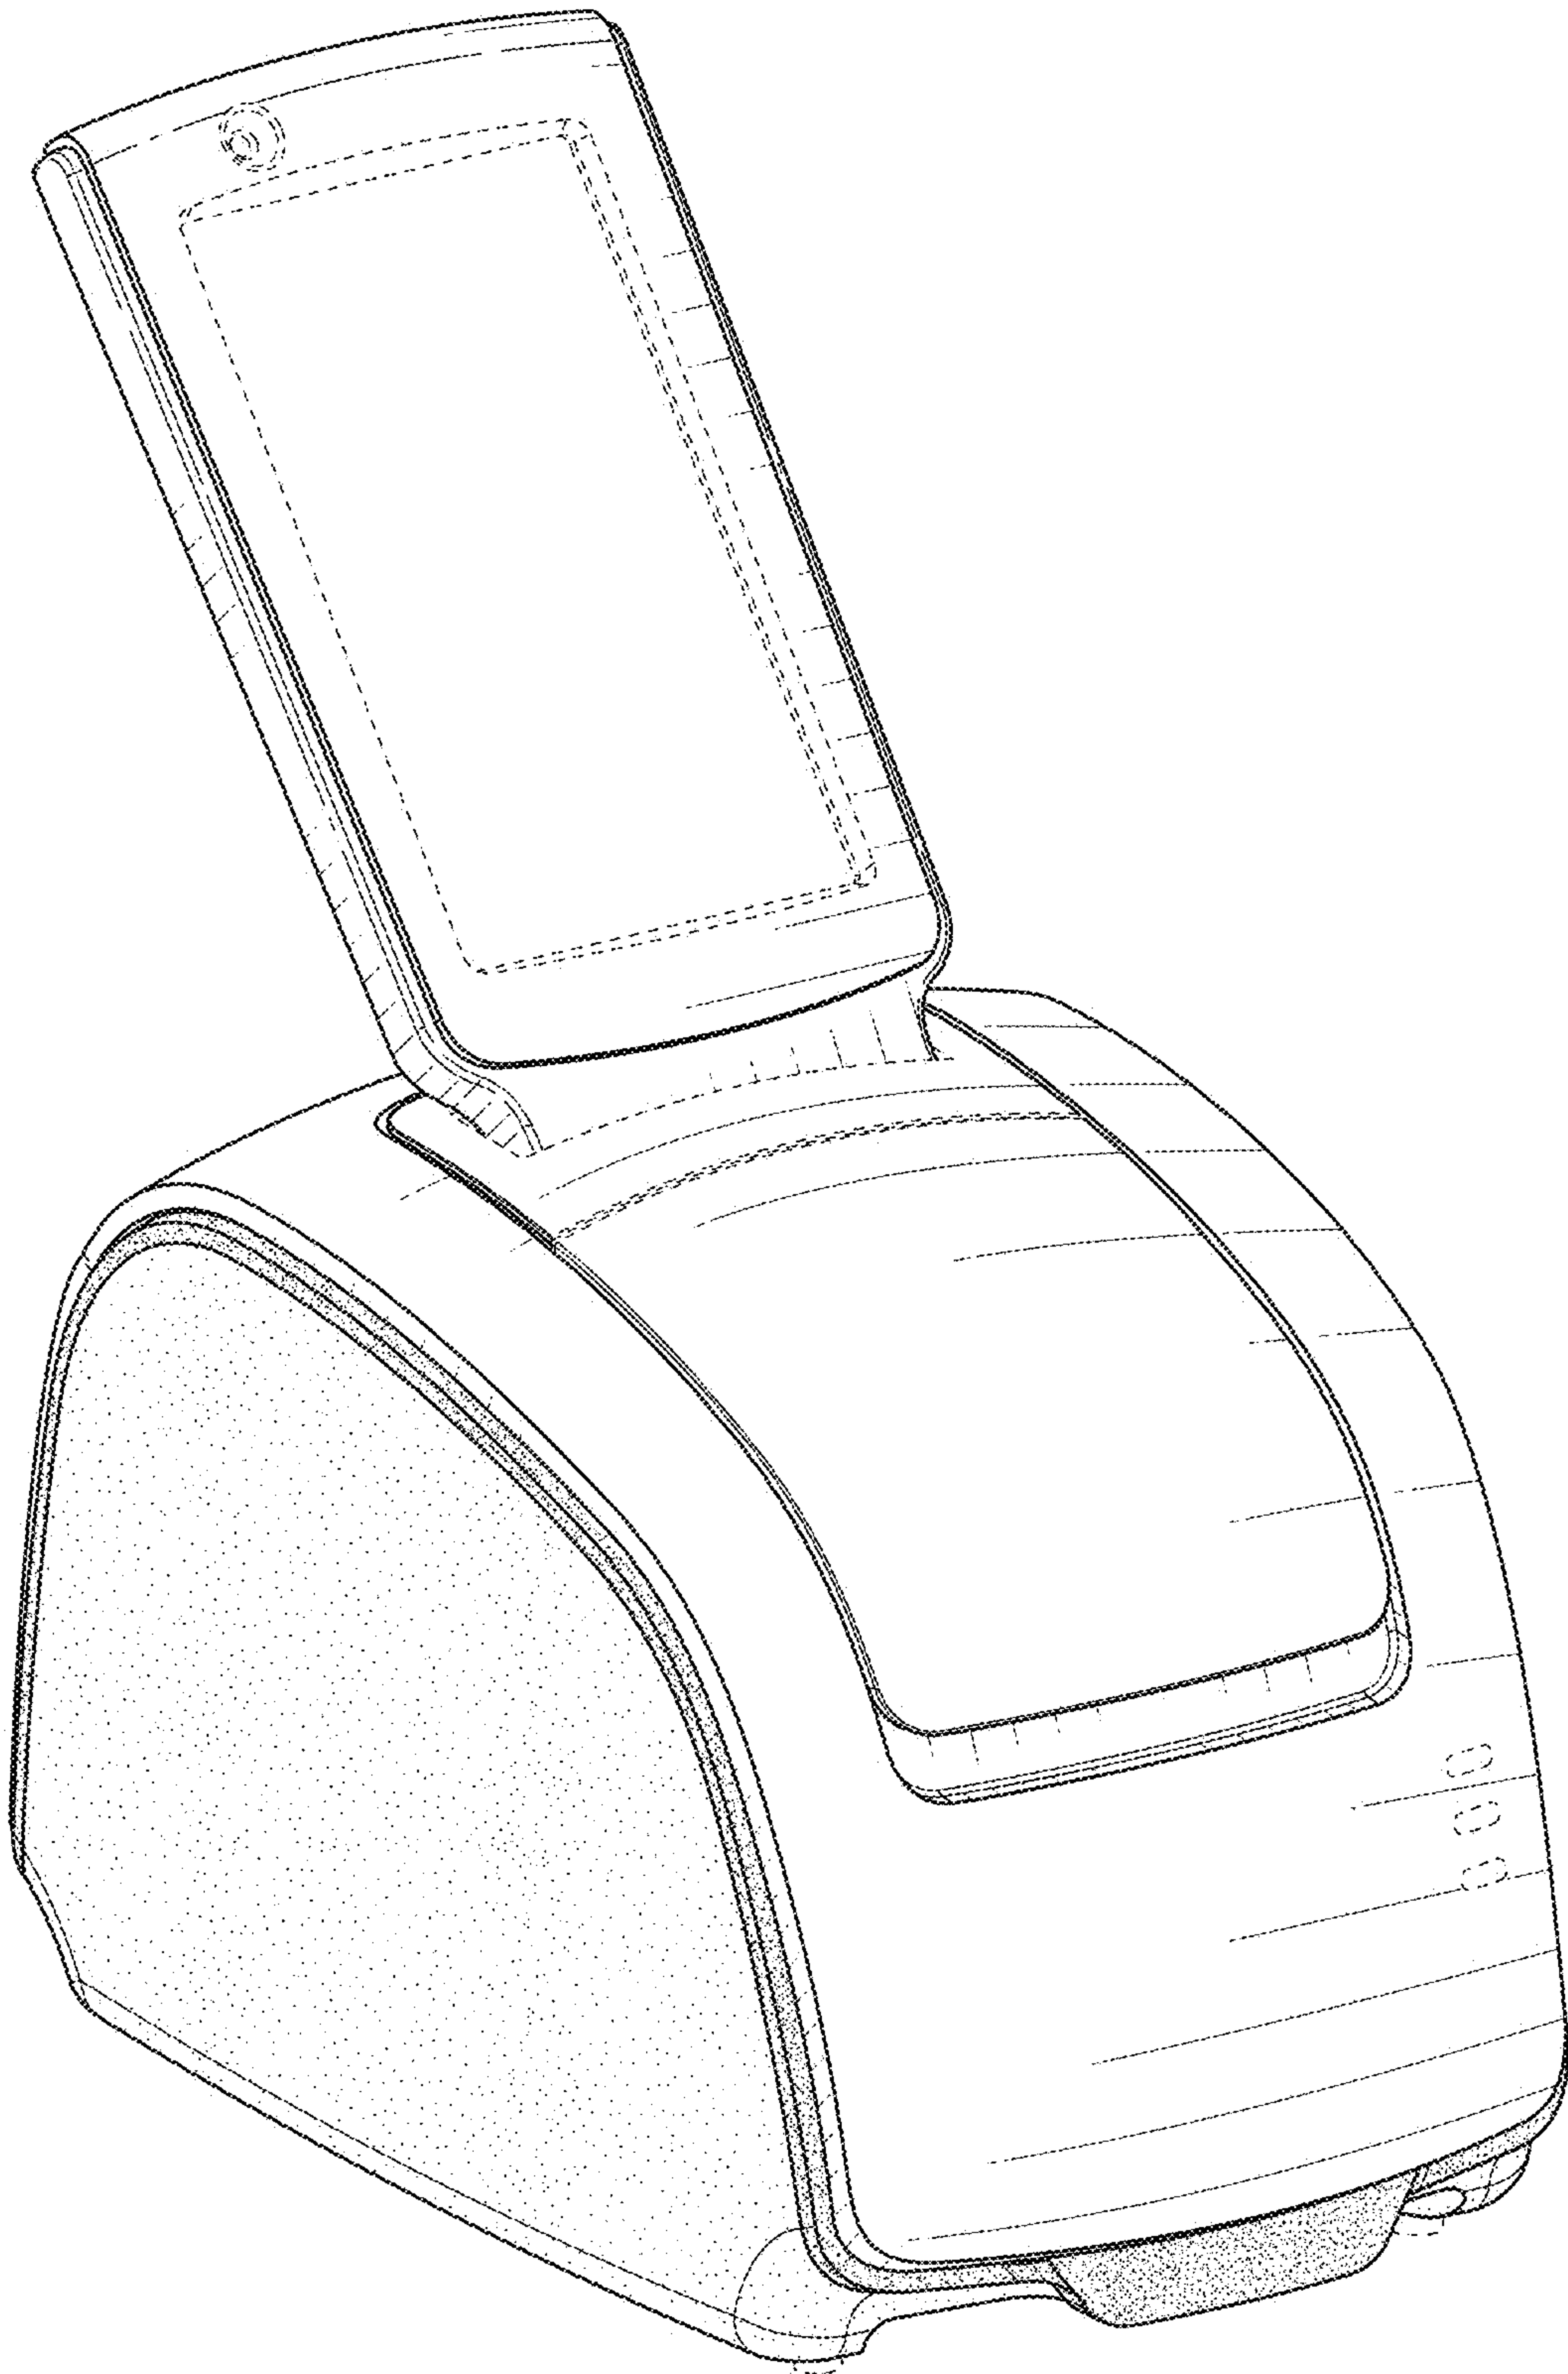


FIG. 10

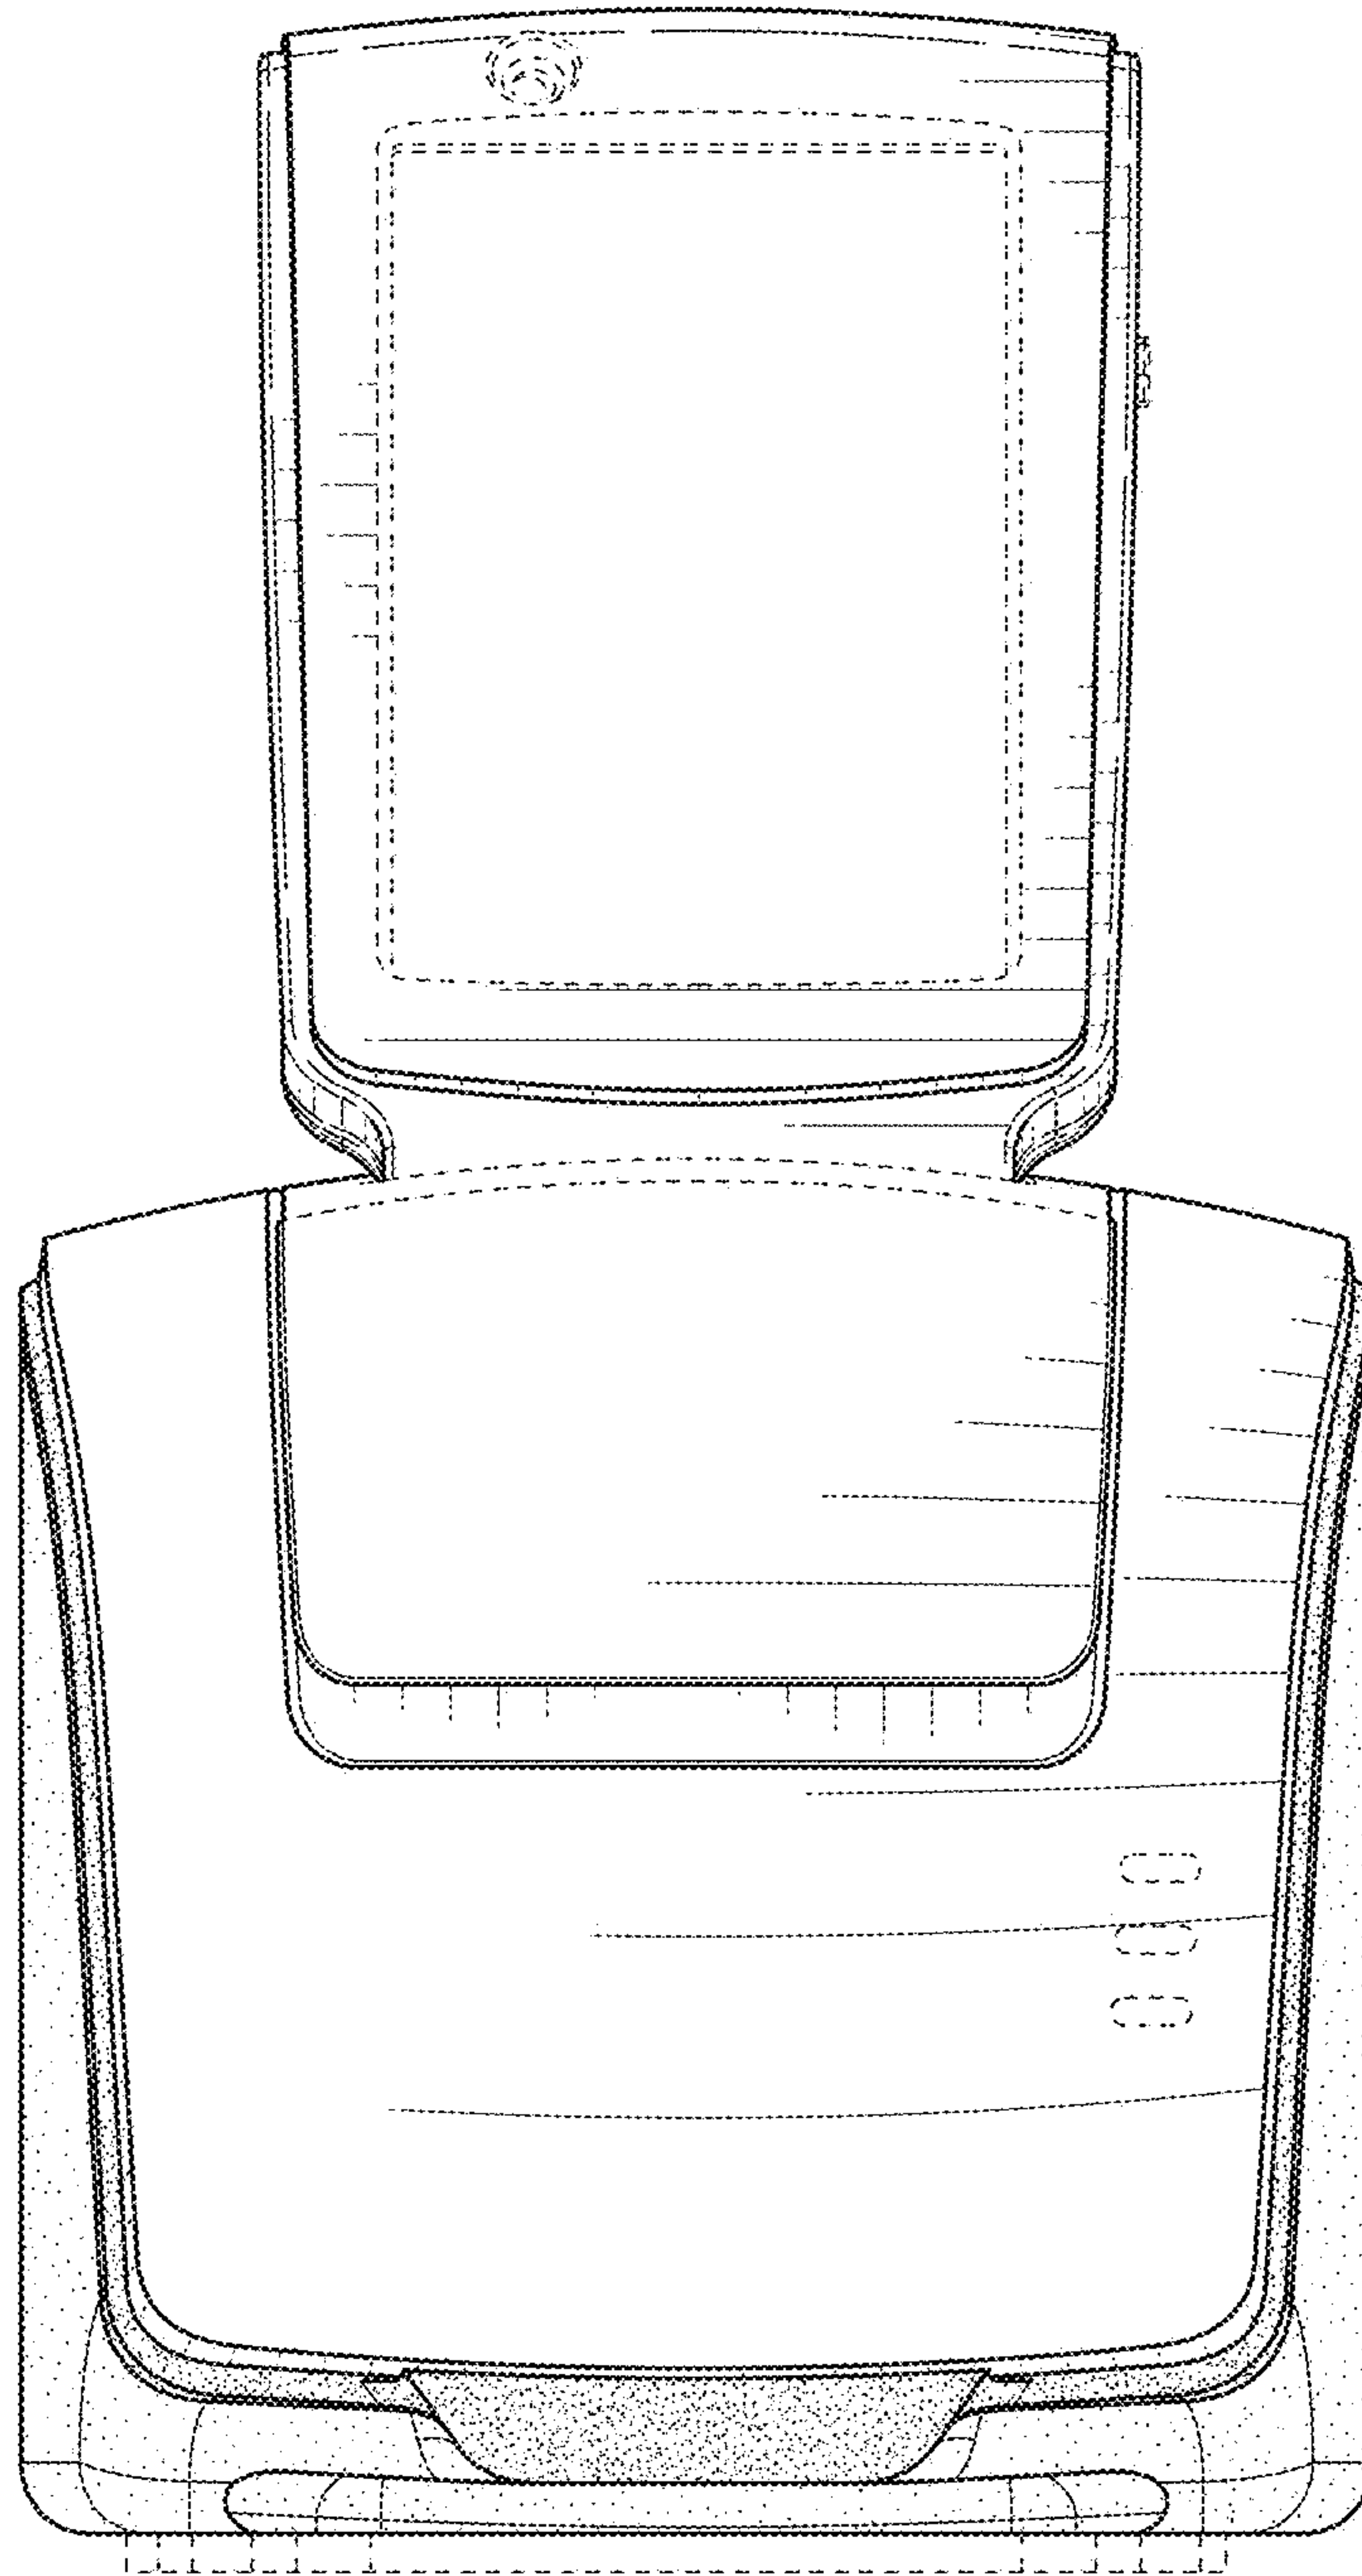


FIG. 11

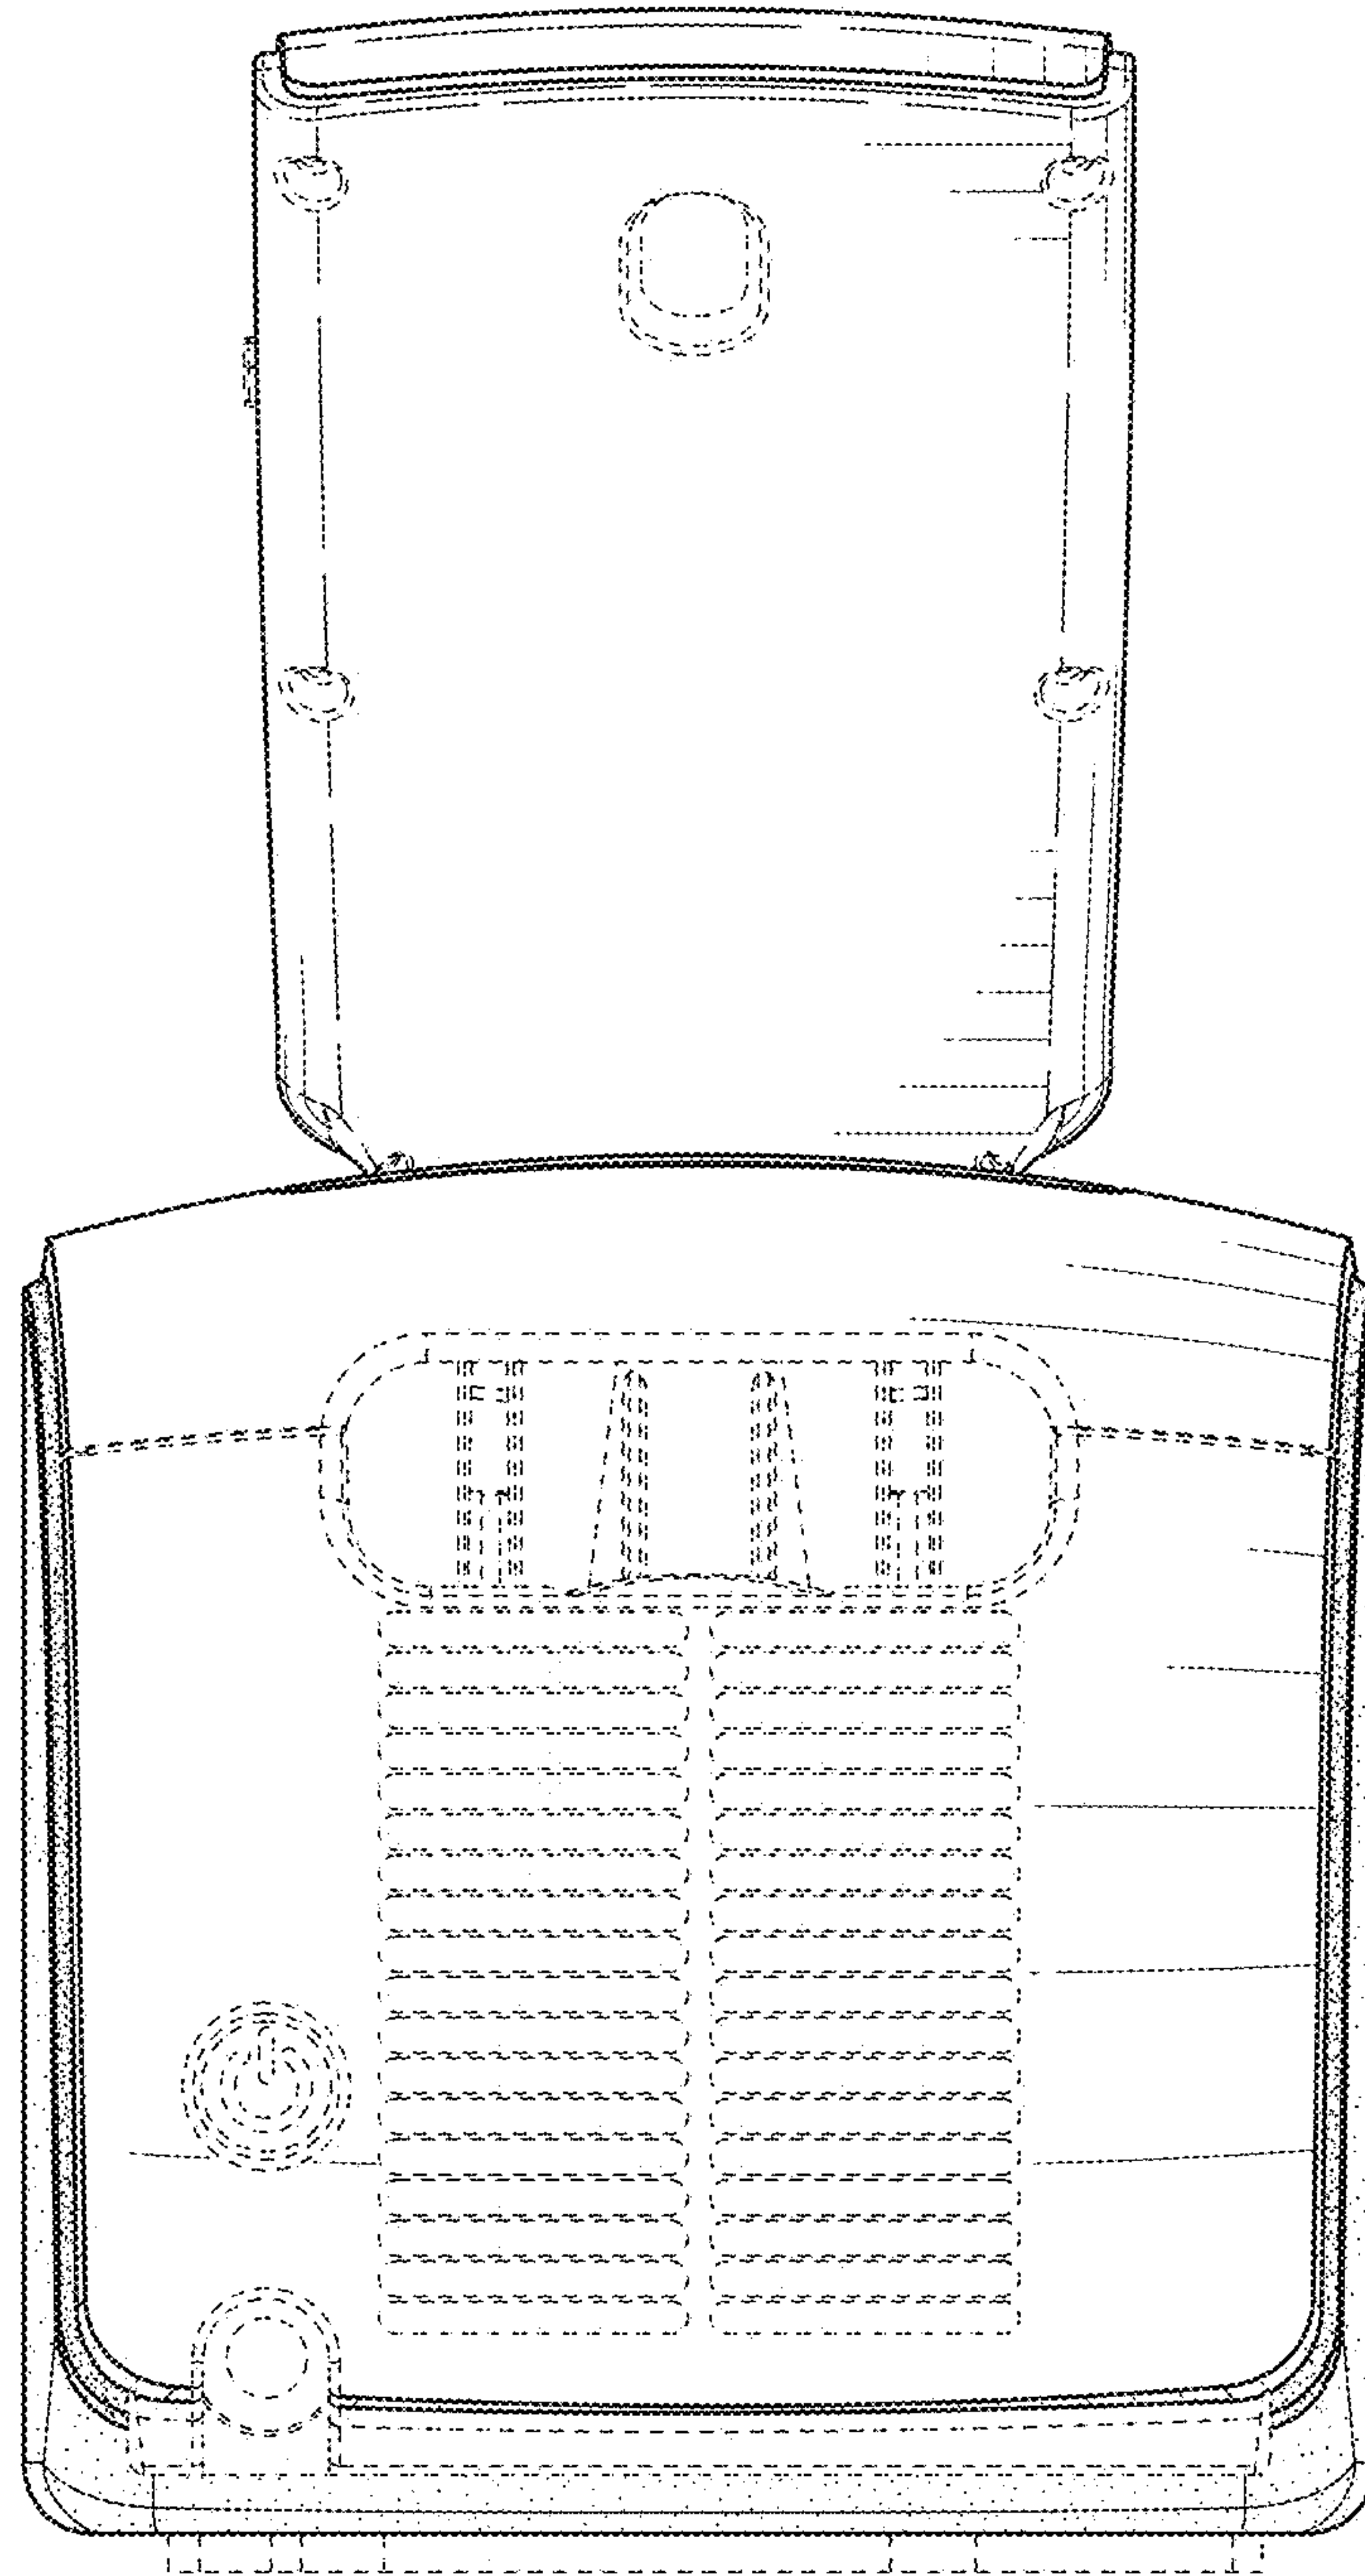


FIG. 12

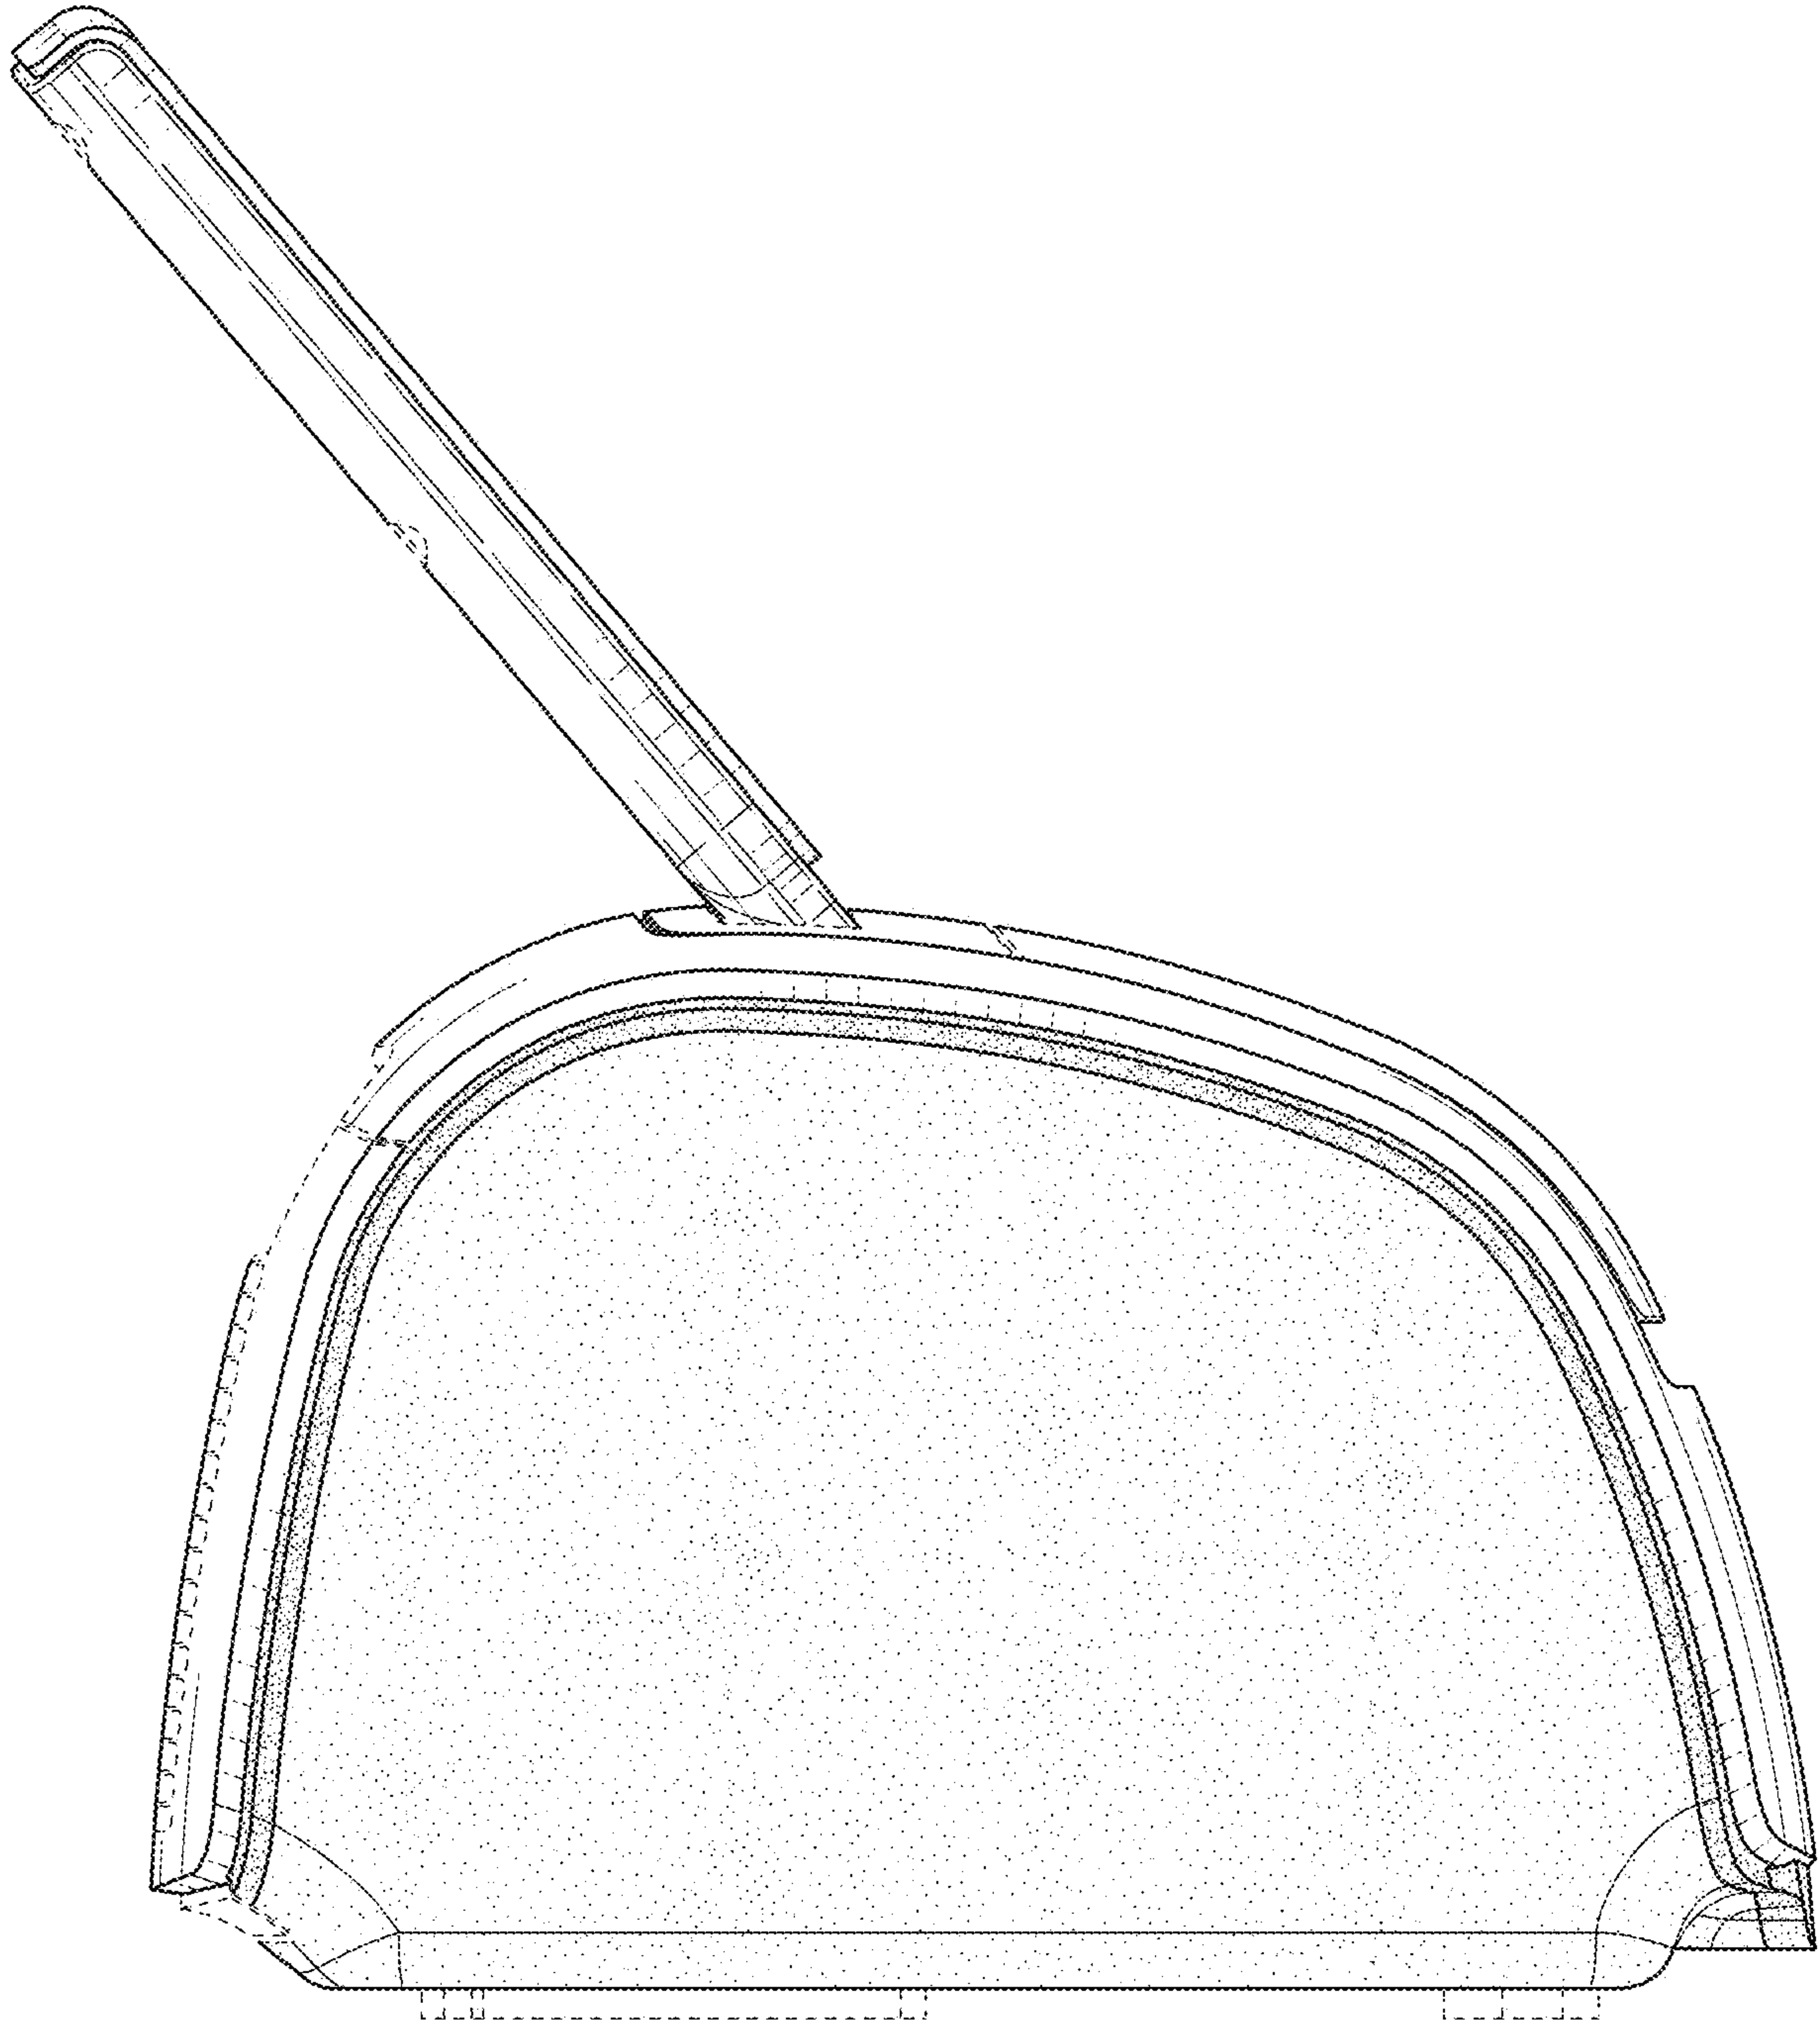


FIG. 13

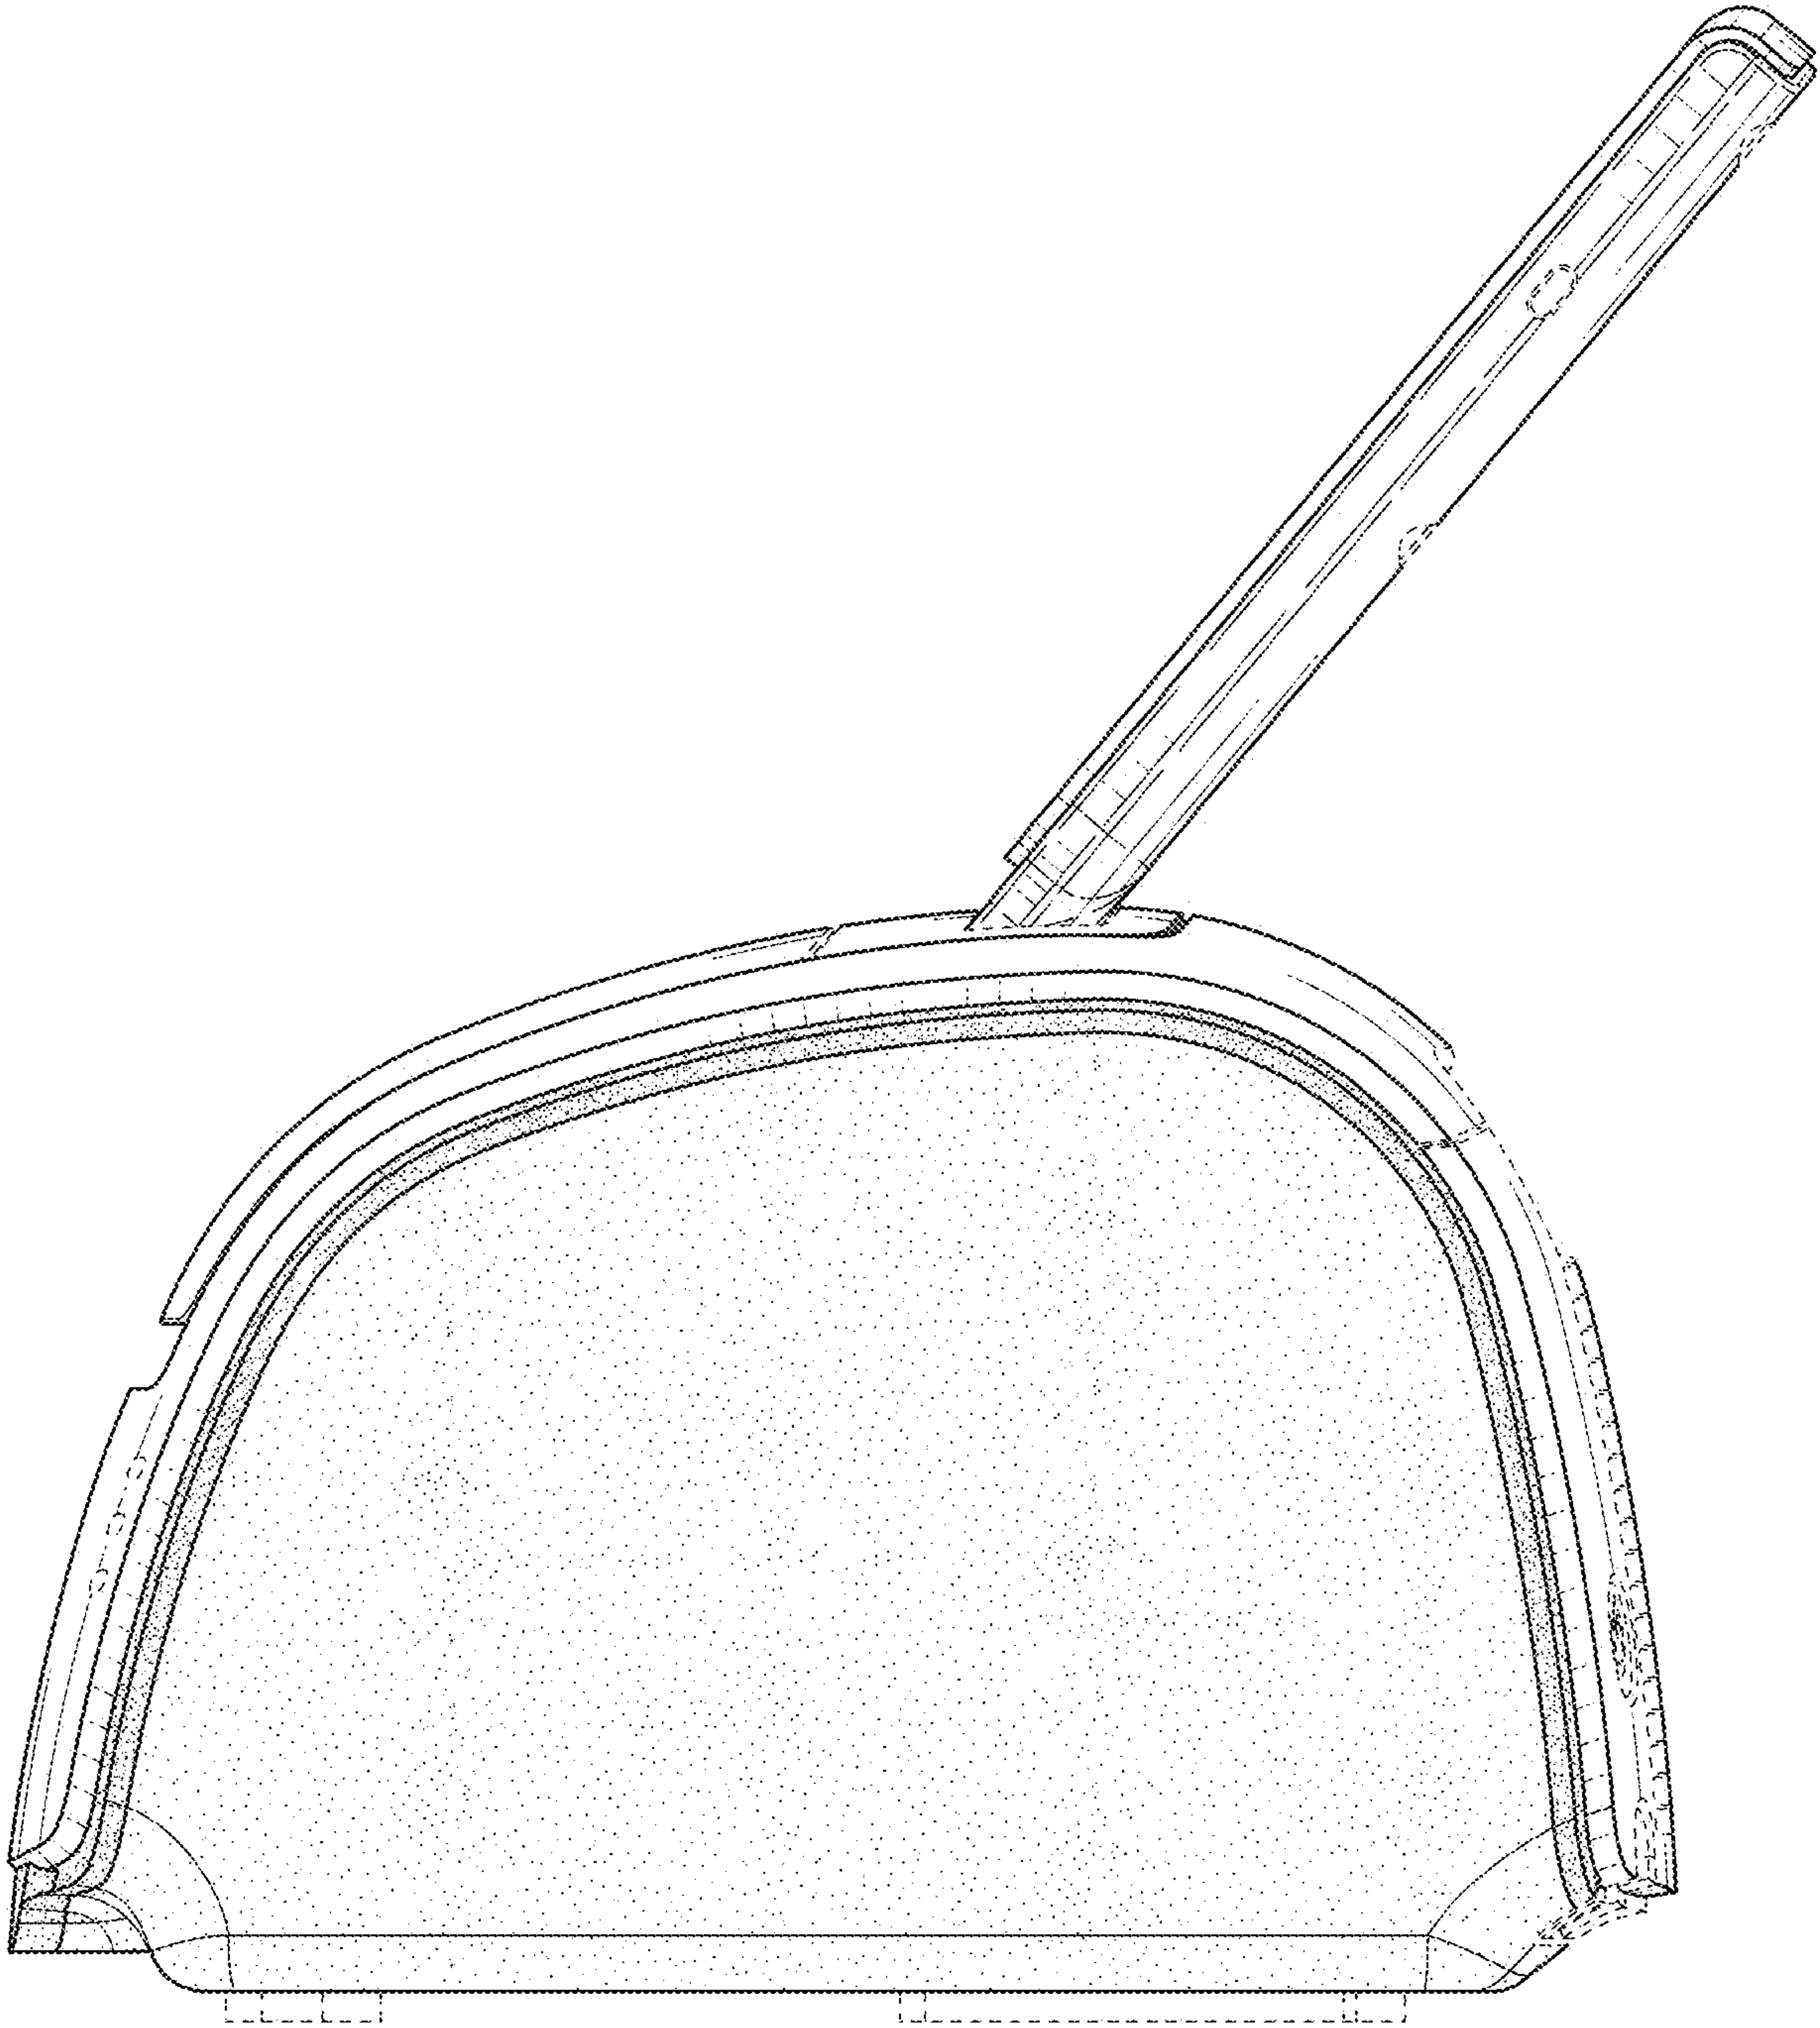


FIG. 14

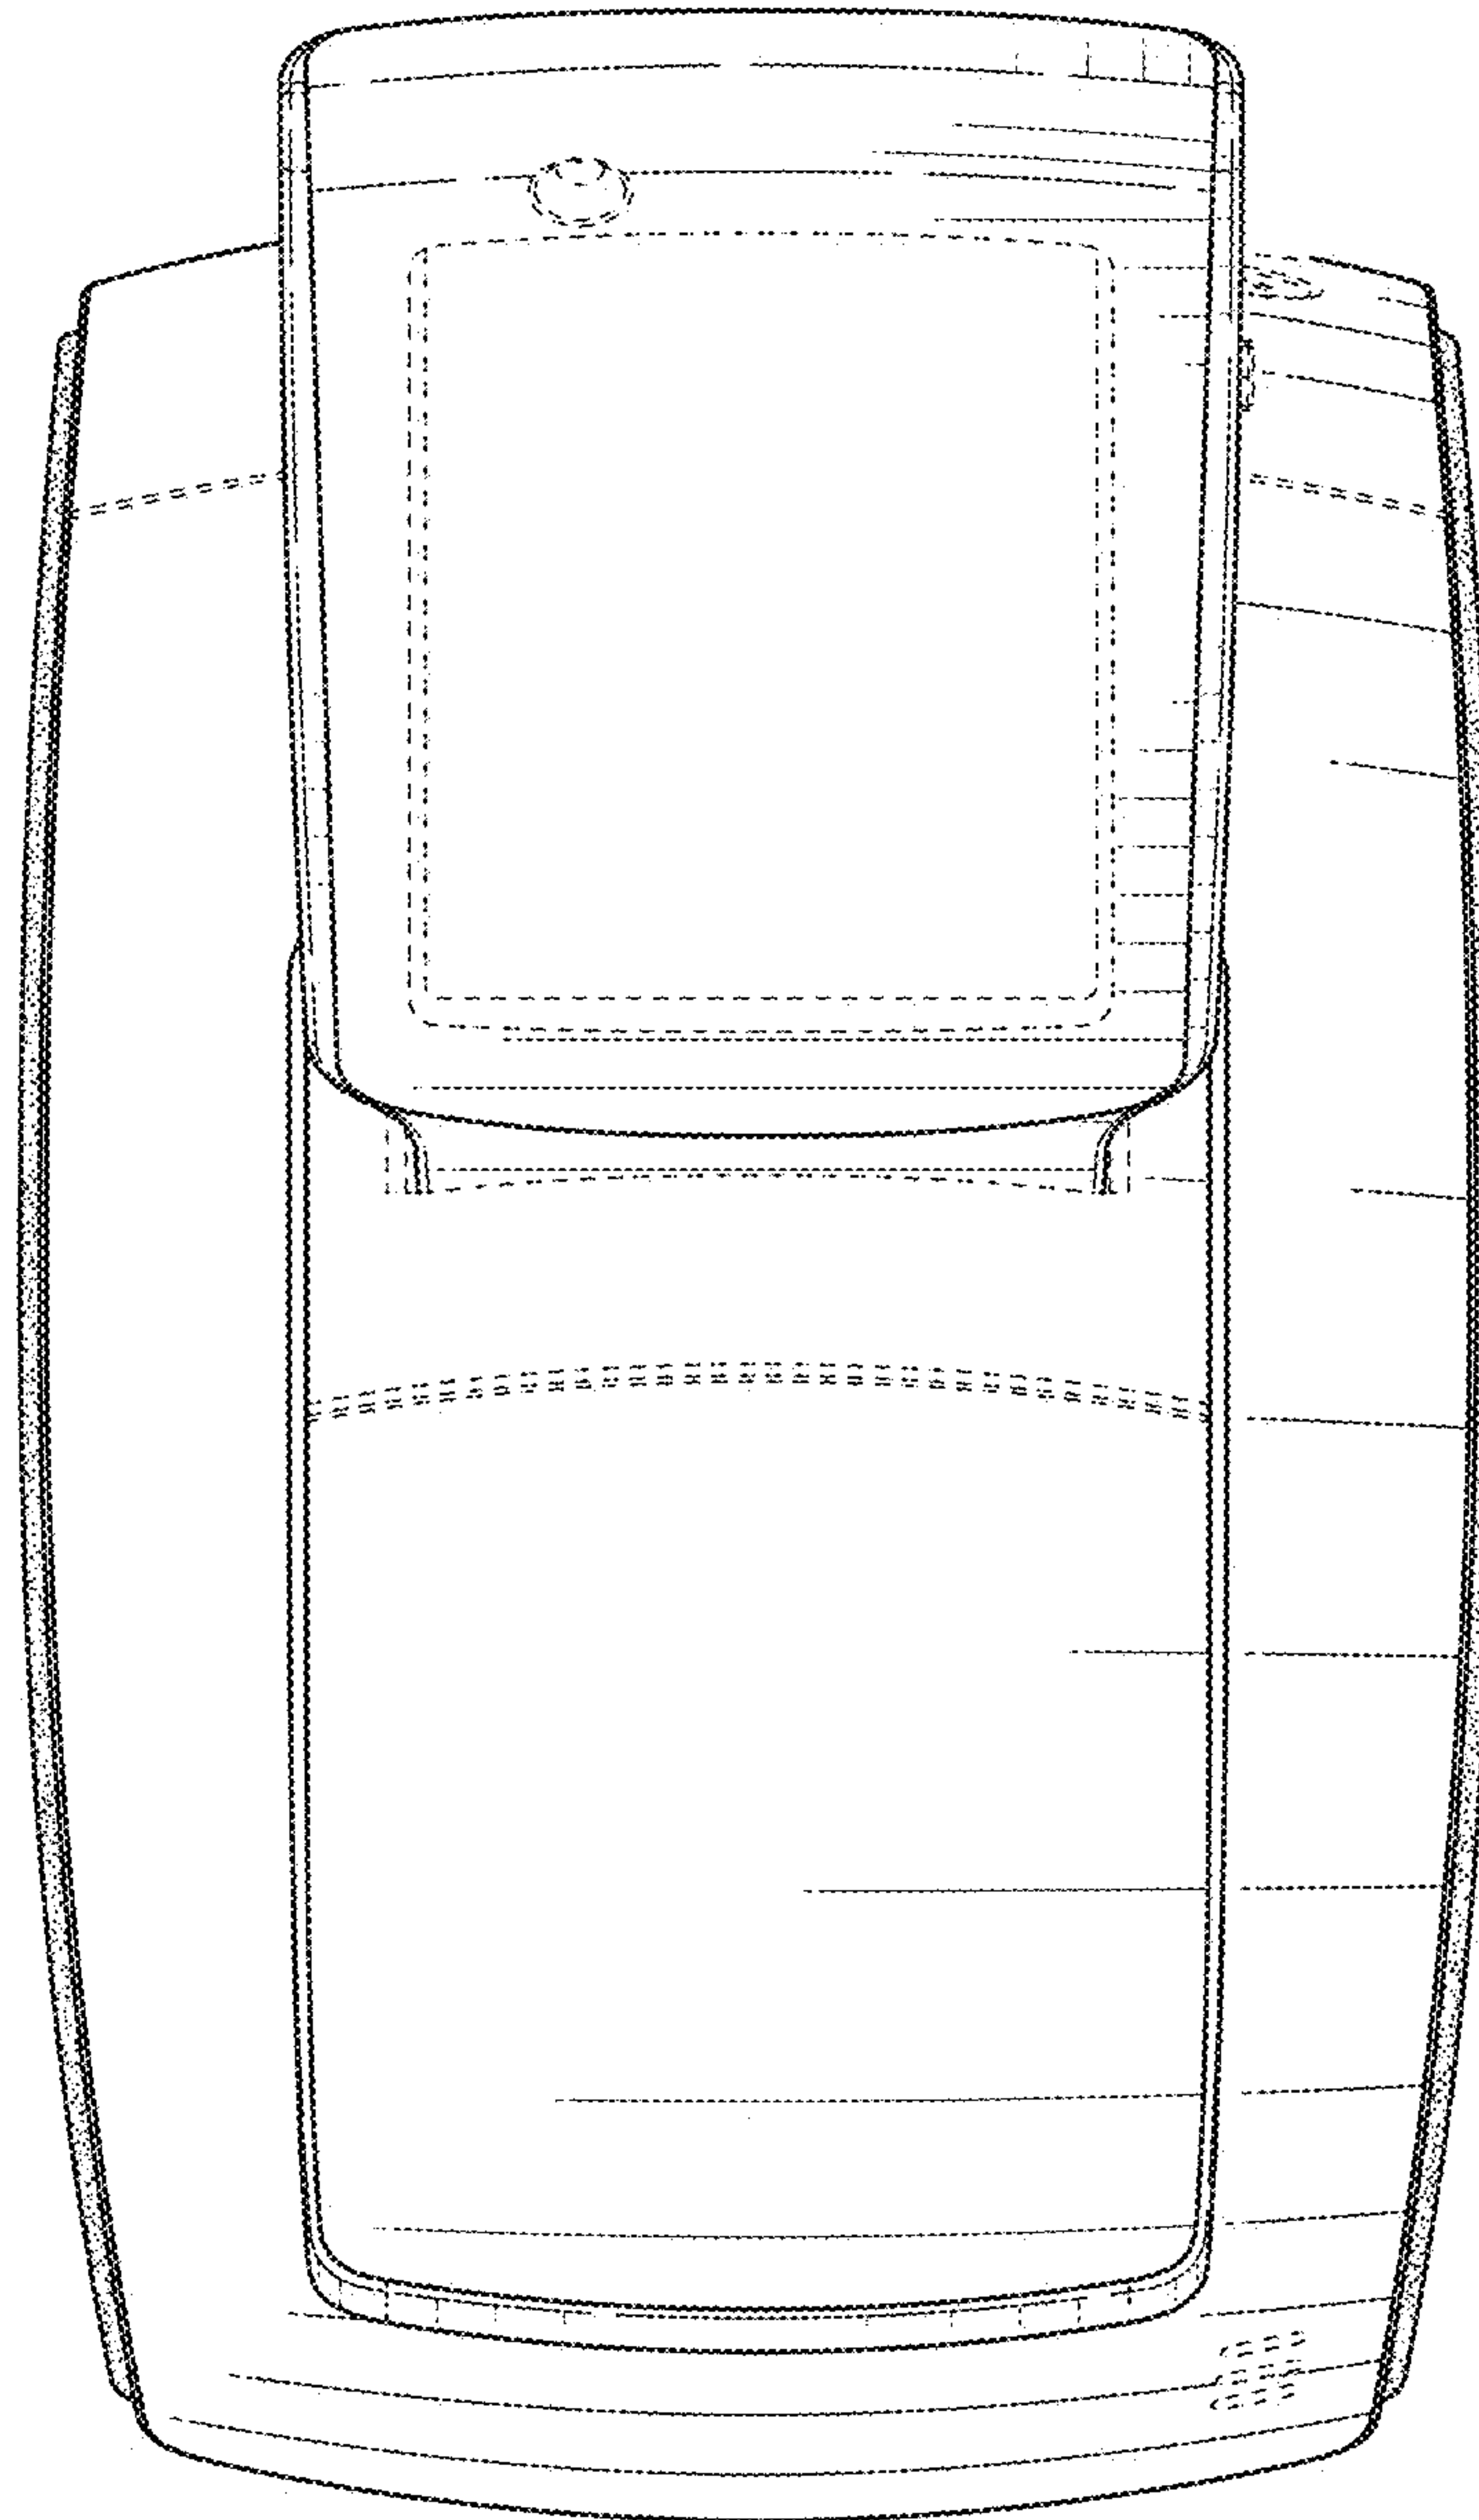


FIG. 15

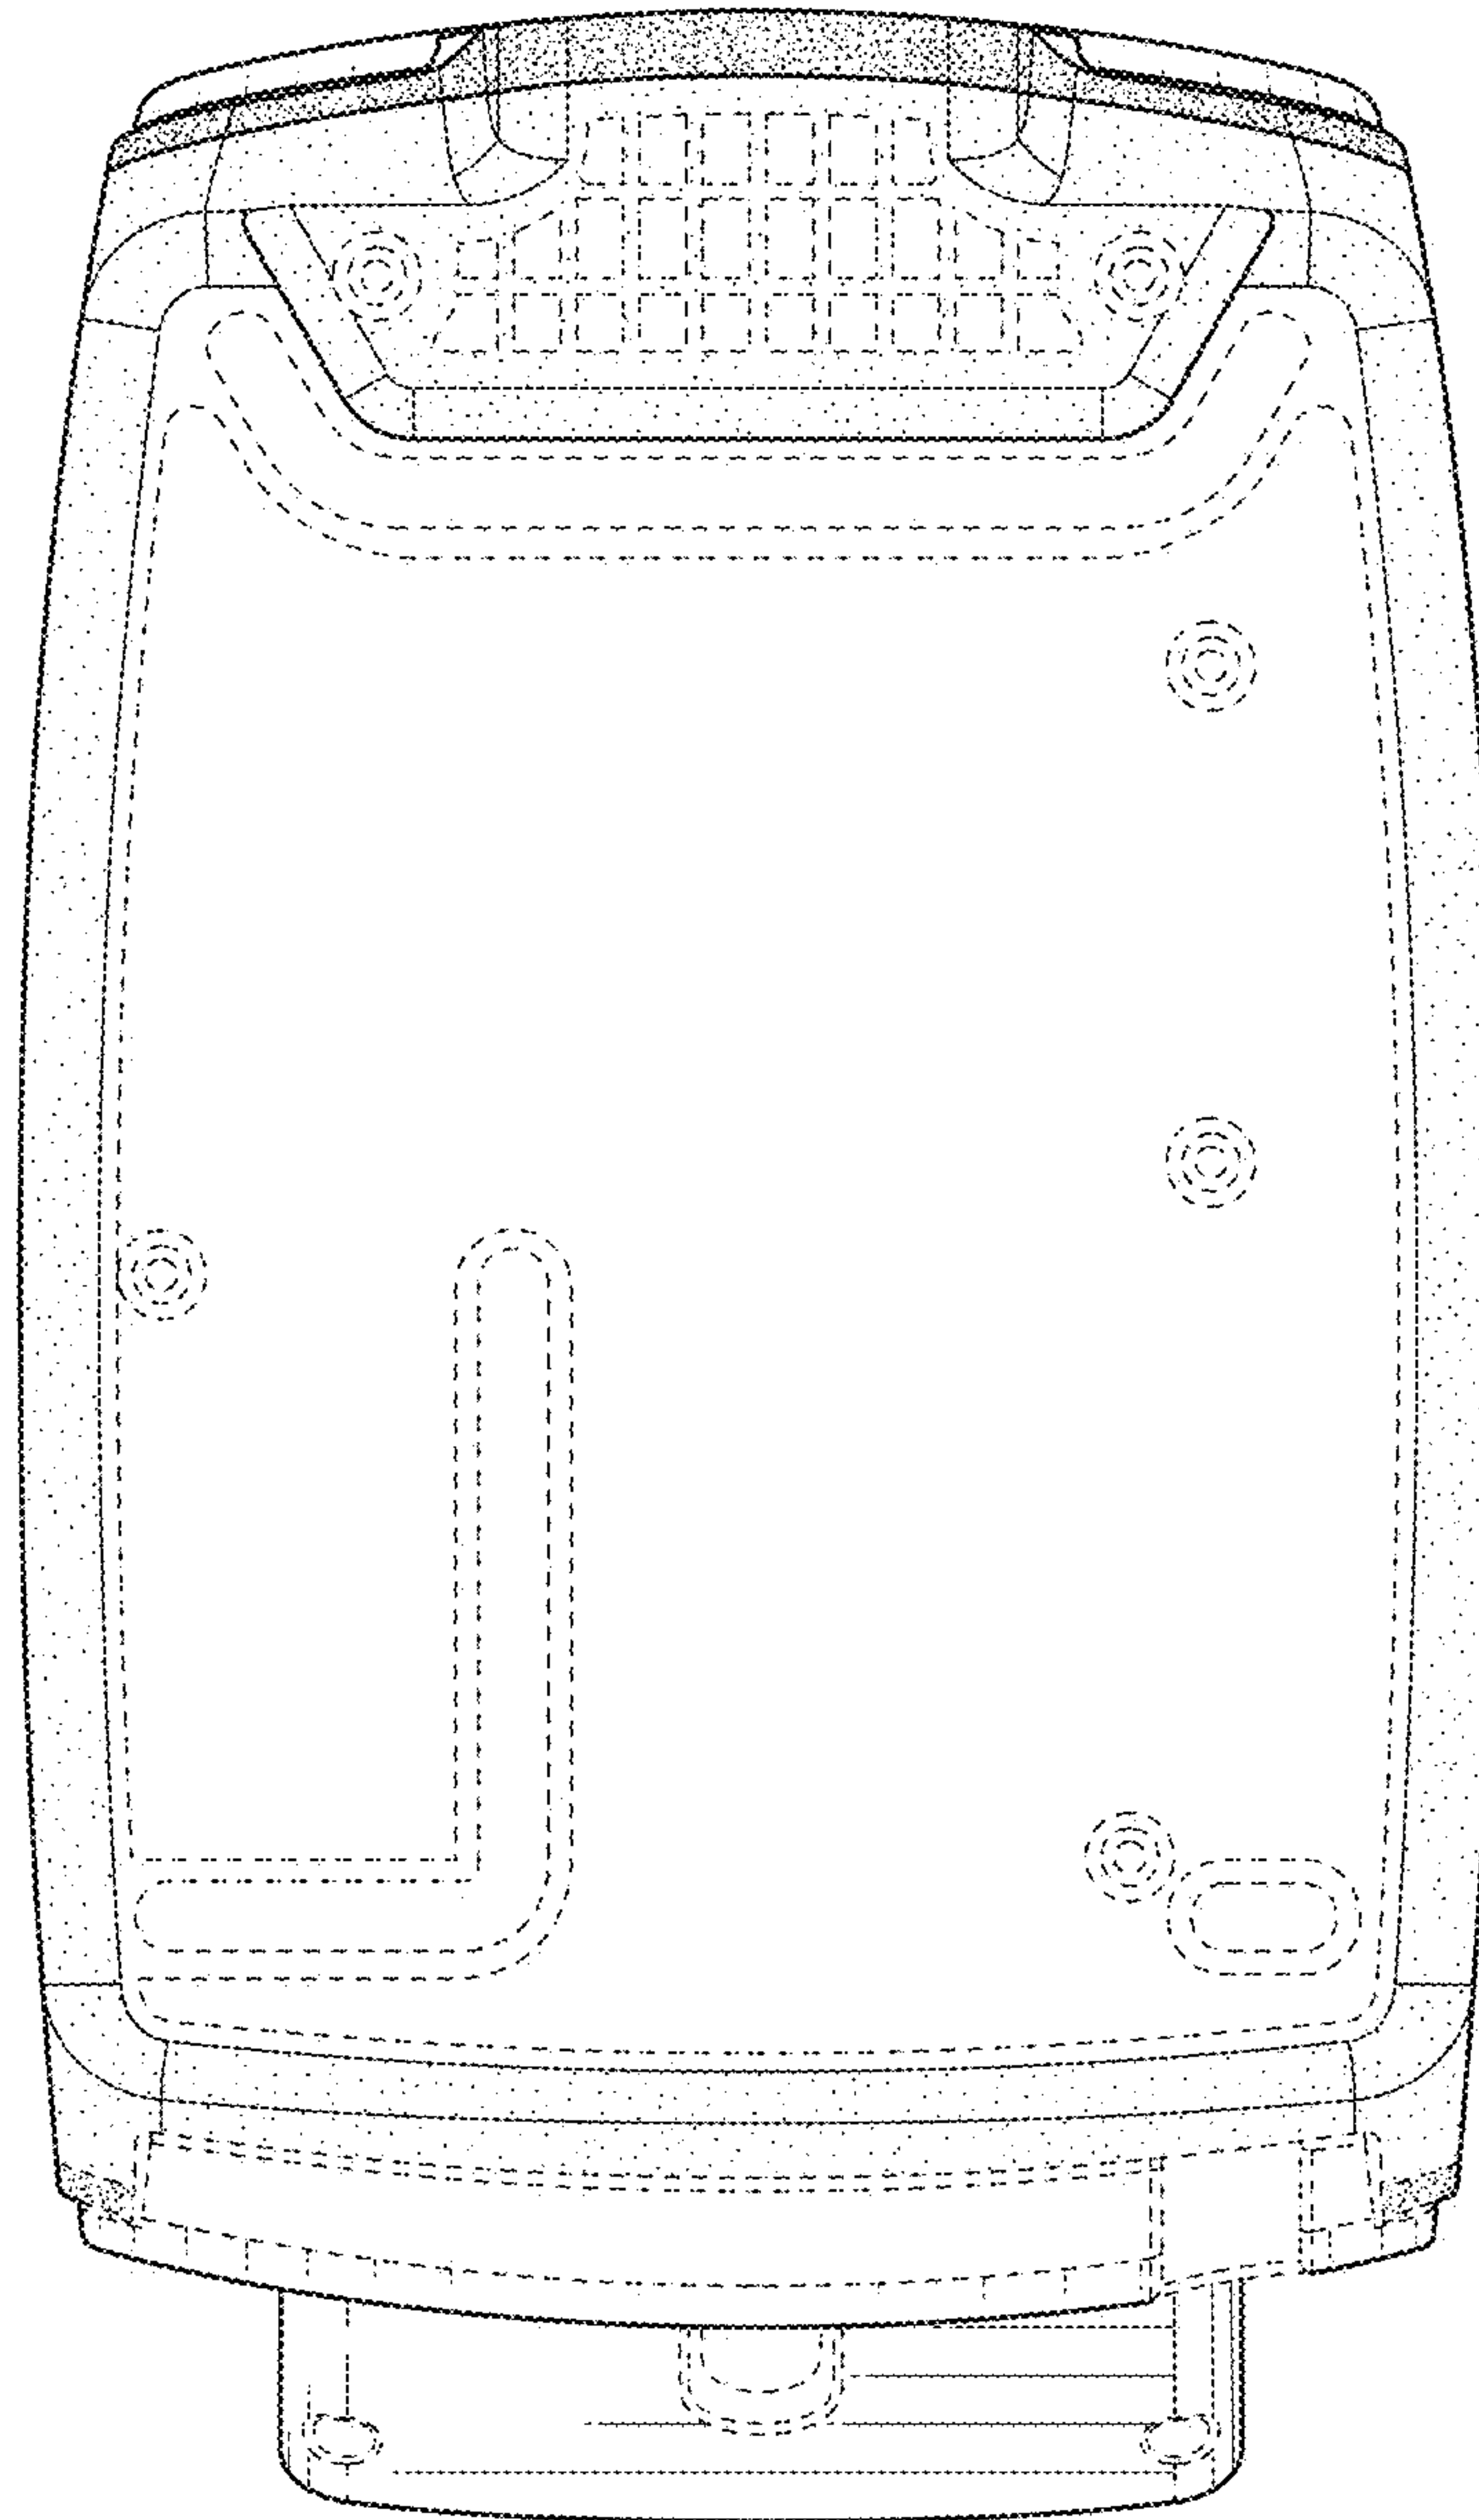


FIG. 16

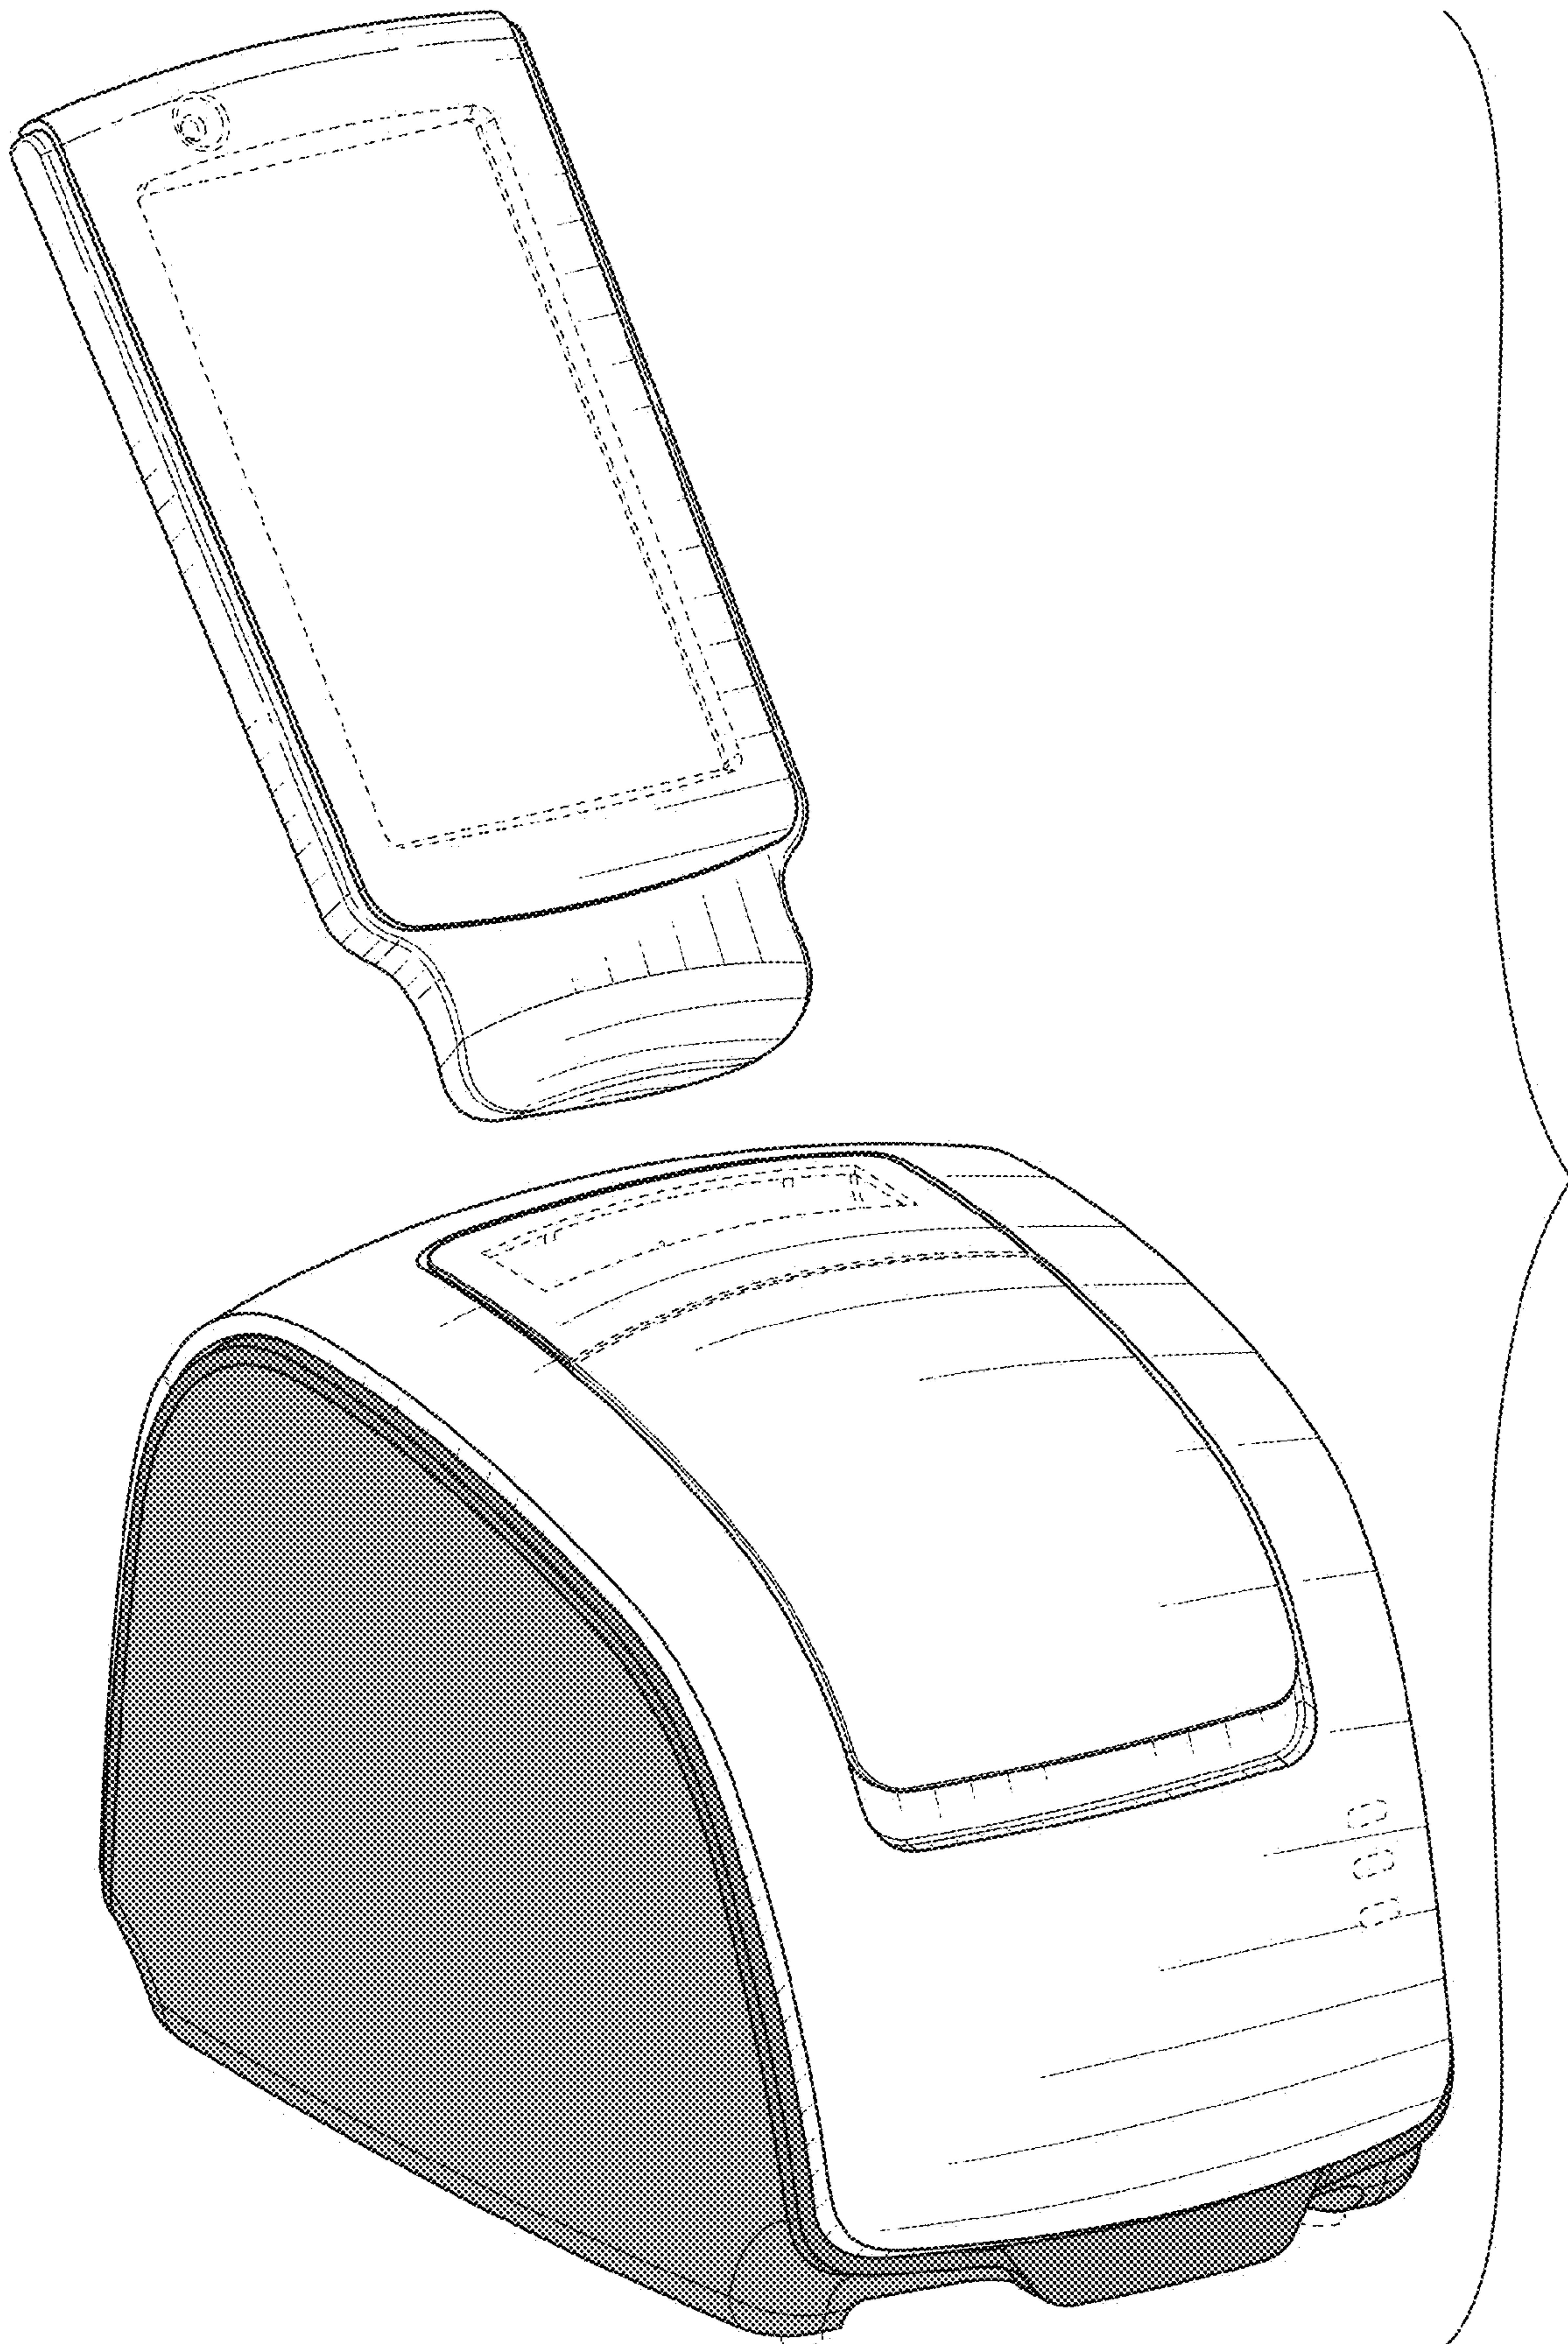


FIG. 17

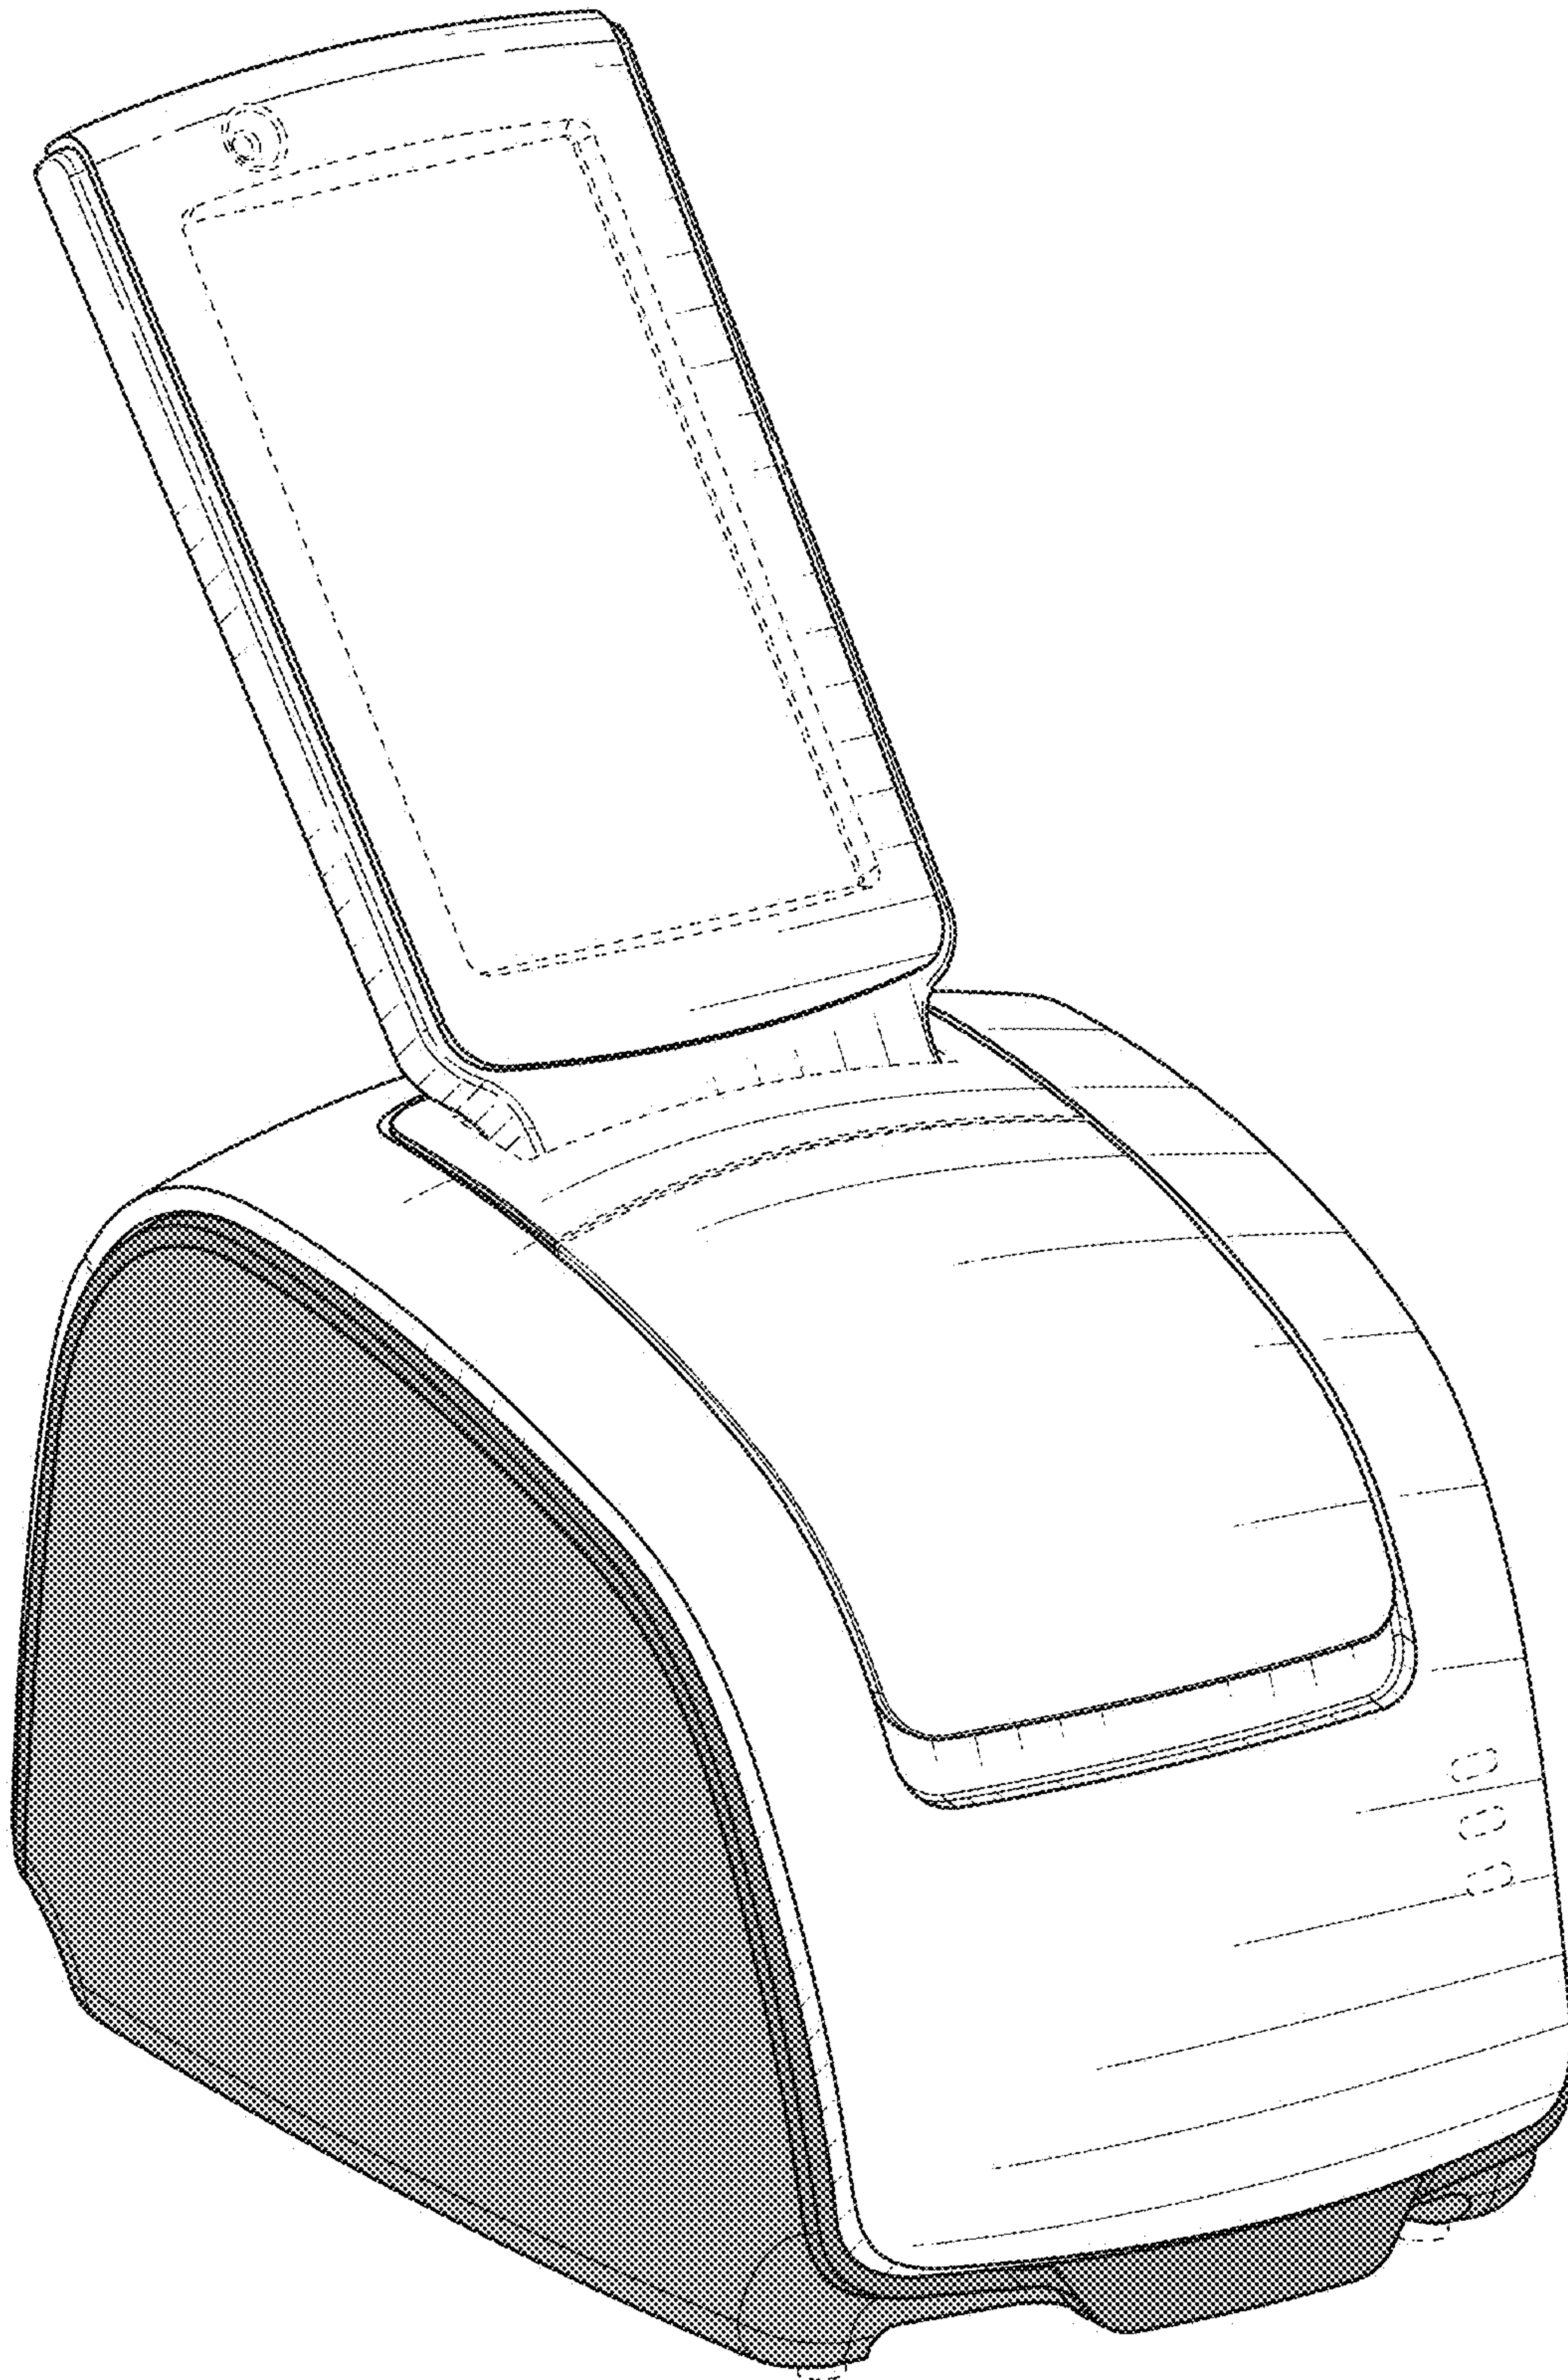


FIG. 18

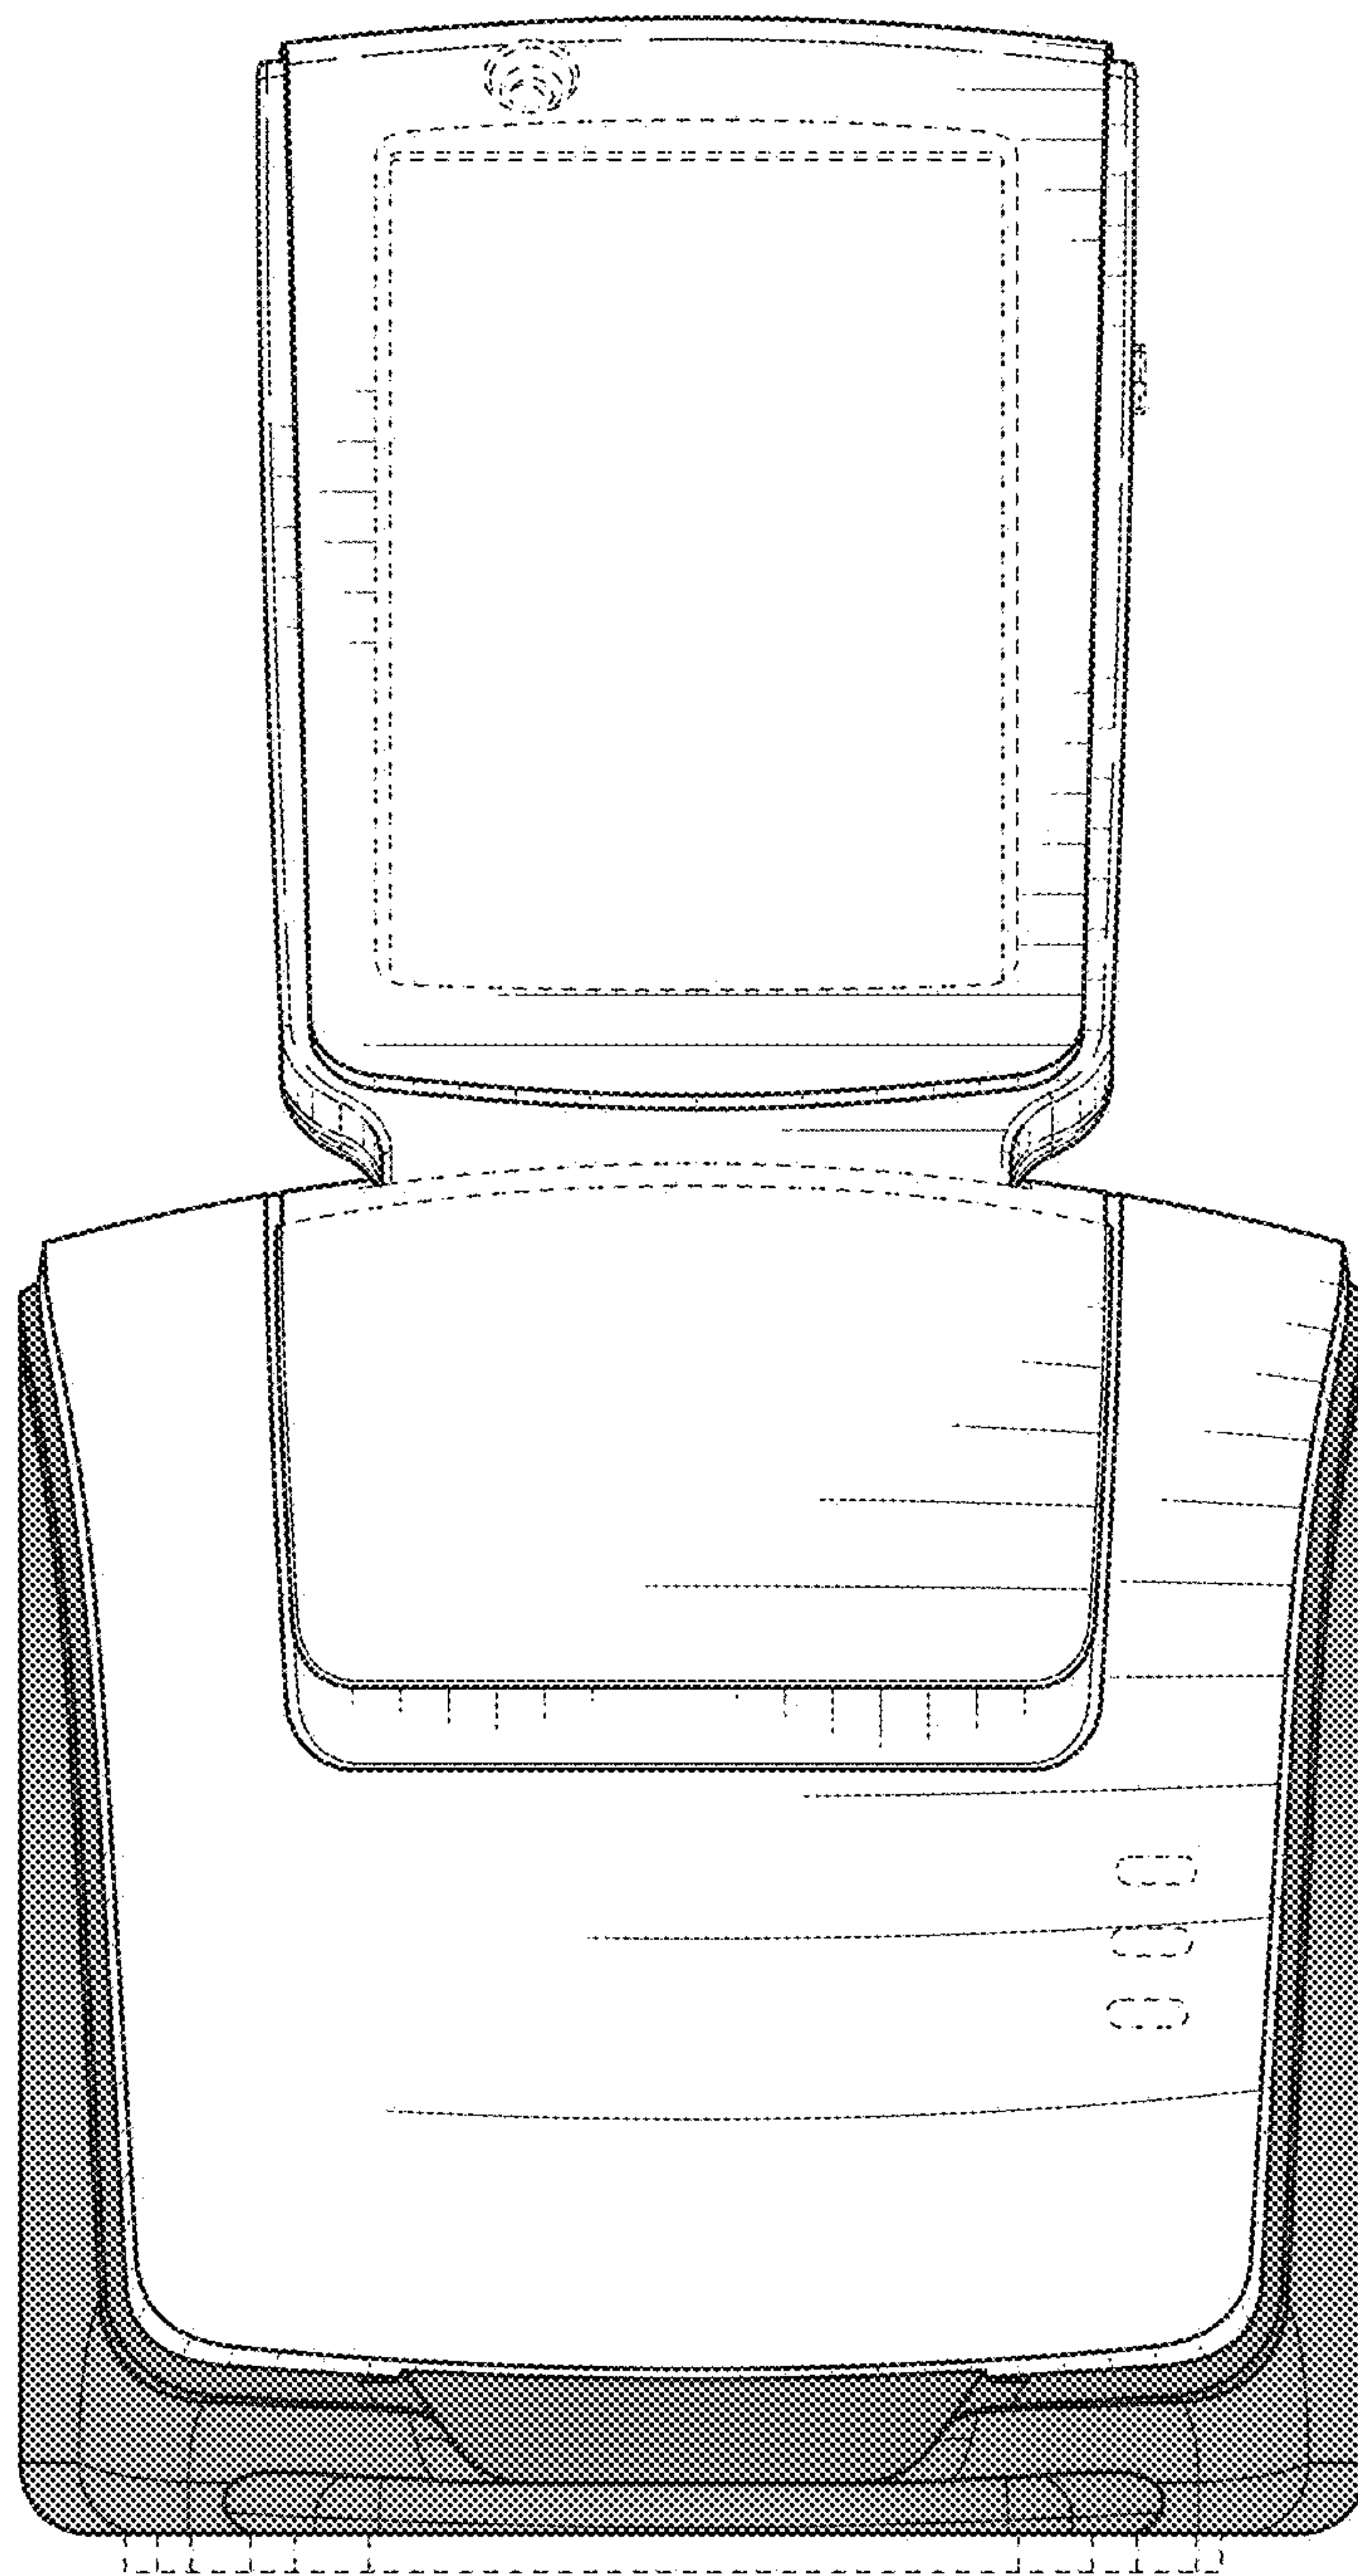


FIG. 19

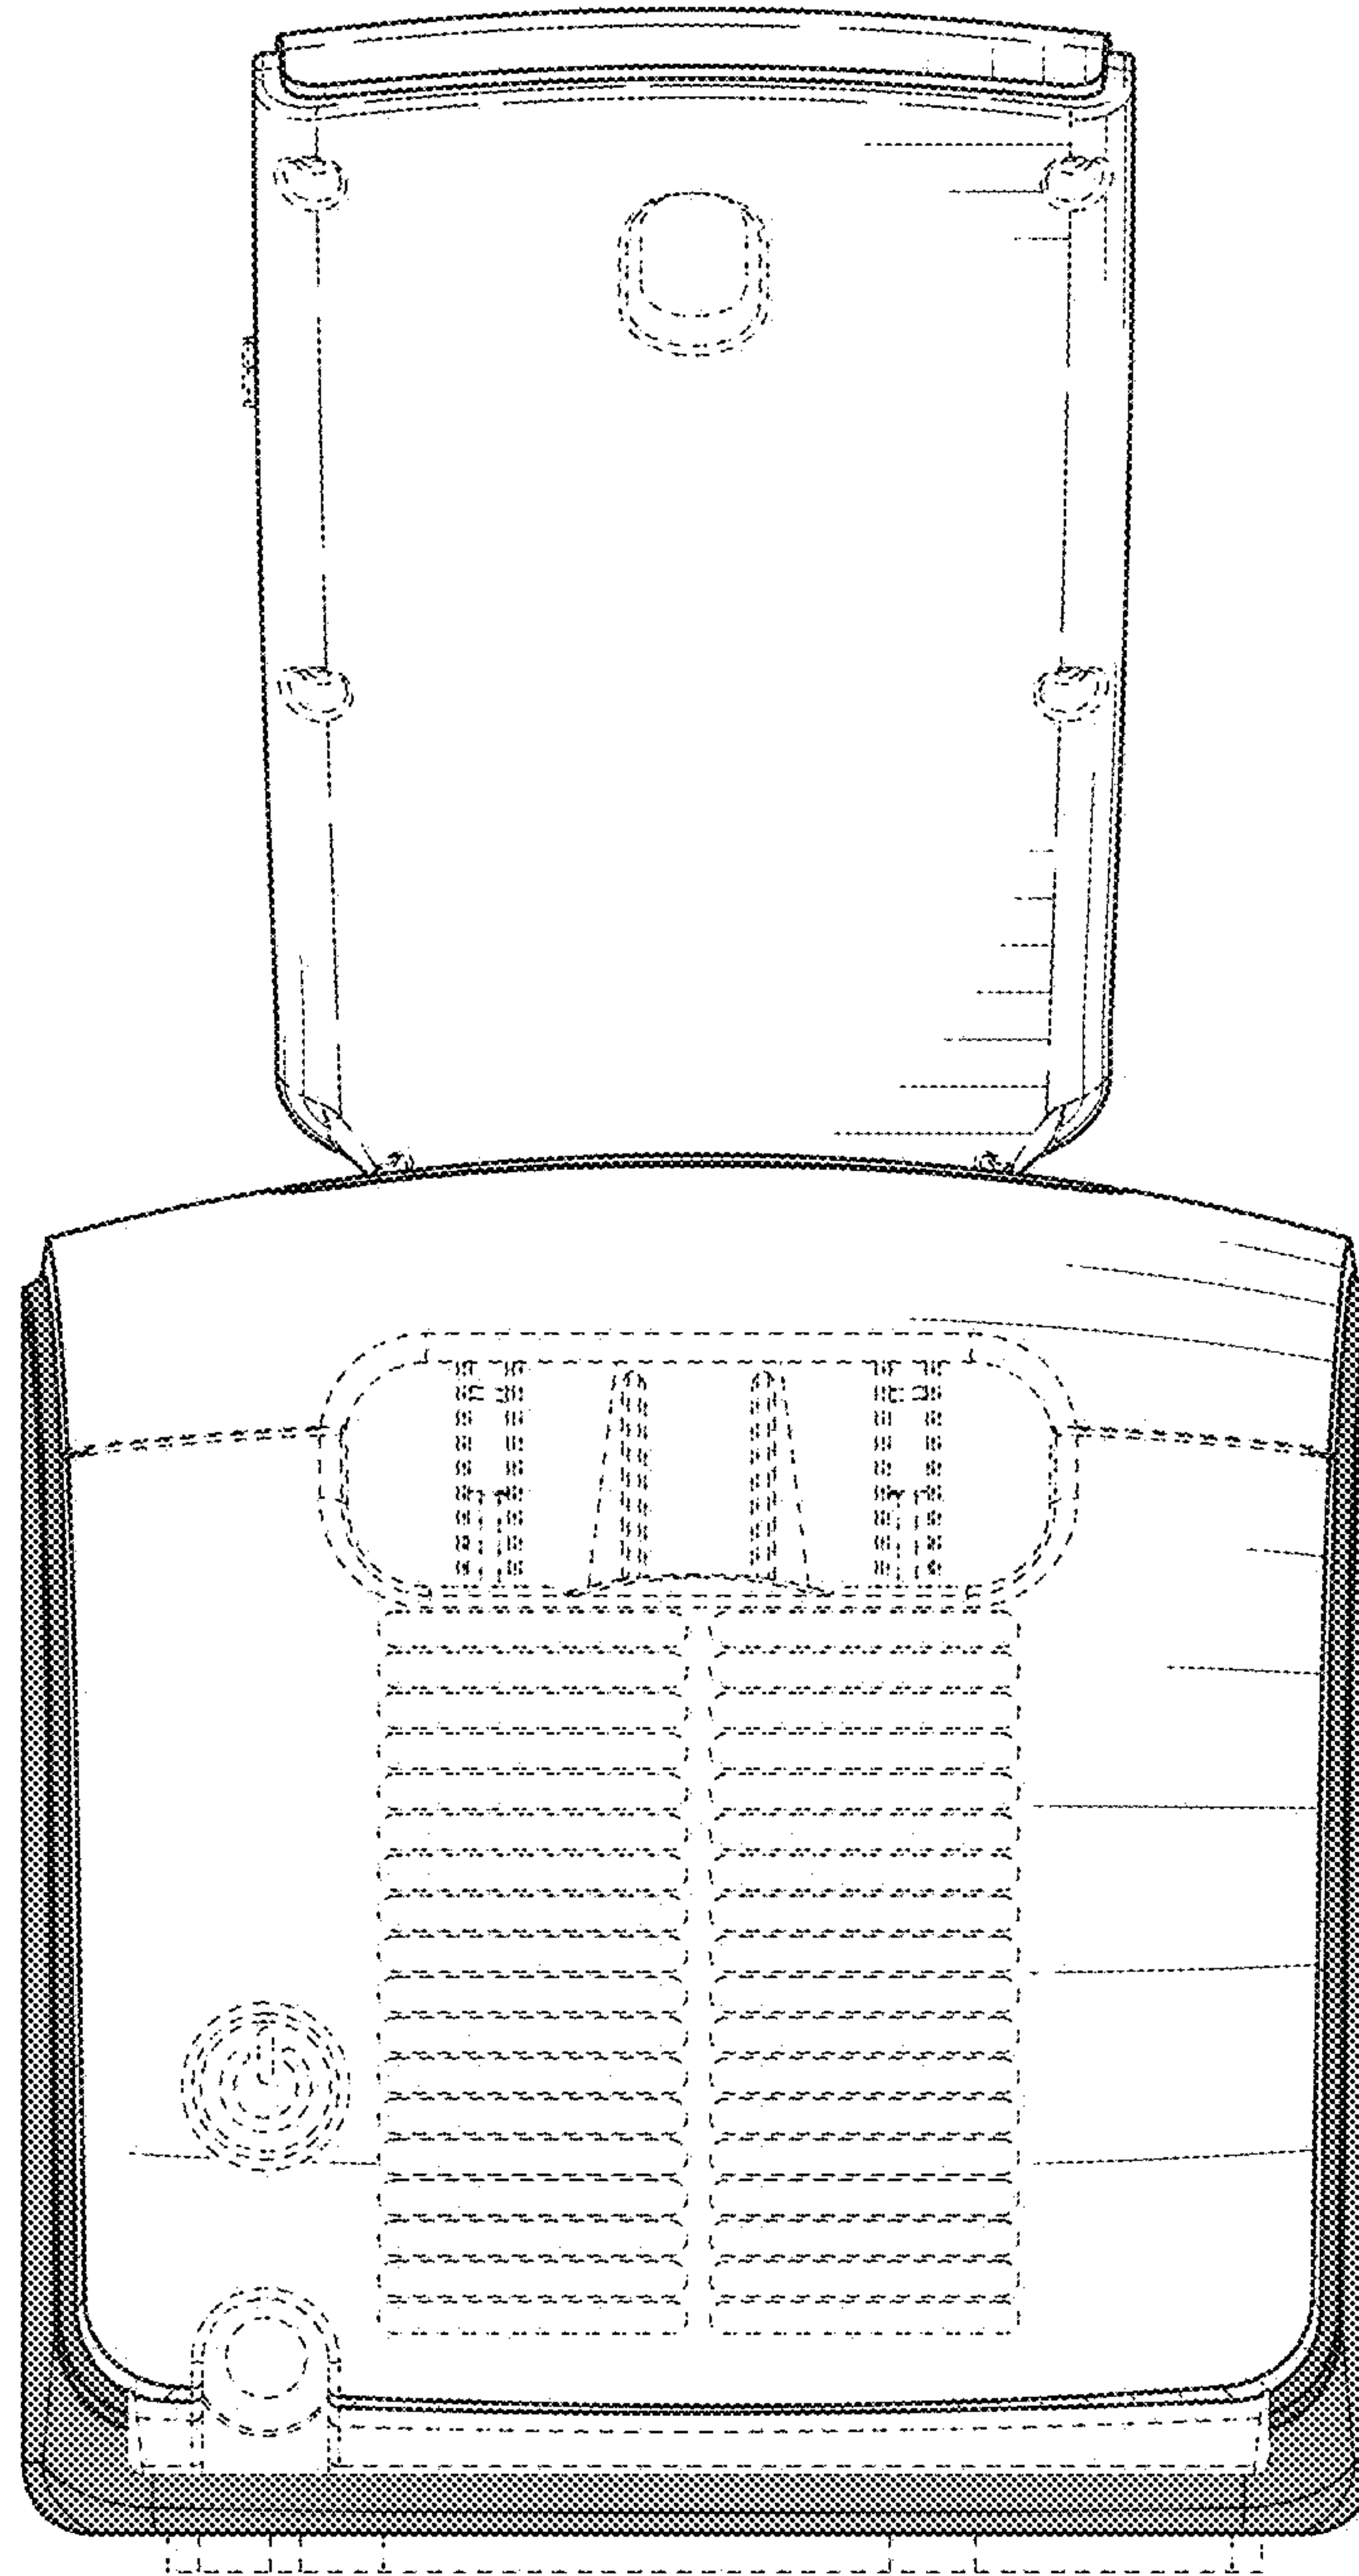


FIG. 20

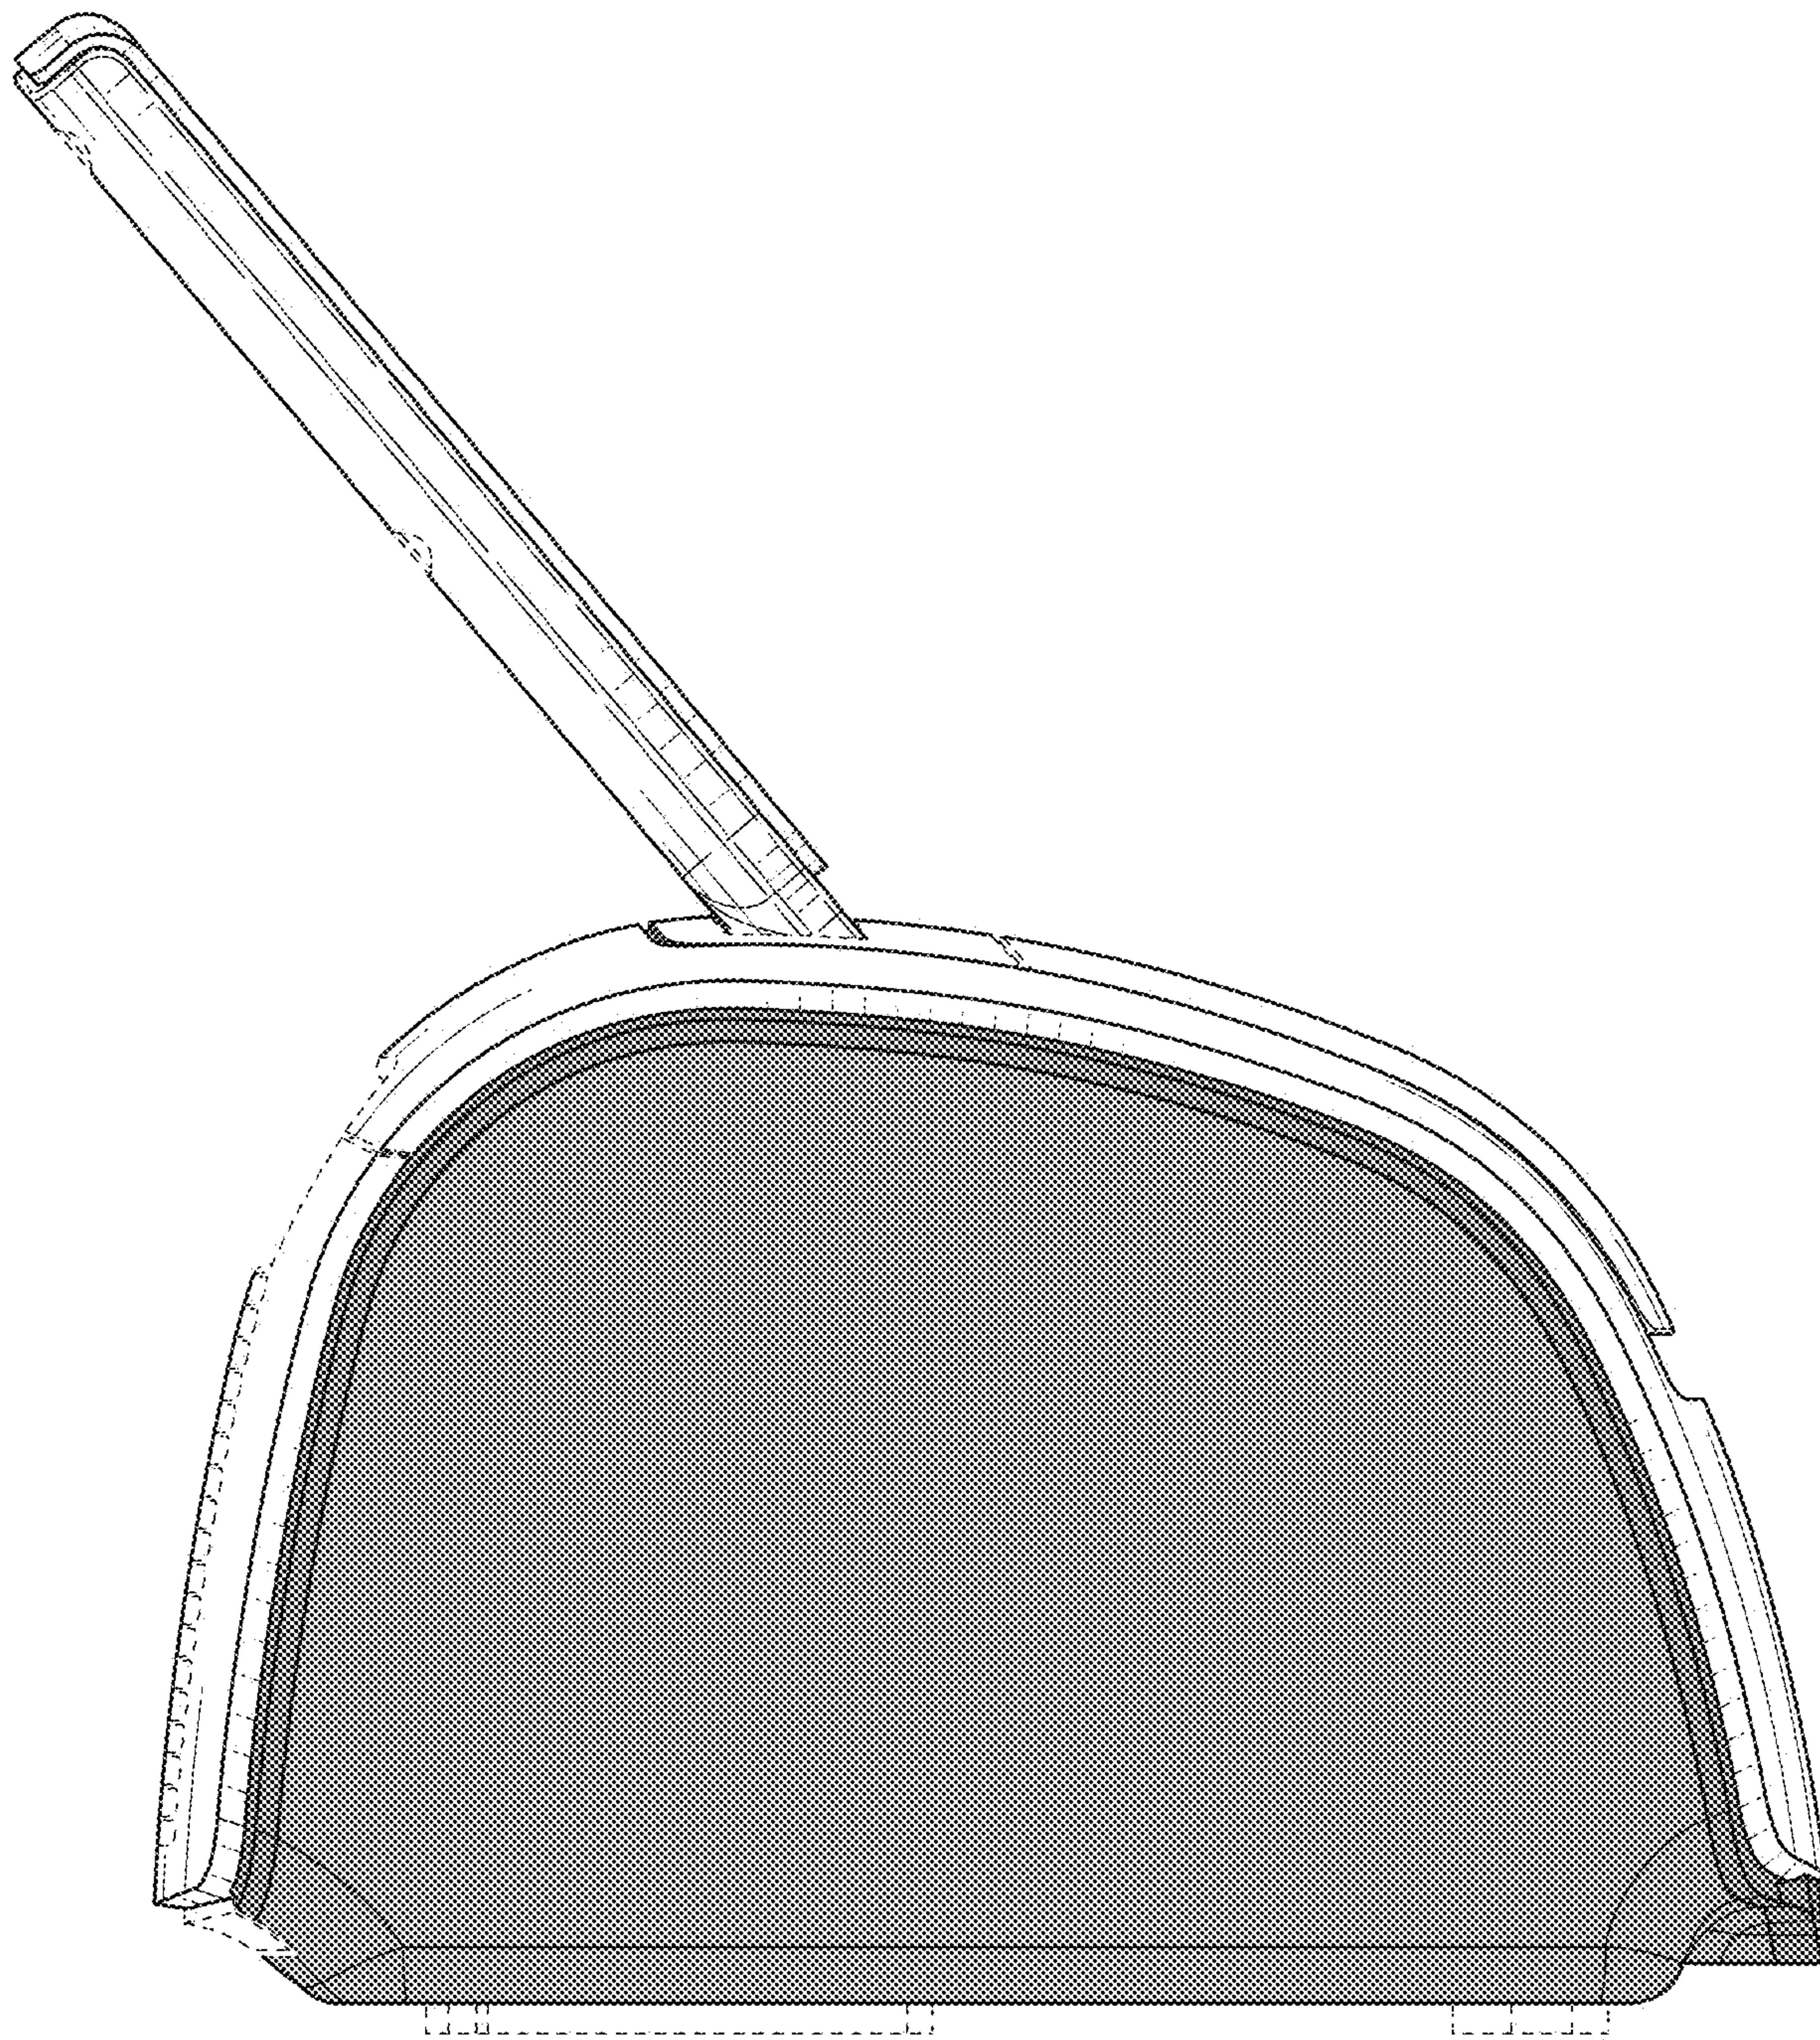


FIG. 21

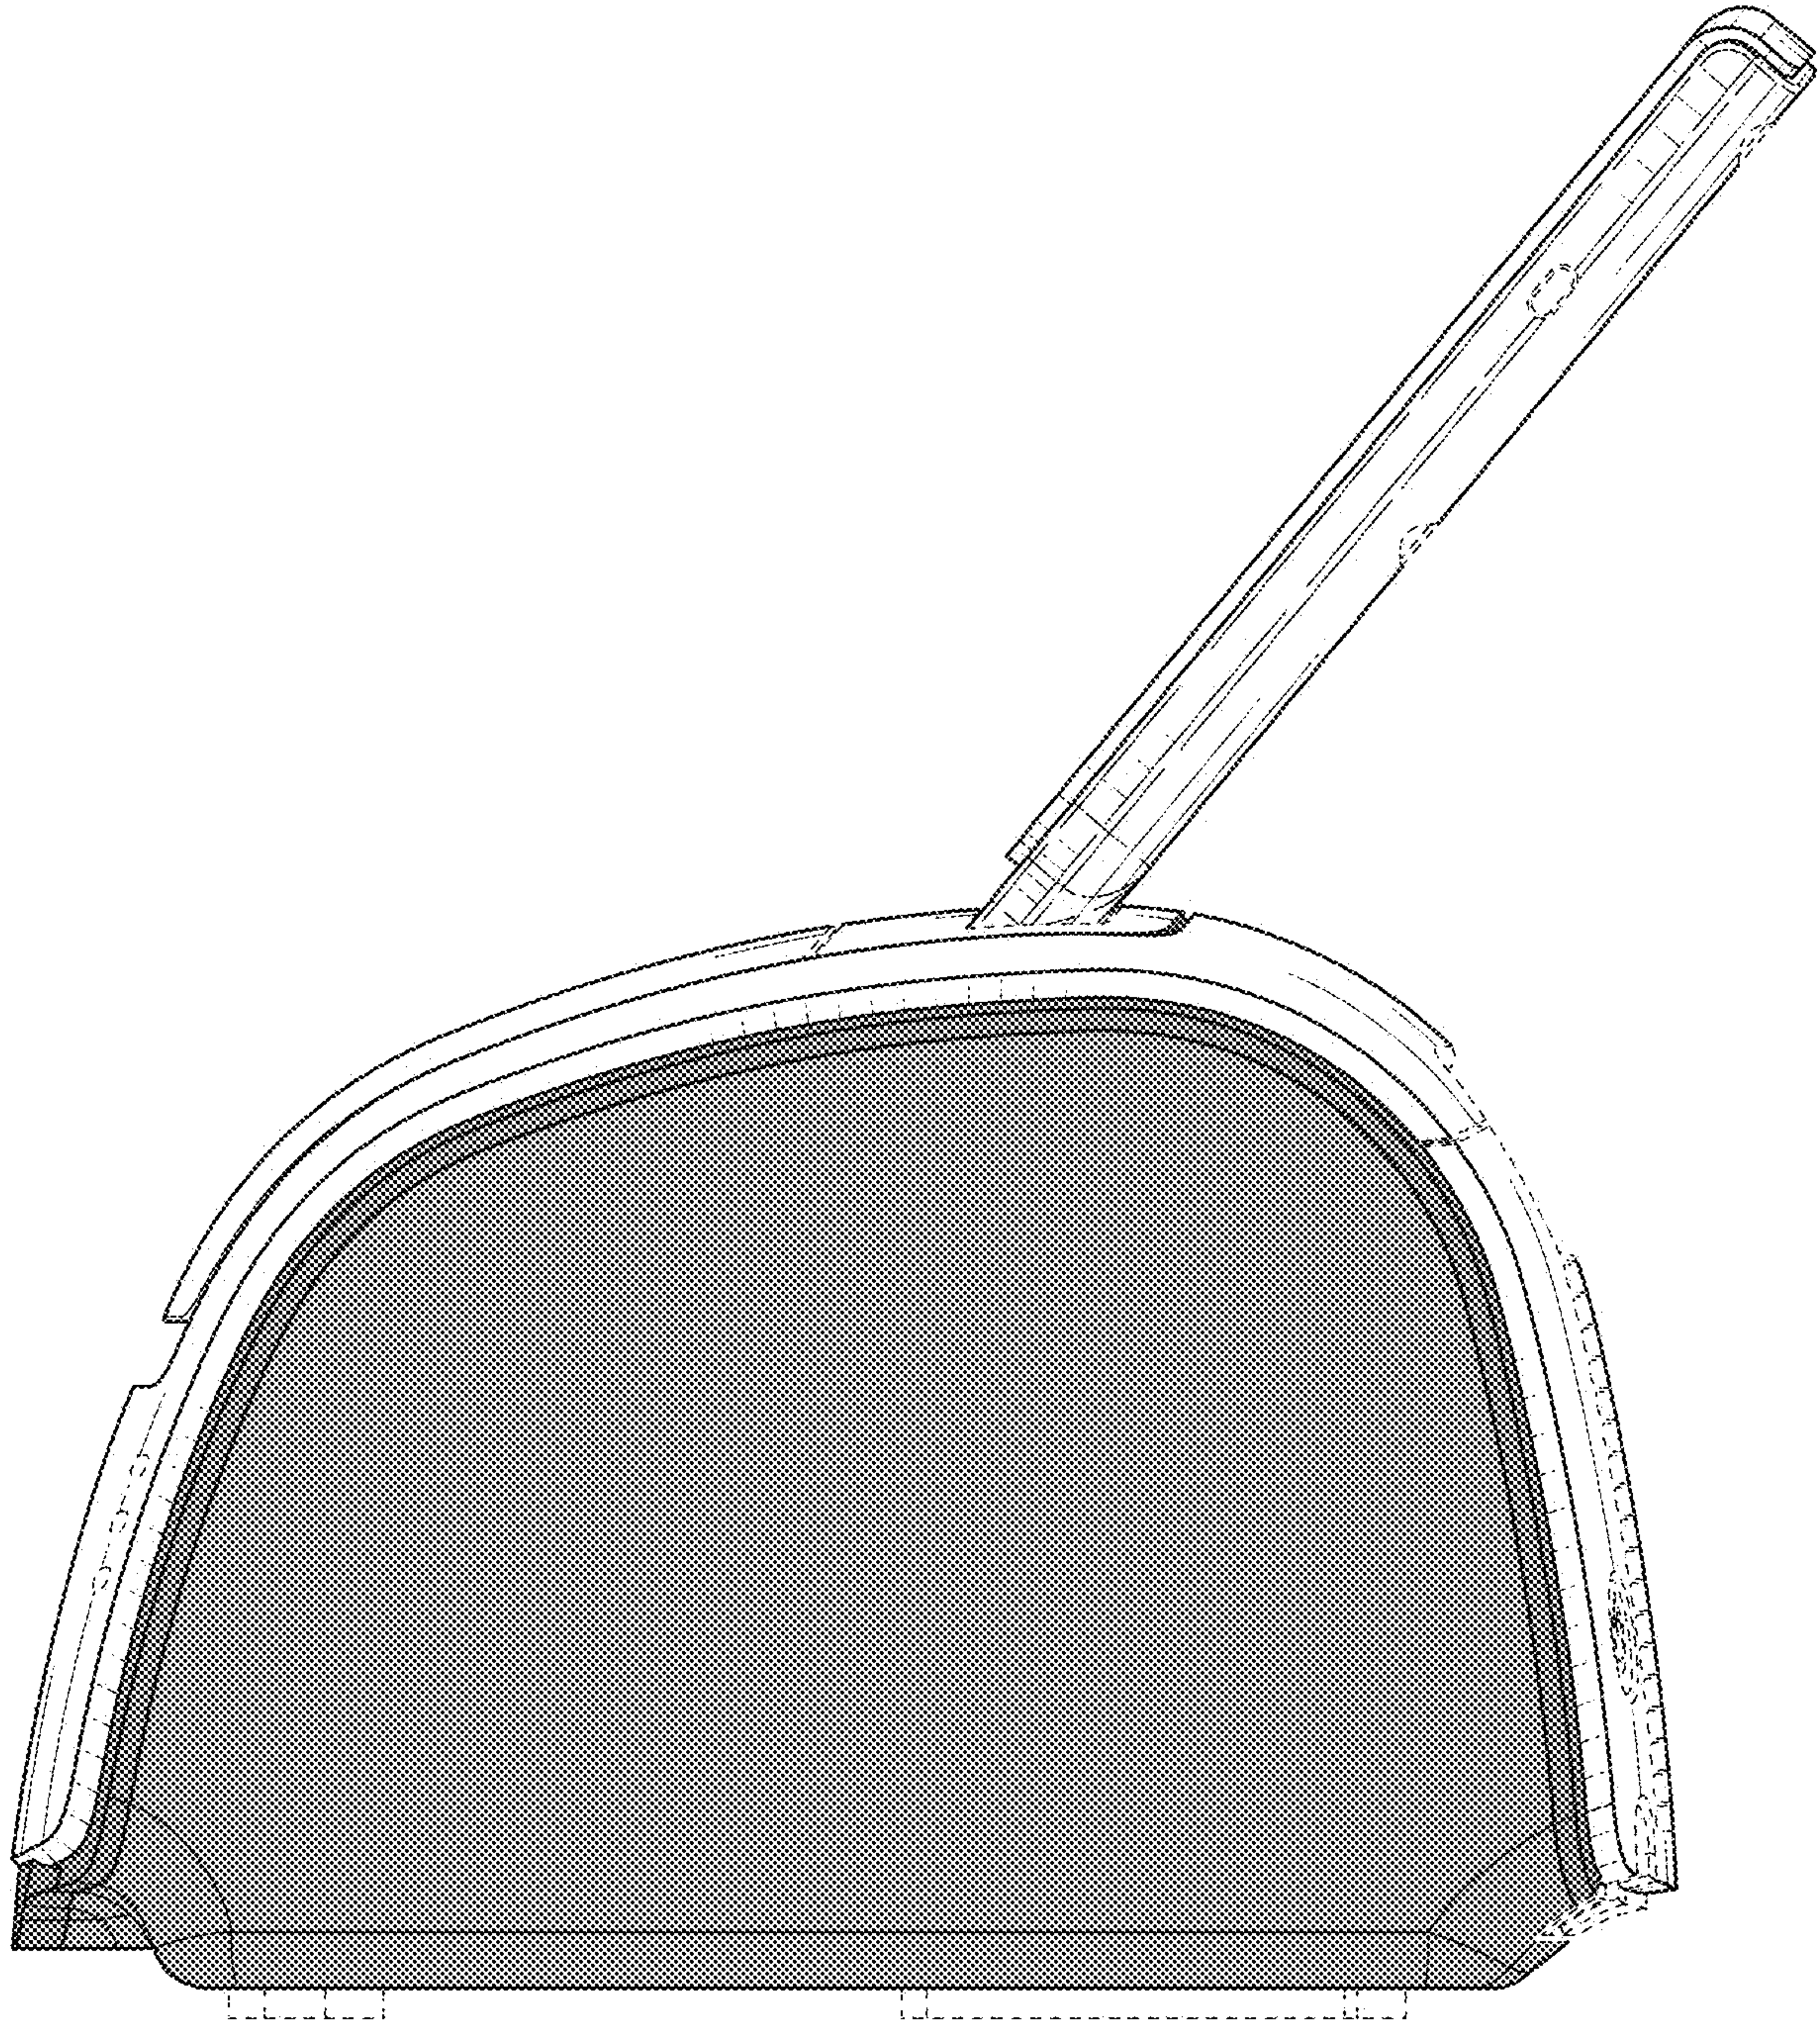


FIG. 22

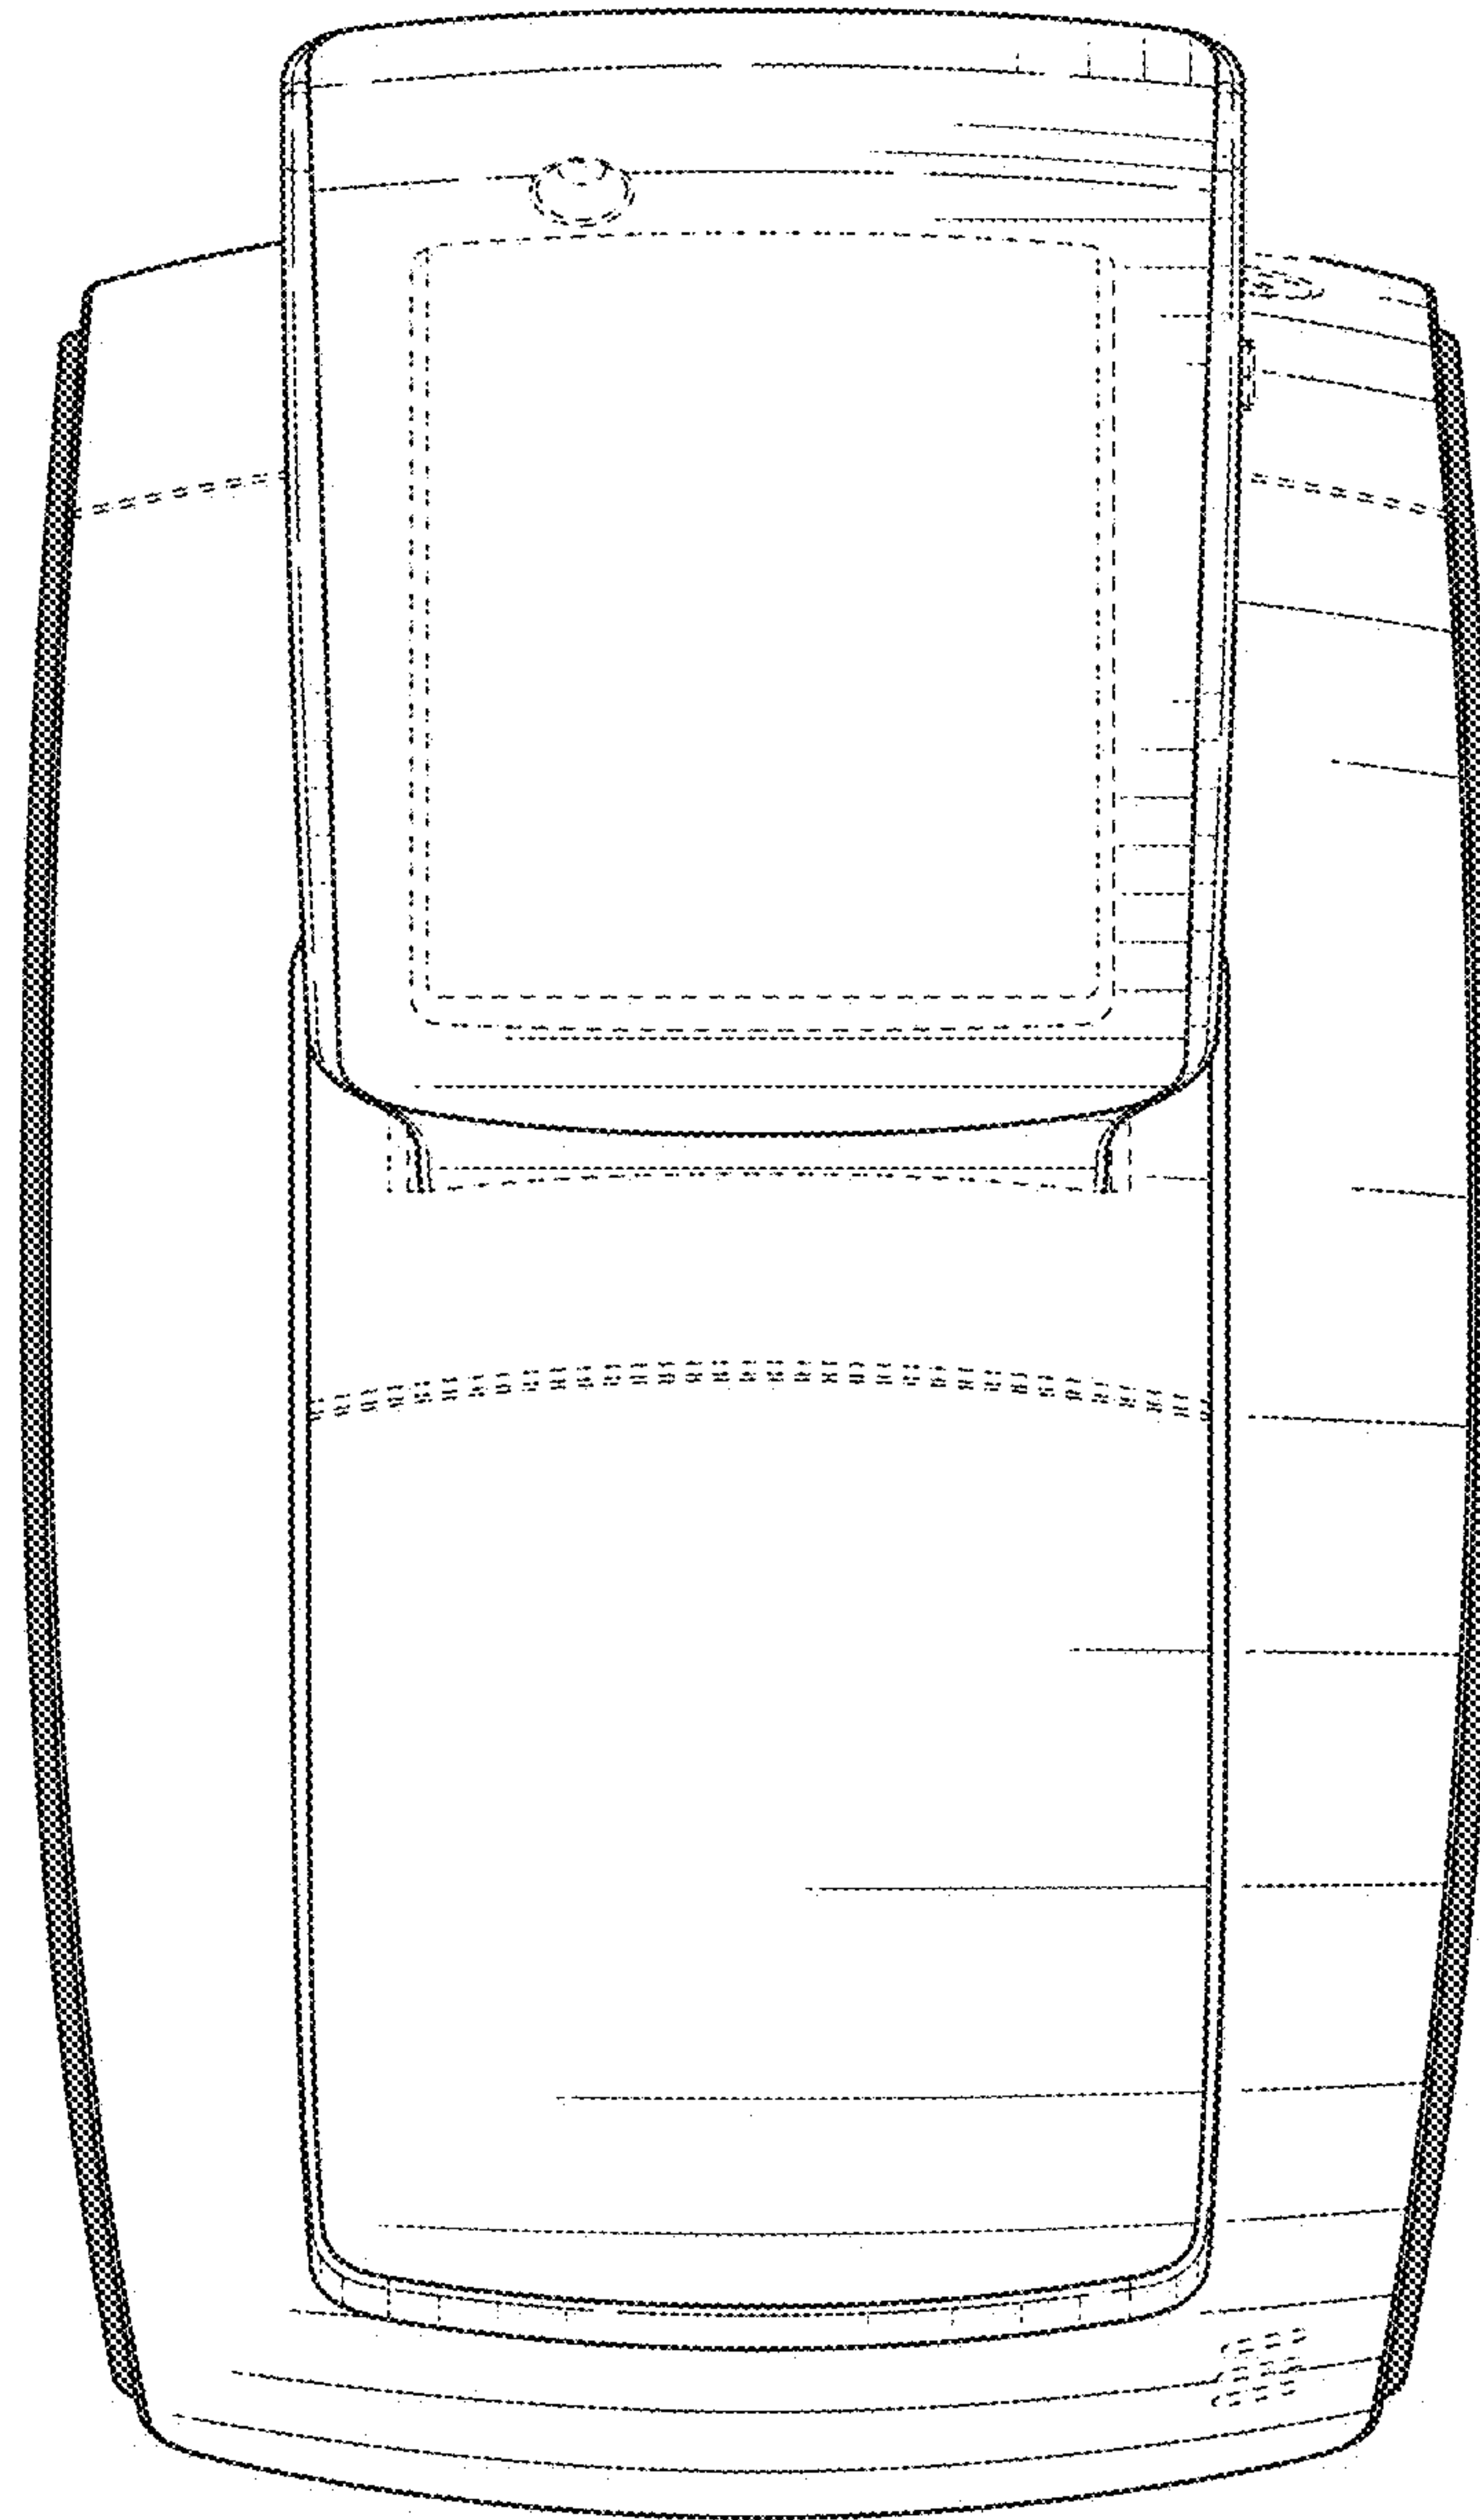


FIG. 23

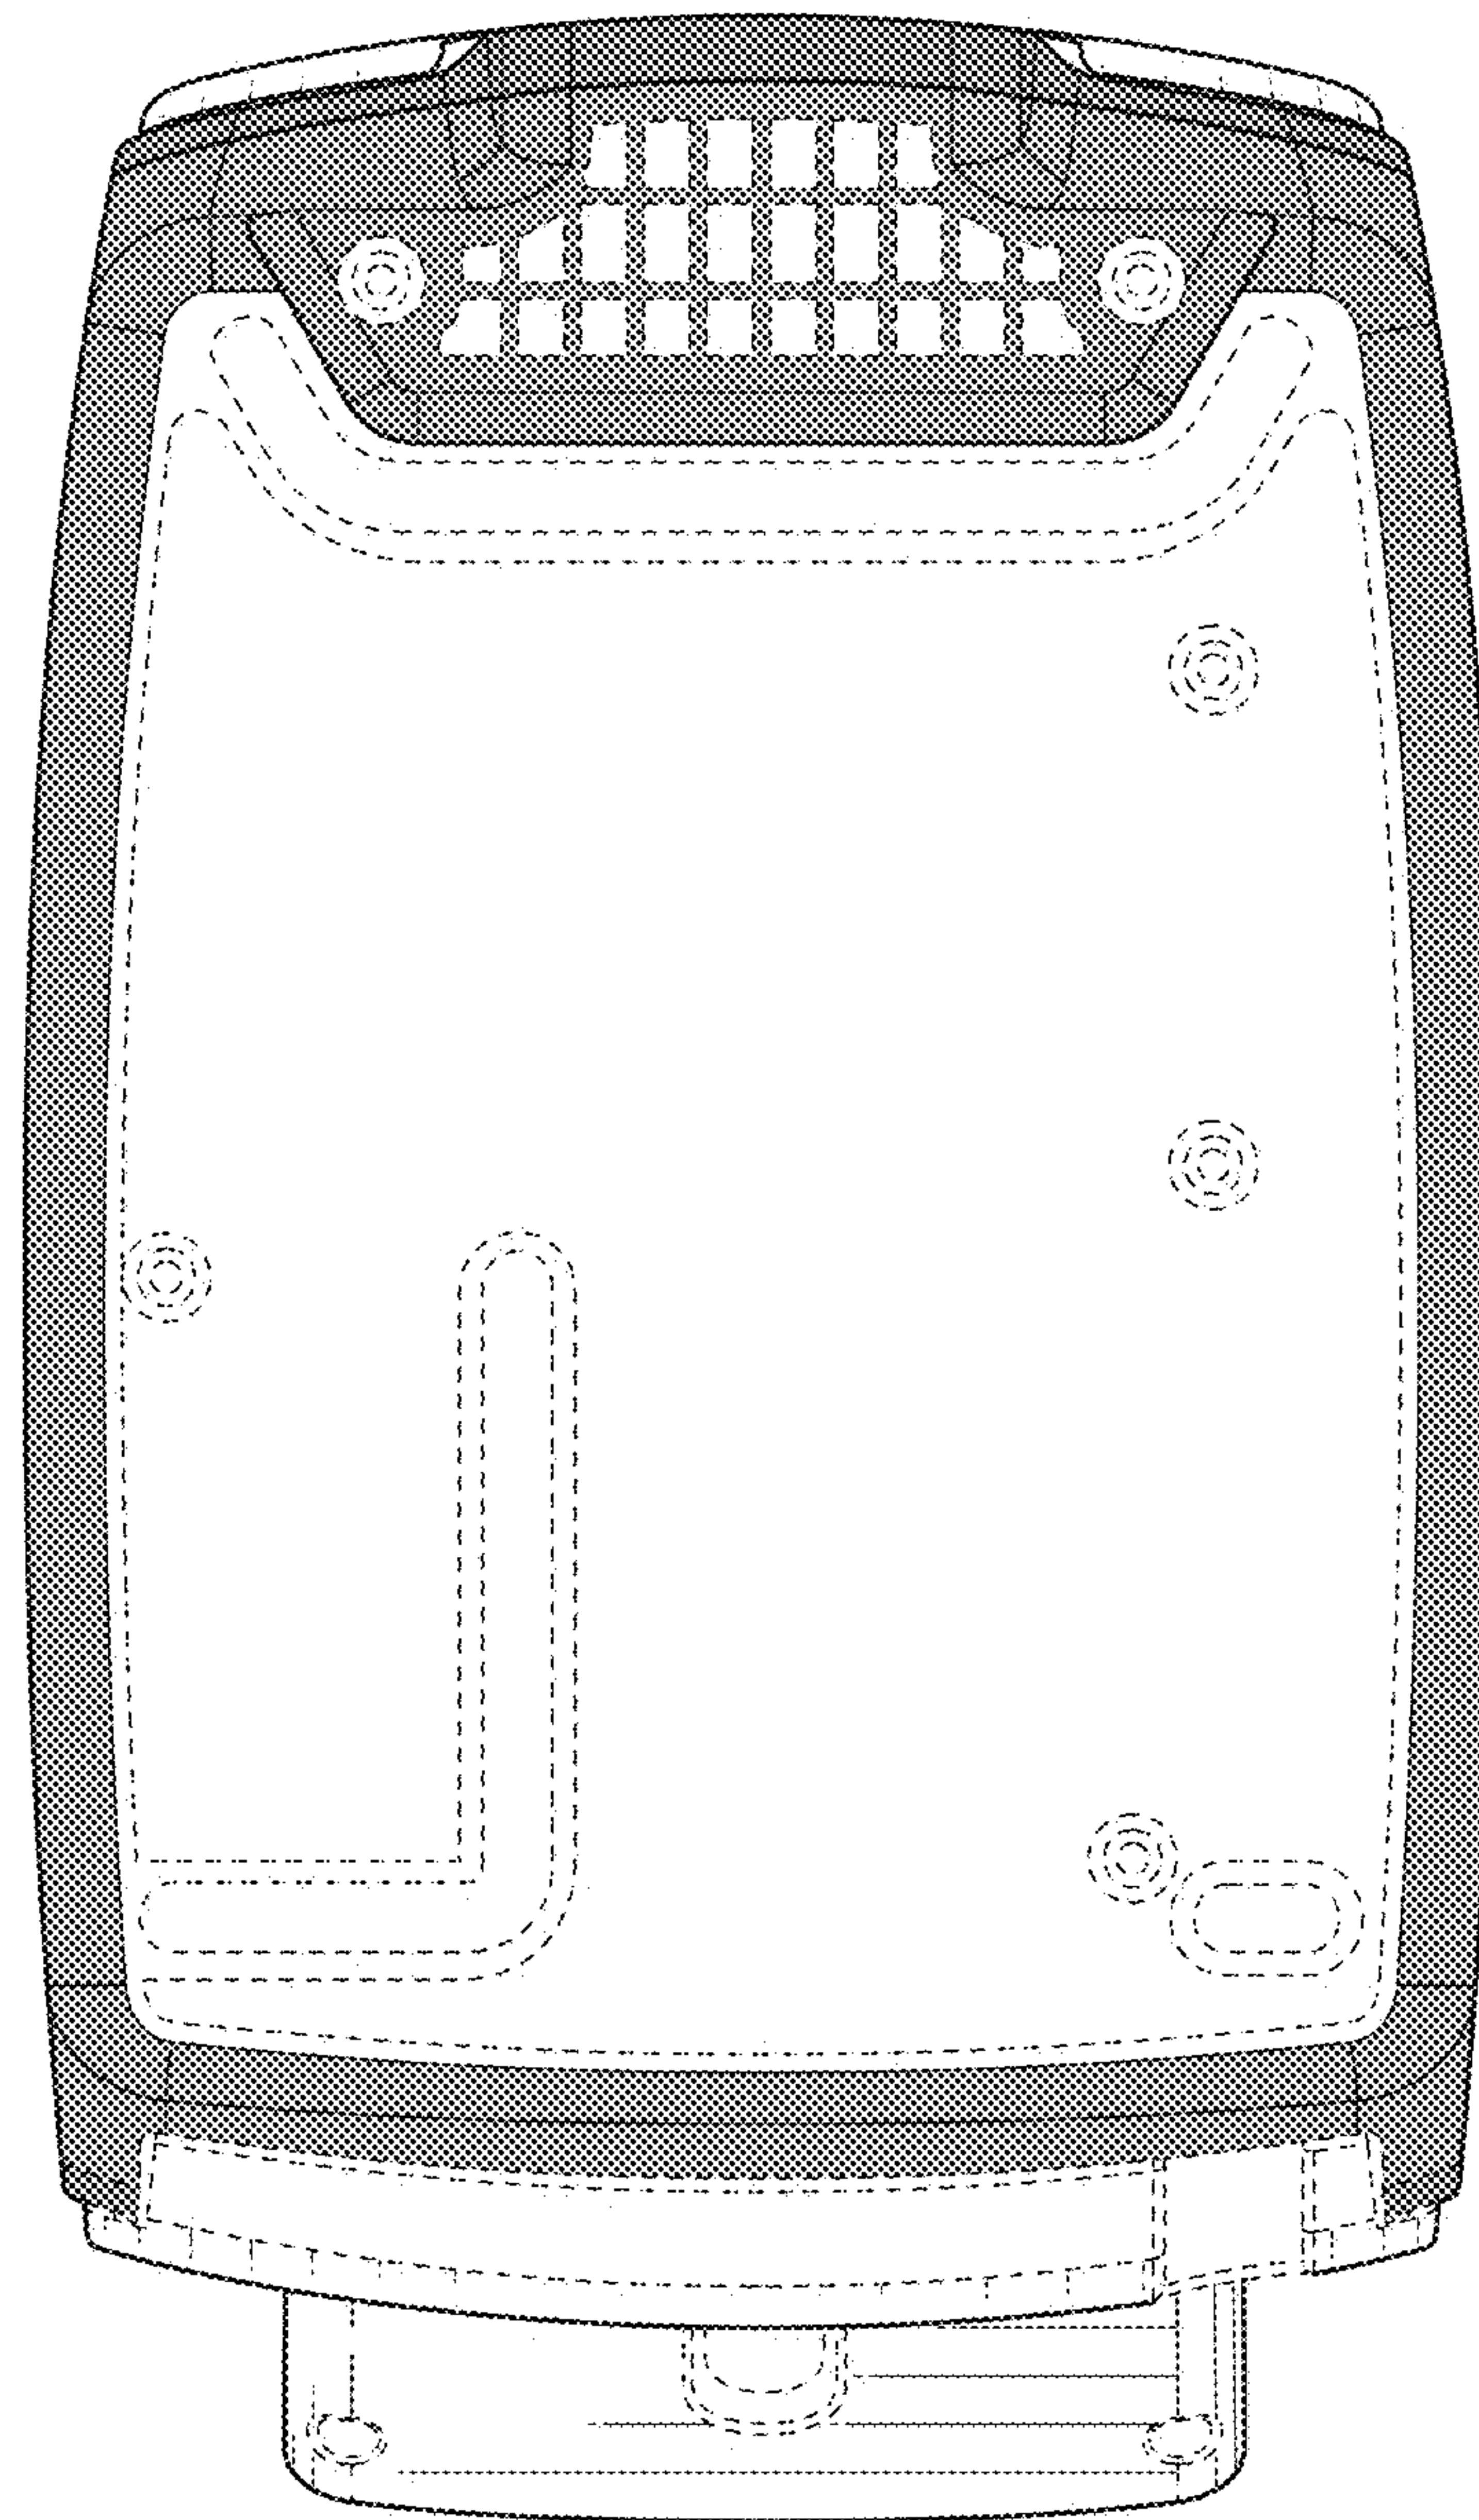


FIG. 24