



US00D909580S

(12) **United States Design Patent** (10) **Patent No.:** **US D909,580 S**  
**Edwards et al.** (45) **Date of Patent:** **\*\* Feb. 2, 2021**

(54) **SURGICAL MESH IMPLANT**

OTHER PUBLICATIONS

(71) Applicant: **SUNNYBROOK RESEARCH INSTITUTE**, Toronto (CA)

Bioplate, Cranial Fixation Biomesh System brochure, (Downloaded 2015), 2 pages.

(72) Inventors: **Glenn Edwards**, Toronto (CA); **Oleh Antonyshyn**, Etobicoke (CA); **James Mainprize**, Toronto (CA)

(Continued)

*Primary Examiner* — Charles D Hanson  
(74) *Attorney, Agent, or Firm* — Hill & Schumacher

(73) Assignee: **SUNNYBROOK RESEARCH INSTITUTE**, Toronto (CA)

(57) **CLAIM**

(\*\*) Term: **15 Years**

The ornamental design for surgical mesh implant, as shown and described.

(21) Appl. No.: **29/686,688**

**DESCRIPTION**

(22) Filed: **Apr. 5, 2019**

(51) **LOC (13) Cl.** ..... **24-03**

(52) **U.S. Cl.**

USPC ..... **D24/155**

(58) **Field of Classification Search**

USPC ..... D24/155

CPC .... A61F 2/07; A61F 2/90; A61F 2/958; A61F 2002/016; A61F 2002/072; A61F 2002/075; A61F 2002/91541; A61F 2220/0075; A61F 2230/0069

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,431,980 A 7/1995 McCarthy  
5,468,242 A 11/1995 Reisberg  
5,690,631 A 11/1997 Duncan et al.  
5,743,913 A 4/1998 Wellisz  
5,752,958 A 5/1998 Wellisz

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 105326554 A 2/2016  
EP 0433852 B1 3/1996

(Continued)

FIG. 1 is a front view of a unit of a surgical mesh implant, shown within a larger surgical mesh implant covering material;

FIG. 2 is an enlarged front view thereof;

FIG. 3 is a cross-sectional view thereof along the arrows provided in FIG. 2;

FIG. 4 is a right side view thereof. The left side view is a mirror image of the right side view;


FIG. 5 is a bottom view thereof. The top view is a mirror image of the bottom view;

FIG. 6 is a back view thereof; and,

FIG. 7 is a perspective view thereof from the bottom right corner. The perspective view from either the adjacent bottom left corner or adjacent top right corner is a mirror image of the perspective view of FIG. 7 from the bottom right corner. The perspective view from the opposite top left corner is an identical image to the perspective view of FIG. 7 from the bottom right corner.

The dotted lines depict portions of the surgical mesh implant that form no part of the claimed design. The arrows on either side of FIG. 2 form no part of the claimed design, and are provided to denote the cross-sectional view of FIG. 3. Shading shown throughout the drawings does not denote any specific material and is shown for contrast purposes only.

**1 Claim, 5 Drawing Sheets**

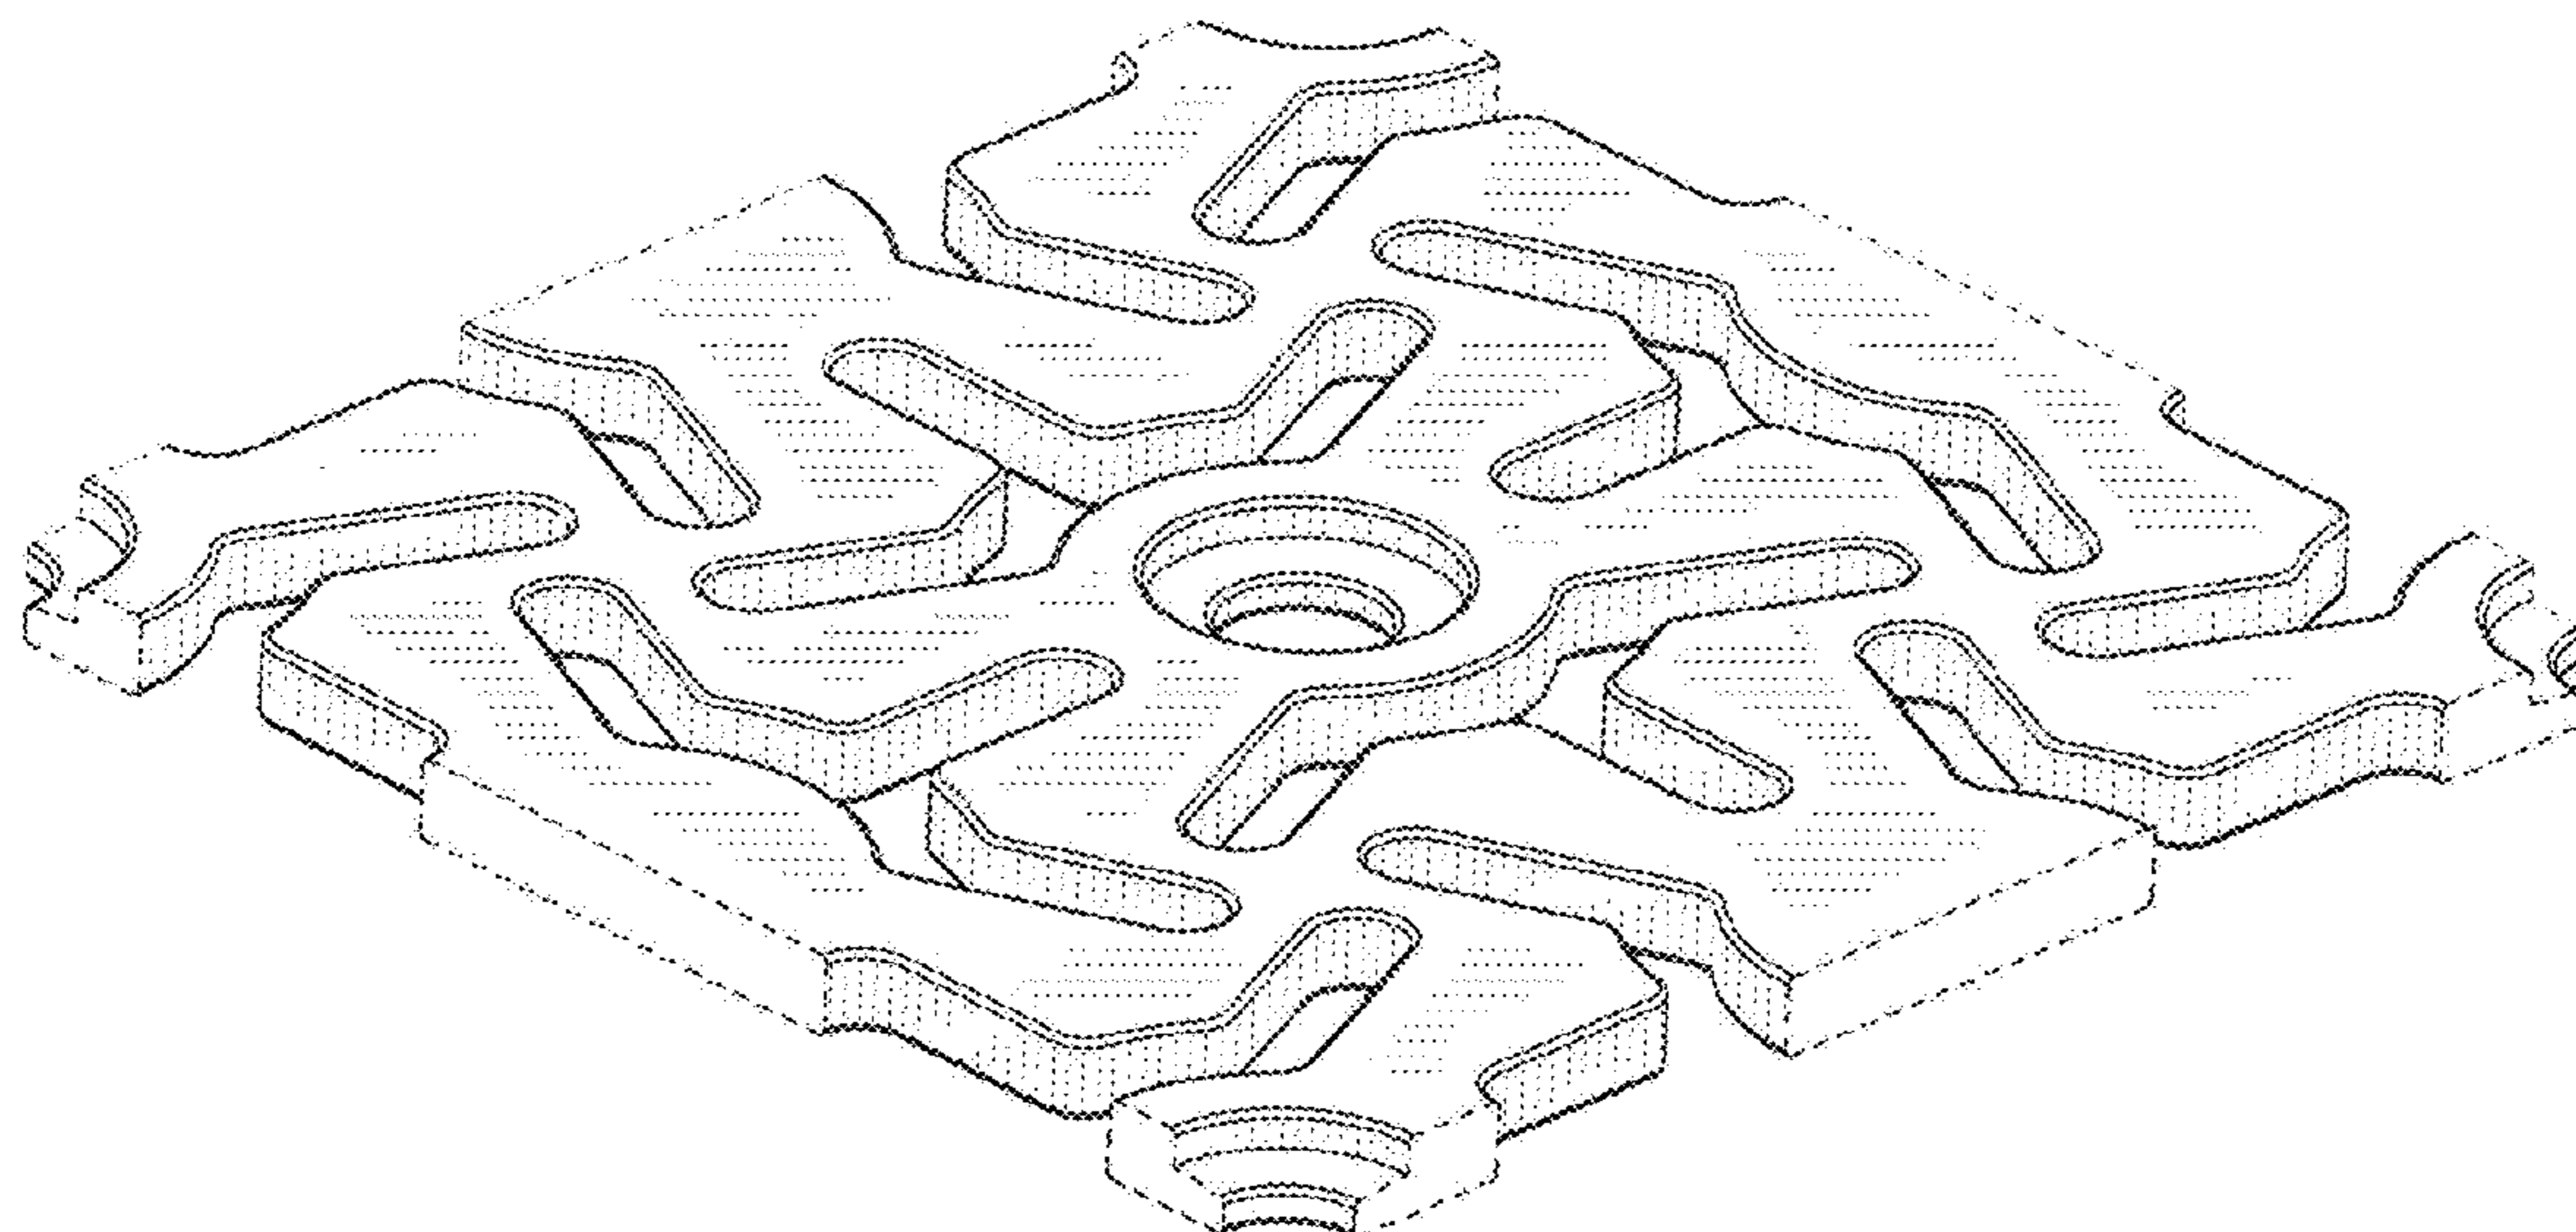

(56)

References Cited

U.S. PATENT DOCUMENTS

5,766,176 A 6/1998 Duncan  
 5,814,048 A 9/1998 Morgan  
 5,980,540 A 11/1999 Bruce  
 6,071,291 A 6/2000 Forst et al.  
 6,093,188 A 7/2000 Murray  
 6,206,883 B1 3/2001 Tunc  
 7,662,155 B2 2/2010 Metzger et al.  
 7,942,913 B2 5/2011 Ziolo et al.  
 8,084,117 B2 12/2011 Lalvani  
 8,298,286 B2 10/2012 Trieu  
 8,298,292 B2 10/2012 Swords et al.  
 8,337,533 B2 12/2012 Raines et al.  
 8,398,720 B2 3/2013 Swords  
 D680,649 S \* 4/2013 Jagger ..... D24/155  
 D681,813 S \* 5/2013 Jagger ..... D24/155  
 D685,476 S \* 7/2013 Jagger ..... D24/155  
 D694,886 S \* 12/2013 Jagger ..... D24/155  
 D751,202 S 3/2016 Gabele  
 9,549,819 B1 1/2017 Bravo et al.  
 D815,741 S 4/2018 Schuldt-Hempe  
 D837,988 S \* 1/2019 Khubani ..... D24/192  
 10,588,731 B2 \* 3/2020 Priewe ..... A61F 2/0063  
 2005/0261780 A1 11/2005 Heino et al.  
 2005/0288790 A1 12/2005 Swords  
 2007/0213838 A1 9/2007 Hengelmolen  
 2009/0216338 A1 8/2009 Gingras et al.  
 2011/0282452 A1 11/2011 Koerner et al.  
 2011/0301717 A1 12/2011 Becker  
 2012/0330435 A1 12/2012 Engqvist et al.  
 2013/0096371 A1 \* 4/2013 Arcand ..... A61F 2/0063  
 600/37  
 2013/0103079 A1 4/2013 Lau et al.  
 2013/0236853 A1 9/2013 Axelsson et al.  
 2014/0114266 A1 4/2014 Arcand  
 2014/0257348 A1 \* 9/2014 Priewe ..... A61F 2/0063  
 606/151

2014/0276995 A1 9/2014 Lau et al.  
 2015/0057762 A1 \* 2/2015 Harms ..... B29C 43/18  
 623/23.74  
 2015/0105806 A1 4/2015 Dorafshr et al.  
 2015/0238300 A1 \* 8/2015 Wang ..... A61L 31/10  
 606/151  
 2015/0250574 A1 9/2015 Egnelov  
 2015/0374497 A1 12/2015 Engstrand et al.  
 2017/0143872 A1 5/2017 Limem et al.

FOREIGN PATENT DOCUMENTS

EP 2030596 A1 3/2009  
 JP 2014046025 A 3/2014  
 KR 100952730 B1 4/2010  
 WO 2008047415 A1 4/2008  
 WO 2012036129 A1 3/2012  
 WO 2012079611 A1 6/2012  
 WO 2016024248 A1 2/2016

OTHER PUBLICATIONS

Biomet, CranioCurve brochure, (Downloaded 2013), 2 pages.  
 Codman Neuro Device Biomech Catalogue, (Downloaded 2015), 1 page.  
 Mikami et al., "Explosure of titanium implants after cranioplasty: A matter of long-term consequences", Interdis. Neuro.: Adv. Tech. and Case Manage. 8, (2017), pp. 64-67.  
 Lau et al., "A Method for Combining Thin and Thick Malleable Titanium Mesh in the Repair of Cranial Defects", Cereus 7, e267. DOI 10.7759/cereus.267, (2015), 9 pages.  
 KLS Martin Group, "Neurosurgery" brochure, (2018), 28 pages.  
 International Search Report dated Jul. 11, 2019, in PCT/CA2019/050419 filed Apr. 5, 2019, 3 pages.

\* cited by examiner

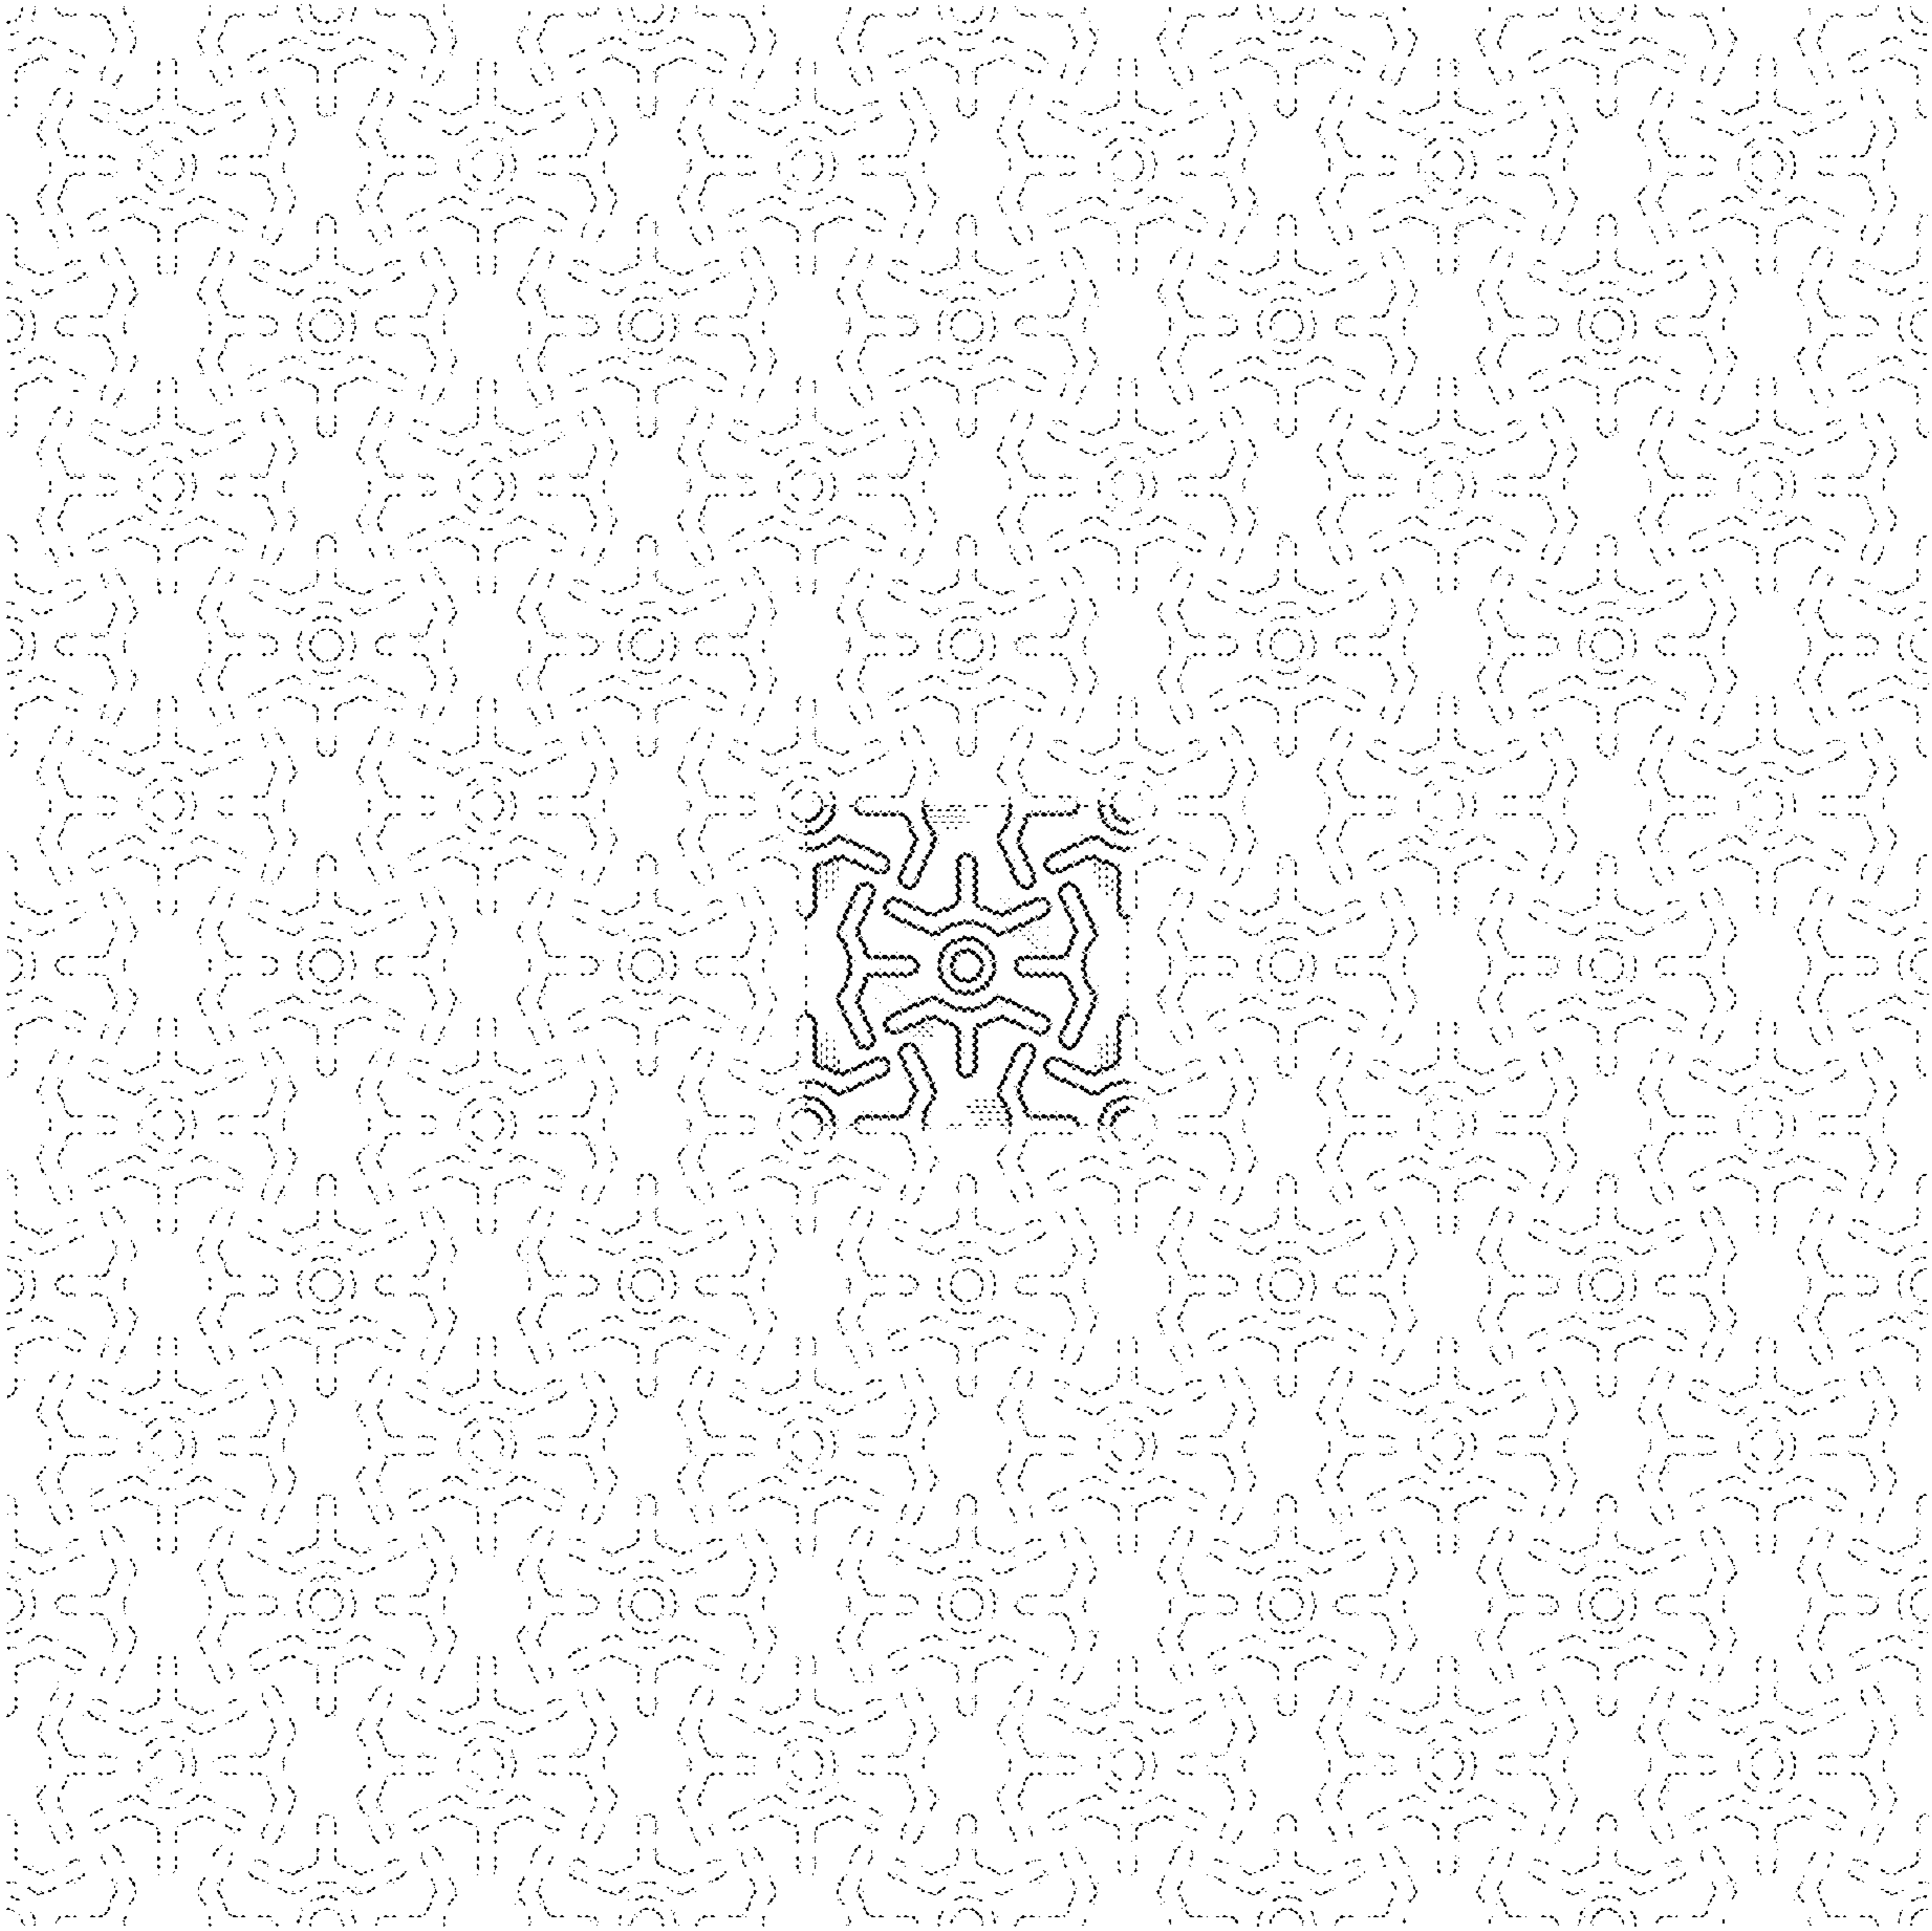


FIG. 1

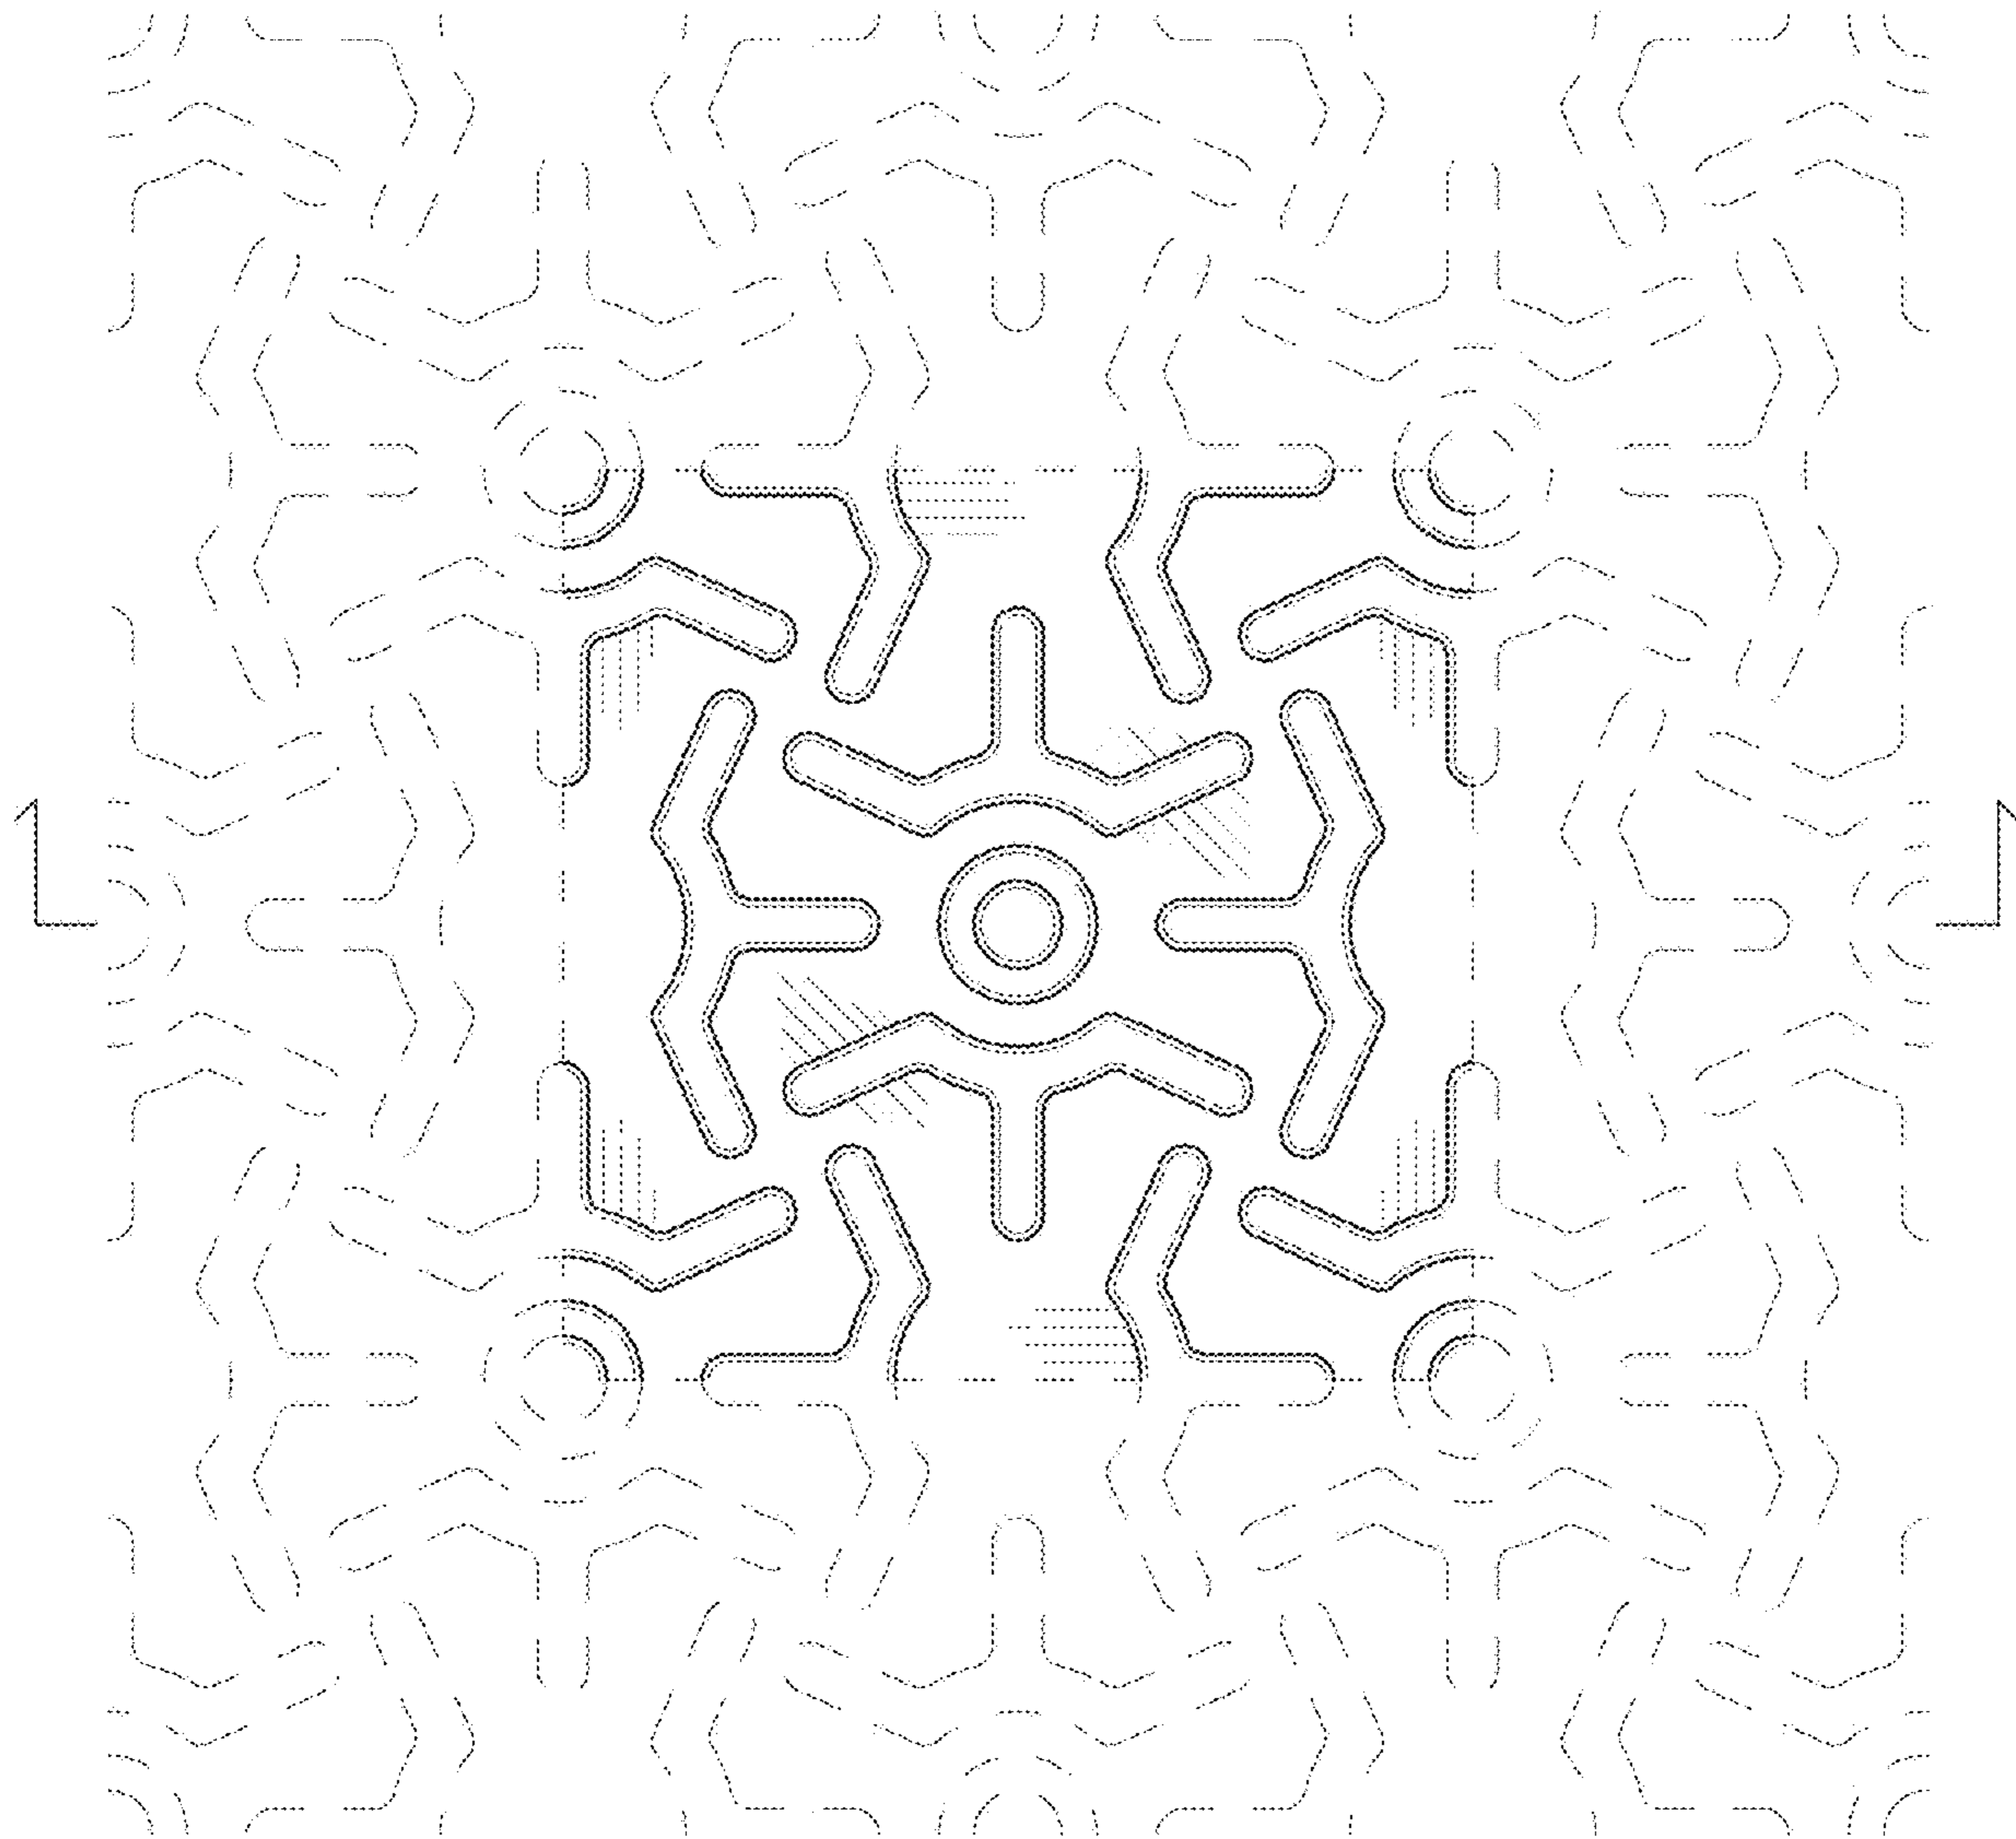


FIG. 2

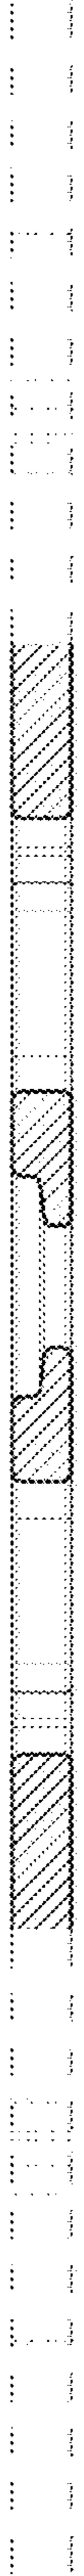


FIG. 3



FIG. 4

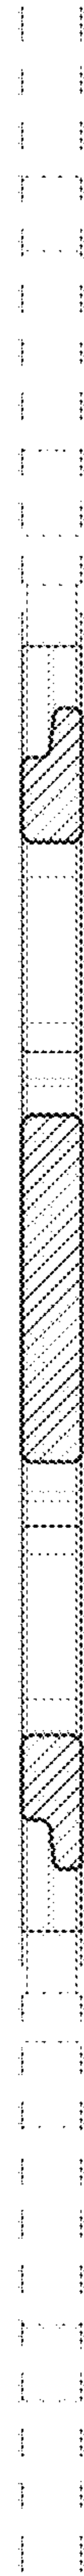


FIG. 5

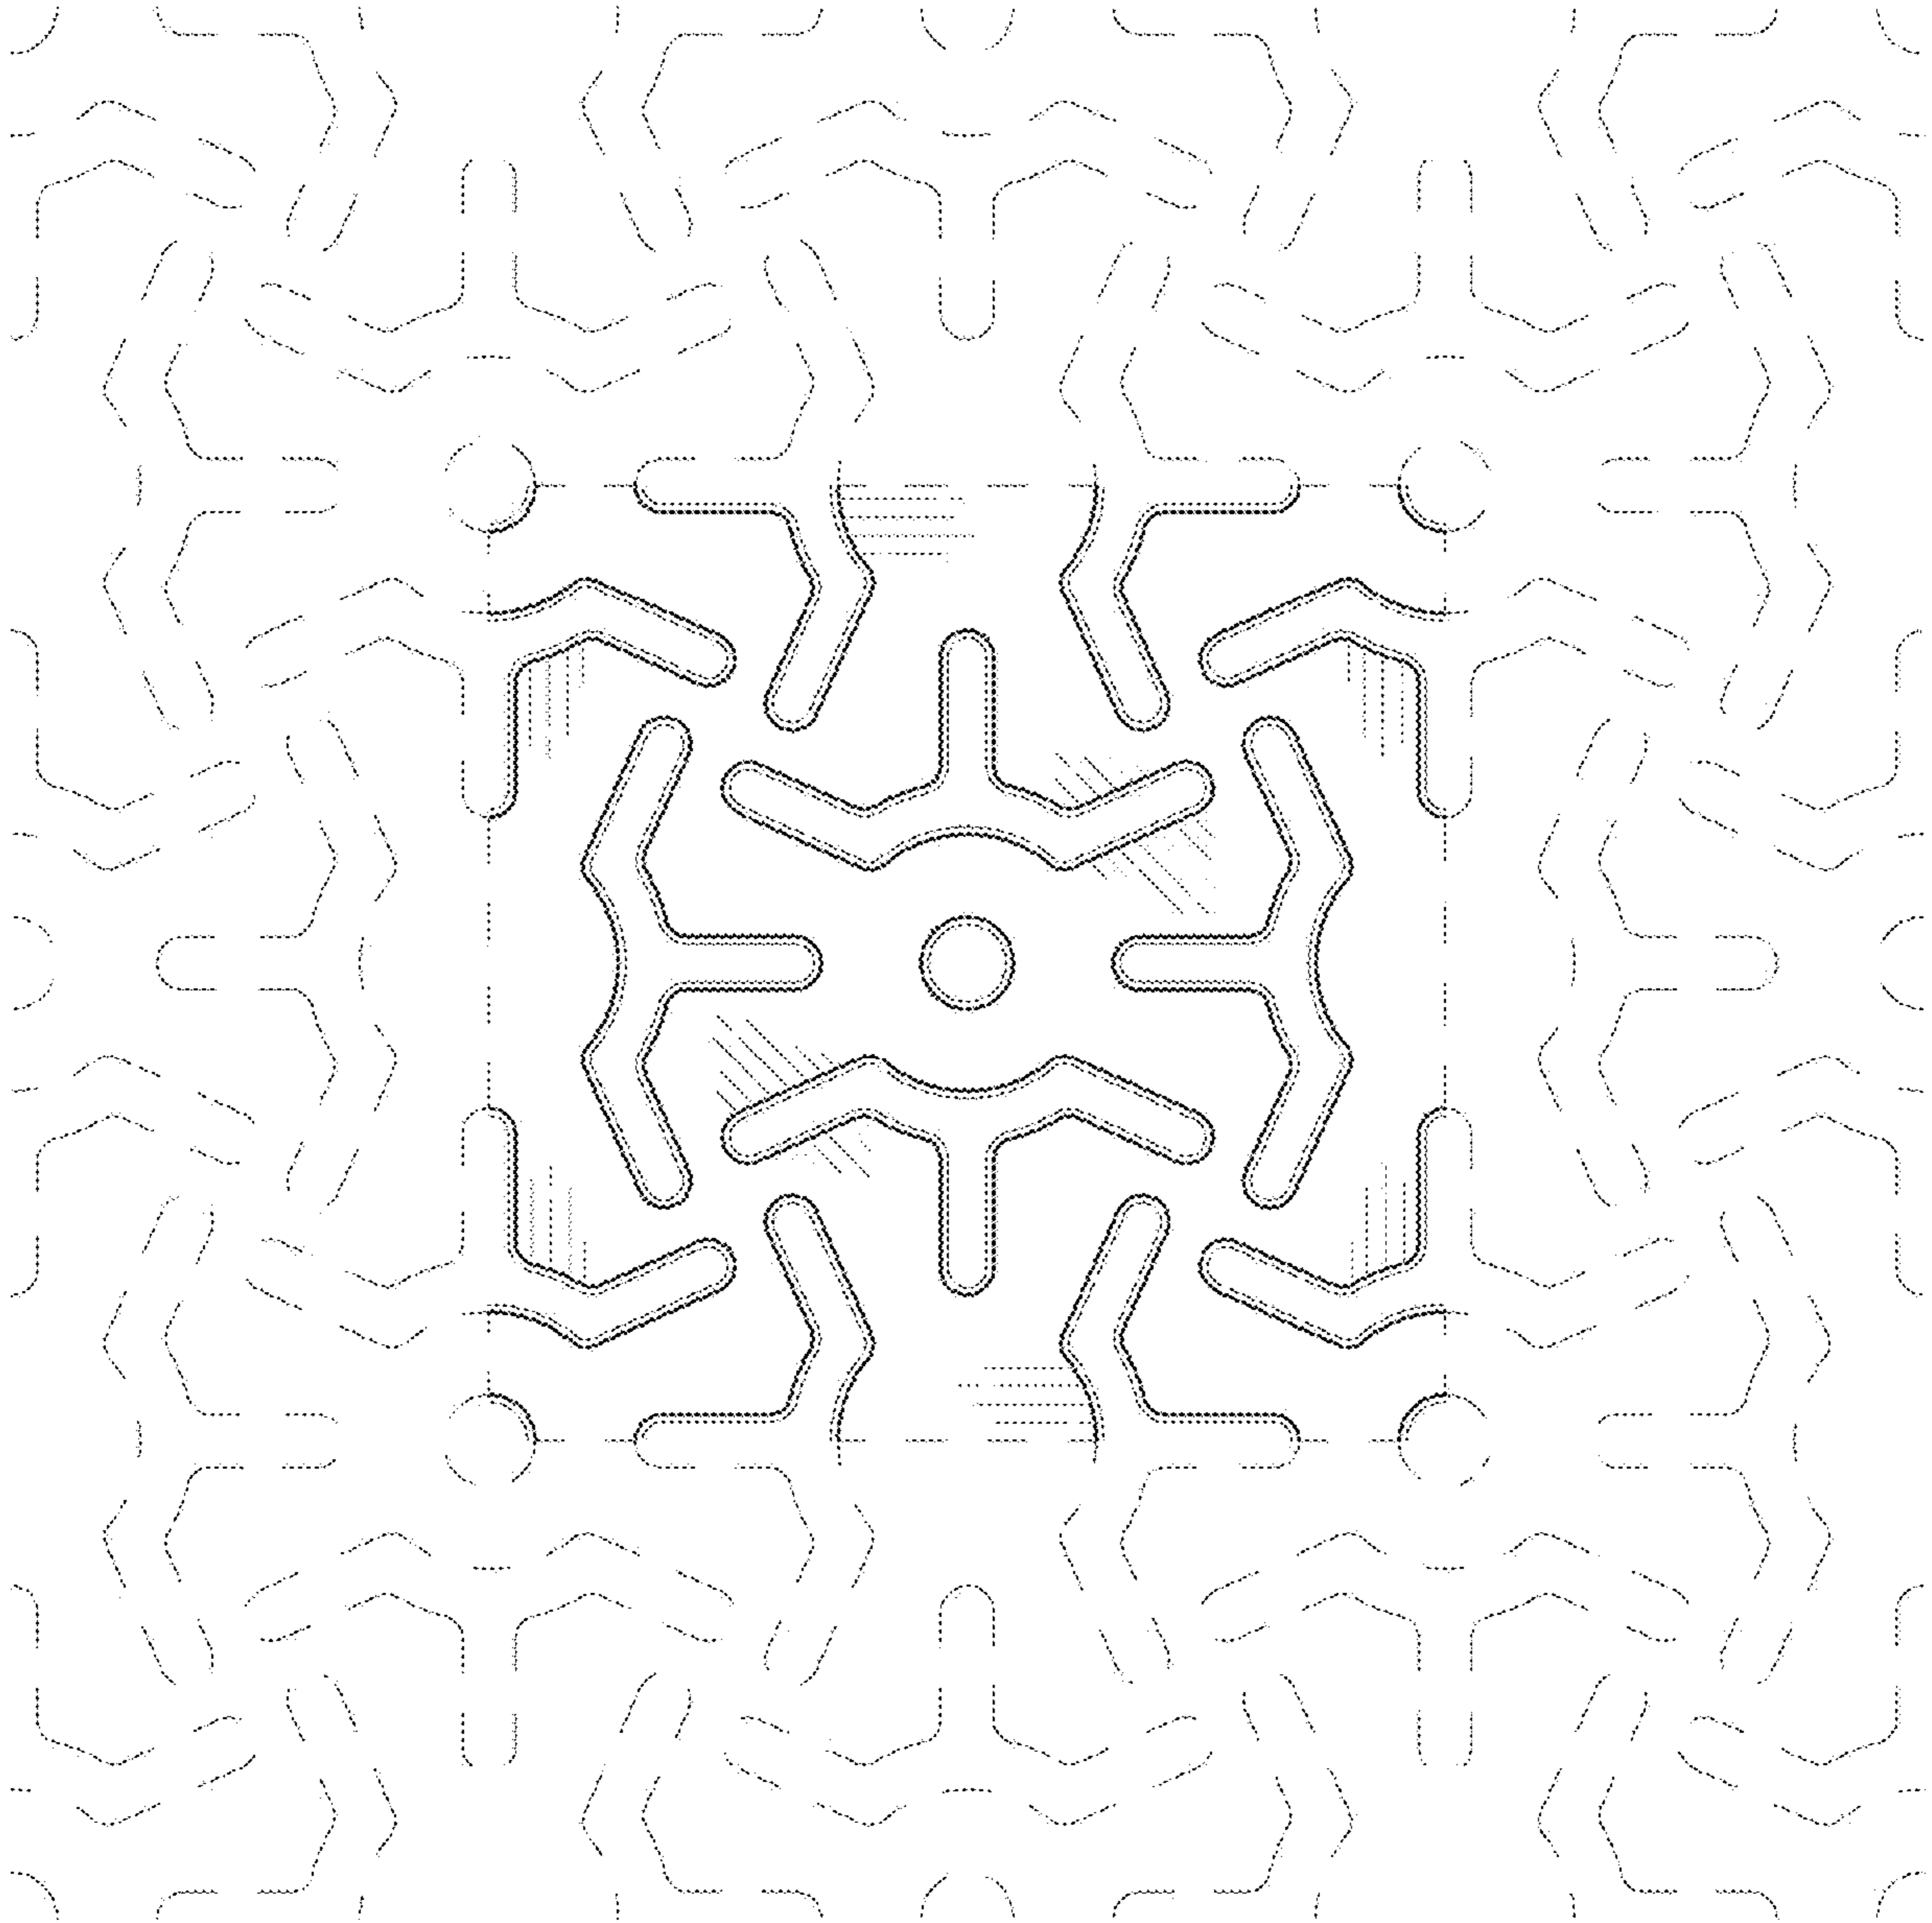


FIG. 6

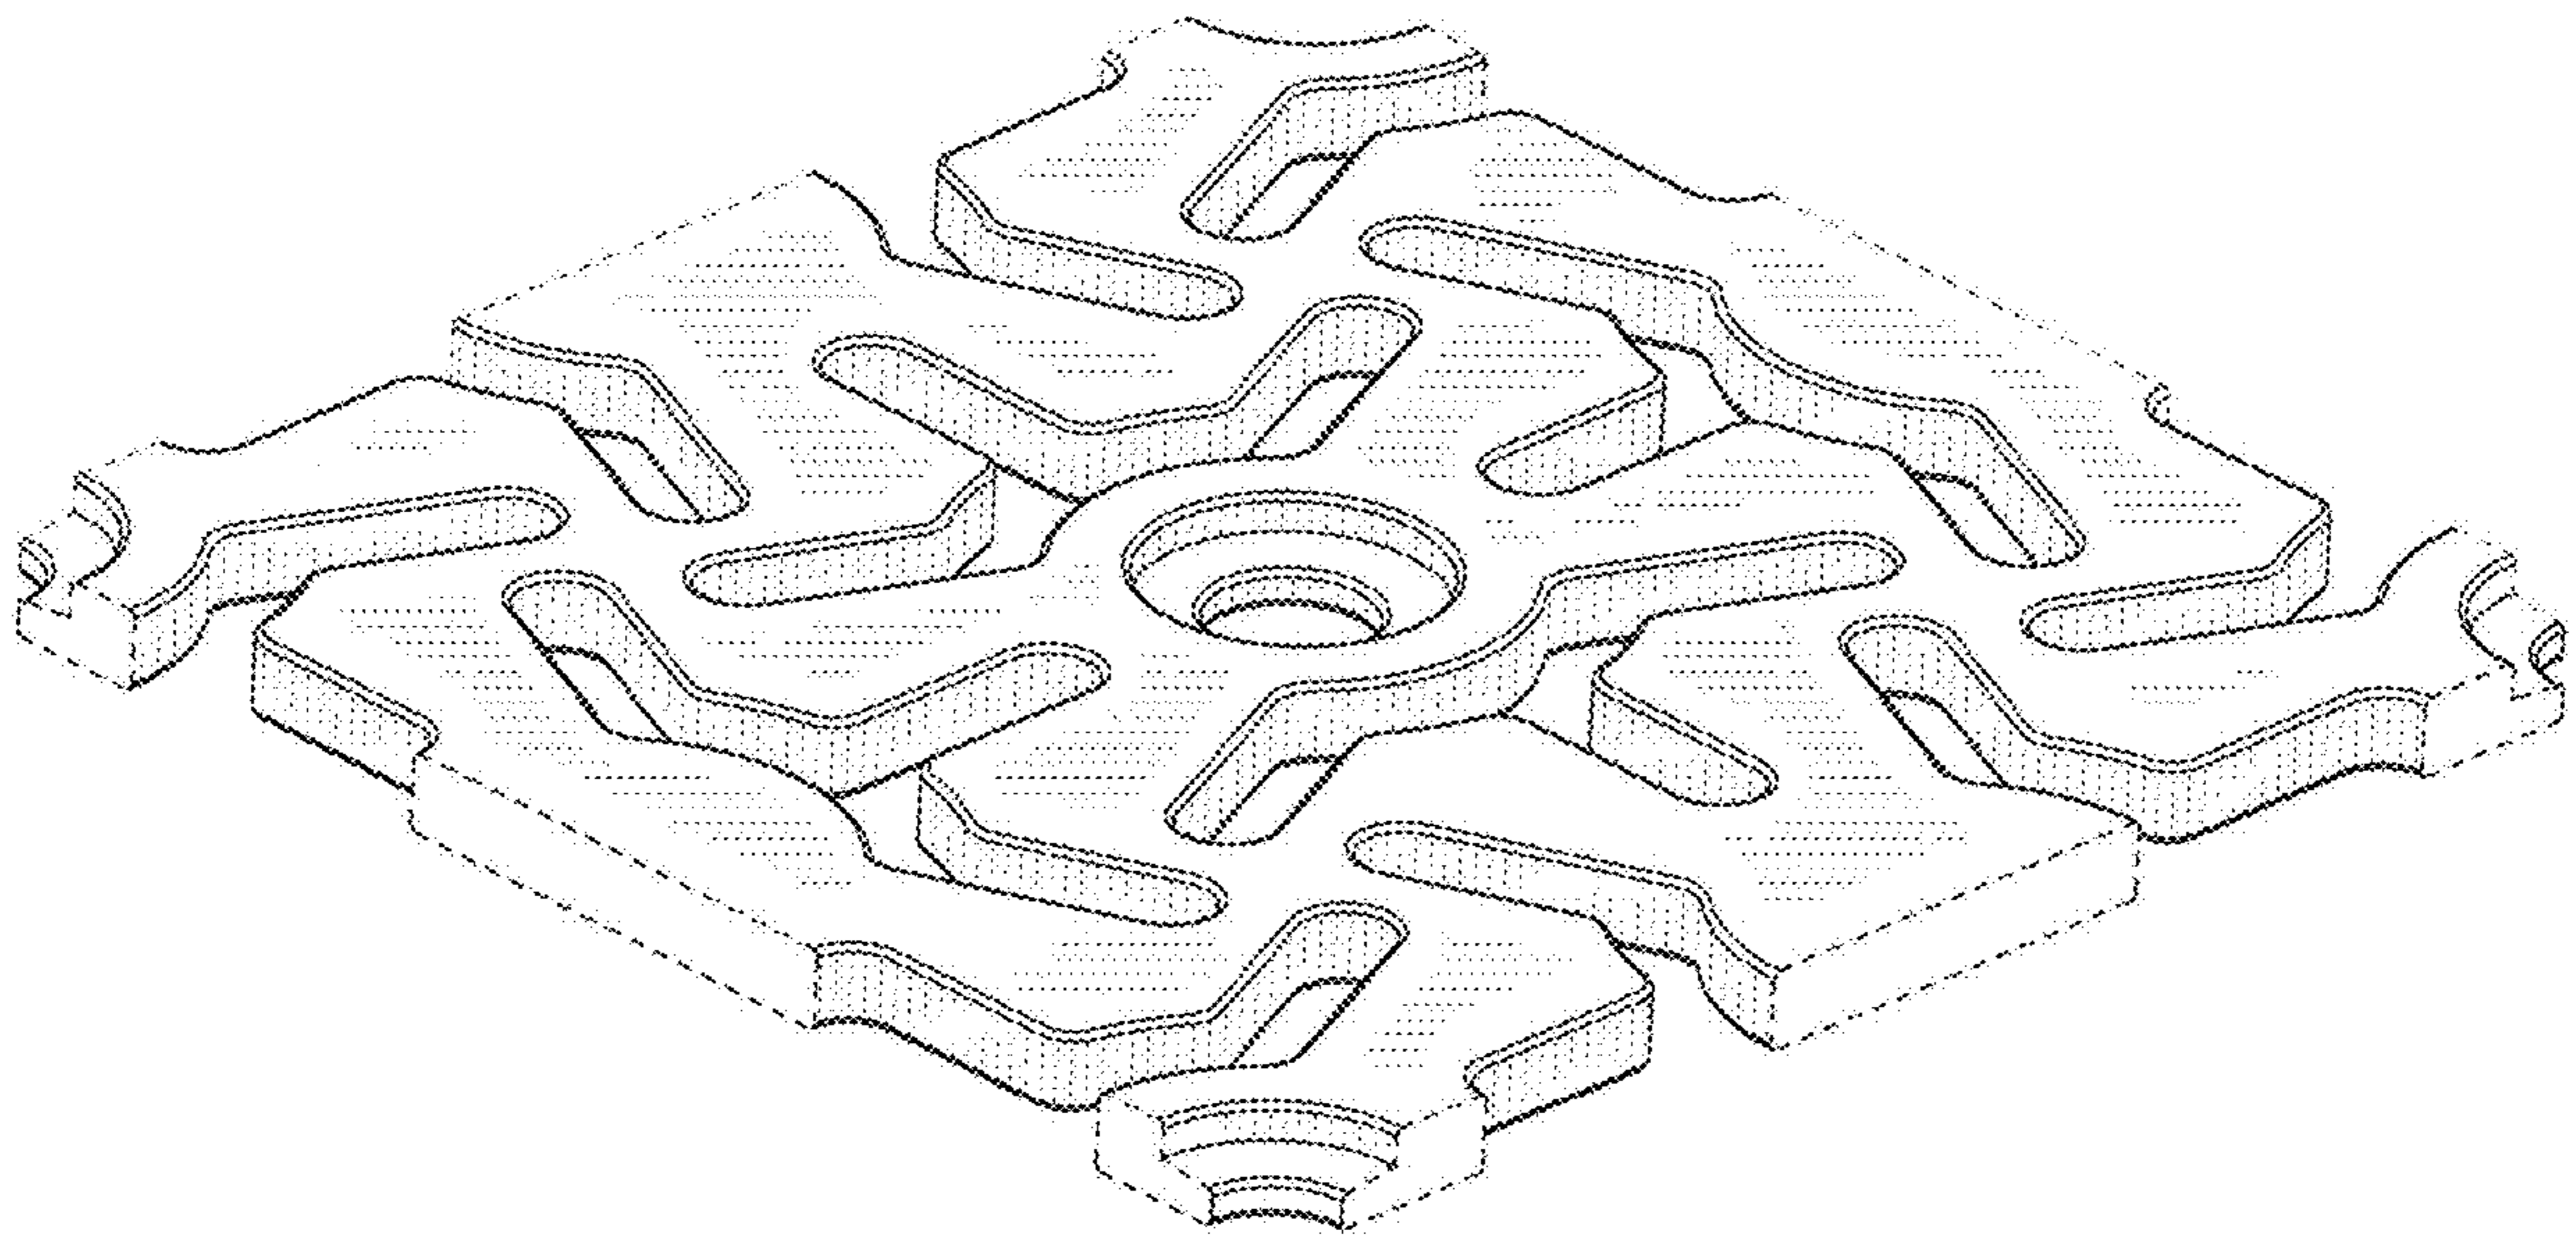


FIG. 7