



US00D909580S

(12) **United States Design Patent** (10) **Patent No.:** **US D909,580 S**
Edwards et al. (45) **Date of Patent:** **** Feb. 2, 2021**

(54) **SURGICAL MESH IMPLANT**

OTHER PUBLICATIONS

(71) Applicant: **SUNNYBROOK RESEARCH INSTITUTE**, Toronto (CA)

Bioplate, Cranial Fixation Biomesh System brochure, (Downloaded 2015), 2 pages.

(72) Inventors: **Glenn Edwards**, Toronto (CA); **Oleh Antonyshyn**, Etobicoke (CA); **James Mainprize**, Toronto (CA)

(Continued)

Primary Examiner — Charles D Hanson
(74) *Attorney, Agent, or Firm* — Hill & Schumacher

(73) Assignee: **SUNNYBROOK RESEARCH INSTITUTE**, Toronto (CA)

(57) **CLAIM**

(**) Term: **15 Years**

The ornamental design for surgical mesh implant, as shown and described.

(21) Appl. No.: **29/686,688**

DESCRIPTION

(22) Filed: **Apr. 5, 2019**

(51) **LOC (13) Cl.** **24-03**

(52) **U.S. Cl.**

USPC **D24/155**

(58) **Field of Classification Search**

USPC D24/155

CPC A61F 2/07; A61F 2/90; A61F 2/958; A61F 2002/016; A61F 2002/072; A61F 2002/075; A61F 2002/91541; A61F 2220/0075; A61F 2230/0069

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,431,980 A 7/1995 McCarthy
5,468,242 A 11/1995 Reisberg
5,690,631 A 11/1997 Duncan et al.
5,743,913 A 4/1998 Wellisz
5,752,958 A 5/1998 Wellisz

(Continued)

FOREIGN PATENT DOCUMENTS

CN 105326554 A 2/2016
EP 0433852 B1 3/1996

(Continued)

FIG. 1 is a front view of a unit of a surgical mesh implant, shown within a larger surgical mesh implant covering material;

FIG. 2 is an enlarged front view thereof;

FIG. 3 is a cross-sectional view thereof along the arrows provided in FIG. 2;

FIG. 4 is a right side view thereof. The left side view is a mirror image of the right side view;


FIG. 5 is a bottom view thereof. The top view is a mirror image of the bottom view;

FIG. 6 is a back view thereof; and,

FIG. 7 is a perspective view thereof from the bottom right corner. The perspective view from either the adjacent bottom left corner or adjacent top right corner is a mirror image of the perspective view of FIG. 7 from the bottom right corner. The perspective view from the opposite top left corner is an identical image to the perspective view of FIG. 7 from the bottom right corner.

The dotted lines depict portions of the surgical mesh implant that form no part of the claimed design. The arrows on either side of FIG. 2 form no part of the claimed design, and are provided to denote the cross-sectional view of FIG. 3. Shading shown throughout the drawings does not denote any specific material and is shown for contrast purposes only.

1 Claim, 5 Drawing Sheets

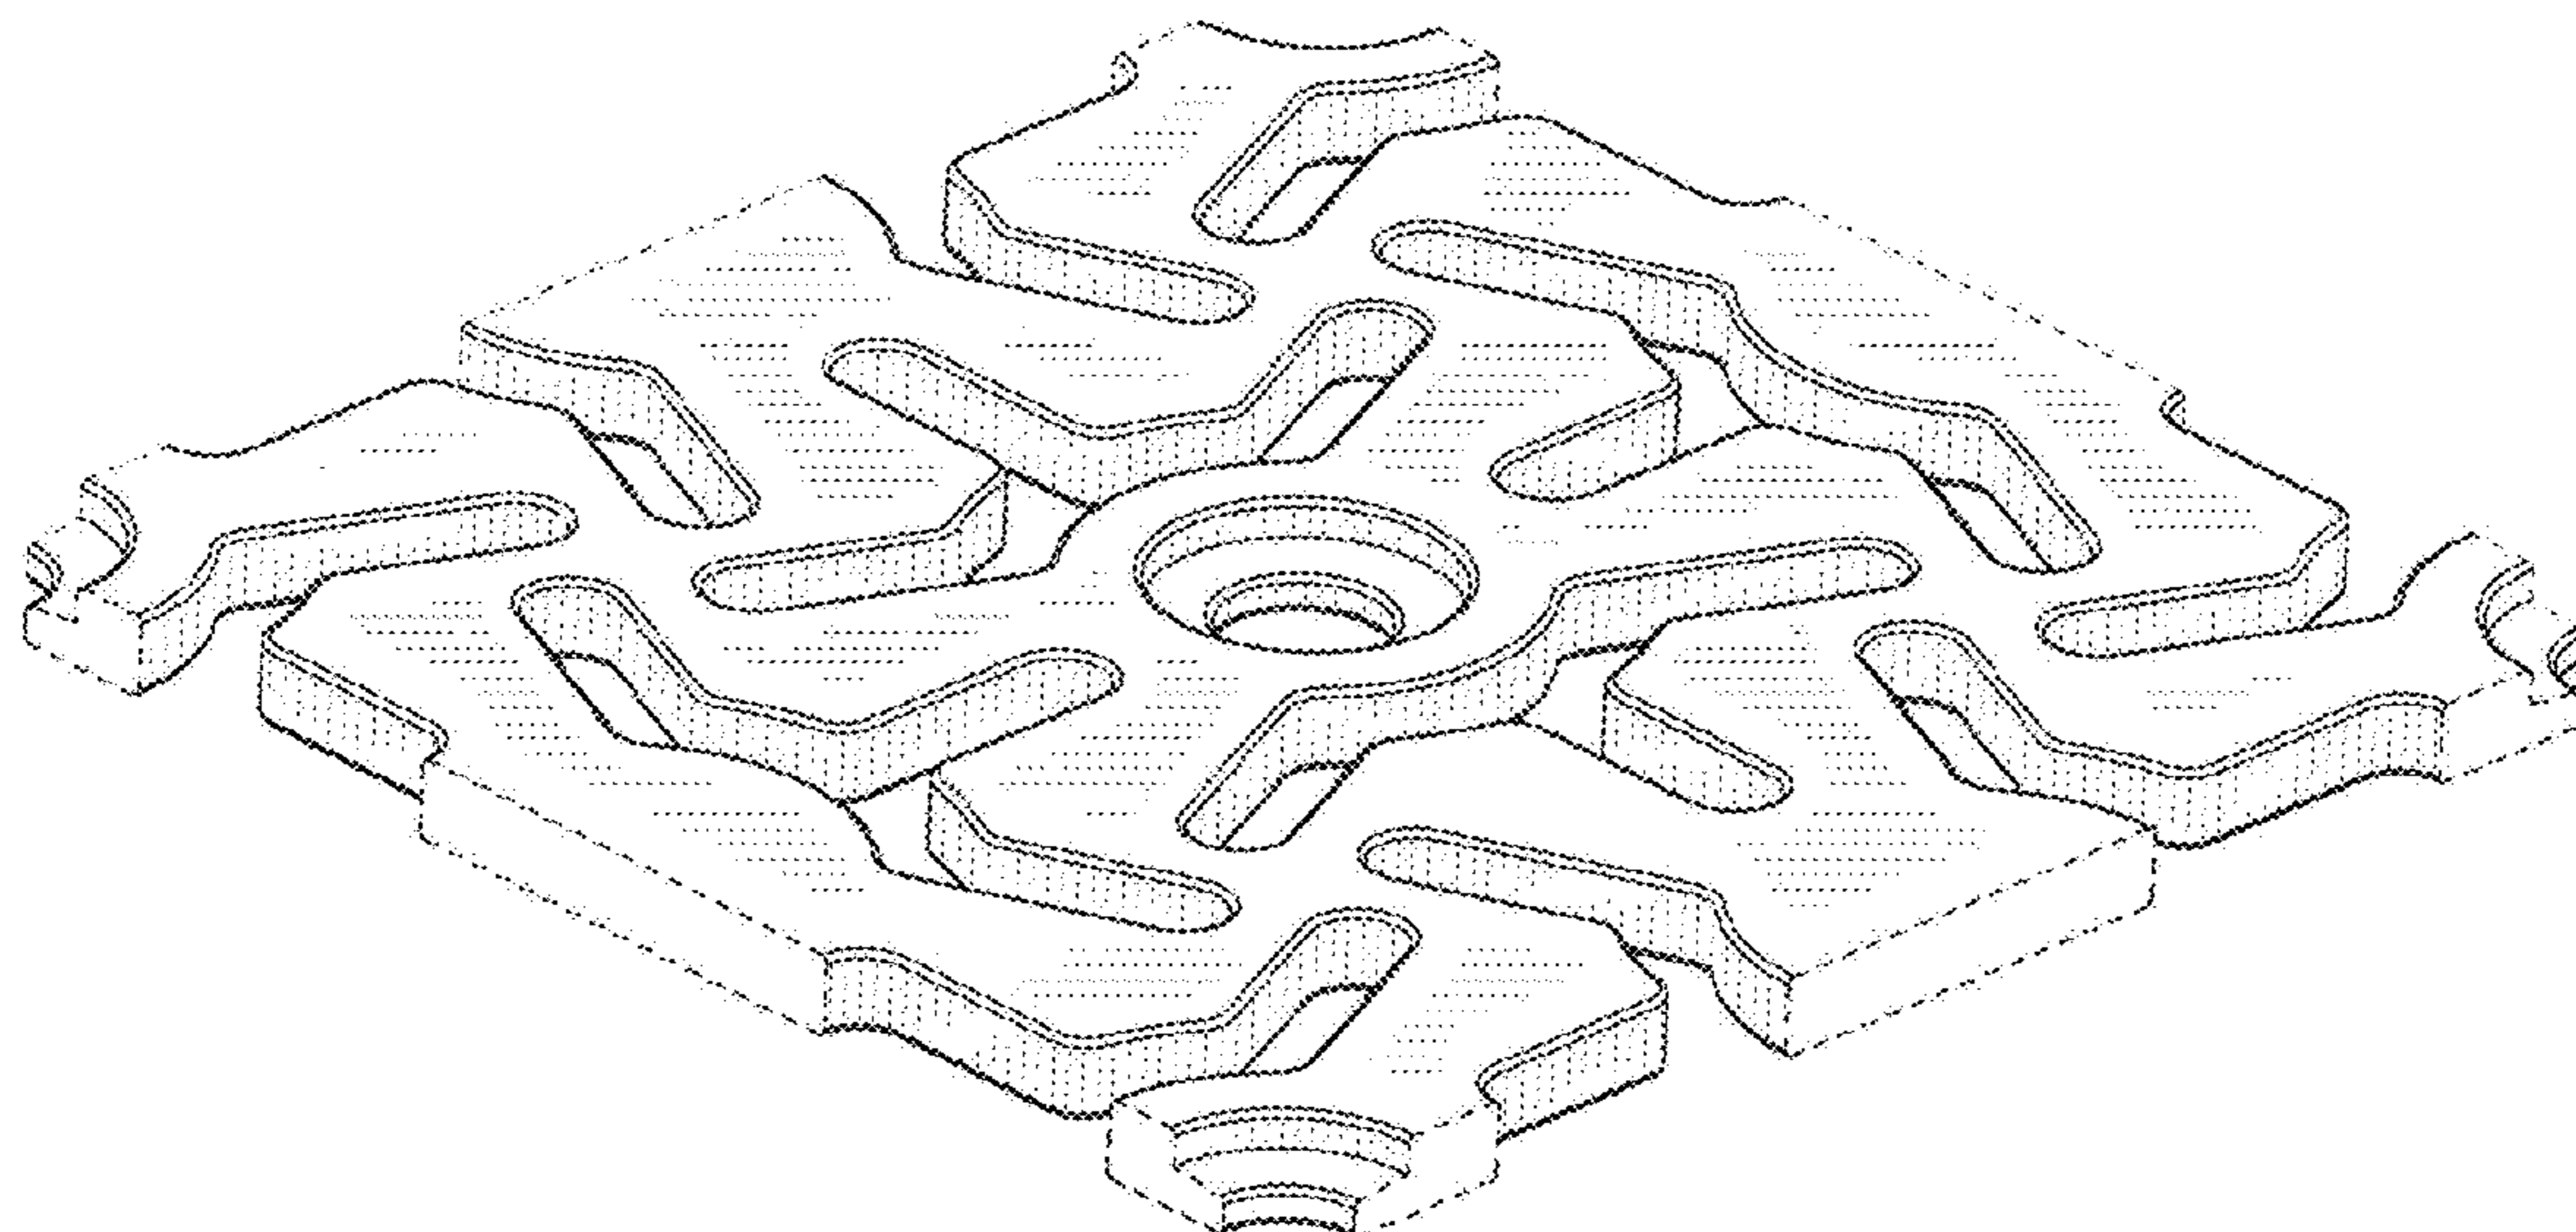

(56)

References Cited

U.S. PATENT DOCUMENTS

5,766,176 A 6/1998 Duncan
 5,814,048 A 9/1998 Morgan
 5,980,540 A 11/1999 Bruce
 6,071,291 A 6/2000 Forst et al.
 6,093,188 A 7/2000 Murray
 6,206,883 B1 3/2001 Tunc
 7,662,155 B2 2/2010 Metzger et al.
 7,942,913 B2 5/2011 Ziolo et al.
 8,084,117 B2 12/2011 Lalvani
 8,298,286 B2 10/2012 Trieu
 8,298,292 B2 10/2012 Swords et al.
 8,337,533 B2 12/2012 Raines et al.
 8,398,720 B2 3/2013 Swords
 D680,649 S * 4/2013 Jagger D24/155
 D681,813 S * 5/2013 Jagger D24/155
 D685,476 S * 7/2013 Jagger D24/155
 D694,886 S * 12/2013 Jagger D24/155
 D751,202 S 3/2016 Gabele
 9,549,819 B1 1/2017 Bravo et al.
 D815,741 S 4/2018 Schuldt-Hempe
 D837,988 S * 1/2019 Khubani D24/192
 10,588,731 B2 * 3/2020 Priewe A61F 2/0063
 2005/0261780 A1 11/2005 Heino et al.
 2005/0288790 A1 12/2005 Swords
 2007/0213838 A1 9/2007 Hengelmolen
 2009/0216338 A1 8/2009 Gingras et al.
 2011/0282452 A1 11/2011 Koerner et al.
 2011/0301717 A1 12/2011 Becker
 2012/0330435 A1 12/2012 Engqvist et al.
 2013/0096371 A1 * 4/2013 Arcand A61F 2/0063
 600/37
 2013/0103079 A1 4/2013 Lau et al.
 2013/0236853 A1 9/2013 Axelsson et al.
 2014/0114266 A1 4/2014 Arcand
 2014/0257348 A1 * 9/2014 Priewe A61F 2/0063
 606/151

2014/0276995 A1 9/2014 Lau et al.
 2015/0057762 A1 * 2/2015 Harms B29C 43/18
 623/23.74
 2015/0105806 A1 4/2015 Dorafshr et al.
 2015/0238300 A1 * 8/2015 Wang A61L 31/10
 606/151
 2015/0250574 A1 9/2015 Egnelov
 2015/0374497 A1 12/2015 Engstrand et al.
 2017/0143872 A1 5/2017 Limem et al.

FOREIGN PATENT DOCUMENTS

EP 2030596 A1 3/2009
 JP 2014046025 A 3/2014
 KR 100952730 B1 4/2010
 WO 2008047415 A1 4/2008
 WO 2012036129 A1 3/2012
 WO 2012079611 A1 6/2012
 WO 2016024248 A1 2/2016

OTHER PUBLICATIONS

Biomet, CranioCurve brochure, (Downloaded 2013), 2 pages.
 Codman Neuro Device Biomech Catalogue, (Downloaded 2015), 1 page.
 Mikami et al., "Explosure of titanium implants after cranioplasty: A matter of long-term consequences", Interdis. Neuro.: Adv. Tech. and Case Manage. 8, (2017), pp. 64-67.
 Lau et al., "A Method for Combining Thin and Thick Malleable Titanium Mesh in the Repair of Cranial Defects", Cereus 7, e267. DOI 10.7759/cereus.267, (2015), 9 pages.
 KLS Martin Group, "Neurosurgery" brochure, (2018), 28 pages.
 International Search Report dated Jul. 11, 2019, in PCT/CA2019/050419 filed Apr. 5, 2019, 3 pages.

* cited by examiner

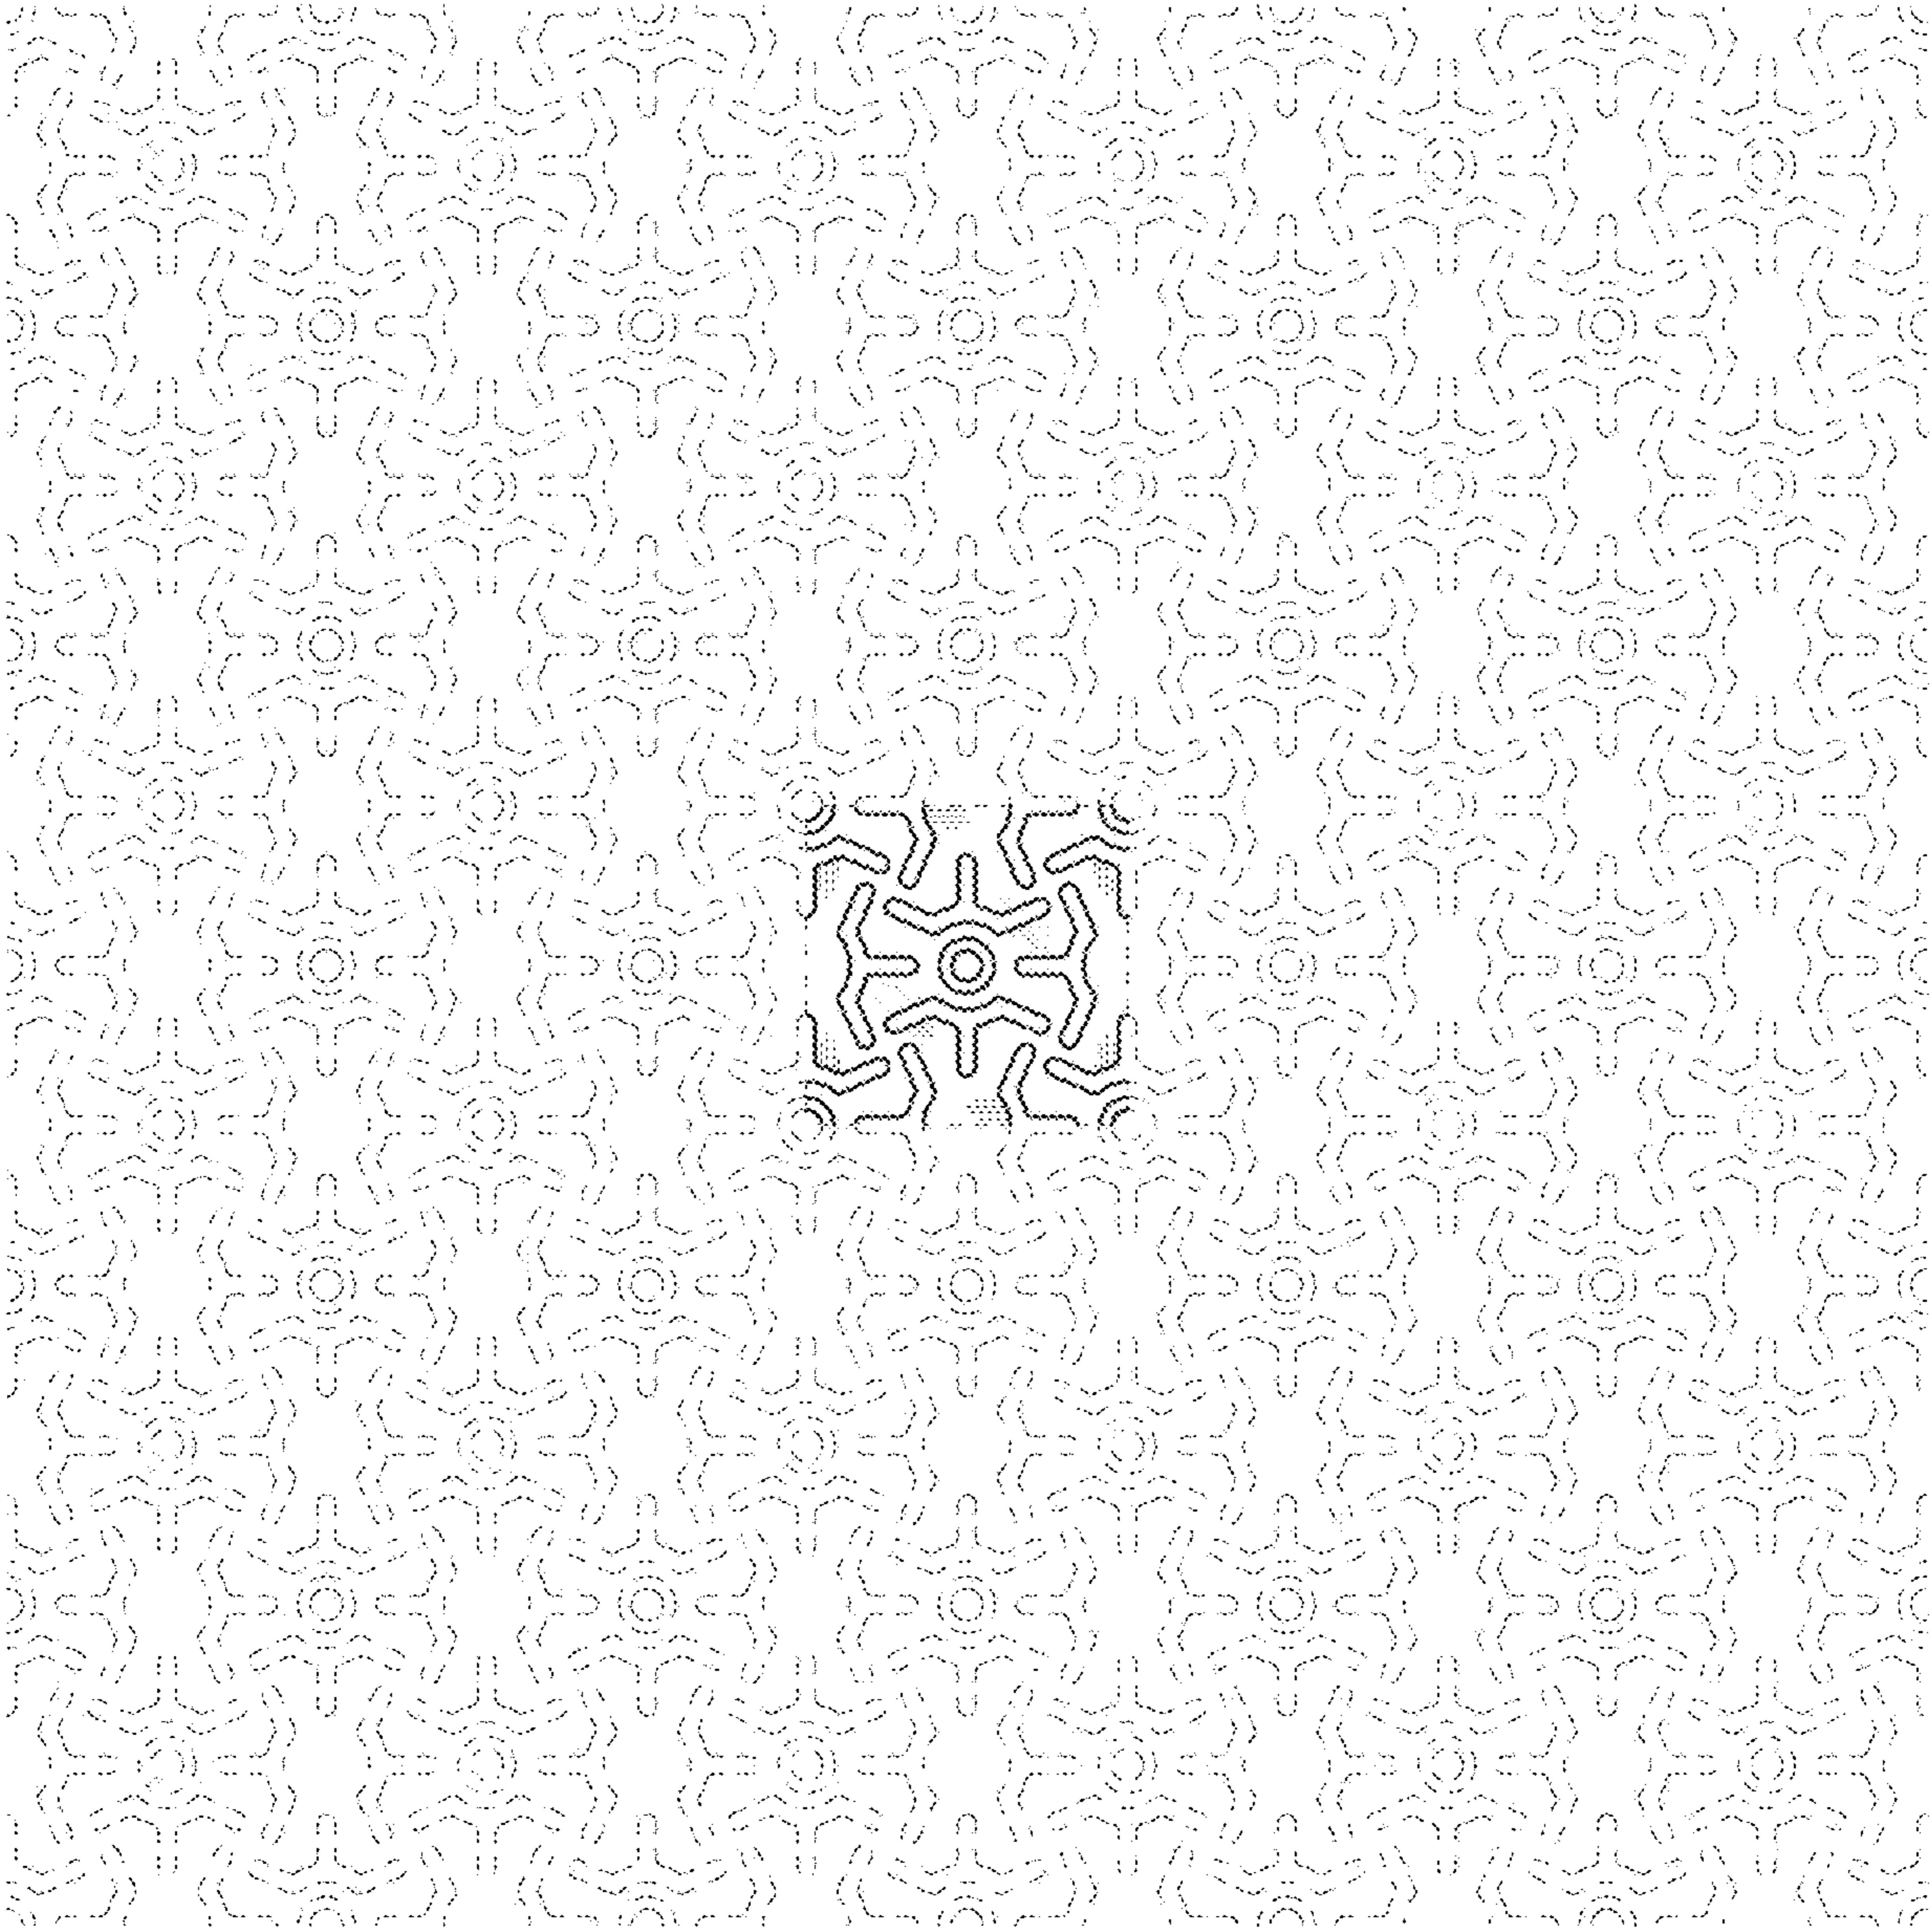


FIG. 1

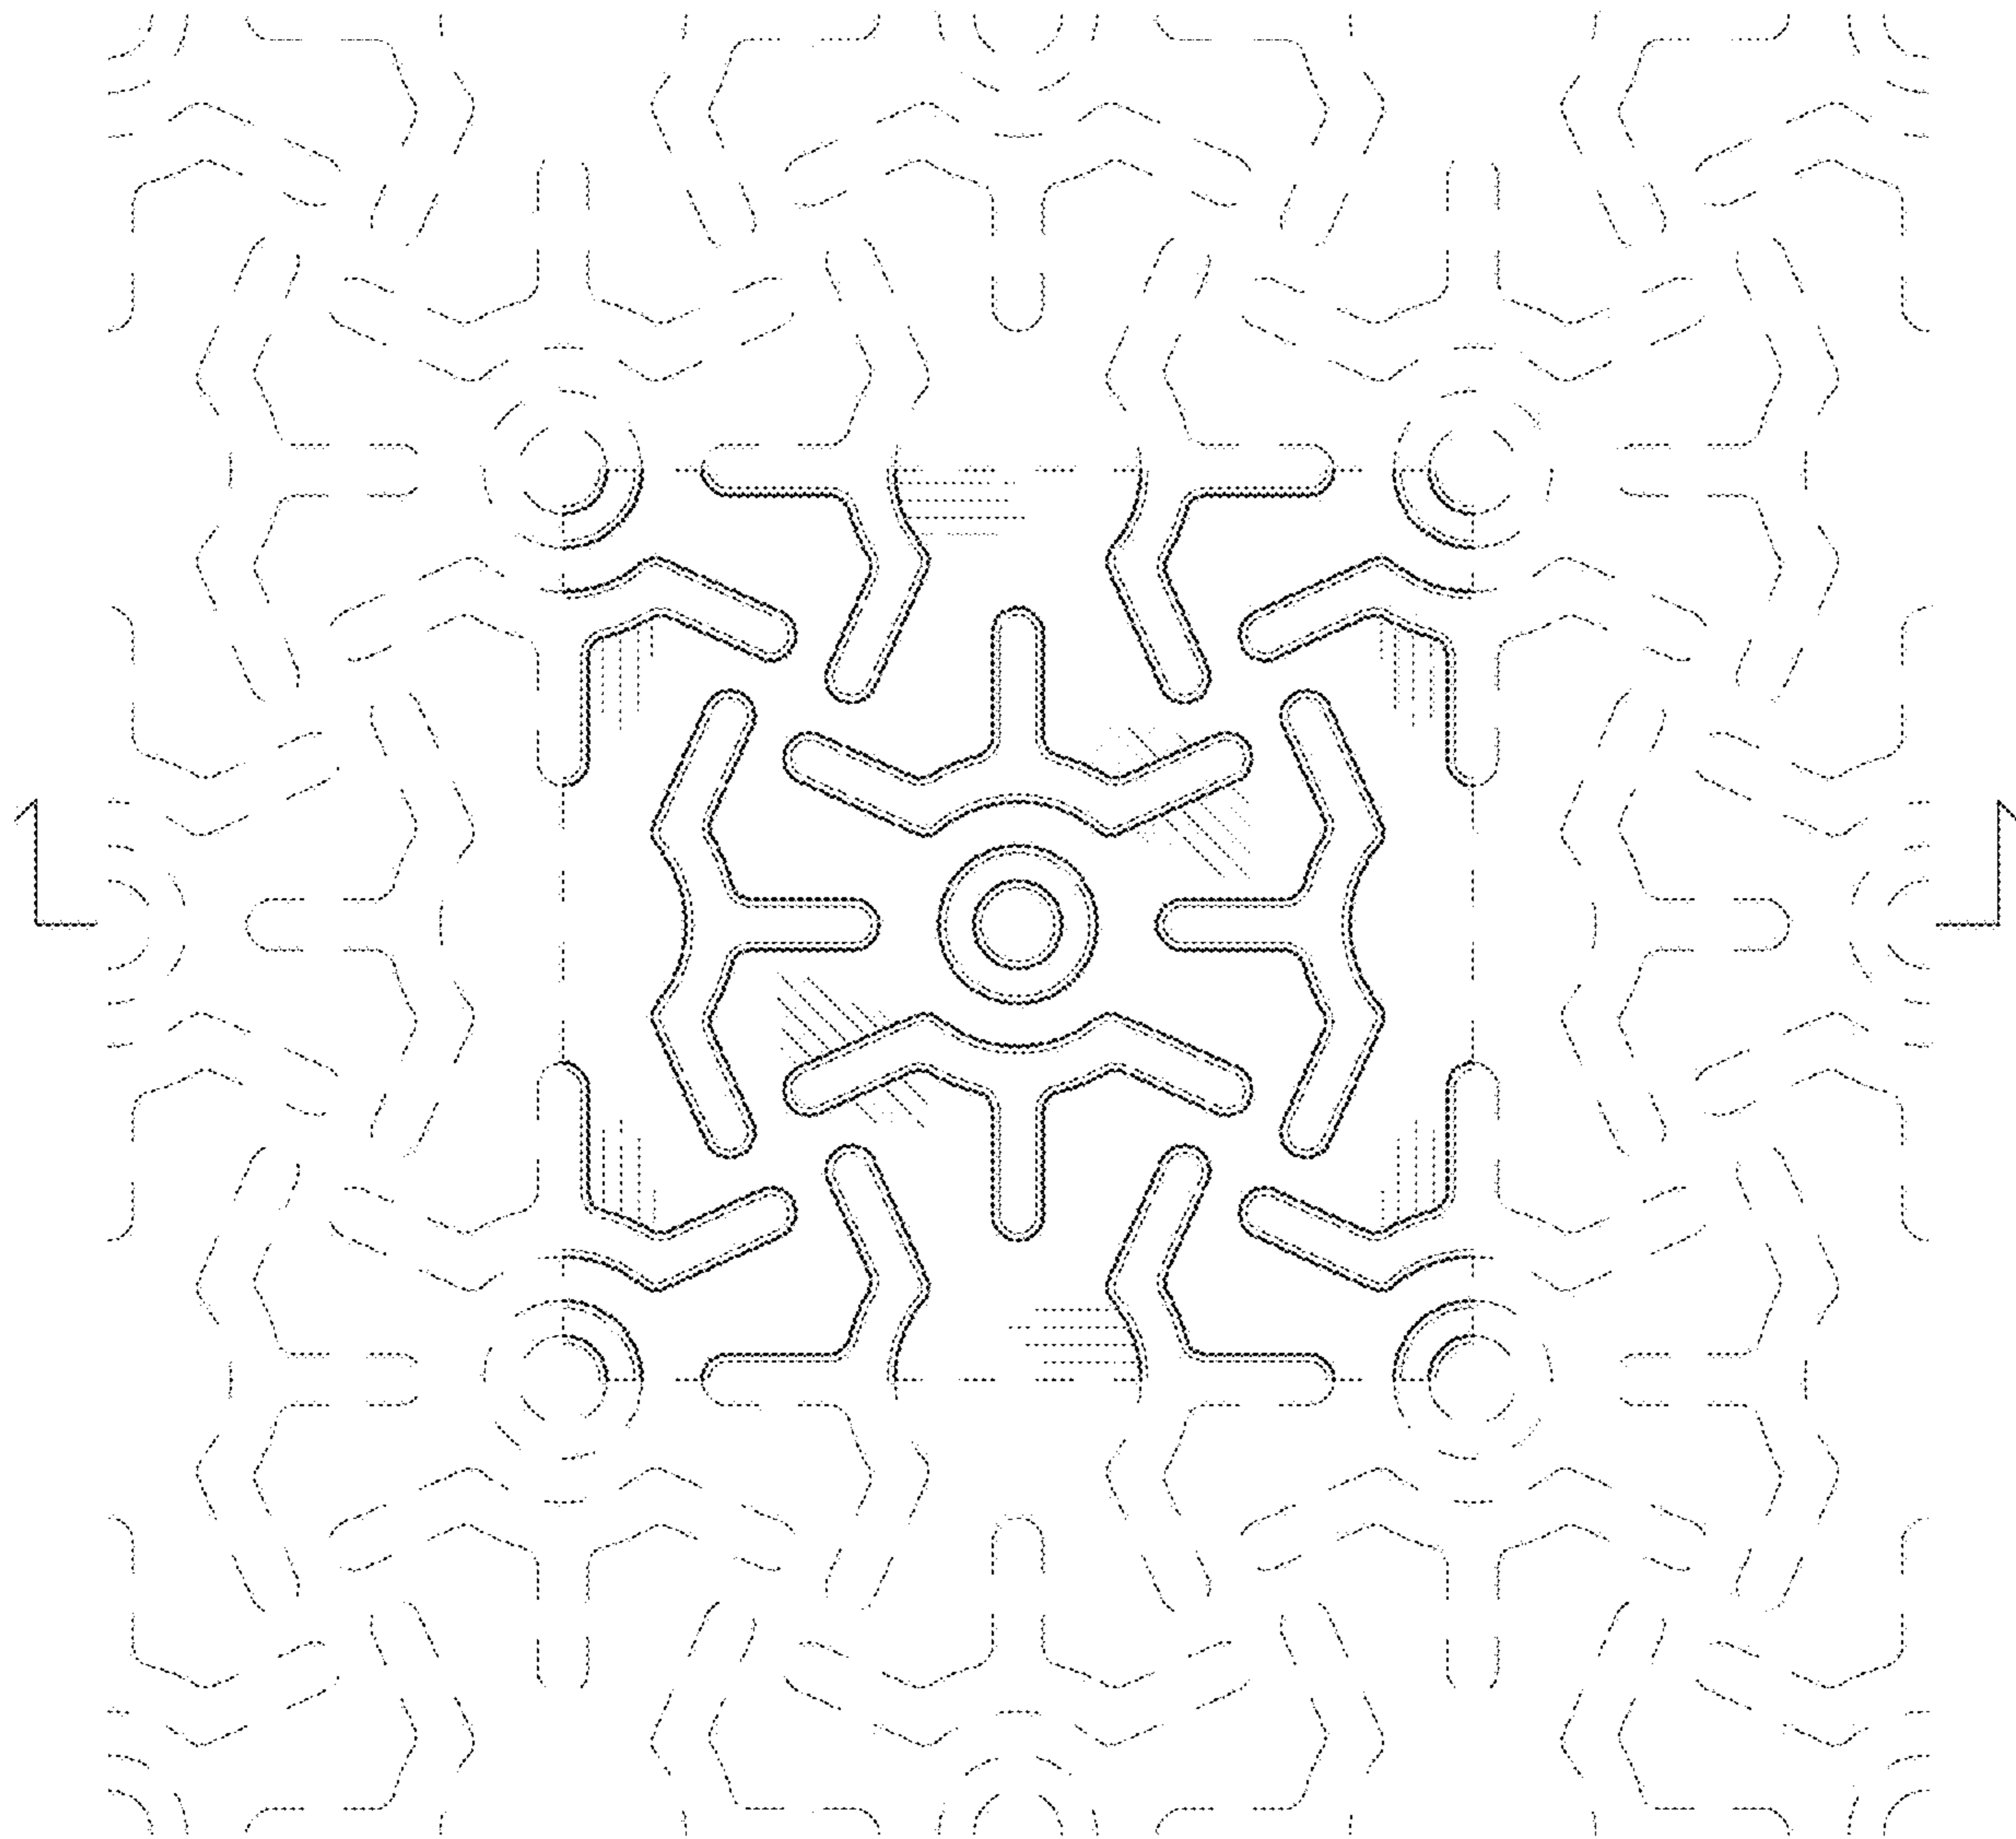


FIG. 2

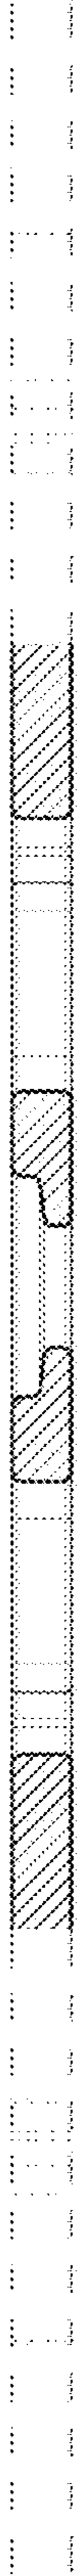


FIG. 3



FIG. 4



FIG. 5

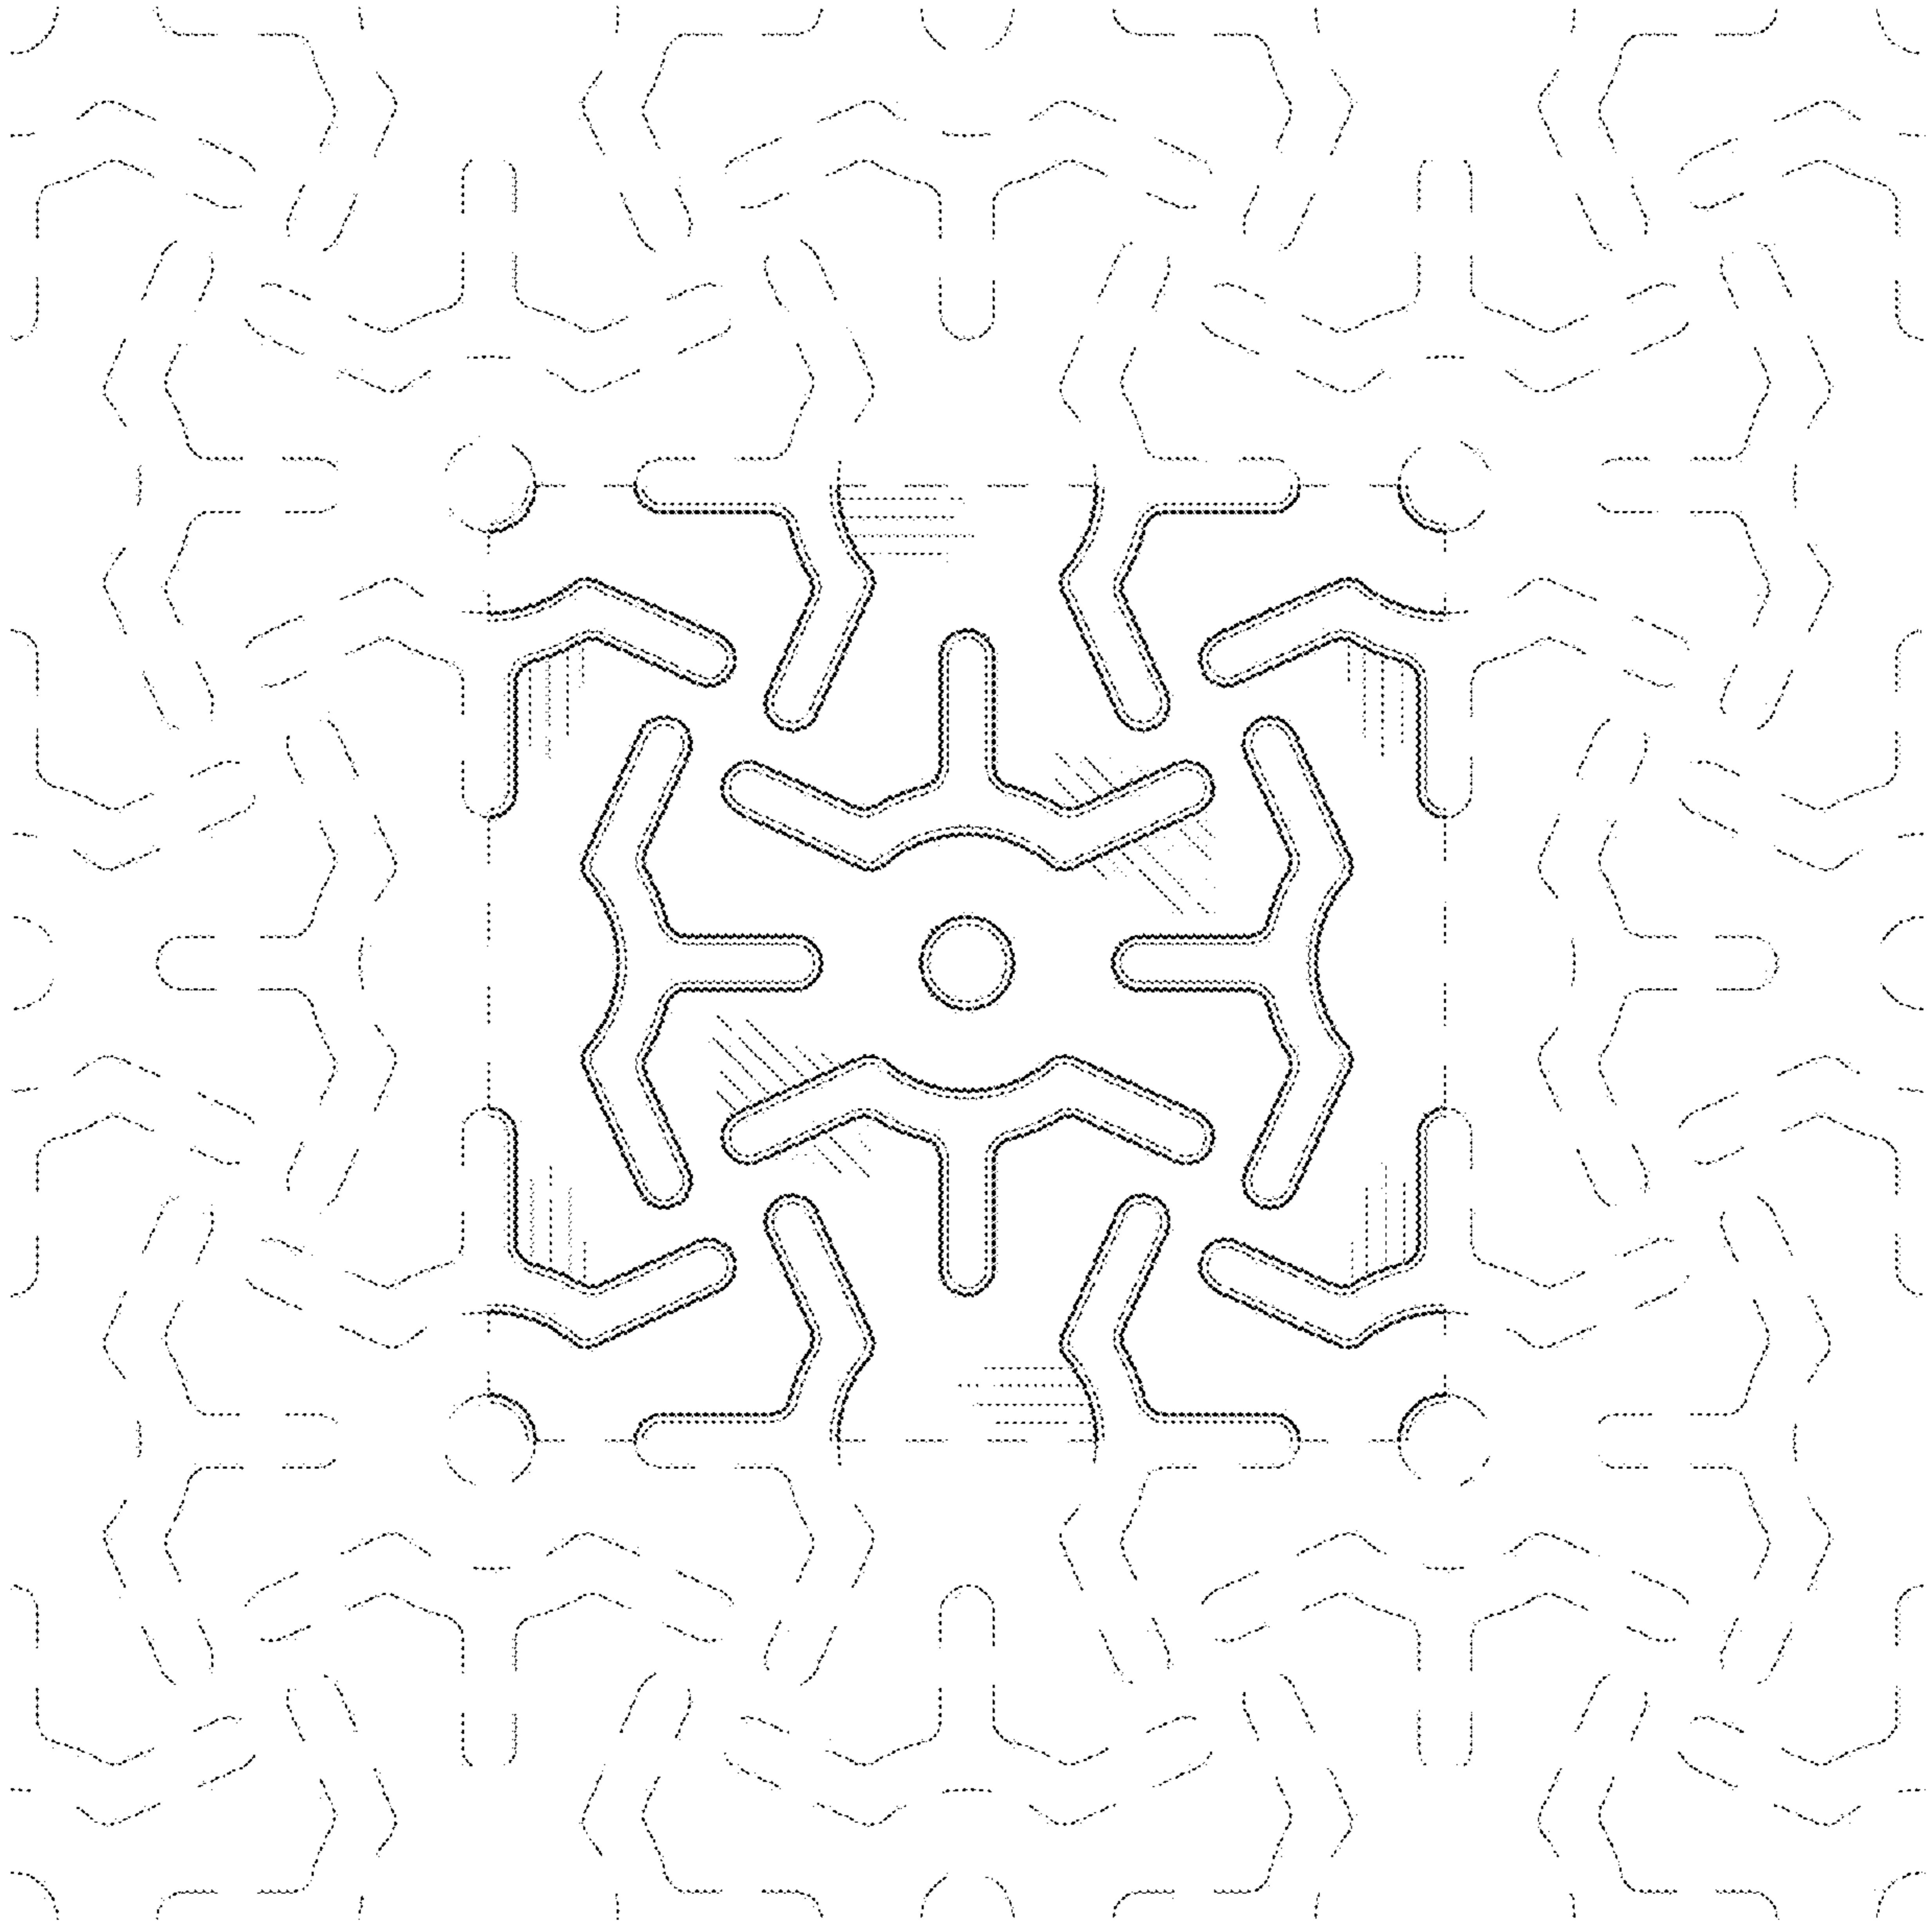


FIG. 6

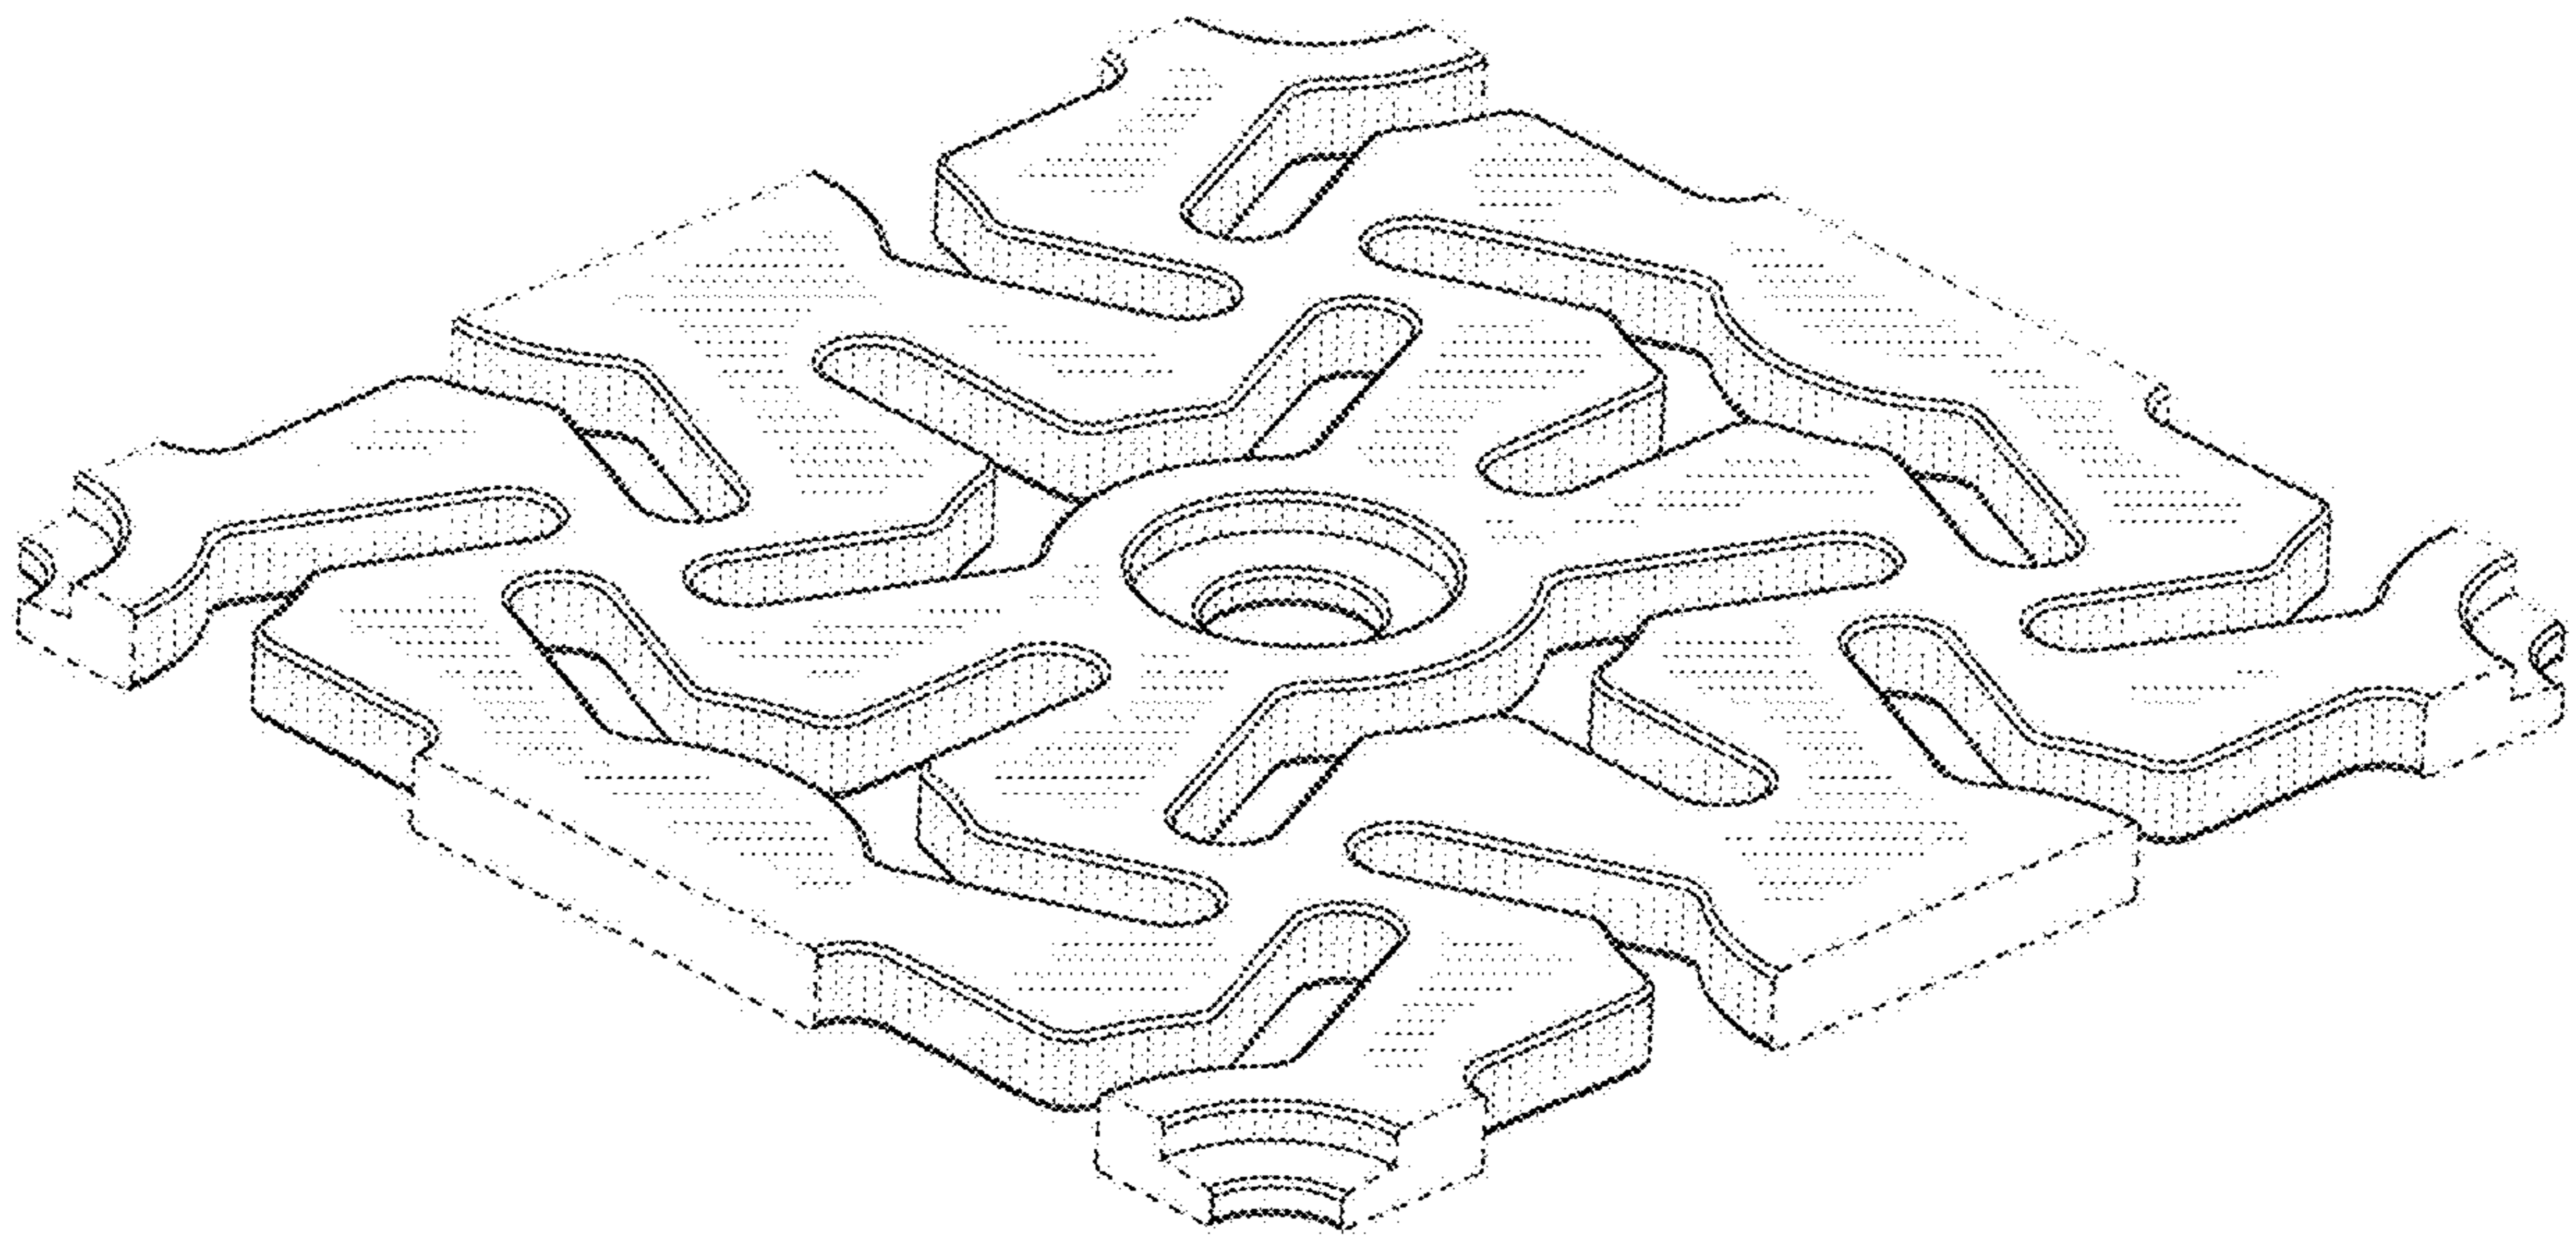


FIG. 7