



US00D910930S

(12) **United States Design Patent** (10) **Patent No.:** **US D910,930 S**
Hull et al. (45) **Date of Patent:** **** Feb. 16, 2021**

(54) **GLOVE WITH REDUCED FINGERTIP REGIONS AND A TEAR INDICATOR ROLLED CUFF**

FOREIGN PATENT DOCUMENTS

CA 3005865 5/2017

(71) Applicant: **Summit Glove Inc.**, Minerva, OH (US)

OTHER PUBLICATIONS

(72) Inventors: **James L. Hull**, Malvern, OH (US);
Christopher J. Pearen, Brampton (CA); **Ronald J. Thatcher**, Bond Head (CA)

CURAD Germ Shield Nitrile Exam Gloves, posted at amazon.com, posting date Aug. 20, 2018, [online], [site visited Dec. 17, 2020]. Available from Internet, URL: <https://www.amazon.ca/Nitrile-Disposable-Resistant-Cleaning-Improvement/dp/B07GP3MB3D> (Year: 2018).*

(73) Assignee: **Summit Glove Inc.**, Minerva, OH (US)

(Continued)

(**) Term: **15 Years**

Primary Examiner — George D. Kirschbaum

(21) Appl. No.: **29/734,655**

Assistant Examiner — Maria J. Edwards

(22) Filed: **May 14, 2020**

Related U.S. Application Data

(57) **CLAIM**

(60) Division of application No. 29/672,281, filed on Dec. 4, 2018, now Pat. No. Des. 890,999, which is a continuation-in-part of application No. 15/136,191, filed on Apr. 22, 2016, now Pat. No. 10,390,575.

The ornamental design for a glove with reduced fingertip regions and a tear indicator rolled cuff, as shown and described.

(51) **LOC (13) Cl.** **02-06**

(52) **U.S. Cl.**
USPC **D29/117.1; D2/617**

(58) **Field of Classification Search**
USPC D29/113, 117.1; D2/617
CPC A41D 19/015; A41D 2600/20; A41D 19/01558

DESCRIPTION

See application file for complete search history.

(56) **References Cited**


U.S. PATENT DOCUMENTS

1,559,114 A 10/1925 Maranville
2,058,221 A 10/1936 Ferguson
2,075,550 A * 3/1937 Smith A41D 19/0062
2/168
2,266,716 A * 12/1941 Robertson A41D 19/0058
2/168
2,335,871 A * 12/1943 Milligan A41D 19/0058
2/168

FIG. 1 is a front elevational view of a hand-specific glove with reduced fingertip regions and a tear indicator rolled cuff in accordance with our design, where the glove is designed to be worn on the left hand of a user; a glove for a right hand of the user being a mirror-image thereof; FIG. 2 is a rear elevation view thereof; FIG. 3 is a left side elevation view thereof; FIG. 4 is a right side elevation view thereof; FIG. 5 is a top plan view thereof; FIG. 6 is a bottom plan view thereof; and, FIG. 7 is a longitudinal cross-section of a middle finger region taken along line 7-7 of FIG. 2. The broken lines illustrate environment and form no part of the claimed design.

(Continued)

1 Claim, 4 Drawing Sheets

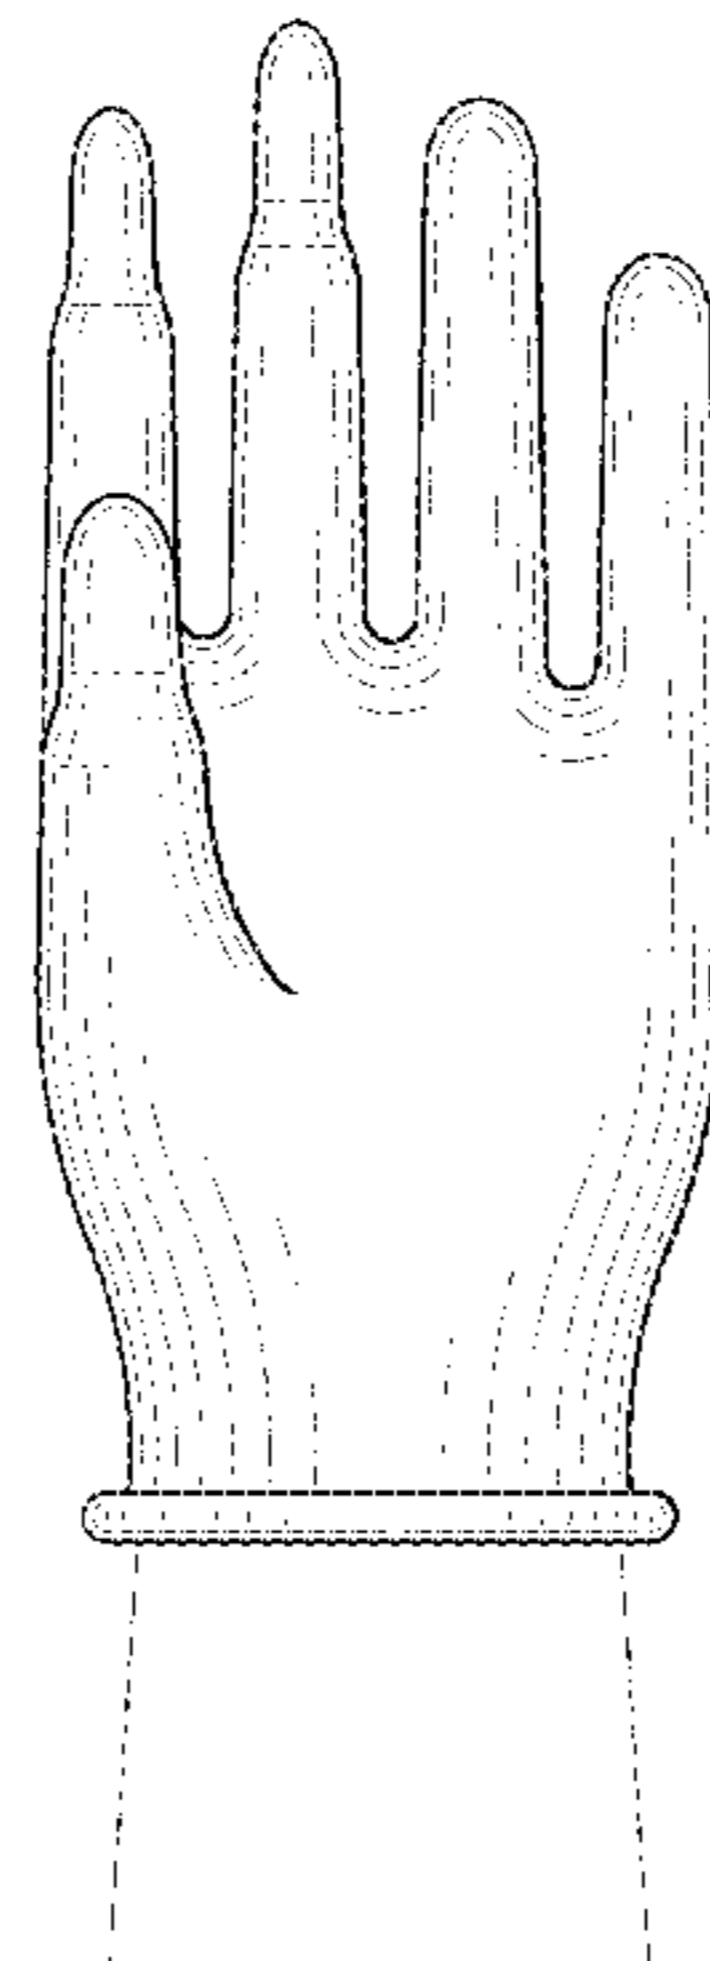

(56)

References Cited

U.S. PATENT DOCUMENTS

2,348,773 A * 5/1944 Wyman A61B 42/20
2/21
3,283,338 A 11/1966 Landau
4,149,601 A * 4/1979 Taylor A41D 19/01594
172/370
4,507,807 A 4/1985 Karkanen
4,742,578 A 5/1988 Seid
4,843,014 A 6/1989 Cukier
5,323,490 A 6/1994 Yarbrough
5,442,816 A 8/1995 Seketa
5,687,424 A * 11/1997 Masley A41D 19/01547
2/163
5,924,137 A 7/1999 Gold
6,031,042 A 2/2000 Lipinski
6,092,238 A 7/2000 Fierabend, Jr.
6,451,893 B1 9/2002 Tao
D513,827 S * 1/2006 Ward D2/619
9,179,718 B2 11/2015 Anstey
9,302,171 B1 4/2016 Iacono
9,968,145 B2 * 5/2018 Hull A41D 19/0082
10,238,159 B2 3/2019 Hull
10,390,575 B2 8/2019 Hull
10,602,787 B2 * 3/2020 Hull B32B 25/14
10,602,788 B2 * 3/2020 Hull B32B 25/14
D890,999 S * 7/2020 Hull D29/117.1
10,820,639 B2 * 11/2020 Hull A41D 19/0006
10,820,640 B2 * 11/2020 Hull A41D 19/0082
2009/0139007 A1 6/2009 Bevier
2012/0036612 A1 2/2012 Hull
2013/0239291 A1 9/2013 Harris
2013/0291282 A1 11/2013 Anstey
2015/0164160 A1 6/2015 Furlong
2016/0309815 A1 * 10/2016 Hull A61B 42/10
2017/0142931 A1 5/2017 Michaelson et al.

2017/0231705 A1 8/2017 Madison
2017/0295868 A1 10/2017 Yahnite
2017/0318879 A1 11/2017 Gleser
2017/0348065 A1 12/2017 Bluecher
2018/0263315 A1 9/2018 Visokey
2019/0098944 A1 * 4/2019 Hull A41D 31/02
2019/0104782 A1 * 4/2019 Hull A41D 19/0003
2019/0104783 A1 * 4/2019 Hull A41D 19/0055
2019/0104784 A1 * 4/2019 Hull A41D 19/0003
2019/0125013 A1 * 5/2019 Hull A41D 19/0082

OTHER PUBLICATIONS

Milker's Helpers Gloves, posted at rjmatthews.com, posting date not given, [online], [site visited Dec. 17, 2020]. Available from Internet, URL: <https://www.rjmatthews.com/details/Milkers-Helpers-Gloves/19-71820.html> (Year: 2020).*

Nick Gardner, Accelerator Free Fact or Fiction, Shield Scientific B.V., Health & Safety International, pp. 77-82, Oct. 2008.

SemperSure™ Nitrile, www.sempermedusa.com/products/semperure, Sempermed USA, Inc., 2 pages, document is indated but was publically available as of Aug. 18, 2014.

Nitrile Accelerator-Free Micro-Touch®, www.ansell.be/medical/pdf/gloves/EN/Micro-Touch%20Nitrile%20Accelerator-Free.pdf, Ansell, 2 pages, document is undated but was publically available as of Aug. 18, 2014.

Accelerator-Free Nitrile Exam Gloves—A Better Alternative, <http://hourglass-intl.com/2011/04/18/accelerator-free-nitrile-exam-gloves-a-better-alternative/>, Hourglass International, 4 pages, Apr. 18, 2011.

New Glove Materials Make Nitrile Gloves Better, <http://hourglass-intl.com/2011/01/24/new-glove-materials-make-nitrile-gloves-better/>, Hourglass International, 2 pages, Jan. 24, 2011.

* cited by examiner

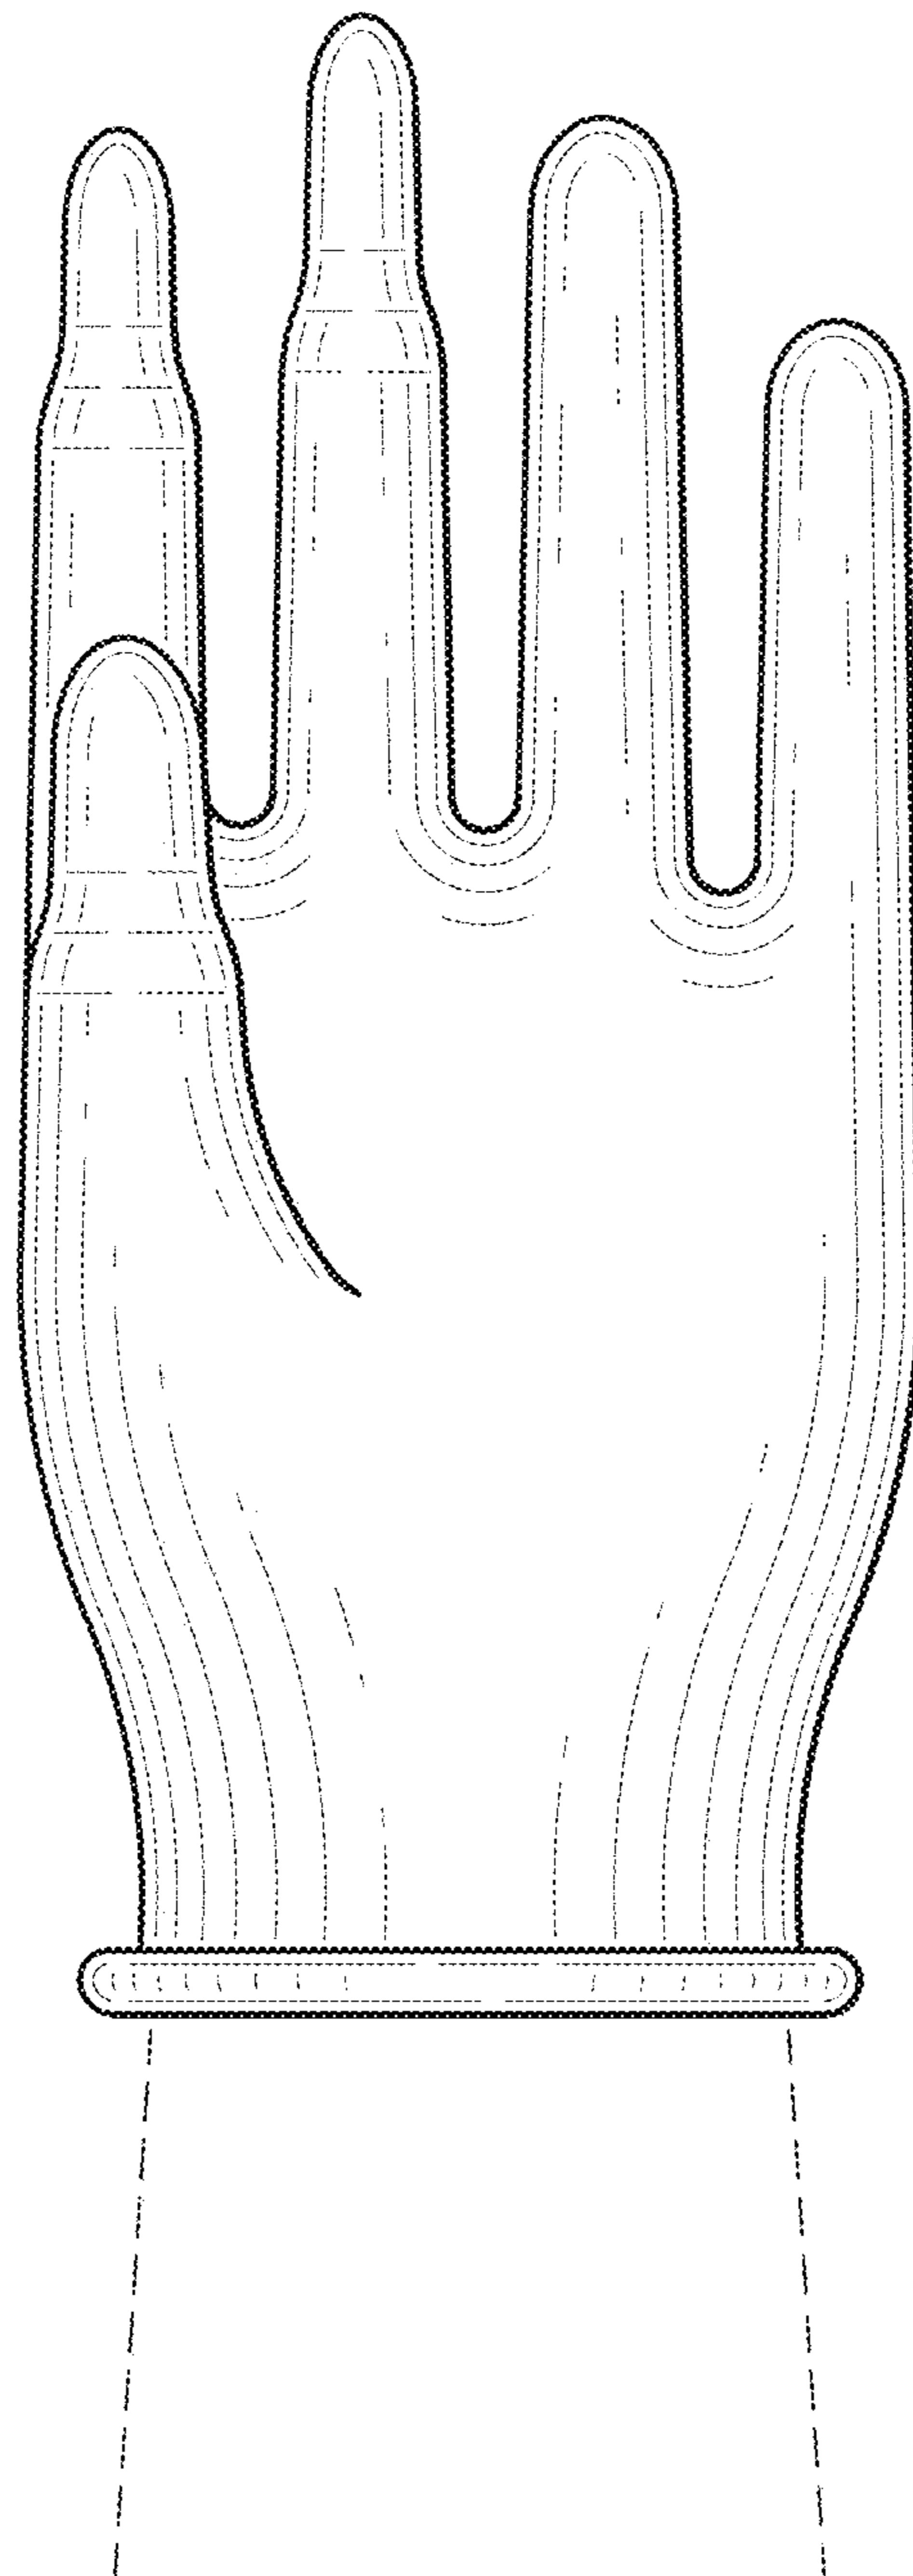


FIG. 1

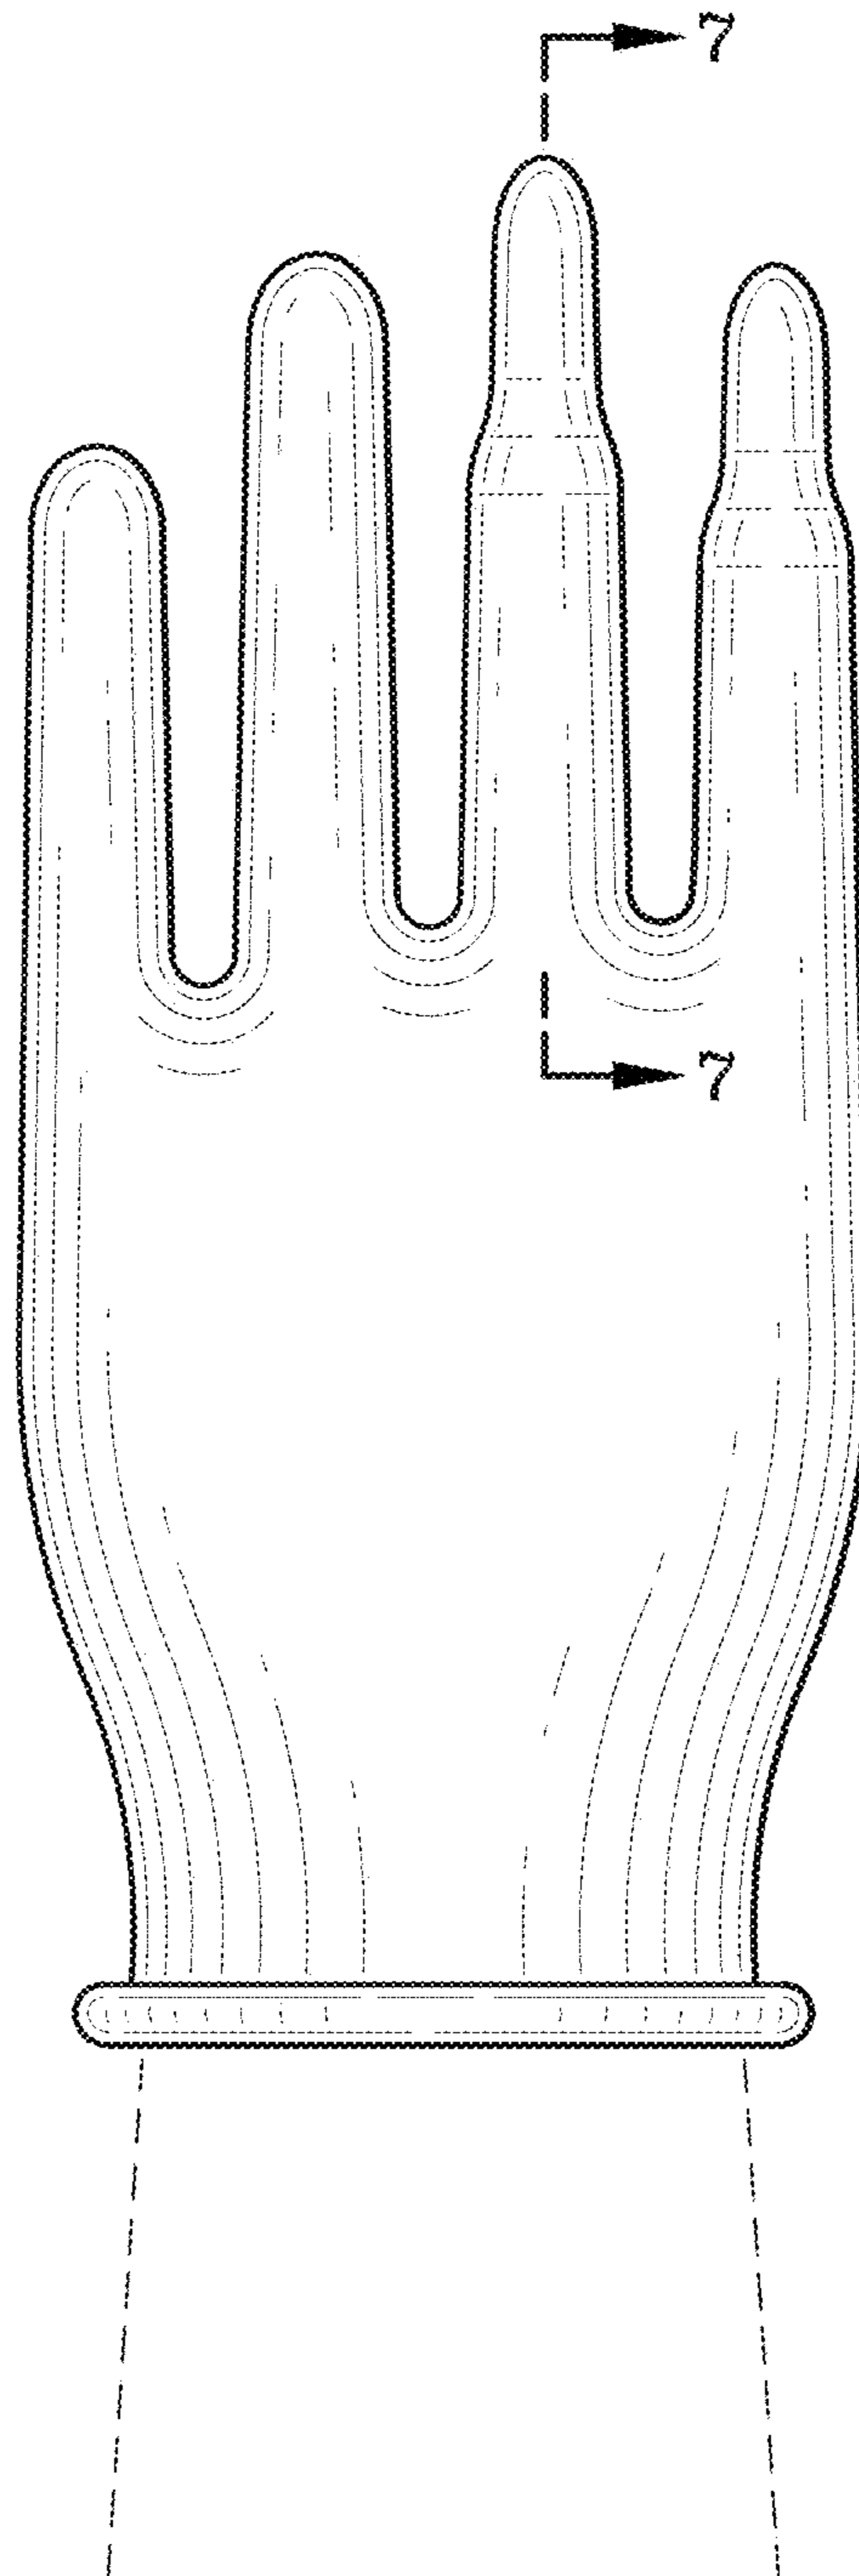


FIG. 2

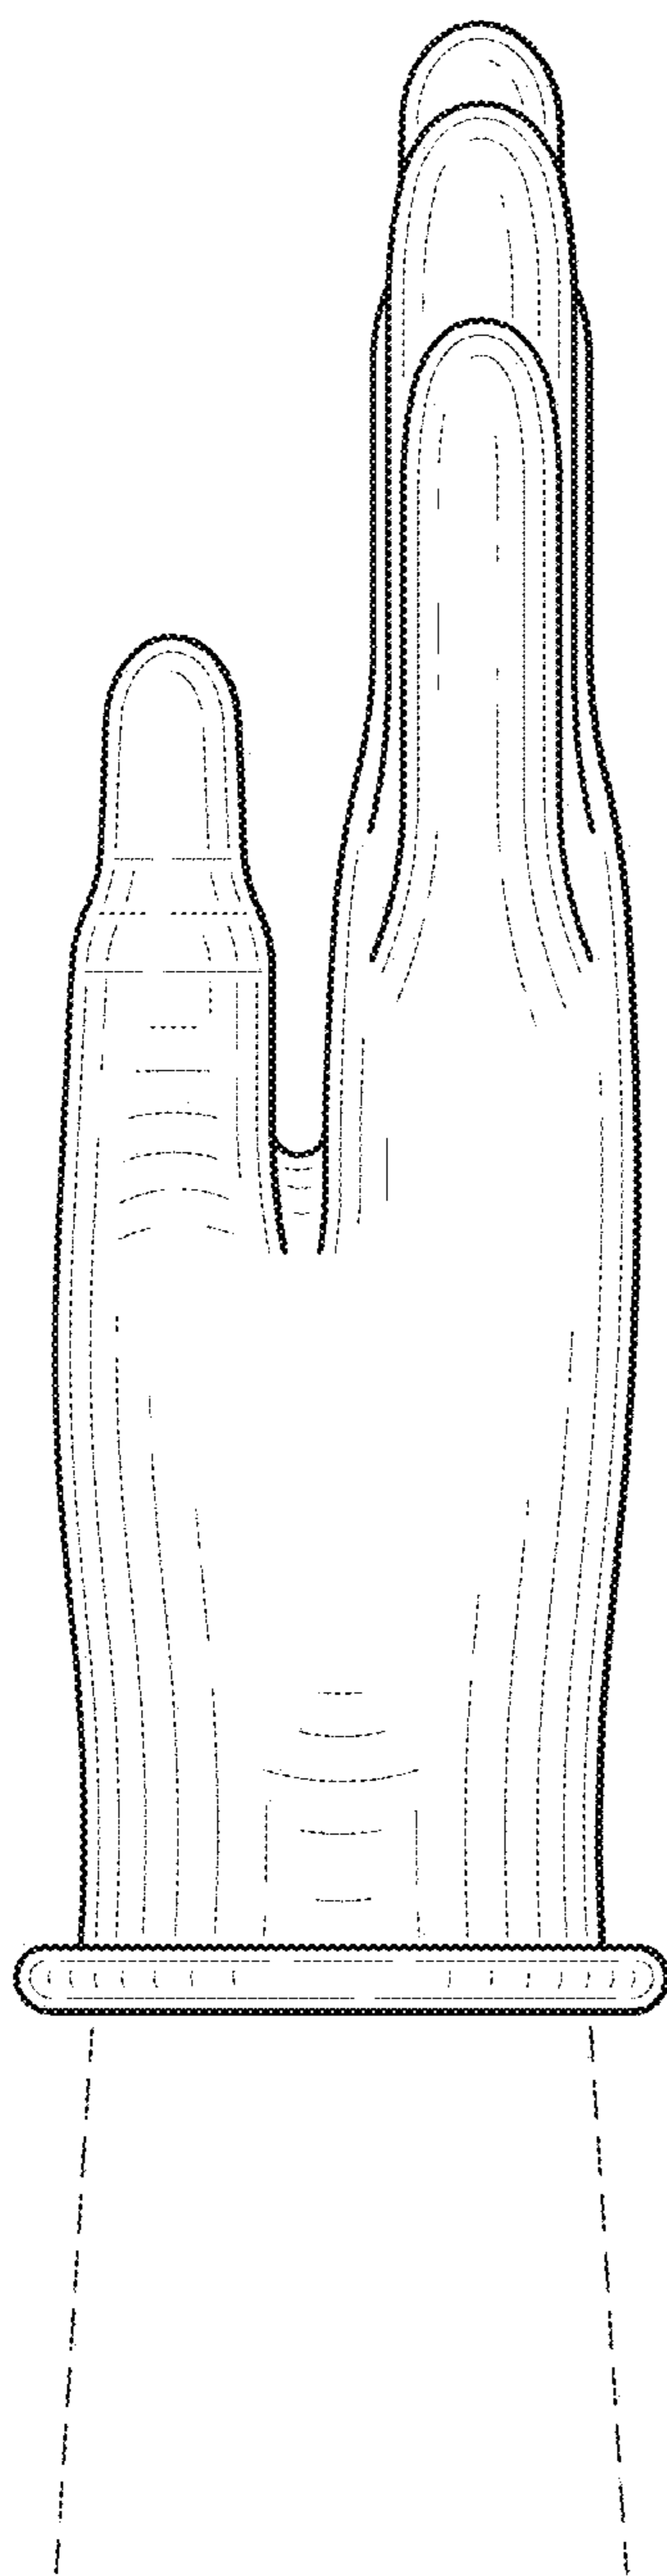


FIG. 3

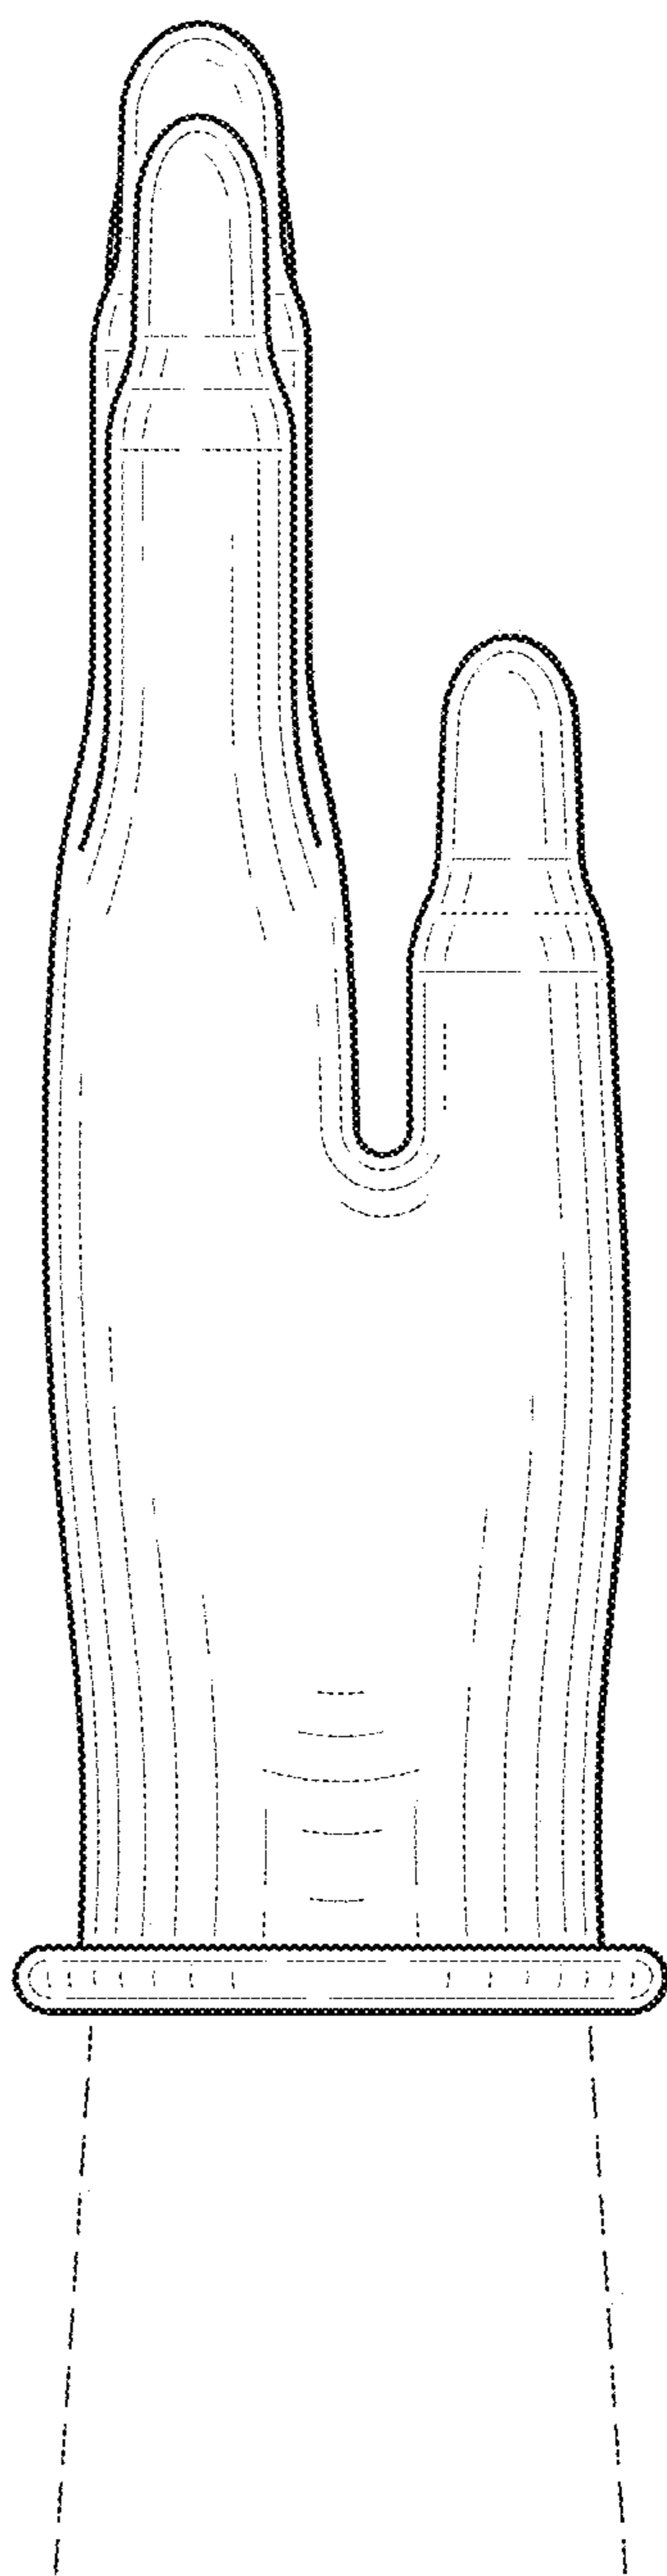


FIG. 4

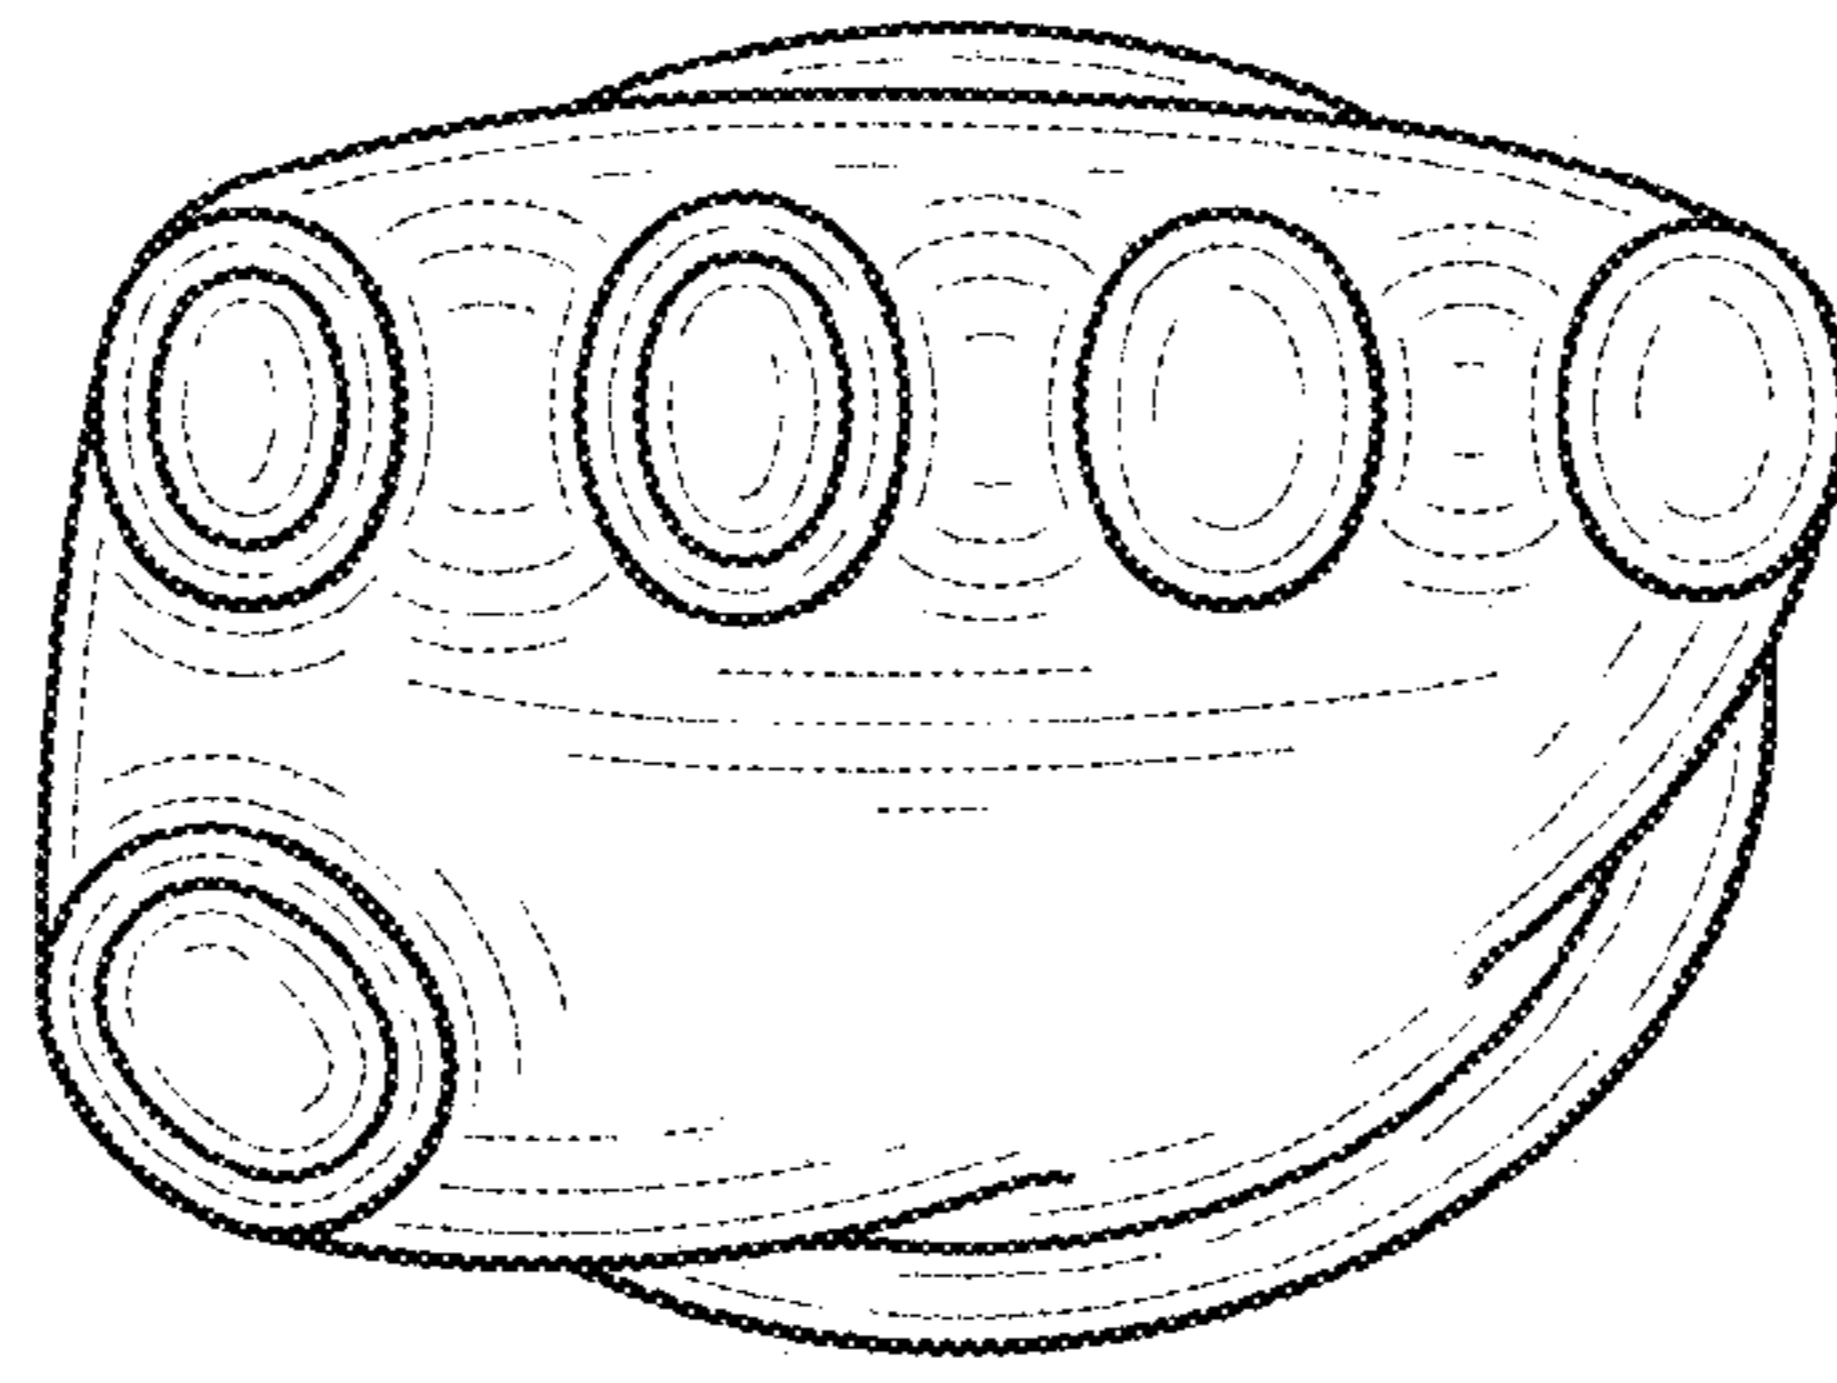


FIG. 5

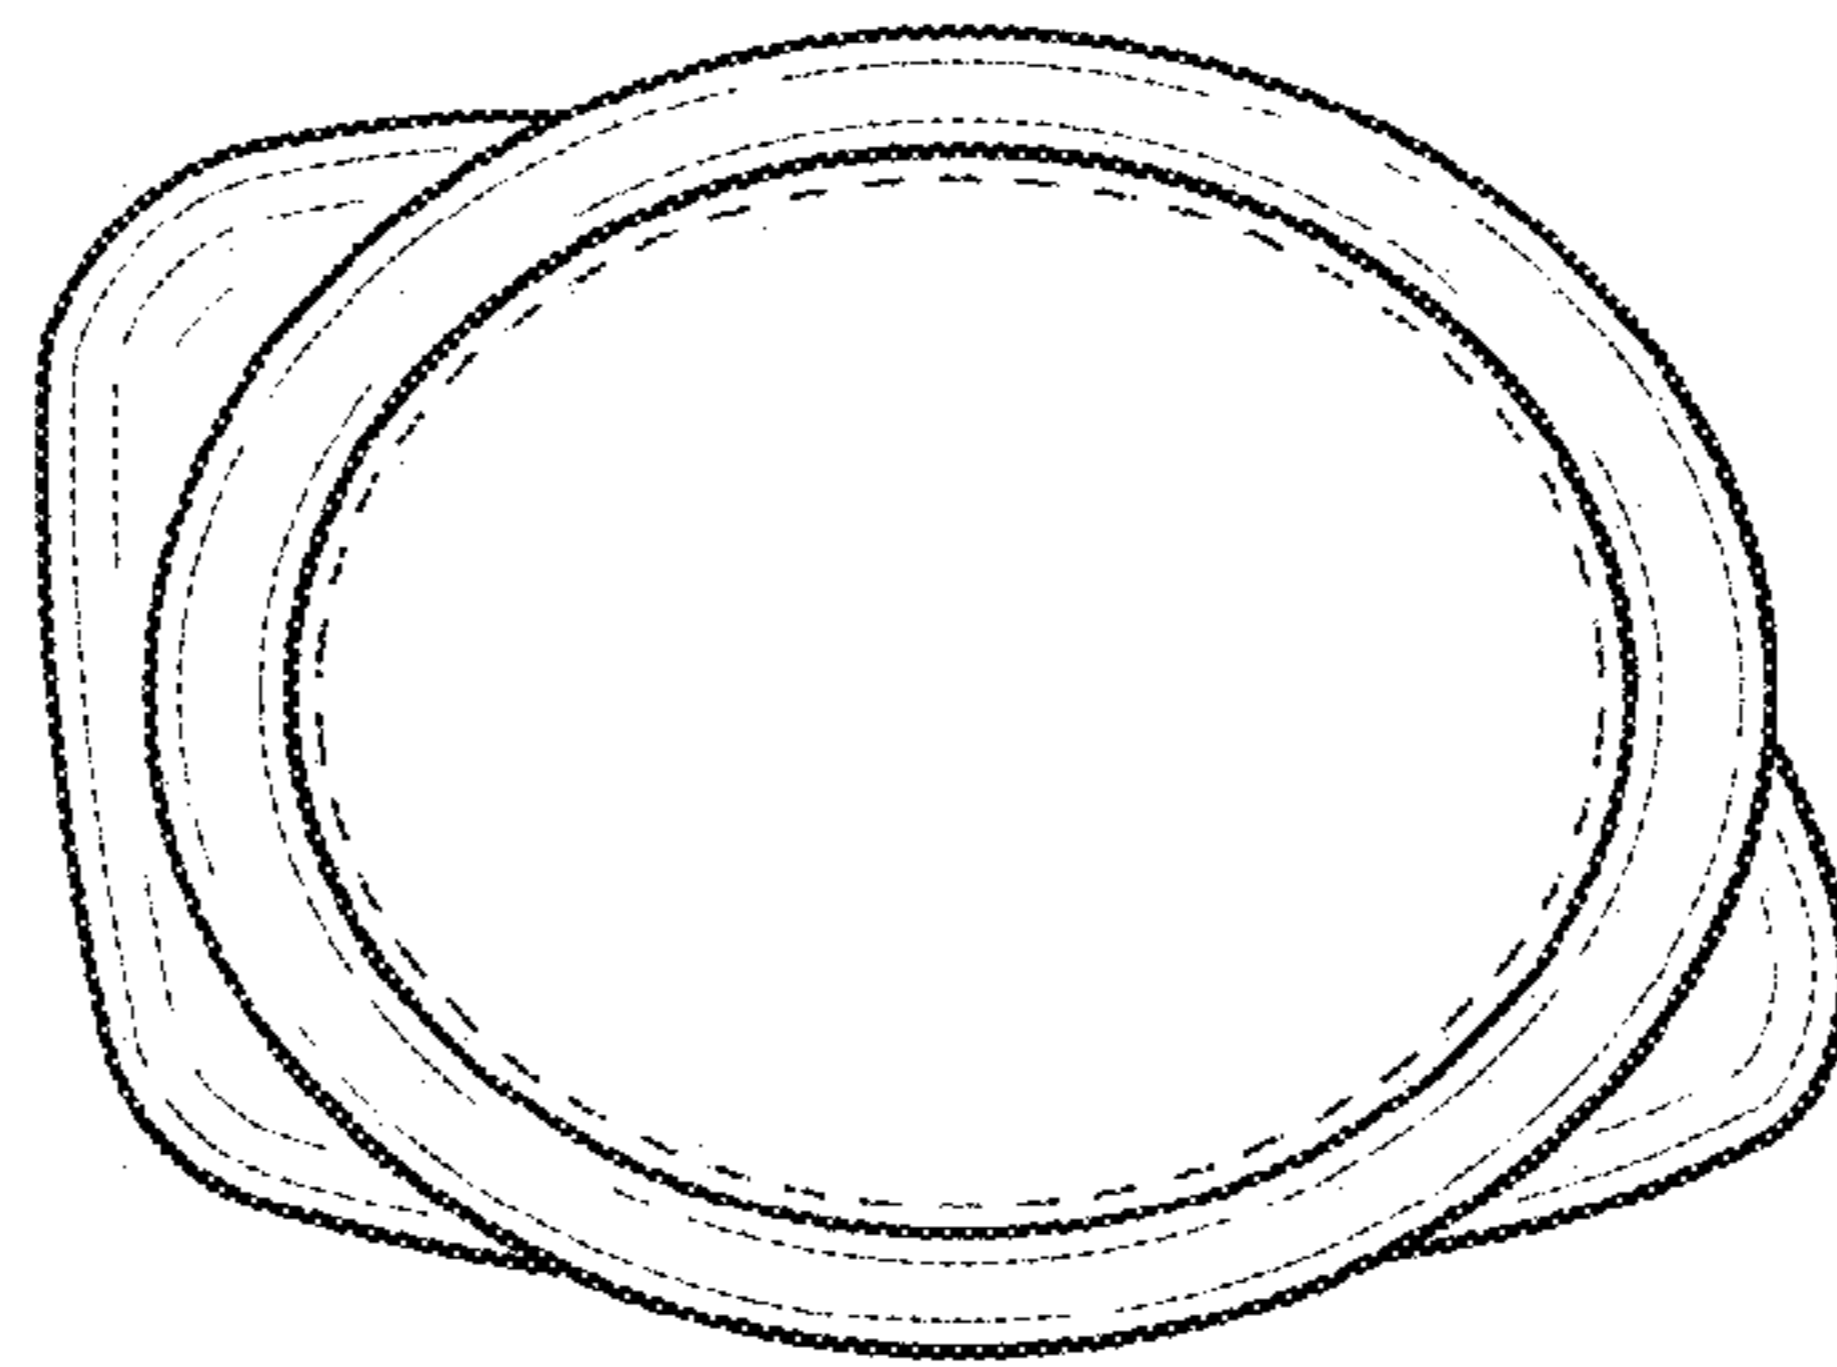


FIG. 6

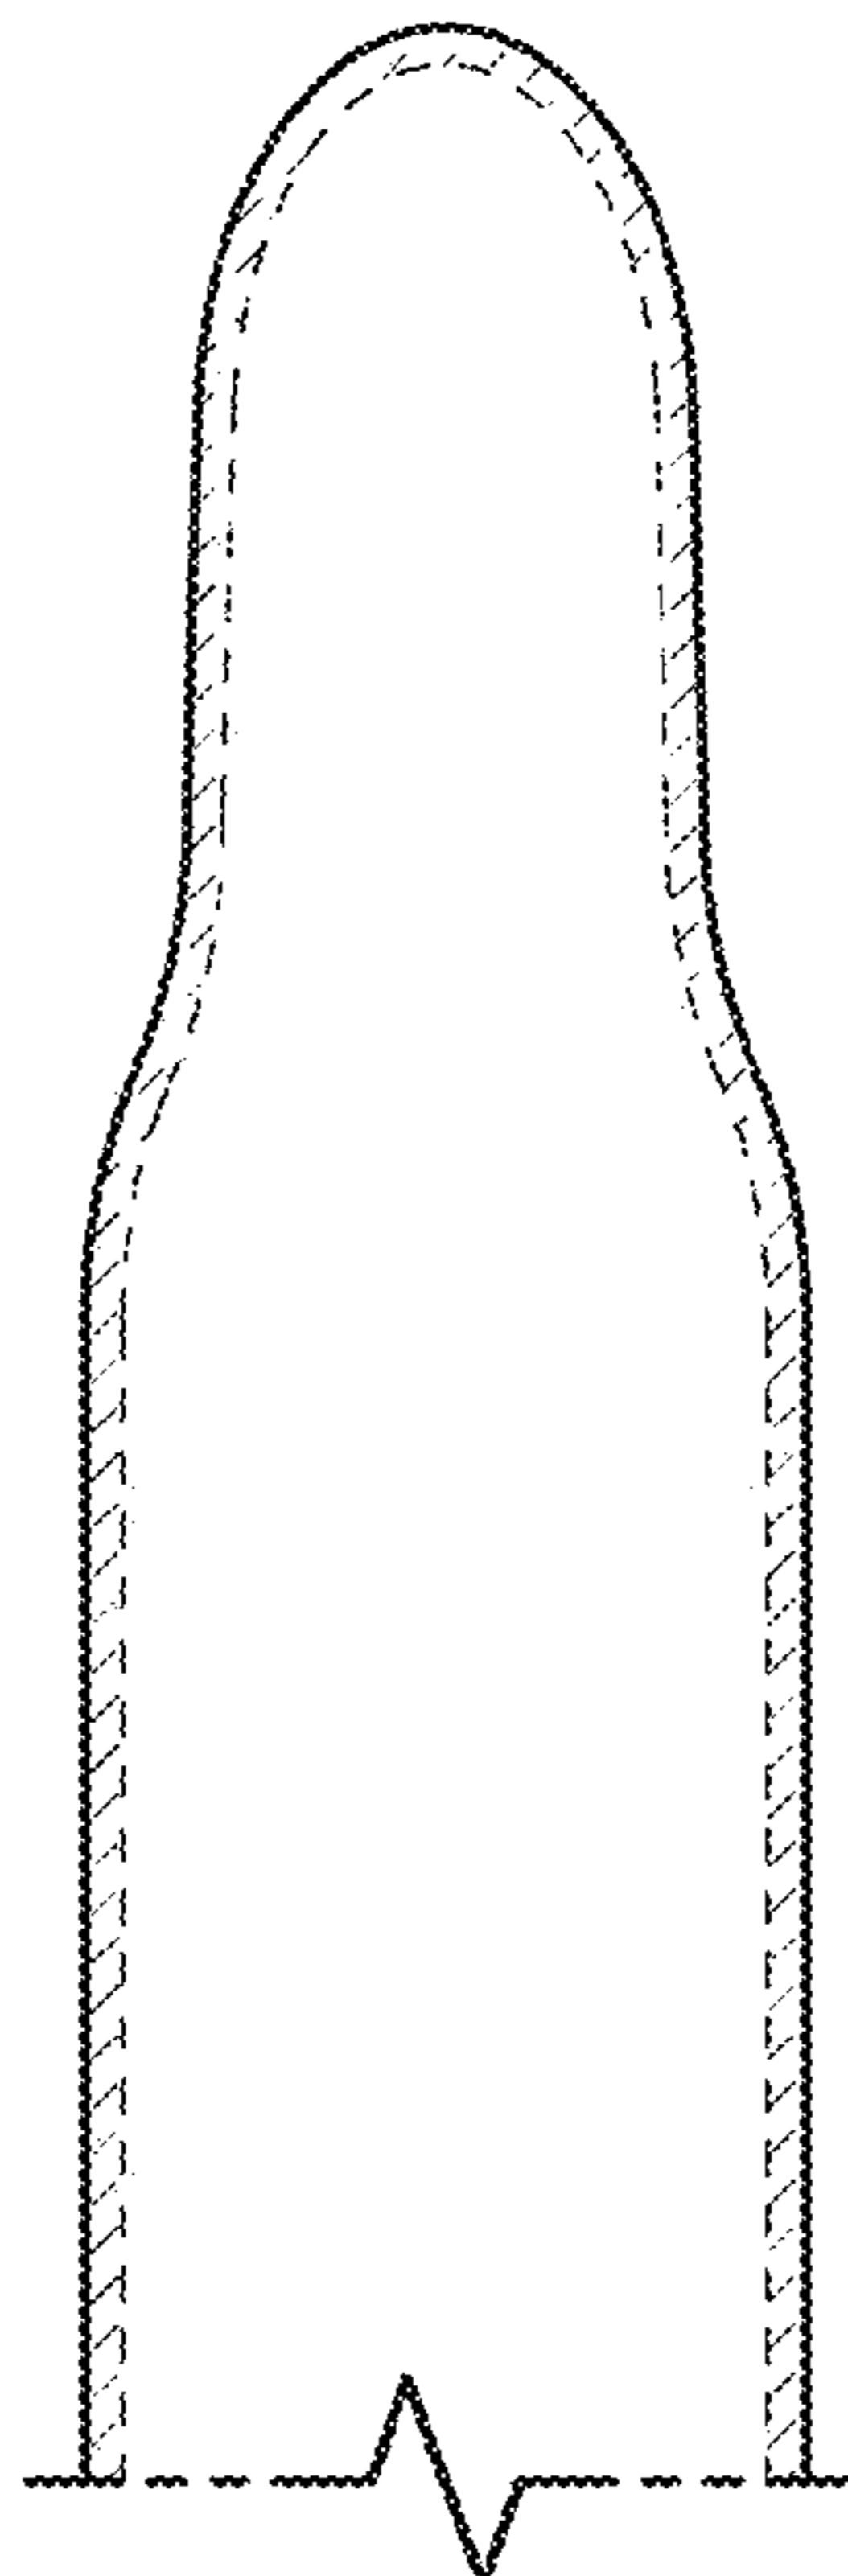


FIG. 7