



US00D911358S

(12) **United States Design Patent** (10) **Patent No.:** **US D911,358 S**
Ishikawa (45) **Date of Patent:** **** Feb. 23, 2021**

(54) **COMPUTER DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR DISPLAYING MEDICAL INFORMATION**

(71) Applicant: **FUJIFILM CORPORATION**, Tokyo (JP)

(72) Inventor: **Shigetoshi Ishikawa**, Kanagawa (JP)

(73) Assignee: **FUJIFILM CORPORATION**, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/683,929**

(22) Filed: **Mar. 18, 2019**

(30) **Foreign Application Priority Data**

Sep. 27, 2018 (JP) 2018-020991

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**

USPC D14/485-495
CPC G06F 17/211; G06F 17/212; G06F 3/048;
G06F 3/04817; G06F 3/0482; G06F
3/04842; A61B 2576/02; G06T 1/00;
G06T 11/00; G16H 10/00

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D655,710 S * 3/2012 Inada D14/485
8,280,166 B2 * 10/2012 Milanski H04N 1/6013
382/174
D694,253 S * 11/2013 Helm D14/485

(Continued)

OTHER PUBLICATIONS

“Thermal Cyclers: Thermal Gradient” Sep. 12, 2014, Bio-Rad, site visited Aug. 10, 2020: http://www.bio-rad.com/webroot/web/pdf/lsr/literature/Bulletin_5633.pdf (Year: 2014).*

(Continued)

Primary Examiner — Jack Reickel

Assistant Examiner — Christopher M Spivey

(74) *Attorney, Agent, or Firm* — Solaris Intellectual Property Group, PLLC

(57) **CLAIM**

The ornamental design for a computer display screen with graphical user interface for displaying medical information, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a computer display screen, showing the new design;

FIG. 2 is a top view thereof;

FIG. 3 is a left side view thereof;

FIG. 4 is an enlarged view of a portion of the image in FIG. 1.


FIG. 5 is an enlarged view of the portion surrounded by the dashed-dotted line in FIG. 1.

FIG. 6 is an enlarged view of the square lying at the intersection of the horizontal and vertical lines marked 6 in FIG. 5; and,

FIG. 7 is an enlarged view of the square lying at the intersection of the horizontal and vertical lines marked 7 in FIG. 5.

The broken lines showing the display screen and the graphical user interface are included for the purpose of illustrating portions of the article and form no part of the claimed design. The rectangle formed by the dashed-dotted line in FIG. 1 and FIG. 4 only indicates a boundary between the portion for which a design registration is sought as a partial design and other portions in FIG. 1 and FIG. 4.

1 Claim, 7 Drawing Sheets

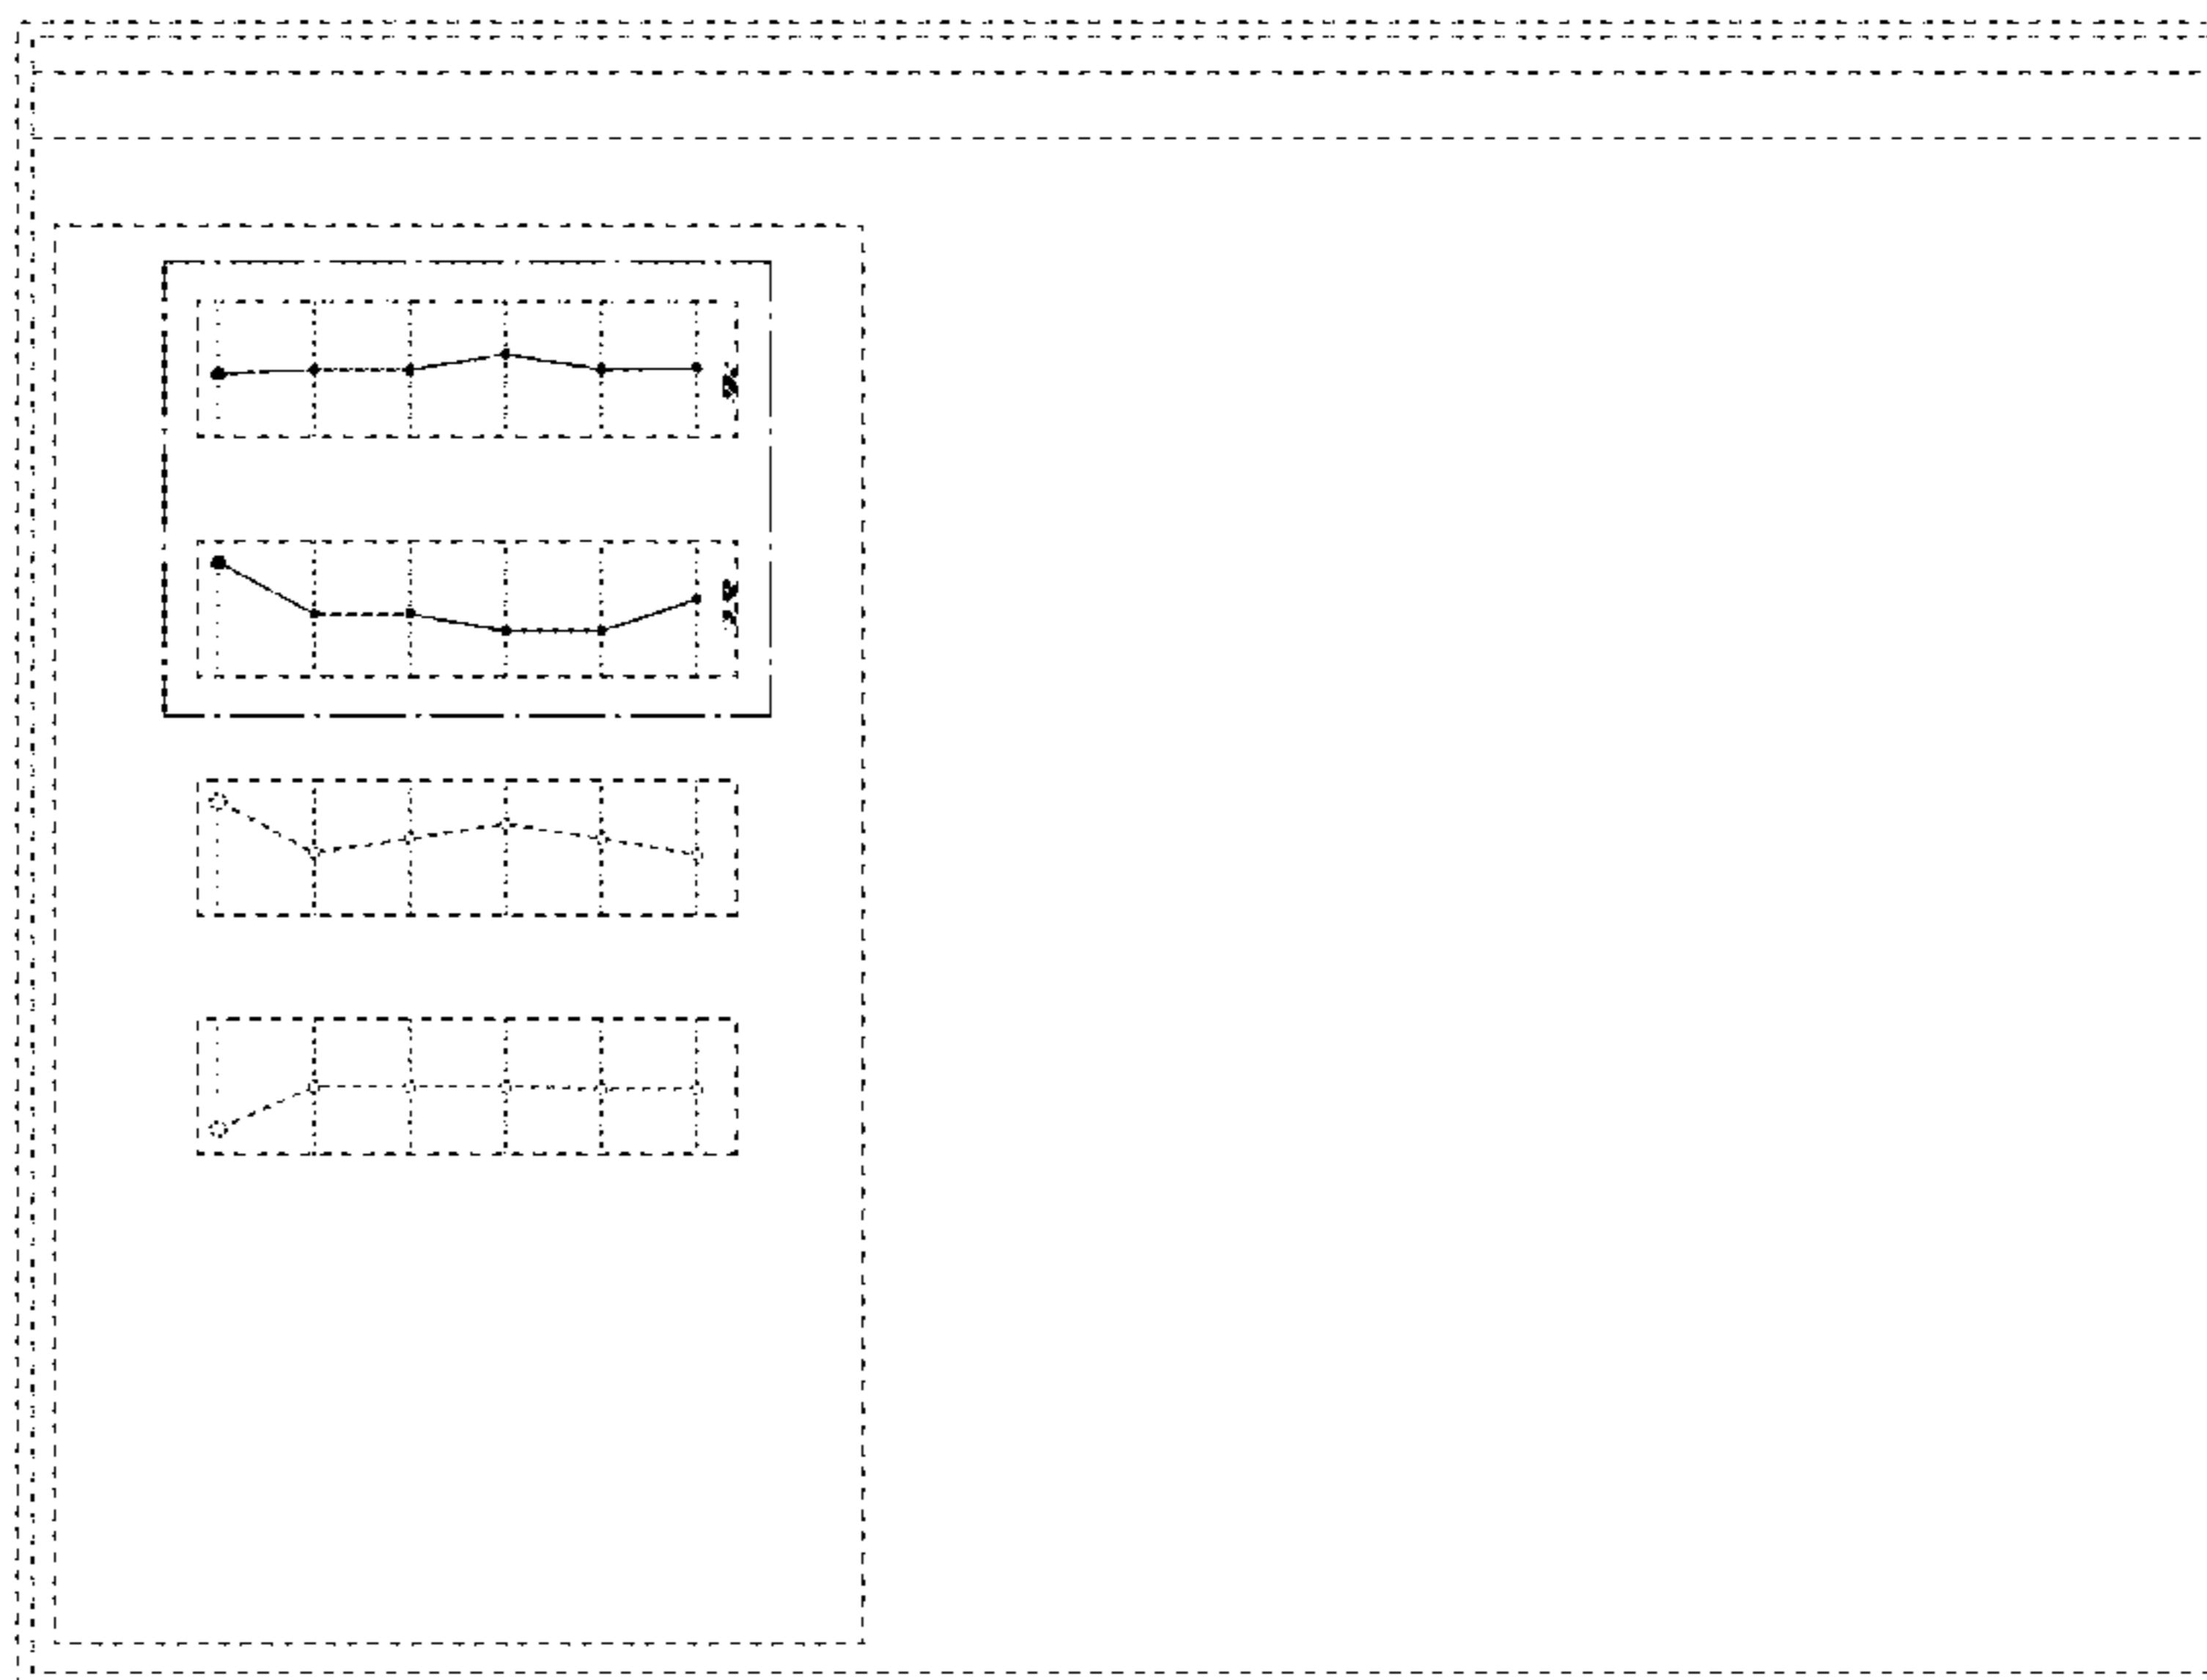

(56)

References Cited

U.S. PATENT DOCUMENTS

D768,142 S * 10/2016 Lee D14/485
D786,268 S * 5/2017 Blanchard D14/485
D788,786 S * 6/2017 Eddins D14/485
D802,608 S * 11/2017 Hicks D14/486
D829,752 S * 10/2018 Chauhan D14/486
10,636,523 B2 * 4/2020 Stocker G16H 40/63
2015/0213211 A1 * 7/2015 Zaleski G06F 16/9535
715/753
2019/0348170 A1 * 11/2019 Ishikawa G06F 9/3004
2019/0362809 A1 * 11/2019 Okimoto G06K 9/00127
2019/0365350 A1 * 12/2019 Chiang A61B 8/4427
2020/0105222 A1 * 4/2020 Ishikawa G09G 3/2003

OTHER PUBLICATIONS

“Advanced Reporting Guide” Apr. 2017, Microstrategy, site visited Aug. 10, 2020: <https://doc-archives.microstrategy.com/producthelp/10.7/manuals/en/AdvancedReporting.pdf> (Year: 2017).*

Sarwar, Ahmed et al. “Biomechanical Measurement Error Can Be Caused by Fujifilm Thickness: A Theoretical, Experimental, and Computational Analysis” Aug. 16, 2017, Hindawi, site visited Aug. 10, 2020: <http://downloads.hindawi.com/journals/bmri/2017/4310314.pdf> (Year: 2017).*

* cited by examiner

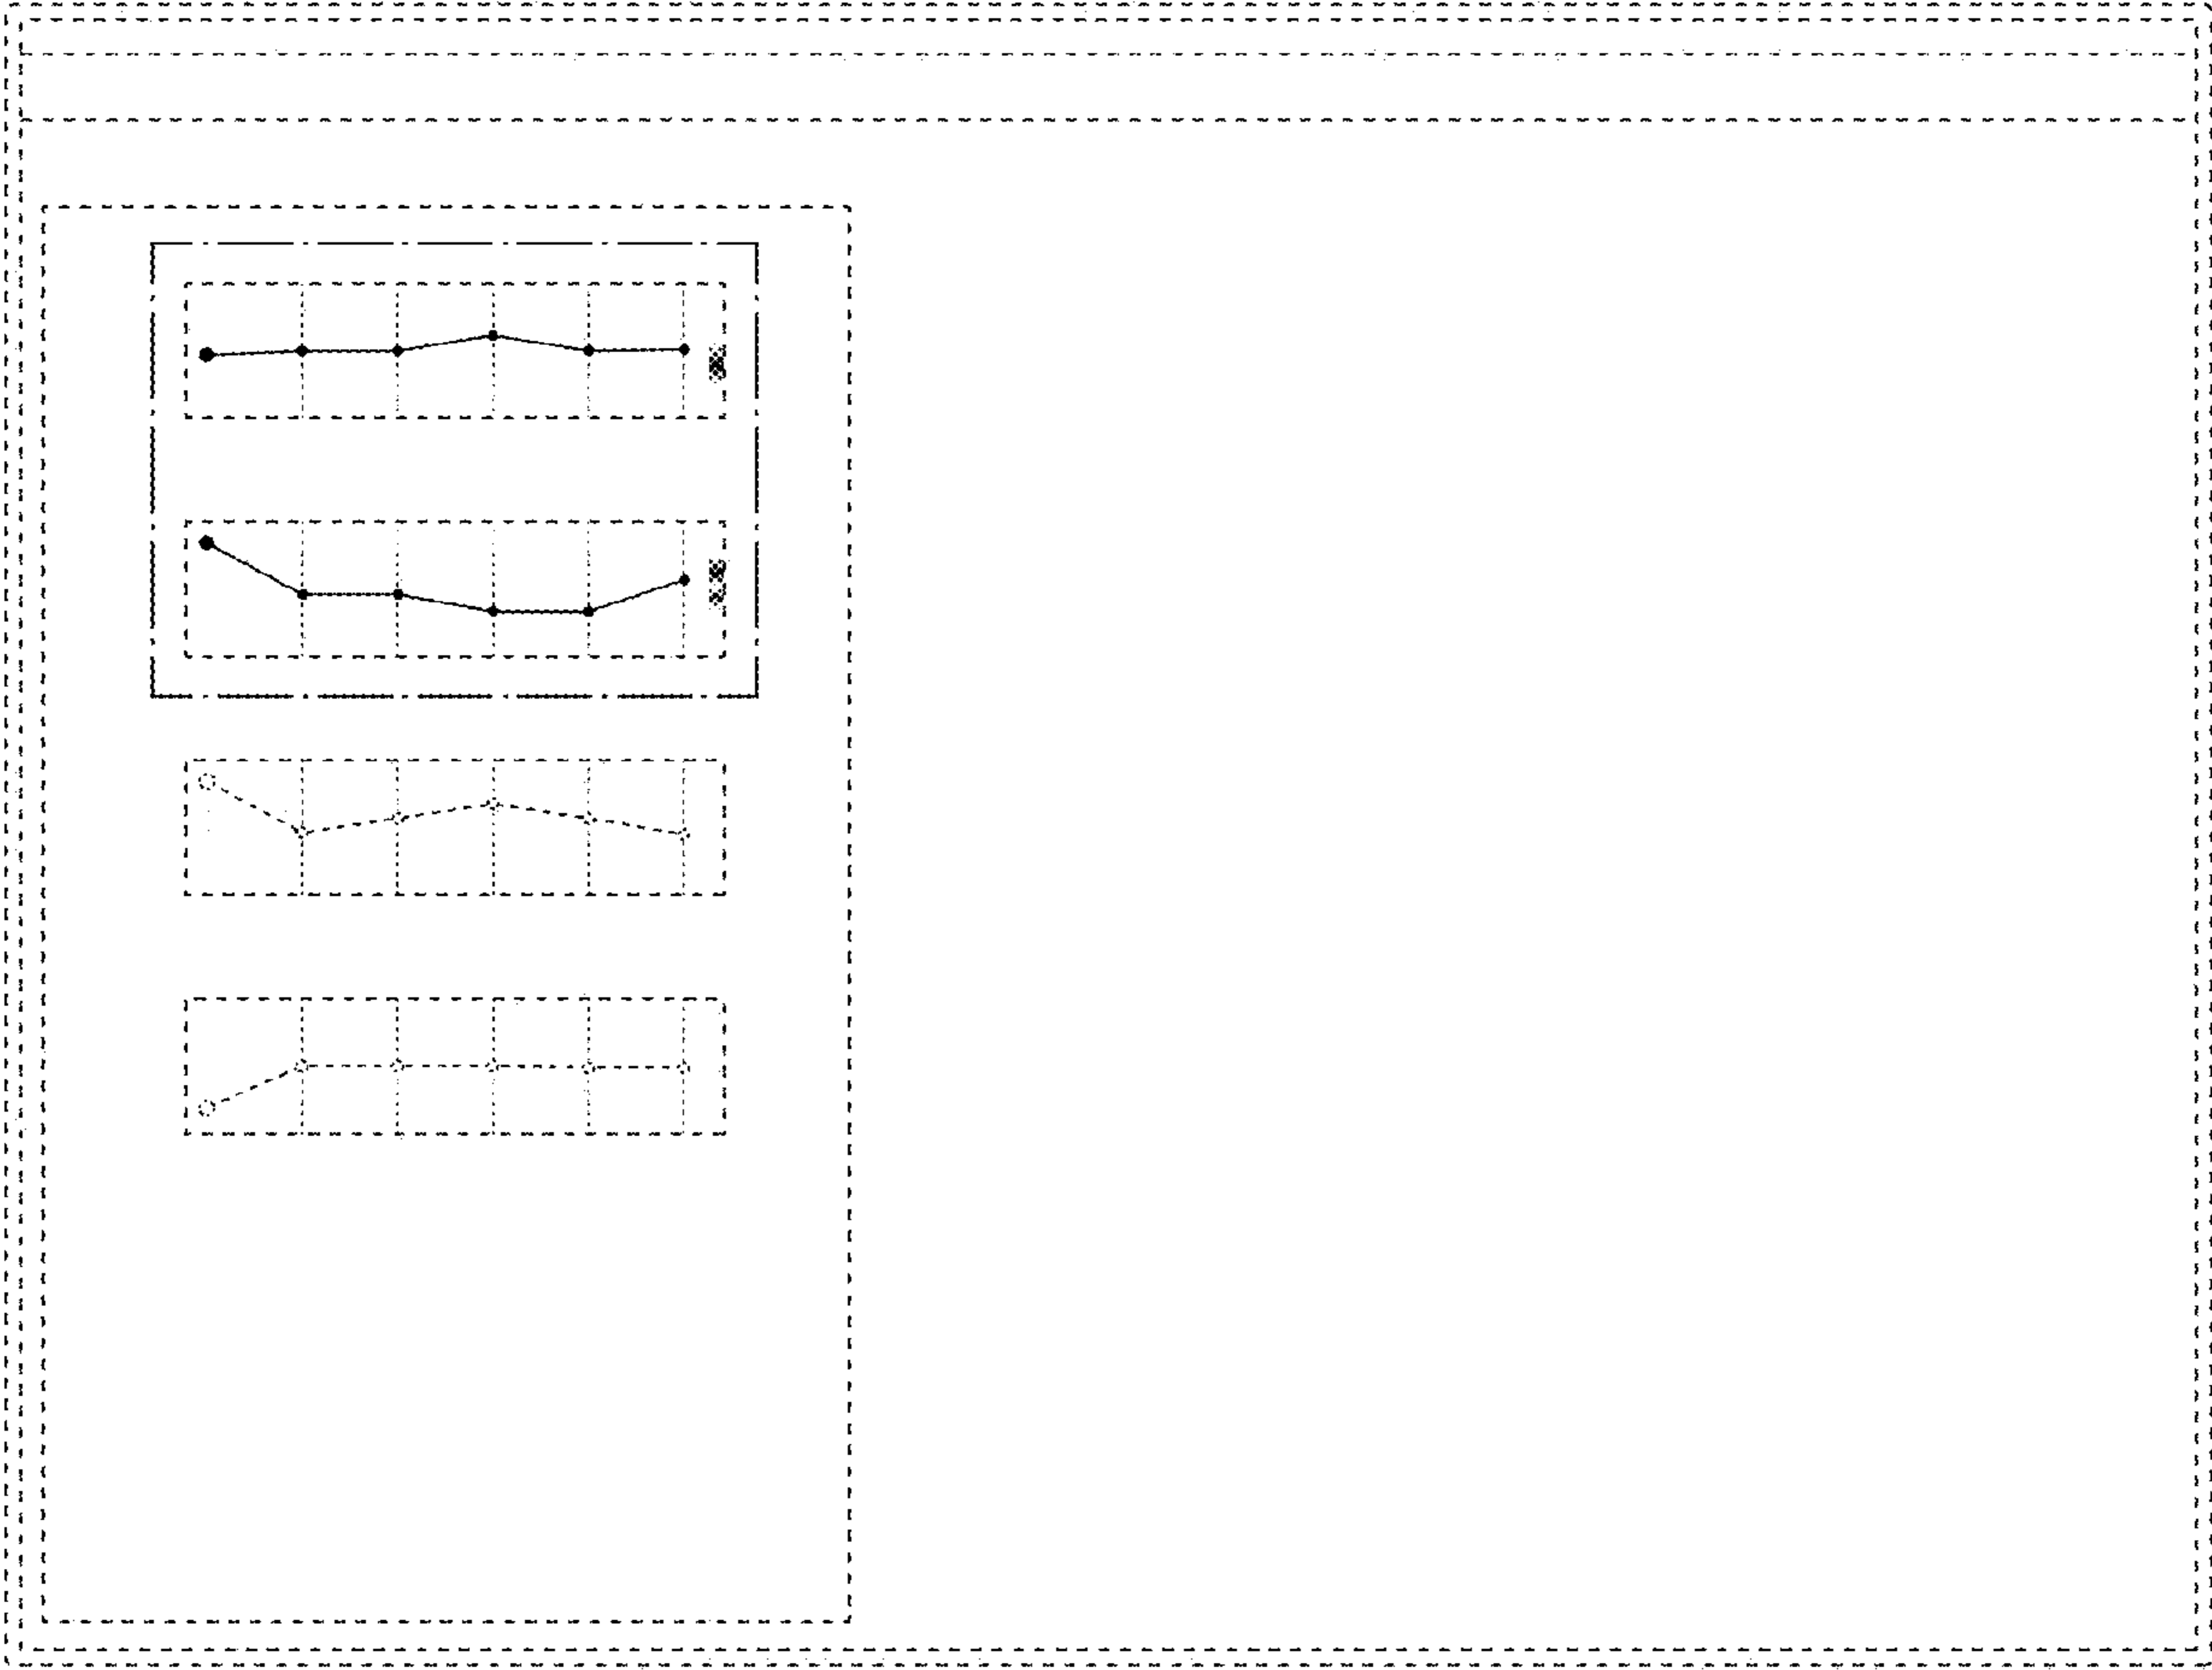


FIG.1



FIG.2

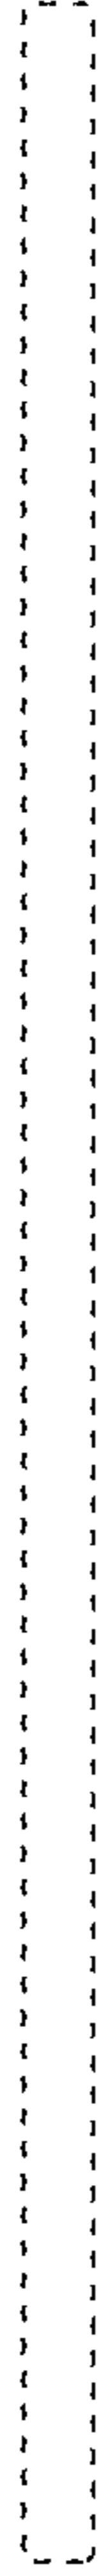


FIG.3

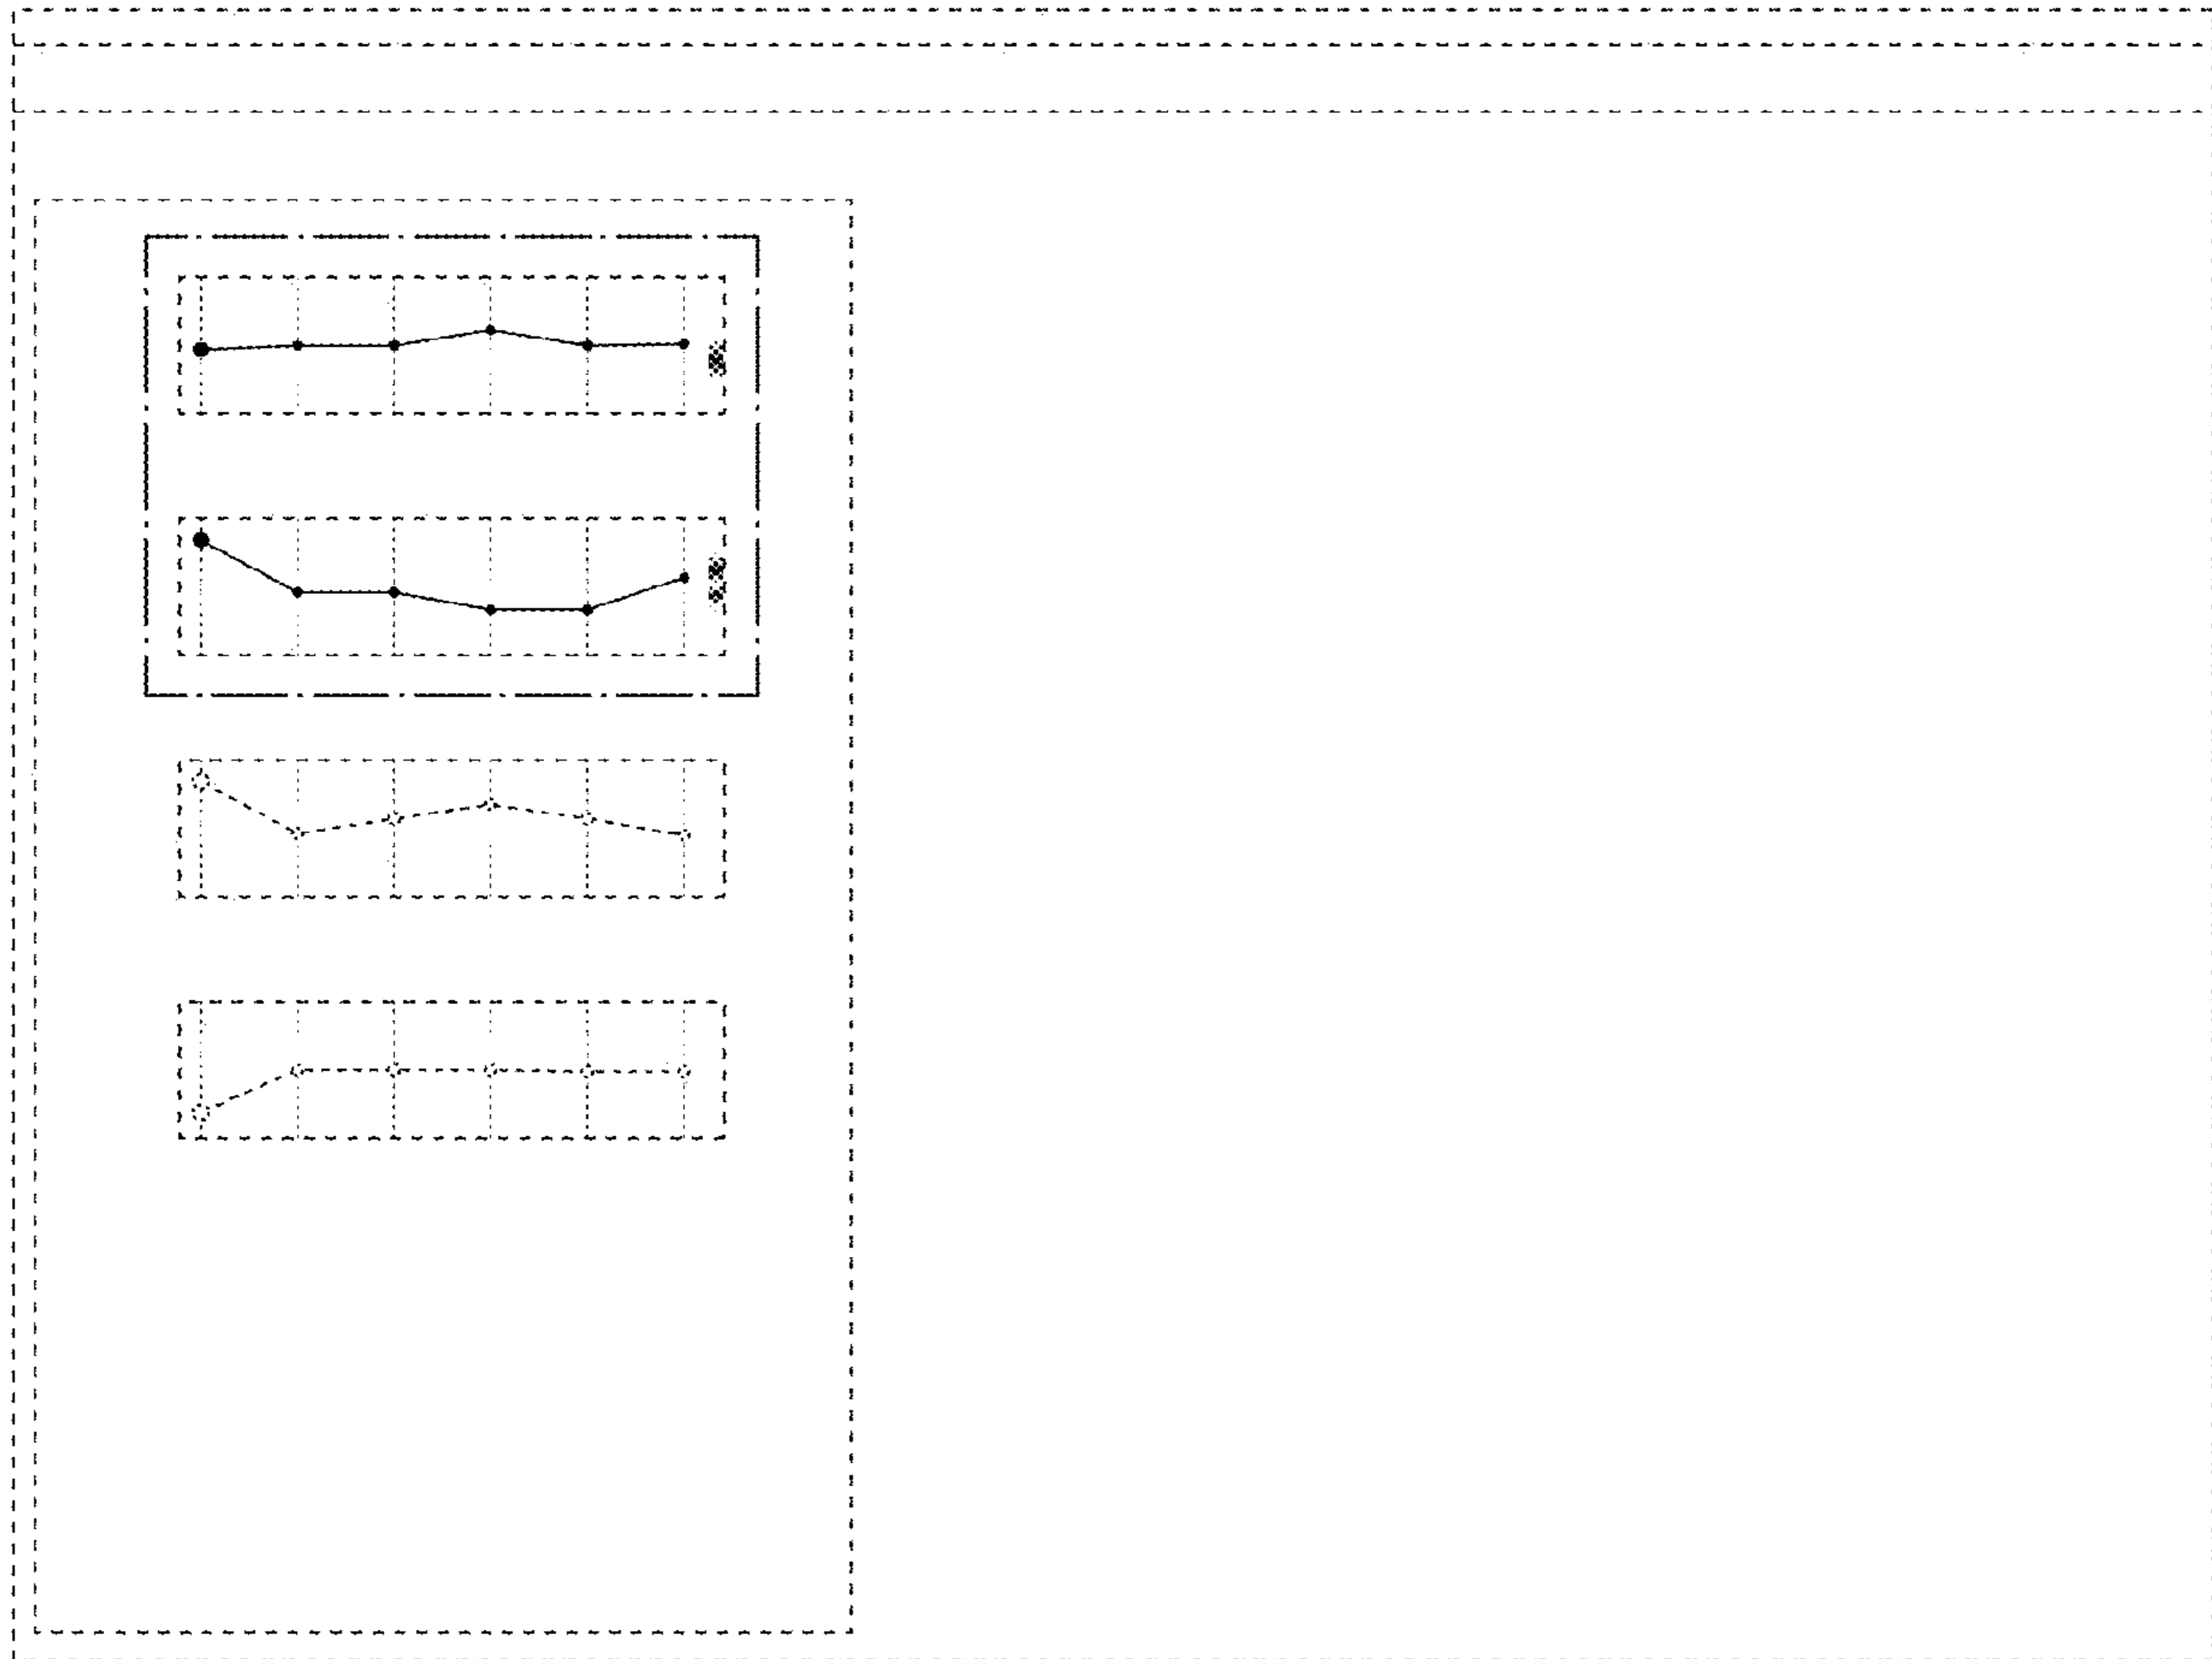


FIG.4

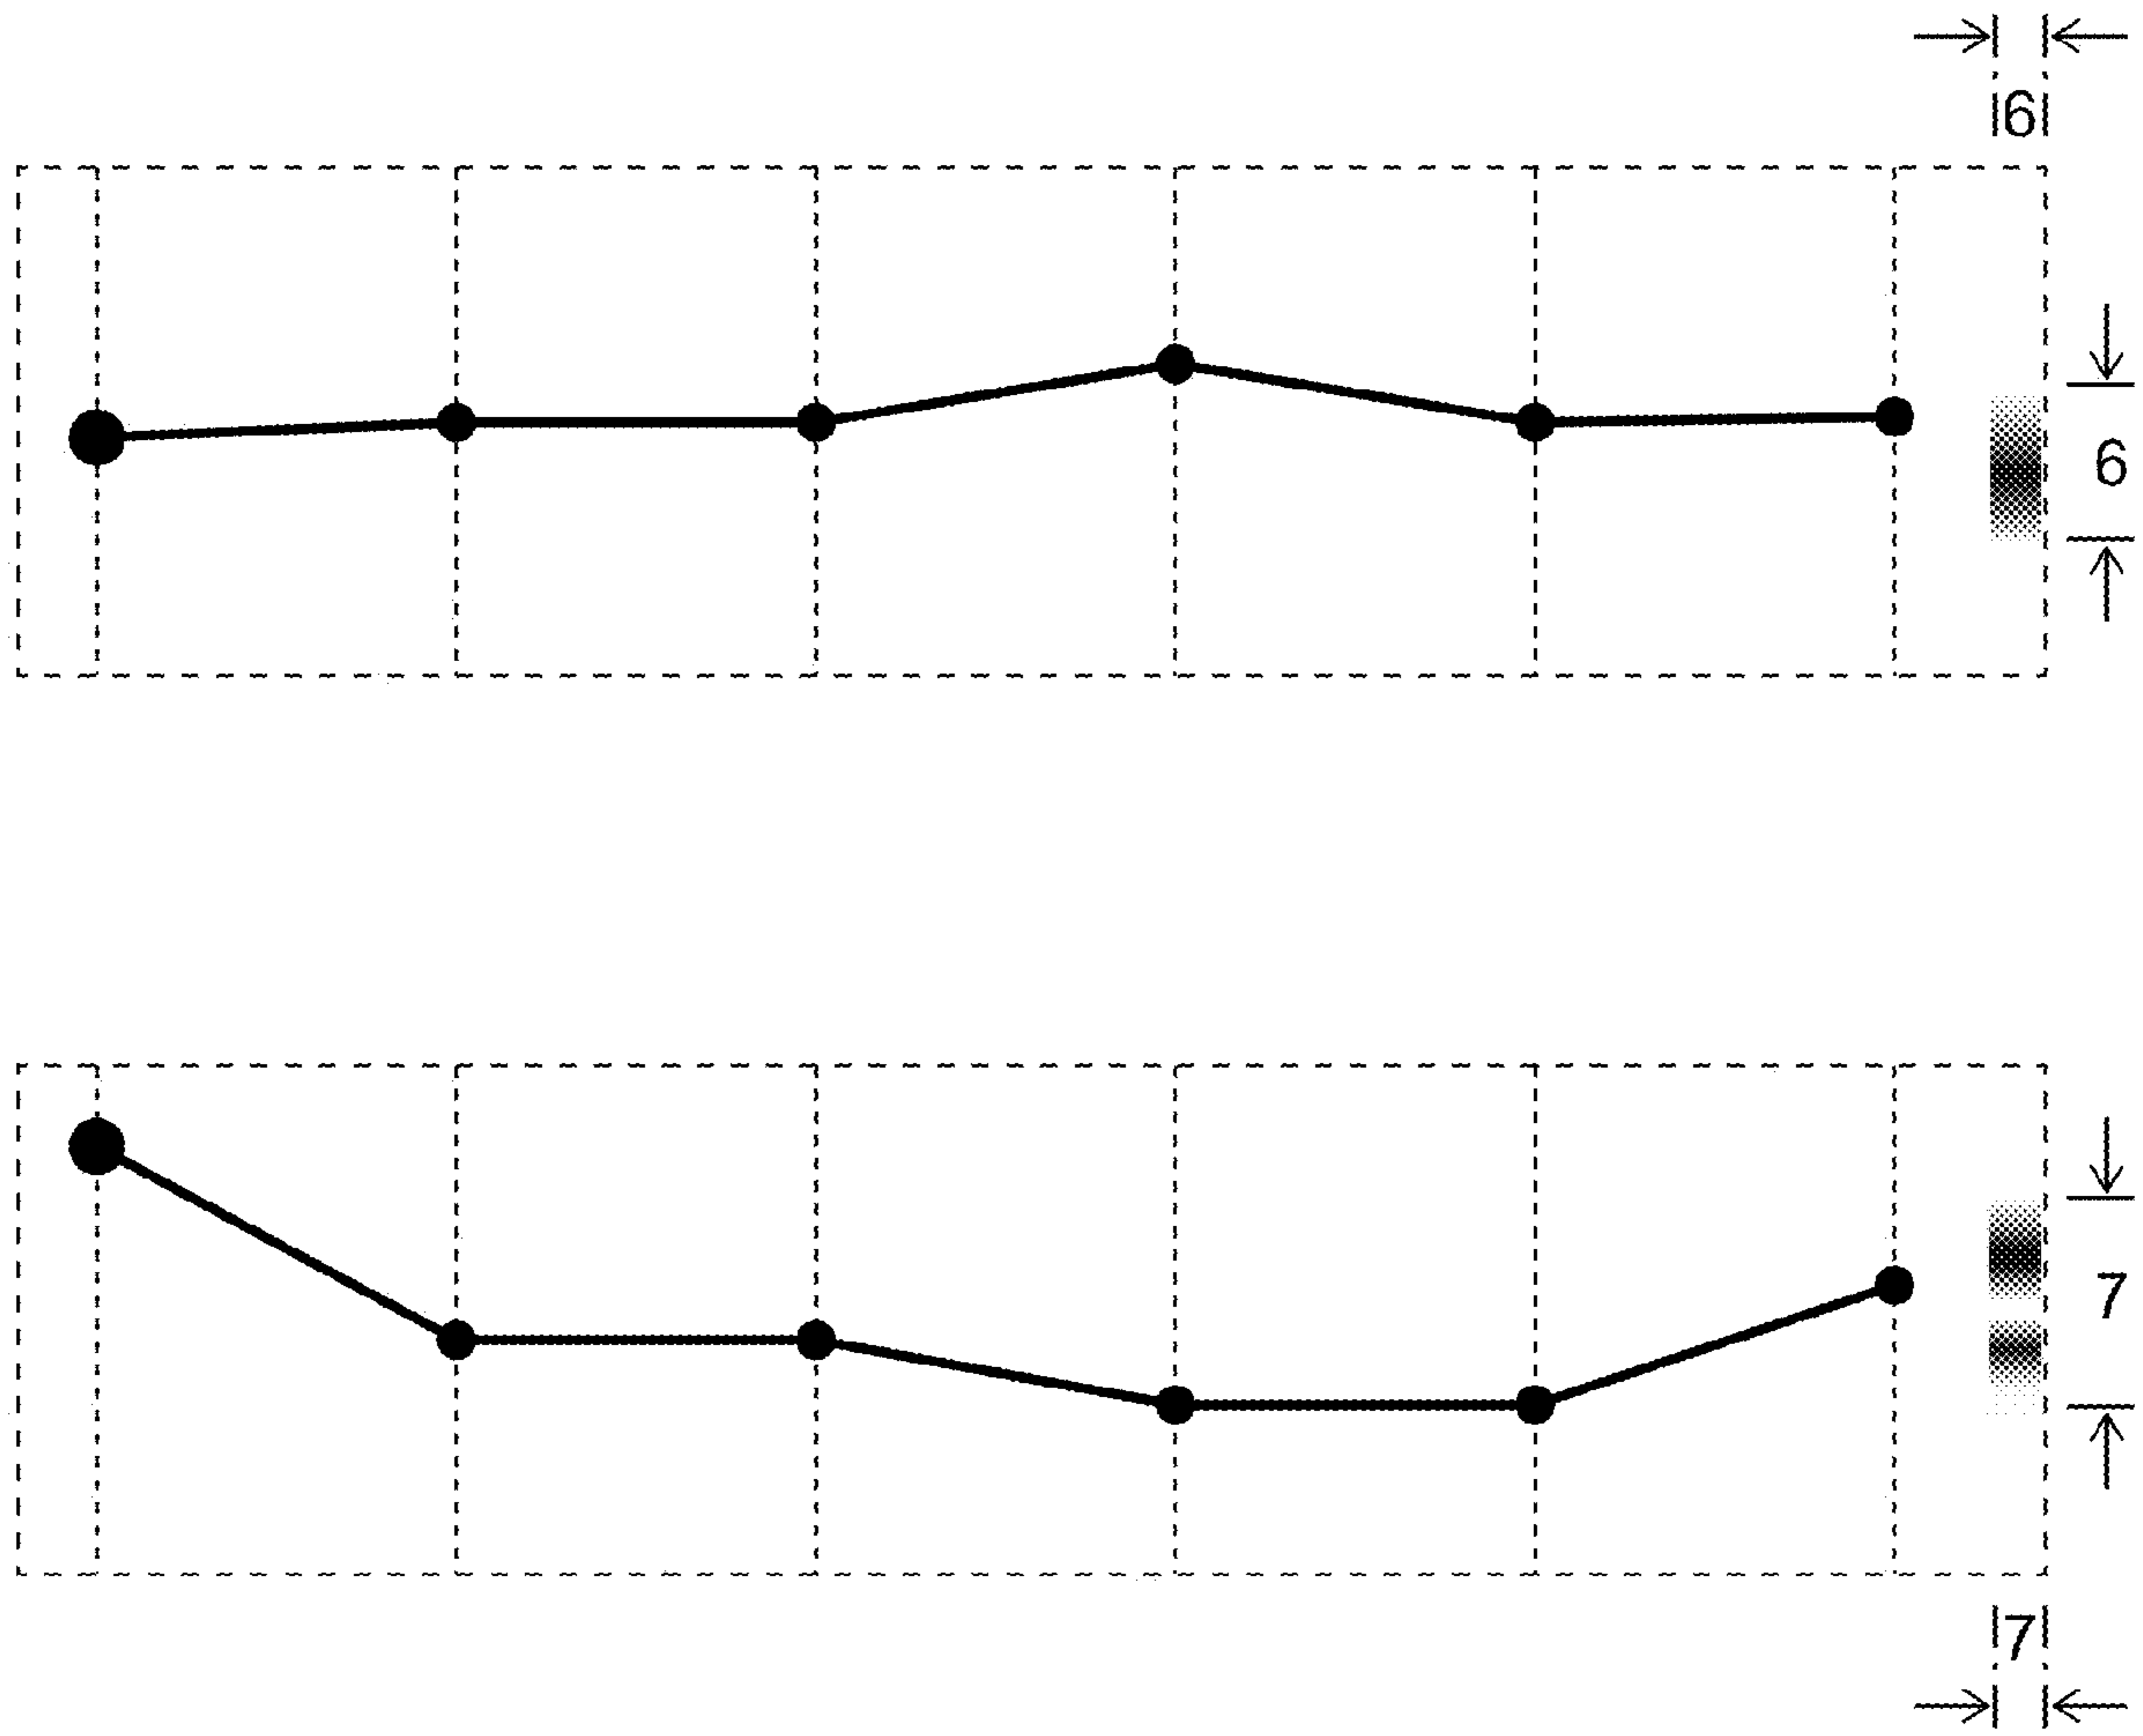


FIG.5

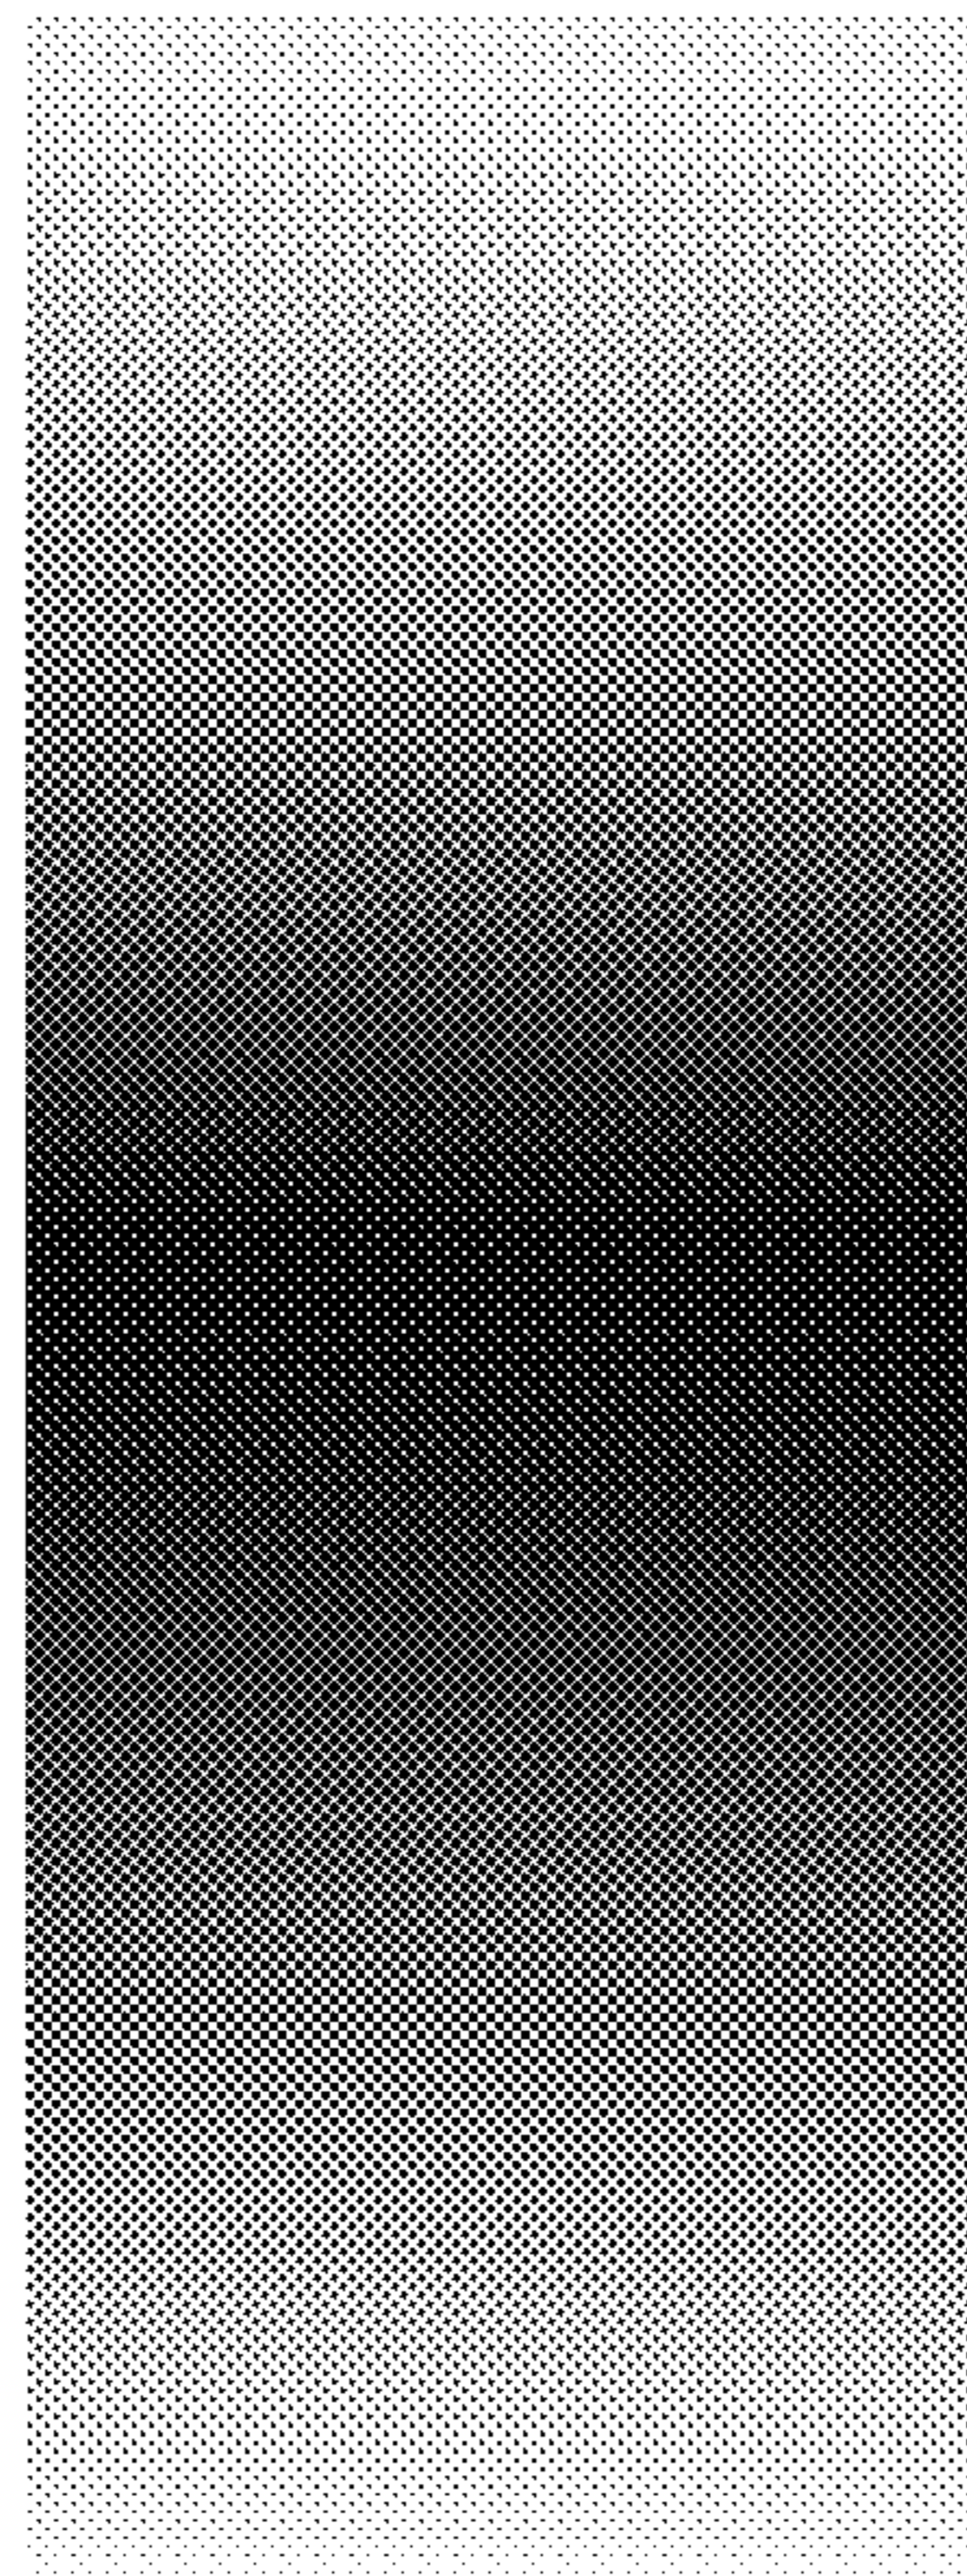


FIG.6

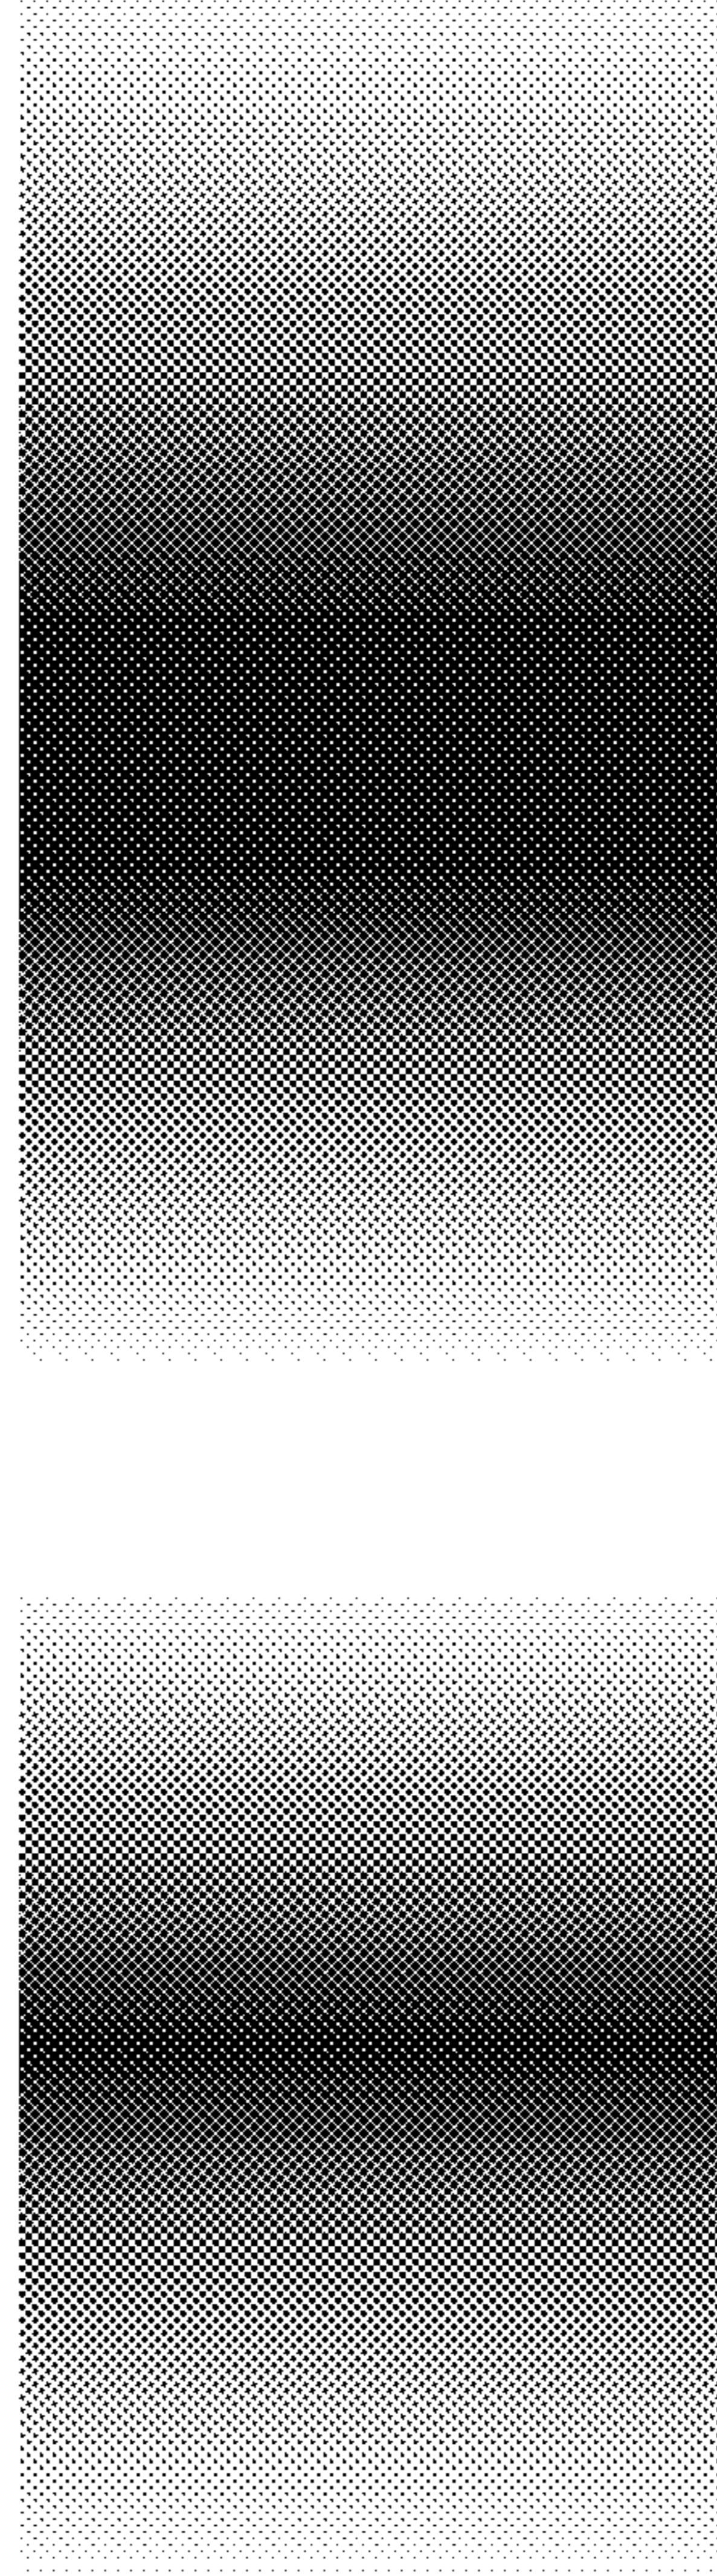


FIG.7