



US00D913301S

(12) **United States Design Patent** (10) **Patent No.:** **US D913,301 S**
Liu (45) **Date of Patent:** **** Mar. 16, 2021**

(54) **DISPLAY SCREEN WITH A GRAPHICAL USER INTERFACE**

(71) Applicant: **TEVA BRANDED PHARMACEUTICAL PRODUCTS R&D, INC.**, Frazer, PA (US)

(72) Inventor: **Xinyu Liu**, Newton, MA (US)

(73) Assignee: **Teva Branded Pharmaceutical Products R&D, Inc.**, Frazer, PA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/681,250**

(22) Filed: **Feb. 22, 2019**

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485–495
CPC G06F 3/048; G06F 3/0481; G06F 3/04812; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/0484; G06F 3/04847; G06F 3/0485; G06F 3/04855; G06F 3/04886; G06Q 30/00; H03J 1/00; H03J 1/0008; H03J 1/0016; H03J 1/0025; H04N 5/00; H04N 5/08; H04N 5/14; H04N 5/222; H04N 5/225; H04N 5/232; H04N 5/445; H04N 5/44543; H04N 5/45; H04N 2005/44517; H04N 2005/44521; H04N 2005/44526; H04N 2005/4453; H04N 2005/44534; H04N 2005/44539; H04N 2005/44547; H04N 2005/44556; H04N 2005/4456; H04N 2005/44565; H04N 2005/44569; H04N 2005/44573; H04N 21/00; H04N 21/234; H04N 21/431; H04N 21/4312; H04N 21/4314; H04N 21/4316

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D640,274 S * 6/2011 Arnold D14/487
D756,398 S * 5/2016 Ng D14/487
(Continued)

OTHER PUBLICATIONS

Tenenbaum, David. “Marrying an asthma inhaler to a wireless monitor and a smartphone app.” medicalxpress.com. Apr. 20, 2017. Accessed Jun. 1, 2020. Available online at URL: <https://medicalxpress.com/news/2017-04-asthma-inhaler-wireless-smartphone-app.html> (Year: 2017).*

(Continued)

Primary Examiner — Christian P. McLean
(74) *Attorney, Agent, or Firm* — Flaster Greenberg, P.C.


(57) **CLAIM**

The ornamental design for a display screen with a graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a display screen with a graphical user interface, showing the new design in a first embodiment;
FIG. 2 is a front view of a second image thereof;
FIG. 3 is a front view of a third image thereof;
FIG. 4 is a front view of a fourth image thereof;
FIG. 5 is a front view of a fifth image thereof; and
FIG. 6 is a front view of a sixth image thereof.
The appearance of the animated images sequentially transition between the images shown in FIGS. 1 through 6. The process or period in which one image transitions into another forms no part of the claimed design.
The outermost broken lines illustrated a mobile device, which is the environment of the design and forms no part of

(Continued)

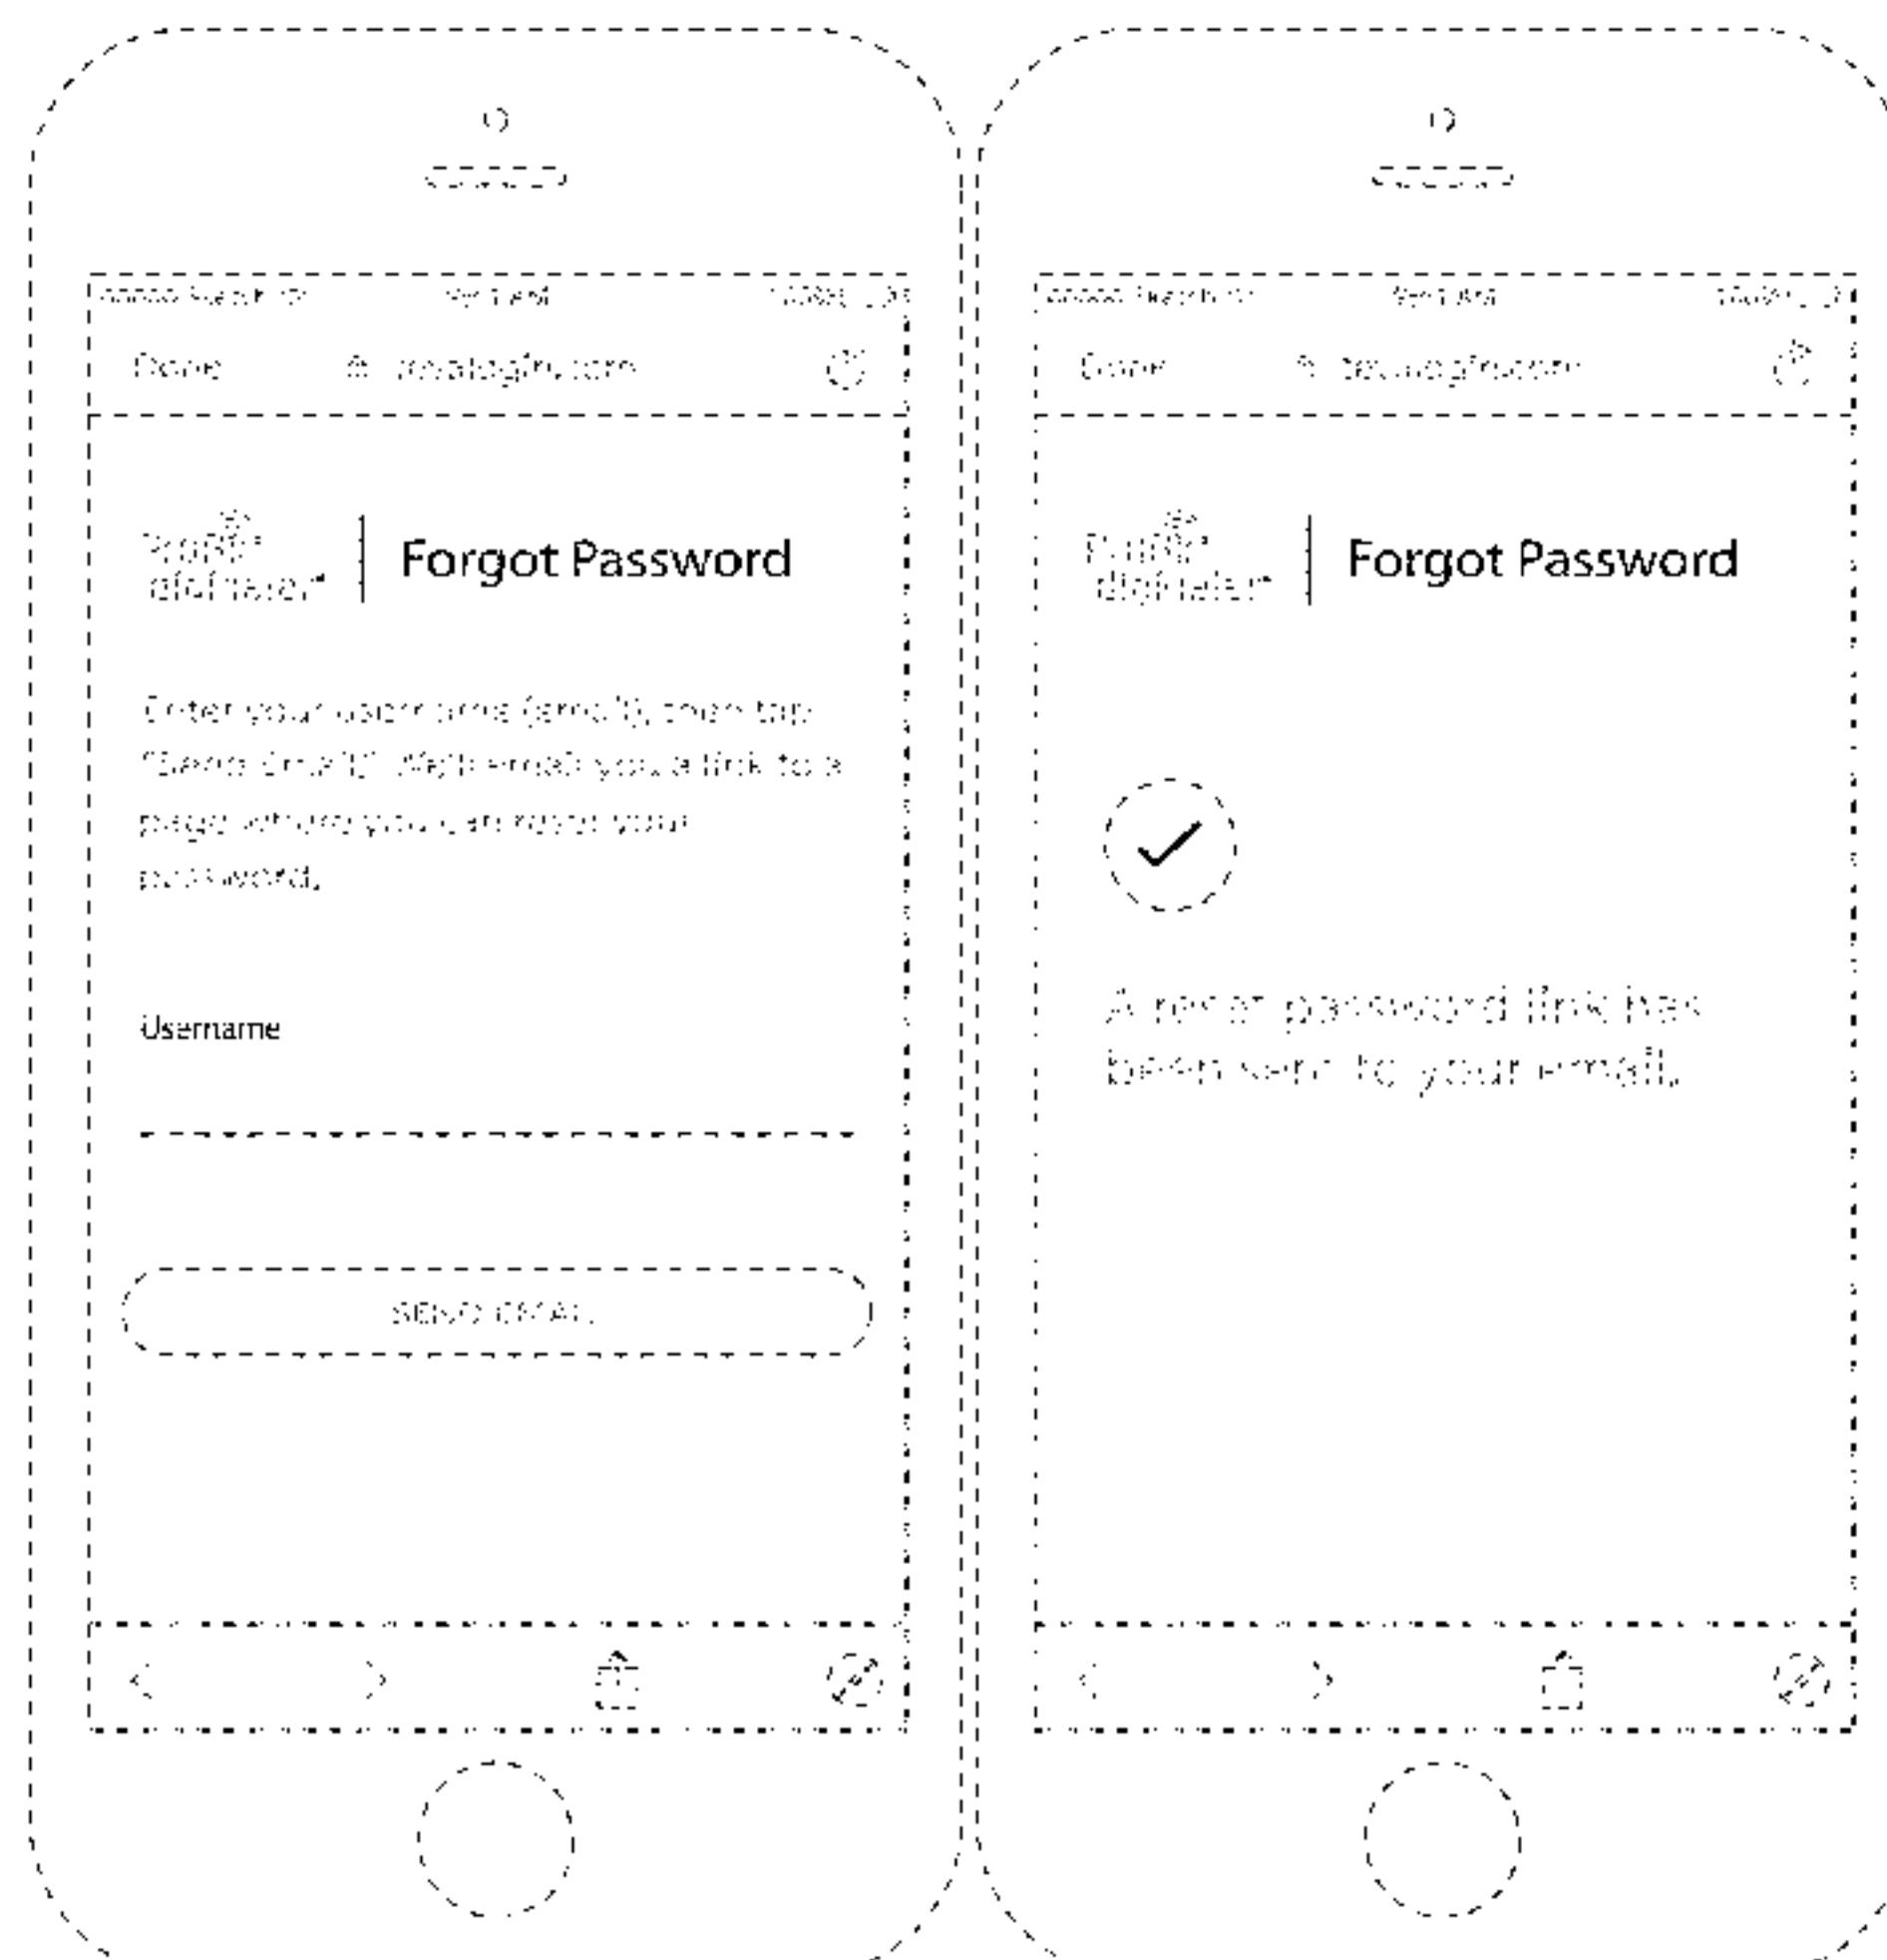

the claim. The remaining broken lines illustrate a display screen and portions of the graphical user interface that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

(56)

References Cited

U.S. PATENT DOCUMENTS

D771,654	S	*	11/2016	Chaudhri	D14/485
D772,249	S	*	11/2016	Choi	D14/485
D772,261	S	*	11/2016	Kothe	D14/486
D778,944	S	*	2/2017	Kim	D14/488
D789,956	S	*	6/2017	Ortega	D14/486
D803,257	S	*	11/2017	Graham	D14/487
D803,258	S	*	11/2017	Graham	D14/487
D810,772	S	*	2/2018	Wang	D14/486
D821,409	S	*	6/2018	Chang	D14/485
D845,988	S	*	4/2019	Alexander	D14/486
D858,563	S	*	9/2019	Xu	D14/488
D863,329	S	*	10/2019	Hu	D14/486
D868,813	S	*	12/2019	Oles	D14/486
D872,128	S	*	1/2020	Apodaca	D14/489
D878,402	S	*	3/2020	Turner	D14/486
D881,231	S	*	4/2020	Hansen	D14/486
D888,738	S	*	6/2020	Chang	D14/486
D889,477	S	*	7/2020	Tsurkan	D14/485
D893,530	S	*	8/2020	Zhang	D14/486
D894,951	S	*	9/2020	Krishna	D14/488

10,805,177	B2	*	10/2020	Kanojia	H04L 41/06
2013/0275899	A1	*	10/2013	Schubert	G06F 3/0481 715/765
2015/0348001	A1	*	12/2015	Van Os	G06Q 20/32 705/44
2016/0132234	A1	*	5/2016	Riscutia	G06F 3/017 715/773
2019/0121495	A1	*	4/2019	Latheef	G06F 9/453
2019/0318319	A1	*	10/2019	Blackburn	G06Q 10/1053
2020/0293189	A1	*	9/2020	Chaudhri	G06F 3/04842

OTHER PUBLICATIONS

“Teva’s ProAir Digihaler FDA Approved to Monitor Asthma and COPD Treatment.” medgadget.com. Dec. 26, 2018. Accessed Jun. 1, 2020. Available online at URL: <https://www.medgadget.com/2018/12/tevas-proair-digihaler-fda-approved-to-monitor-asthma-and-copd-treatment.html> (Year: 2018).*

Agrawal, Abhinav. “Android login Screen UI design.” behance.net. Published Jun. 28, 2016. Accessed Nov. 7, 2020. Available online at URL: <https://www.behance.net/gallery/40102375/Android-login-Screen-UI-design> (Year: 2016).*

Sipovich, Julia. “Login and Menu.” dribbble.com. Posted Aug. 11, 2015. Accessed Nov. 7, 2020. Available online at URL: <https://dribbble.com/shots/2189593-Login-and-Menu> (Year: 2015).*

Richman, James. “News App—App Login.” dribbble.com. Posted Oct. 12, 2015. Accessed Nov. 7, 2020. Available online at URL: <https://dribbble.com/shots/2288072-News-App-App-Login> (Year: 2015).*

* cited by examiner

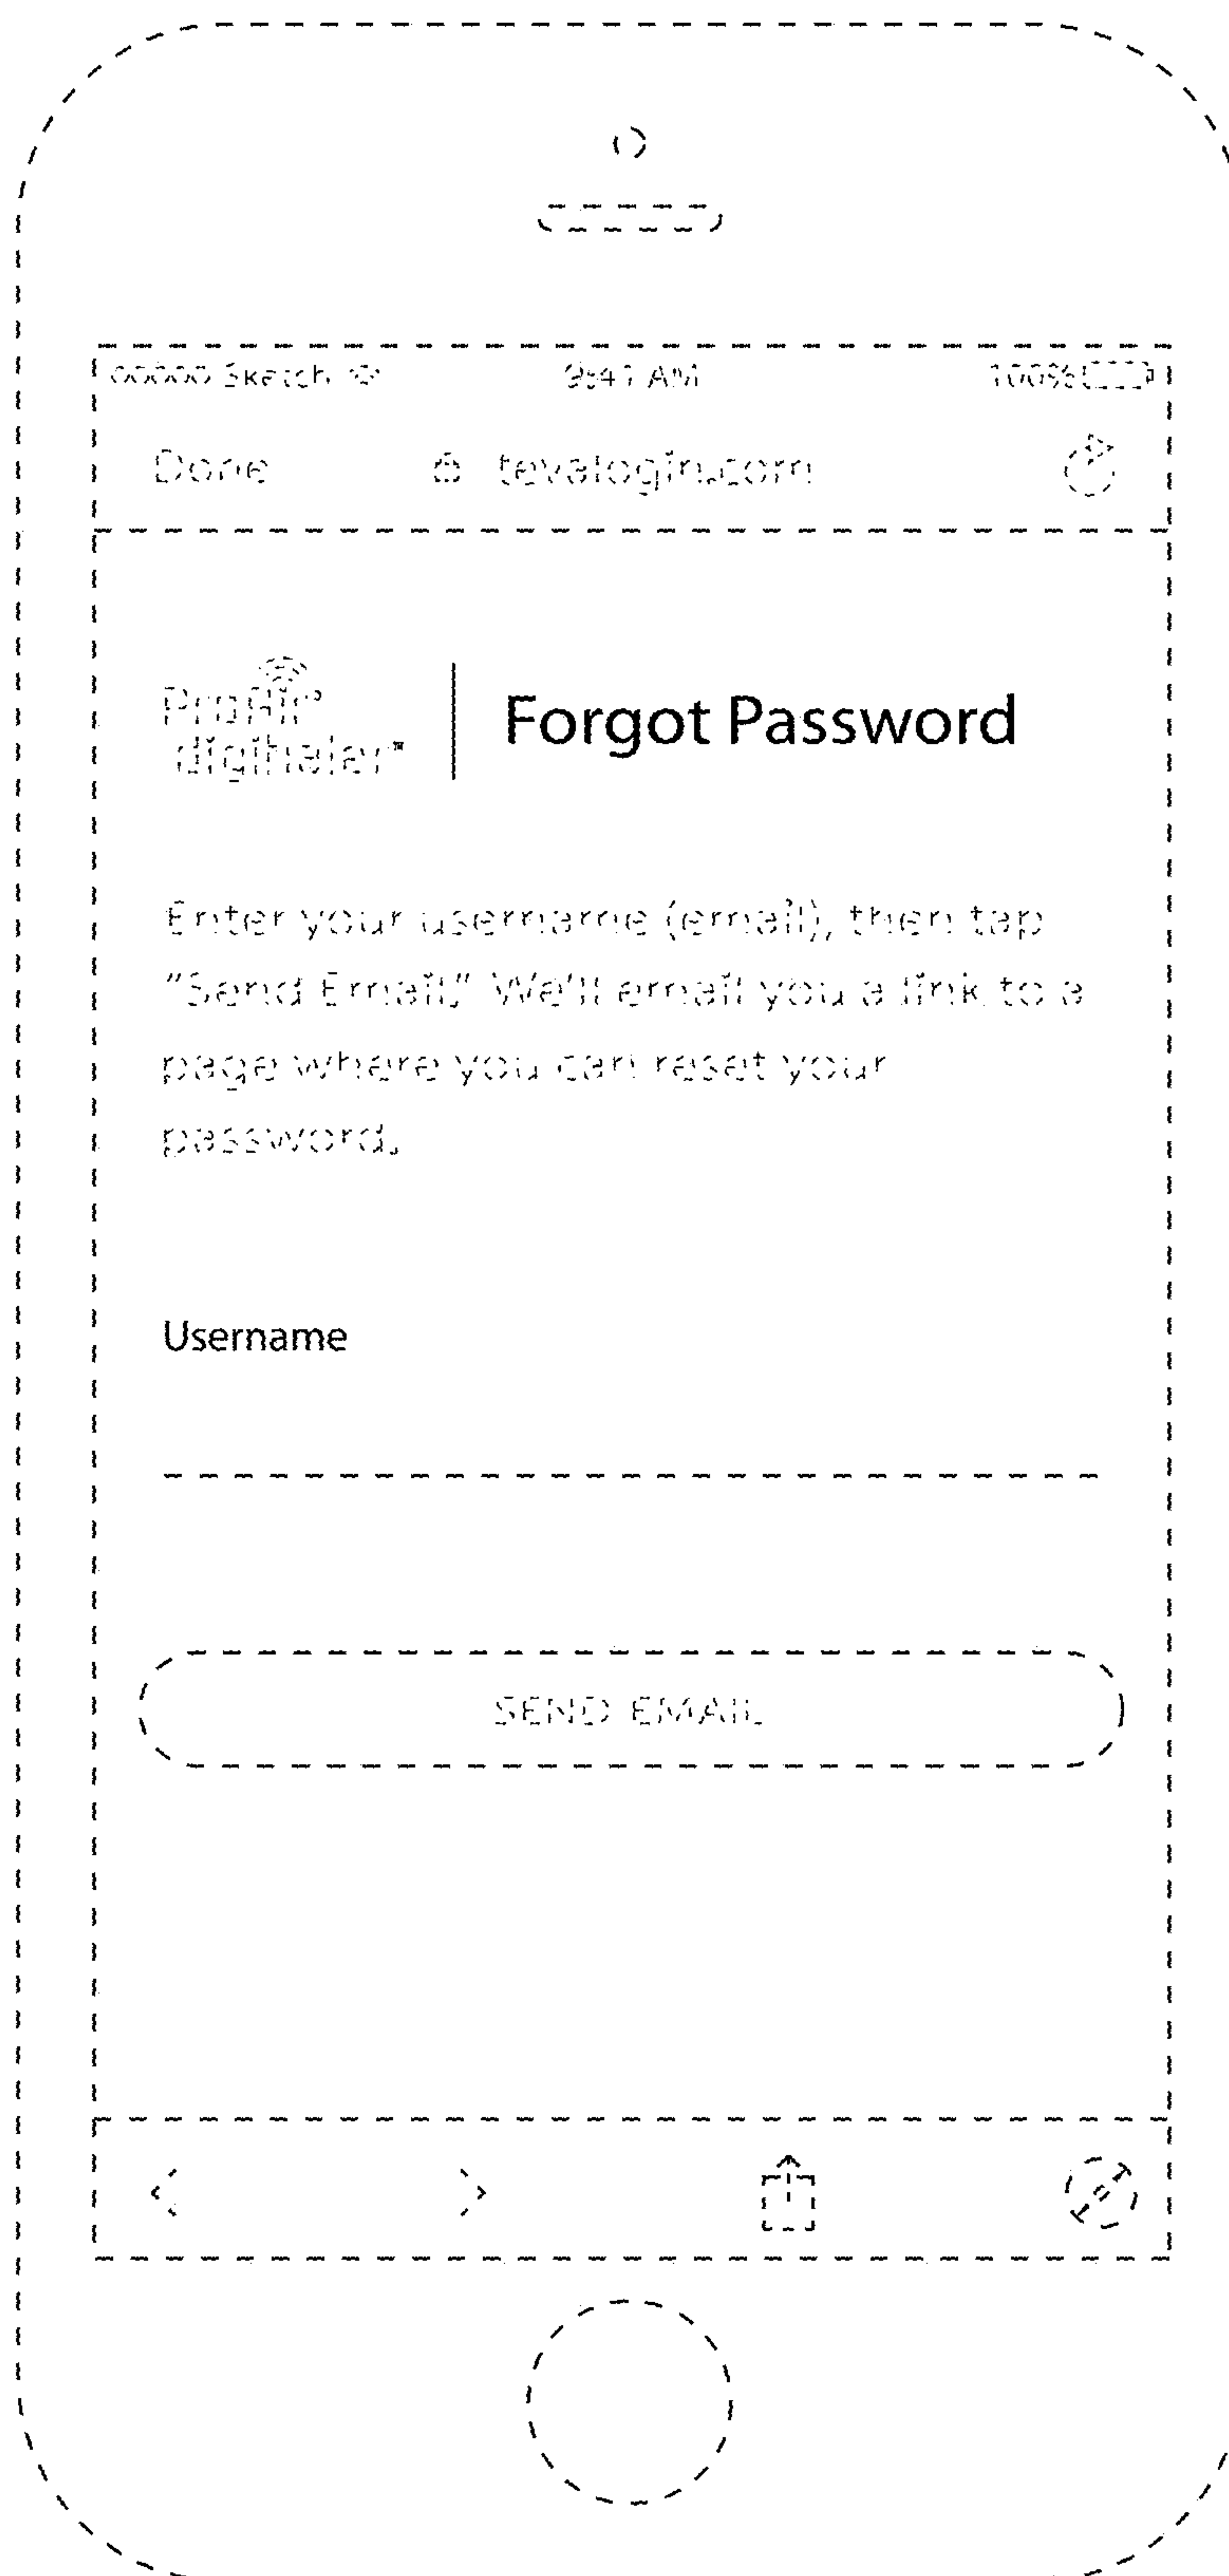


FIG. 1

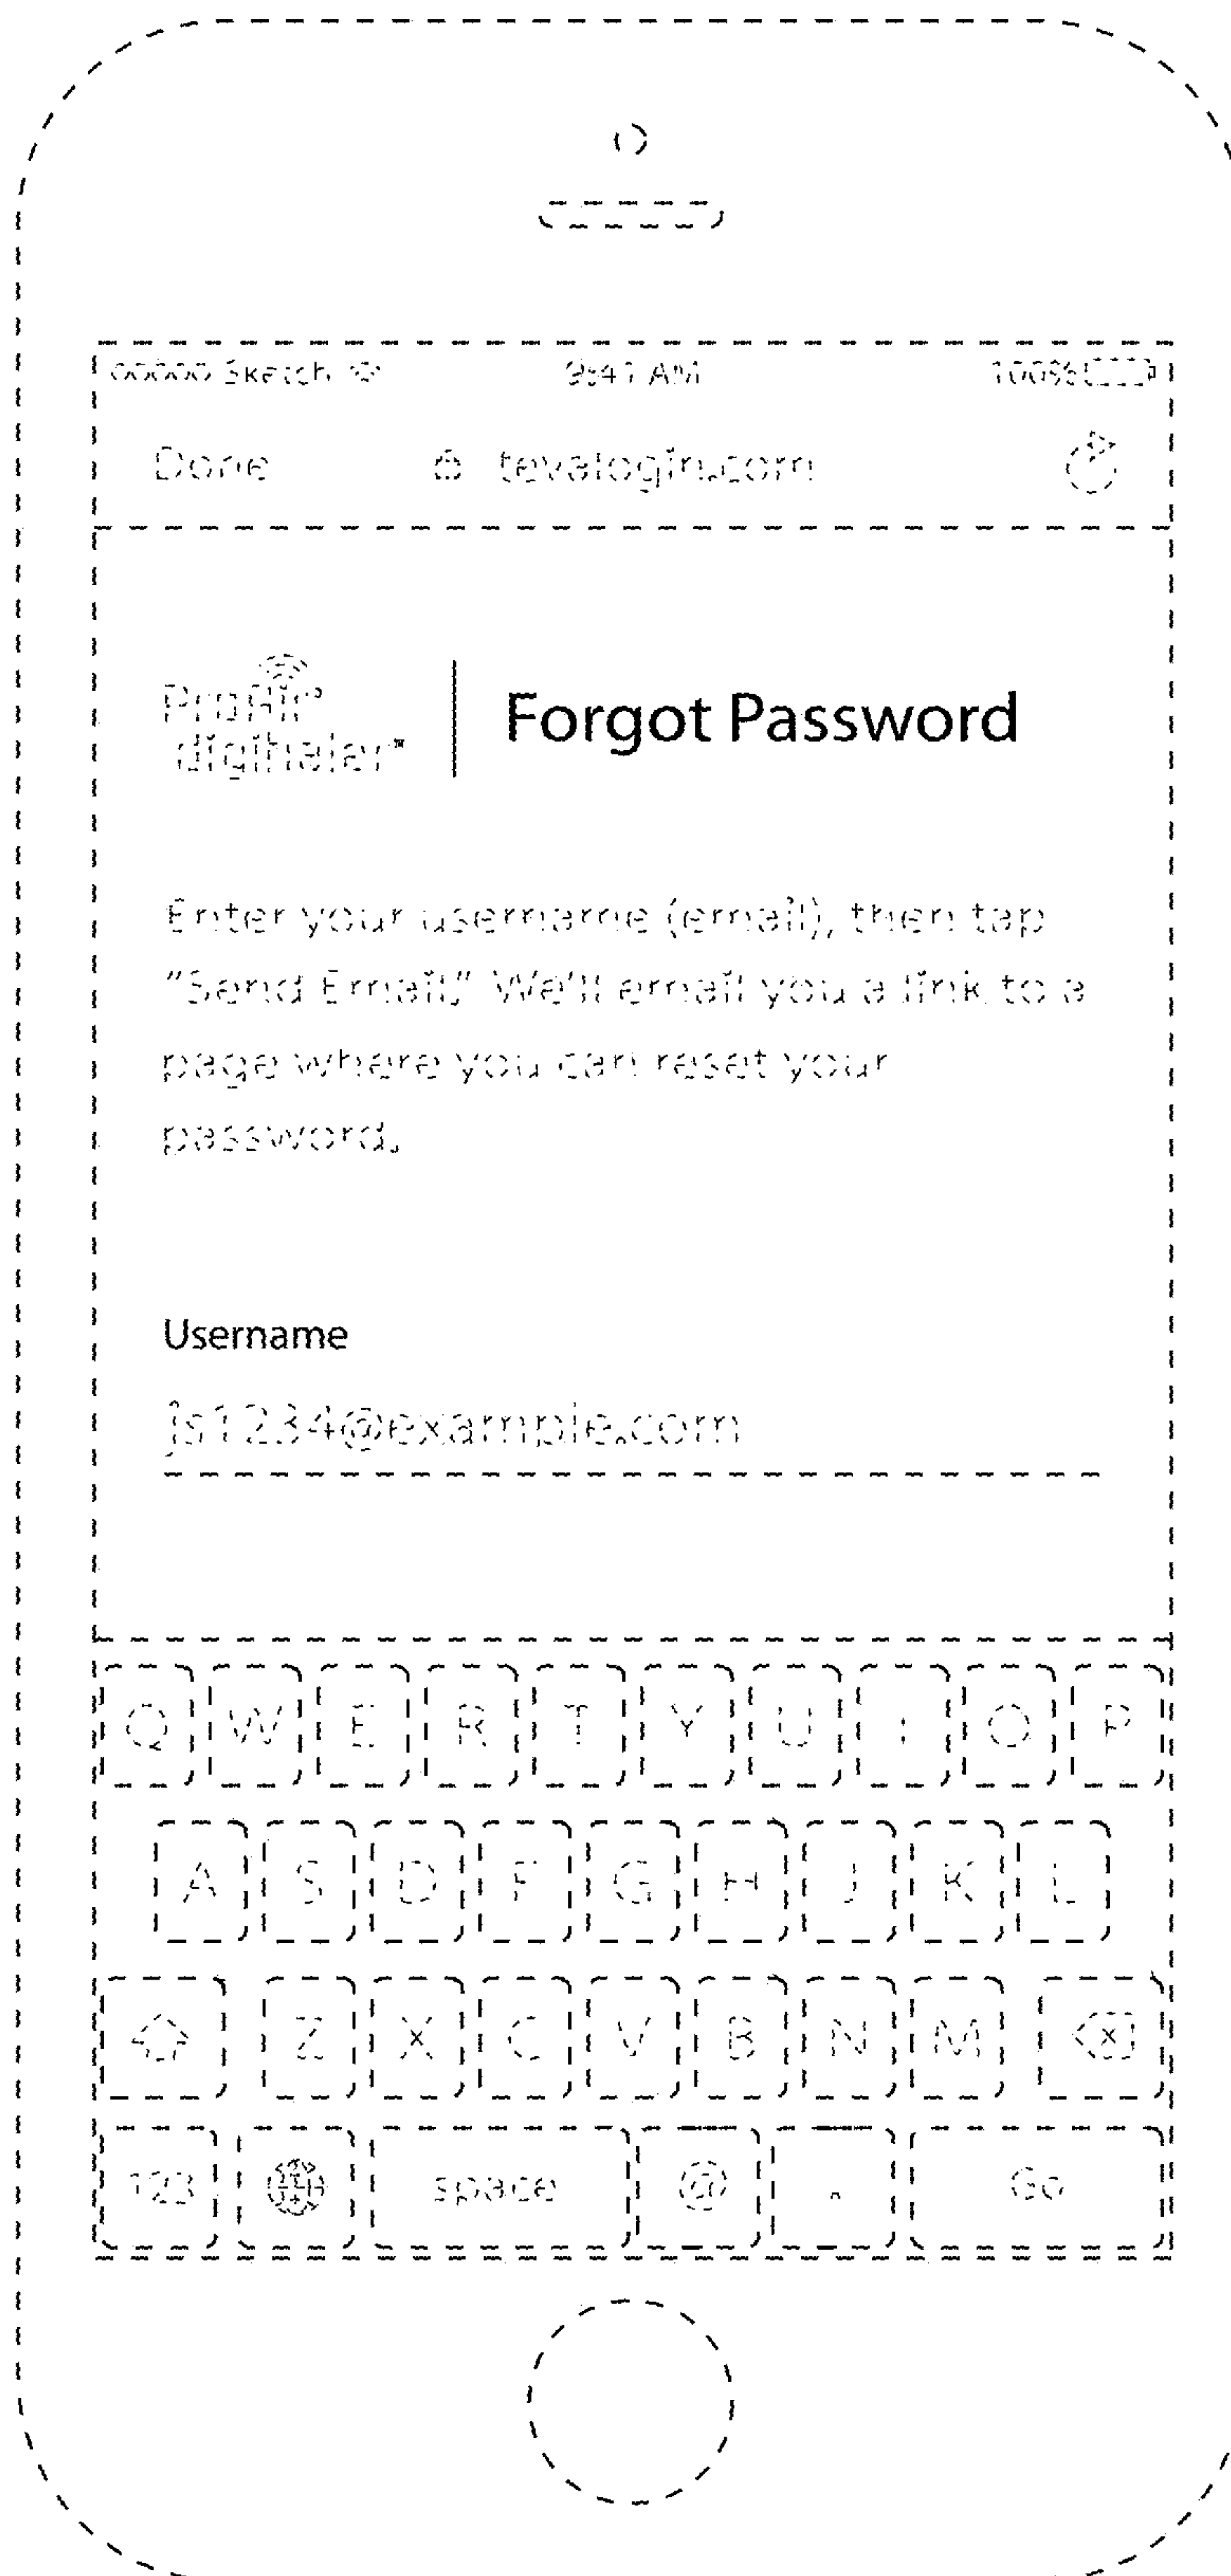


FIG. 2

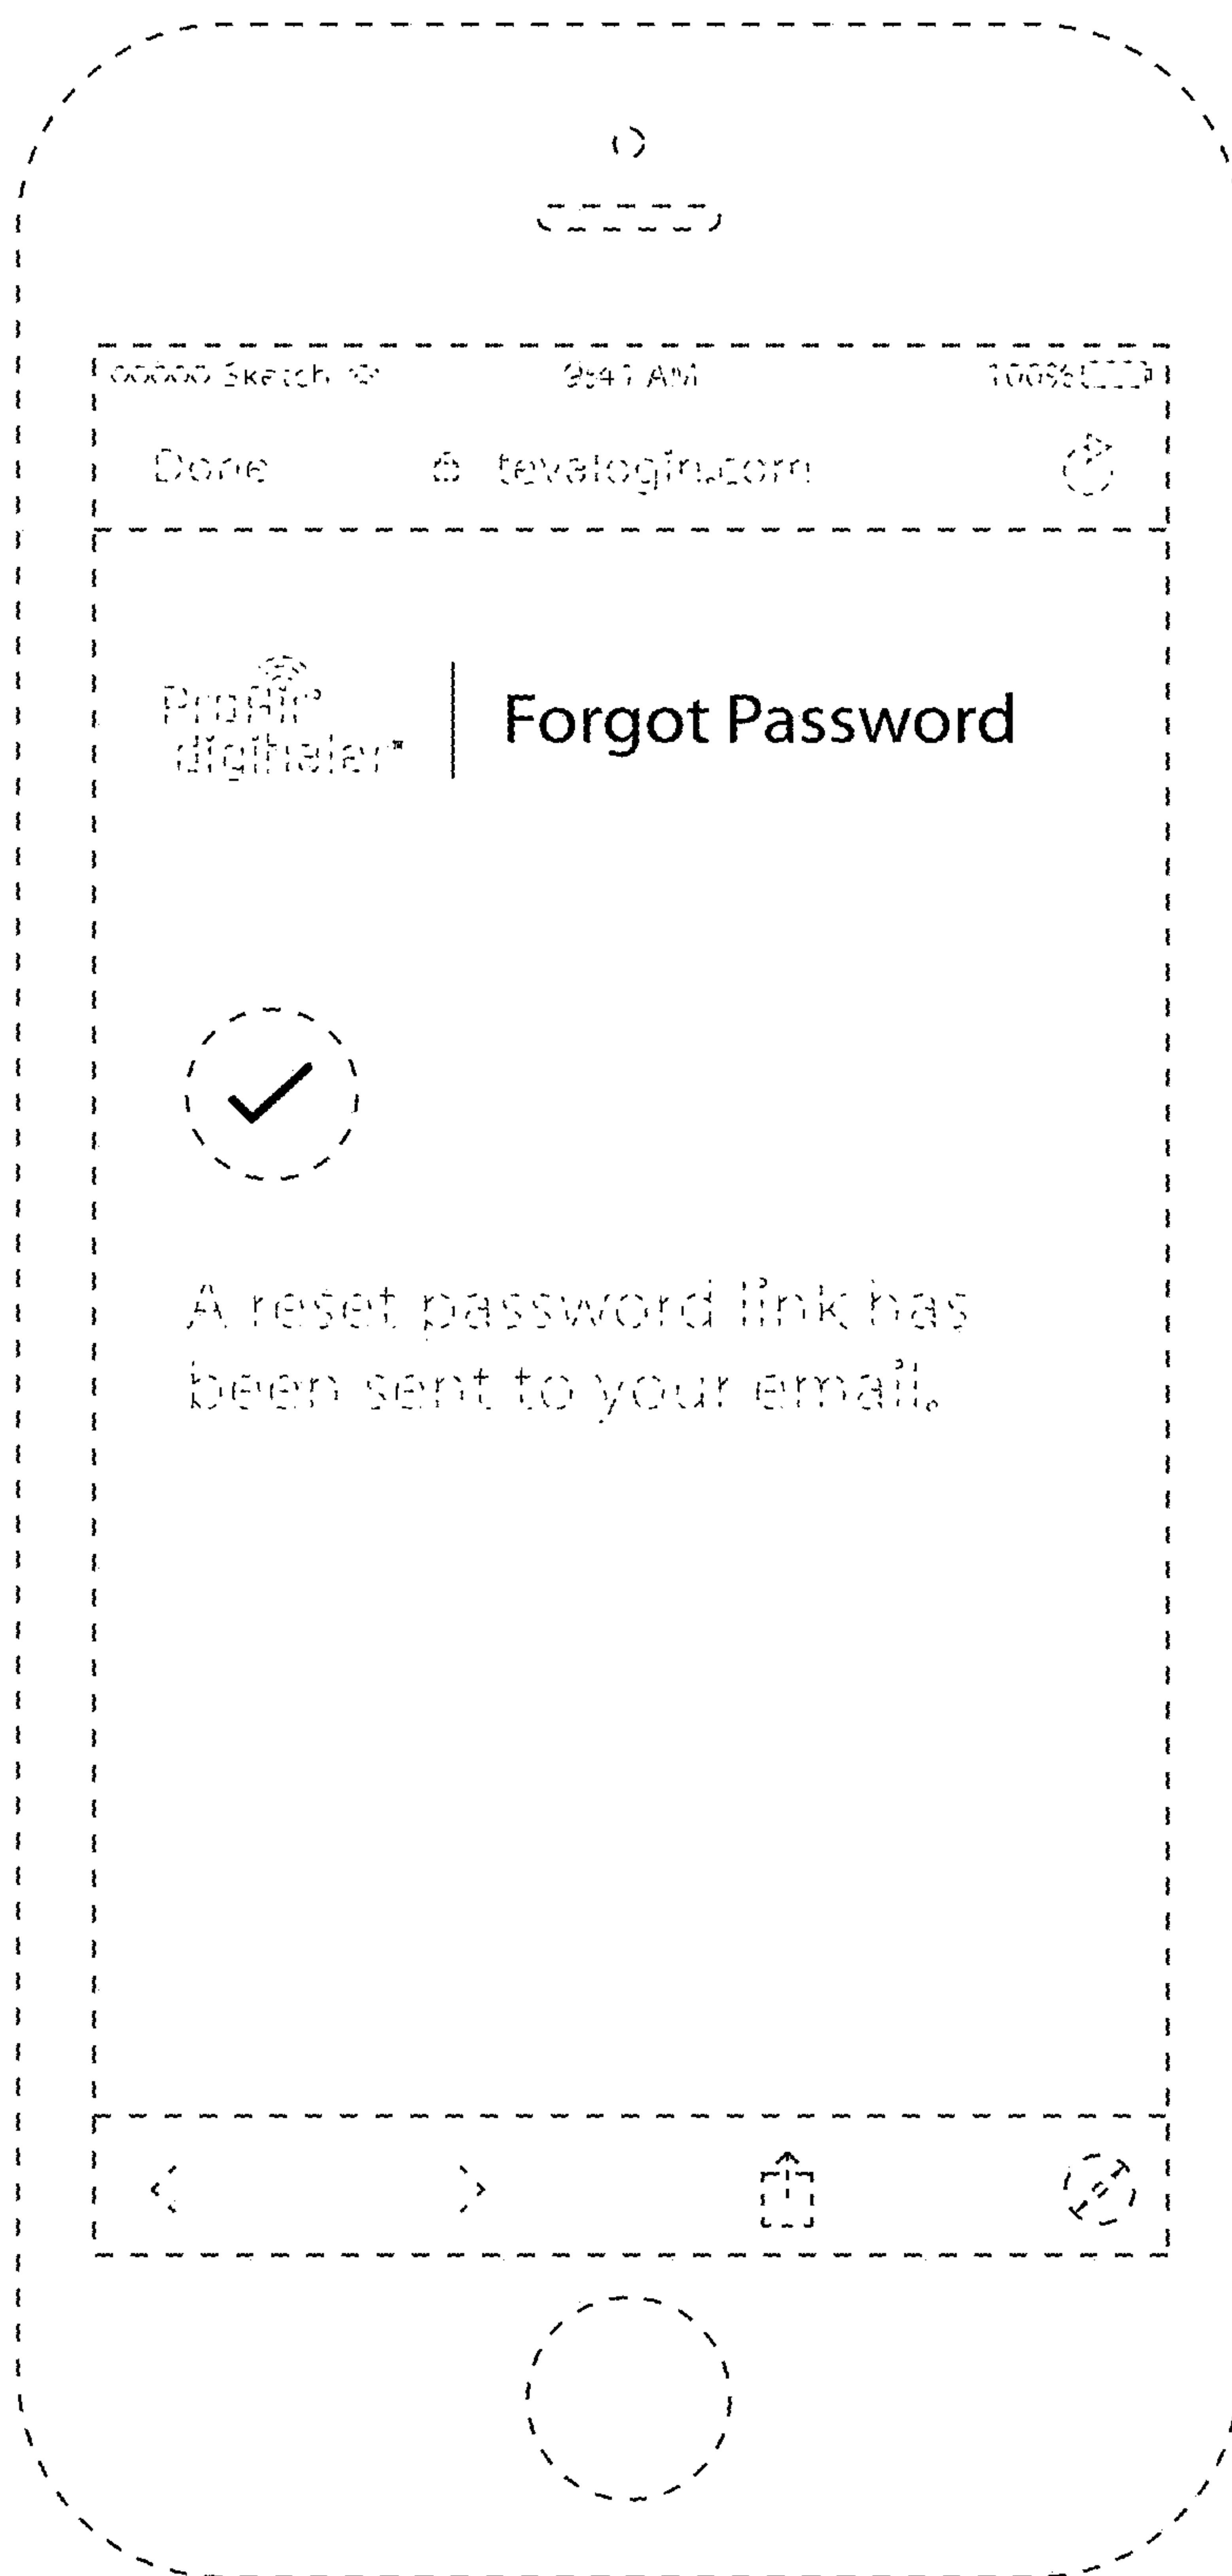


FIG. 3

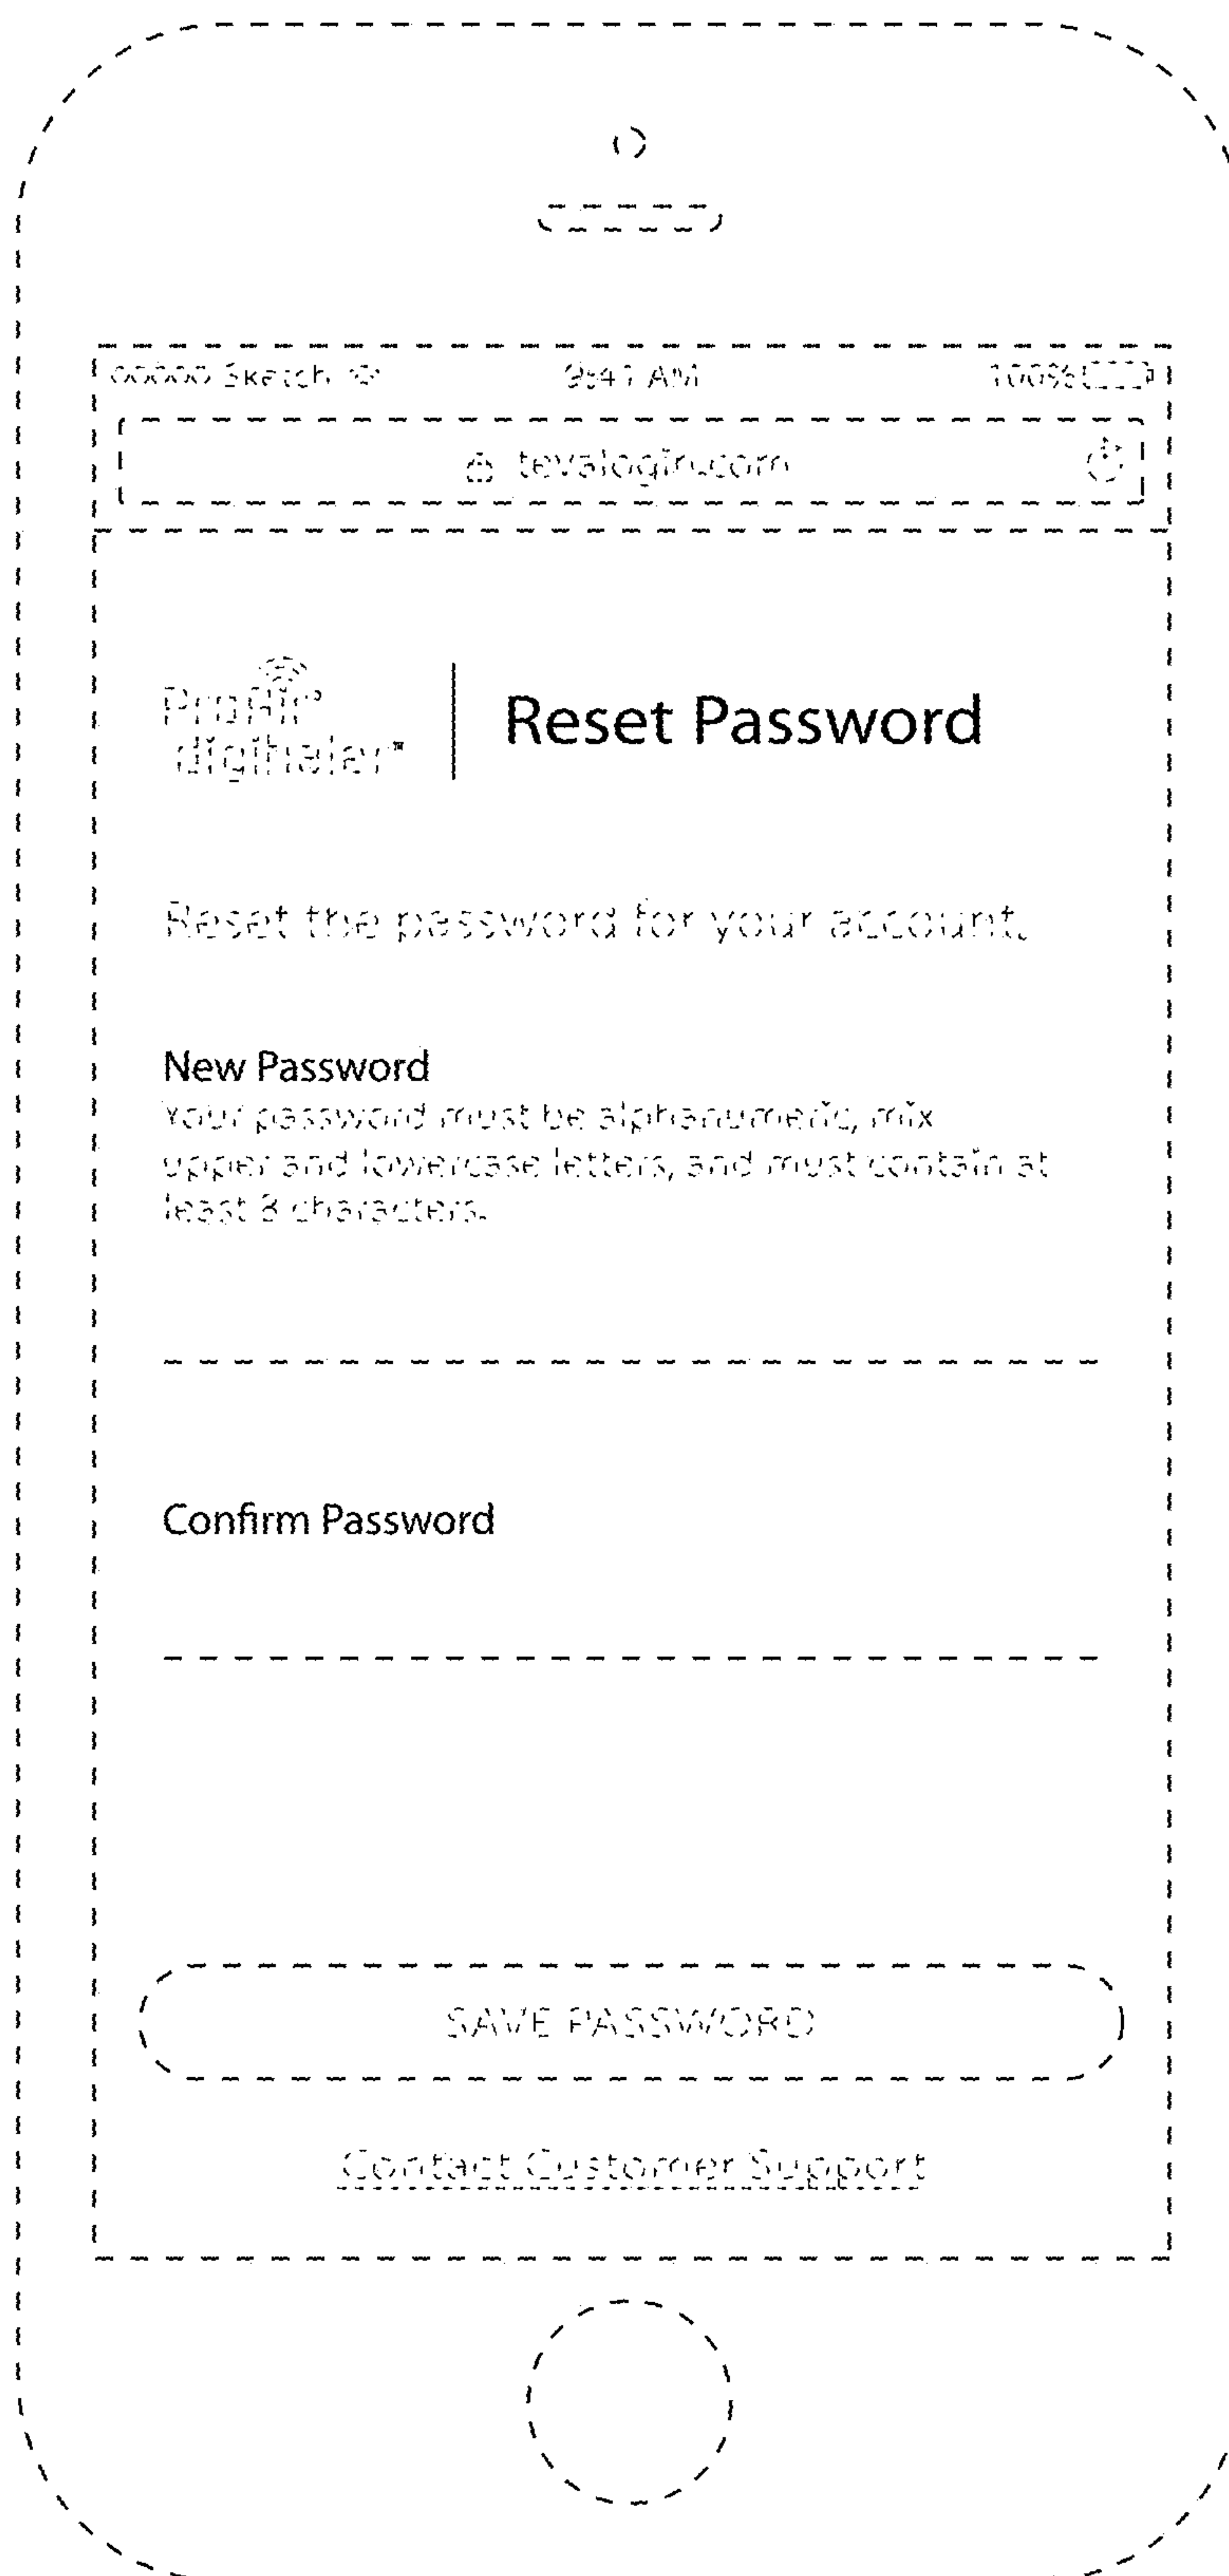


FIG. 4

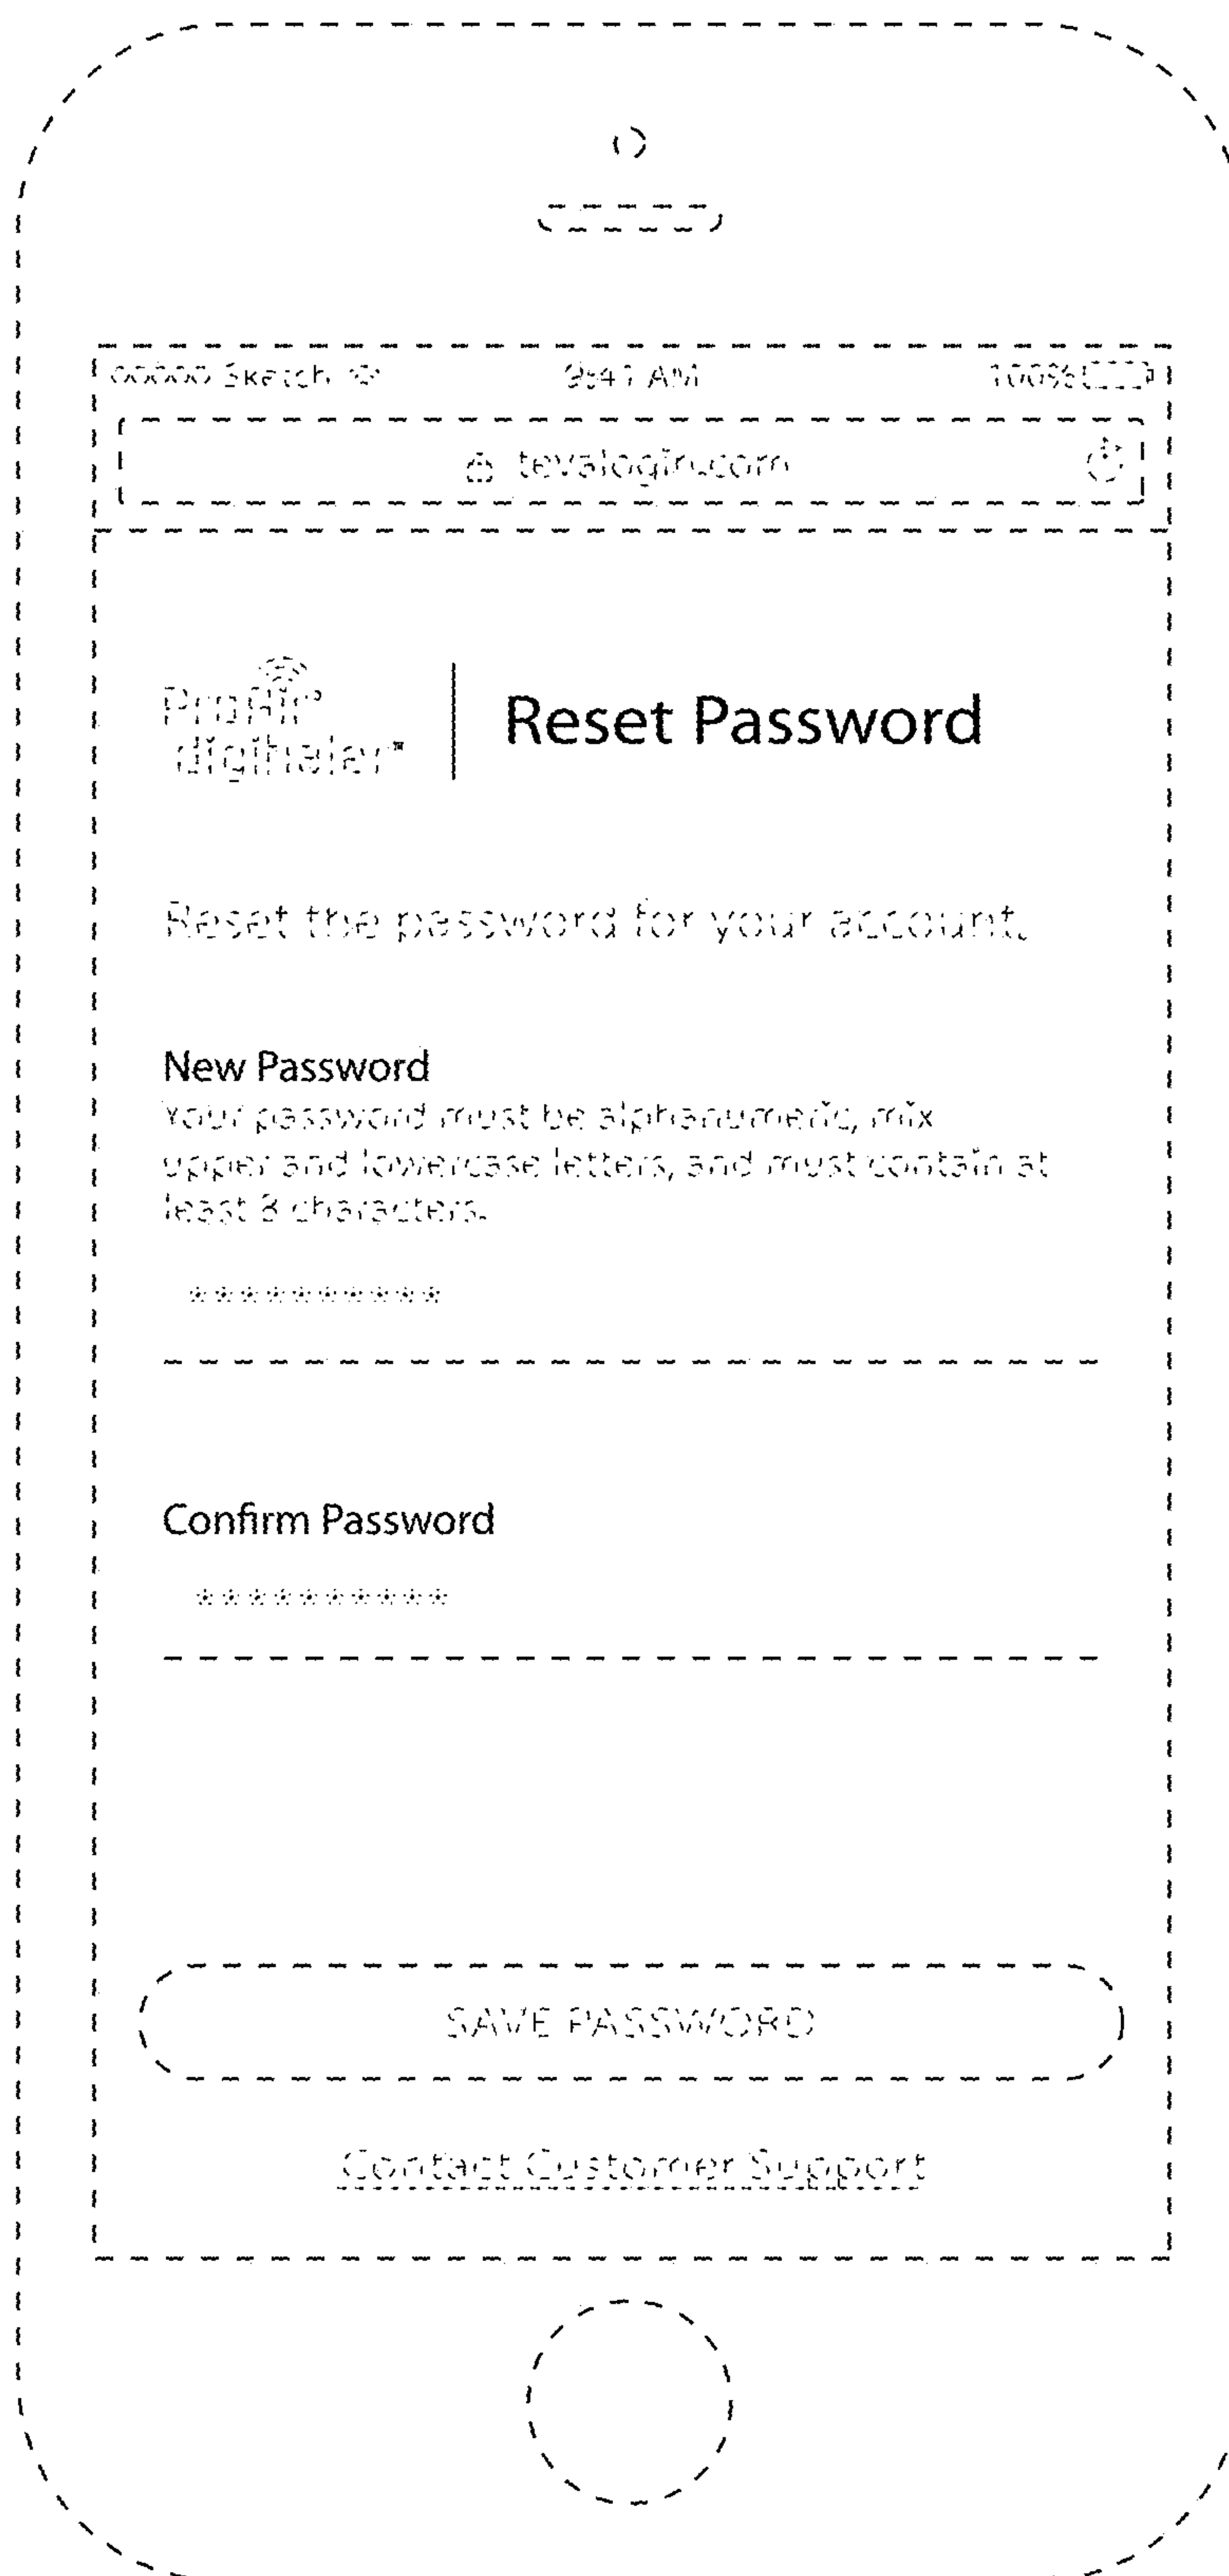


FIG. 5

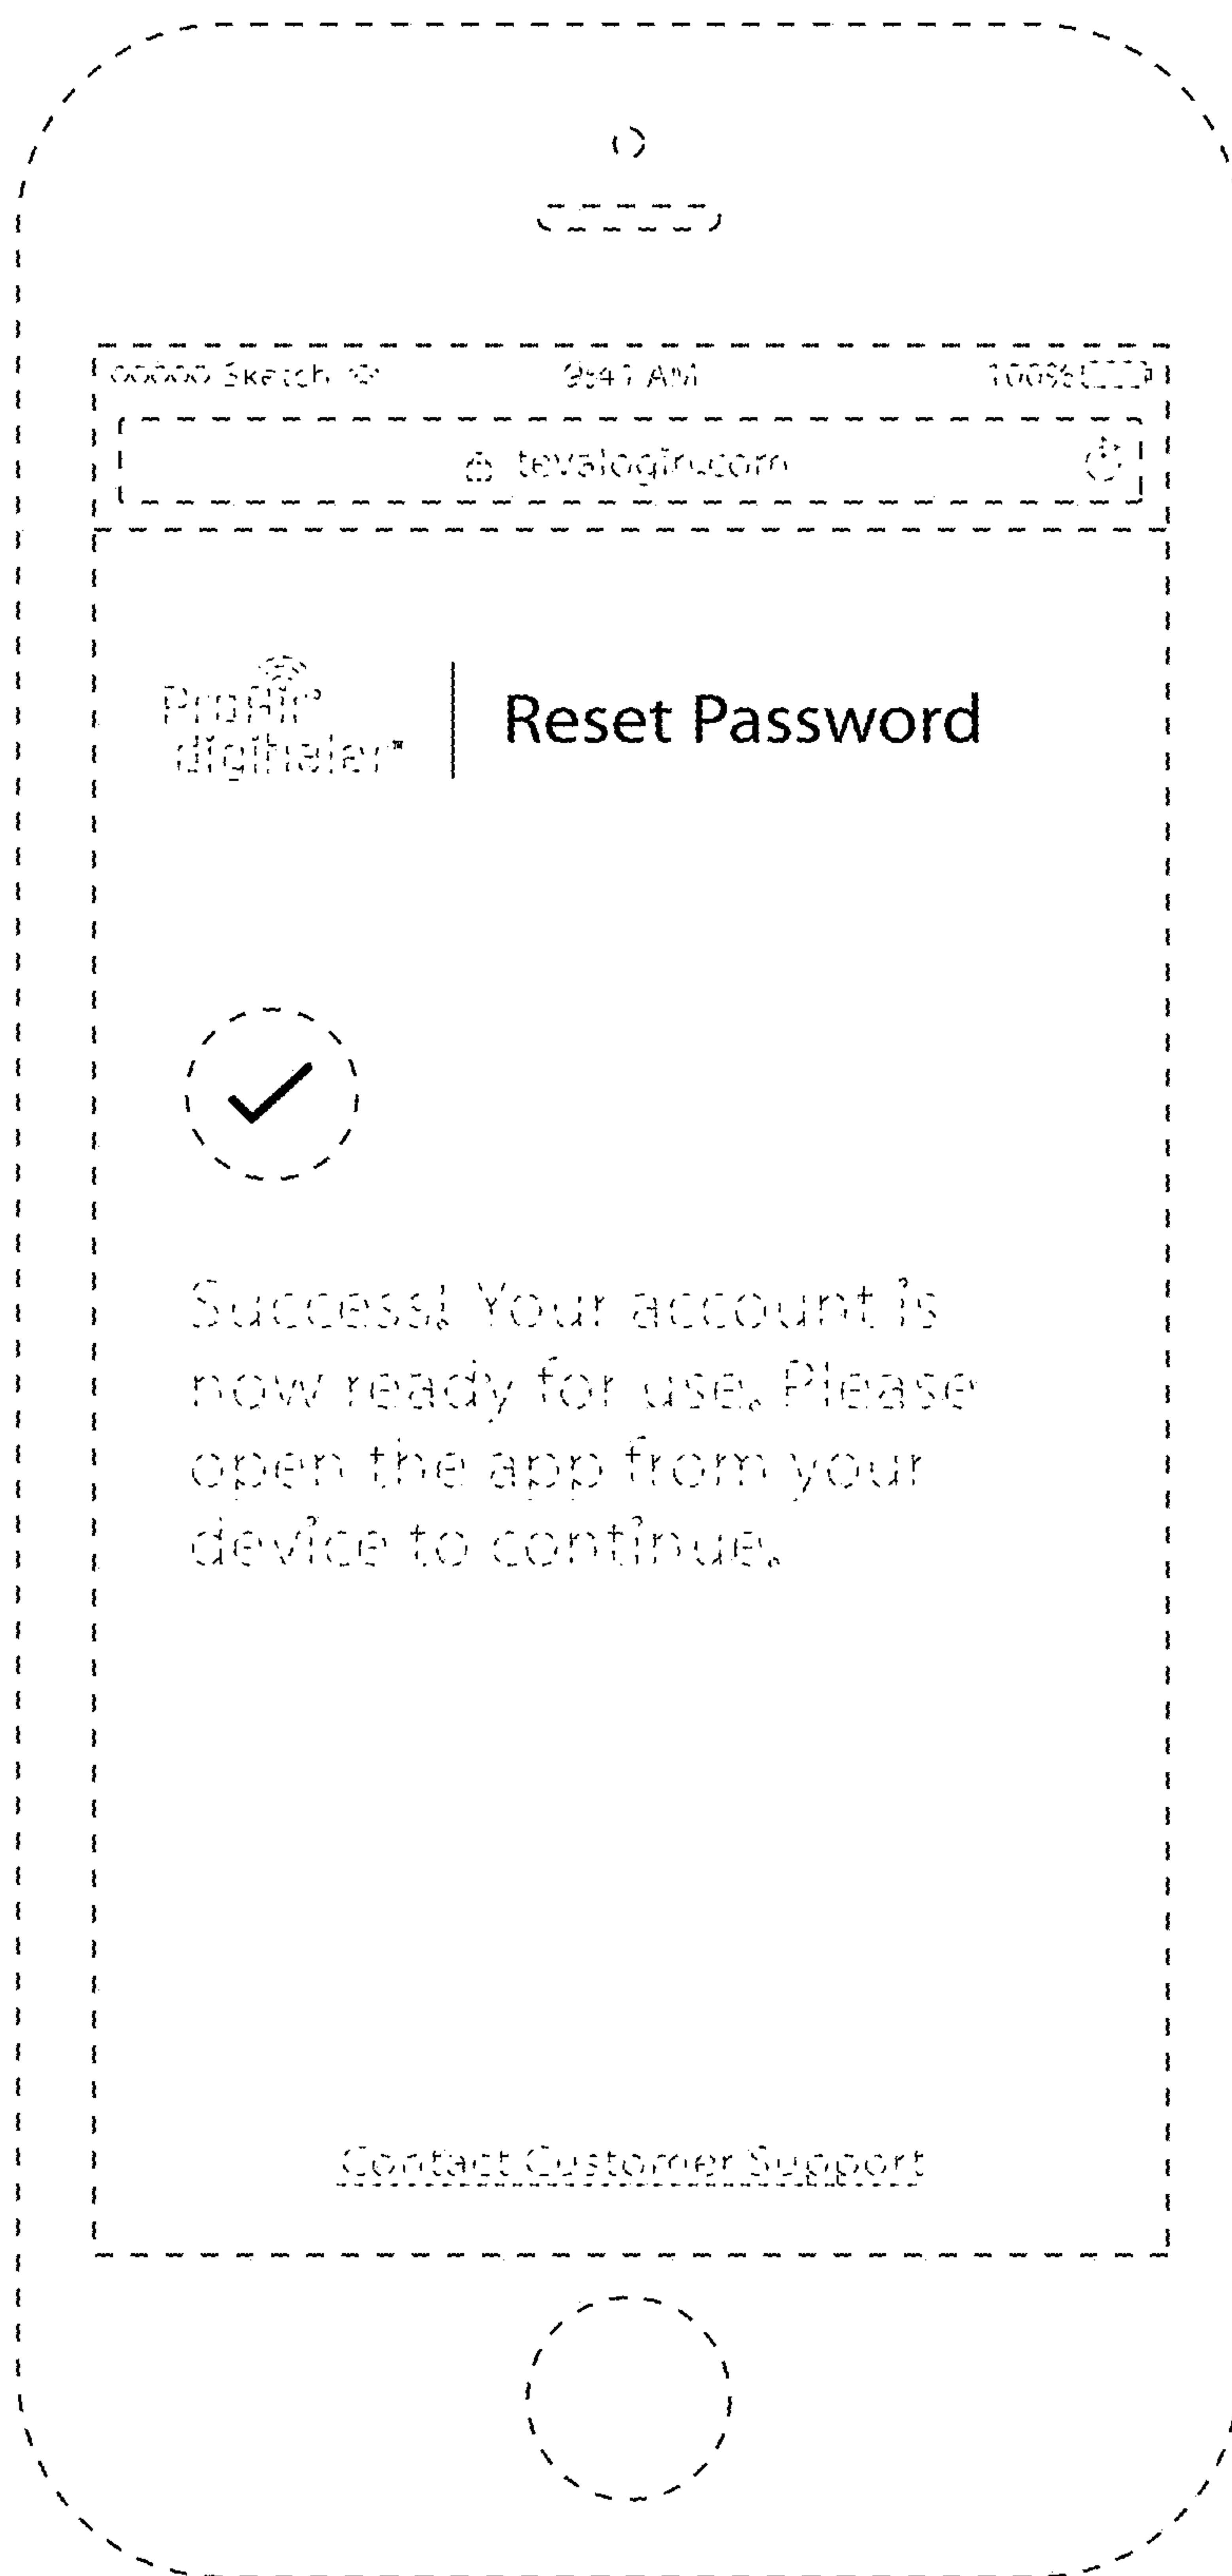


FIG. 6