



US00D914238S

(12) **United States Design Patent** (10) **Patent No.:** **US D914,238 S**  
**Leavitt et al.** (45) **Date of Patent:** **\*\* Mar. 23, 2021**

(54) **TISSUE SAMPLE RECEPTACLE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Leavitt Medical, Inc.**, Lehi, UT (US)

WO 2006039396 A2 4/2006

(72) Inventors: **Matthew O. Leavitt**, Salt Lake City, UT (US); **Sorin Musat**, Bucharest (RO)

OTHER PUBLICATIONS

(73) Assignee: **Leavitt Medical, Inc.**, Lehi, UT (US)

Eguiluz et al., Multiitissue array review: A chronological description of tissue array techniques, applications and procedures, Apr. 14, 2006, Elsevier.

(\*\*) Term: **15 Years**

Themis Biopsy Chip, Sectionable Matrix for Biopsy Chip for the Operating Room/PathLab/Training—Paraffin Frozen, Themis Pathology, Feb. 2016.

(21) Appl. No.: **29/674,485**

(22) Filed: **Dec. 21, 2018**

\* cited by examiner

**Related U.S. Application Data**

(63) Continuation of application No. 29/593,566, filed on Feb. 9, 2017, now Pat. No. Des. 836,796.

*Primary Examiner* — Lilyana Bekic

*Assistant Examiner* — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — FisherBroyles, LLP

(51) **LOC (13) Cl.** ..... **24-01**

(57) **CLAIM**

(52) **U.S. Cl.**

USPC ..... **D24/229**

The ornamental design for a tissue sample receptacle, as shown and described.

(58) **Field of Classification Search**

USPC ..... D24/216, 222, 224–232

CPC ... G01N 1/30; G01N 2001/368; C12M 23/10;

C12M 23/12; C12M 23/34

See application file for complete search history.

**DESCRIPTION**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,661,458 A \* 4/1987 Berry ..... C12M 23/34  
210/321.75  
D473,318 S \* 4/2003 Barbera-Guillem ..... D24/216  
D622,407 S \* 8/2010 Brown ..... D24/229  
D638,137 S \* 5/2011 Gross ..... D24/227  
D718,466 S \* 11/2014 So ..... D24/224  
D718,471 S \* 11/2014 So ..... D24/224  
D755,986 S \* 5/2016 Green ..... D24/224  
D792,602 S \* 7/2017 Meng ..... D24/216  
9,851,349 B2 \* 12/2017 Musat ..... G01N 33/5436  
2012/0208273 A1 \* 8/2012 Tarunina ..... C12M 23/34  
435/366  
2014/0073004 A1 3/2014 Williamson, IV et al.  
2014/0135236 A1 5/2014 Musat

FIG. 1 is a front perspective view of a tissue sample receptacle showing our new design.

FIG. 2 is a front side view of the tissue sample receptacle shown in FIG. 1.

FIG. 3 is a back side view of the tissue sample receptacle shown in FIG. 1.

FIG. 4 is a left side view of the tissue sample receptacle shown in FIG. 1.


FIG. 5 is a right side view of the tissue sample receptacle shown in FIG. 1.


FIG. 6 is a top view of the tissue sample receptacle shown in FIG. 1; and,

FIG. 7 is a bottom view of the tissue sample receptacle shown in FIG. 1.

The broken lines show portions of the tissue sample receptacle that form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

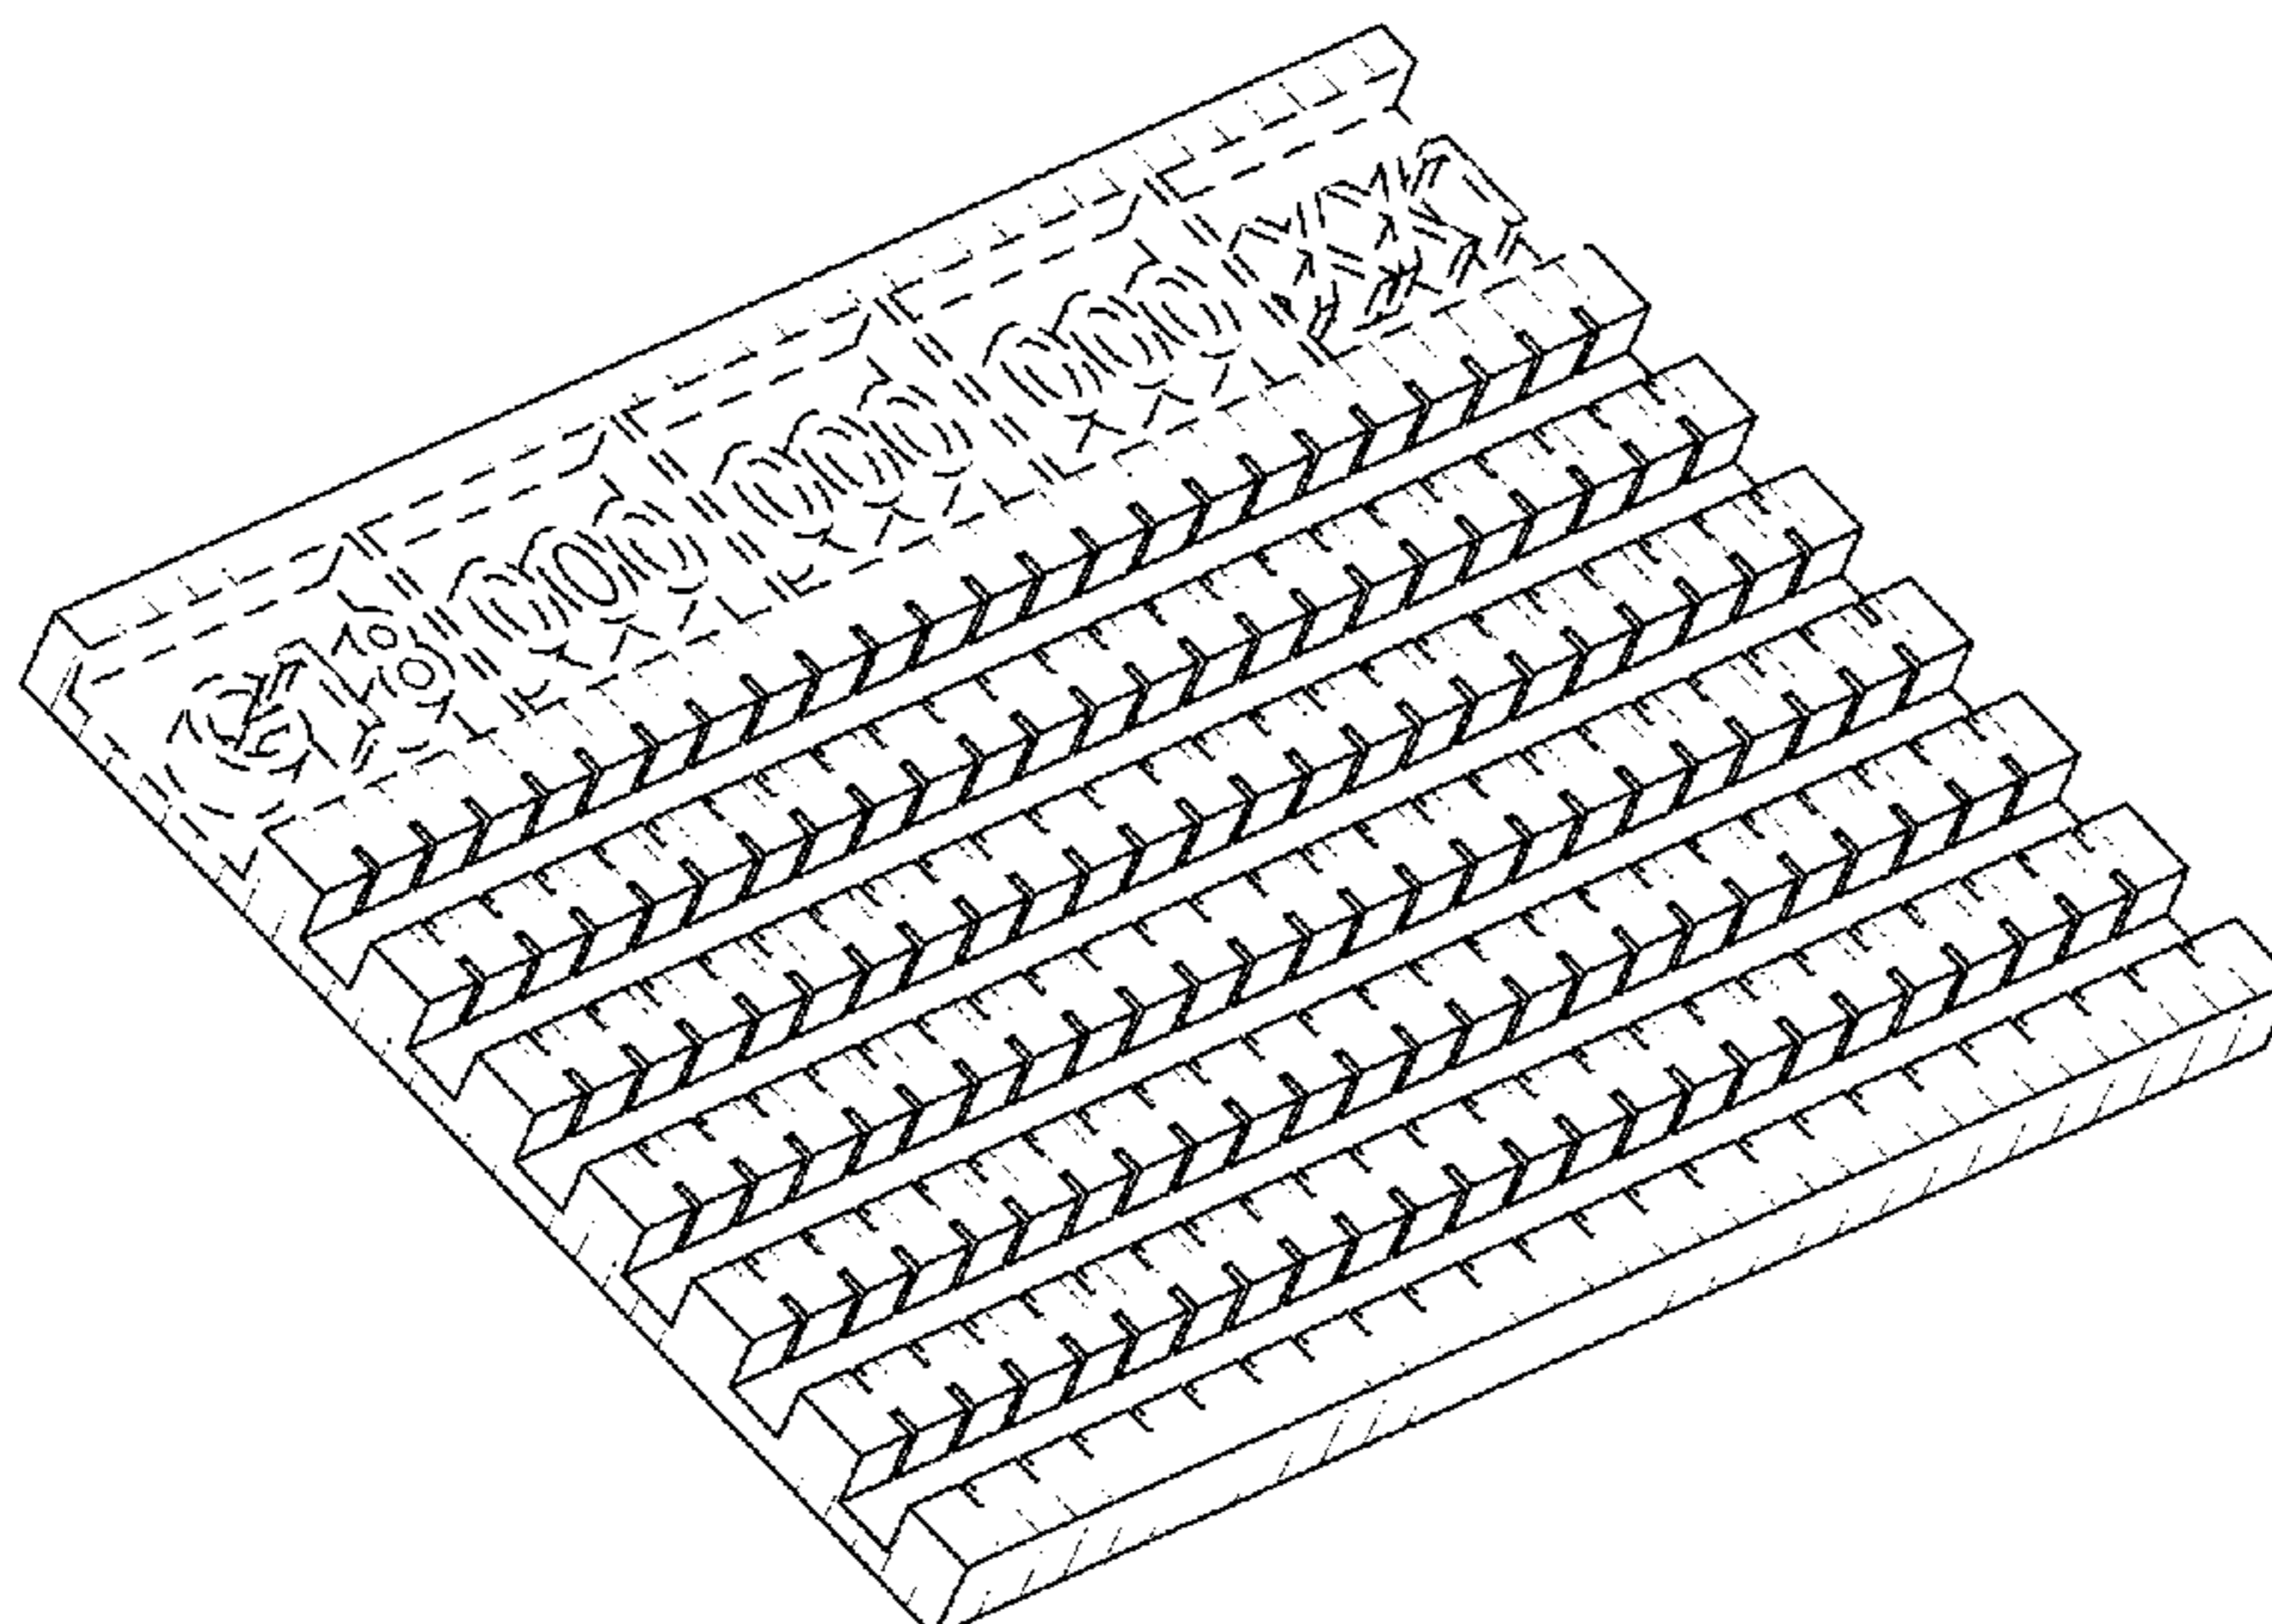


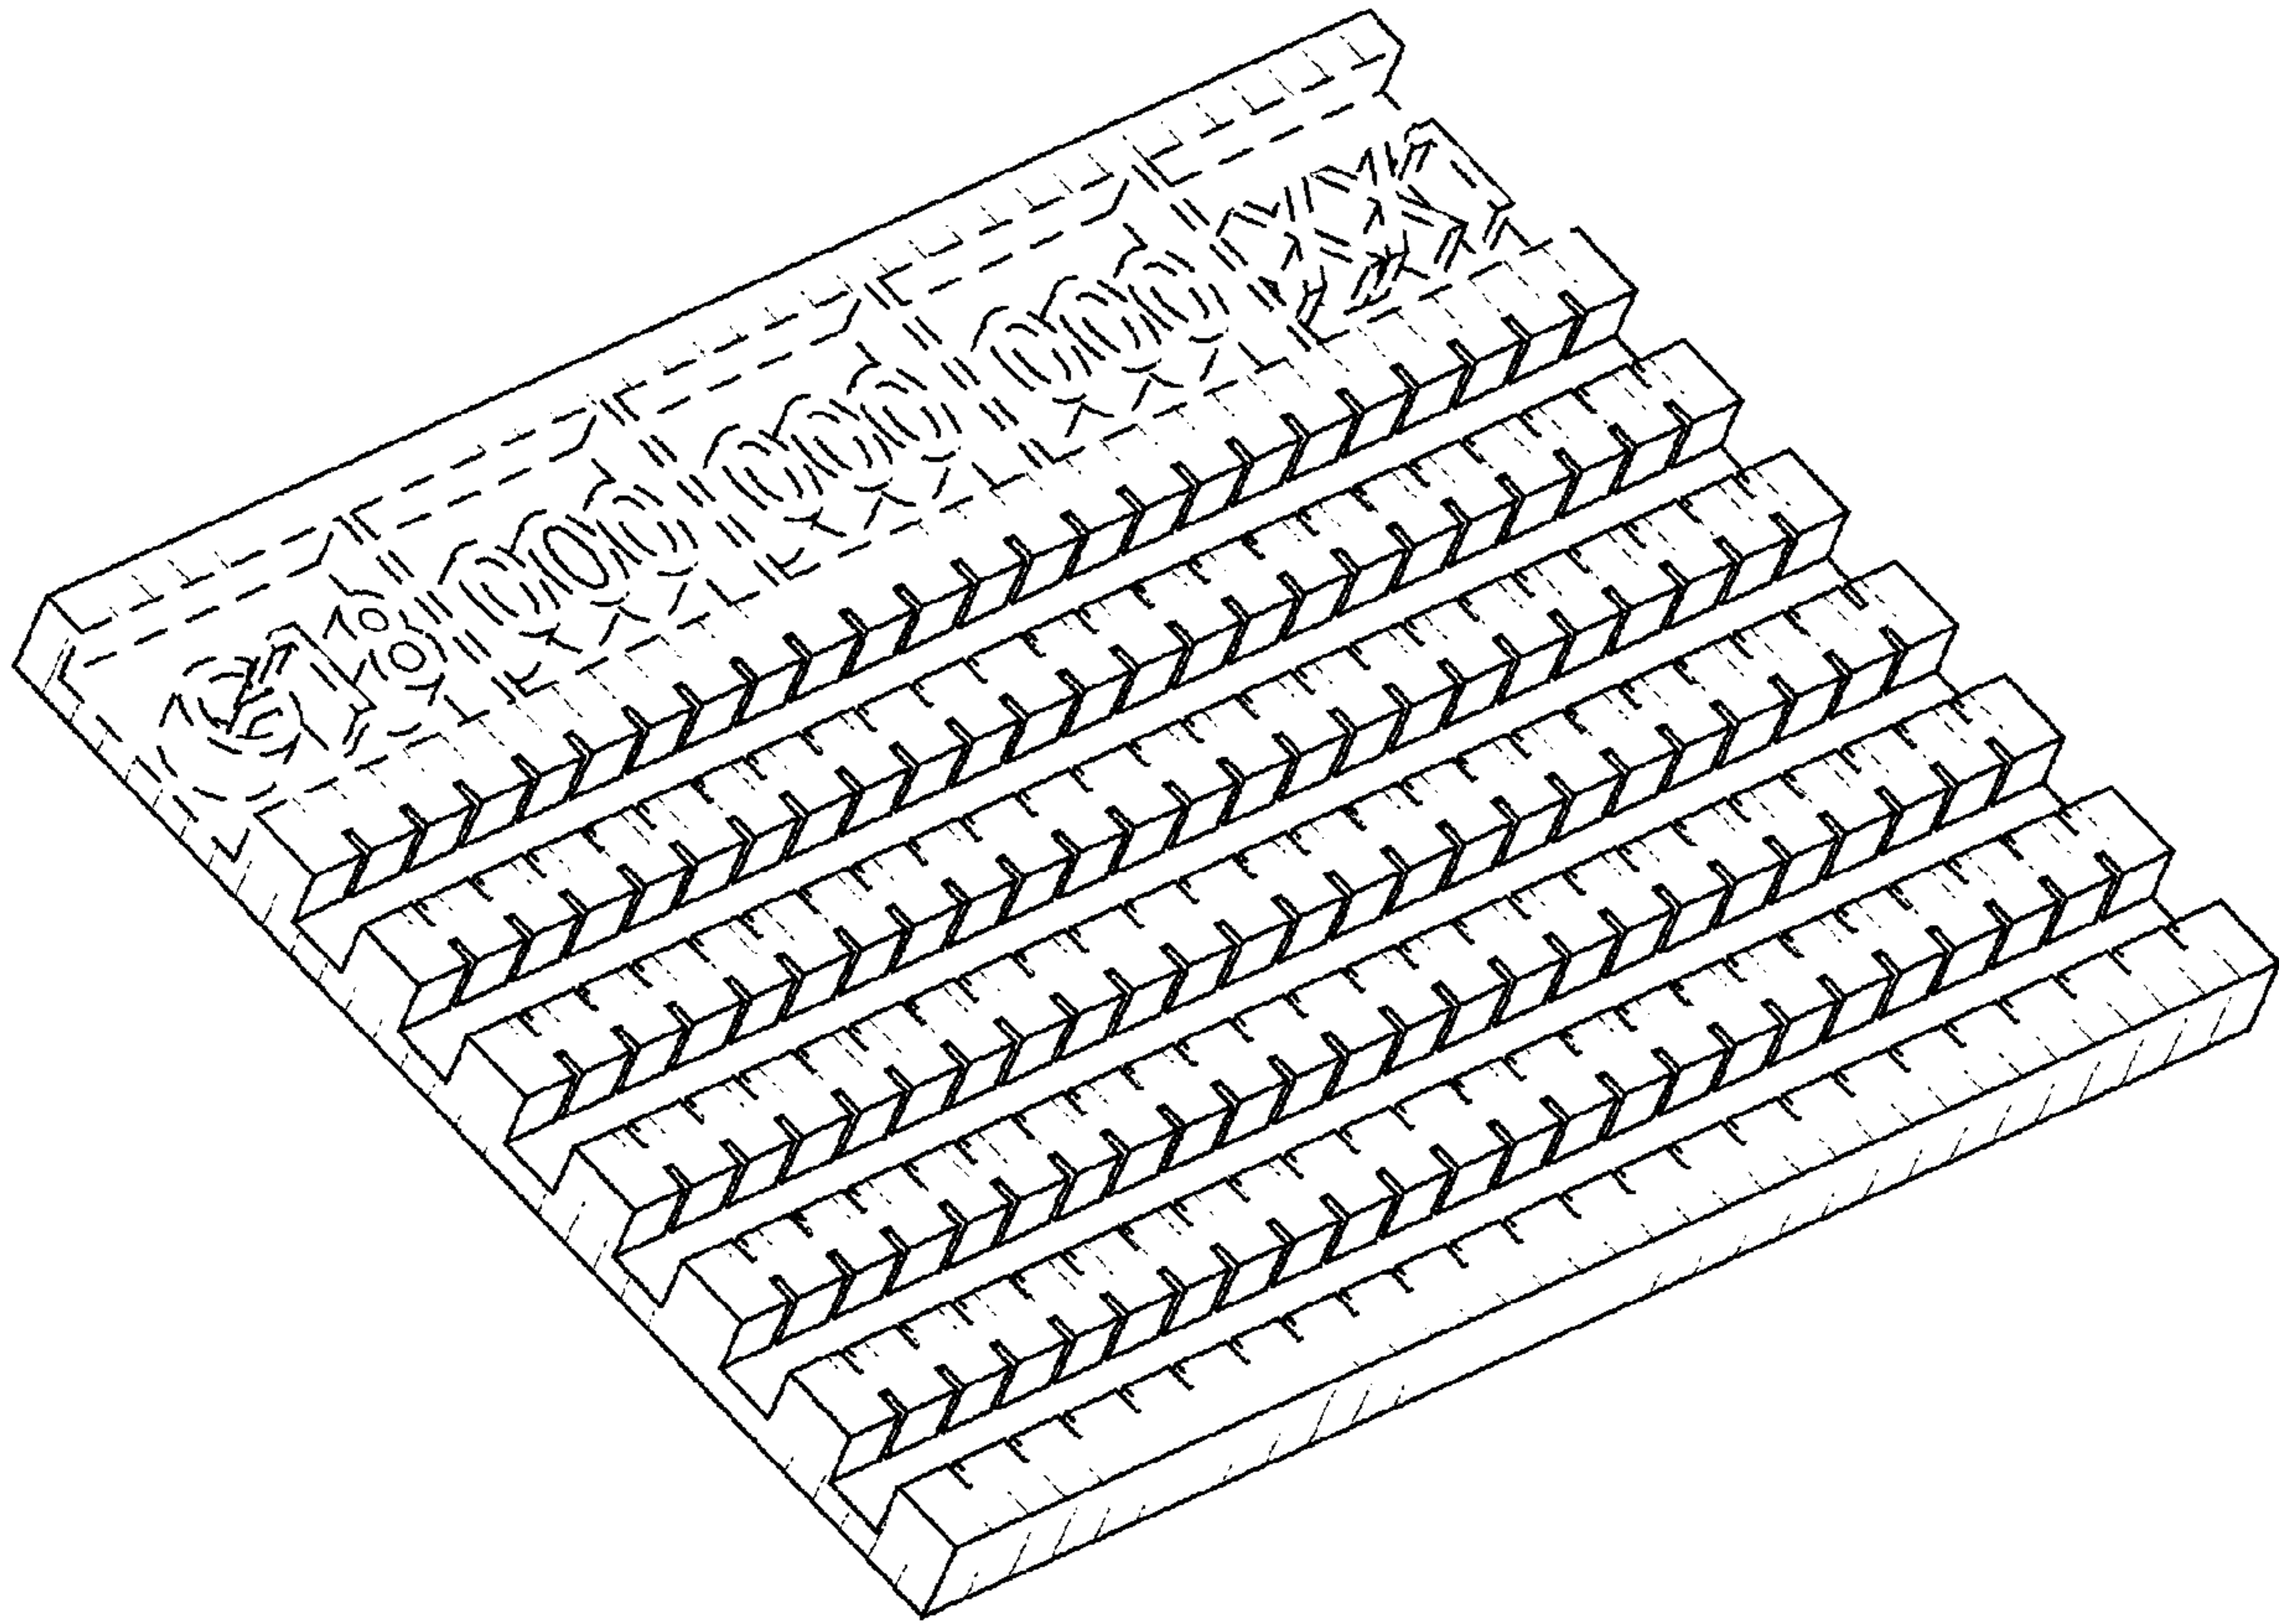

**FIG. 1**




**FIG. 2**

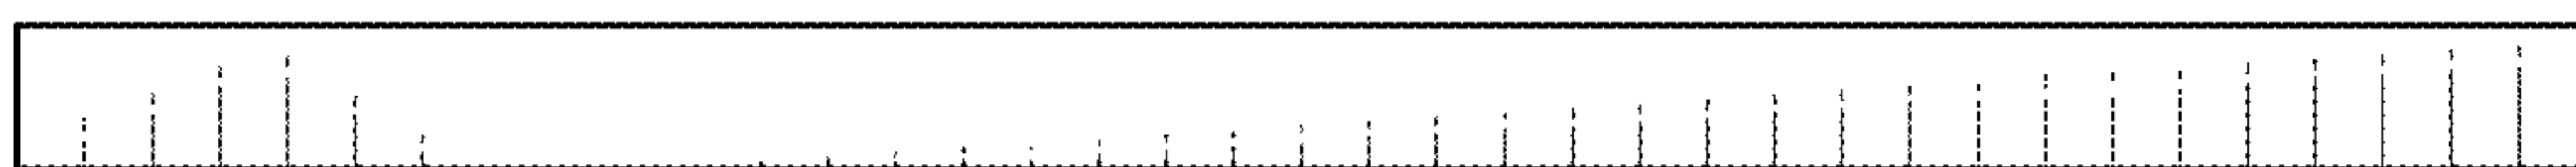


**FIG. 3**




**FIG. 4**

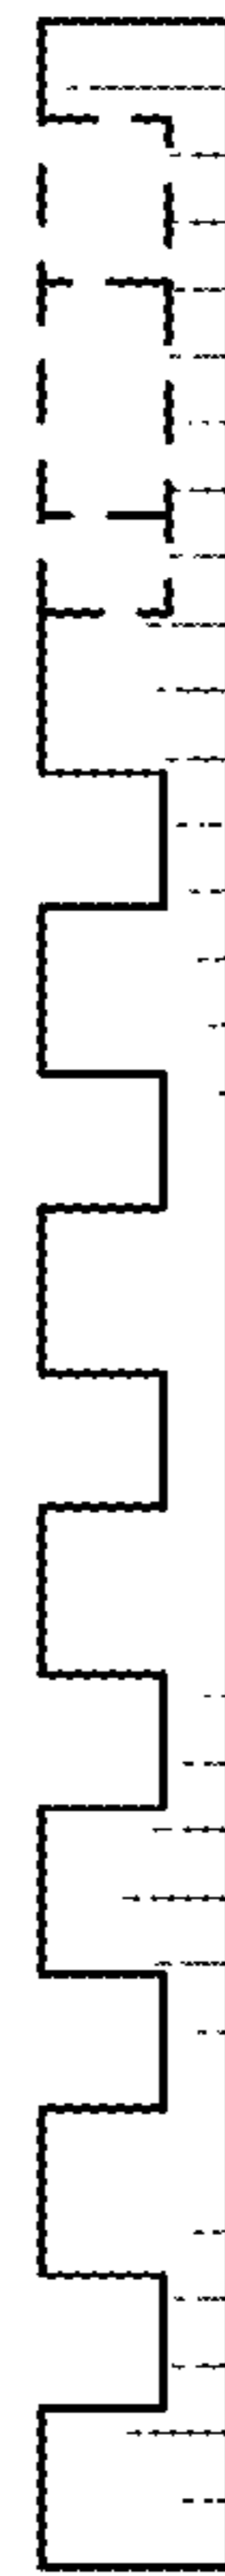

**FIG. 5**

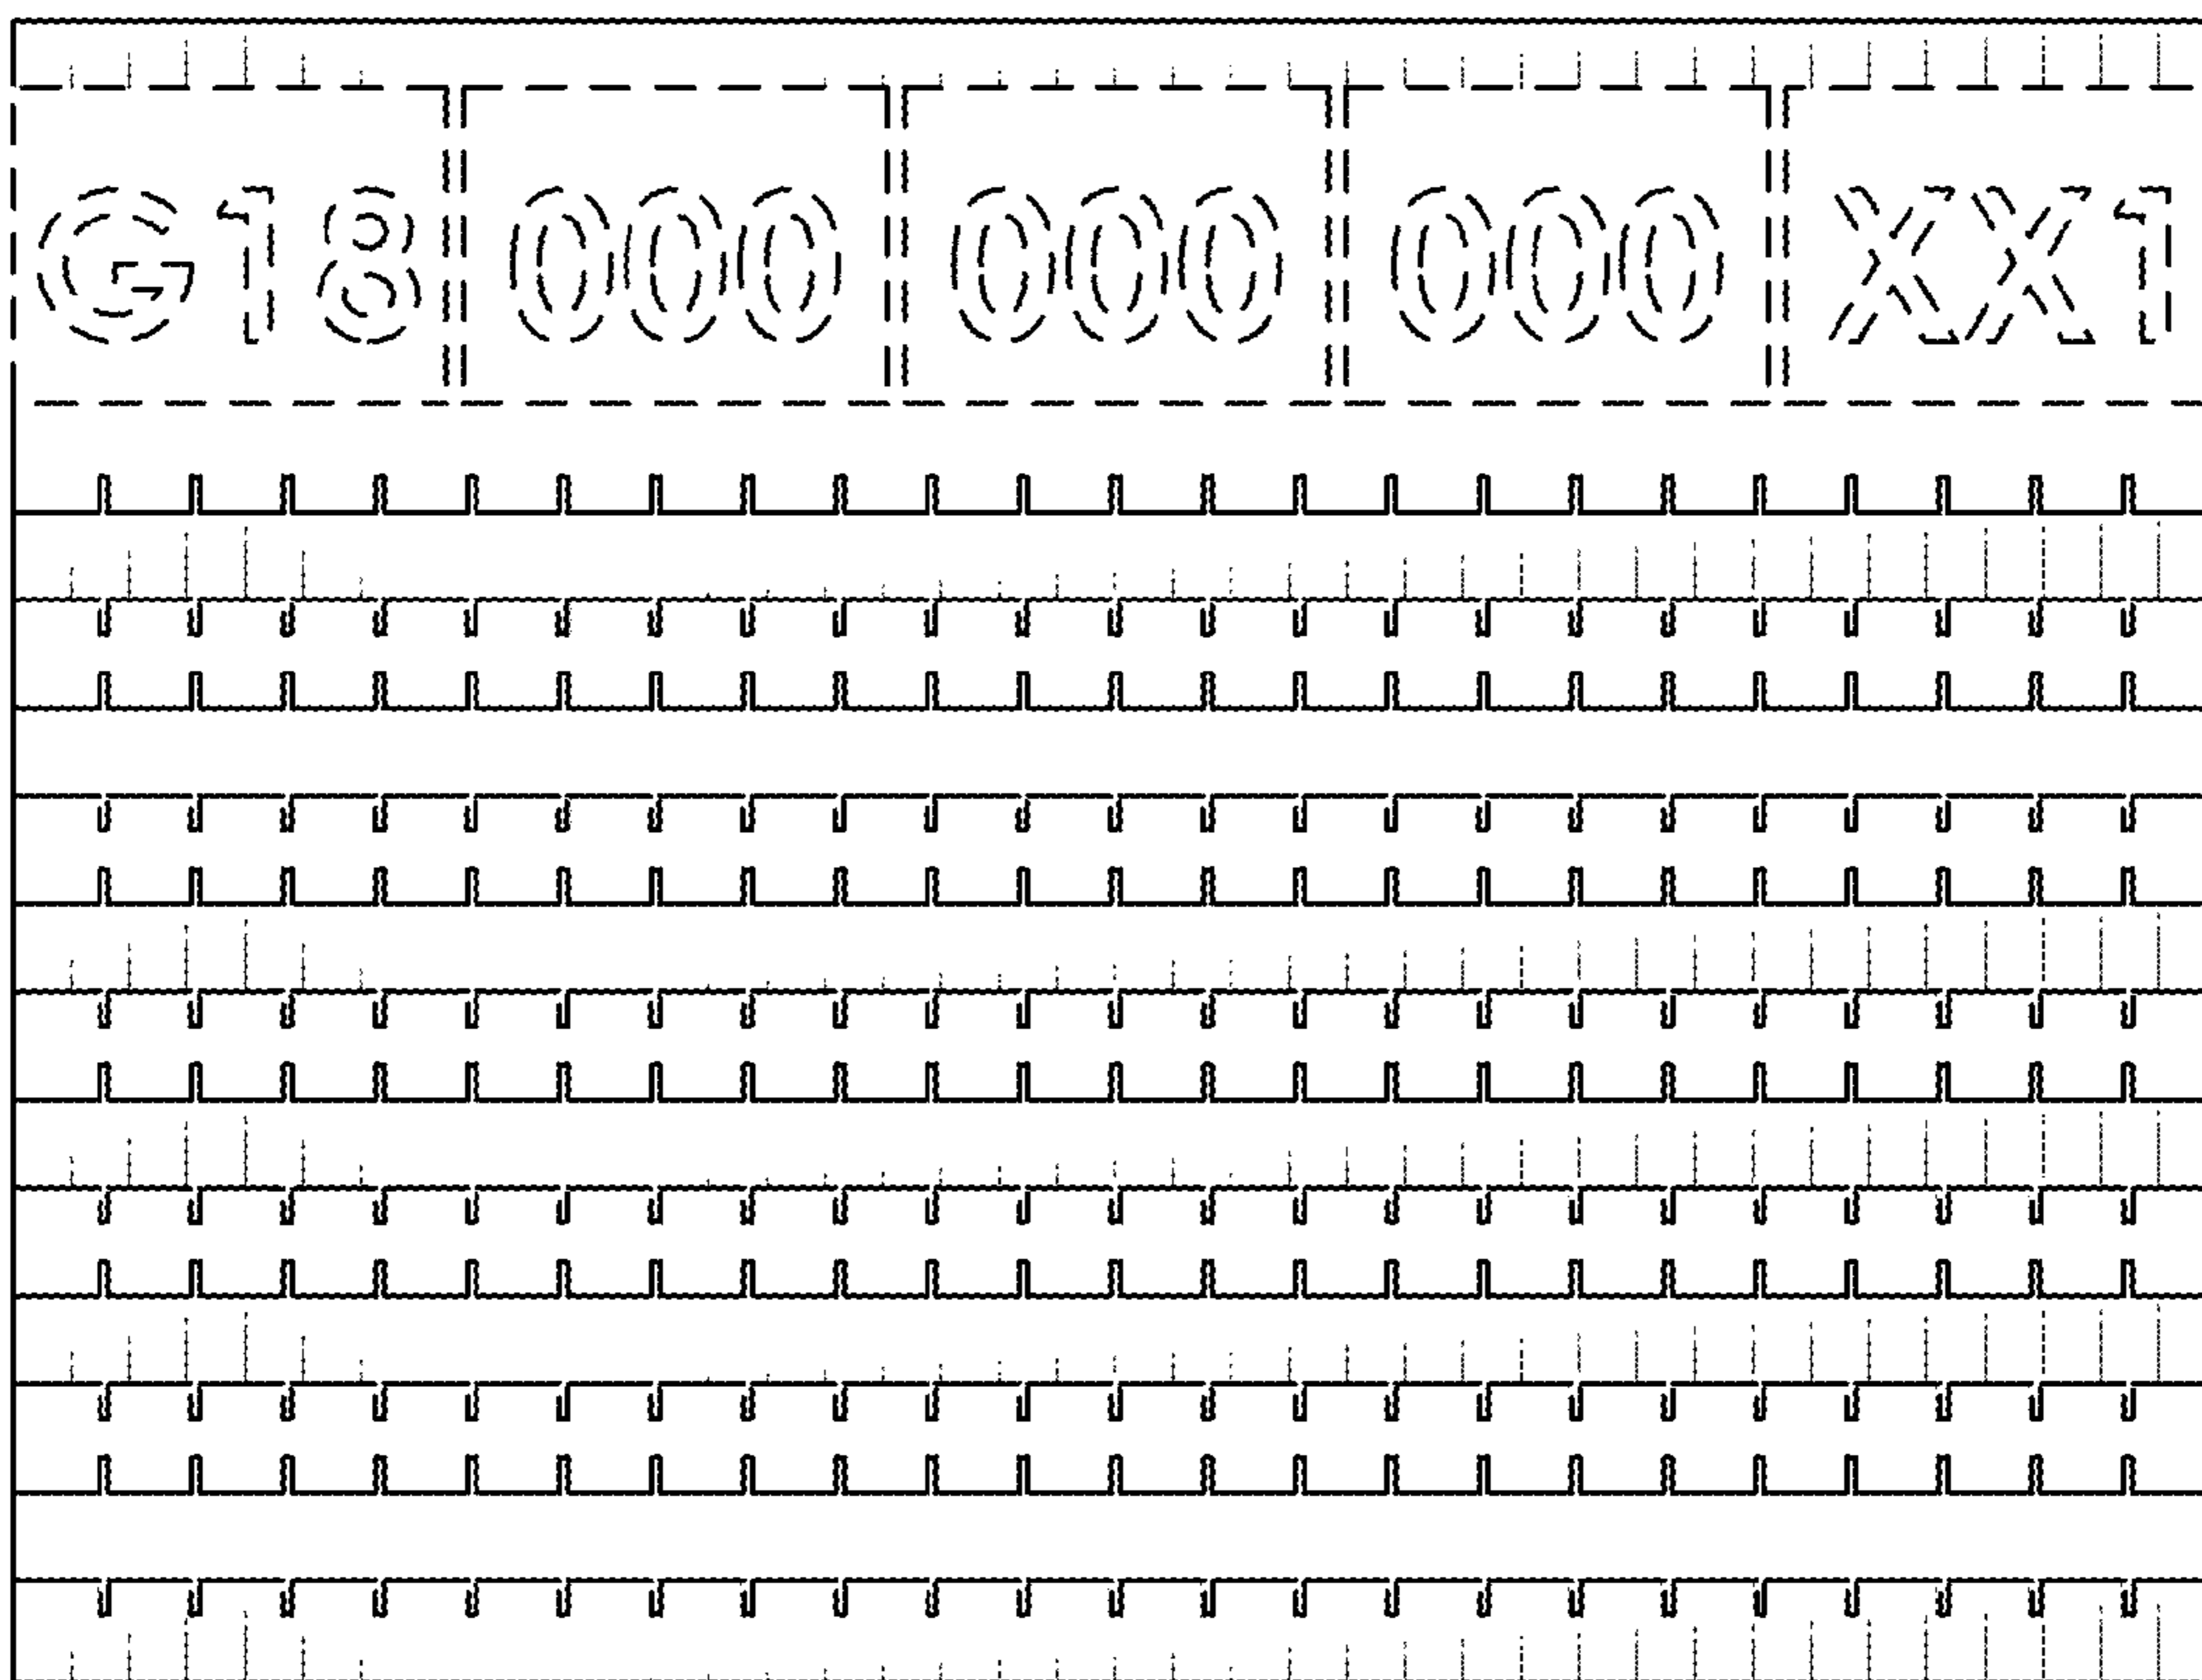

**FIG. 6**

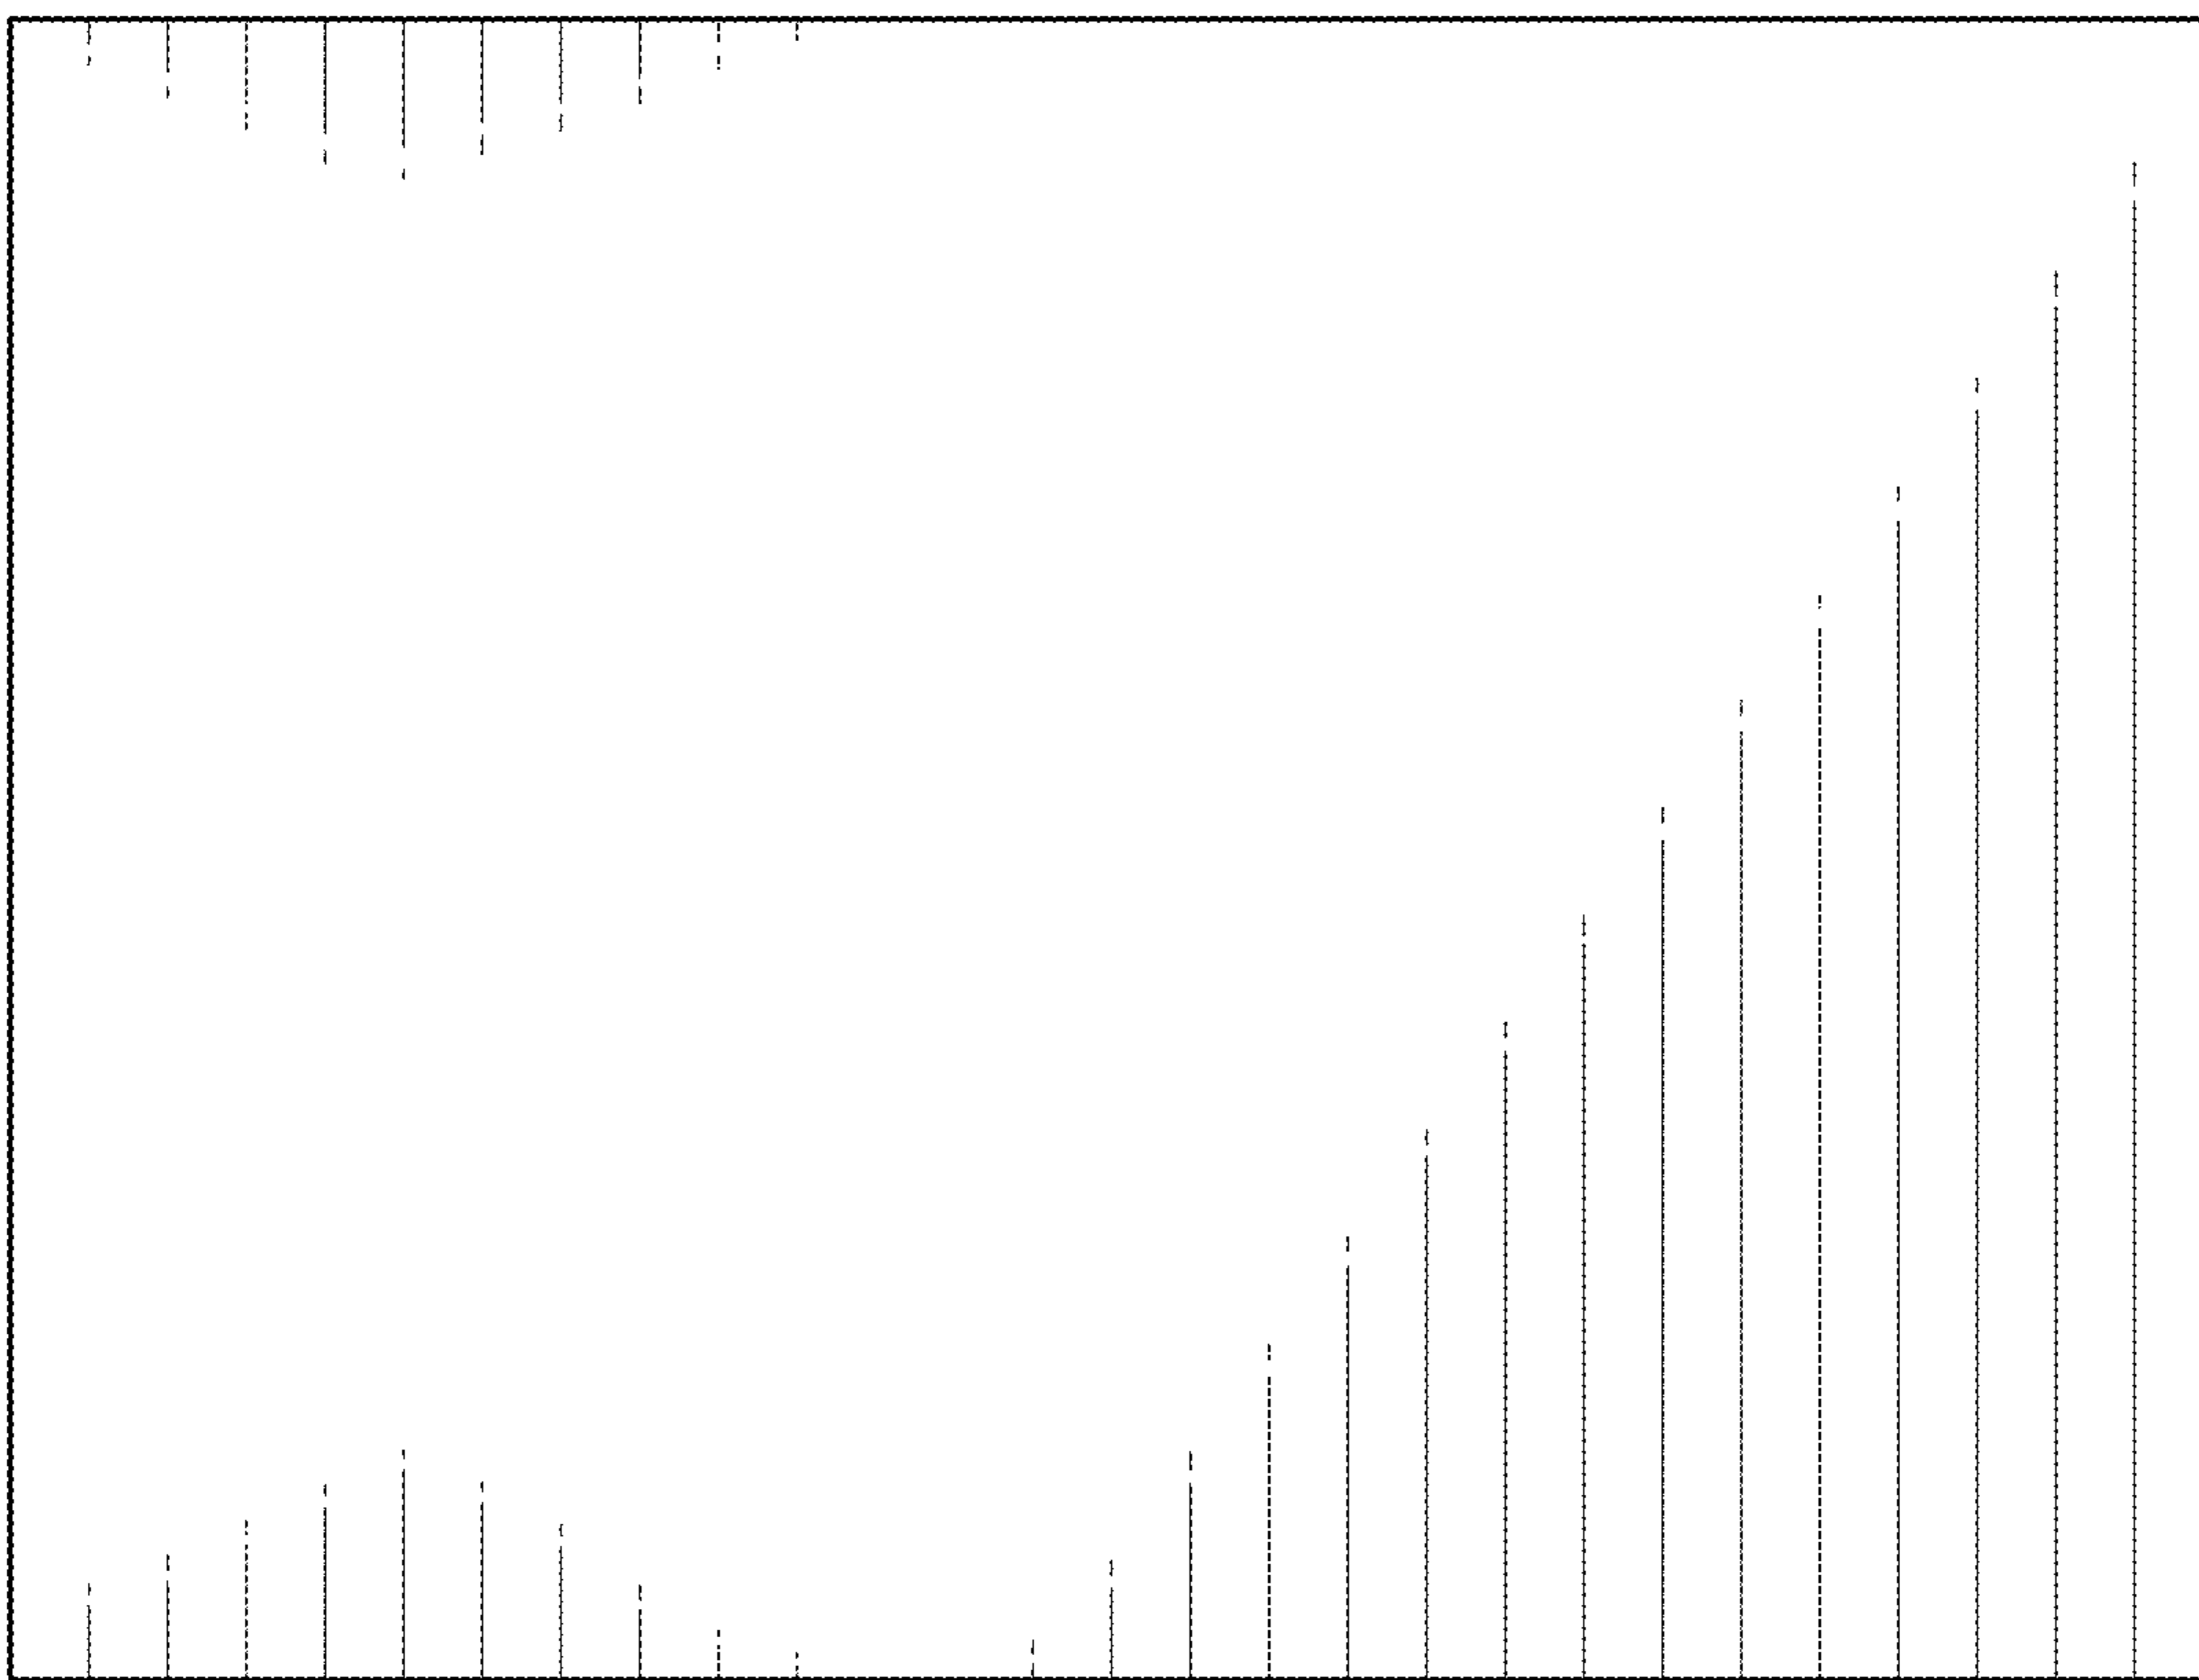

**FIG. 7**