



US00D914238S

(12) **United States Design Patent**  
**Leavitt et al.**

(10) **Patent No.: US D914,238 S**  
(45) **Date of Patent: \*\* Mar. 23, 2021**

(54) **TISSUE SAMPLE RECEPTACLE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Leavitt Medical, Inc.**, Lehi, UT (US)

WO 2006039396 A2 4/2006

(72) Inventors: **Matthew O. Leavitt**, Salt Lake City, UT (US); **Sorin Musat**, Bucharest (RO)

OTHER PUBLICATIONS

(73) Assignee: **Leavitt Medical, Inc.**, Lehi, UT (US)

Eguiluz et al., Multiitissue array review: A chronological description of tissue array techniques, applications and procedures, Apr. 14, 2006, Elsevier.

(\*\*) Term: **15 Years**

Themis Biopsy Chip, Sectionable Matrix for Biopsy Chip for the Operating Room/PathLab/Training—Paraffin Frozen, Themis Pathology, Feb. 2016.

(21) Appl. No.: **29/674,485**

(22) Filed: **Dec. 21, 2018**

\* cited by examiner

**Related U.S. Application Data**

(63) Continuation of application No. 29/593,566, filed on Feb. 9, 2017, now Pat. No. Des. 836,796.

*Primary Examiner* — Lilyana Bekic

*Assistant Examiner* — Mary Shannon Malley

(51) **LOC (13) Cl.** ..... **24-01**

(74) *Attorney, Agent, or Firm* — FisherBroyles, LLP

(52) **U.S. Cl.**

USPC ..... **D24/229**

(57) **CLAIM**

The ornamental design for a tissue sample receptacle, as shown and described.

(58) **Field of Classification Search**

USPC ..... D24/216, 222, 224–232

CPC ... G01N 1/30; G01N 2001/368; C12M 23/10;

C12M 23/12; C12M 23/34

See application file for complete search history.

**DESCRIPTION**

FIG. 1 is a front perspective view of a tissue sample receptacle showing our new design.

FIG. 2 is a front side view of the tissue sample receptacle shown in FIG. 1.

FIG. 3 is a back side view of the tissue sample receptacle shown in FIG. 1.

FIG. 4 is a left side view of the tissue sample receptacle shown in FIG. 1.

FIG. 5 is a right side view of the tissue sample receptacle shown in FIG. 1.

FIG. 6 is a top view of the tissue sample receptacle shown in FIG. 1; and,

FIG. 7 is a bottom view of the tissue sample receptacle shown in FIG. 1.


The broken lines show portions of the tissue sample receptacle that form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

4,661,458	A *	4/1987	Berry	.....	C12M 23/34
					210/321.75
D473,318	S *	4/2003	Barbera-Guillem	.....	D24/216
D622,407	S *	8/2010	Brown	.....	D24/229
D638,137	S *	5/2011	Gross	.....	D24/227
D718,466	S *	11/2014	So	.....	D24/224
D718,471	S *	11/2014	So	.....	D24/224
D755,986	S *	5/2016	Green	.....	D24/224
D792,602	S *	7/2017	Meng	.....	D24/216
9,851,349	B2 *	12/2017	Musat	.....	G01N 33/5436
2012/0208273	A1 *	8/2012	Tarunina	.....	C12M 23/34
					435/366
2014/0073004	A1	3/2014	Williamson, IV et al.		
2014/0135236	A1	5/2014	Musat		

**1 Claim, 3 Drawing Sheets**

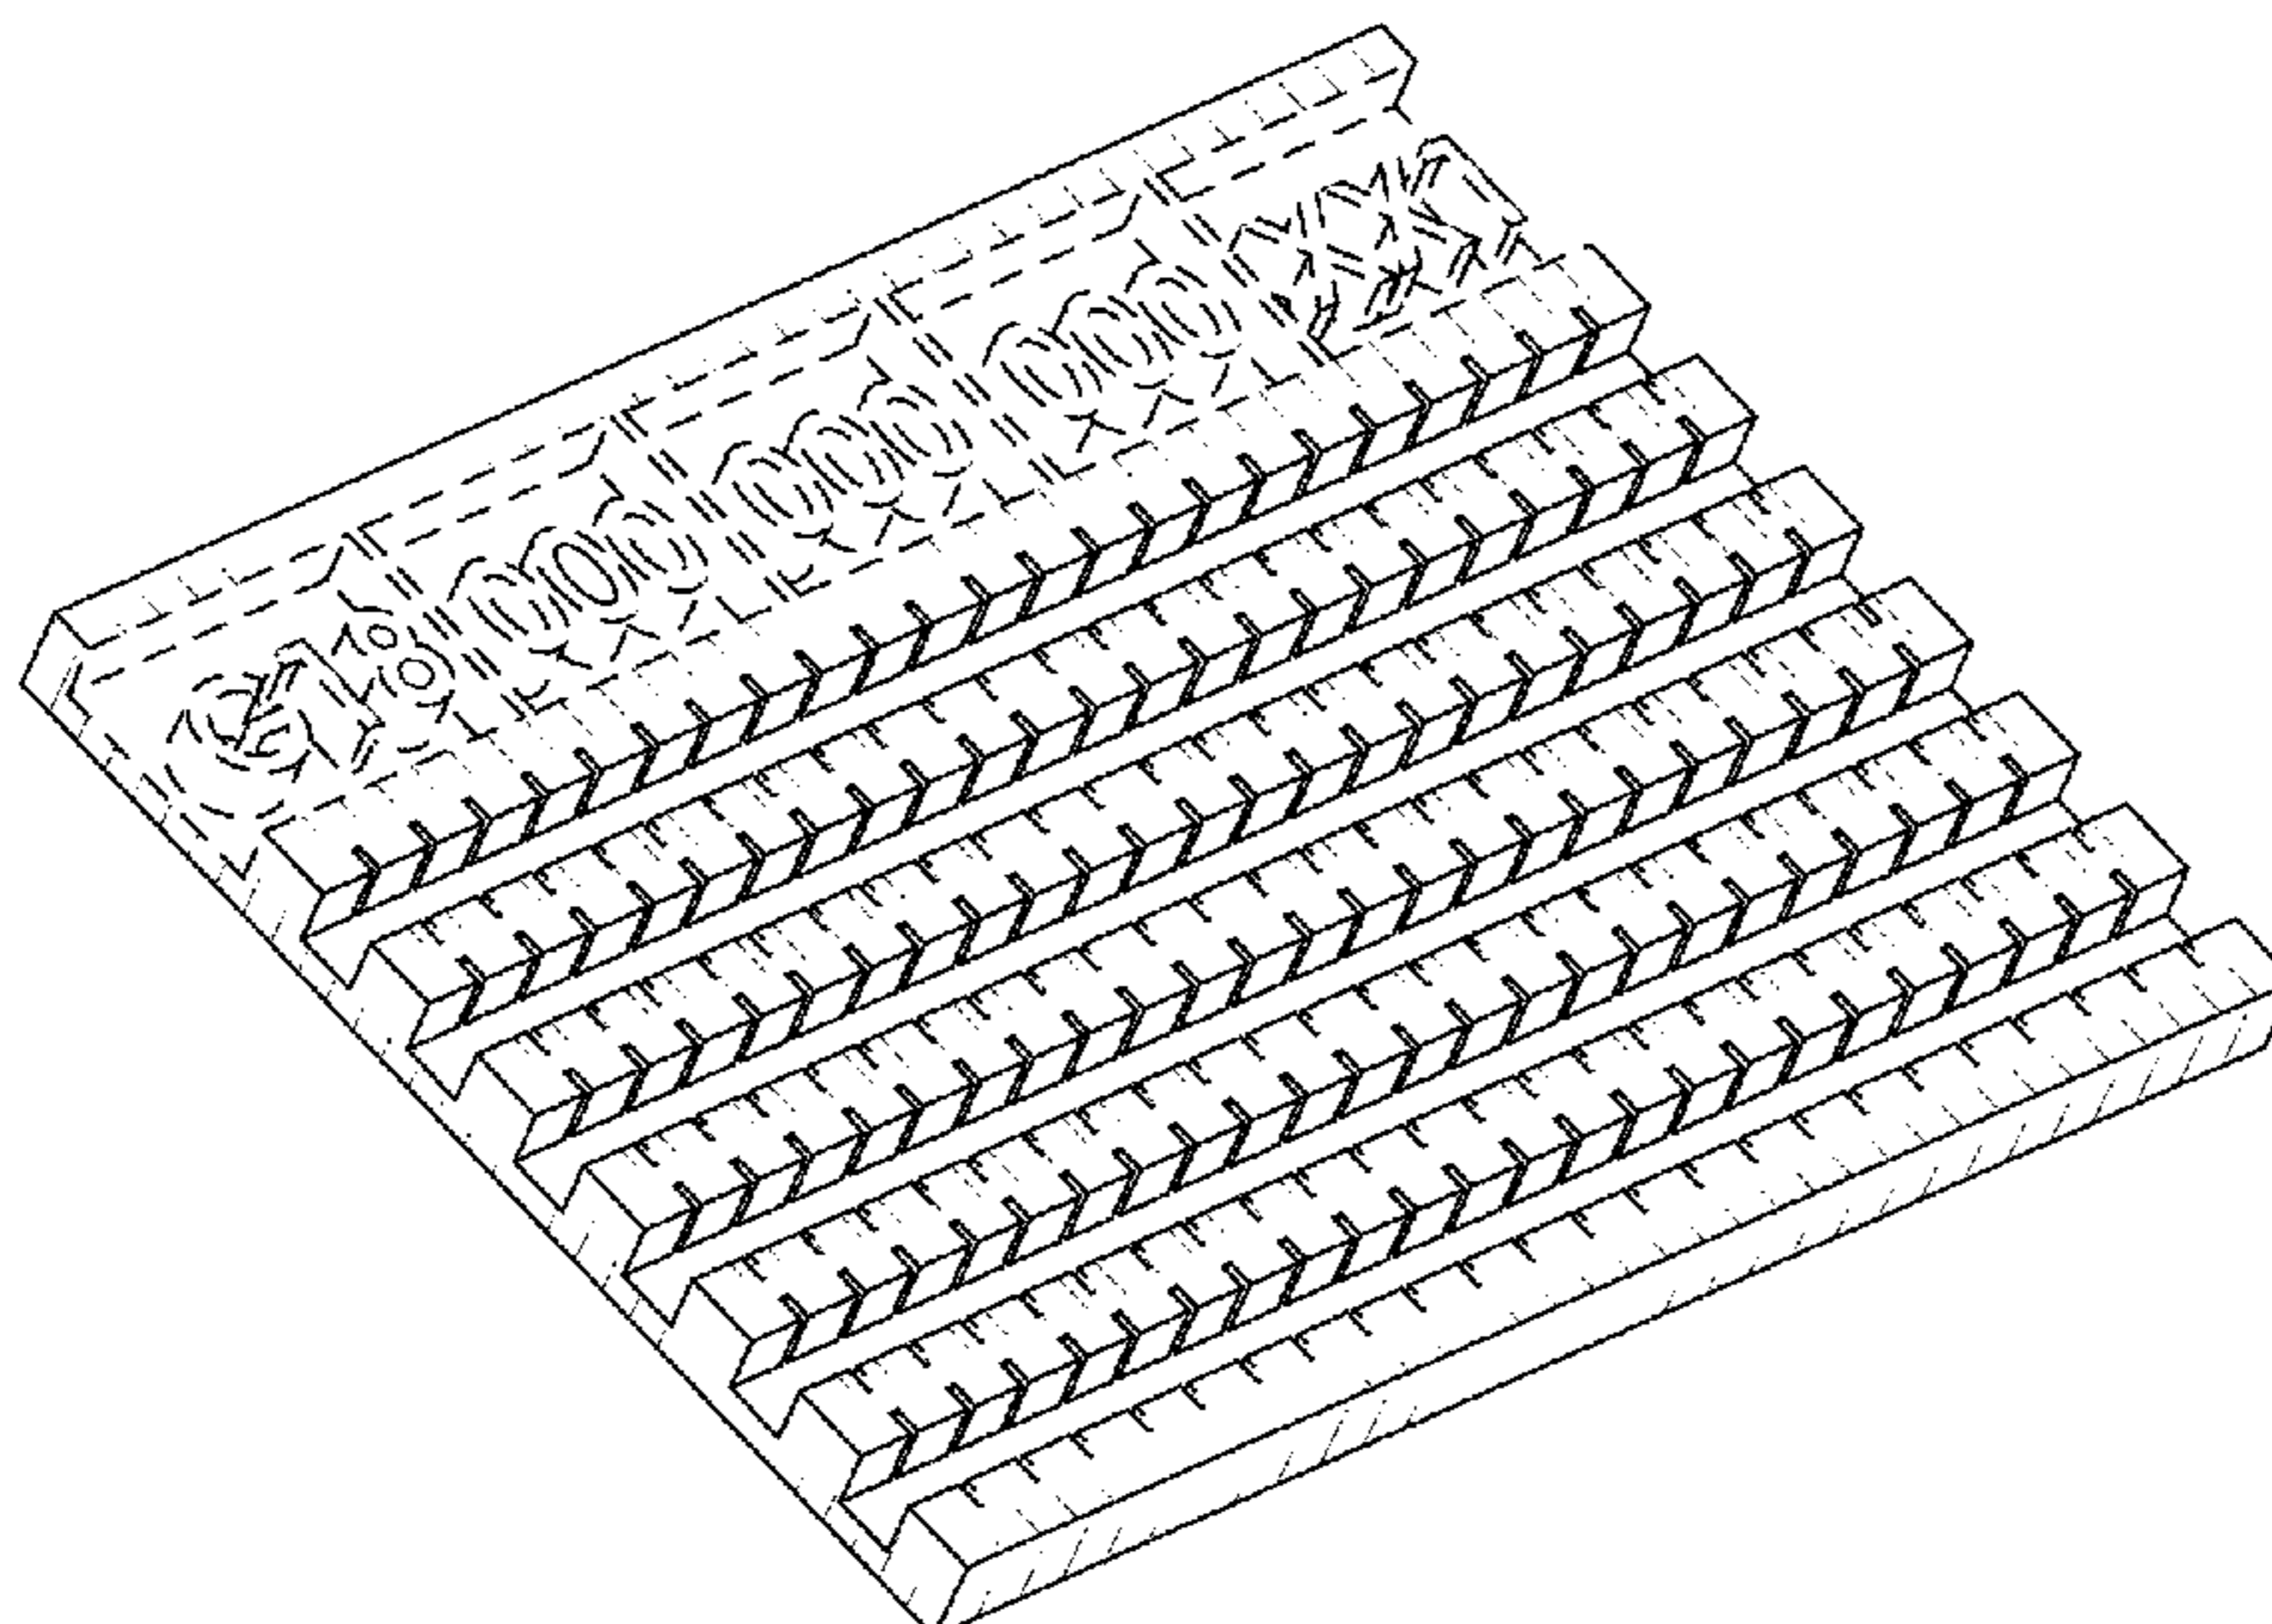


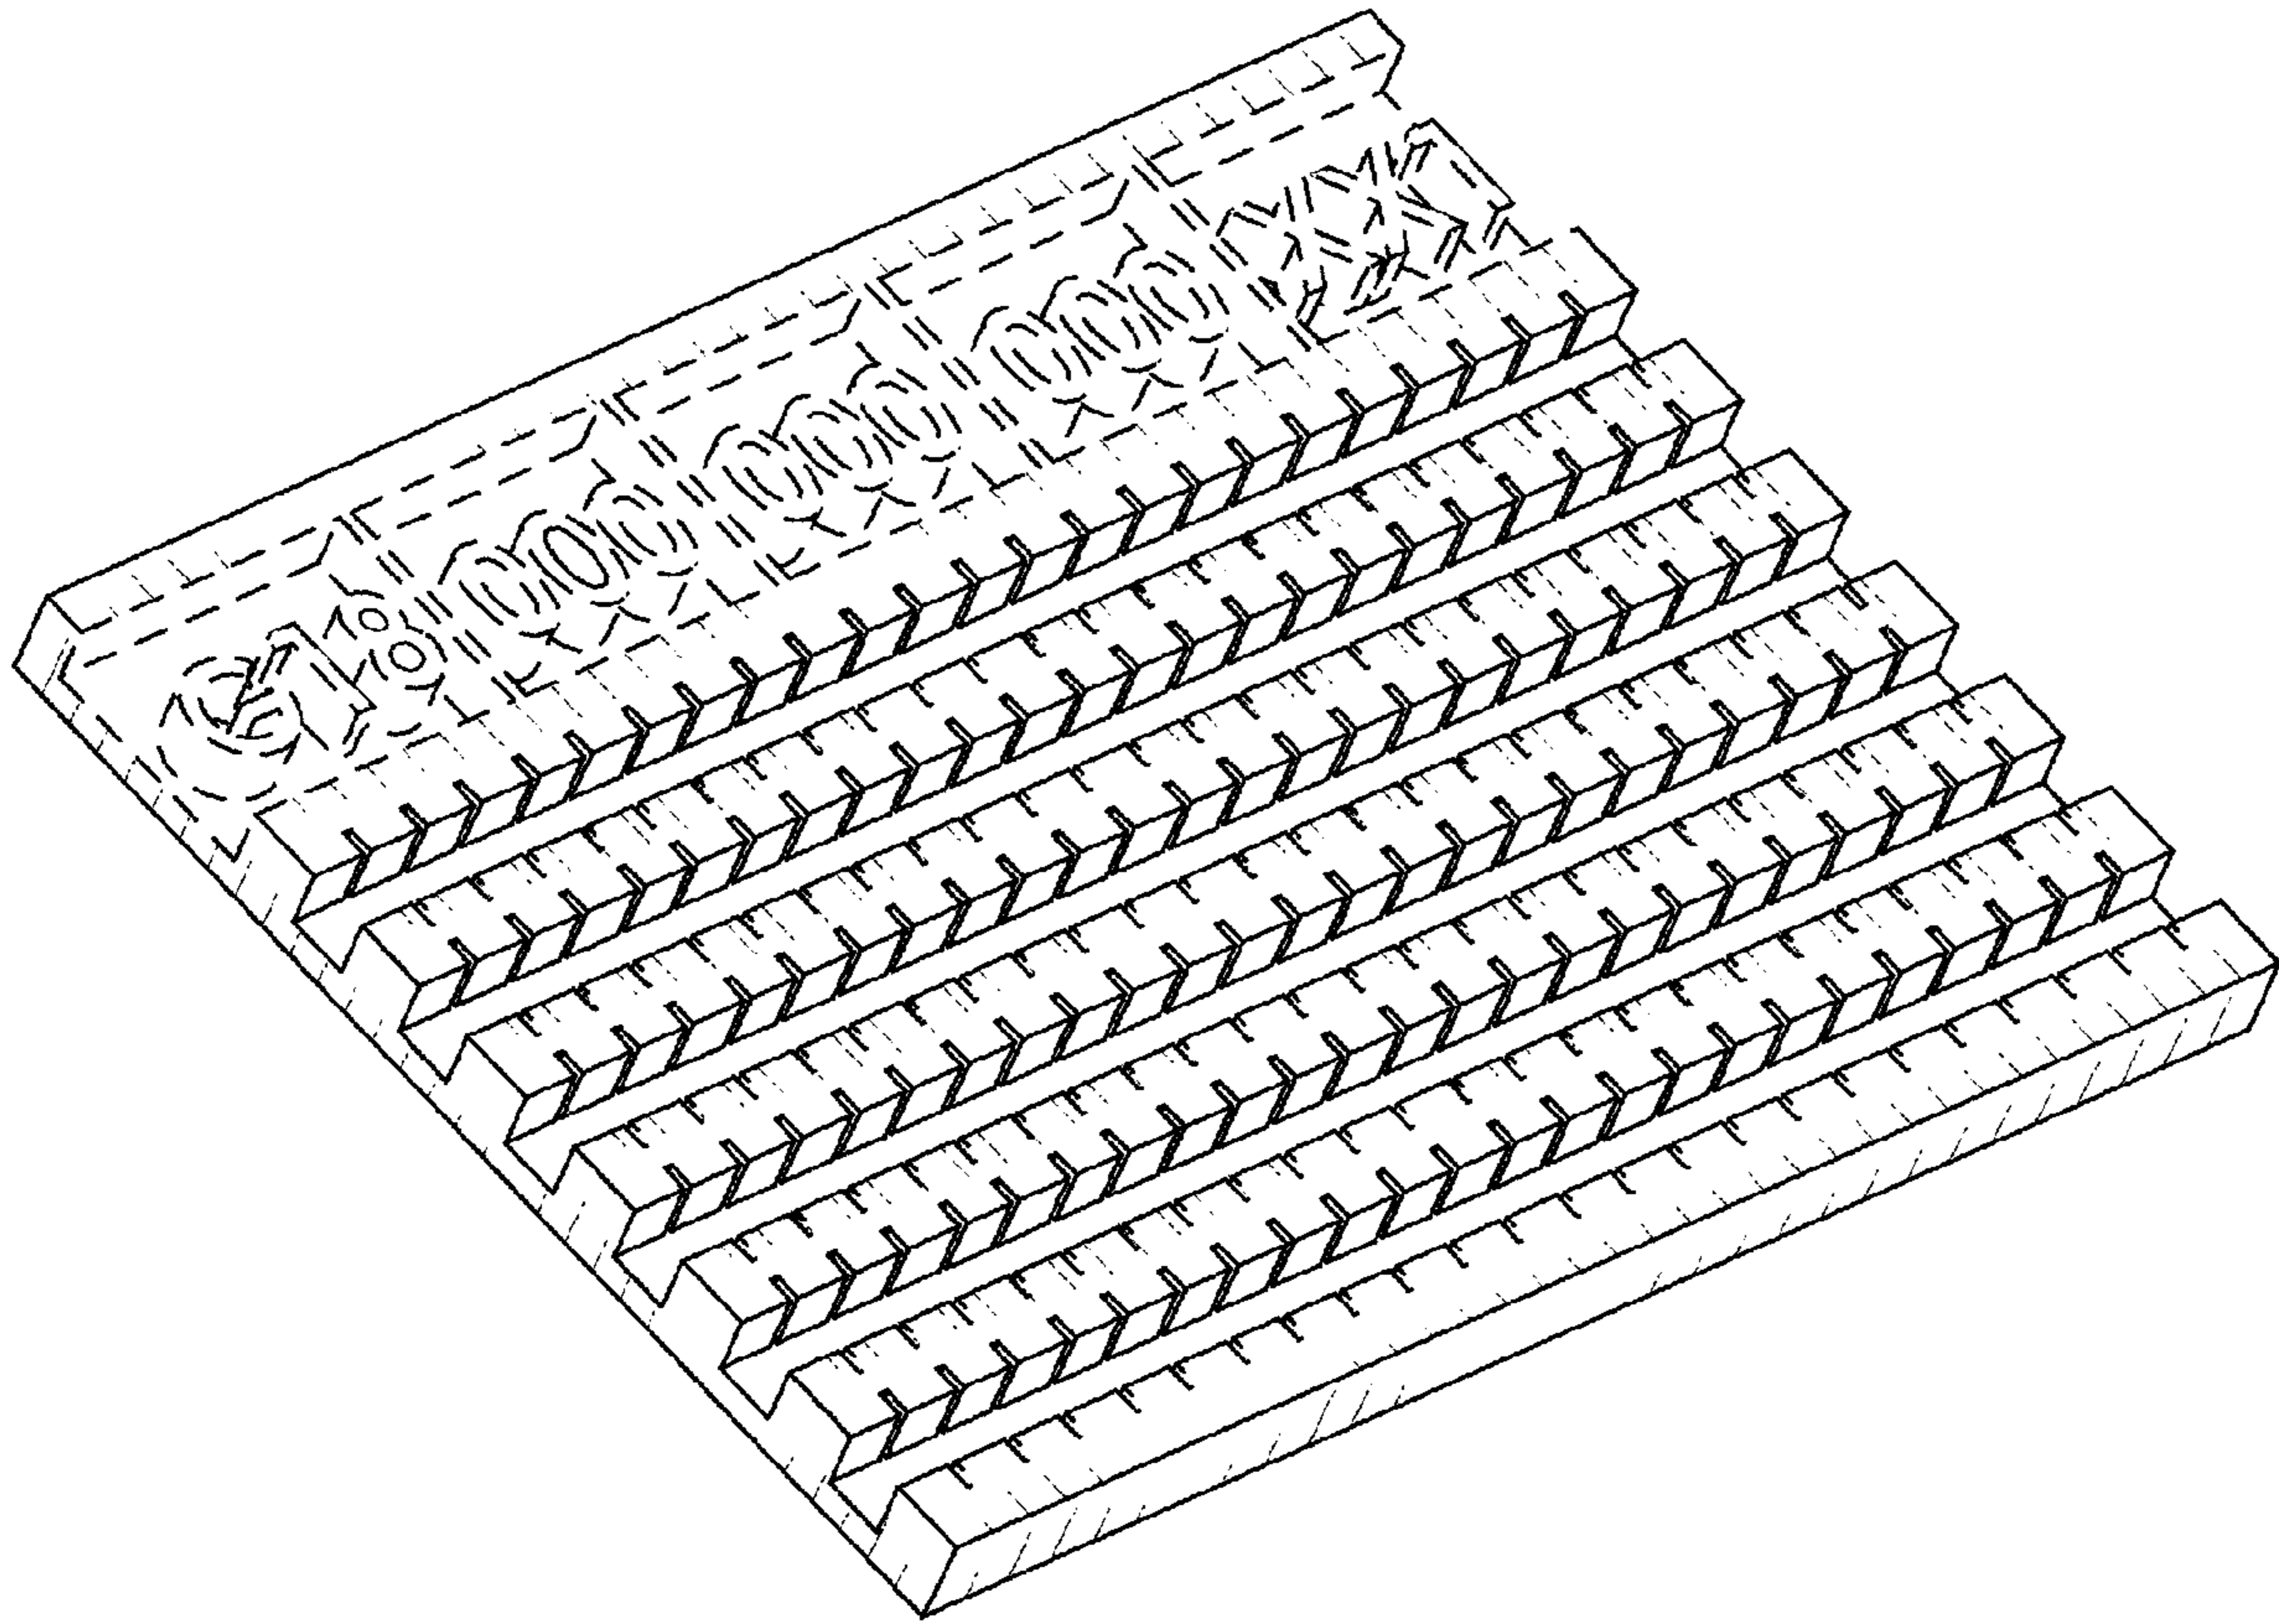


**FIG. 1**




**FIG. 2**

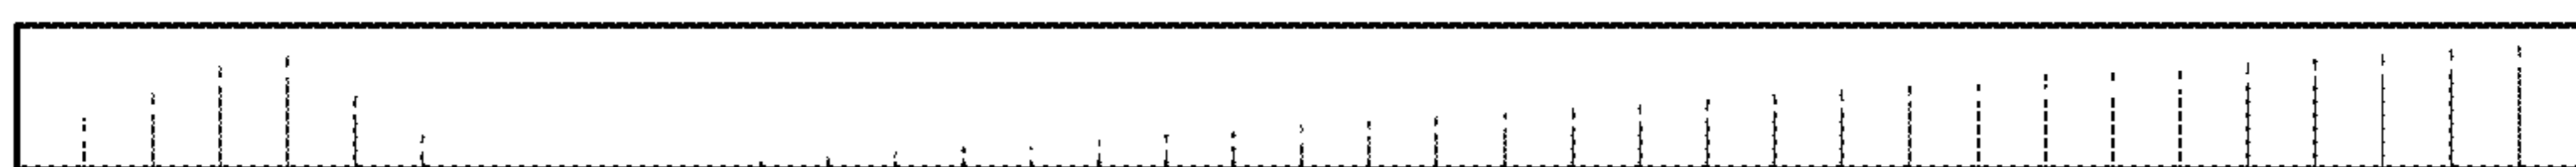


**FIG. 3**

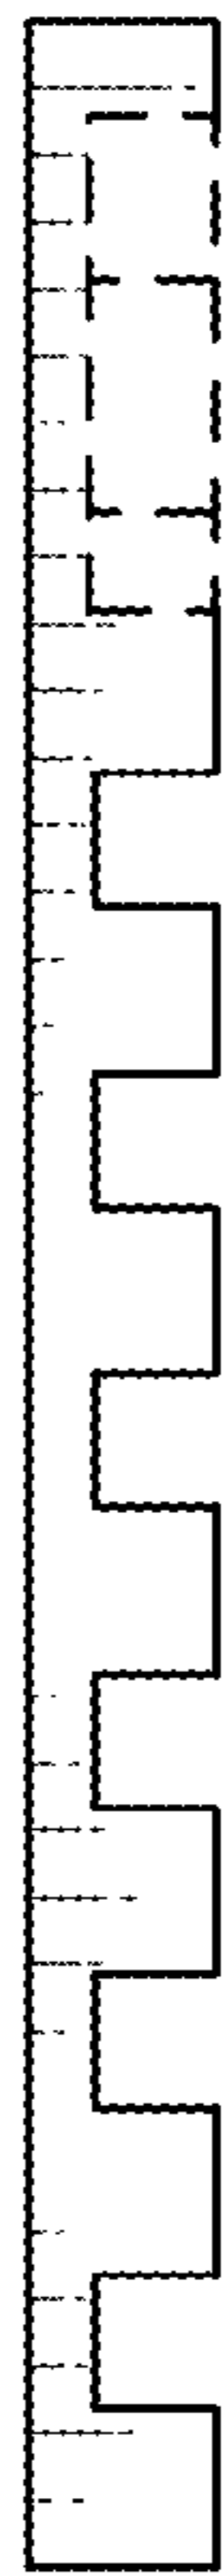


**FIG. 4**

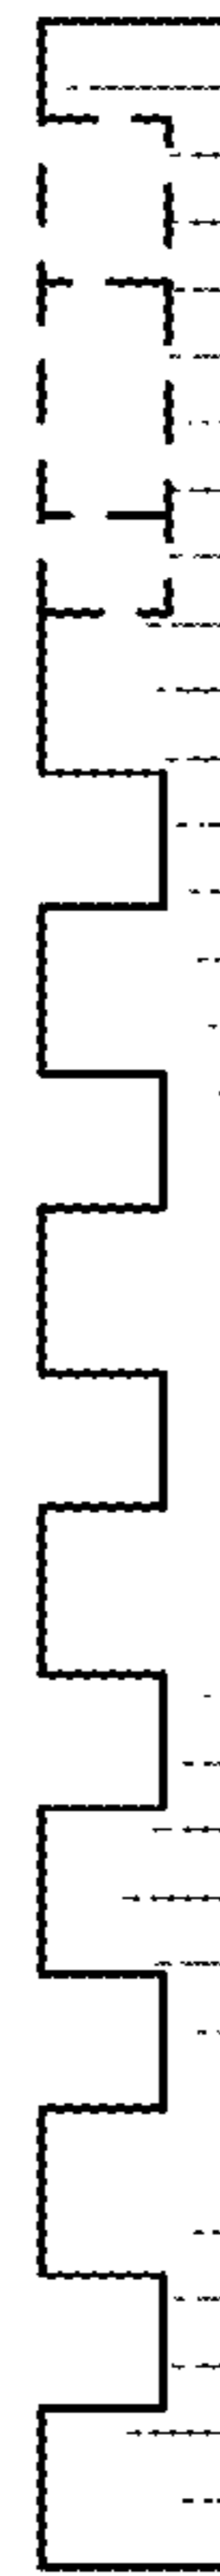

**FIG. 5**

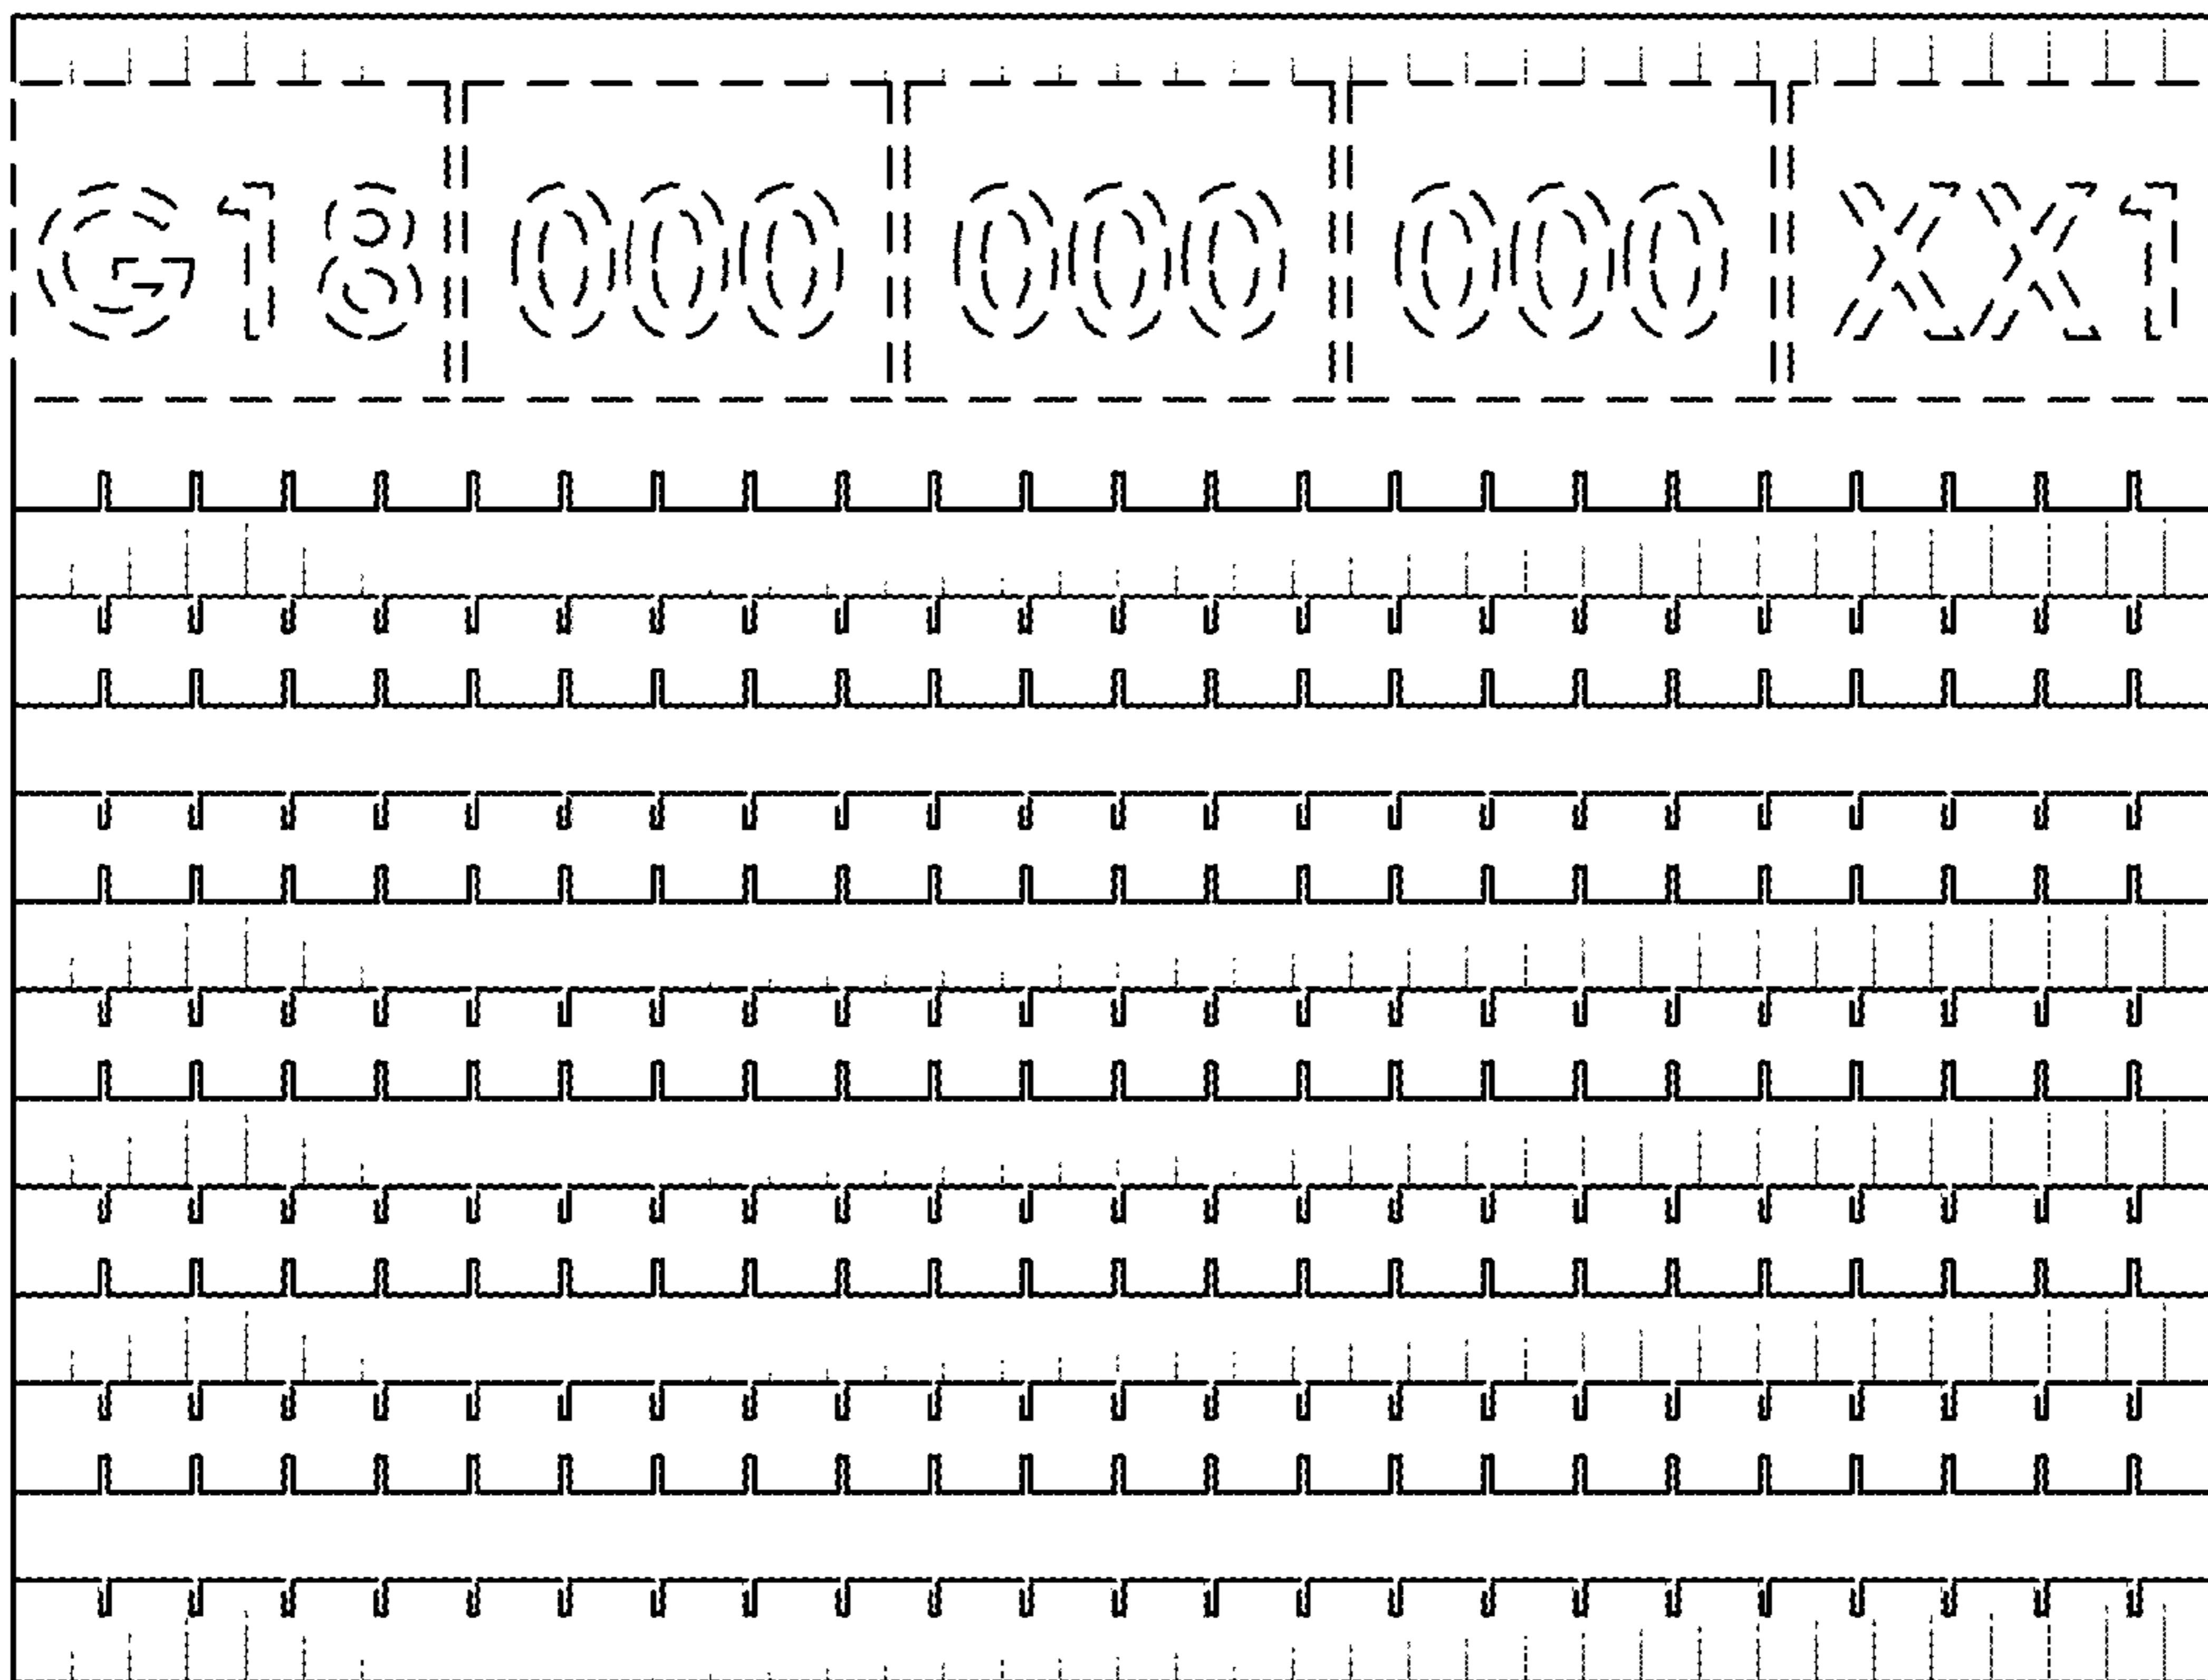

**FIG. 6**

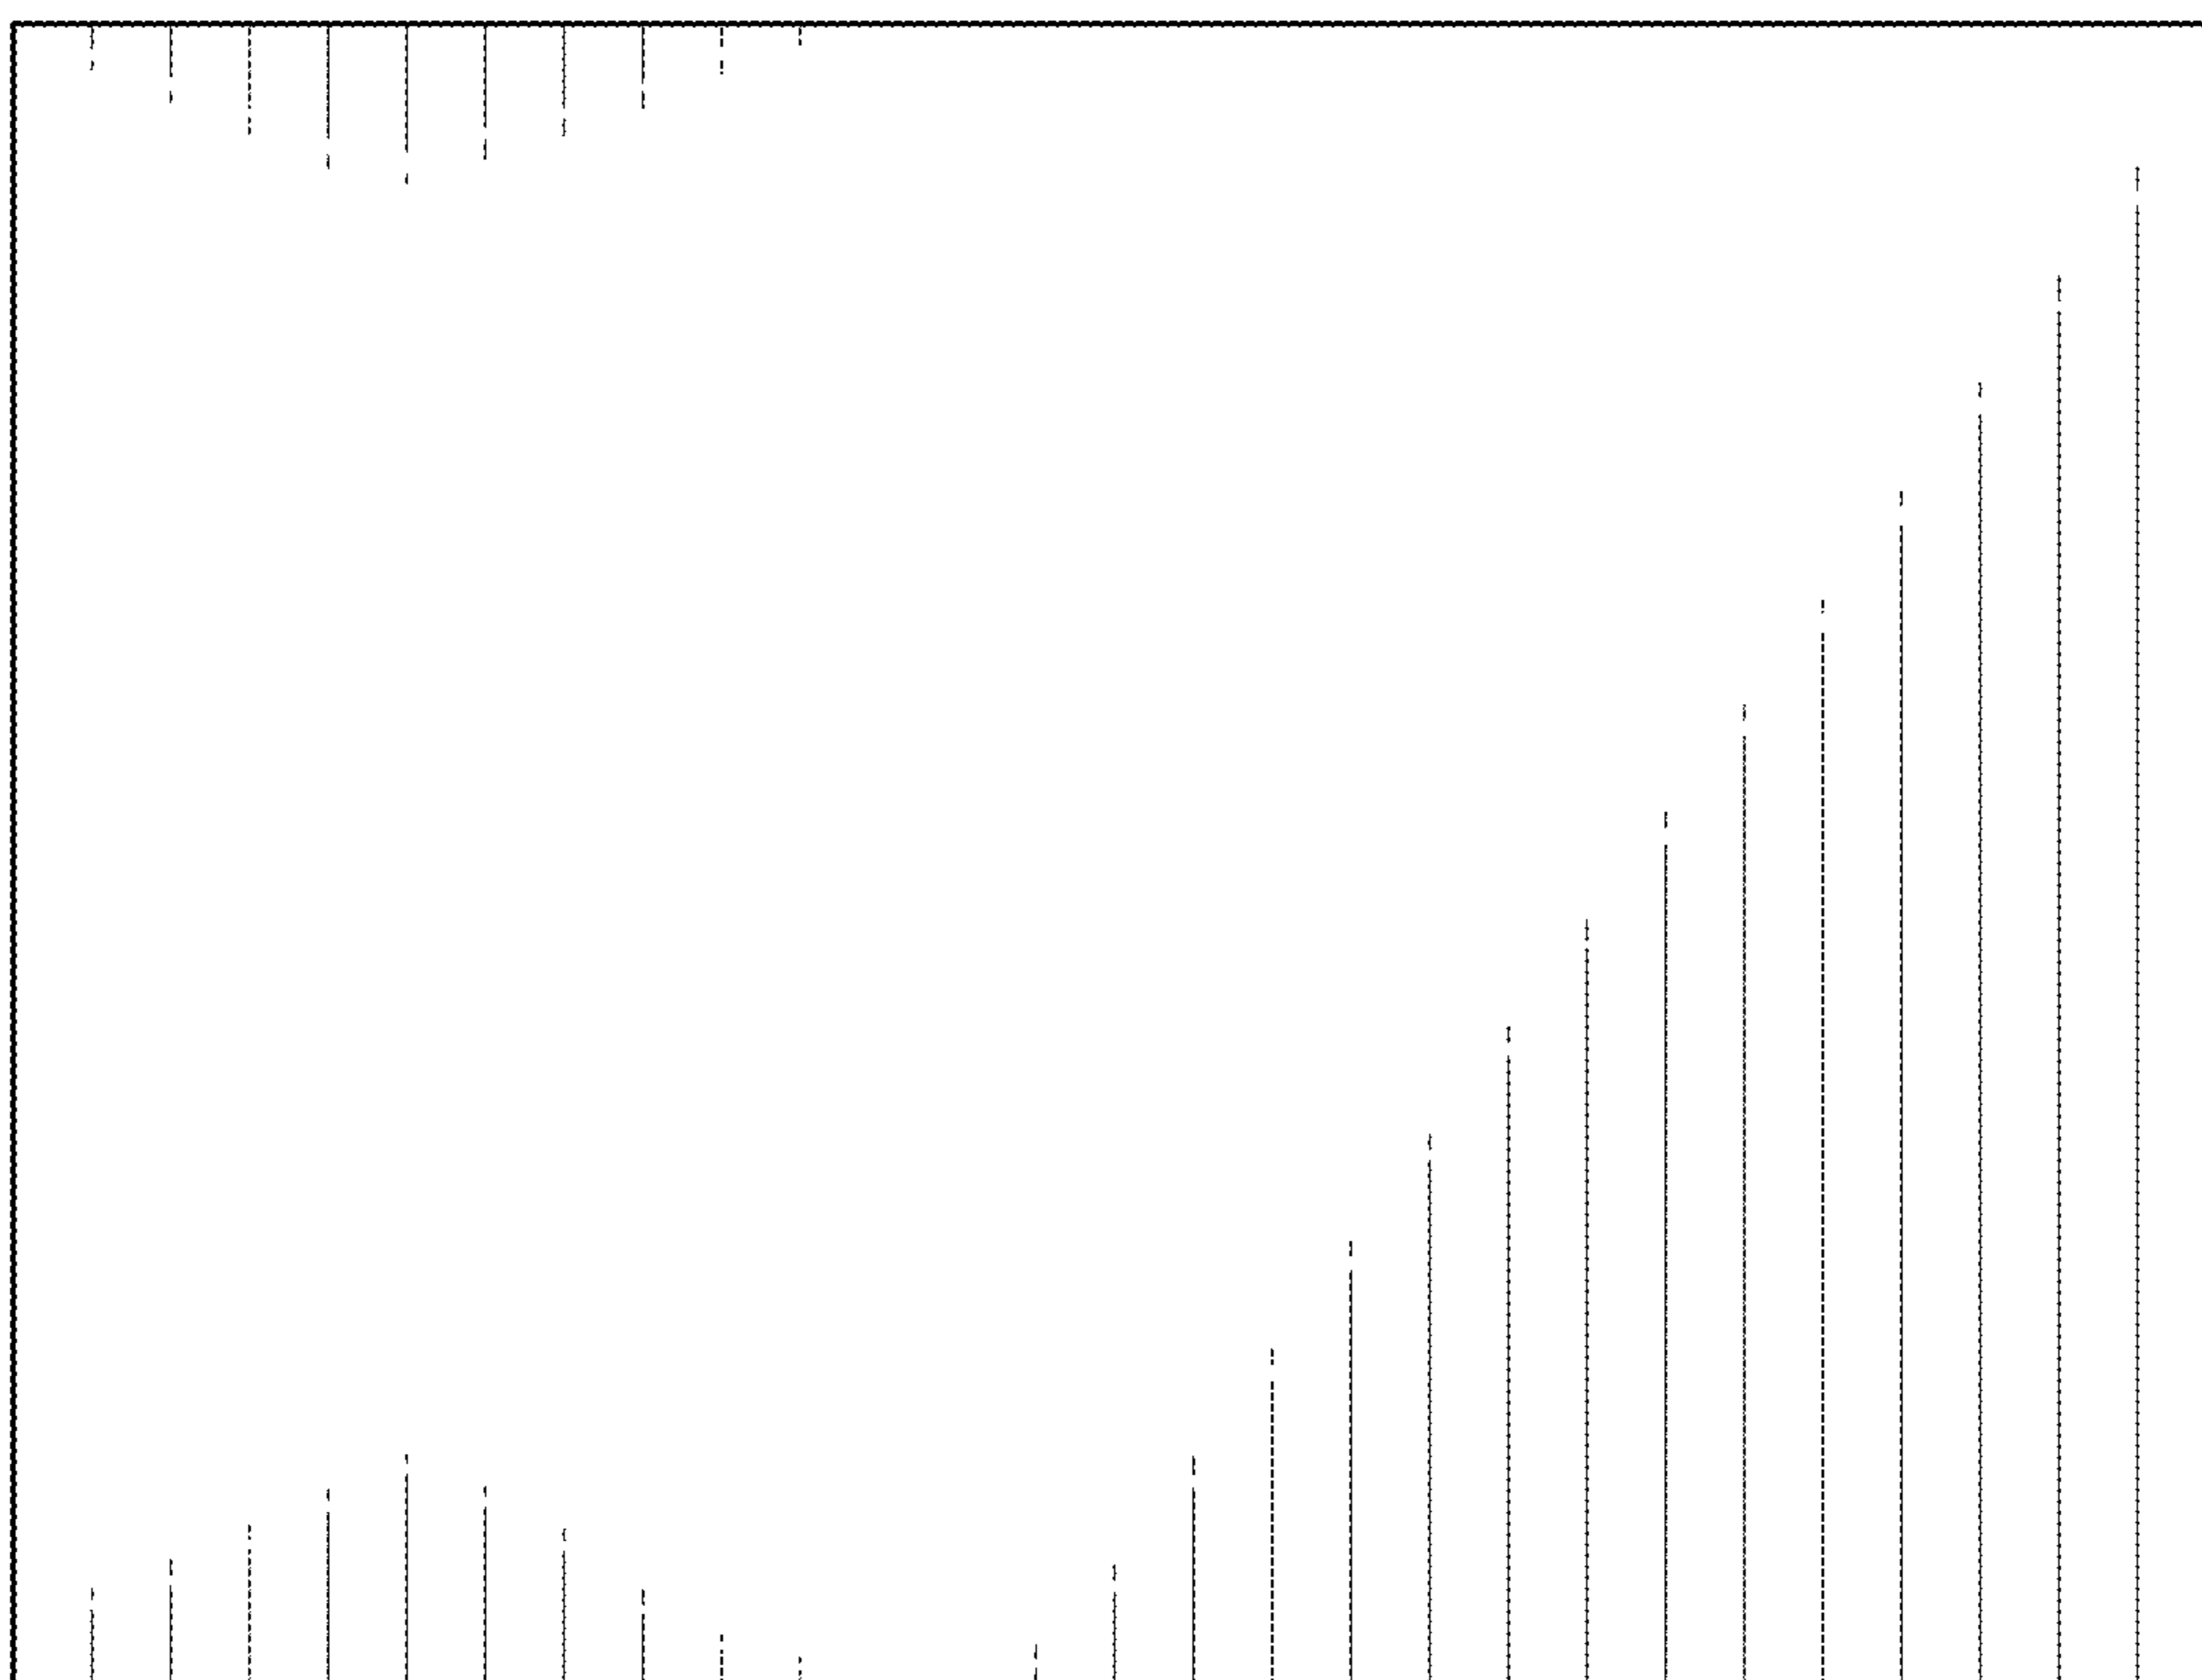

**FIG. 7**