



US00D914239S

(12) **United States Design Patent** (10) **Patent No.:** **US D914,239 S**
Kuitunen (45) **Date of Patent:** **** Mar. 23, 2021**

(54) **PIPETTE TIP RACK**

(71) Applicant: **Sartorius Biohit Liquid Handling Oy,**
Helsinki (FI)

(72) Inventor: **Tuomas Kuitunen,** Haarajoki (FI)

(**) Term: **15 Years**

(21) Appl. No.: **29/681,800**

(22) Filed: **Feb. 28, 2019**

(30) **Foreign Application Priority Data**

Aug. 29, 2018 (EM) 005623196-0001

Aug. 29, 2018 (EM) 005623196-0002

(Continued)

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/230**

(58) **Field of Classification Search**

USPC D24/108, 127-130, 216, 222, 224-232;

D9/756-758; D6/406.1-406.3, 406.6;

D19/37; D3/203.1, 304

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D271,239 S * 11/1983 Lemieux D24/230

D679,025 S * 3/2013 Motadel D24/227

(Continued)

OTHER PUBLICATIONS

Thermo Scientific™ Finntip™ Flex Filtered Pipette Tips. Online,
published date unknown. Retrieved on Aug. 7, 2020 from URL:
<https://www.fishersci.se/shop/products/finntip-flex-filter-pipette-tips/p-4525516>.*

(Continued)

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Jeffrey Joyce, Esq.

(57) **CLAIM**

The ornamental design for a pipette tip rack, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the first embodiment of a pipette tip rack according to the invention showing the side, front and top.

FIG. 2 is a perspective view of the first embodiment of the pipette tip rack showing the front, top and side.

FIG. 3 is a perspective view of the first embodiment of the pipette tip rack showing the top, front and side.

FIG. 4 is a bottom view of the first embodiment of the pipette tip rack.

FIG. 5 is a perspective view of the bottom of the first embodiment of the pipette tip rack.

FIG. 6 is a right side view of the first embodiment of the pipette tip rack.

FIG. 7 is a left side view of first embodiment of the pipette tip rack.

FIG. 8 is a front side view of the first embodiment of the pipette tip rack.

FIG. 9 is a rear view of the first embodiment of the pipette tip rack.

FIG. 10 is a top view of the first embodiment of the pipette tip rack

FIG. 11 is a perspective view of the second embodiment of the pipette tip rack according to the invention showing the side, top, and front.

FIG. 12 is a perspective view of the second embodiment of the pipette tip rack showing the front, top and side.

FIG. 13 is a perspective view of the second embodiment of the pipette tip rack showing the top, front and side.

FIG. 14 is a bottom view of the second embodiment of the pipette tip rack.

FIG. 15 is a perspective view of the bottom of the second embodiment of the pipette tip rack.

FIG. 16 is a right side view of the second embodiment of the pipette tip rack.

(Continued)

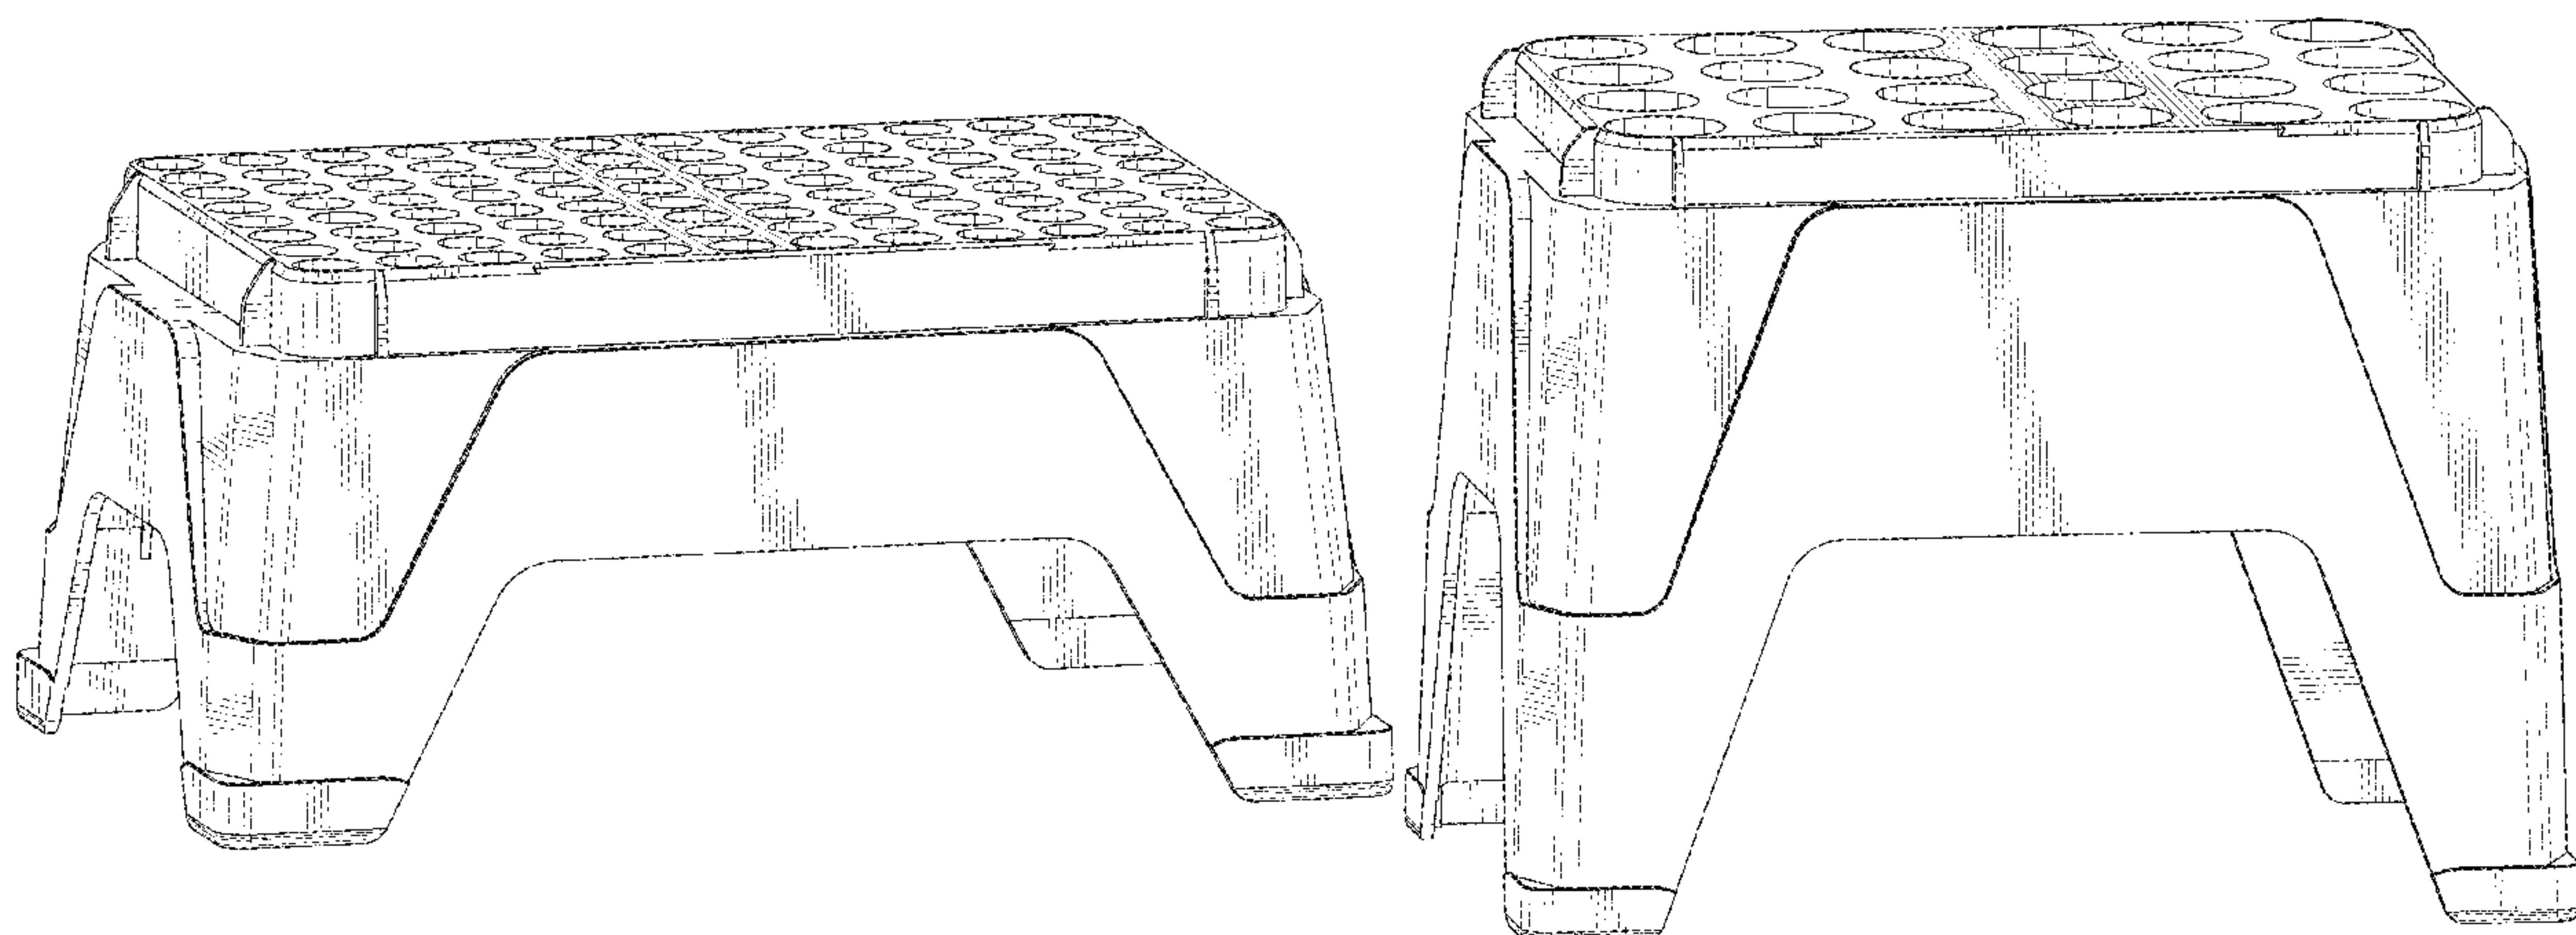


FIG. 17 is a left side view of second embodiment of the pipette tip rack.

FIG. 18 is a front end view of the second embodiment of the pipette tip rack.

FIG. 19 is a rear end view of the second embodiment of the pipette tip rack.

FIG. 20 is a top view of the second embodiment of the pipette tip rack.

FIG. 21 is a perspective view of the third embodiment of the pipette tip rack according to the invention showing the side, front and top.

FIG. 22 is a perspective view of the third embodiment of the pipette tip rack showing the front, top and side.

FIG. 23 is a perspective view of the third embodiment of the pipette tip rack showing the top, front and side.

FIG. 24 is a bottom view of the third embodiment of the pipette tip rack.

FIG. 25 is a perspective view of the bottom of the third embodiment of the pipette tip rack.

FIG. 26 is a right side view of the third embodiment of the pipette tip rack.

FIG. 27 is a left side view of third embodiment of the pipette tip rack.

FIG. 28 is a front end view of the third embodiment of the pipette tip rack.

FIG. 29 is a rear end view of the third embodiment of the pipette tip rack.

FIG. 30 is a top view of the third embodiment of the pipette tip rack.

FIG. 31 is a perspective view of a stack of pipette tip racks showing the side, front and top of the stack, each individual pipette tip rack in the stack having the ornamental appearance shown in the first embodiment of the pipette tip rack.

FIG. 32 is a perspective view of the stack of pipette tip racks showing the front, top and side.

FIG. 33 is a bottom view of the stack of pipette tip racks.

FIG. 34 is a right side view of the stack of pipette tip racks.

FIG. 35 is a left side view of the stack of pipette tip racks.

FIG. 36 is a front end view of the stack of pipette tip racks.

FIG. 37 is a rear end view of the stack of pipette tip racks; and,

FIG. 38 is a top view of the stack of pipette tip racks.

The broken lines are for the purpose of illustrating the environment of the article only and form no part of the claimed design.

1 Claim, 38 Drawing Sheets

(30) Foreign Application Priority Data

Aug. 29, 2018 (EM) 005623196-0003

Aug. 29, 2018 (EM) 005623196-0004

(58) Field of Classification Search

CPC B01L 9/543

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D699,370	S *	2/2014	Motadel		D24/229
D724,236	S *	3/2015	Motadel		D24/227
D873,436	S *	1/2020	O'Connell		D24/229
D875,968	S *	2/2020	Curry		D24/227
D886,321	S *	6/2020	Motadel		D24/229
D888,280	S *	6/2020	Motadel		D24/229
2011/0306051	A1 *	12/2011	Belz		G01N 35/0098 435/6.12
2014/0234182	A1 *	8/2014	Motadel		B01L 9/543 422/526
2014/0308181	A1 *	10/2014	Blumentritt		B01L 9/543 422/560
2017/0008001	A1 *	1/2017	Motadel		B01L 9/543
2017/0043346	A1 *	2/2017	Welch		B65D 25/108
2019/0009277	A1 *	1/2019	Kofler		B01L 9/543

OTHER PUBLICATIONS

Aerofit Aerobic Small Stepper for Strength. Online, published date unknown. Retrieved on Aug. 17, 2020 from URL: <https://www.indiamart.com/proddetail/aerobic-small-stepper-21654155148.html>.*

* cited by examiner

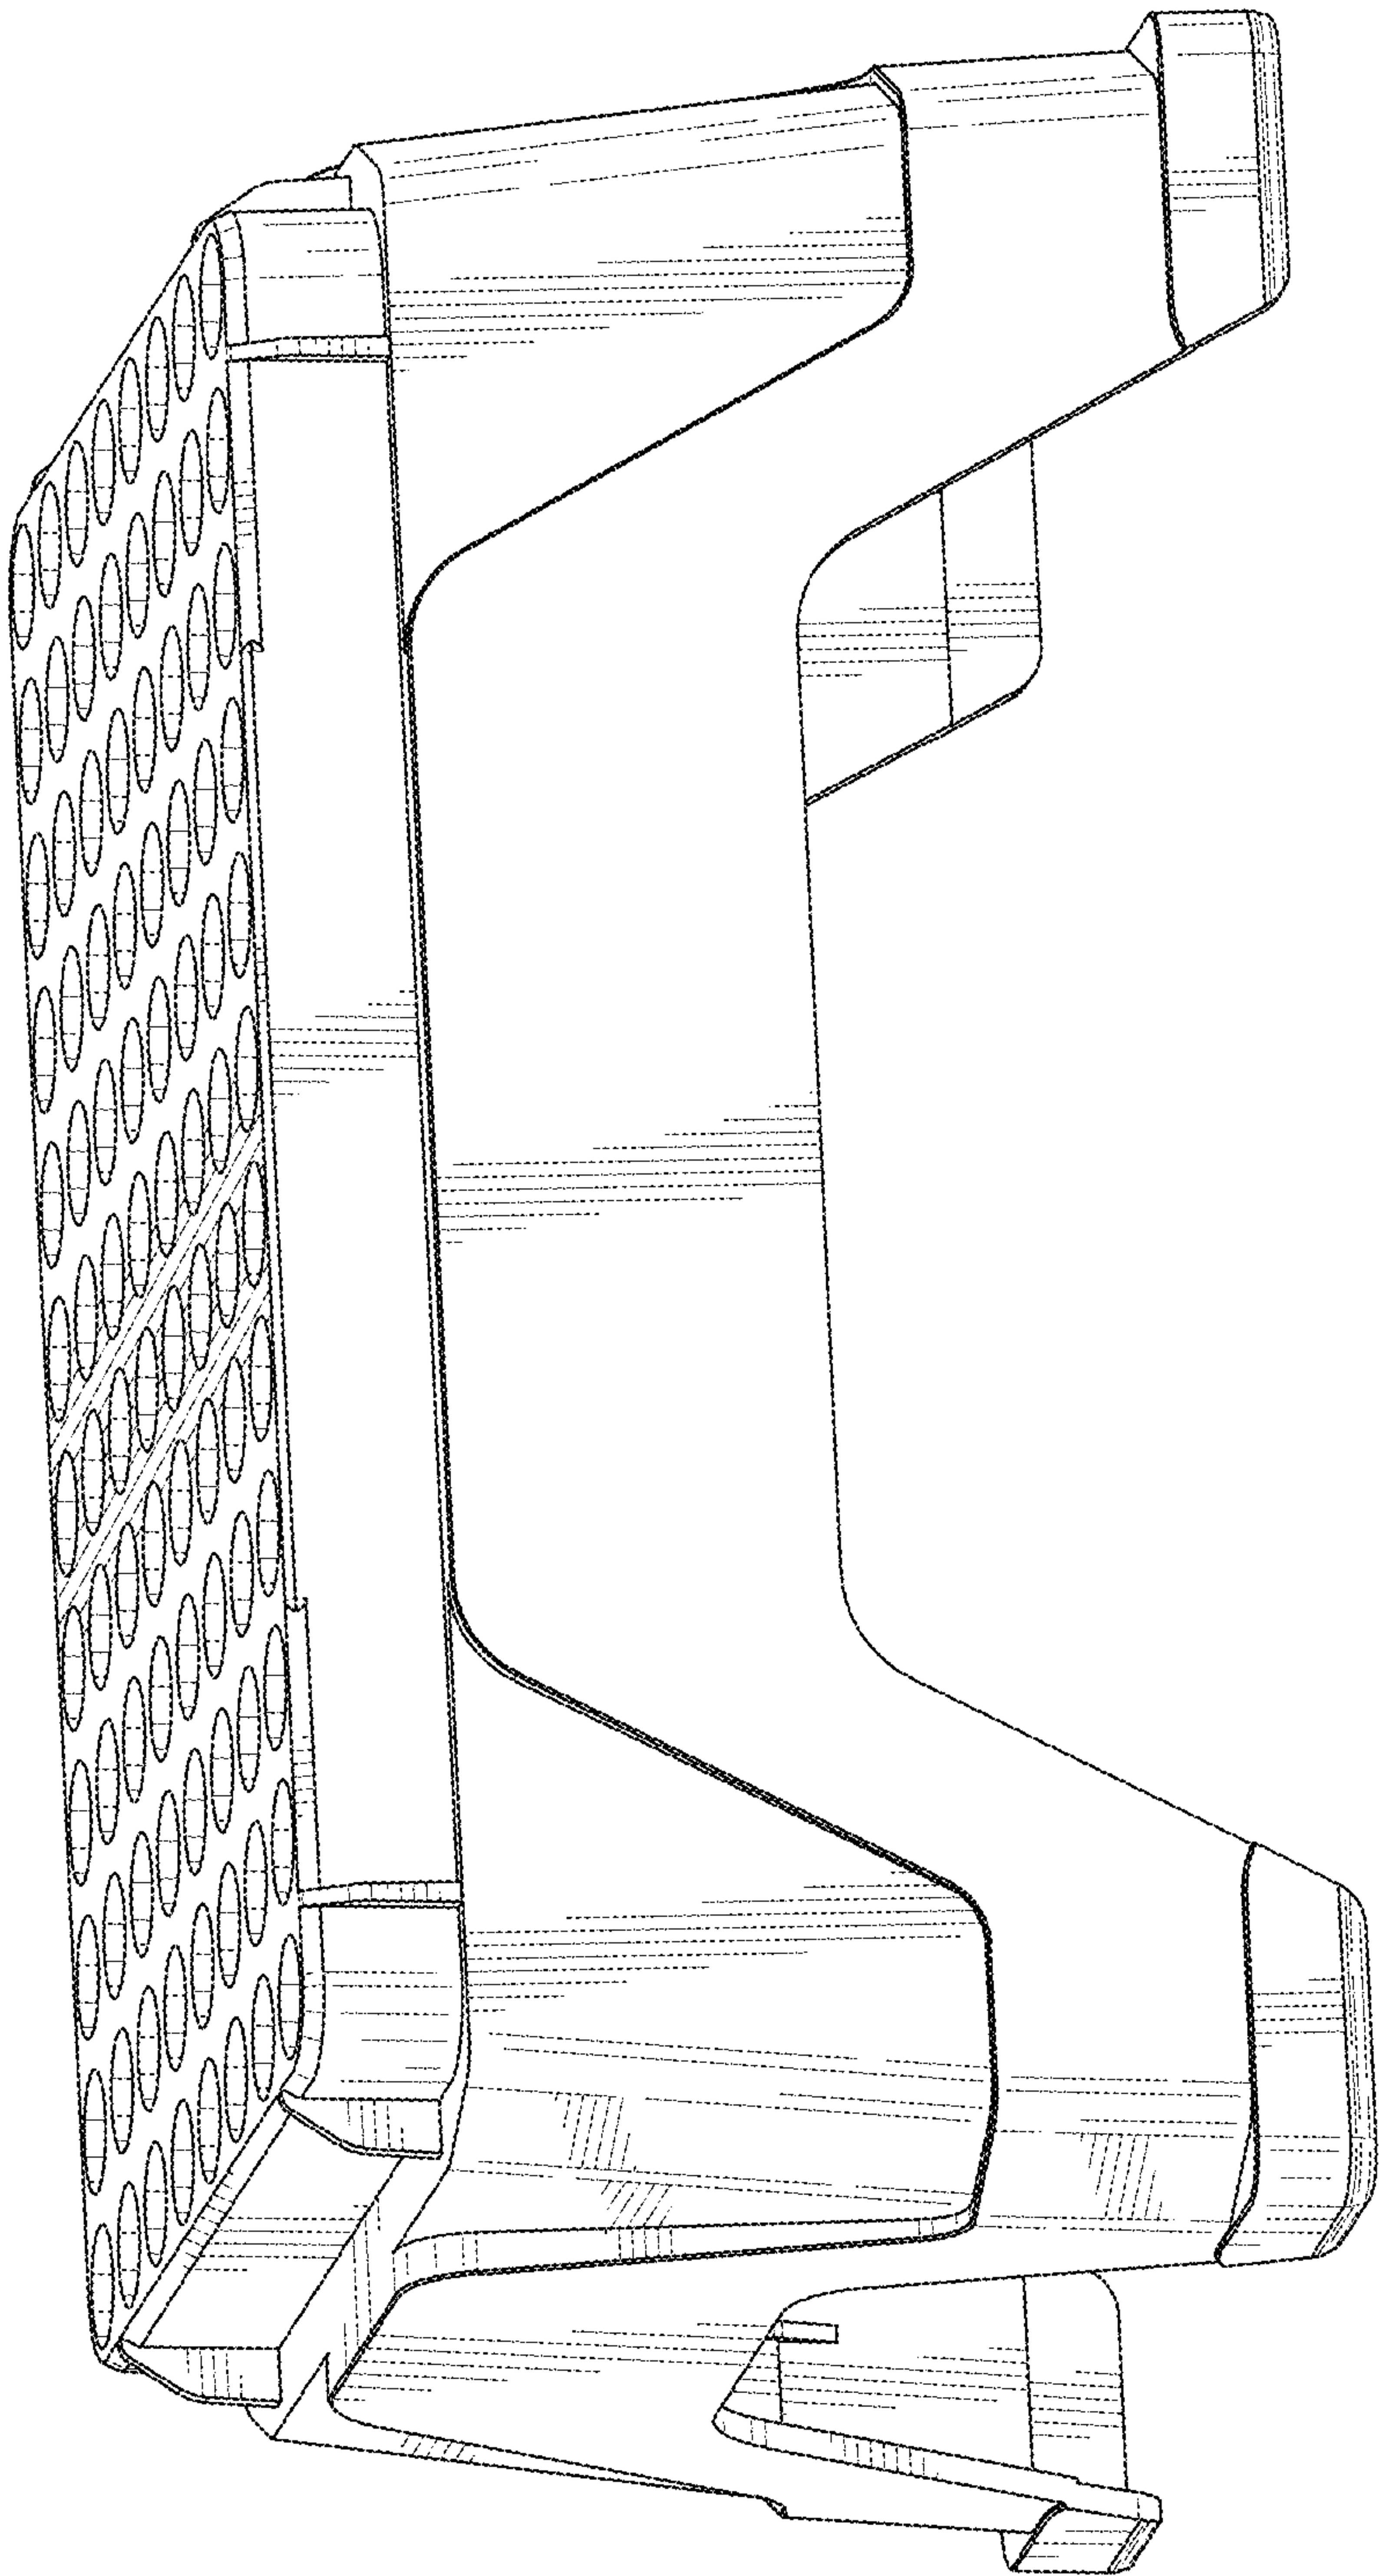


FIG. 1

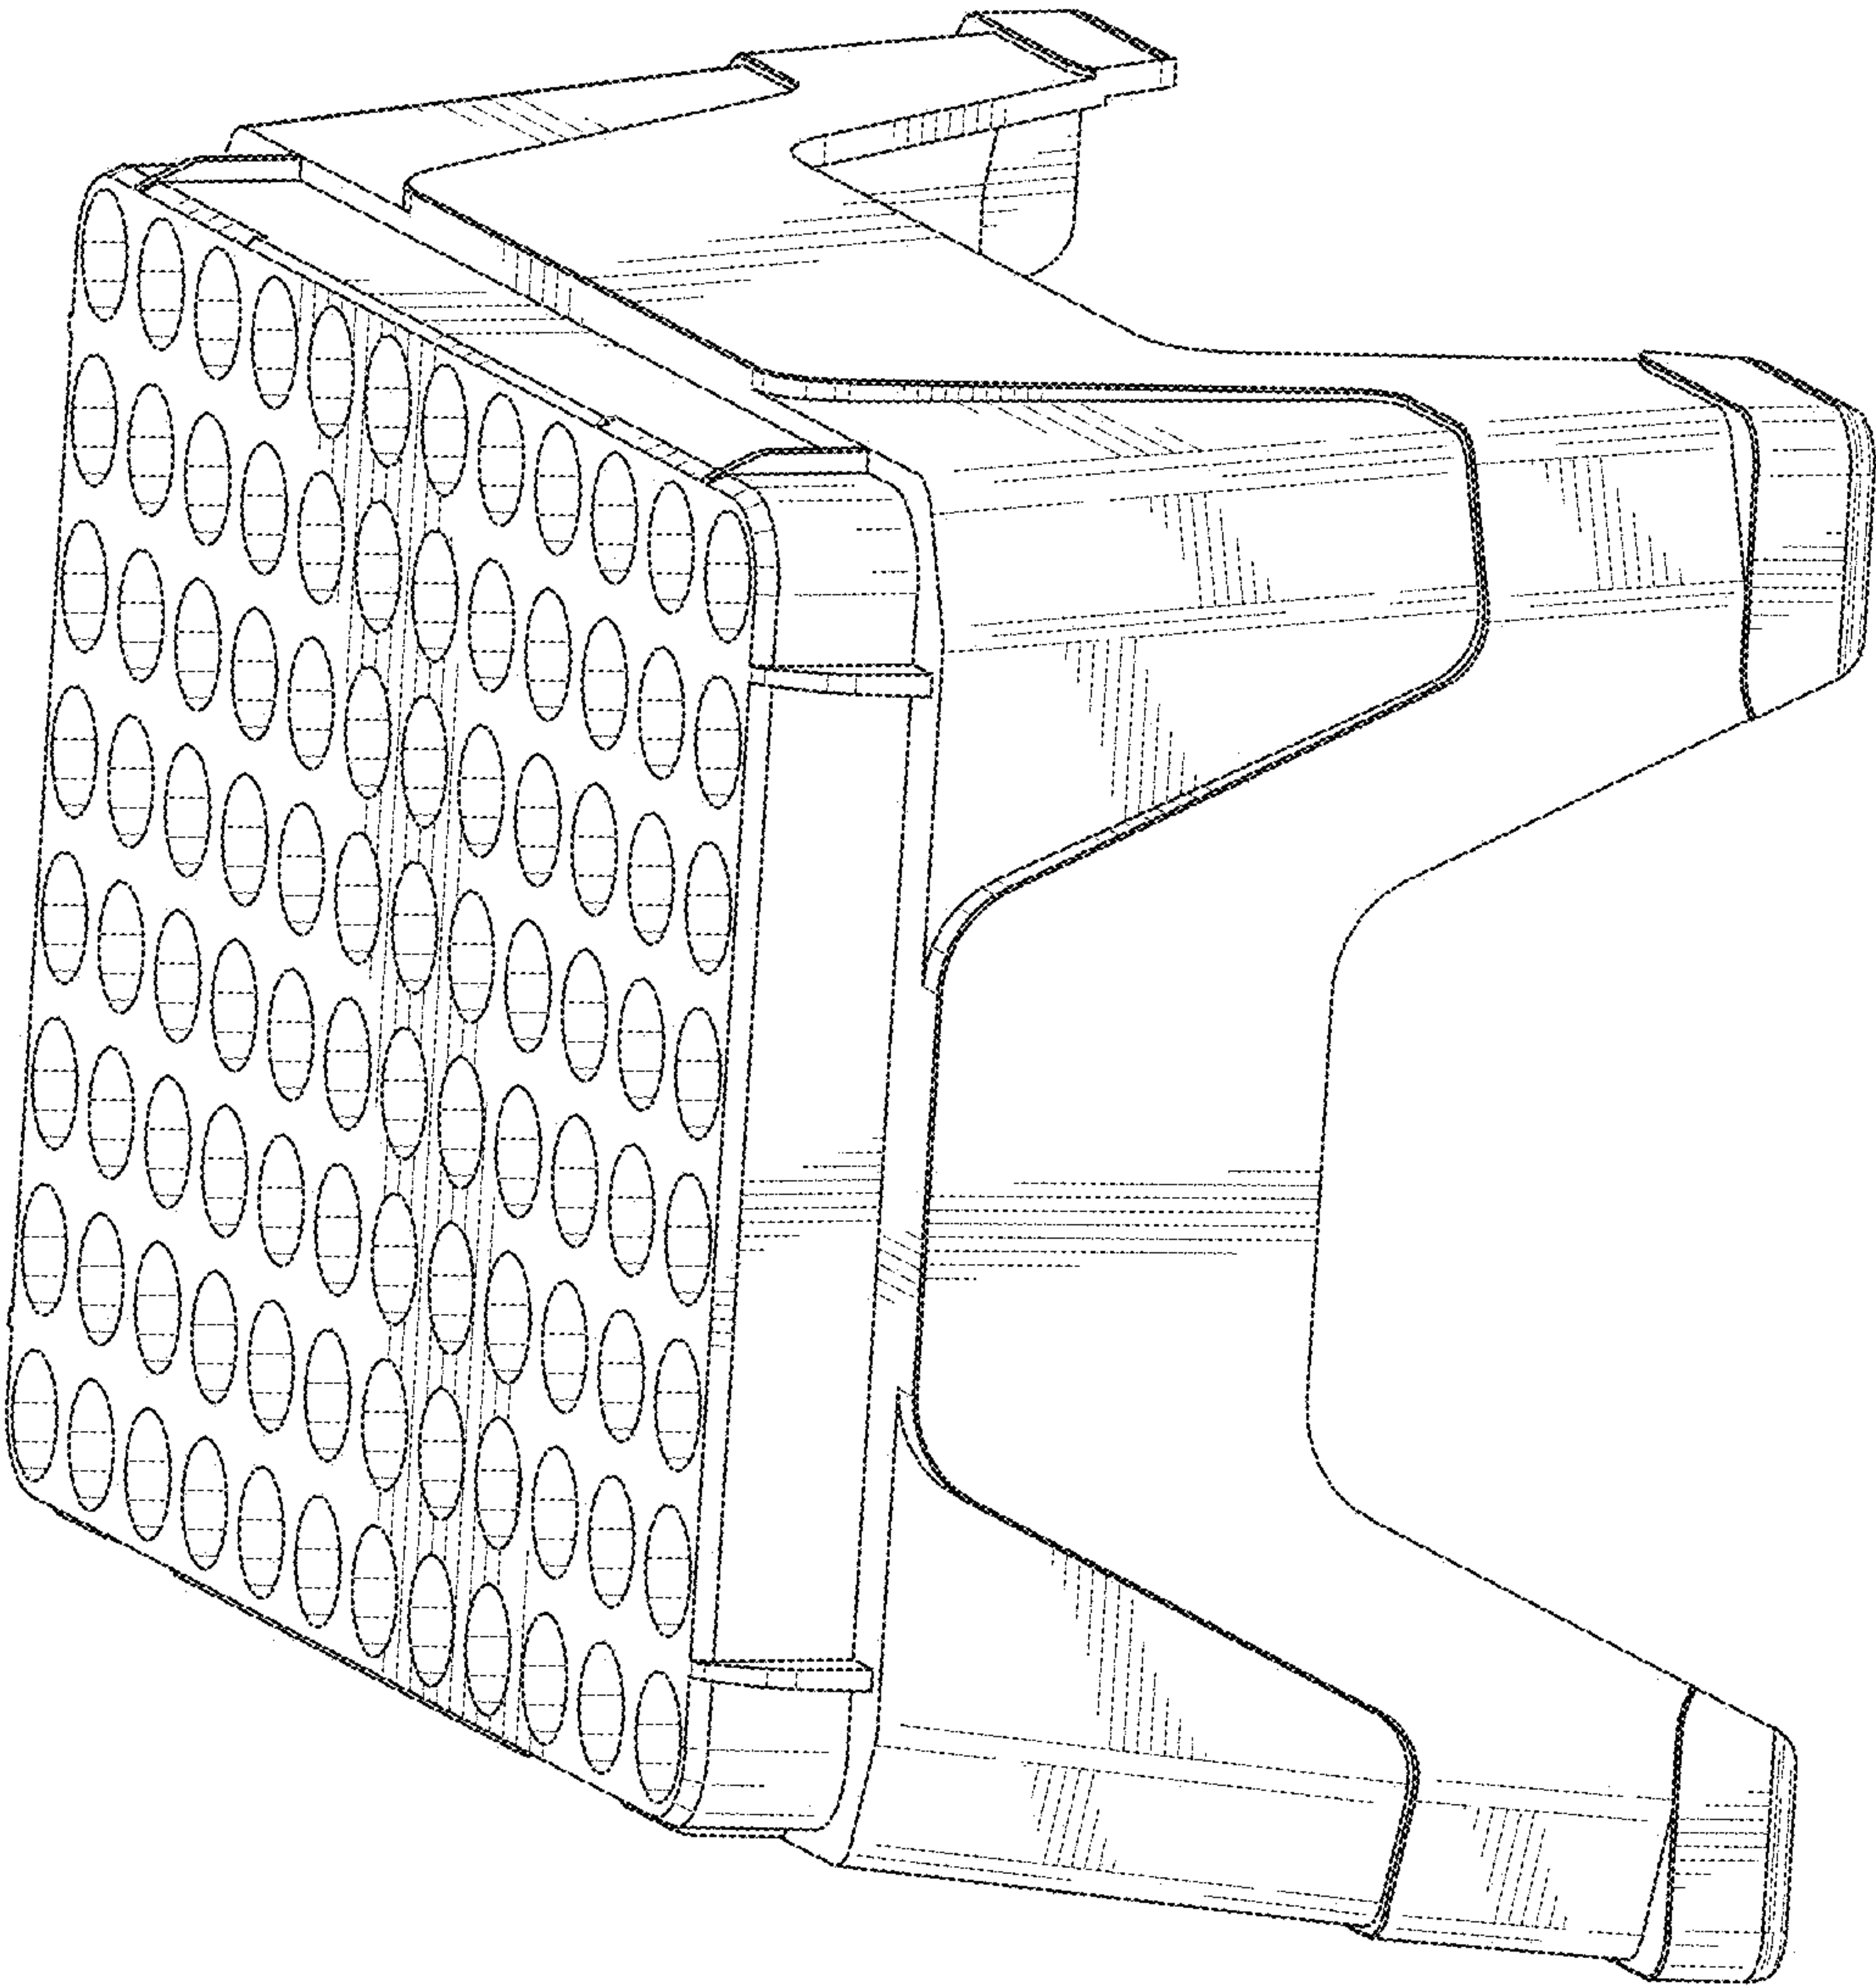


FIG. 2

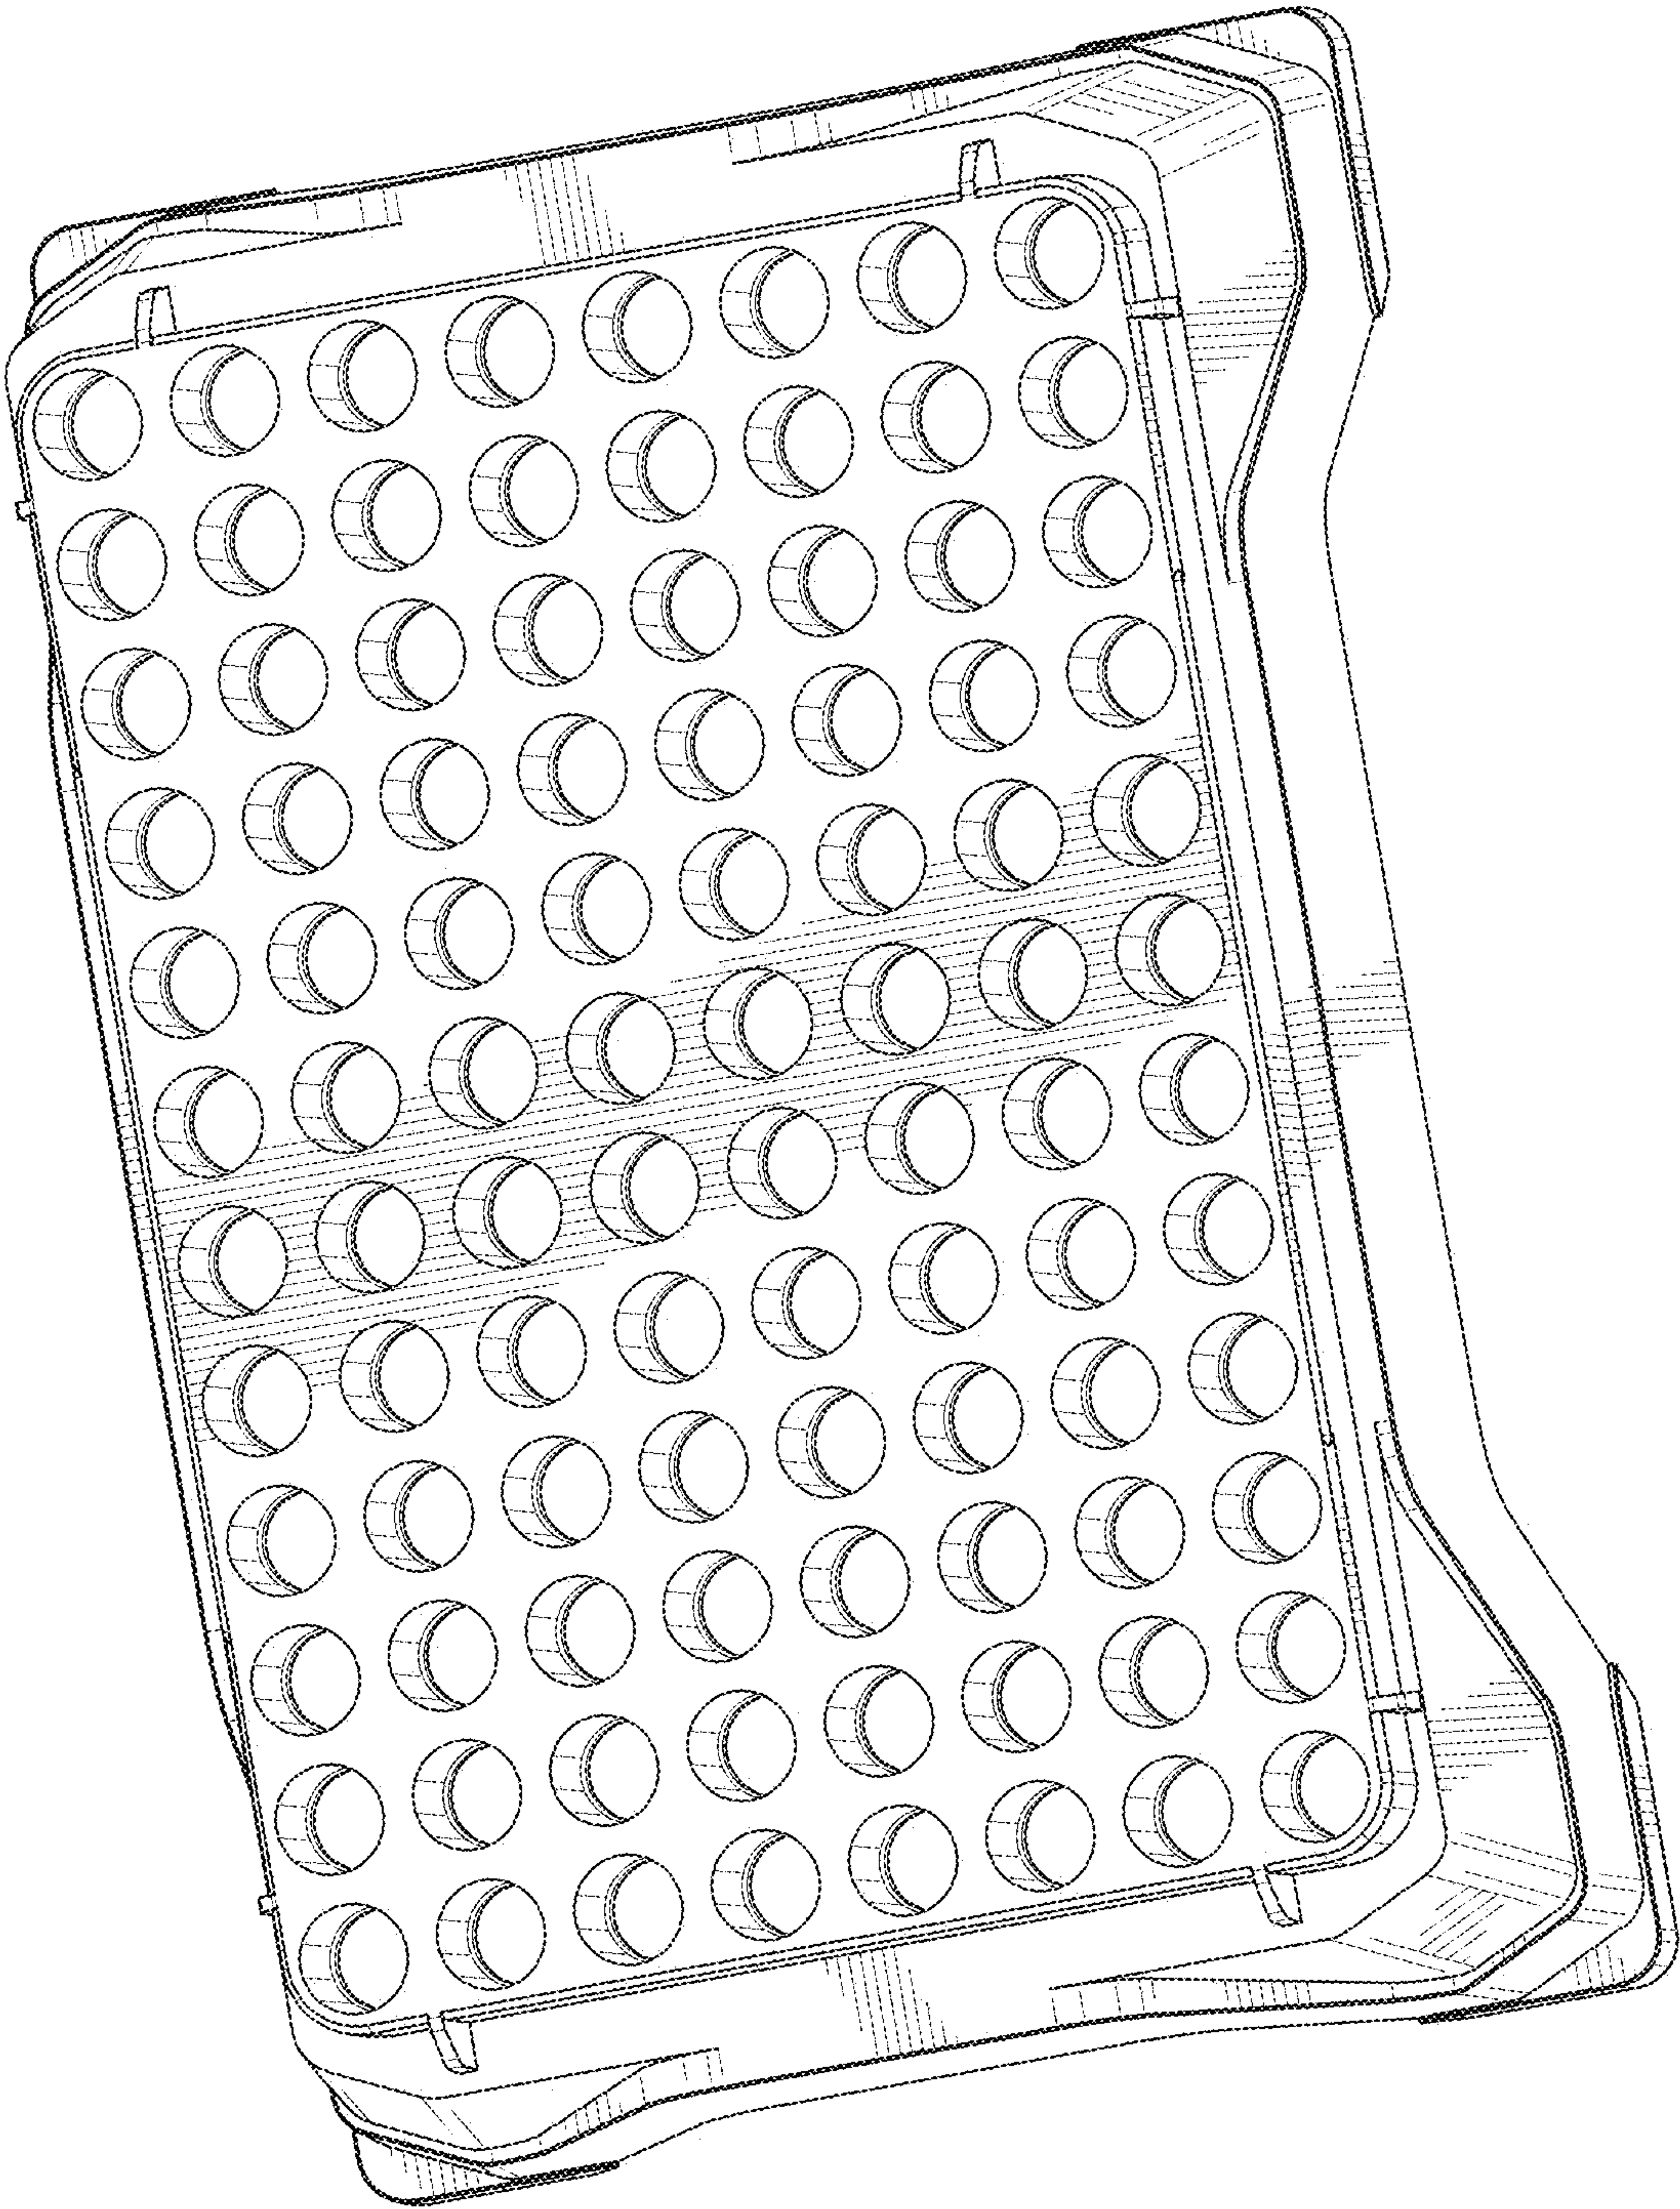


FIG. 3

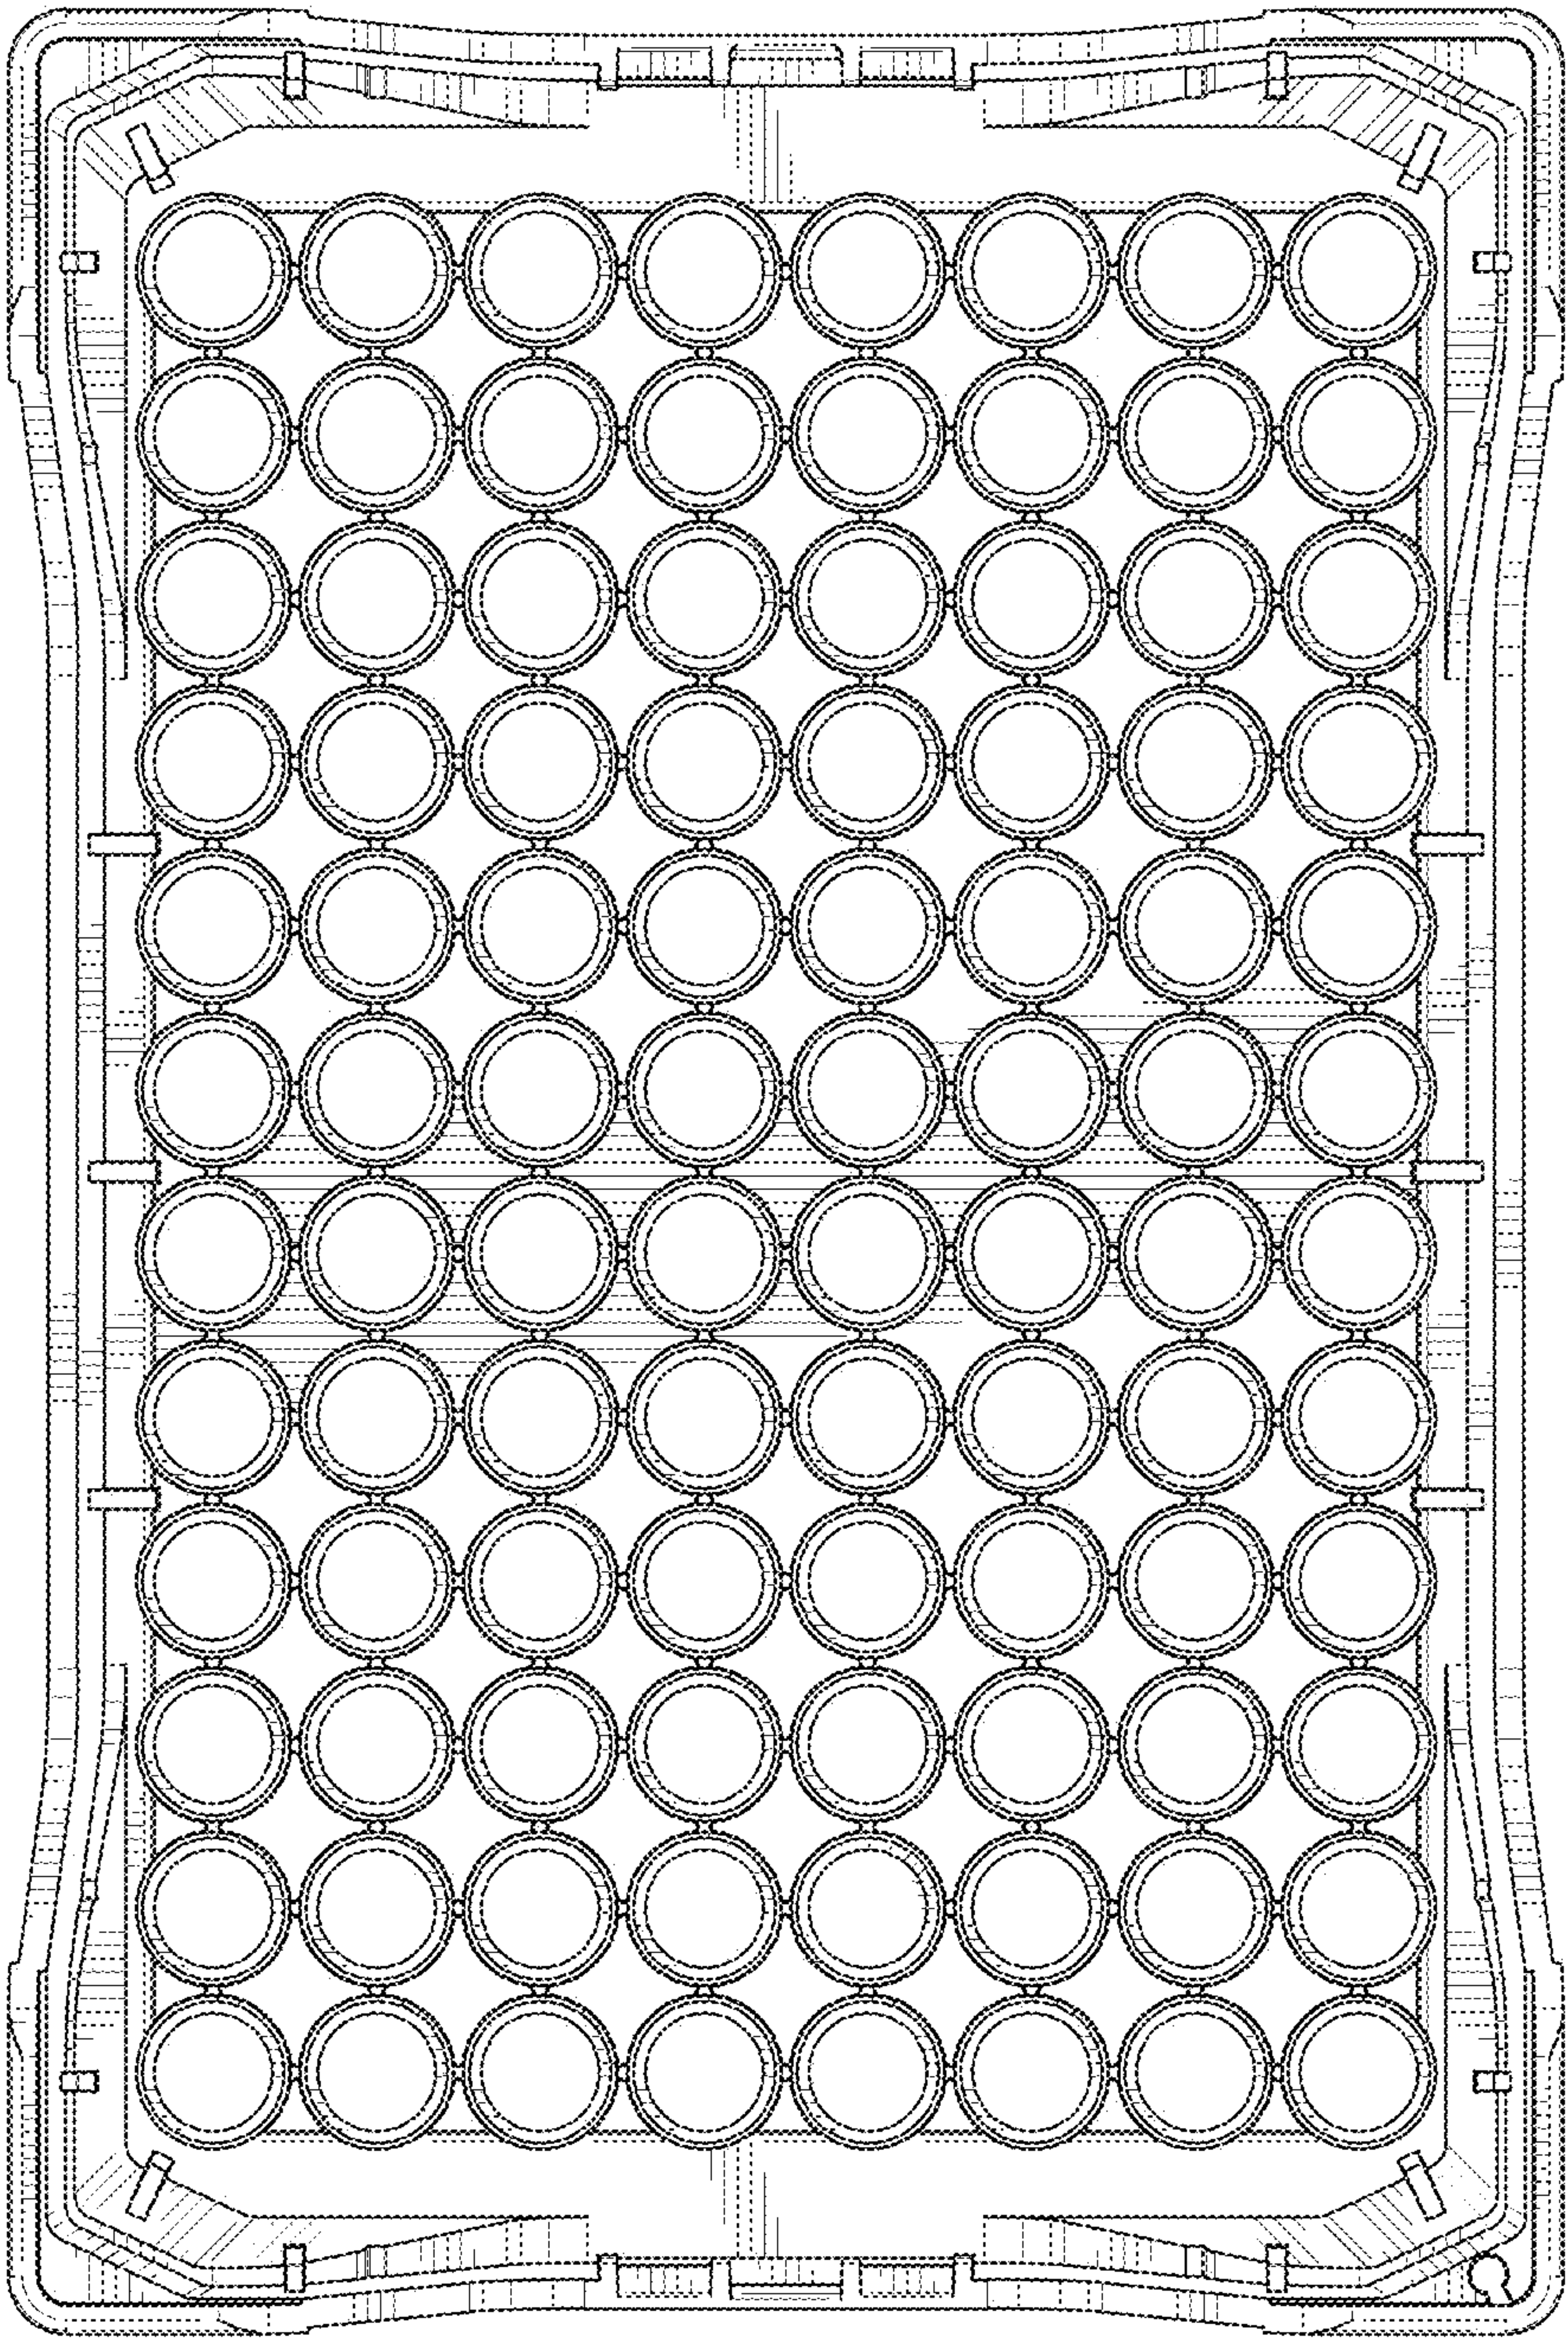


FIG. 4

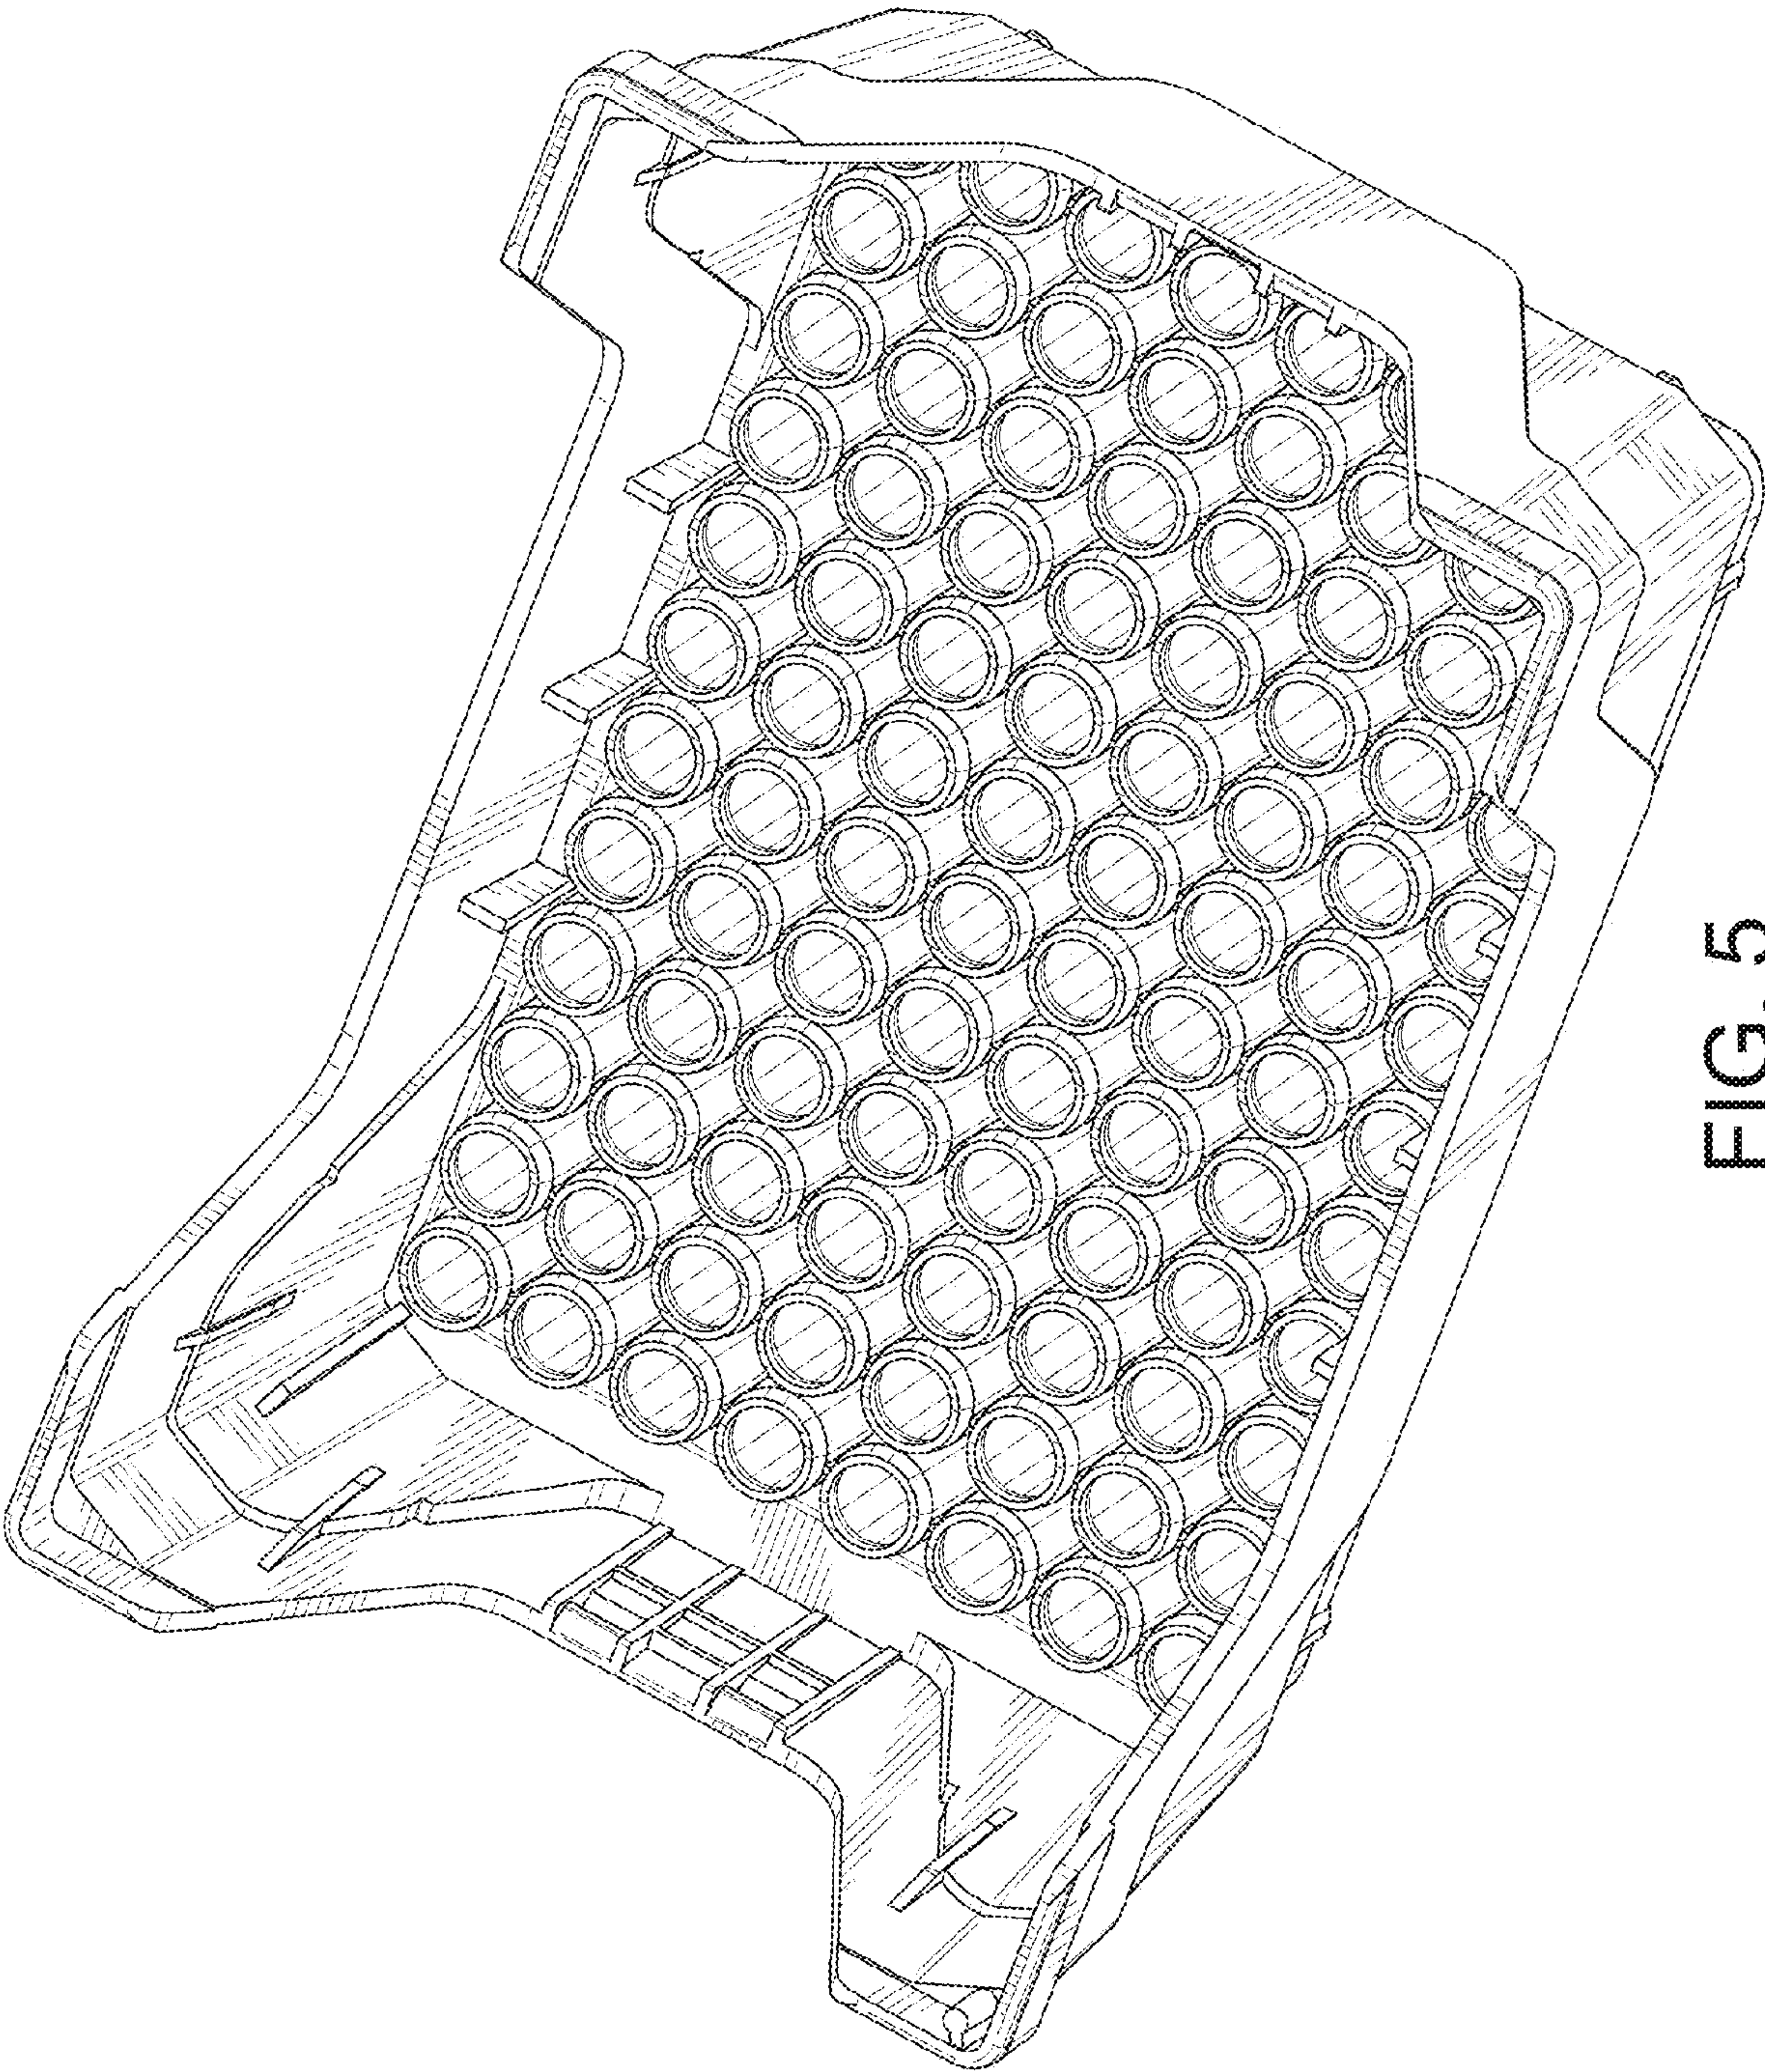


FIG. 5

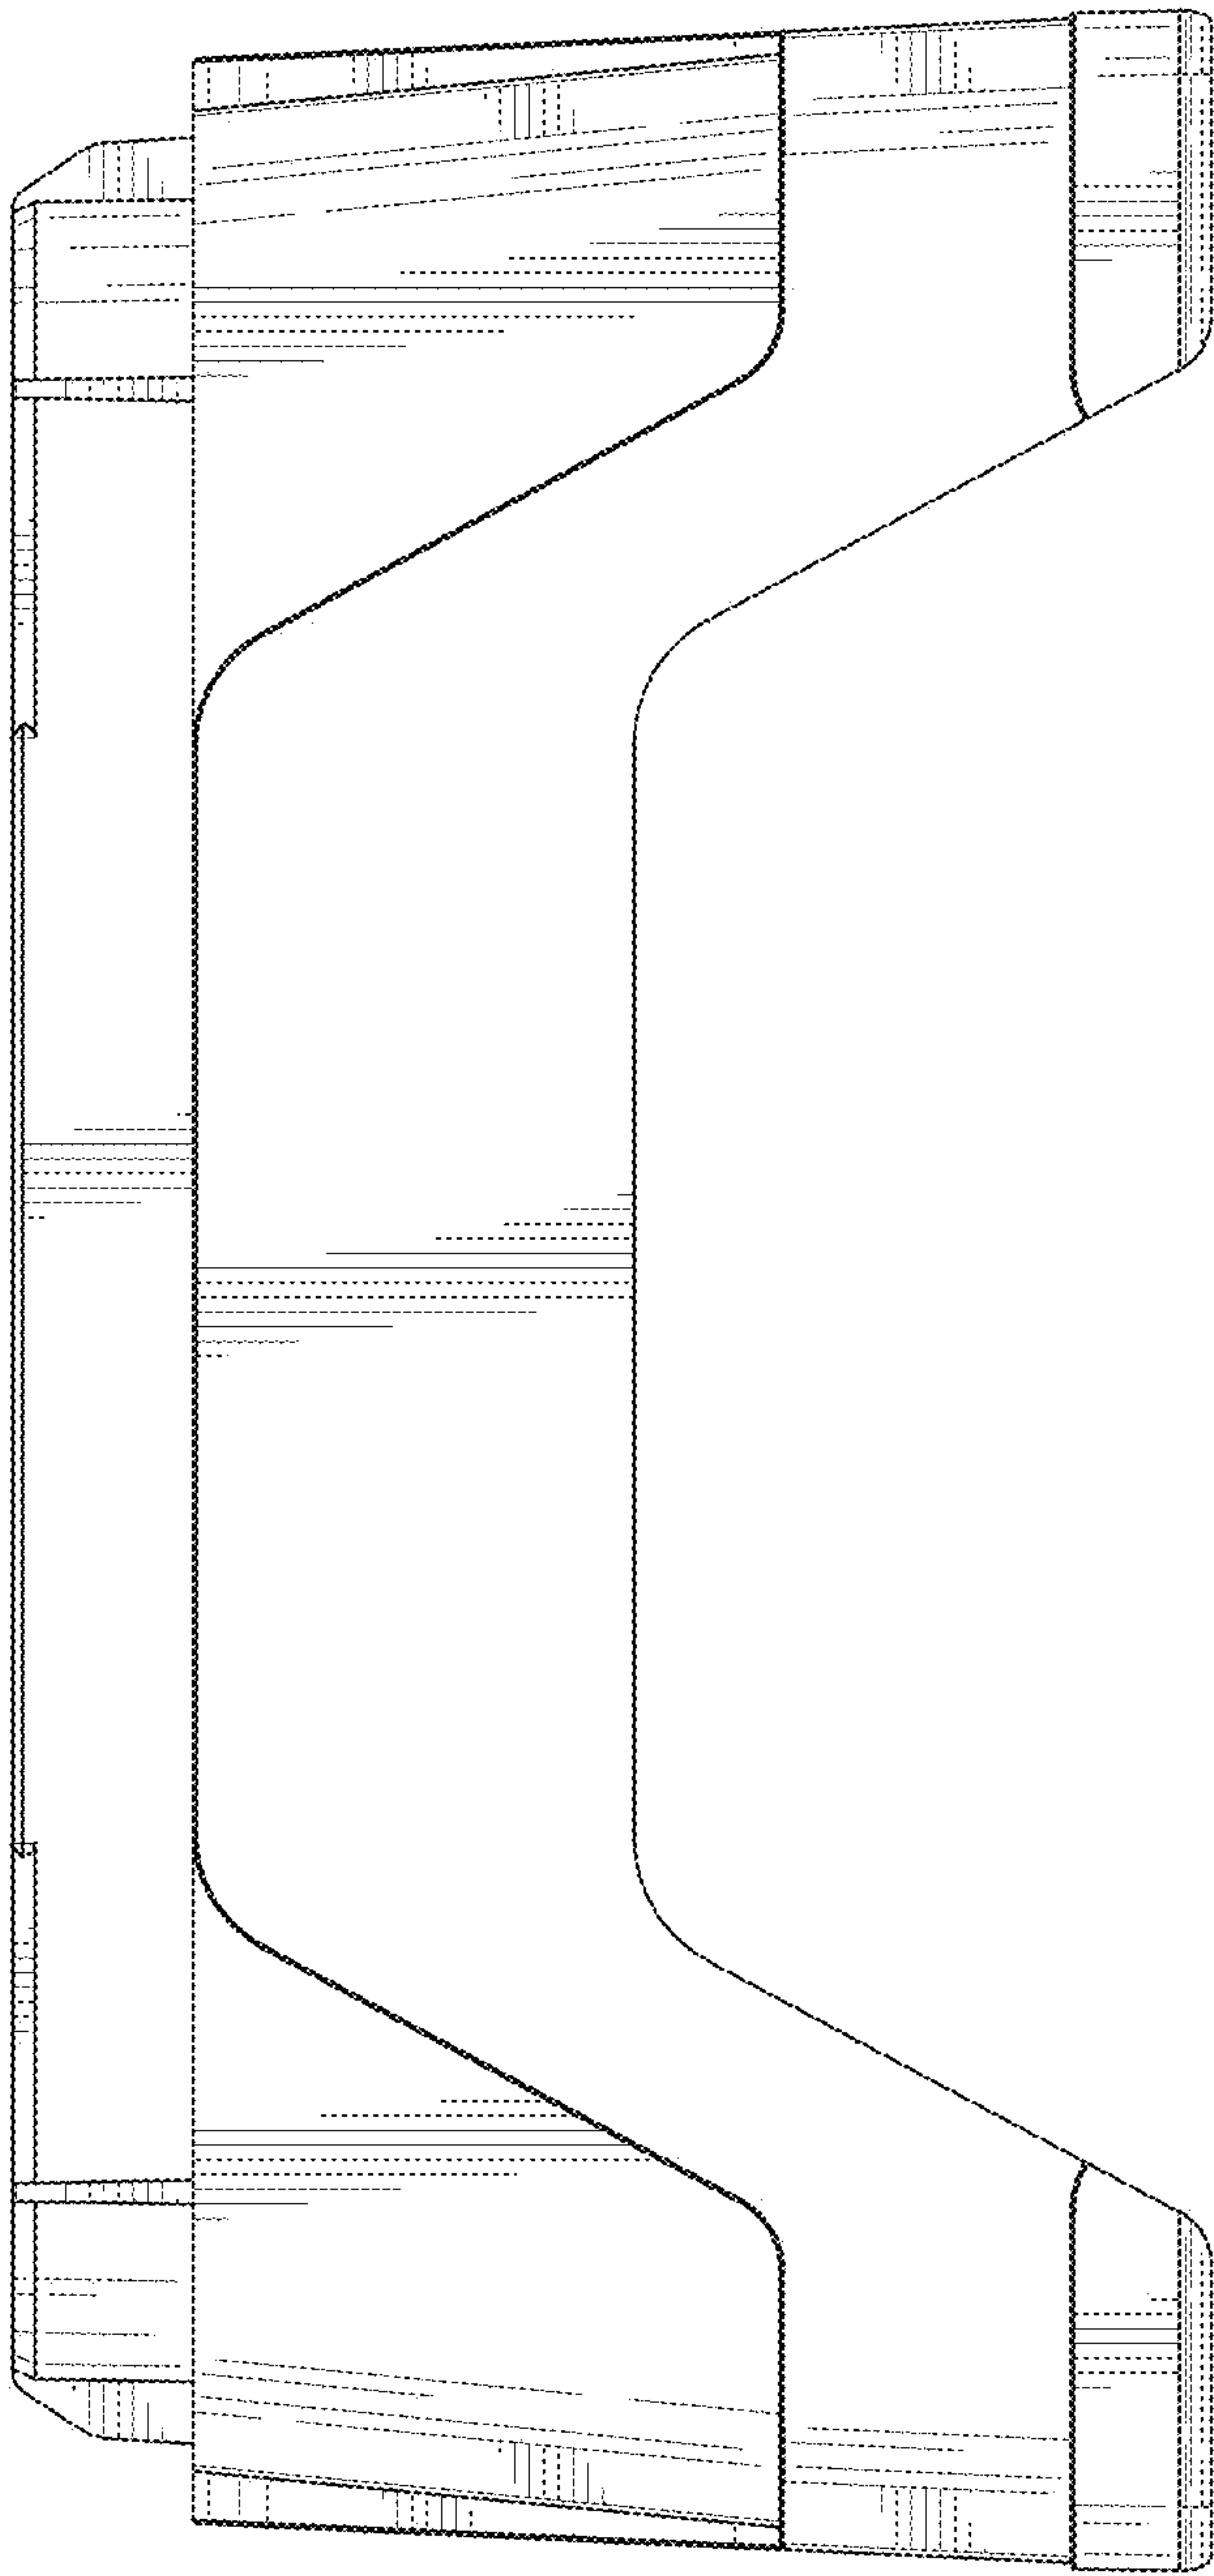


FIG. 6

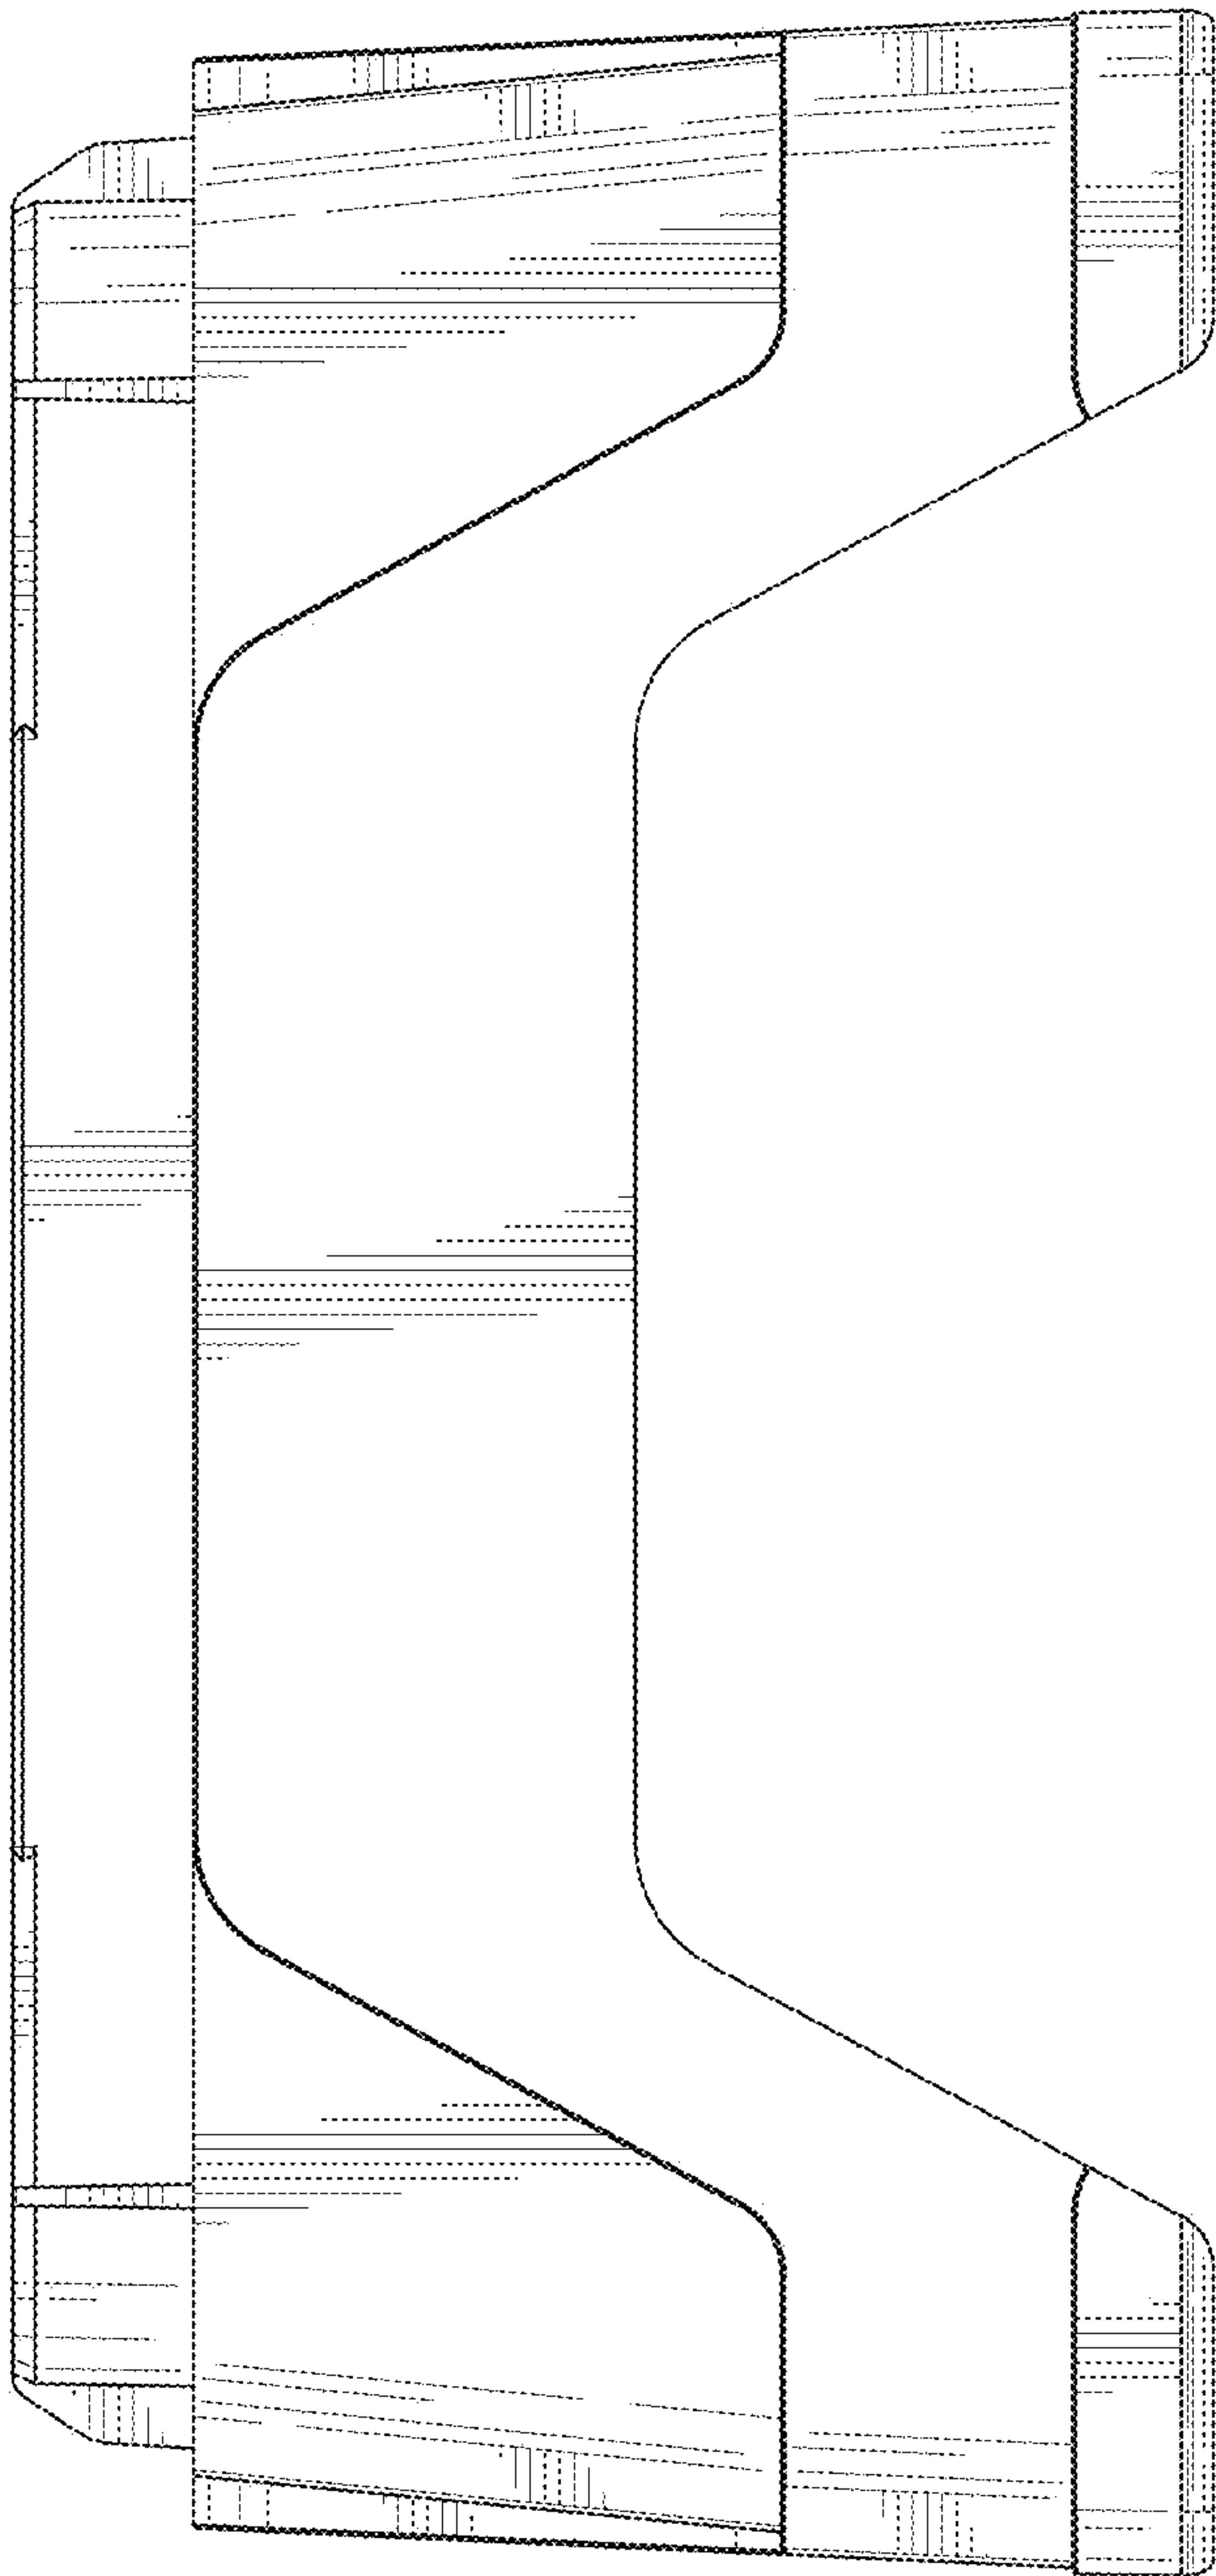


FIG. 7

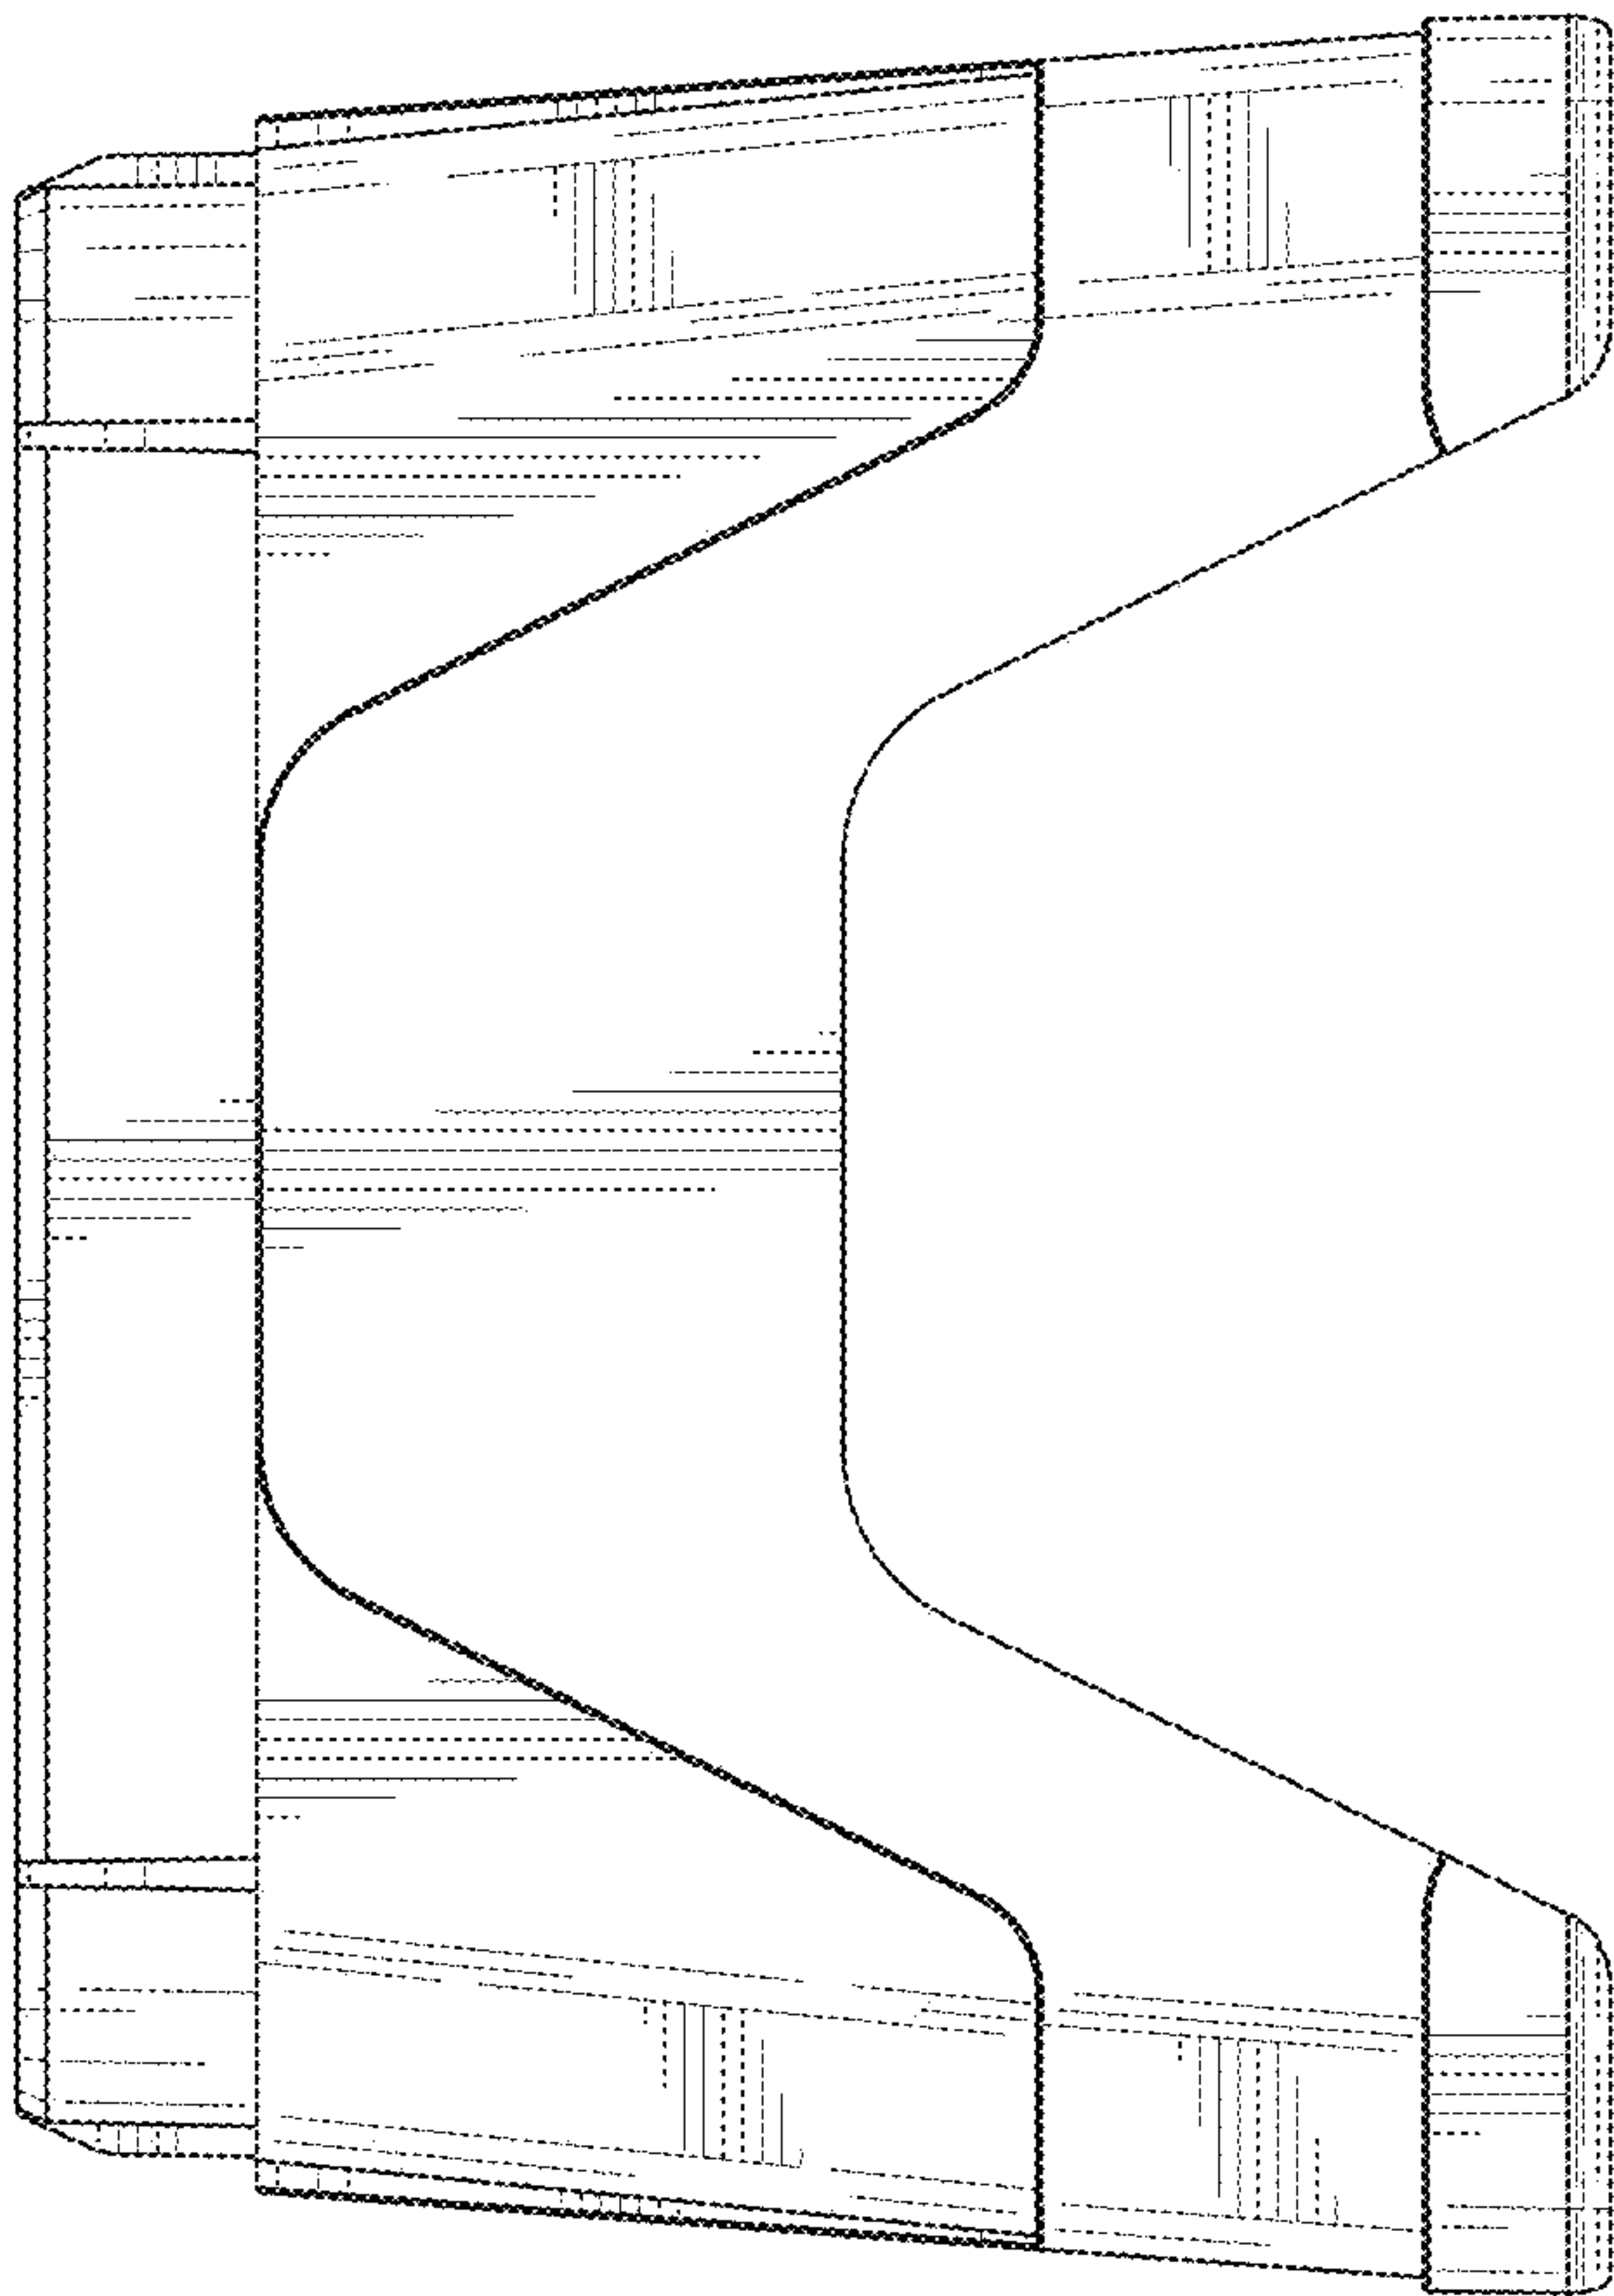


FIG. 8

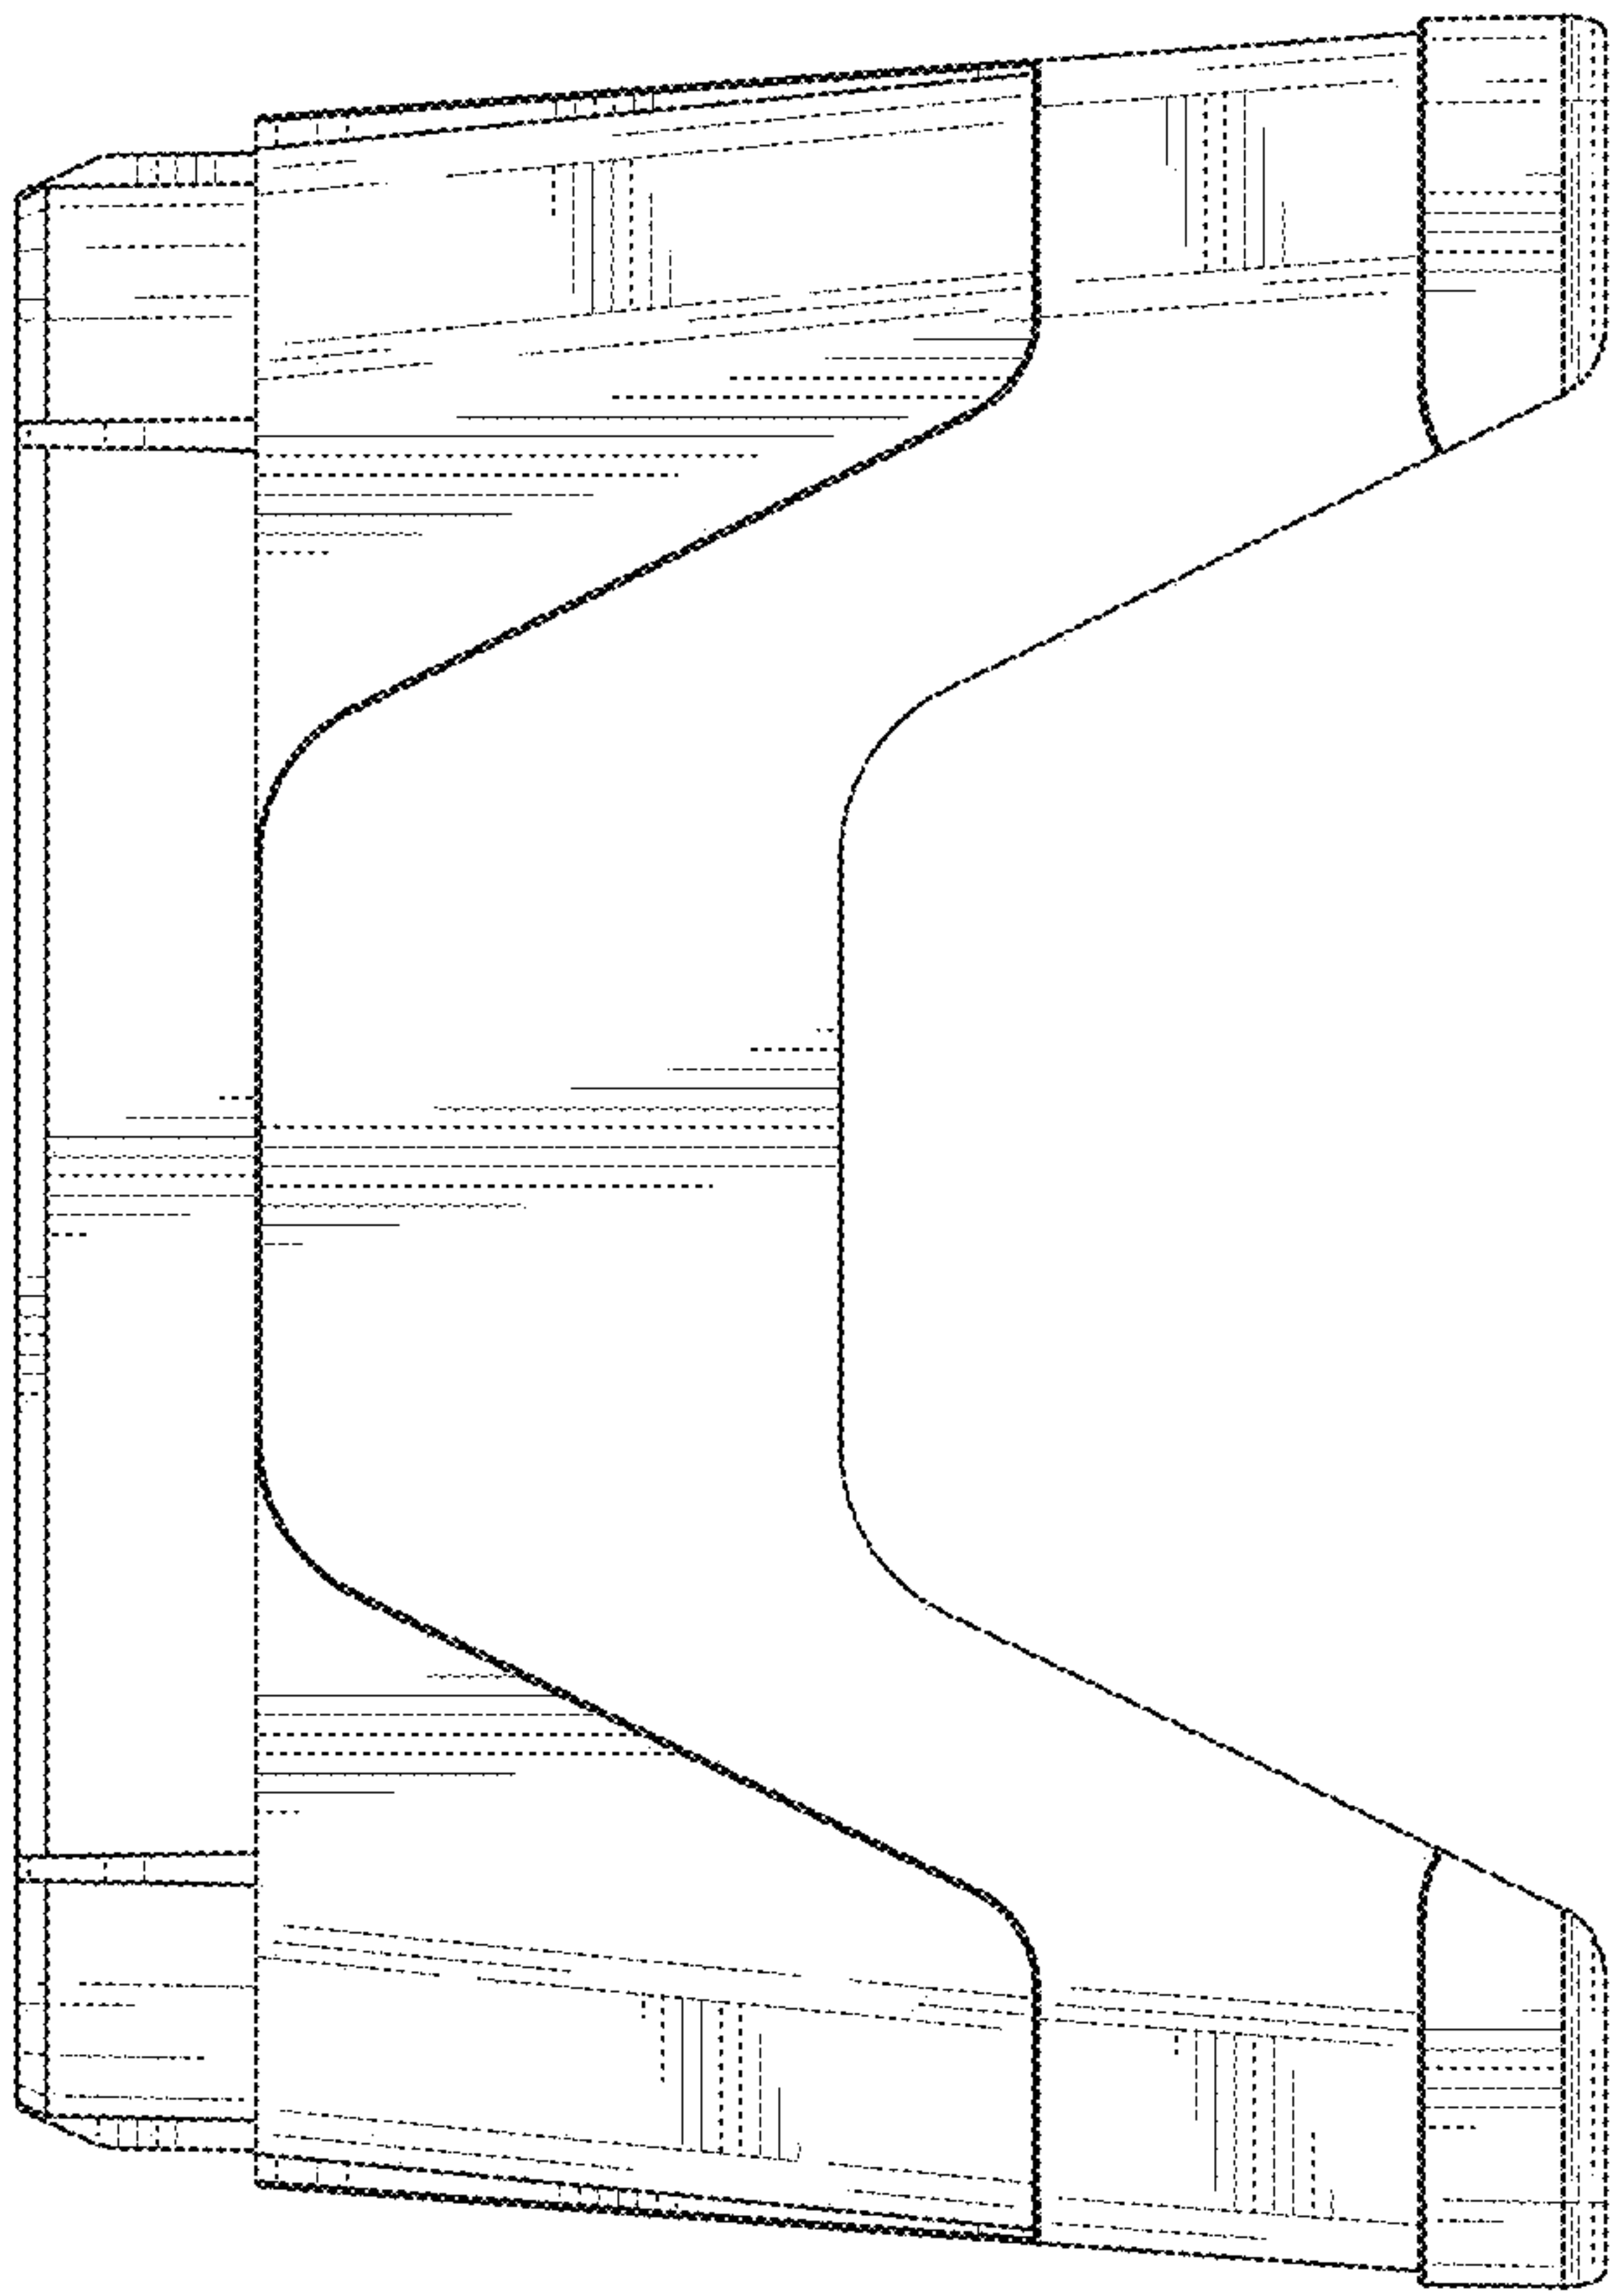


FIG. 9

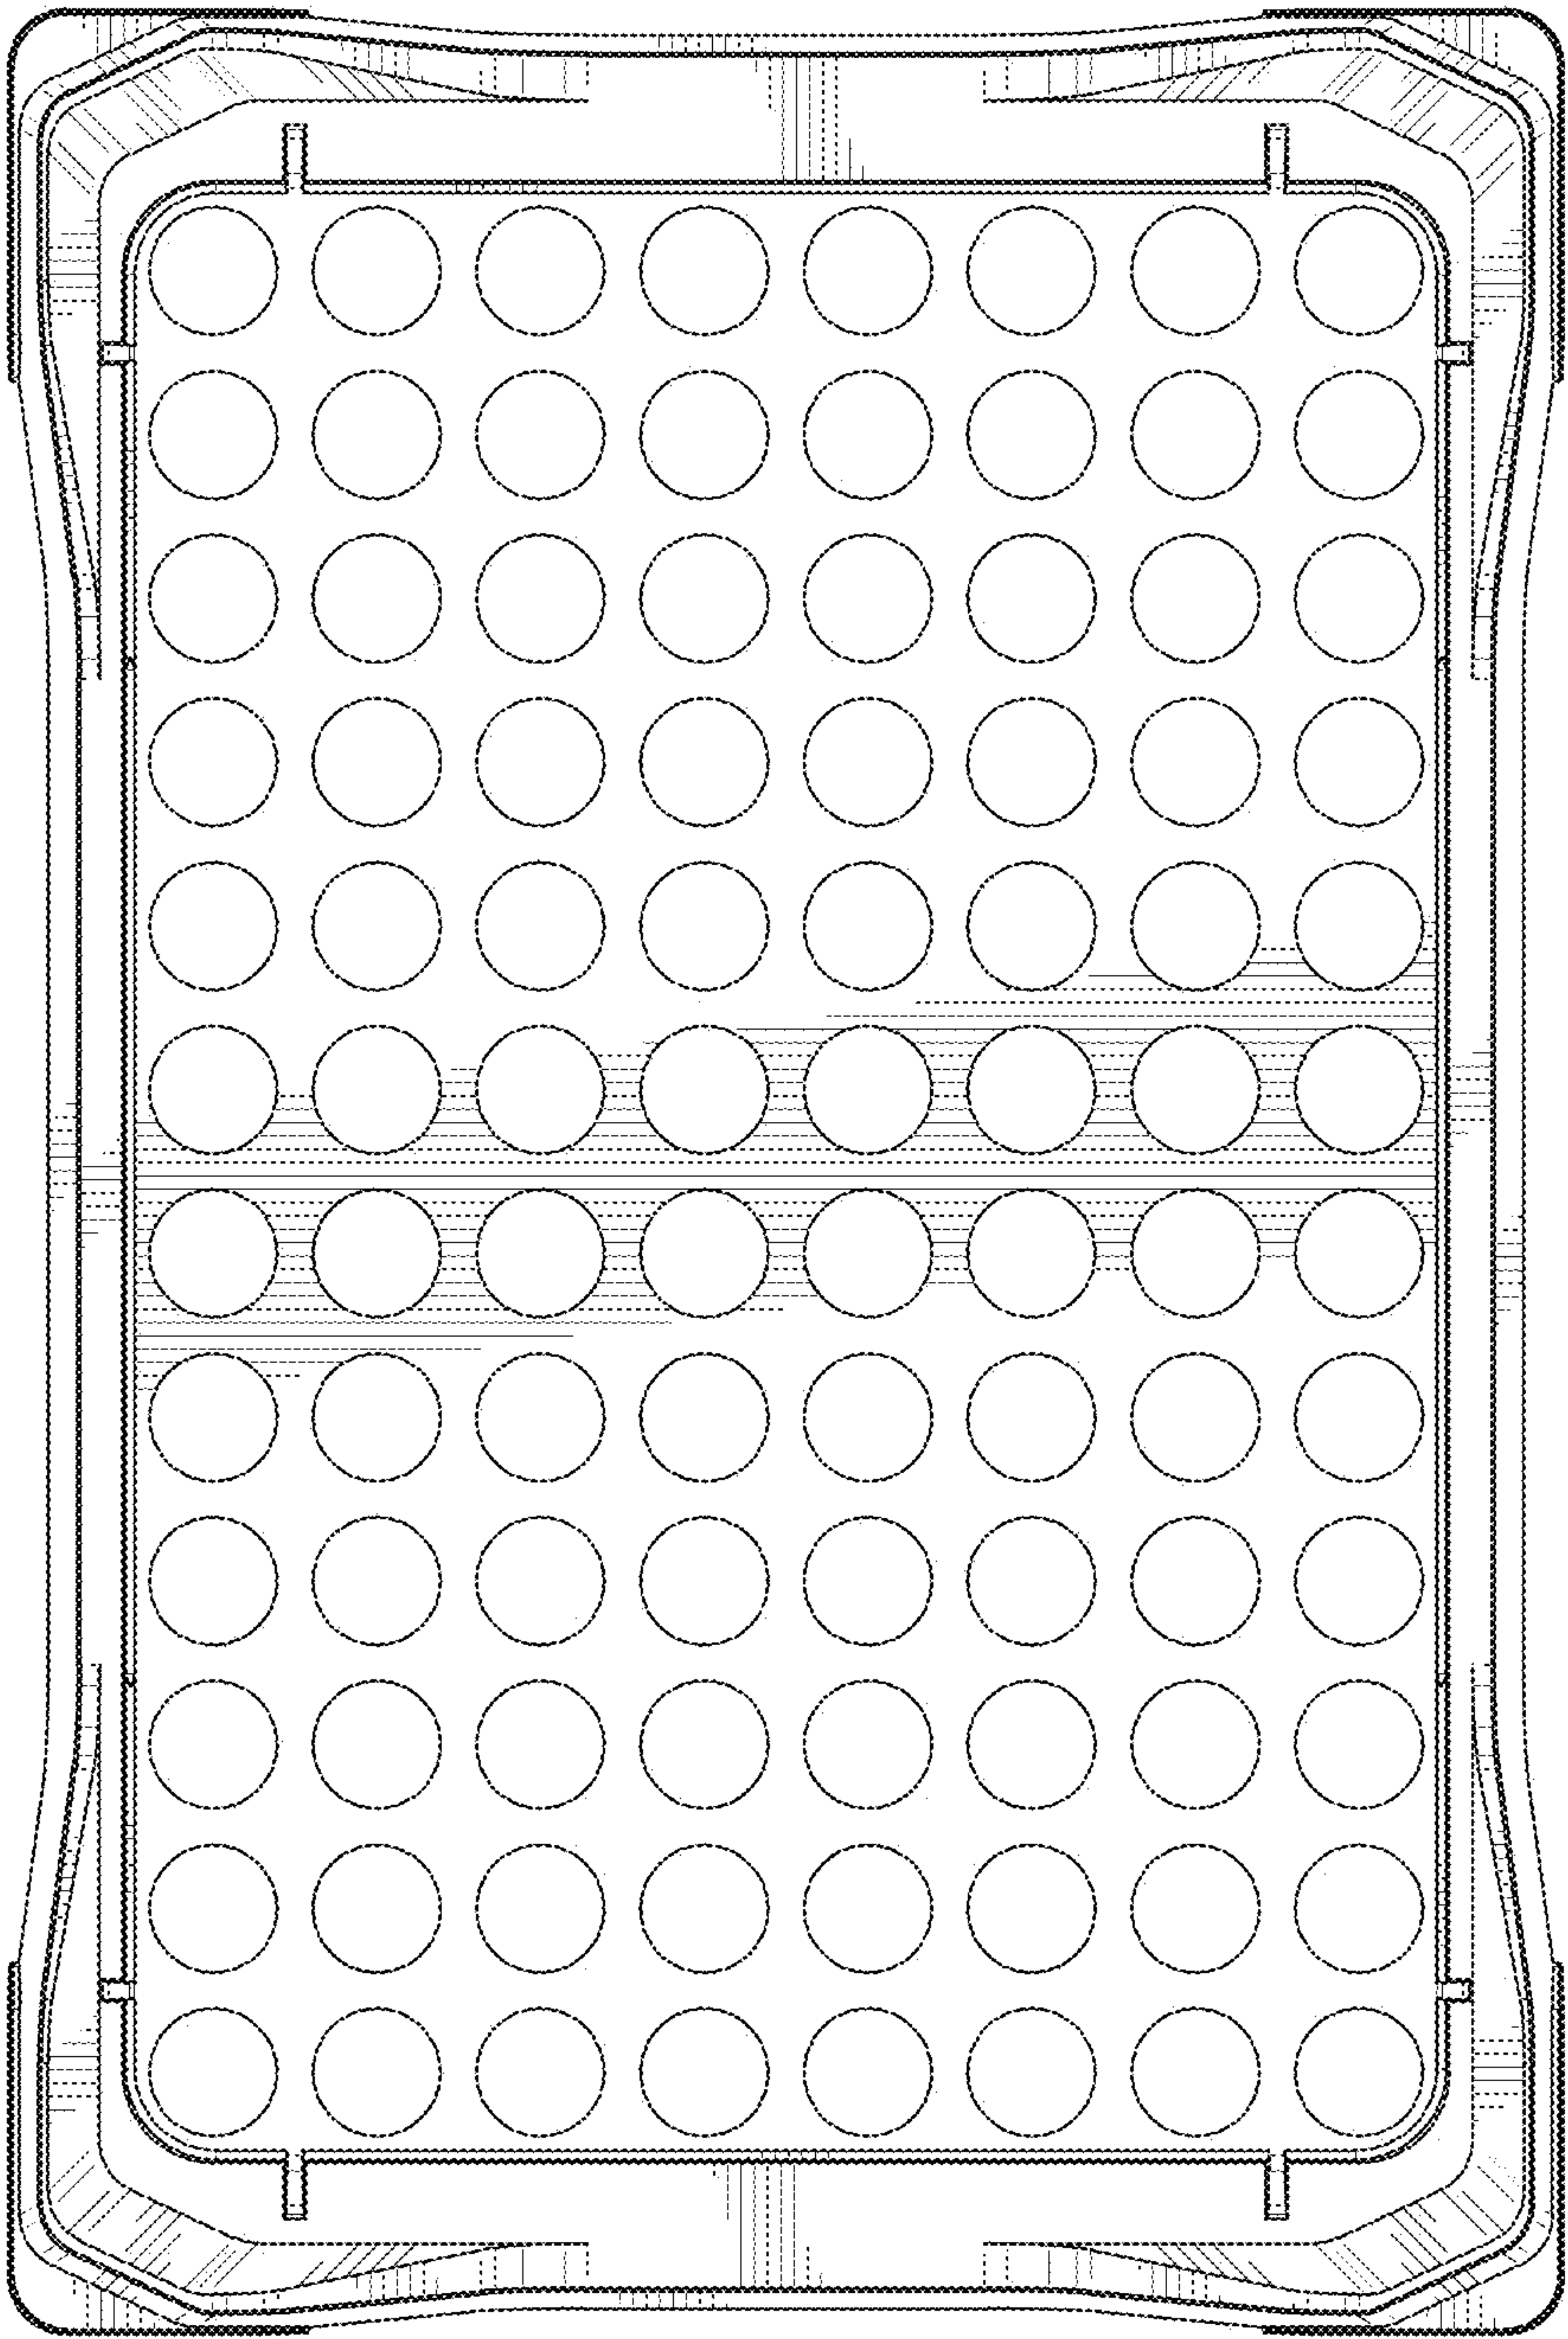


FIG. 10

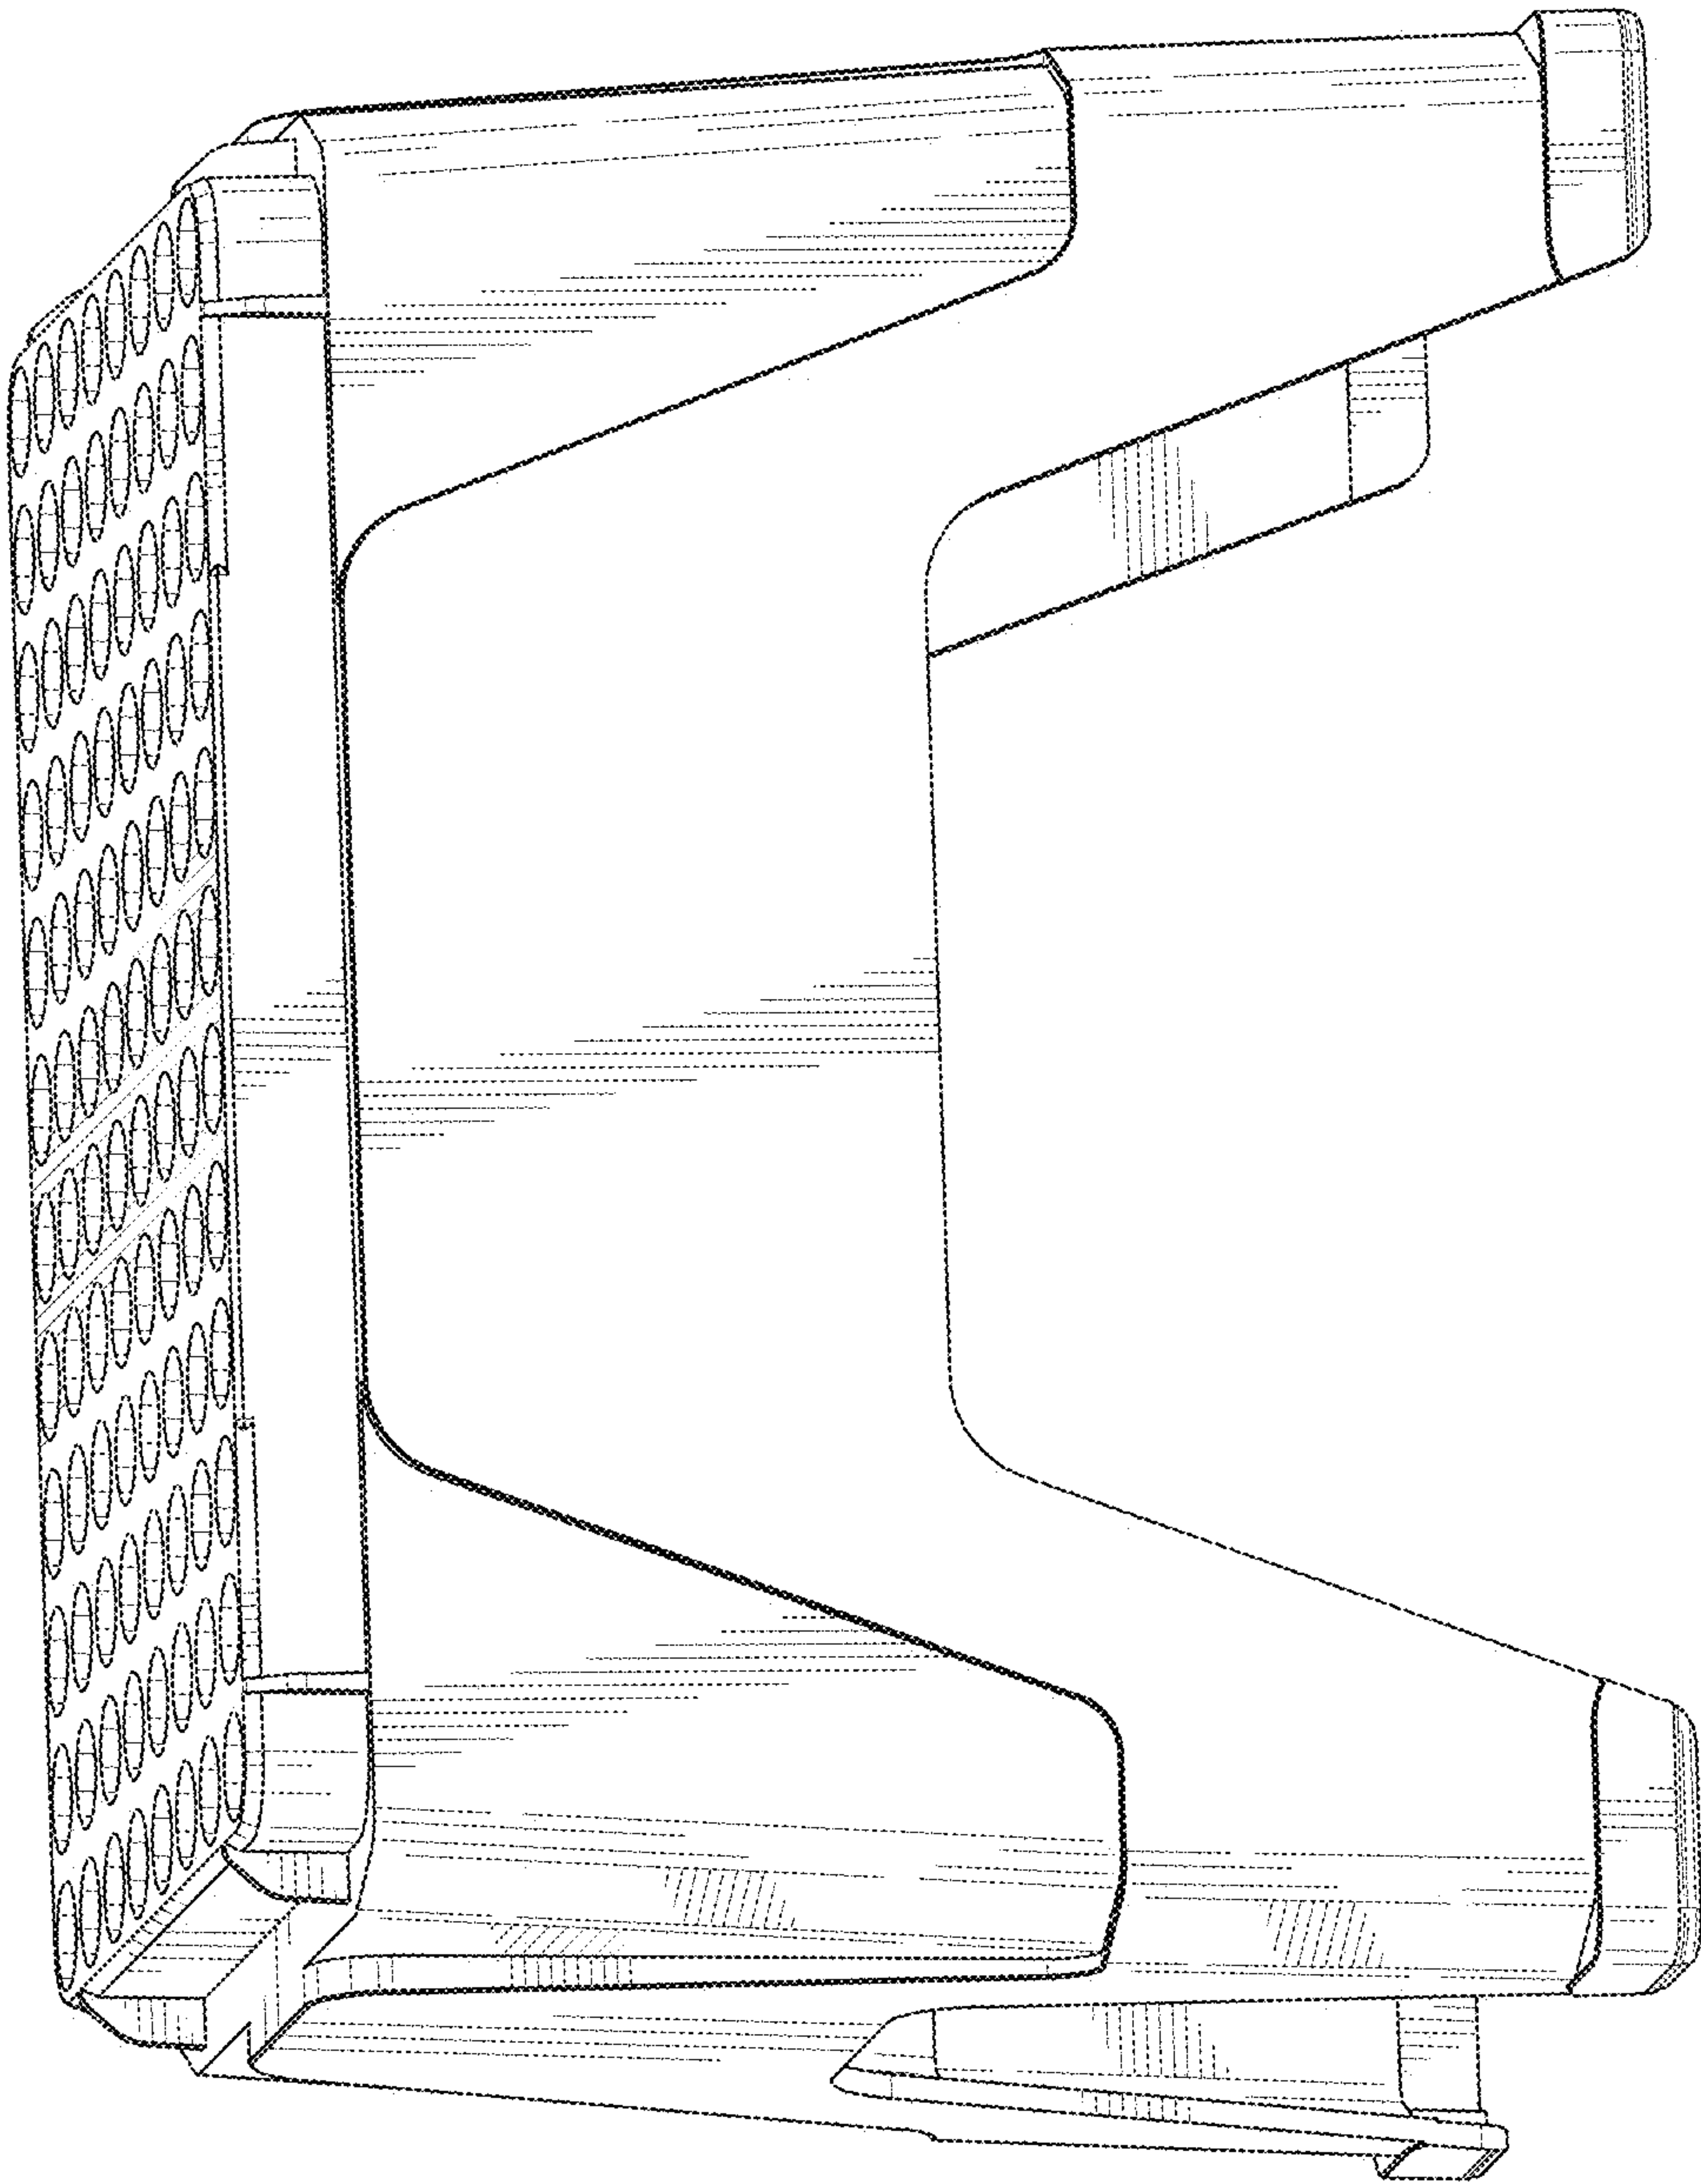


FIG. 11

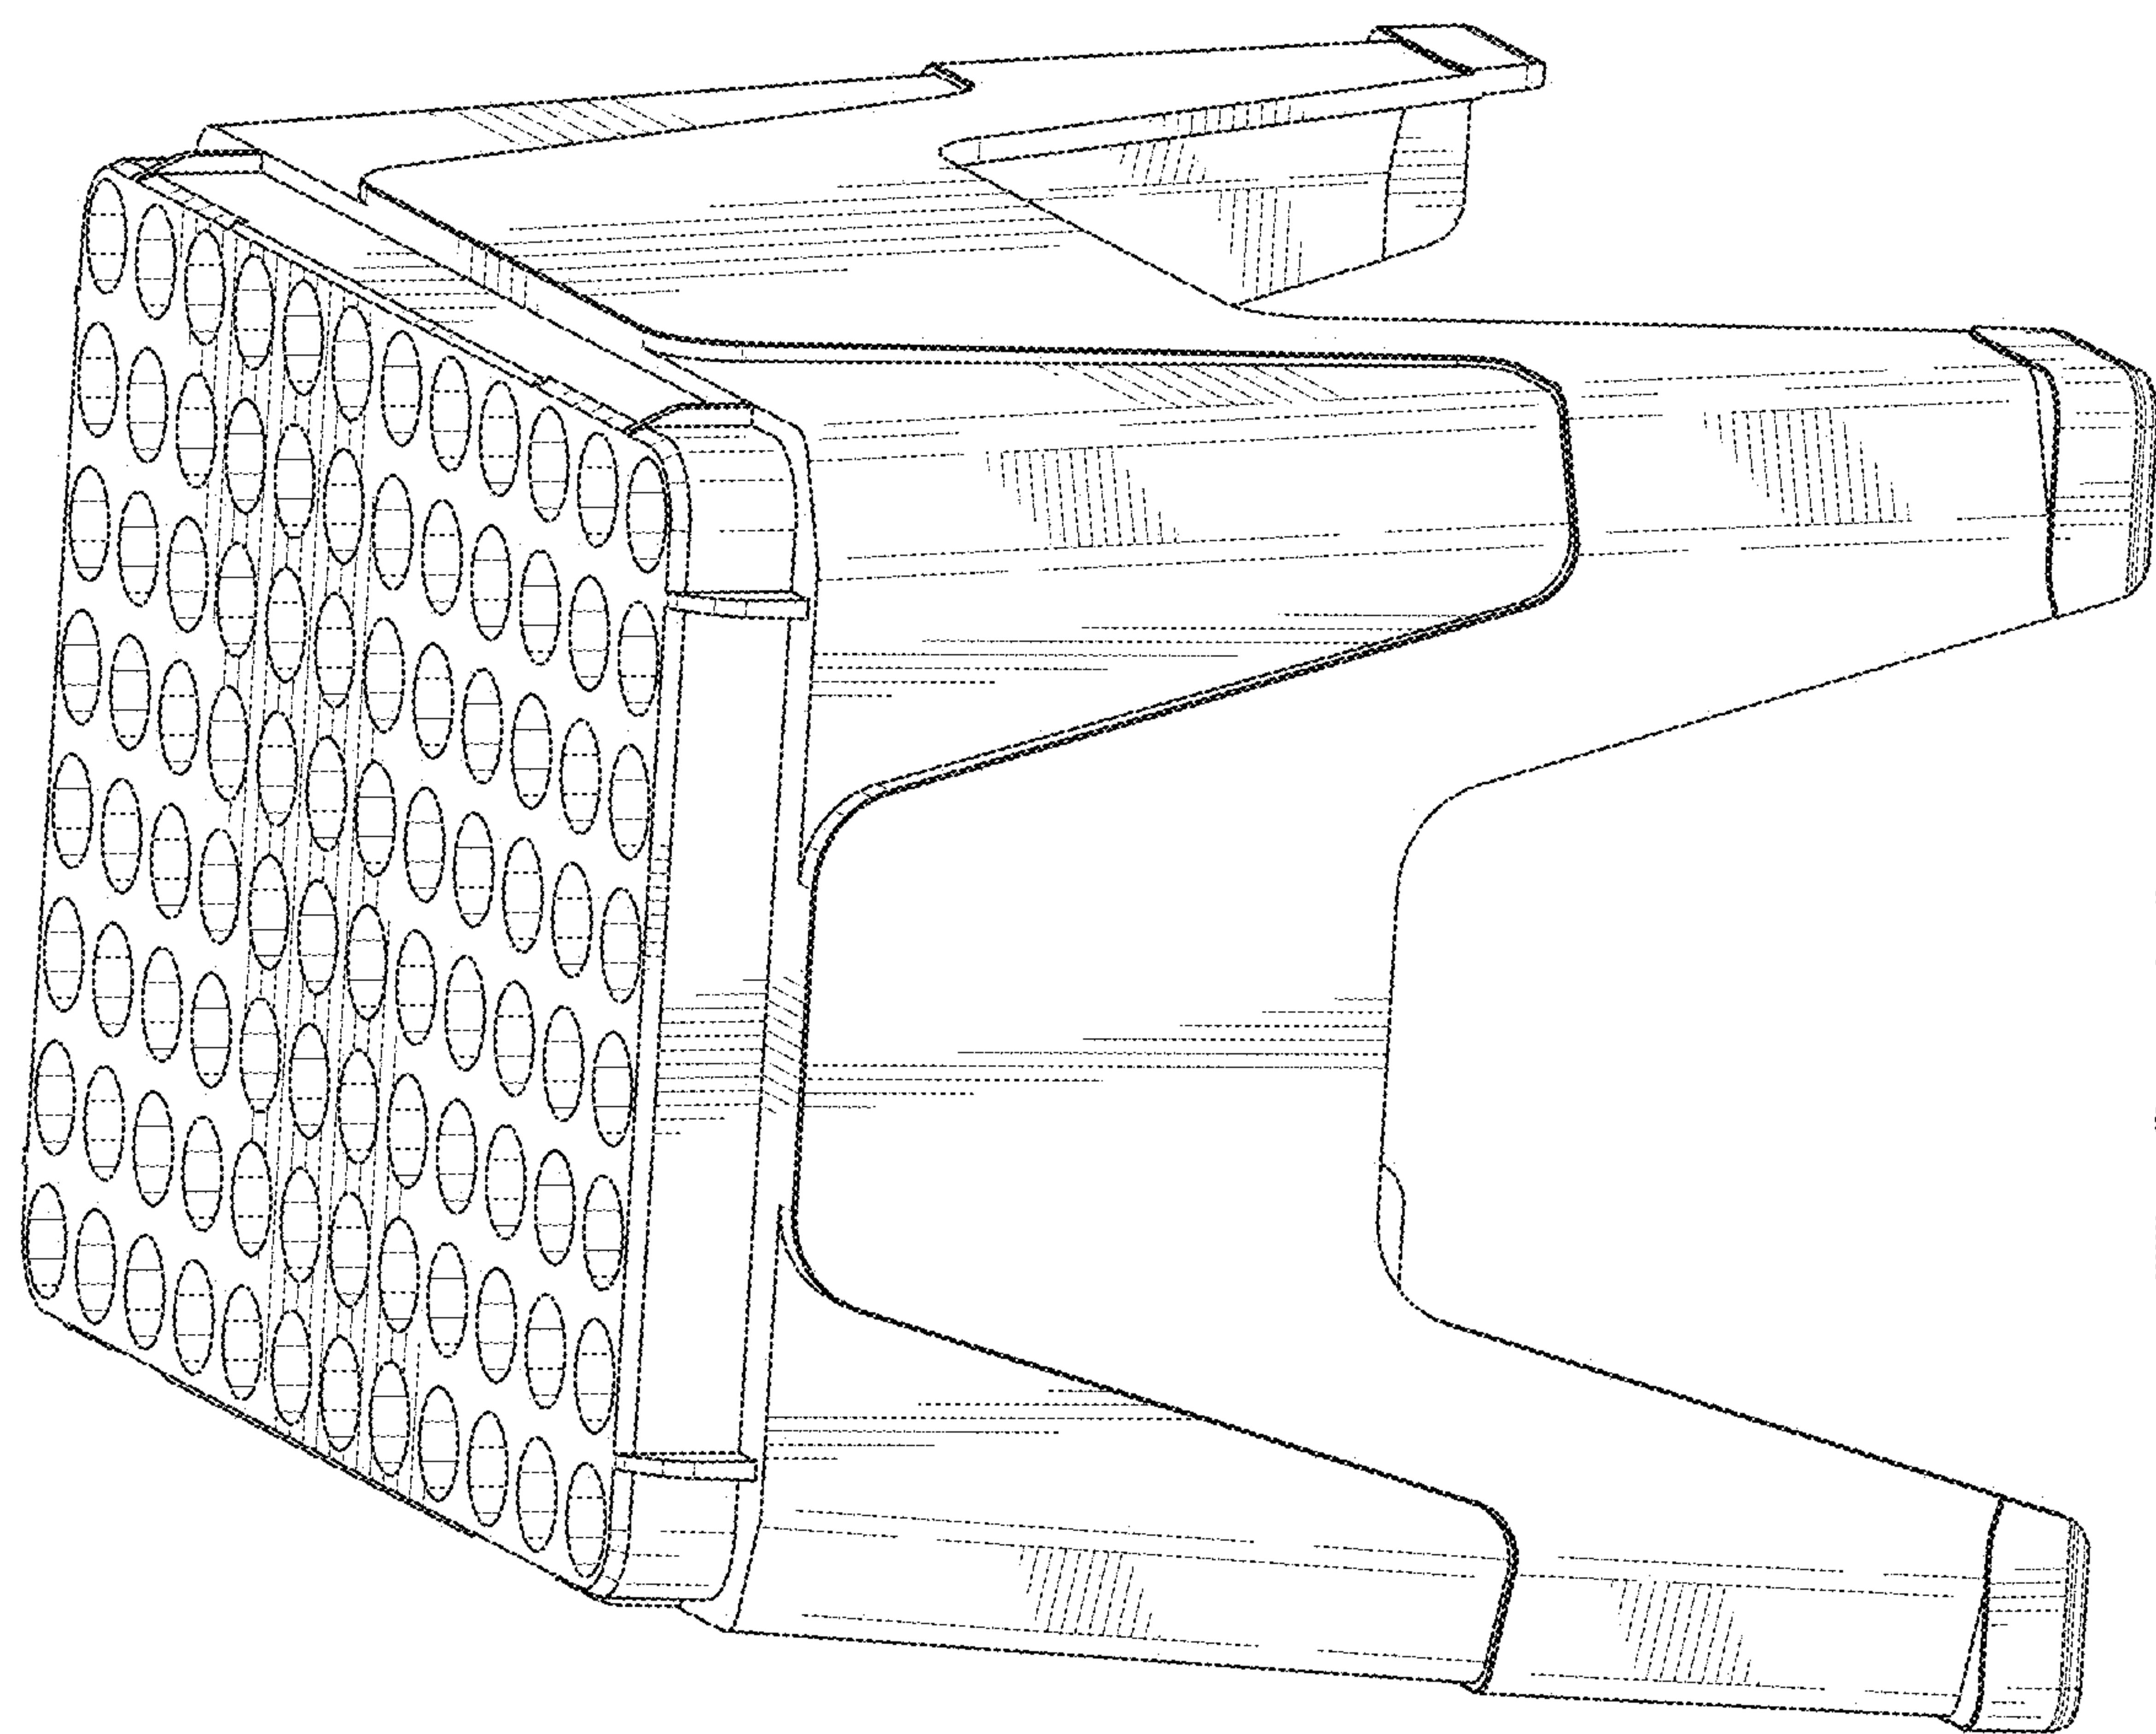


FIG. 12

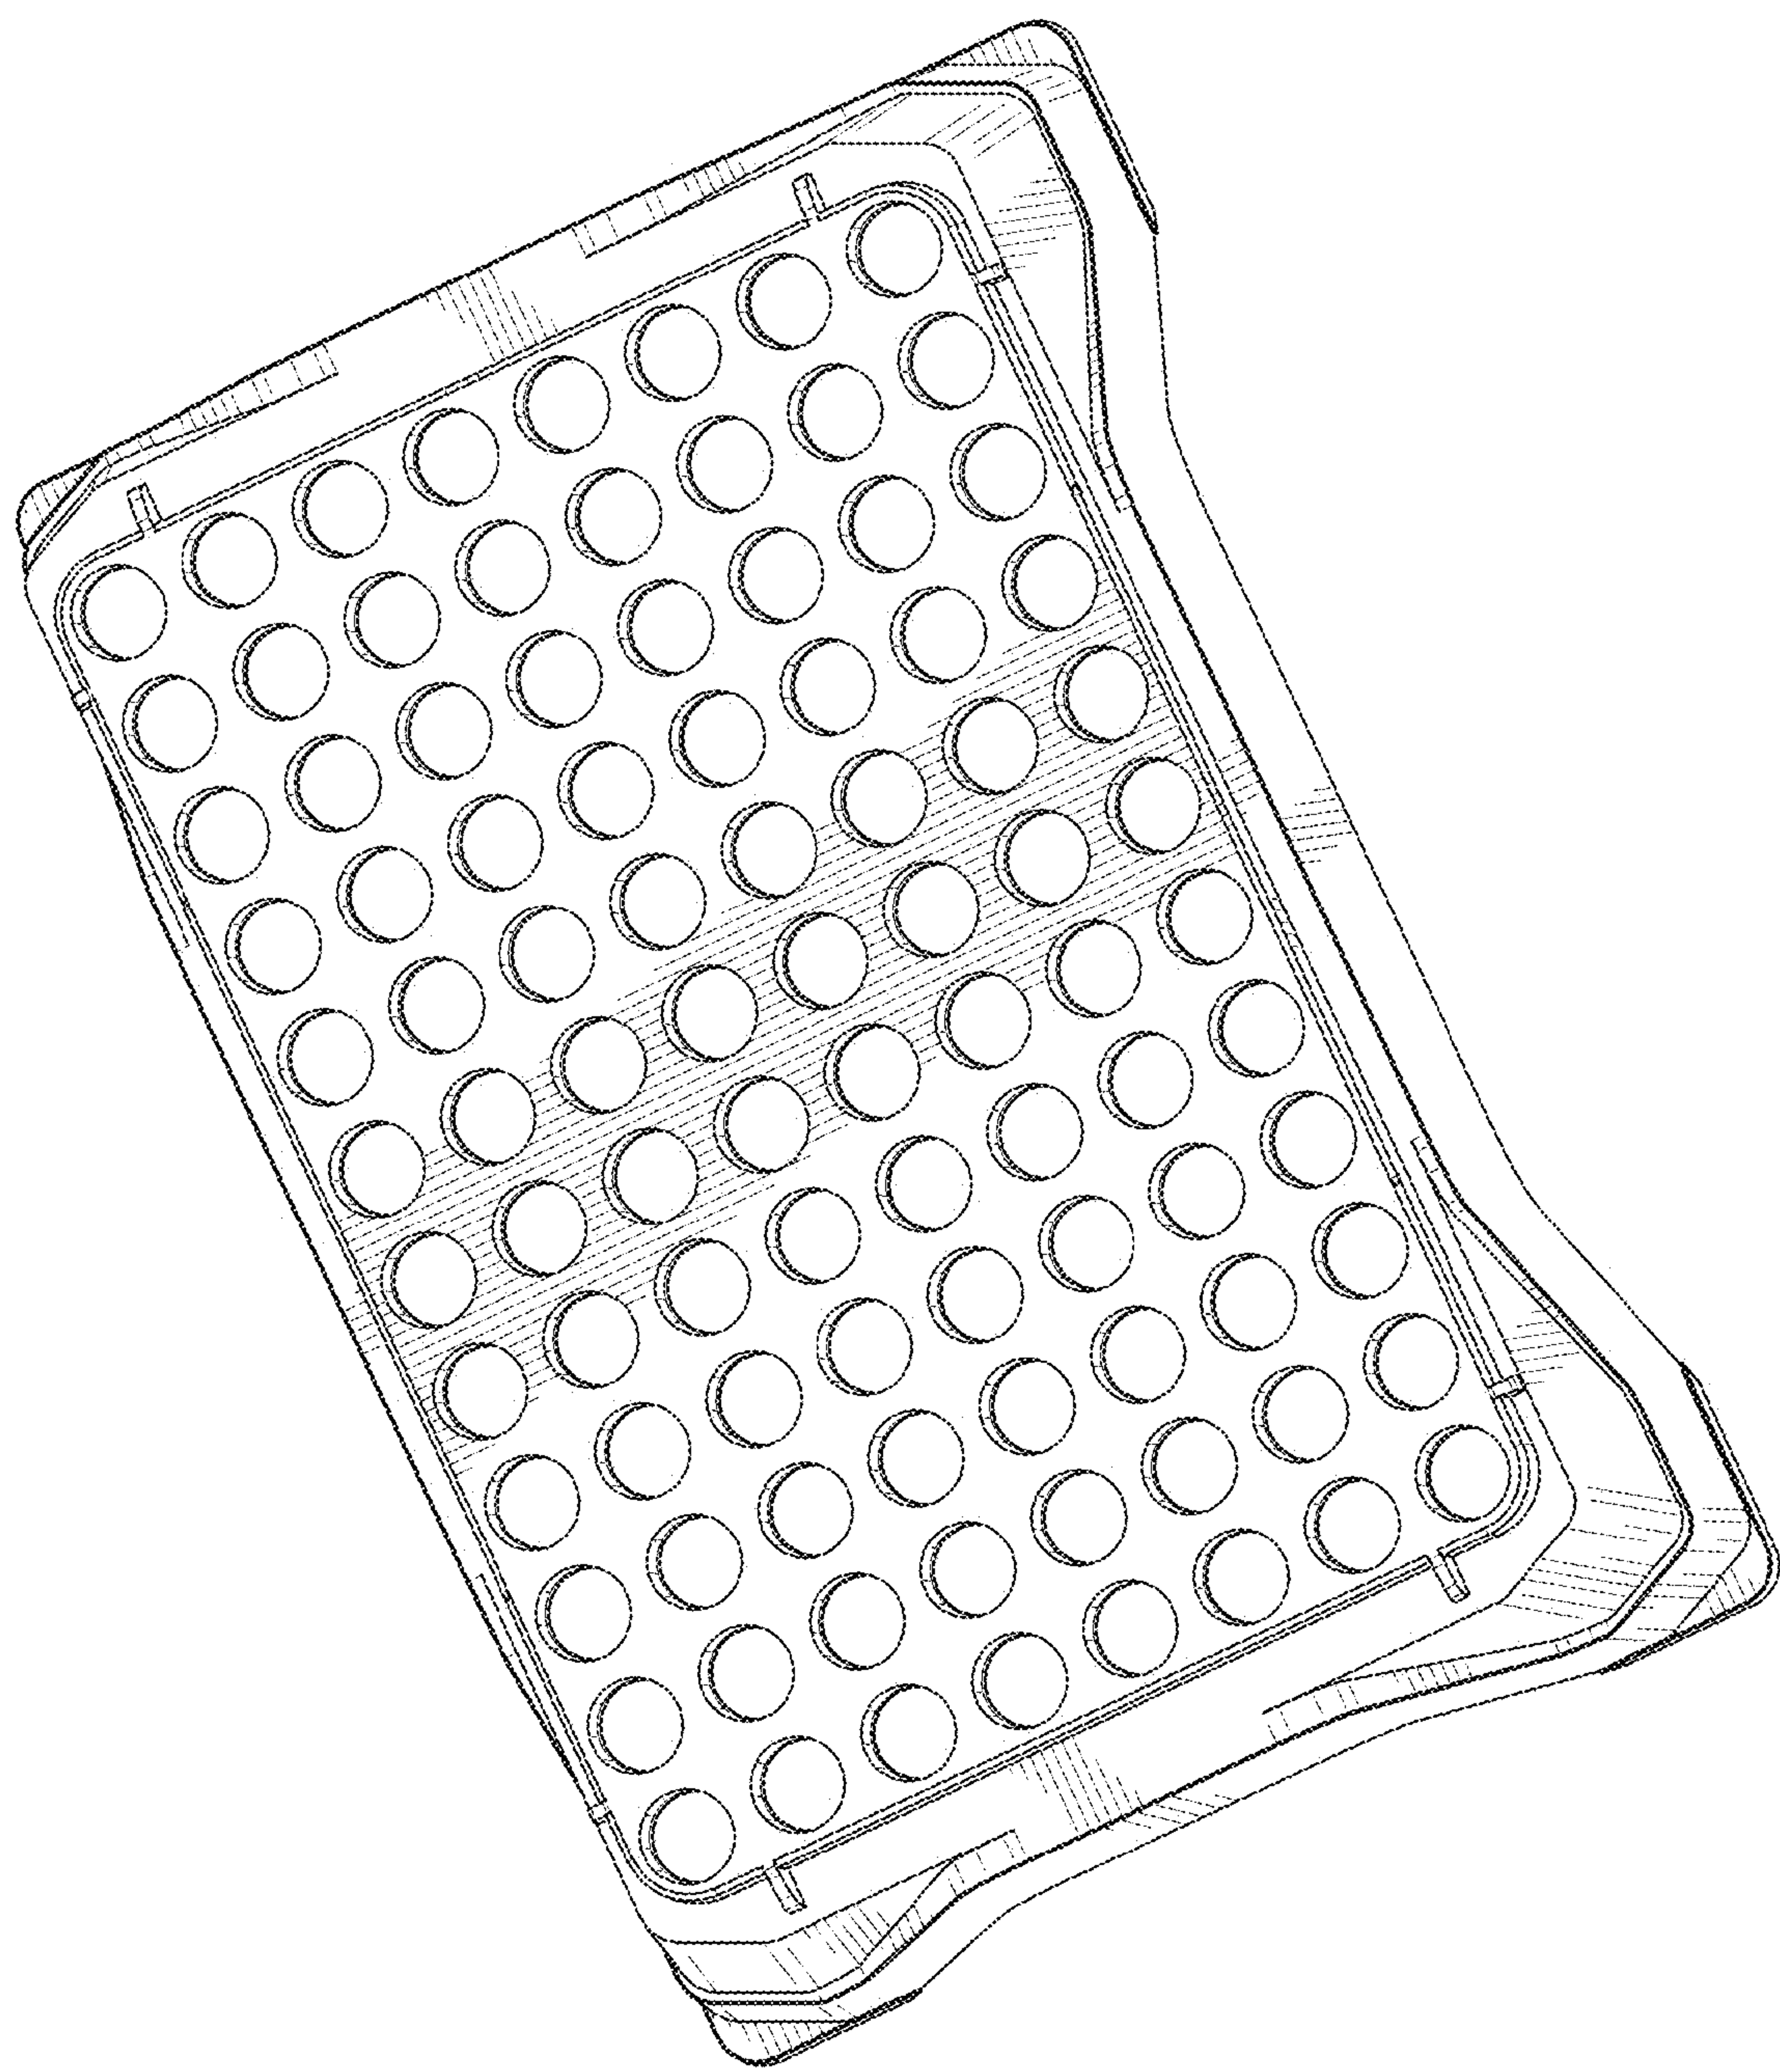


FIG. 13

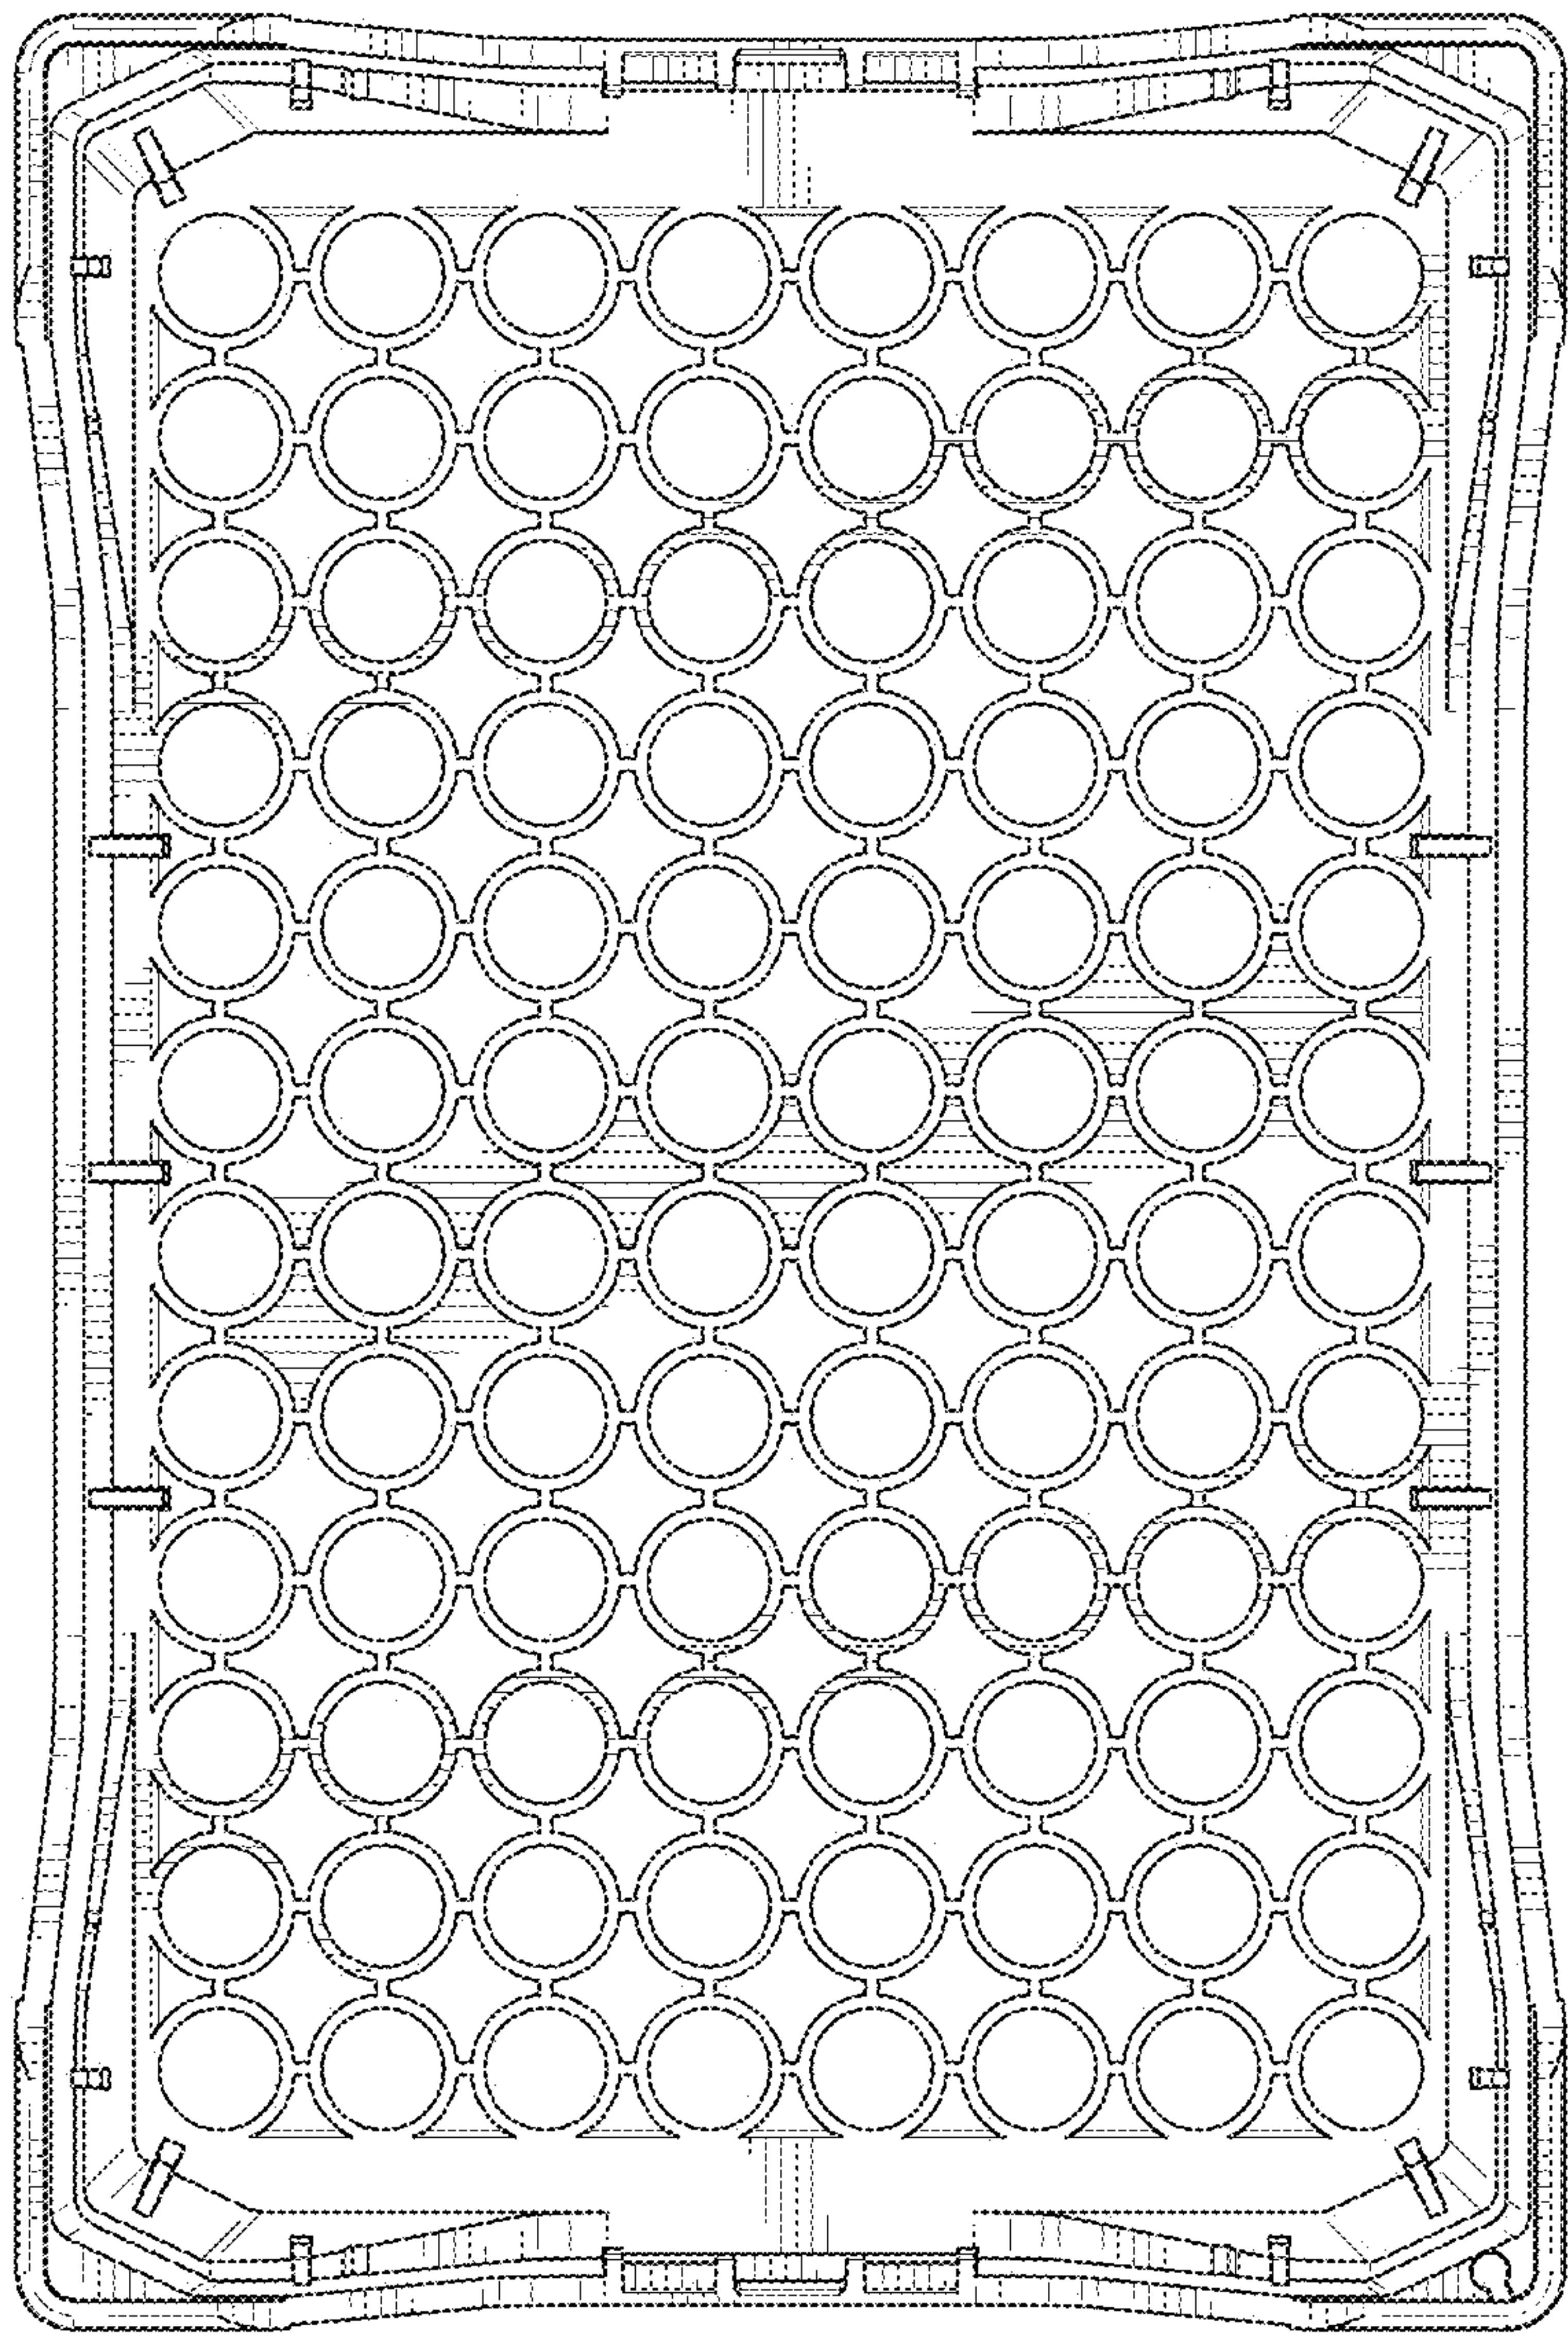


FIG. 14

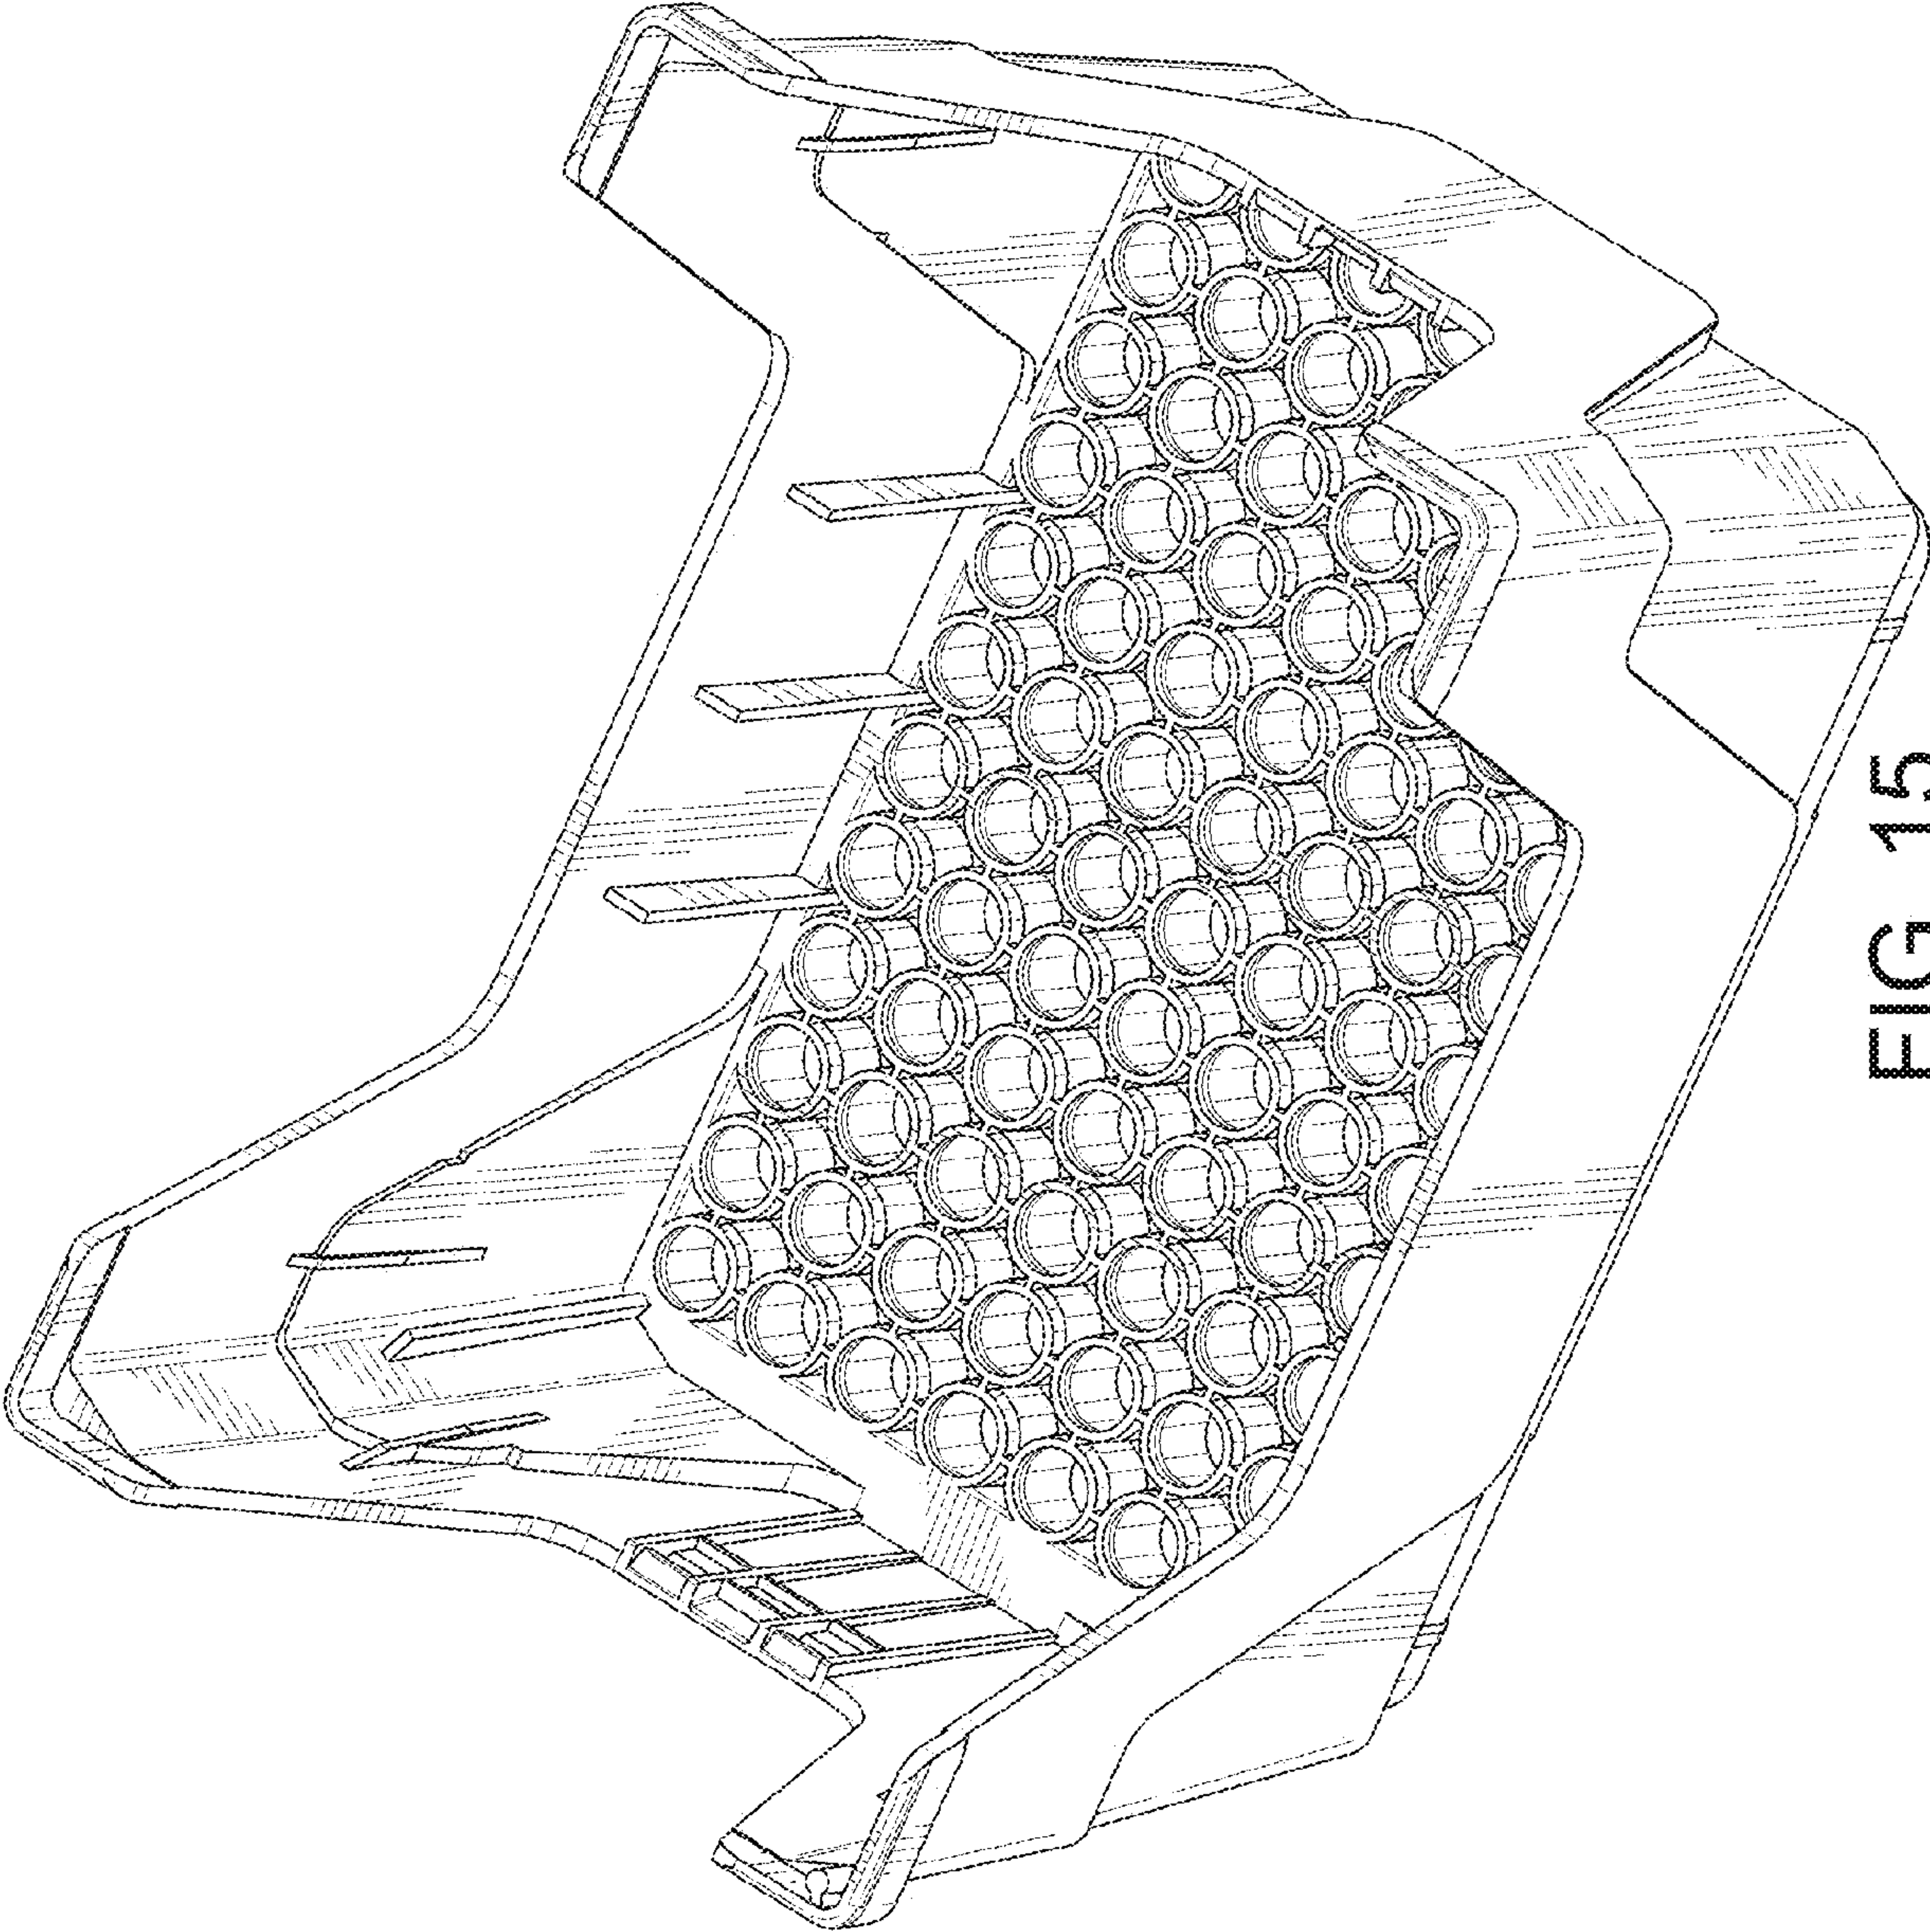


FIG. 15

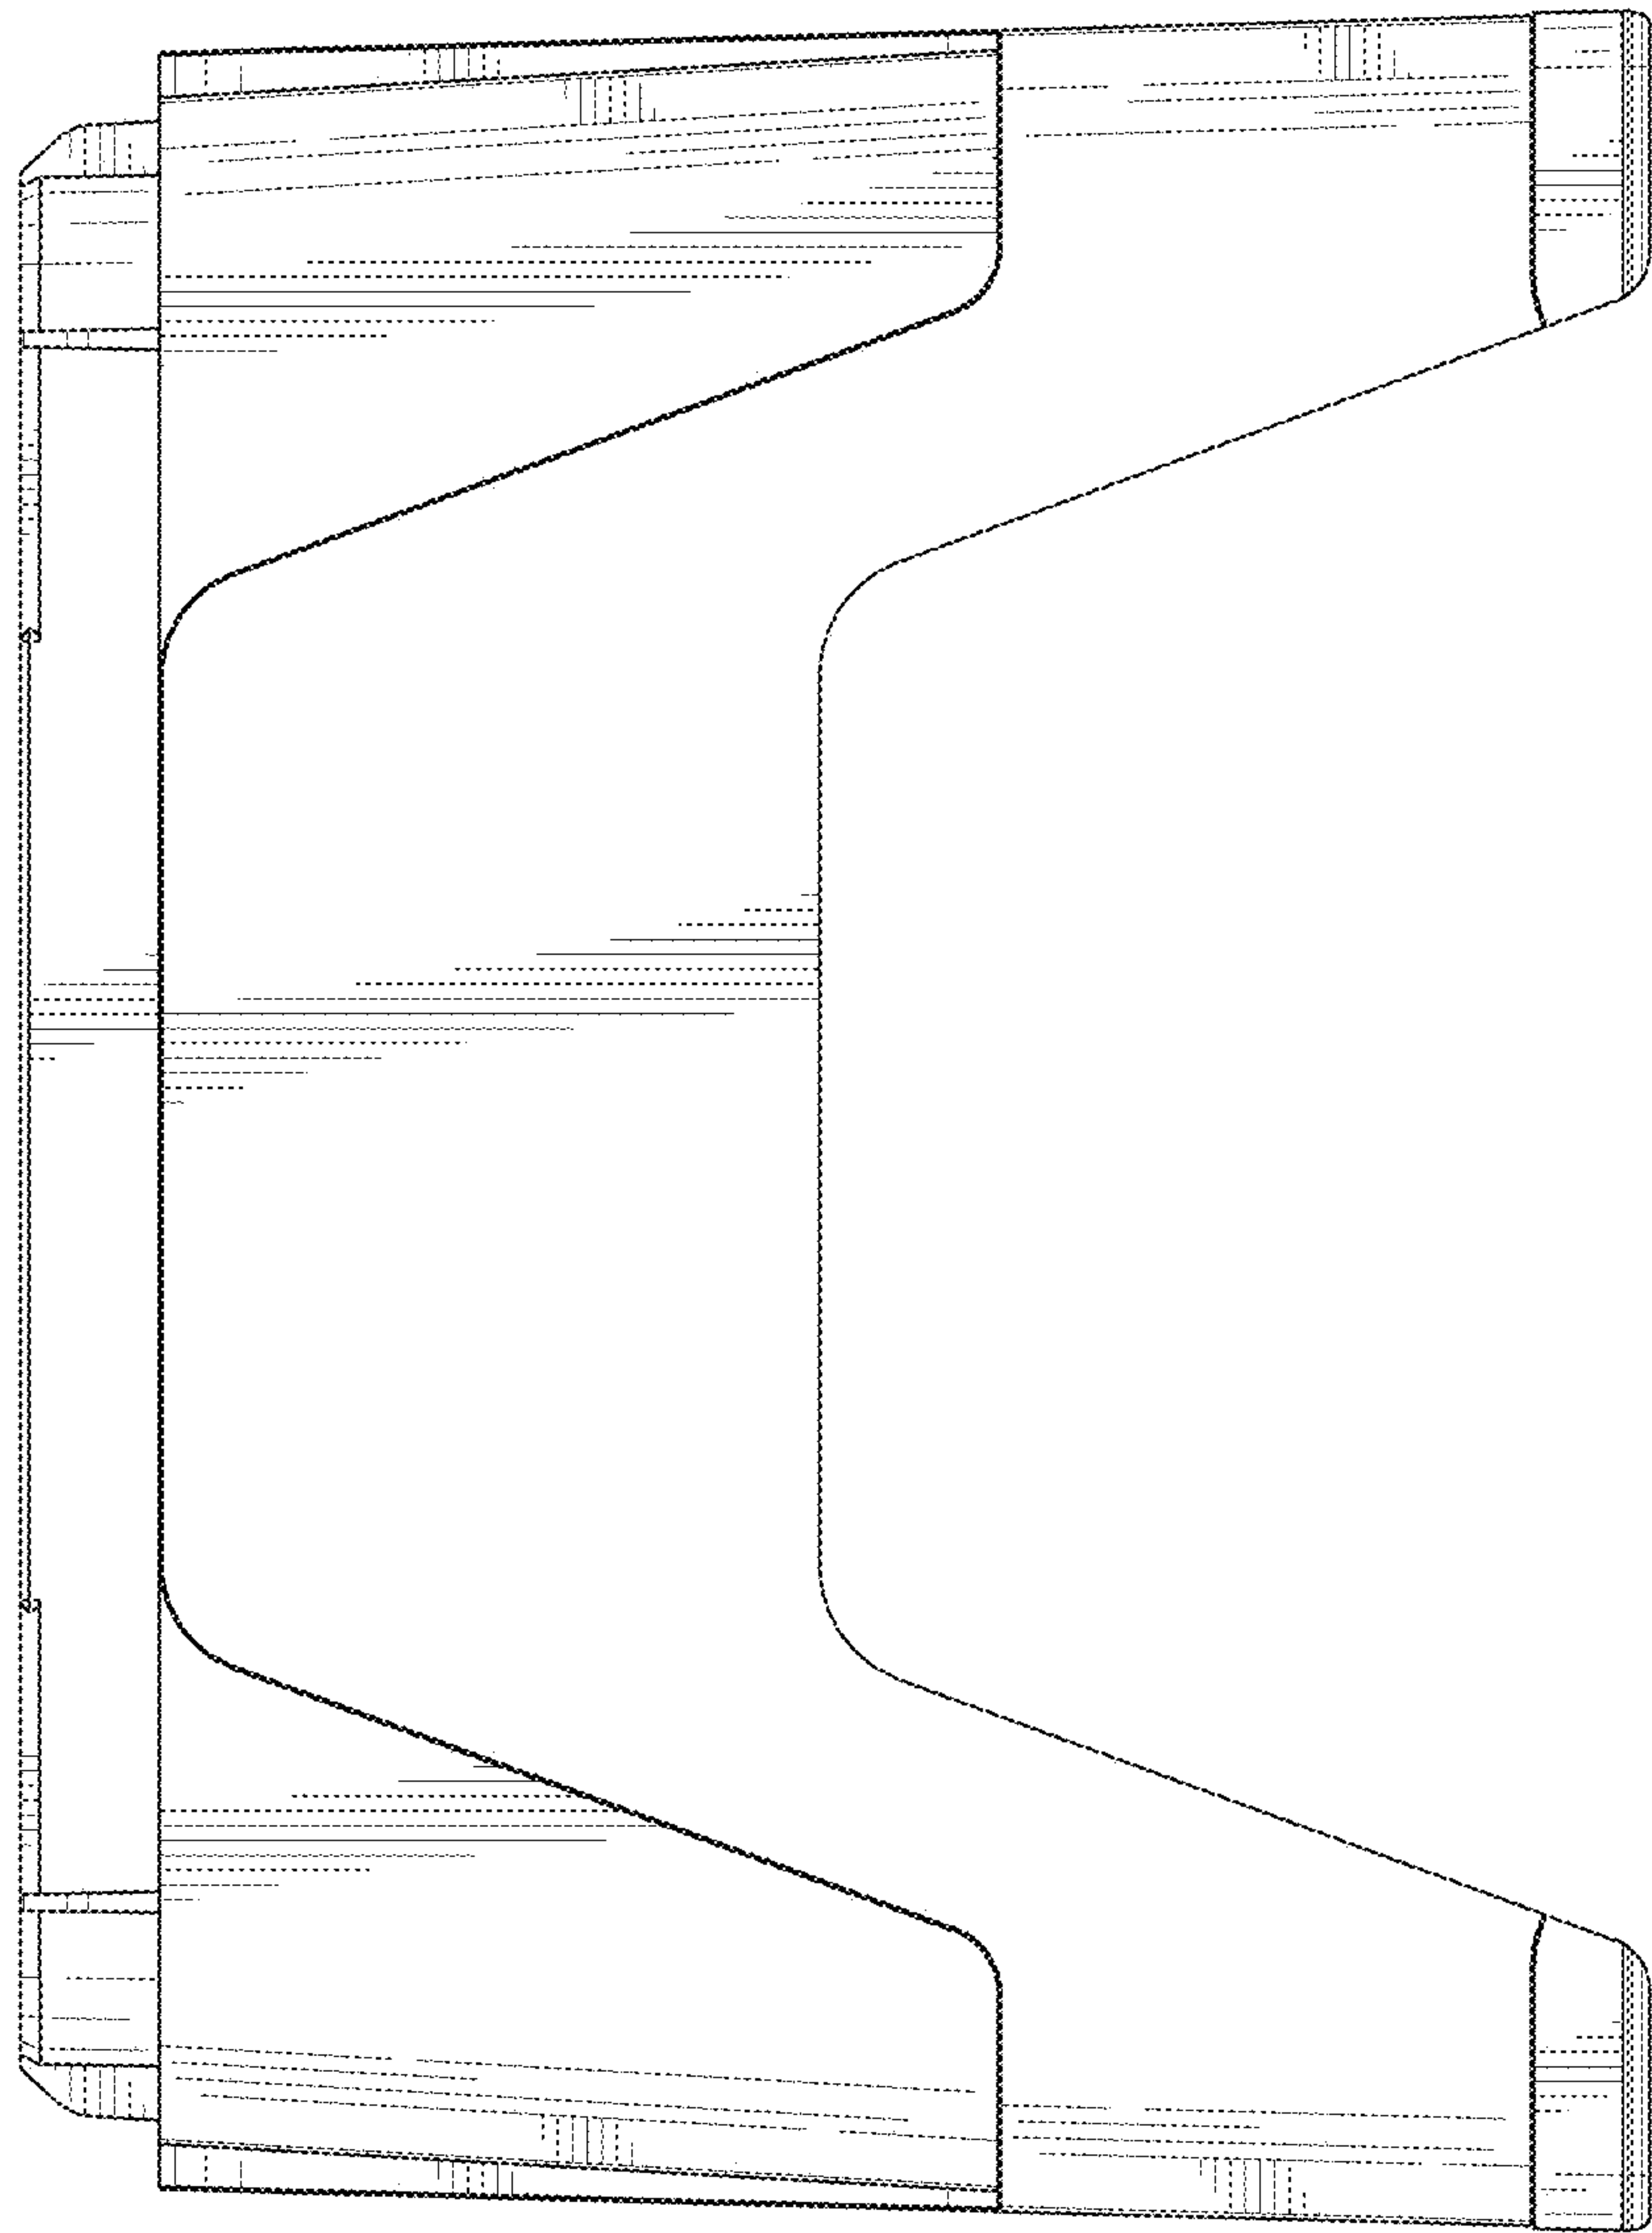


FIG. 16

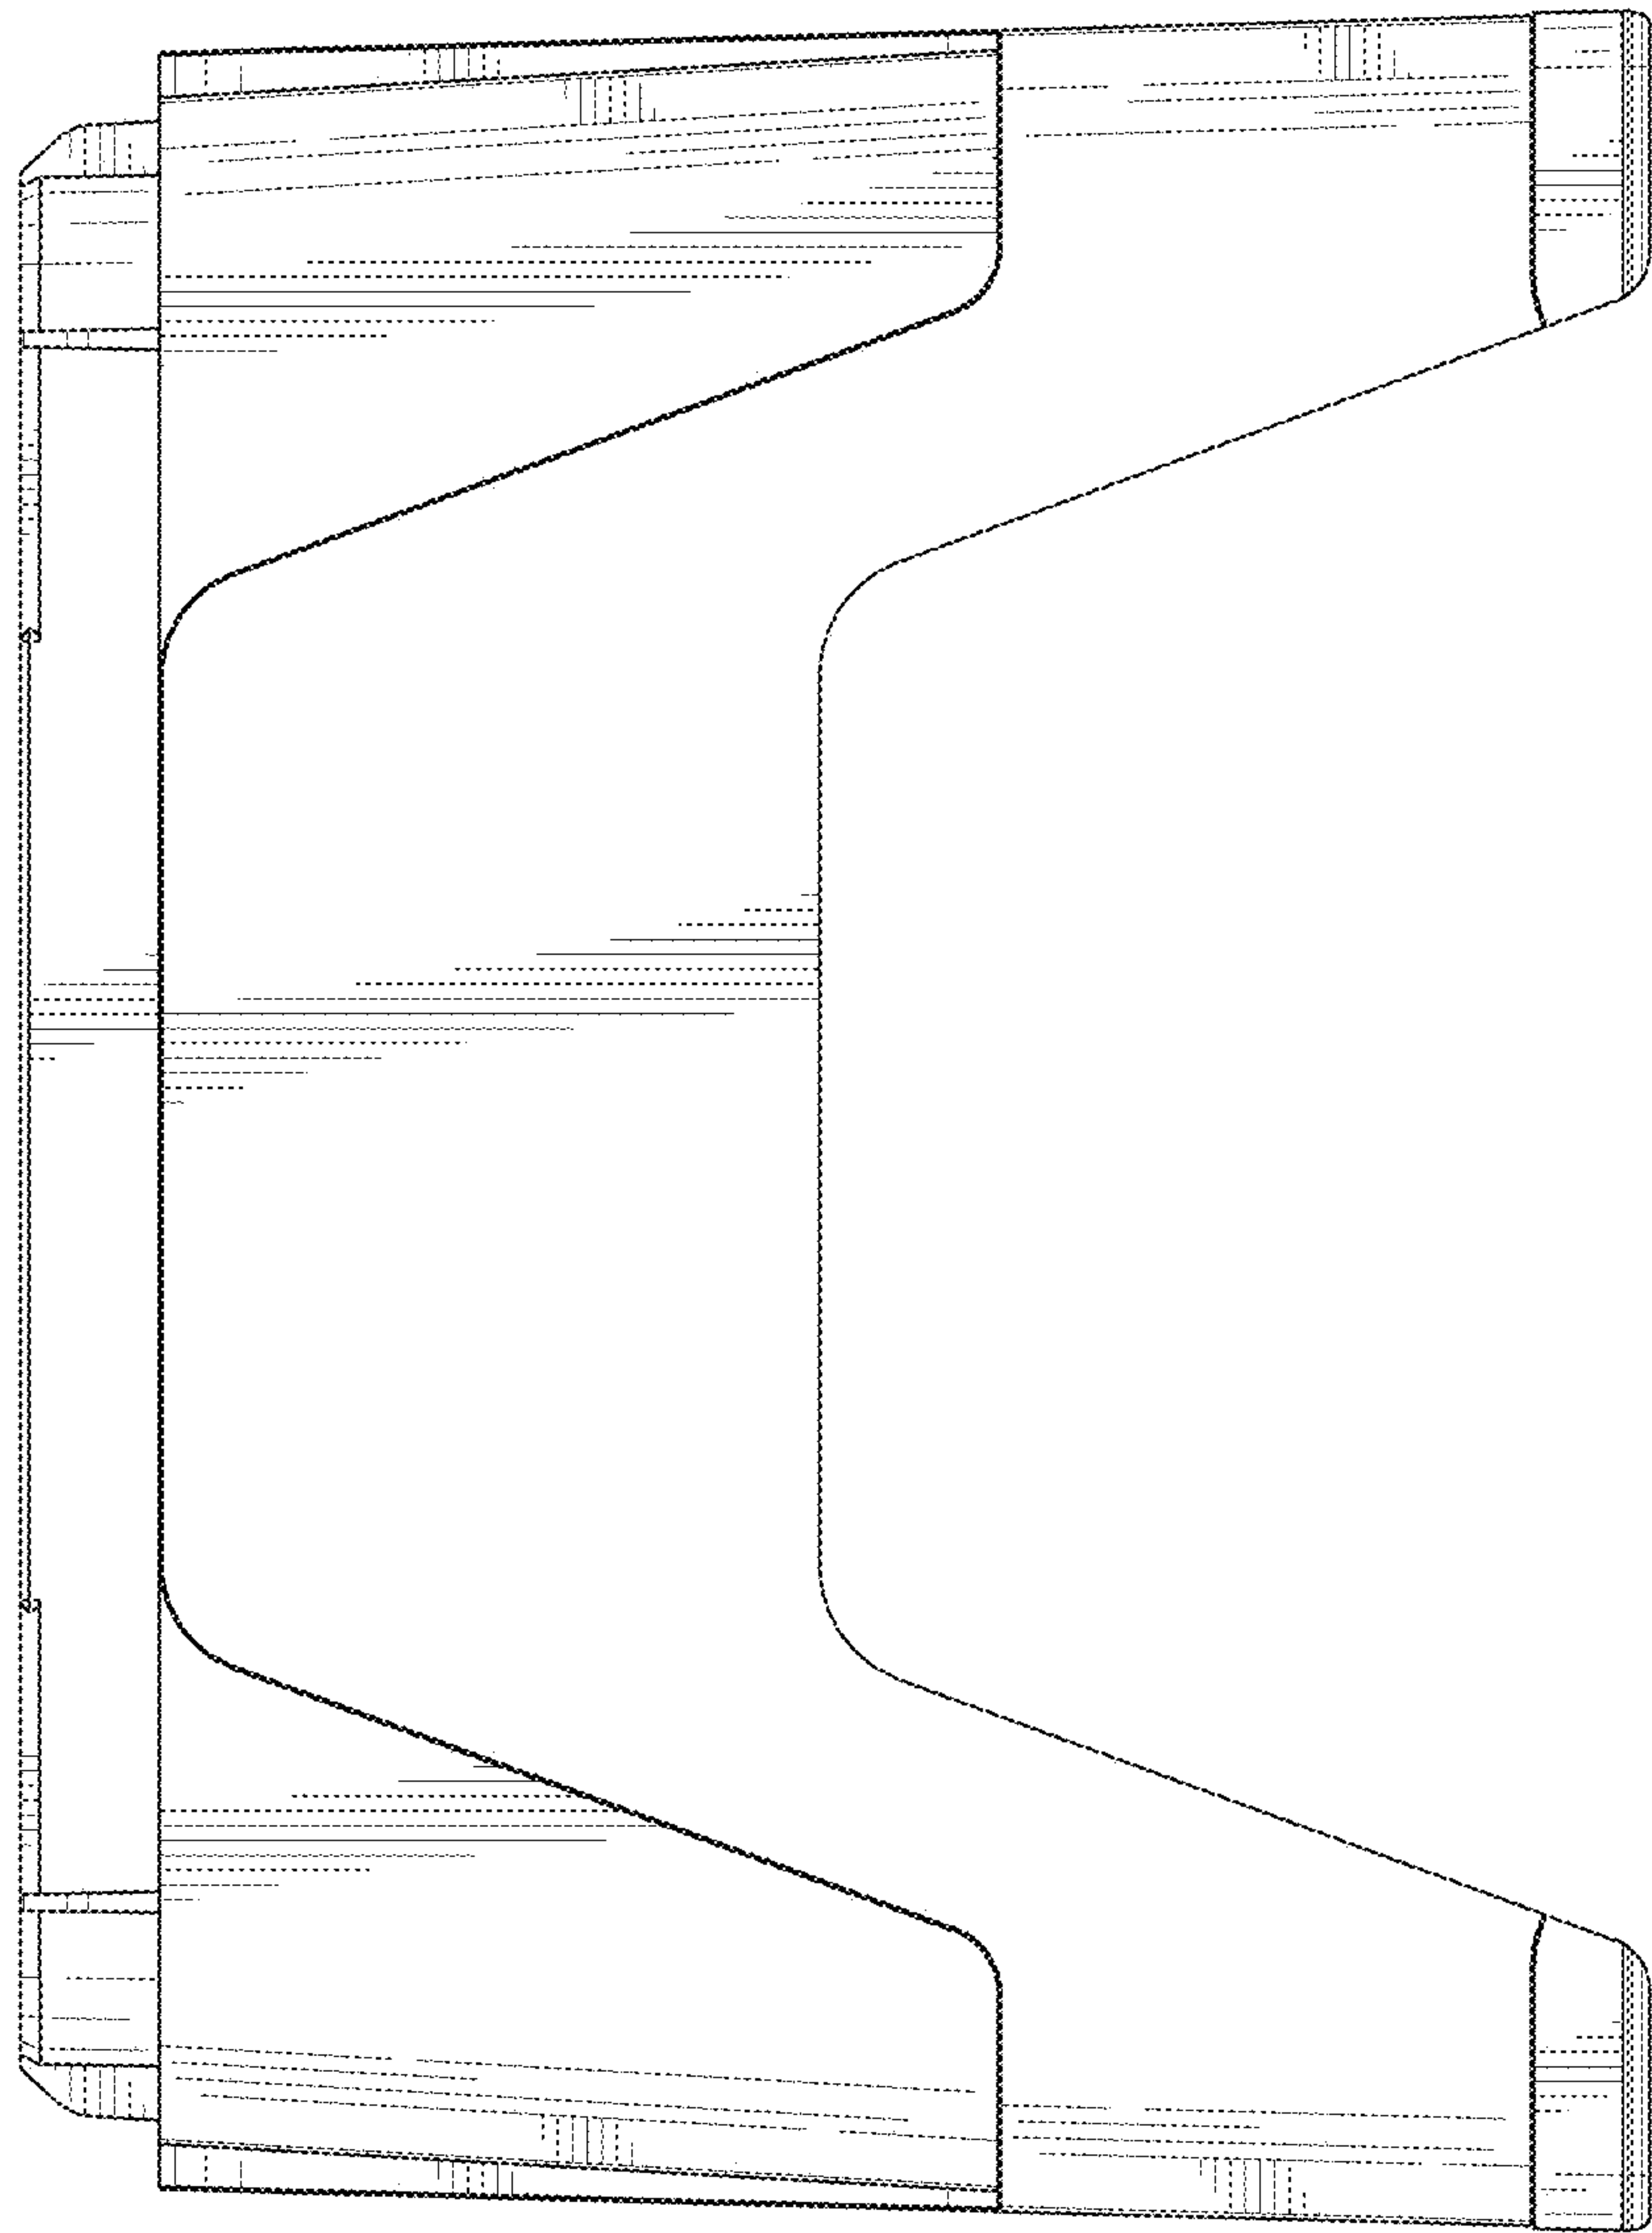


FIG. 17

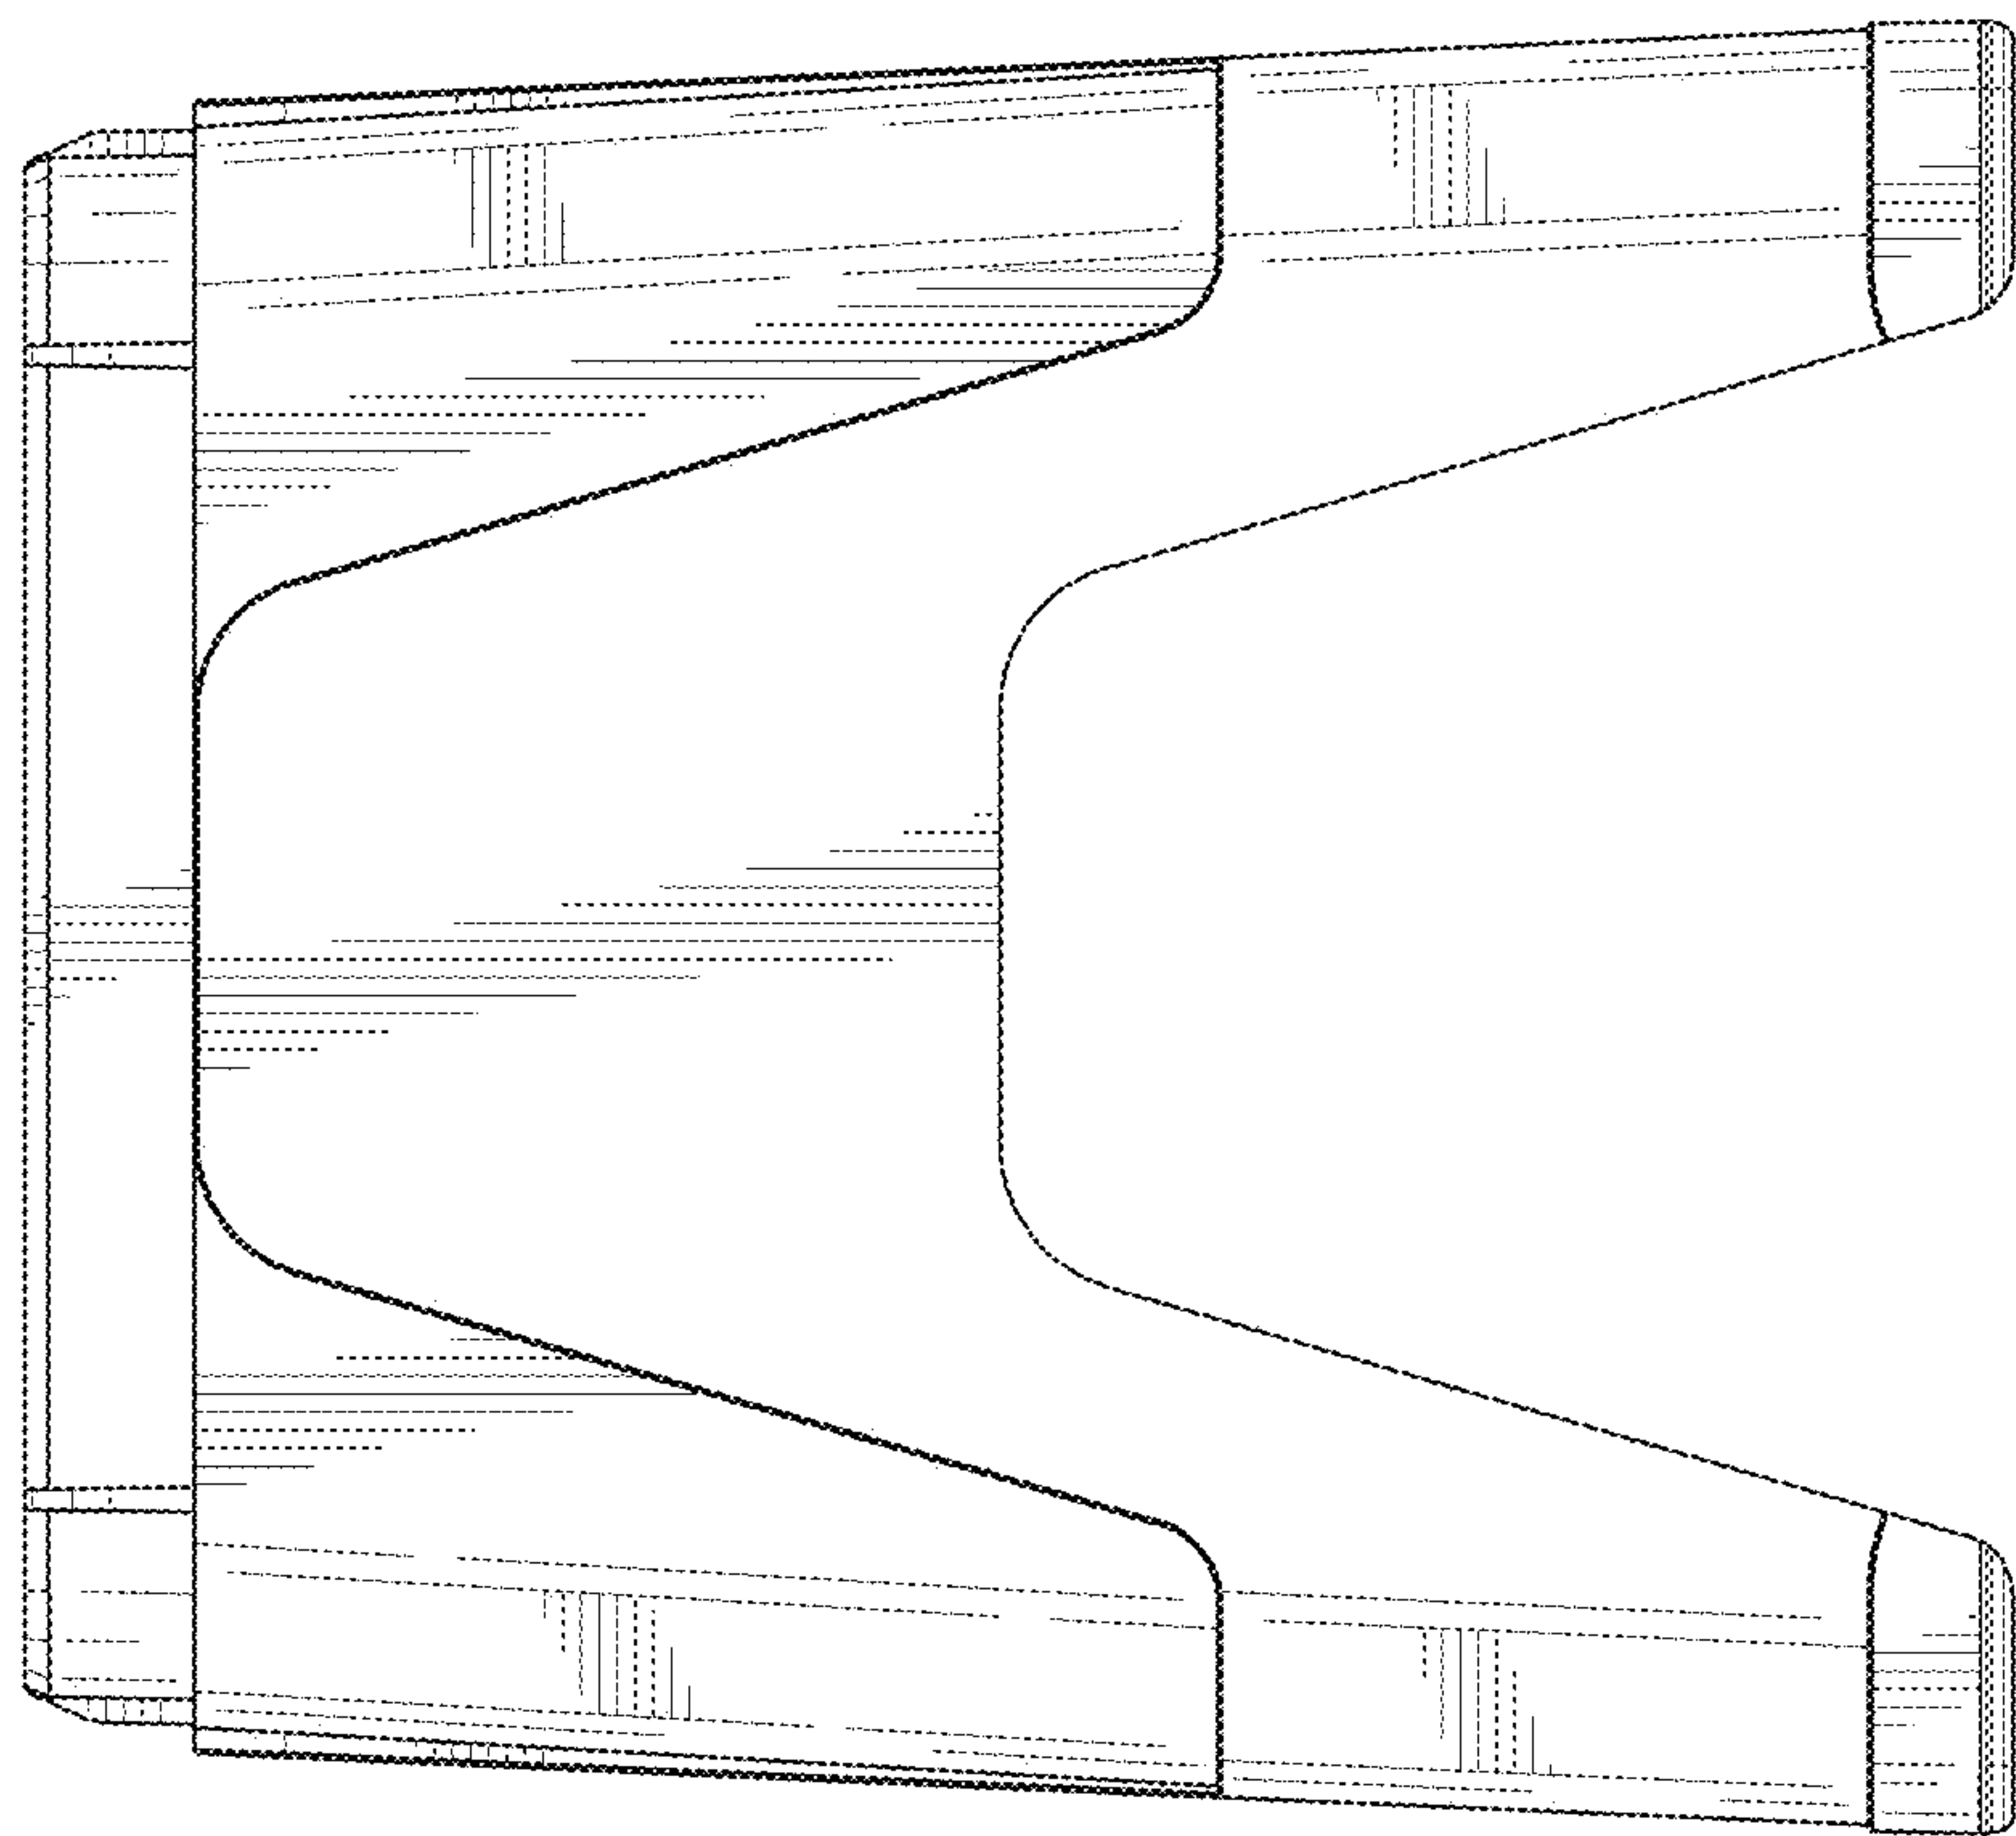


FIG. 18

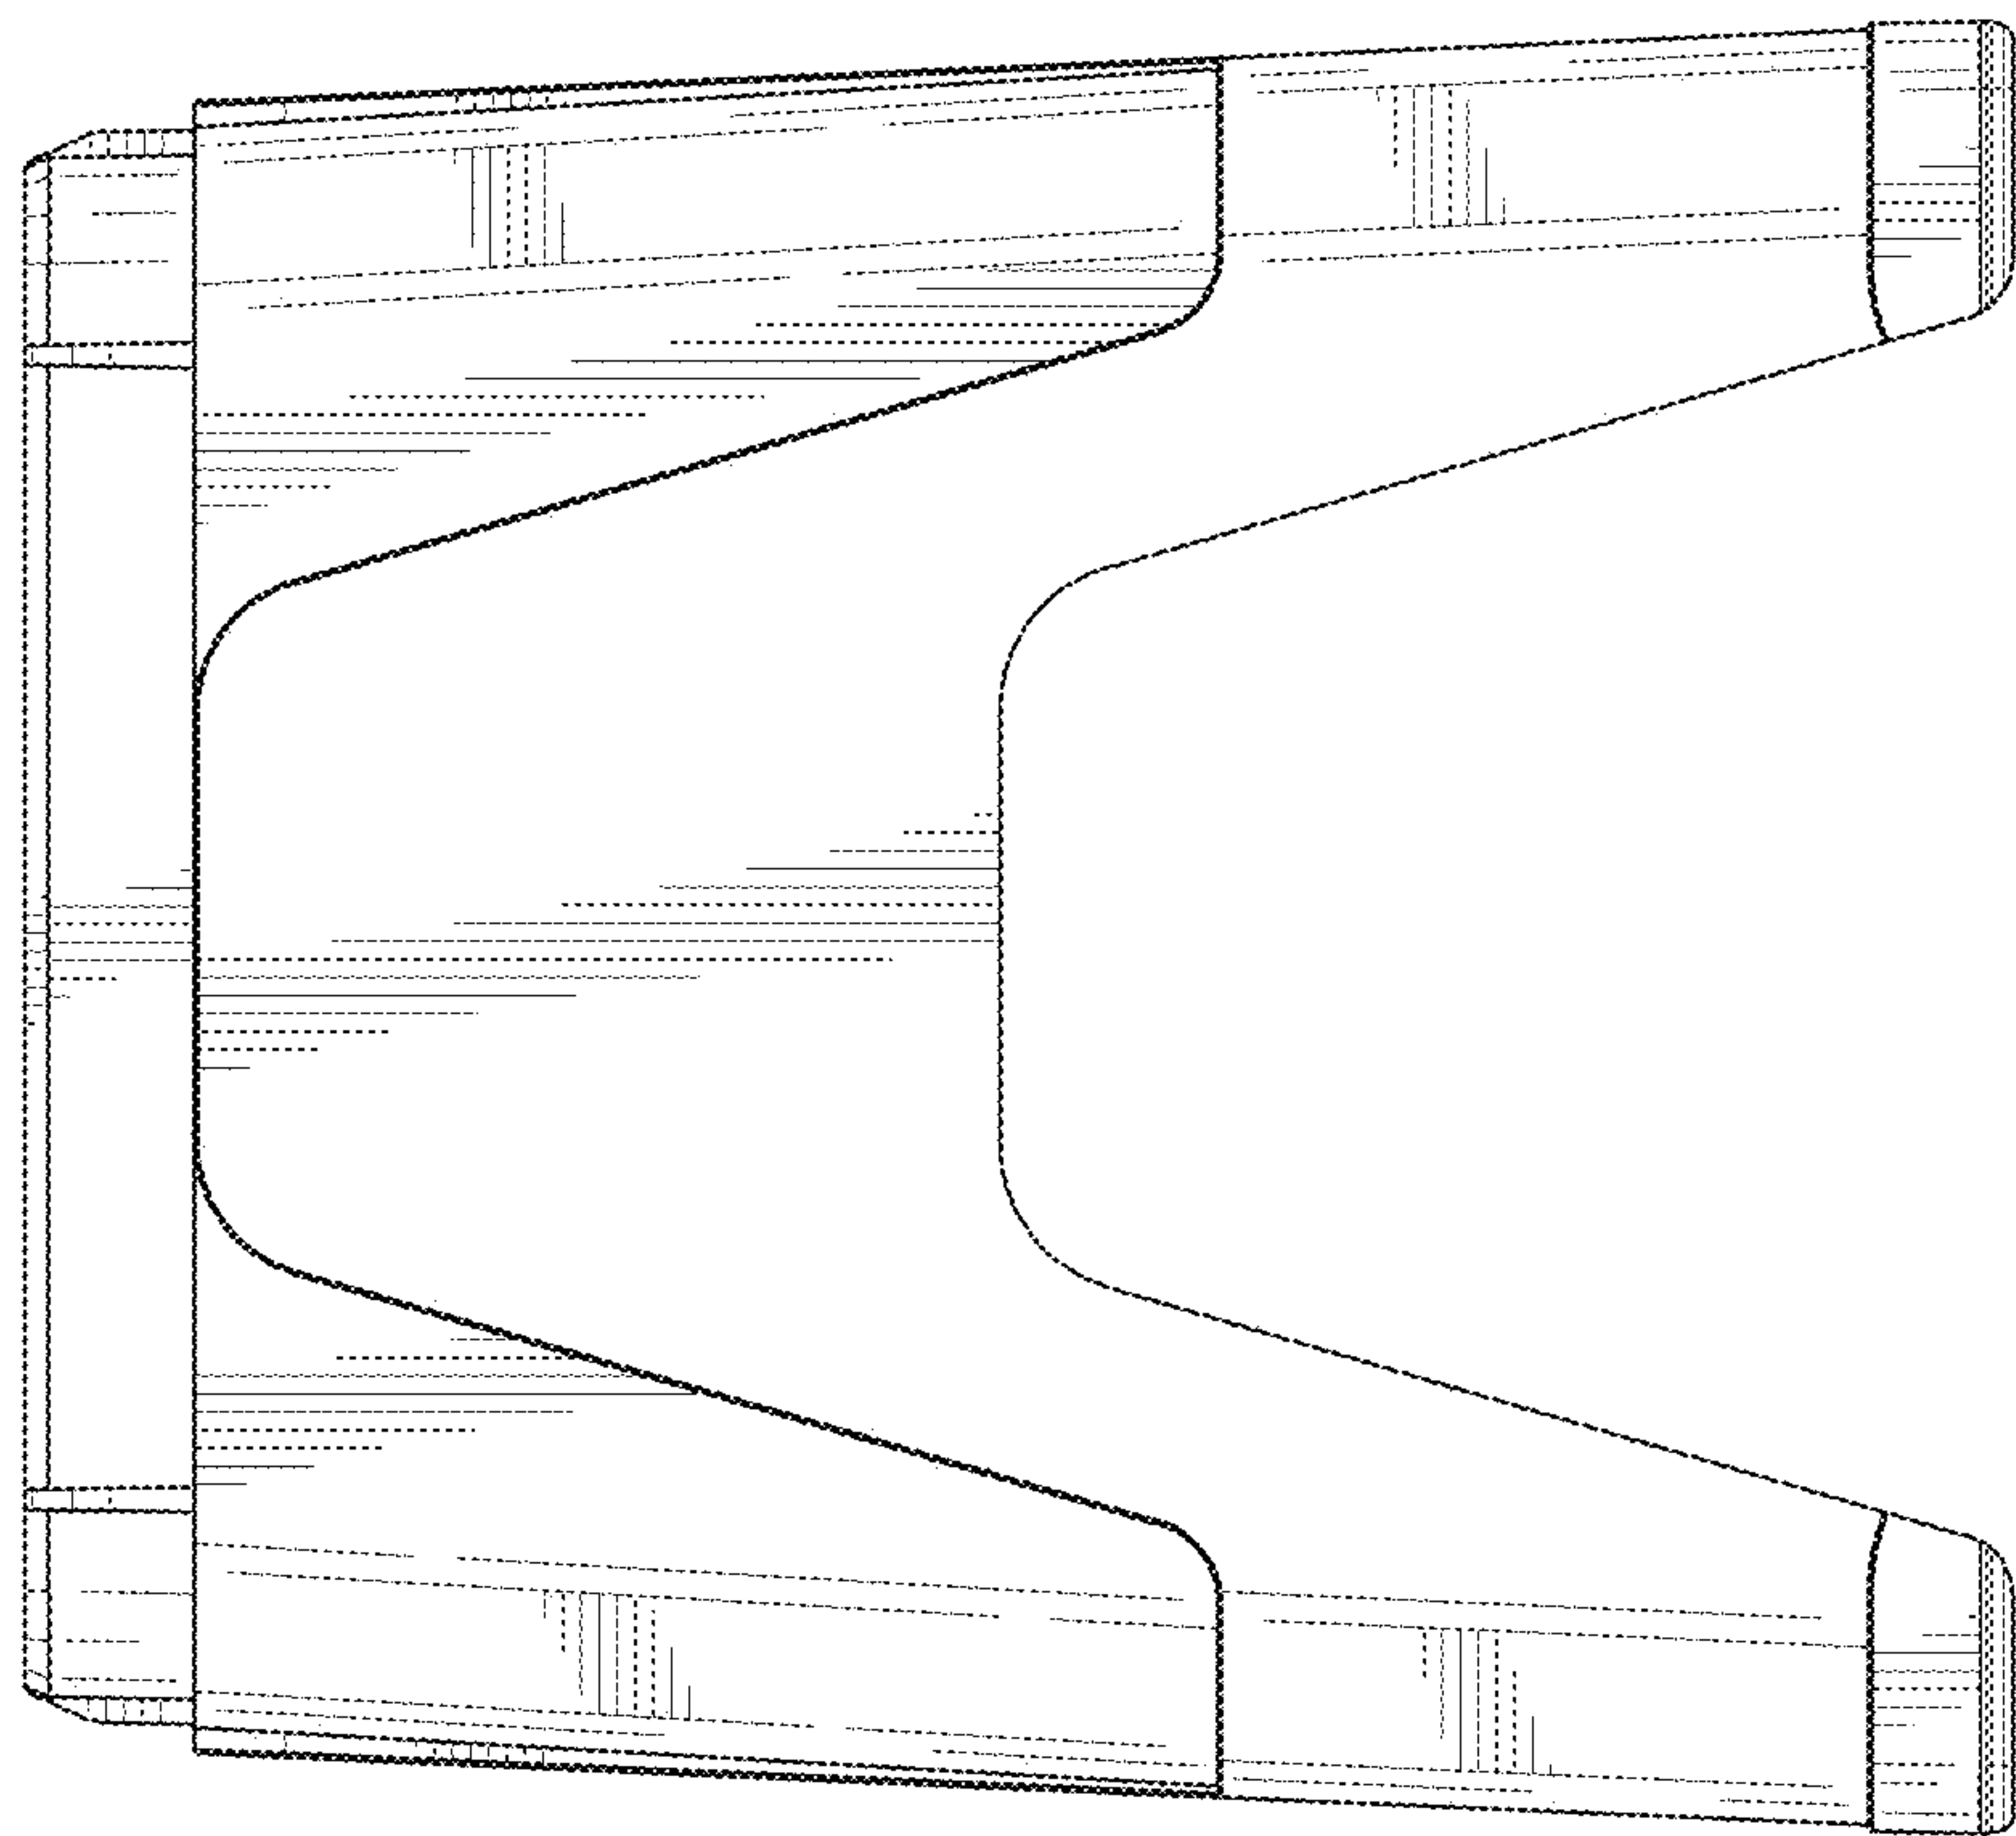


FIG. 19

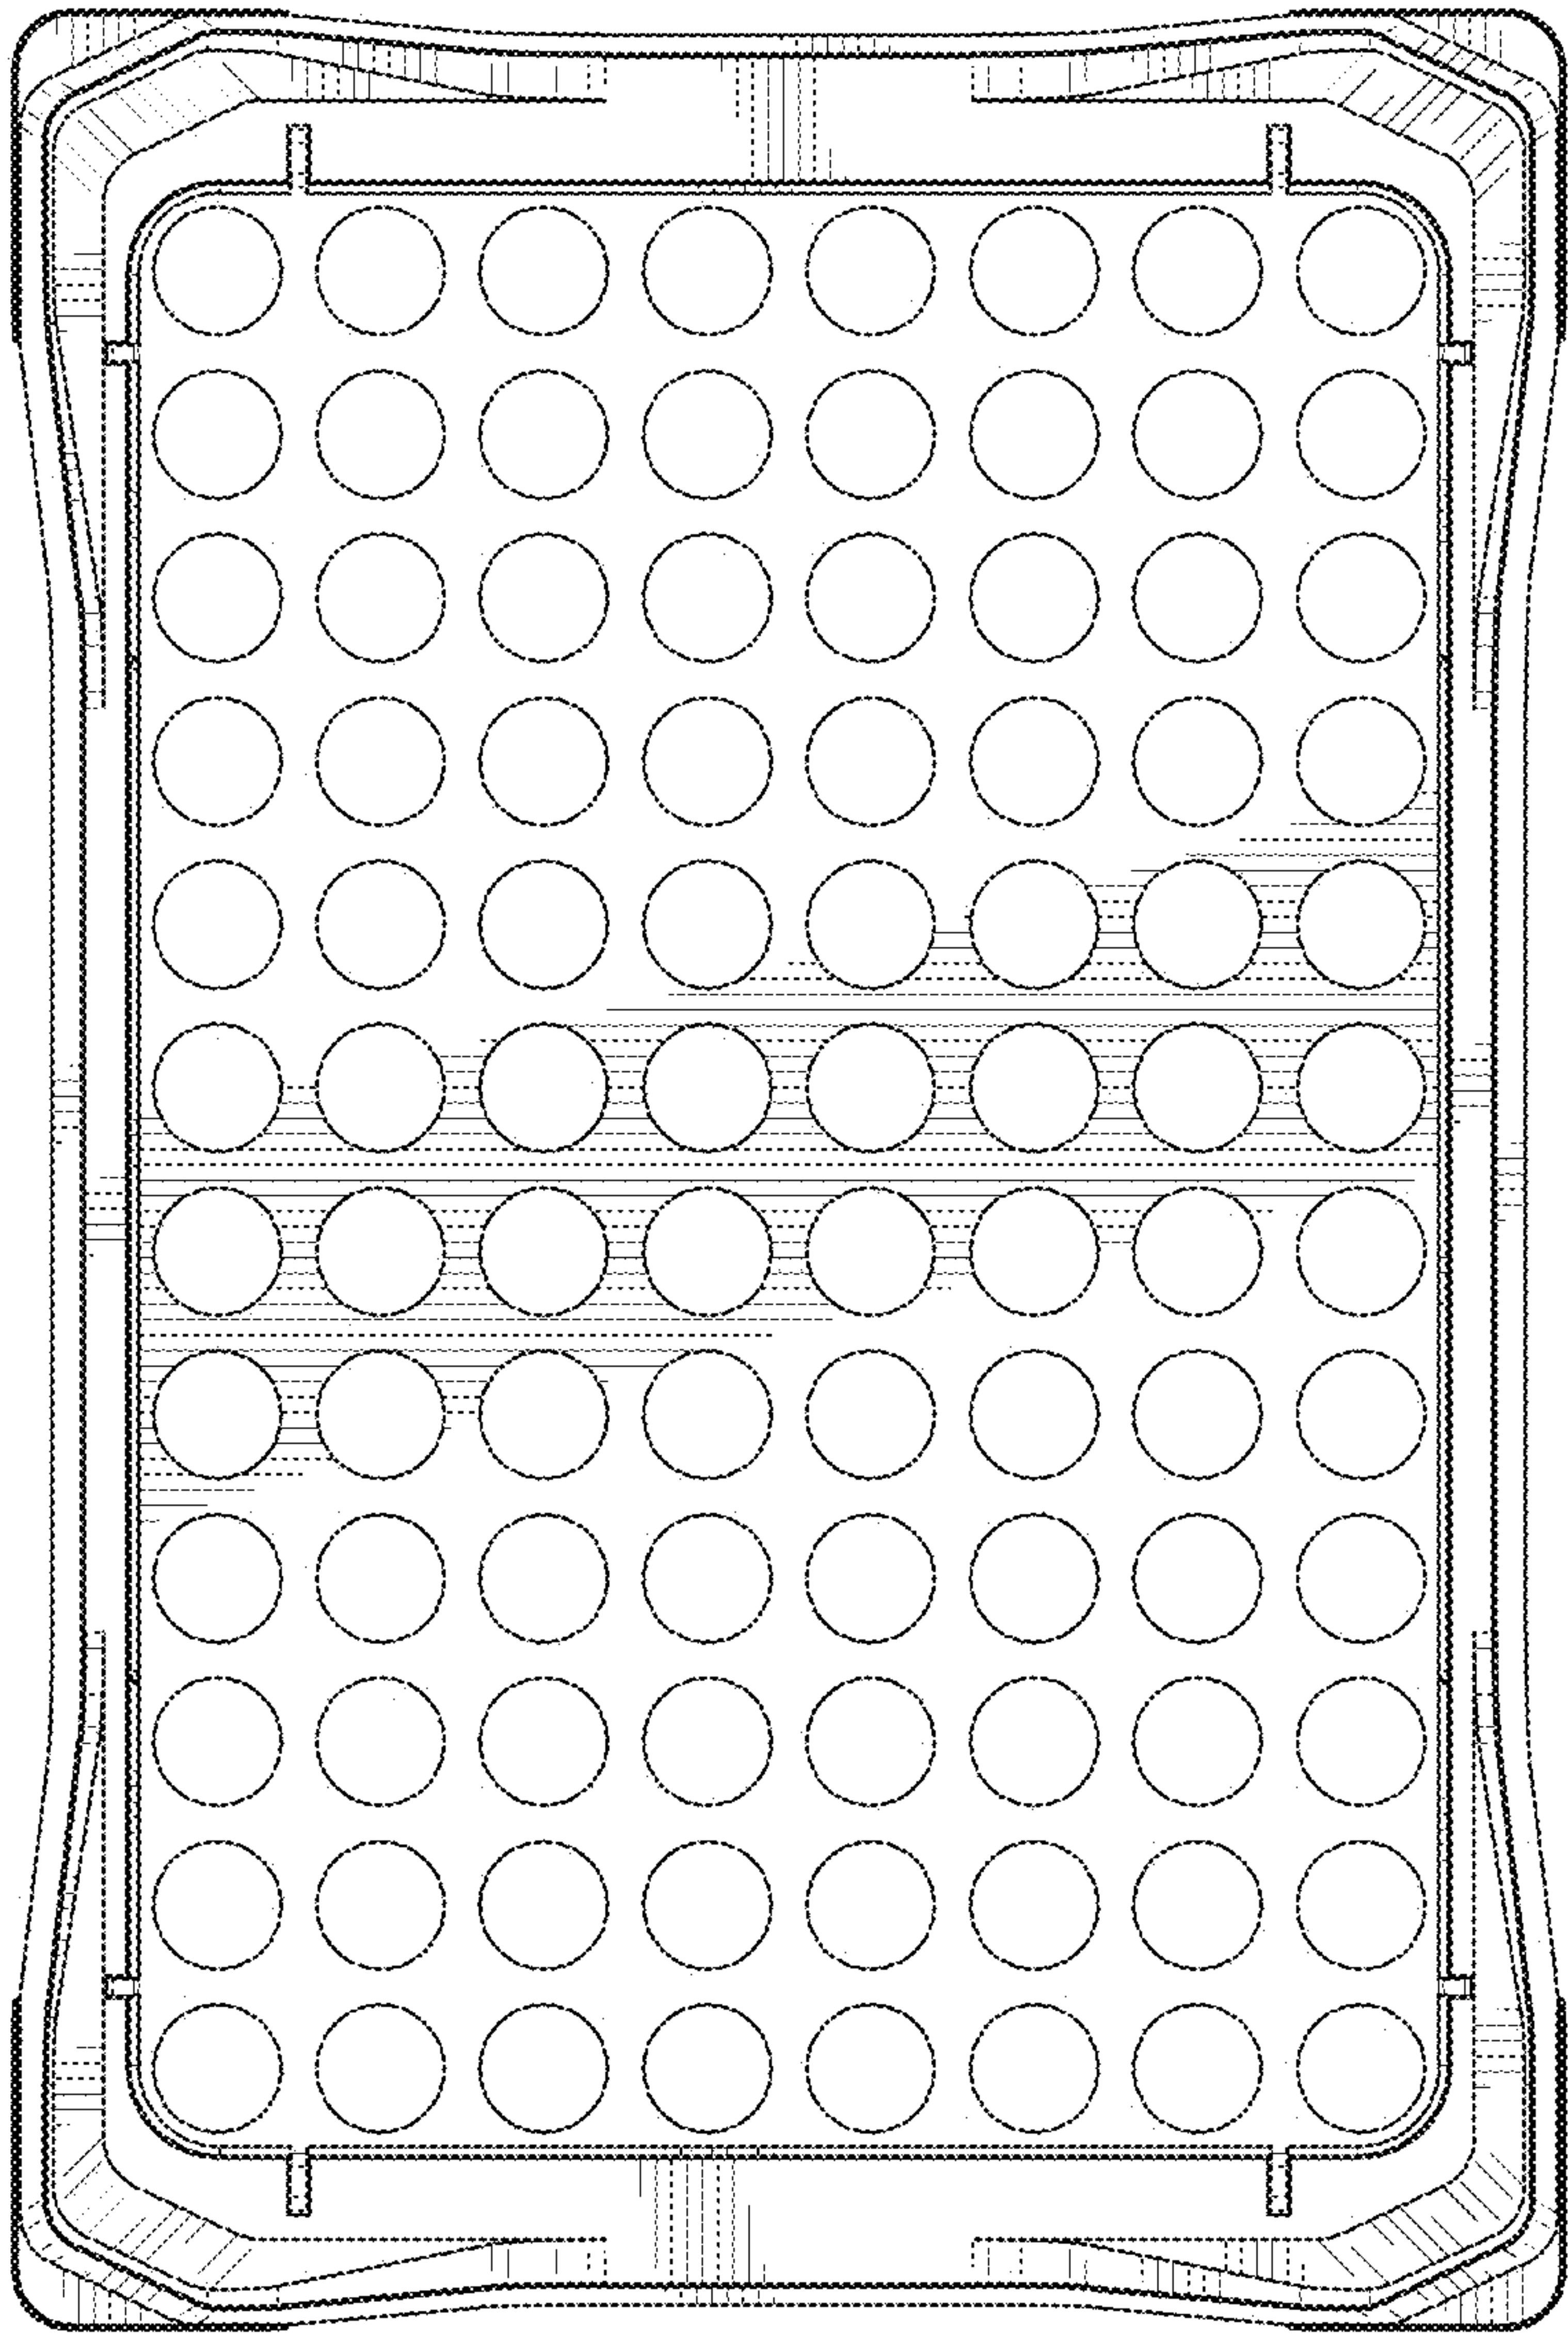


FIG. 20

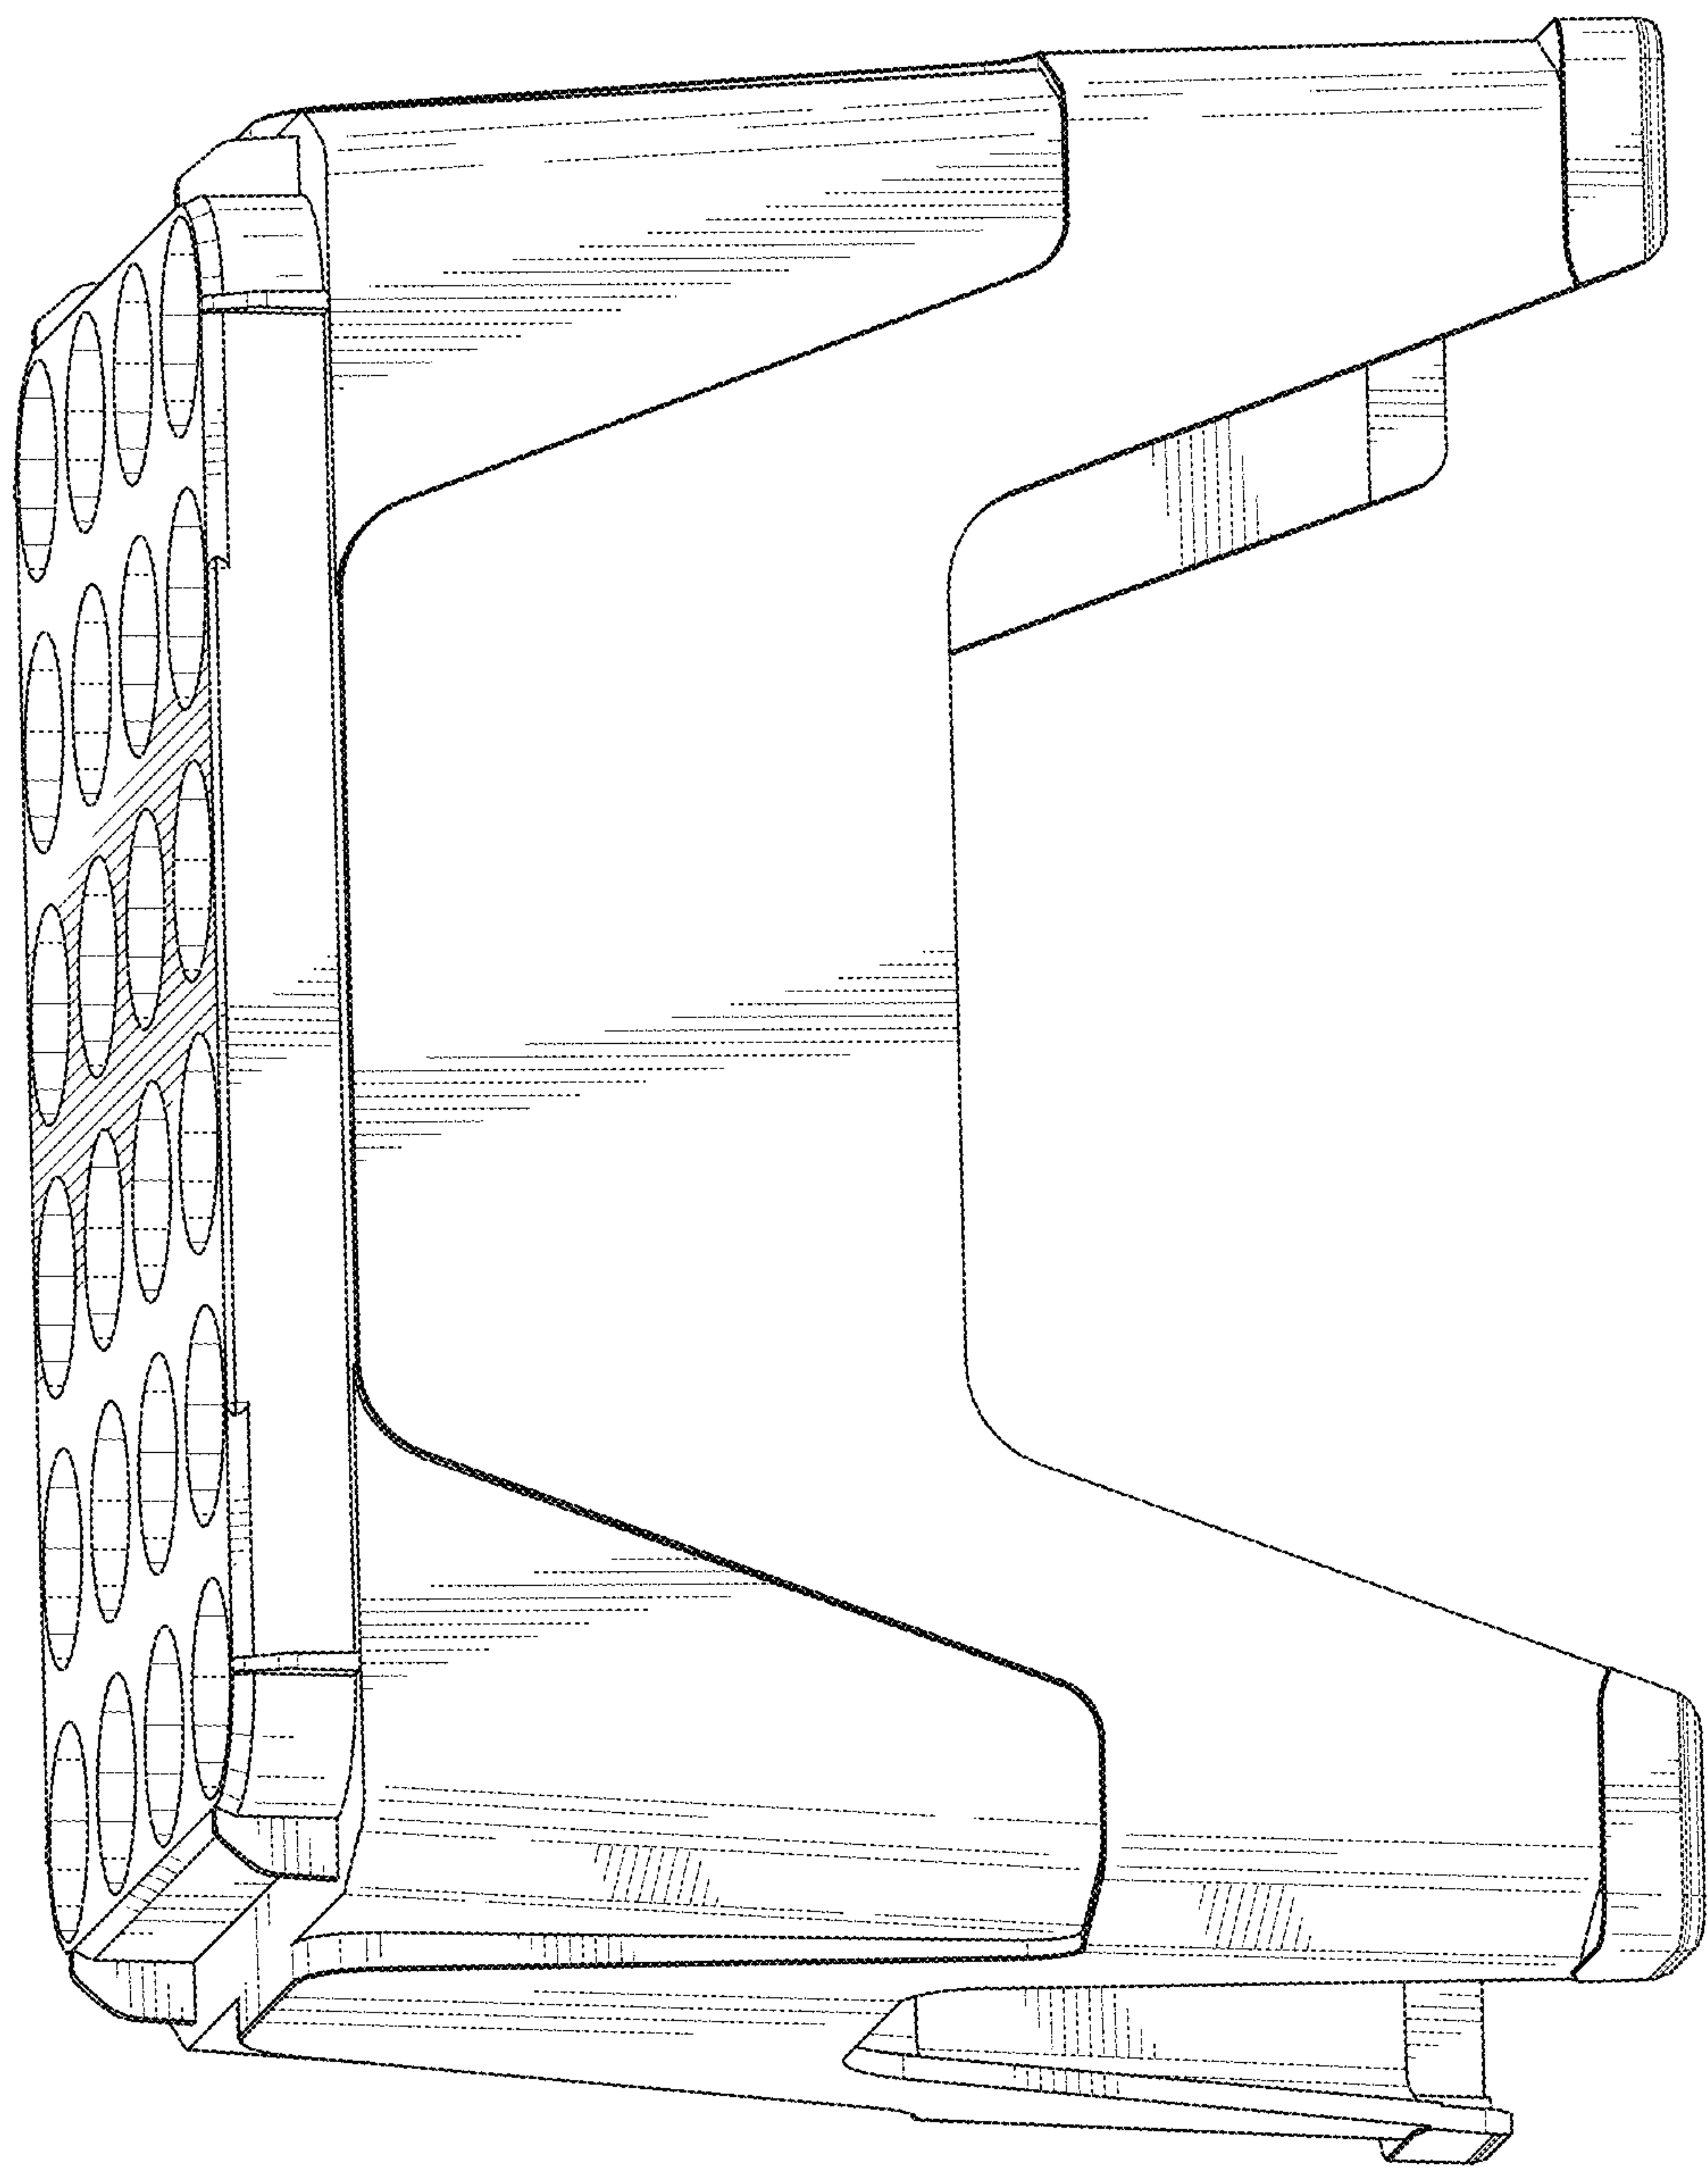


FIG. 21

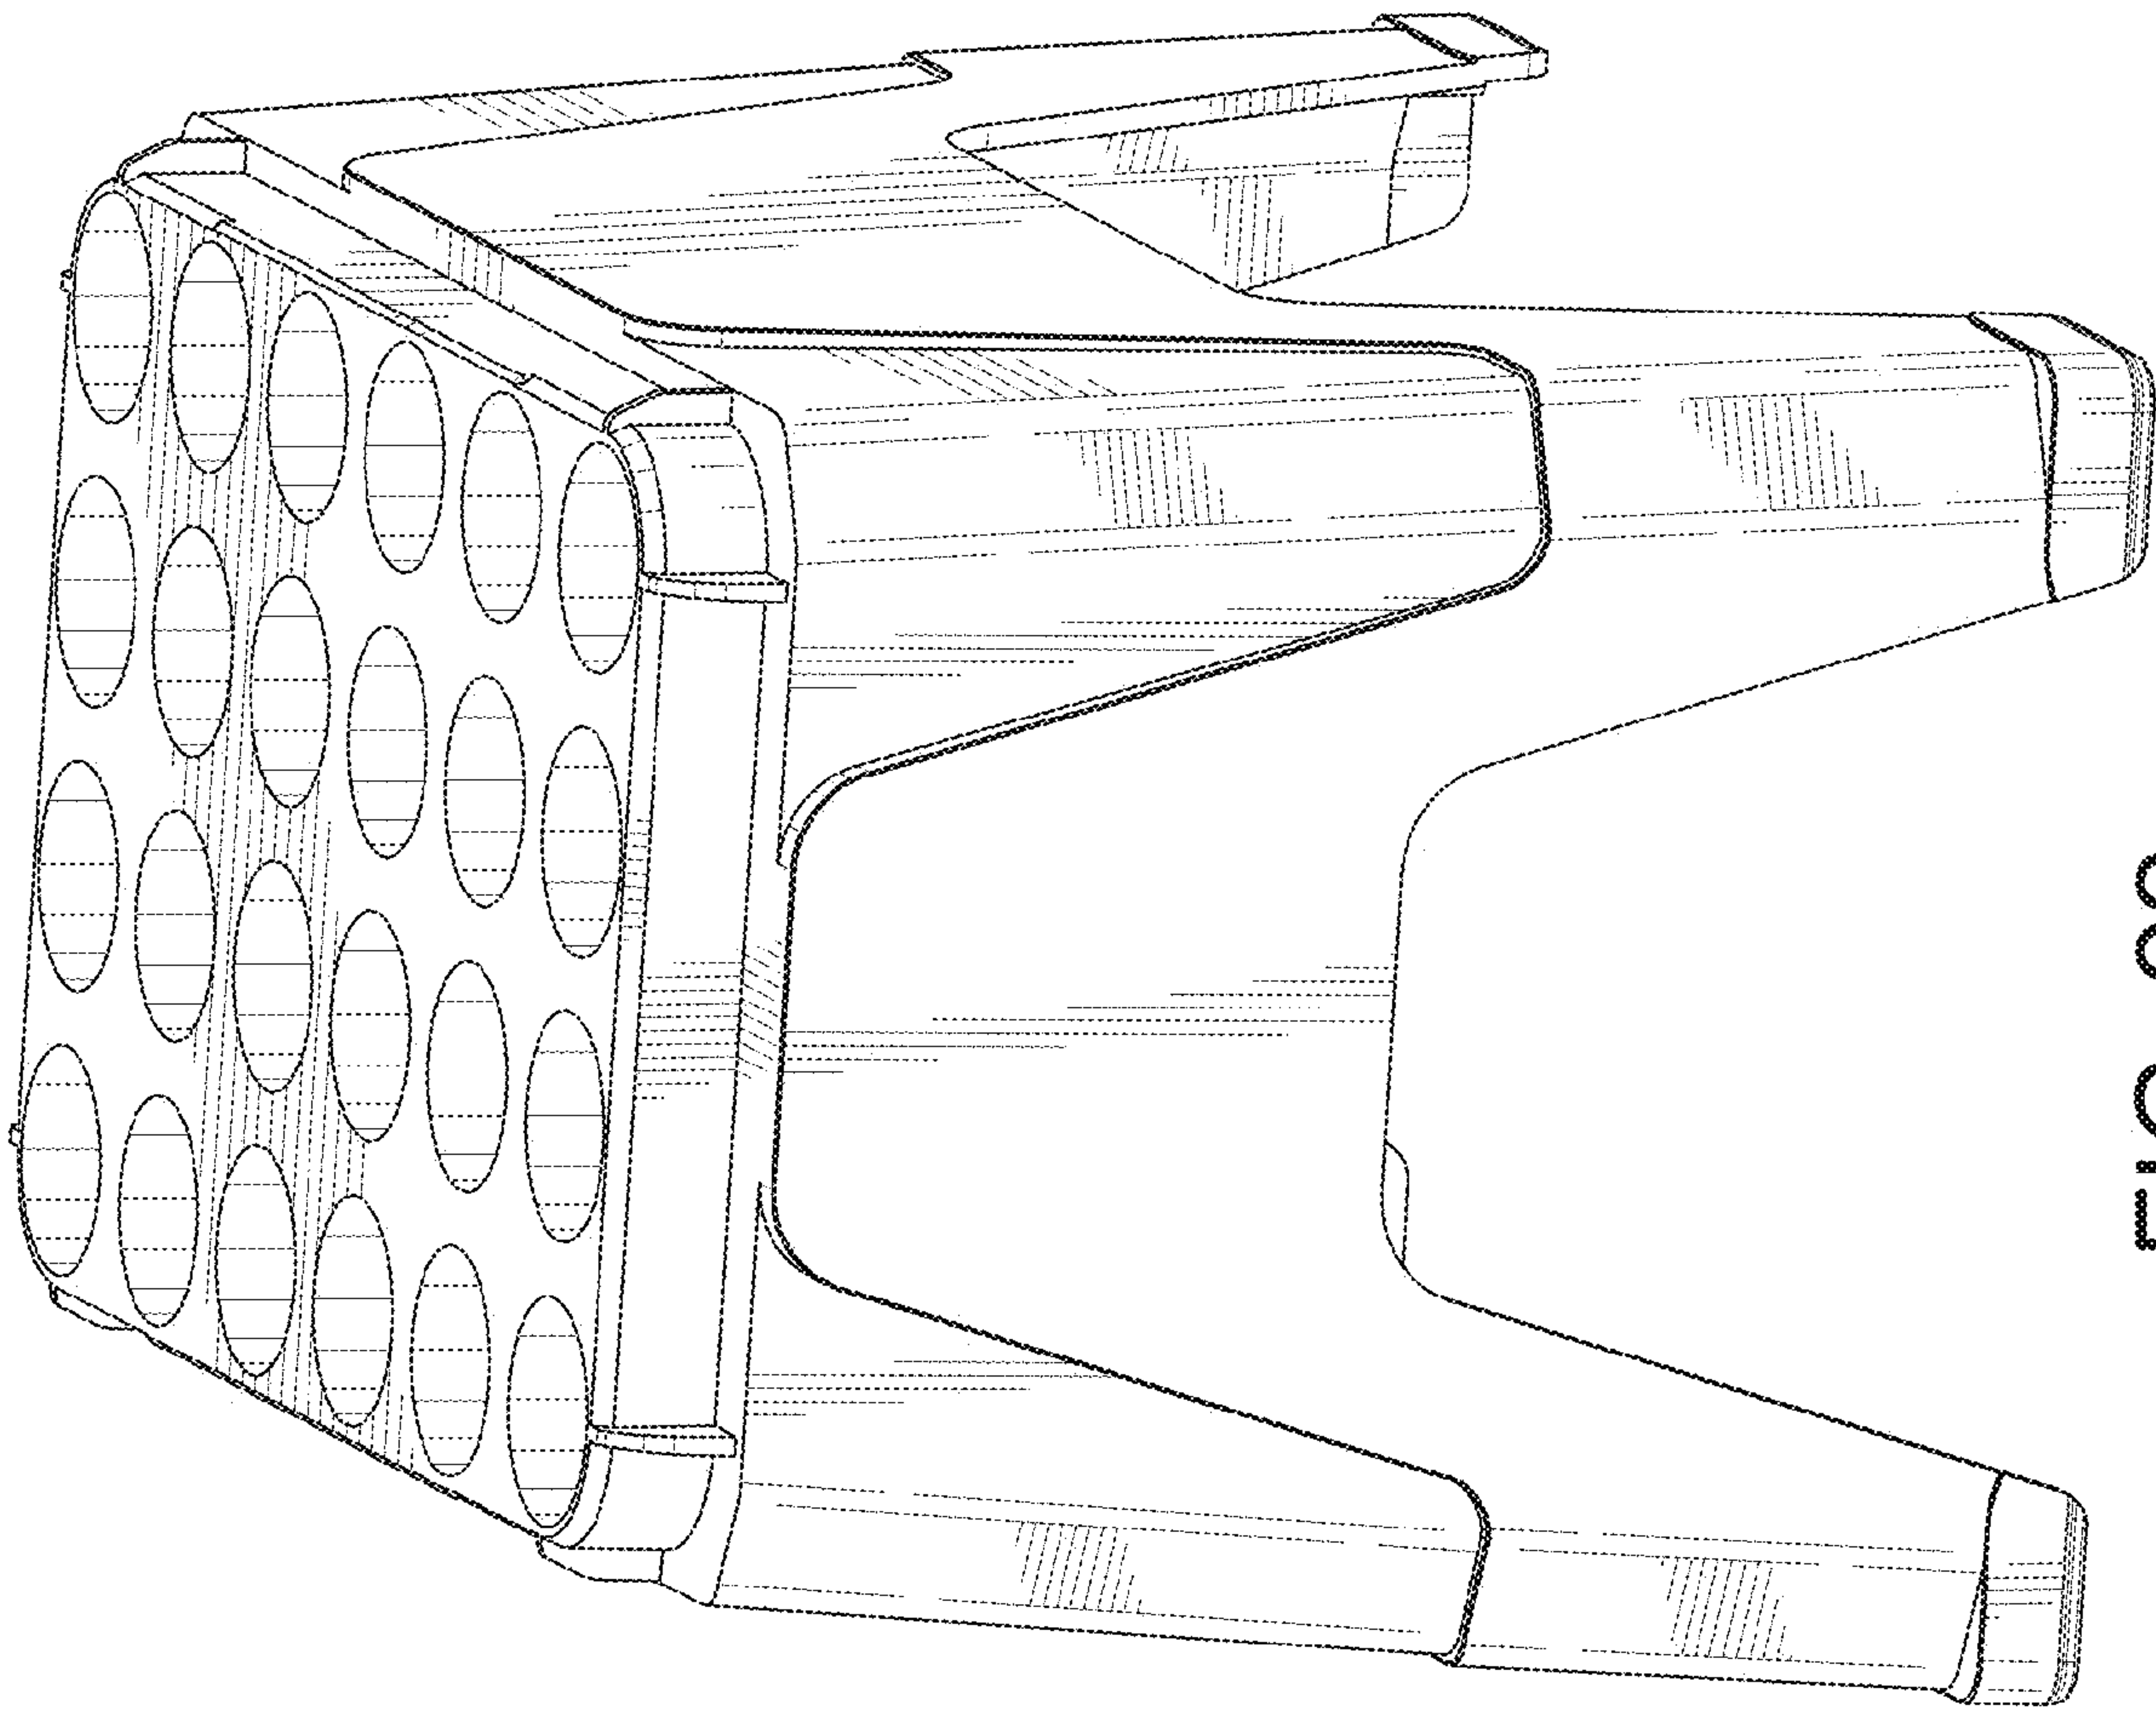


FIG. 22

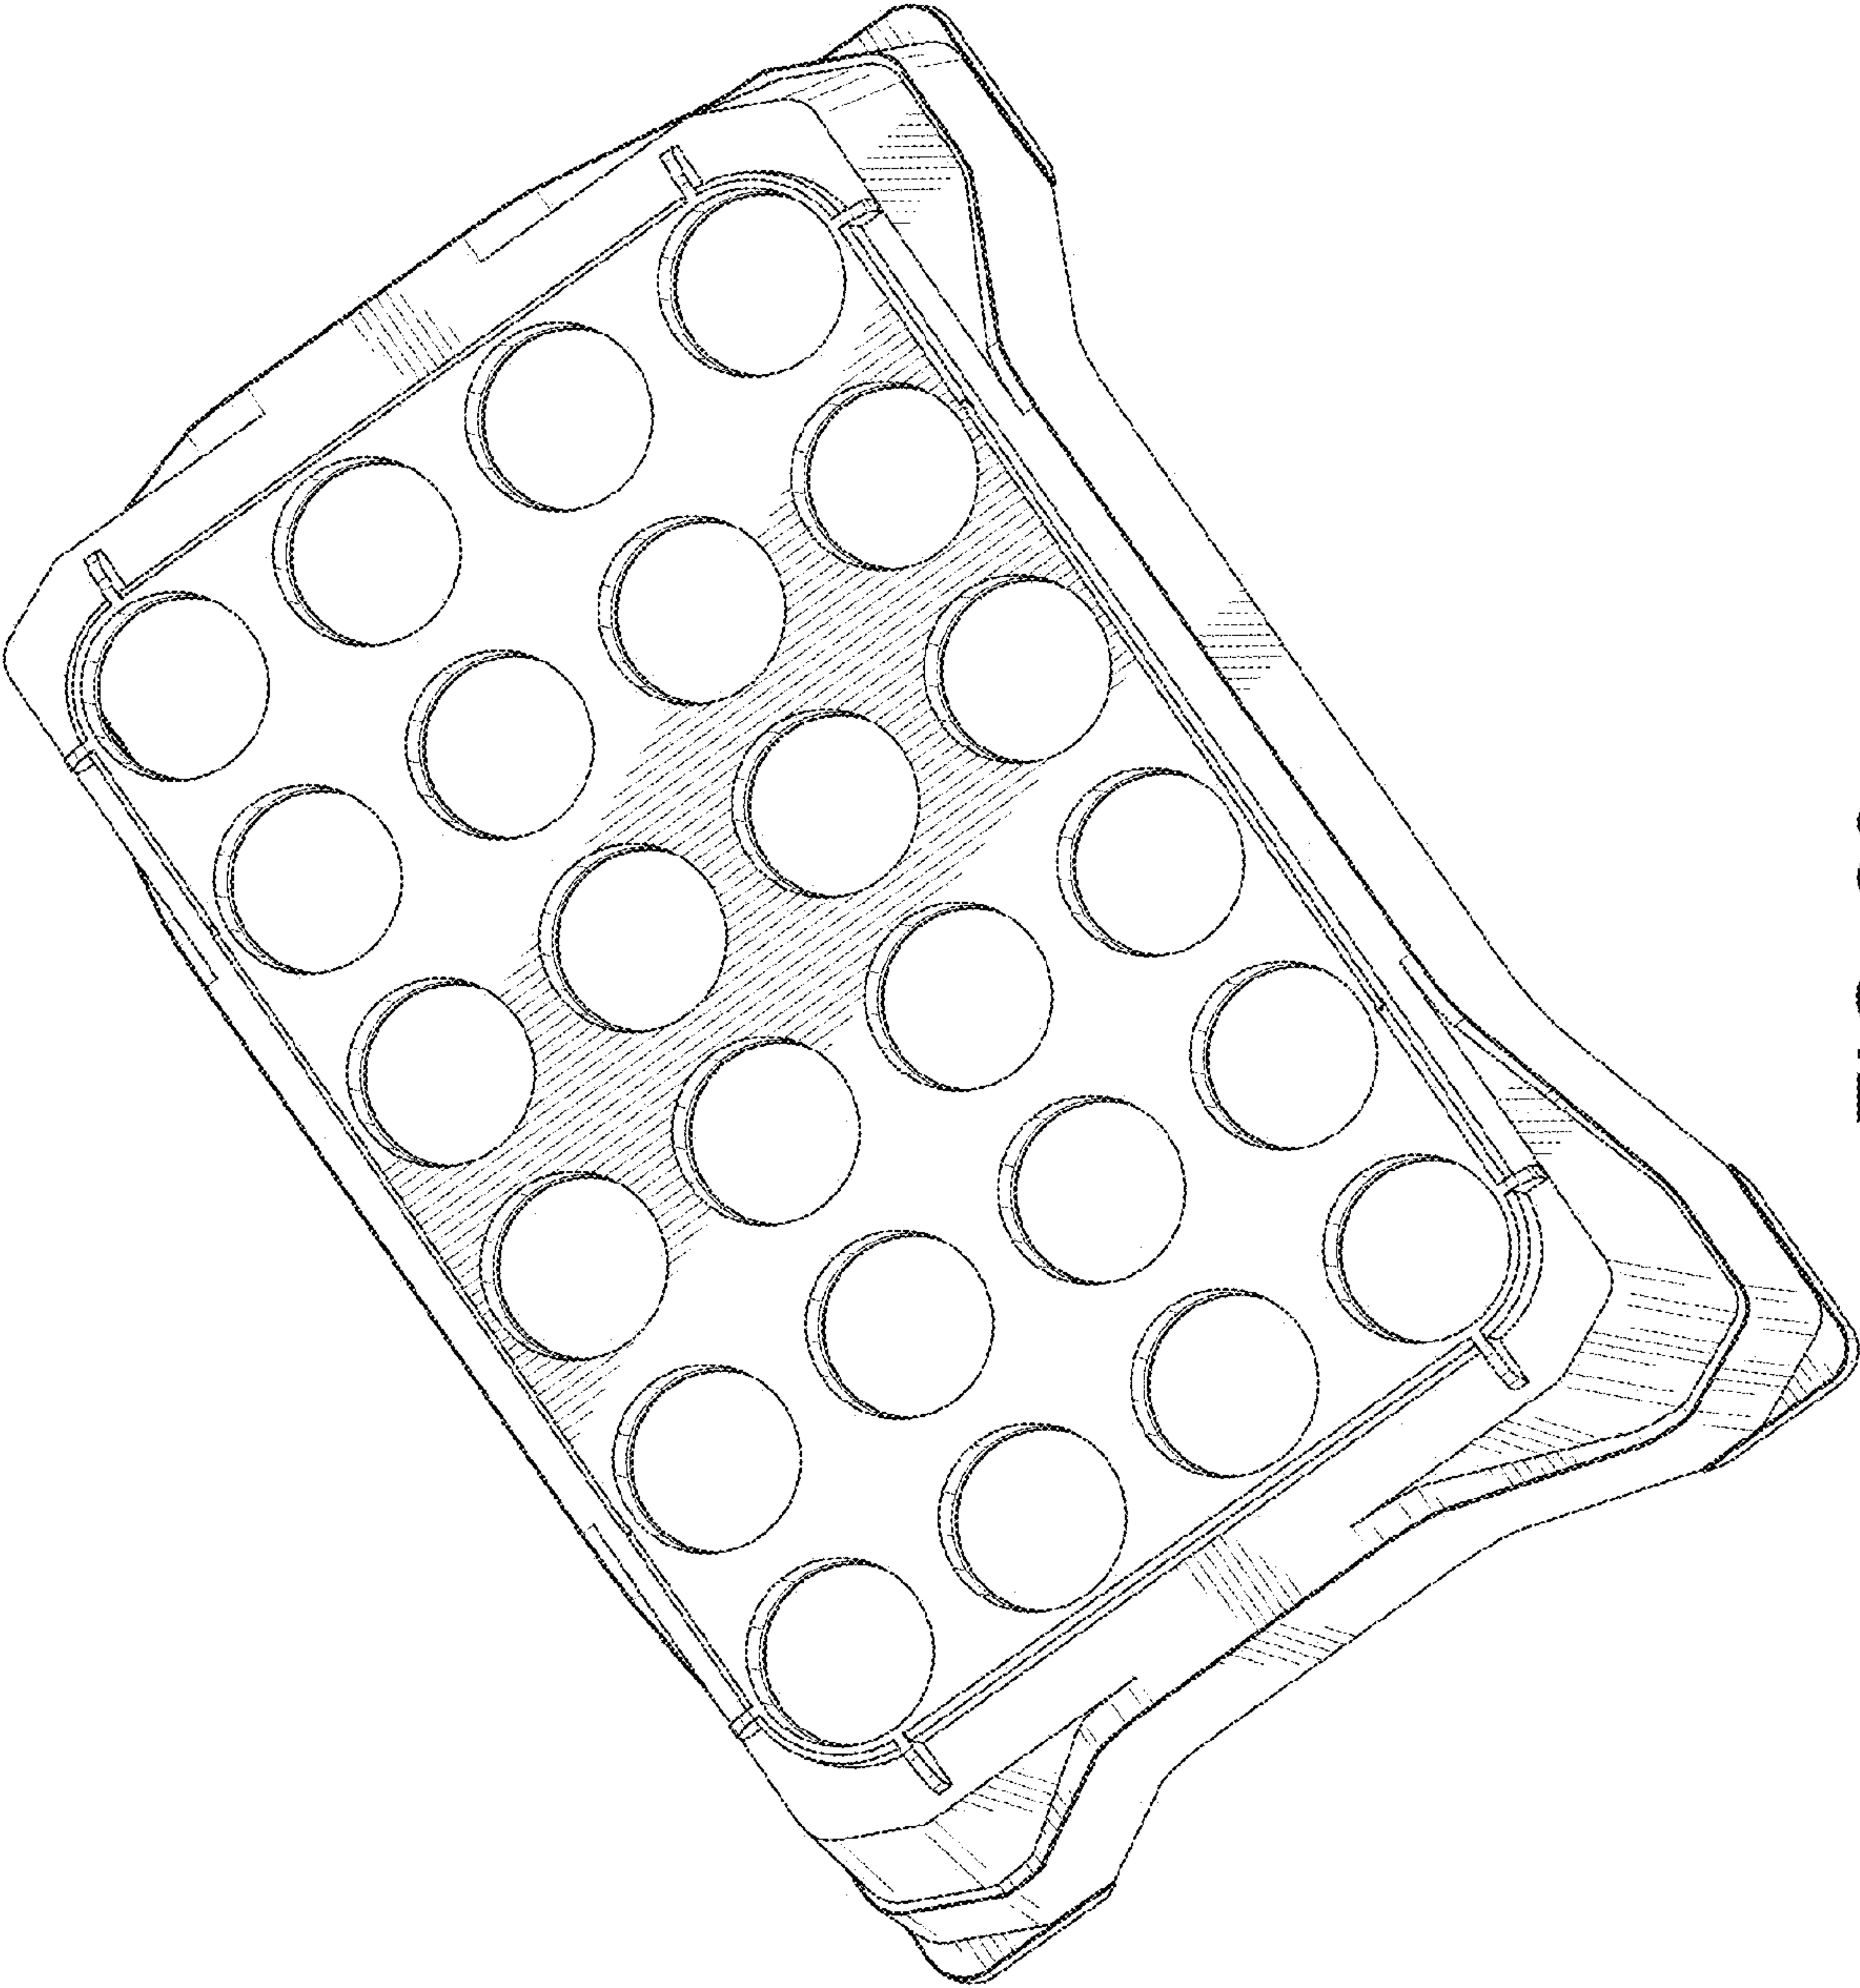


FIG. 23

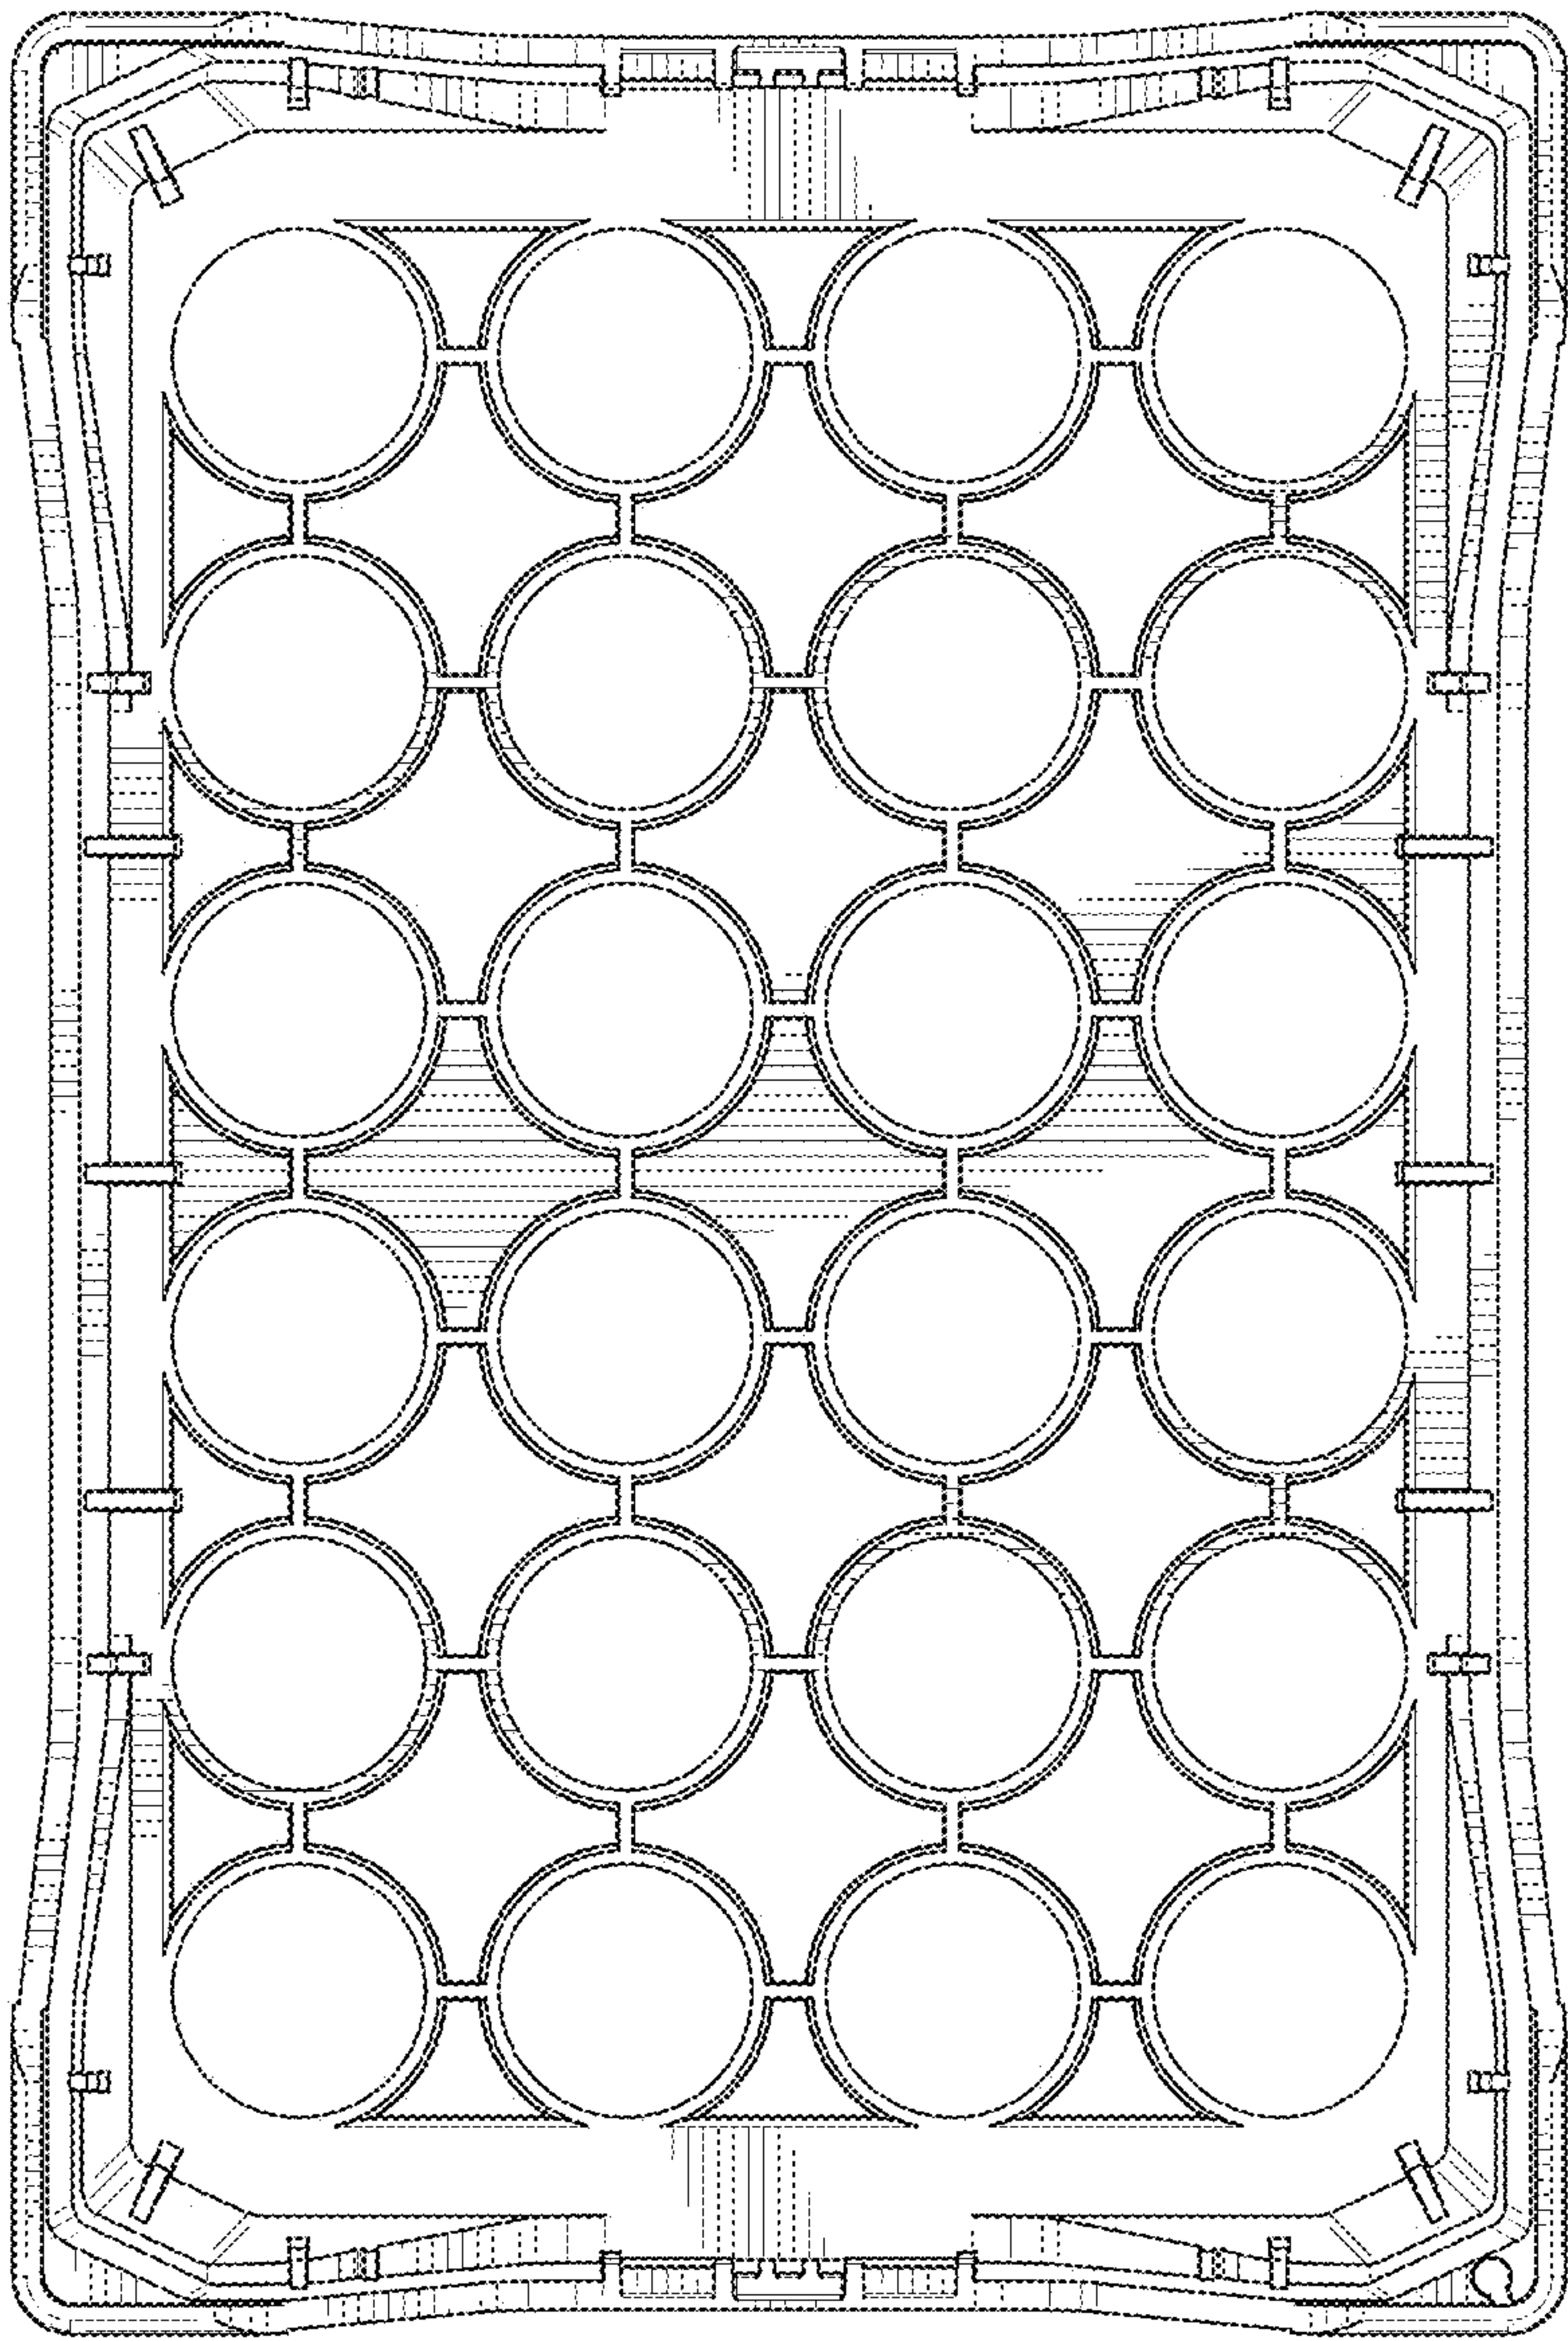


FIG. 24

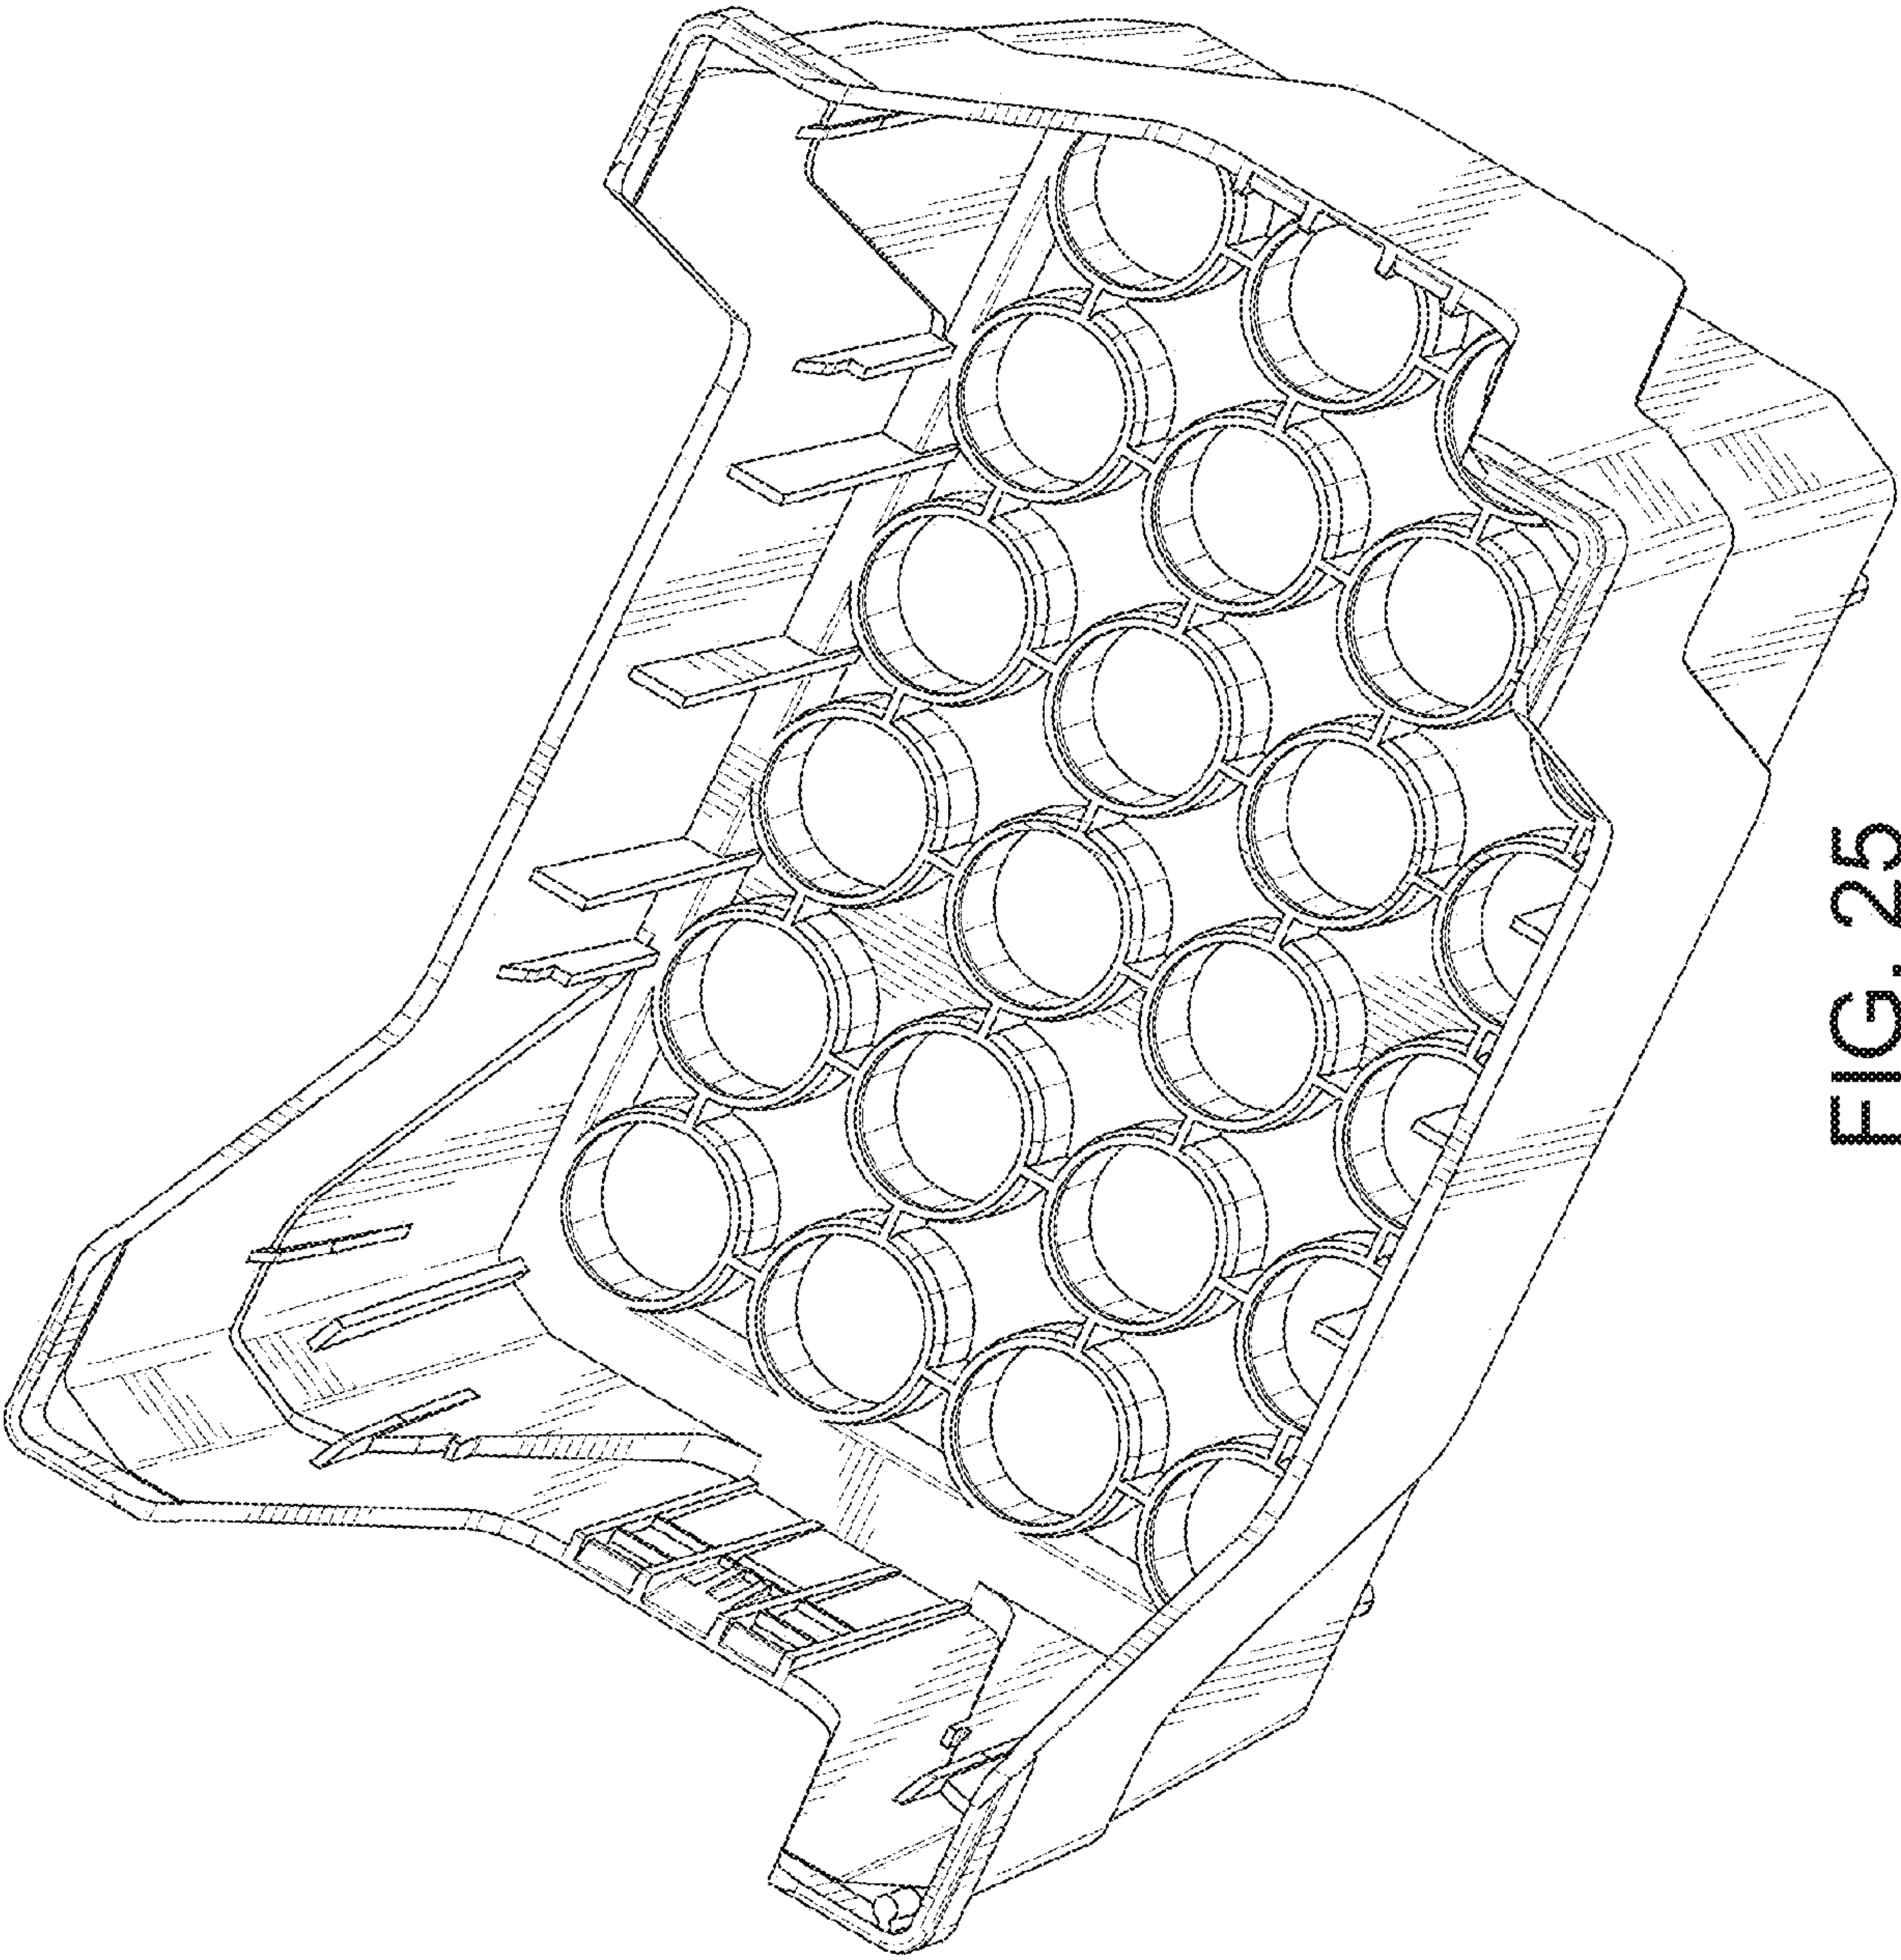


FIG. 25

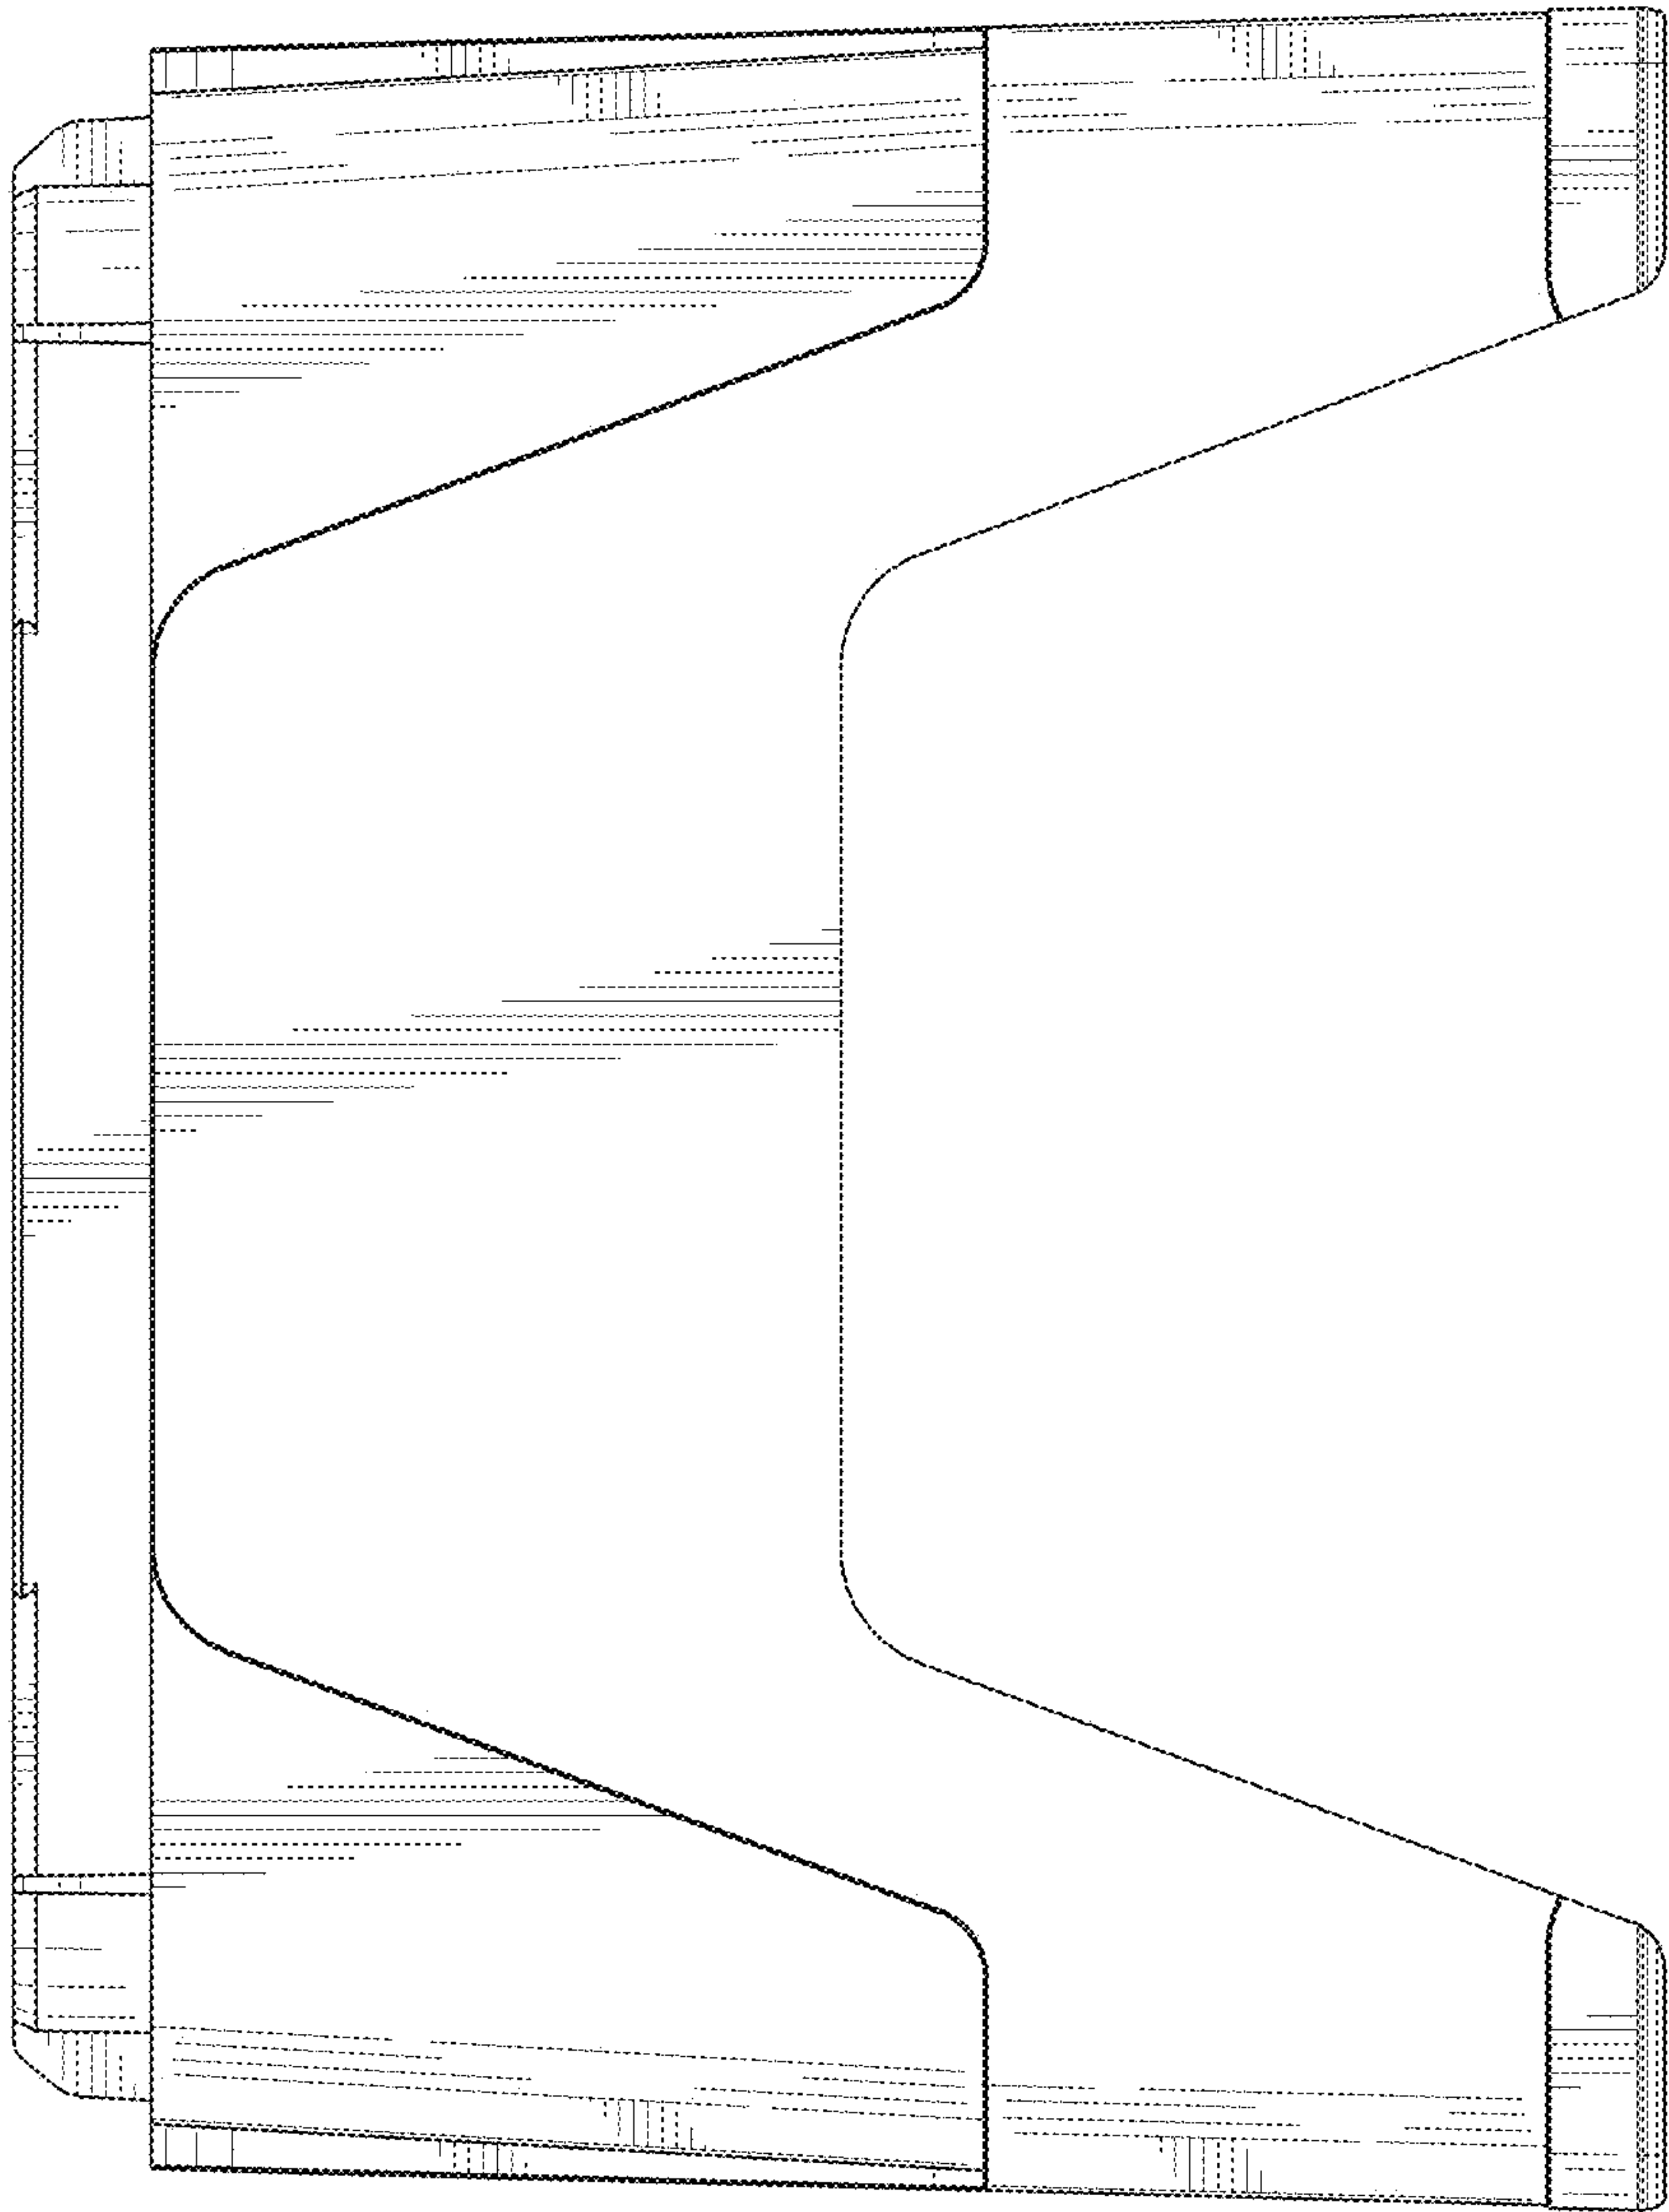


FIG. 26

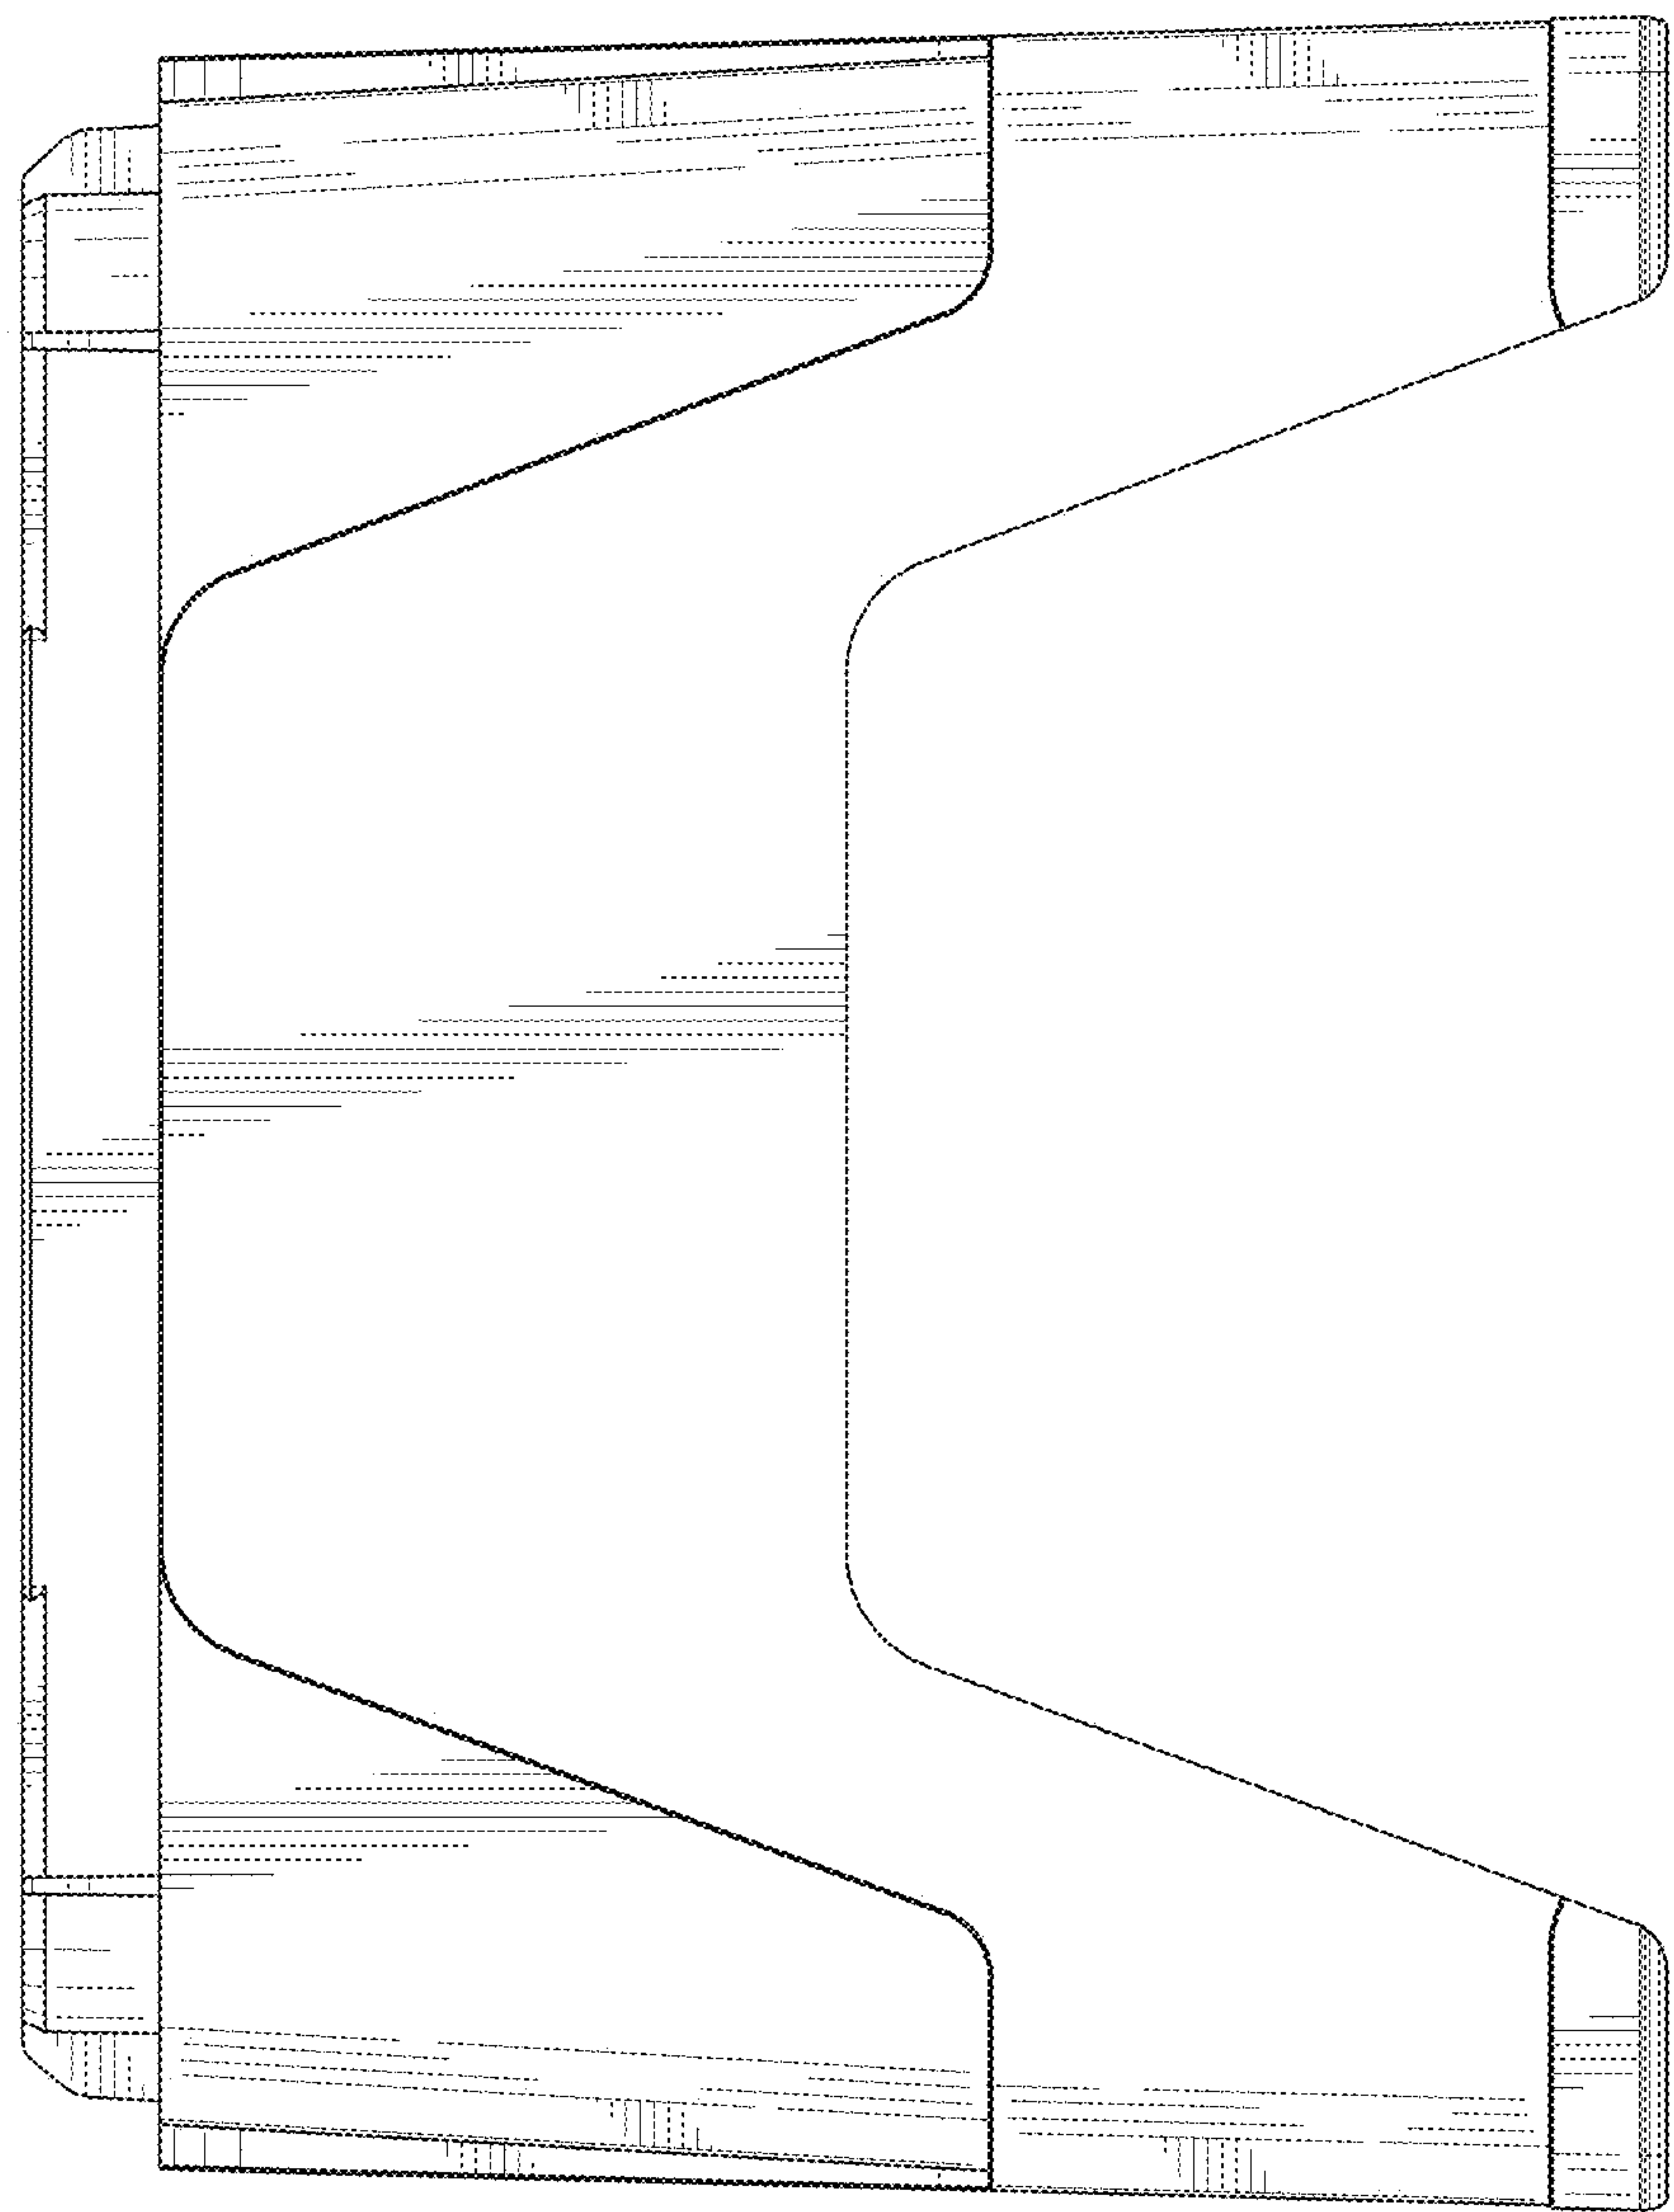


FIG. 27

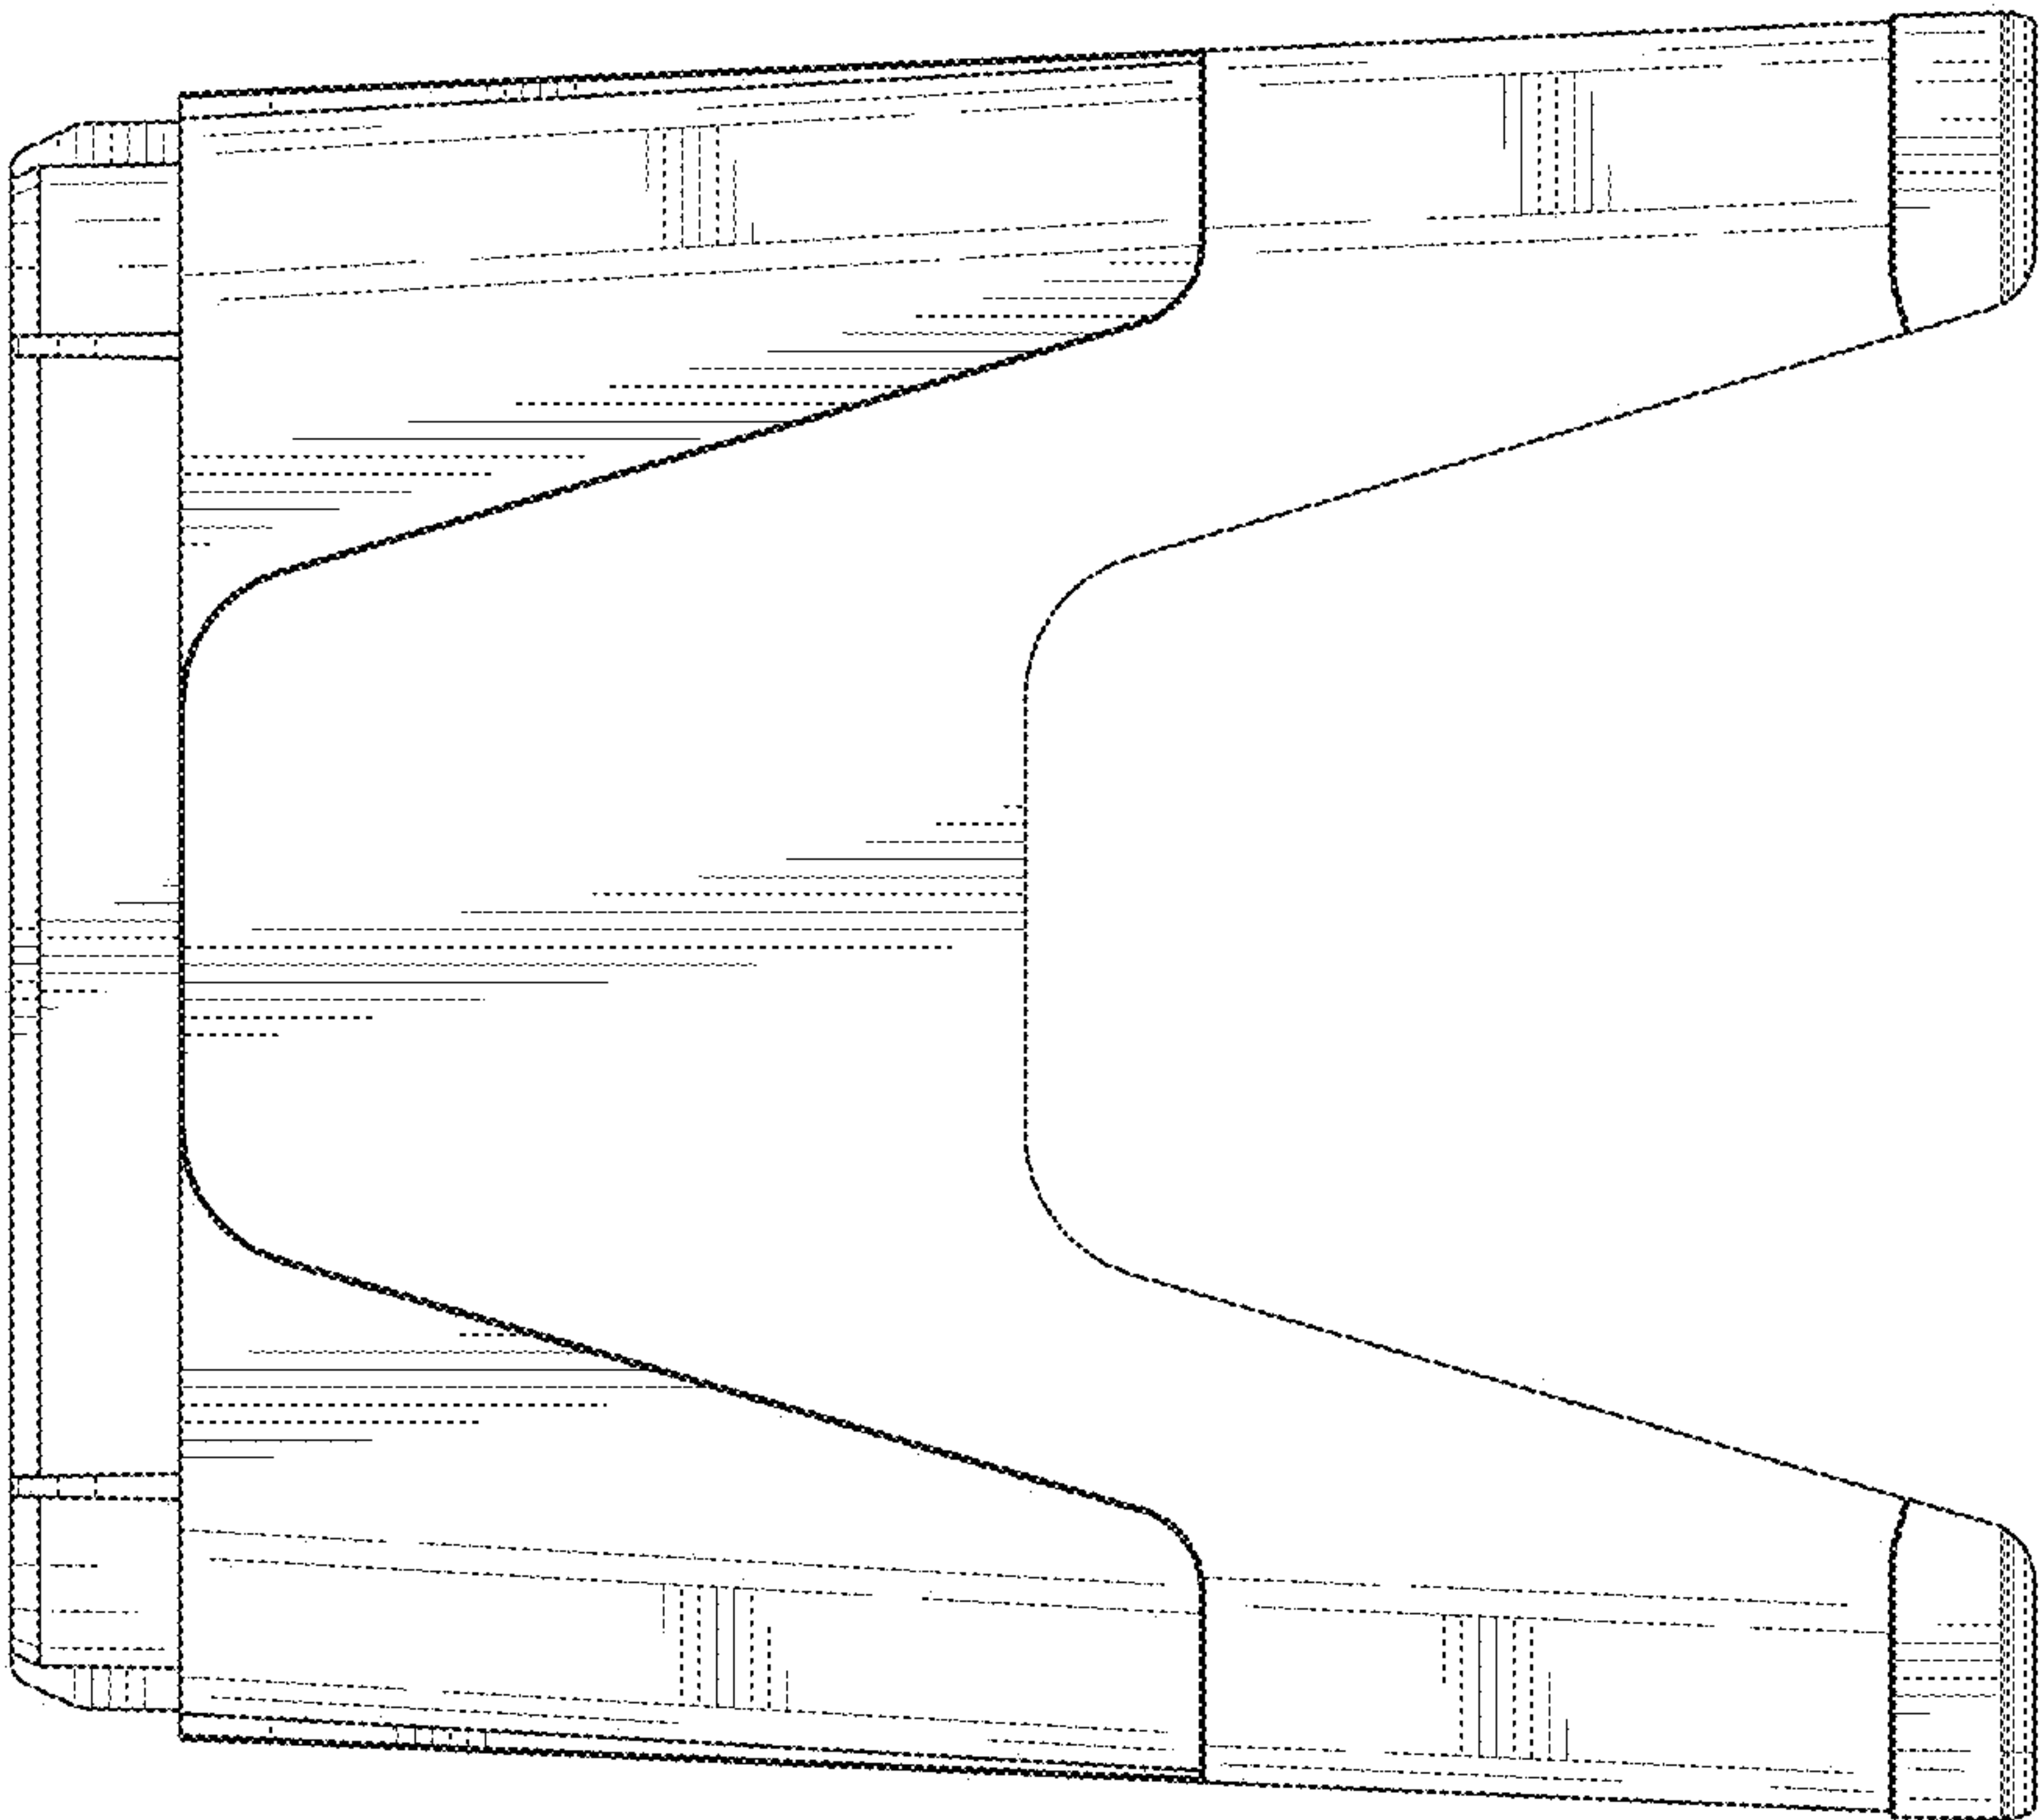


FIG. 28

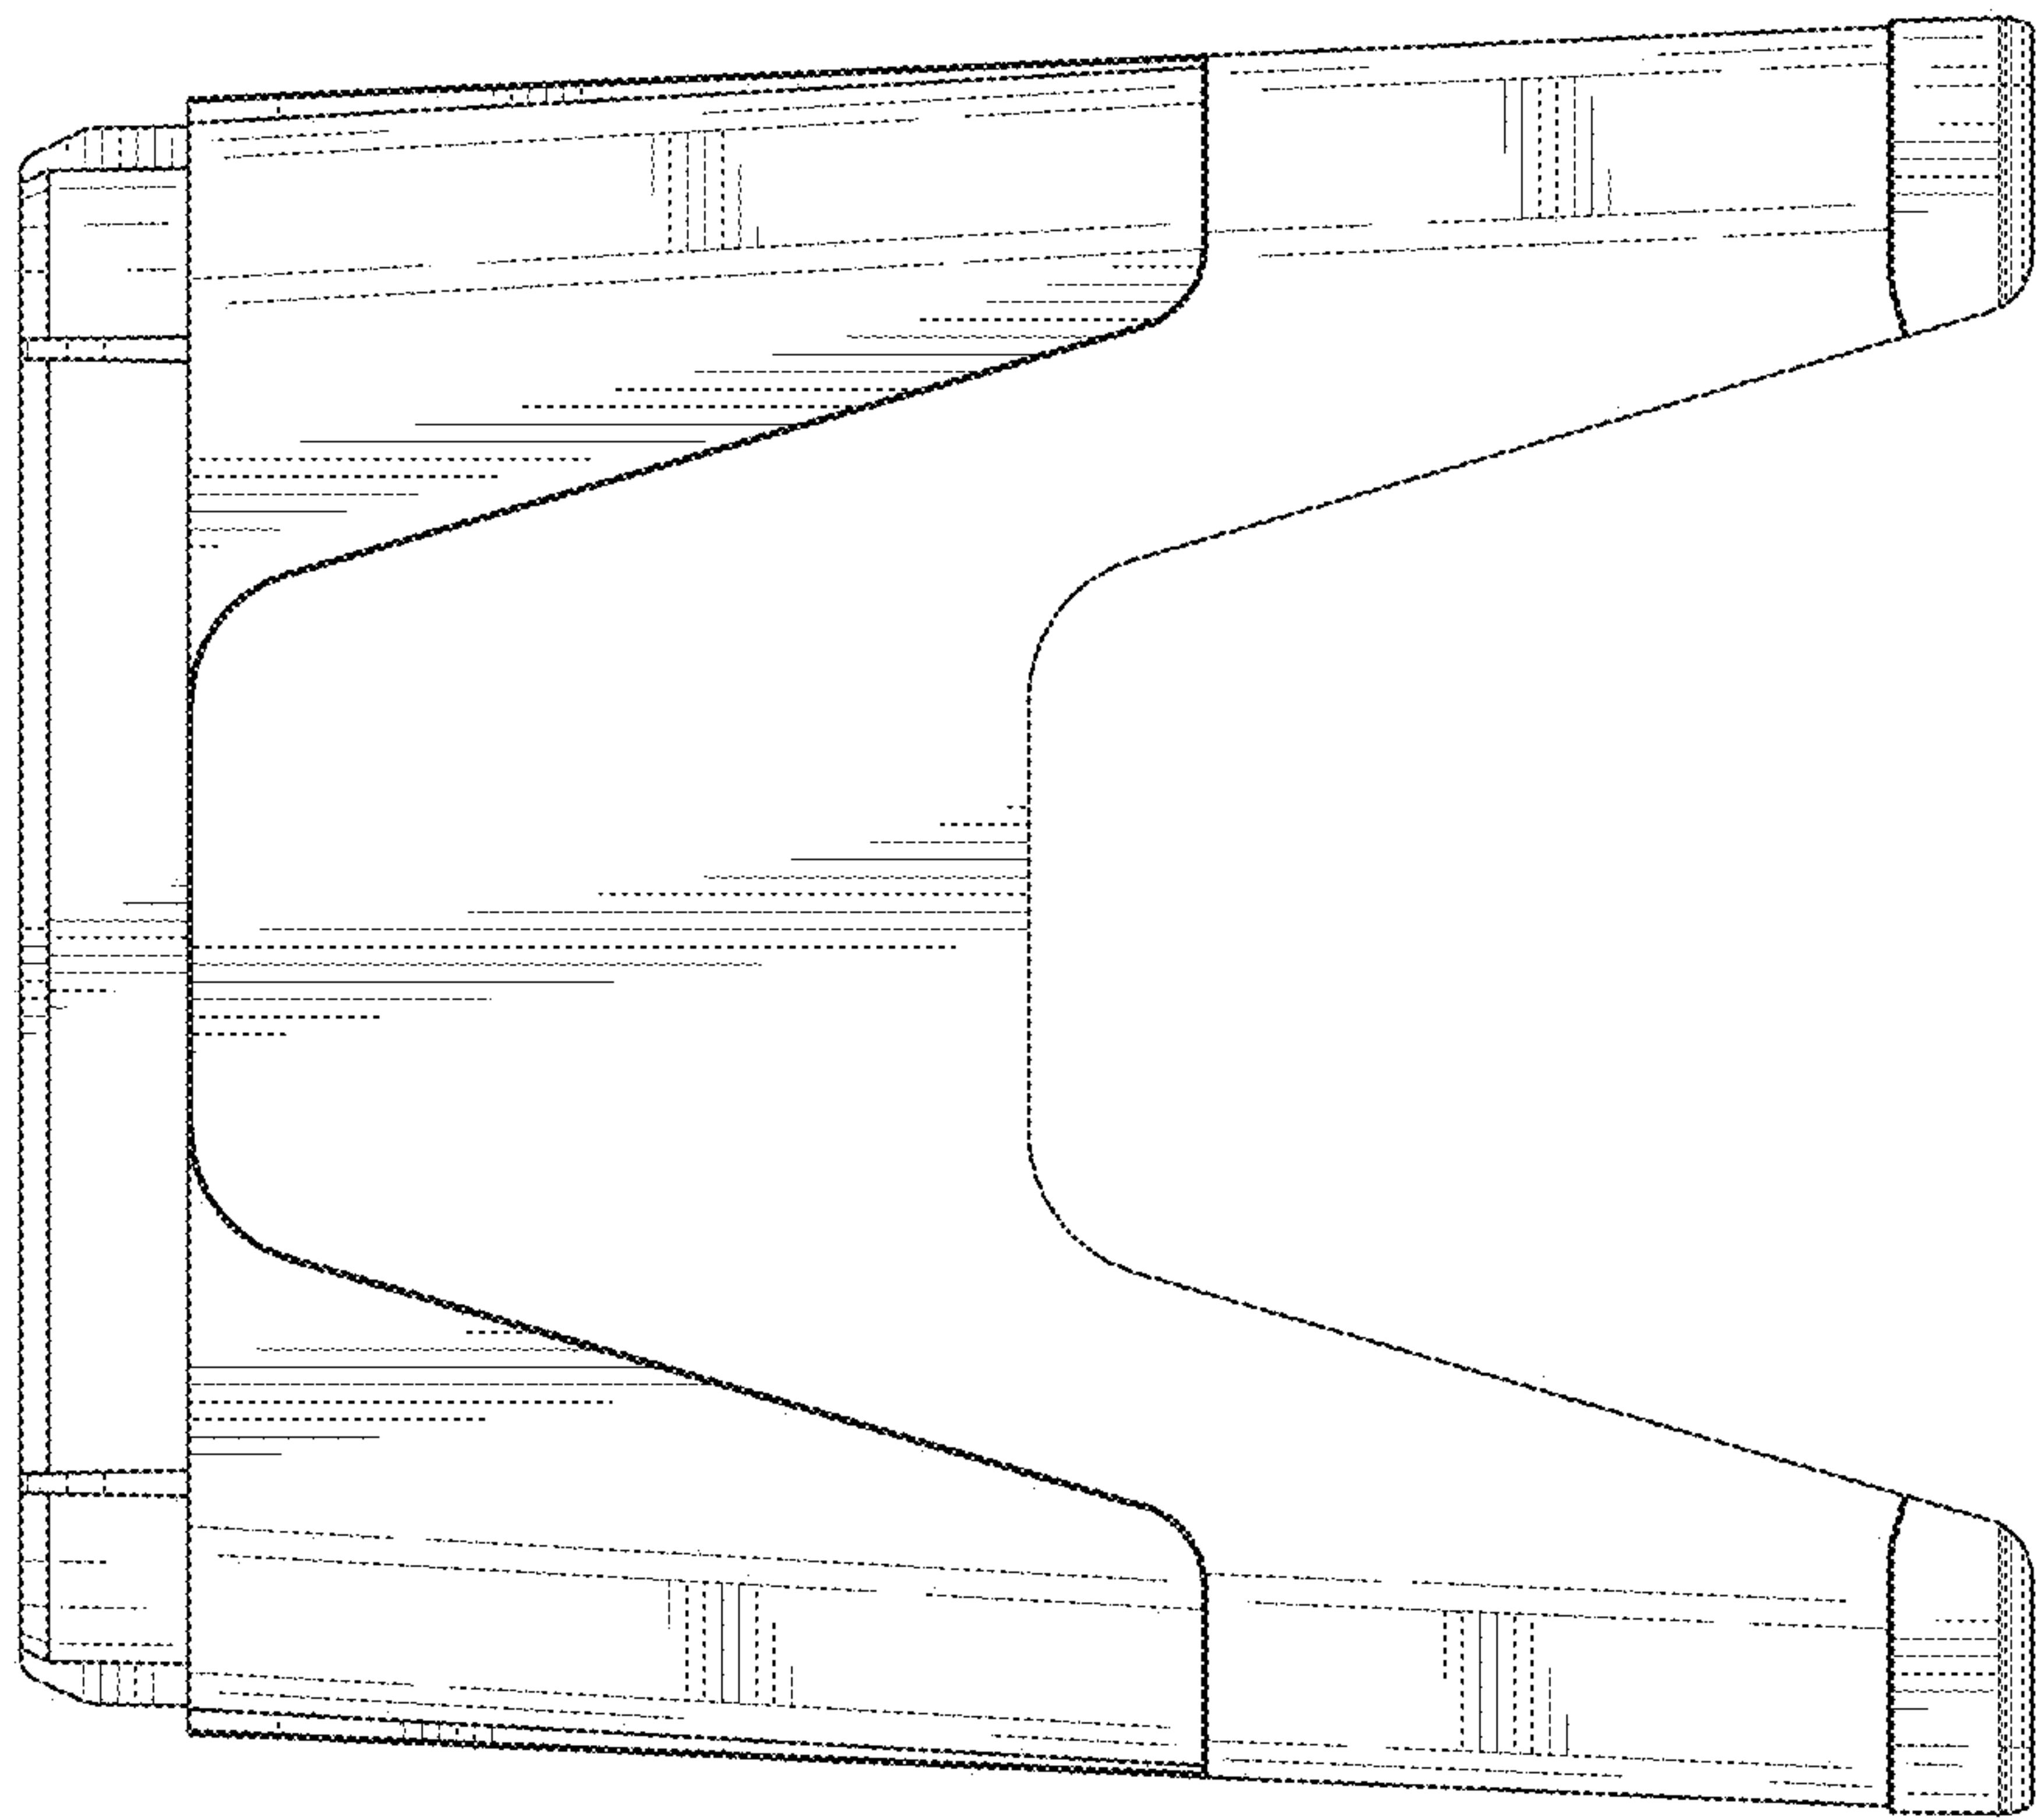


FIG. 29

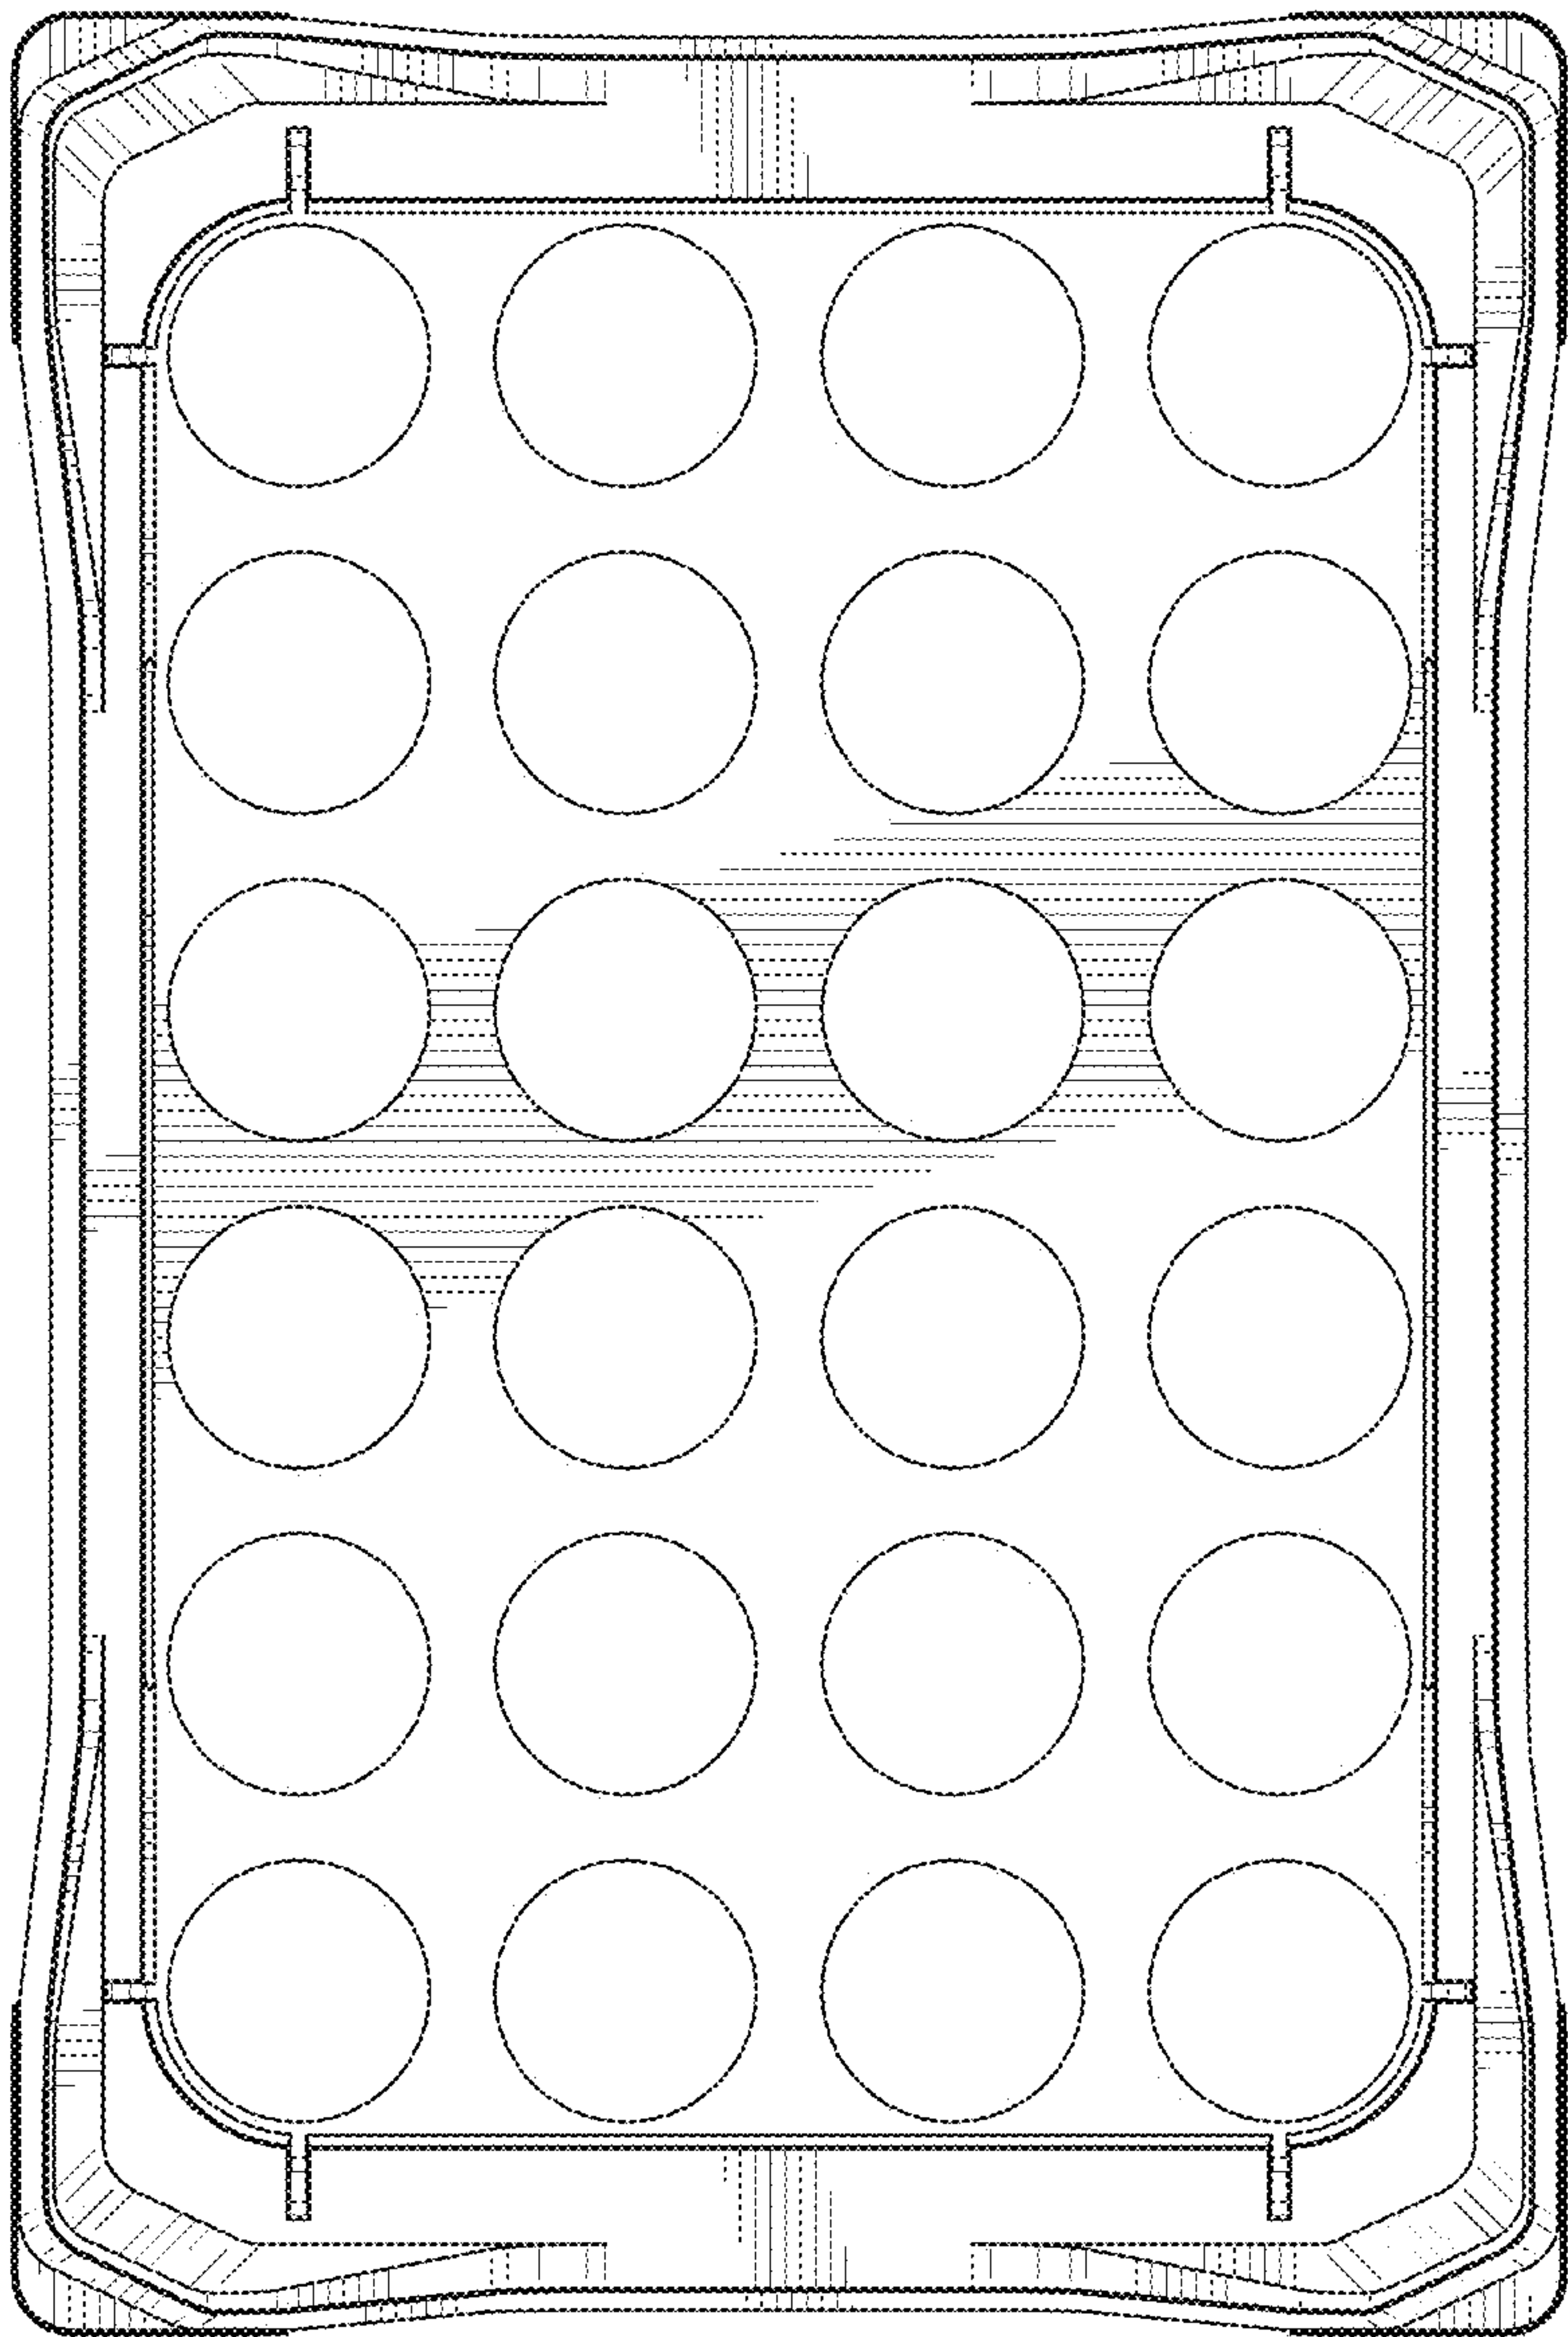


FIG. 30

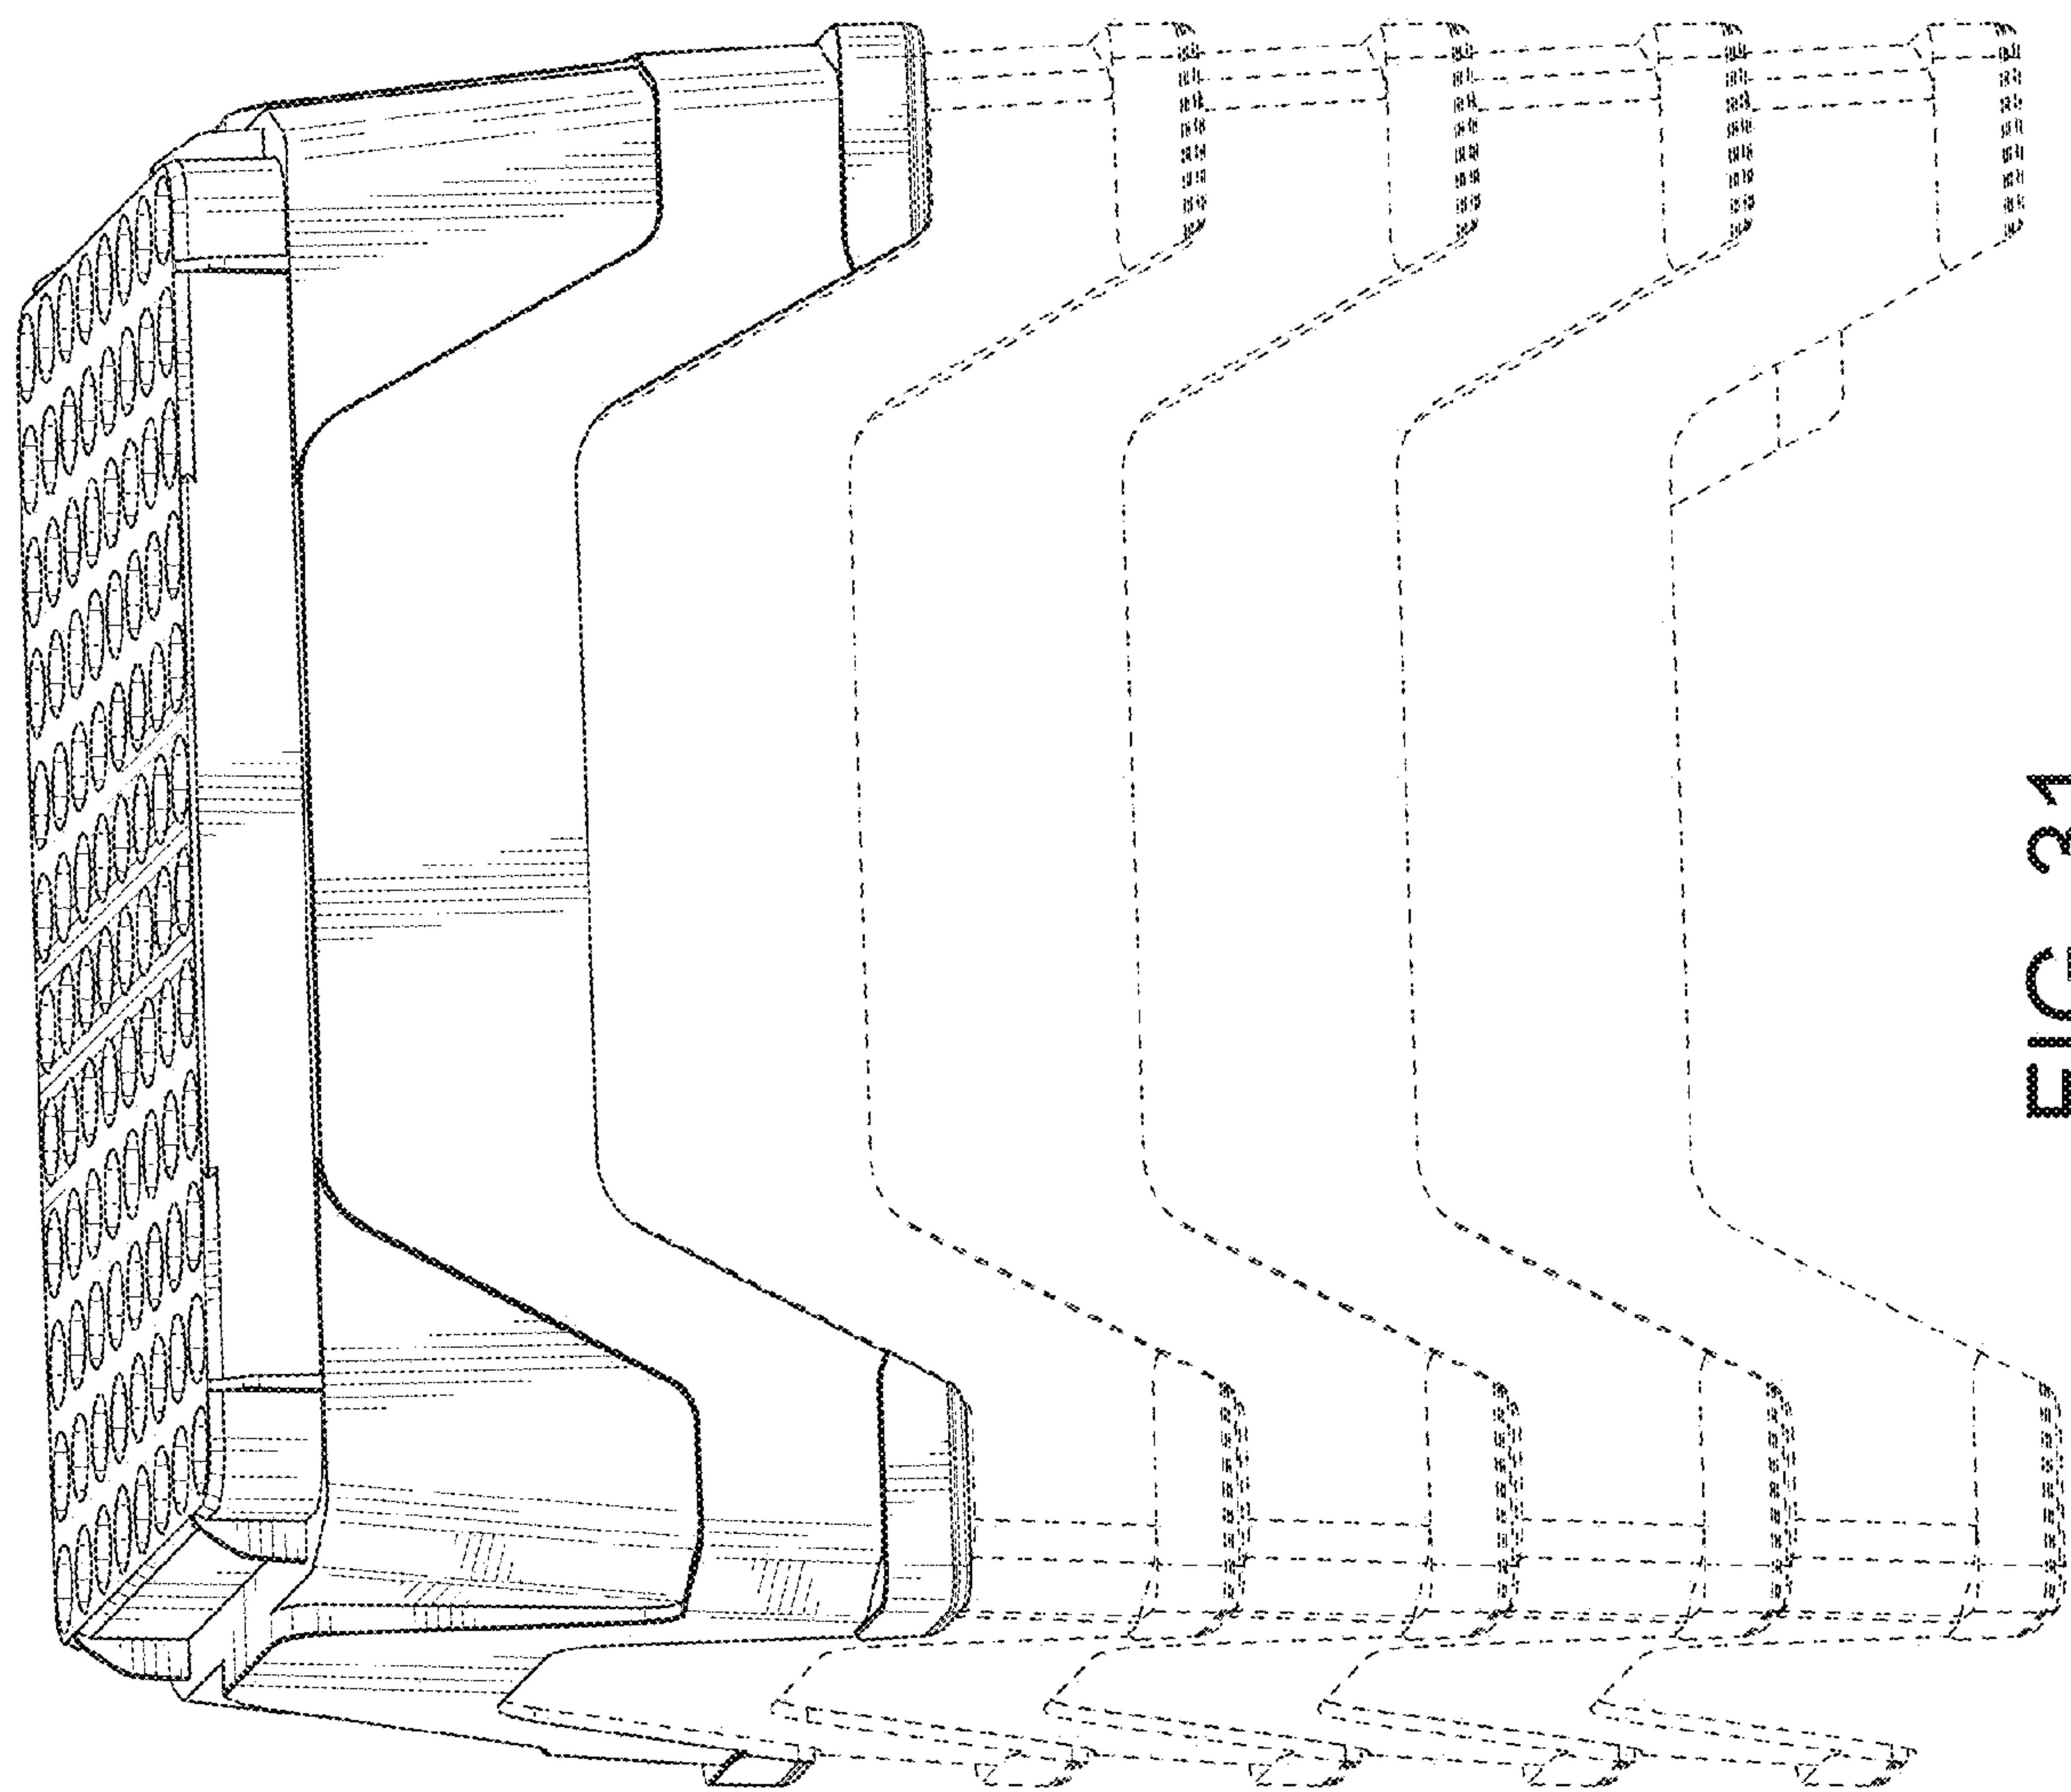


FIG. 31

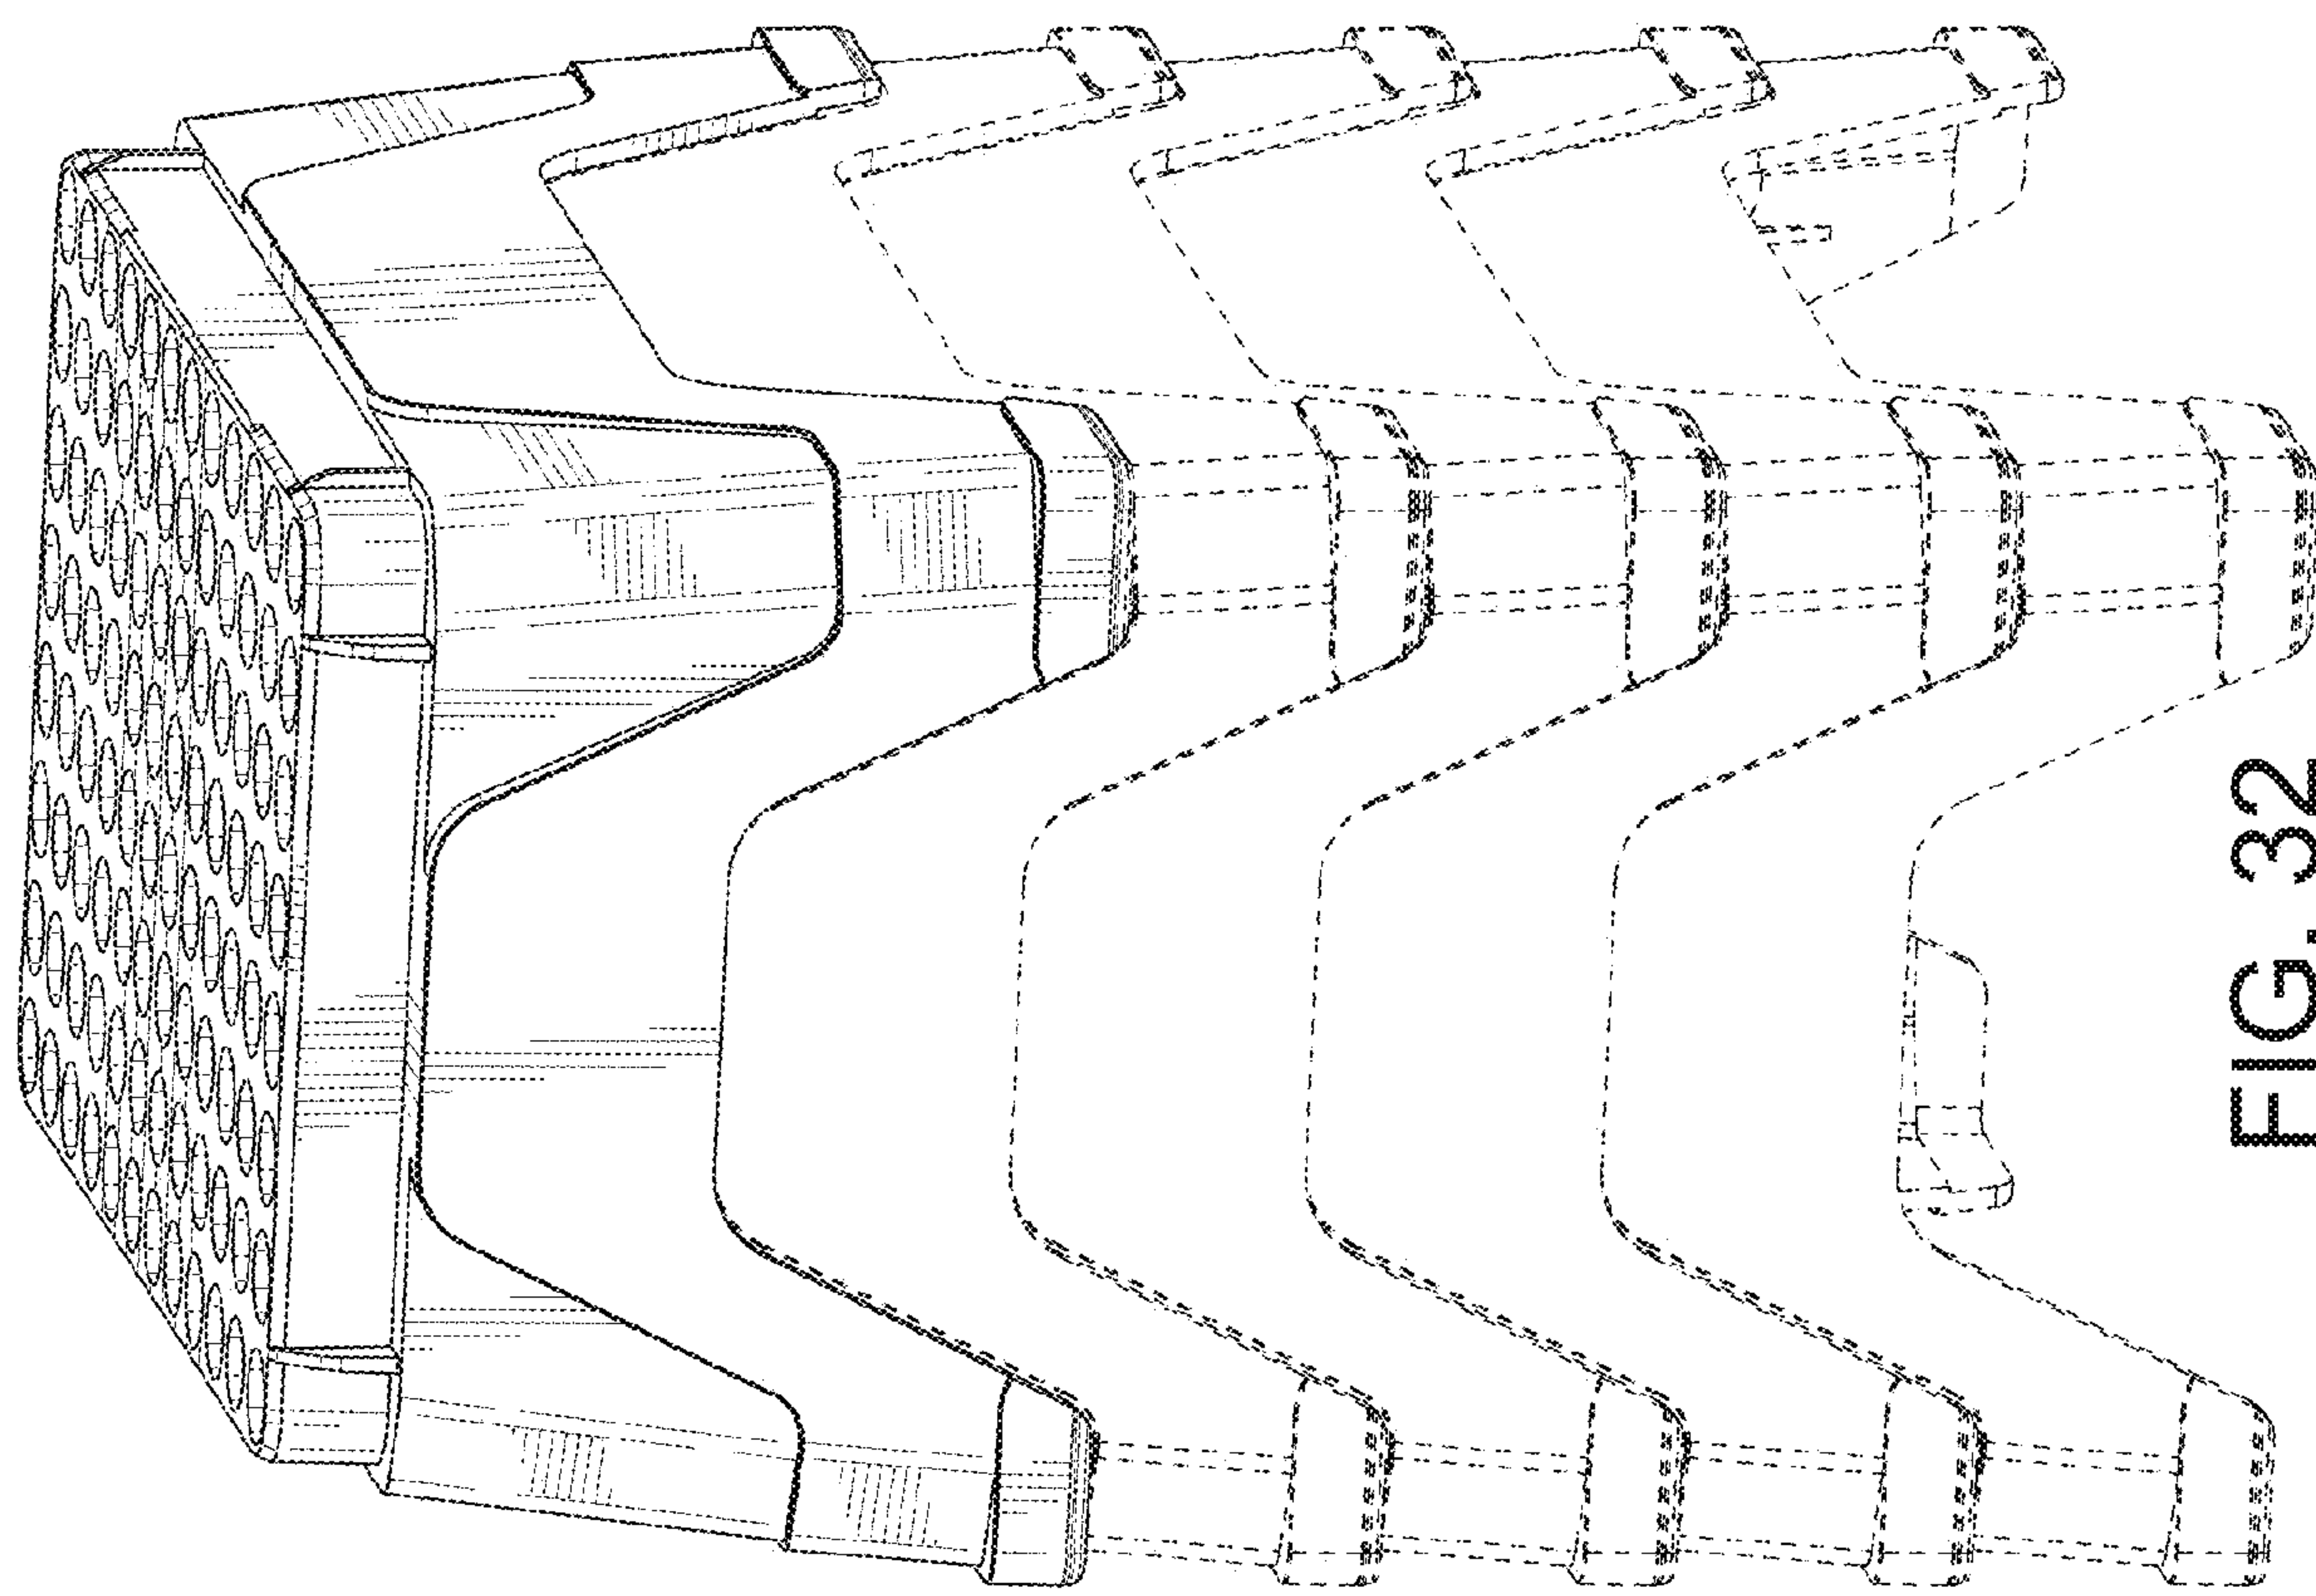


FIG. 32

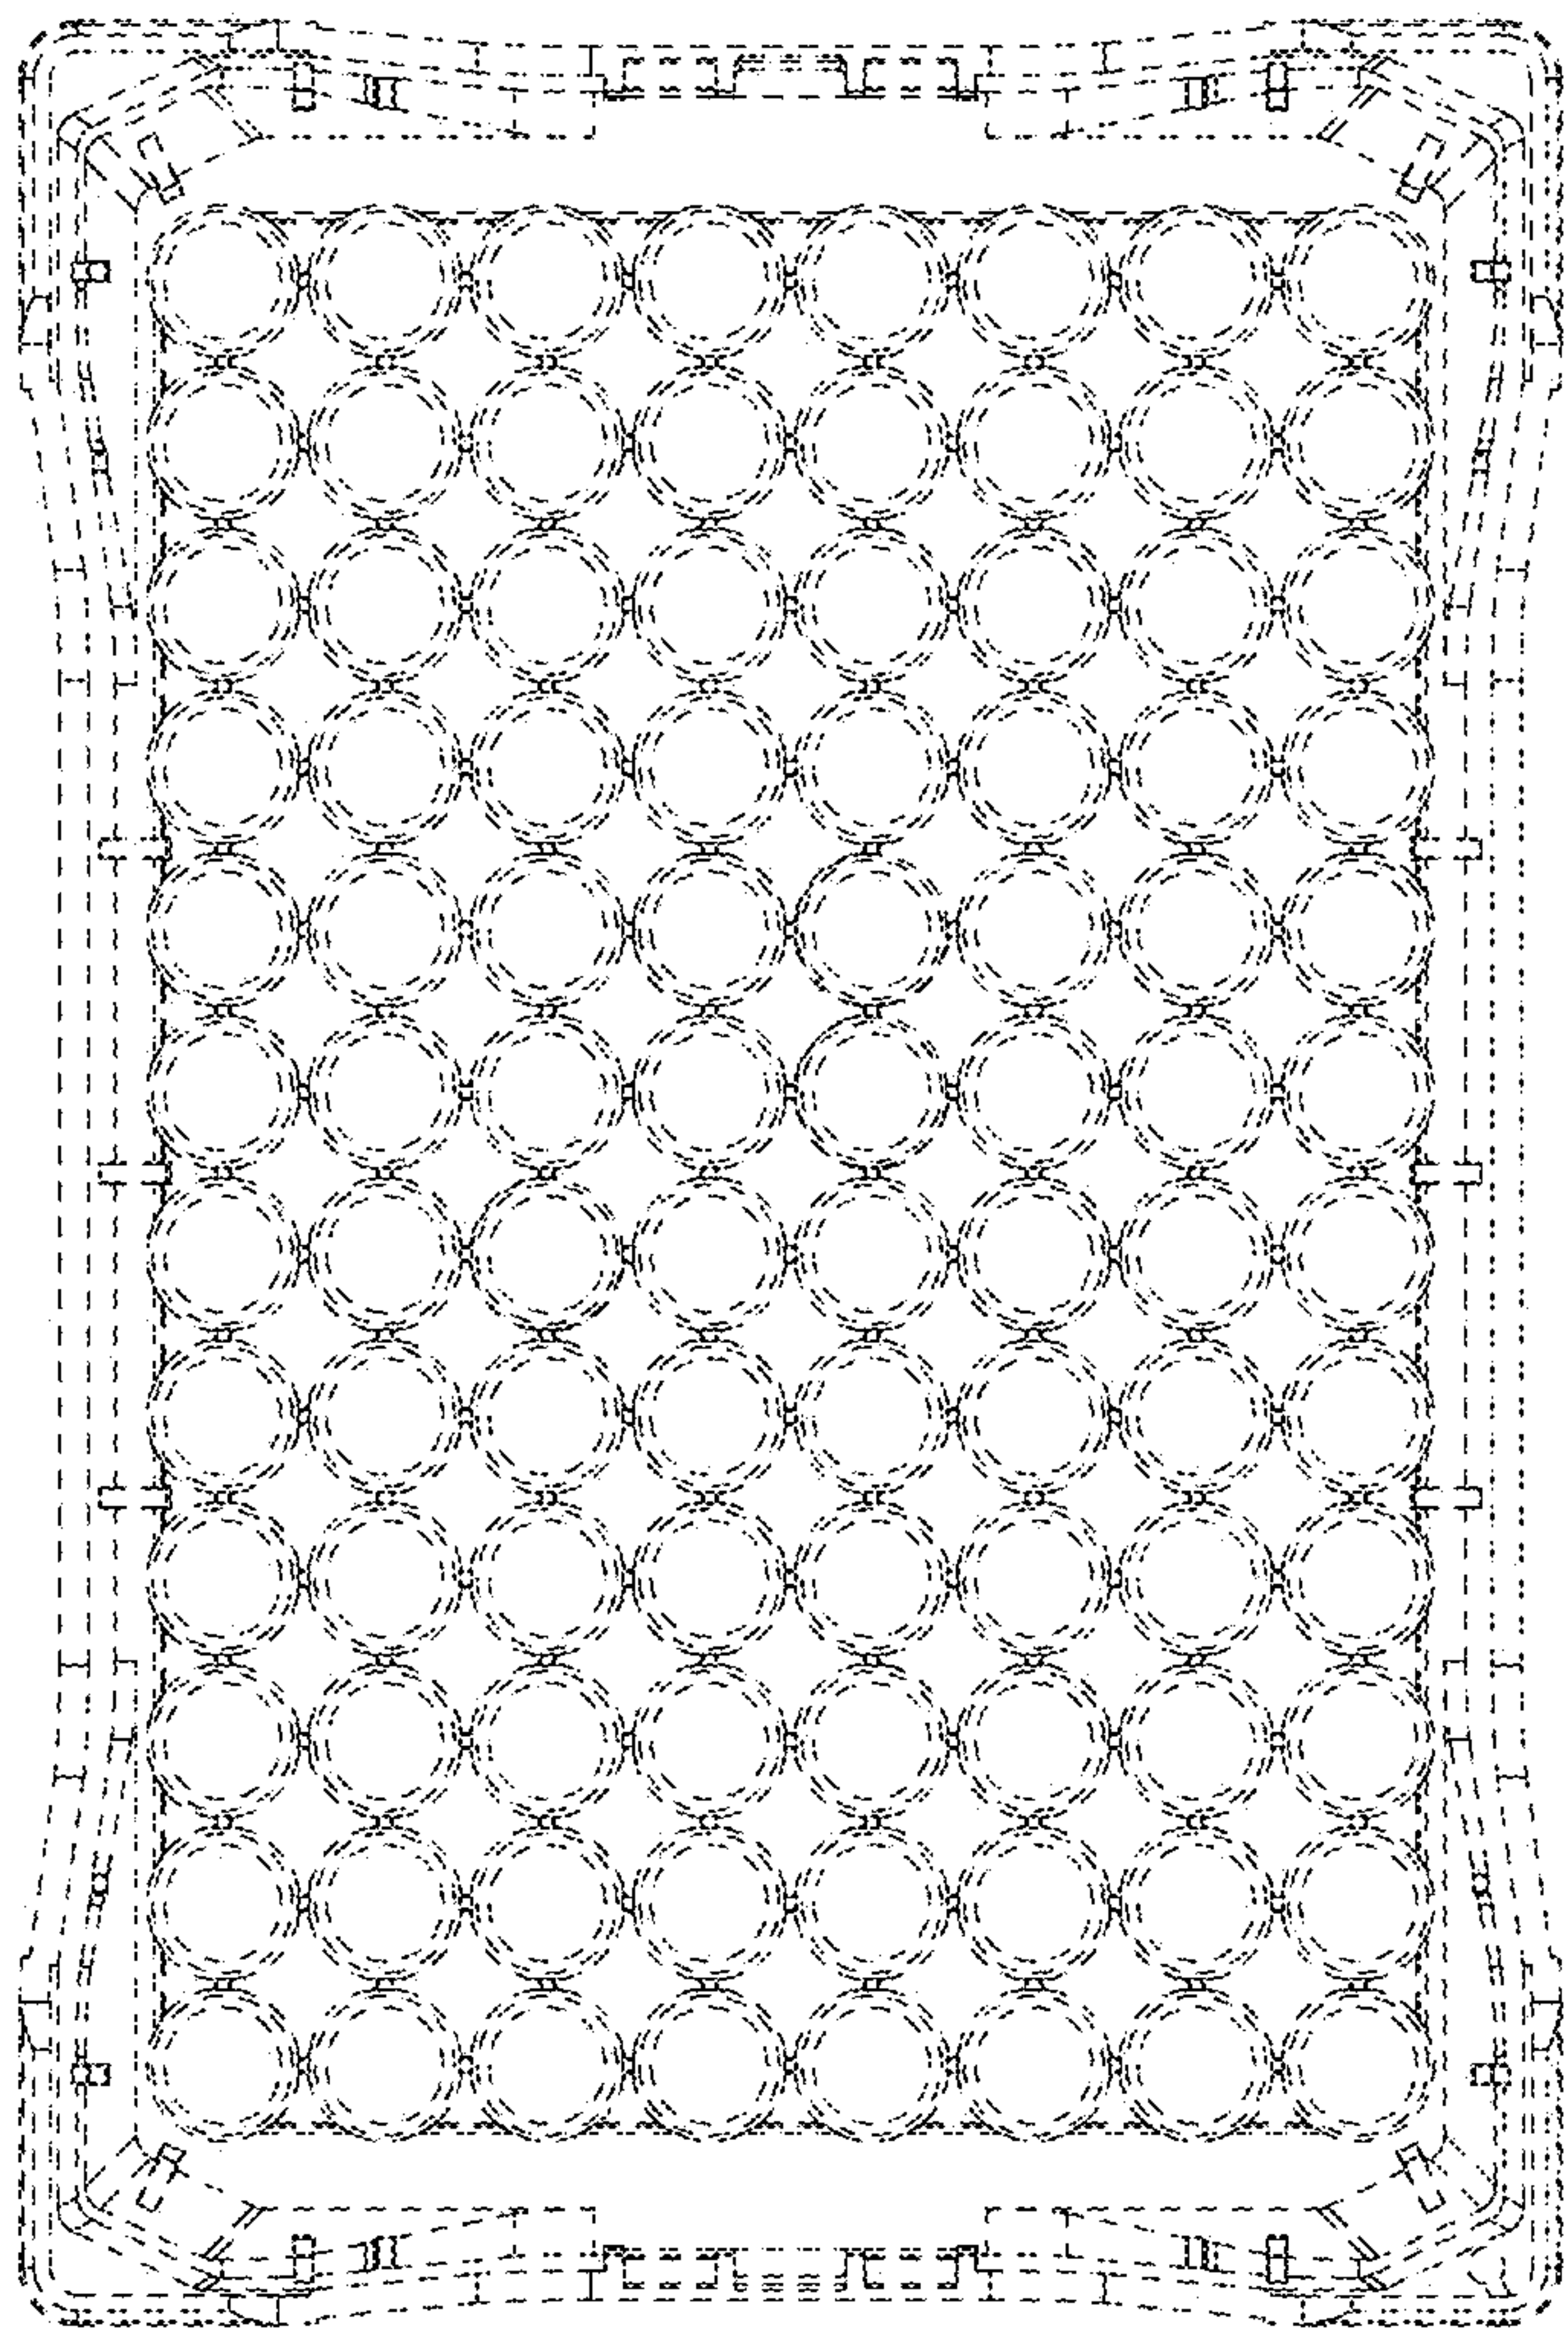


FIG. 33

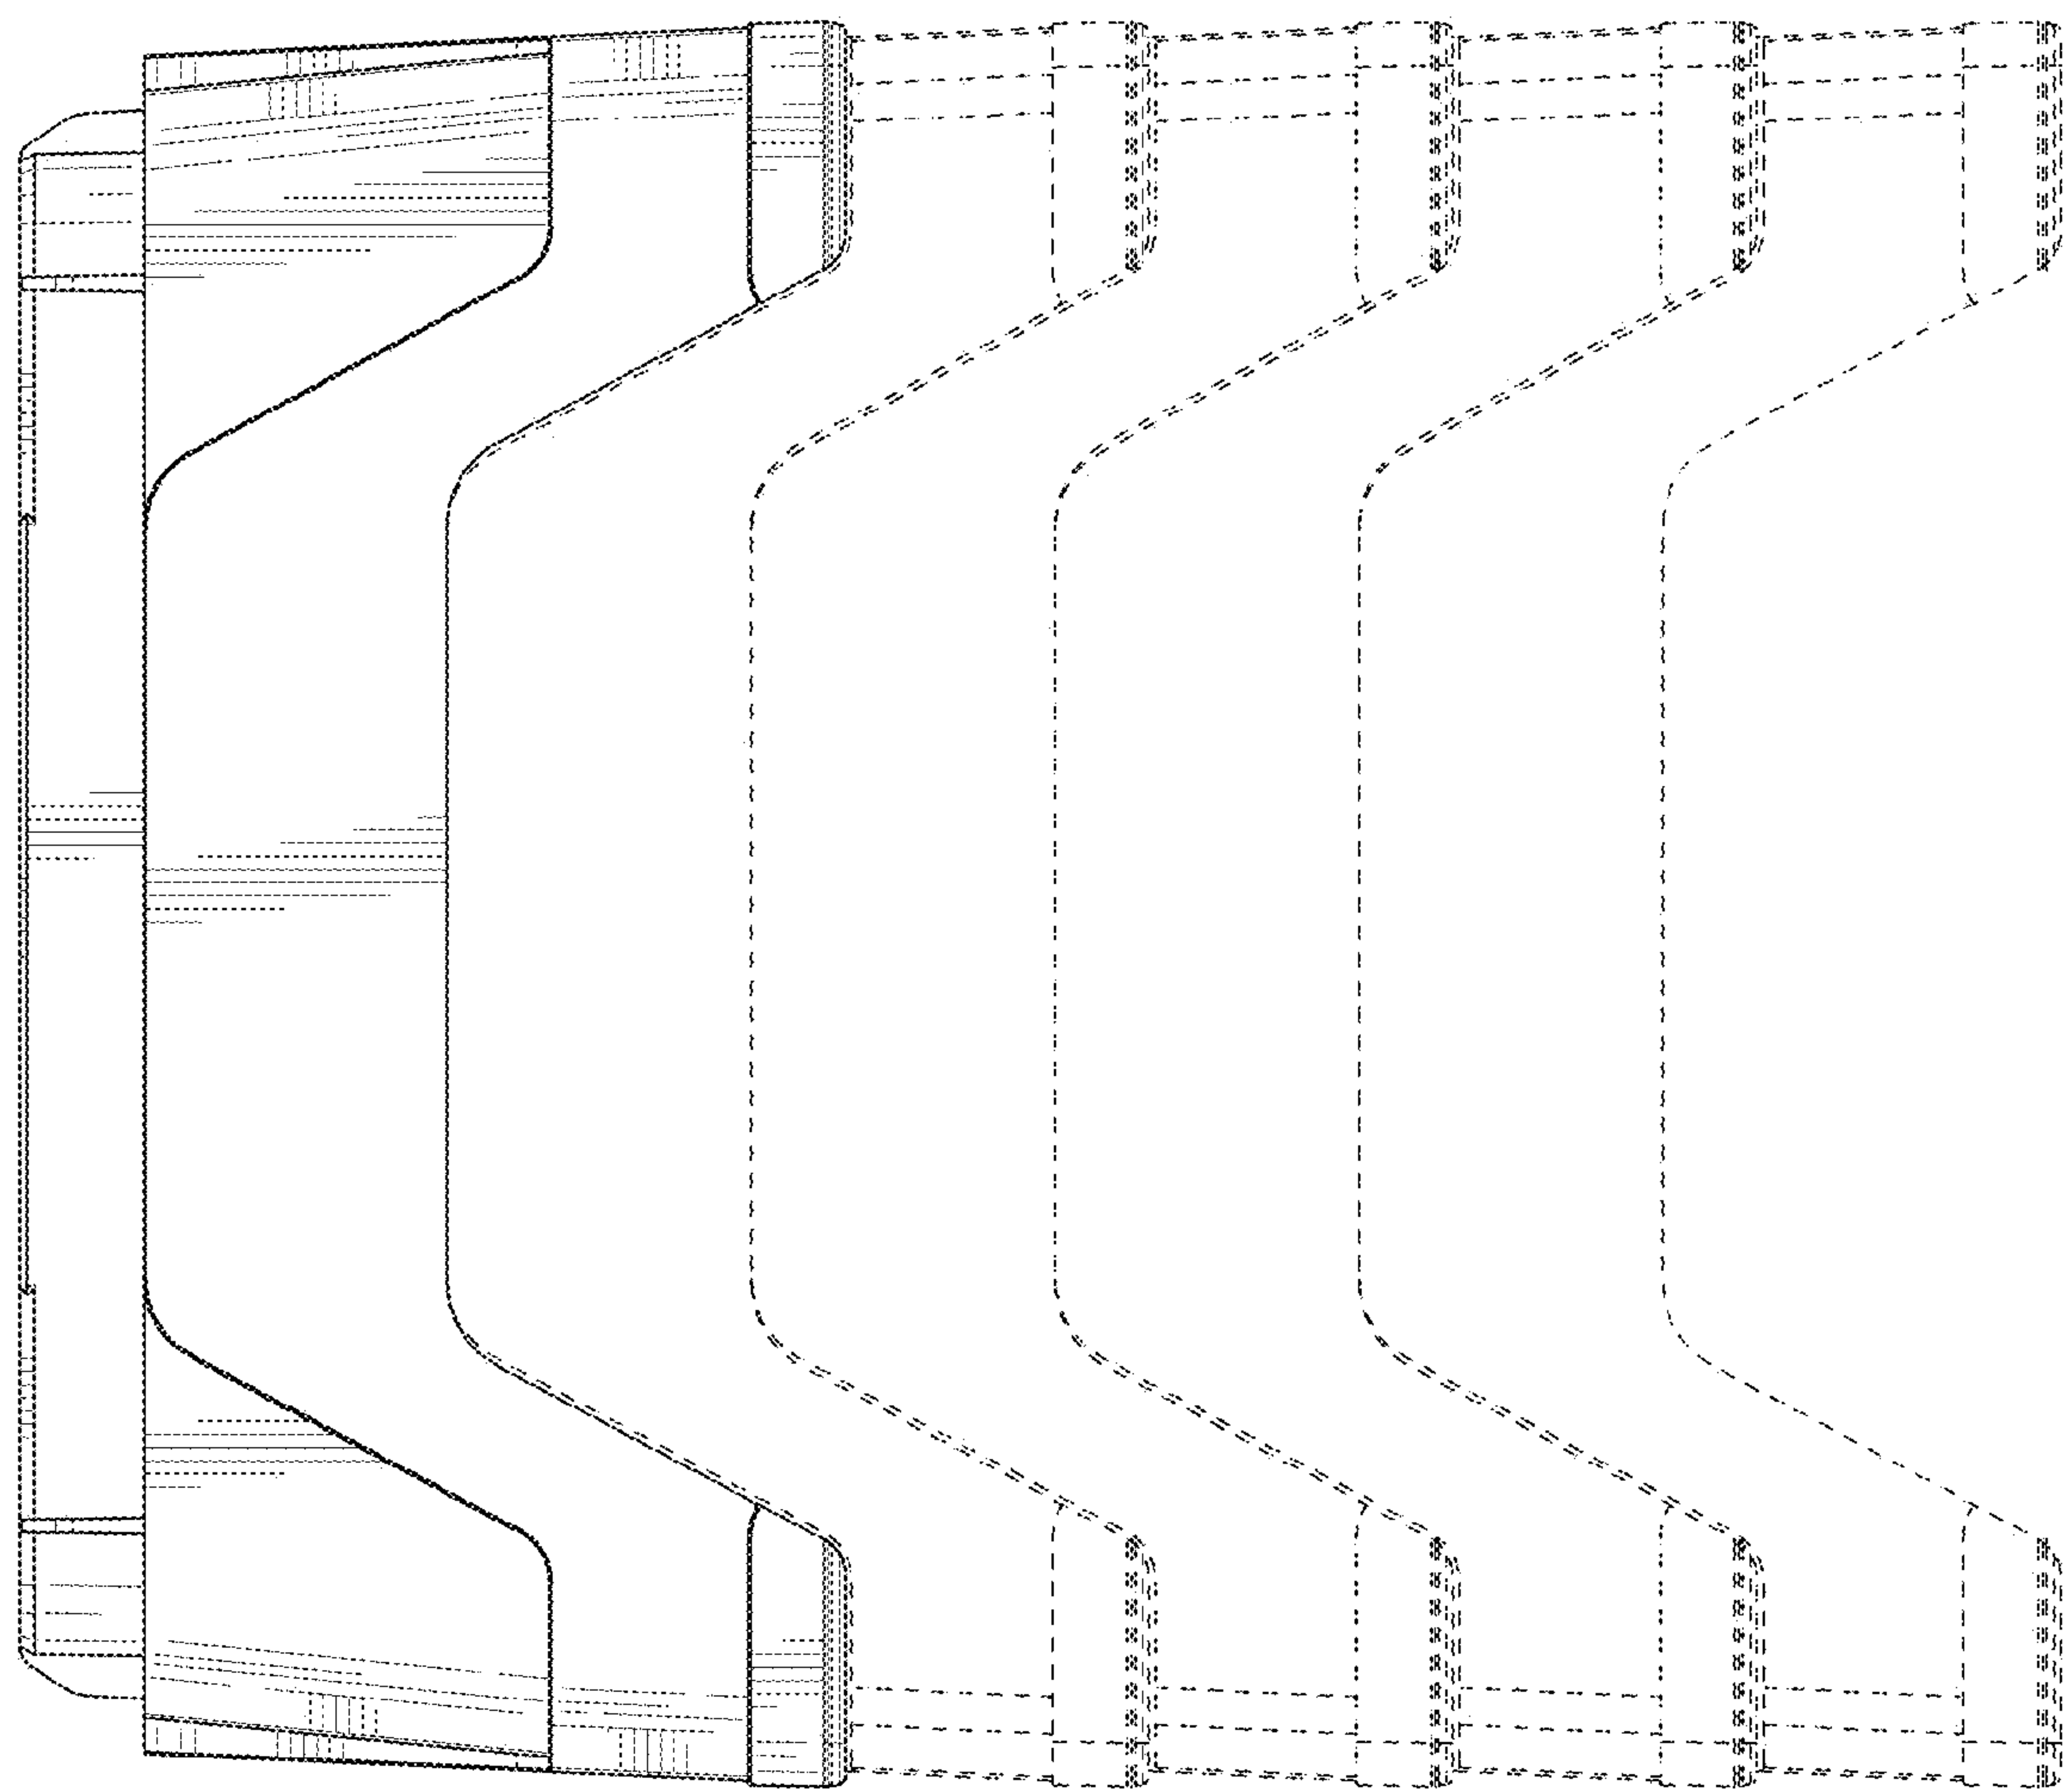


FIG. 34

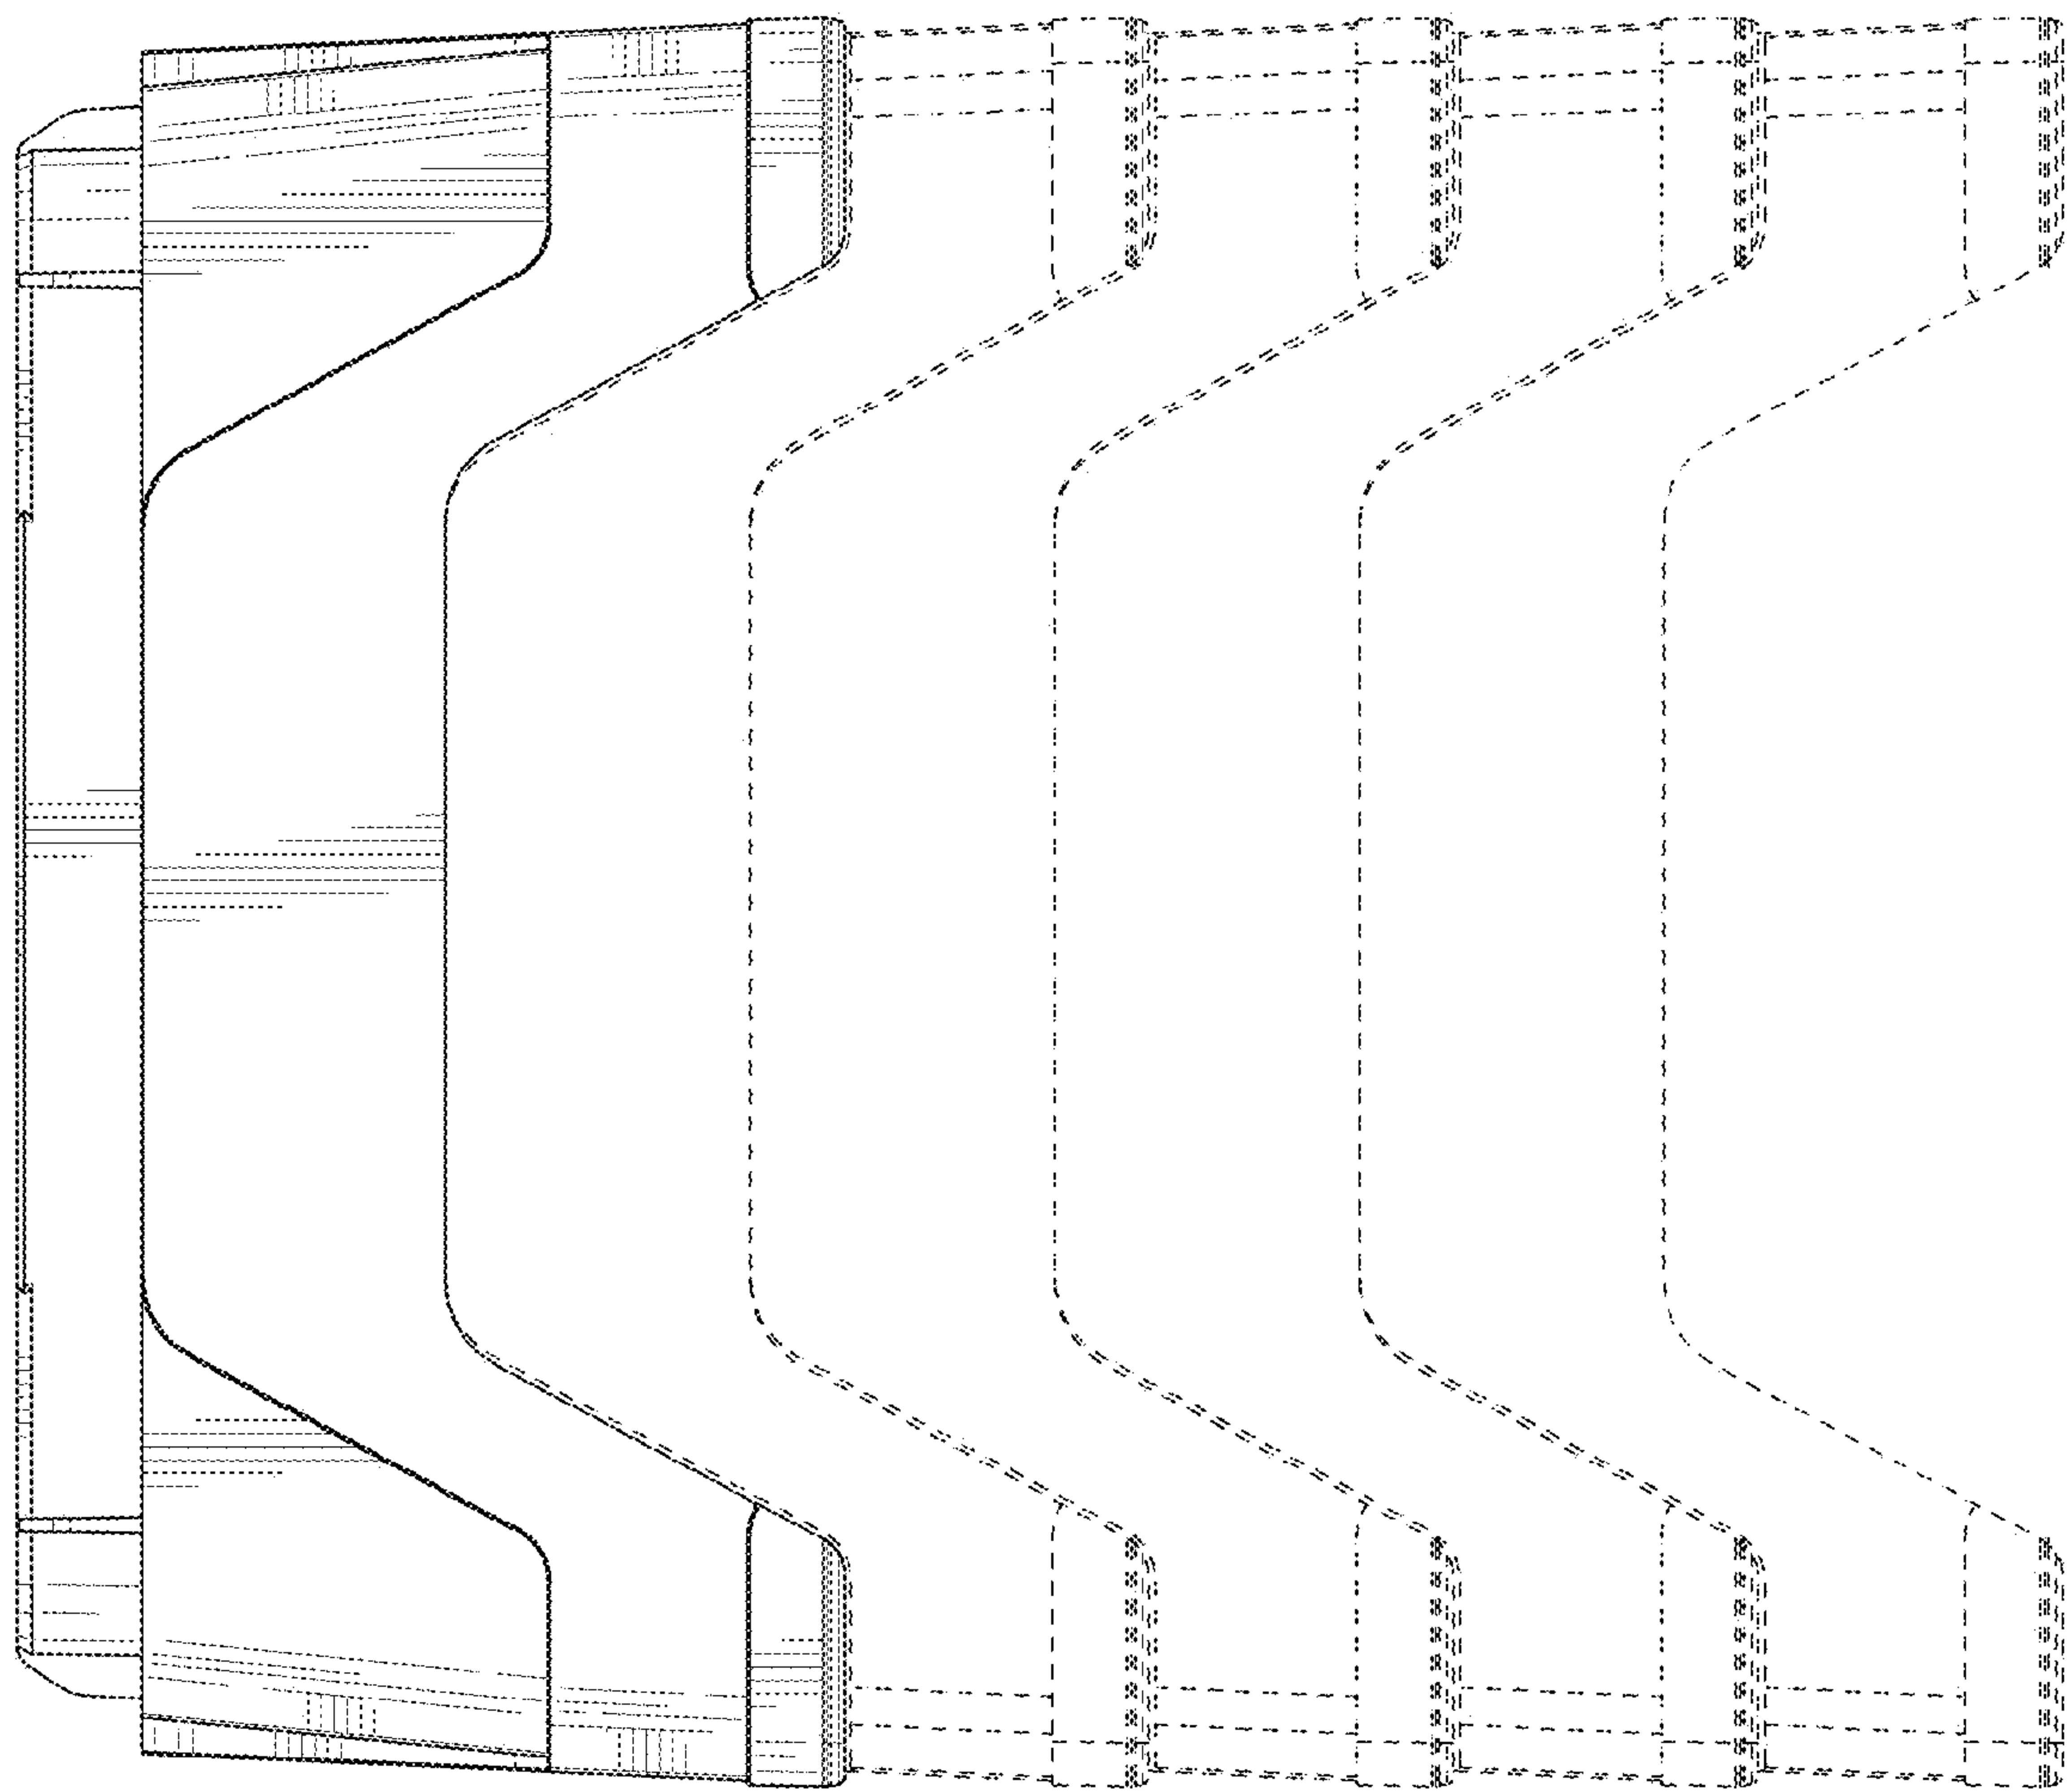


FIG. 35

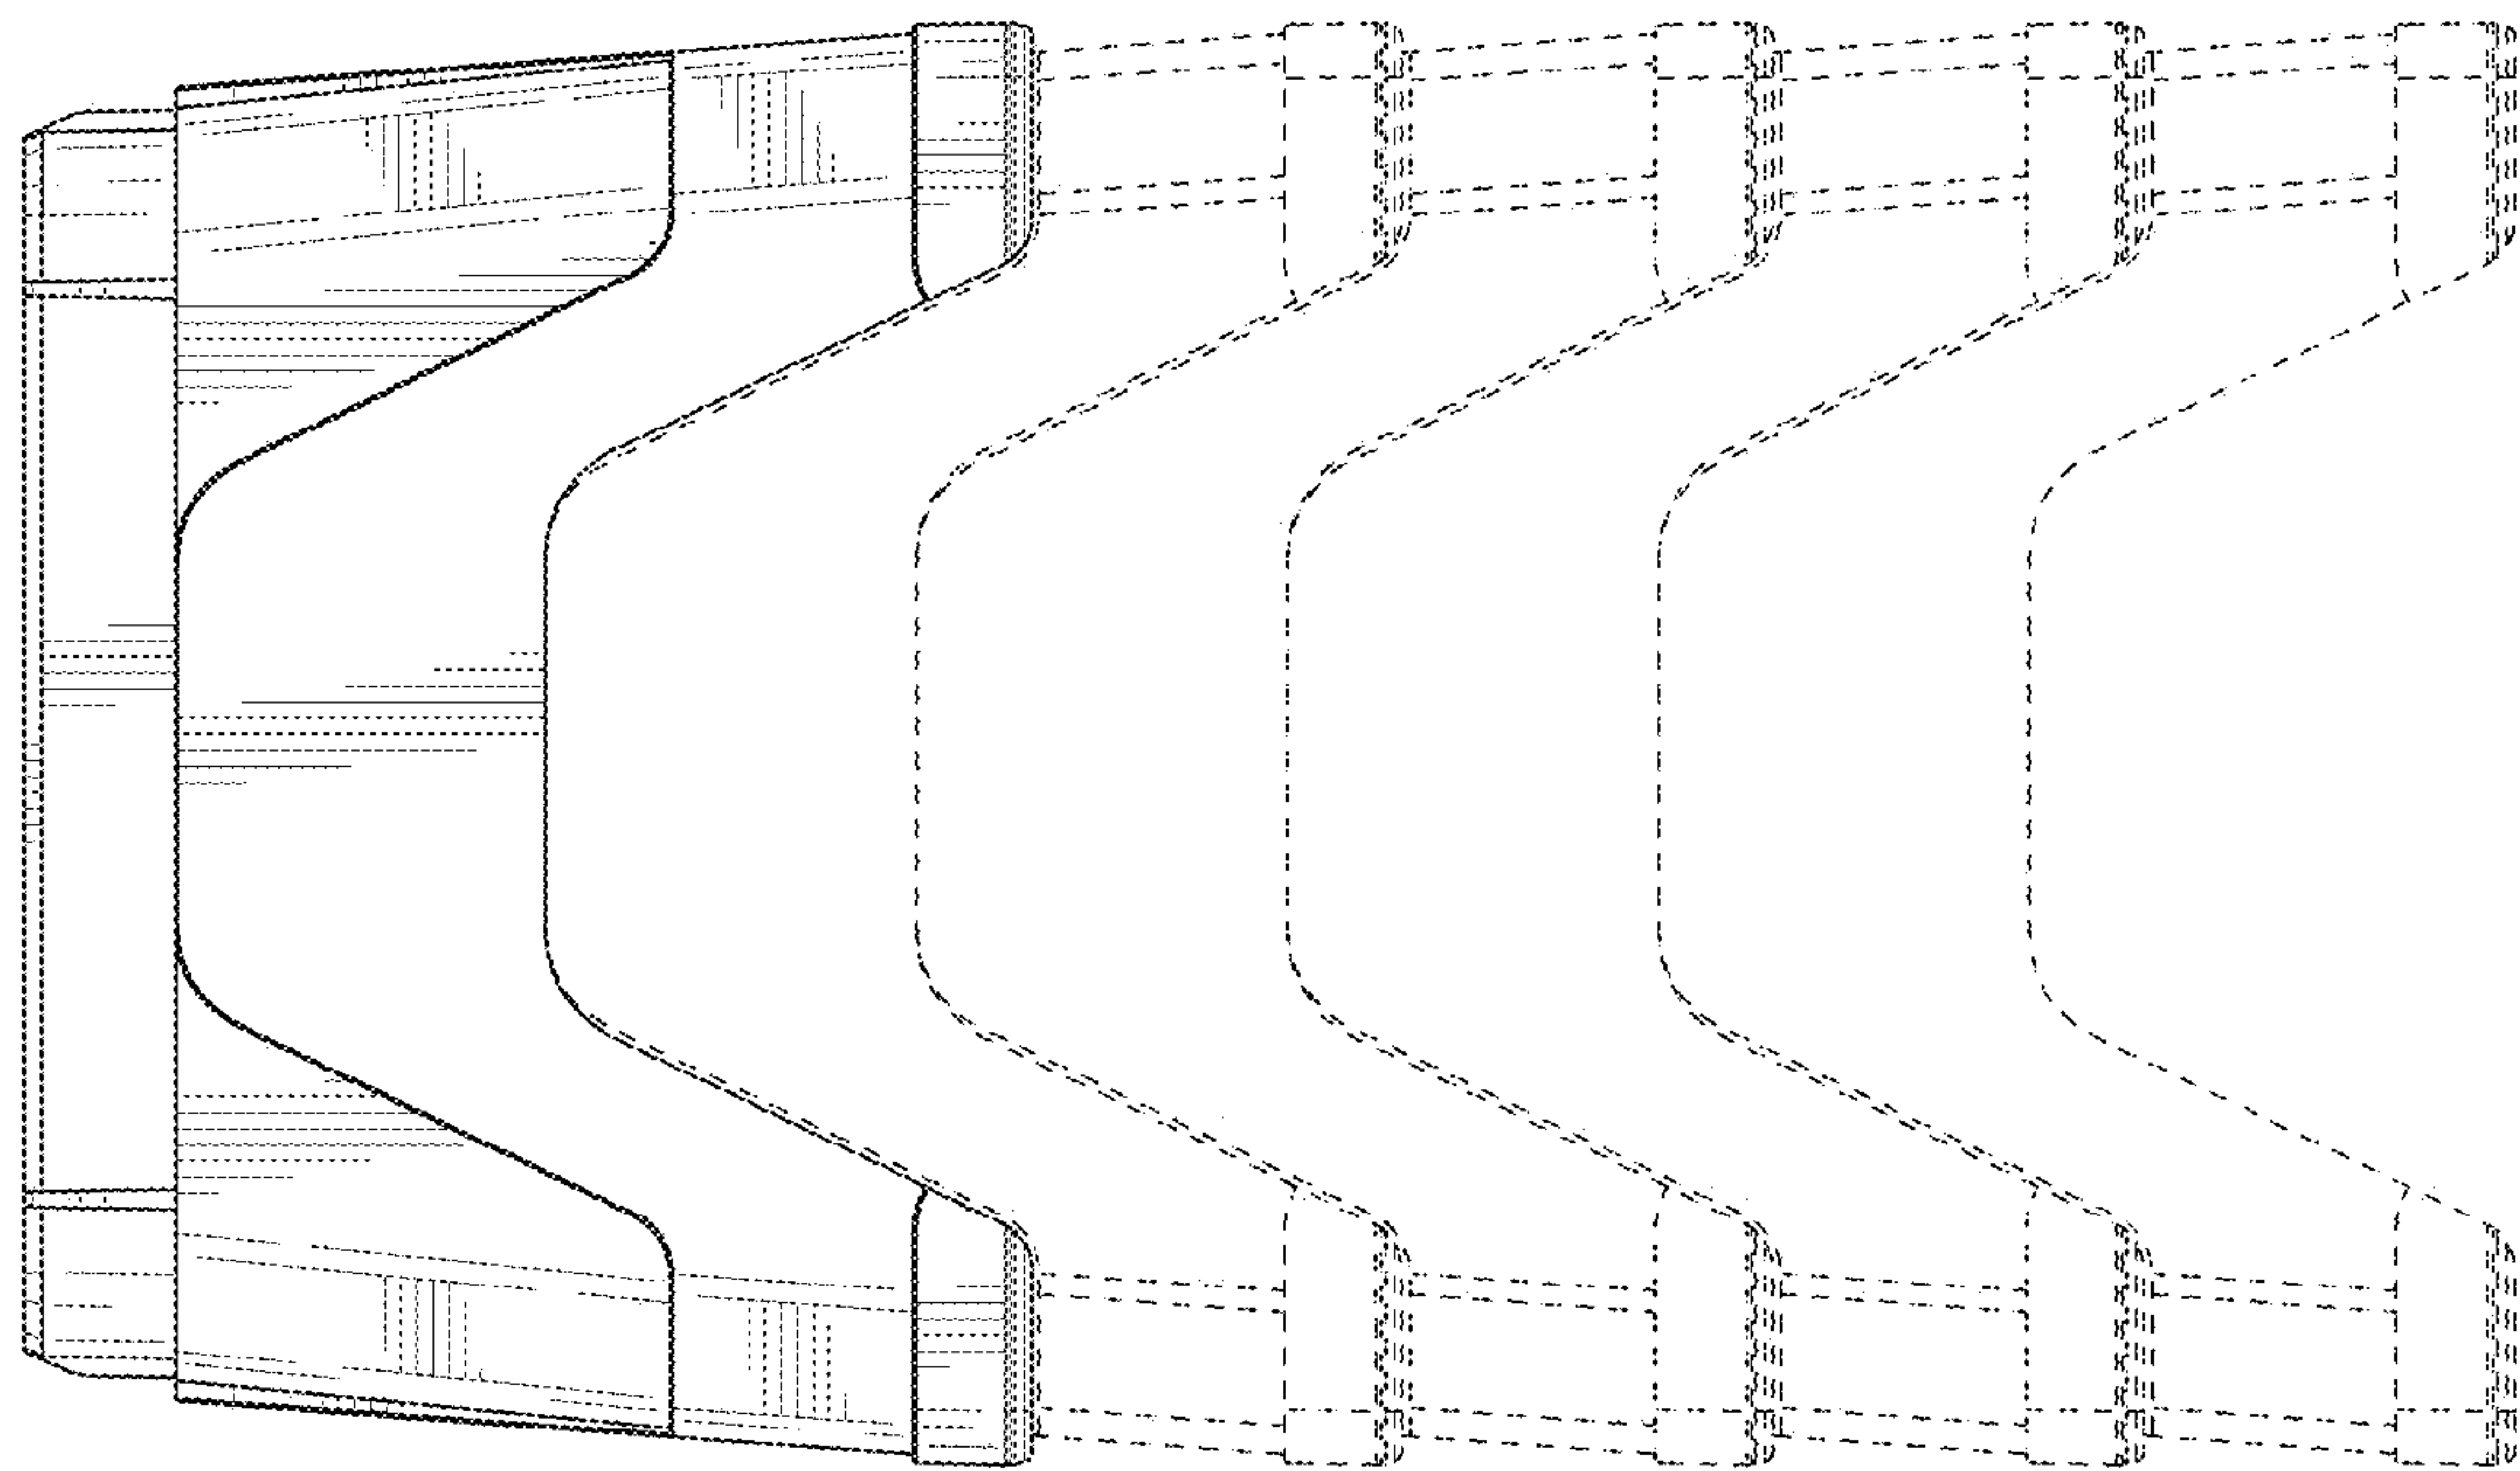


FIG. 36

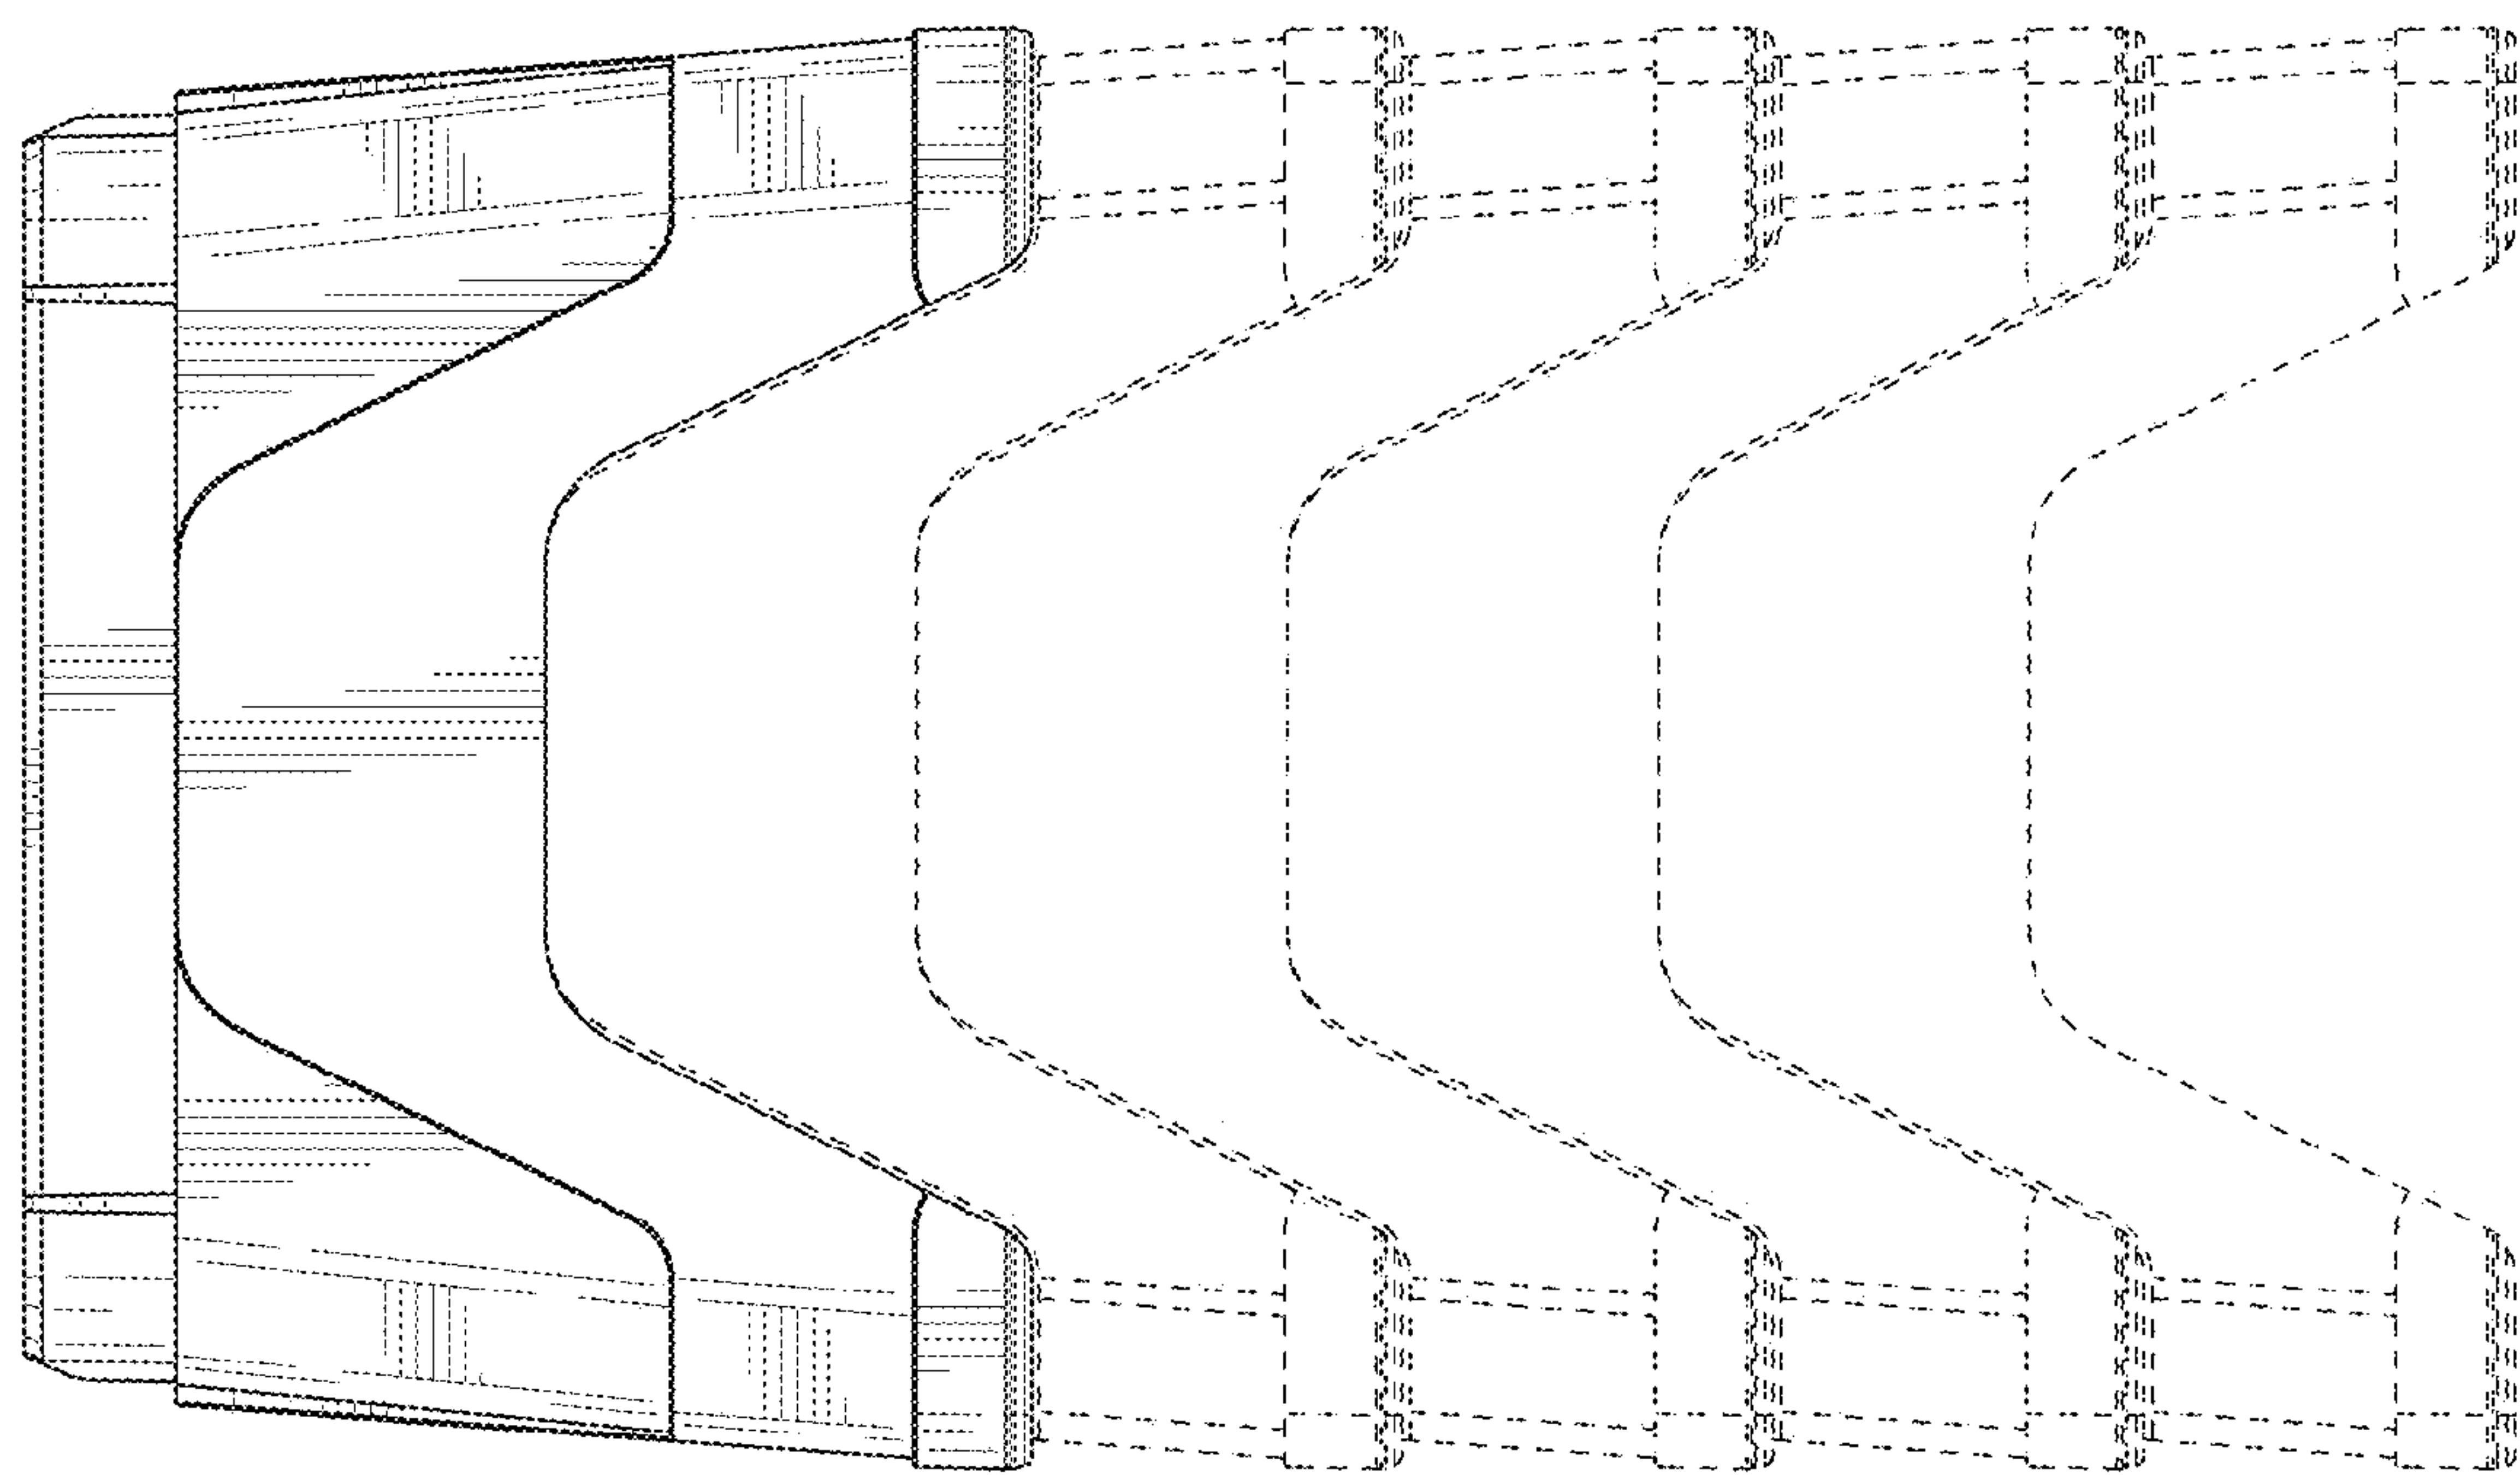


FIG. 37

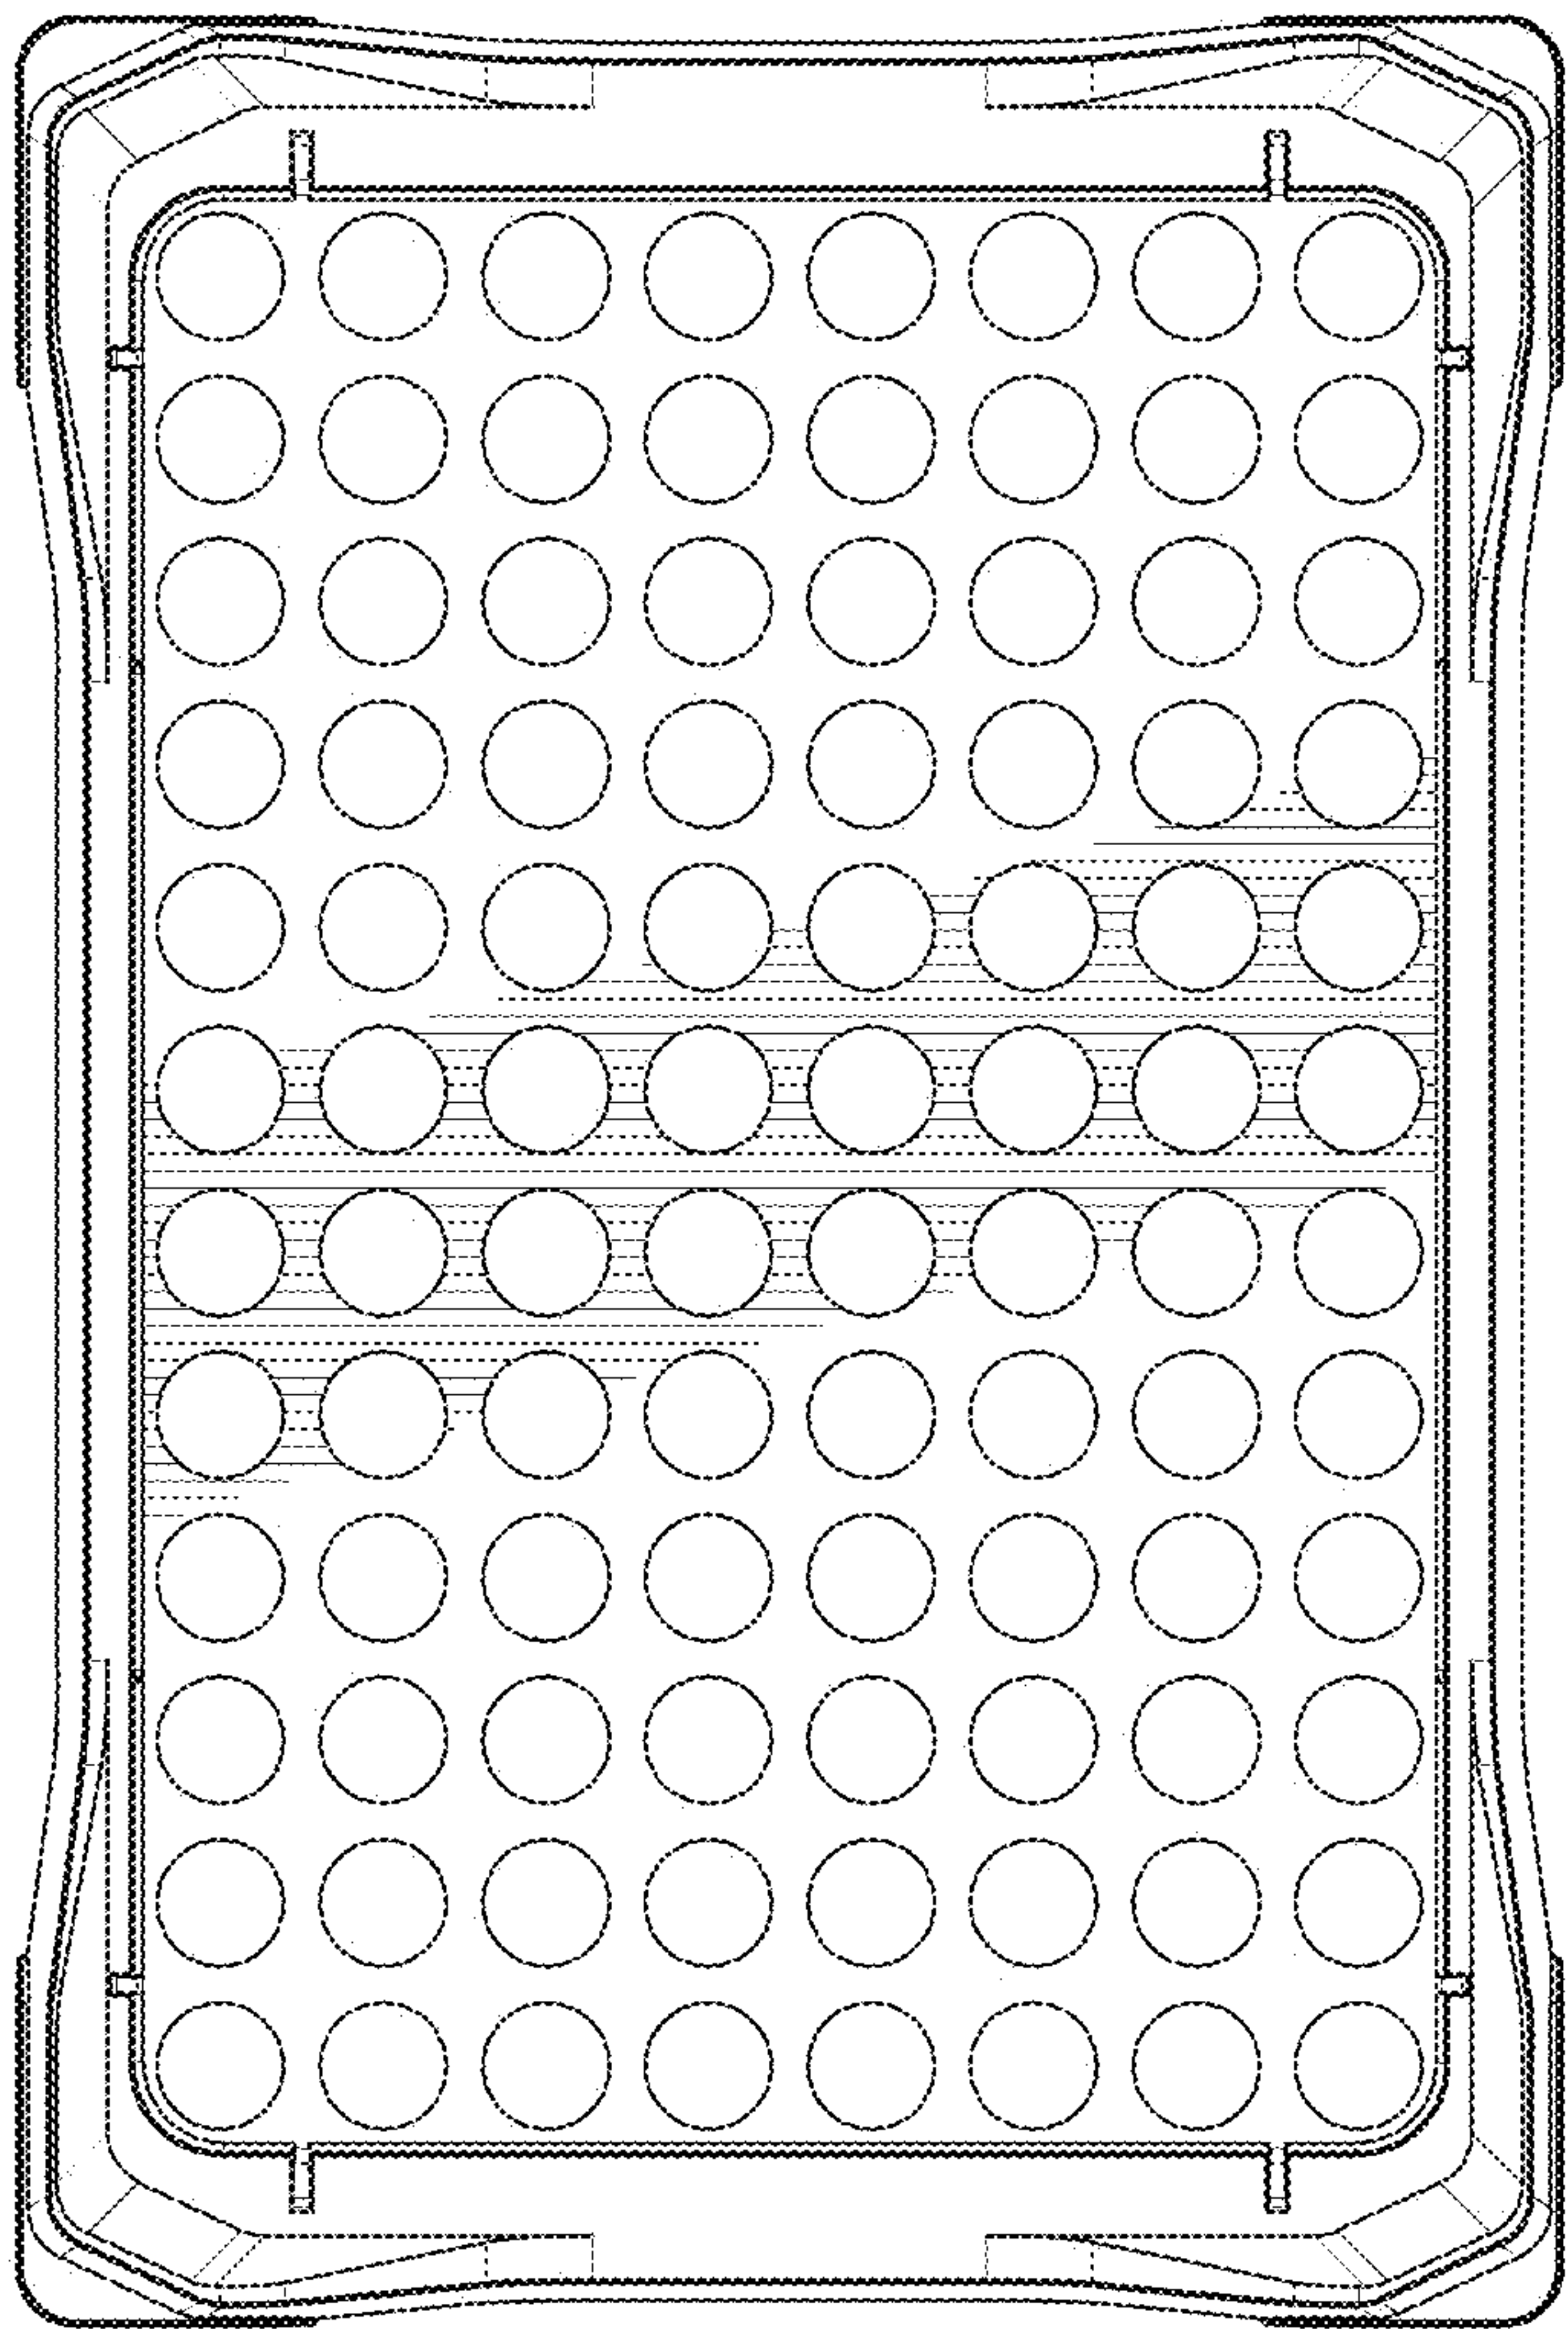


FIG. 38