



US00D915594S

(12) **United States Design Patent** (10) **Patent No.:** **US D915,594 S**
Chang et al. (45) **Date of Patent:** **** Apr. 6, 2021**

(54) **DENTAL SCANNER**

(71) Applicant: **Medit Corp.**, Seoul (KR)

(72) Inventors: **Min Ho Chang**, Seoul (KR); **Jin Pyo Chun**, Seoul (KR)

(73) Assignee: **Medit Corp.**, Seoul (KR)

(**) Term: **15 Years**

(21) Appl. No.: **29/699,725**

(22) Filed: **Jul. 29, 2019**

Related U.S. Application Data

(63) Continuation of application No. 35/504,952, filed on Apr. 12, 2018 (U.S. filing date under 35 U.S.C. 384), and having an international filing date of Apr. 12, 2018, now Pat. No. Des. 878,588.

(30) **Foreign Application Priority Data**

Oct. 18, 2017 (KR) 30-2017-0048356

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/152**

(58) **Field of Classification Search**
USPC D24/152, 127, 153, 154, 133, 177, 176
CPC .. G06T 7/75; G06T 15/08; G06T 7/55; H04N 13/271; H04N 13/254; H04N 13/257; H04N 13/246; H04N 13/221; A61B 5/7435; A61B 5/7203; A61B 5/0086; A61B 5/0062; A61B 1/24; A61C 9/0053
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,771,067 A * 6/1998 Williams A61B 1/00177
348/66
D414,867 S * 10/1999 Moriwaki D24/152

D558,345 S * 12/2007 Witt D24/152
D722,164 S * 2/2015 Graham, II D24/152
D780,182 S * 2/2017 Klein D14/426
D780,920 S * 3/2017 Pukall D24/152
D785,176 S * 4/2017 Tseng D24/152
D813,392 S * 3/2018 Wang D24/152
D829,325 S * 9/2018 Frenkler D24/138
D862,697 S * 10/2019 Kenworthy D24/158
D878,588 S * 3/2020 Chang D24/152
D884,175 S * 5/2020 Aubailly D24/152
D892,327 S * 8/2020 Jacob D24/152

* cited by examiner

Primary Examiner — Eliza Z Bennett-Hattan

(74) *Attorney, Agent, or Firm* — Millen, White, Zelano & Branigan, PC; William Nixon; Ryan Pool

(57) **CLAIM**

The ornamental design for a dental scanner, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the dental scanner showing our new design.

FIG. 2 is a front view thereof.

FIG. 3 is a back view thereof.

FIG. 4 is a side view thereof.

FIG. 5 is an another side view thereof.


FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The article is used to scan and measure with precision, objects such as teeth plaster molds shaped from the actual patient for the purpose of making a dental prosthesis.

The broken lines in the figures depict portions of the dental scanner that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

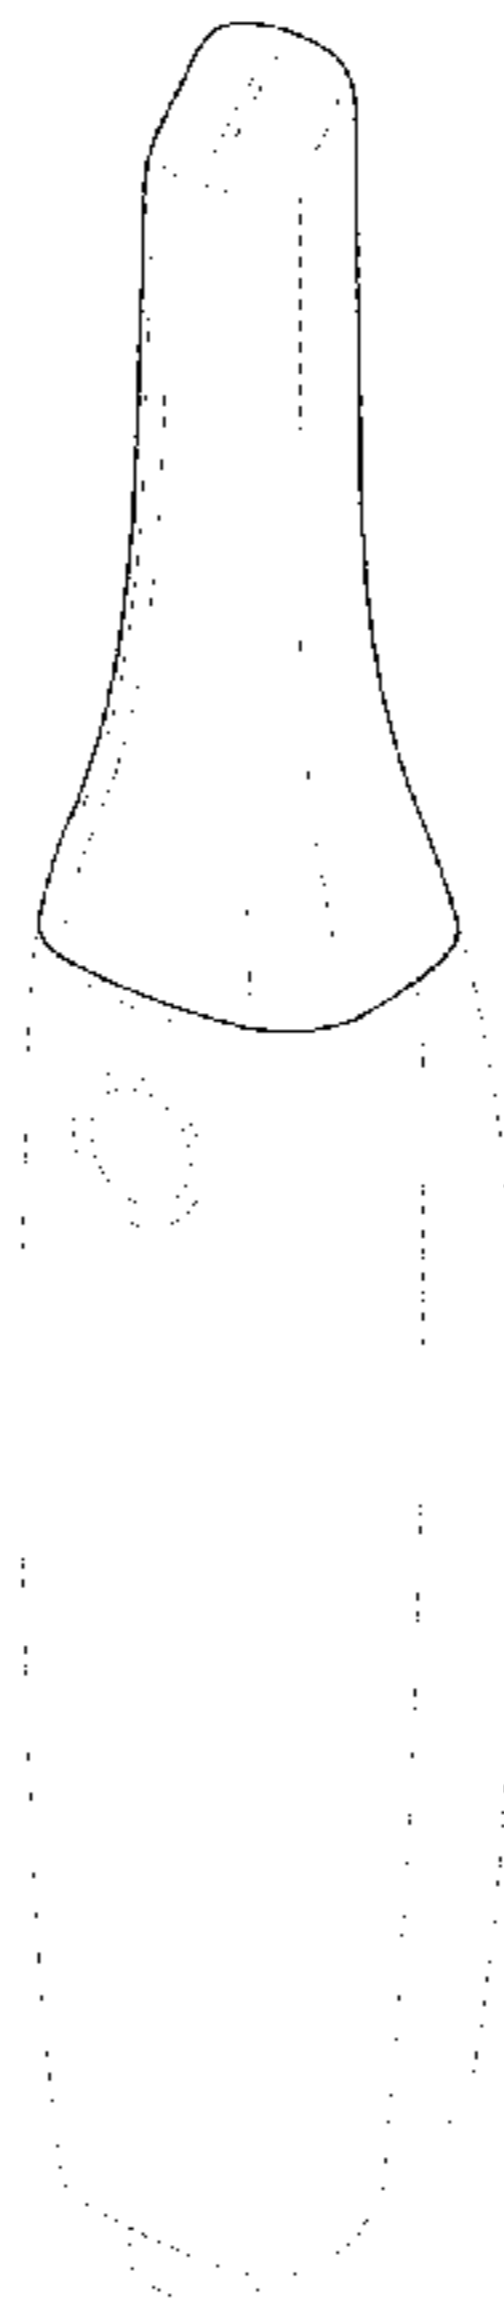

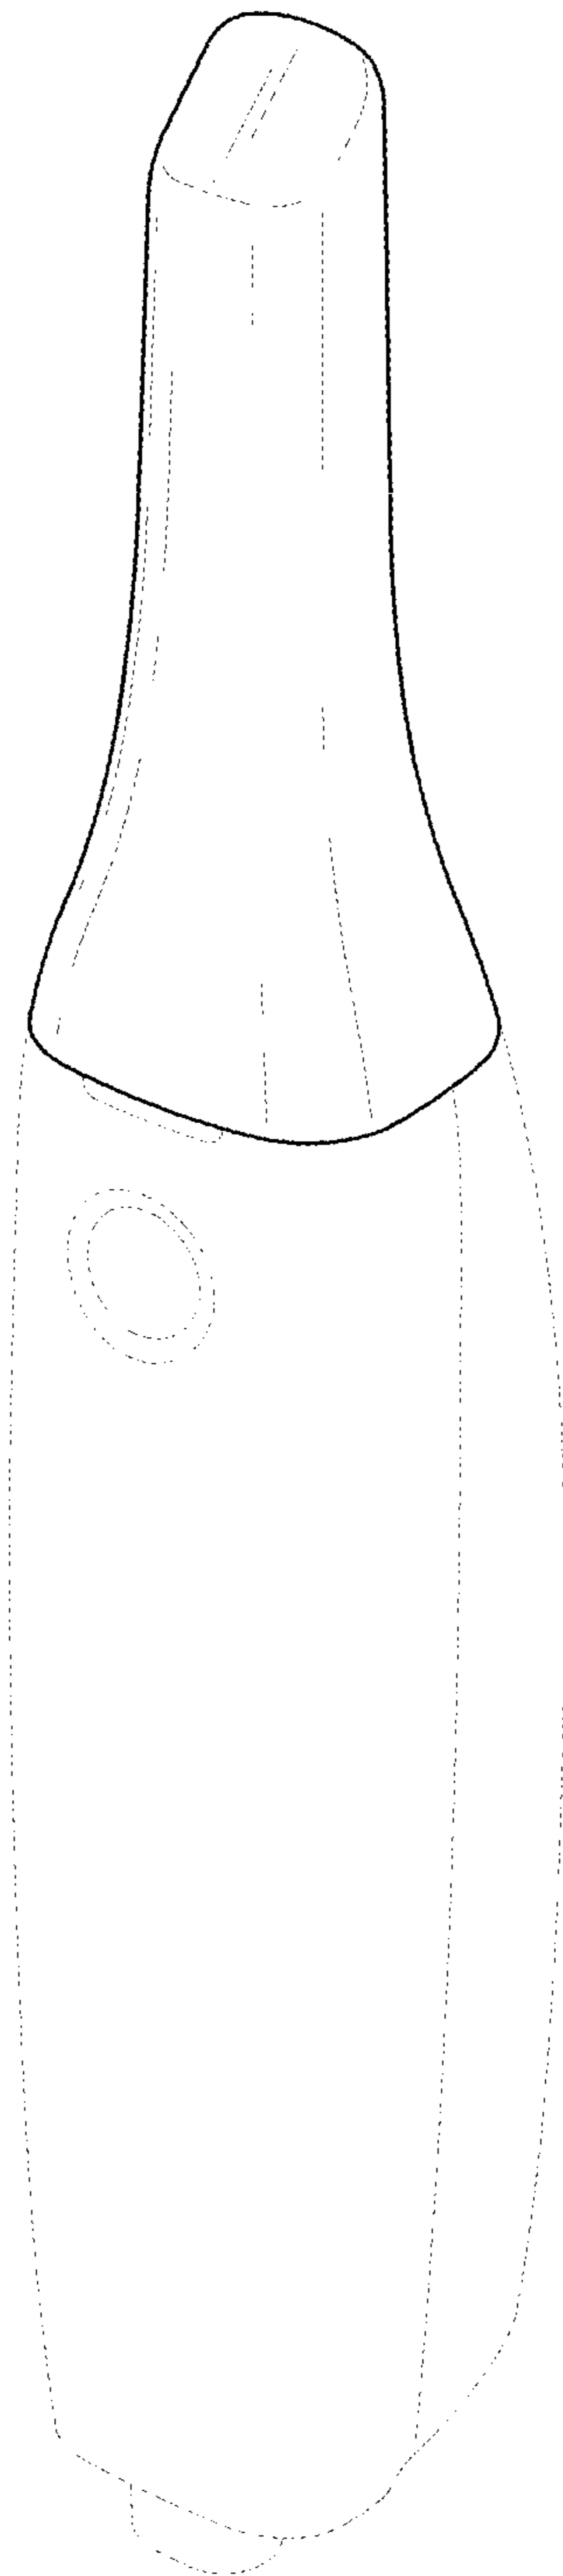


FIG. 1

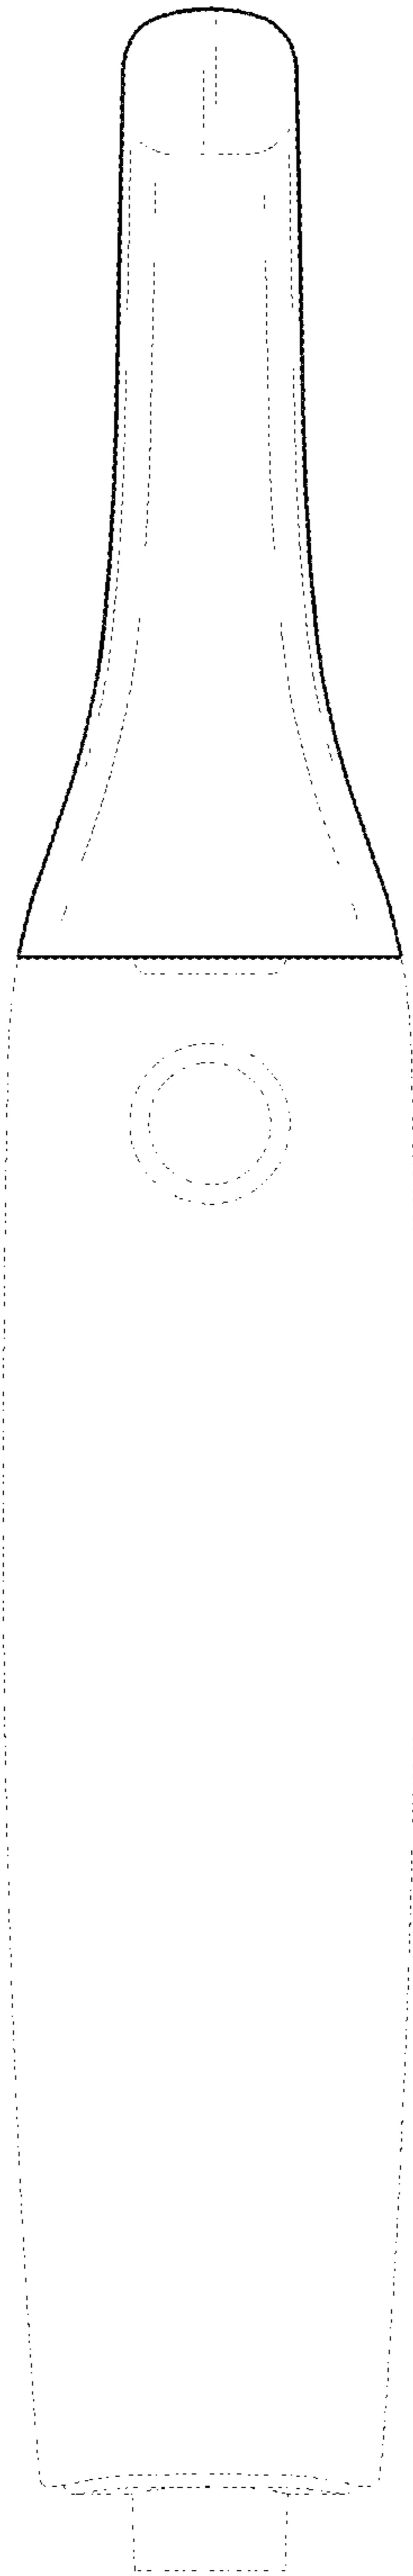


FIG. 2

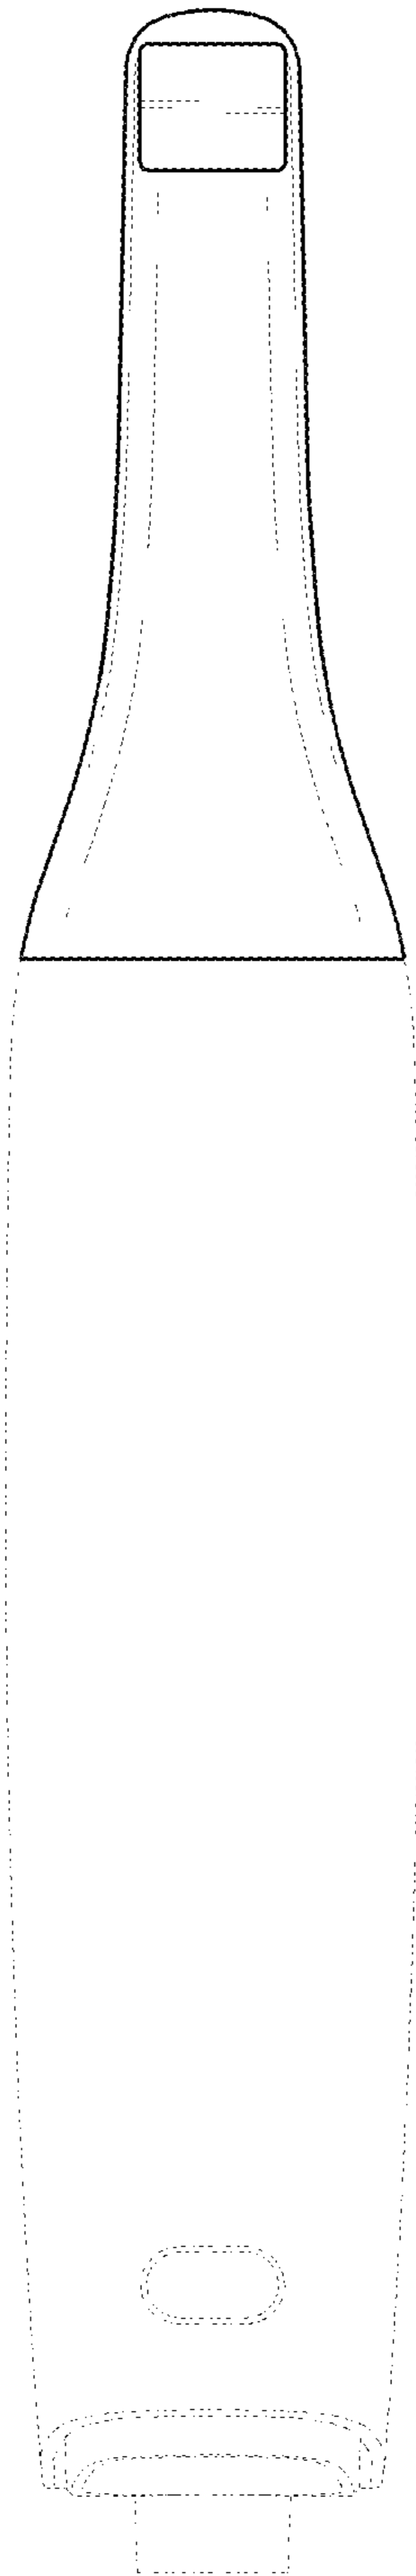


FIG. 3



FIG. 4



FIG. 5

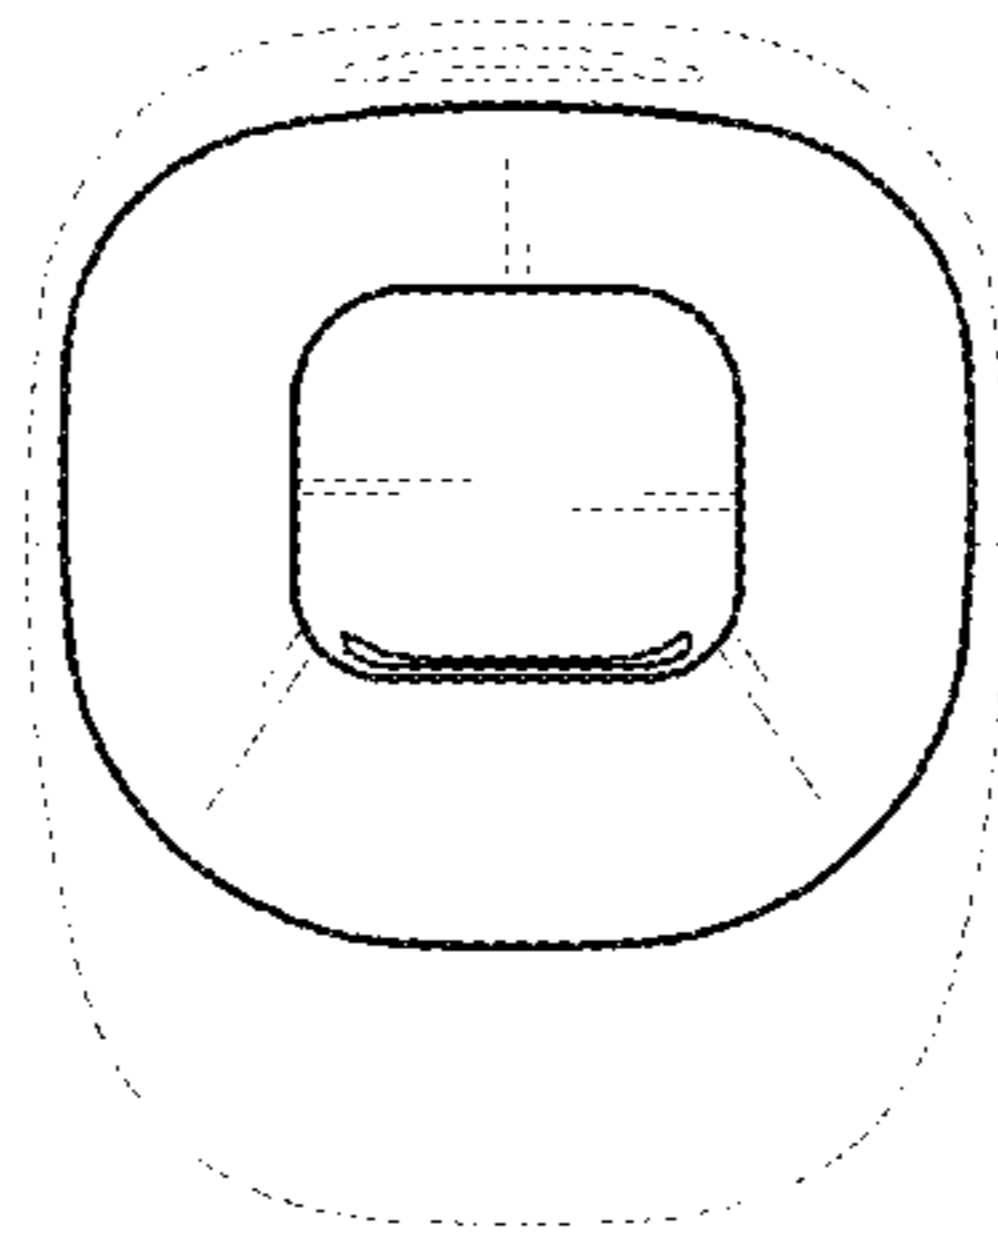


FIG. 6

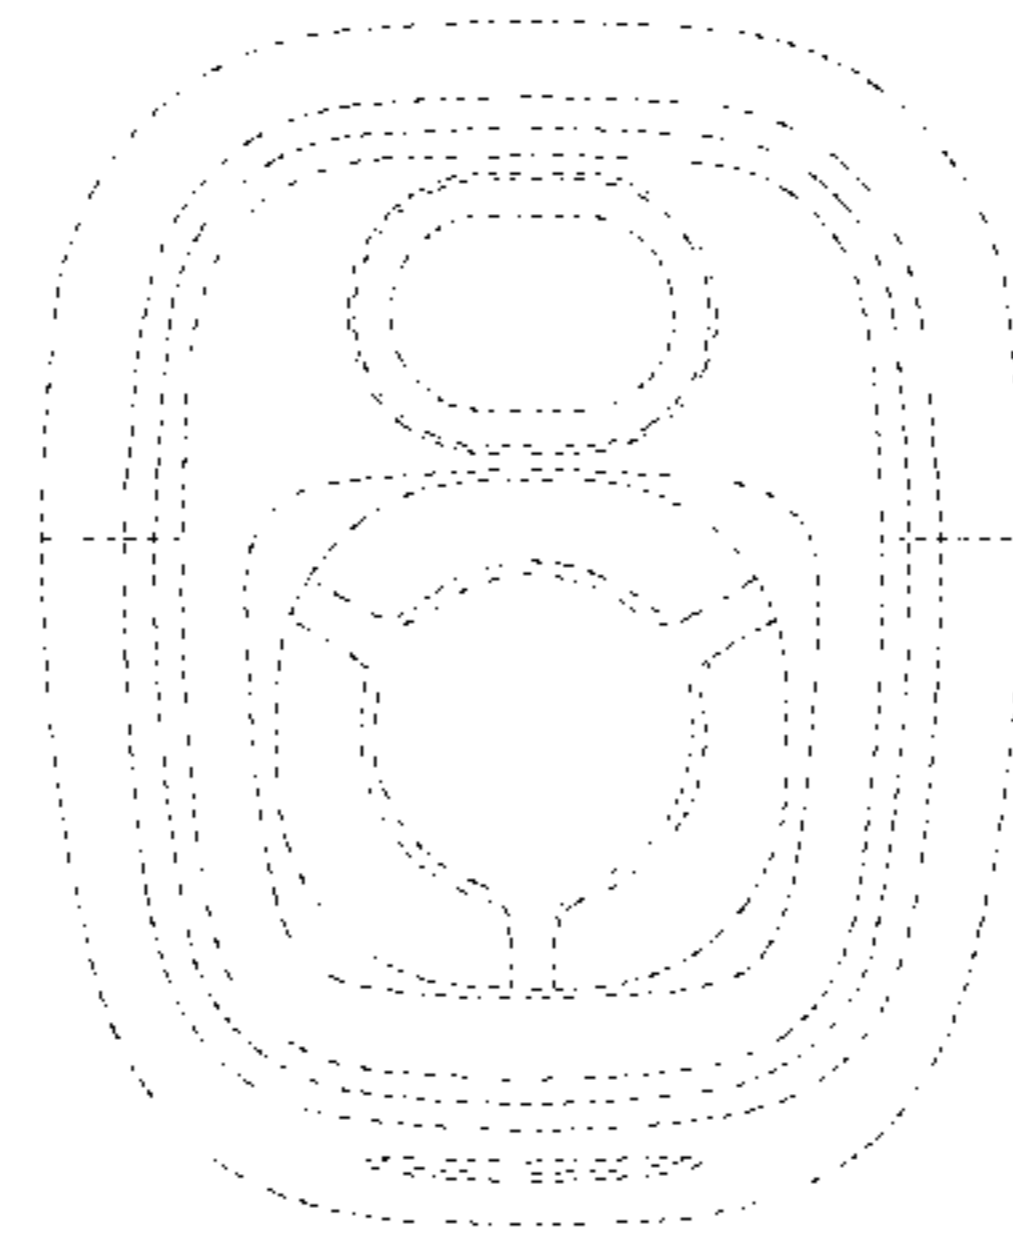


FIG. 7