



US00D916293S

(12) **United States Design Patent**
Toure

(10) **Patent No.:** **US D916,293 S**

(45) **Date of Patent:** **** Apr. 13, 2021**

(54) **LATERAL C-ARM DRAPE**

(71) Applicant: **TIDI Products, LLC**, Neenah, WI (US)

(72) Inventor: **Samba Toure**, Grand Blanc, MI (US)

(73) Assignee: **TIDI Products, LLC**, Neenah, WI (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/649,813**

(22) Filed: **Jun. 1, 2018**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/184; D24/189**

(58) **Field of Classification Search**
USPC D24/129, 132, 138, 158, 184, 188-190,
D24/225, 231, 234, 128; D6/602, 603;
D2/720, 841

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,791,382 A 2/1974 Collins
D256,161 S * 7/1980 Oliver D24/189
(Continued)

FOREIGN PATENT DOCUMENTS

CN 102112068 7/2013
CN 103356296 3/2016
(Continued)

OTHER PUBLICATIONS

TIDI Products "C-Armor Instructional Video"; YouTube video published on Jan. 24, 2018 <https://www.youtube.com/watch?v=nqg-1FfQScI>.

(Continued)

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Epiphany Law, LLC

(57) **CLAIM**

The ornamental design for a lateral C-arm drape, as shown and described.

DESCRIPTION

FIG. 1 is a side perspective view of the first embodiment of a lateral C-arm drape in a raised position;
FIG. 2 is a side perspective view of the lateral C-arm drape of FIG. 1 in an expanded position;
FIG. 3 is a side, raised perspective view of the lateral C-arm drape of FIGS. 1 and 2 in a middle position between the collapsed position and the expanded position where the fasteners have been disengaged;
FIG. 4 is a front elevation view of the lateral C-arm drape of FIG. 3 in the middle position;
FIG. 5 is a rear elevation view of the lateral C-arm drape of FIGS. 3 and 4 in the middle position showing a fastener that can be used to attach the drape to the operating table or patient drape;
FIG. 6 is a right side elevation view of the lateral C-arm drape of FIGS. 3-5 in the middle position;
FIG. 7 is a left side elevation view of the lateral C-arm drape of FIGS. 3-6 in the middle position;
FIG. 8 is a top plan view of the lateral C-arm drape of FIGS. 3-7 in the middle position;
FIG. 9 is a top plan view of the lateral C-arm drape of FIGS. 3-8 in the middle position;
FIG. 10 is a side perspective view of the second embodiment of a lateral C-arm drape in a raised position;
FIG. 11 is a side perspective view of the lateral C-arm drape of FIG. 10 in an expanded position;
FIG. 12 is a side, raised perspective view of the lateral C-arm drape of FIGS. 10 and 11 in a middle position between the collapsed position and the expanded position where the fasteners have been disengaged;
FIG. 13 is a front elevation view of the lateral C-arm drape of FIG. 12 in the middle position;

(Continued)

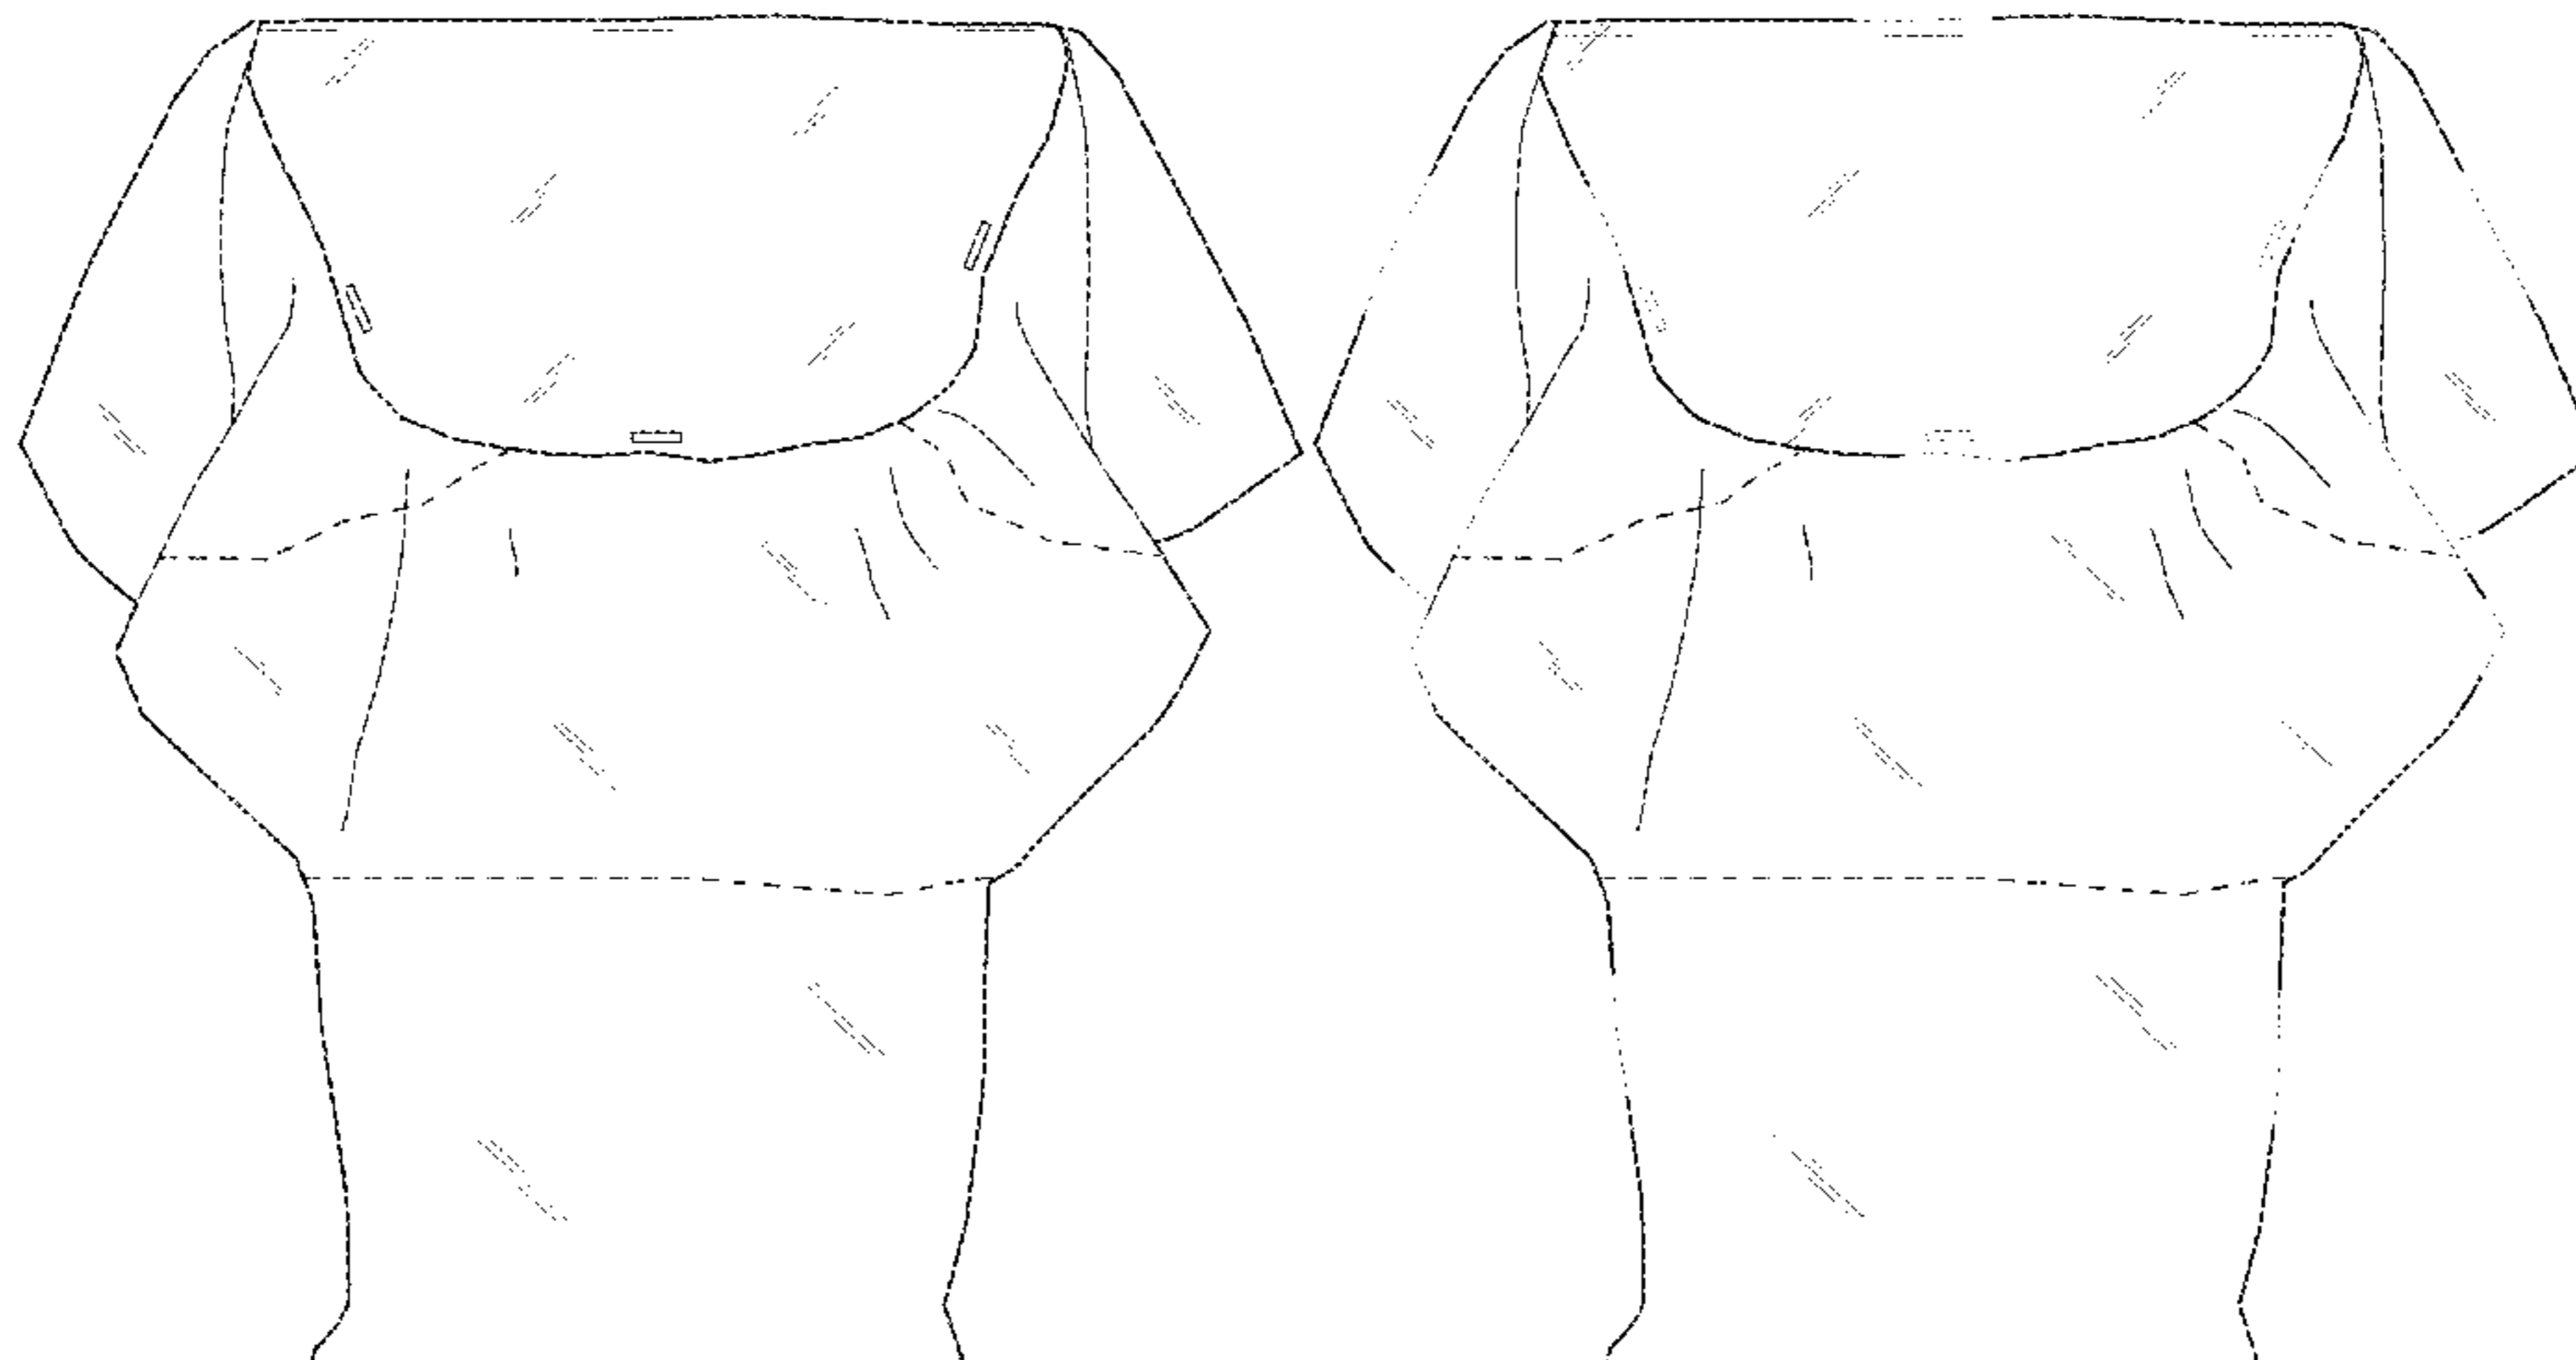


FIG. 14 is a rear elevation view of the lateral C-arm drape of FIGS. 12 and 13 in the middle position showing a fastener that can be used to attach the drape to the operating table or patient drape;

FIG. 15 is a right side elevation view of the lateral C-arm drape of FIGS. 12-14 in the middle position;

FIG. 16 is a left side elevation view of the lateral C-arm drape of FIGS. 12-15 in the middle position;

FIG. 17 is a top plan view of the lateral C-arm drape of FIGS. 12-16 in the middle position; and,

FIG. 18 is a top plan view of the lateral C-arm drape of FIGS. 12-17 in the middle position.

The dash dot broken lines in the drawings depict environmental subject matter and form no part of the claimed design. The lighter dash lines depict portions of the Lateral C-Arm Drape that form no part of the claimed design. The bold dash lines depict fold lines that form no part of the claimed design.

1 Claim, 18 Drawing Sheets

(58) Field of Classification Search

CPC A61B 46/23; A61B 46/30; A61B 46/40; A61B 5/411; A61B 50/33; A61B 19/00

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

4,489,720	A	12/1984	Morris	
4,730,609	A	3/1988	McConnell	
5,445,165	A	8/1995	Fenwick	
D370,822	S *	6/1996	Palomo	D24/192
D373,921	S *	9/1996	Palomo	D24/189
D428,137	S *	7/2000	Phelan	D24/108
D467,345	S *	12/2002	Gingles	D24/189
6,615,836	B1 *	9/2003	Griesbach	A61B 46/23 128/849
6,644,317	B1 *	11/2003	Lawton	A61B 46/23 128/849
7,044,132	B2	5/2006	Masini	
D598,546	S *	8/2009	Melder	D24/138

7,717,117	B2	5/2010	Duarte	
7,727,244	B2	6/2010	Orban, III	
D622,389	S *	8/2010	Henke-Sarmiento	D24/158
8,042,549	B2	10/2011	Kaska	
8,286,637	B2	10/2012	Kaska	
D690,078	S *	9/2013	Anderson	D2/720
D721,870	S *	2/2015	Levine	D2/720
D831,937	S *	10/2018	James	D2/860
D851,772	S *	6/2019	Haines	D24/184
2006/0020152	A1	1/2006	Theobald	
2006/0076024	A1	4/2006	Duarte	
2006/0201521	A1	9/2006	Masini	
2008/0006278	A1	1/2008	Henke-Sarmiento	
2008/0047567	A1	2/2008	Bonutti	
2010/0242150	A1 *	9/2010	Trouillot	A41D 13/1245 2/114
2016/0166323	A1	6/2016	Tylka	
2018/0214228	A1	8/2018	Toure	

FOREIGN PATENT DOCUMENTS

EP	2265209	1/2017
EP	3178437	6/2017
WO	WO1996038096	12/1996
WO	WO0215198	2/2002
WO	WO2006038096	1/2006
WO	WO2007041093	4/2007

OTHER PUBLICATIONS

TIDI Products "C-Armor Instructional Video"; YouTube video published on Mar. 7, 2016 <https://www.youtube.com/Watch?v=GMbV2IWQcFU>.

Tyler Martin "C-Armor—Defend the Sterile Field"; YouTube video published on Apr. 17, 2012 <https://www.youtube.com/watch?v=BmcFGO2986o>.

Serge C. Kaska; "A standardized and safe method of sterile field maintenance during intra-operative horizontal plane fluoroscopy"; Article published Dec. 13, 2010; Patient Safety in Surgery 4, Article No. 20.

Case 3:13-cv-01105—United States District Court Southern District of California Complaint; Published May 8, 2013 *Rawcar Group, LLC d/b/a CFI Medical Solutions v. Grace Medical, Inc., Pulse Medical, Inc., Preferred Medical Products, and A&B Medical Specialties, LLC*.

European Search Report for European App. No. 19209846.5 dated Mar. 17, 2020; 7 pages.

* cited by examiner

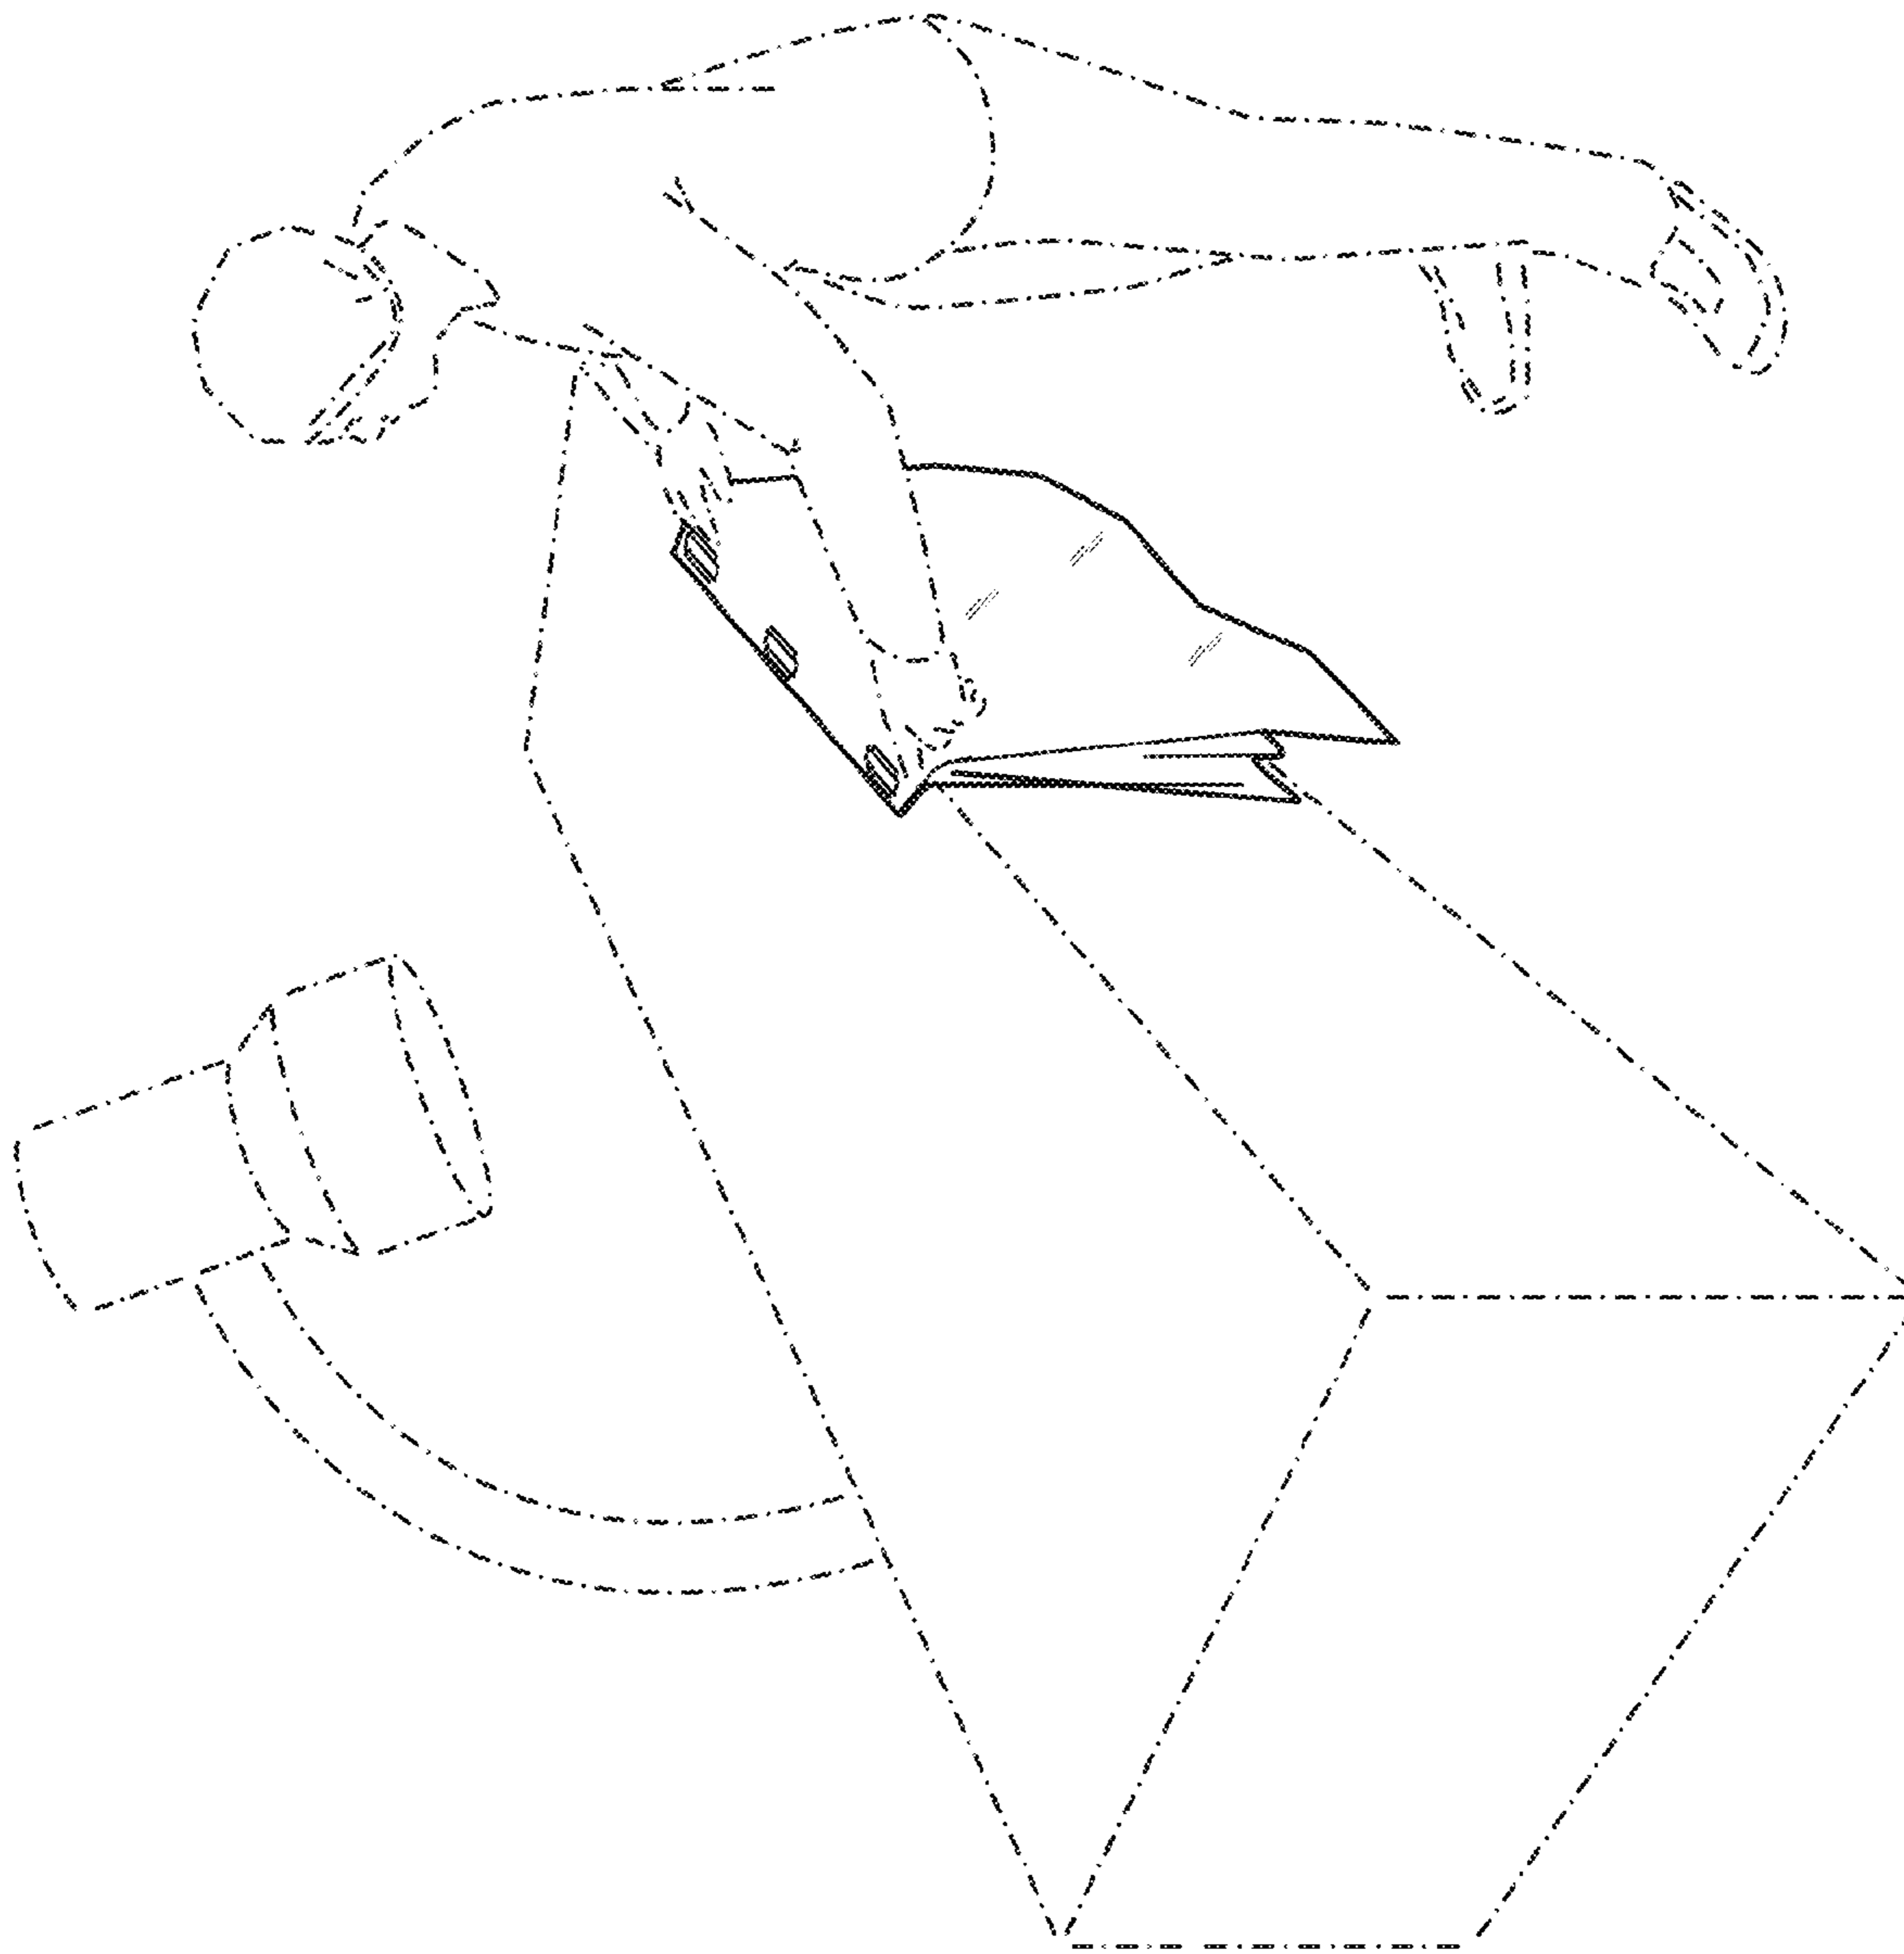


Fig. 1

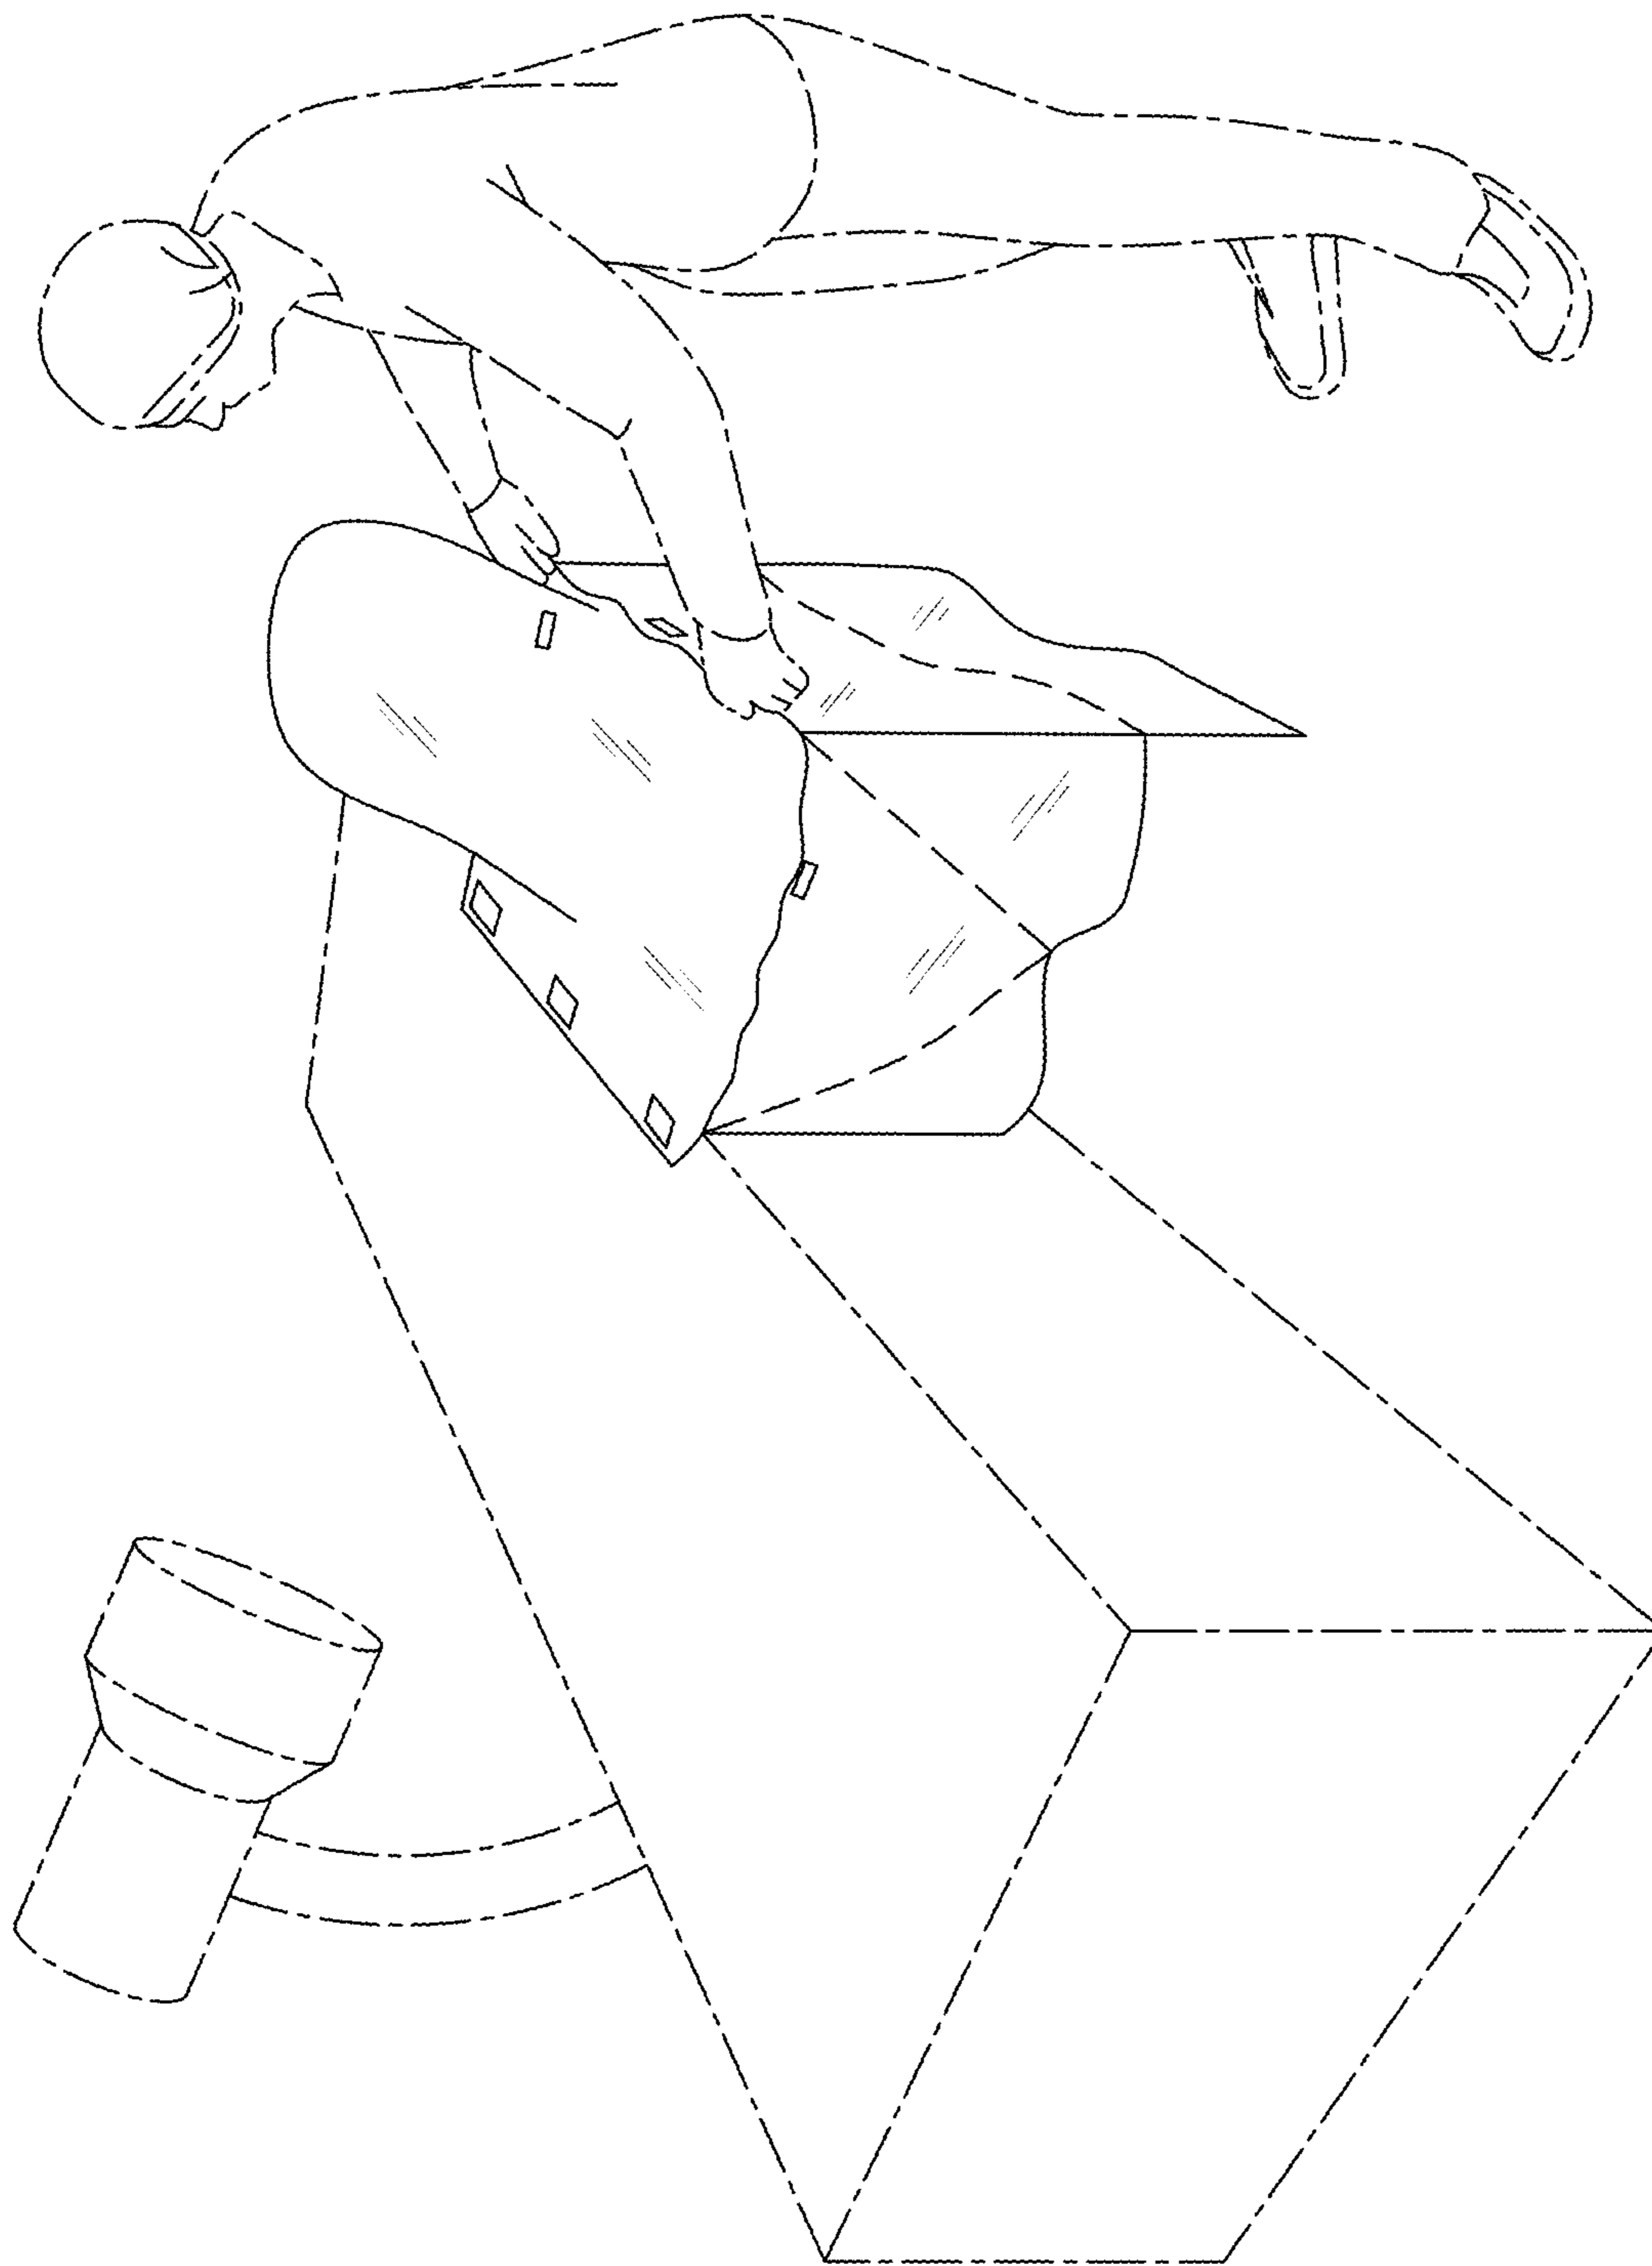


FIG. 2

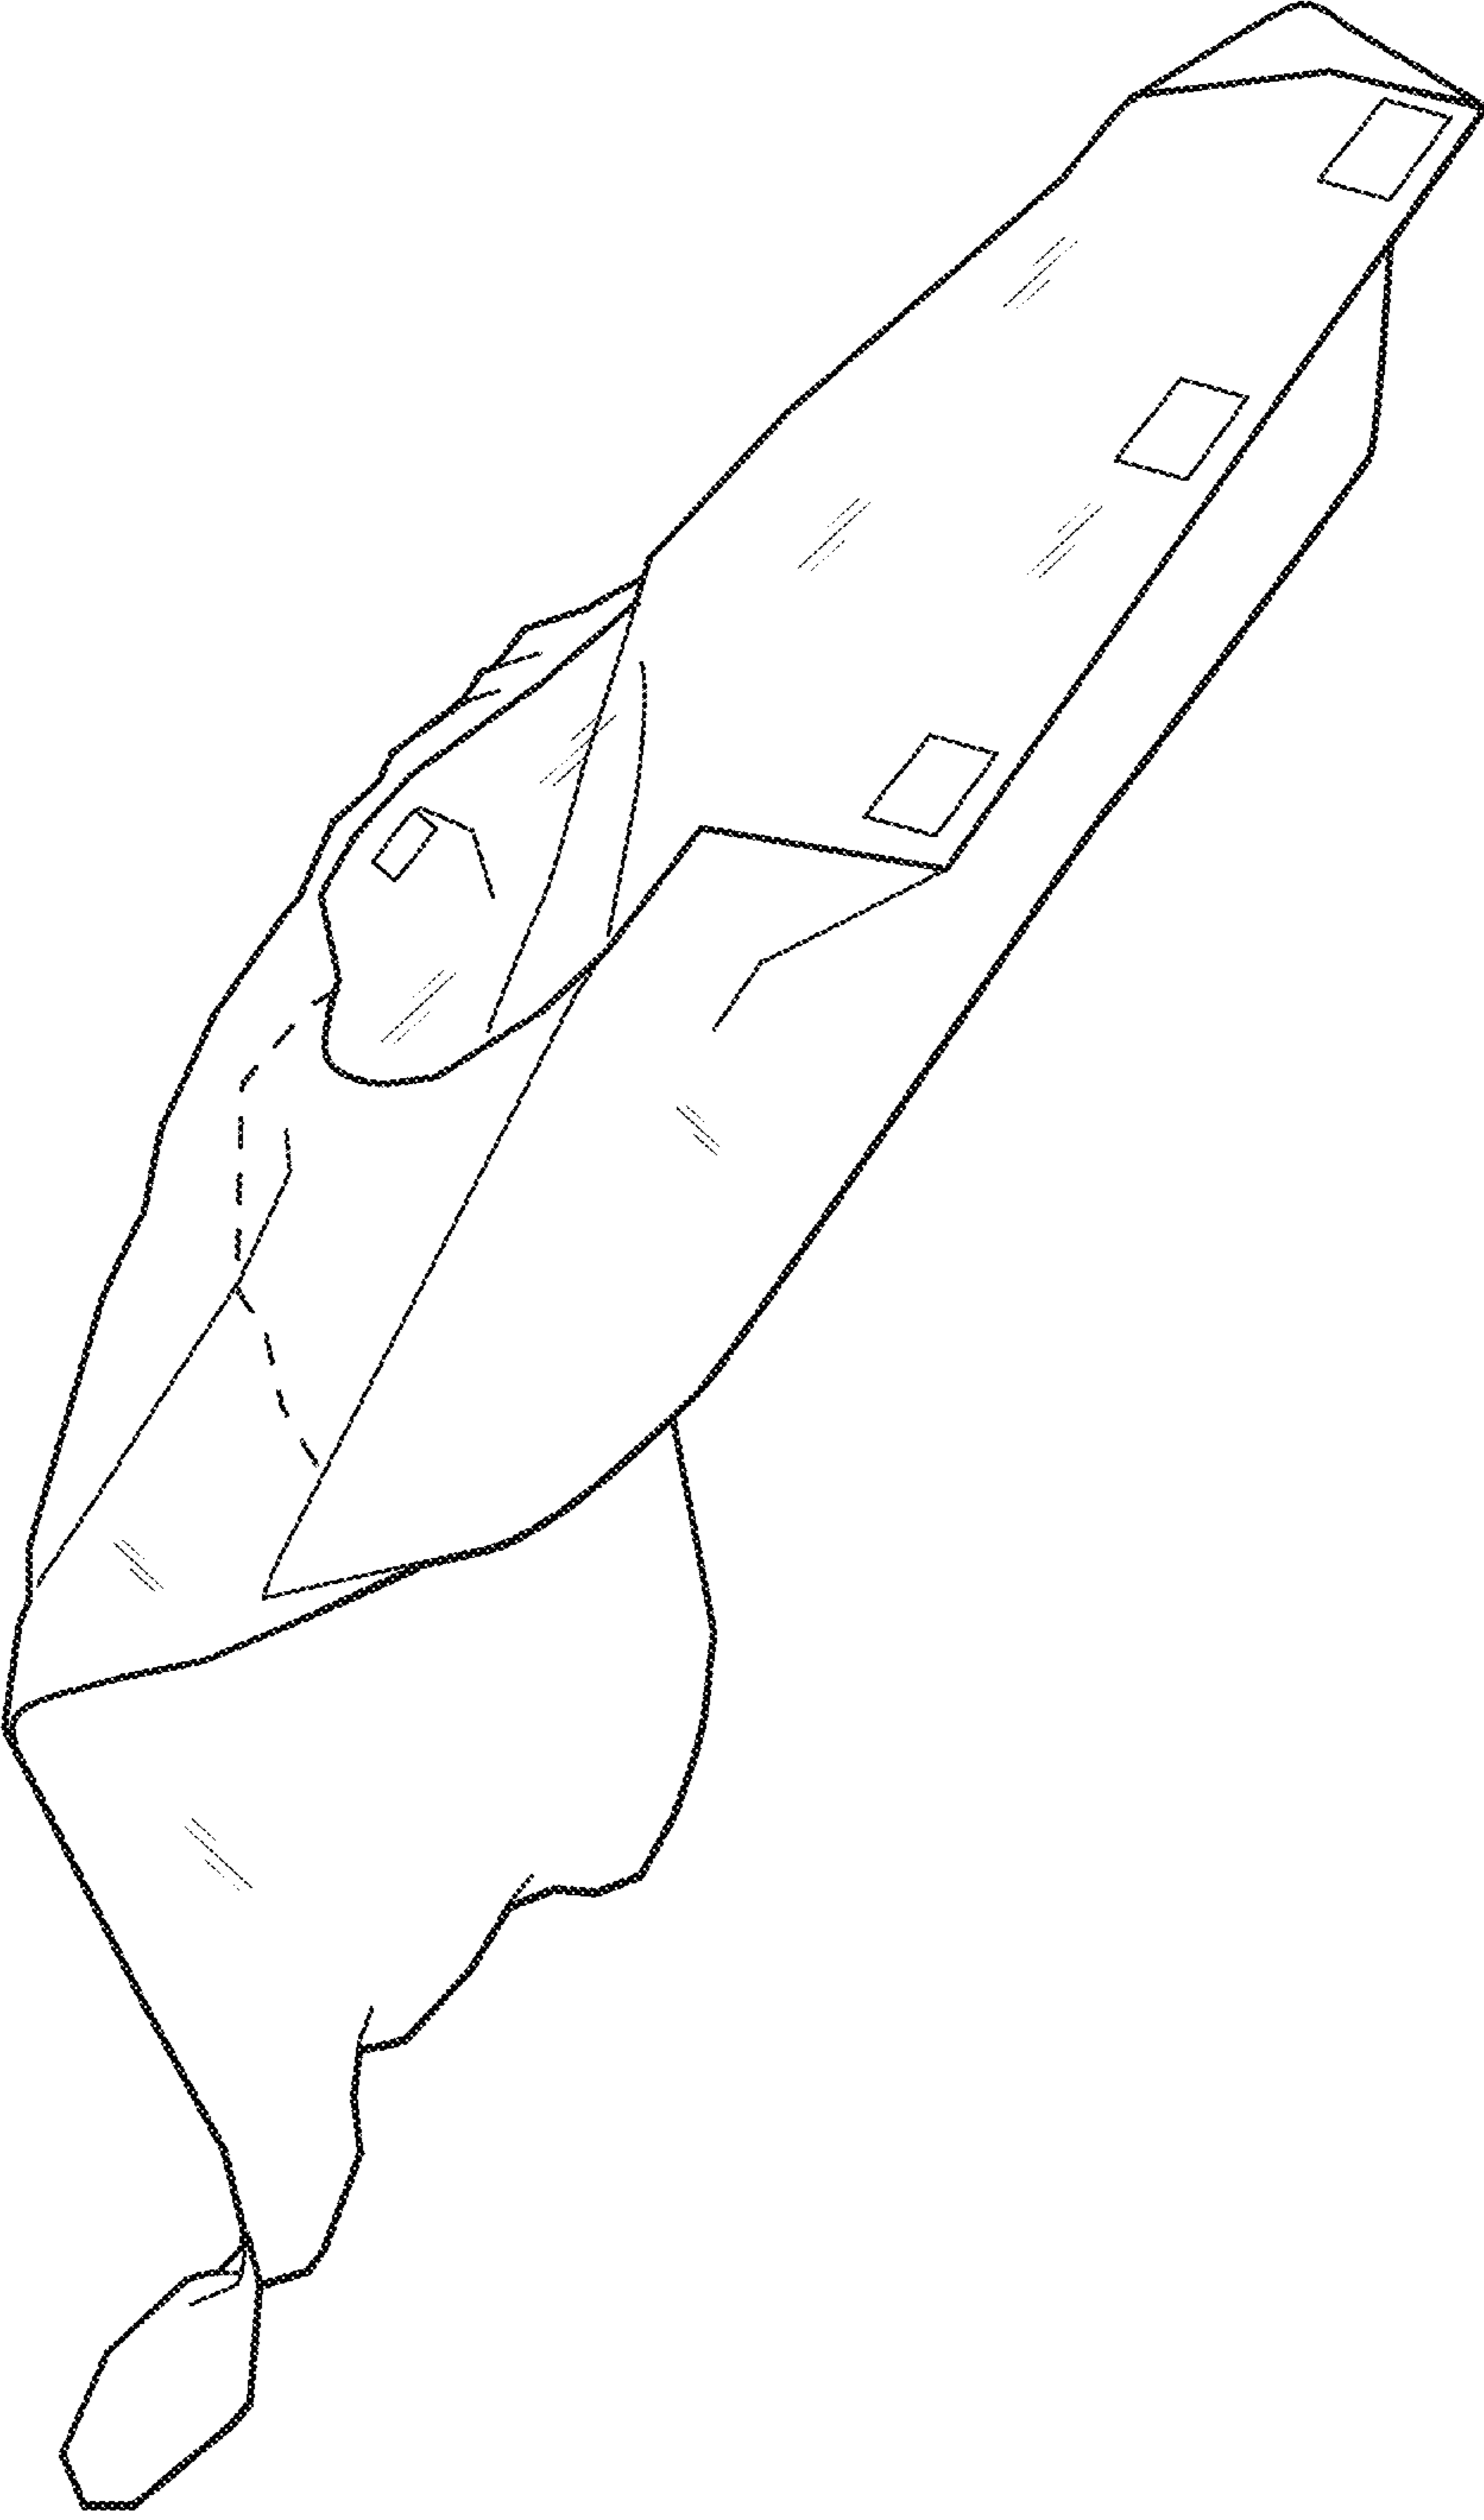


Fig. 3

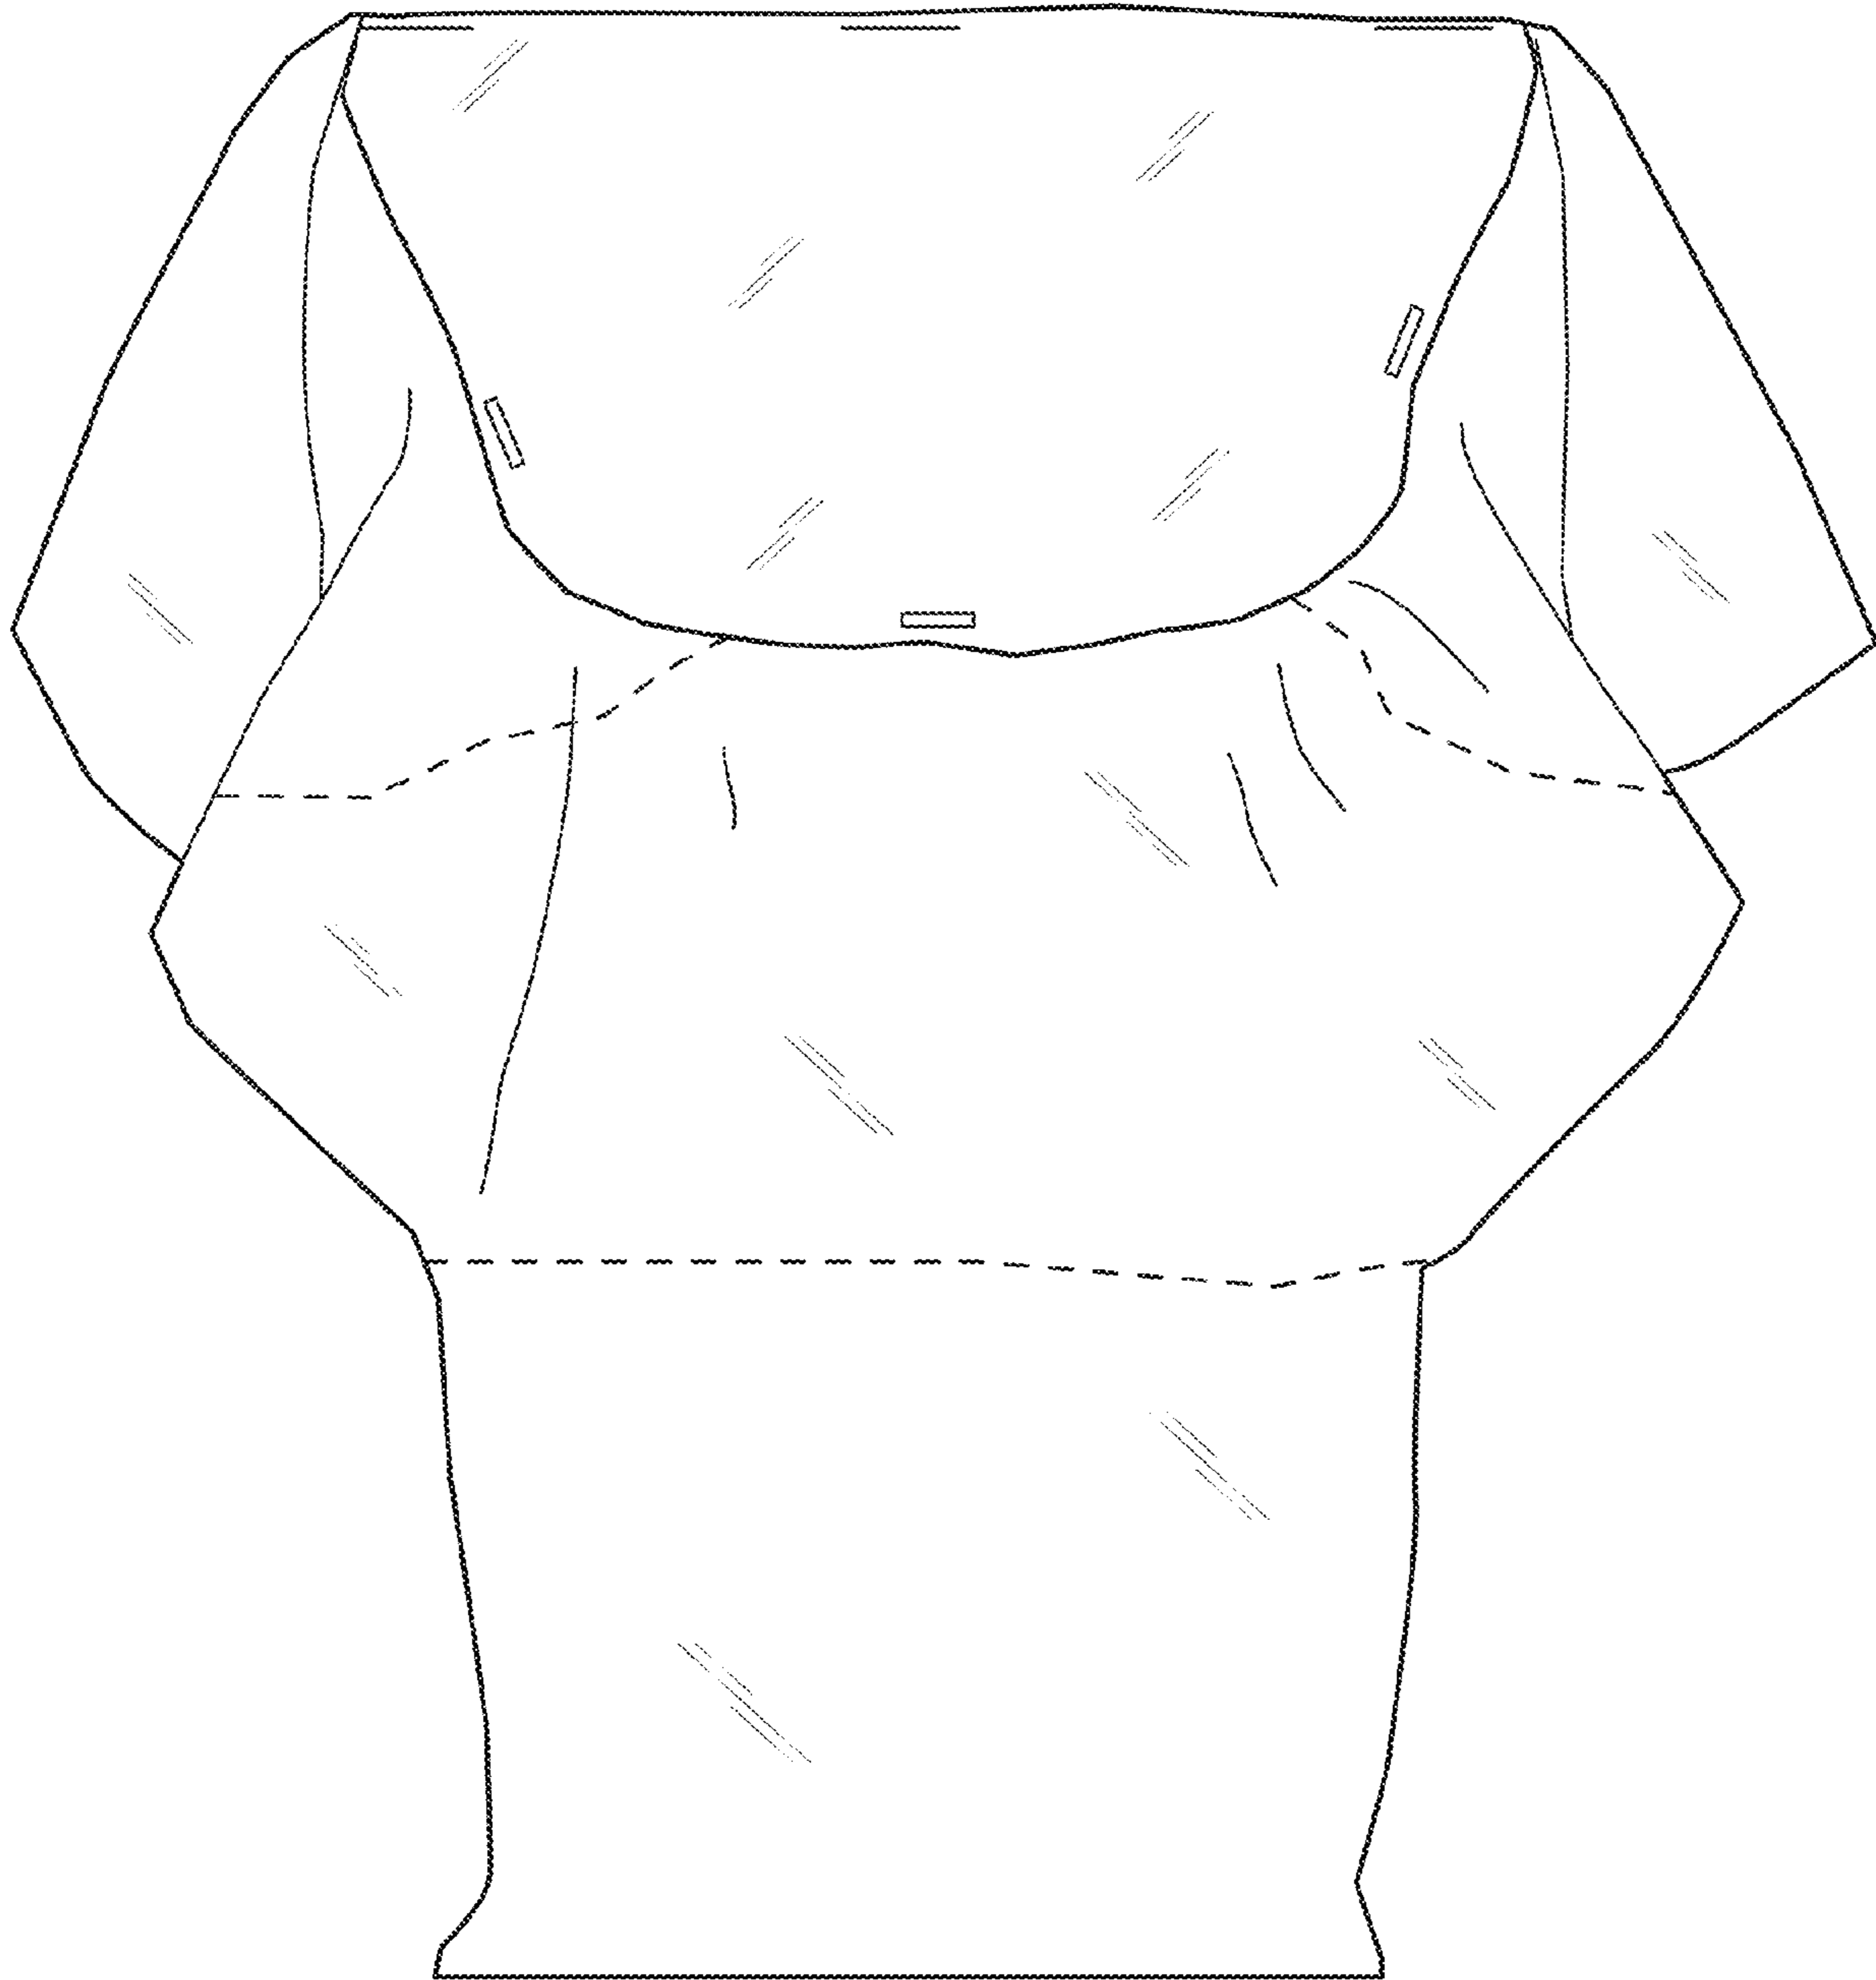


Fig. 4

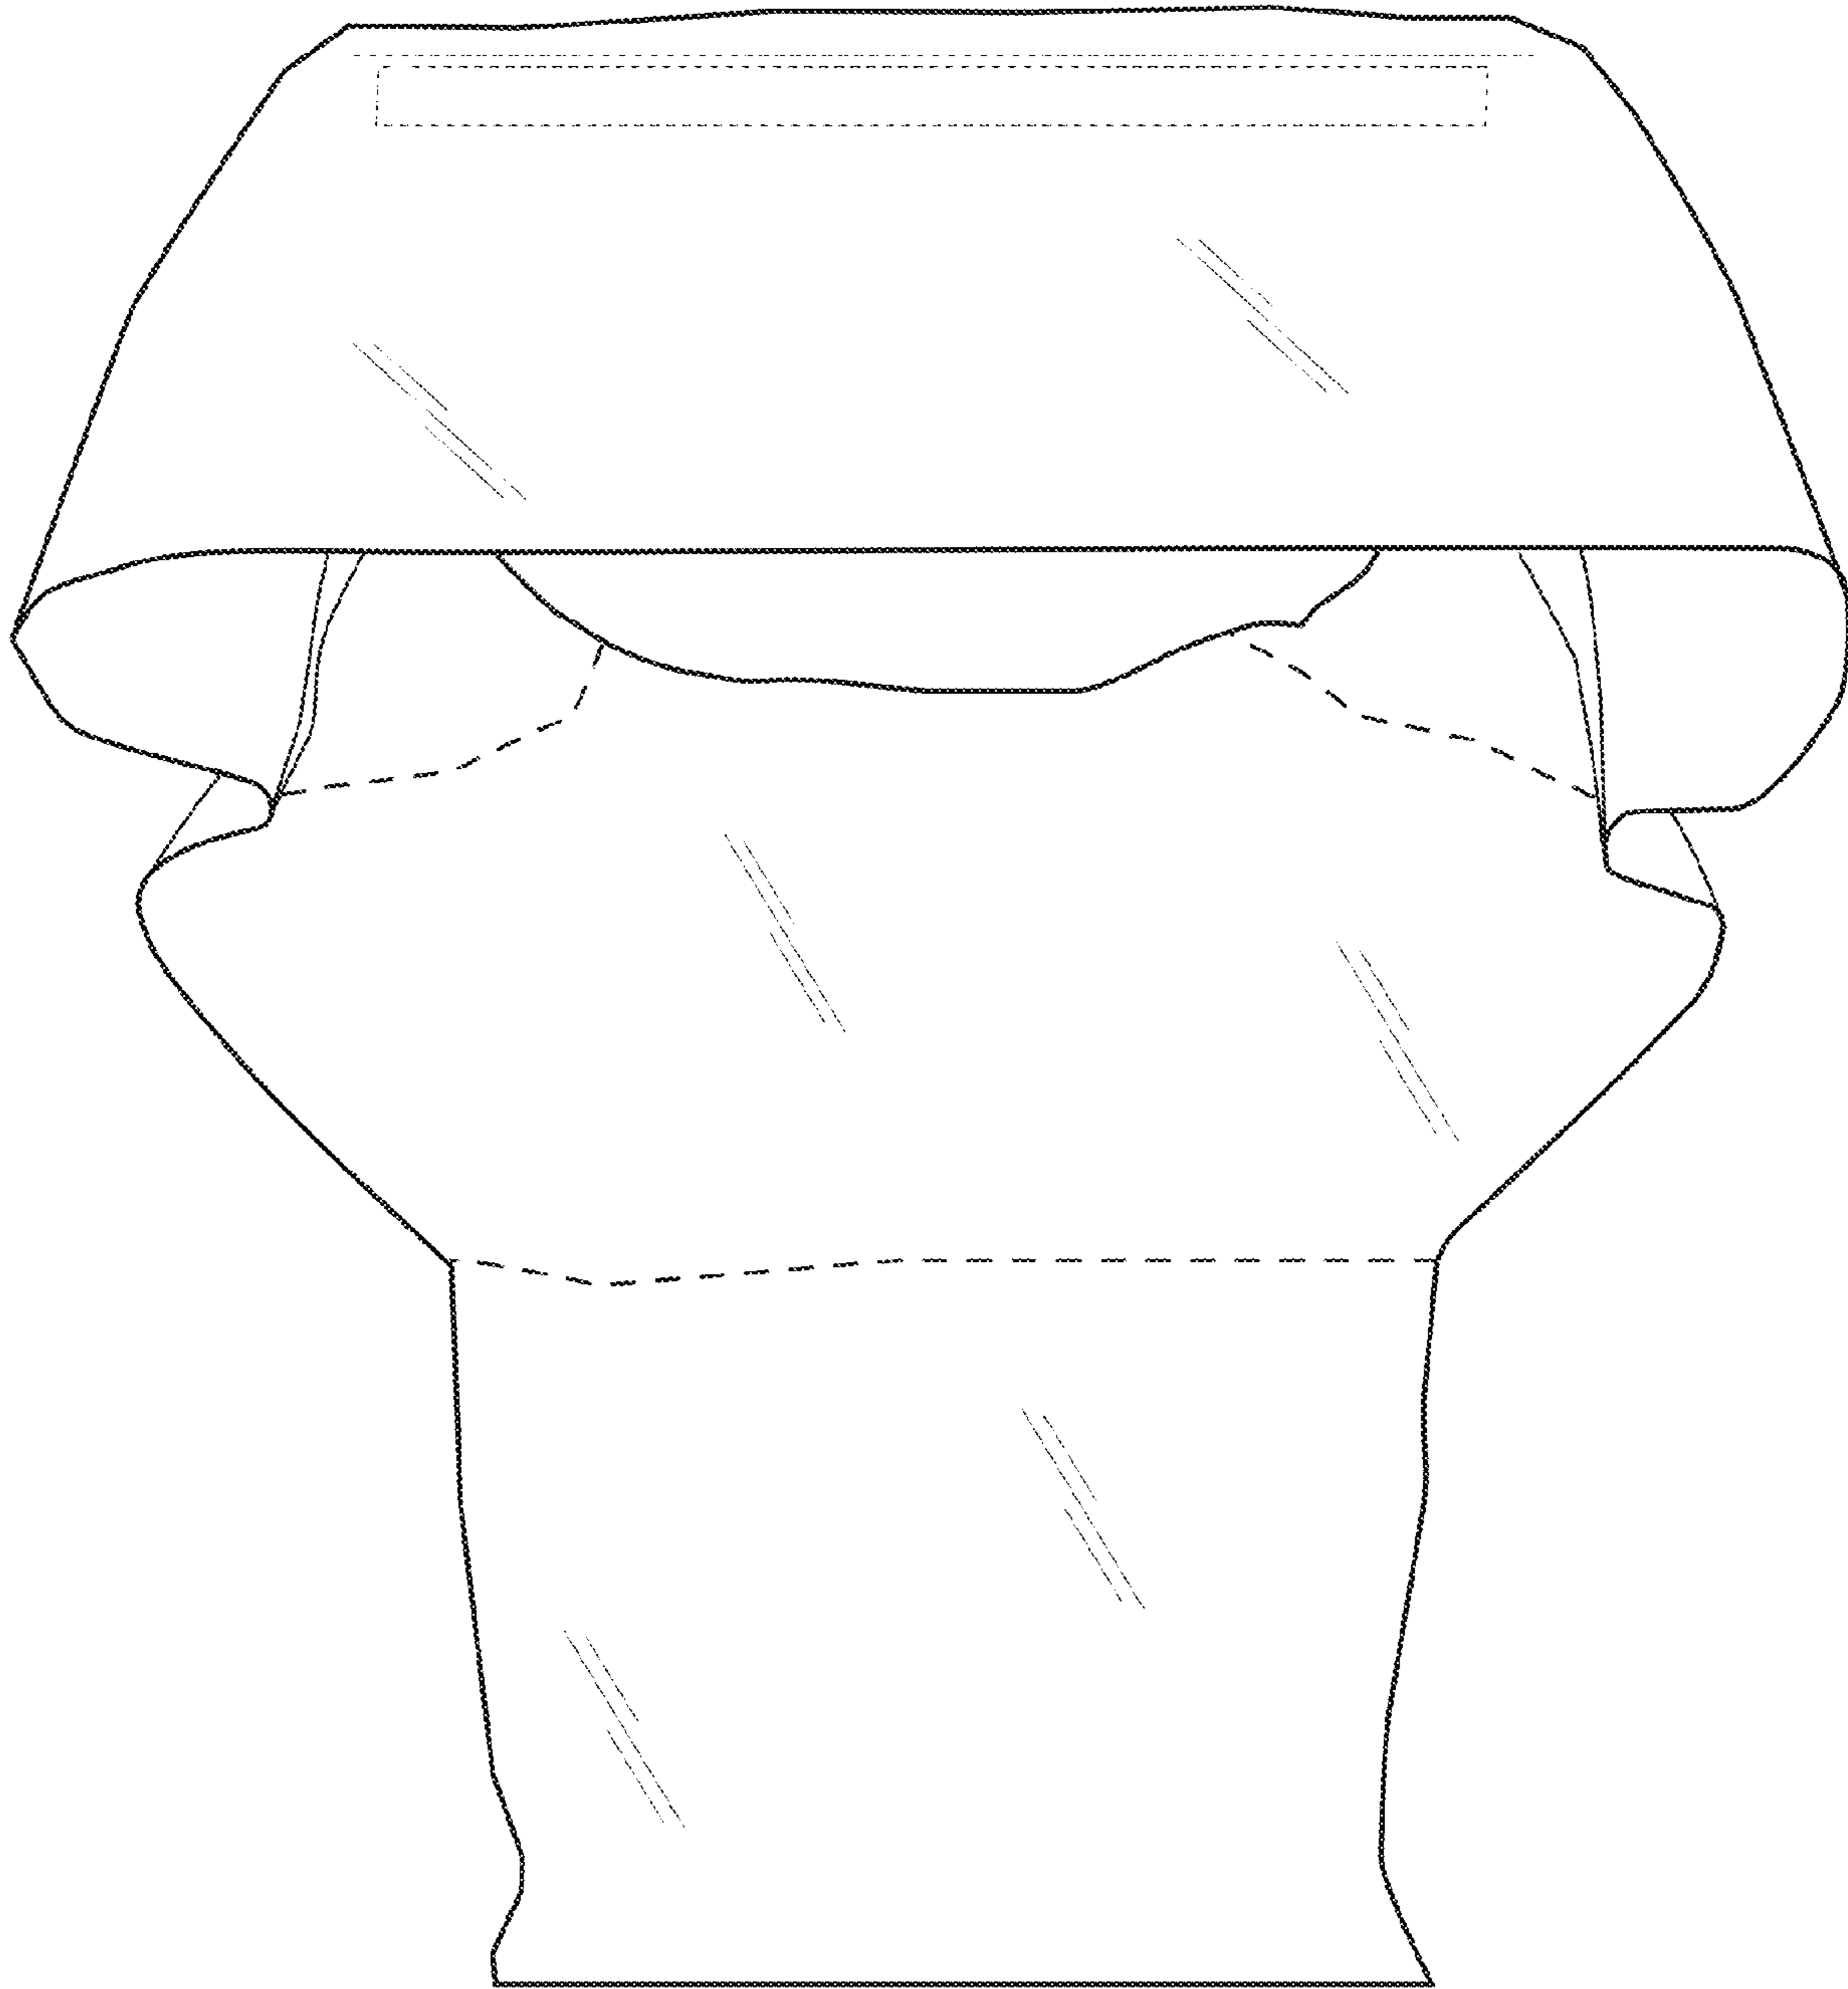


Fig. 5

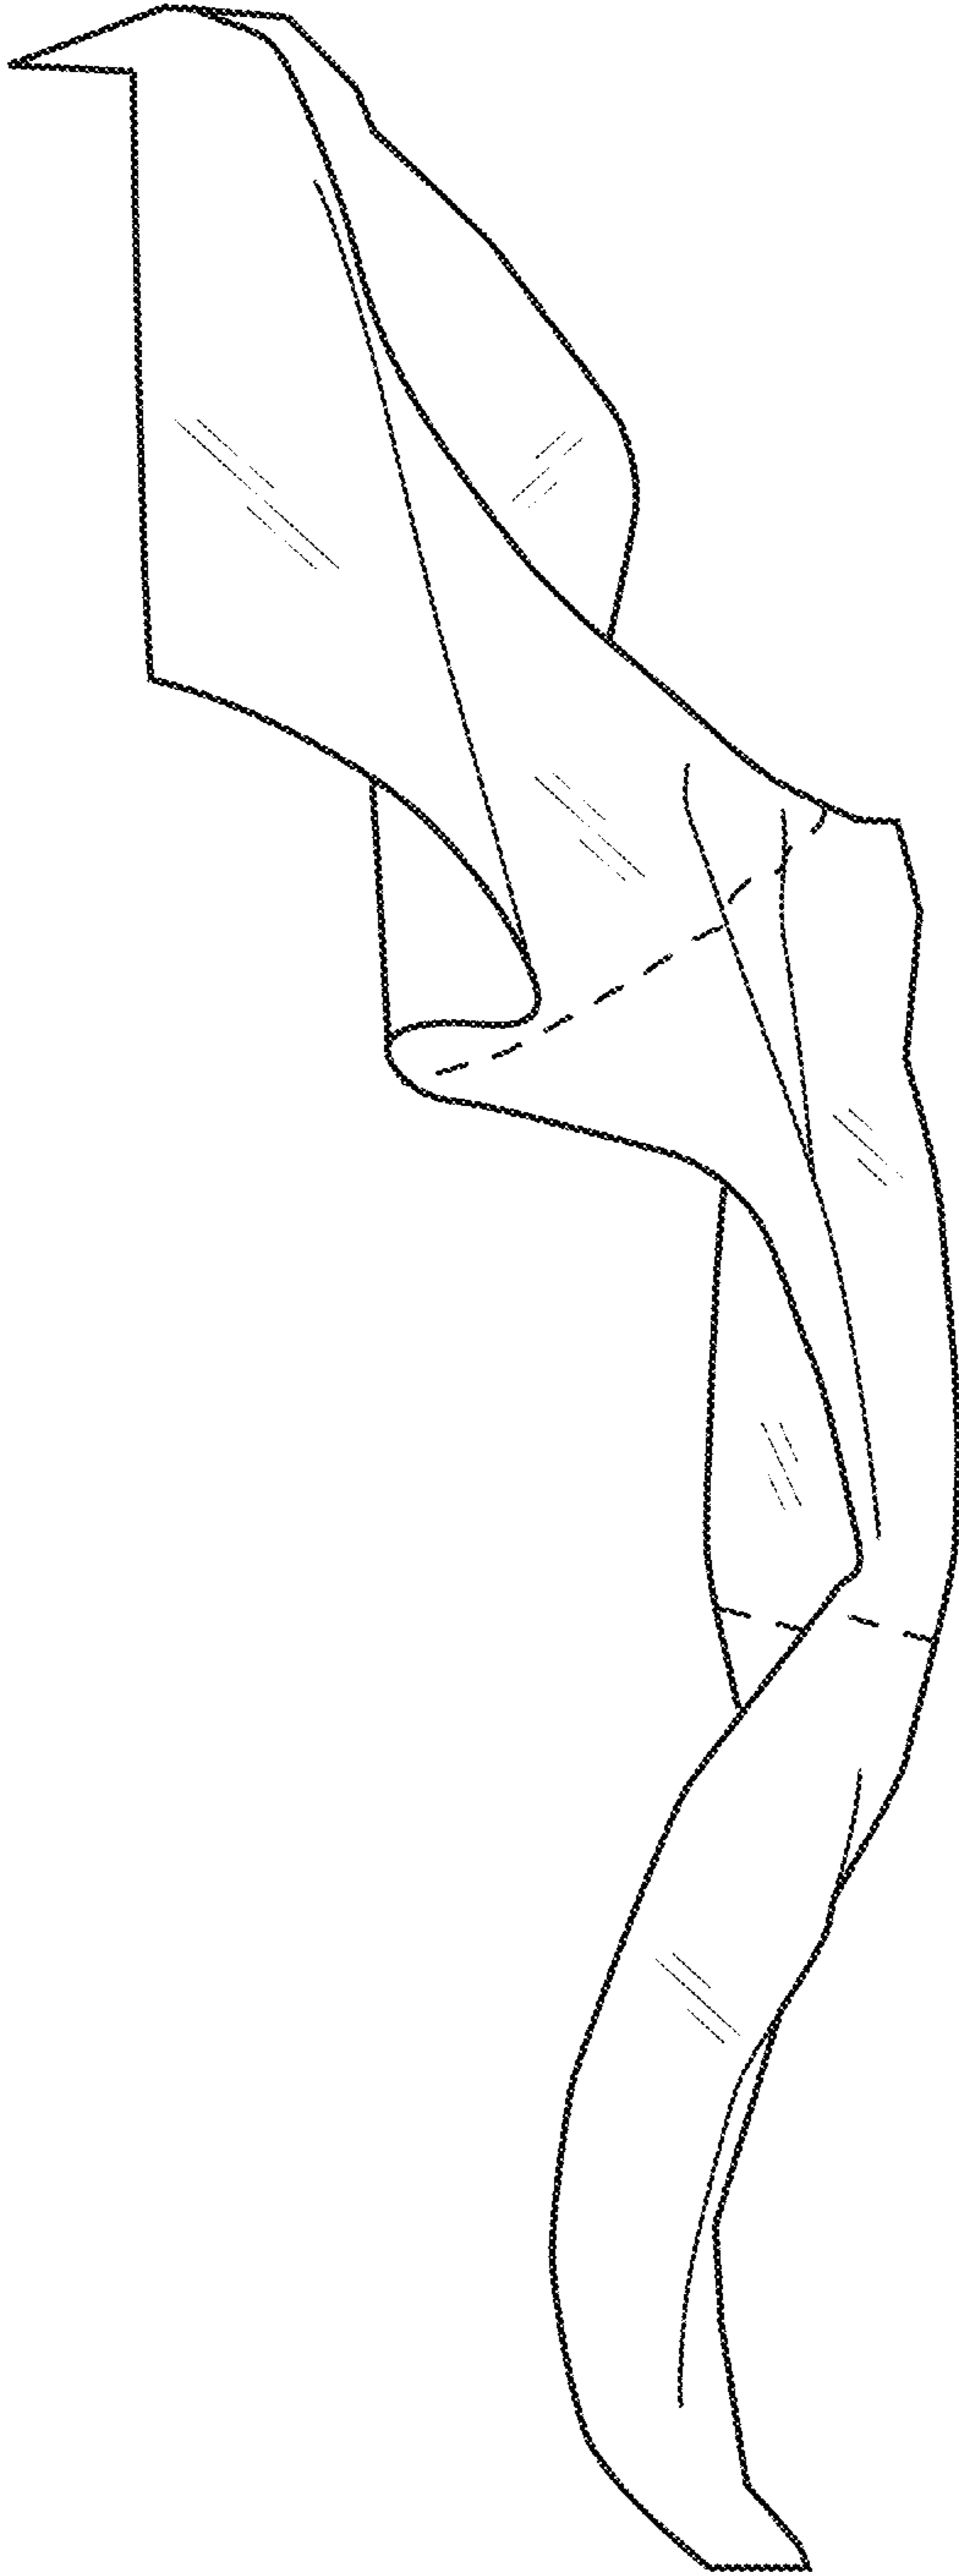


Fig. 6



Fig. 7

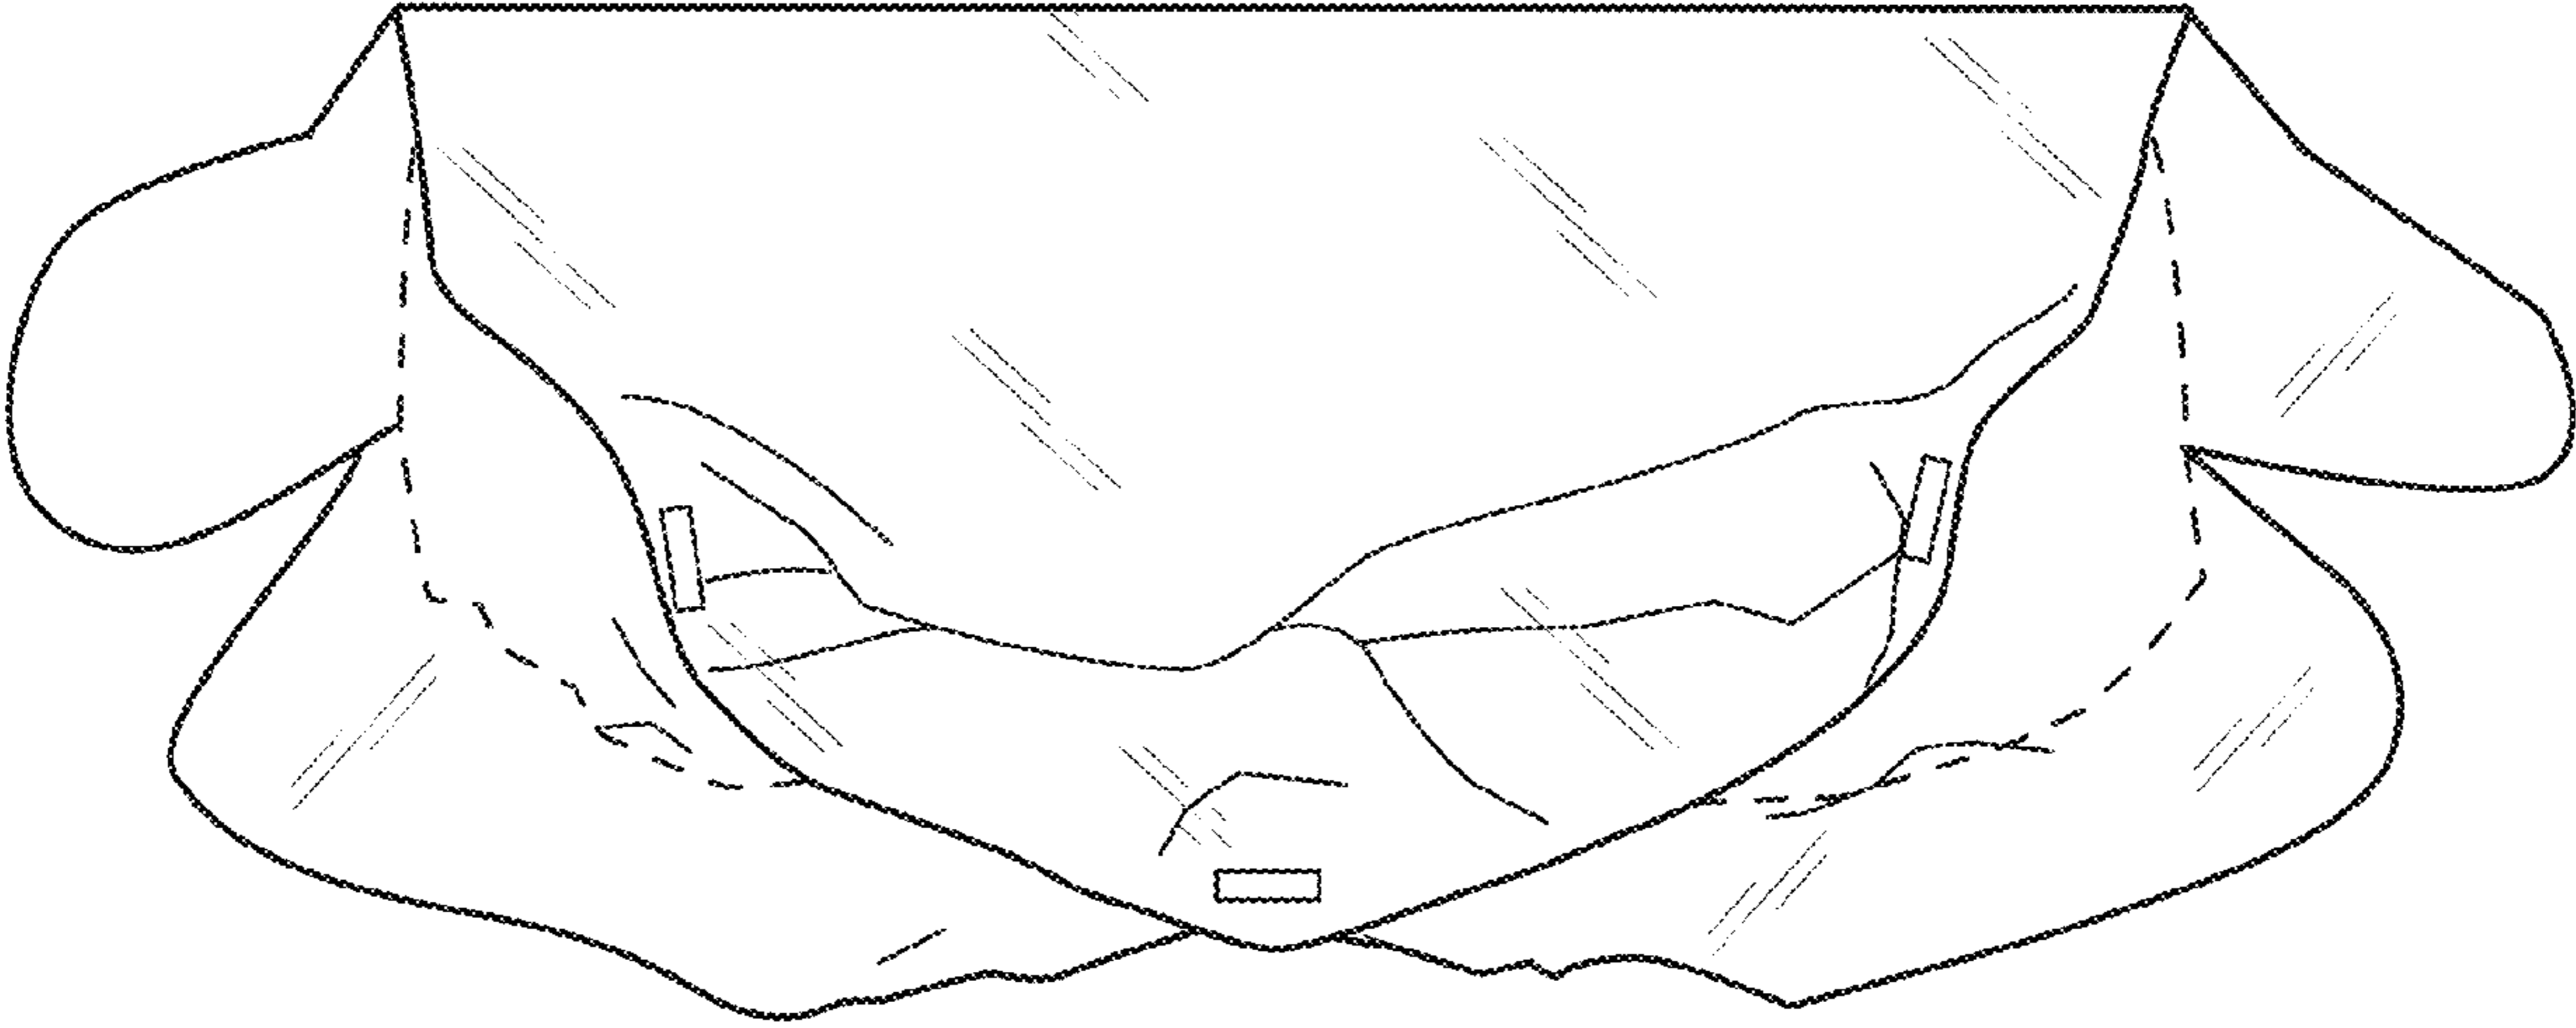


Fig. 8

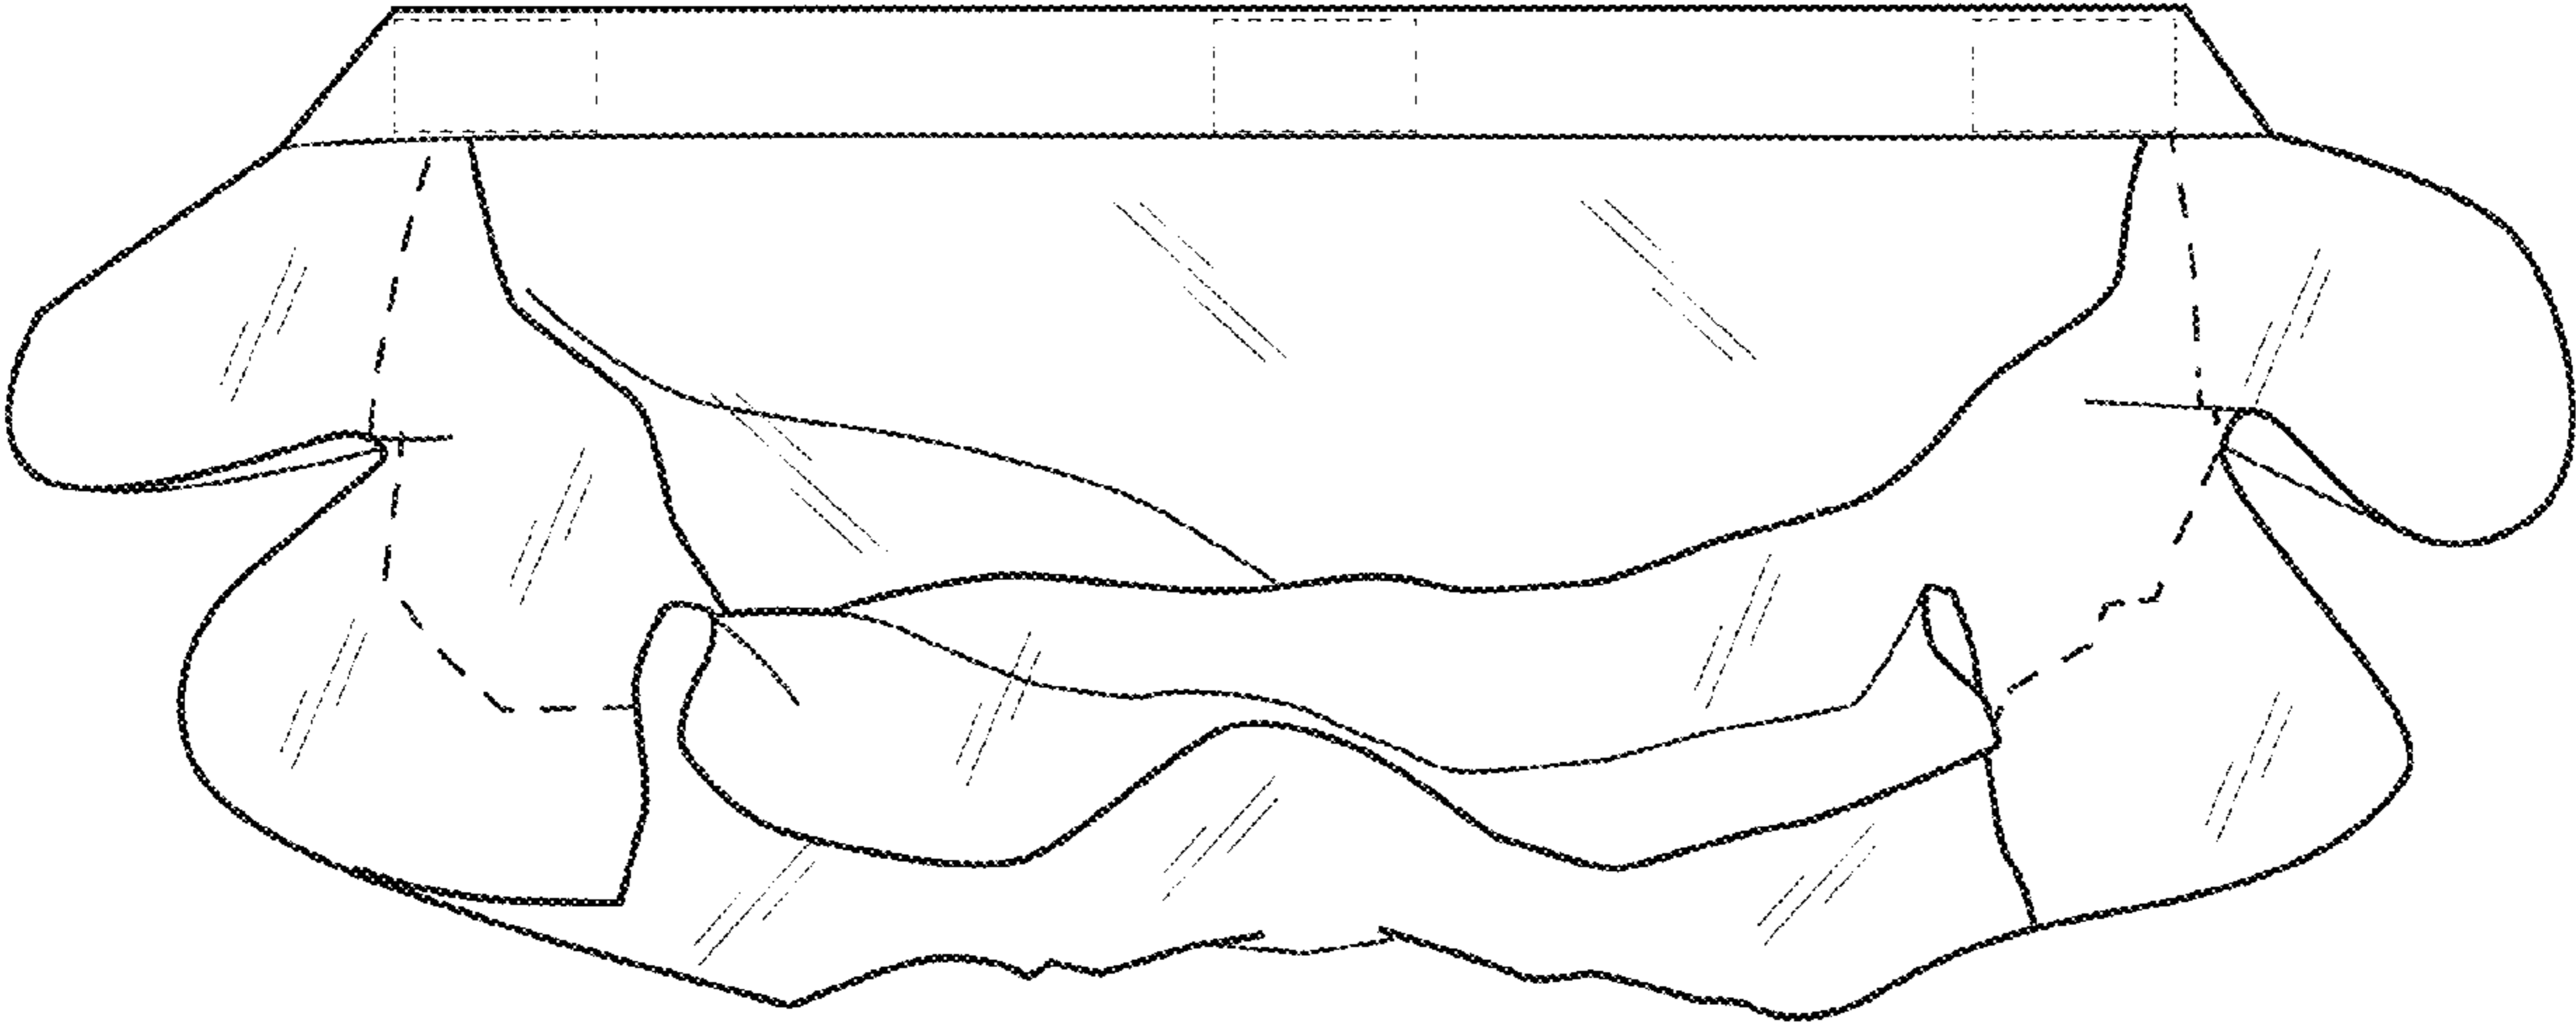


Fig. 9

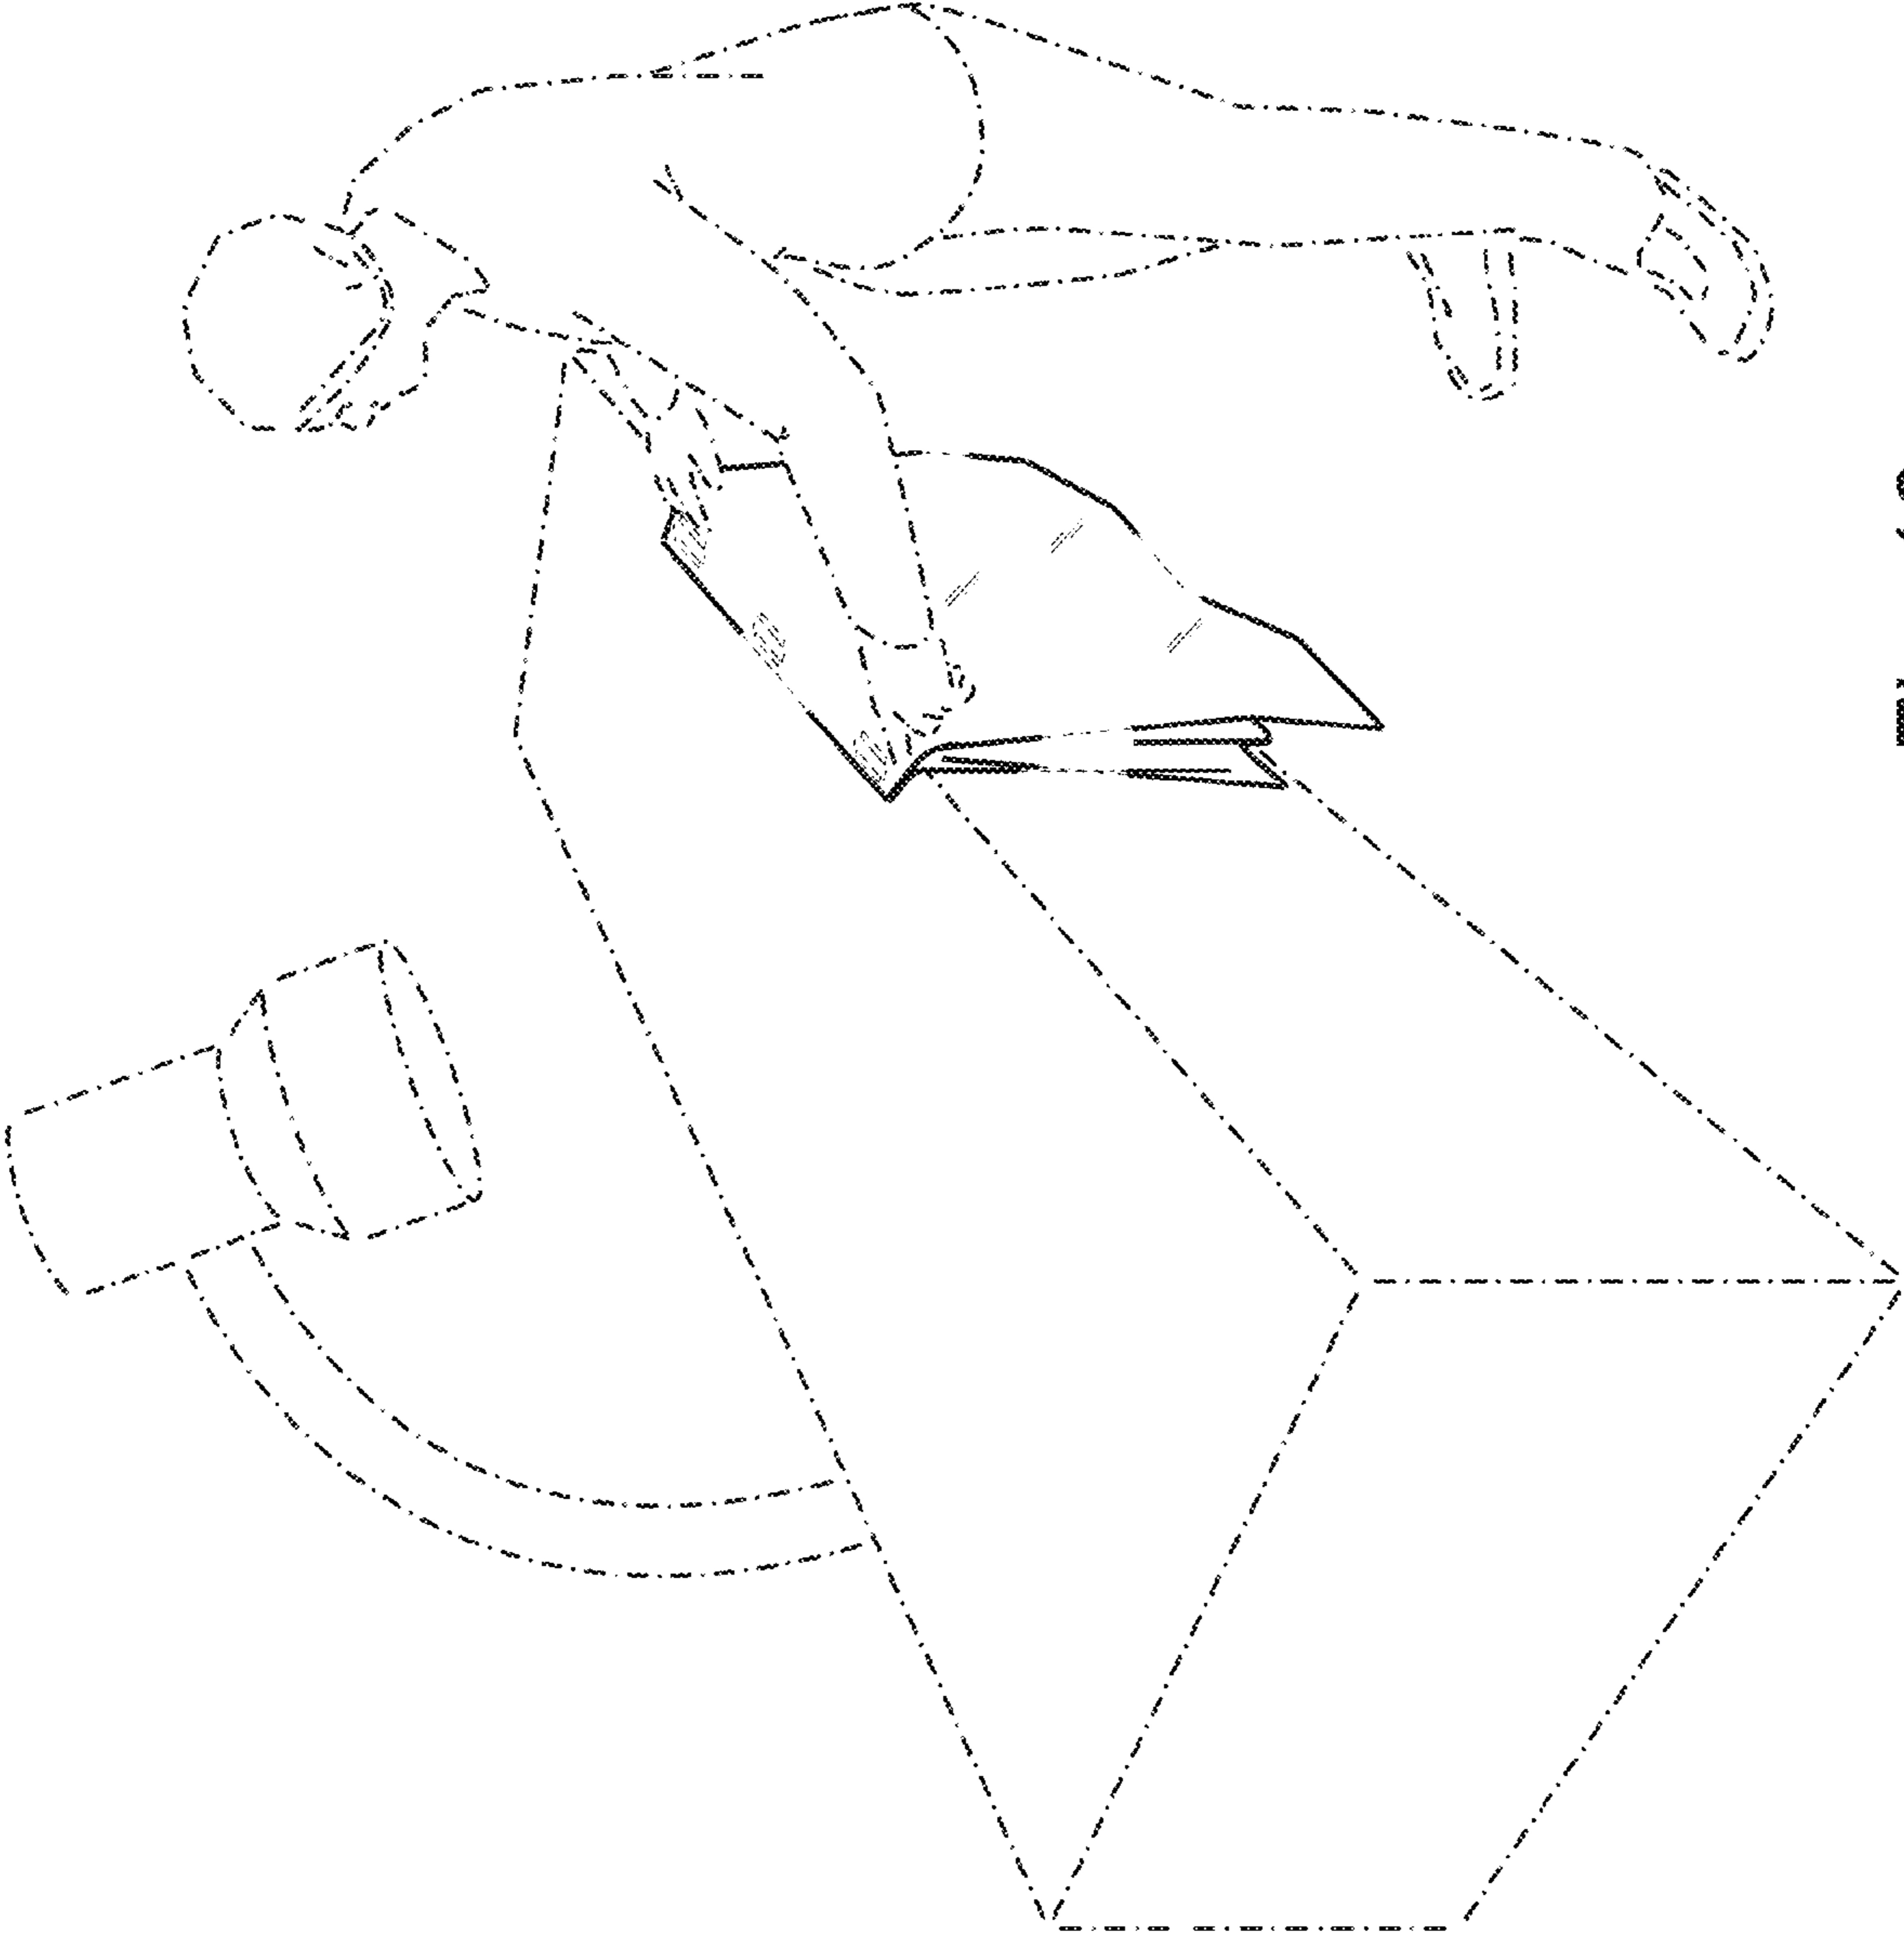


Fig. 10

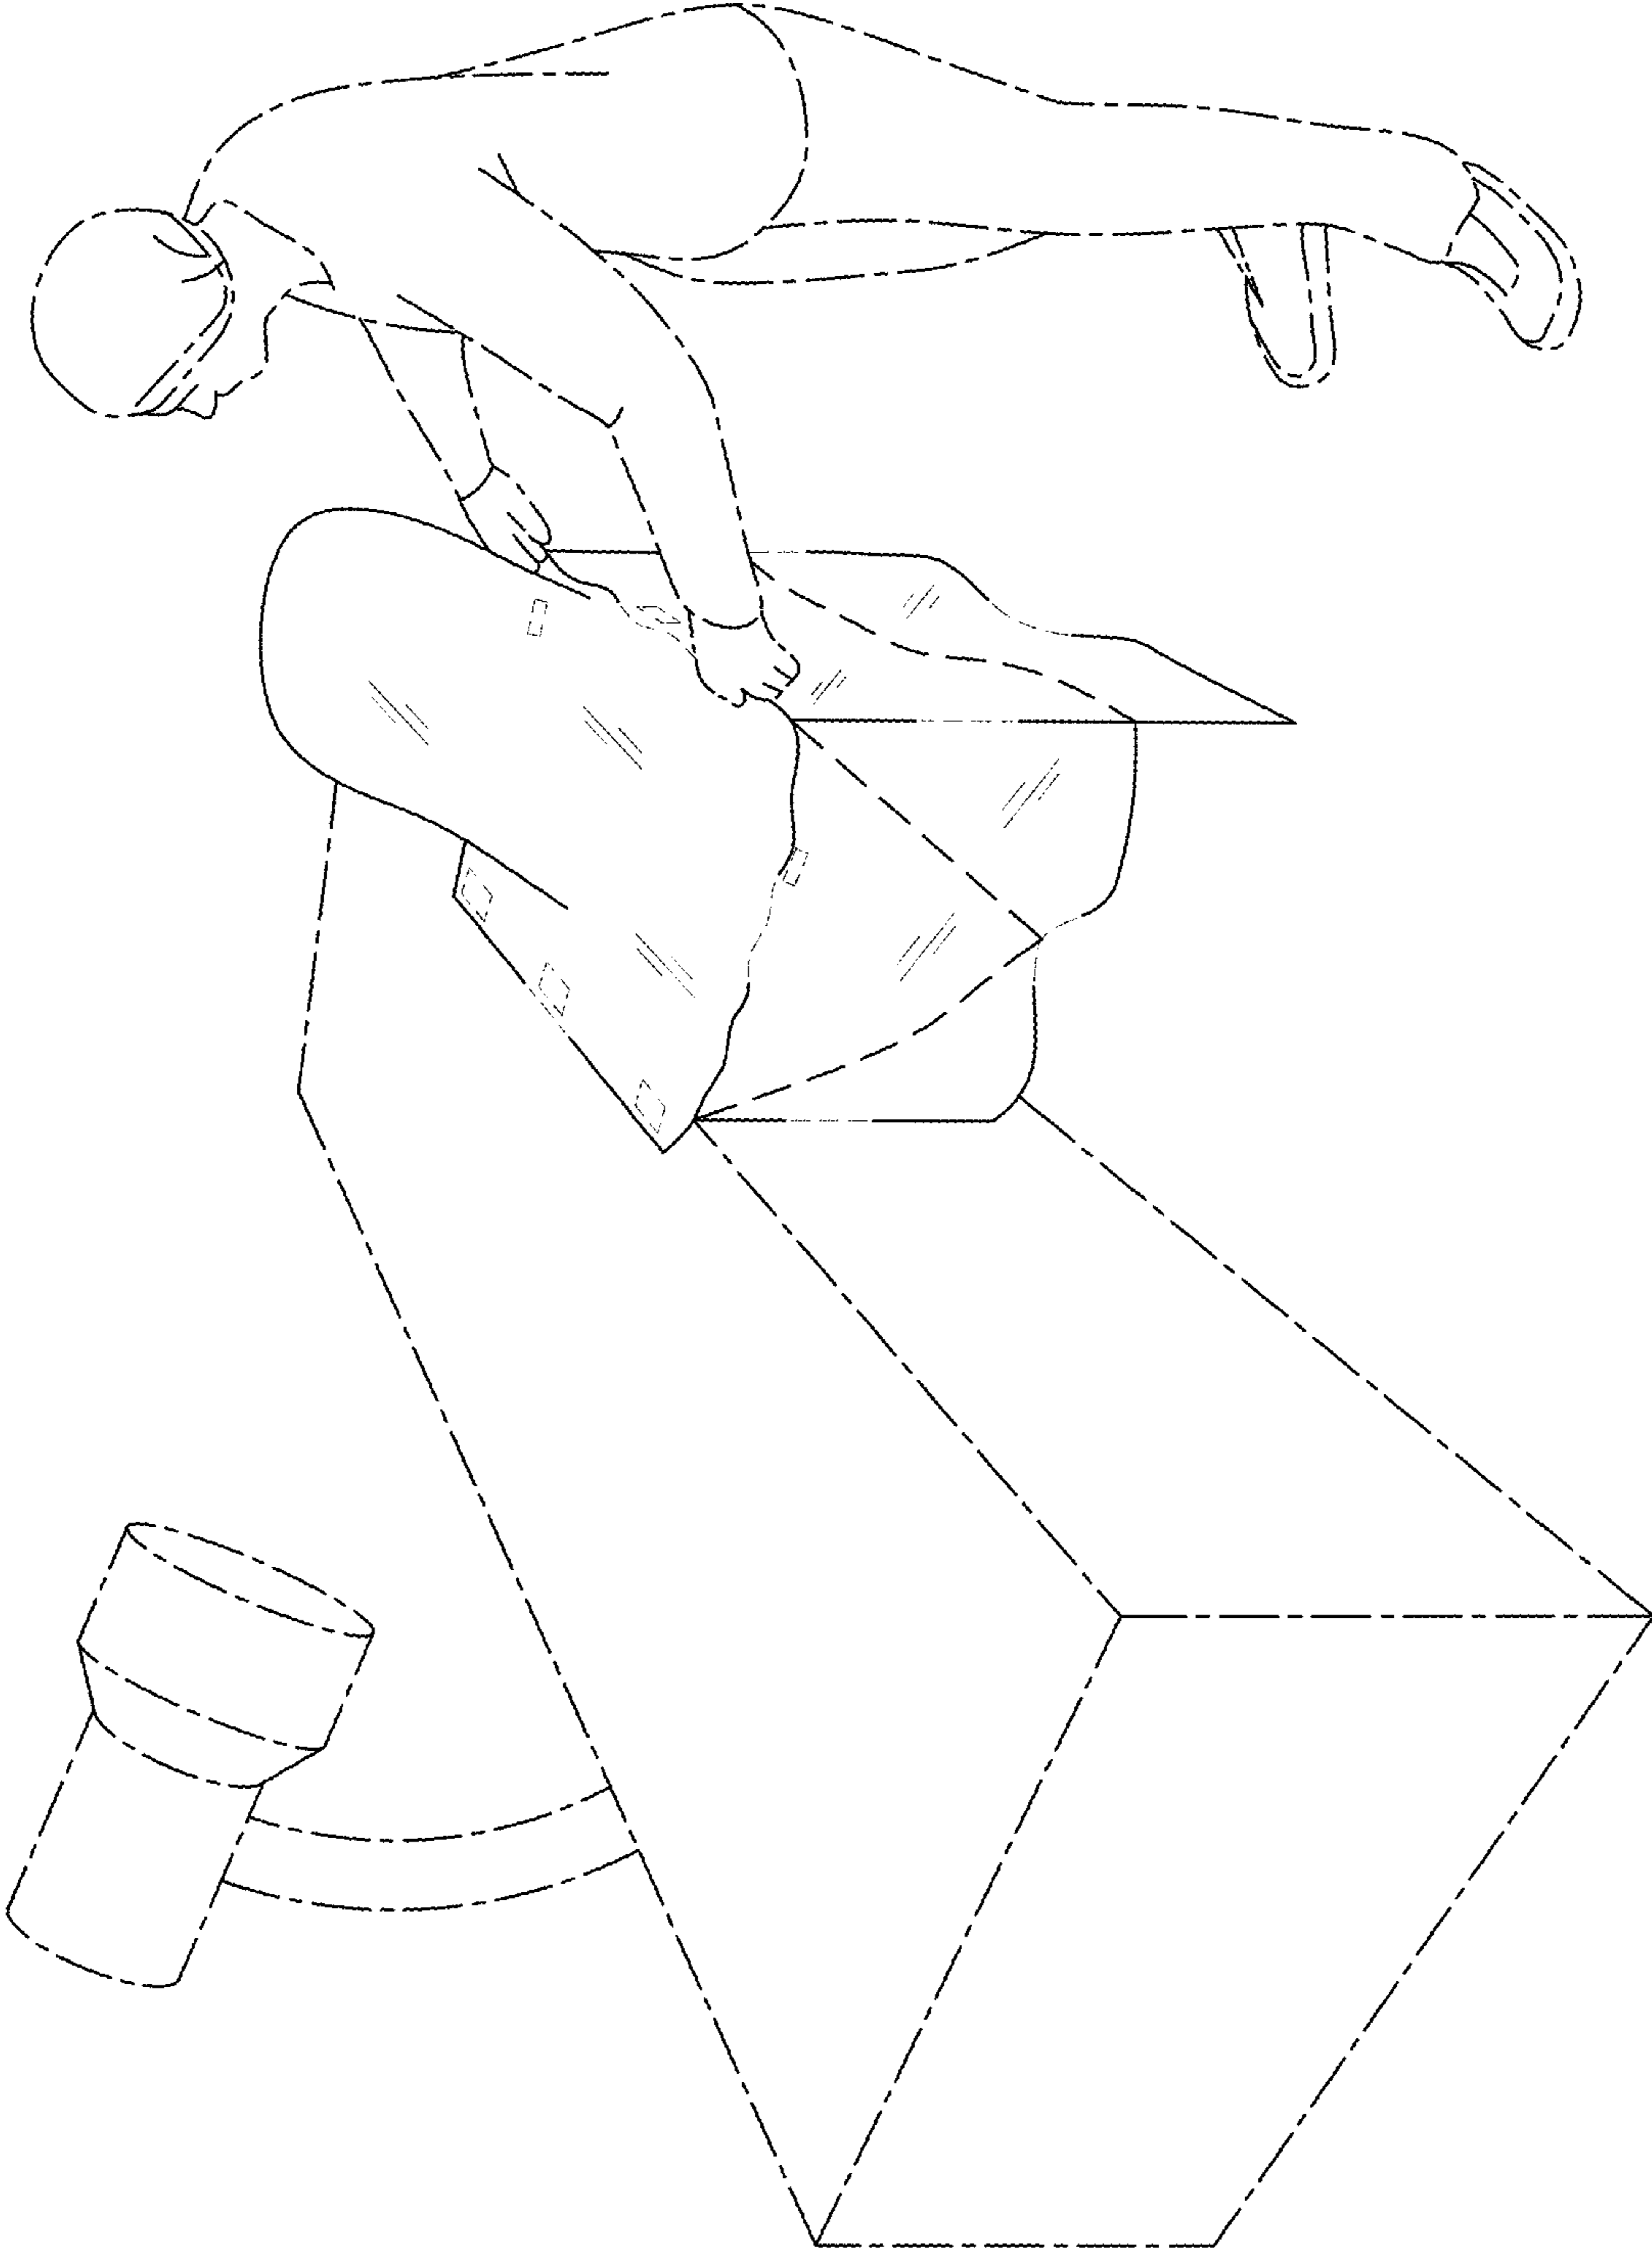


FIG. 11

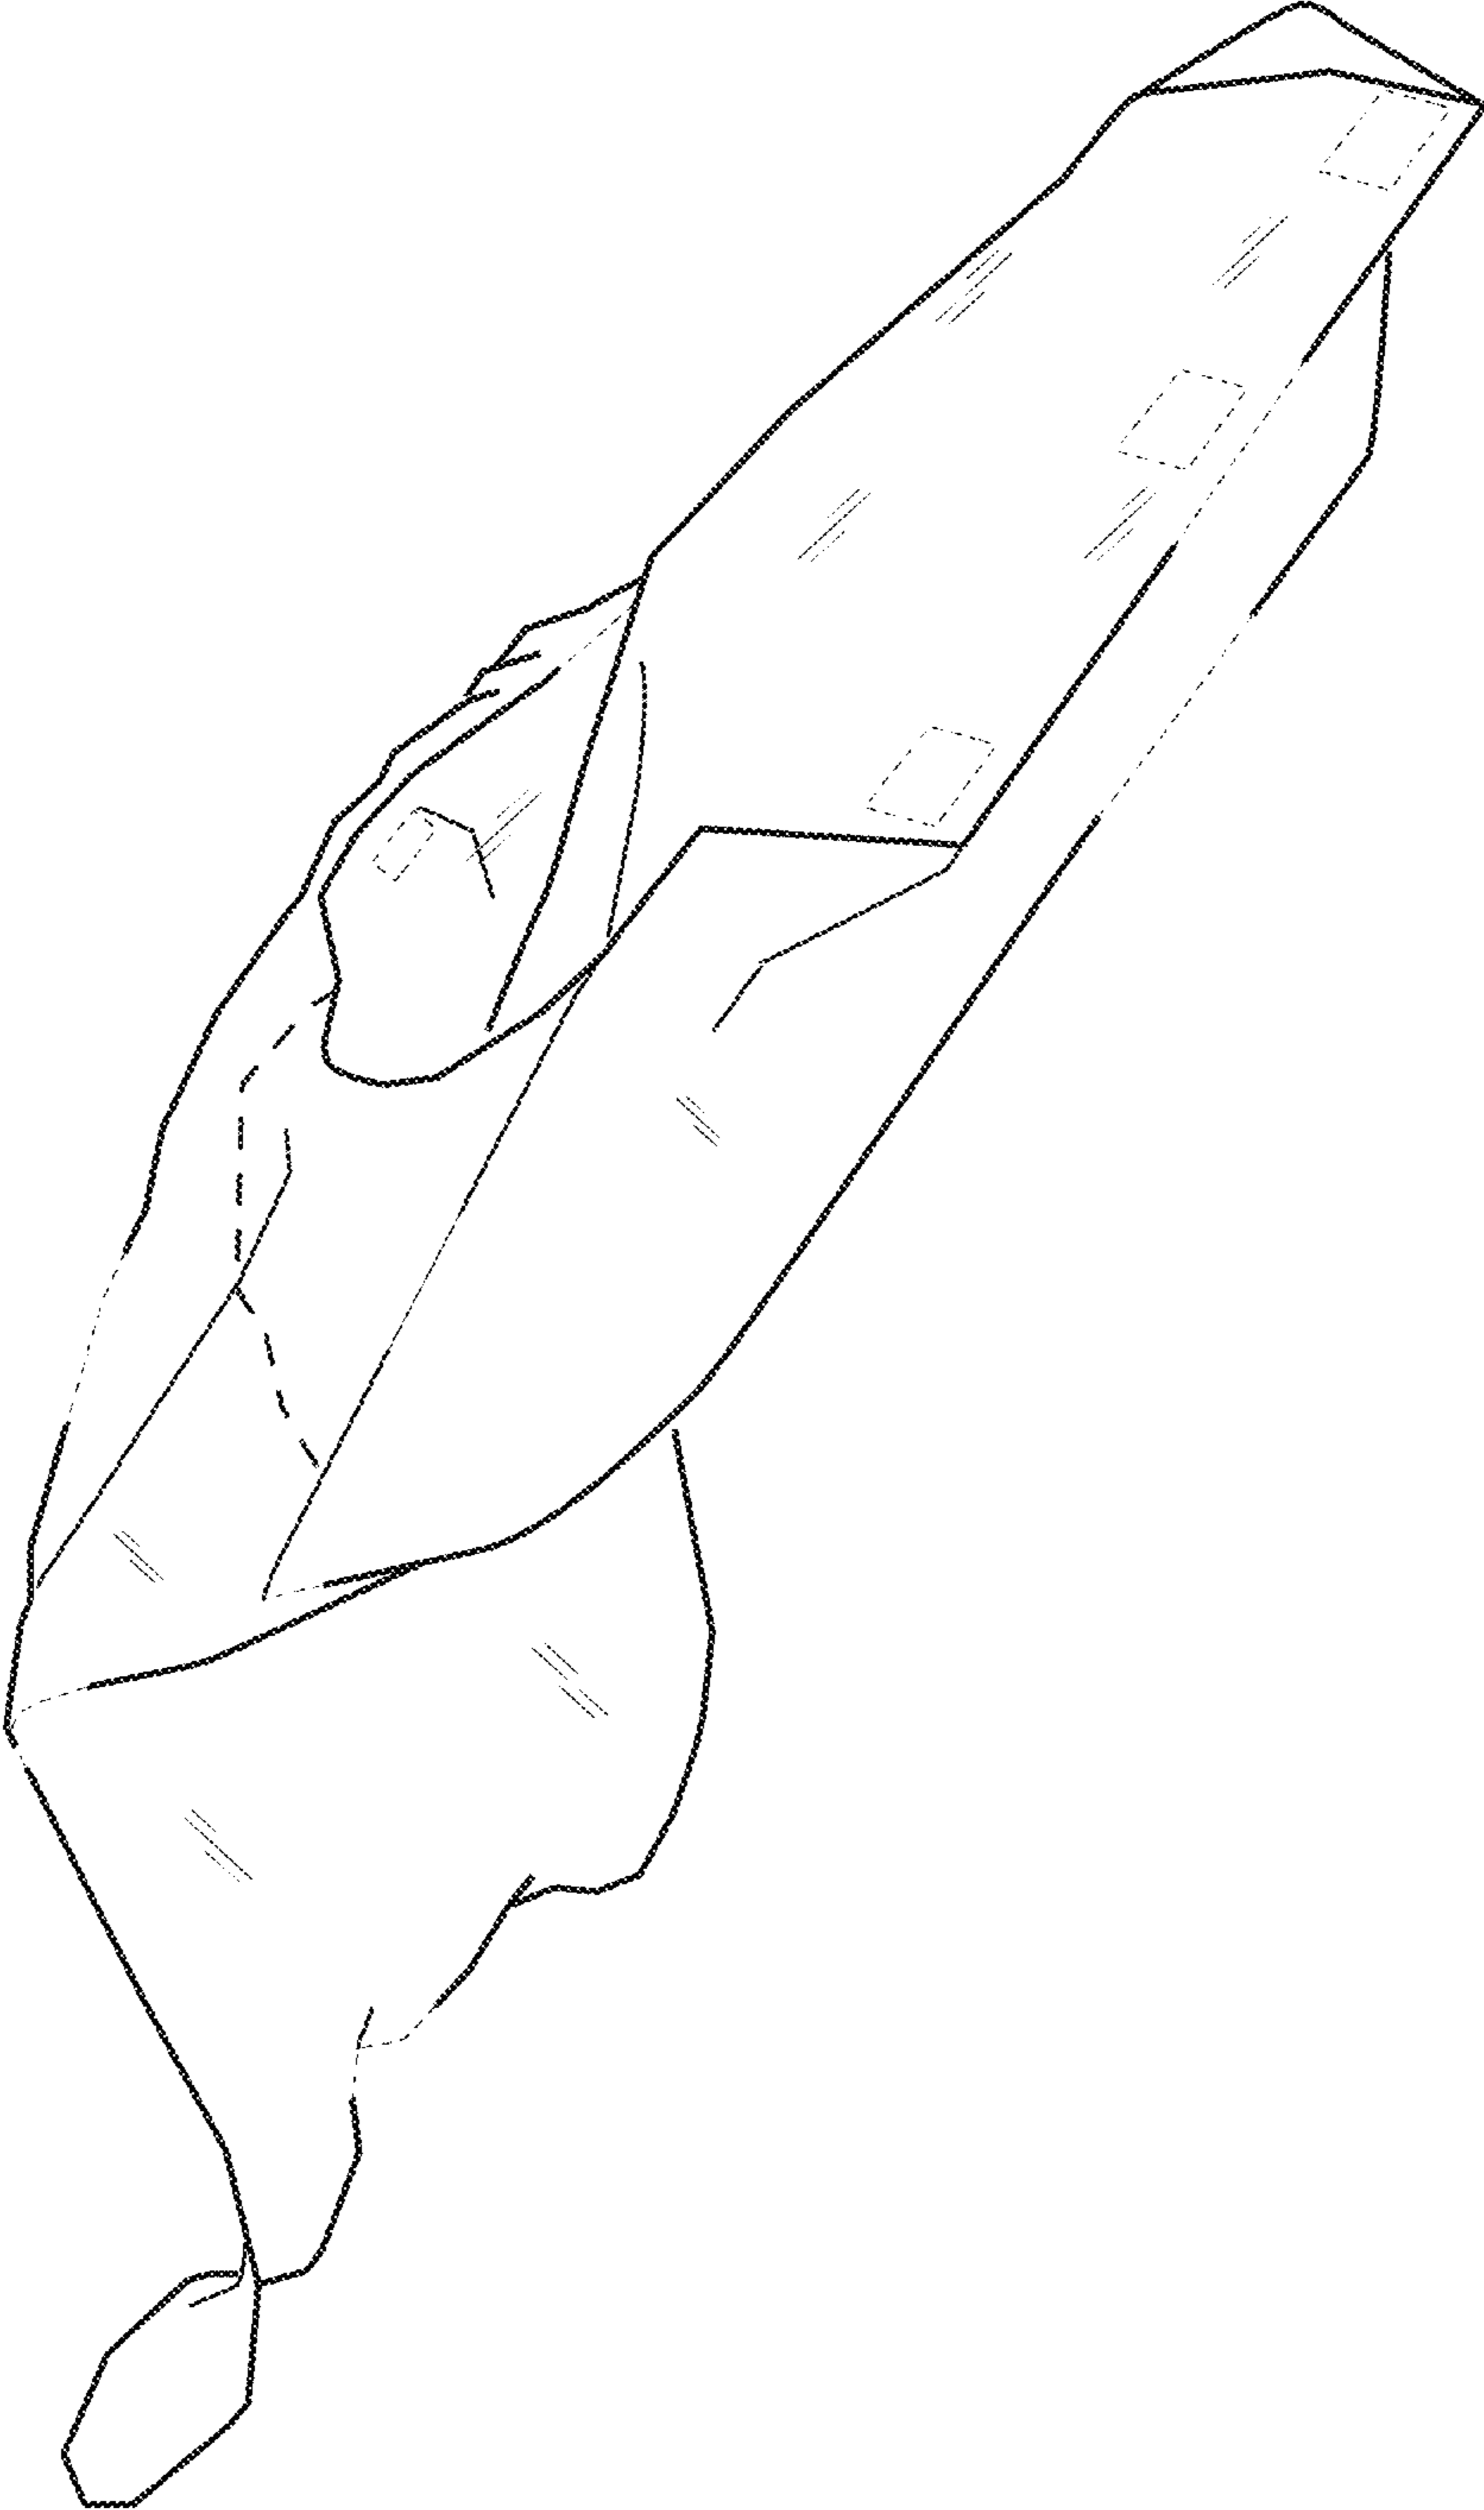


Fig. 12

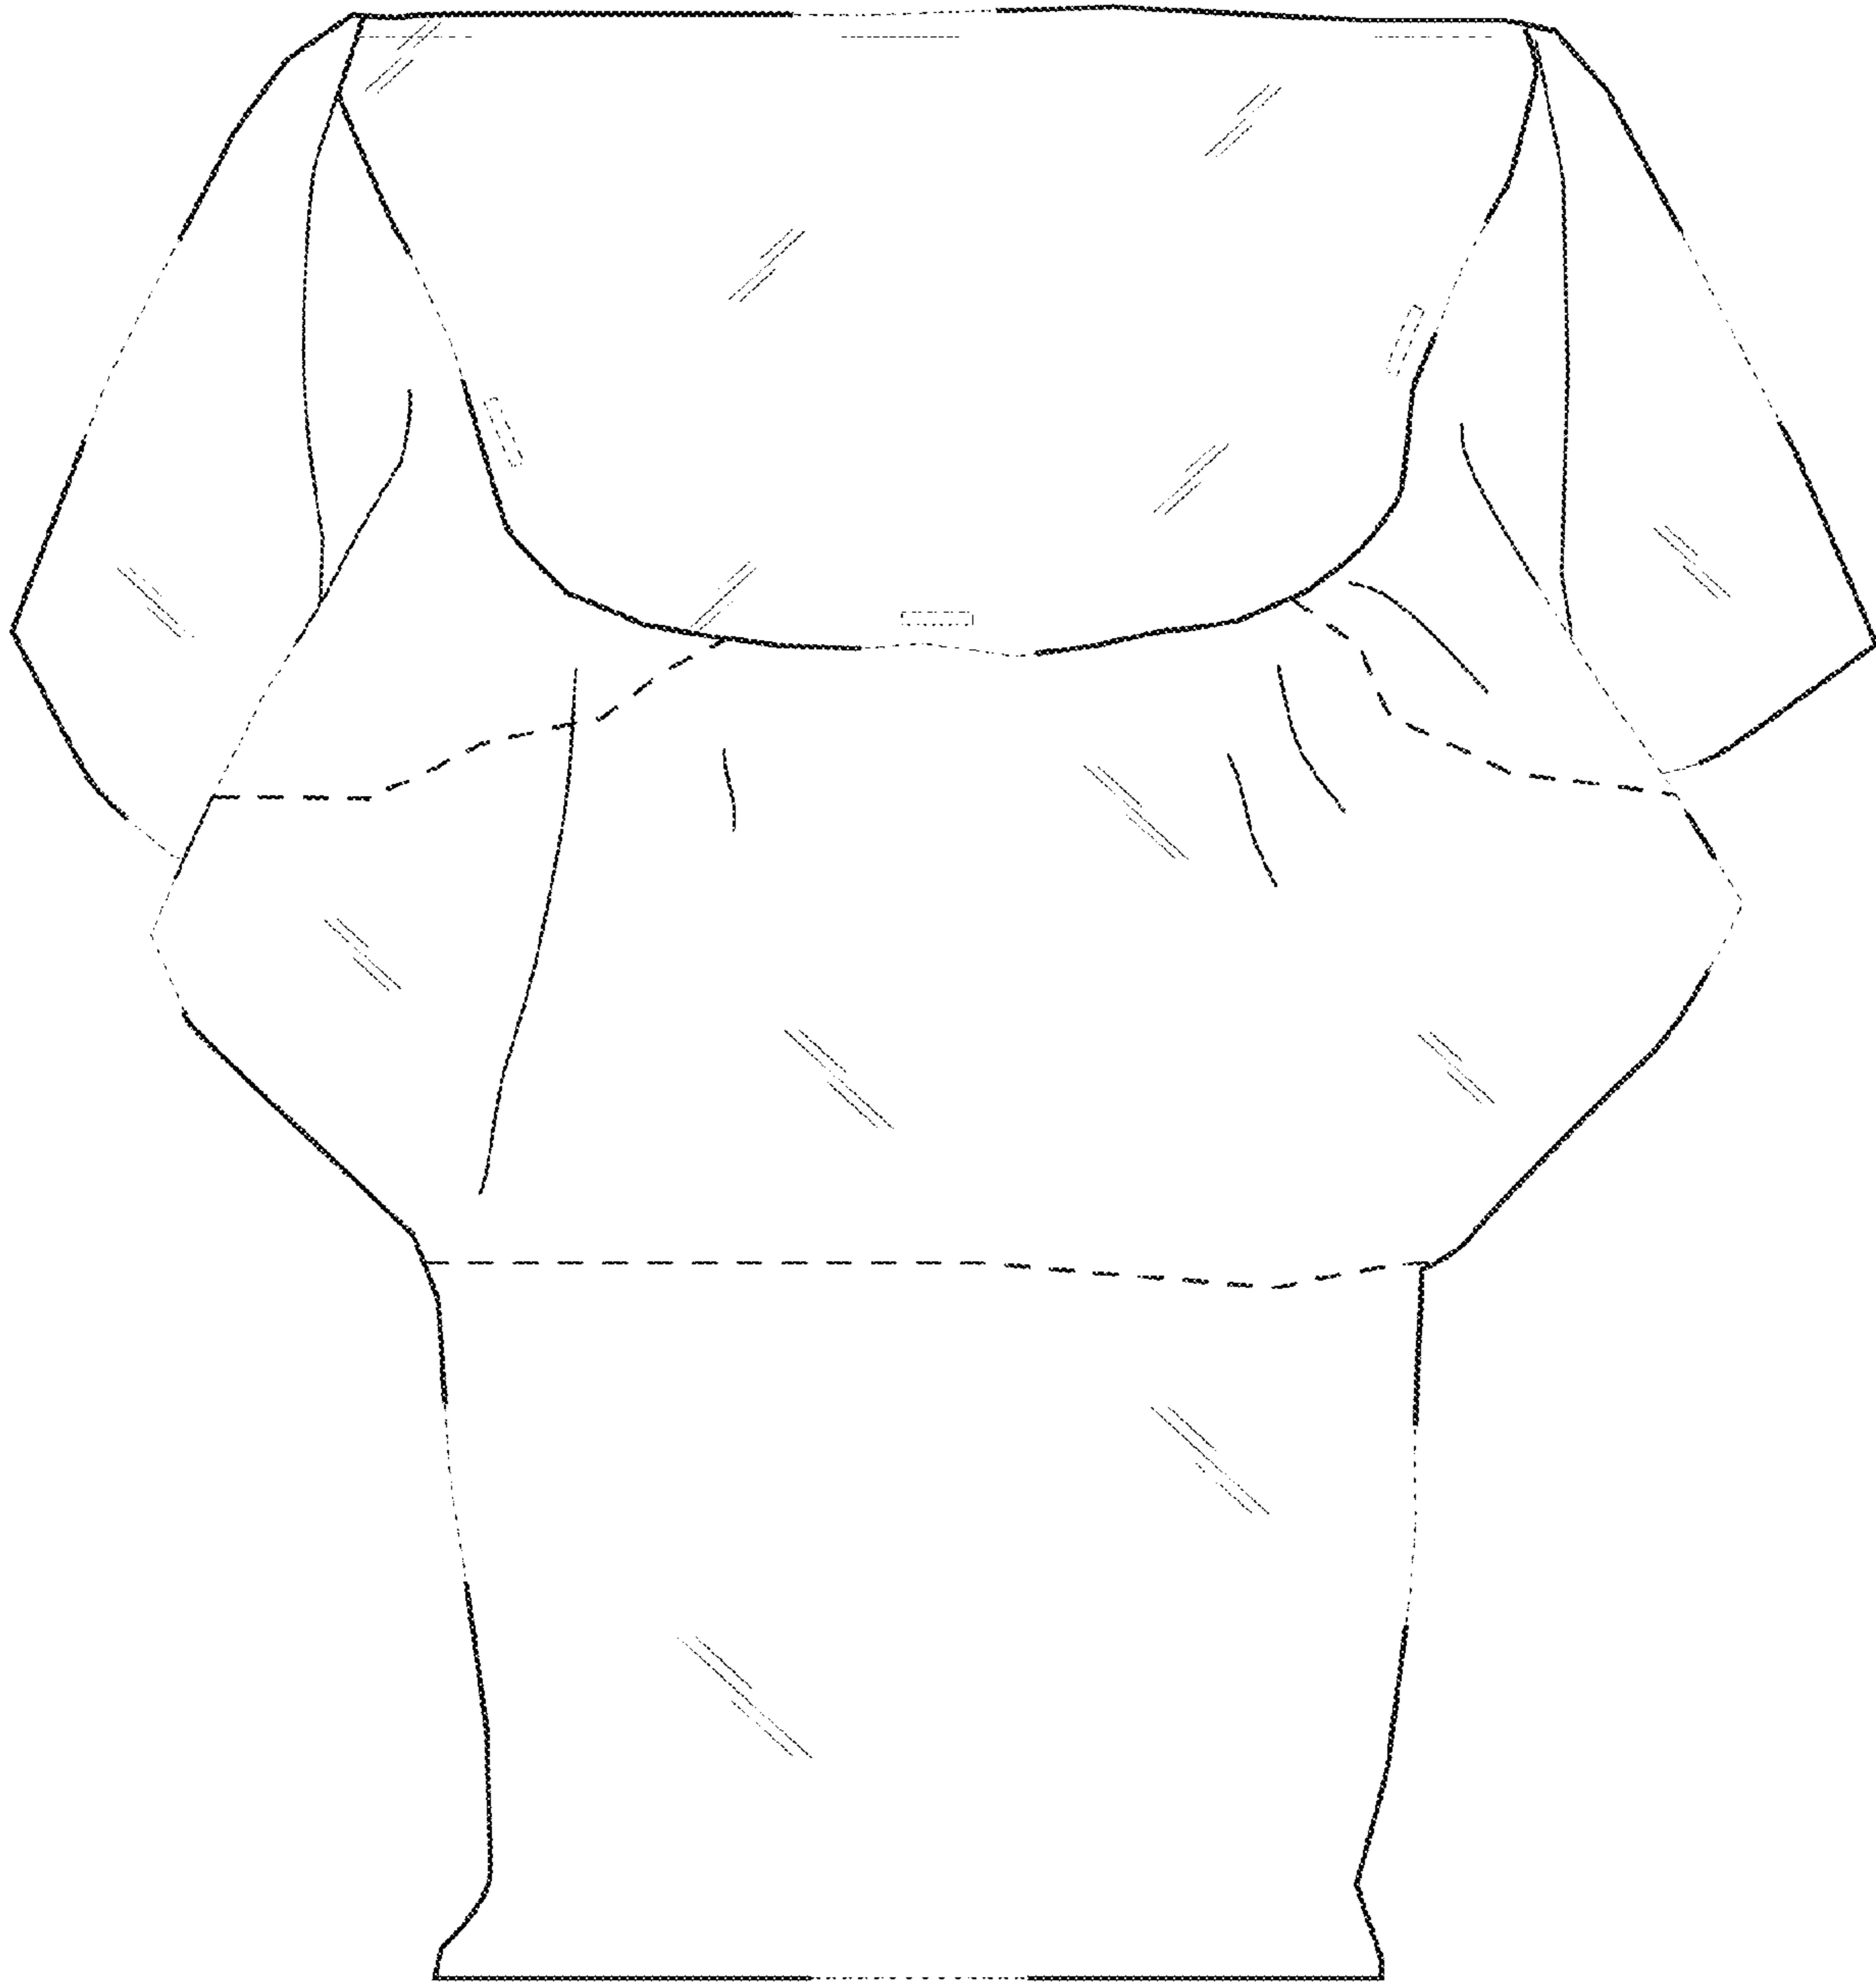


Fig. 13

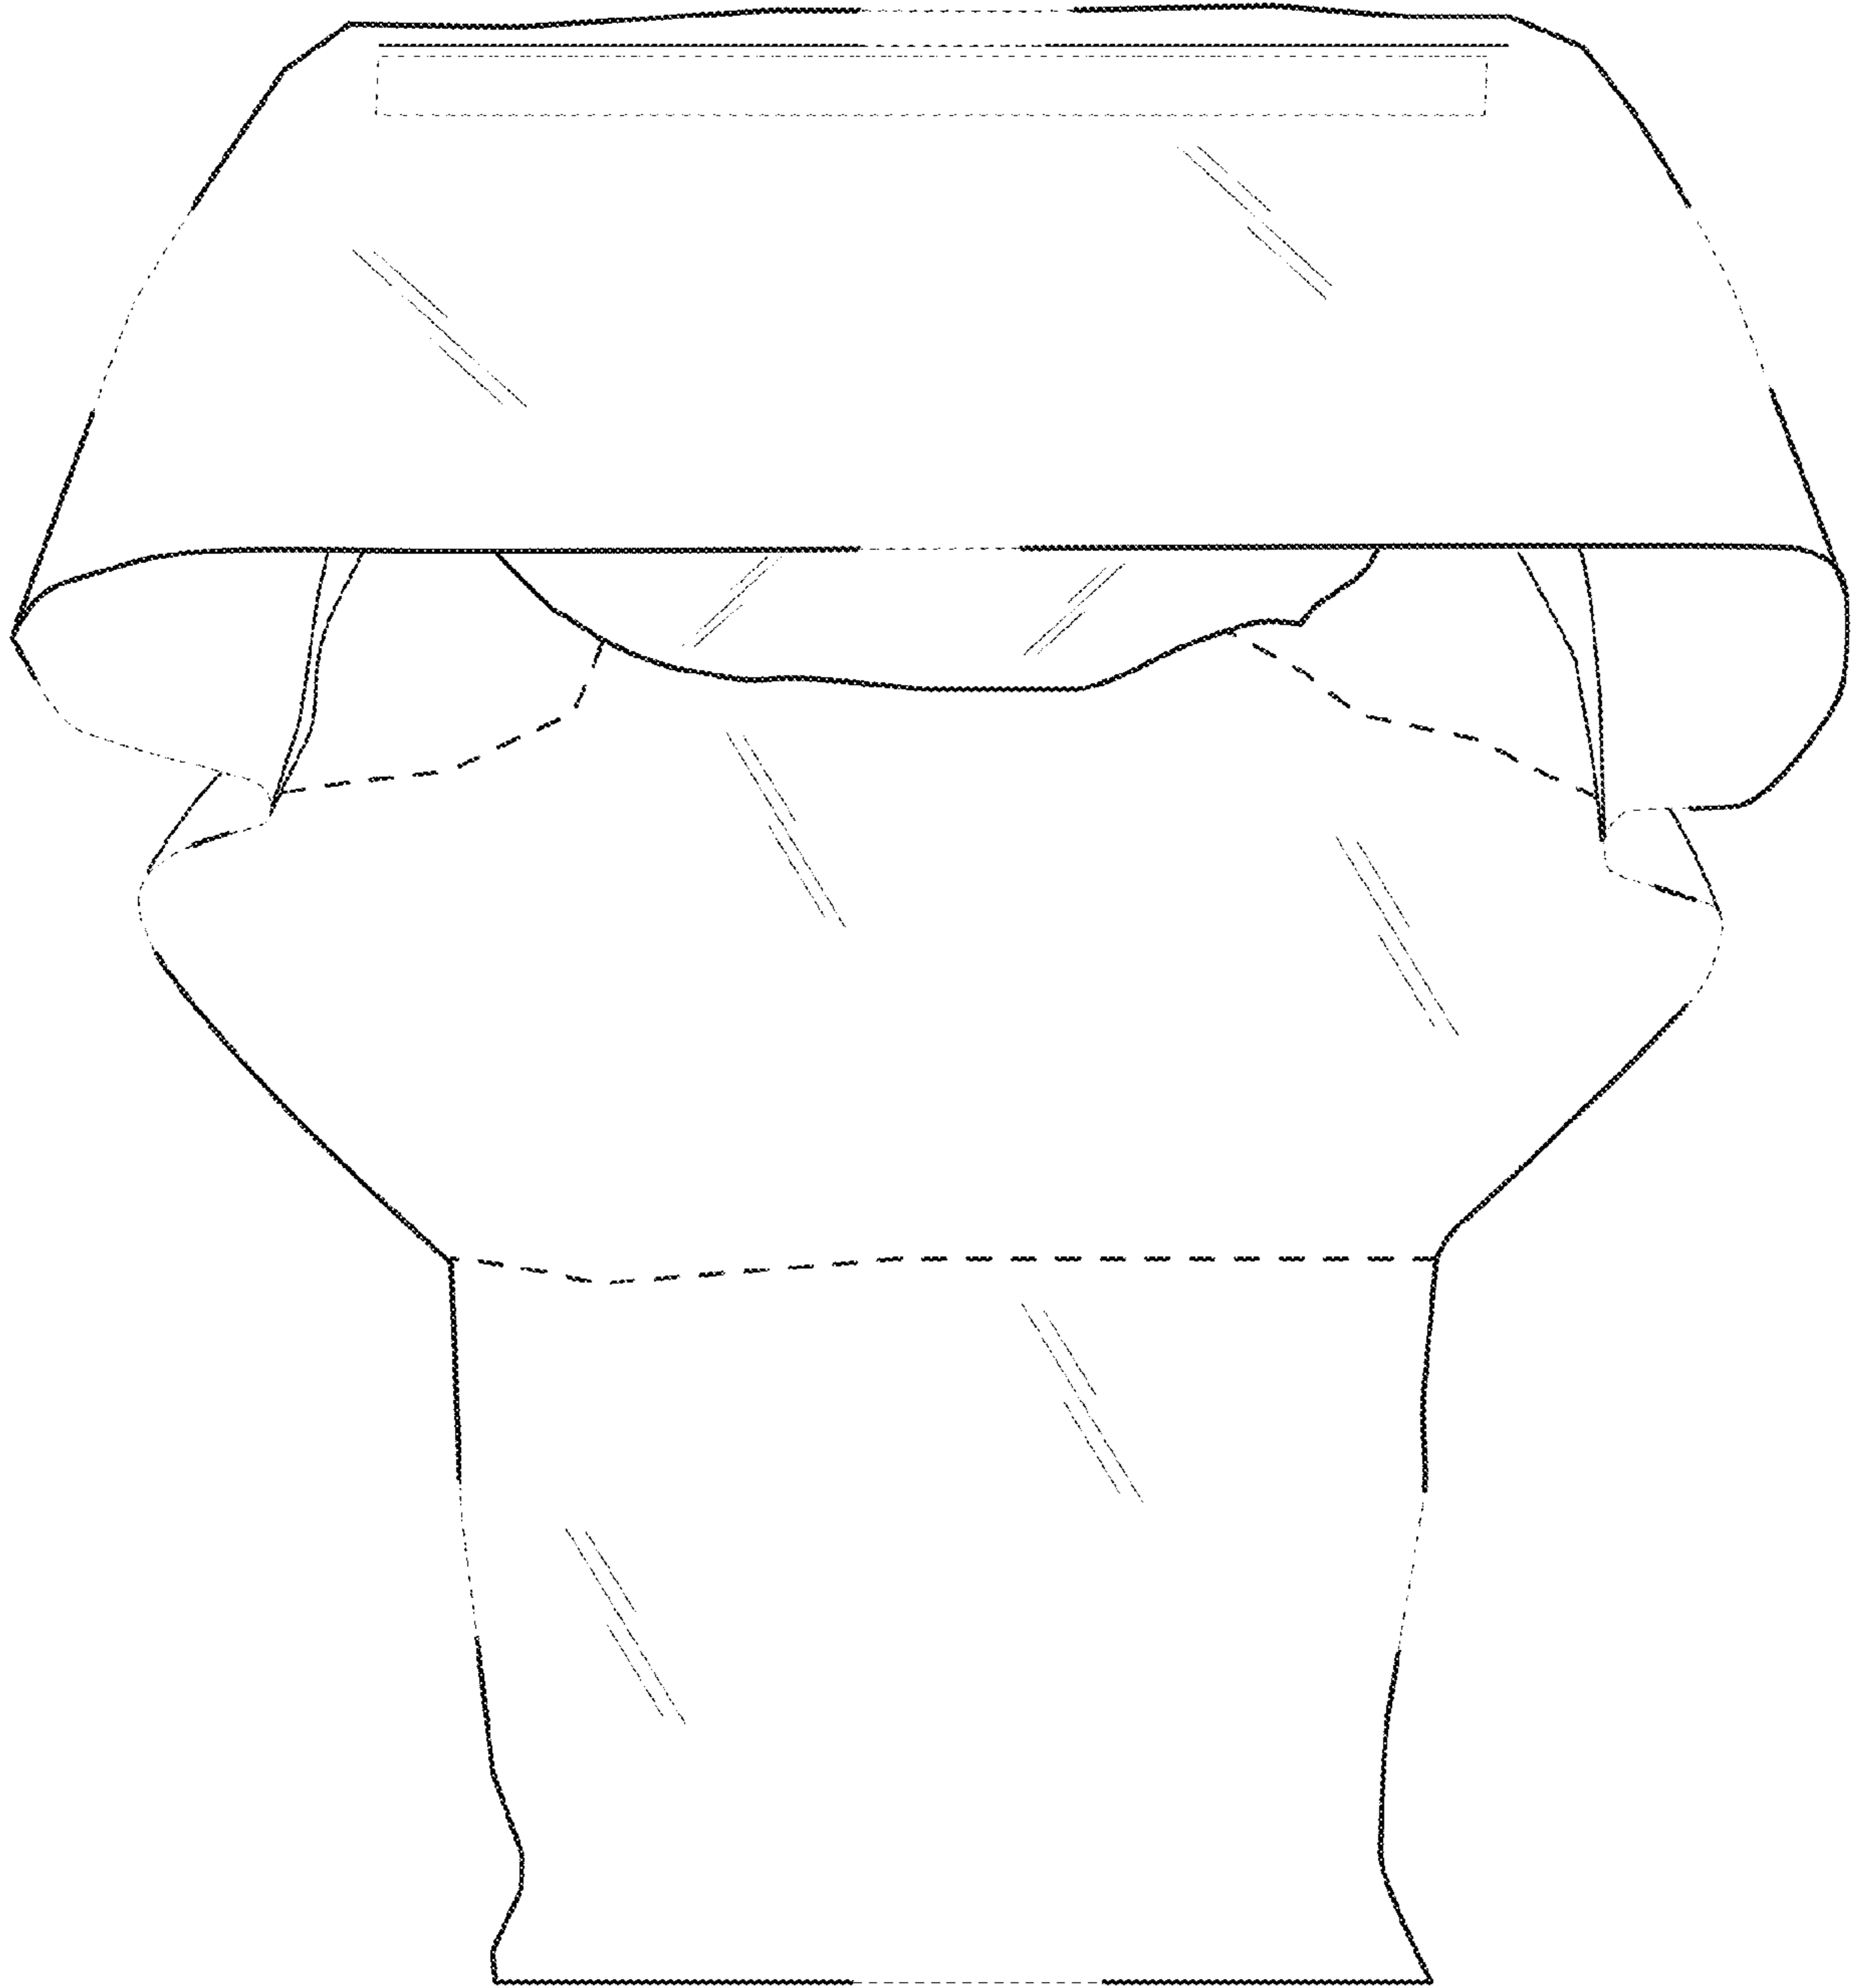


Fig. 14

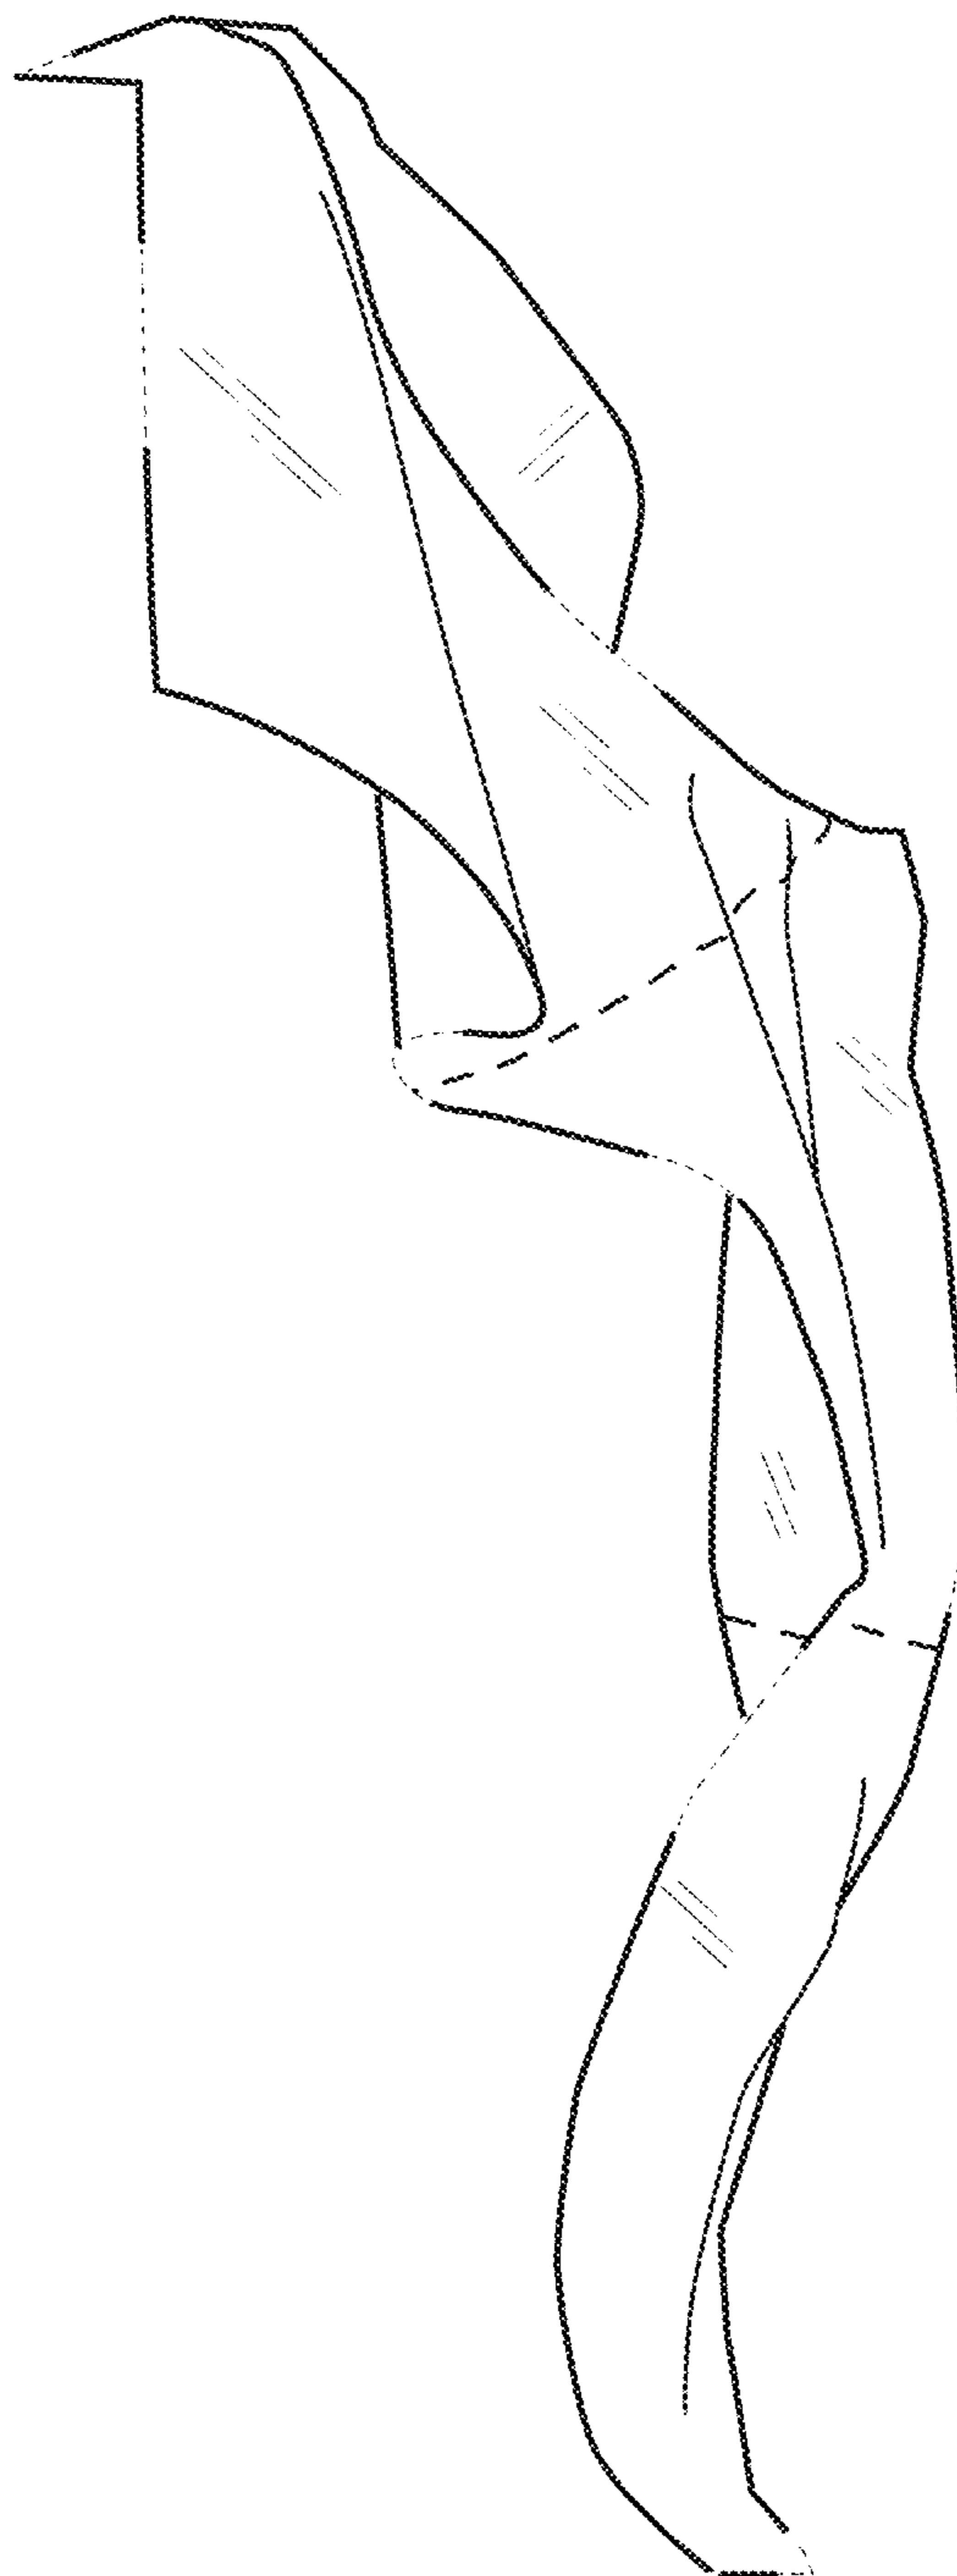


Fig. 15



Fig. 16

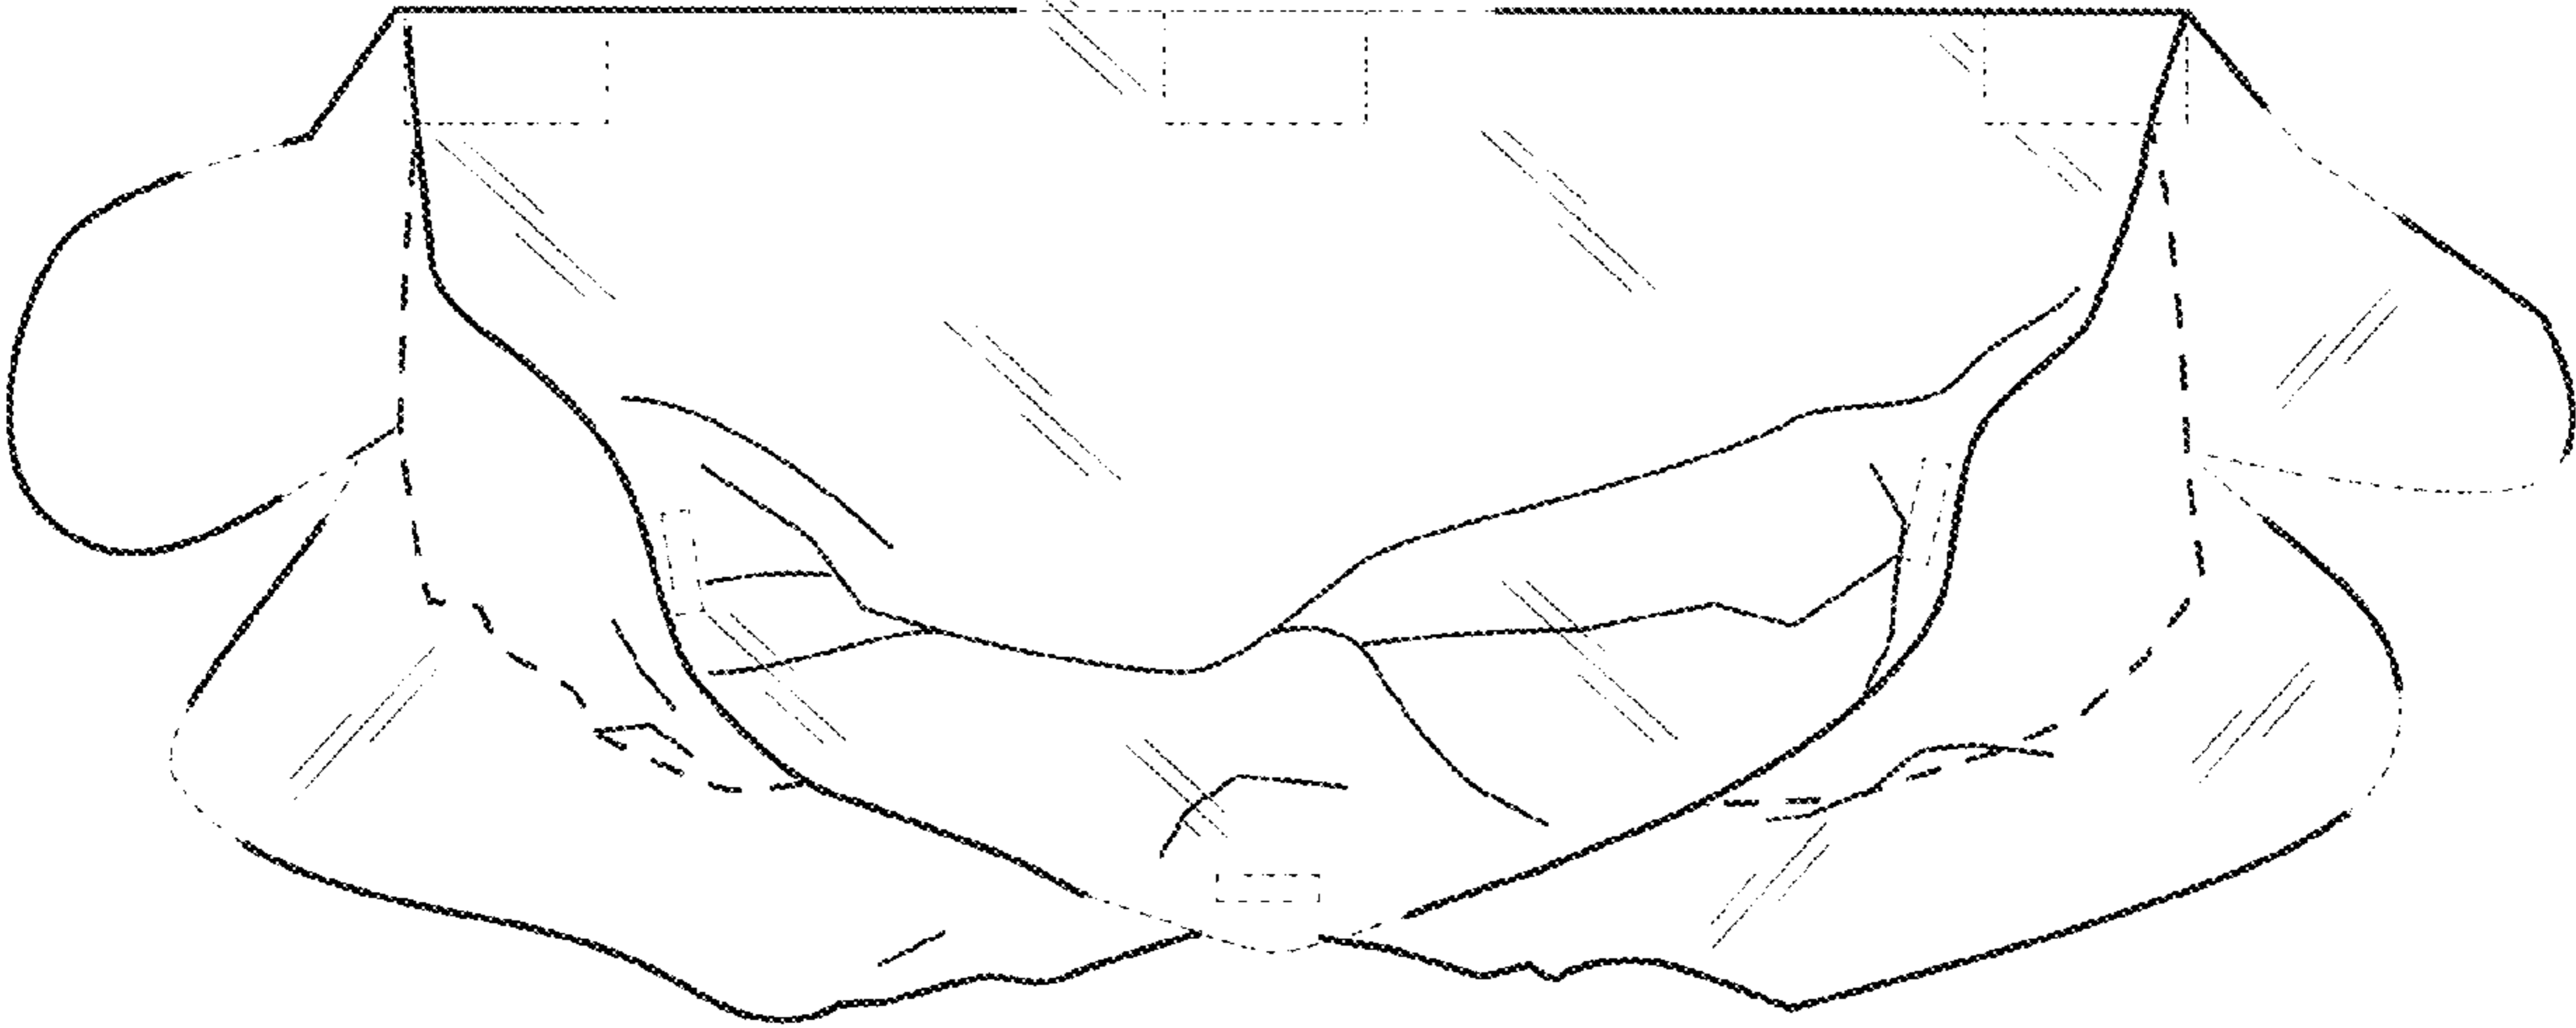


Fig. 17

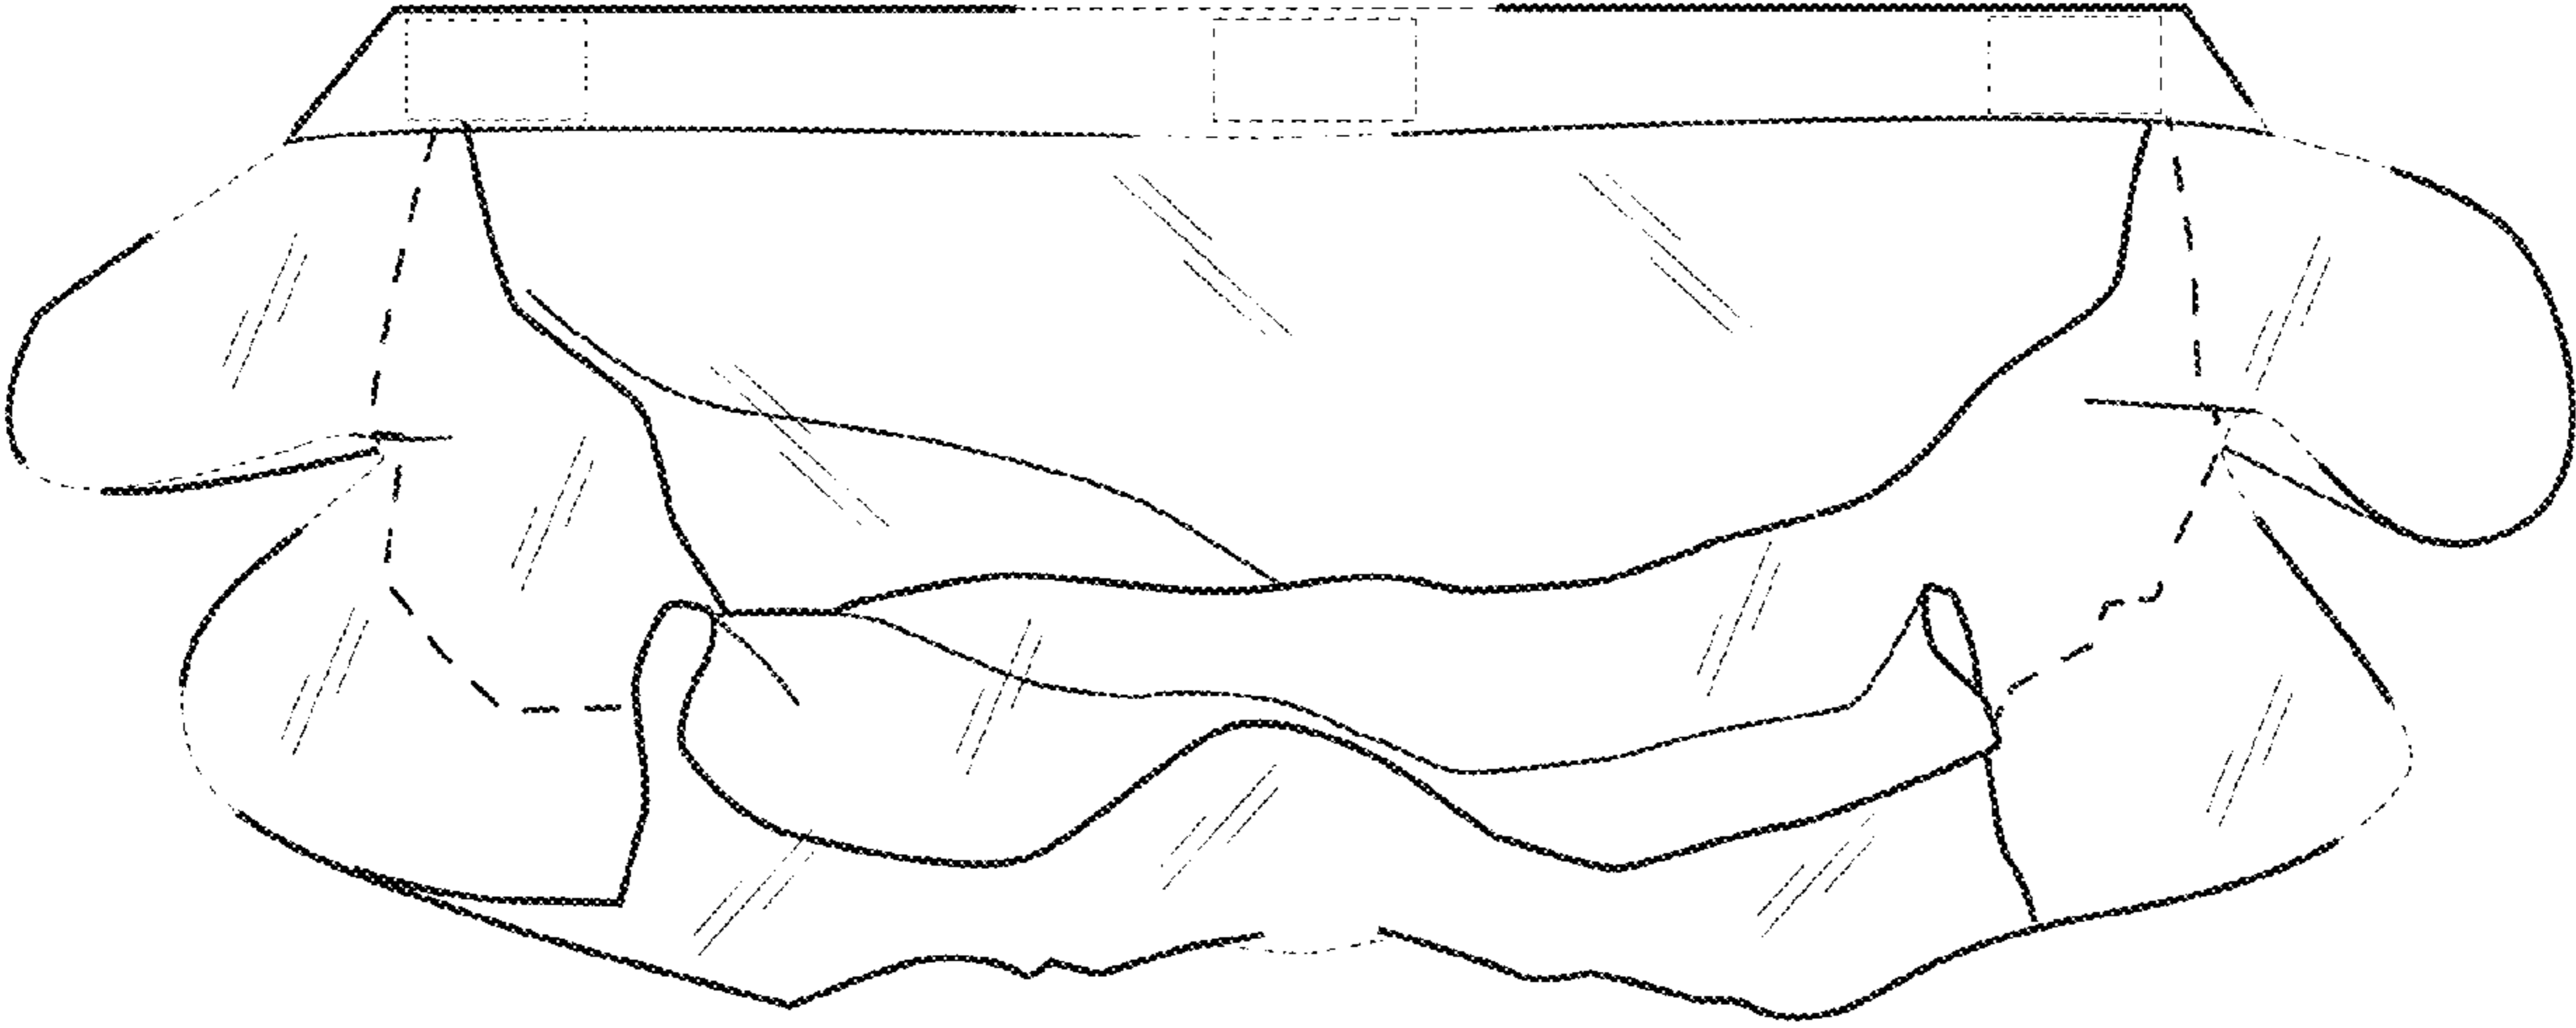


Fig. 18