



US00D916295S

(12) **United States Design Patent** (10) **Patent No.:** **US D916,295 S**  
**Shibayama et al.** (45) **Date of Patent:** **\*\* Apr. 13, 2021**

- (54) **MEDICAL PROBE**
- (71) Applicant: **KONICA MINOLTA, INC.**, Tokyo (JP)
- (72) Inventors: **Jun Shibayama**, Tokyo (JP); **Hirohisa Miyazaki**, Tokyo (JP); **Kenichiro Uchihara**, Nagareyama (JP)
- (73) Assignee: **KONICA MINOLTA, INC.**, Tokyo (JP)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/693,441**
- (22) Filed: **Jun. 3, 2019**

(30) **Foreign Application Priority Data**

Dec. 7, 2018 (JP) ..... 2018-026766

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC ..... D24/133, 137, 138, 141, 158, 160, 164,  
D24/165, 167, 170, 186, 187, 200;  
D10/57, 60, 78, 80  
CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455;  
G01S 7/5208  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D389,919 S \* 1/1998 Ninomiya ..... D24/186
- 6,436,050 B2 \* 8/2002 Garrison ..... B25F 5/02  
600/459
- D681,825 S \* 5/2013 Shinohara ..... D24/186
- D681,828 S \* 5/2013 Shinohara ..... D24/186
- D703,821 S \* 4/2014 Moon ..... D24/187
- D770,629 S \* 11/2016 Nieminen ..... D24/187
- D770,630 S \* 11/2016 Nieminen ..... D24/187
- D811,606 S \* 2/2018 Kitayama ..... D24/187

- D831,219 S \* 10/2018 Henderson ..... D24/187
- D842,482 S \* 3/2019 Harada ..... D24/187
- D844,148 S \* 3/2019 Wilson ..... D24/187
- D861,884 S \* 10/2019 Moon ..... D24/187
- D862,710 S \* 10/2019 Moon ..... D24/187
- D869,665 S \* 12/2019 De Jonge ..... D24/187

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 201330286275 \* 6/2013

**OTHER PUBLICATIONS**

For Sale Mindray Linear Ultrasound Transducer. Online, published date unknown. Retrieved on May 4, 2020 from URL: <https://www.dotmed.com/listing/ultrasound-transducer/mindray/linear/2892592>.\*

(Continued)

*Primary Examiner* — Susan Bennett Hattan  
*Assistant Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Buchanan Ingersoll & Rooney PC


(57) **CLAIM**

The ornamental design for a medical probe, as shown and described.

**DESCRIPTION**

FIG. 1 is a front elevational view of a medical probe showing our new design.  
FIG. 2 is a rear elevational view thereof.  
FIG. 3 is a left side elevational view thereof.  
FIG. 4 is a right side elevational view thereof.  
FIG. 5 is a top plan view thereof.  
FIG. 6 is a bottom plan view thereof; and,  
FIG. 7 is a front, left side and top perspective view thereof.  
The broken lines depict portions of the medical probe that form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

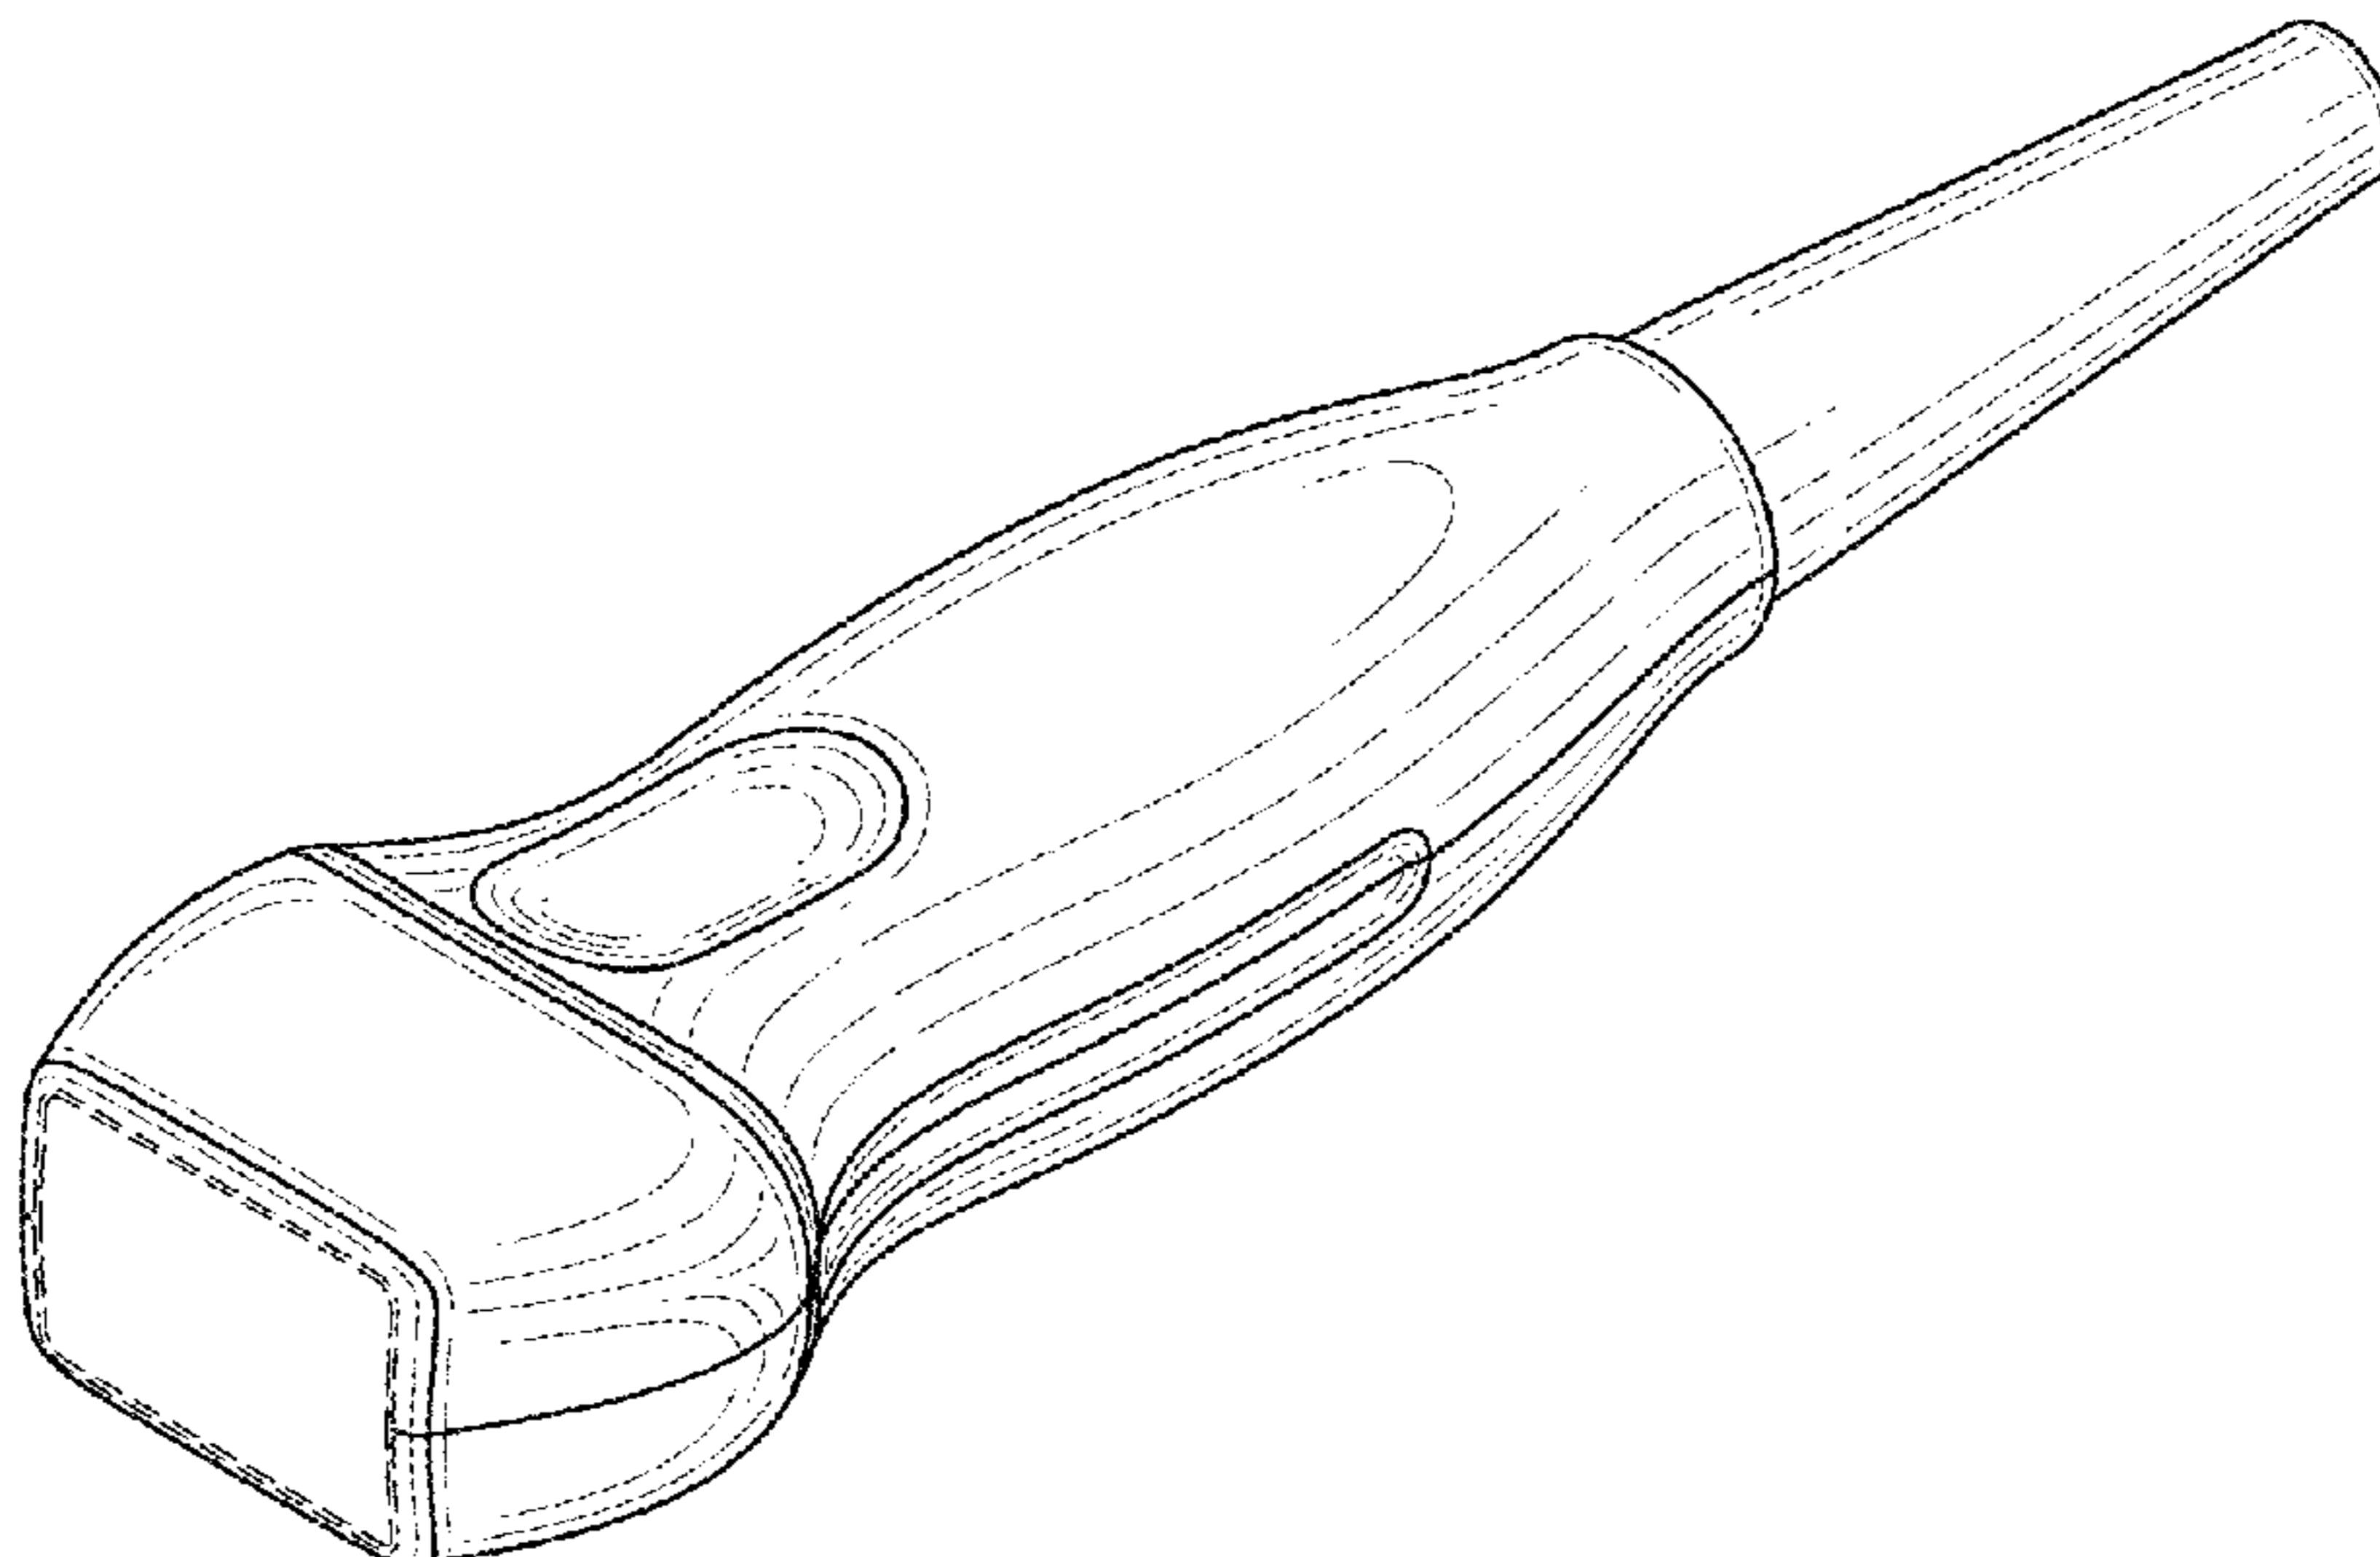

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D870,296 S \* 12/2019 De Jonge ..... D24/187  
D882,096 S \* 4/2020 Dekock ..... D24/187  
2018/0313943 A1\* 11/2018 Bruestle ..... B06B 1/064  
2019/0125313 A1\* 5/2019 Mastri ..... H02J 7/025  
2019/0282207 A1\* 9/2019 Chen ..... A61B 8/4483

OTHER PUBLICATIONS

Phased array ultrasound transducer / cranial. Online, published date unknown. Retrieved on May 4, 2020 from URL: <https://www.medicaexpo.com/prod/esaote/product-68409-625931.html>.\*

\* cited by examiner

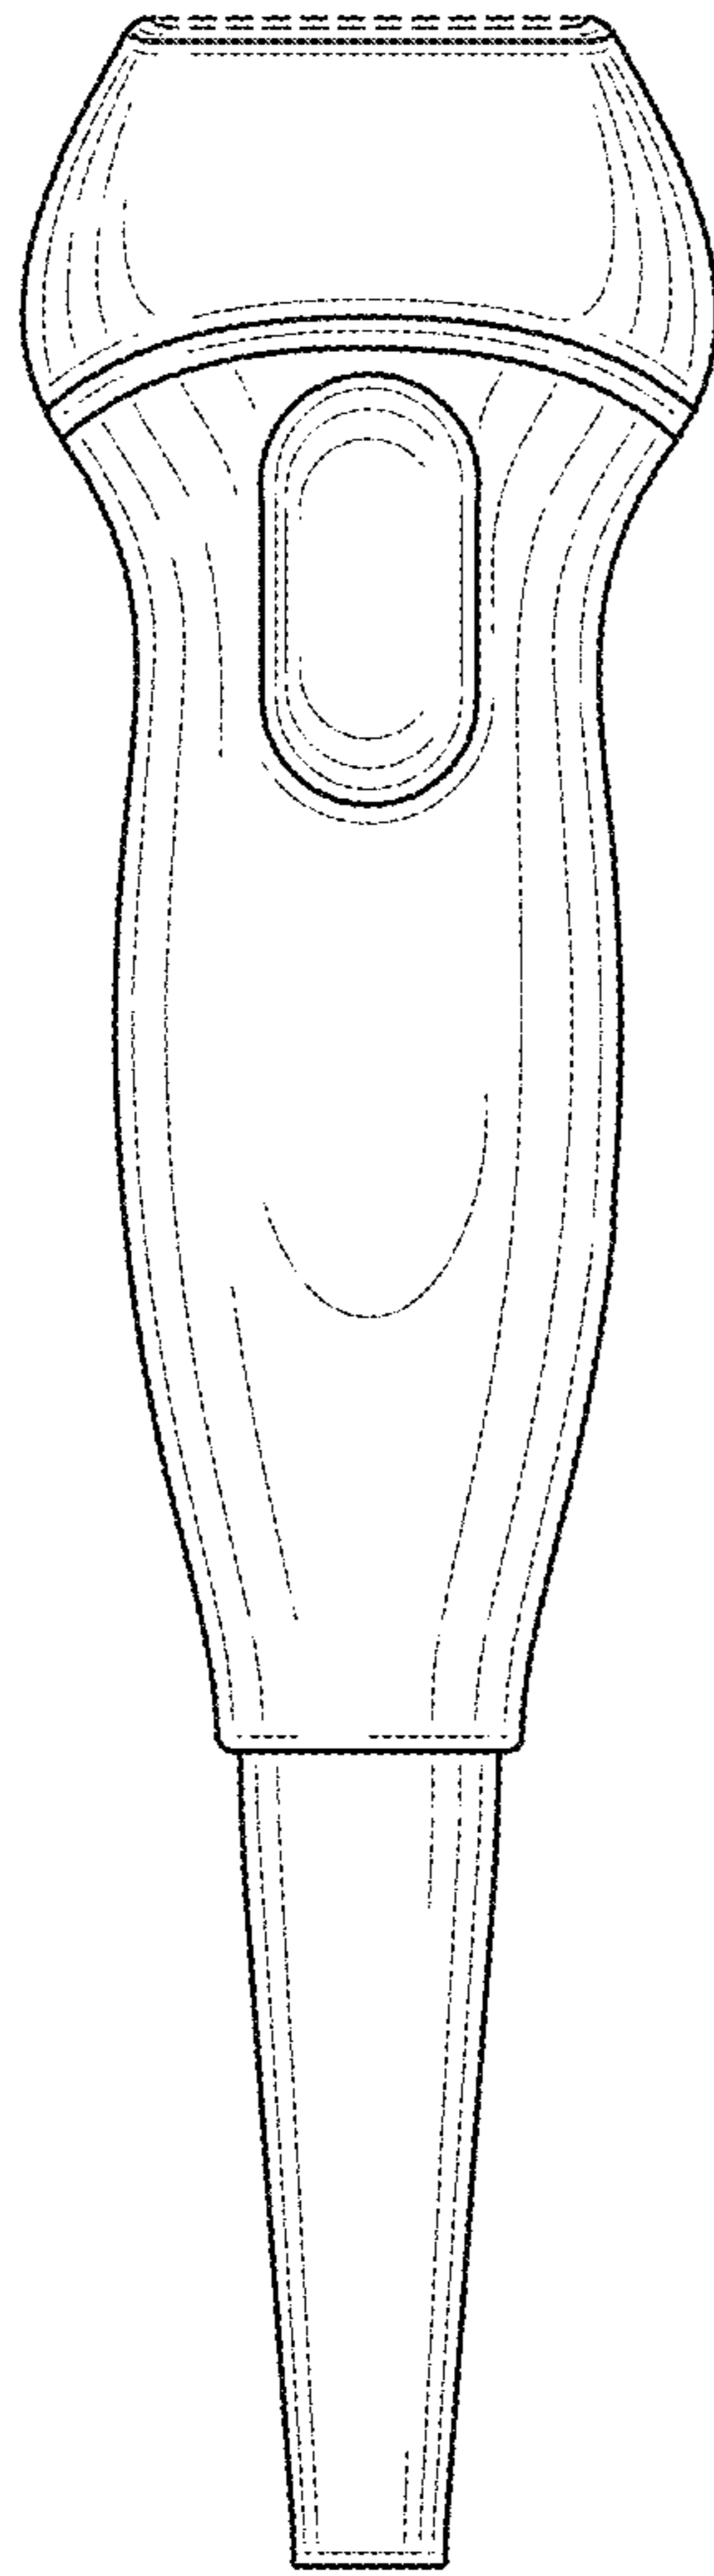


FIG. 1

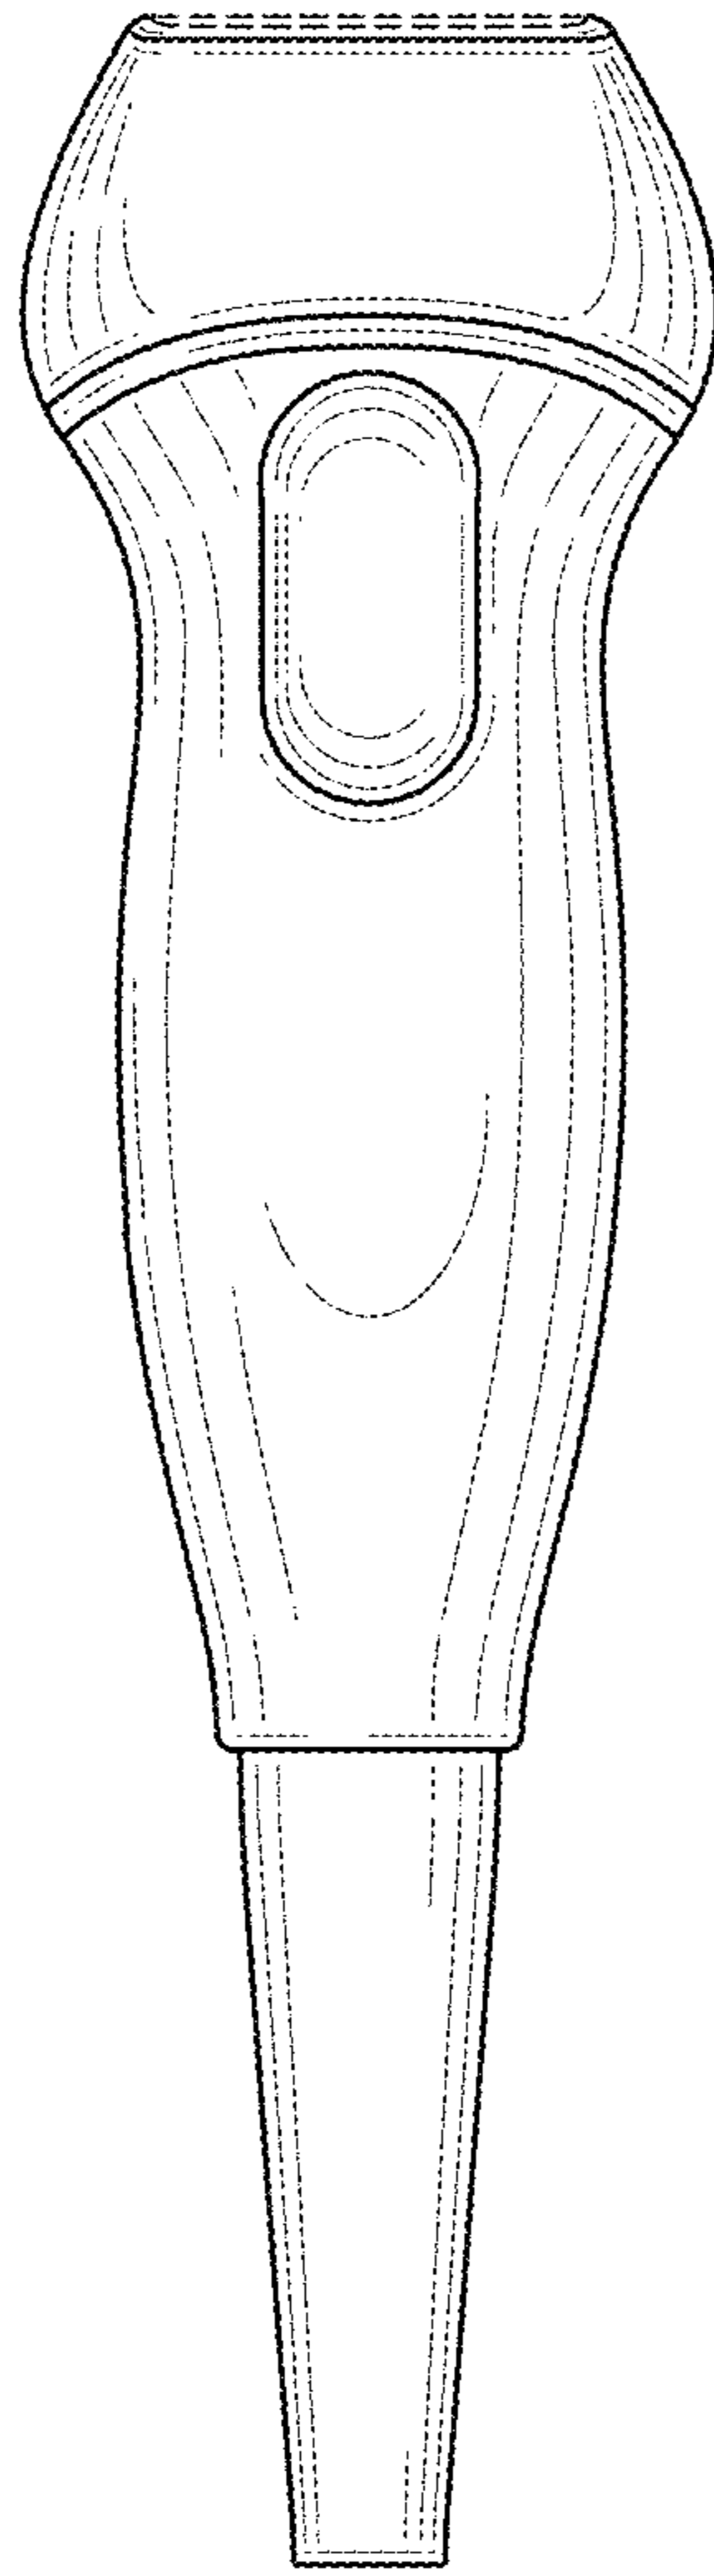


FIG. 2

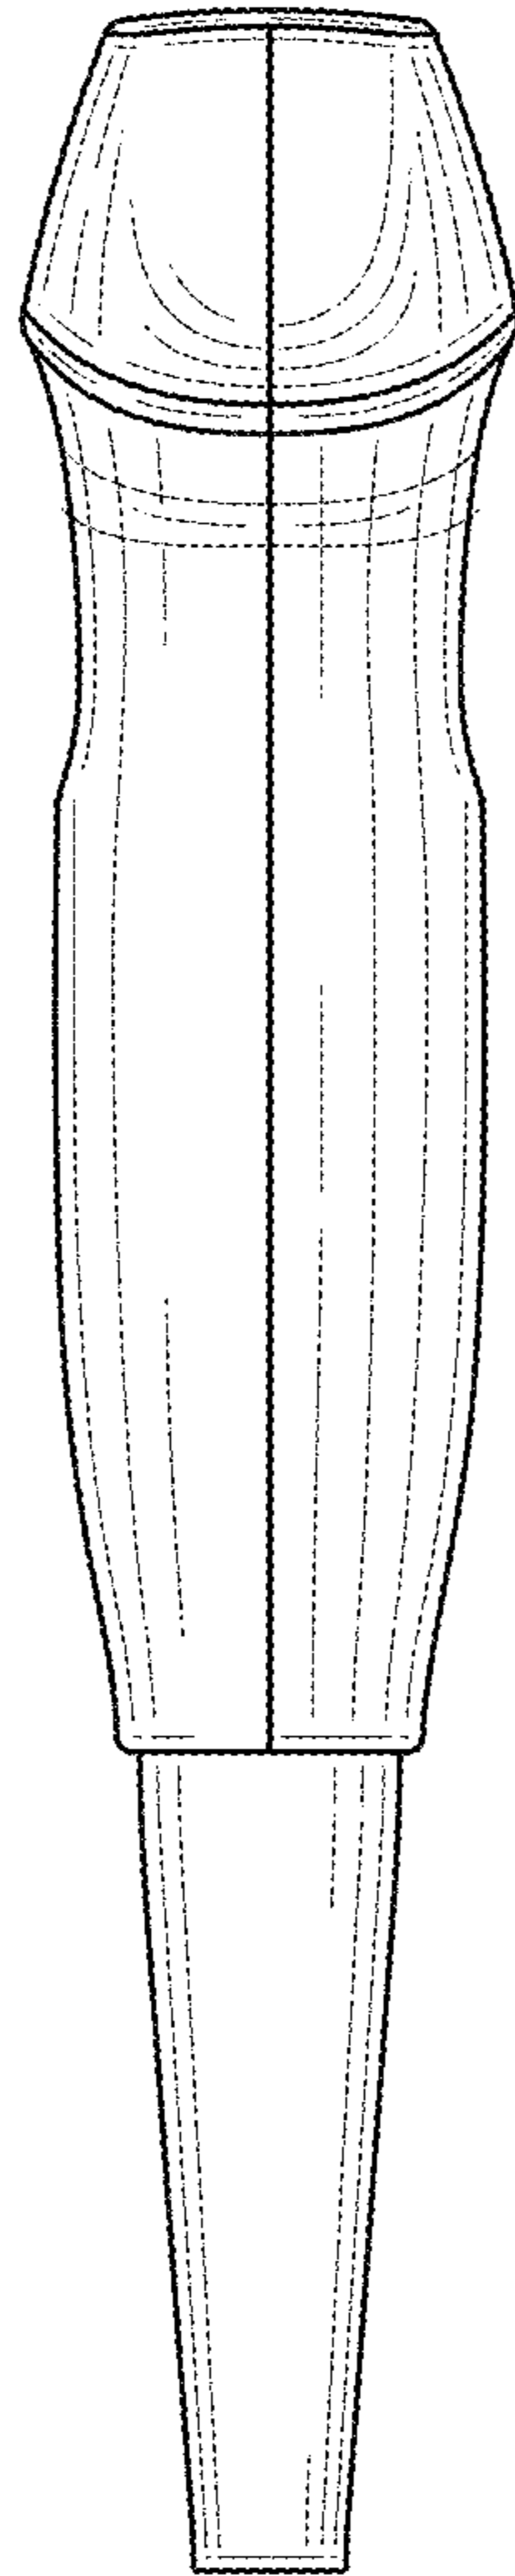


FIG. 3

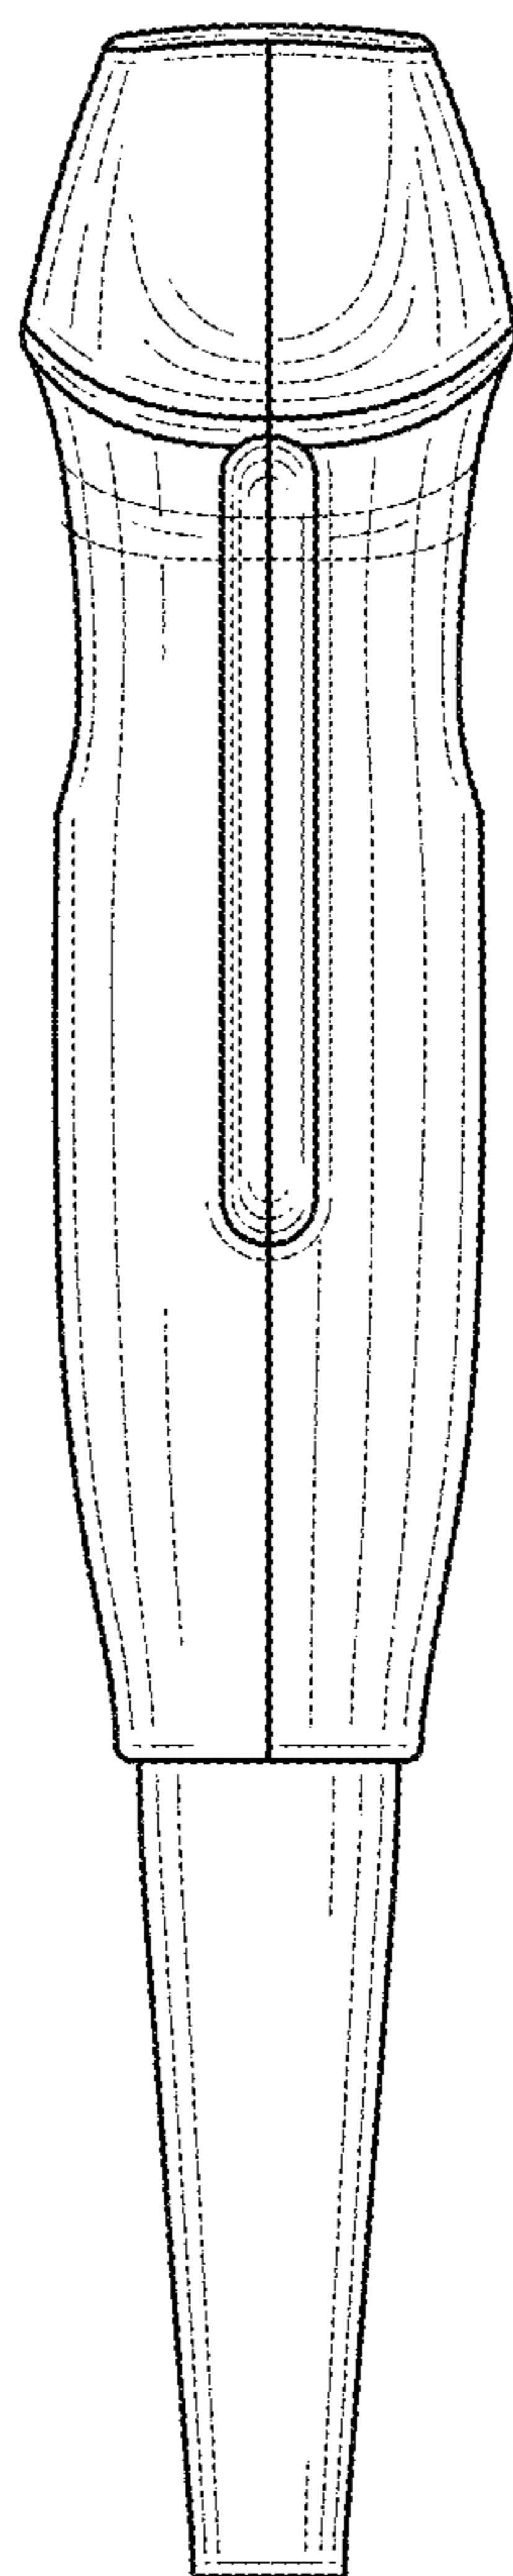


FIG. 4

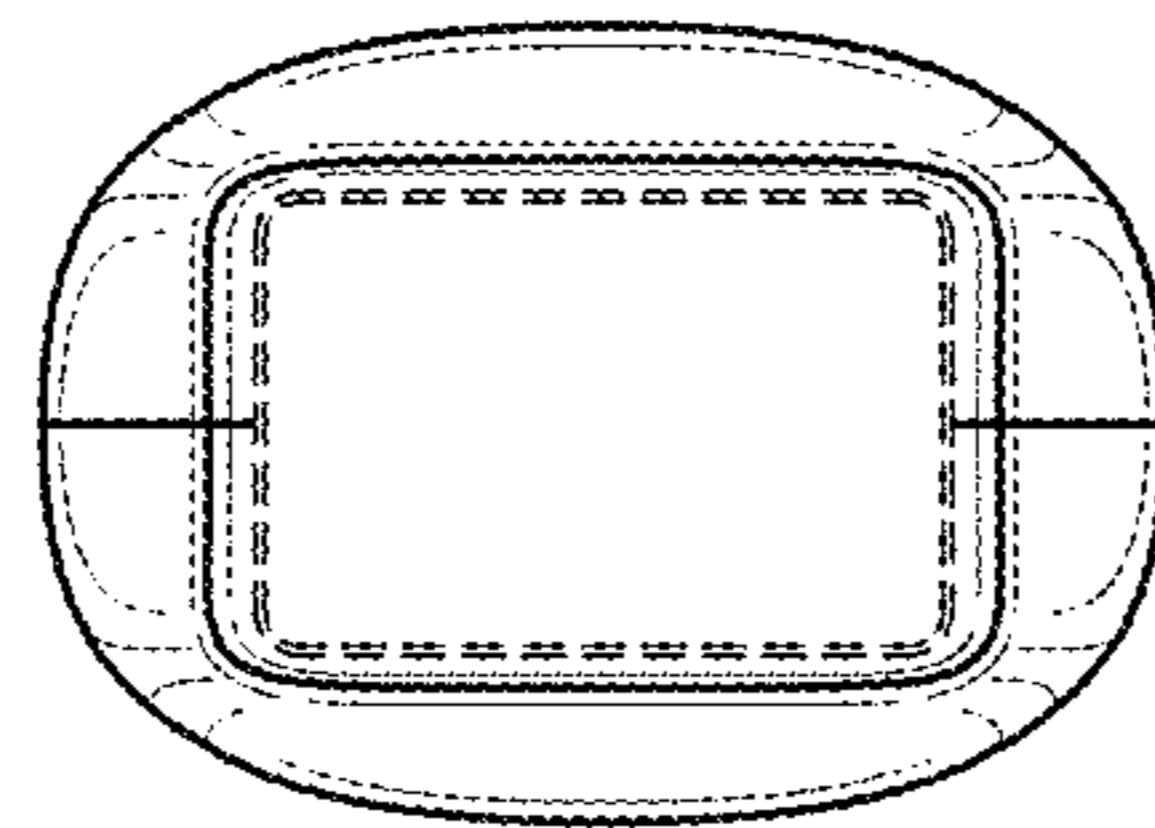


FIG. 5

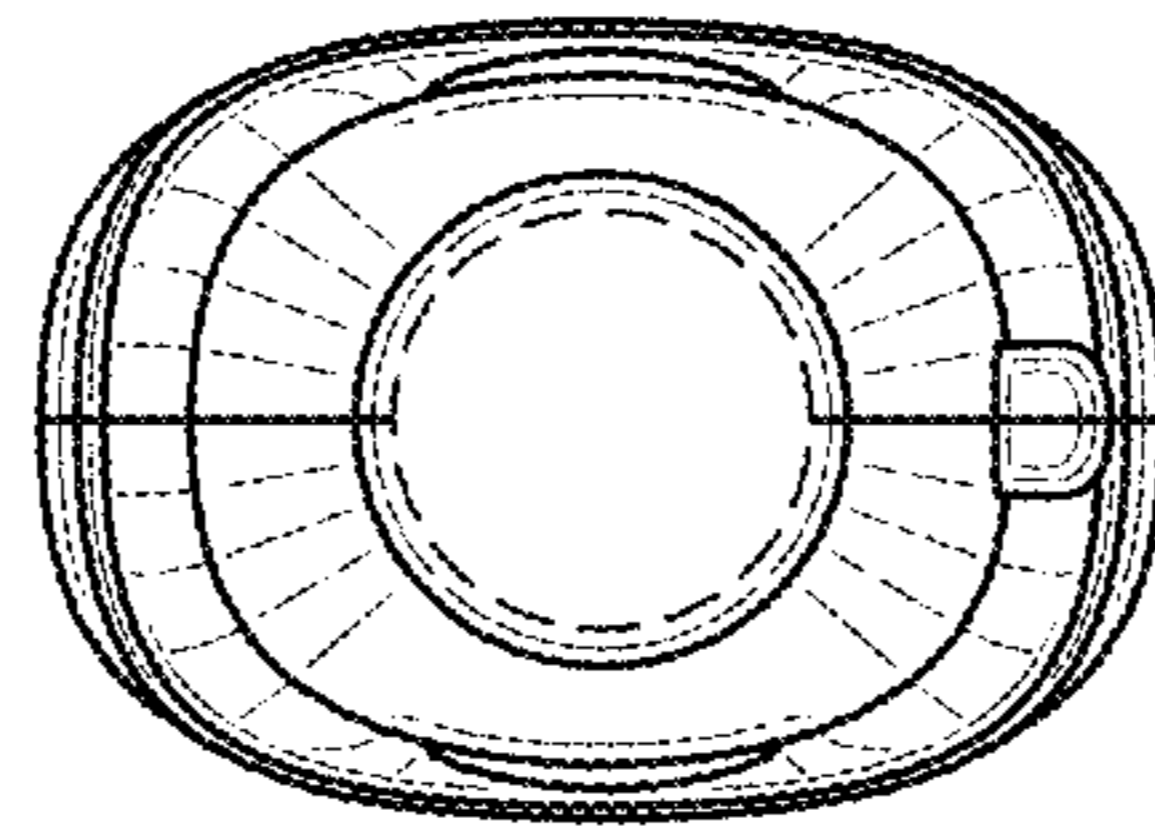


FIG. 6



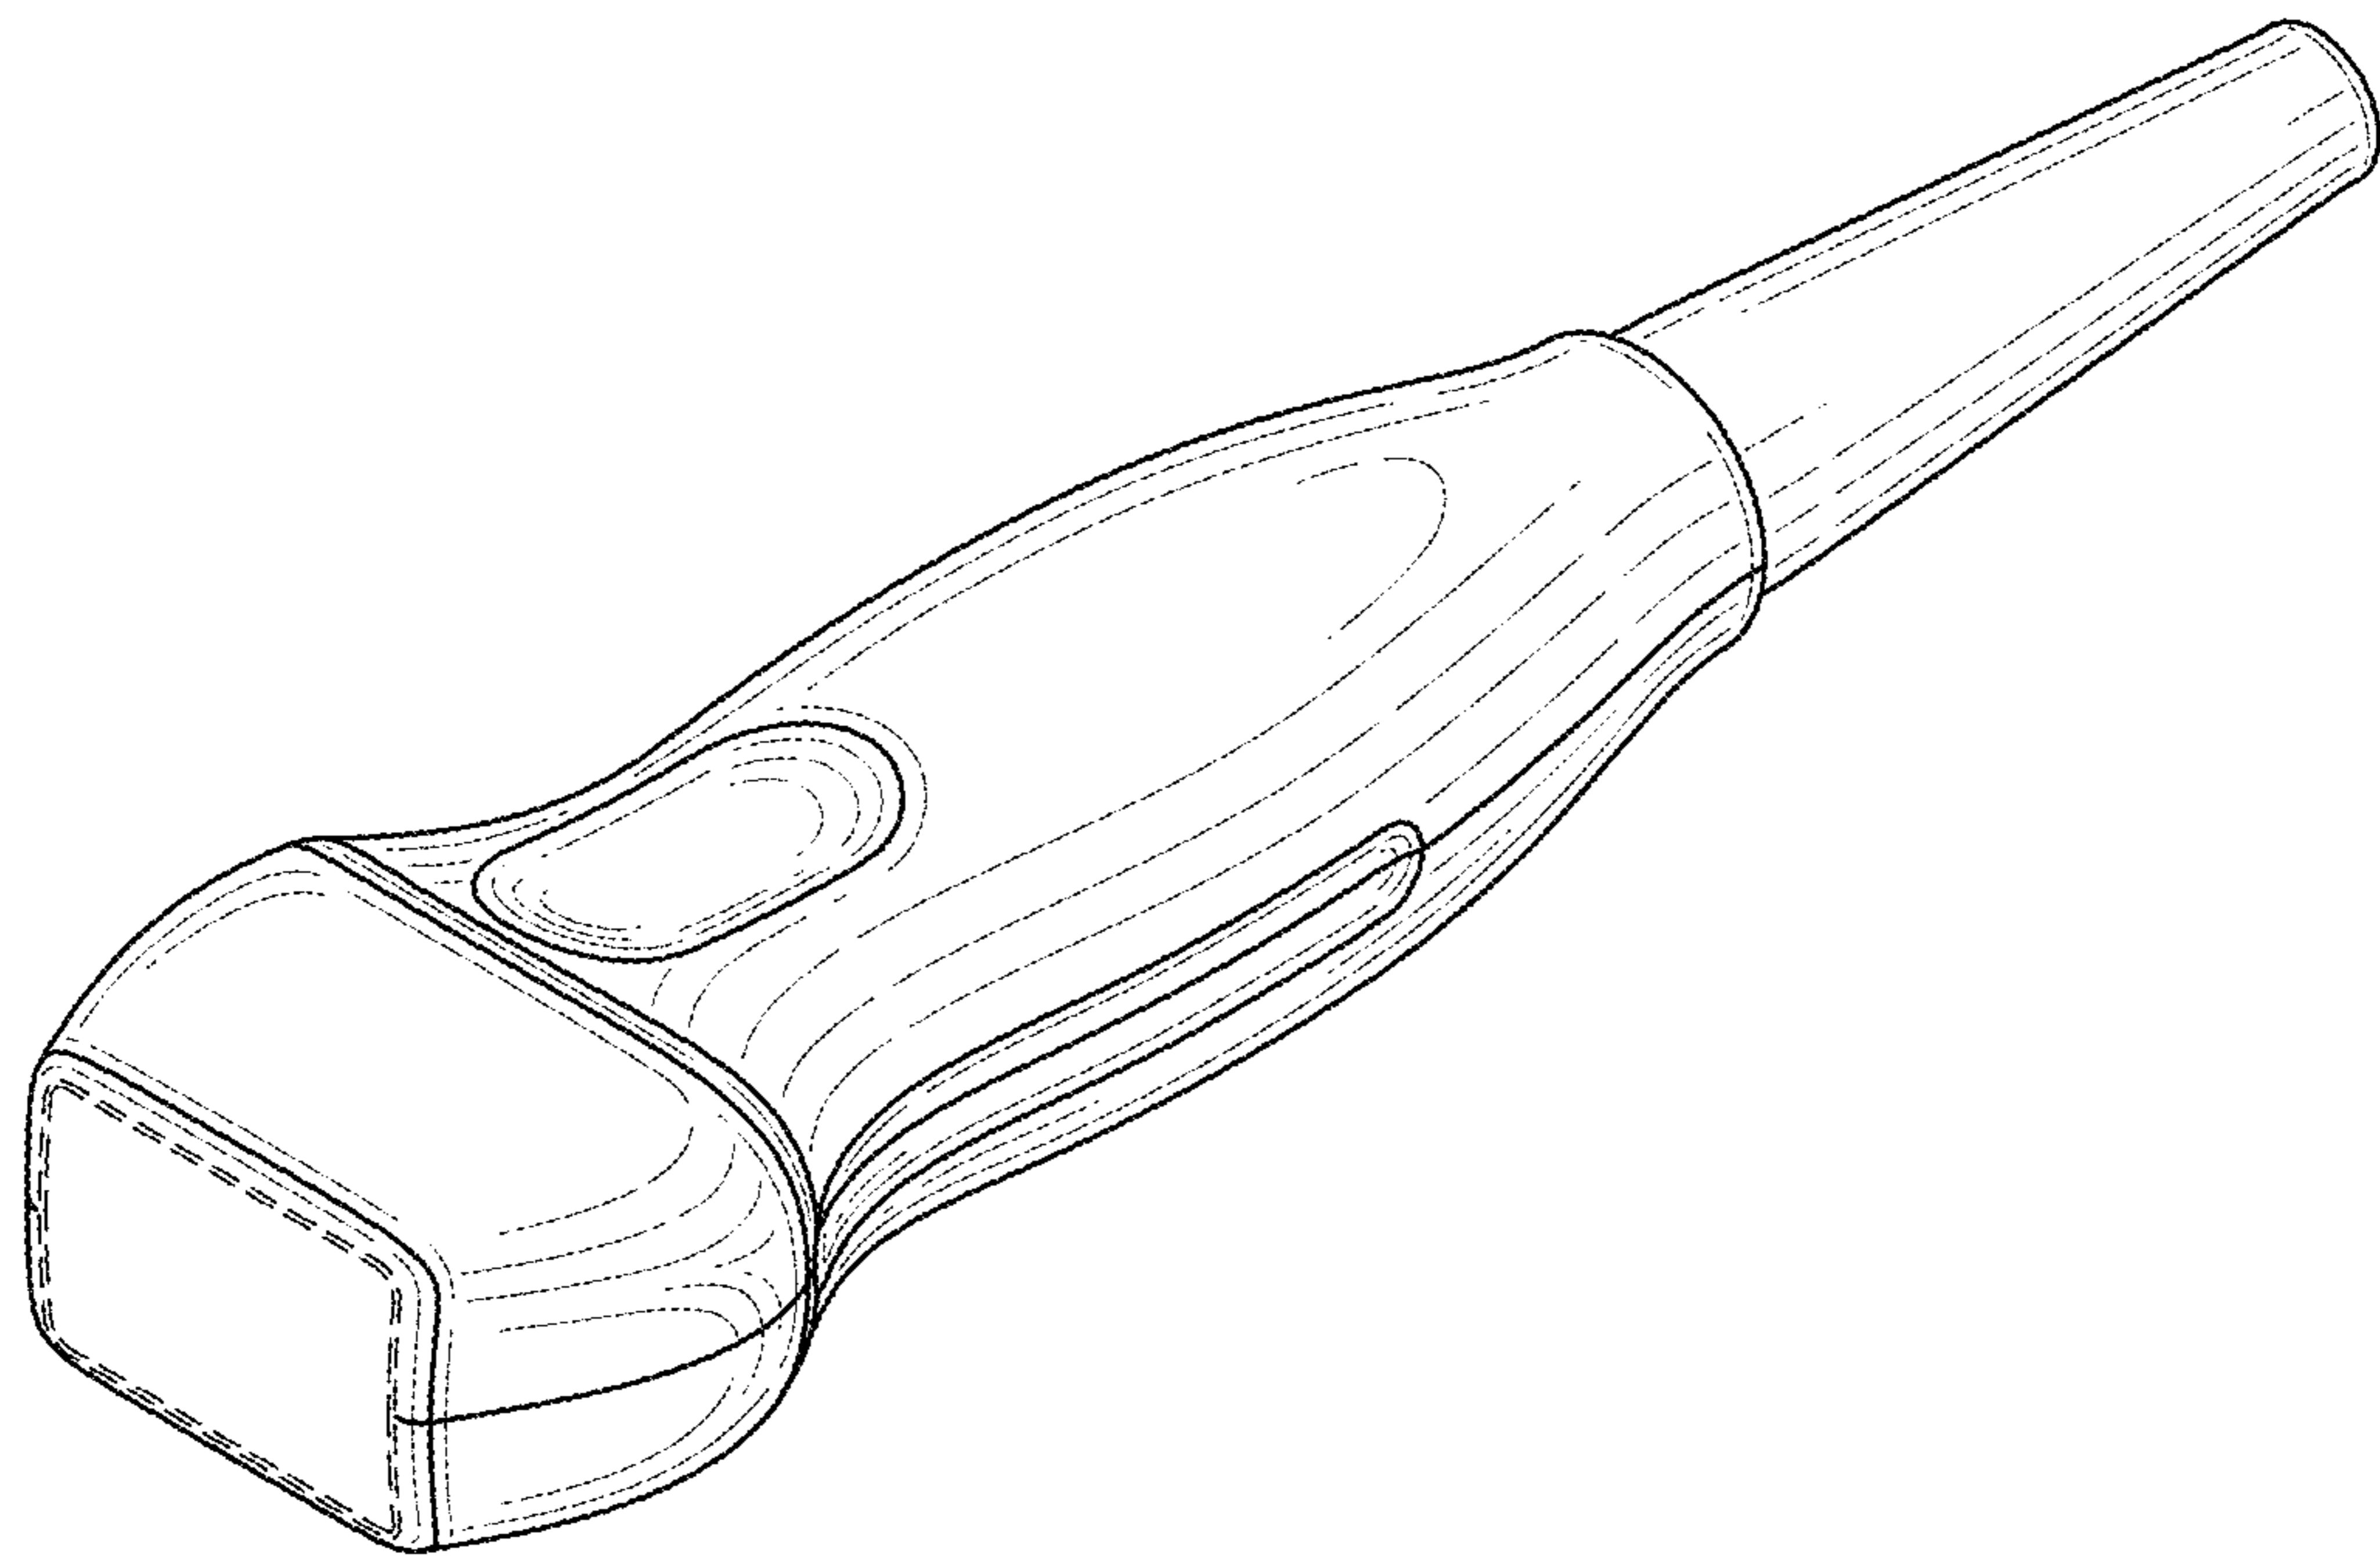


FIG. 7