



US00D917698S

(12) **United States Design Patent** (10) **Patent No.:** **US D917,698 S**
Serbousek et al. (45) **Date of Patent:** **** Apr. 27, 2021**

(54) **SPINAL IMPLANT**
(71) Applicant: **IN QUEUE INNOVATIONS, LLC**,
Winona Lake, IN (US)
(72) Inventors: **Jon C. Serbousek**, Winona Lake, IN
(US); **Jeffrey Nycz**, Warsaw, IN (US)
(73) Assignee: **IN QUEUE INNOVATIONS, LLC**,
Winona Lake, IN (US)

D855,184 S 7/2019 Predick
D875,938 S * 2/2020 Serbousek D24/155
D885,578 S * 5/2020 Nycz D24/155
2006/0085071 A1 4/2006 Lechmann et al.
2009/0105830 A1* 4/2009 Jones A61F 2/4455
623/17.16
2012/0065734 A1 3/2012 Barrett et al.
2014/0066995 A1 3/2014 McCormick
2016/0228257 A1* 8/2016 Predick A61B 17/8042

(**) Term: **15 Years**
(21) Appl. No.: **29/735,485**
(22) Filed: **May 21, 2020**

* cited by examiner
Primary Examiner — Charles D Hanson
(74) *Attorney, Agent, or Firm* — Heslin Rothenberg
Farley & Mesiti P.C.

Related U.S. Application Data

(63) Continuation of application No. 29/678,865, filed on
Jan. 31, 2019, now Pat. No. Des. 885,578.
(51) **LOC (13) Cl.** **24-03**
(52) **U.S. Cl.**
USPC **D24/155**
(58) **Field of Classification Search**
USPC D24/155–157
CPC A61B 17/7037; A61B 17/7032; A61B
17/7291; A61B 17/8605; A61B 17/864;
A61B 17/8685; A61B 17/70; A61B
17/7011; A61B 17/7035; A61B 17/7082
See application file for complete search history.

(57) **CLAIM**

The ornamental design for a spinal implant, as shown and
described.


DESCRIPTION

FIG. 1 is a top, front perspective view of a spinal implant
comprising the new design;
FIG. 2 is a bottom, back perspective view of the design of
FIG. 1;
FIG. 3 is a front elevational view of the design of FIG. 1;
FIG. 4 is a back elevational view of the design of FIG. 1;
FIG. 5 is a left side elevational view of the design of FIG.
1;
FIG. 6 is a right side elevational view of the design of FIG.
1;
FIG. 7 is a top view of the design of FIG. 1; and,
FIG. 8 is a bottom view of the design of FIG. 1.
The broken lines shown in the figures are directed to the
environment and are for illustrative purposes only; the
broken lines form no part of the claimed spinal implant
invention.
The relatively light intermittently broken surface shading
depicts contour, not surface decoration.

(56) **References Cited**
U.S. PATENT DOCUMENTS

7,322,983 B2* 1/2008 Harris A61B 17/8057
606/273
D720,458 S * 12/2014 Hagenmeyer D24/155
D789,540 S 6/2017 Gyorgy
9,713,537 B2 7/2017 Bray, Jr.
D819,209 S 5/2018 DaCosta et al.

1 Claim, 7 Drawing Sheets

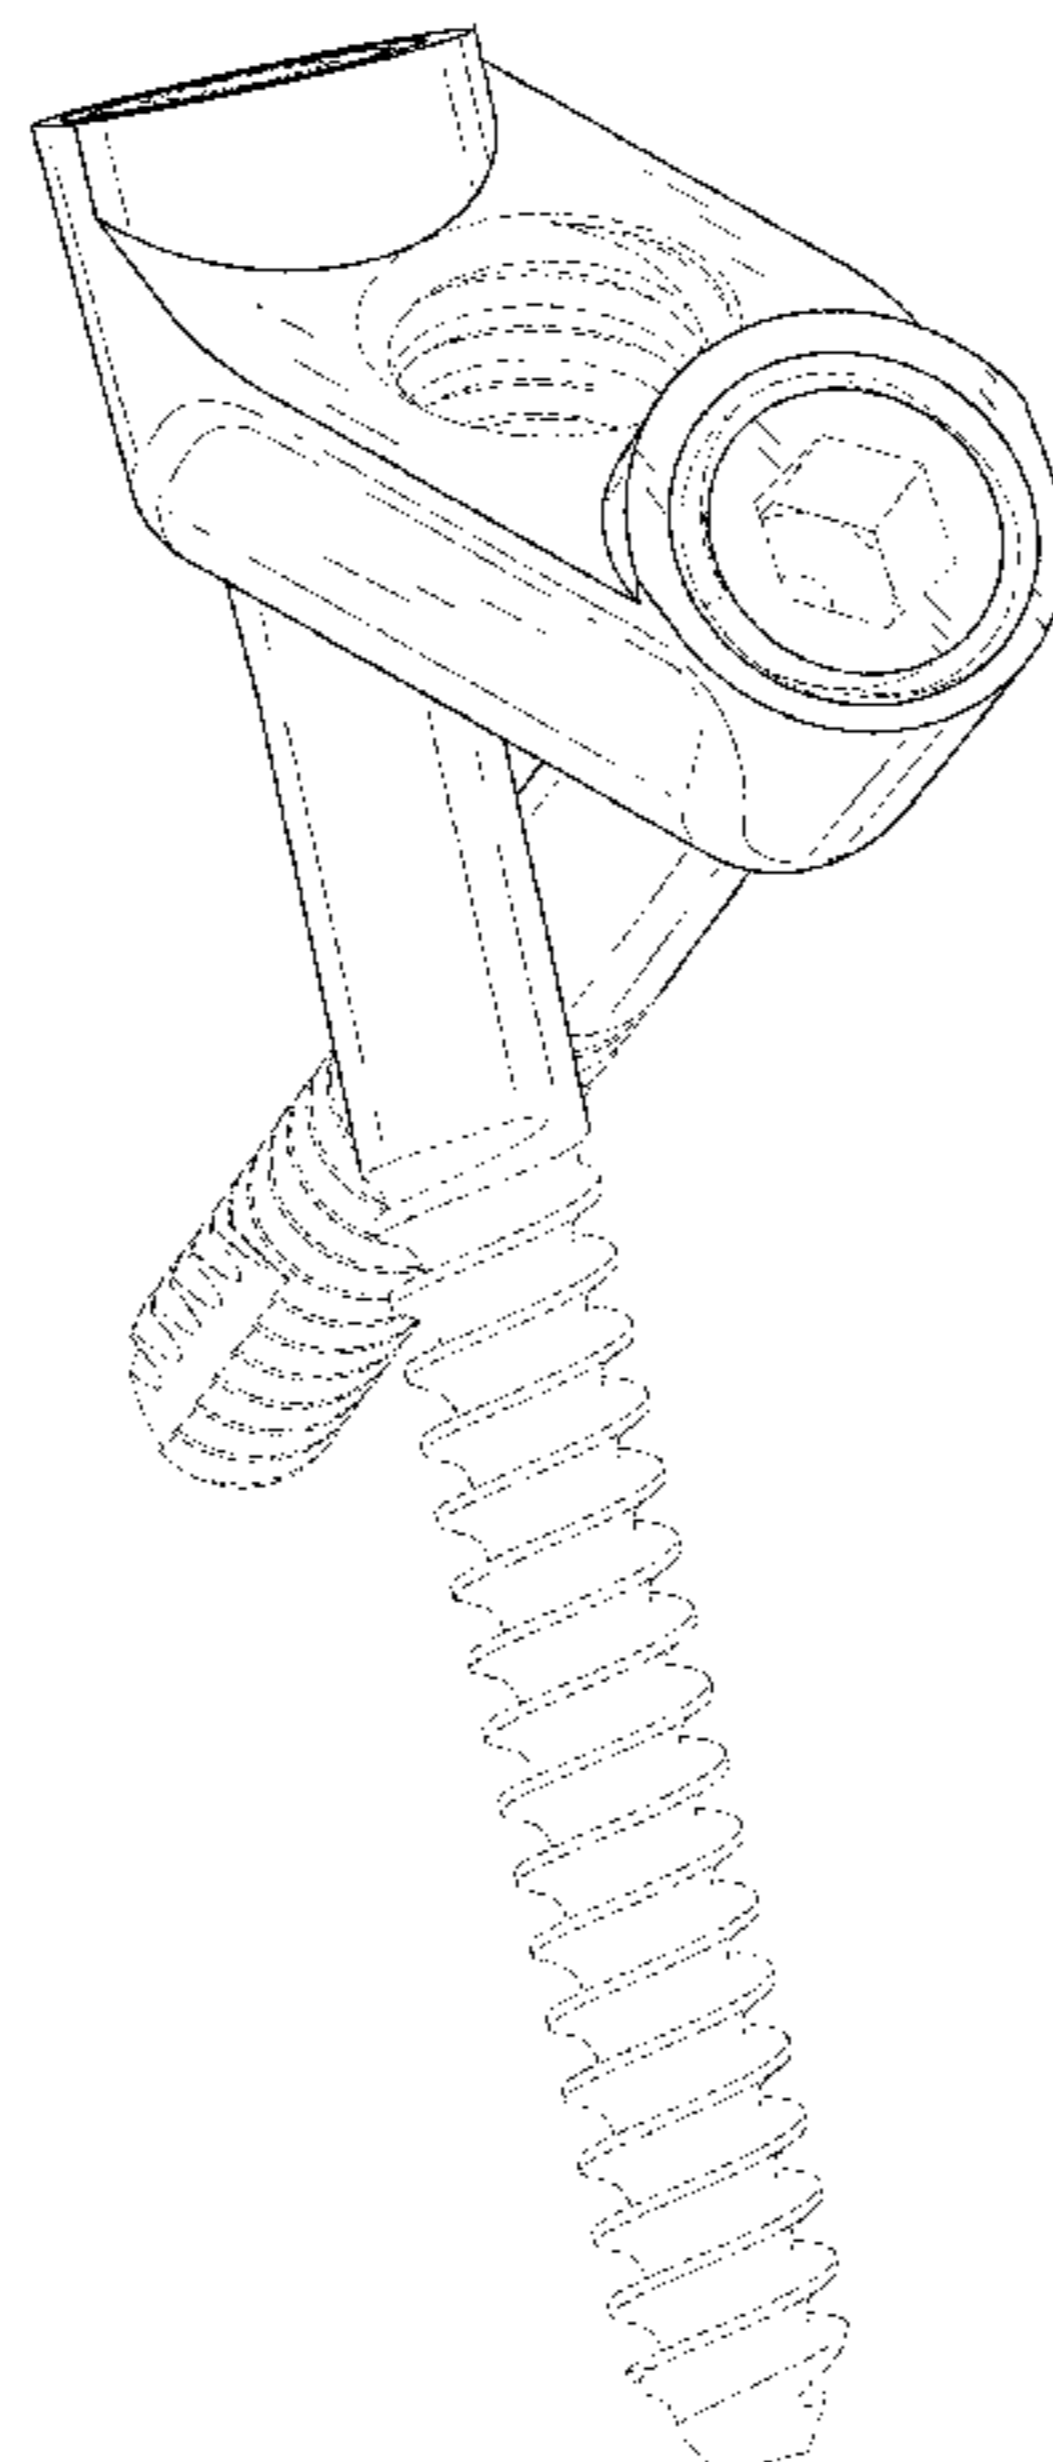

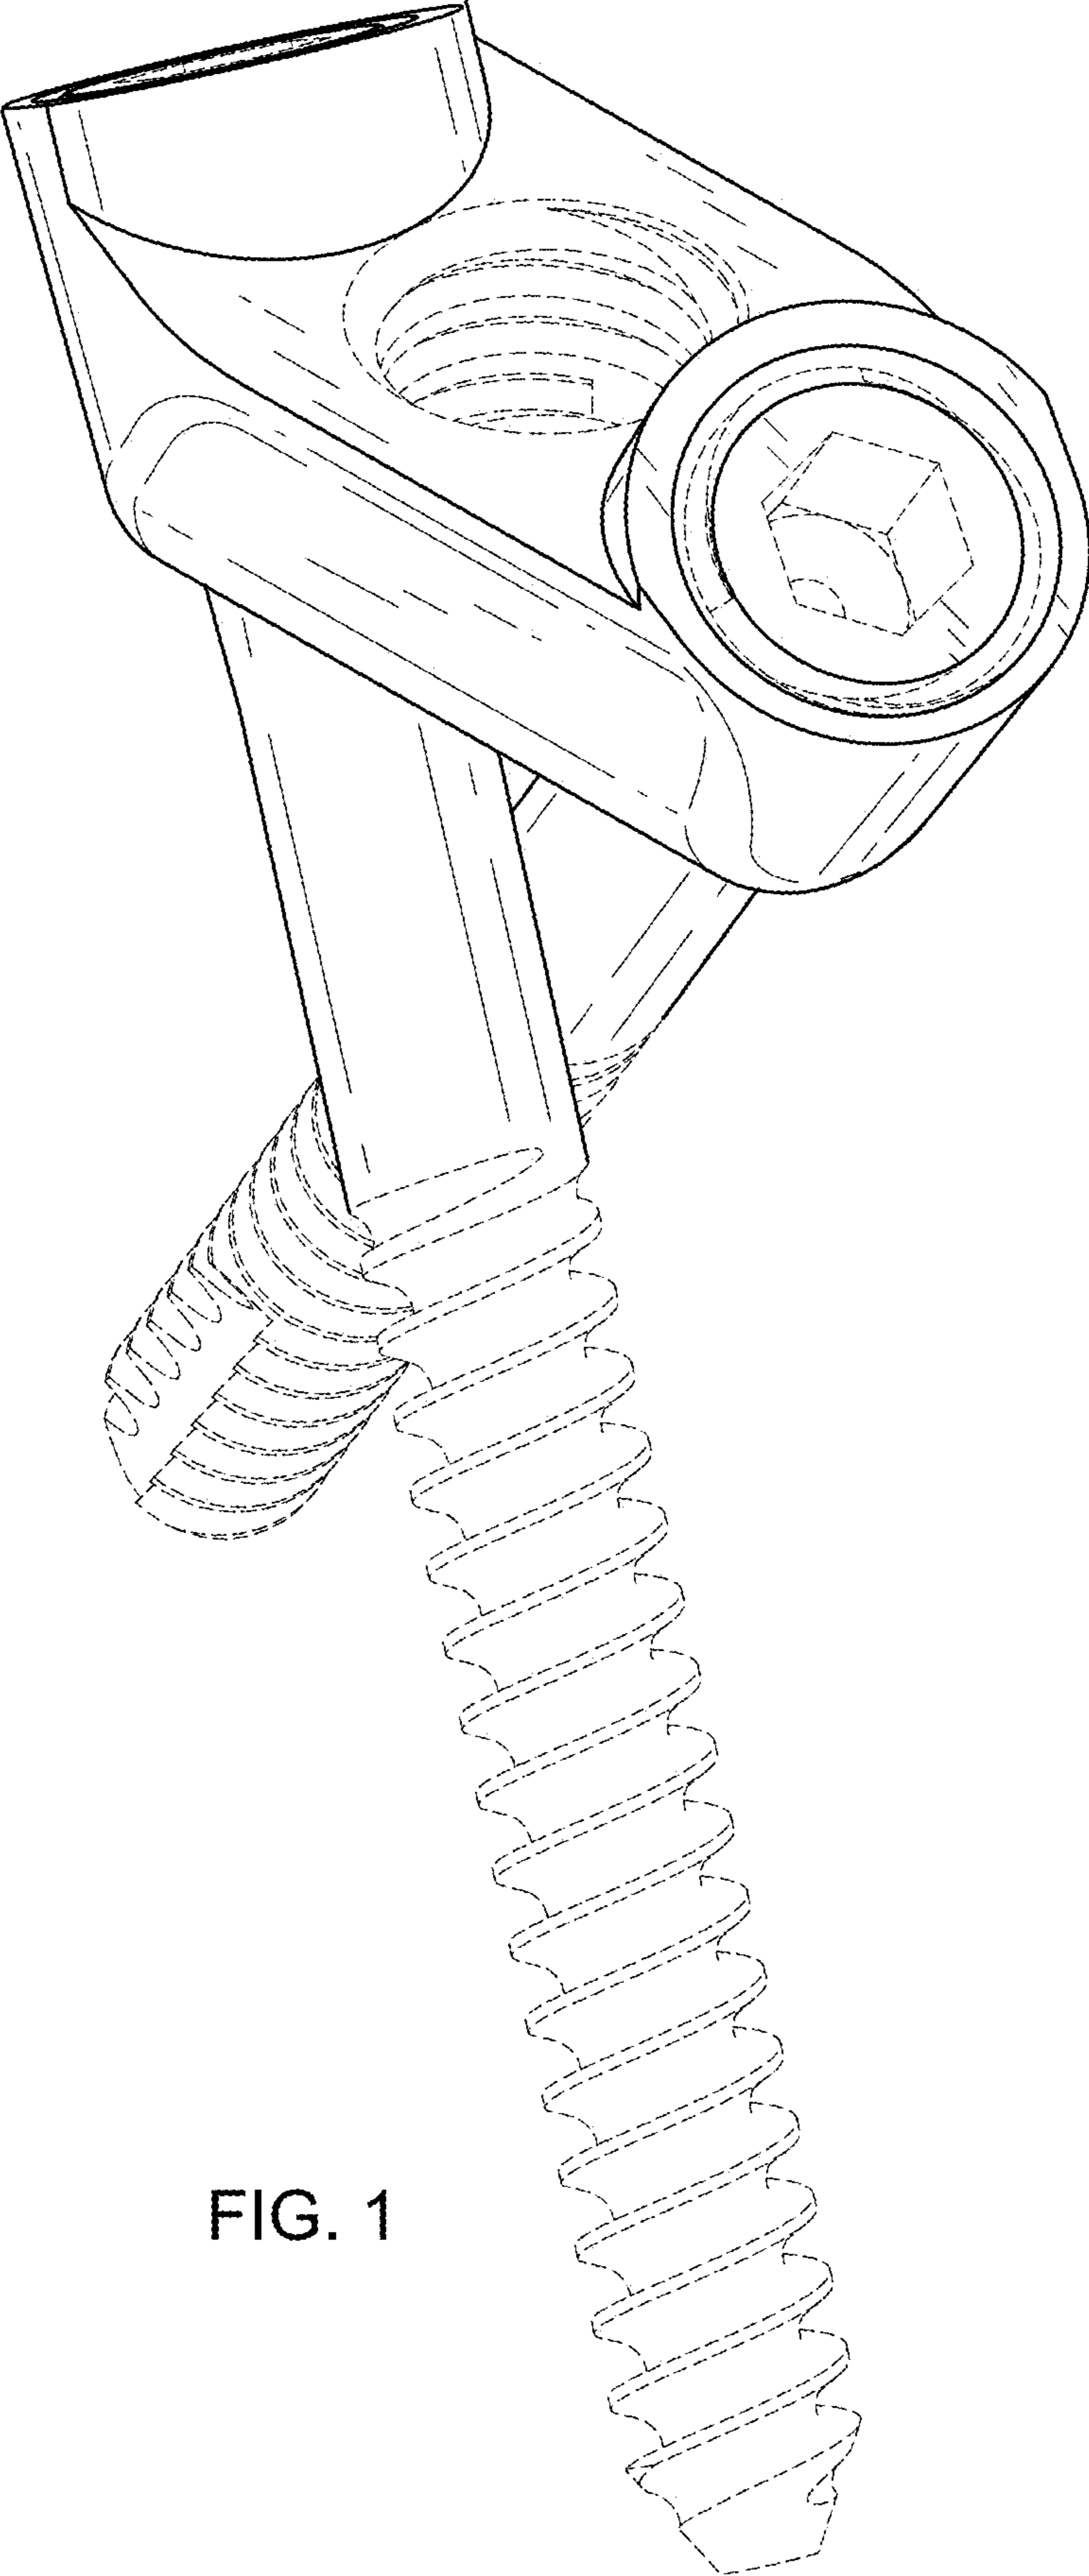


FIG. 1

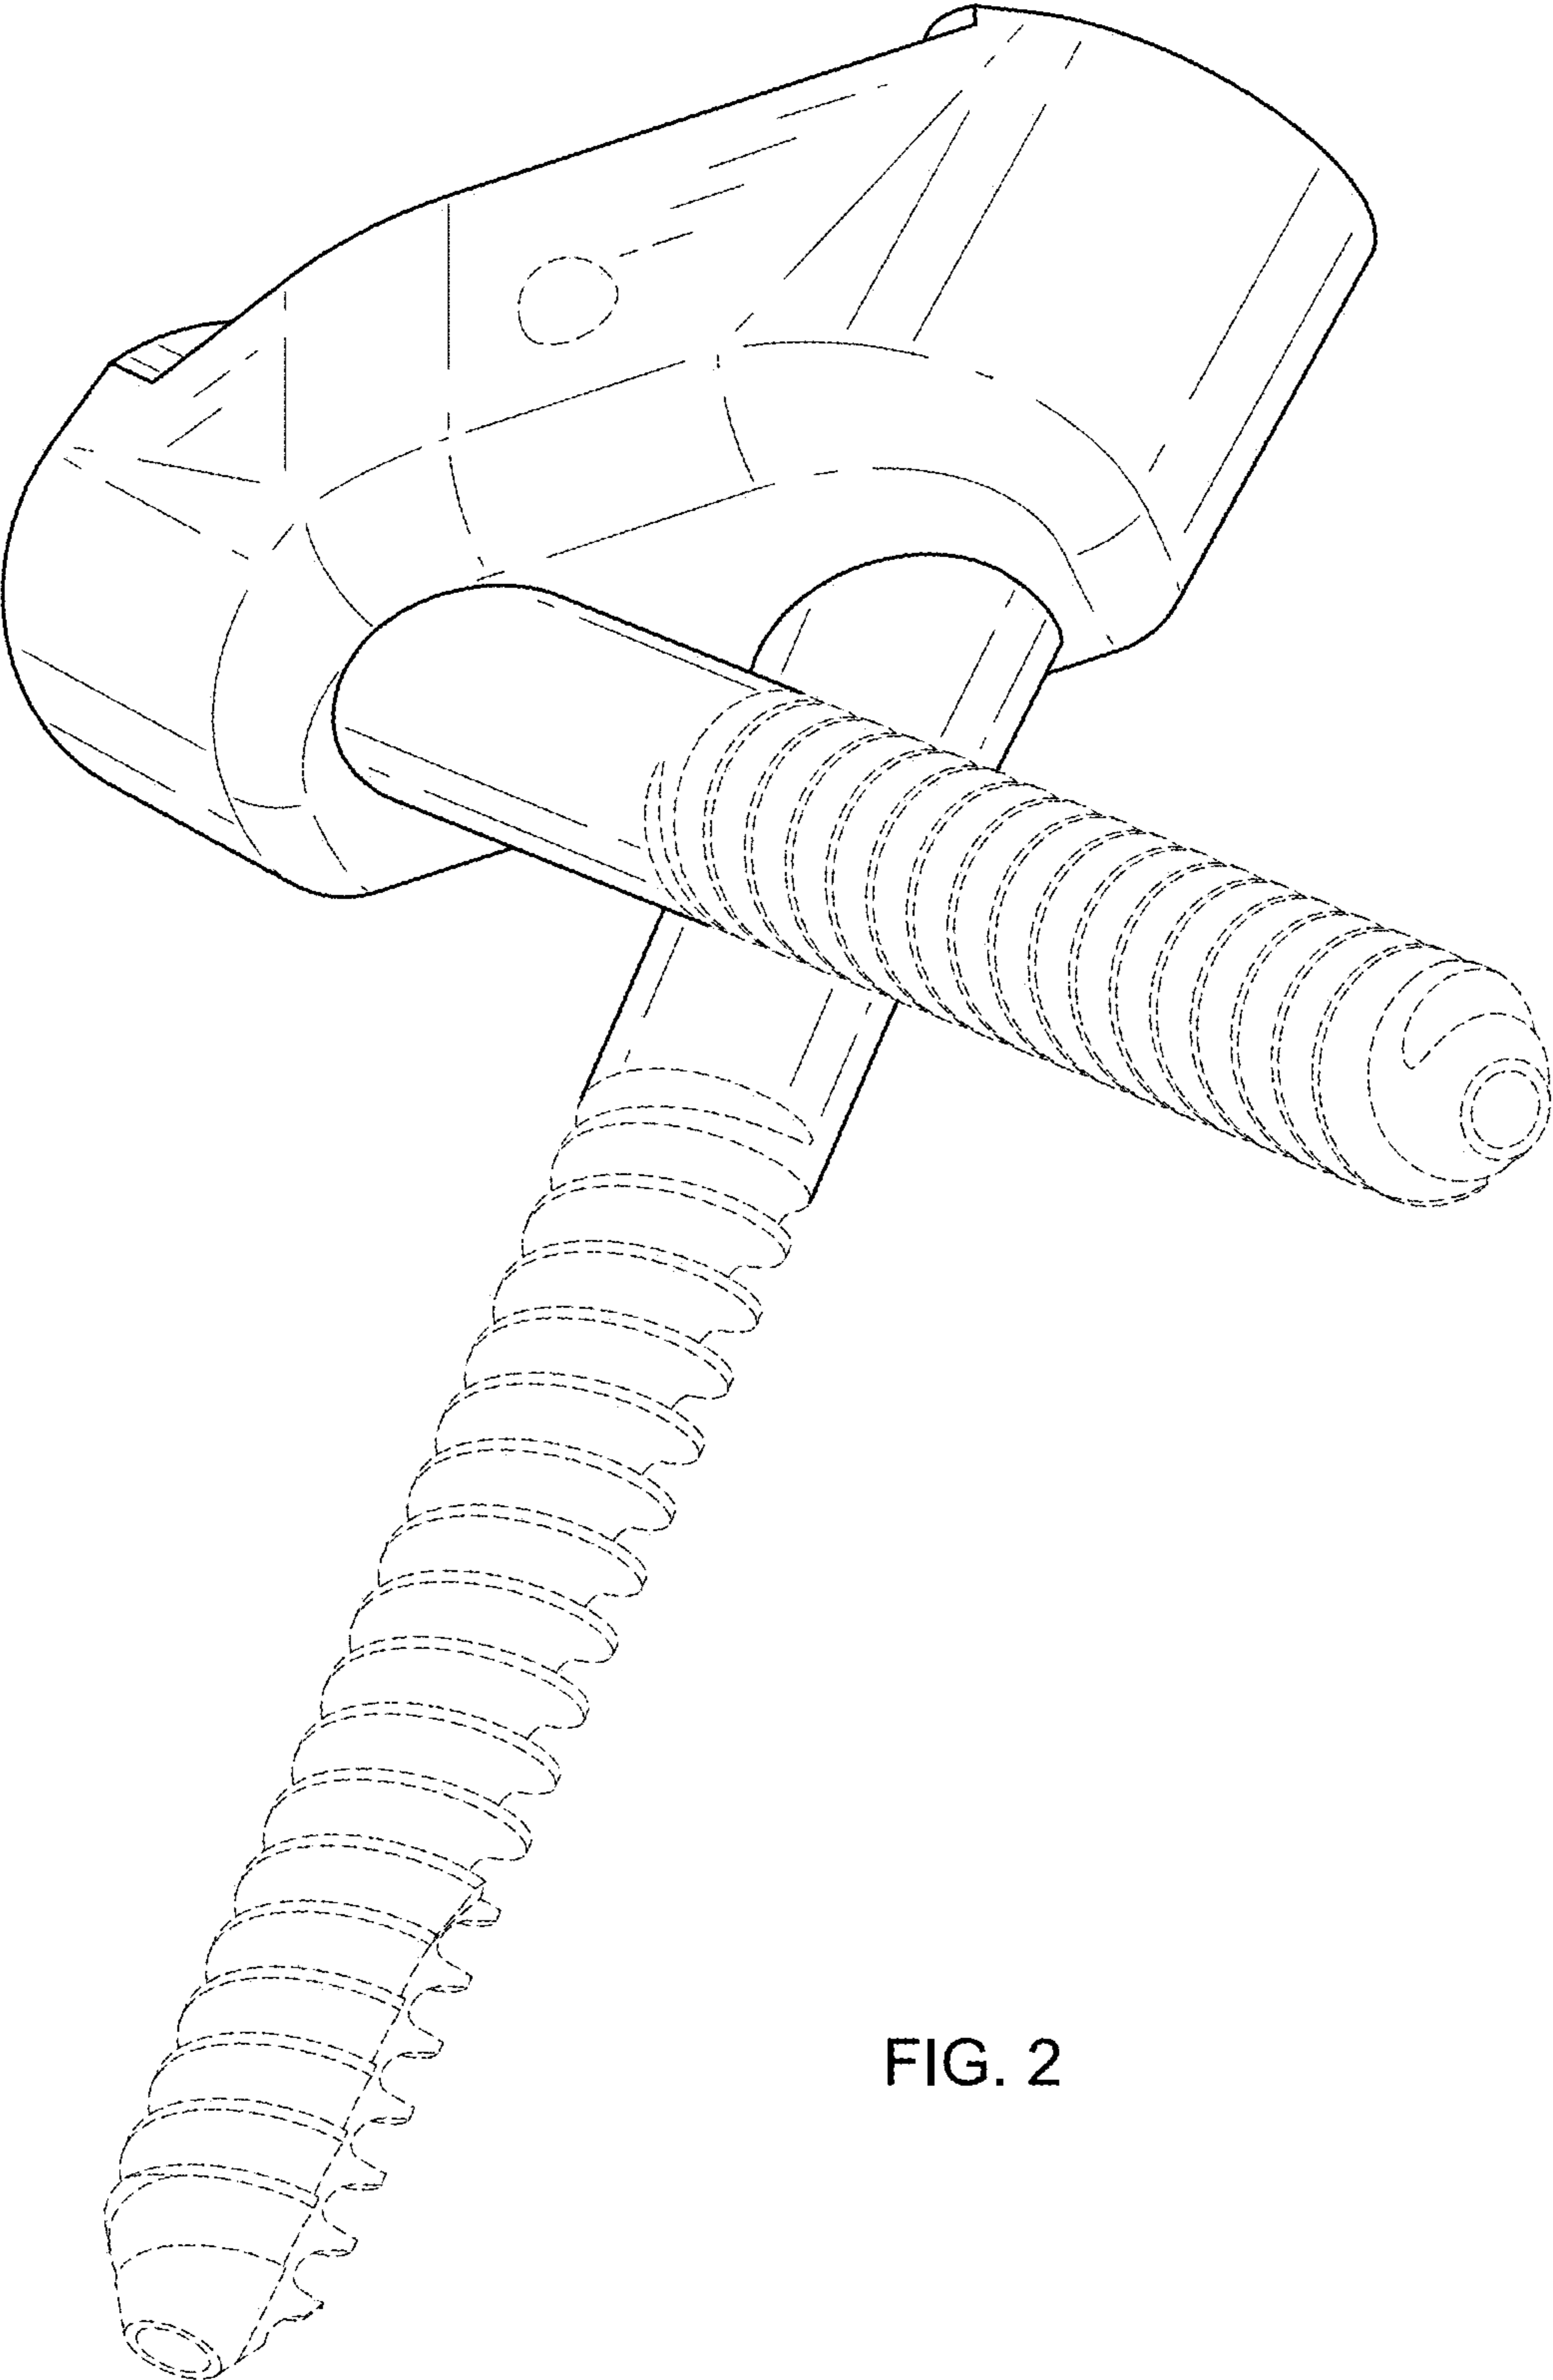


FIG. 2

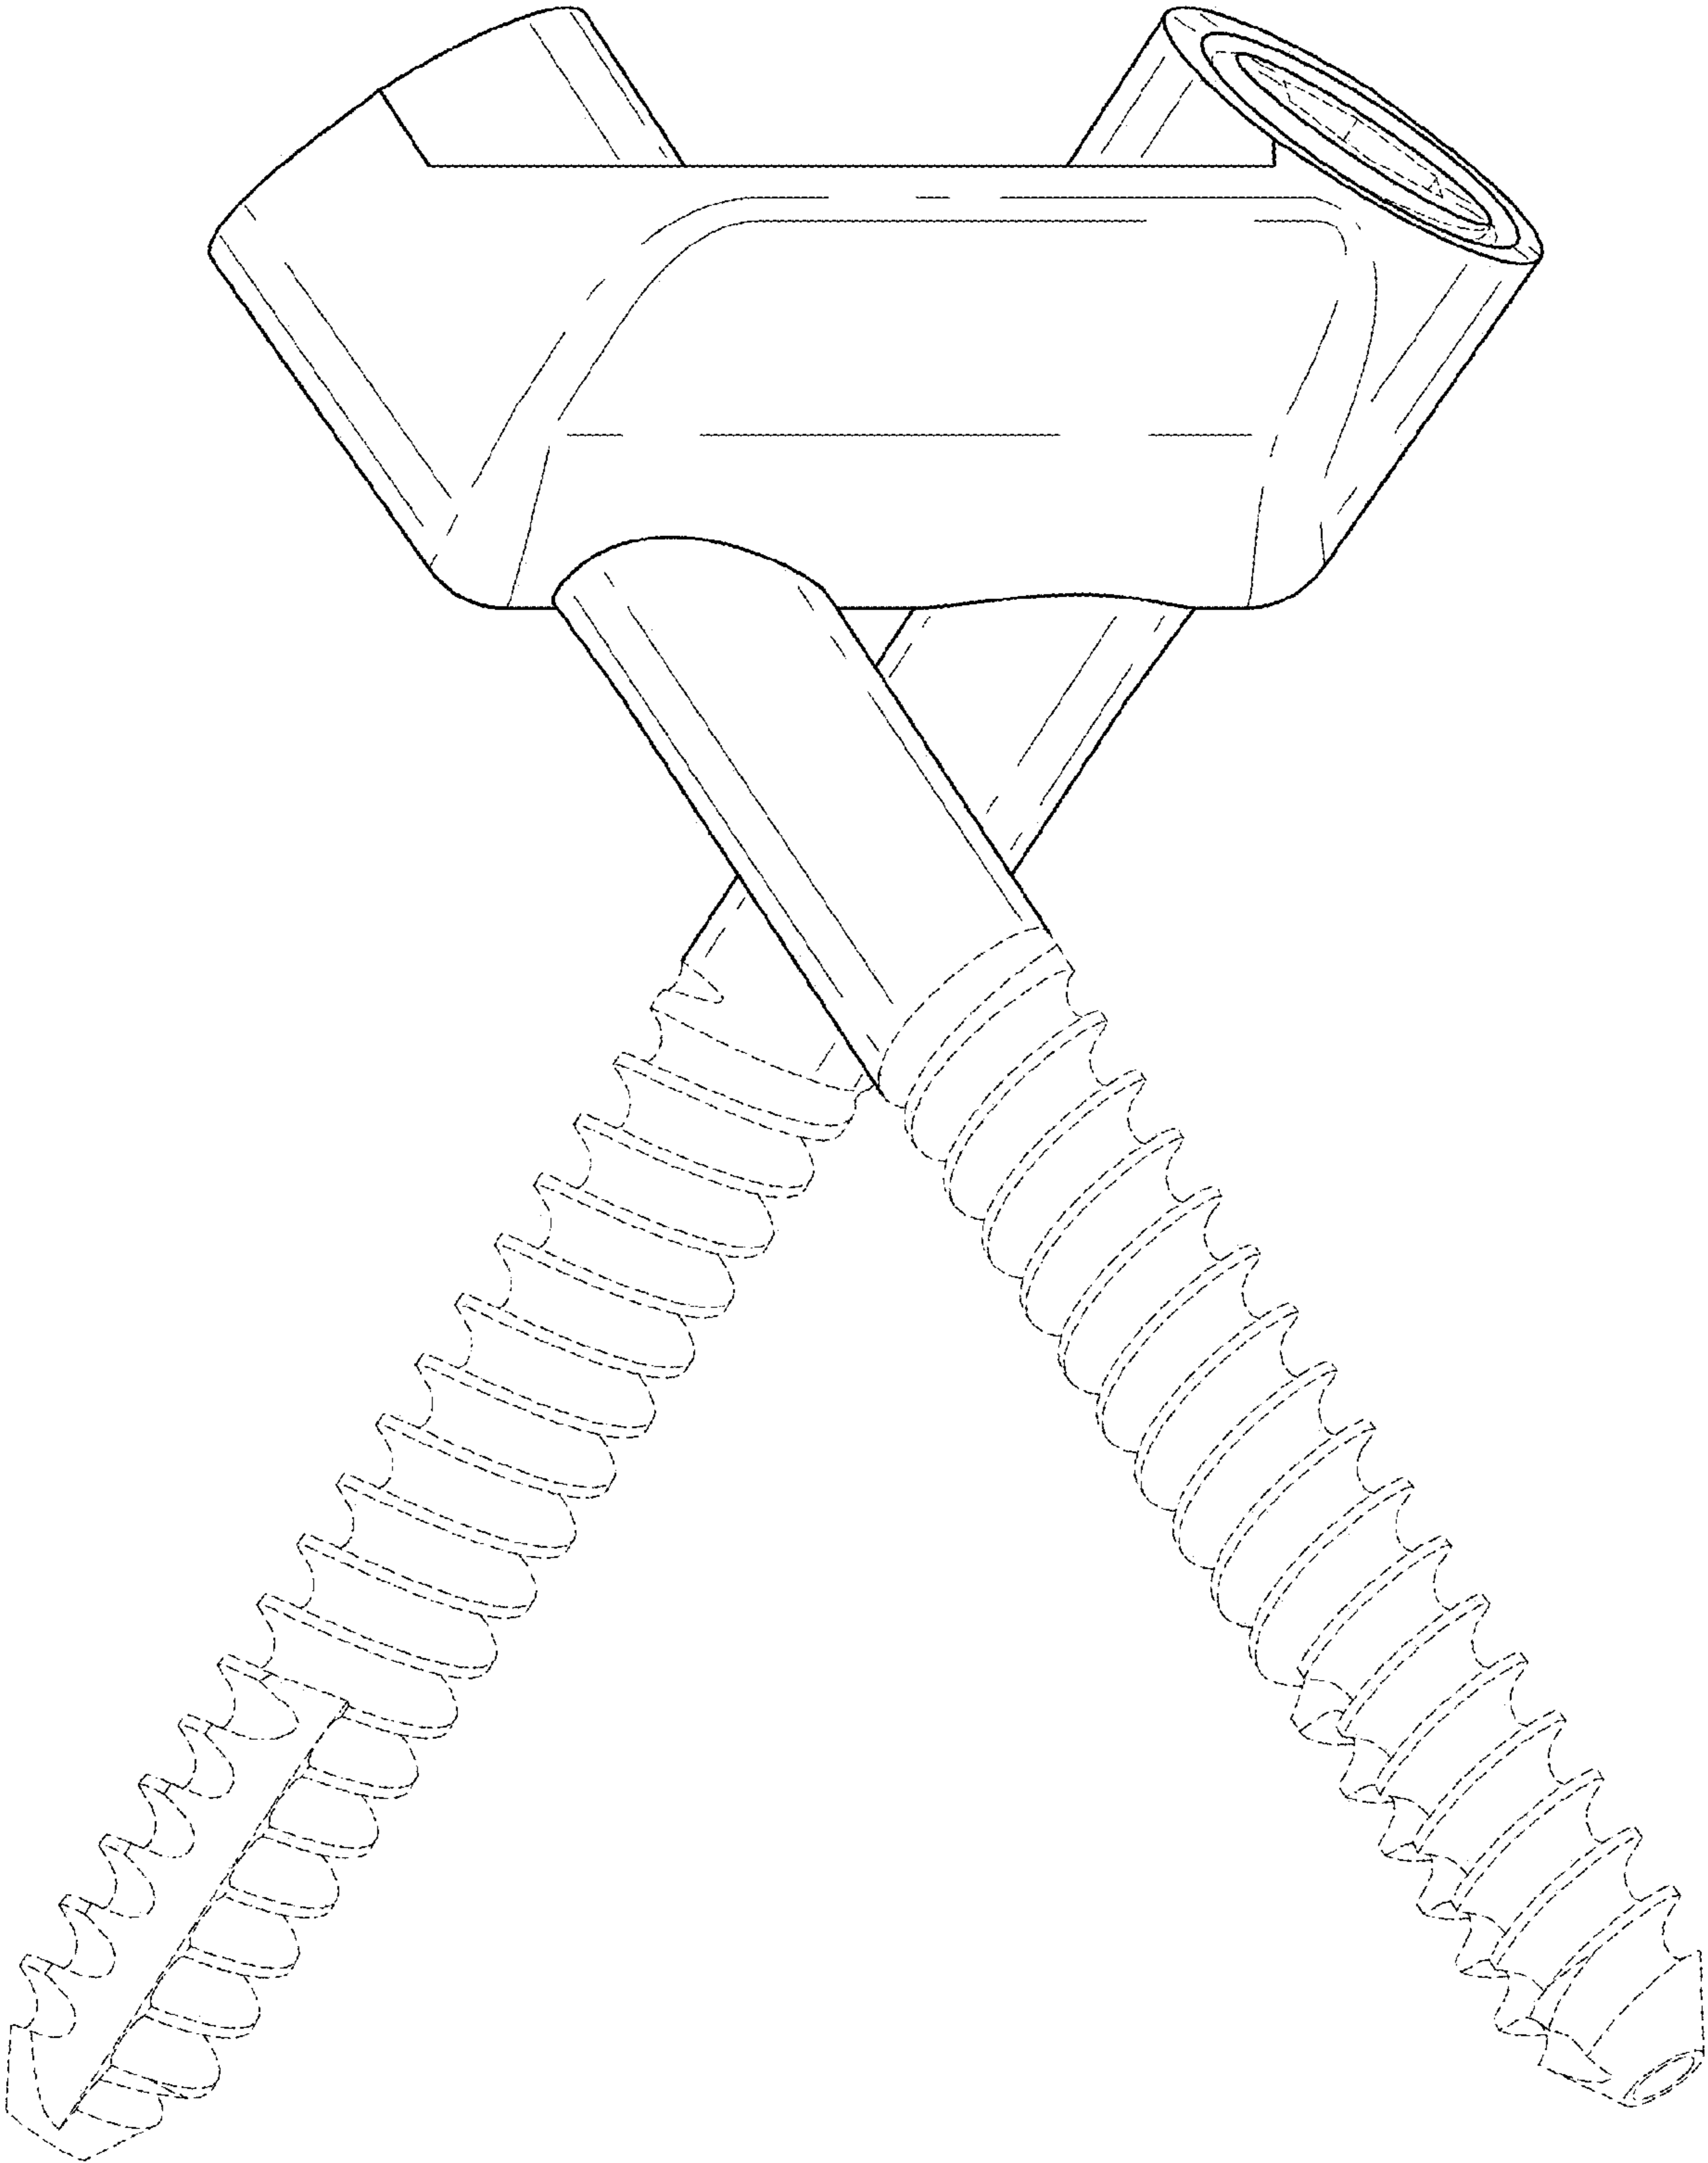


FIG. 3

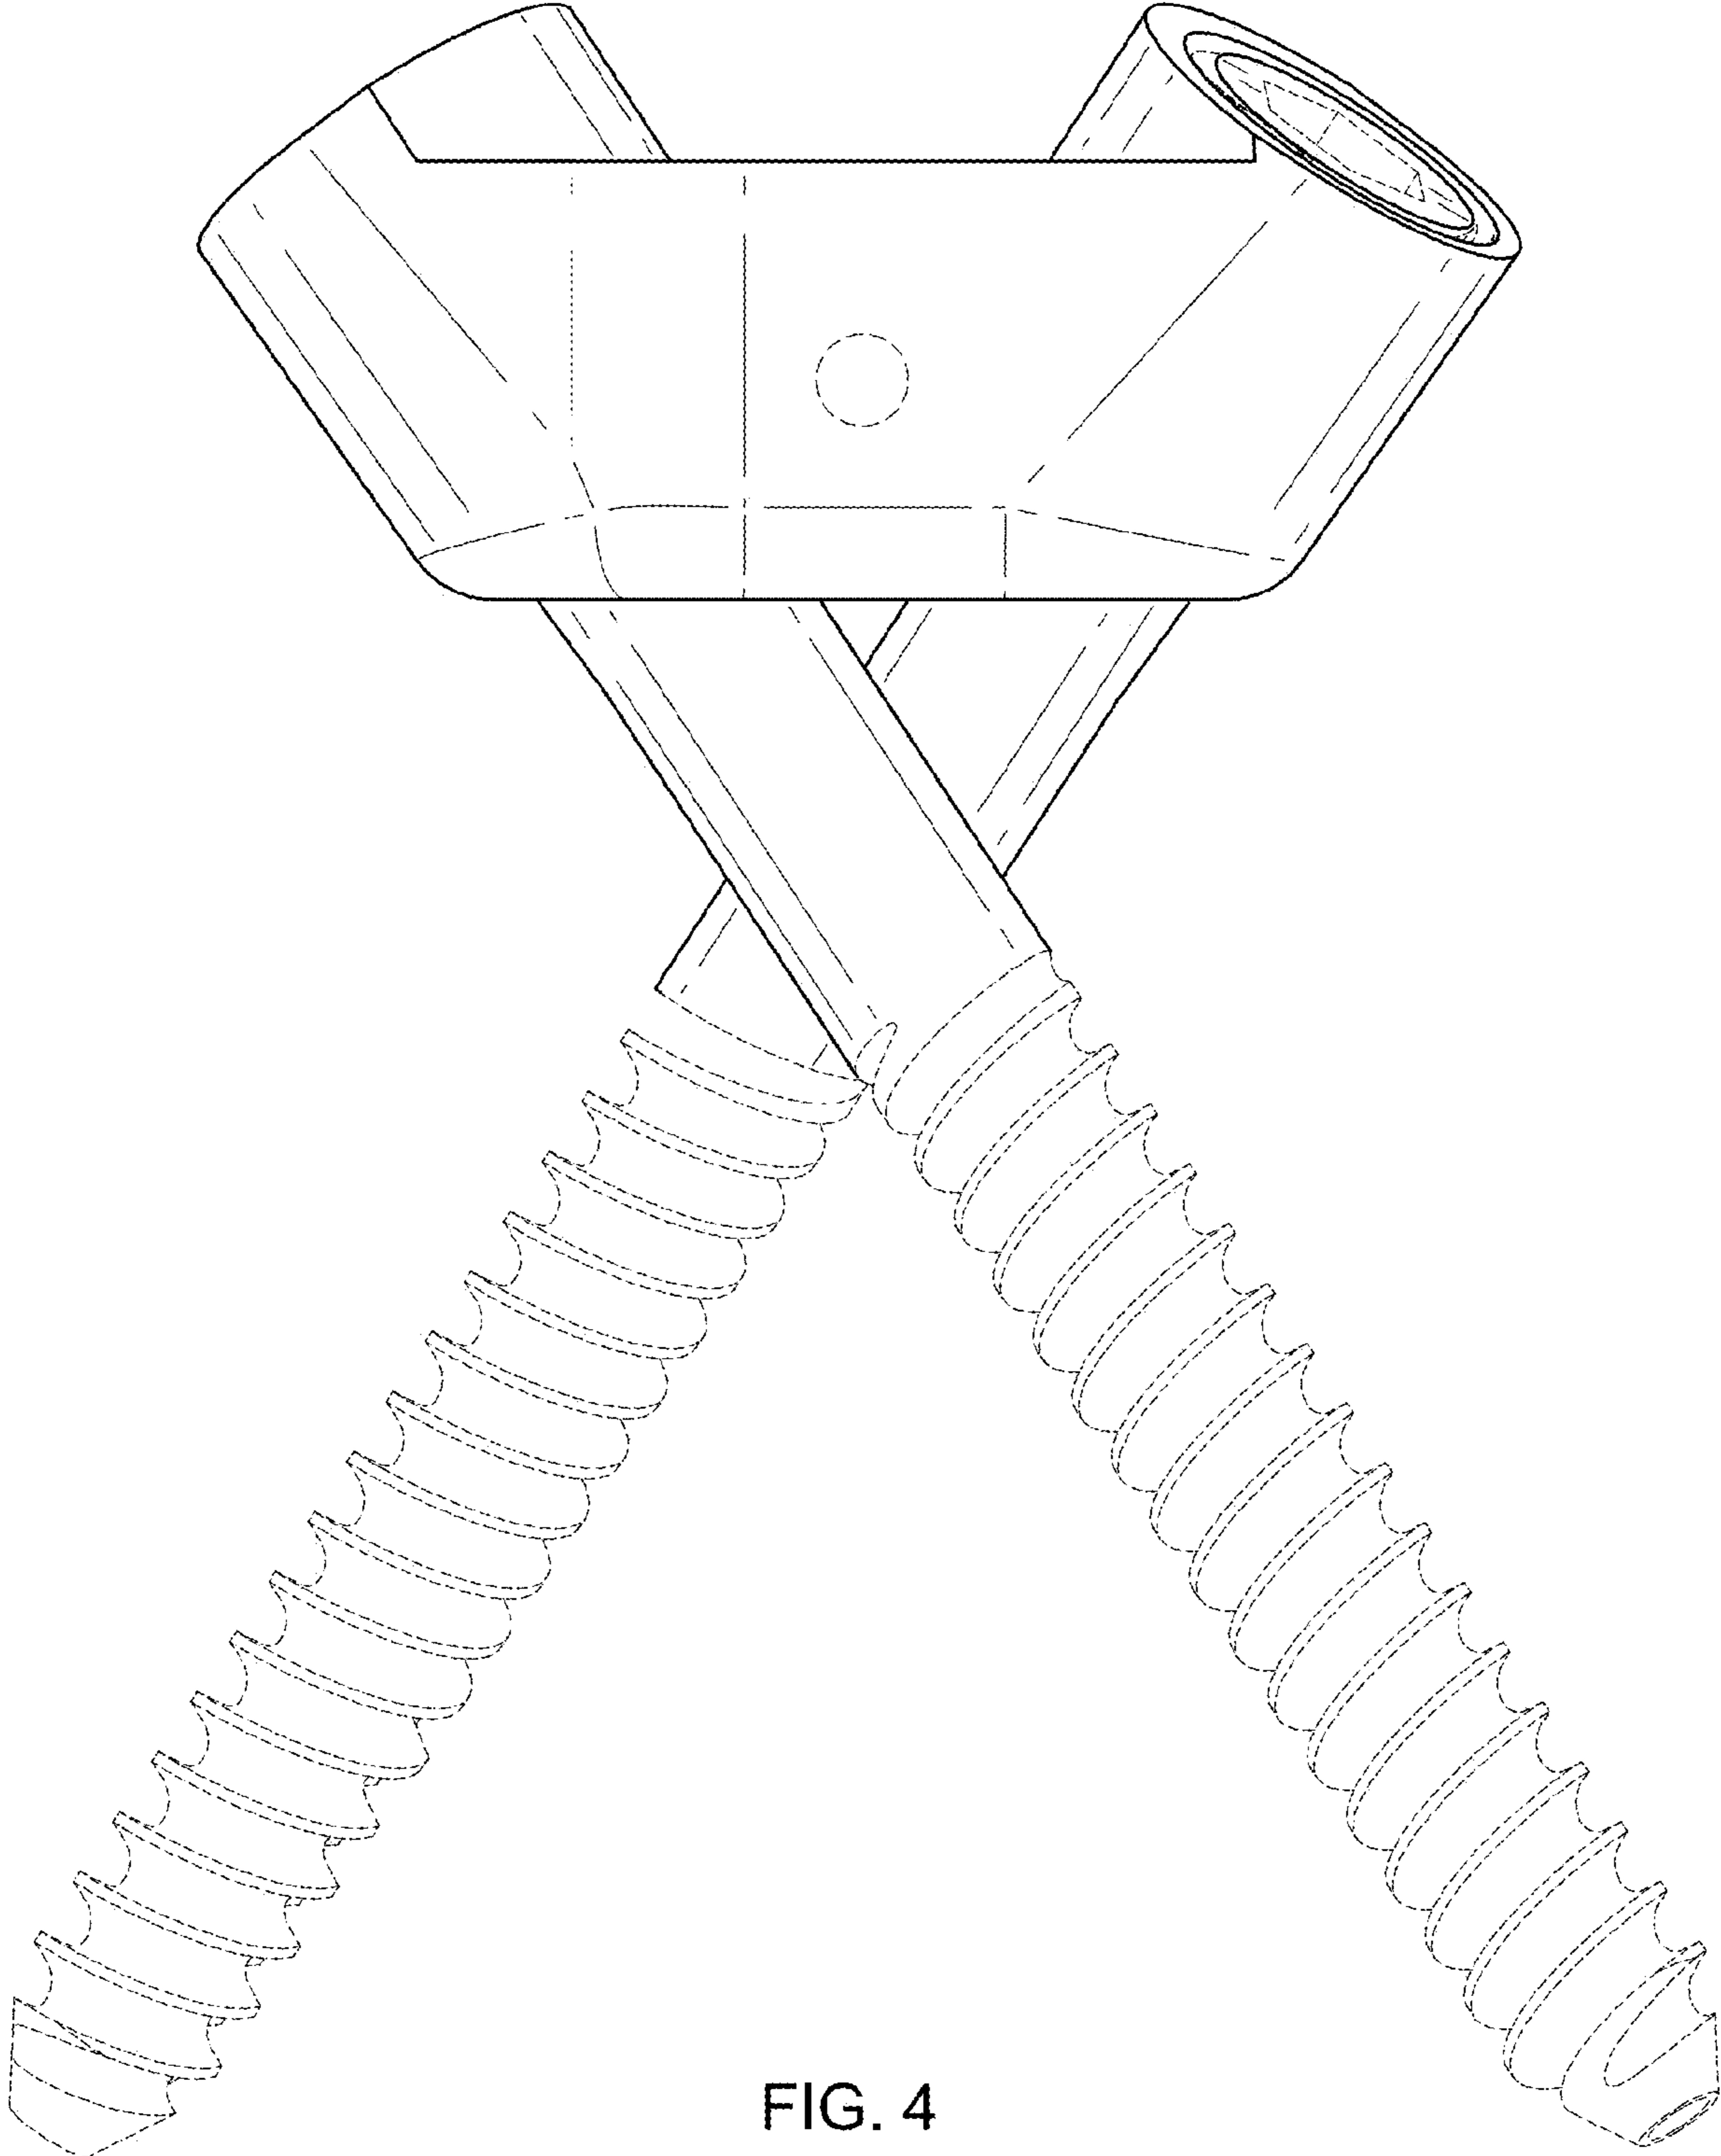


FIG. 4

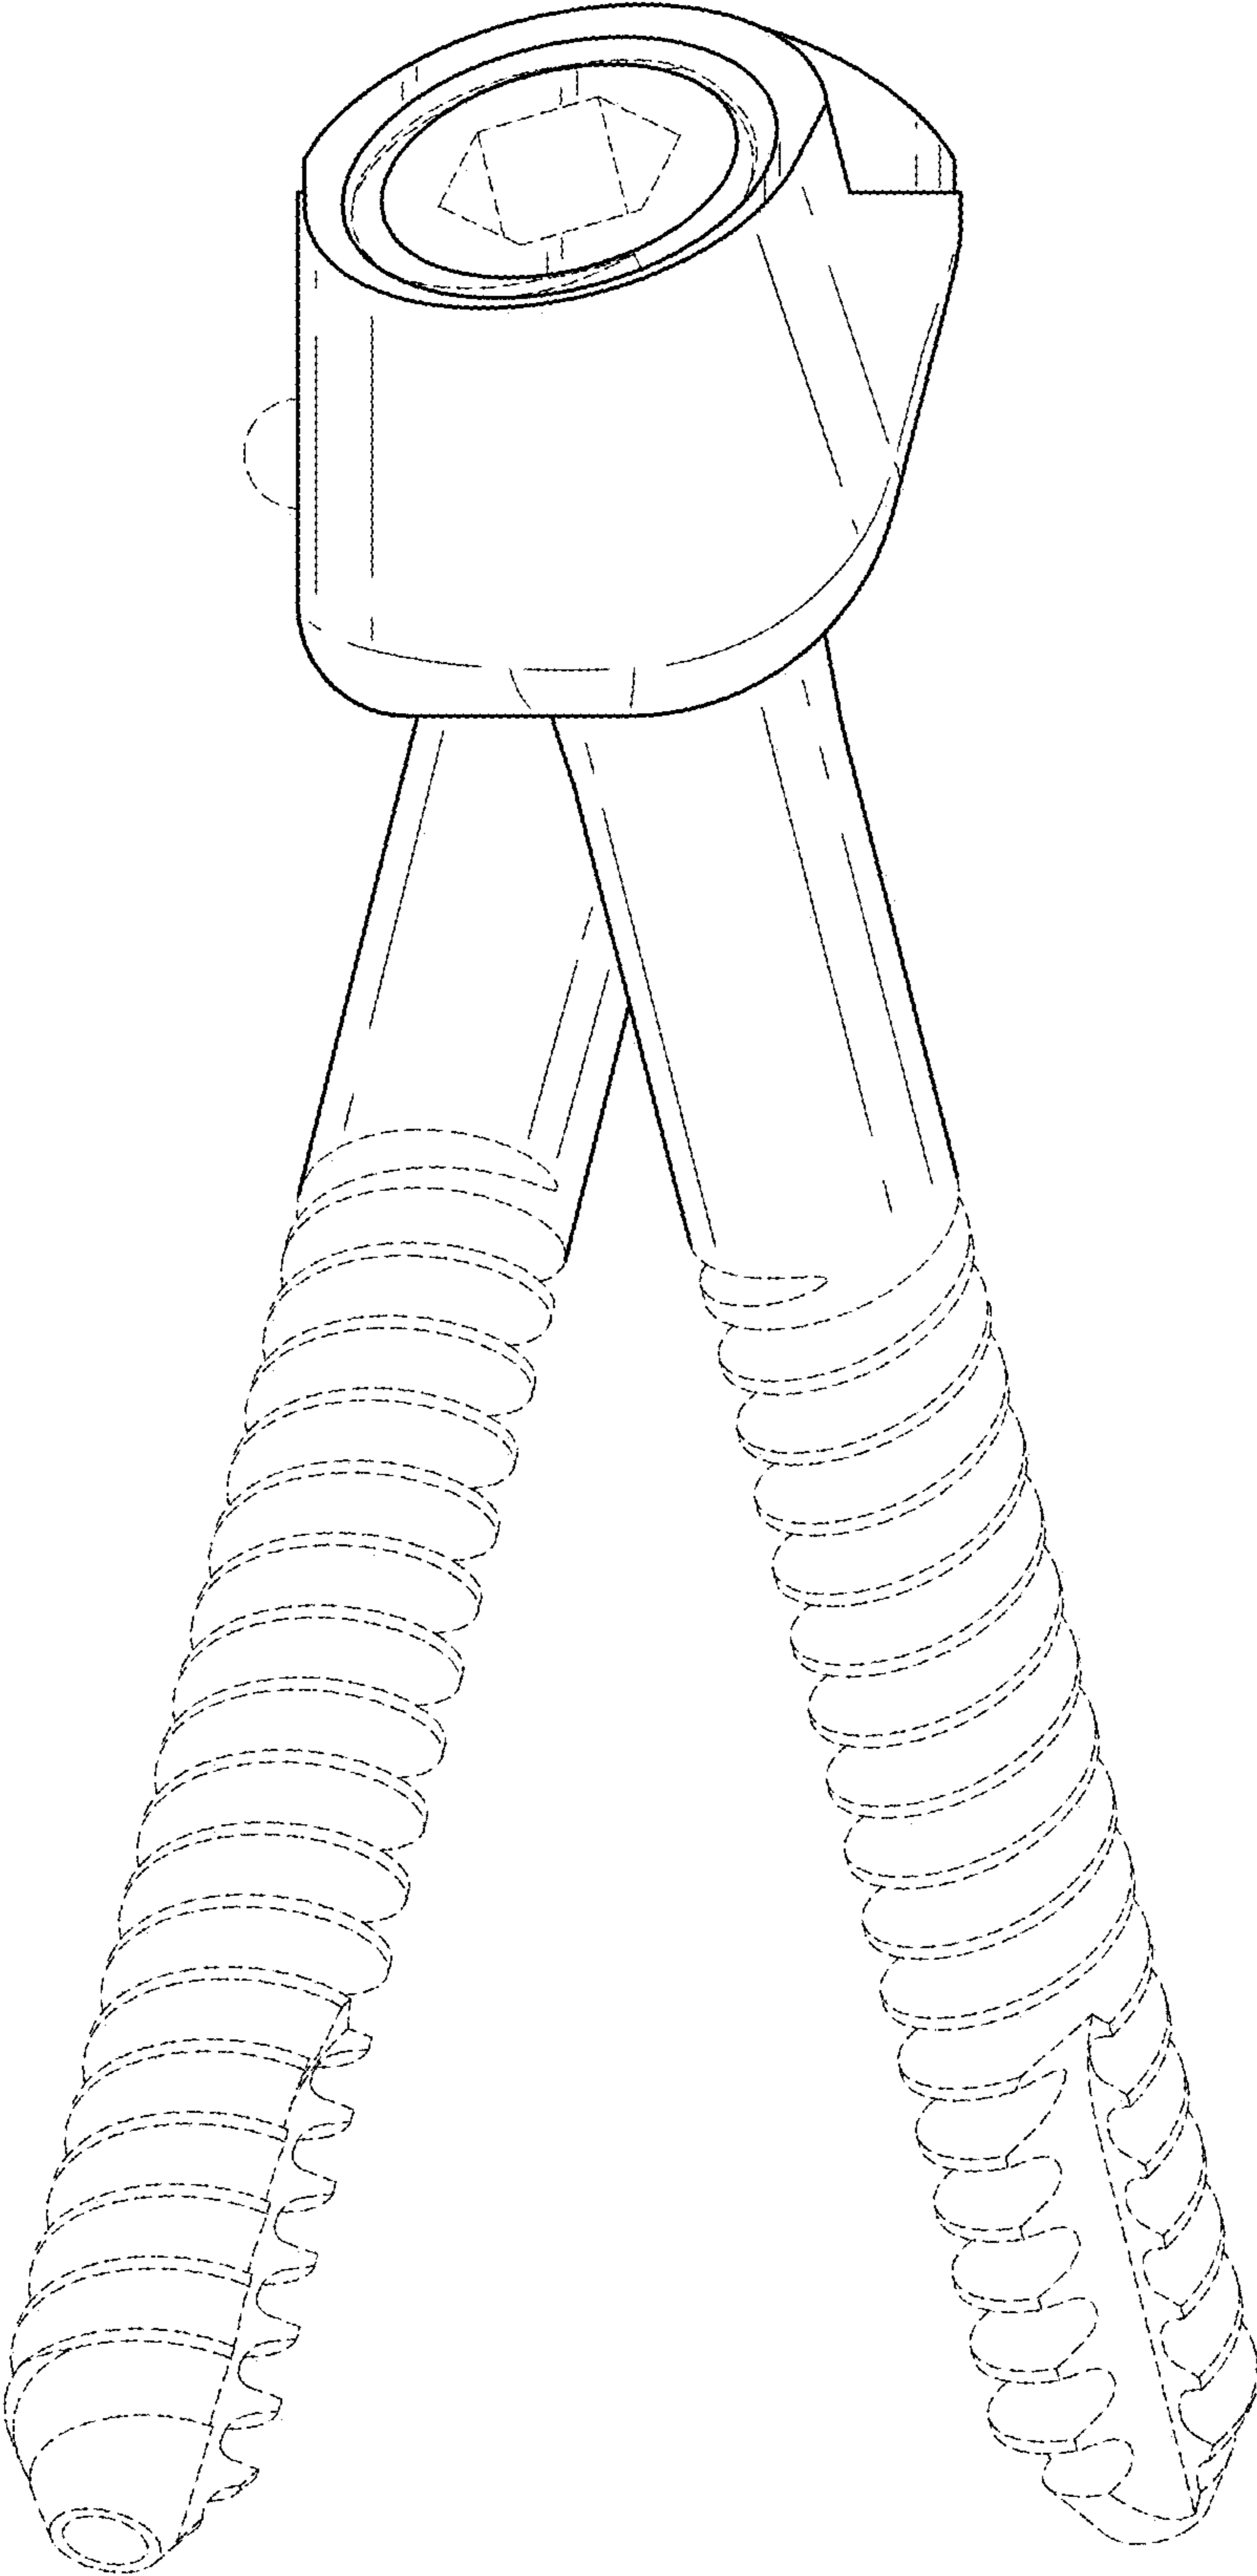


FIG. 5

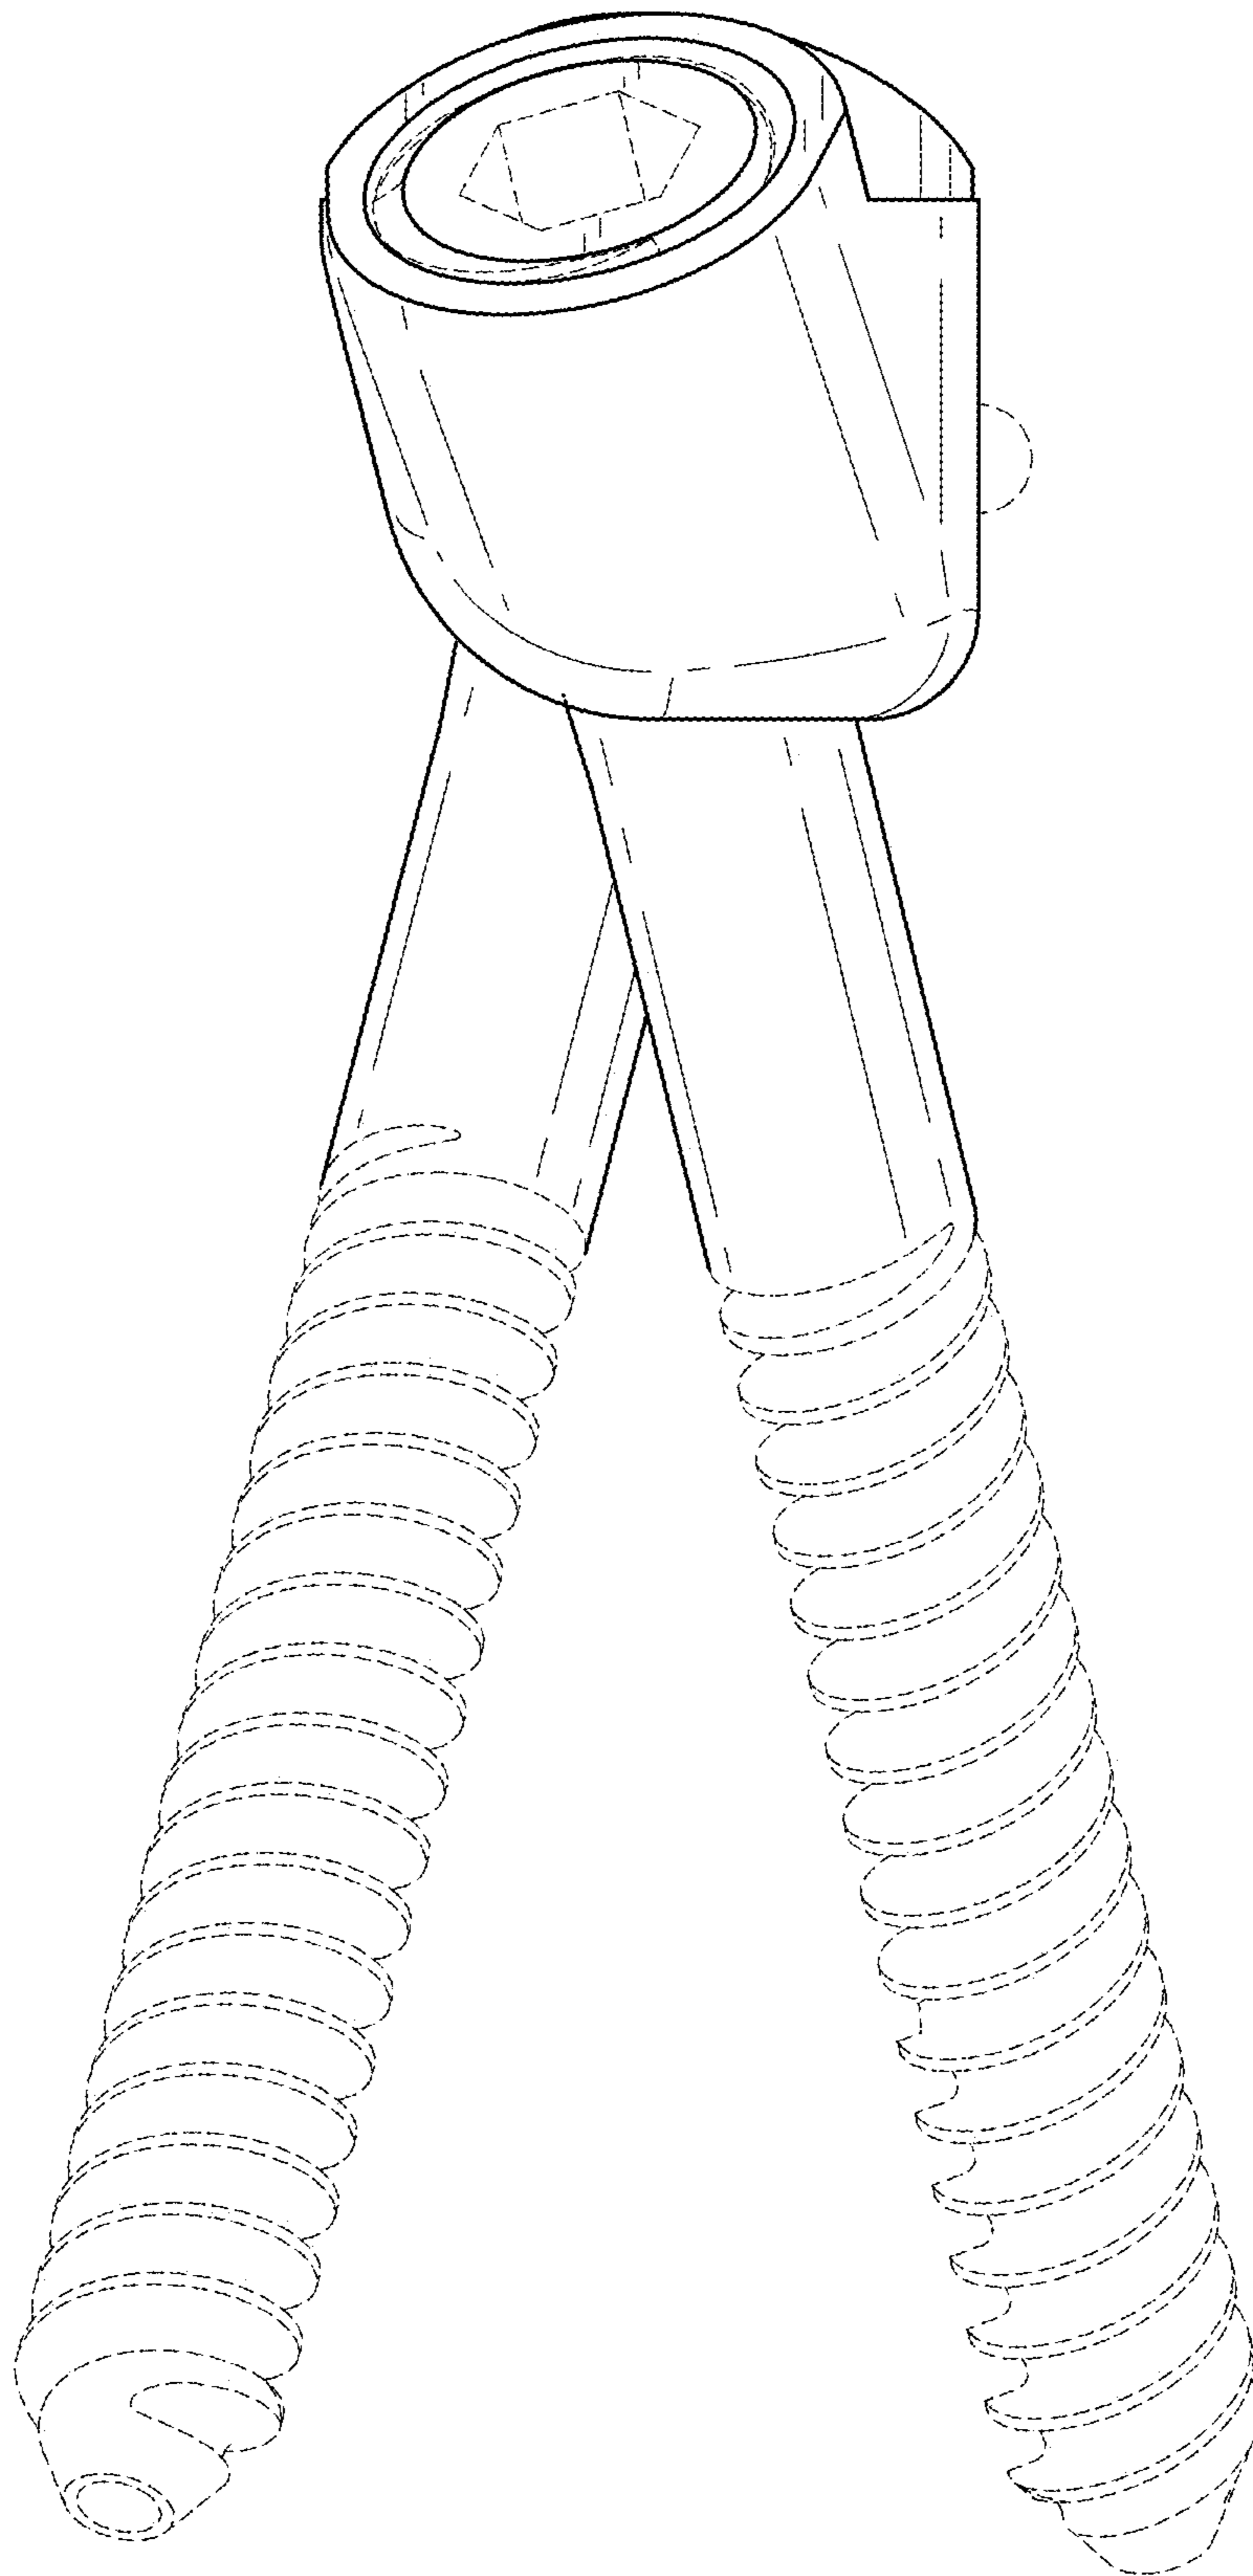


FIG. 6

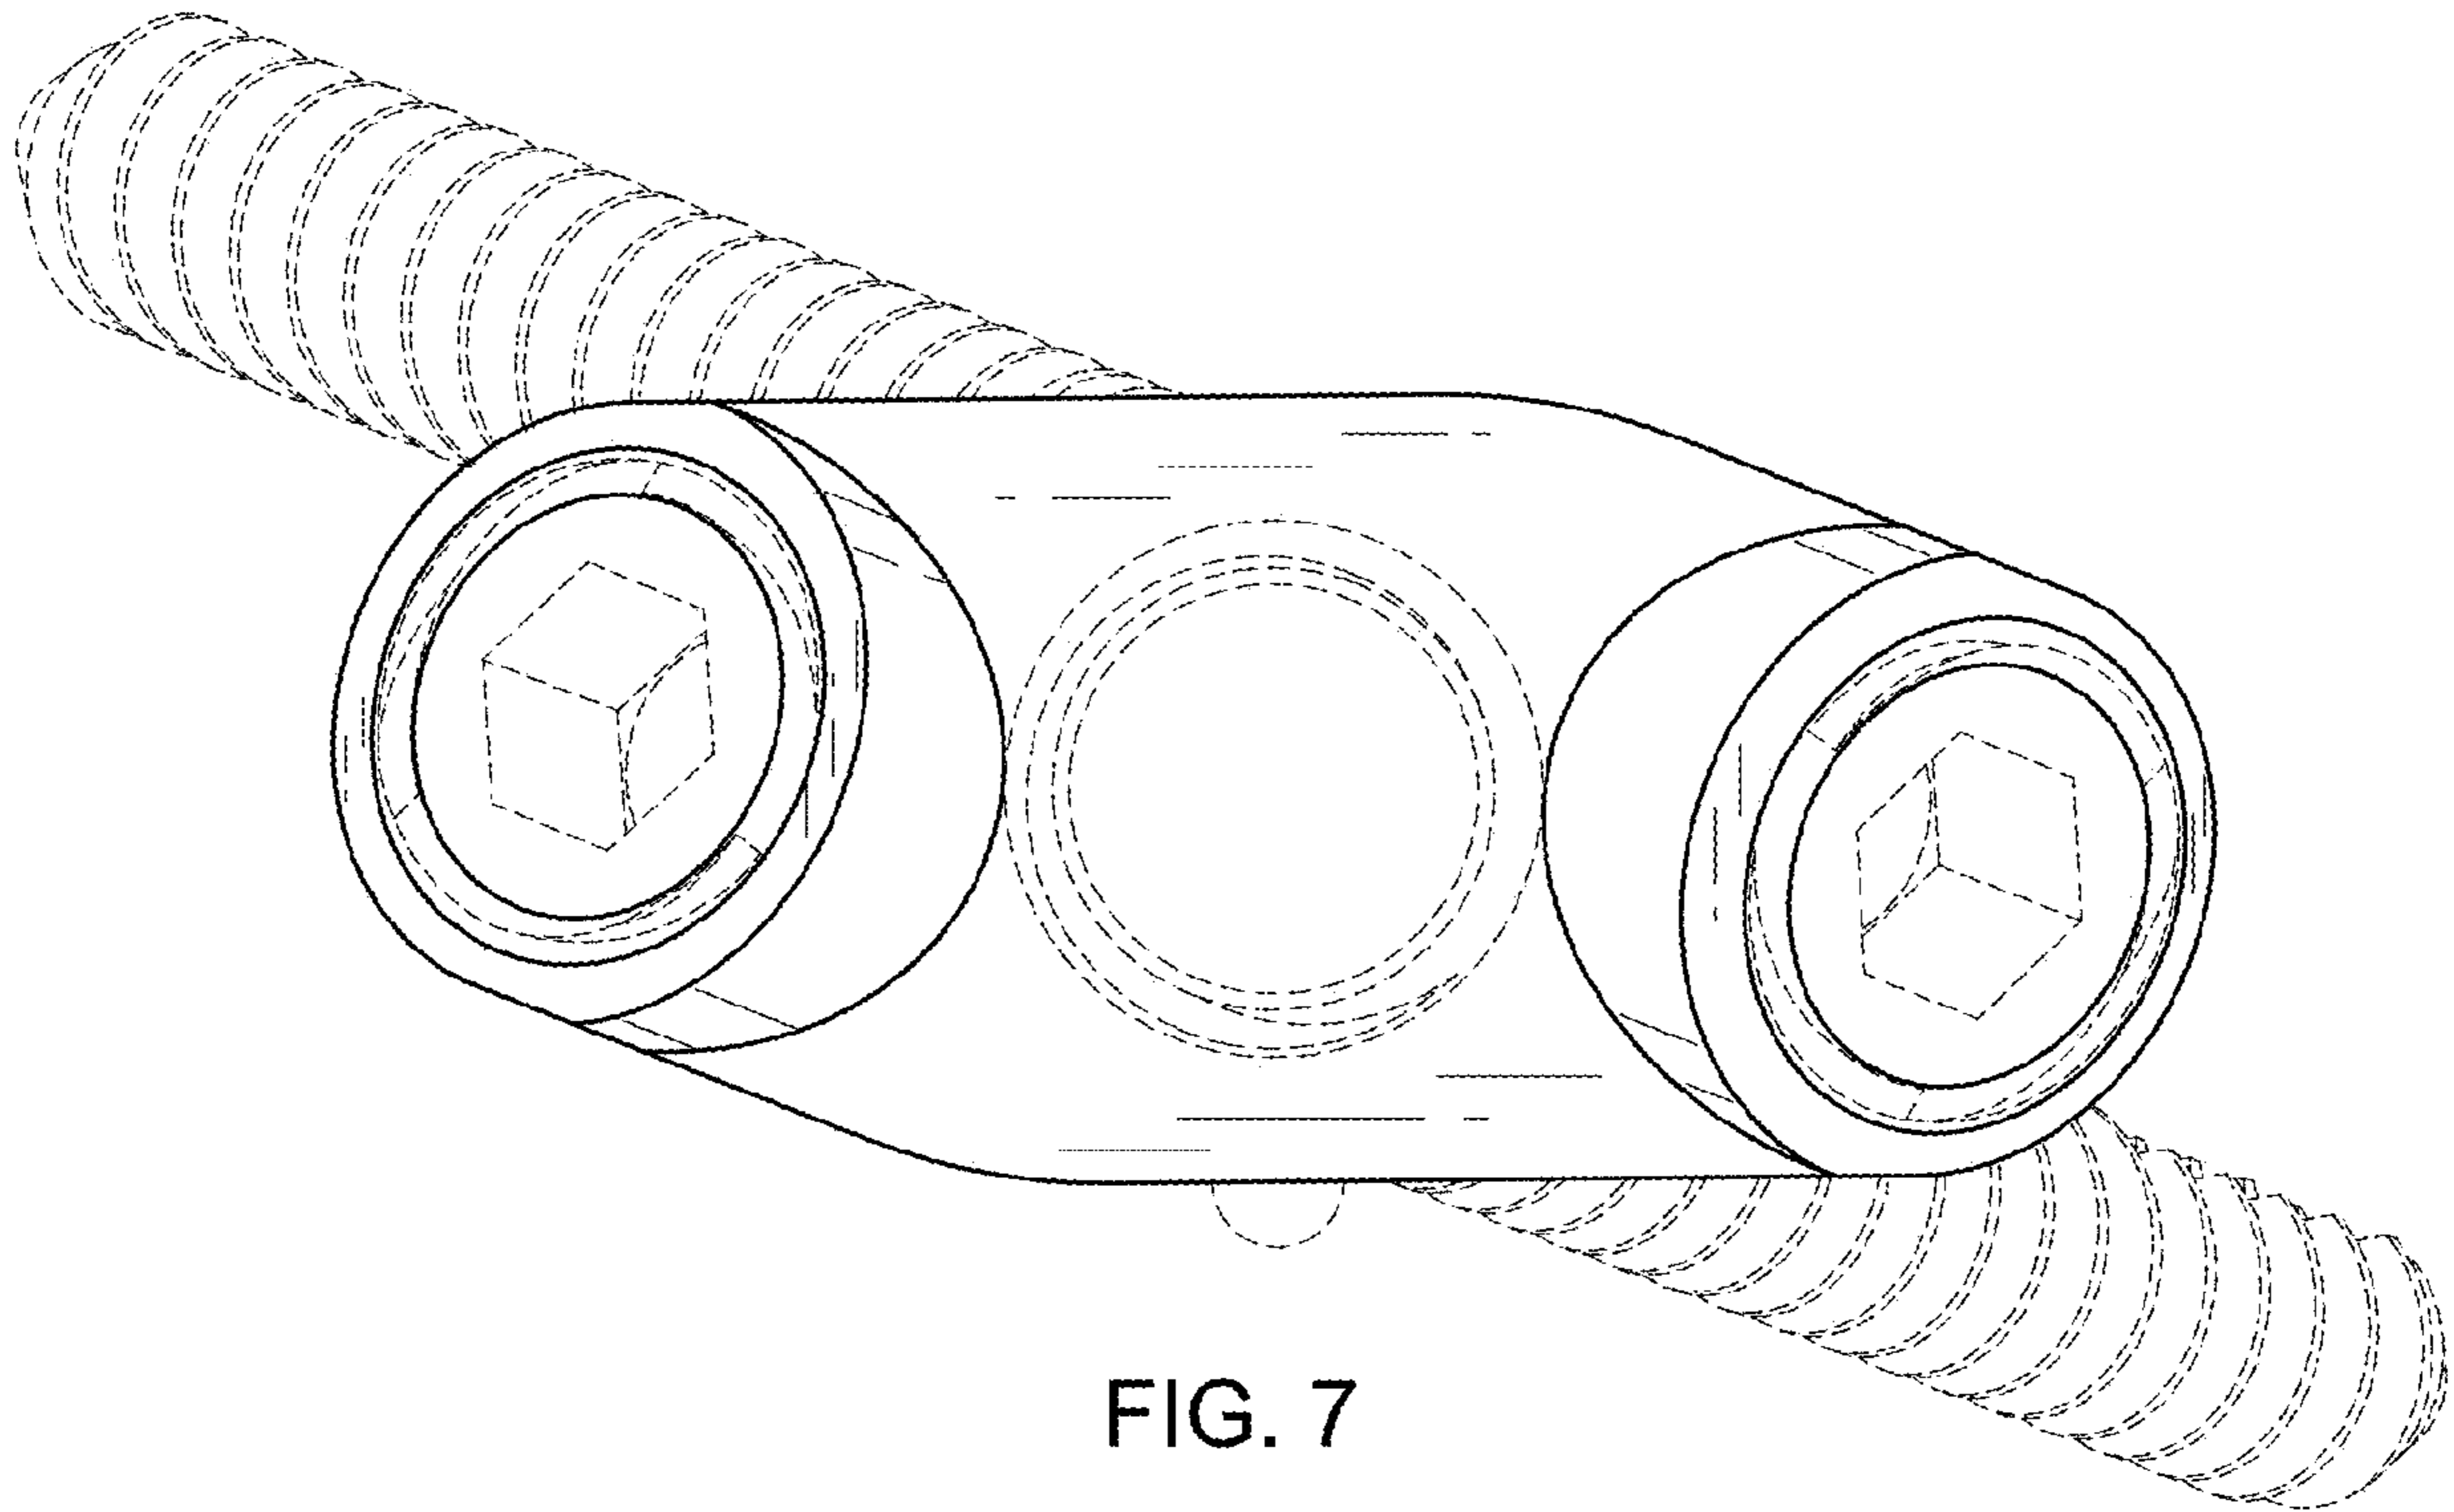


FIG. 7

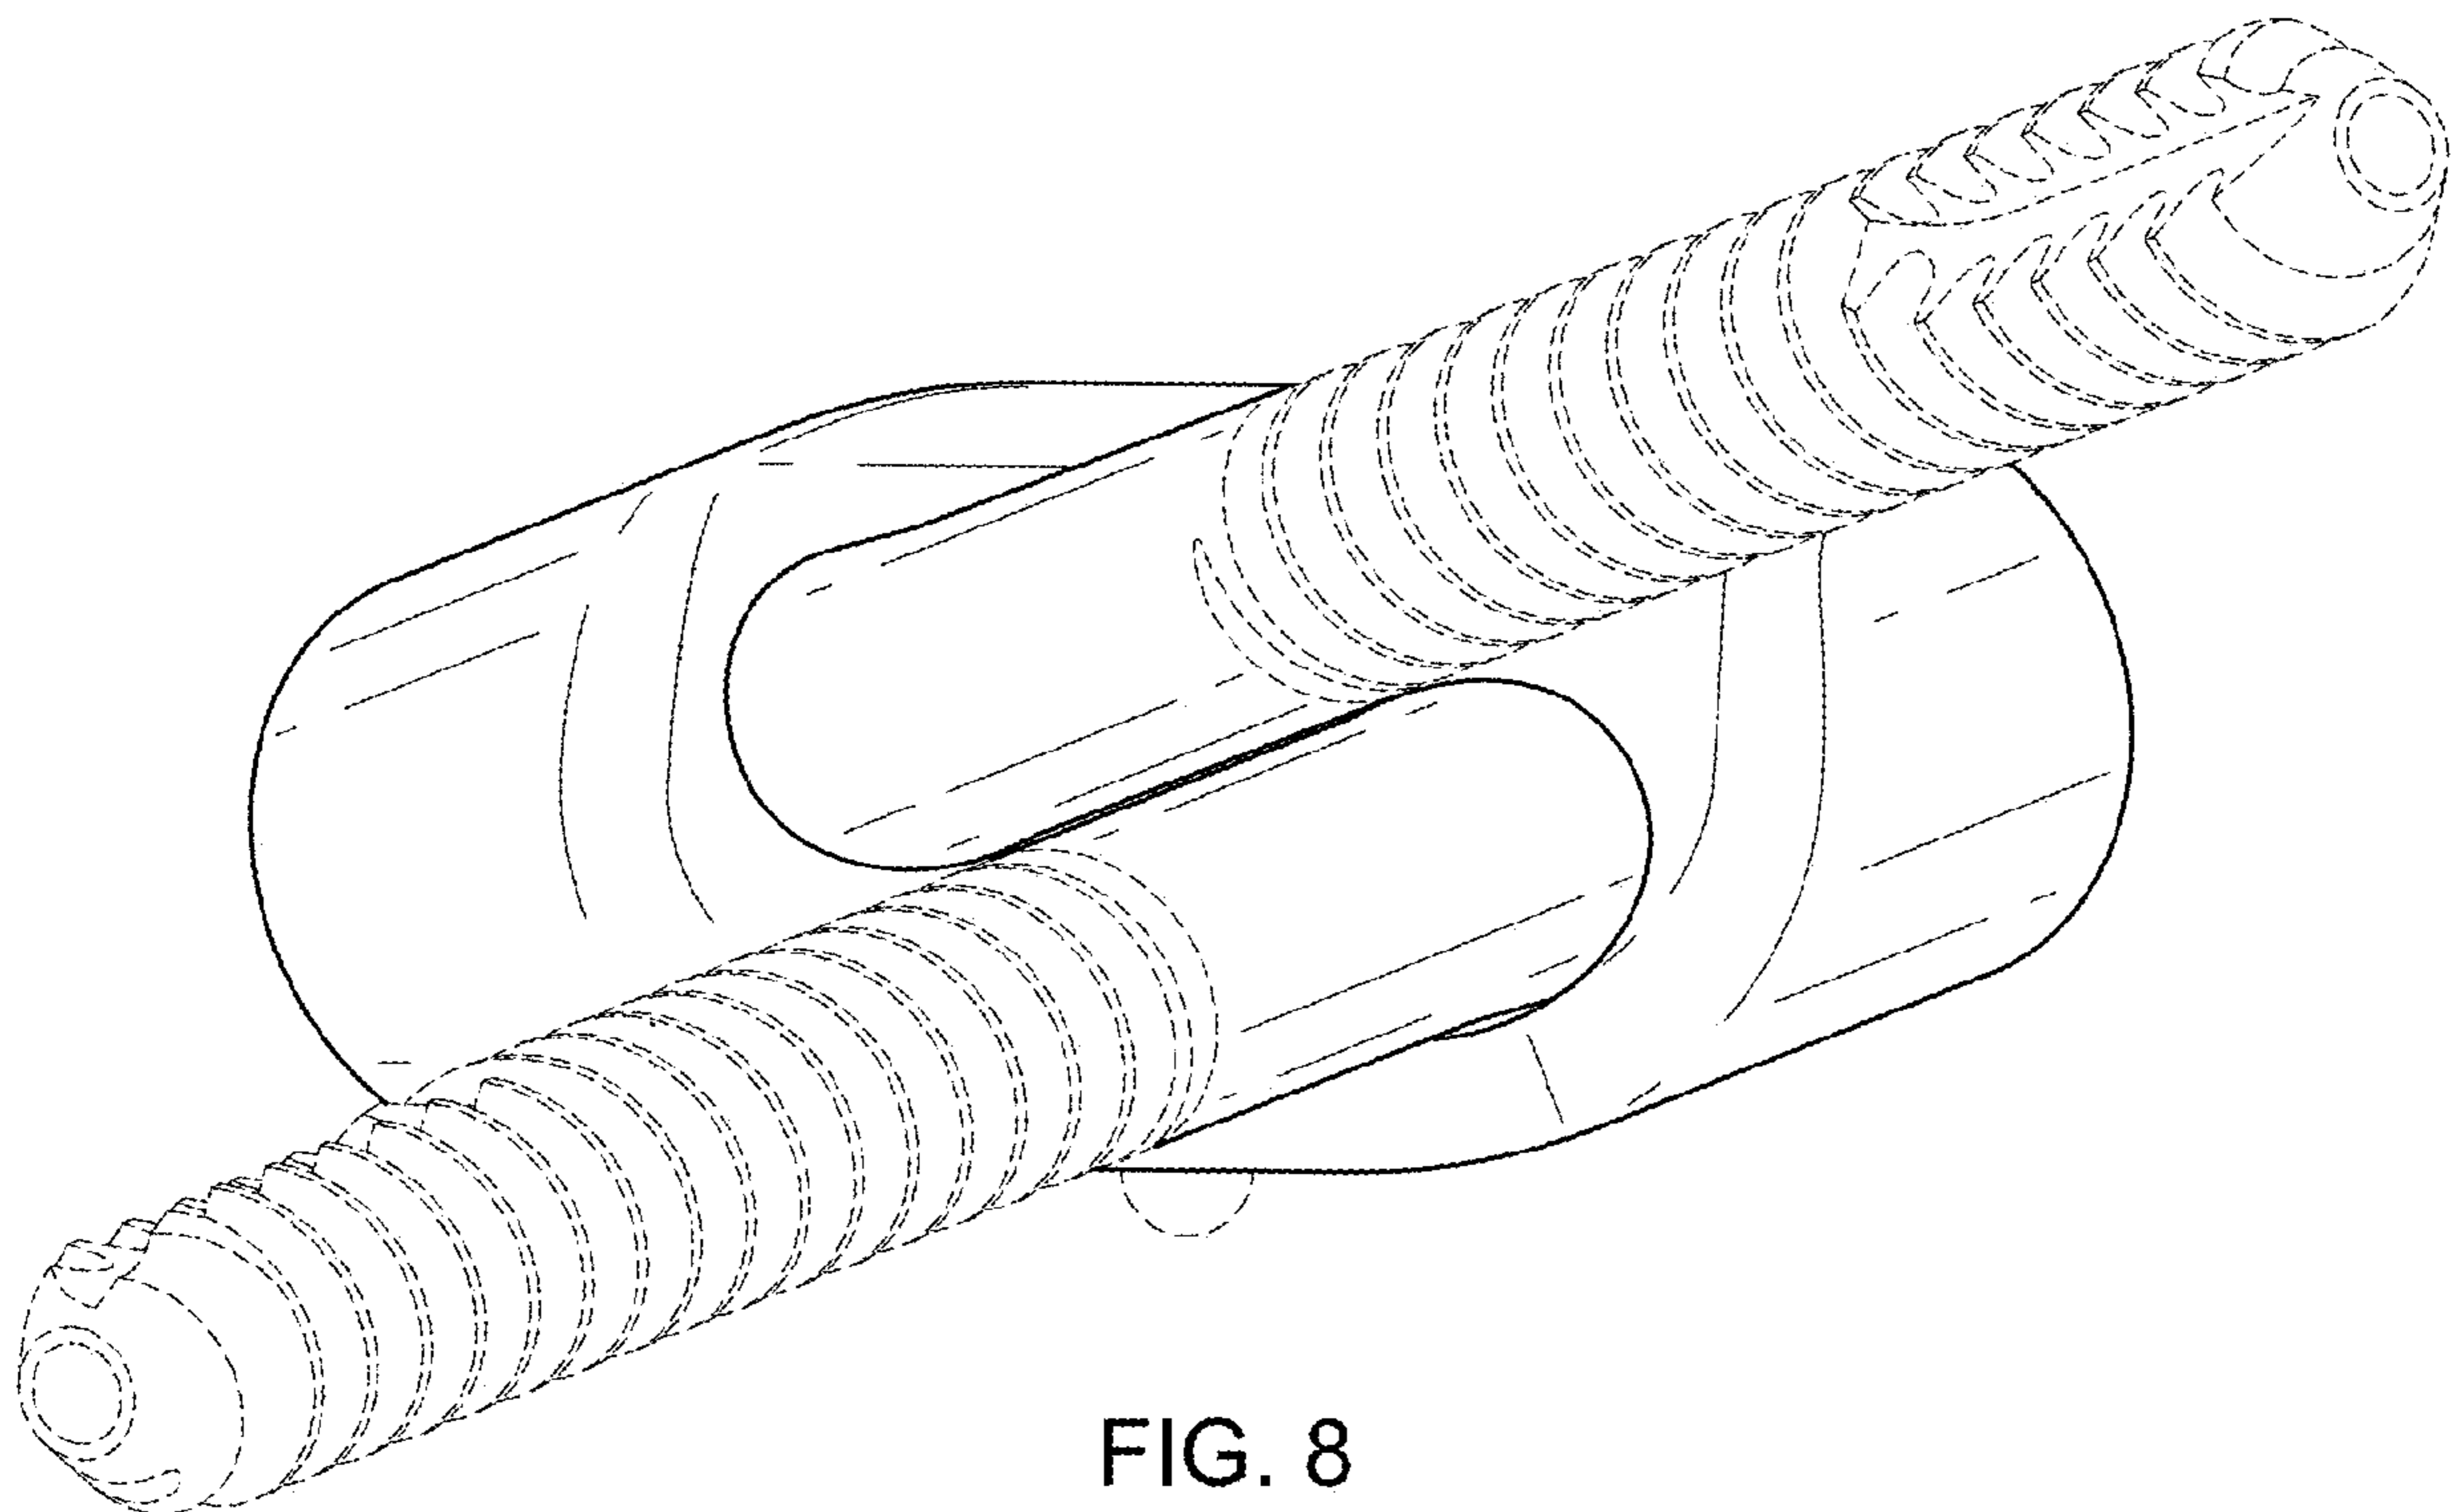


FIG. 8