



US00D920145S

(12) **United States Design Patent** (10) **Patent No.:** **US D920,145 S**  
**Livingston et al.** (45) **Date of Patent:** **\*\* May 25, 2021**

(54) **SAMPLE PREPARATION MODULE**

D357,484 S 4/1995 Montague et al.  
D491,272 S 6/2004 Alden et al.  
D515,707 S 2/2006 Shinohara et al.  
D618,570 S \* 6/2010 Ihara ..... D10/81  
(Continued)

(71) Applicant: **Becton, Dickinson and Company,**  
Franklin Lakes, NJ (US)

(72) Inventors: **Dwight Livingston,** Fallston, MD (US);  
**Michael T. VanSickler,** Columbia, MD  
(US); **Christopher John Murray,**  
Philadelphia, PA (US); **John Depler**  
**Coleman,** Philadelphia, PA (US);  
**Mathieu Dominic Turpault,**  
Philadelphia, PA (US)

**OTHER PUBLICATIONS**

Livingston, Dwight, "Sample Preparation Module, Diagnostic Test-  
ing Module, and Machine Assembly," U.S. Appl. No. 29/703,722,  
filed Aug. 29, 2019.

(Continued)

(73) Assignee: **Becton, Dickinson and Company,**  
Franklin Lakes, NJ (US)

*Primary Examiner* — Michael C Stout  
*Assistant Examiner* — Fritzgerald L Butac  
(74) *Attorney, Agent, or Firm* — Lerner, David,  
Littenberg, Krumholz & Mentlik, LLP

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/703,740**

(22) Filed: **Aug. 29, 2019**

**Related U.S. Application Data**

(62) Division of application No. 29/594,016, filed on Feb.  
15, 2017, now Pat. No. Des. 870,910.

(51) **LOC (13) Cl.** ..... **10-04**

(52) **U.S. Cl.**  
USPC ..... **D10/81; D24/216**

(58) **Field of Classification Search**

USPC ..... D10/47, 81; D13/158–160;  
D14/420–425; D15/122, 127, 135;  
D18/14, 19, 36–39, 50, 53, 54, 54.1, 55,  
D18/81; D24/107, 181, 185, 186, 216,  
D24/219, 231–234  
CPC ..... G01N 15/1434; G01N 15/1459; G01N  
2015/008; G01N 2015/1477; G01N  
2015/1486; G01N 2021/4716  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D323,895 S 2/1992 Protzmann  
D336,479 S 6/1993 Shuji Shinagawa et al.


(57) **CLAIM**

The ornamental design for a sample preparation module, as  
shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a sample preparation  
module according to our design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a rear elevational view thereof;  
FIG. 4 is a right side elevational view thereof;  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a top plan view thereof;  
FIG. 7 is a bottom plan view thereof; and,  
FIG. 8 is a view showing an example use thereof.  
Some of the broken lines in FIGS. 1, 2, 7, and 8 illustrate  
portions of the diagnostic testing module that form no part  
of the claimed design. The remaining broken lines in FIGS.  
1, 2, 7, and 8, as well as the broken lines in the remaining  
figures illustrate environmental structure that forms no part  
of the claimed design.

**1 Claim, 8 Drawing Sheets**

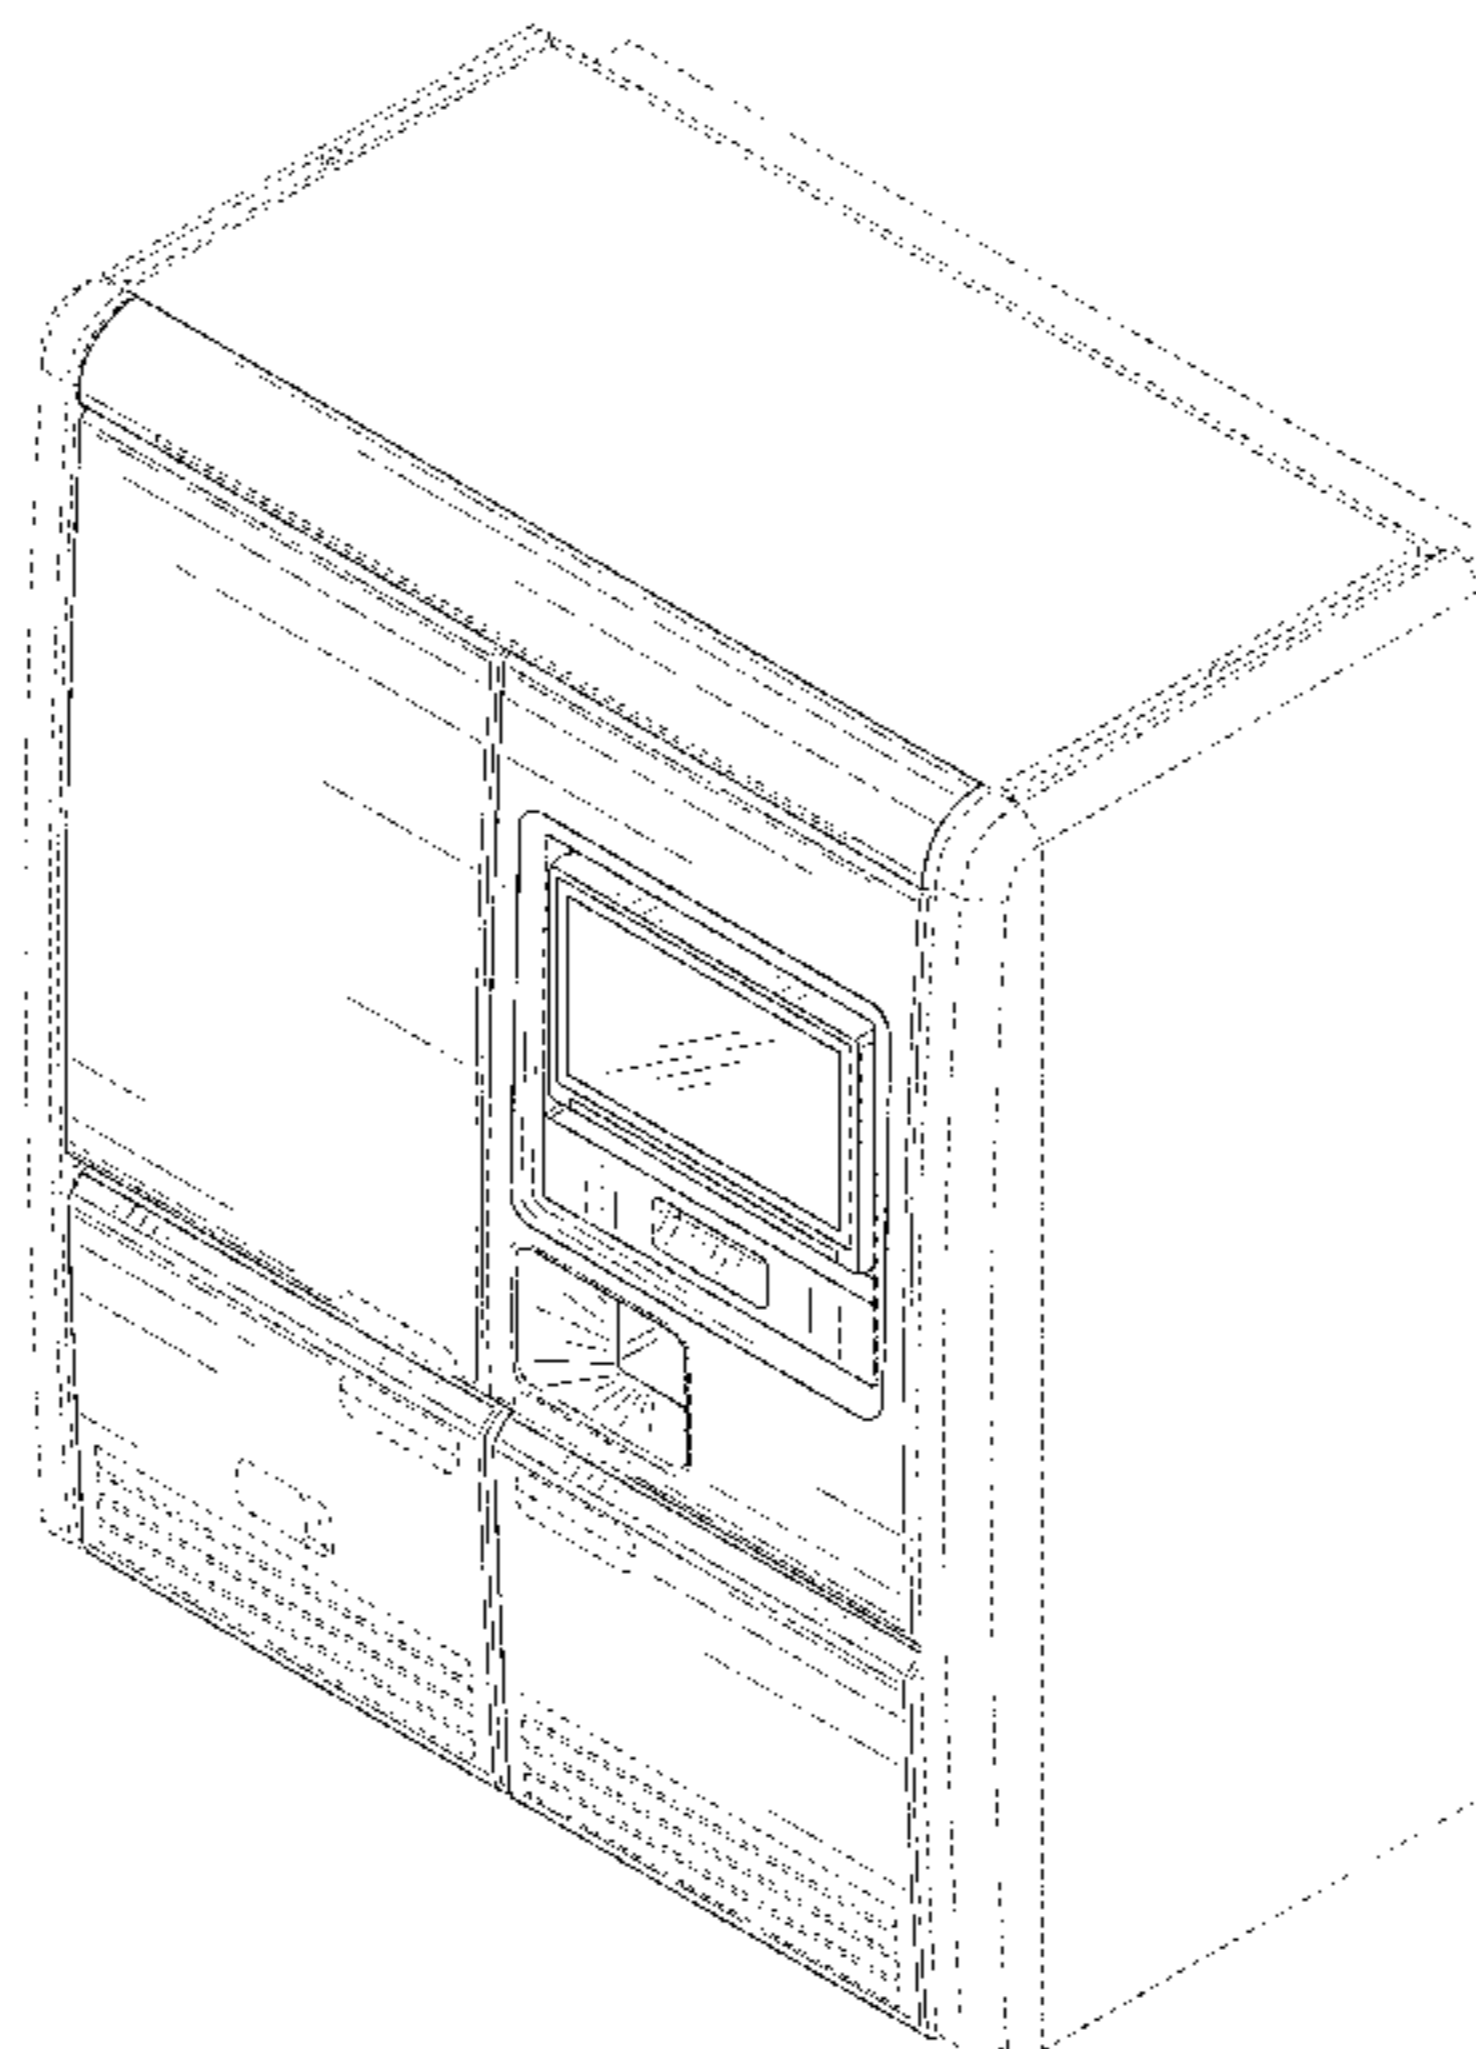

(56)

References Cited

U.S. PATENT DOCUMENTS

D650,417 S 12/2011 Brown et al.  
 D652,947 S 1/2012 Philipak et al.  
 D659,174 S 5/2012 Mueller  
 D663,040 S 7/2012 Oonuma et al.  
 D676,568 S 2/2013 Liu et al.  
 D685,483 S 7/2013 LiCalzi  
 D686,261 S 7/2013 Sunter et al.  
 D686,262 S 7/2013 Sunter et al.  
 D686,263 S 7/2013 Sunter et al.  
 D690,330 S 9/2013 Tsuchiyama et al.  
 D690,745 S 10/2013 Koide et al.  
 D719,275 S 12/2014 Gutmann et al.  
 D724,753 S 3/2015 Gutmann et al.  
 D730,959 S 6/2015 Kirkland et al.  
 D731,563 S 6/2015 Kirkland et al.  
 D735,253 S 7/2015 Bausback  
 D736,840 S 8/2015 Kirkland et al.  
 D753,734 S 4/2016 Hanschen  
 D759,738 S 6/2016 Schonherr et al.  
 D762,748 S 8/2016 Schonherr et al.  
 D777,049 S 1/2017 Barton et al.  
 D781,357 S 3/2017 Inaba et al.  
 D788,617 S 6/2017 Barton et al.  
 D794,099 S 8/2017 Gallo  
 D800,000 S 10/2017 Barton et al.  
 D802,156 S 11/2017 Barton et al.  
 D803,712 S 11/2017 Kurata  
 D811,913 S 3/2018 Barton et al.  
 D813,410 S 3/2018 LiCalzi et al.  
 D816,738 S 5/2018 Kim

D816,741 S 5/2018 Nicaise  
 D822,724 S 7/2018 Hanschen  
 D823,359 S 7/2018 Krebber  
 D825,489 S 8/2018 Yoshida et al.  
 D838,613 S \* 1/2019 Barton ..... D10/81  
 D840,048 S 2/2019 Barton et al.  
 D841,188 S 2/2019 Choudhary et al.  
 D843,597 S 3/2019 Kurz-Ottenwaelder et al.  
 D846,138 S 4/2019 Masuda et al.  
 D846,139 S 4/2019 Masuda et al.  
 D846,140 S 4/2019 Masuda et al.  
 D848,019 S 5/2019 Barton et al.  
 D850,955 S 6/2019 Barton et al.  
 D857,536 S \* 8/2019 Zhang ..... D10/81  
 D859,192 S 9/2019 Barton et al.  
 D869,309 S 12/2019 Barton et al.  
 D870,910 S \* 12/2019 Livingston ..... D24/216  
 D876,259 S \* 2/2020 Barton ..... D10/81  
 2019/0107547 A1 \* 4/2019 VanSickler ..... B01L 9/52

OTHER PUBLICATIONS

Livingston, Dwight, "Sample Preparation Module, Diagnostic Testing Module, and Machine Assembly," U.S. Appl. No. 29/703,739, filed Aug. 29, 2019.  
 Livingston, Dwight, "Sample Preparation Module, Diagnostic Testing Module, and Machine Assembly," U.S. Appl. No. 29/703,752, filed Aug. 29, 2019.  
 Figures publicly disclosed at a seminar in Sweden some time after Apr. 22, 2016 and prior to the filing of the present application.

\* cited by examiner

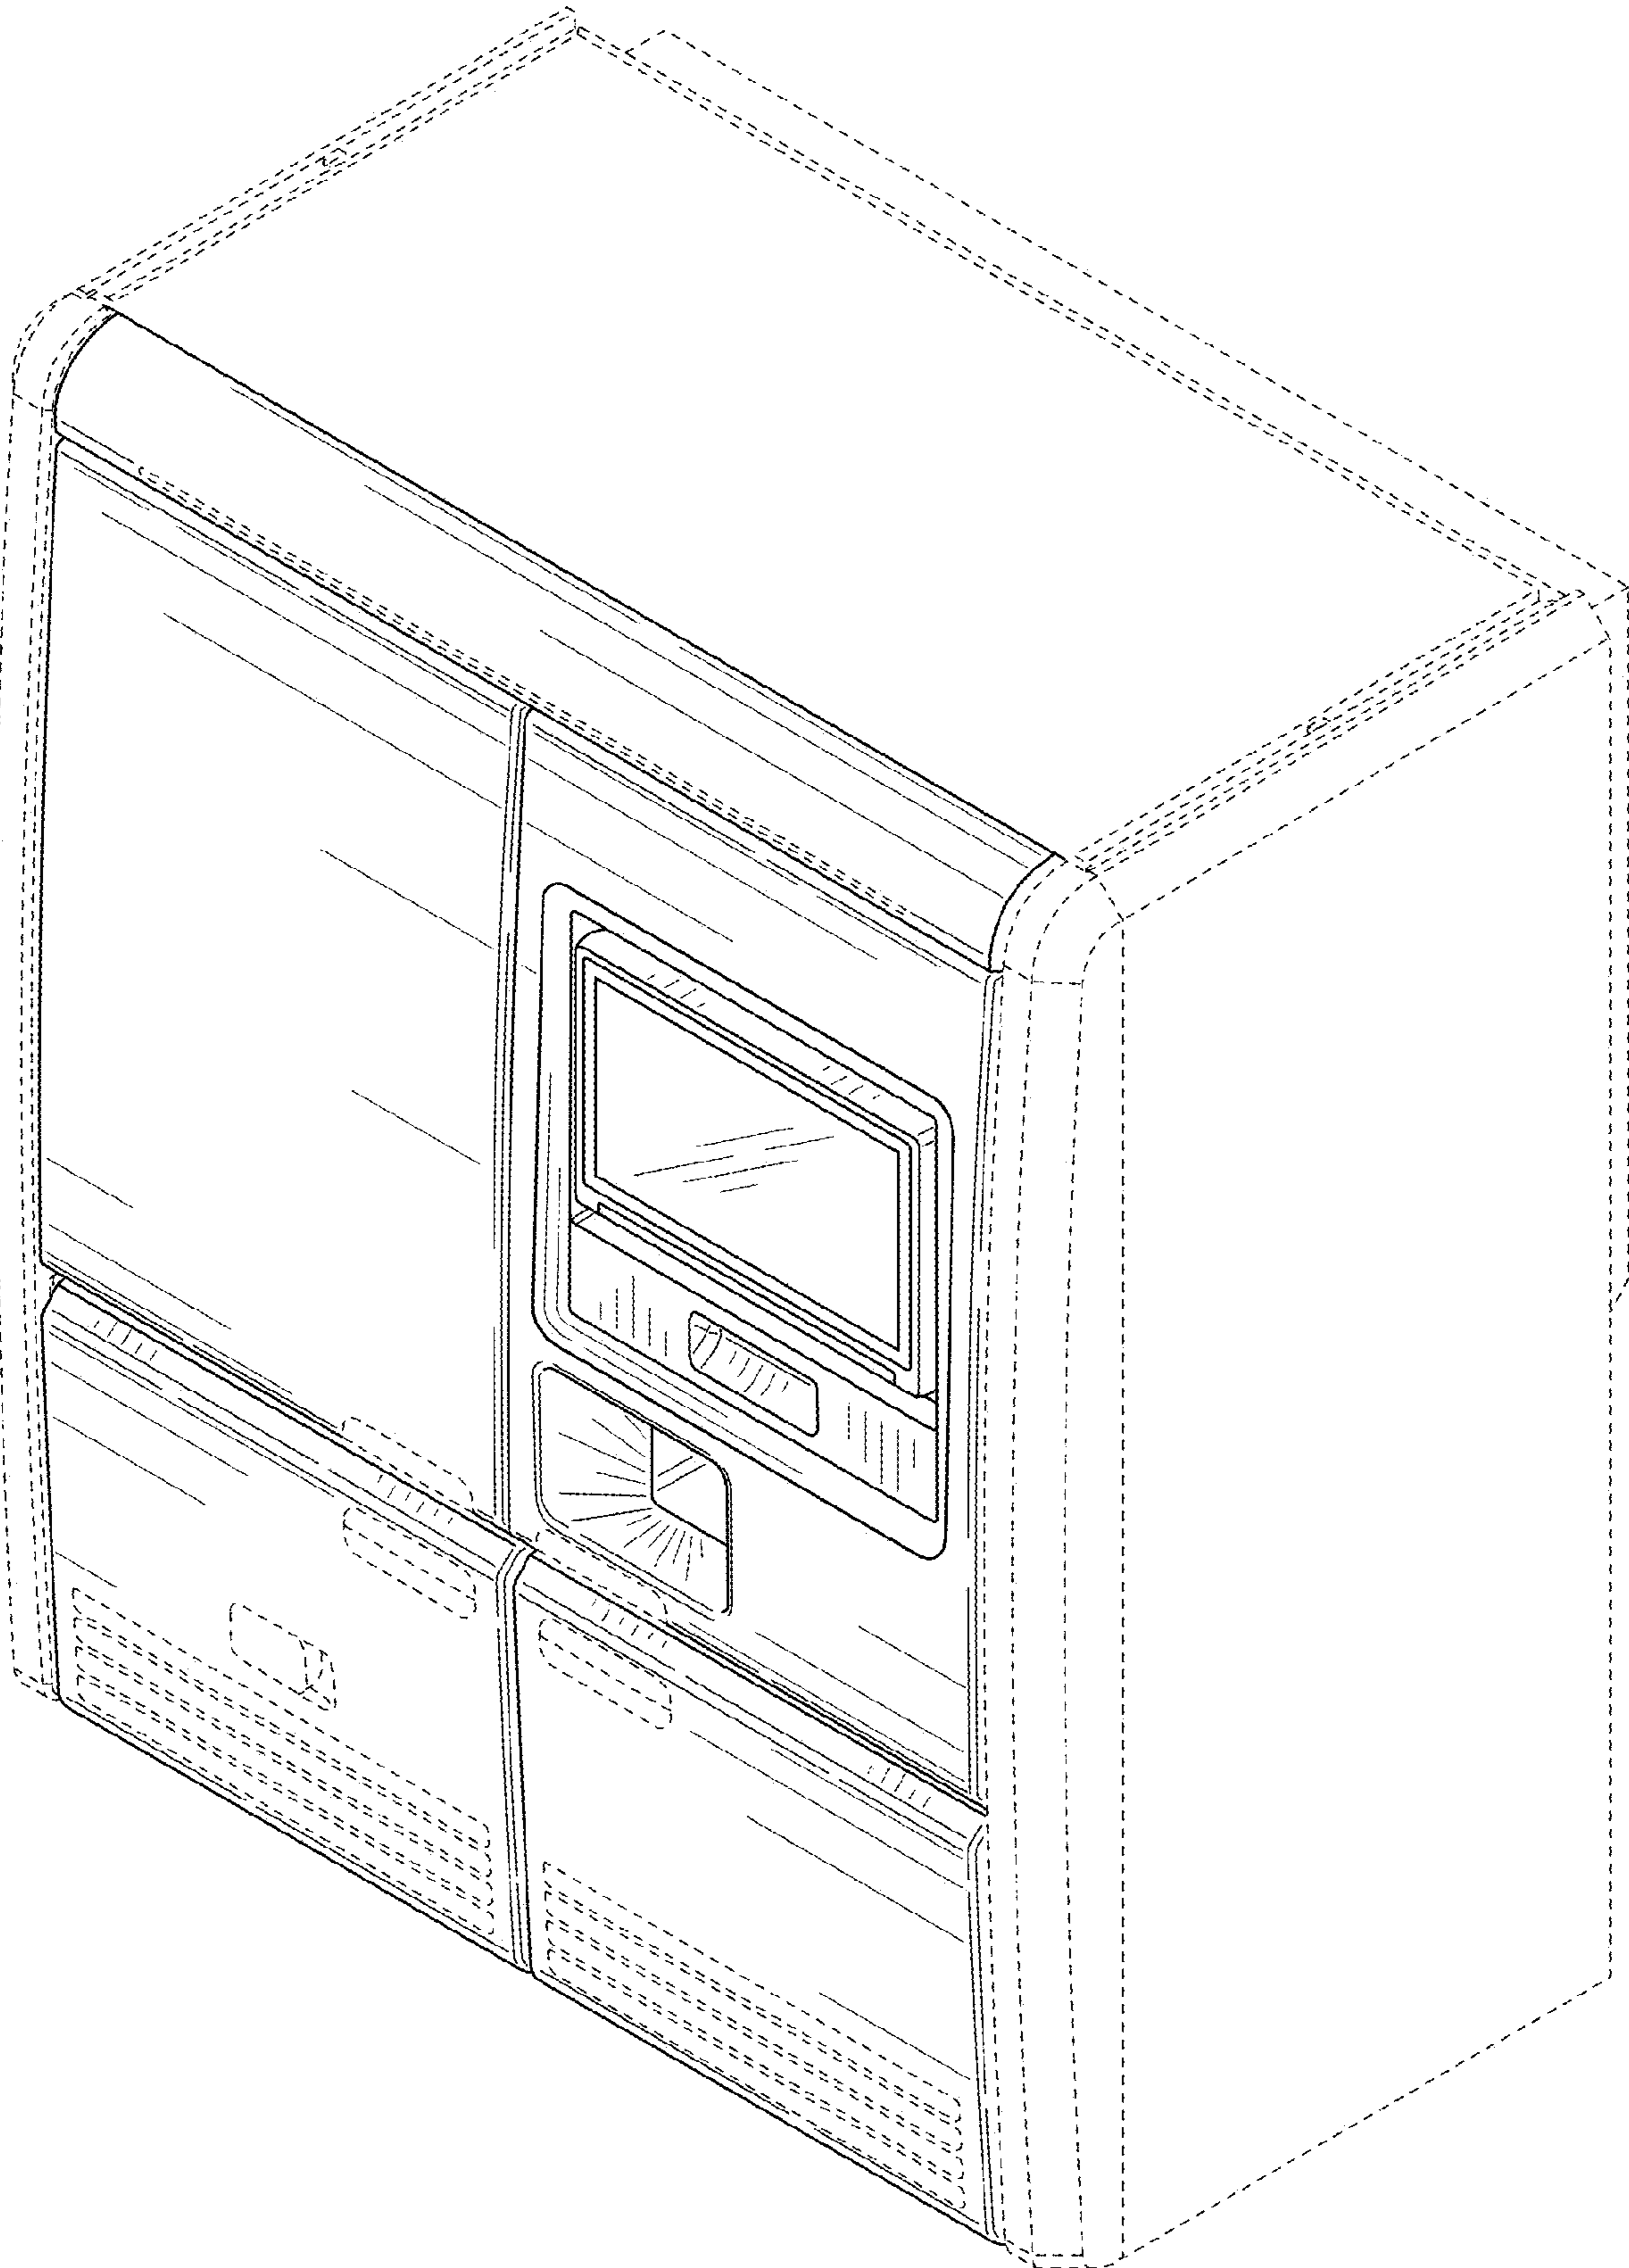


FIG. 1



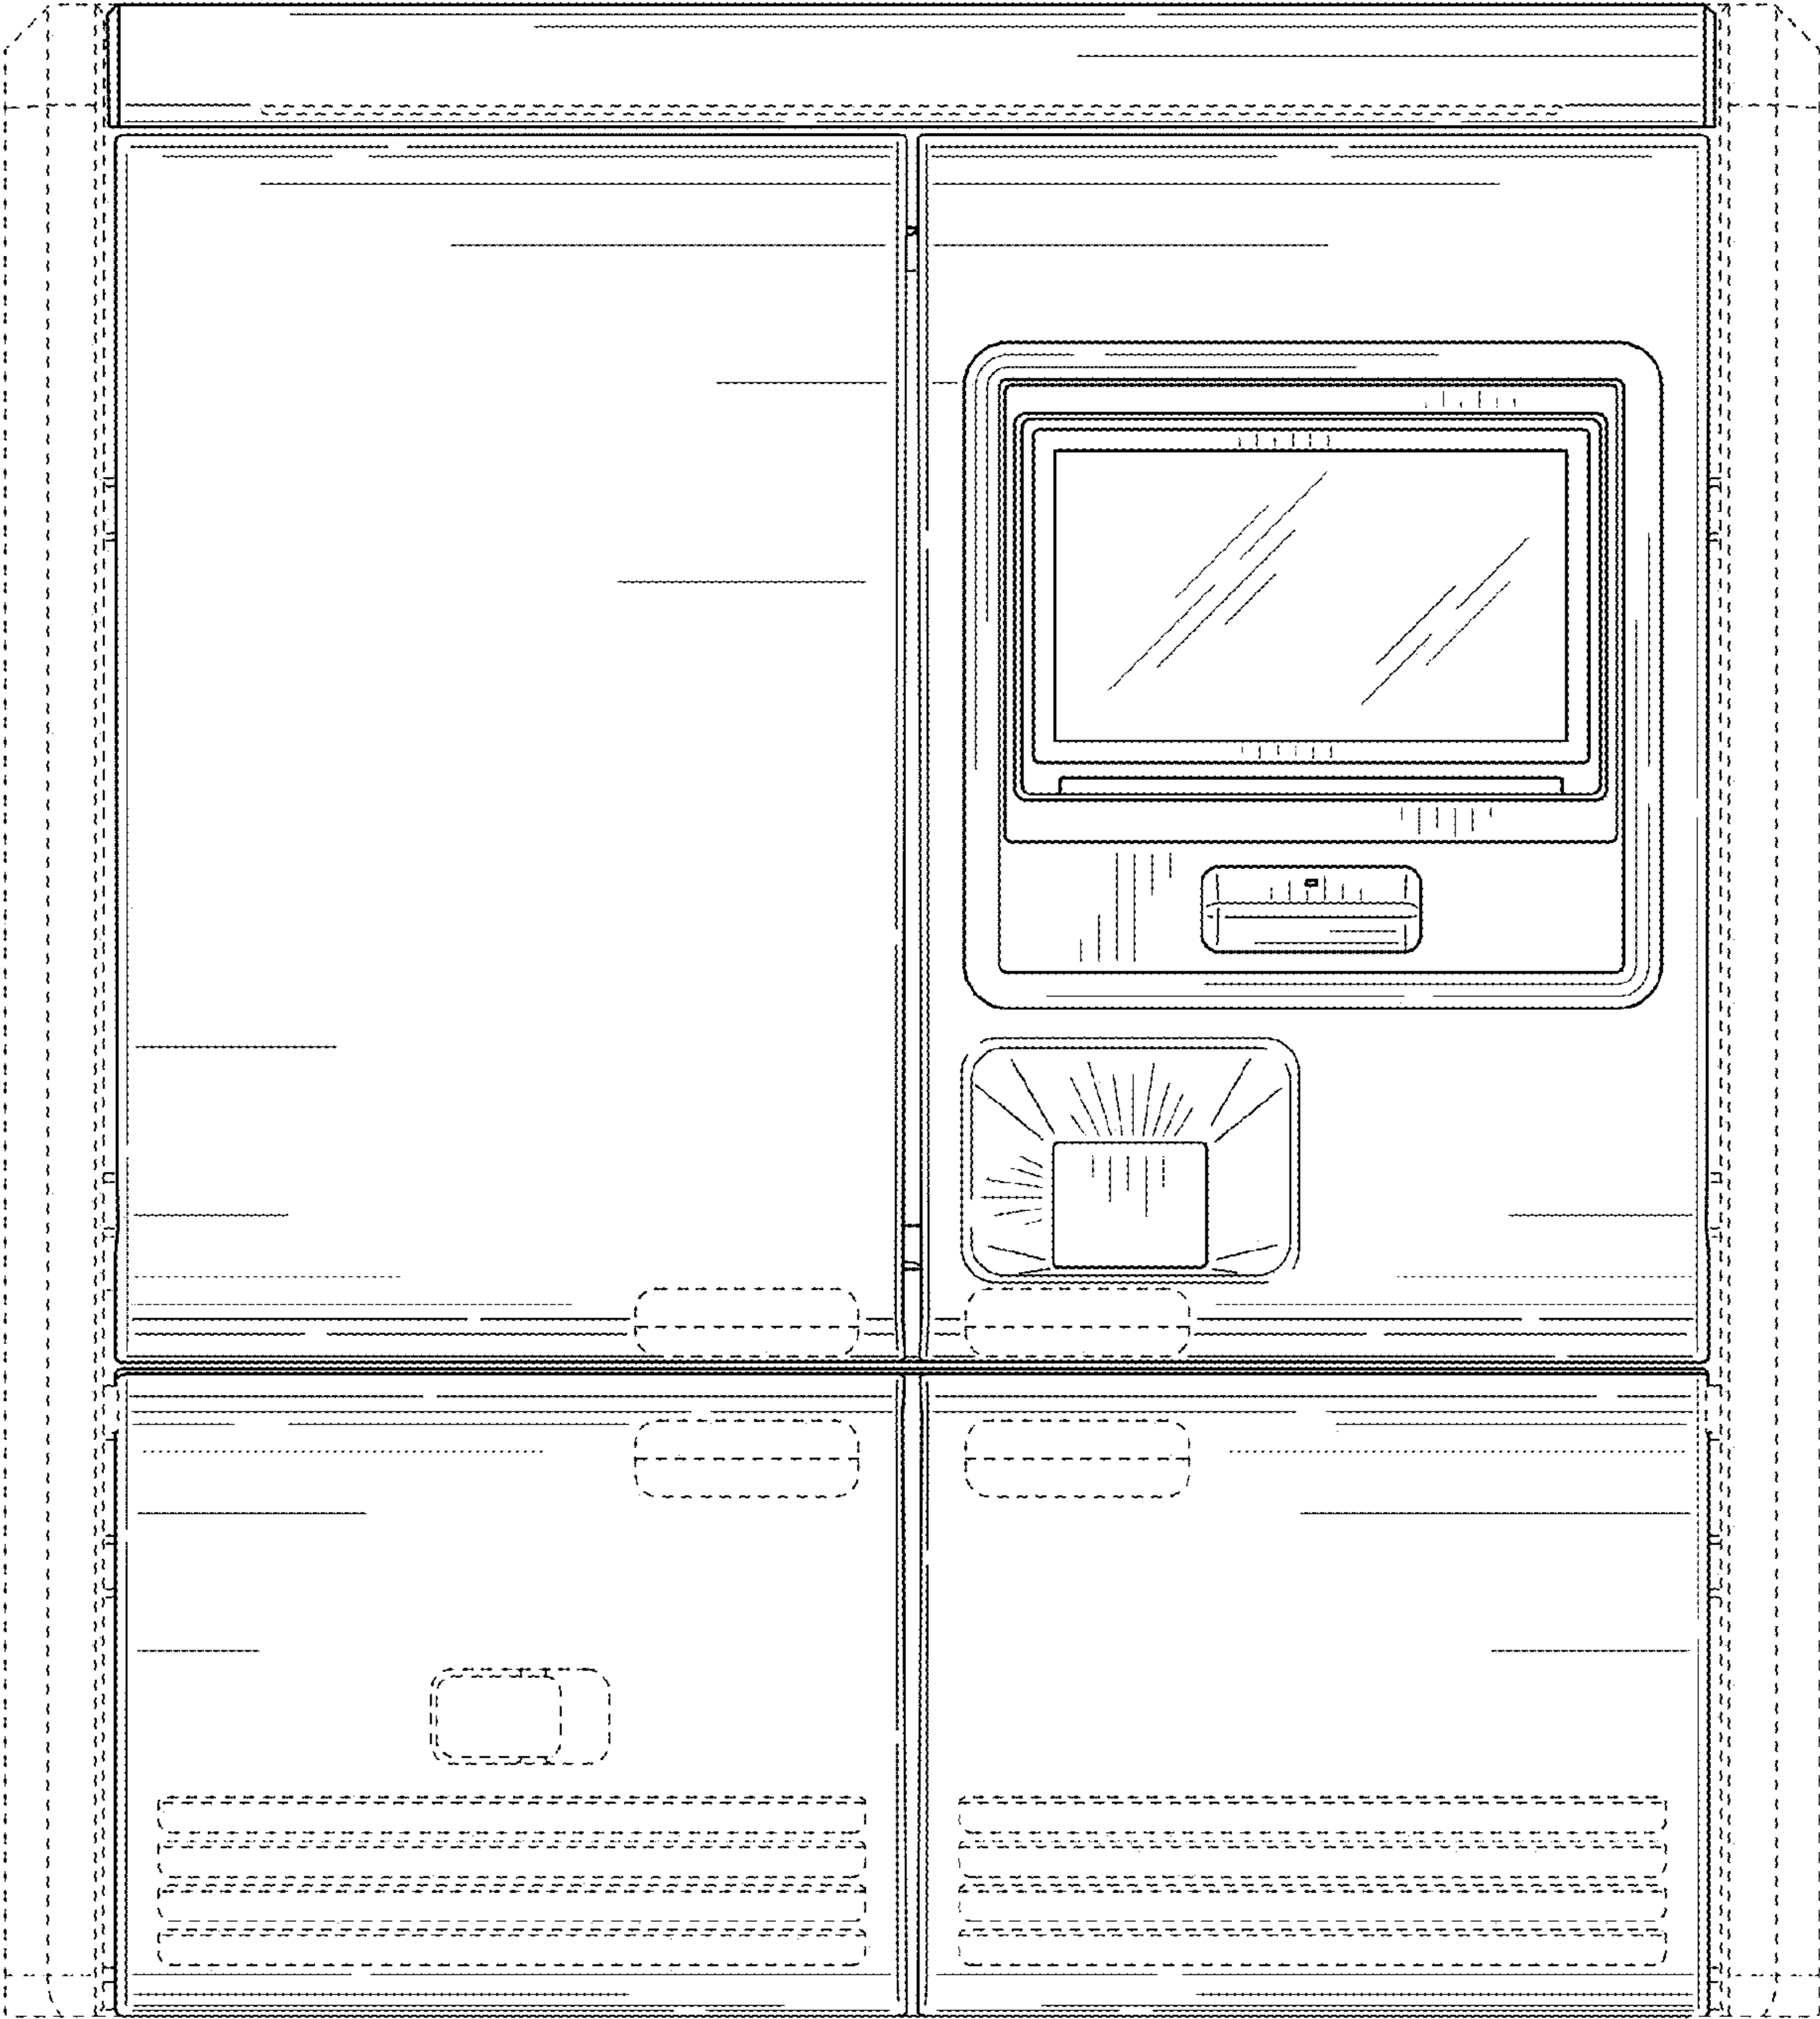


FIG. 2

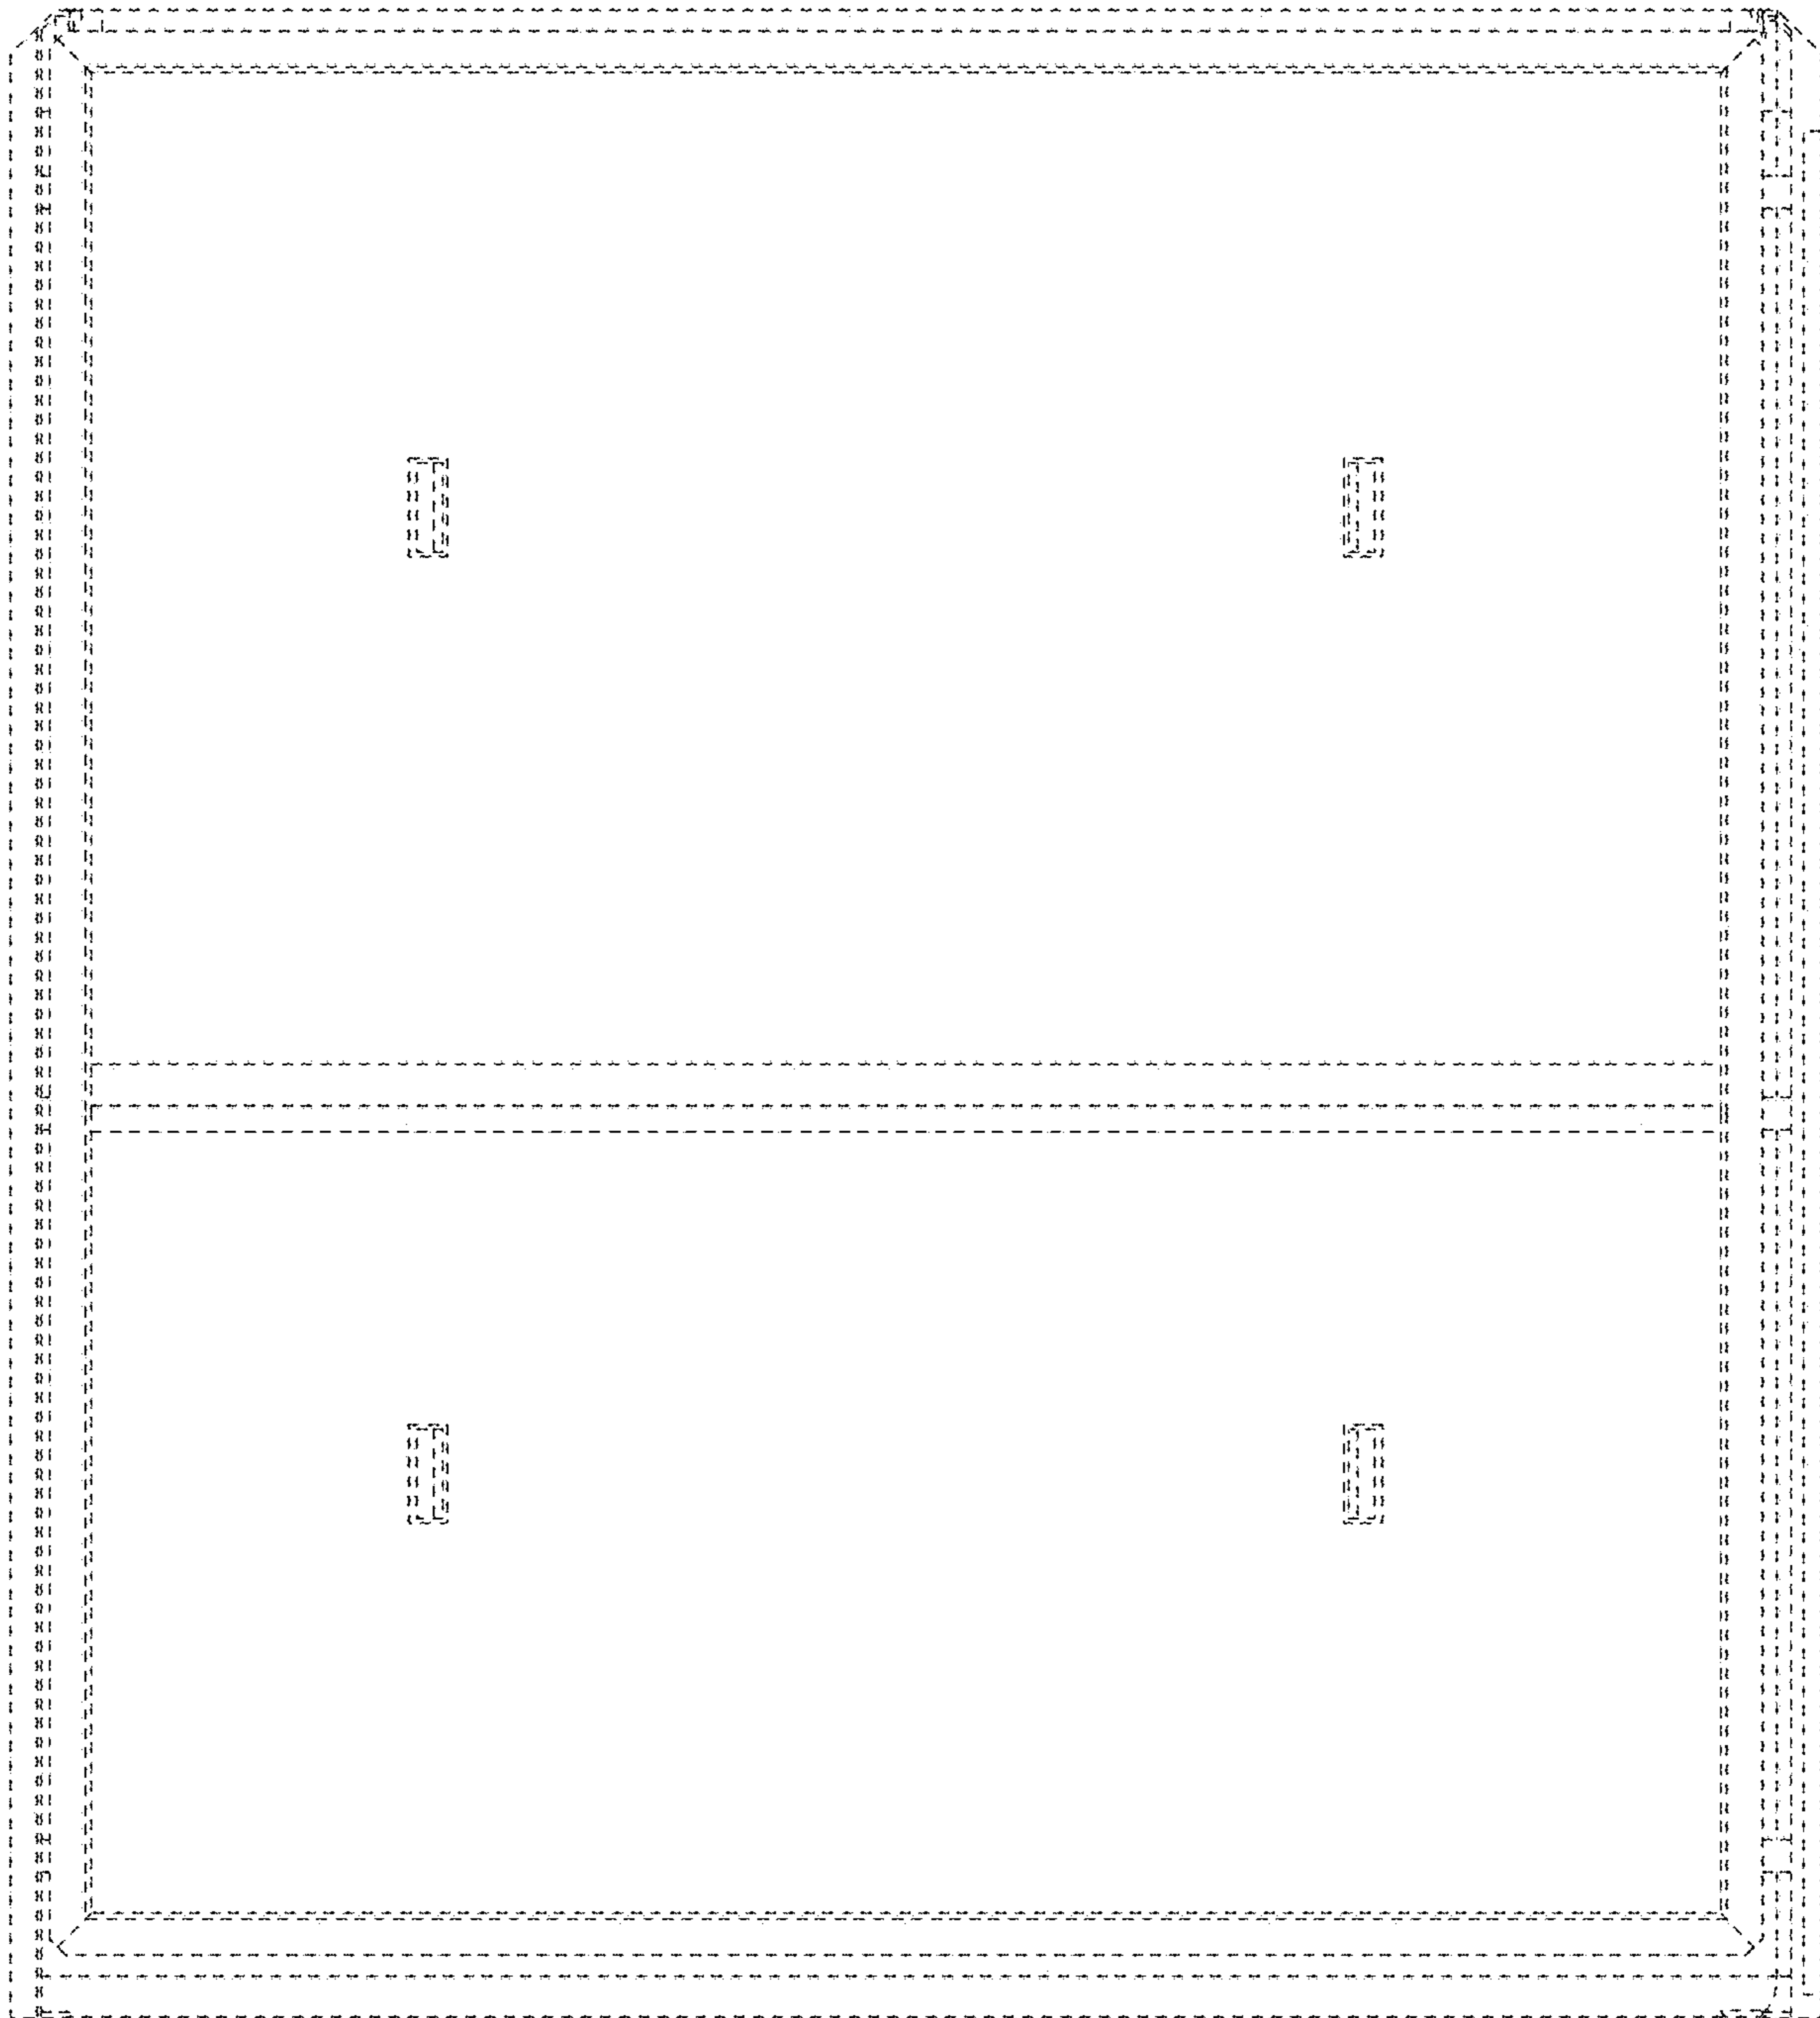


FIG. 3

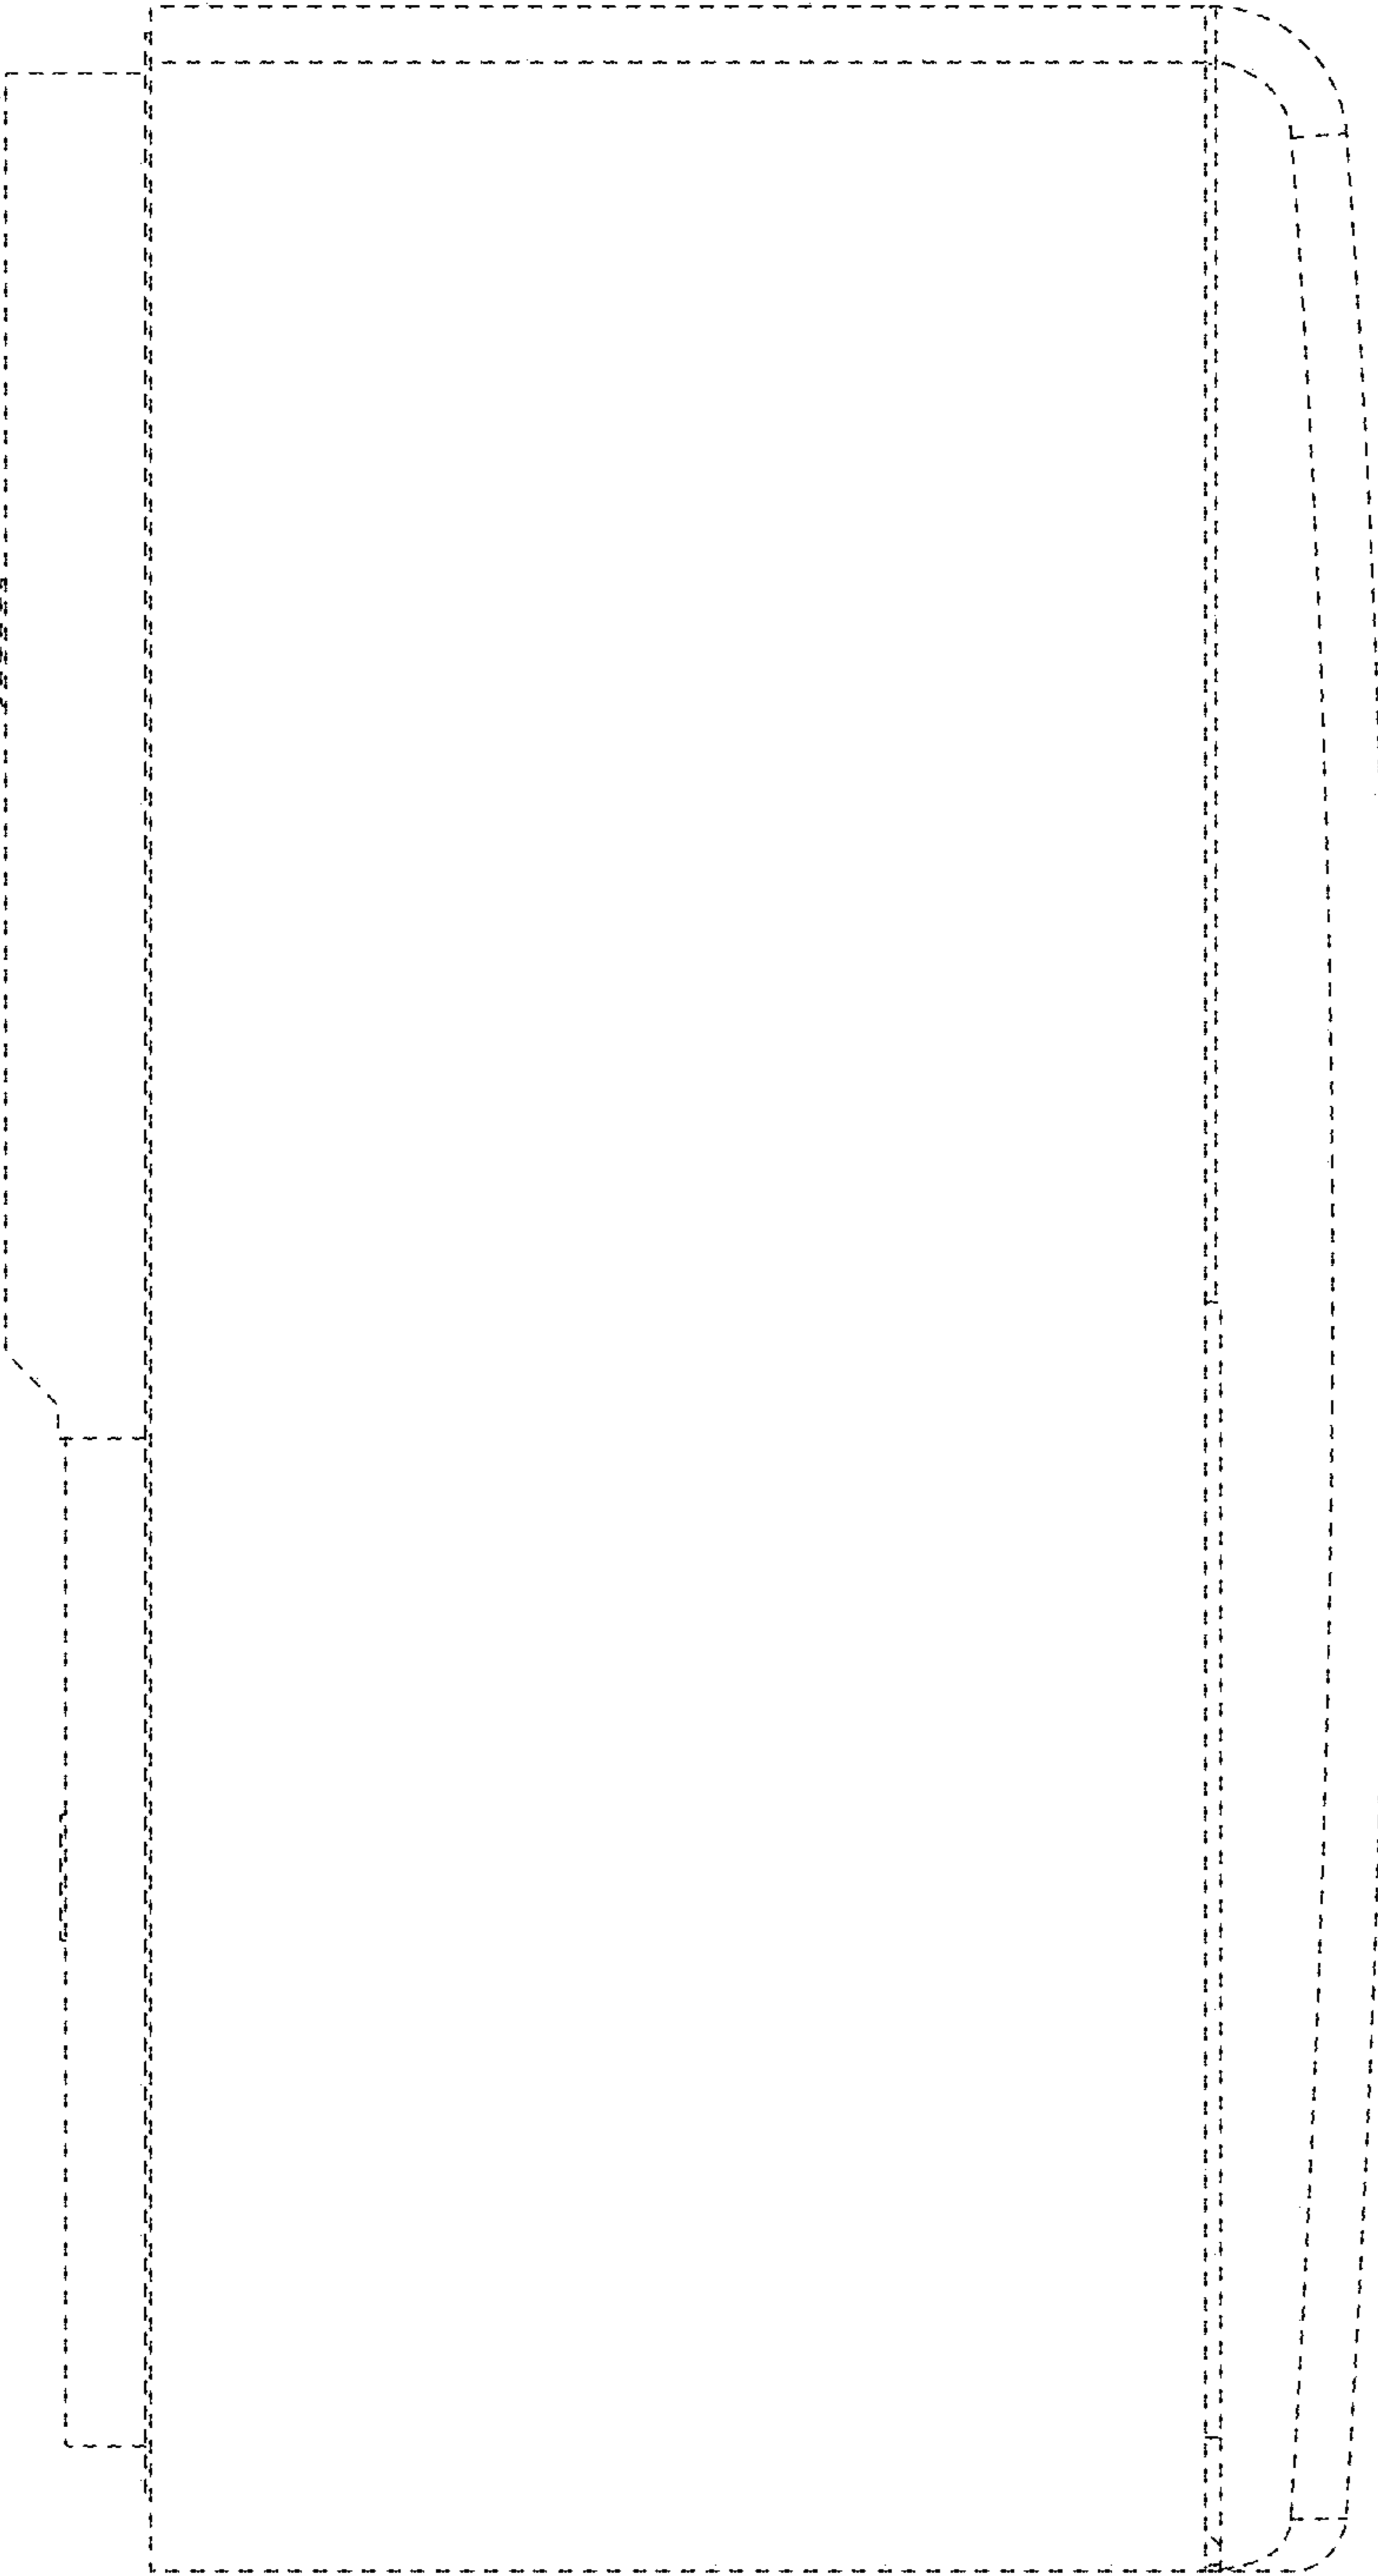


FIG. 4

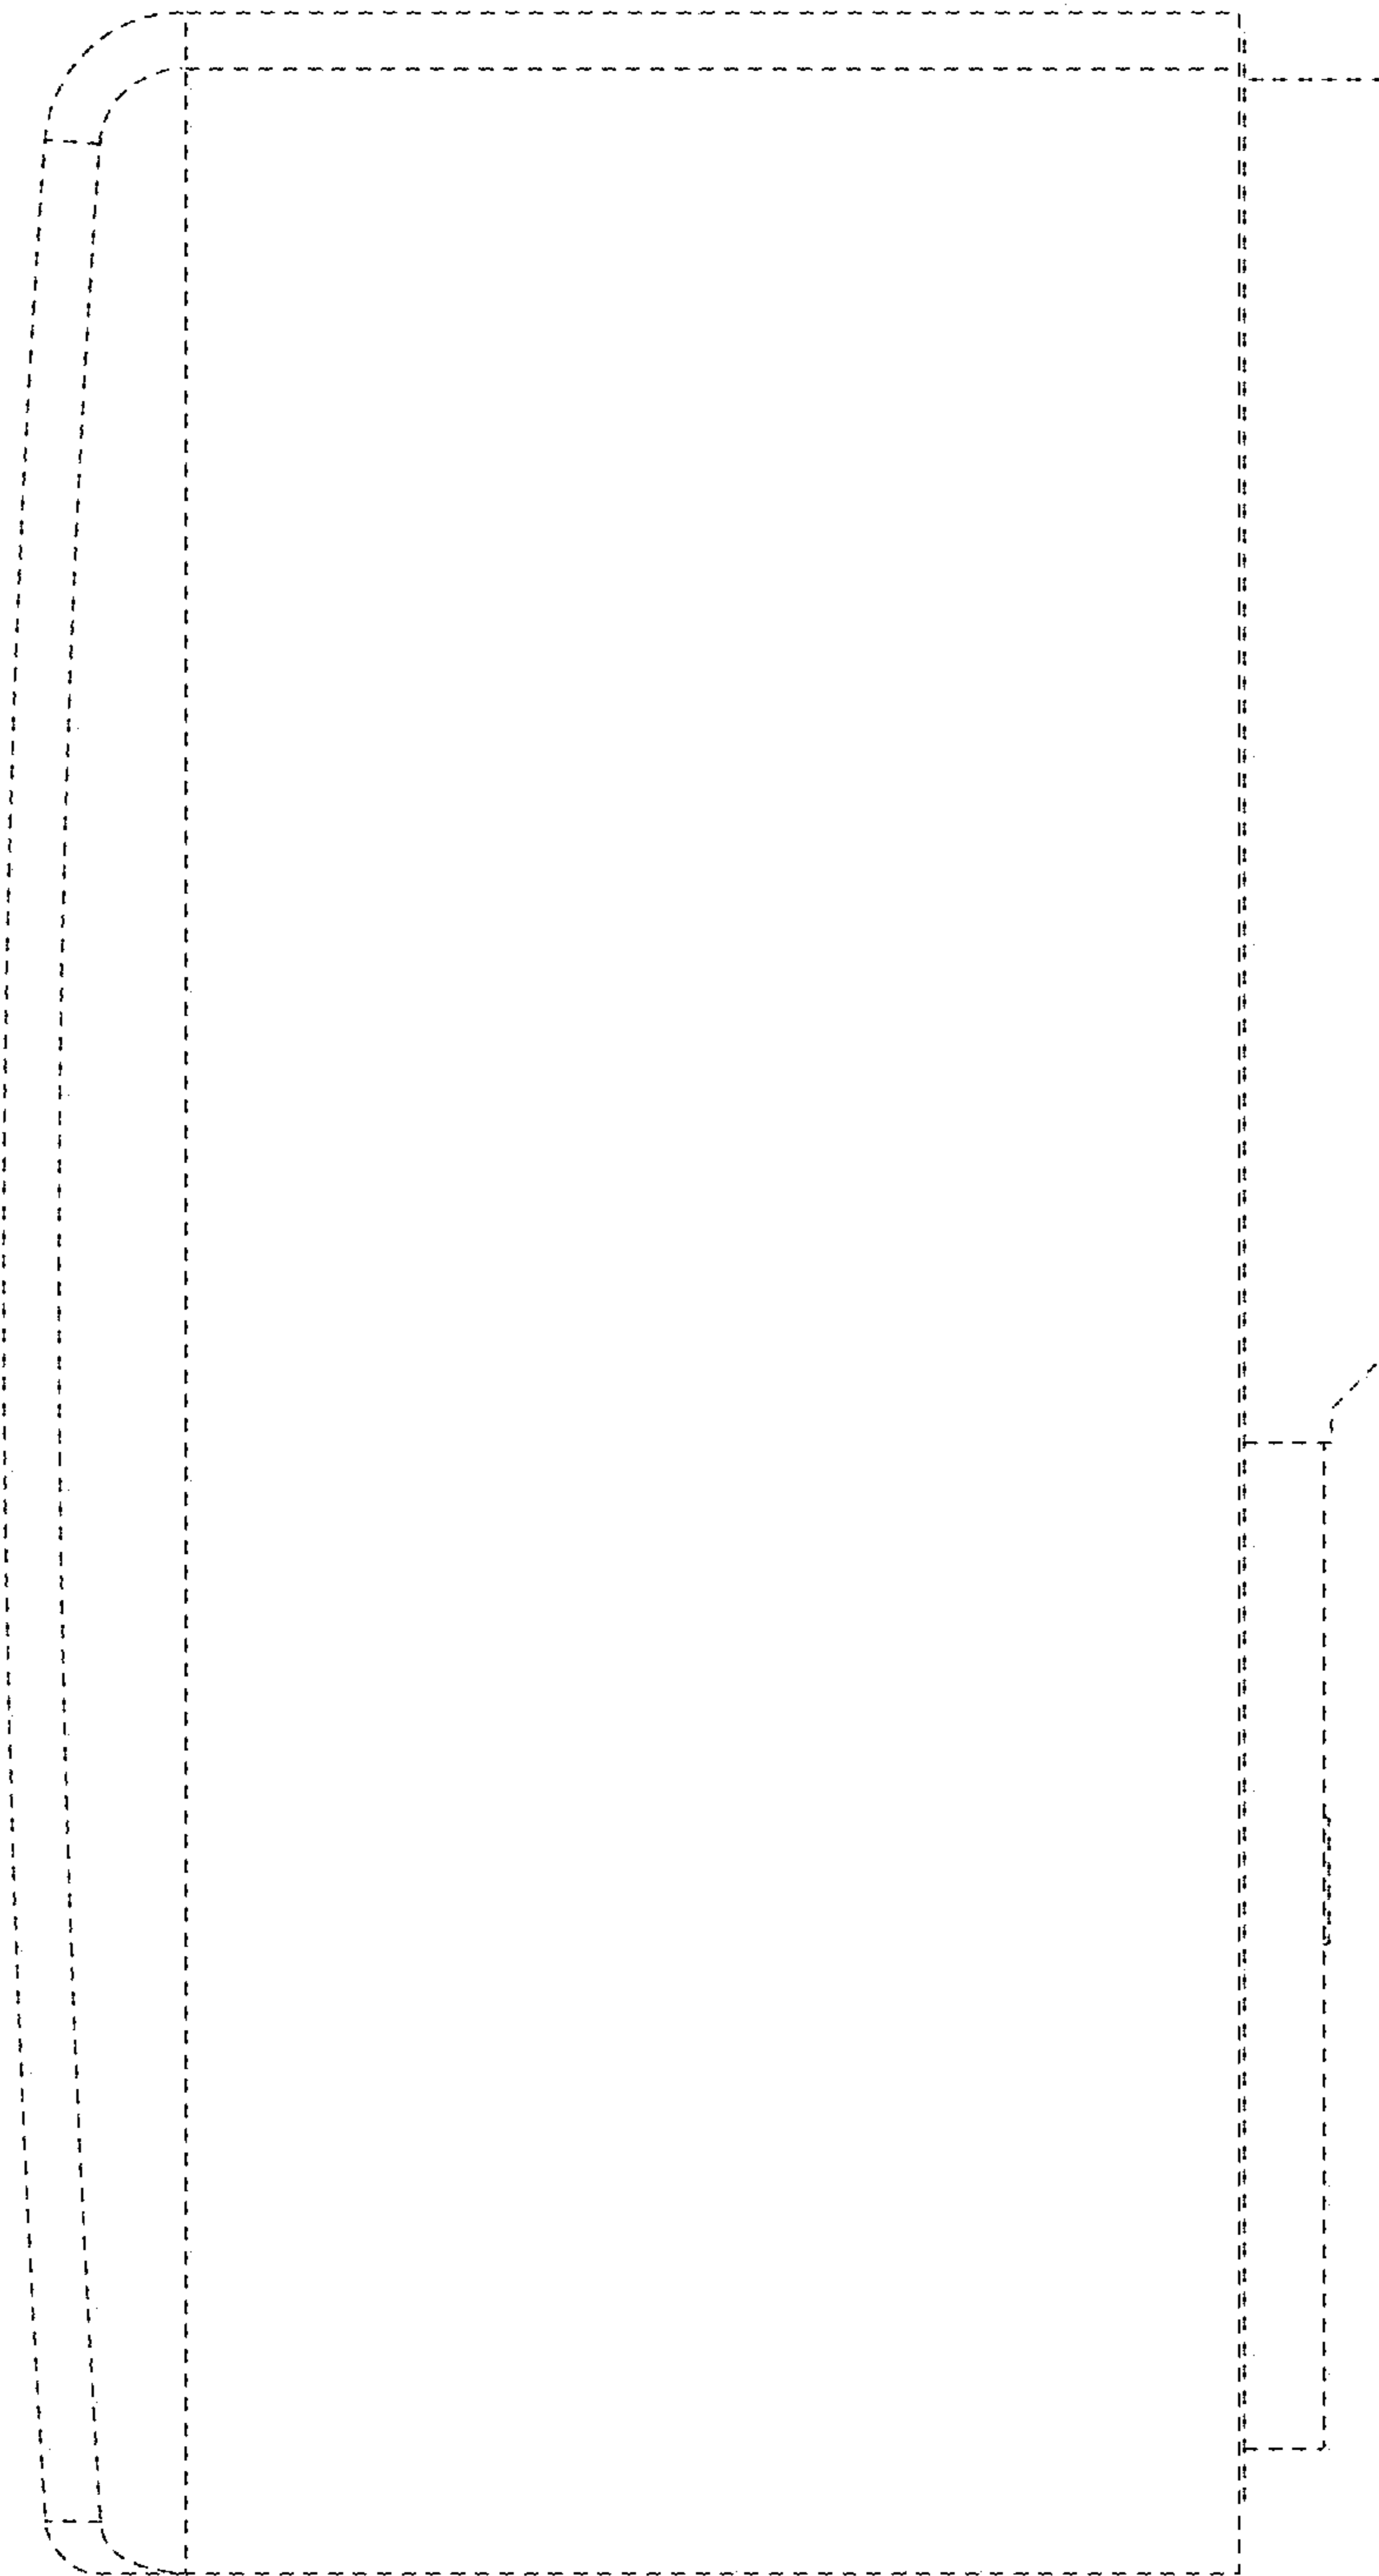


FIG. 5



FIG. 6



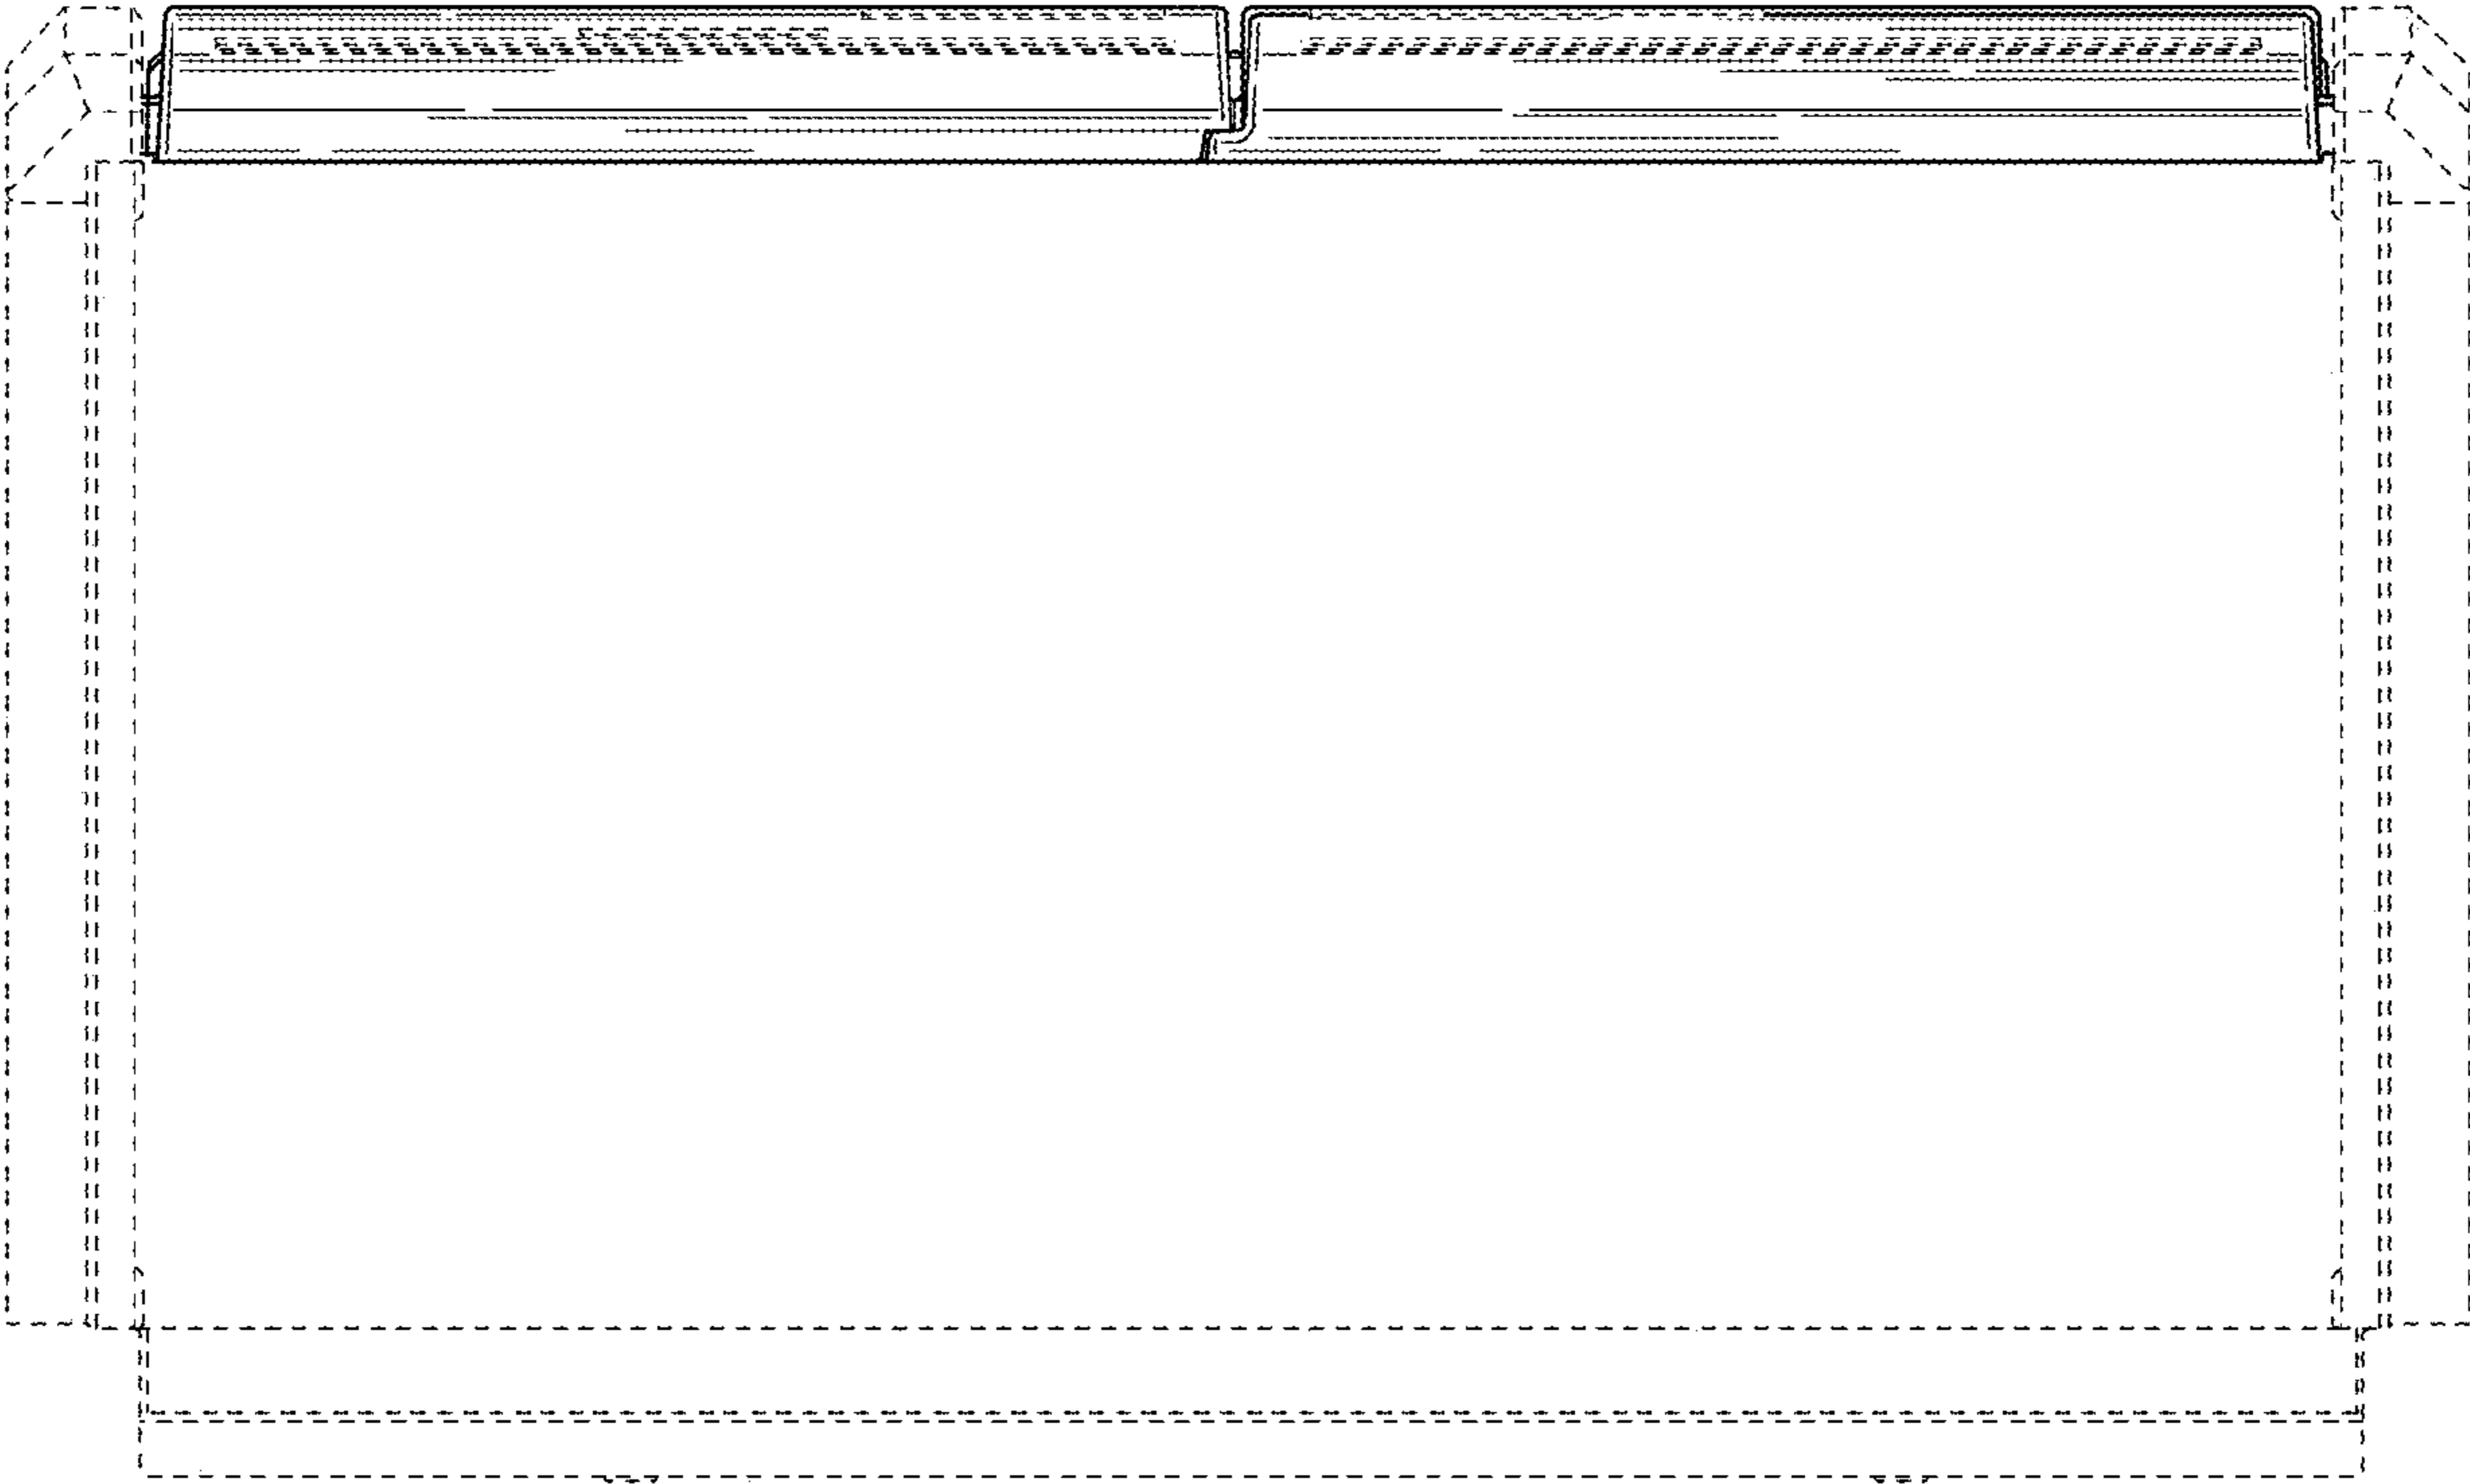


FIG. 7

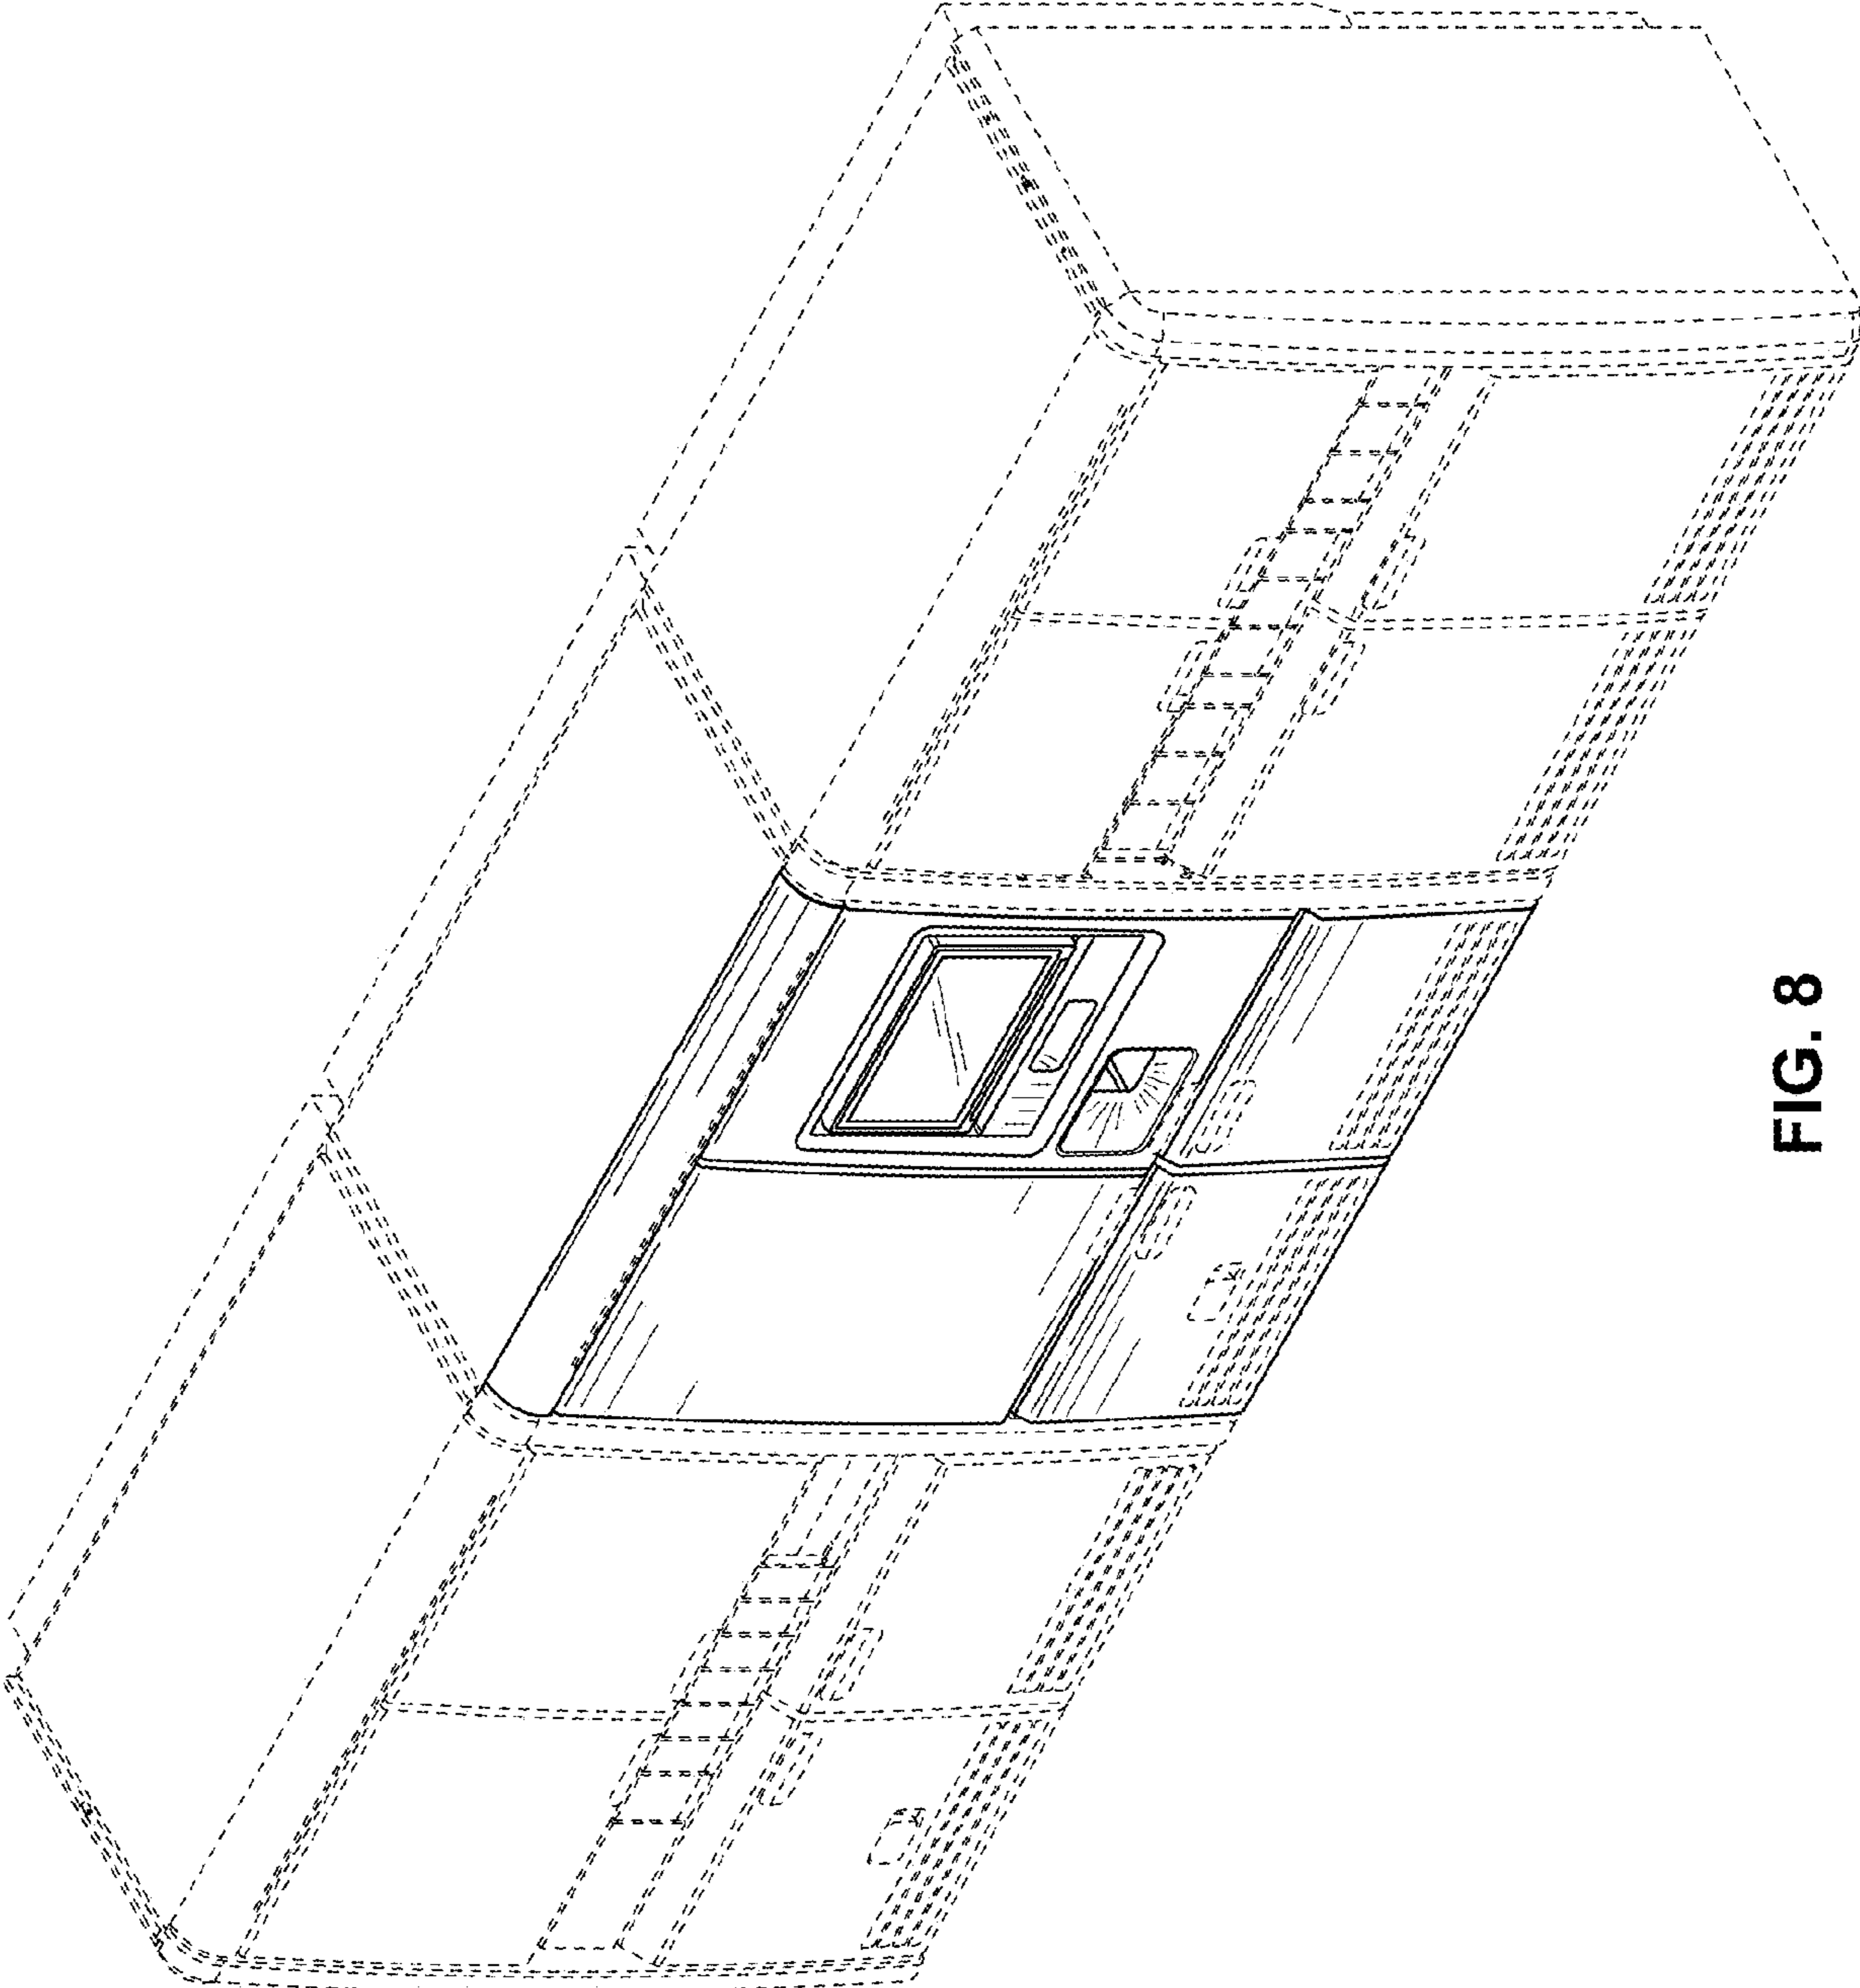


FIG. 8