



US00D920515S

(12) **United States Design Patent** (10) **Patent No.:** **US D920,515 S**
Miller et al. (45) **Date of Patent:** **** May 25, 2021**

(54) **SPINAL IMPLANT**

(71) Applicant: **restor3d, Inc.**, Durham, NC (US)

(72) Inventors: **Andrew Todd Miller**, Durham, NC (US); **Matthew Rexrode**, Durham, NC (US); **Cambre Kelly**, Durham, NC (US); **Ken Gall**, Durham, NC (US)

(73) Assignee: **RESTOR3D, INC.**, Durham, NC (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/719,880**

(22) Filed: **Jan. 8, 2020**

(51) **LOC (13) Cl.** **24-03**

(52) **U.S. Cl.**
USPC **D24/155**

(58) **Field of Classification Search**
USPC D2/896, 902, 905, 906, 907, 908, 919, D2/920, 921, 922, 923, 946, 947, 948, D2/949, 950, 951, 952, 953, 954, 960, D2/968, 980, 983; D8/349, 382, 387, 47, D8/388, 391, 392, 393, 394, 395, 396, D8/397, 398, 399, 721; D24/107, 133, D24/141, 143, 155, 171, 188, 190, 192, D24/213, 215

CPC A61B 17/151; A61B 17/154; A61B 17/8095; A61B 17/7058; A61B 17/58; A61F 2/00; A61F 2/0009; A61F 2/0022; A61F 2/0063; A61F 2/0077; A61F 2002/0081; A61F 2002/0086; A61F 2002/009; A61F 2002/0091; A61F 2/28; A61F 2/30; A61F 2002/30108; A61F 2002/30112; A61F 2002/30125; A61F 2002/30151; A61F 2002/30153; A61F 2002/30154; A61F 2002/30158; A61F 2002/30199; A61F 2002/30224; A61F 2002/30263; A61F 2002/30266; A61F 2002/30281; A61F 2/38; A61F 2/42; A61F 2/4225; A61F 2/44; A61F 2/4405; A61F 2/441; A61F 2002/4415; A61F

2/442; A61F 2/4425; A61F 2002/443; A61F 2/446; A61F 2/447; A61F 2/60; A61F 2002/6614; A61F 2002/6657; A61F 2002/665; A61F 2/78; A61L 27/00; A61L 2430/38; G06T 2207/30052

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,440,835 A 4/1984 Vignaud
4,588,574 A 5/1986 Felder et al.
(Continued)

OTHER PUBLICATIONS

Sina, "Application logic of triple periodic minimum surface", first available Oct. 24, 2020. (https://k.sina.com.cn/article_2422410454_90630cd600100tlbm.html?from=science) (Year: 2020).*

(Continued)

Primary Examiner — April Rivas
Assistant Examiner — Justin A Johnson
(74) *Attorney, Agent, or Firm* — Morris, Manning & Martin, LLP; Bryan D. Stewart


(57) **CLAIM**

The ornamental design for a spinal implant, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an exemplary spinal implant; FIG. 2 is a top view of an exemplary spinal implant; FIG. 3 is a bottom view of an exemplary spinal implant; FIG. 4 is a side view of an exemplary spinal implant; FIG. 5 is a side view of an exemplary spinal implant; FIG. 6 is a front view of an exemplary spinal implant; and, FIG. 7 is a back view of an exemplary spinal implant. The broken lines illustrate portions of the spinal implant and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

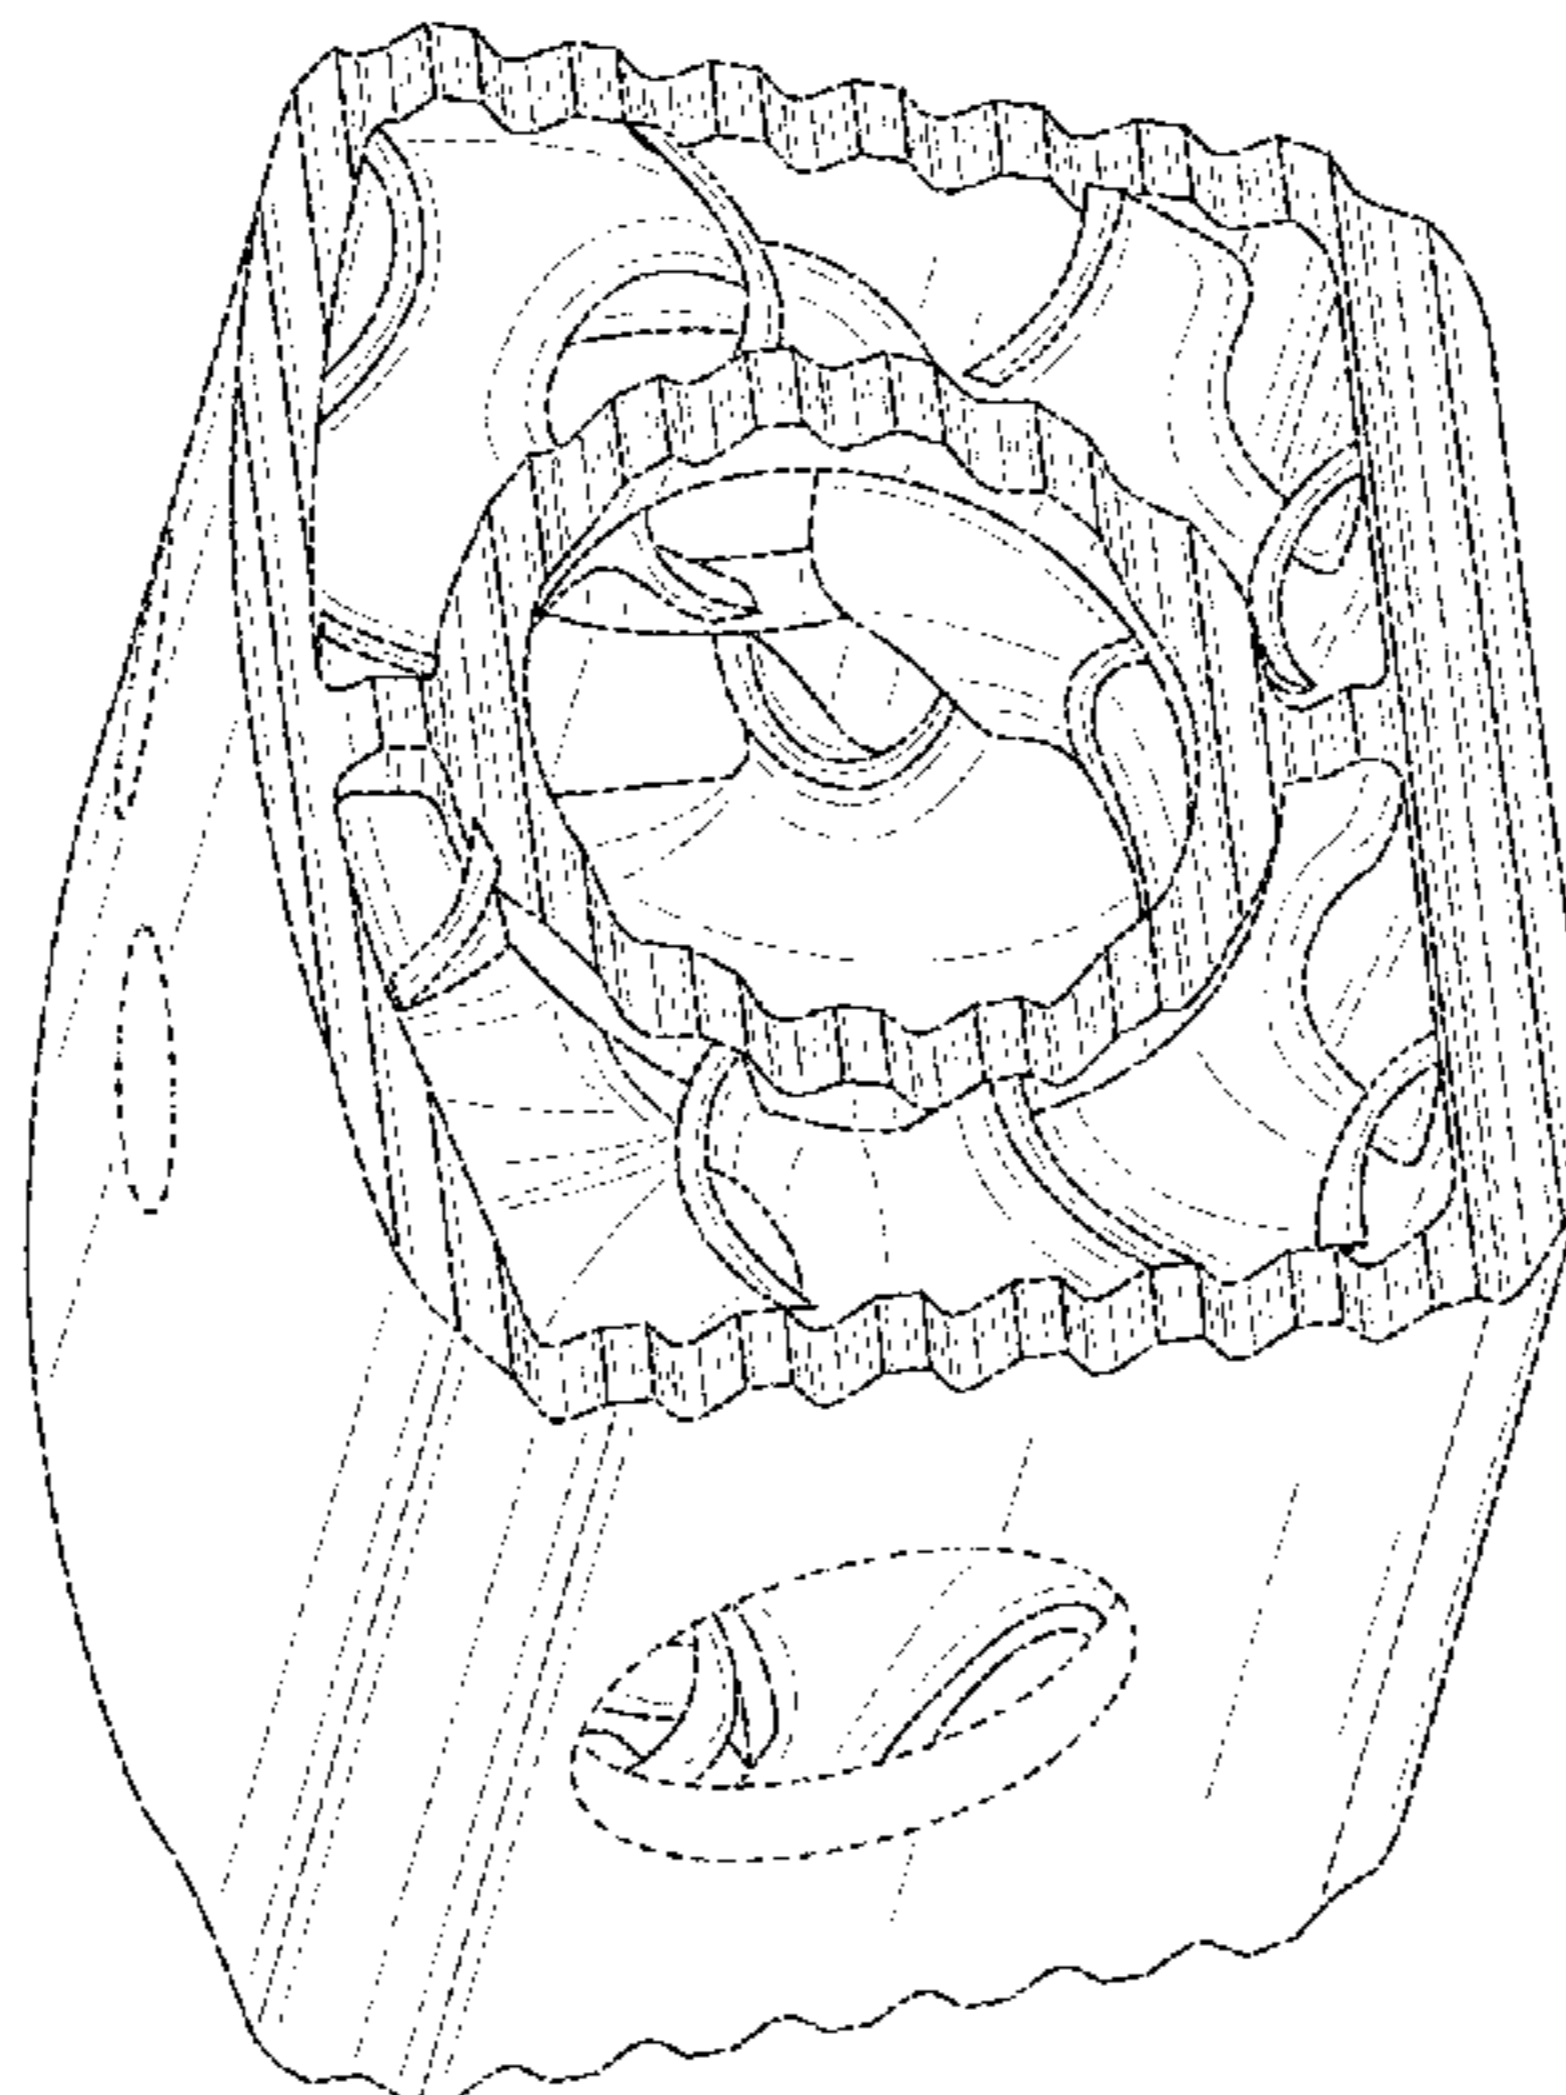

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | | | |
|--------------|-----|---------|--------------------|--------------|--------------|------------------|--------------------------|
| | | | 2007/0118243 | A1 | 5/2007 | Schroeder et al. | |
| | | | 2008/0206297 | A1 | 8/2008 | Roeder et al. | |
| | | | 2009/0093668 | A1 | 4/2009 | Marten et al. | |
| | | | 2009/0182430 | A1* | 7/2009 | Tyber | A61F 2/4465 623/17.16 |
| 5,248,456 | A | 9/1993 | Evans, Jr. et al. | | | | |
| 7,001,672 | B2 | 2/2006 | Justin et al. | | 2010/0137990 | A1 | 6/2010 |
| 7,632,575 | B2 | 12/2009 | Justin et al. | | 2010/0168798 | A1* | 7/2010 |
| 7,666,522 | B2 | 2/2010 | Justin et al. | | | | |
| D653,756 | S | 2/2012 | Courtney et al. | | 2010/0286791 | A1 | 11/2010 |
| 8,142,886 | B2 | 3/2012 | Noble et al. | | 2011/0144752 | A1 | 6/2011 |
| D675,320 | S | 1/2013 | Oi | | 2011/0224796 | A1 | 9/2011 |
| 8,430,930 | B2 | 4/2013 | Hunt | | 2011/0230974 | A1 | 9/2011 |
| 8,457,930 | B2 | 6/2013 | Schroeder | | 2012/0064288 | A1 | 3/2012 |
| 8,485,820 | B1 | 7/2013 | Ali | | 2012/0215310 | A1 | 8/2012 |
| 8,551,173 | B2 | 10/2013 | Lechmann et al. | | 2013/0123935 | A1 | 5/2013 |
| D708,747 | S * | 7/2014 | Curran | D24/155 | 2013/0158651 | A1 | 6/2013 |
| 8,775,133 | B2 | 7/2014 | Schroeder | | 2013/0197657 | A1 | 8/2013 |
| 8,828,311 | B2 | 9/2014 | Medina et al. | | 2013/0218282 | A1 | 8/2013 |
| 8,843,229 | B2 | 9/2014 | Vanasse et al. | | 2014/0107786 | A1 | 4/2014 |
| 8,888,485 | B2 | 11/2014 | Ali | | 2014/0236299 | A1 | 8/2014 |
| D722,693 | S * | 2/2015 | Kaufmann | D24/155 | 2014/0277443 | A1 | 9/2014 |
| 9,034,237 | B2 | 5/2015 | Sperry et al. | | 2014/0288650 | A1 | 9/2014 |
| 9,180,029 | B2 | 11/2015 | Hollister et al. | | 2014/0336680 | A1 | 11/2014 |
| 9,186,257 | B2 | 11/2015 | Geisler et al. | | 2014/0371863 | A1 | 12/2014 |
| D745,159 | S * | 12/2015 | Lin | D24/155 | 2015/0105858 | A1 | 4/2015 |
| D747,485 | S | 1/2016 | Oi | | 2015/0282945 | A1 | 10/2015 |
| 9,271,845 | B2 | 3/2016 | Hunt et al. | | 2015/0282946 | A1 | 10/2015 |
| 9,295,562 | B2 | 3/2016 | Lechmann et al. | | 2015/0320461 | A1 | 11/2015 |
| 9,308,060 | B2 | 4/2016 | Ali | | 2015/0335434 | A1 | 11/2015 |
| 9,339,279 | B2 | 5/2016 | Dubois et al. | | 2015/0343709 | A1 | 12/2015 |
| 9,364,896 | B2 | 6/2016 | Christensen et al. | | 2015/0351915 | A1 | 12/2015 |
| 9,370,426 | B2 | 6/2016 | Gabbrielli et al. | | 2016/0051371 | A1 | 2/2016 |
| 9,421,108 | B2 | 8/2016 | Hunt | | 2016/0089138 | A1 | 3/2016 |
| D767,137 | S * | 9/2016 | Lin | D24/155 | 2016/0151833 | A1 | 6/2016 |
| 9,433,510 | B2 | 9/2016 | Lechmann et al. | | 2016/0193055 | A1 | 7/2016 |
| 9,433,707 | B2 | 9/2016 | Swords et al. | | 2016/0199193 | A1 | 7/2016 |
| 9,545,317 | B2 | 1/2017 | Hunt | | 2016/0213485 | A1 | 7/2016 |
| 9,549,823 | B2 | 1/2017 | Hunt et al. | | 2016/0213486 | A1 | 7/2016 |
| 9,561,115 | B2 | 2/2017 | Elahinia et al. | | 2016/0213487 | A1 | 7/2016 |
| 9,572,669 | B2 | 2/2017 | Hunt et al. | | 2016/0213488 | A1 | 7/2016 |
| 9,597,197 | B2 | 3/2017 | Lechmann et al. | | 2016/0220288 | A1 | 8/2016 |
| 9,636,226 | B2 | 5/2017 | Hunt | | 2016/0256279 | A1 | 9/2016 |
| 9,649,178 | B2 | 5/2017 | Ali | | 2016/0256610 | A1 | 9/2016 |
| 9,662,157 | B2 | 5/2017 | Schneider et al. | | 2016/0270931 | A1 | 9/2016 |
| 9,662,226 | B2 | 5/2017 | Wickham | | 2016/0287388 | A1 | 10/2016 |
| 9,668,863 | B2 | 6/2017 | Sharp et al. | | 2016/0303793 | A1 | 10/2016 |
| 9,675,465 | B2 | 6/2017 | Padovani et al. | | 2016/0333152 | A1 | 11/2016 |
| 9,688,026 | B2 | 6/2017 | Ho et al. | | 2016/0374829 | A1 | 12/2016 |
| 9,694,541 | B2 | 7/2017 | Pruett et al. | | 2017/0014169 | A1 | 1/2017 |
| 9,715,563 | B1 | 7/2017 | Schroeder | | 2017/0020685 | A1 | 1/2017 |
| 9,757,235 | B2 | 9/2017 | Hunt et al. | | 2017/0036403 | A1 | 2/2017 |
| 9,757,245 | B2 | 9/2017 | O'Neil et al. | | 2017/0042697 | A1 | 2/2017 |
| 9,782,270 | B2 | 10/2017 | Wickham | | 2017/0056178 | A1 | 3/2017 |
| 9,788,972 | B2 | 10/2017 | Flickinger et al. | | 2017/0056179 | A1 | 3/2017 |
| D809,661 | S * | 2/2018 | Mueller | D24/155 | 2017/0066873 | A1 | 3/2017 |
| 9,907,670 | B2 | 3/2018 | Deridder et al. | | 2017/0105844 | A1 | 4/2017 |
| 9,910,935 | B2 | 3/2018 | Golway et al. | | 2017/0156880 | A1 | 6/2017 |
| 9,918,849 | B2 | 3/2018 | Morris et al. | | 2017/0165085 | A1 | 6/2017 |
| 9,943,627 | B2 | 4/2018 | Zhou et al. | | 2017/0165790 | A1 | 6/2017 |
| D829,909 | S * | 10/2018 | Horton | D24/155 | 2017/0172758 | A1 | 6/2017 |
| D835,278 | S | 12/2018 | Gottlieb | | 2017/0182222 | A1 | 6/2017 |
| 10,183,442 | B1 | 1/2019 | Miller | | 2017/0209274 | A1 | 7/2017 |
| 10,245,152 | B2 | 4/2019 | Kloss | | 2017/0216035 | A1 | 8/2017 |
| D849,944 | S | 5/2019 | Dacosta | | 2017/0216036 | A1 | 8/2017 |
| D850,620 | S * | 6/2019 | Tyber | D24/155 | 2017/0239054 | A1 | 8/2017 |
| D858,769 | S * | 9/2019 | Barela | A61B 17/8852 | 2017/0239064 | A1 | 8/2017 |
| | | | | | 2017/0245998 | A1 | 8/2017 |
| D877,907 | S * | 3/2020 | Linder | A61F 2/4611 | 2017/0252165 | A1 | 9/2017 |
| | | | | | 2017/0258606 | A1 | 9/2017 |
| D878,589 | S * | 3/2020 | Linder | A61F 2/4465 | 2017/0282455 | A1 | 10/2017 |
| | | | | | 2017/0296244 | A1 | 10/2017 |
| D878,590 | S | 3/2020 | Linder et al. | | 2017/0319344 | A1 | 11/2017 |
| D879,295 | S | 3/2020 | Abbasi | | 2017/0323037 | A1 | 11/2017 |
| D879,961 | S | 3/2020 | Linder et al. | | 2017/0333205 | A1 | 11/2017 |
| D881,665 | S | 4/2020 | Zemel et al. | | 2017/0354510 | A1 | 12/2017 |
| 10,624,746 | B2 | 4/2020 | Jones et al. | | 2017/0354513 | A1 | 12/2017 |
| 10,772,732 | B1 | 9/2020 | Miller et al. | | 2017/0355815 | A1 | 12/2017 |
| D899,900 | S | 10/2020 | Blanco | | 2017/0360488 | A1 | 12/2017 |
| 2004/0148032 | A1 | 7/2004 | Rutter et al. | | 2017/0360563 | A1 | 12/2017 |

(56)

References Cited

U.S. PATENT DOCUMENTS

2017/0360578 A1 12/2017 Shin et al.
 2017/0367843 A1 12/2017 Eisen et al.
 2017/0367844 A1 12/2017 Eisen et al.
 2017/0367845 A1 12/2017 Eisen et al.
 2018/0008419 A1* 1/2018 Tyber A61B 17/8852
 2018/0022017 A1 1/2018 Fukumoto et al.
 2018/0064540 A1 3/2018 Hunt
 2018/0085230 A1 3/2018 Hunt
 2018/0104063 A1 4/2018 Asaad
 2018/0110593 A1 4/2018 Khalil
 2018/0110626 A1 4/2018 McShane, III et al.
 2018/0110627 A1 4/2018 Sack
 2018/0117219 A1 5/2018 Yang et al.
 2018/0147319 A1 5/2018 Colucci-Mizenko et al.
 2018/0289515 A1 10/2018 Nemes et al.
 2019/0262101 A1 8/2019 Shanjani et al.
 2019/0343652 A1 11/2019 Petersheim et al.
 2020/0030102 A1 1/2020 Mullens et al.
 2020/0046512 A1 2/2020 Newman et al.

OTHER PUBLICATIONS

Restor3d, "Products", first available Sep. 28, 2020. (<https://web.archive.org/web/20200928123335/https://restor3d.com/products>) (Year: 2020).*

Indiamart, "Anterior Cervical Fusion Cage for Spine Surgery", first accessed Dec. 9, 2020. (<https://www.indiamart.com/proddetail/anterior-cervical-fusion-cage-12402896897.html>) (Year: 2020).*

Instagram, "restor3d", first available Jul. 21, 2020. (https://www.instagram.com/p/CC6dzt0AKcM/?utm_source=ig_web_copy_link) (Year: 2020).*

Larraona et al., "Radiopaque material for 3D printing scaffolds", XXXV Confreso Anual de la Sociedad Espanola de Ingenieria Biomedica. Bilbao, Nov. 29-Dec. 1, 2017, p. 451-454 (Year: 2017).

Rozema et al., The effects of different steam-sterilization programs on material properties of poly(l-lactide), Journal of Applied Biomaterials, vol. 2, 23-28 (1991) (Year: 1991).

Alt, Sami. "Design for Sterilization Part 1: Steam Sterillization." Material, Material Technology Blog, Jun. 3, 2016, www.material-technology.com/single-post/2016/05/24/Design-for-Sterilization-part-1-Steam-Sterillization.

Ducheyne, Paul. "Comprehensive Biomaterials." Comprehensive Biomaterials, vol. 1, Elsevier, 2011, pp. 135-135.

Anat Ratnovsky et al., Mechanical Properties of Different Airway Stents, Med. Eng'g. Physics, Mar. 2011, at 408., [http://www.medengphys.com/article/S1350-4533\(15\)00042-9/fulltext](http://www.medengphys.com/article/S1350-4533(15)00042-9/fulltext).

Andrew T. Miller et al., Fatigue of Injection Molded and 30 Printed Polycarbonate Urethane in Solution, 108 Polymer 121 (2017).

Andrew T. Miller et al., Deformation and Fatigue of Tough 30 Printed Elastomer Scaffolds Processed by Fused 3 Deposition Modeling and Continuous Liquid Interface Production, 75 J. Mechanical Behavior Biomedical Materials 1 (2017).

* cited by examiner

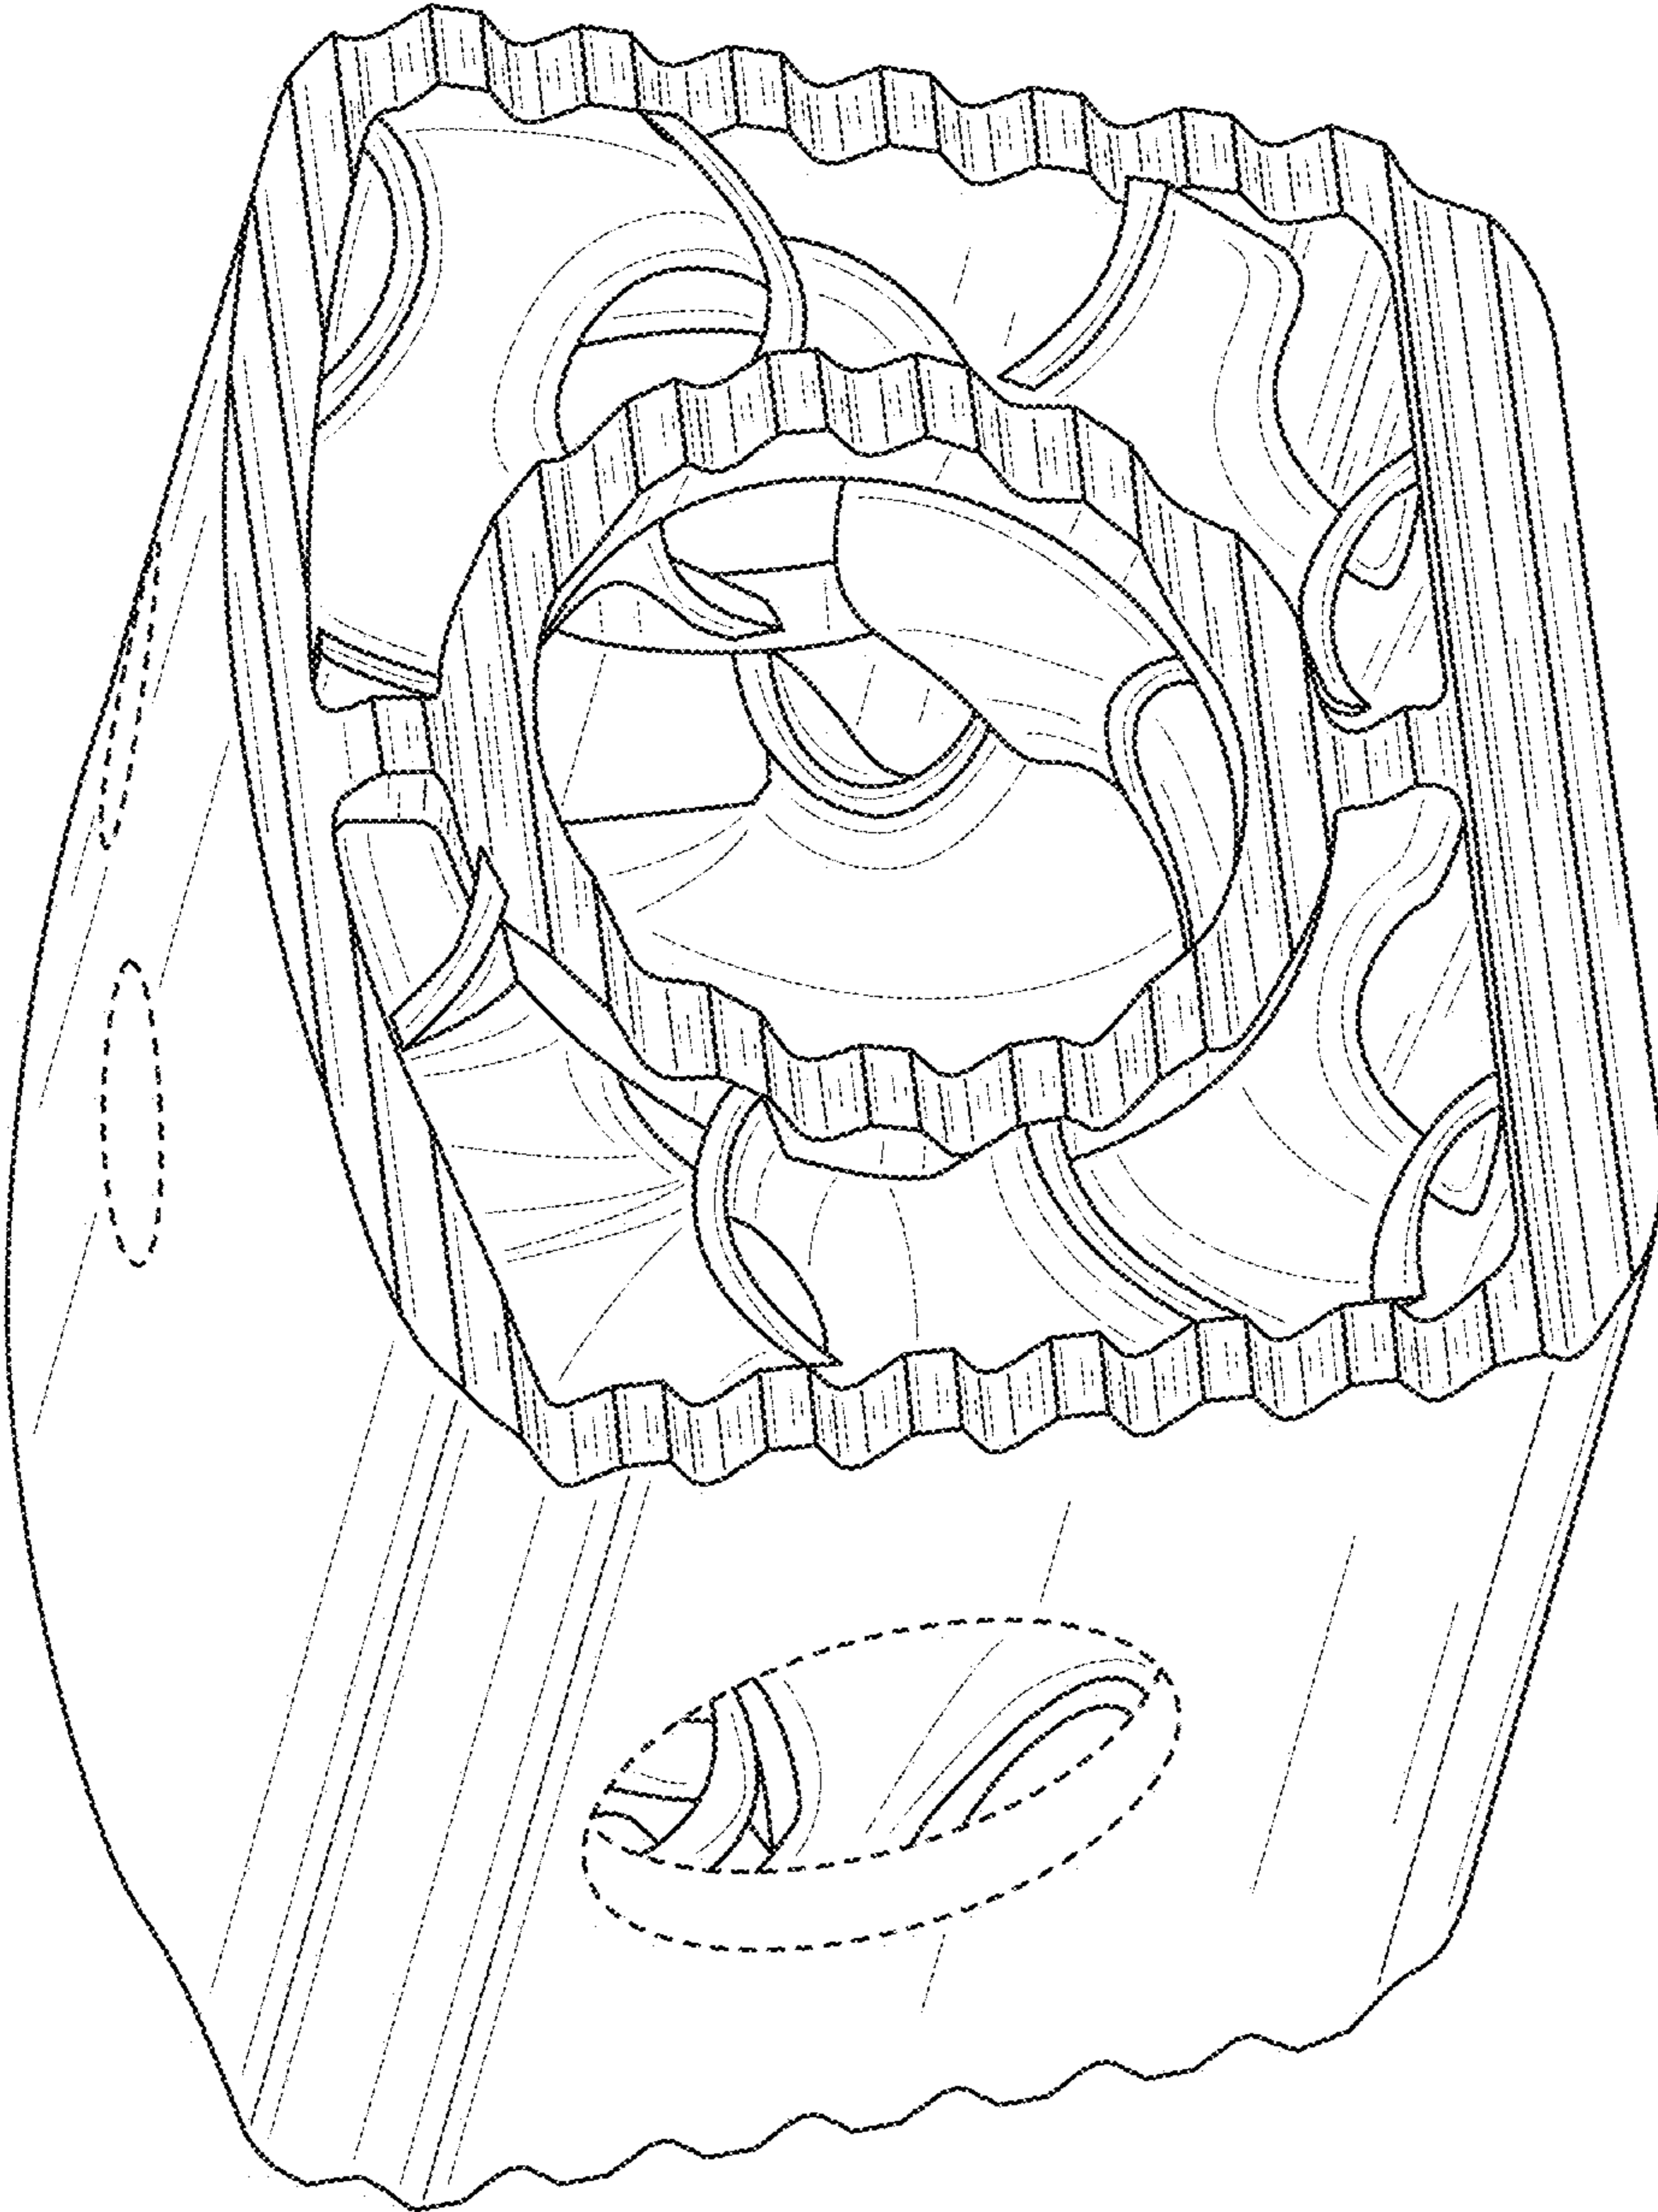


FIG. 1

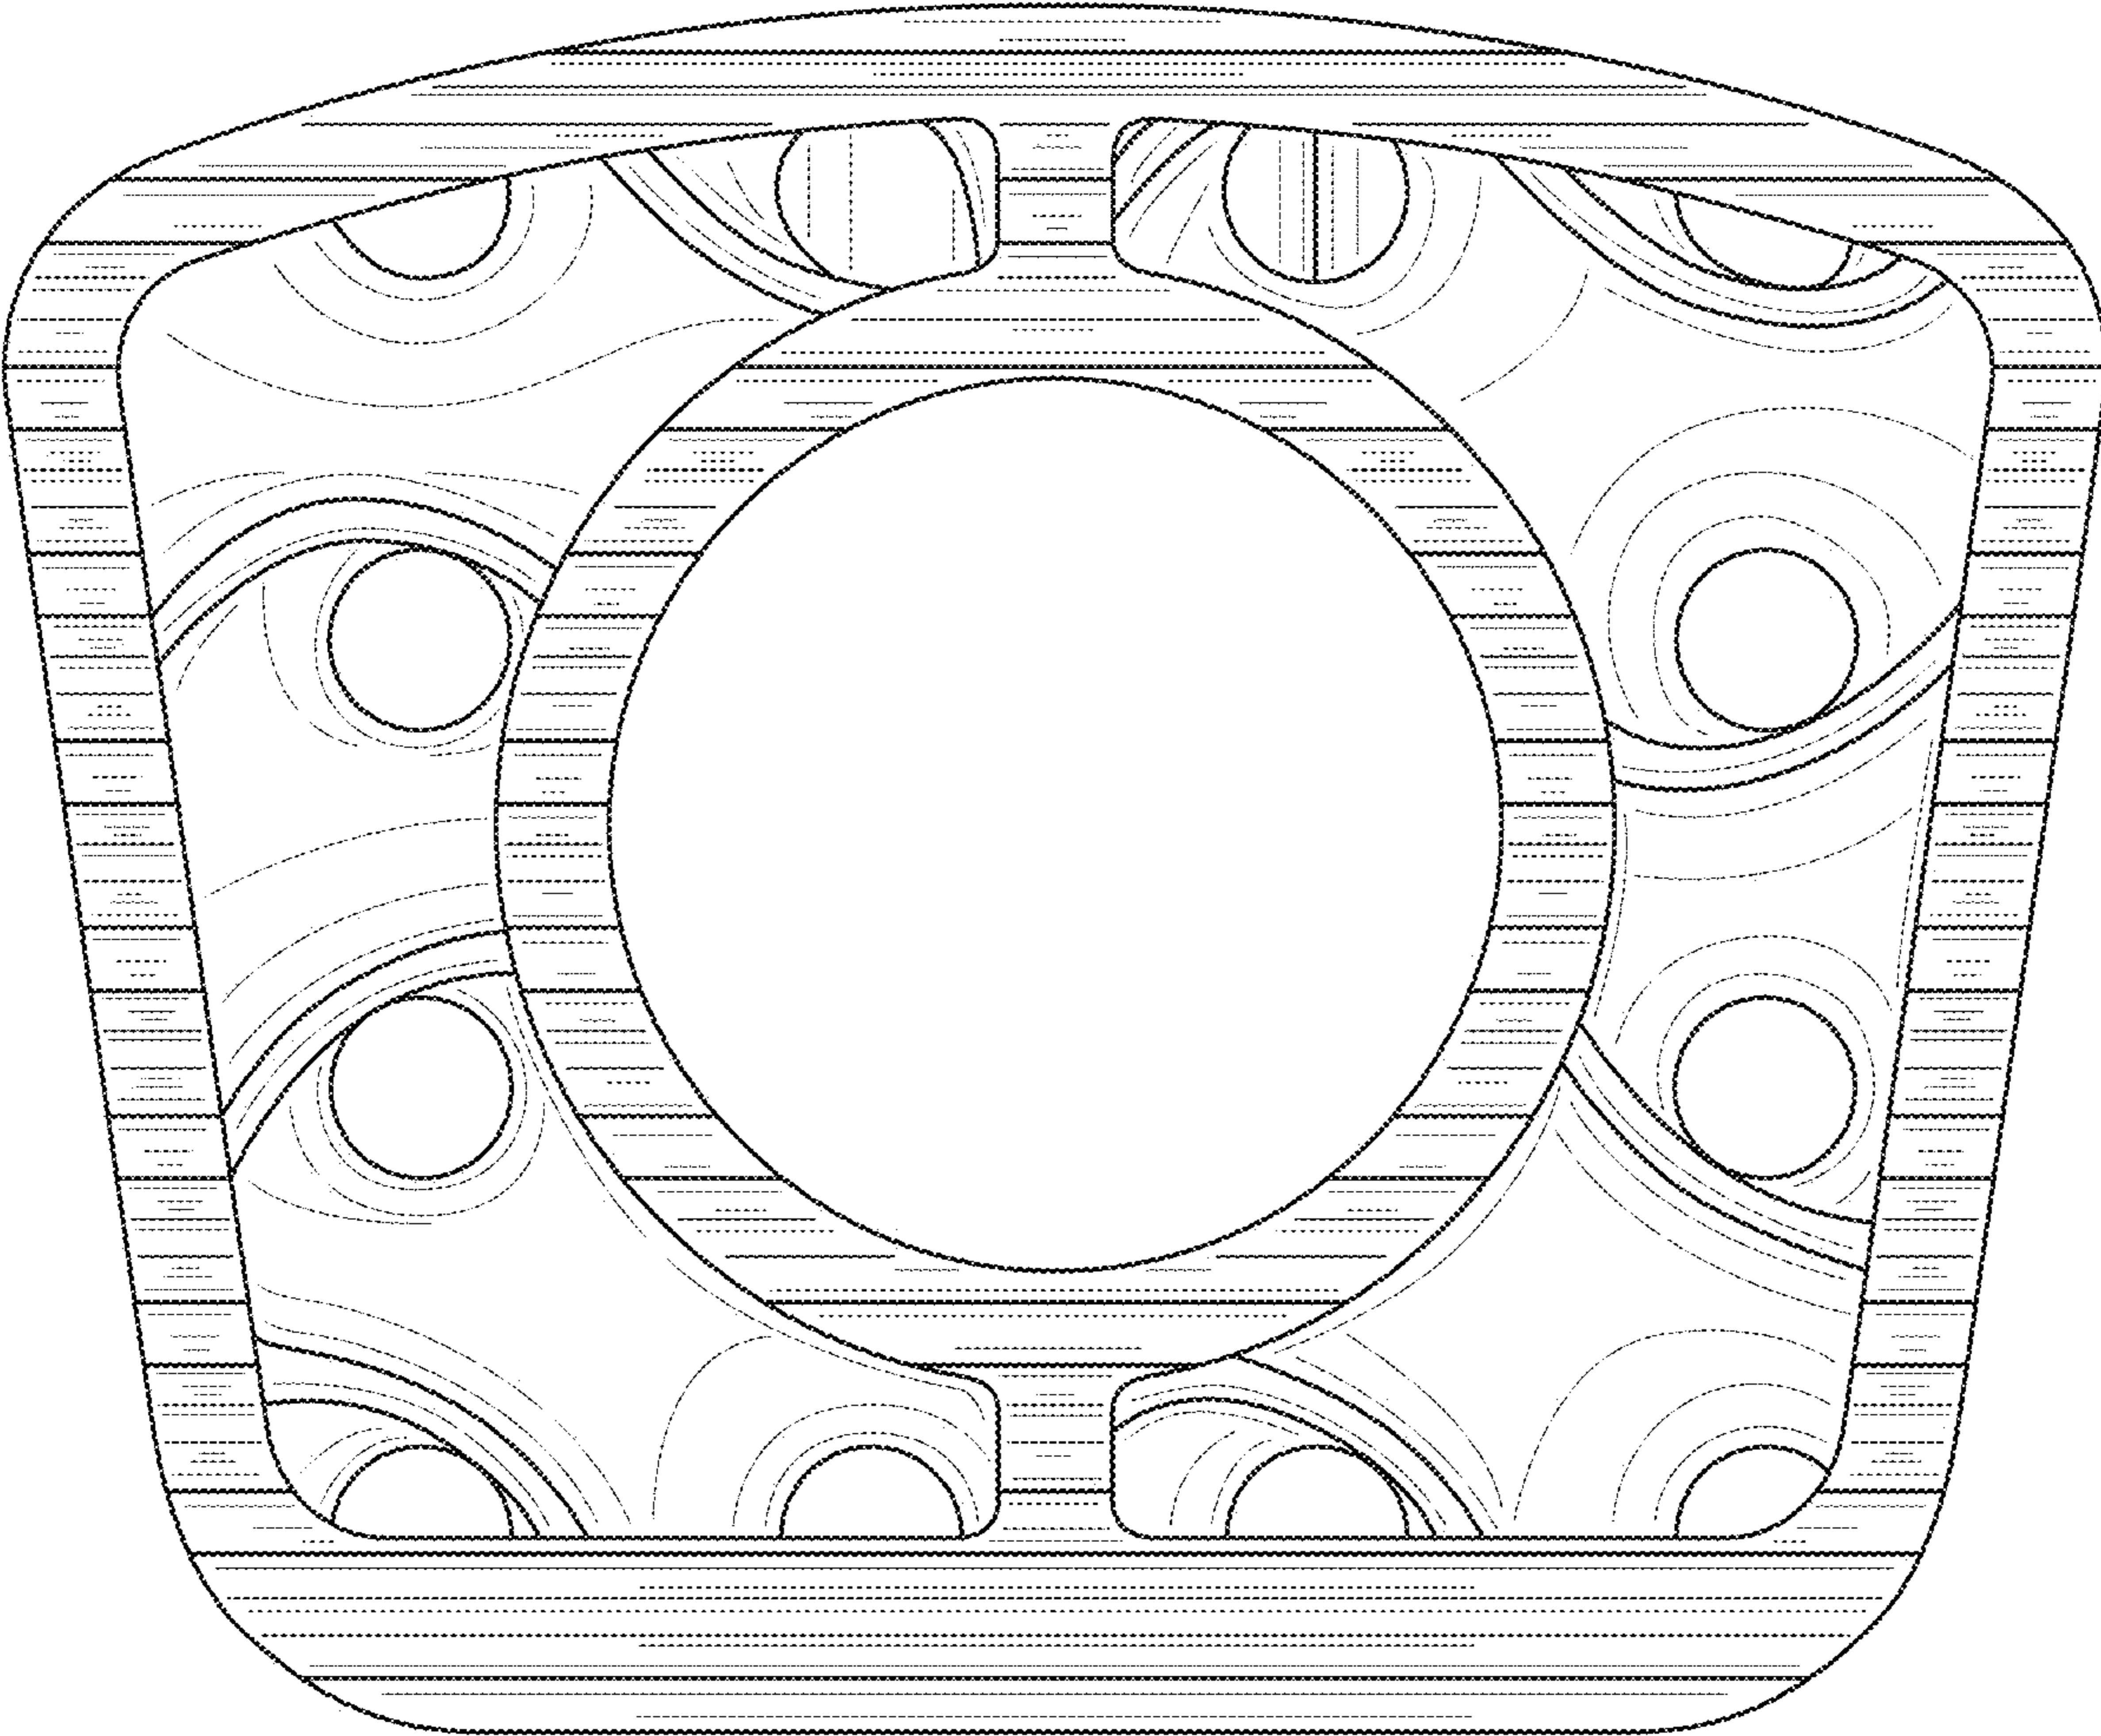


FIG. 2

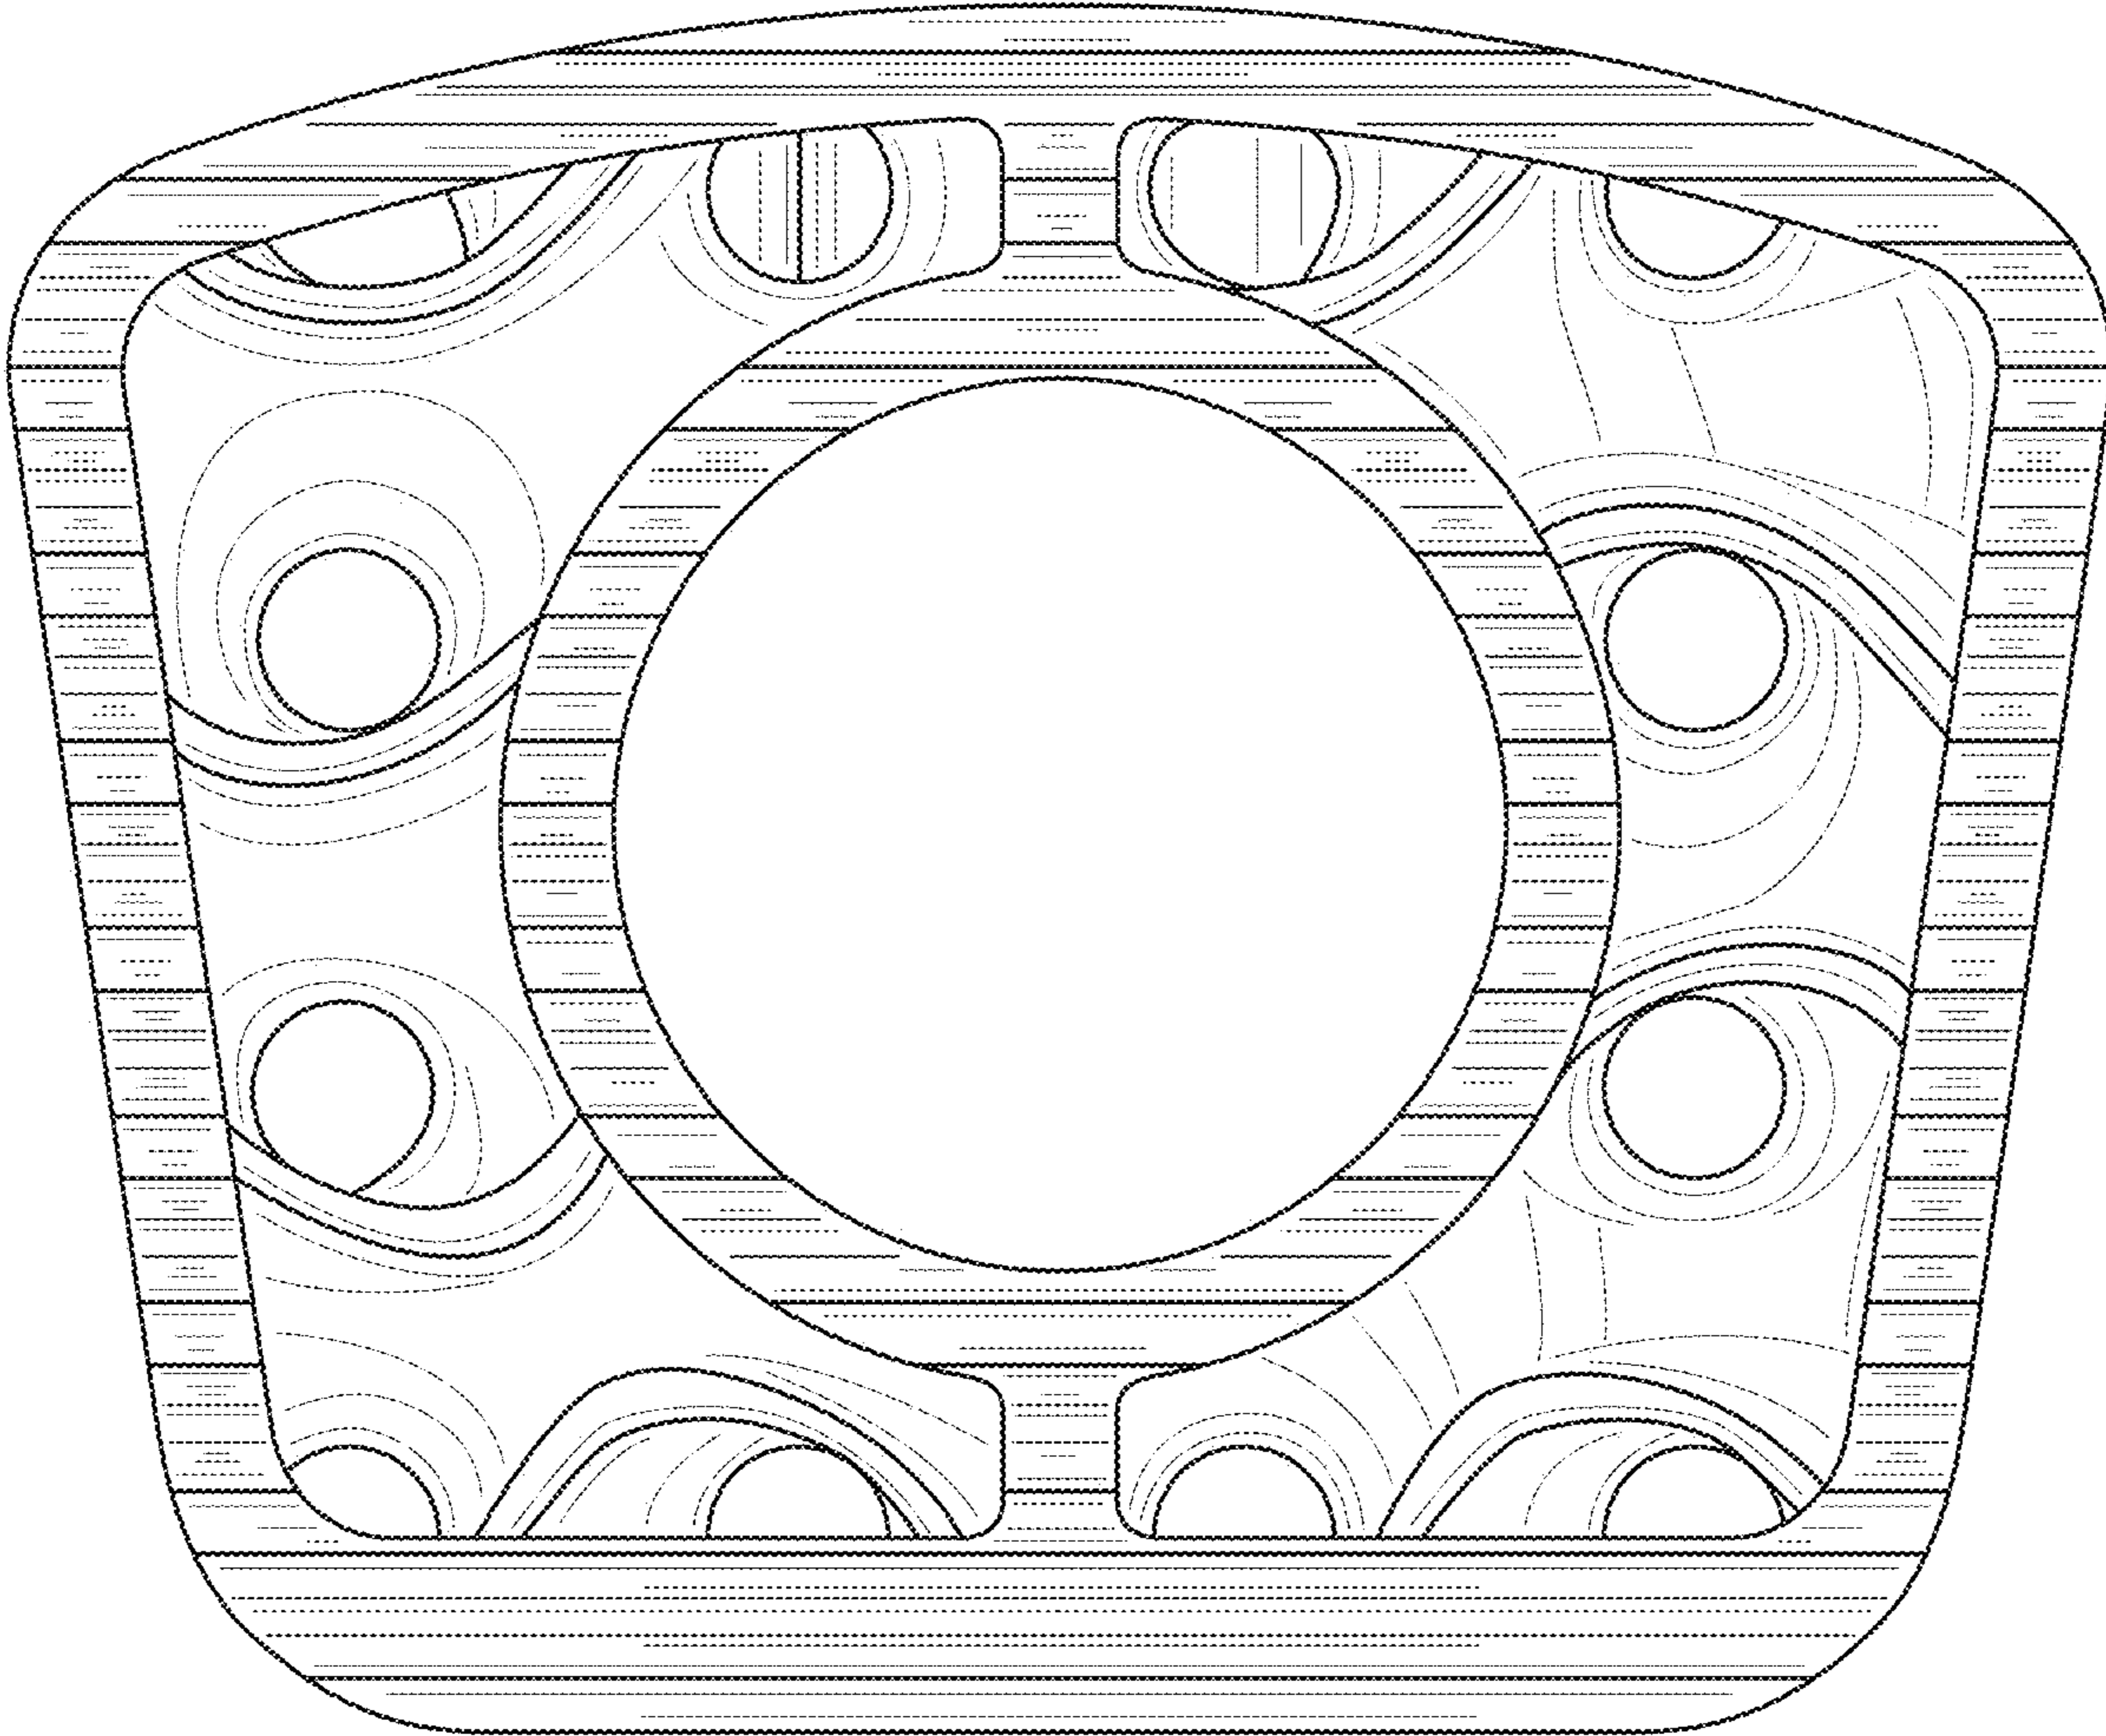


FIG. 3

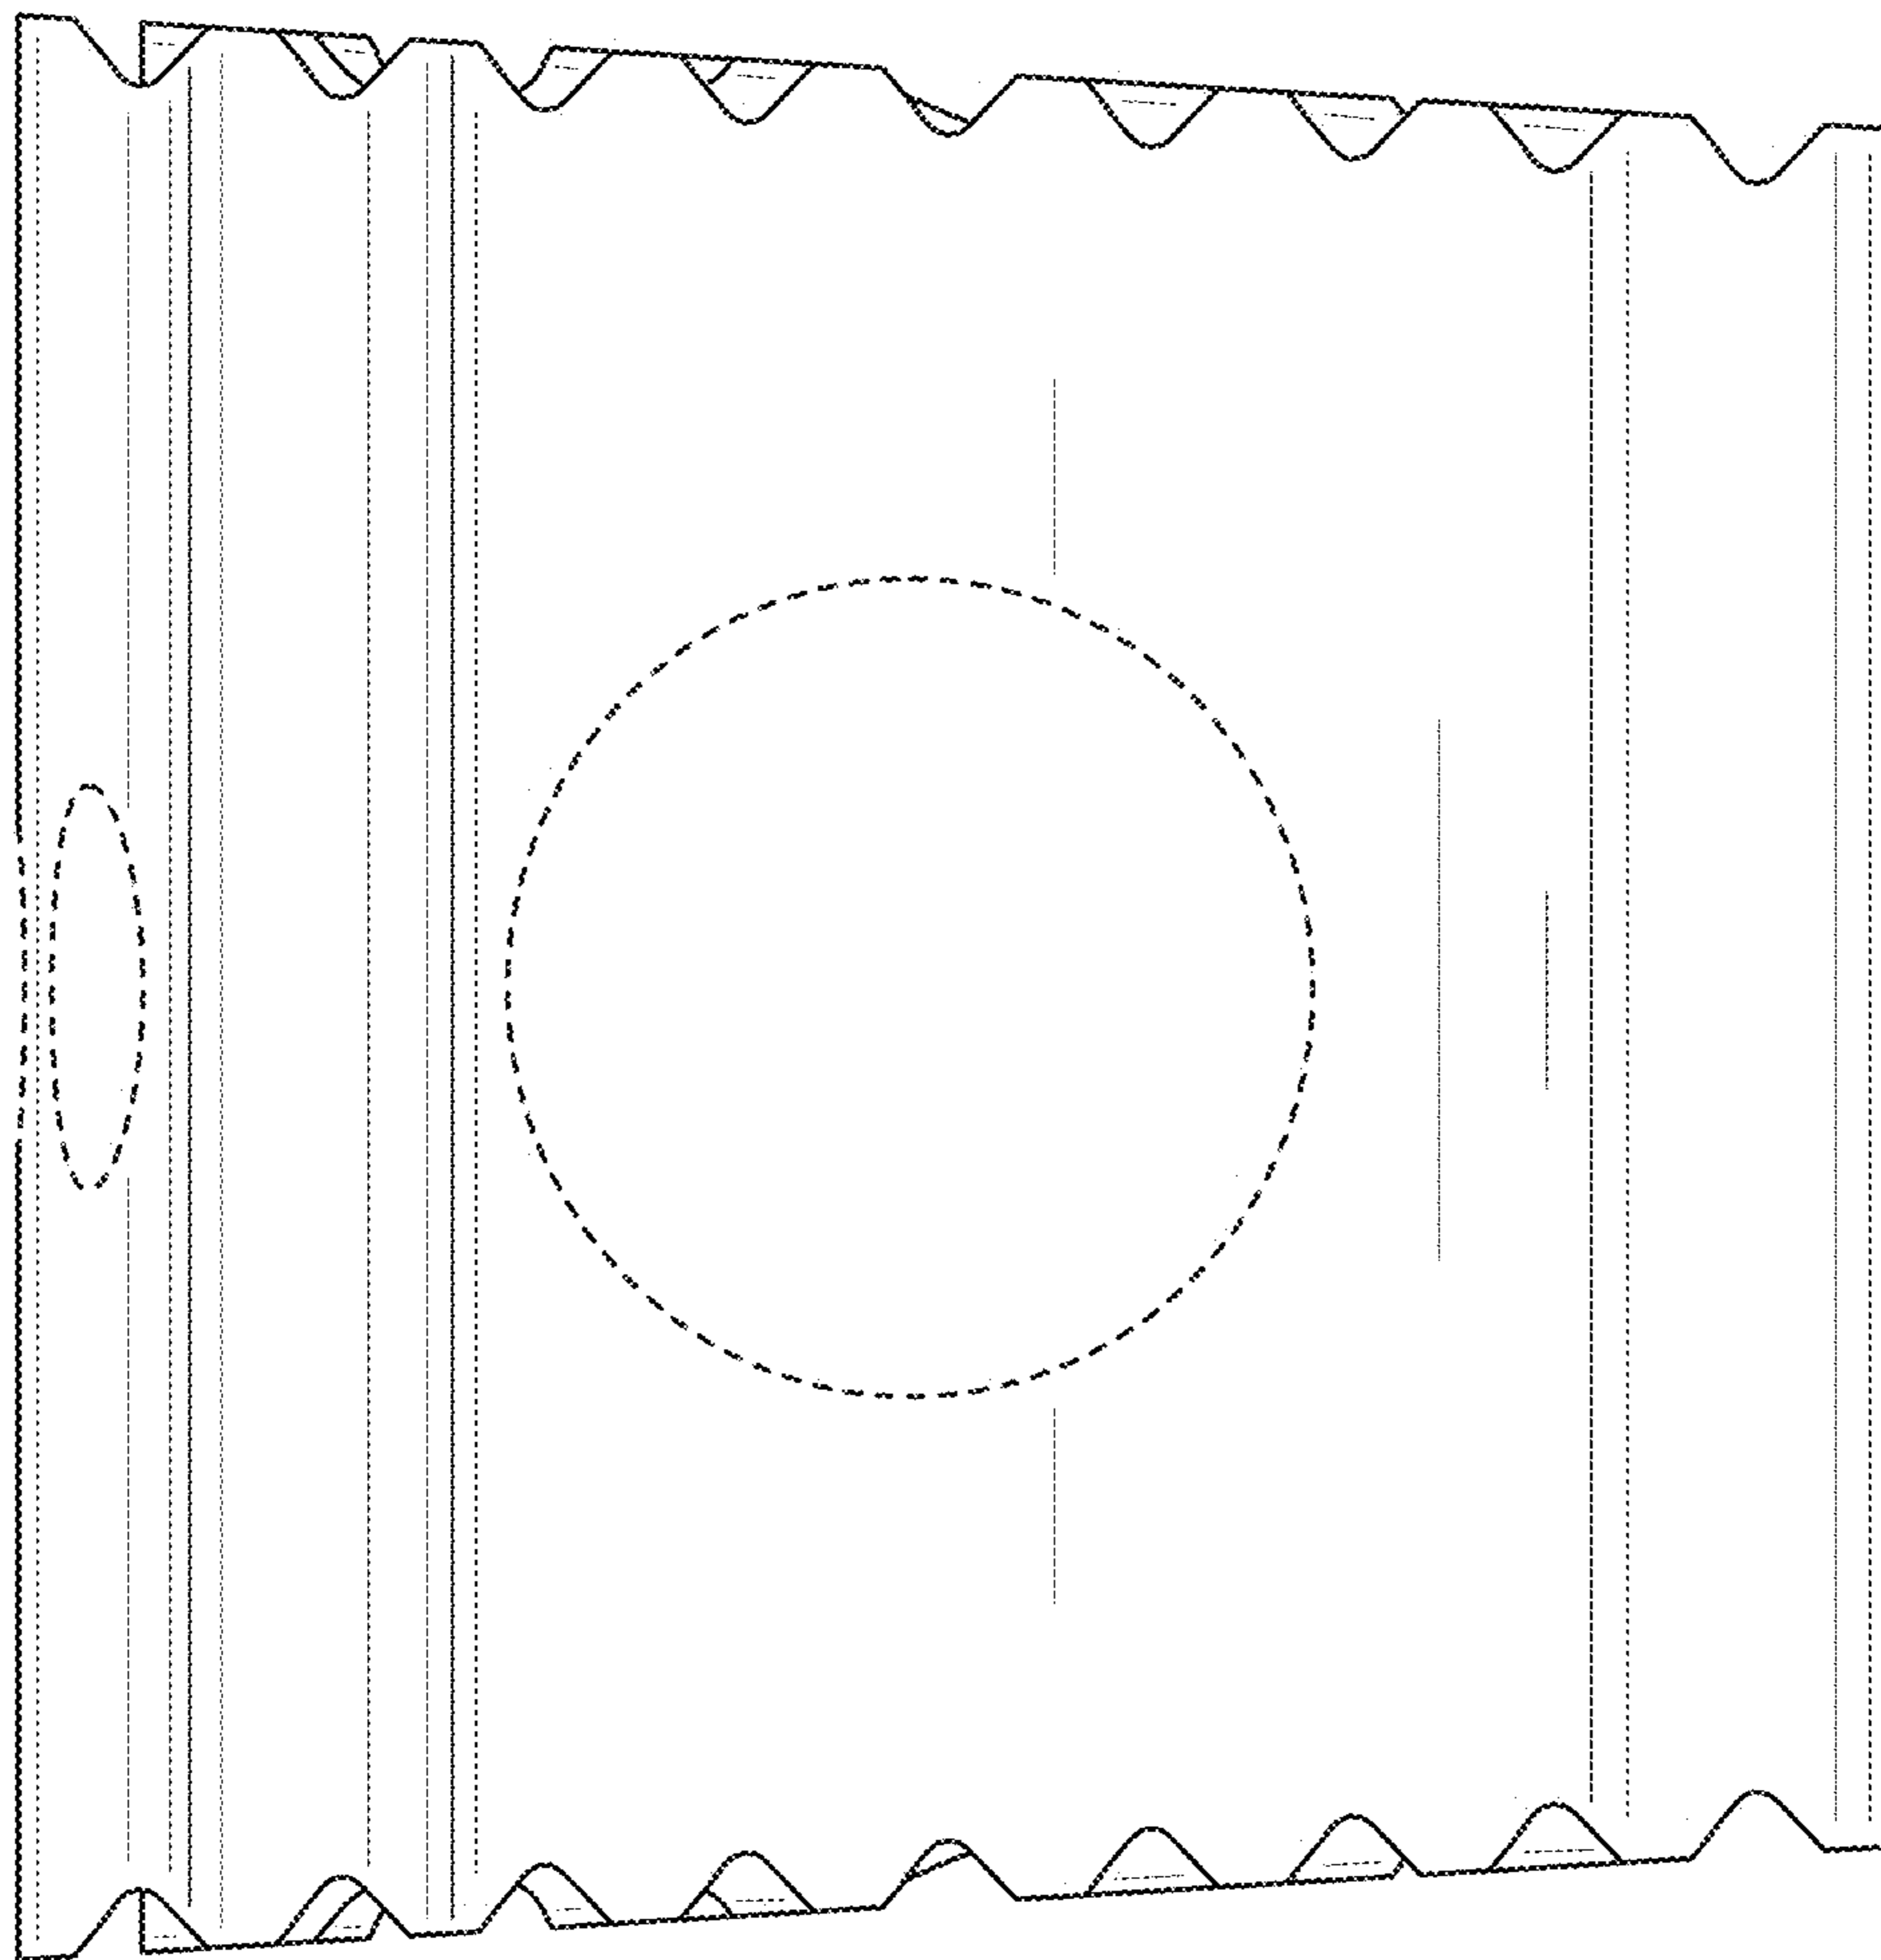


FIG. 4

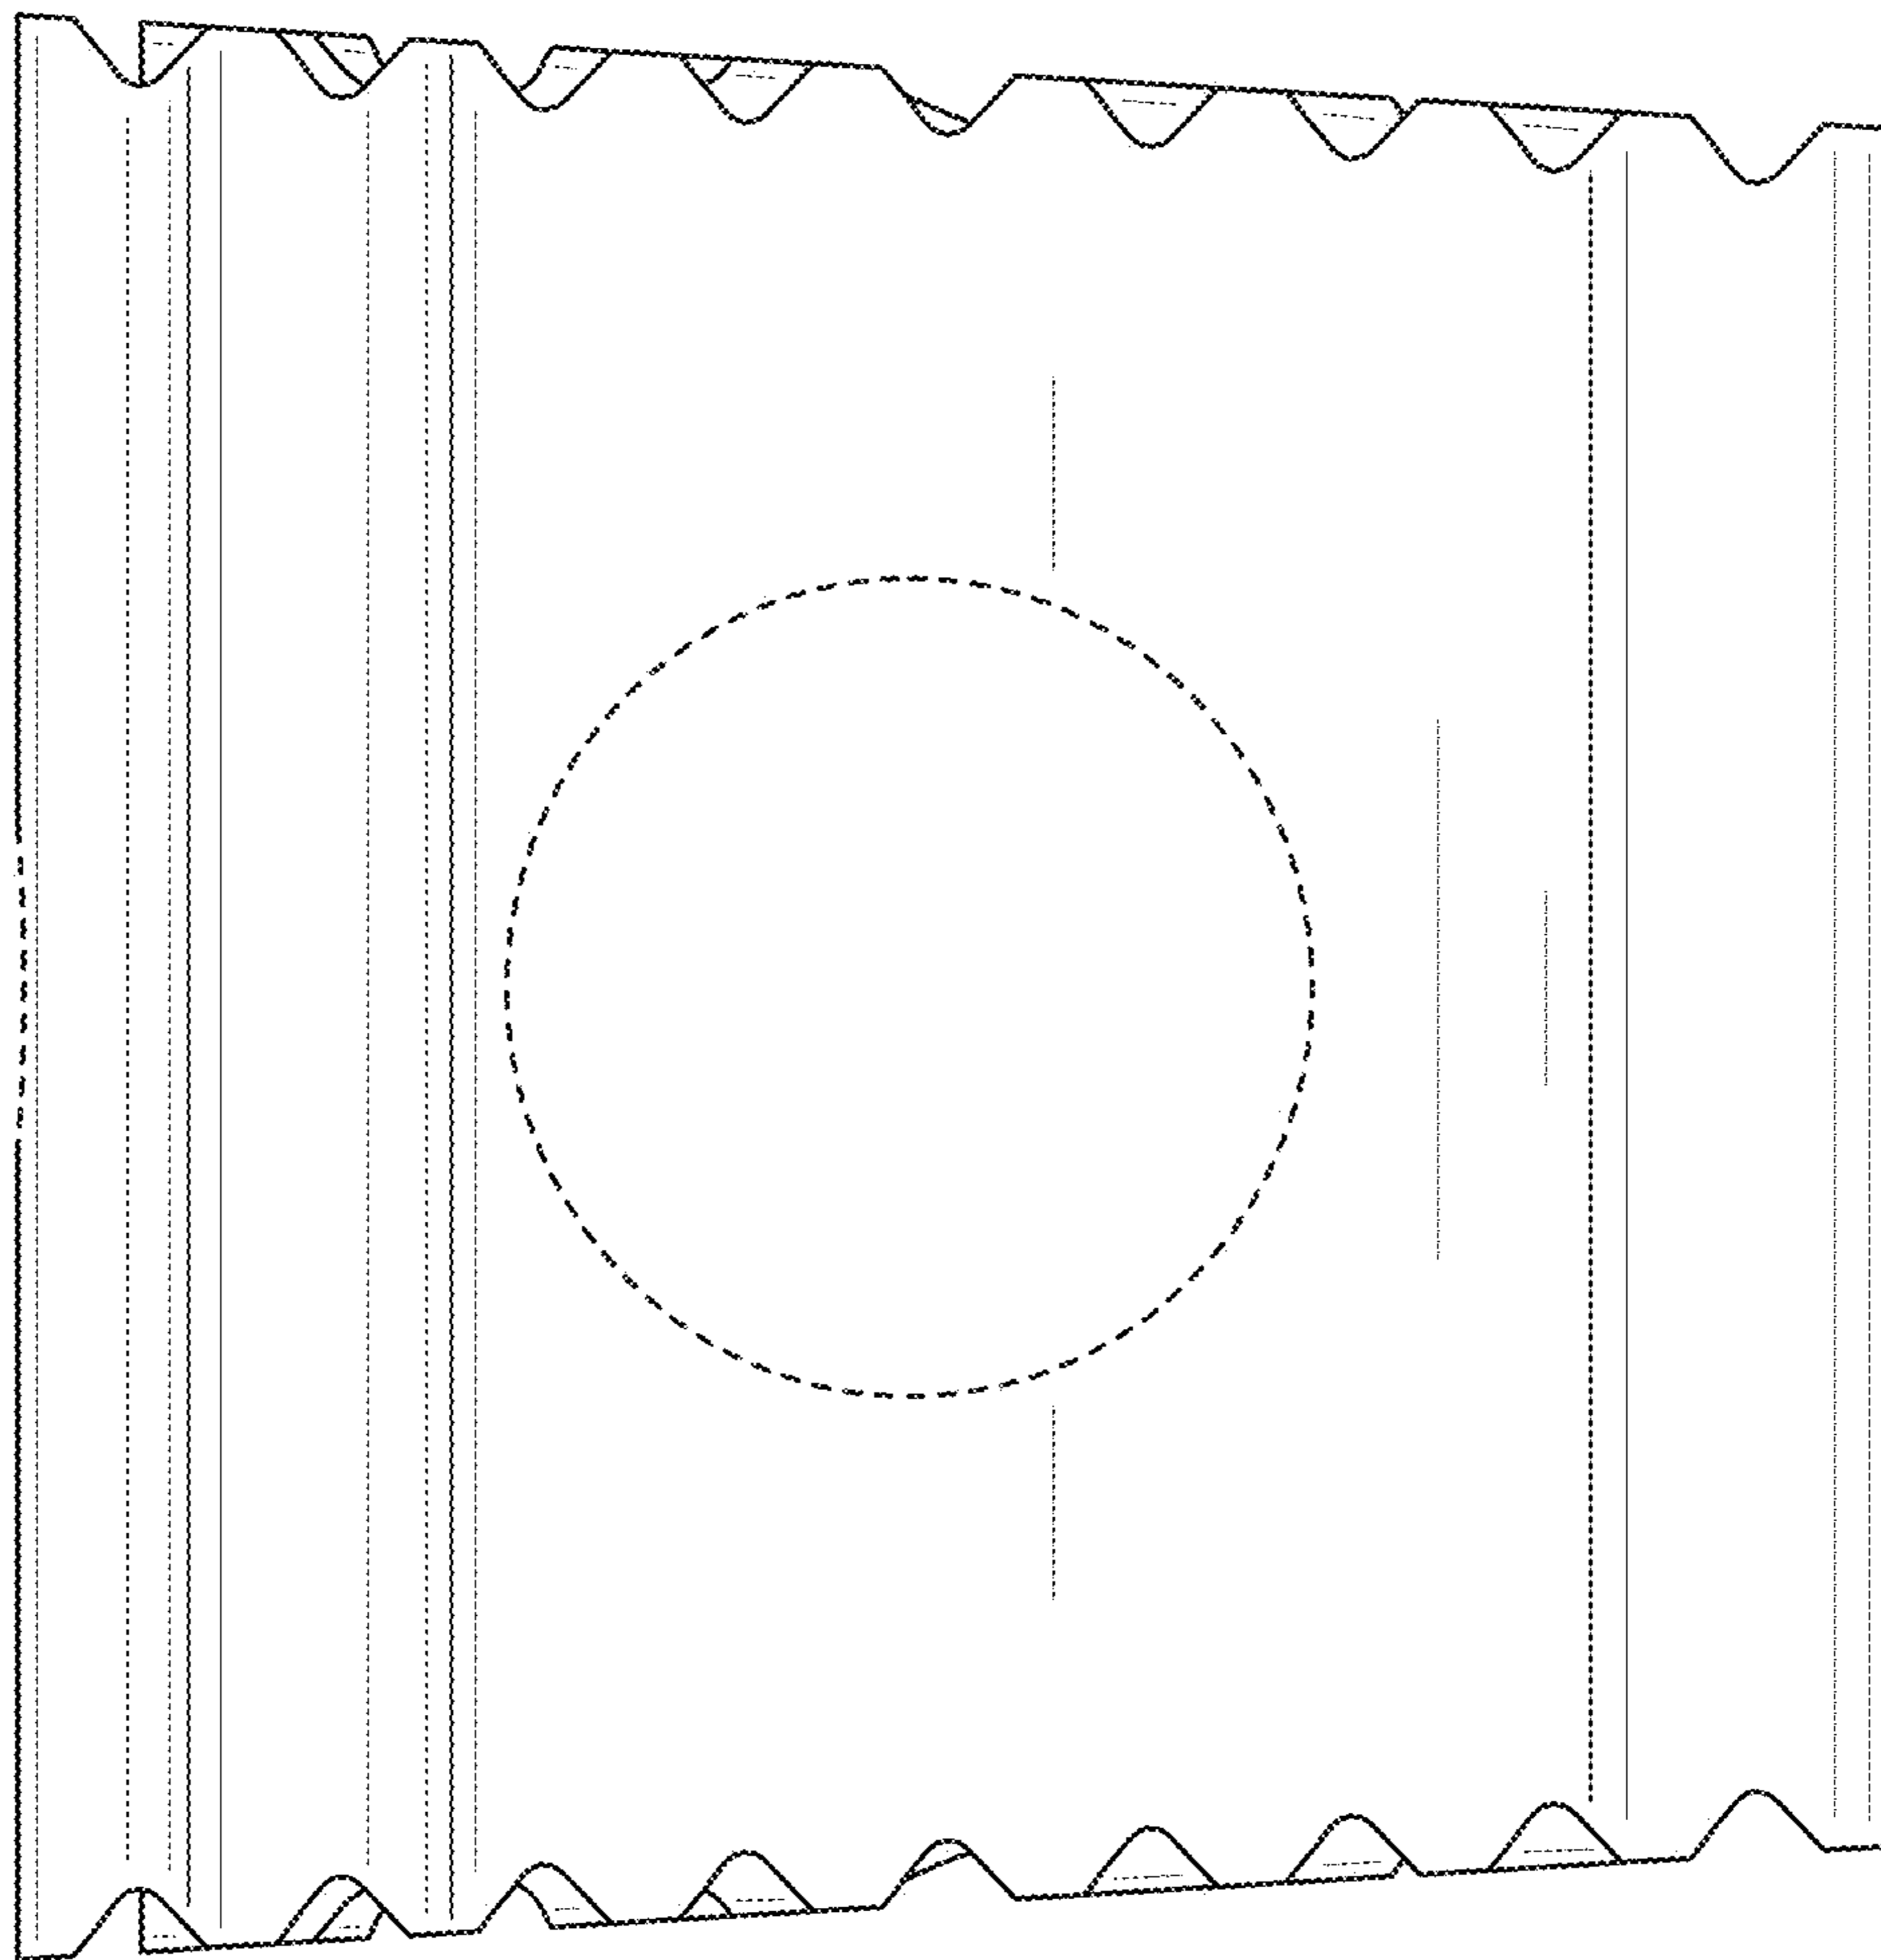


FIG. 5

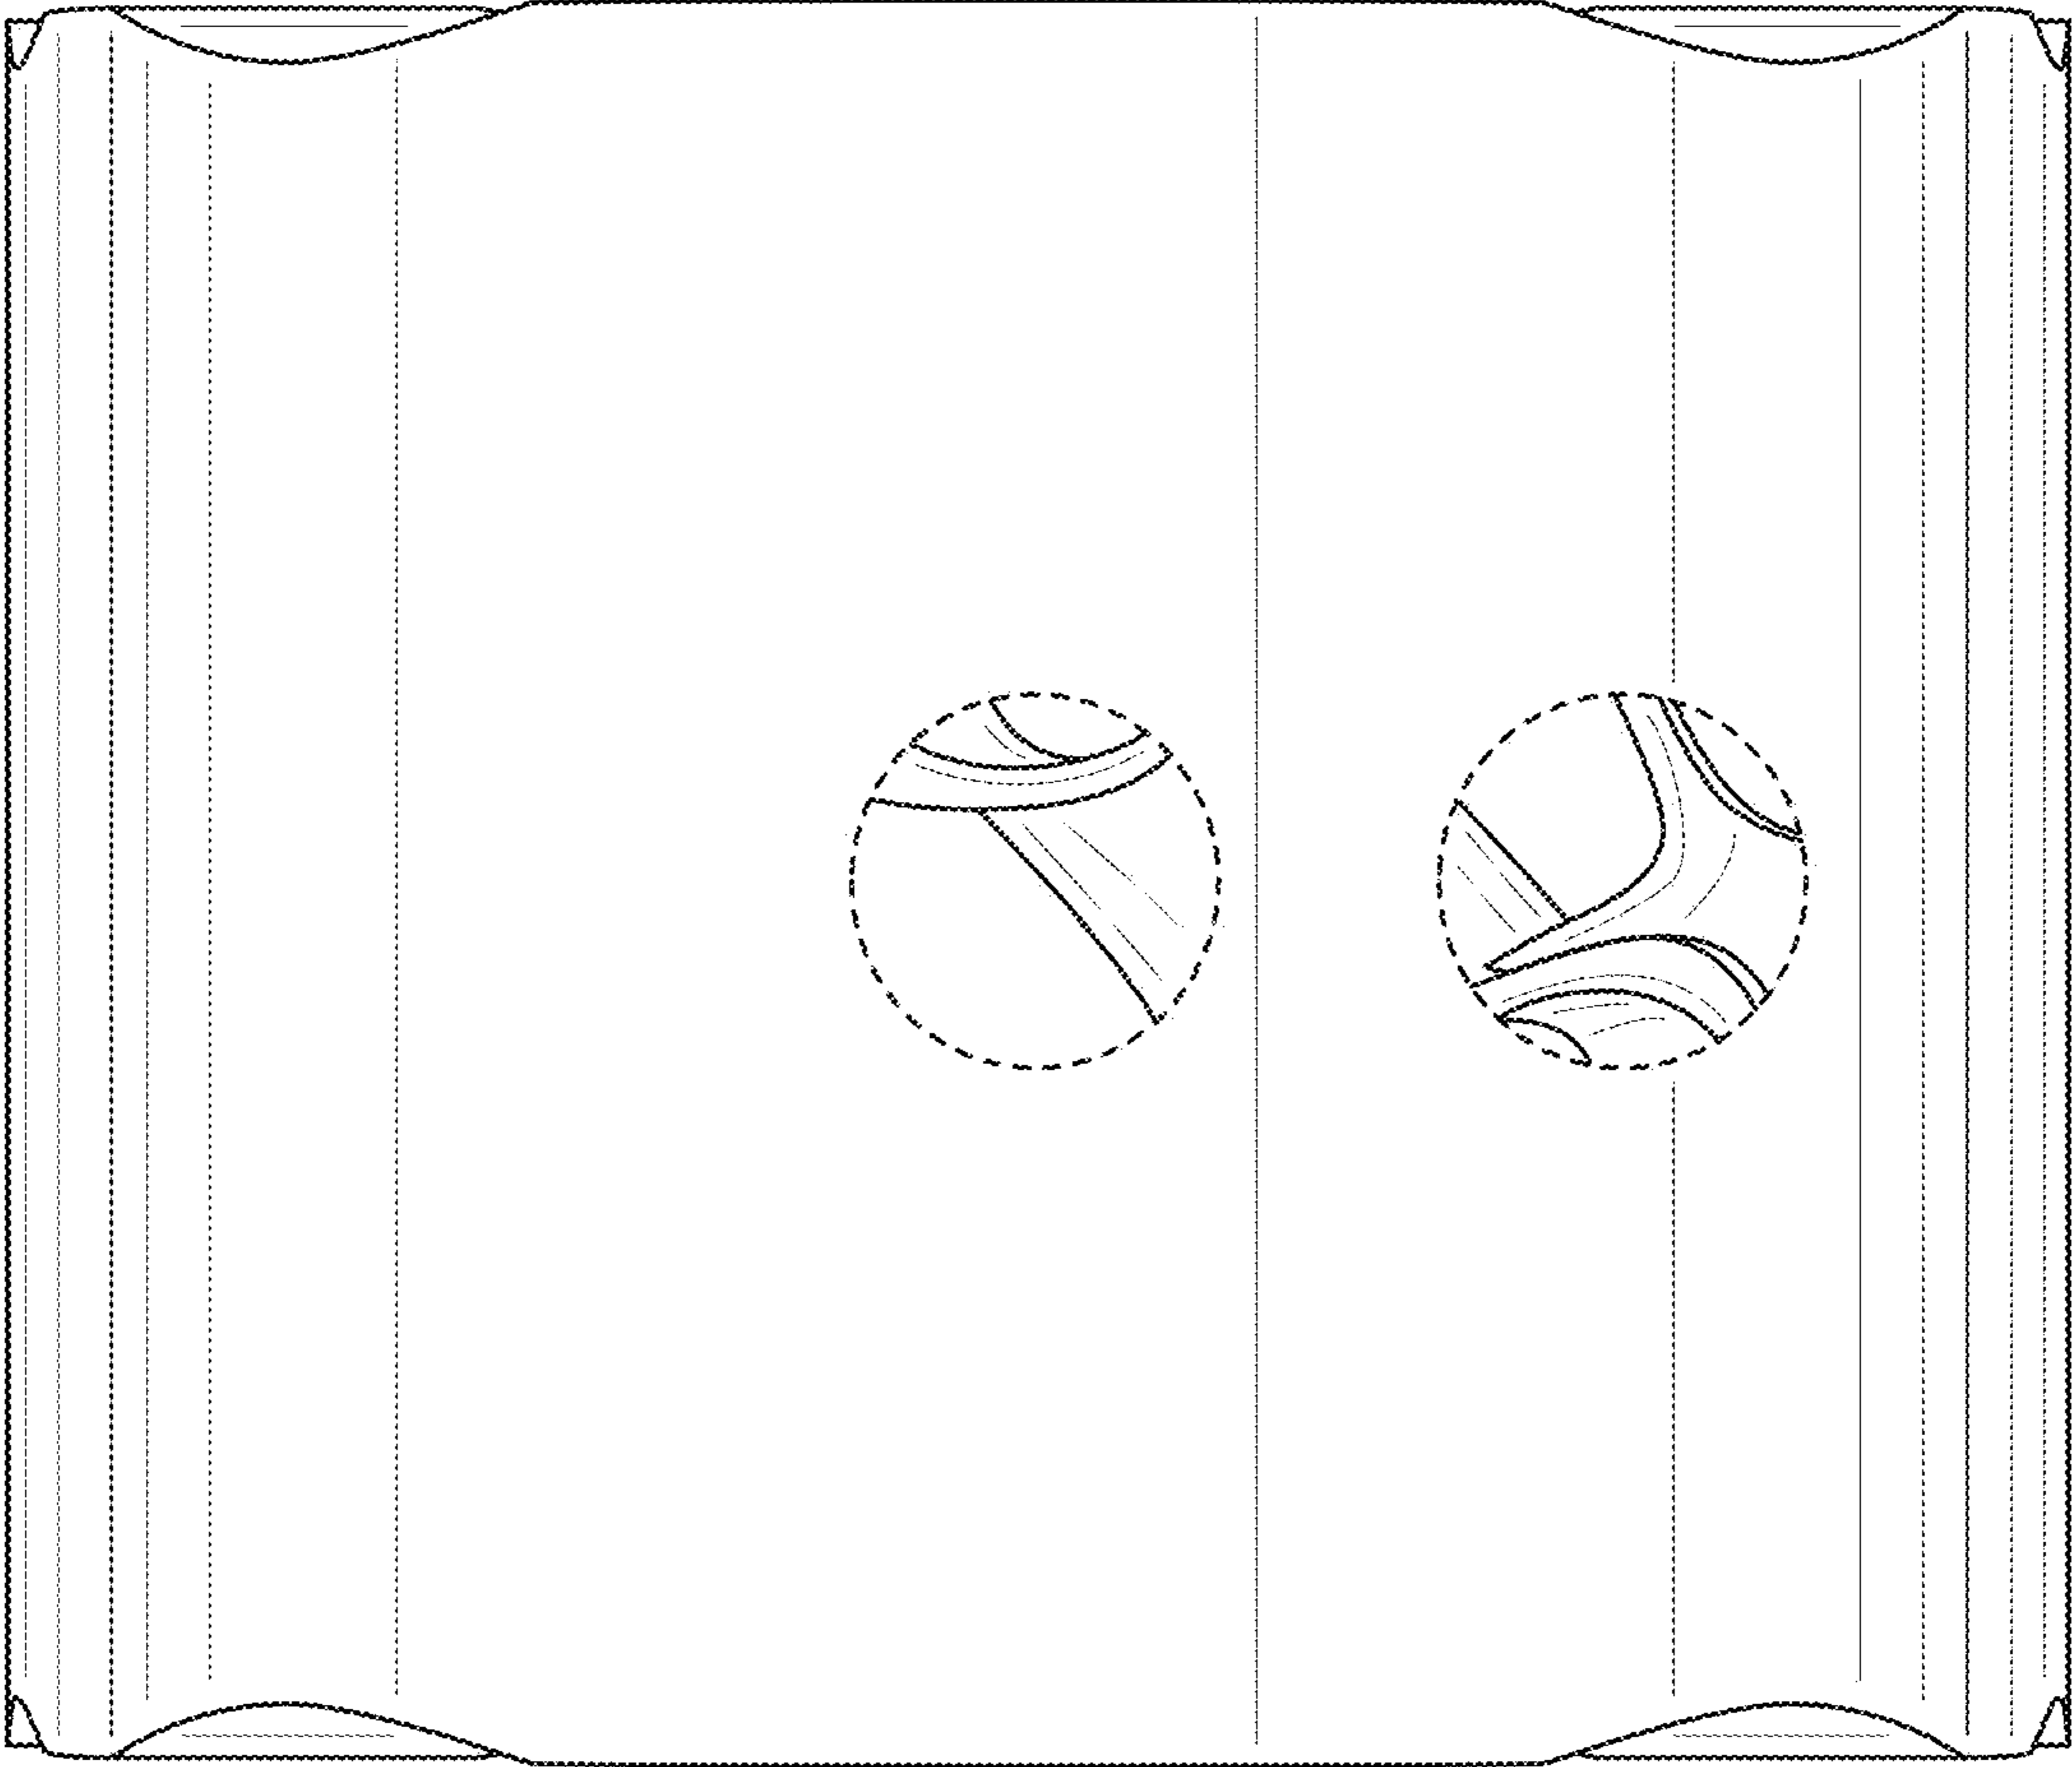


FIG. 6

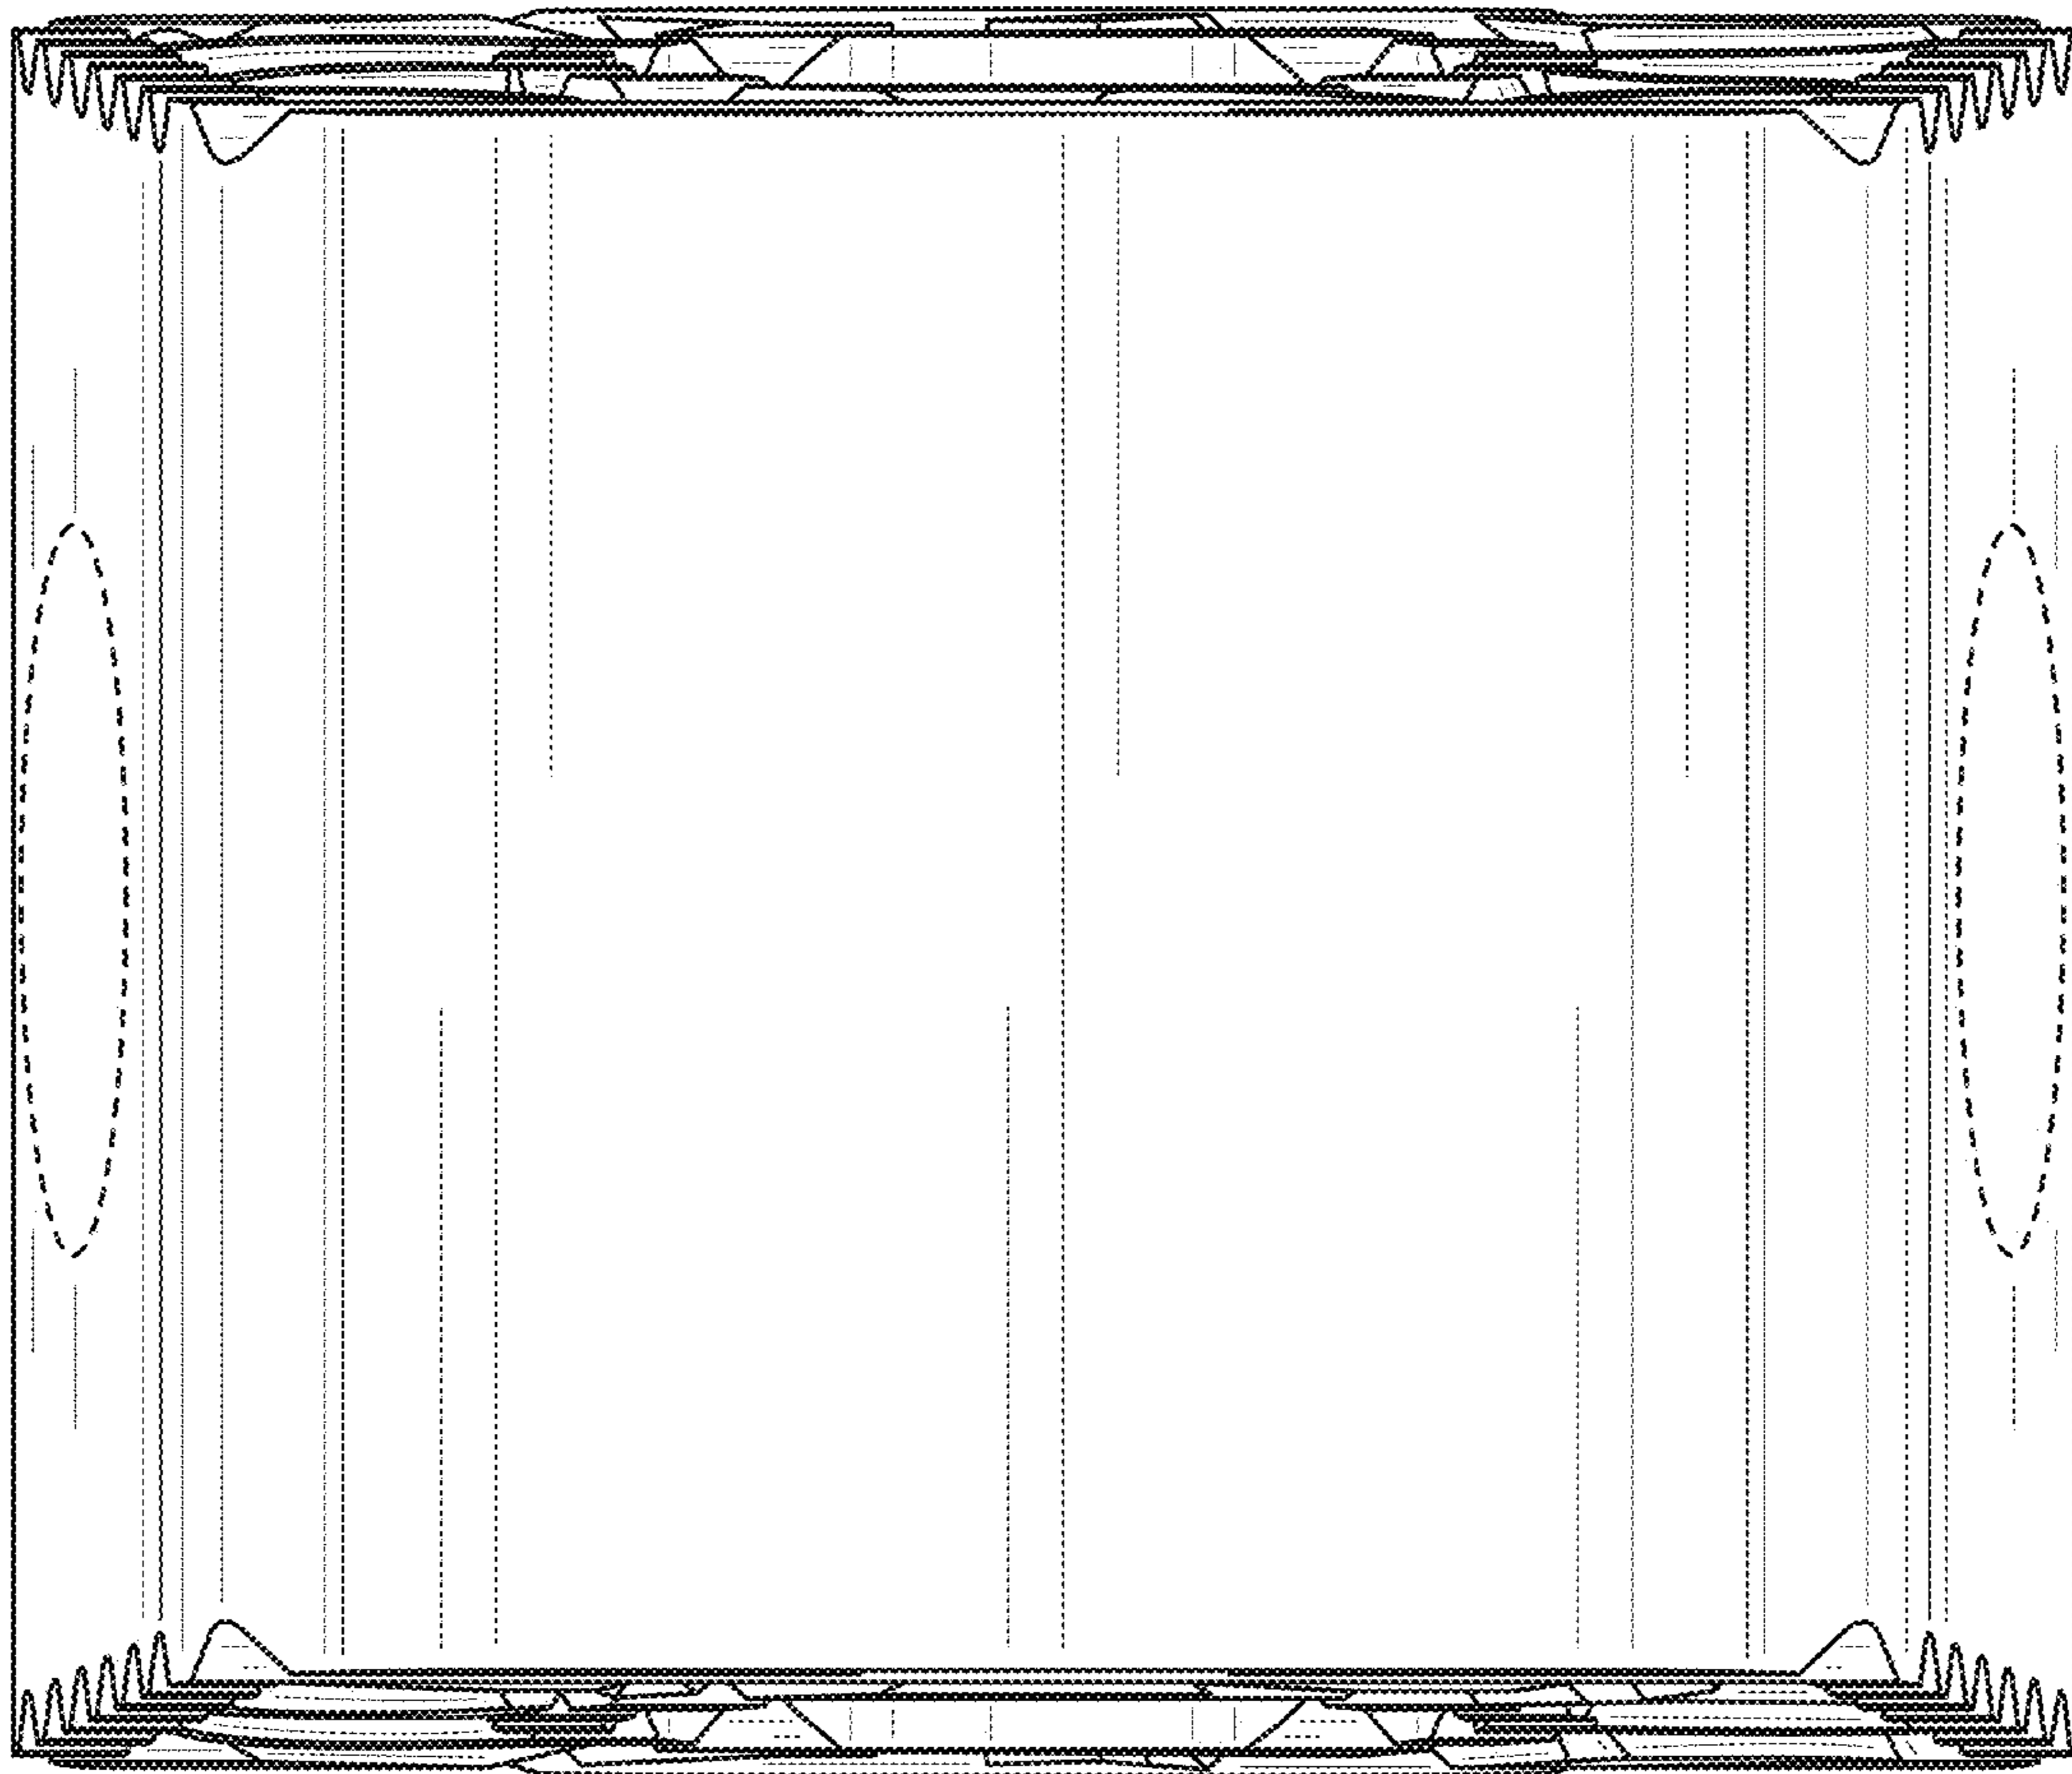


FIG. 7