

US00D920517S

(12) **United States Design Patent** (10) **Patent No.:** **US D920,517 S**
Miller et al. (45) **Date of Patent:** **** May 25, 2021**

(54) **OSTEOTOMY WEDGE**

2/38; A61F 2/42; A61F 2/4225; A61F 2/44; A61F 2/4405; A61F

(71) Applicant: **restor3d, Inc.**, Durham, NC (US)

(Continued)

(72) Inventors: **Andrew Todd Miller**, Durham, NC (US); **Matthew Rexrode**, Durham, NC (US); **Cambre Kelly**, Durham, NC (US); **Ken Gall**, Durham, NC (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,440,835 A	4/1984	Vignaud	
4,588,574 A	5/1986	Felder et al.	
5,248,456 A	9/1993	Evans, Jr. et al.	
7,001,672 B2	2/2006	Justin et al.	
7,632,575 B2	12/2009	Justin et al.	
7,666,522 B2	2/2010	Justin et al.	
D653,756 S *	2/2012	Courtney D24/155

(Continued)

(73) Assignee: **RESTOR3D, INC.**, Durham, NC (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/719,883**

(22) Filed: **Jan. 8, 2020**

OTHER PUBLICATIONS

(51) **LOC (13) Cl.** **24-03**

Ortho Spine News, "SeaSpine Announces 25,000th NanoMetalene Implantation", first available Dec. 18, 2019. (<https://orthospinenews.com/2019/12/18/seaspine-announces-25000th-nanometalene-implantation/>) (Year: 2019).*

(52) **U.S. Cl.**

USPC **D24/155**

(Continued)

(58) **Field of Classification Search**

USPC D2/896, 902, 905, 906, 907, 908, 919, D2/920, 921, 922, 923, 946, 947, 948, D2/949, 950, 951, 952, 953, 954, 960, D2/968, 980, 983; D8/349, 382, 387, 47, D8/388, 391, 392, 393, 394, 395, 396, D8/397, 398, 399, 721; D24/107, 133, D24/141, 143, 155, 171, 188, 190, 192, D24/213, 215

CPC . A61B 17/151; A61B 17/154; A61B 17/8095; A61B 17/7058; A61B 17/58; A61B 2/60; A61B 2002/6614; A61B 2202/6657; A61B 2002/665; A61B 2/78; A61F 2/00; A61F 2/0009; A61F 2/0022; A61F 2/0063; A61F 2/0077; A61F 2002/0081; A61F 2002/0086; A61F 2002/009; A61F 2002/0091; A61F 2/28; A61F 2/30; A61F 2002/30108; A61F 2002/30112; A61F 2002/30125; A61F 2002/30151; A61F 2002/30153; A61F 2002/30154; A61F 2002/30158; A61F 2002/30199; A61F 2002/30224; A61F 2002/30263; A61F 2002/30266; A61F 2002/30281; A61F

Primary Examiner — April Rivas
Assistant Examiner — Justin A Johnson
(74) *Attorney, Agent, or Firm* — Morris, Manning & Martin, LLP; Bryan D. Stewart


(57) **CLAIM**

The ornamental design for an osteotomy wedge, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an exemplary osteotomy wedge;
FIG. 2 is a top view of an exemplary osteotomy wedge;
FIG. 3 is a bottom view of an exemplary osteotomy wedge;
FIG. 4 is a side view of an exemplary osteotomy wedge;
FIG. 5 is a side view of an exemplary osteotomy wedge;
FIG. 6 is a front view of an exemplary osteotomy wedge;
and,
FIG. 7 is a back view of an exemplary osteotomy wedge.
The broken lines illustrate portions of the osteotomy wedge and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

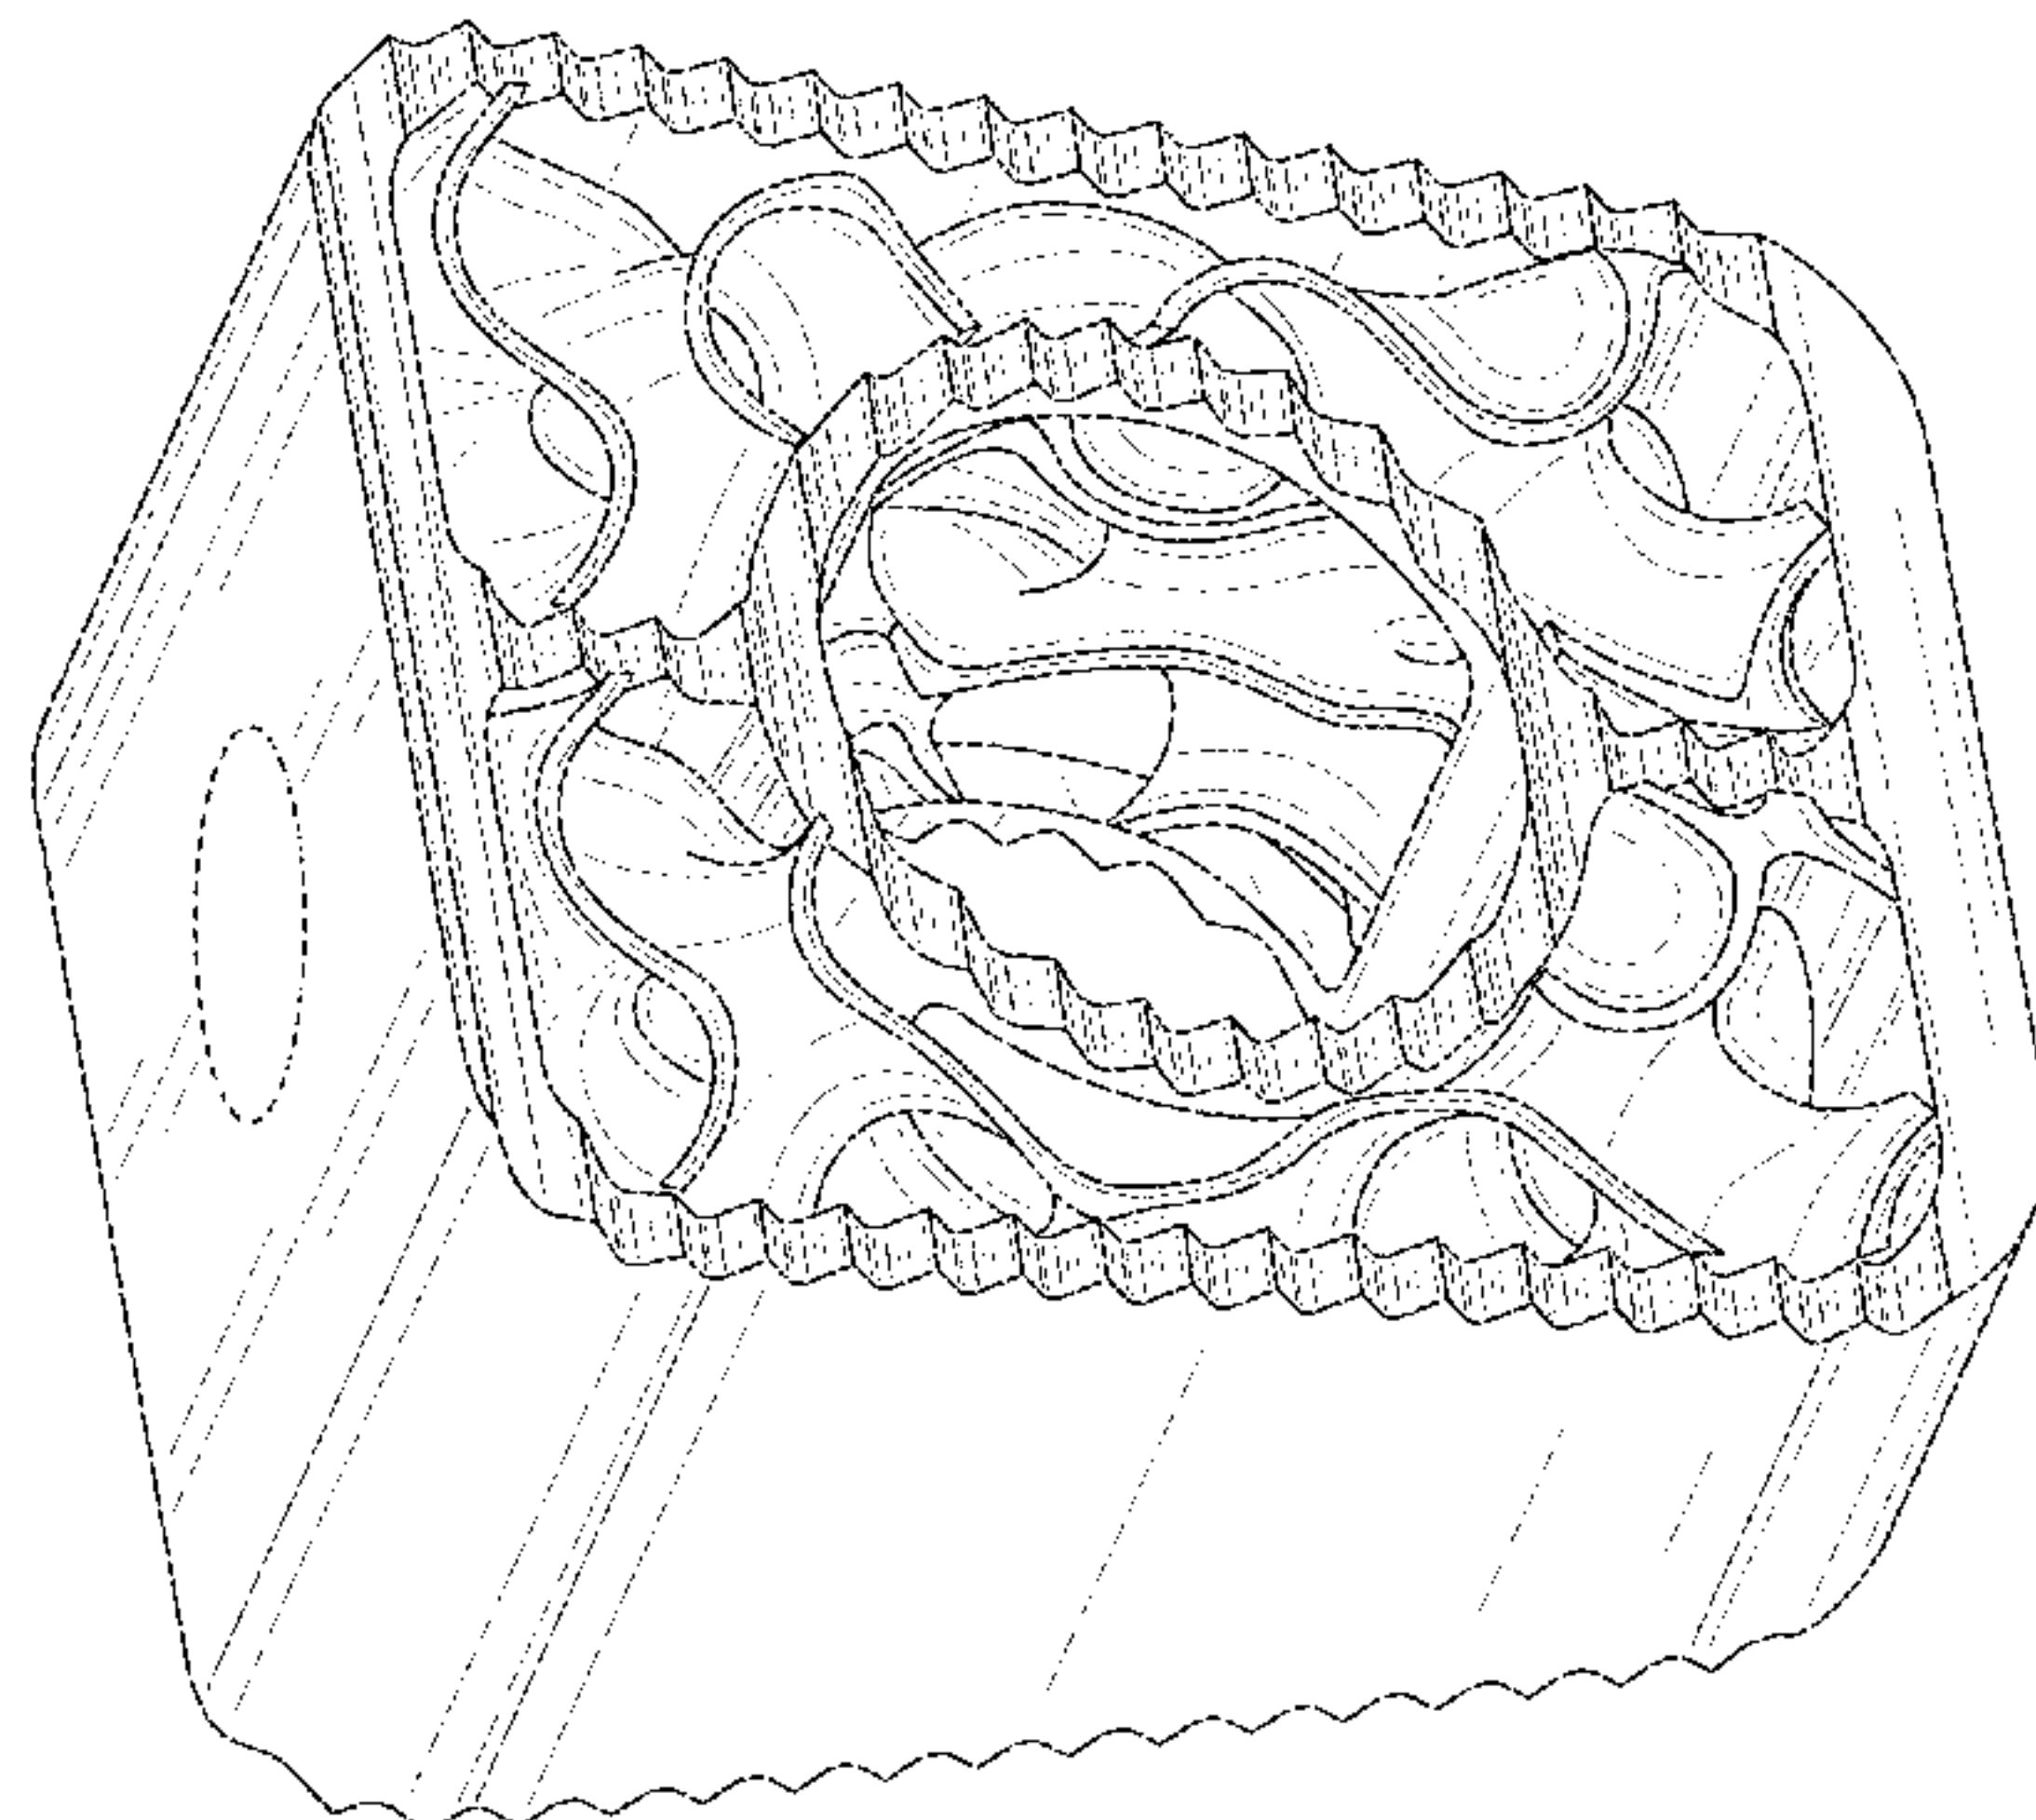

(58)	Field of Classification Search CPC .. 2/441; A61F 2002/4415; A61F 2/442; A61F 2/4425; A61F 2002/443; A61F 2/446; A61F 2/447; A61F 2430/38; A61L 27/00; A61L 2430/38; G06T 2207/30052 See application file for complete search history.	10,772,732 B1 * D899,900 S 2004/0148032 A1 2007/0118243 A1 2008/0206297 A1 2009/0093668 A1 2009/0182430 A1 *	9/2020 10/2020 7/2004 5/2007 8/2008 4/2009 7/2009	Miller A61F 2/4455 Blanco Rutter et al. Schroeder et al. Roeder et al. Marten et al. Tyber A61F 2/4465 623/17.16
(56)	References Cited U.S. PATENT DOCUMENTS	2010/0137990 A1 2010/0168798 A1 * 2010/0286791 A1 2011/0144752 A1 2011/0224796 A1 2011/0230974 A1 2012/0064288 A1 2012/0215310 A1 2013/0123935 A1 2013/0158651 A1 2013/0197657 A1 2013/0218282 A1 2014/0107786 A1 2014/0236299 A1 2014/0277443 A1 2014/0288650 A1 2014/0336680 A1 2014/0371863 A1 2015/0105858 A1 2015/0282945 A1 2015/0282946 A1 2015/0320461 A1 2015/0335434 A1 2015/0343709 A1 2015/0351915 A1 2016/0051371 A1 2016/0089138 A1 2016/0151833 A1 2016/0193055 A1 2016/0199193 A1 2016/0213485 A1 2016/0213486 A1 2016/0213487 A1 2016/0213488 A1 2016/0220288 A1 2016/0256279 A1 2016/0256610 A1 2016/0270931 A1 2016/0287388 A1 2016/0303793 A1 2016/0333152 A1 2016/0374829 A1 2017/0014169 A1 2017/0020685 A1 2017/0036403 A1 2017/0042697 A1 2017/0056178 A1 2017/0056179 A1 2017/0066873 A1 2017/0105844 A1 2017/0156880 A1 2017/0165085 A1 2017/0165790 A1 2017/0172758 A1 2017/0182222 A1 2017/0209274 A1 2017/0216035 A1 2017/0216036 A1 2017/0239054 A1 2017/0239064 A1 2017/0245998 A1 2017/0252165 A1 2017/0258606 A1 2017/0282455 A1 2017/0296244 A1 2017/0319344 A1 2017/0323037 A1 2017/0333205 A1 2017/0354510 A1 2017/0354513 A1	6/2010 7/2010 11/2010 6/2011 9/2011 9/2011 3/2012 8/2012 5/2013 6/2013 8/2013 8/2013 4/2014 8/2014 9/2014 9/2014 11/2014 12/2014 4/2015 10/2015 10/2015 11/2015 11/2015 12/2015 12/2015 2/2016 3/2016 6/2016 6/2016 9/2016 6/2016 7/2016 7/2016 7/2016 7/2016 7/2016 8/2016 9/2016 9/2016 9/2016 10/2016 10/2016 11/2016 12/2016 1/2017 1/2017 2/2017 2/2017 3/2017 3/2017 3/2017 3/2017 4/2017 6/2017 6/2017 6/2017 6/2017 6/2017 6/2017 7/2017 8/2017 8/2017 8/2017 8/2017 9/2017 9/2017 10/2017 10/2017 11/2017 11/2017 11/2017 12/2017 12/2017	Apatsidis et al. Clineff A61F 2/4611 606/279 Goldsmith Defelice et al. Weiland et al. Musani Nakano et al. Sharp et al. Hunt et al. Hollister et al. Anca et al. Hunt Geisler et al. Roeder et al. Fleury et al. Hunt Medina Vanasse et al. Papay et al. Hunt Hunt Ehmke Patterson et al. Gerstle et al. Defelice et al. Defelice et al. Early et al. Tsao Ries Willis et al. Schauffler et al. Nunley et al. Wilson et al. Moore et al. Dubois et al. Sanders et al. Zhou et al. Trieu Hunt et al. Ermoshkin et al. Cook et al. Vogt et al. Dean et al. Geisler et al. Ruff et al. McShane, III et al. Sharp et al. Lorio Gardet Kuyler et al. Halverson et al. Lechmann et al. McCarthy et al. Field et al. Paddock et al. Beerens et al. Hunt Cordaro Engstrand et al. Cordaro Padovani et al. Sharp et al. Afzal Defelice et al. Schneider et al. Hunt Schroeder Joly et al. O'Neil et al. Maglaras et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2017/0355815	A1	12/2017	Becker et al.	
2017/0360488	A1	12/2017	Kowalczyk et al.	
2017/0360563	A1	12/2017	Hunt et al.	
2017/0360578	A1	12/2017	Shin et al.	
2017/0367843	A1	12/2017	Eisen et al.	
2017/0367844	A1	12/2017	Eisen et al.	
2017/0367845	A1	12/2017	Eisen et al.	
2018/0008419	A1*	1/2018	Tyber	A61B 17/8852
2018/0022017	A1	1/2018	Fukumoto et al.	
2018/0064540	A1	3/2018	Hunt	
2018/0085230	A1	3/2018	Hunt	
2018/0104063	A1	4/2018	Asaad	
2018/0110593	A1	4/2018	Khalil	
2018/0110626	A1	4/2018	McShane, III et al.	
2018/0110627	A1	4/2018	Sack	
2018/0117219	A1	5/2018	Yang et al.	
2018/0147319	A1	5/2018	Colucci-Mizenko et al.	
2018/0289515	A1	10/2018	Nemes et al.	
2019/0262101	A1	8/2019	Shanjani et al.	
2019/0343652	A1	11/2019	Petersheim et al.	
2020/0030102	A1	1/2020	Mullens et al.	
2020/0046512	A1	2/2020	Newman et al.	

OTHER PUBLICATIONS

Restor3d, "Products", first available Sep. 28, 2020. (<https://web.archive.org/web/20200928123335/https://restor3d.com/products>) (Year: 2020).*

Ortho Spine News, "Nvision Biomedical Technologies: First FDA Clearance for Osteotomy Wedge System", first available Oct. 28, 2020. (<https://orthospinenews.com/2020/10/28/nvision-biomedical-technologies-first-fda-clearance-for-osteotomy-wedge-system-made-of-peek-optima-ha-enhanced/>) (Year: 2020).*

Sina, "Application logic of triple periodic minimum surface", first available Oct. 24, 2020. (https://k.sina.com.cn/article_2422410454_90630cd600100t1bm.html?from=science) (Year: 2020).*

Larraona et al., "Radiopaque material for 3D printing scaffolds", XXXV Confreso Anual de la Sociedad Espanola de Ingenieria Biomedica. Bilbao, Nov. 29-Dec. 1, 2017, p. 451-454 (Year 2017).

Rozema et al., The effects of different steam-sterilization programs on material properties of poly(1-lactide), Journal of Applied Biomaterials, vol. 2, 23-28 (1991) (Year: 1991).

Alt, Sami. "Design for Sterilization Part 1: Steam Sterillization." Material, Material Technology Blog, Jun. 3, 2016, www.material-technology.com/single-post/2016/05/24/Design-for-Sterilization-part-1-Stream-Sterillization.

Ducheyne, Paul. "Comprehensive Biomaterials." Comprehensive Biomaterials, vol. 1, Elsevier, 2011, pp. 135-135.

Anat Ratnovsky et al., Mechanical Properties of Different Airway Stents, Med. Eng'G. Physics, Mar. 2011, at 408., [http://www.medengphys.com/article/S1350-4533\(15\)00042-9/fulltext](http://www.medengphys.com/article/S1350-4533(15)00042-9/fulltext).

Andrew T. Miller et al., Fatigue of Injection Molded and 30 Printed Polycarbonate Urethane in Solution, 108 Polymer 121 (2017).

Andrew T. Miller et al., Deformation and Fatigue of Tough 30 Printed Elastomer Scaffolds Processed by Fused 3 Deposition Modeling and Continuous Liquid Interface Production, 75 J. Mechanical Behavior Biomedical. Materials 1 (2017).

* cited by examiner

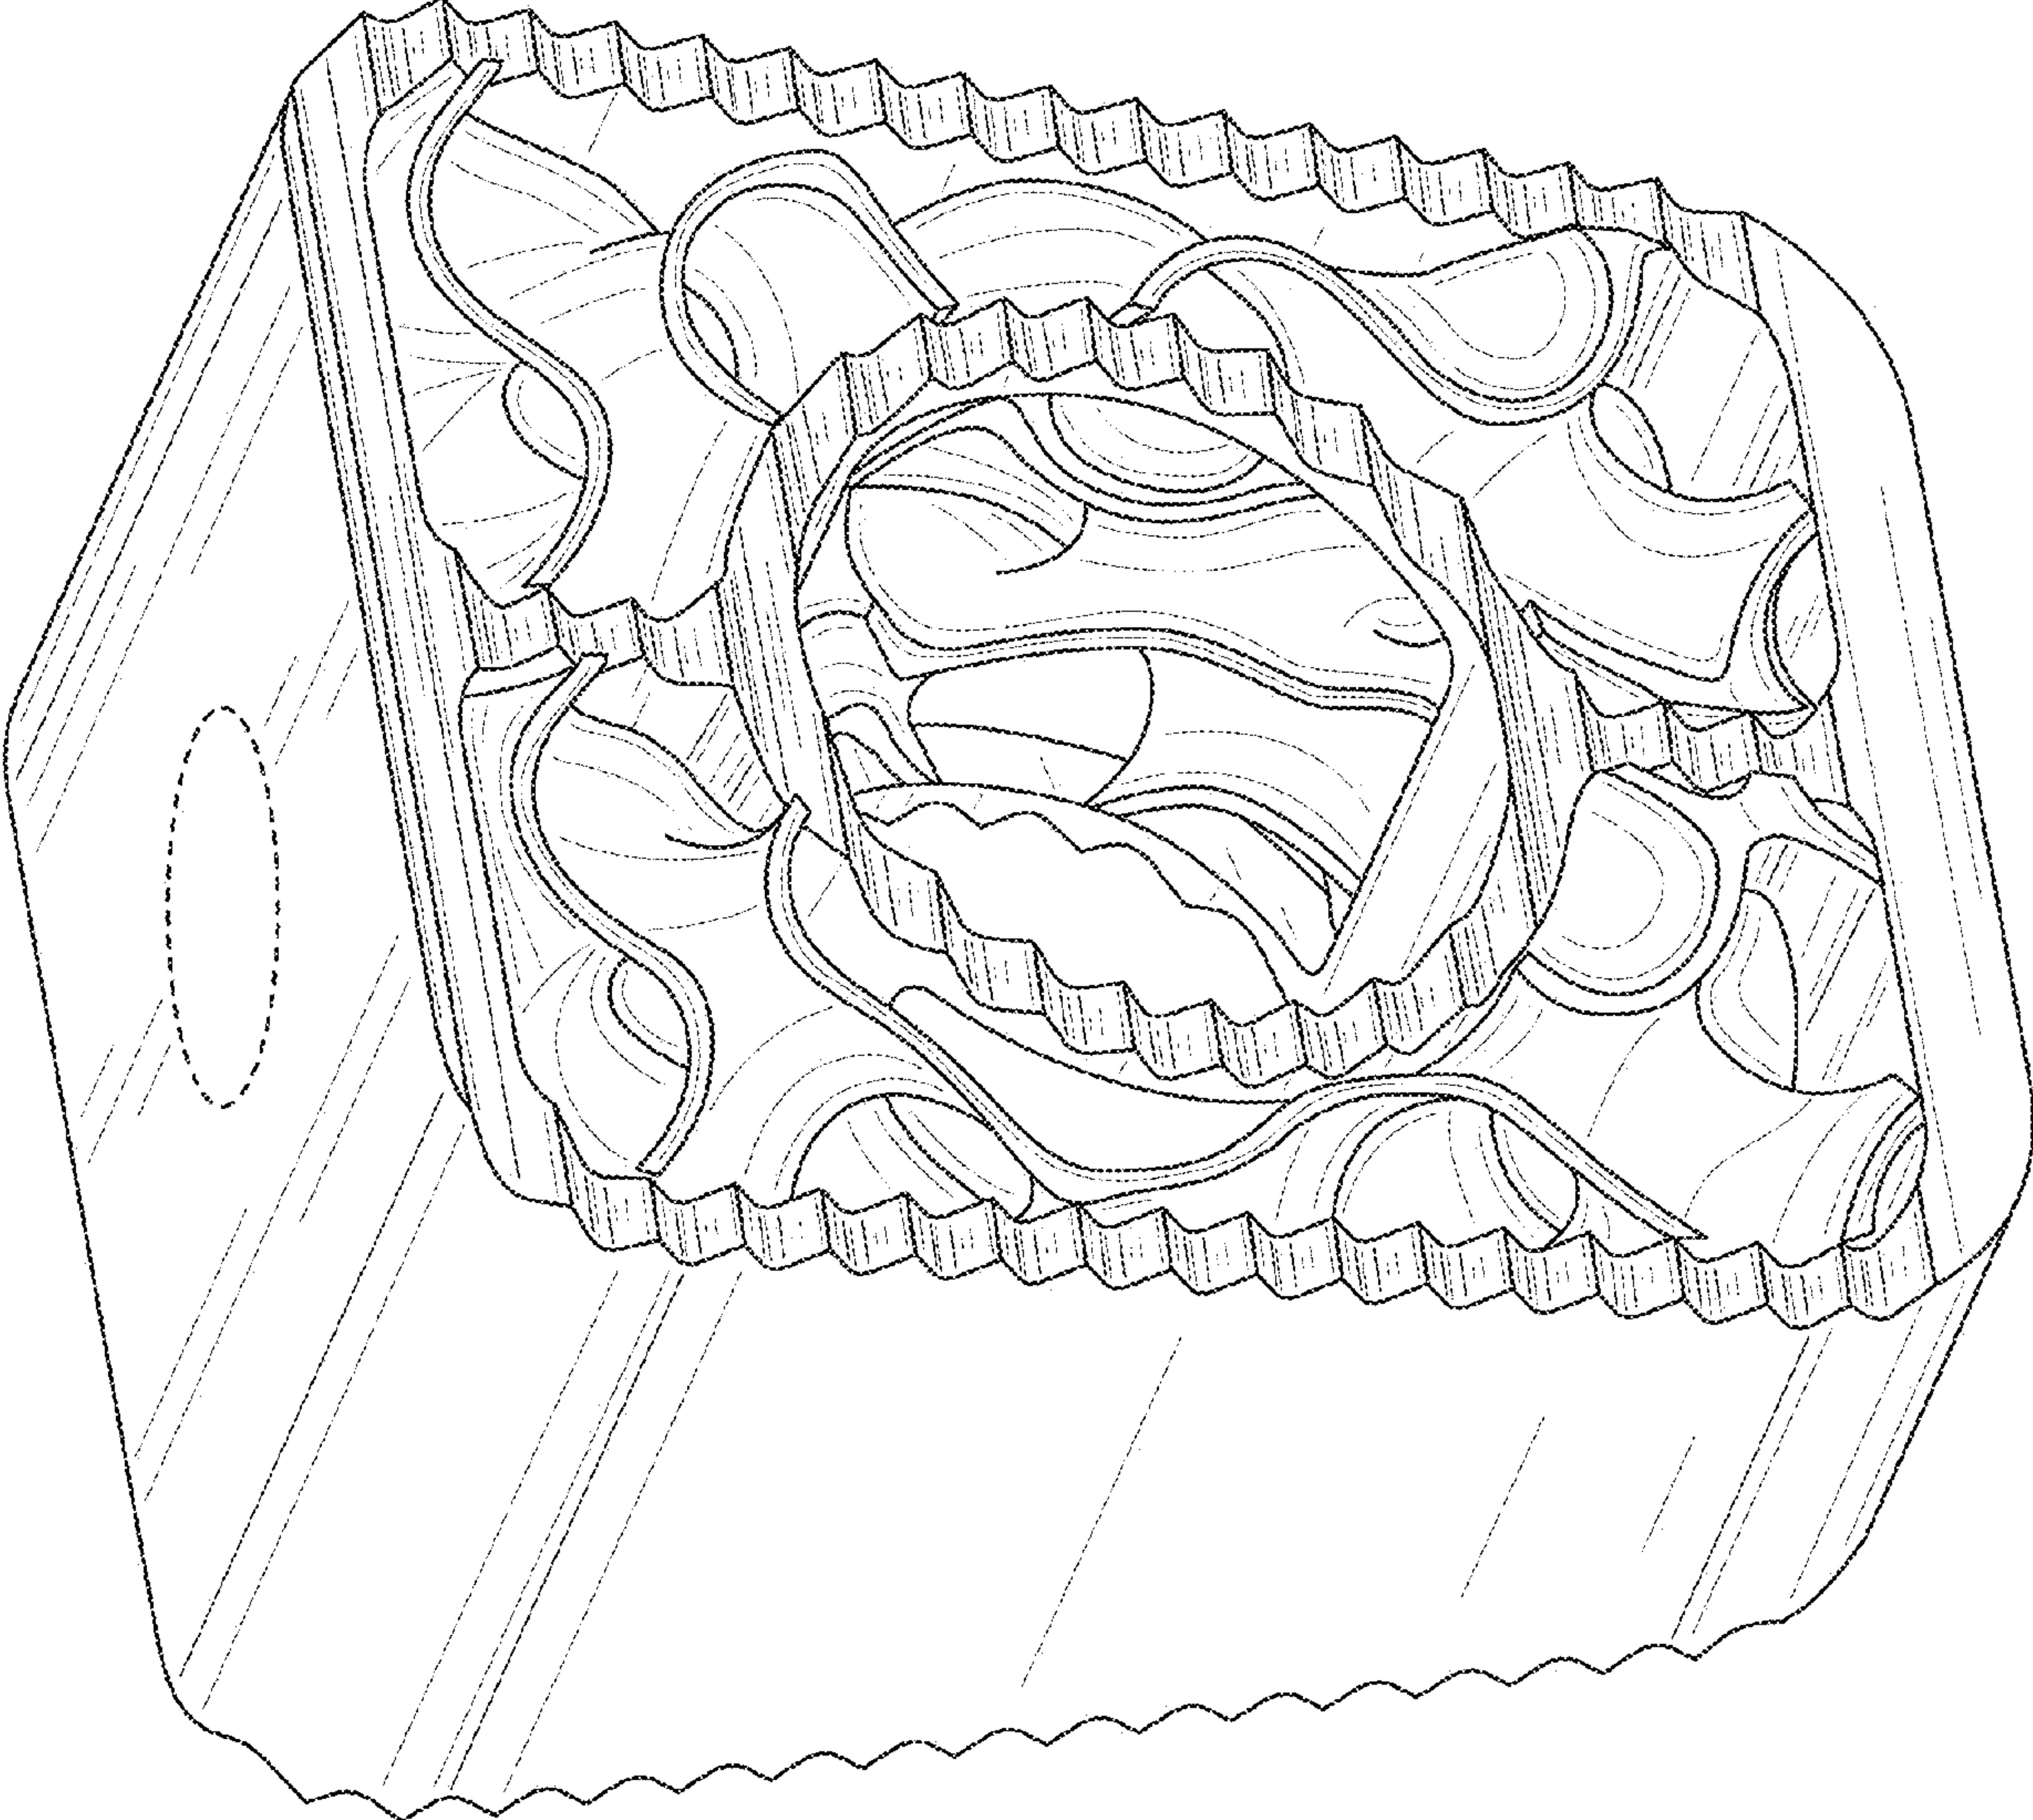


FIG. 1

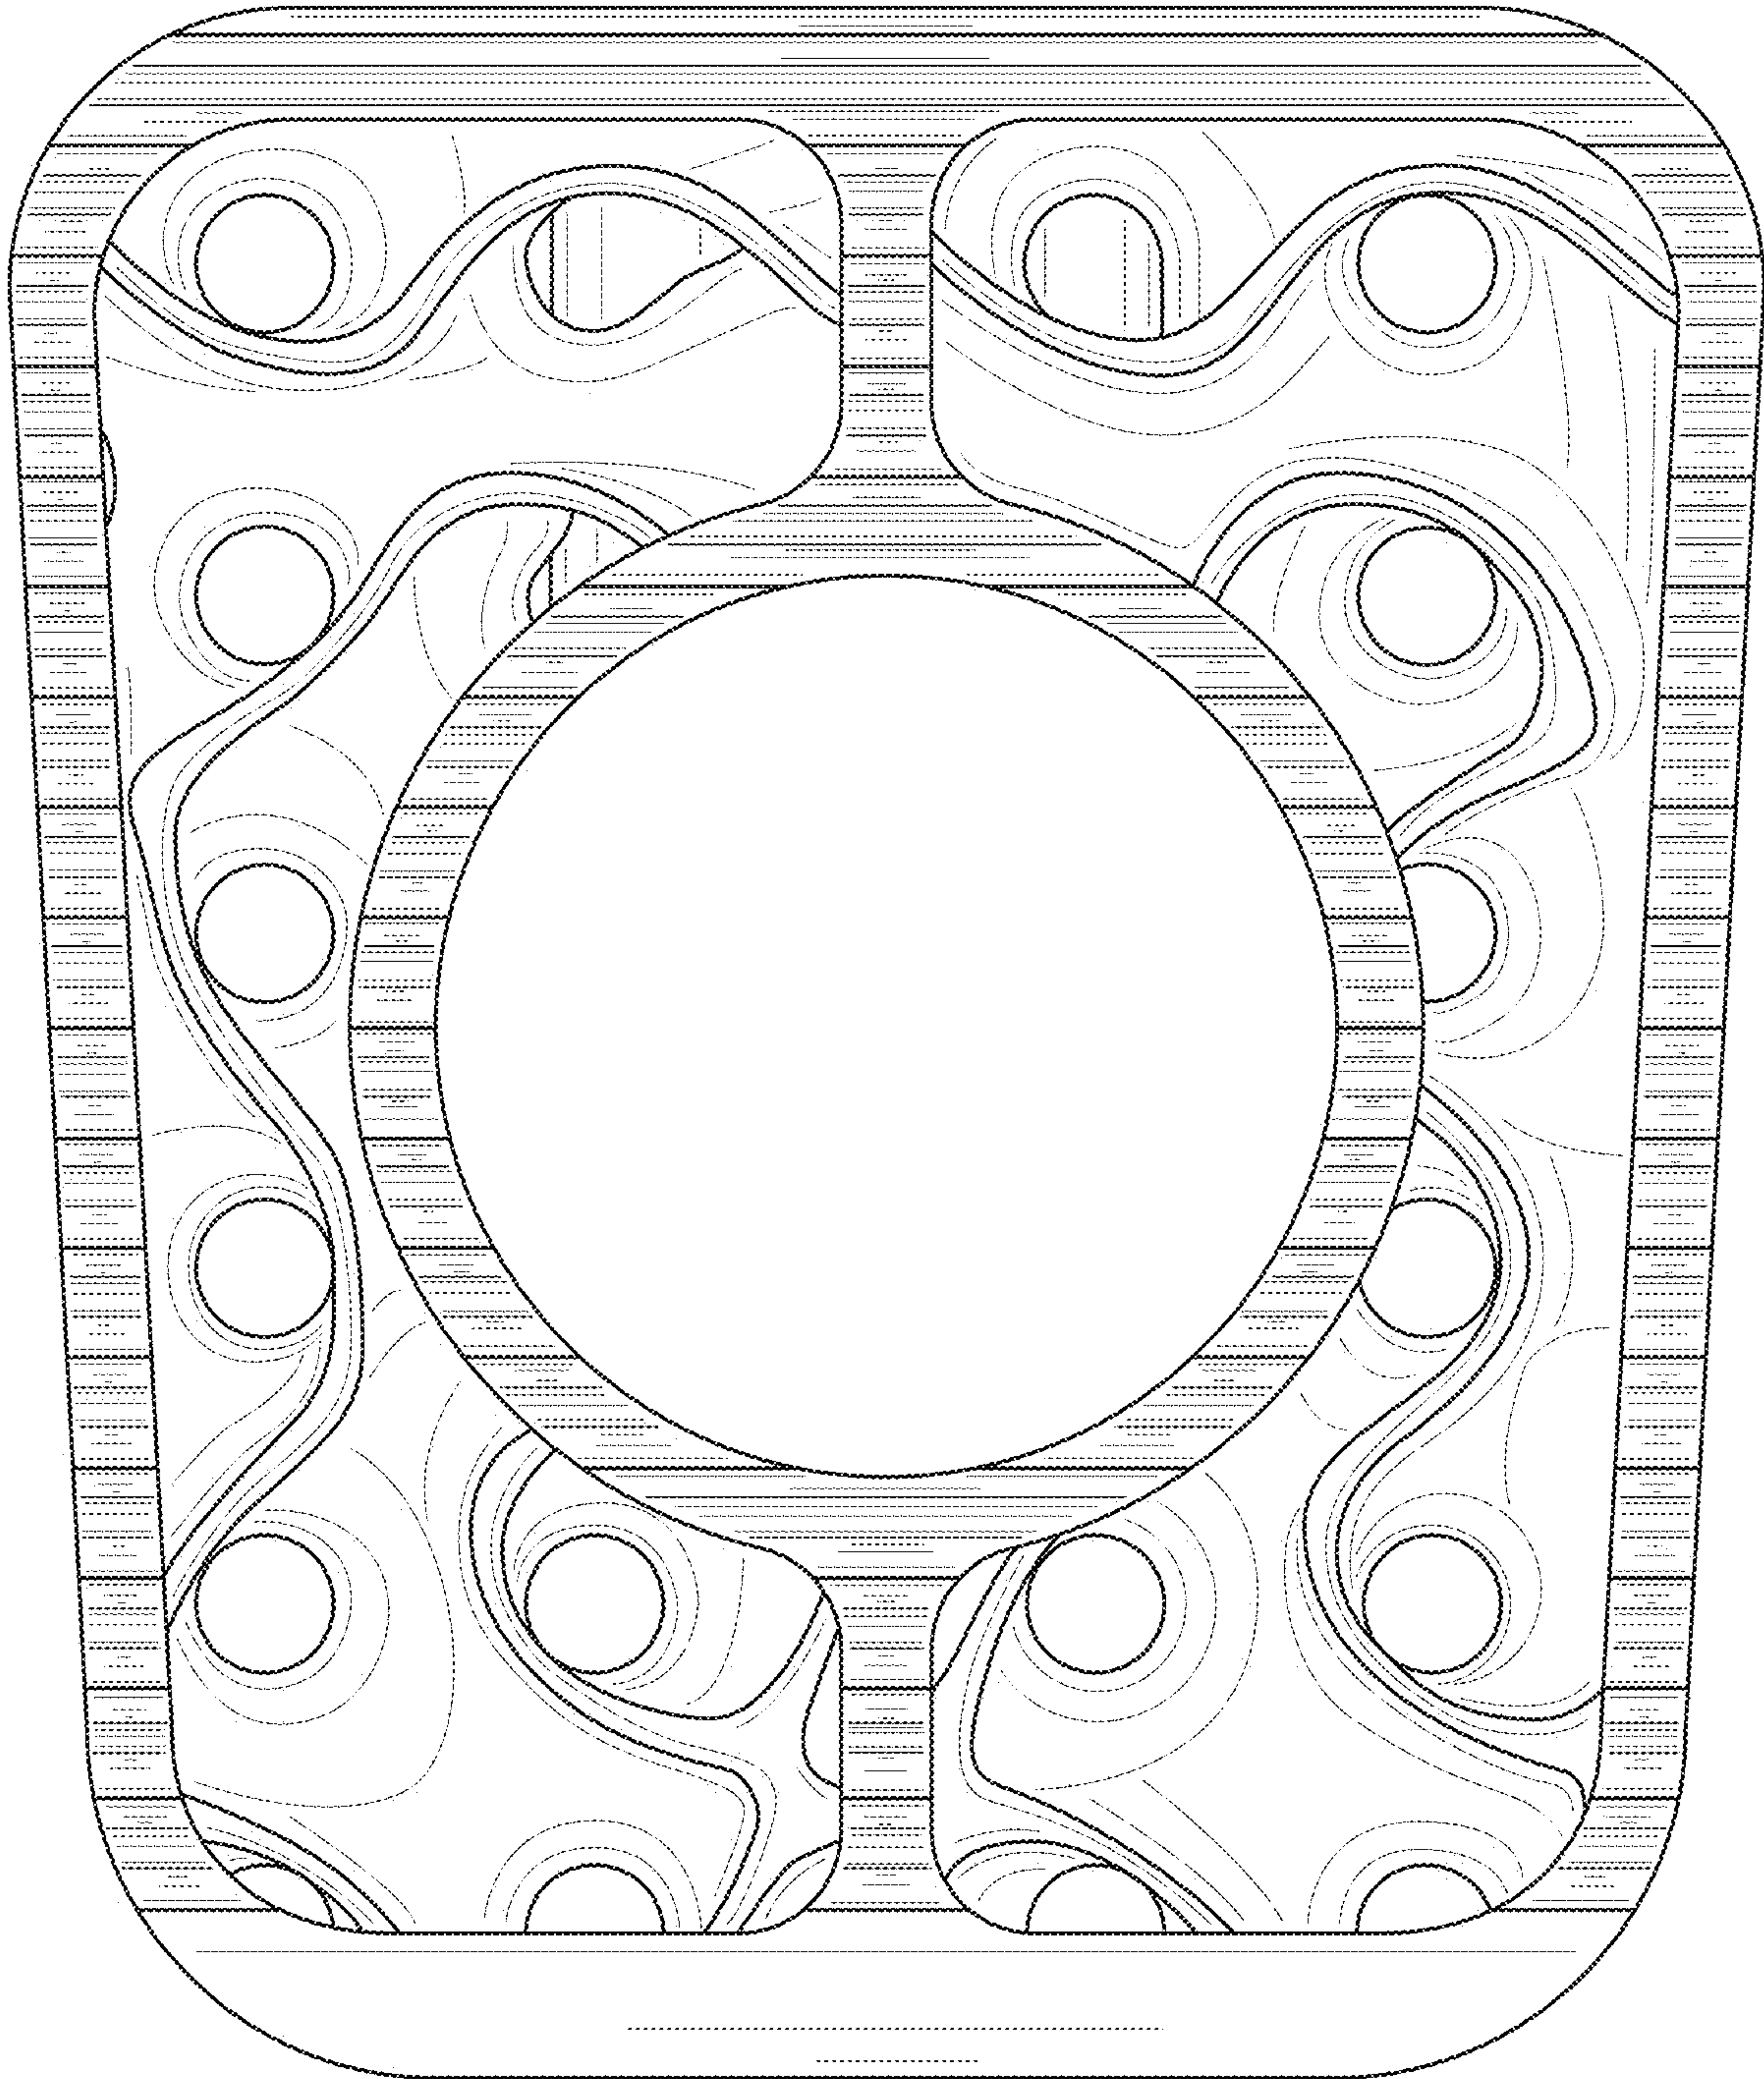


FIG. 2

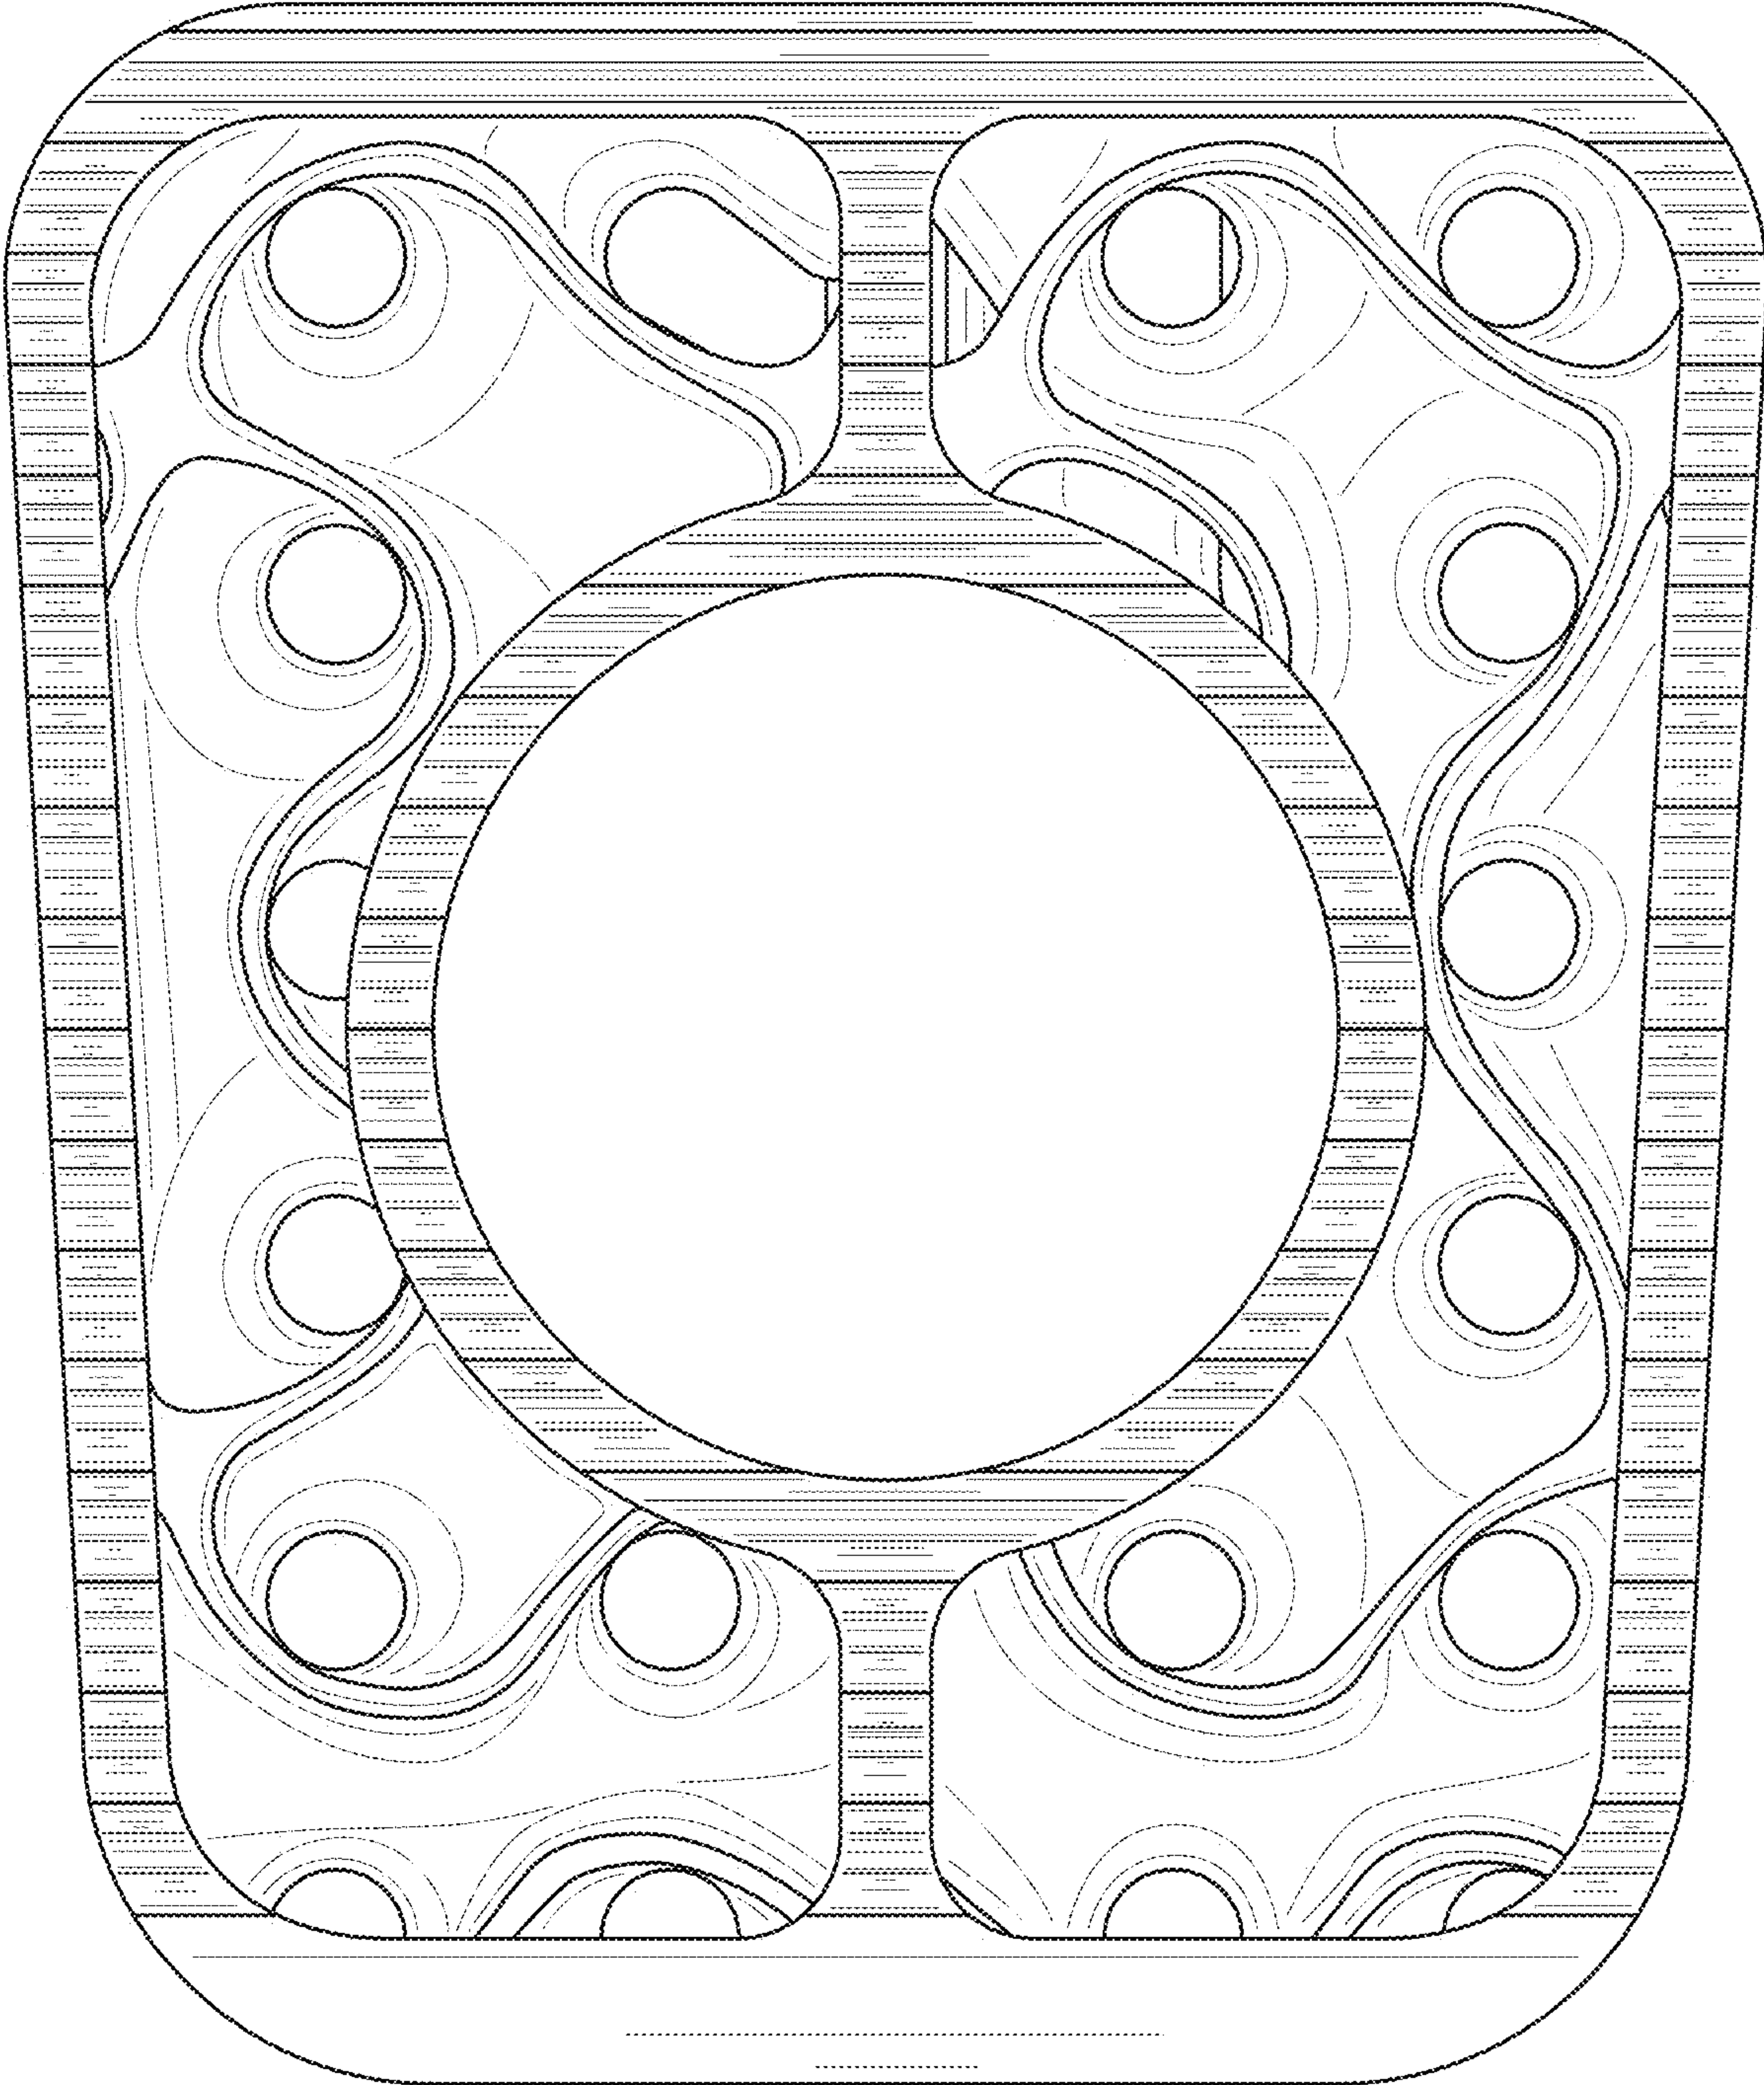


FIG. 3

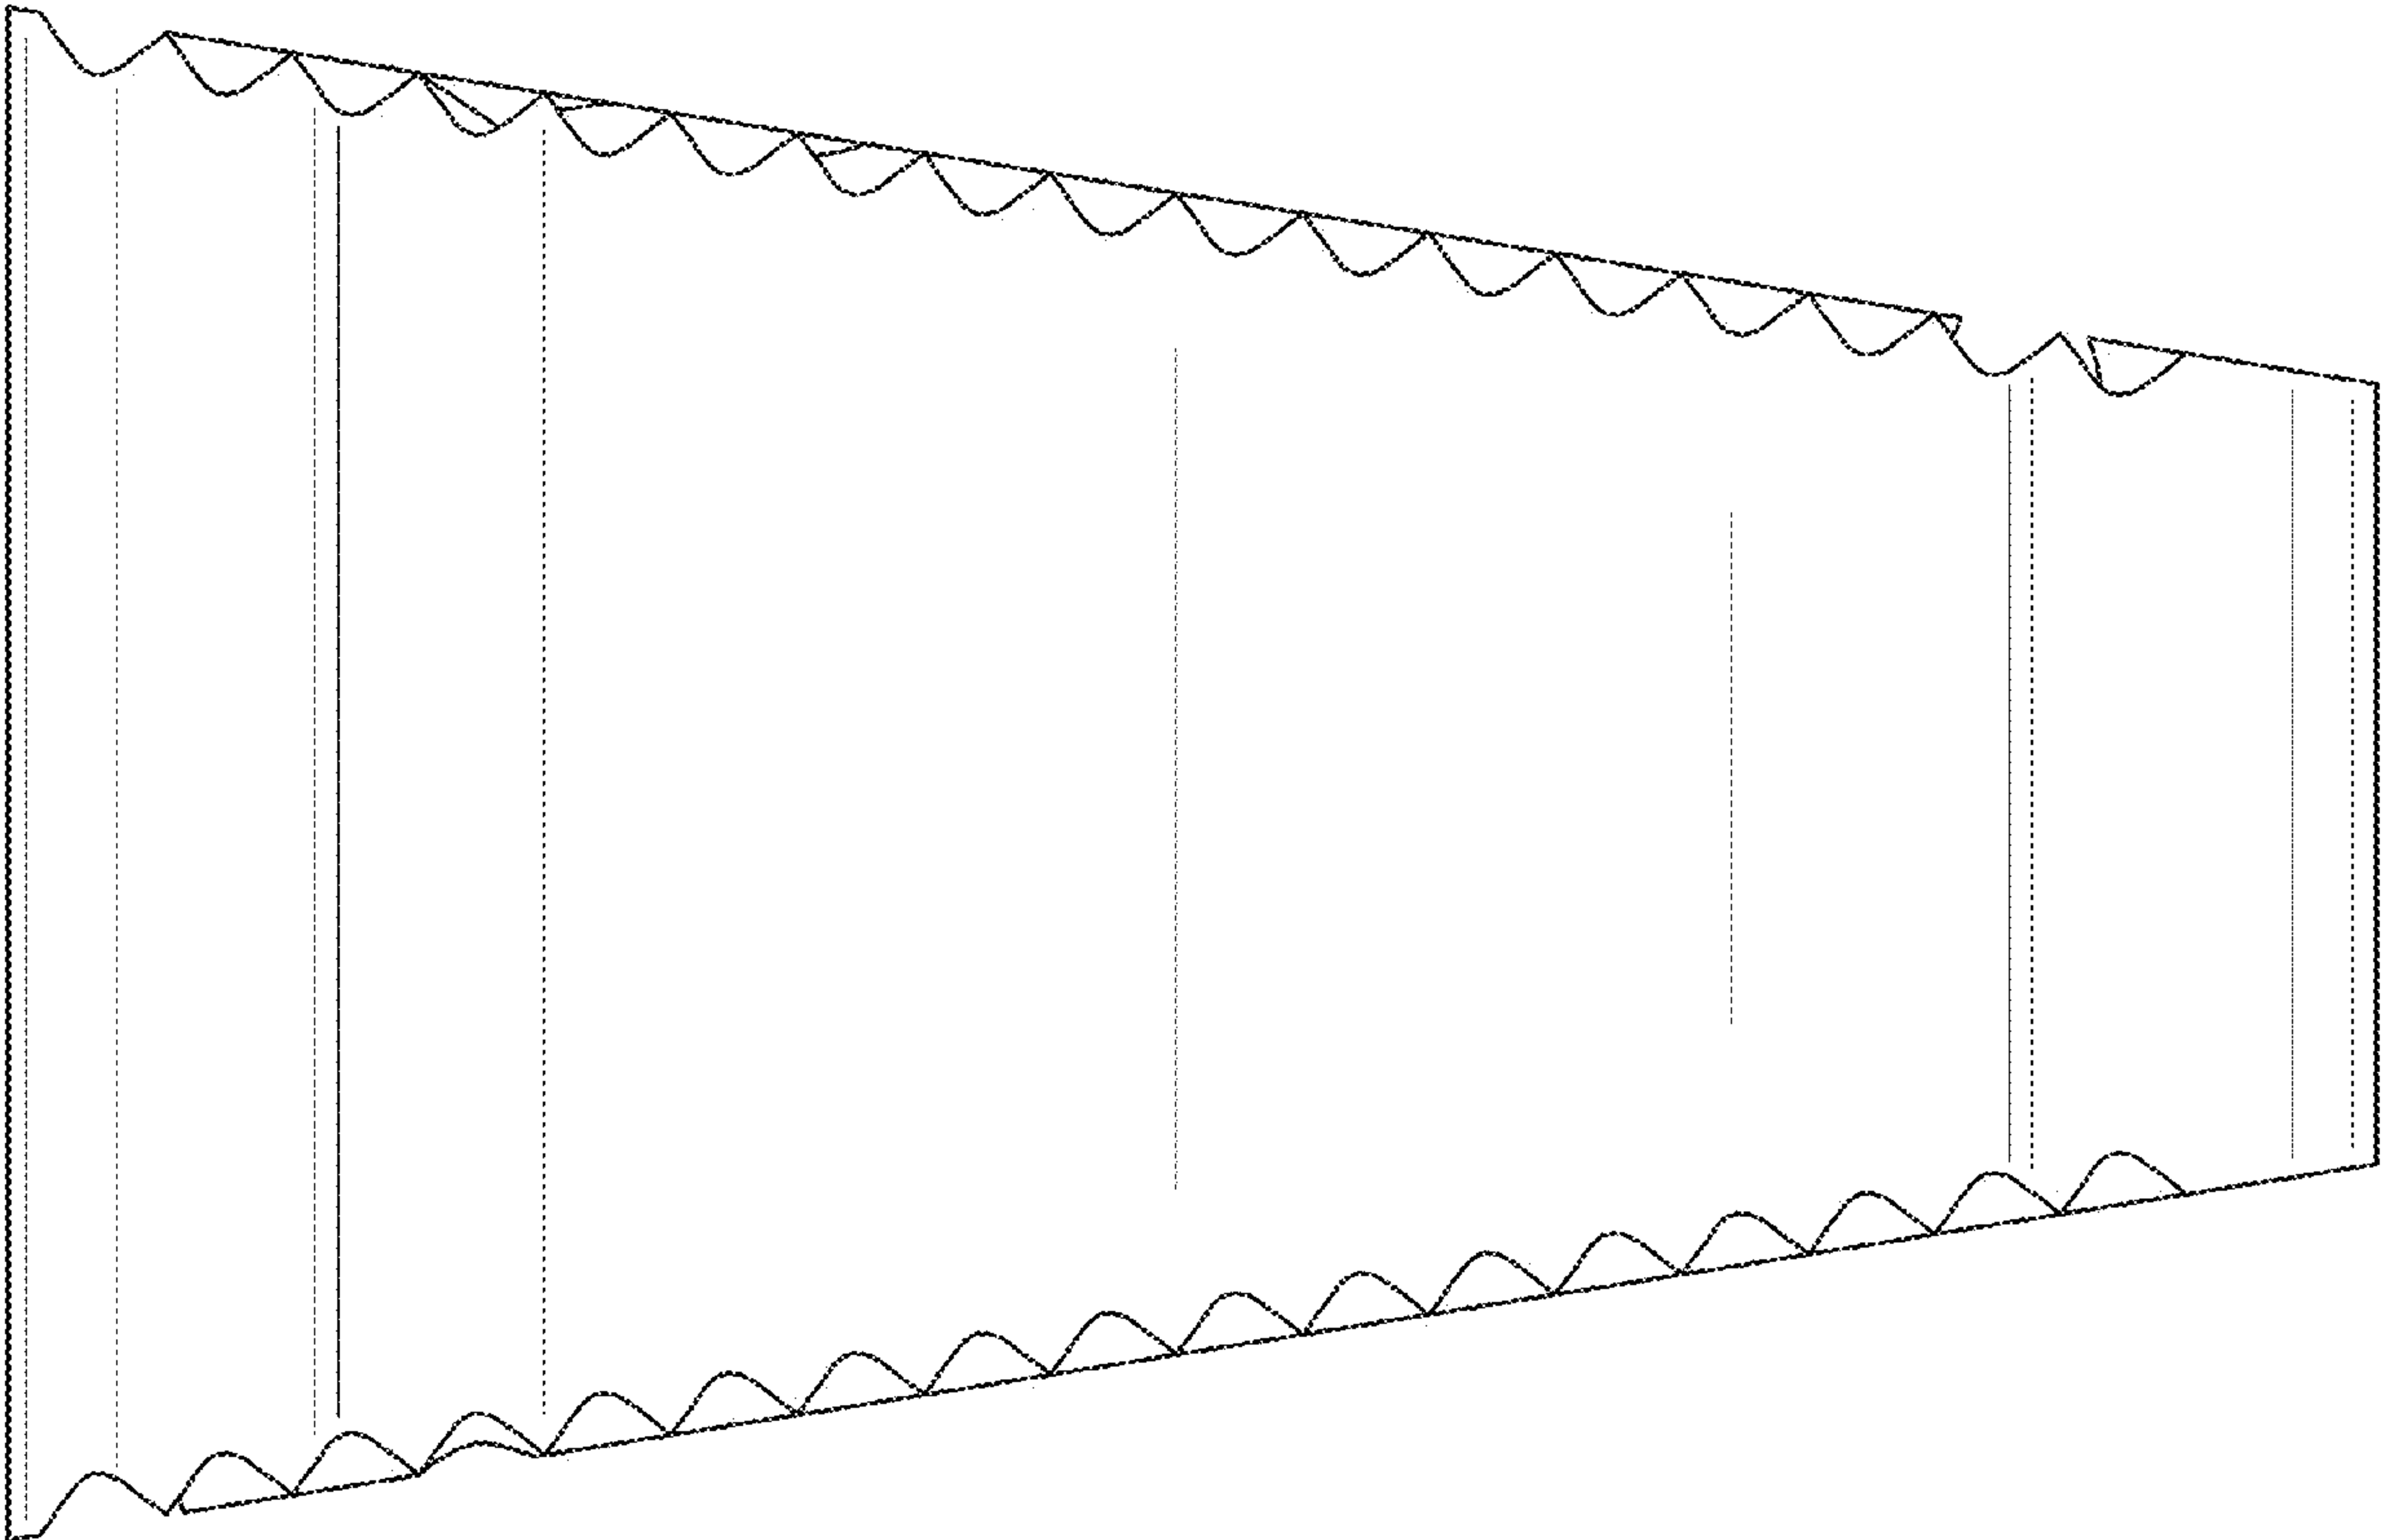


FIG. 4

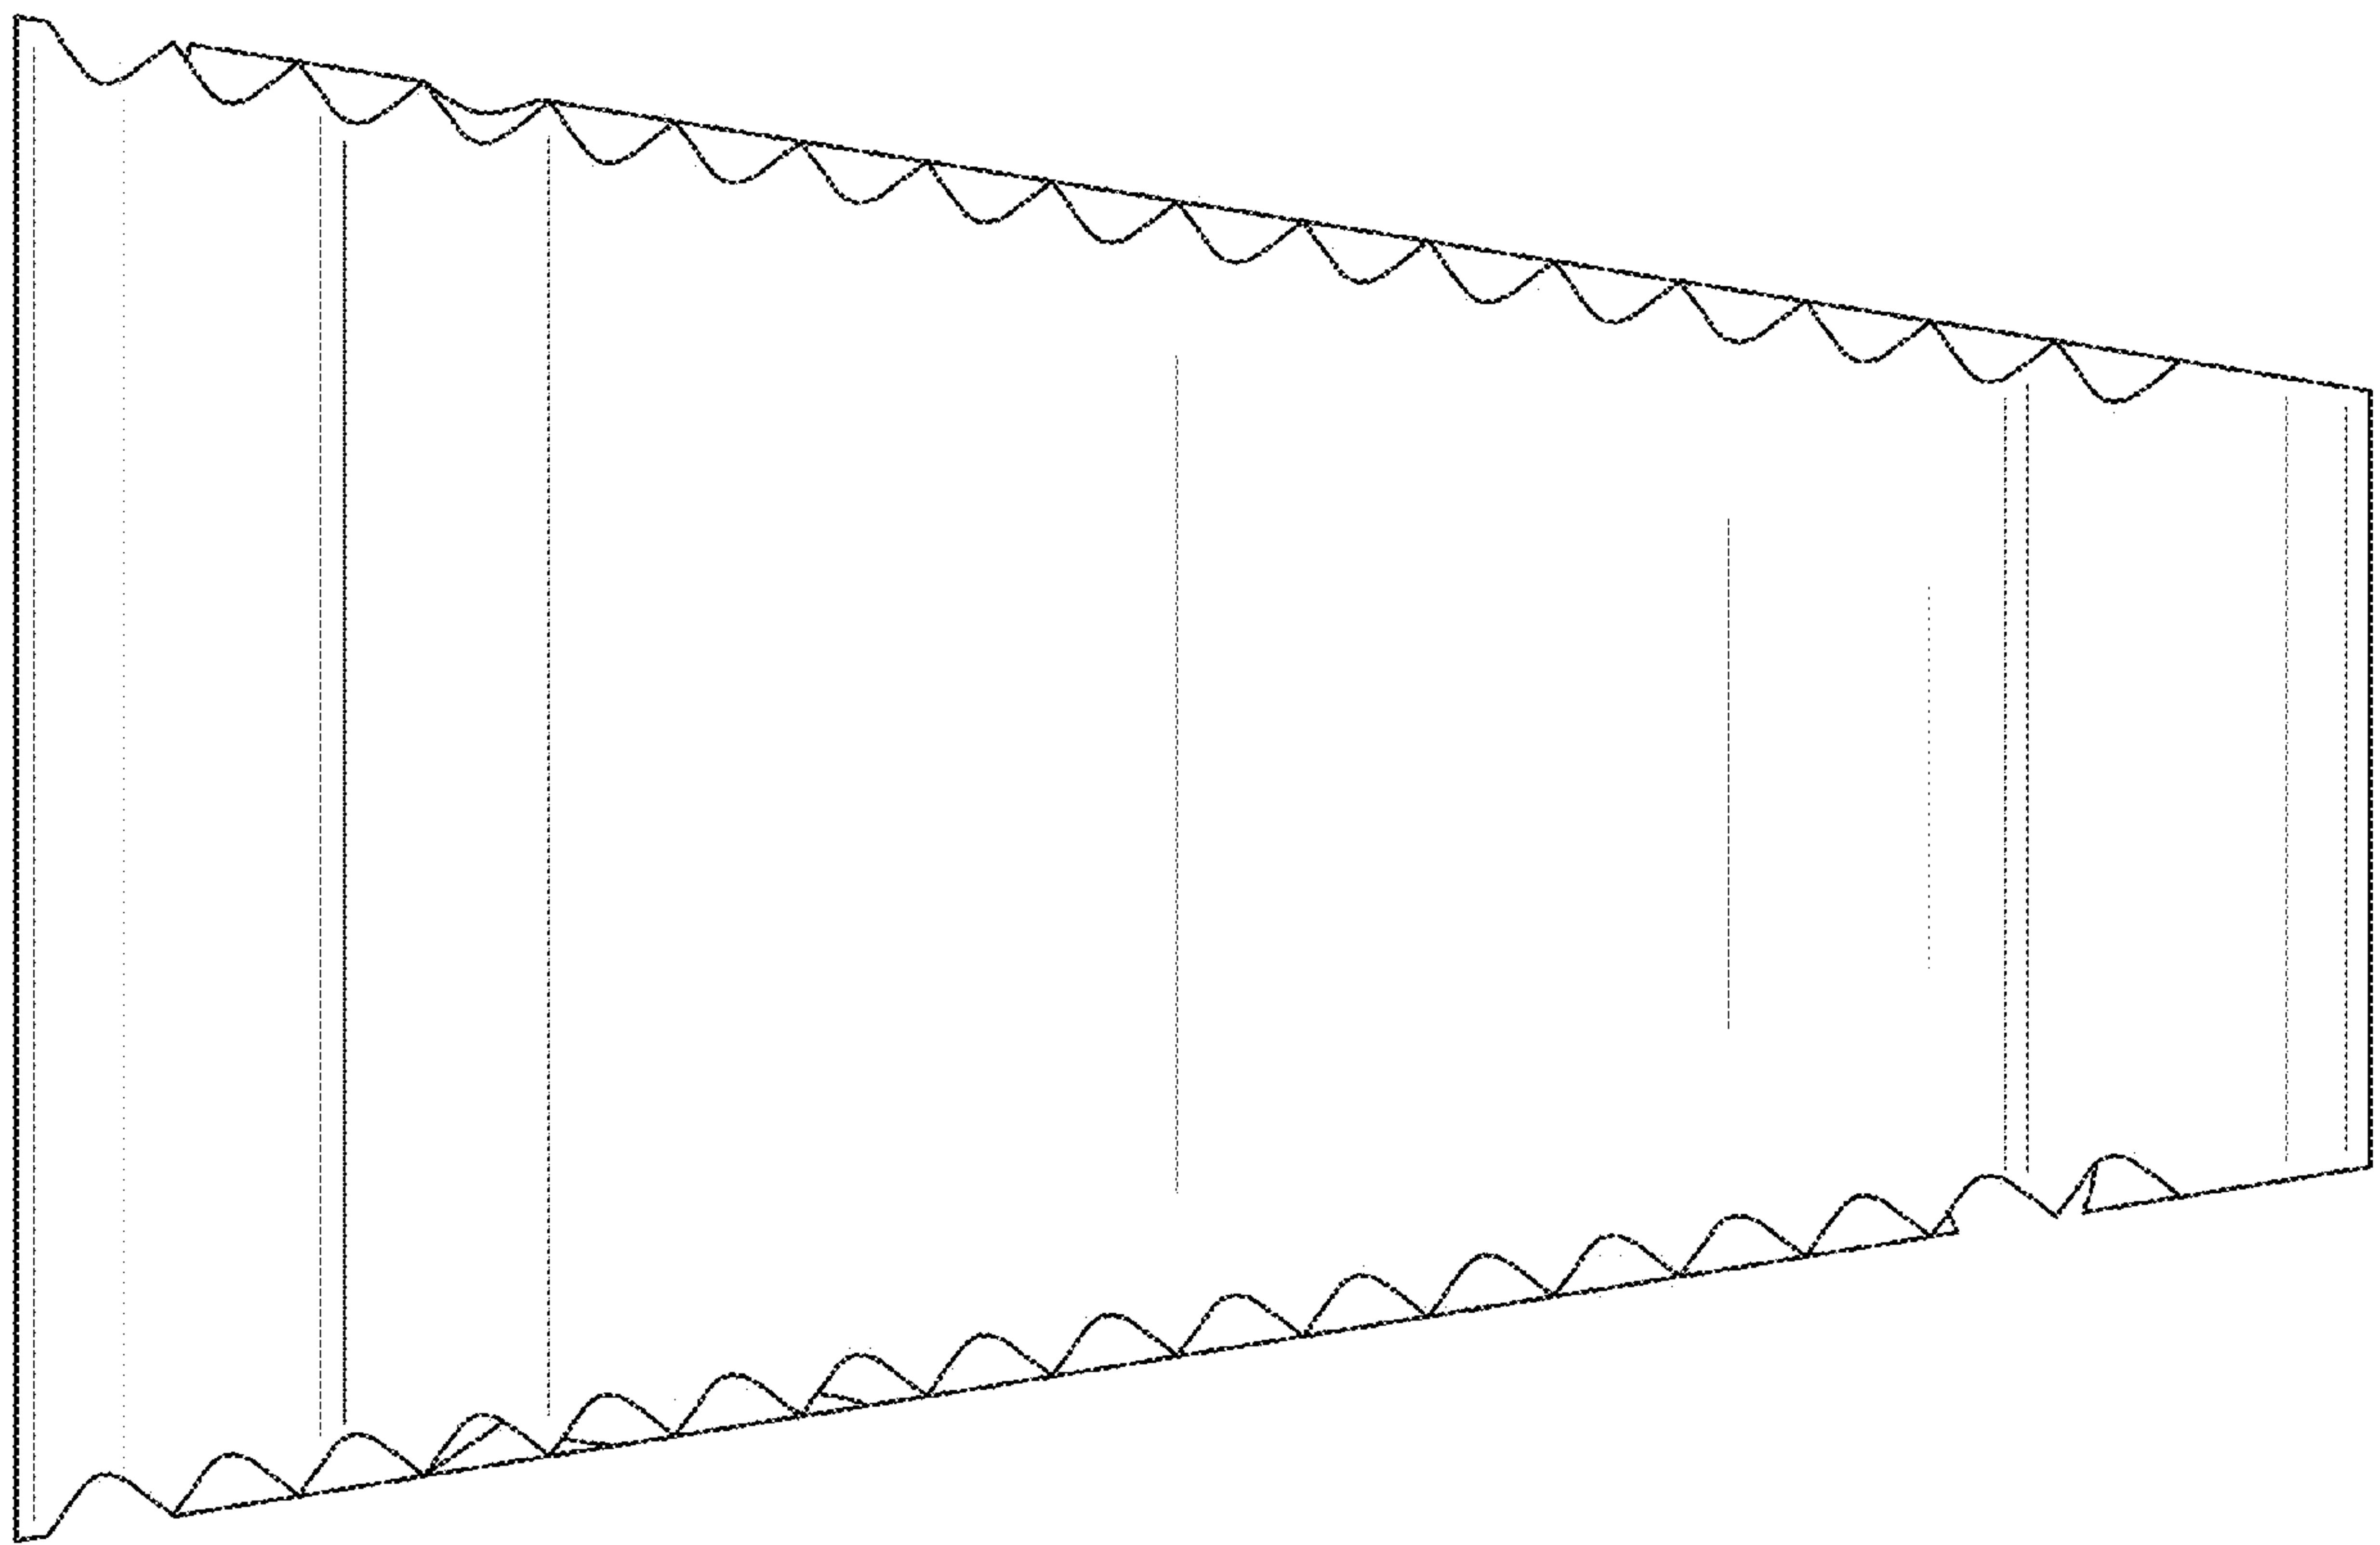


FIG. 5

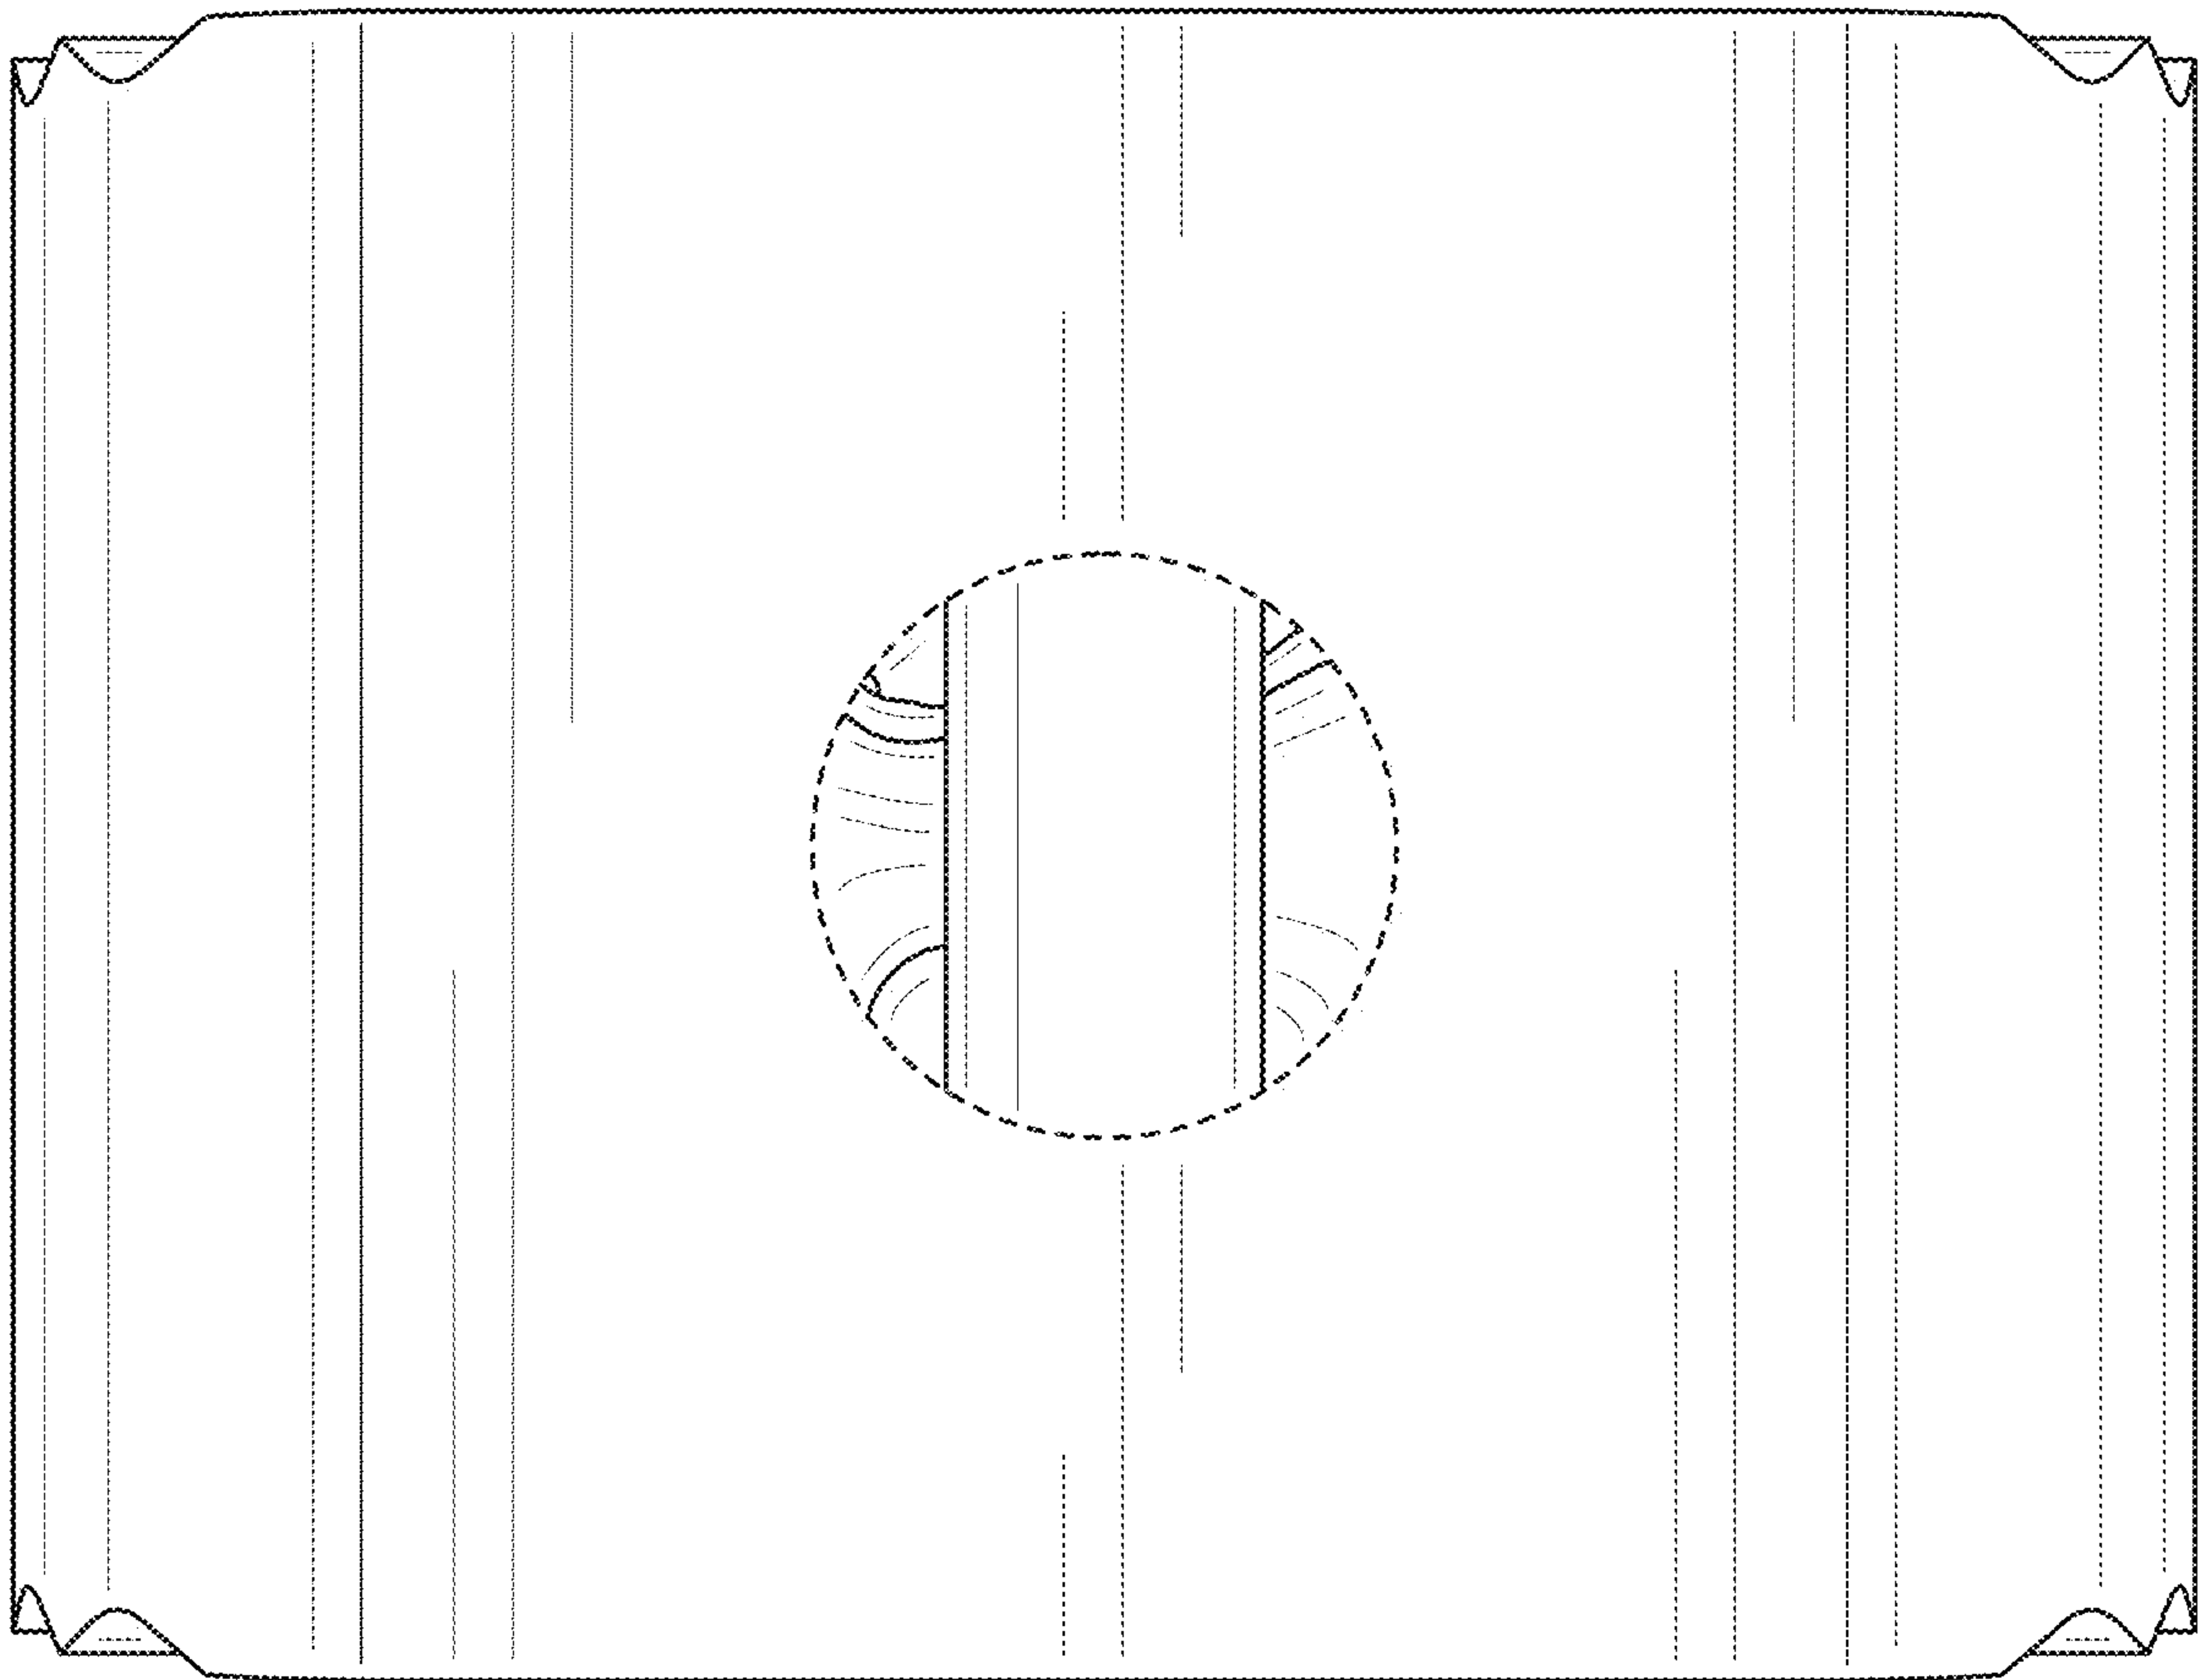


FIG. 6

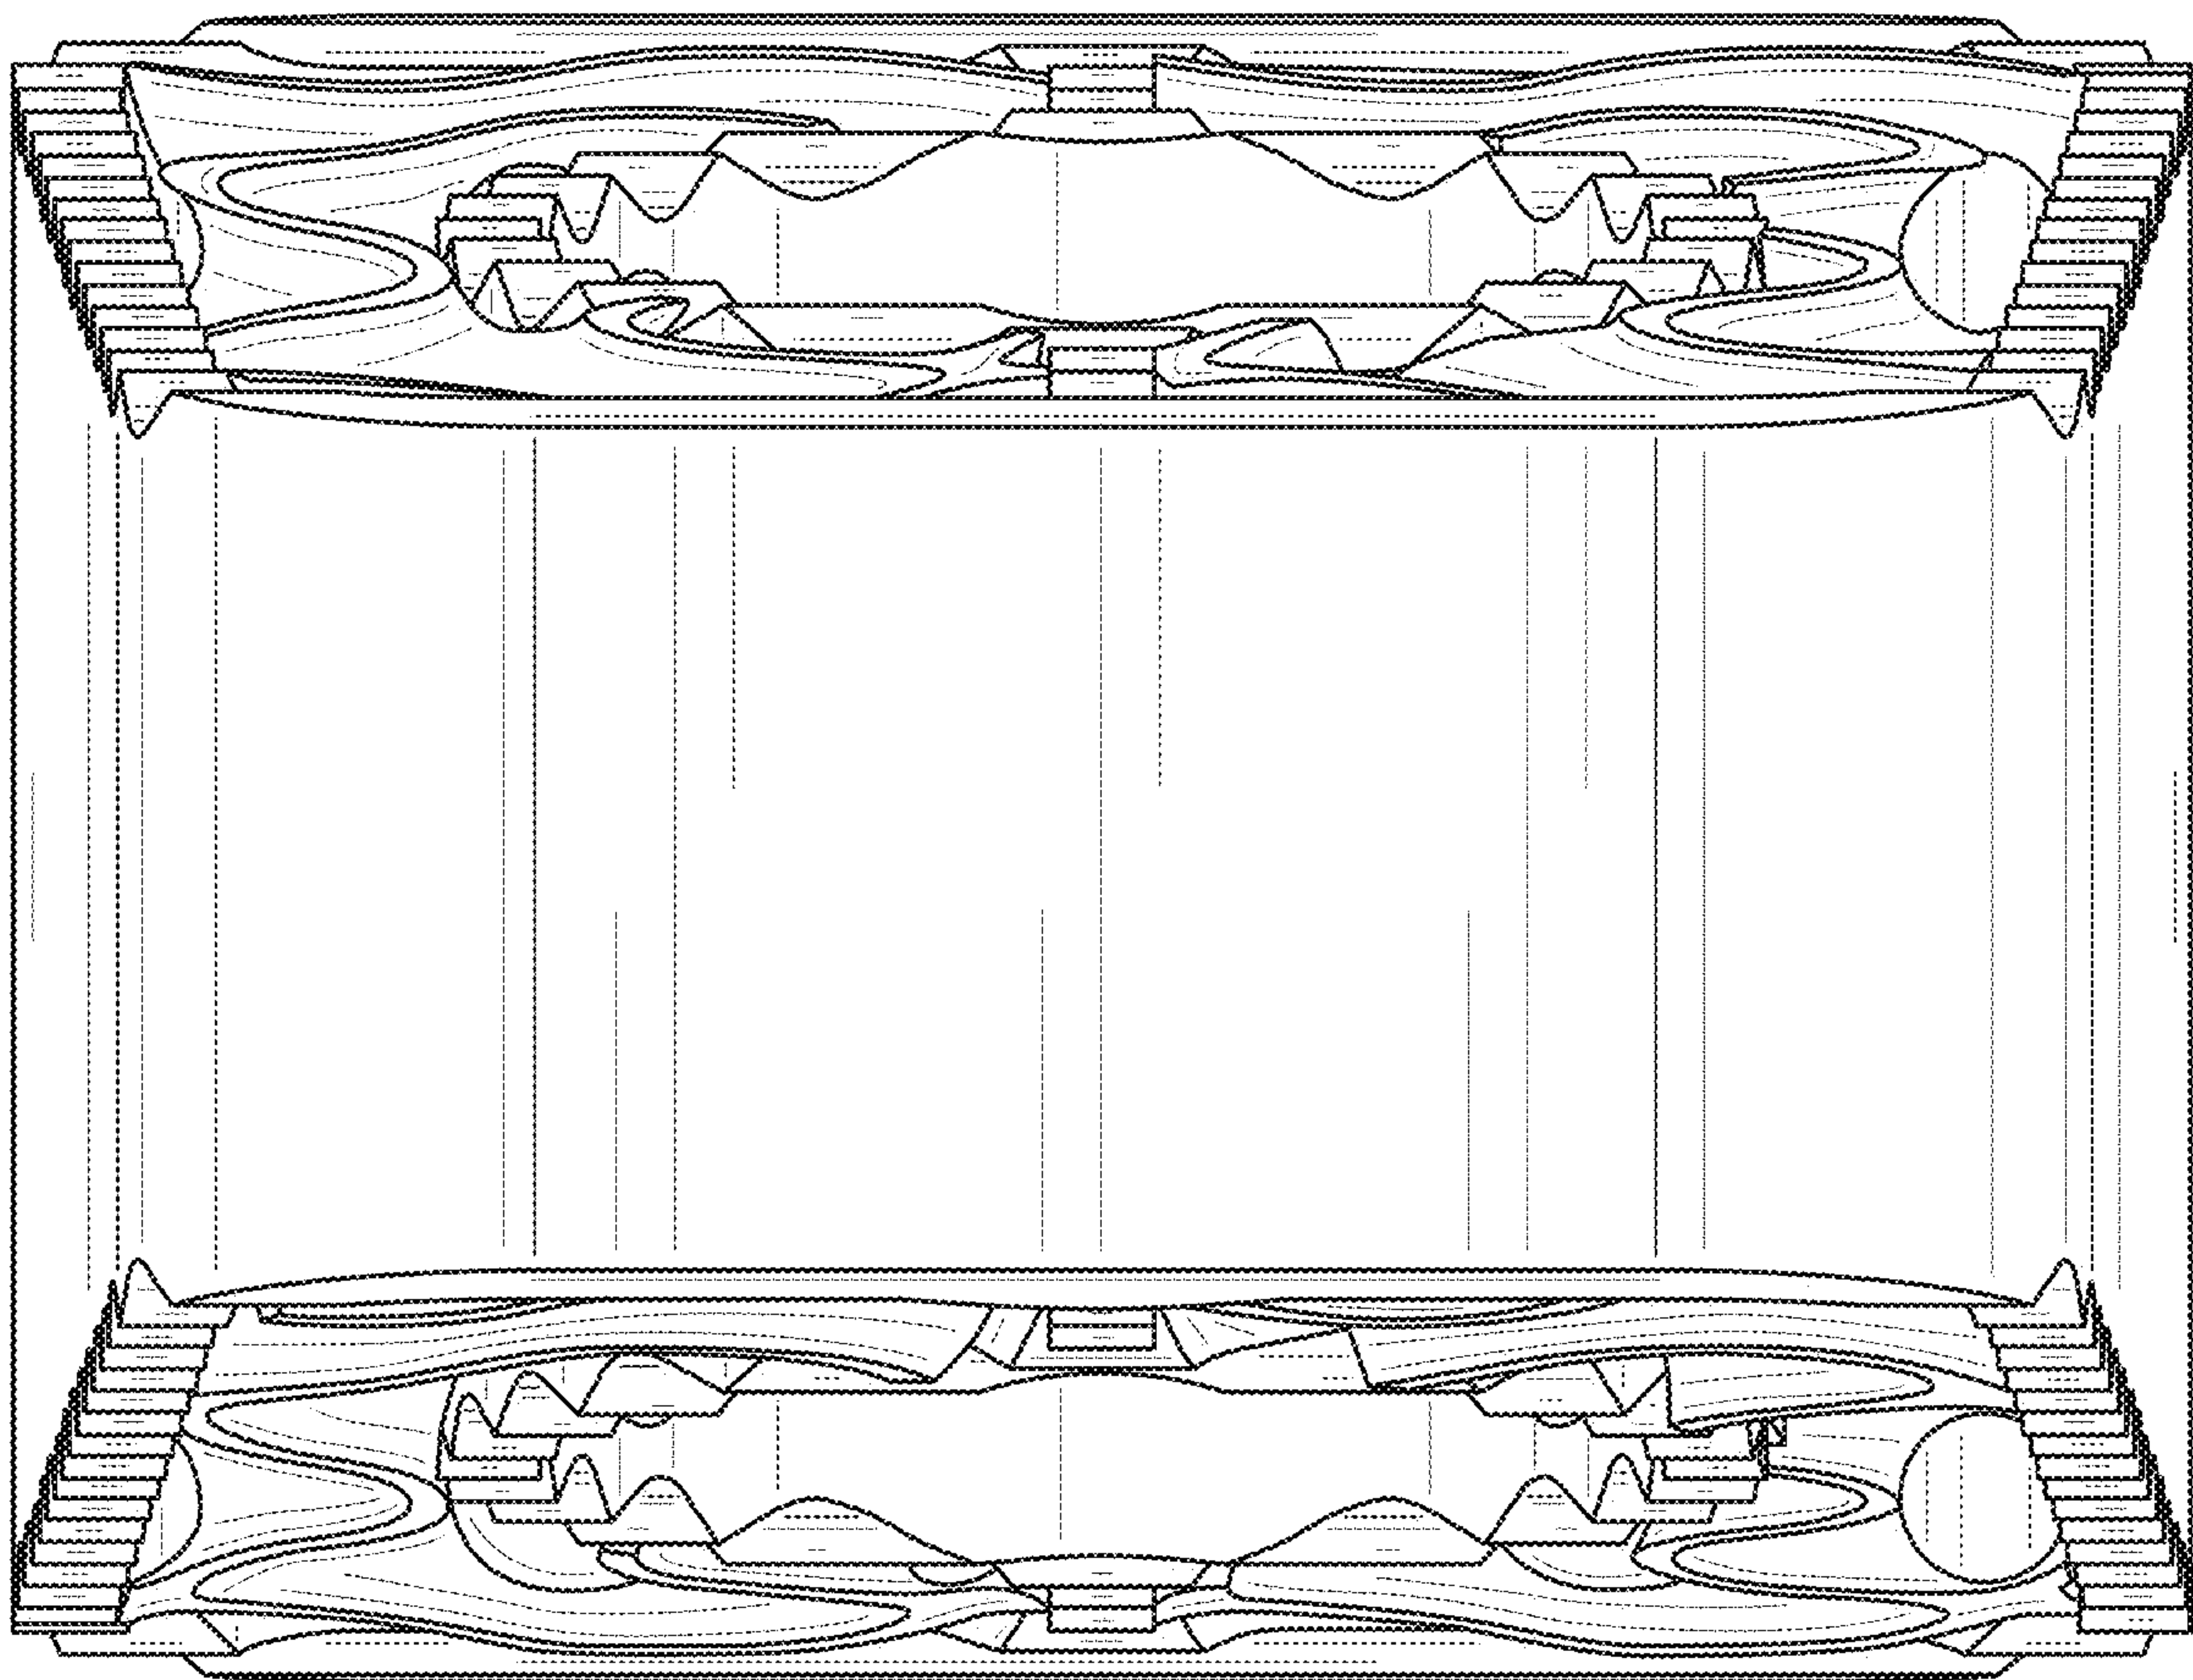


FIG. 7