



US00D920996S

(12) **United States Design Patent**
Liu et al.

(10) **Patent No.:** **US D920,996 S**
(45) **Date of Patent:** **** Jun. 1, 2021**

- (54) **DISPLAY SCREEN WITH A GRAPHICAL USER INTERFACE**
- (71) Applicant: **TEVA BRANDED PHARMACEUTICAL PRODUCTS R&D, INC.**, Frazer, PA (US)
- (72) Inventors: **Xinyu Liu**, Newton, MA (US); **Amir Zur**, Cambridge, MA (US)
- (73) Assignee: **Teva Branded Pharmaceutical Products R&D, Inc.**, Frazer, PA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/681,260**
- (22) Filed: **Feb. 22, 2019**
- (51) **LOC (13) Cl.** **14-04**
- (52) **U.S. Cl.**
USPC **D14/485**
- (58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048; G06F 3/0481; G06F 3/04812; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/0484; G06F 3/04847; G06F 3/0485; G06F 3/04855; G06F 3/04886; G06Q 30/00; H03J 1/00; H03J 1/0008; H03J 1/0016; H03J 1/0025; H04N 5/00; H04N 5/08; H04N 5/14; H04N 5/222; H04N 5/225; H04N 5/232; H04N 5/445; H04N 5/44543; H04N 5/45; H04N 2005/44517; H04N 2005/44521; H04N 2005/44526; H04N 2005/4453; H04N 2005/44534; H04N 2005/44539; H04N 2005/44547; H04N 2005/44556; H04N 2005/4456; H04N 2005/44565; H04N 2005/44569; H04N 2005/44573; H04N 21/00; H04N 21/234; H04N 21/431; H04N 21/4312; H04N 21/4314; H04N 21/4316

See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
D771,654 S * 11/2016 Chaudhri D14/485
D772,249 S * 11/2016 Choi D14/485
D772,261 S * 11/2016 Kothe D14/486
D778,944 S * 2/2017 Kim D14/488
(Continued)

- OTHER PUBLICATIONS**
Tenenbaum, David. "Marrying an asthma inhaler to a wireless monitor and a smartphone app." medicalxpress.com. Apr. 20, 2017. Accessed Jun. 1, 2020. Available online at URL: <https://medicalxpress.com/news/2017-04-asthma-inhaler-wireless-smartphone-app.html> (Year: 2017).*
(Continued)


Primary Examiner — Christian P. McLean
(74) *Attorney, Agent, or Firm* — Flaster Greenberg, P.C.

- (57) **CLAIM**
The ornamental design for a display screen with a graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a first image of a display screen with a graphical user interface, showing the new design; FIG. 2 is a front view of a second image thereof; FIG. 3 is a front view of a third image thereof; and, FIG. 4 is a front view of a fourth image thereof. The appearance of the animated image sequentially transitions between the images shown in FIGS. 1 through 4. The process or period in which one image transitions into another forms no part of the claimed design. The outermost broken lines illustrate a mobile device, which is the environment of the design and forms no part of the claim. The remaining broken lines illustrate a display screen and portions of the graphical user interface that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

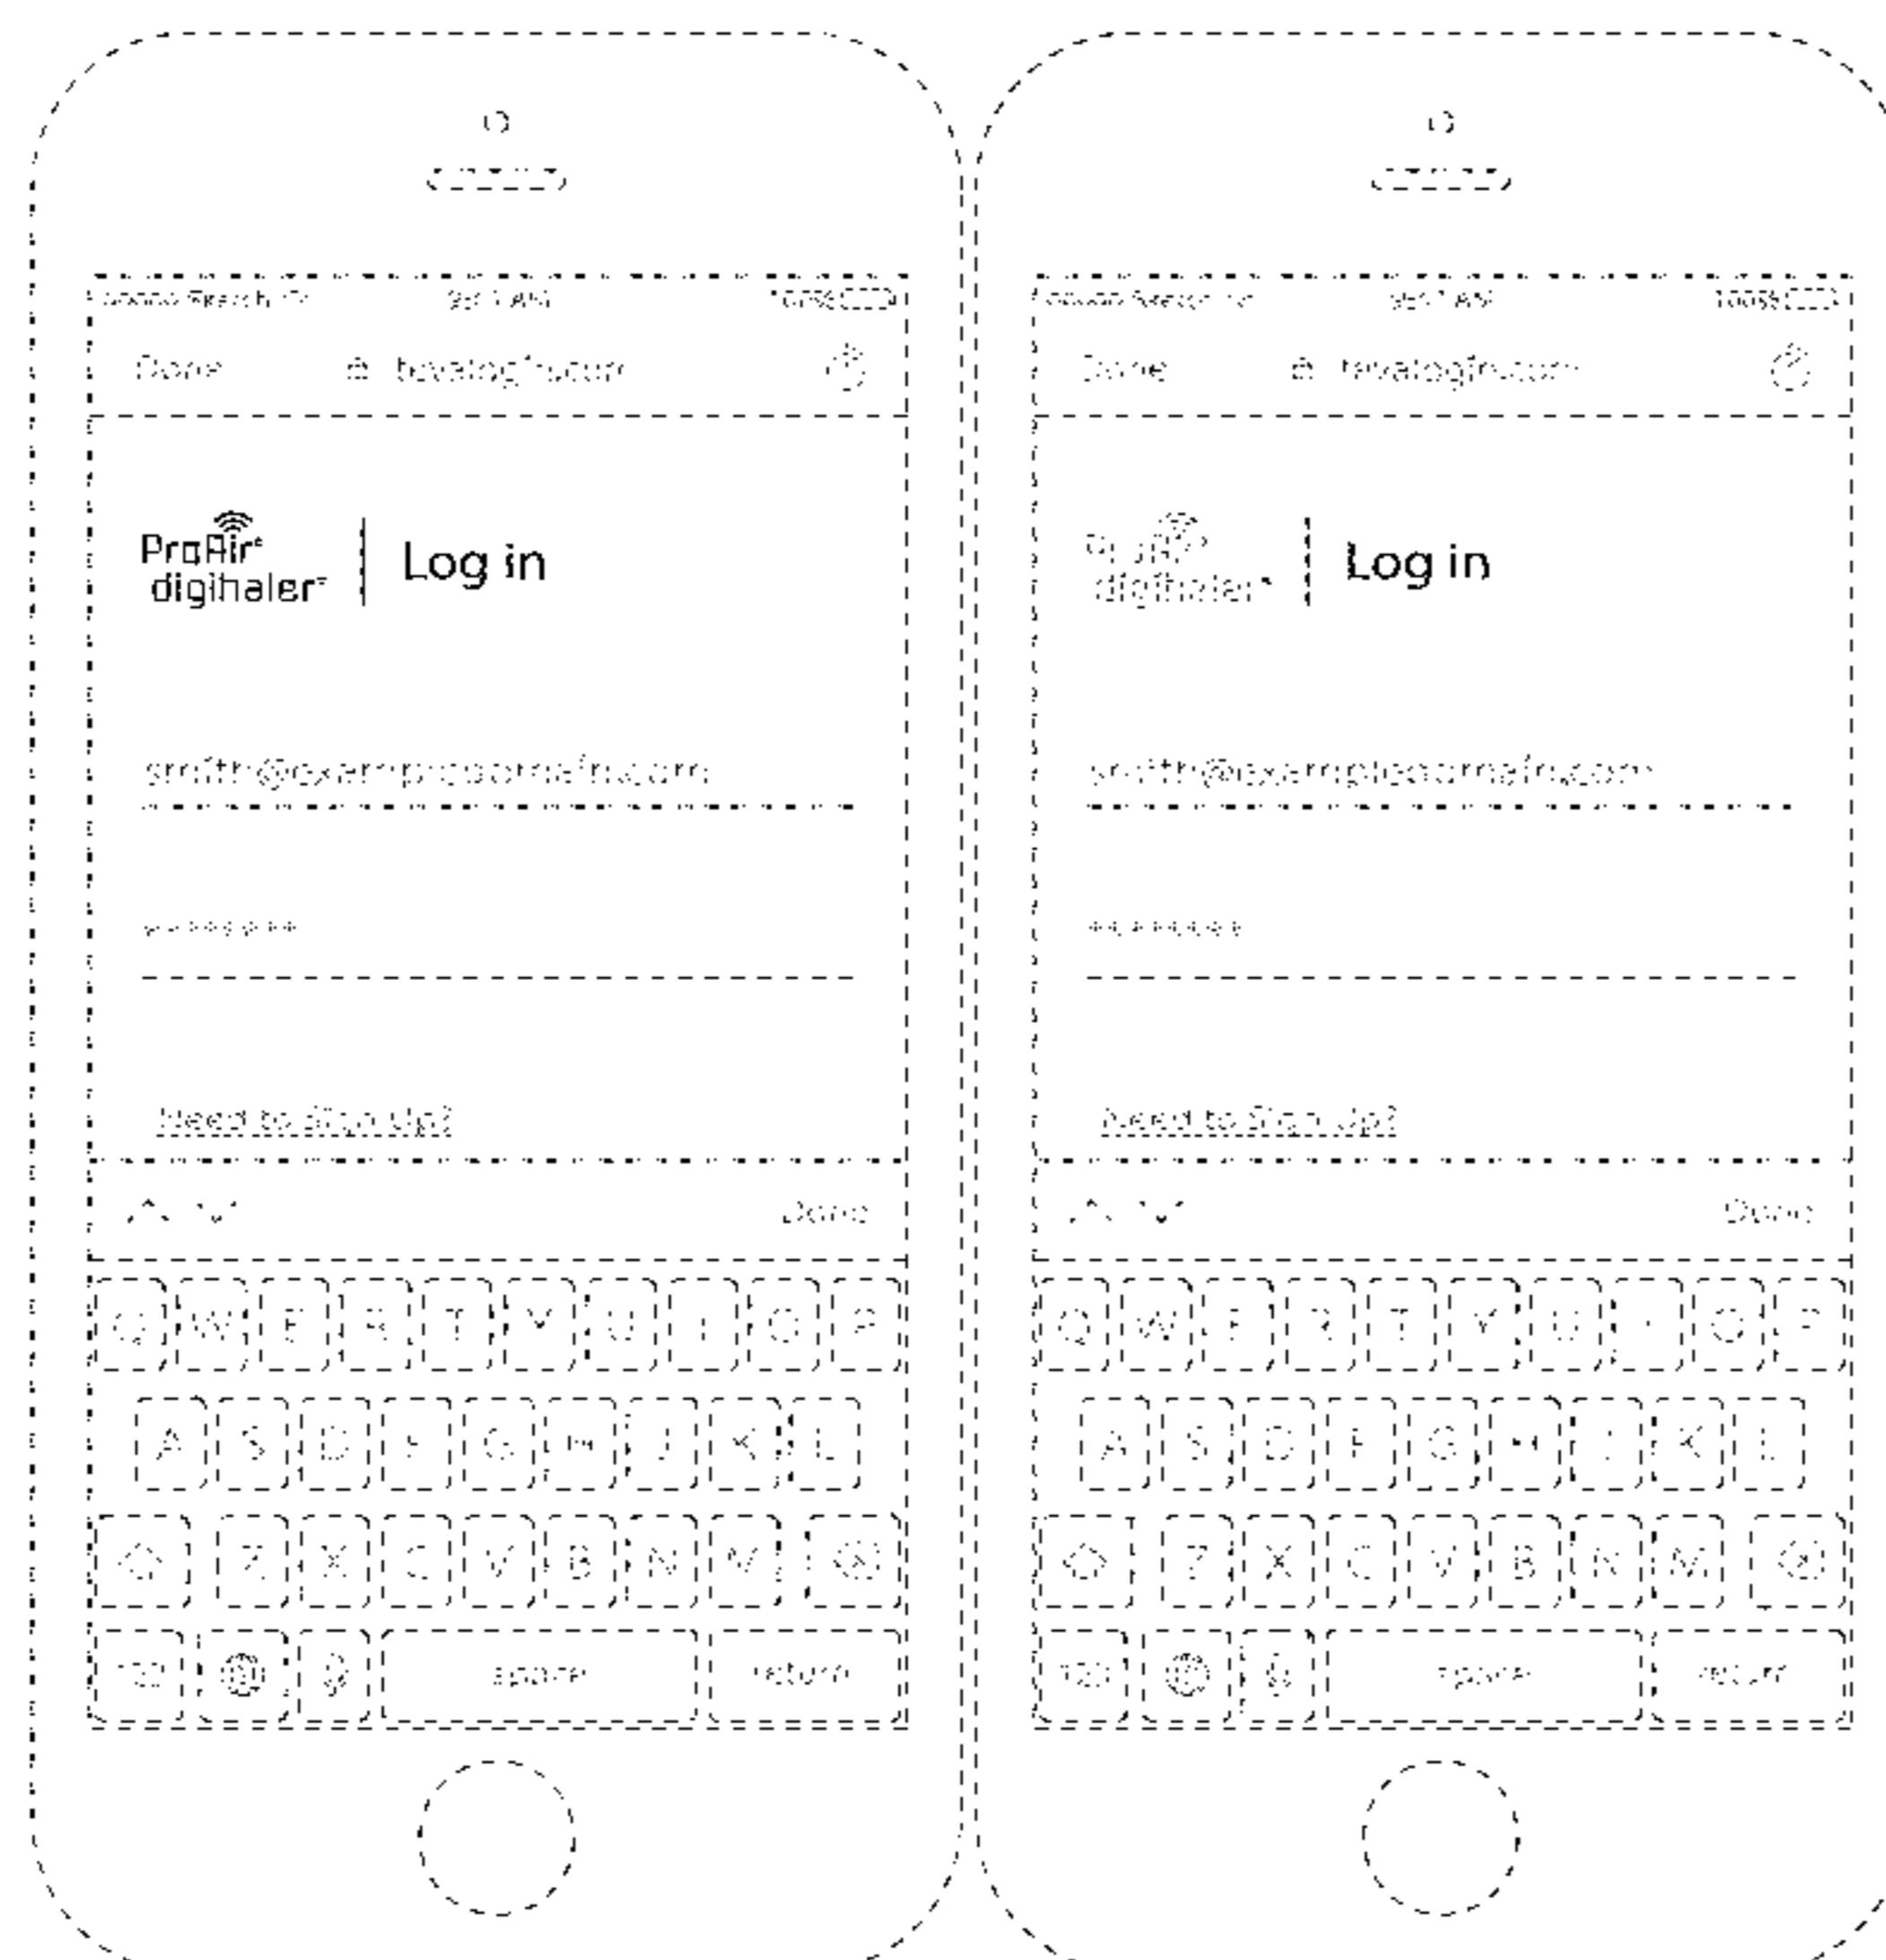

(56)

References Cited

U.S. PATENT DOCUMENTS

D789,956 S * 6/2017 Ortega D14/486
 D803,257 S * 11/2017 Graham D14/487
 D803,258 S * 11/2017 Graham D14/487
 D810,772 S * 2/2018 Wang D14/486
 D821,409 S * 6/2018 Chang D14/485
 D842,884 S * 3/2019 Krainer D14/486
 D845,988 S * 4/2019 Alexander D14/486
 D847,182 S * 4/2019 Maier D14/486
 D858,563 S * 9/2019 Xu D14/488
 D863,329 S * 10/2019 Hu D14/486
 D868,813 S * 12/2019 Oles D14/486
 D872,128 S * 1/2020 Apodaca D14/489
 D878,402 S * 3/2020 Turner D14/486
 D881,231 S * 4/2020 Hansen D14/486
 D888,738 S * 6/2020 Chang D14/486
 D896,256 S * 9/2020 Kawaichi D14/486
 D896,831 S * 9/2020 Honnette D14/486
 D896,832 S * 9/2020 Honnette D14/486
 10,805,177 B2 * 10/2020 Kanojia H04L 41/06
 D903,700 S * 12/2020 Valladares D14/486

D904,425 S * 12/2020 Paul D14/485
 D905,725 S * 12/2020 Derusseau D14/486
 2013/0275899 A1 * 10/2013 Schubert G06F 3/0481
 715/765
 2016/0018978 A1 * 1/2016 Zenoff G06F 3/0488
 715/731
 2016/0132234 A1 * 5/2016 Riscutia G06F 3/017
 715/773
 2017/0221156 A1 * 8/2017 Mingarelli G06Q 50/01
 2019/0121495 A1 * 4/2019 Latheef G06F 9/453
 2019/0318319 A1 * 10/2019 Blackburn G06Q 10/1053
 2020/0293189 A1 * 9/2020 Chaudhri G06F 3/04842

OTHER PUBLICATIONS

“Teva’s ProAir Digihaler FDA Approved to Monitor Asthma and COPD Treatment.” medgadget.com. Dec. 26, 2018. Accessed Jun. 1, 2020. Available online at URL: <https://www.medgadget.com/2018/12/tevas-proair-digihaler-fda-approved-to-monitor-asthma-and-copd-treatment.html> (Year: 2018).*

* cited by examiner



FIG. 1

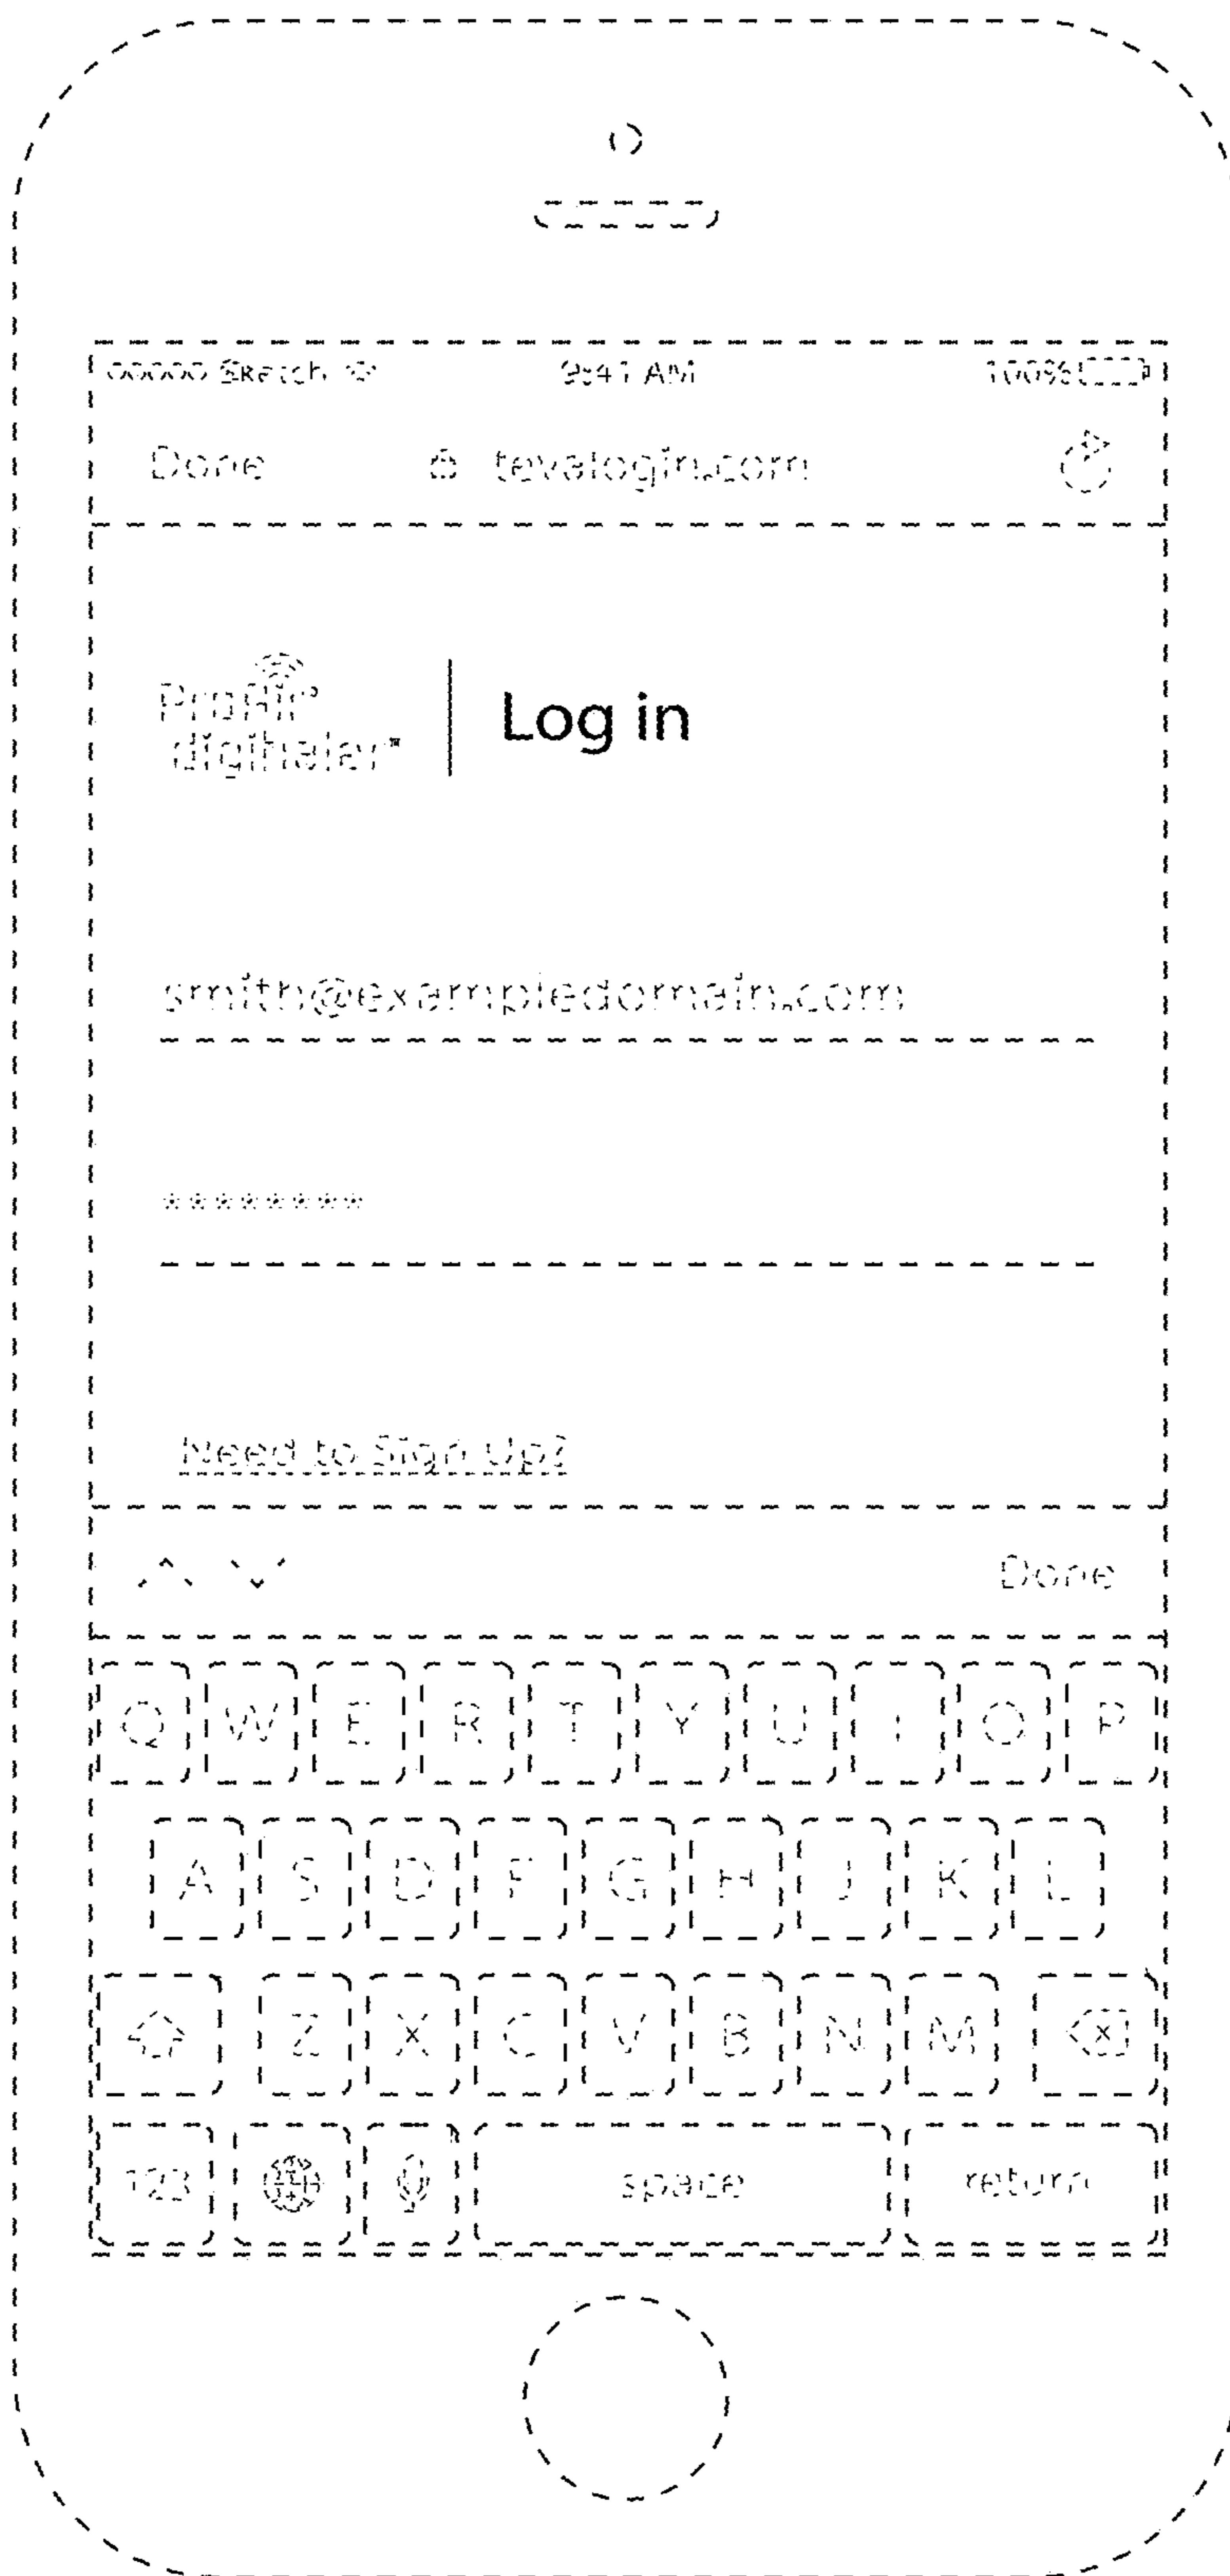


FIG. 2

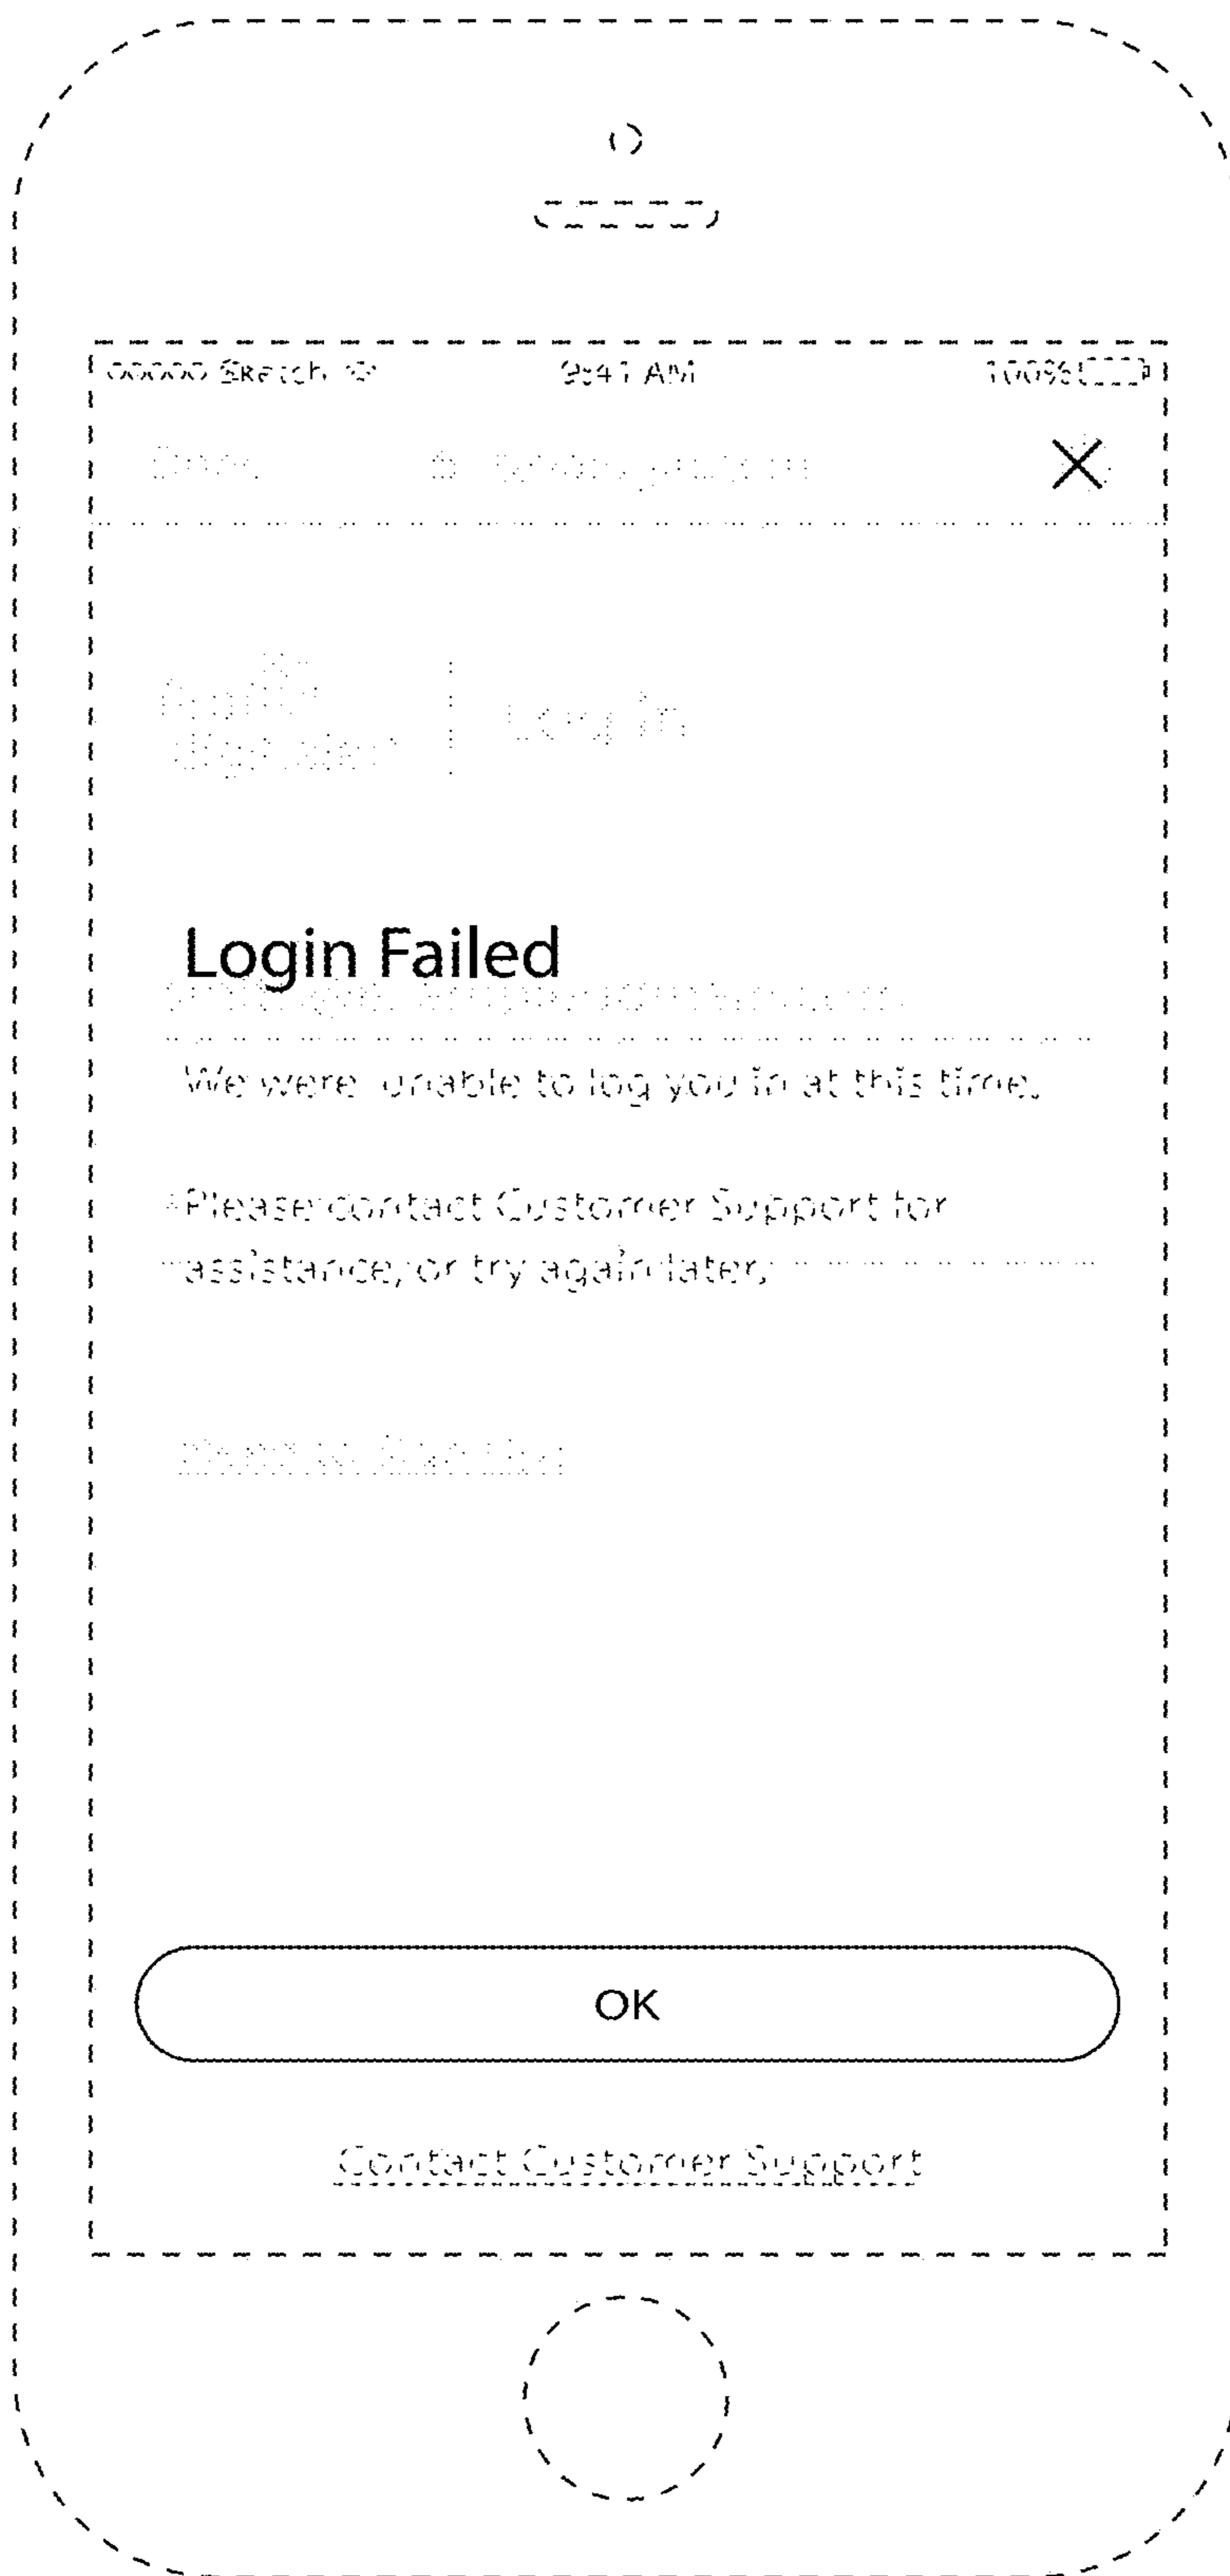


FIG. 3

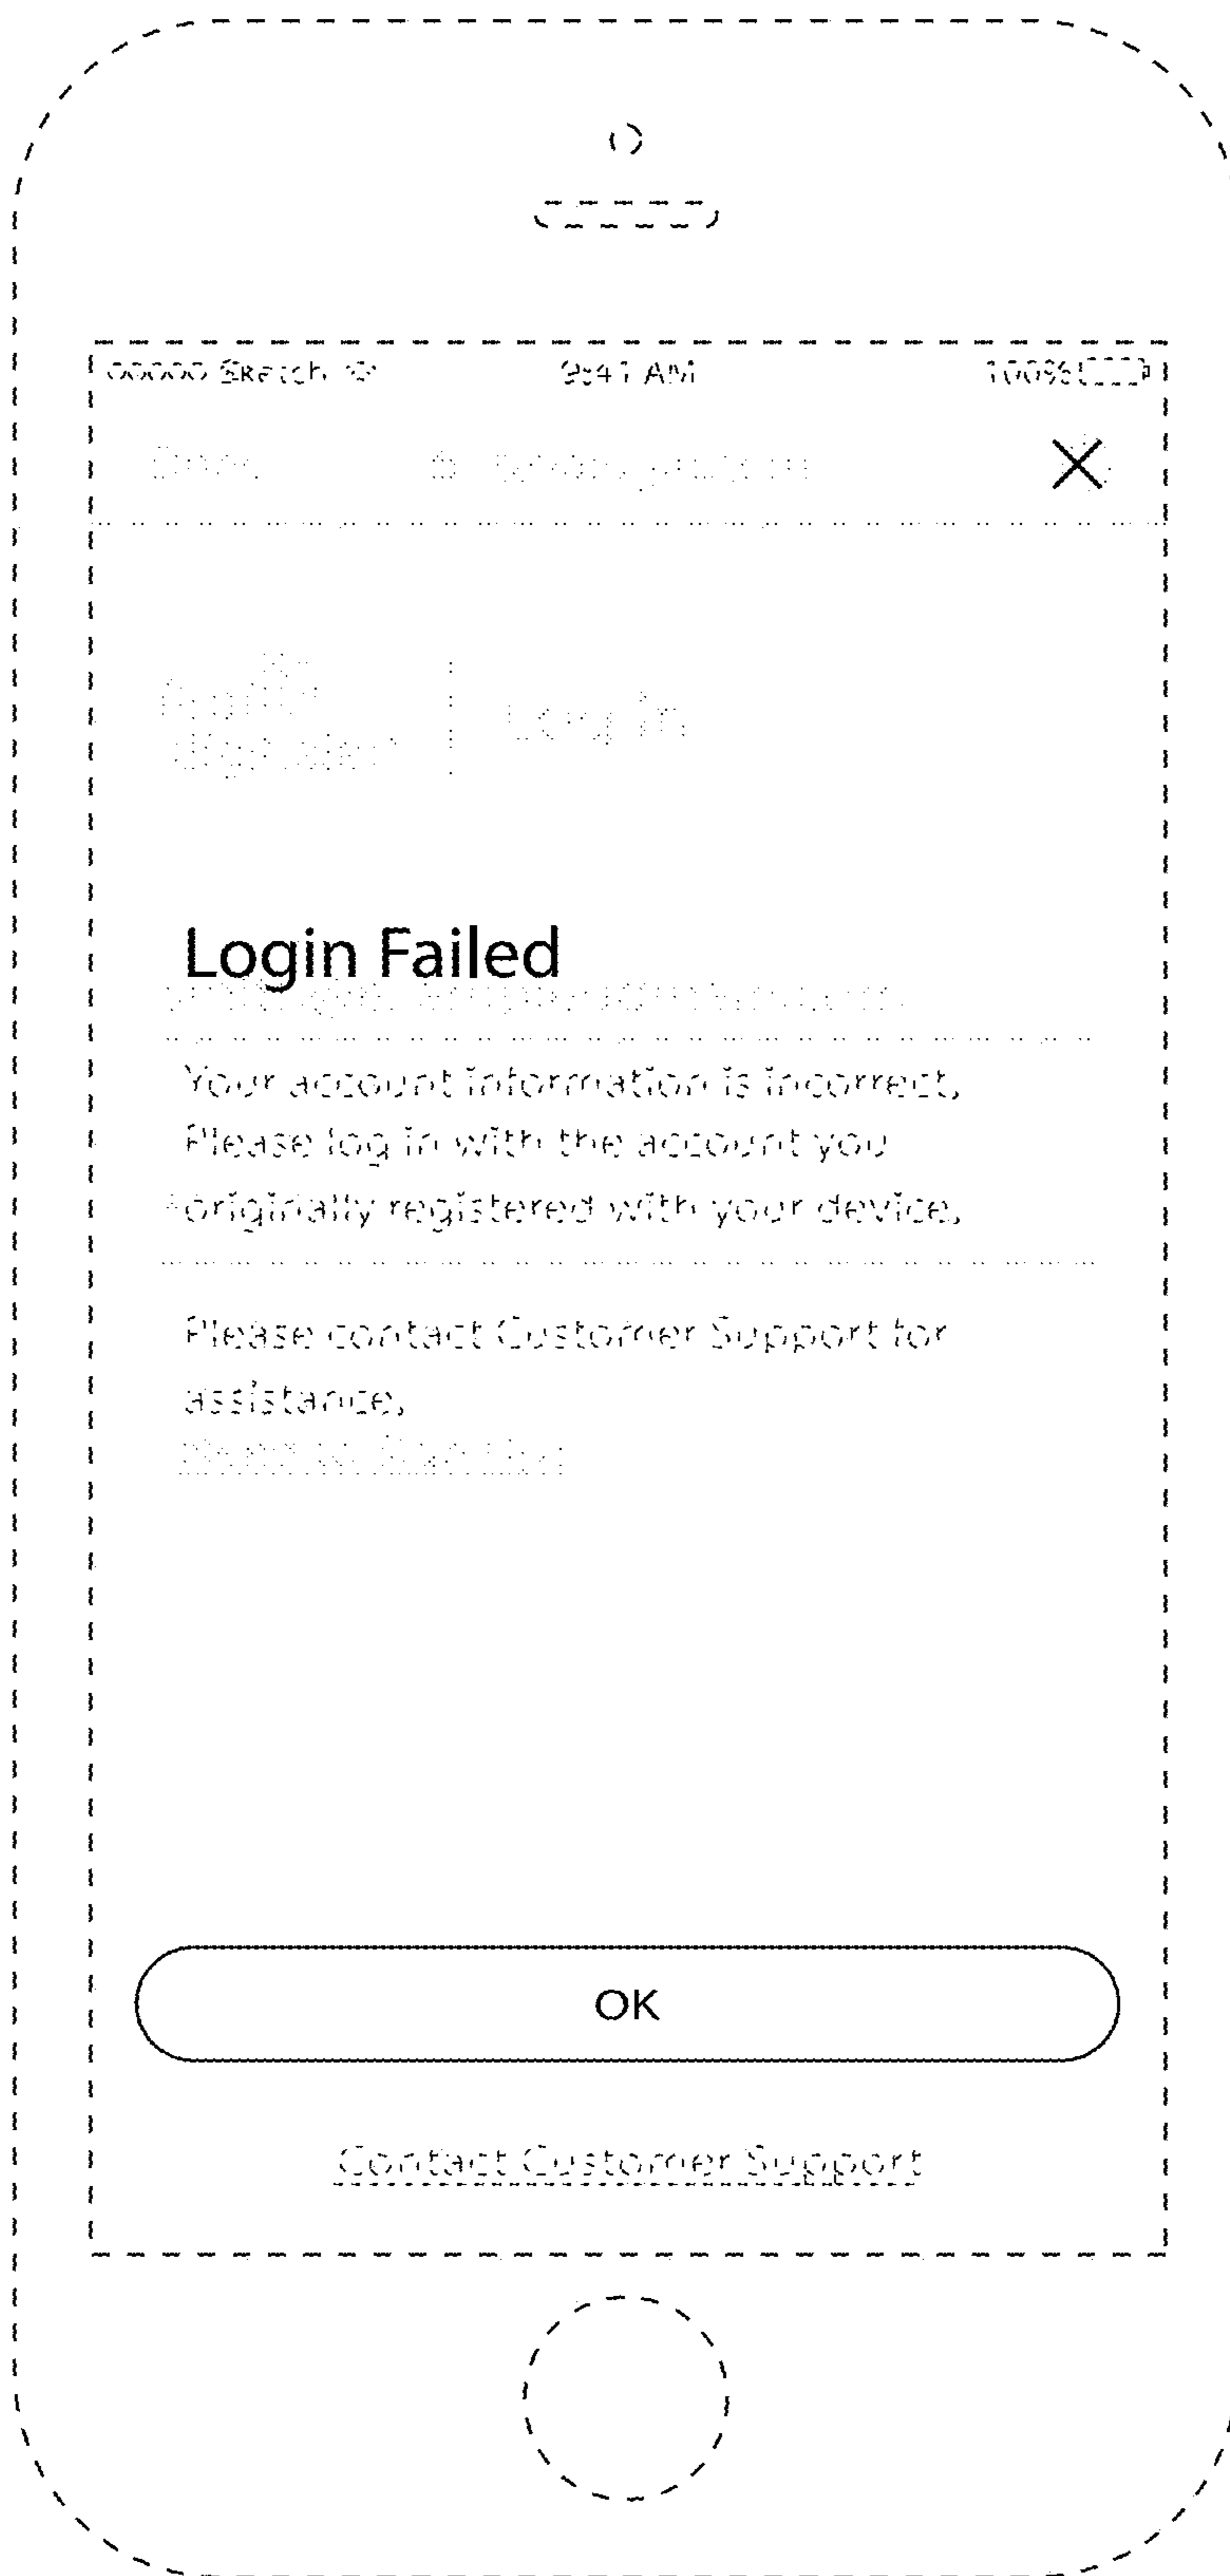


FIG. 4