



US00D921918S

(12) **United States Design Patent** (10) **Patent No.:** **US D921,918 S**
Eriksson (45) **Date of Patent:** **** Jun. 8, 2021**

(54) **APPARATUS FOR BLOOD ANALYSIS**

(71) Applicant: **Hemcheck Sweden Aktiebolag,**
Karlstad (SE)

(72) Inventor: **Björn Olof Eriksson,** Karlstad (SE)

(73) Assignee: **HEMCHECK SWEDEN**
AKTIEBOLAG, Karlstad (SE)

(**) Term: **15 Years**

(21) Appl. No.: **29/666,846**

(22) Filed: **Oct. 16, 2018**

(30) **Foreign Application Priority Data**

Apr. 16, 2018 (EM) 5236114

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**

USPC D24/216, 219, 220, 222, 224, 225, 226,
D24/227, 229, 223, 101, 103, 104, 107

CPC A61B 5/150022; A61B 5/15; A61B
5/150358; A61B 10/02; B01L 3/5635;
B01L 3/5082; B01L 3/5021

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D437,418 S * 2/2001 Suzuki D24/219
- D522,145 S * 5/2006 Best D10/81
- D831,841 S * 10/2018 Tominaga D24/219
- D874,016 S * 1/2020 Figueredo D24/216
- D874,677 S * 2/2020 Stamm D24/216
- D882,110 S * 4/2020 Klein D24/216
- D889,634 S * 7/2020 Tuononen D24/107

- D894,420 S * 8/2020 Nemeth D24/224
- 2013/0267807 A1* 10/2013 MacArthur A61B 5/15146
600/345
- 2017/0224860 A1* 8/2017 Muller C12Q 1/22

OTHER PUBLICATIONS

HemCheck, posted atyoutube.com, posted Mar. 20, 2018, retrieved Sep. 10, 2020, online, URL: <https://www.youtube.com/watch?v=loEINkeXCZw> (Year: 2018).*

* cited by examiner

Primary Examiner — Lilyana Bekic

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **CLAIM**

The ornamental design for an apparatus for blood analysis, as shown and described.

DESCRIPTION

FIG. 1 is front perspective view of an apparatus for blood analysis, showing my new design with the lid lifted.

FIG. 2 is a front elevational view thereof with the lid in place.

FIG. 3 is a back elevational view thereof with the lid in place.


FIG. 4 is a right side elevational view thereof with the lid in place.

FIG. 5 is a left side elevational view thereof with the lid in place.

FIG. 6 is a top plan view thereof with the lid in place; and, FIG. 7 is a bottom plan view thereof with the lid in place.

The dash-dash broken lines in the views illustrate portions of the apparatus for blood analysis that form no part of the claimed design. The dot-dash broken lines in the drawings indicate the boundaries of the claimed design and form no part thereof.

1 Claim, 7 Drawing Sheets

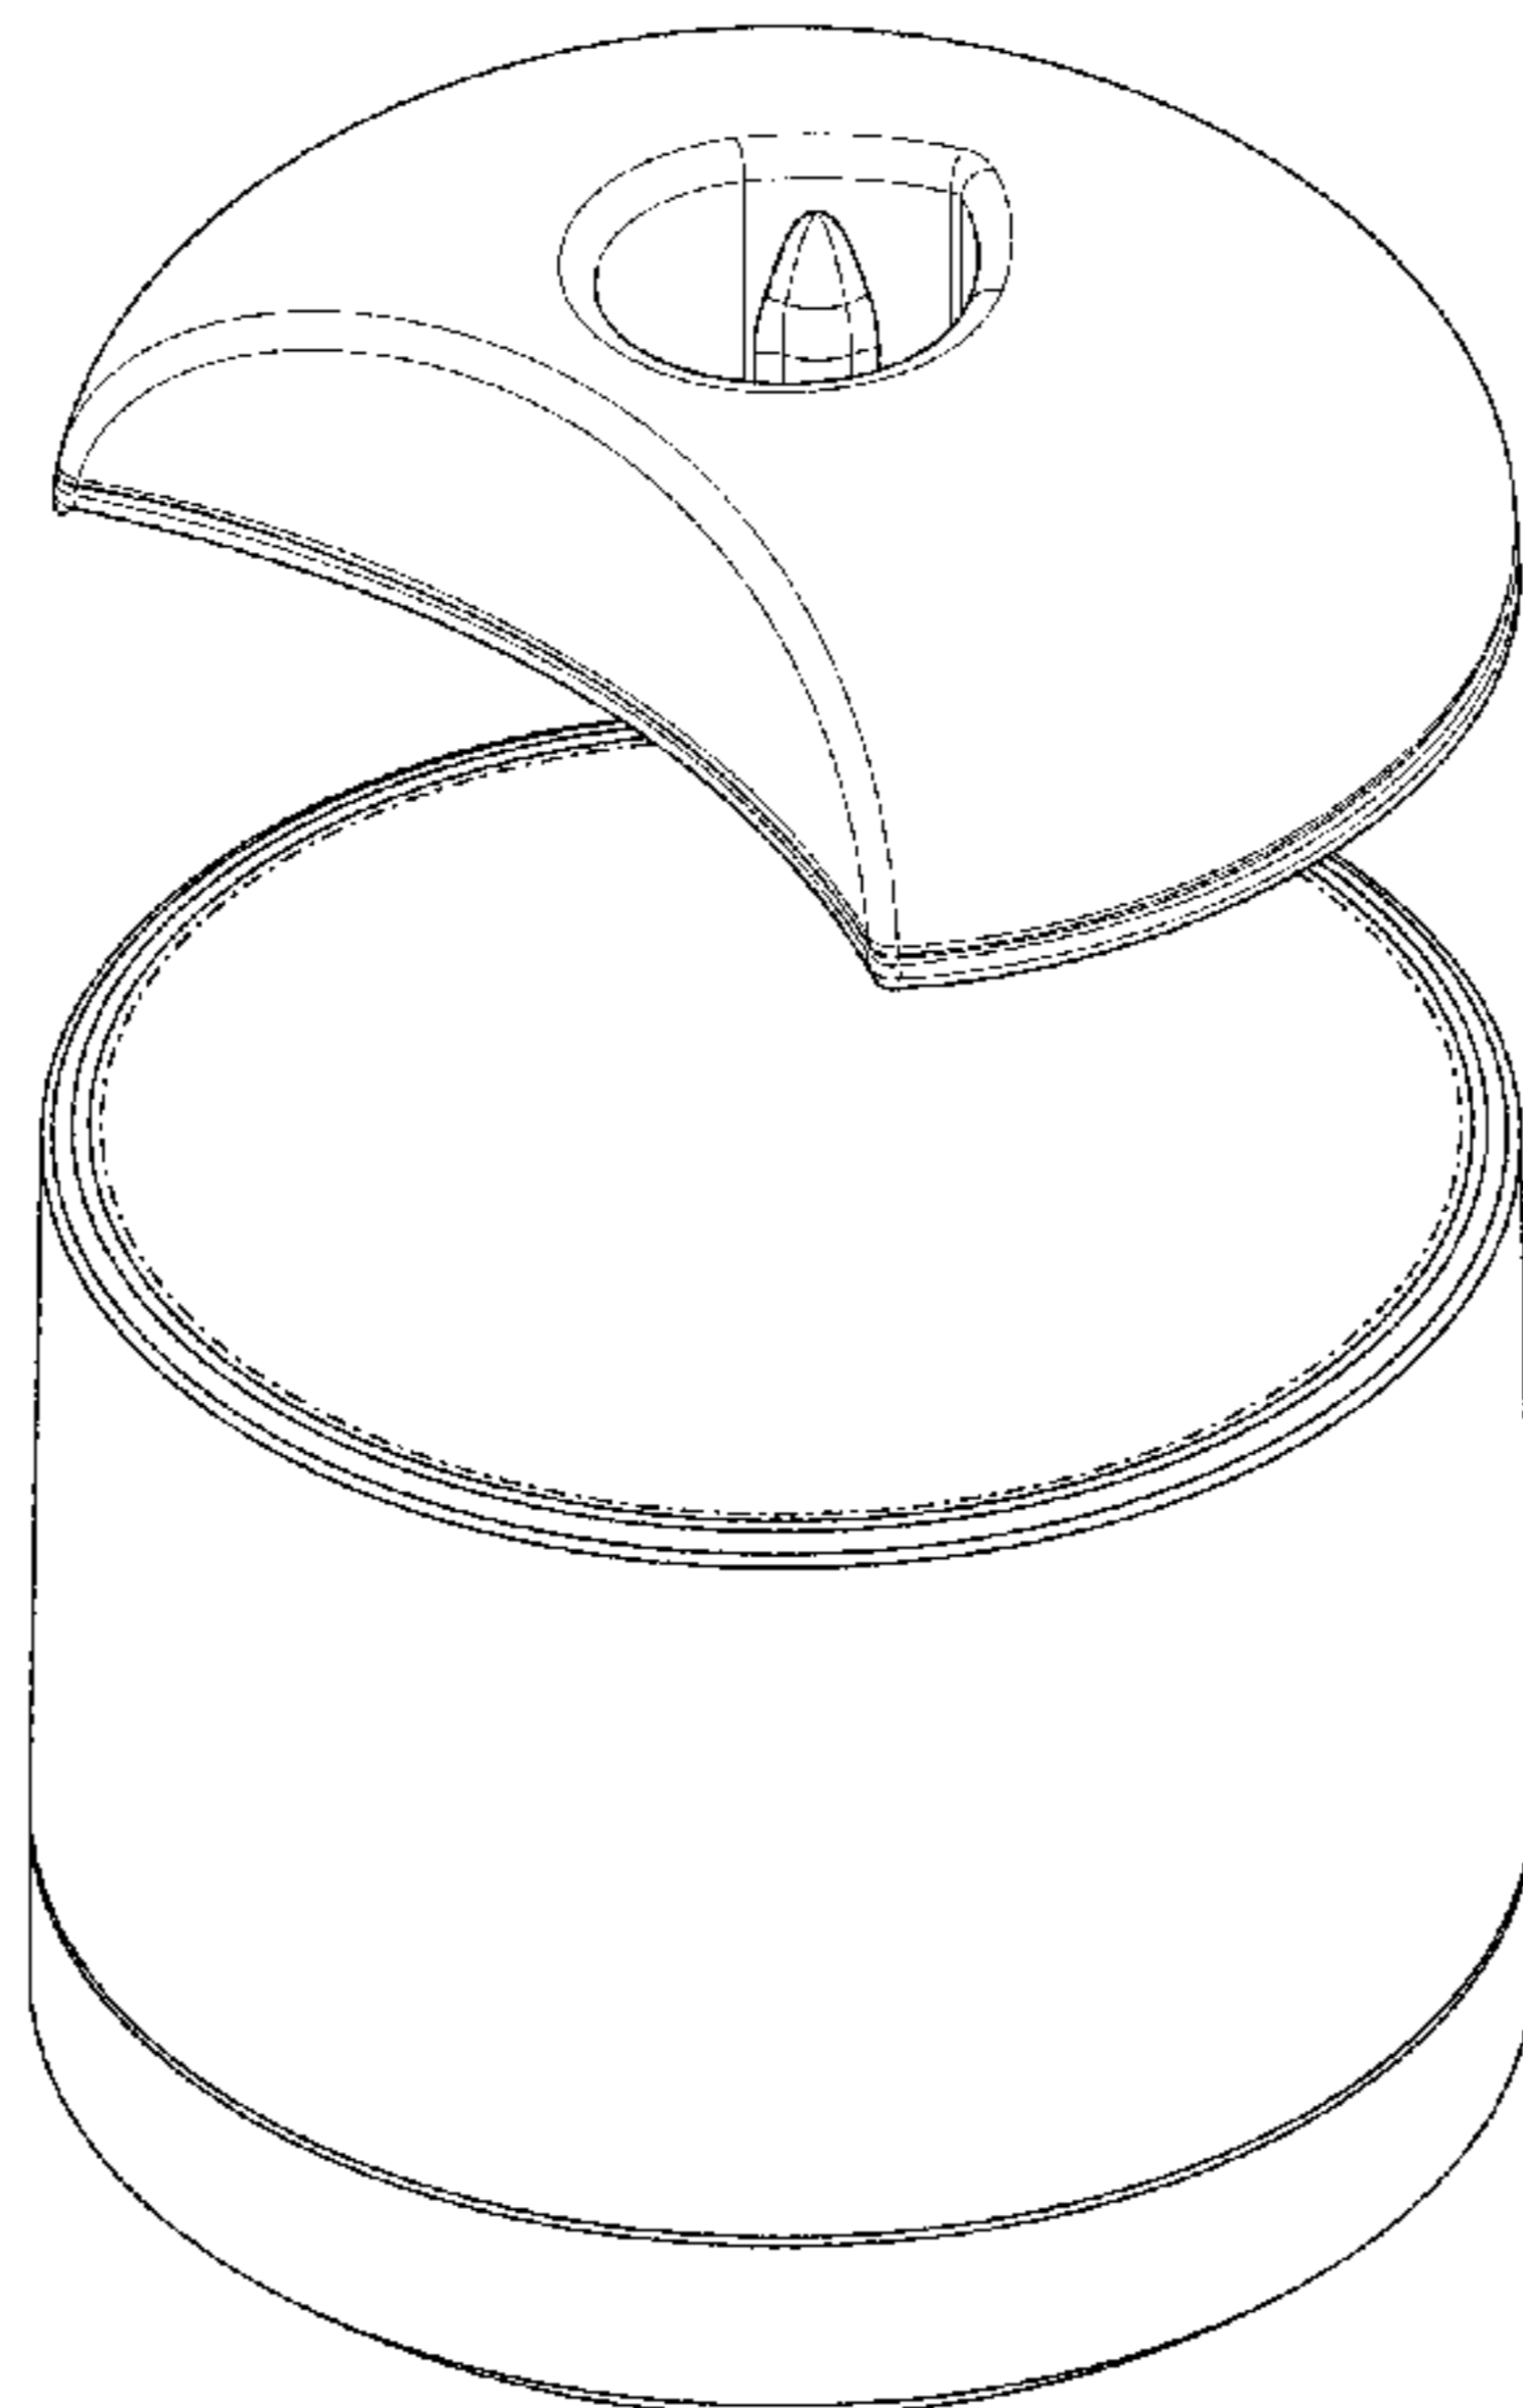

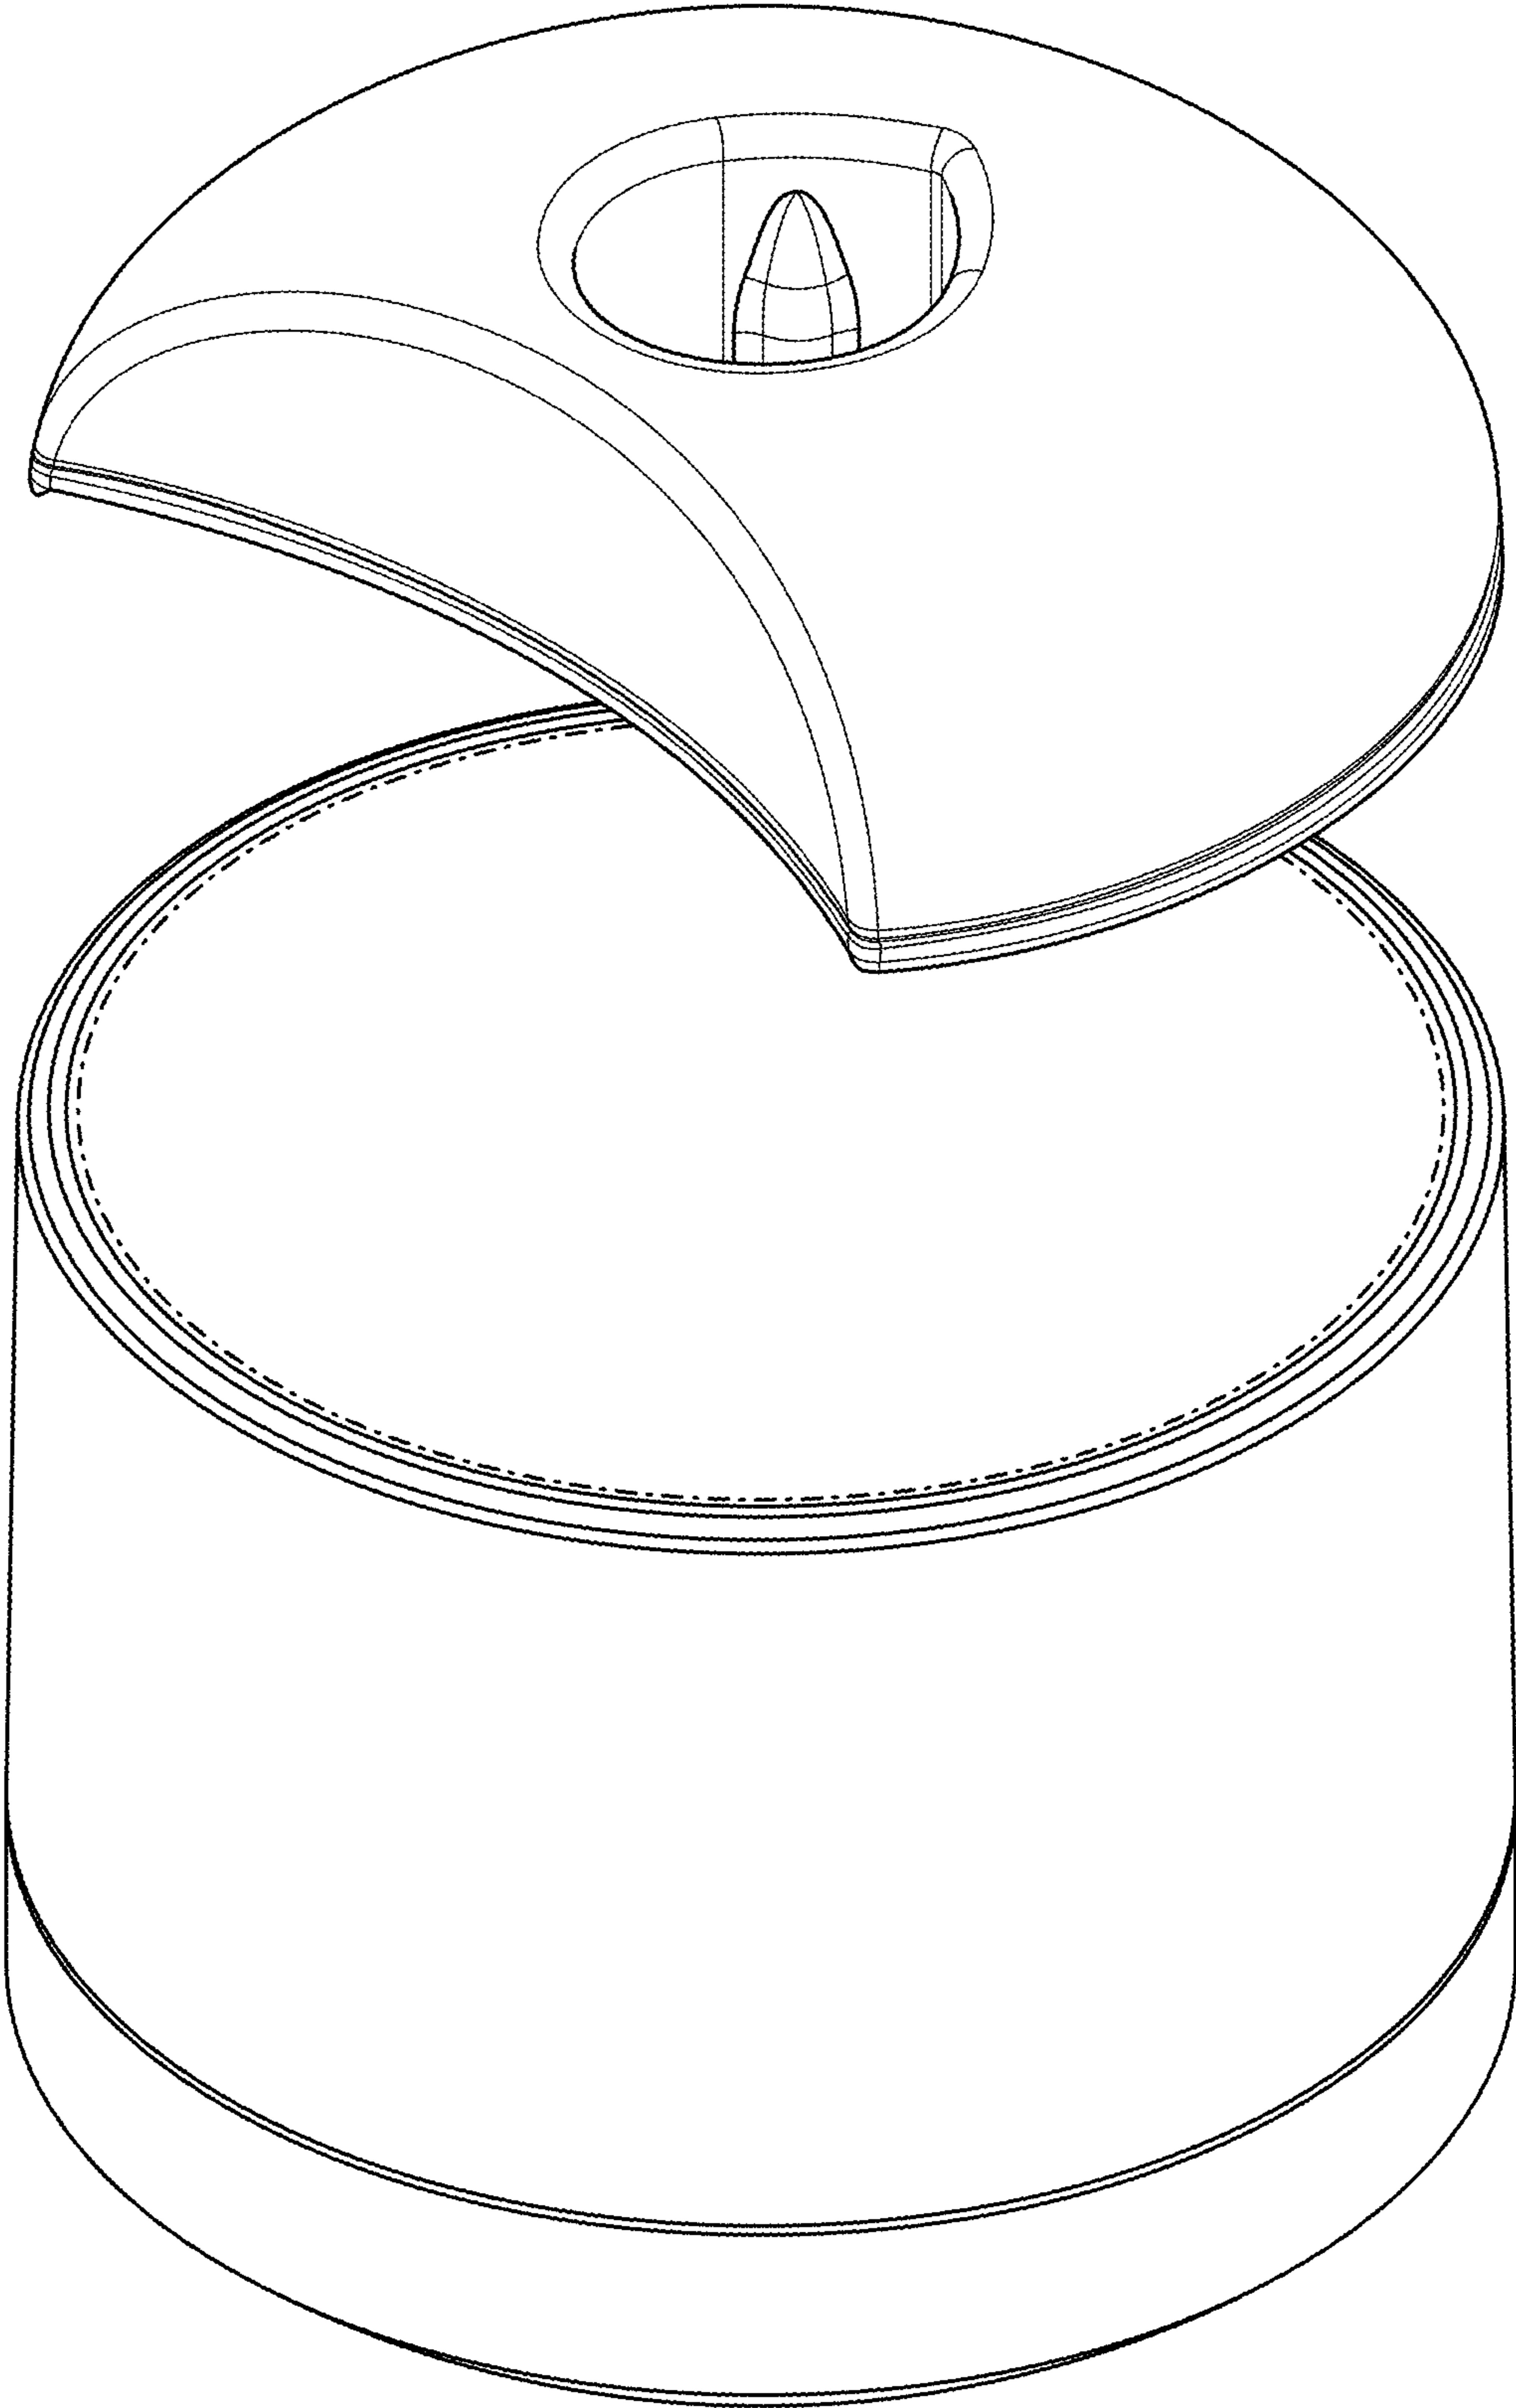


FIG. 1

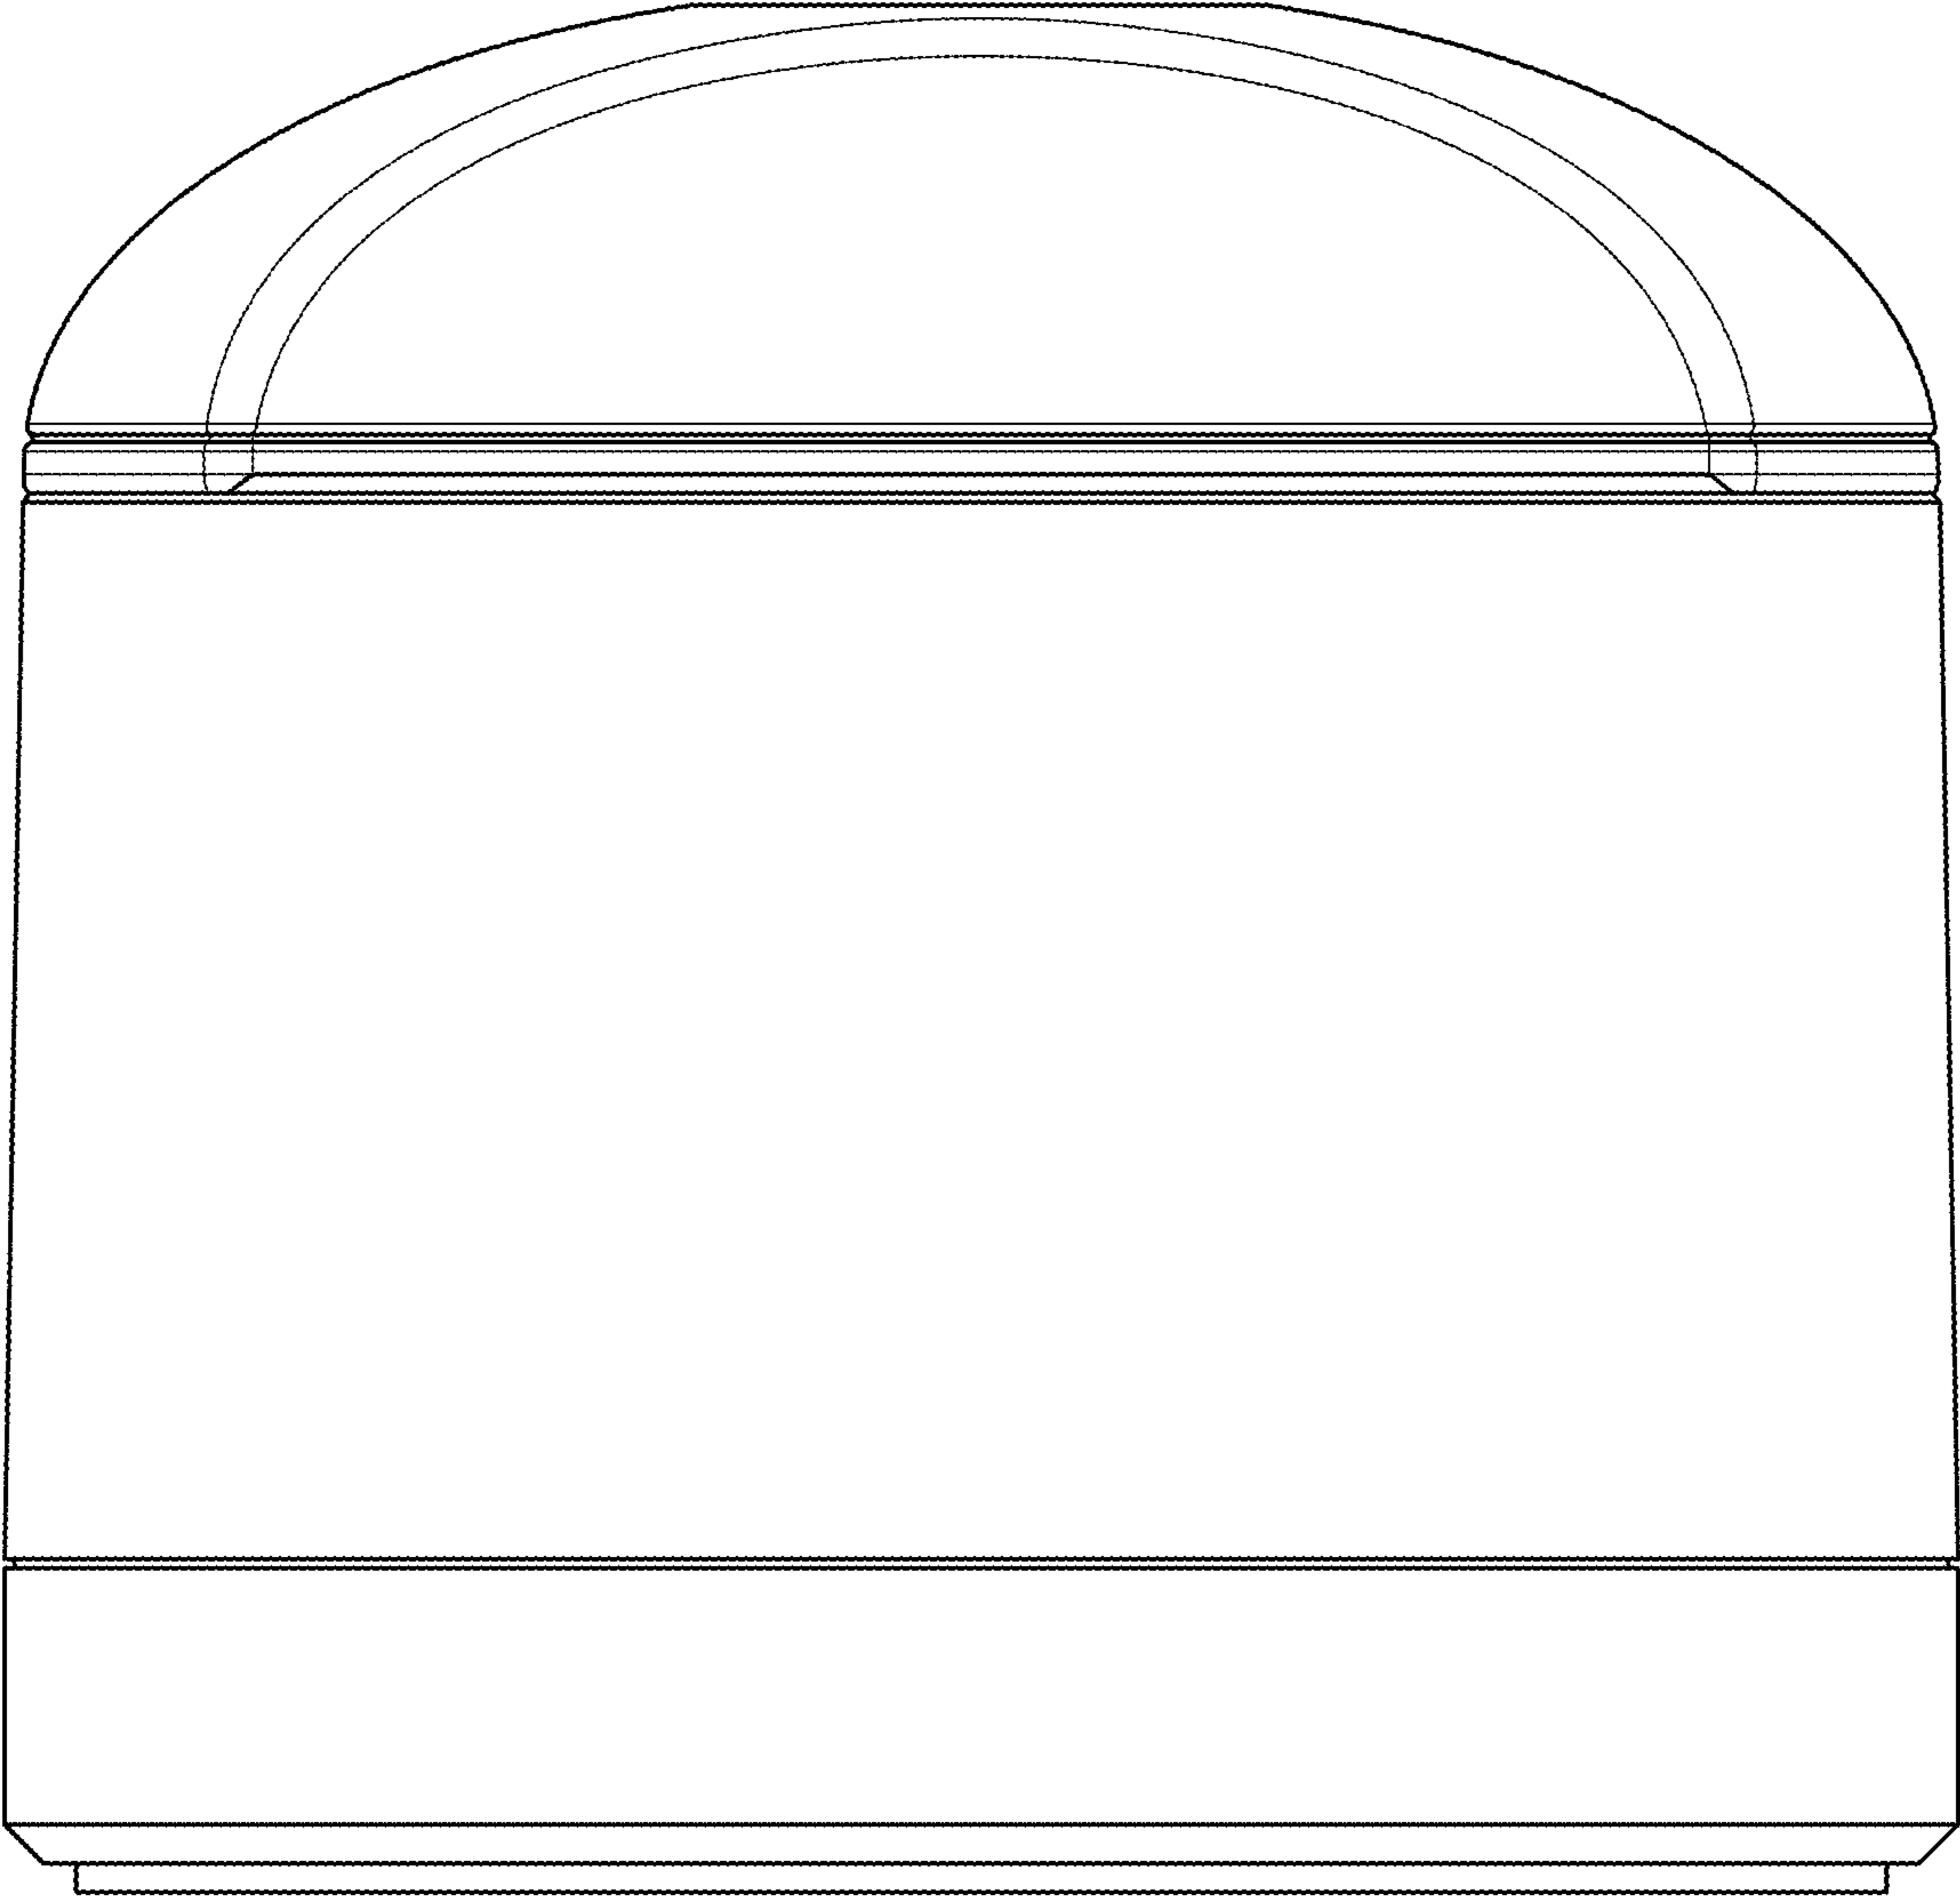


FIG. 2

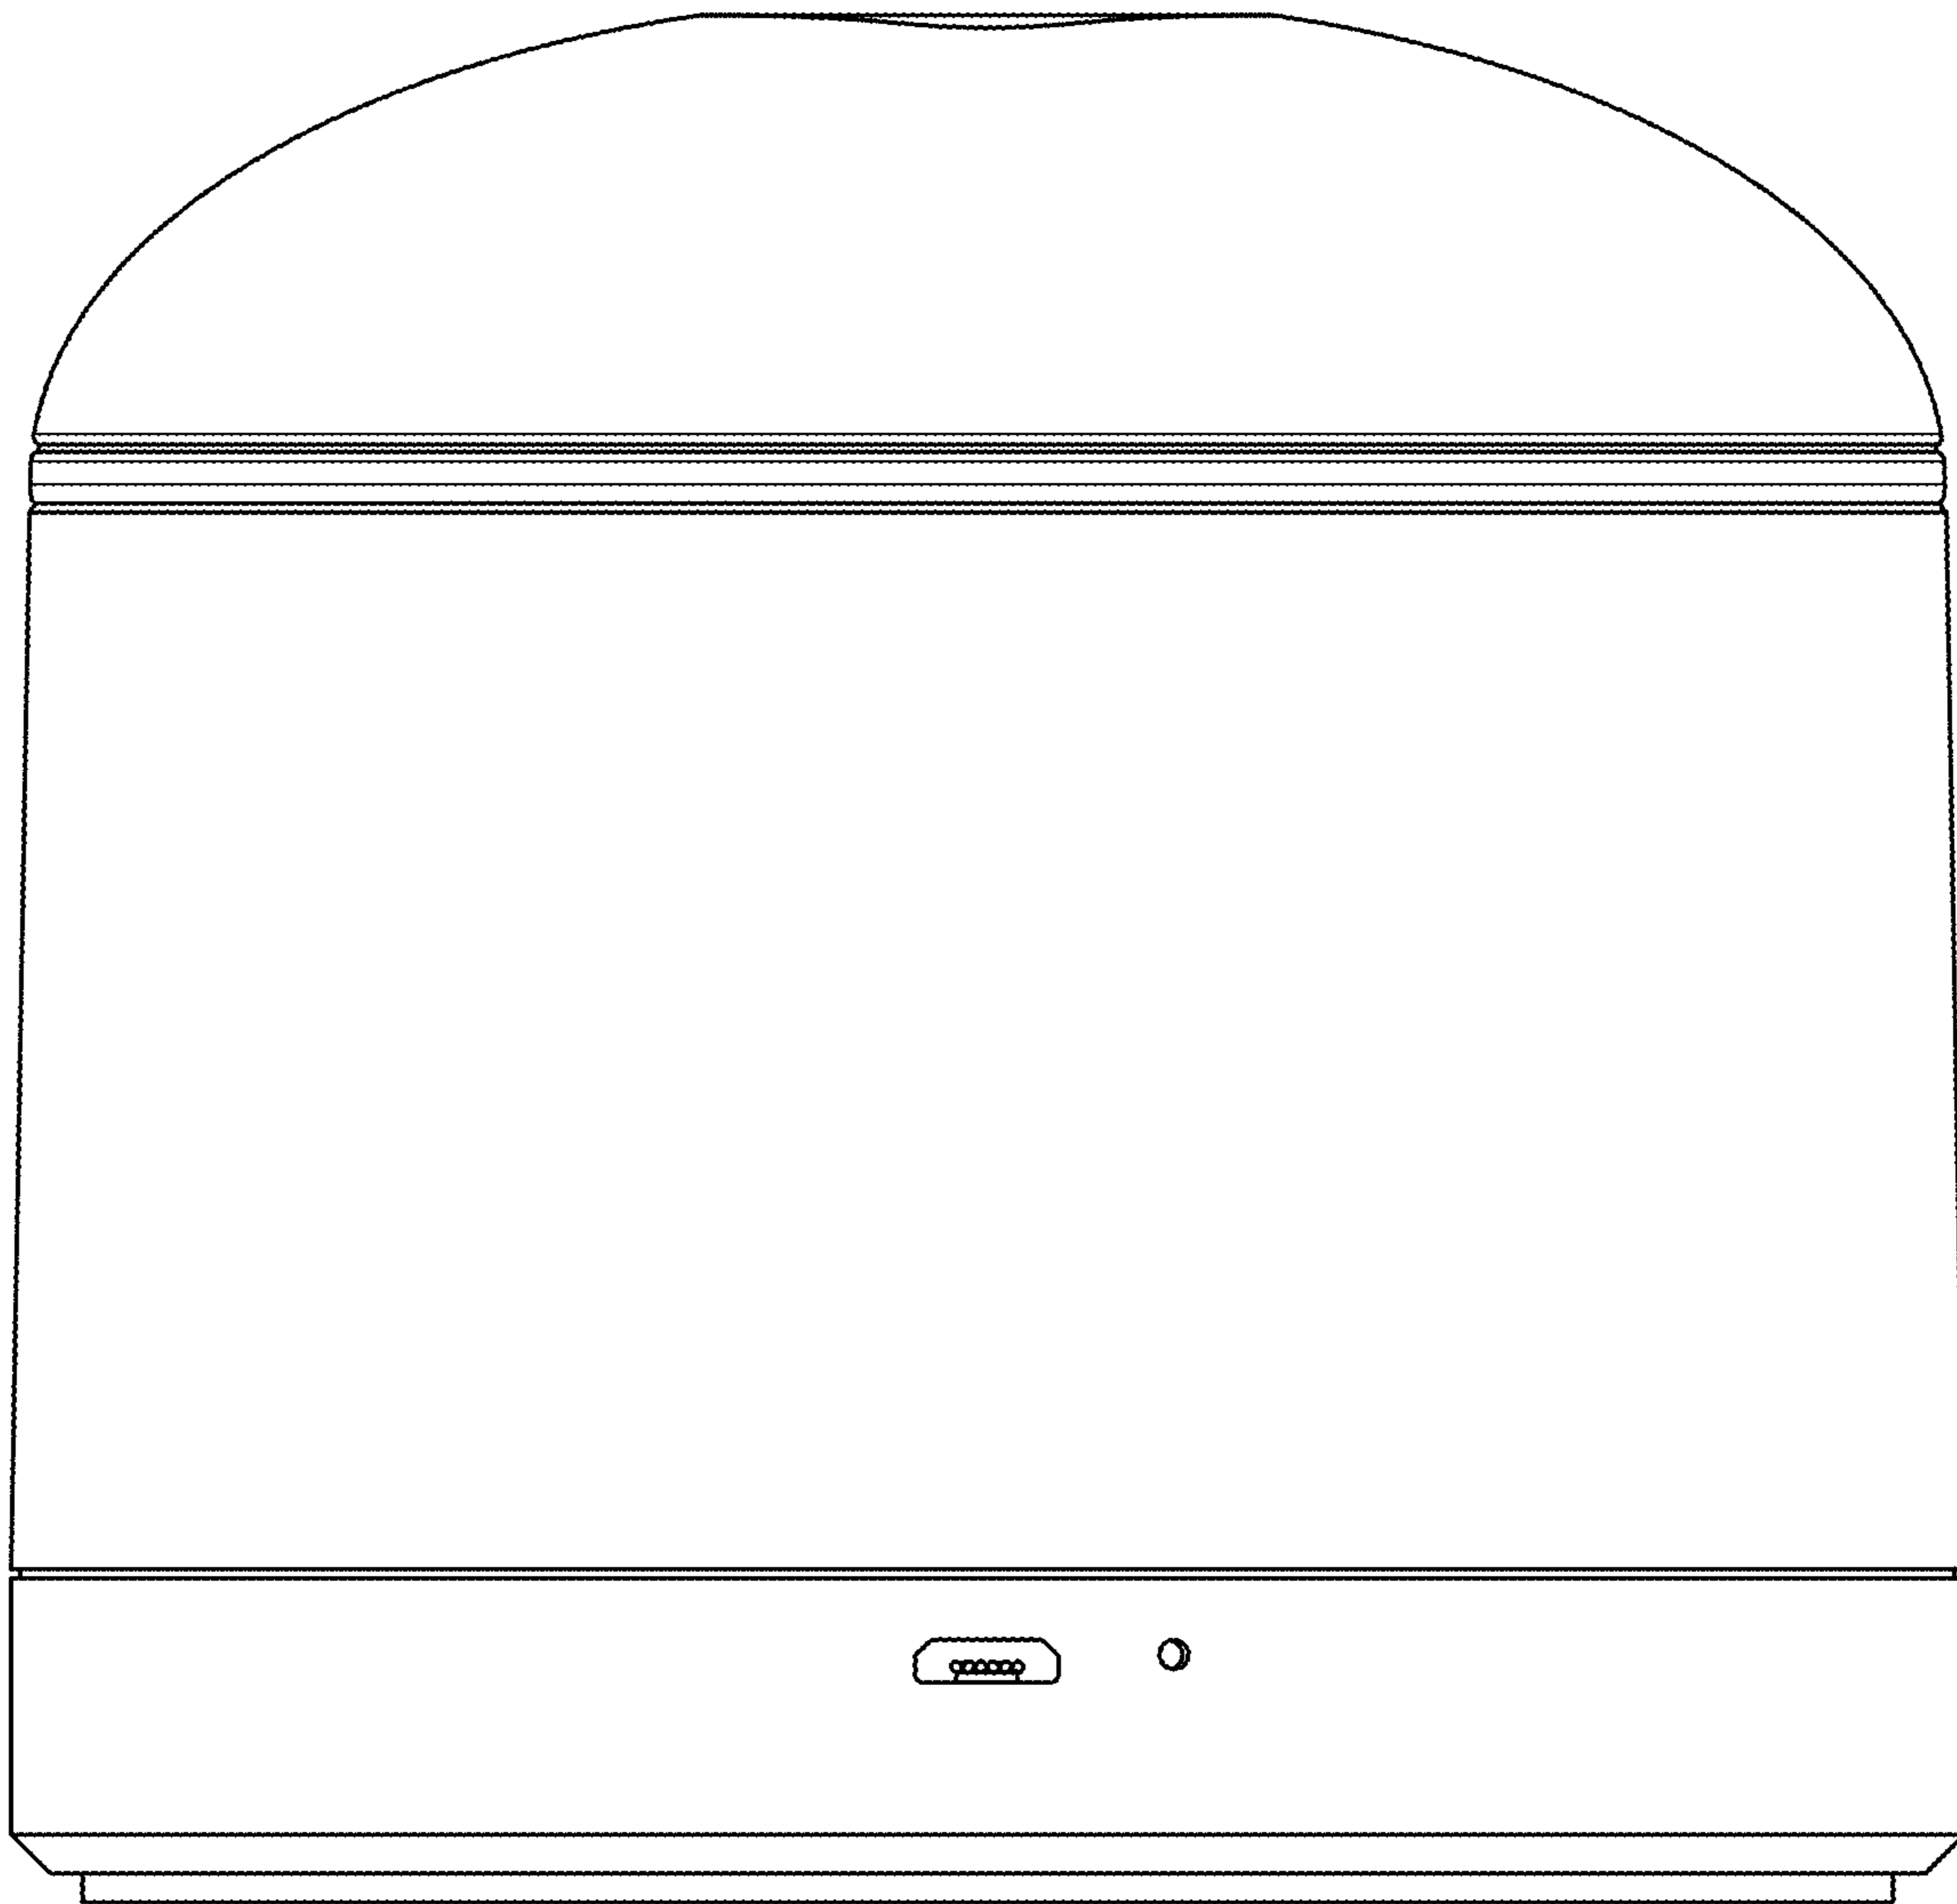


FIG. 3

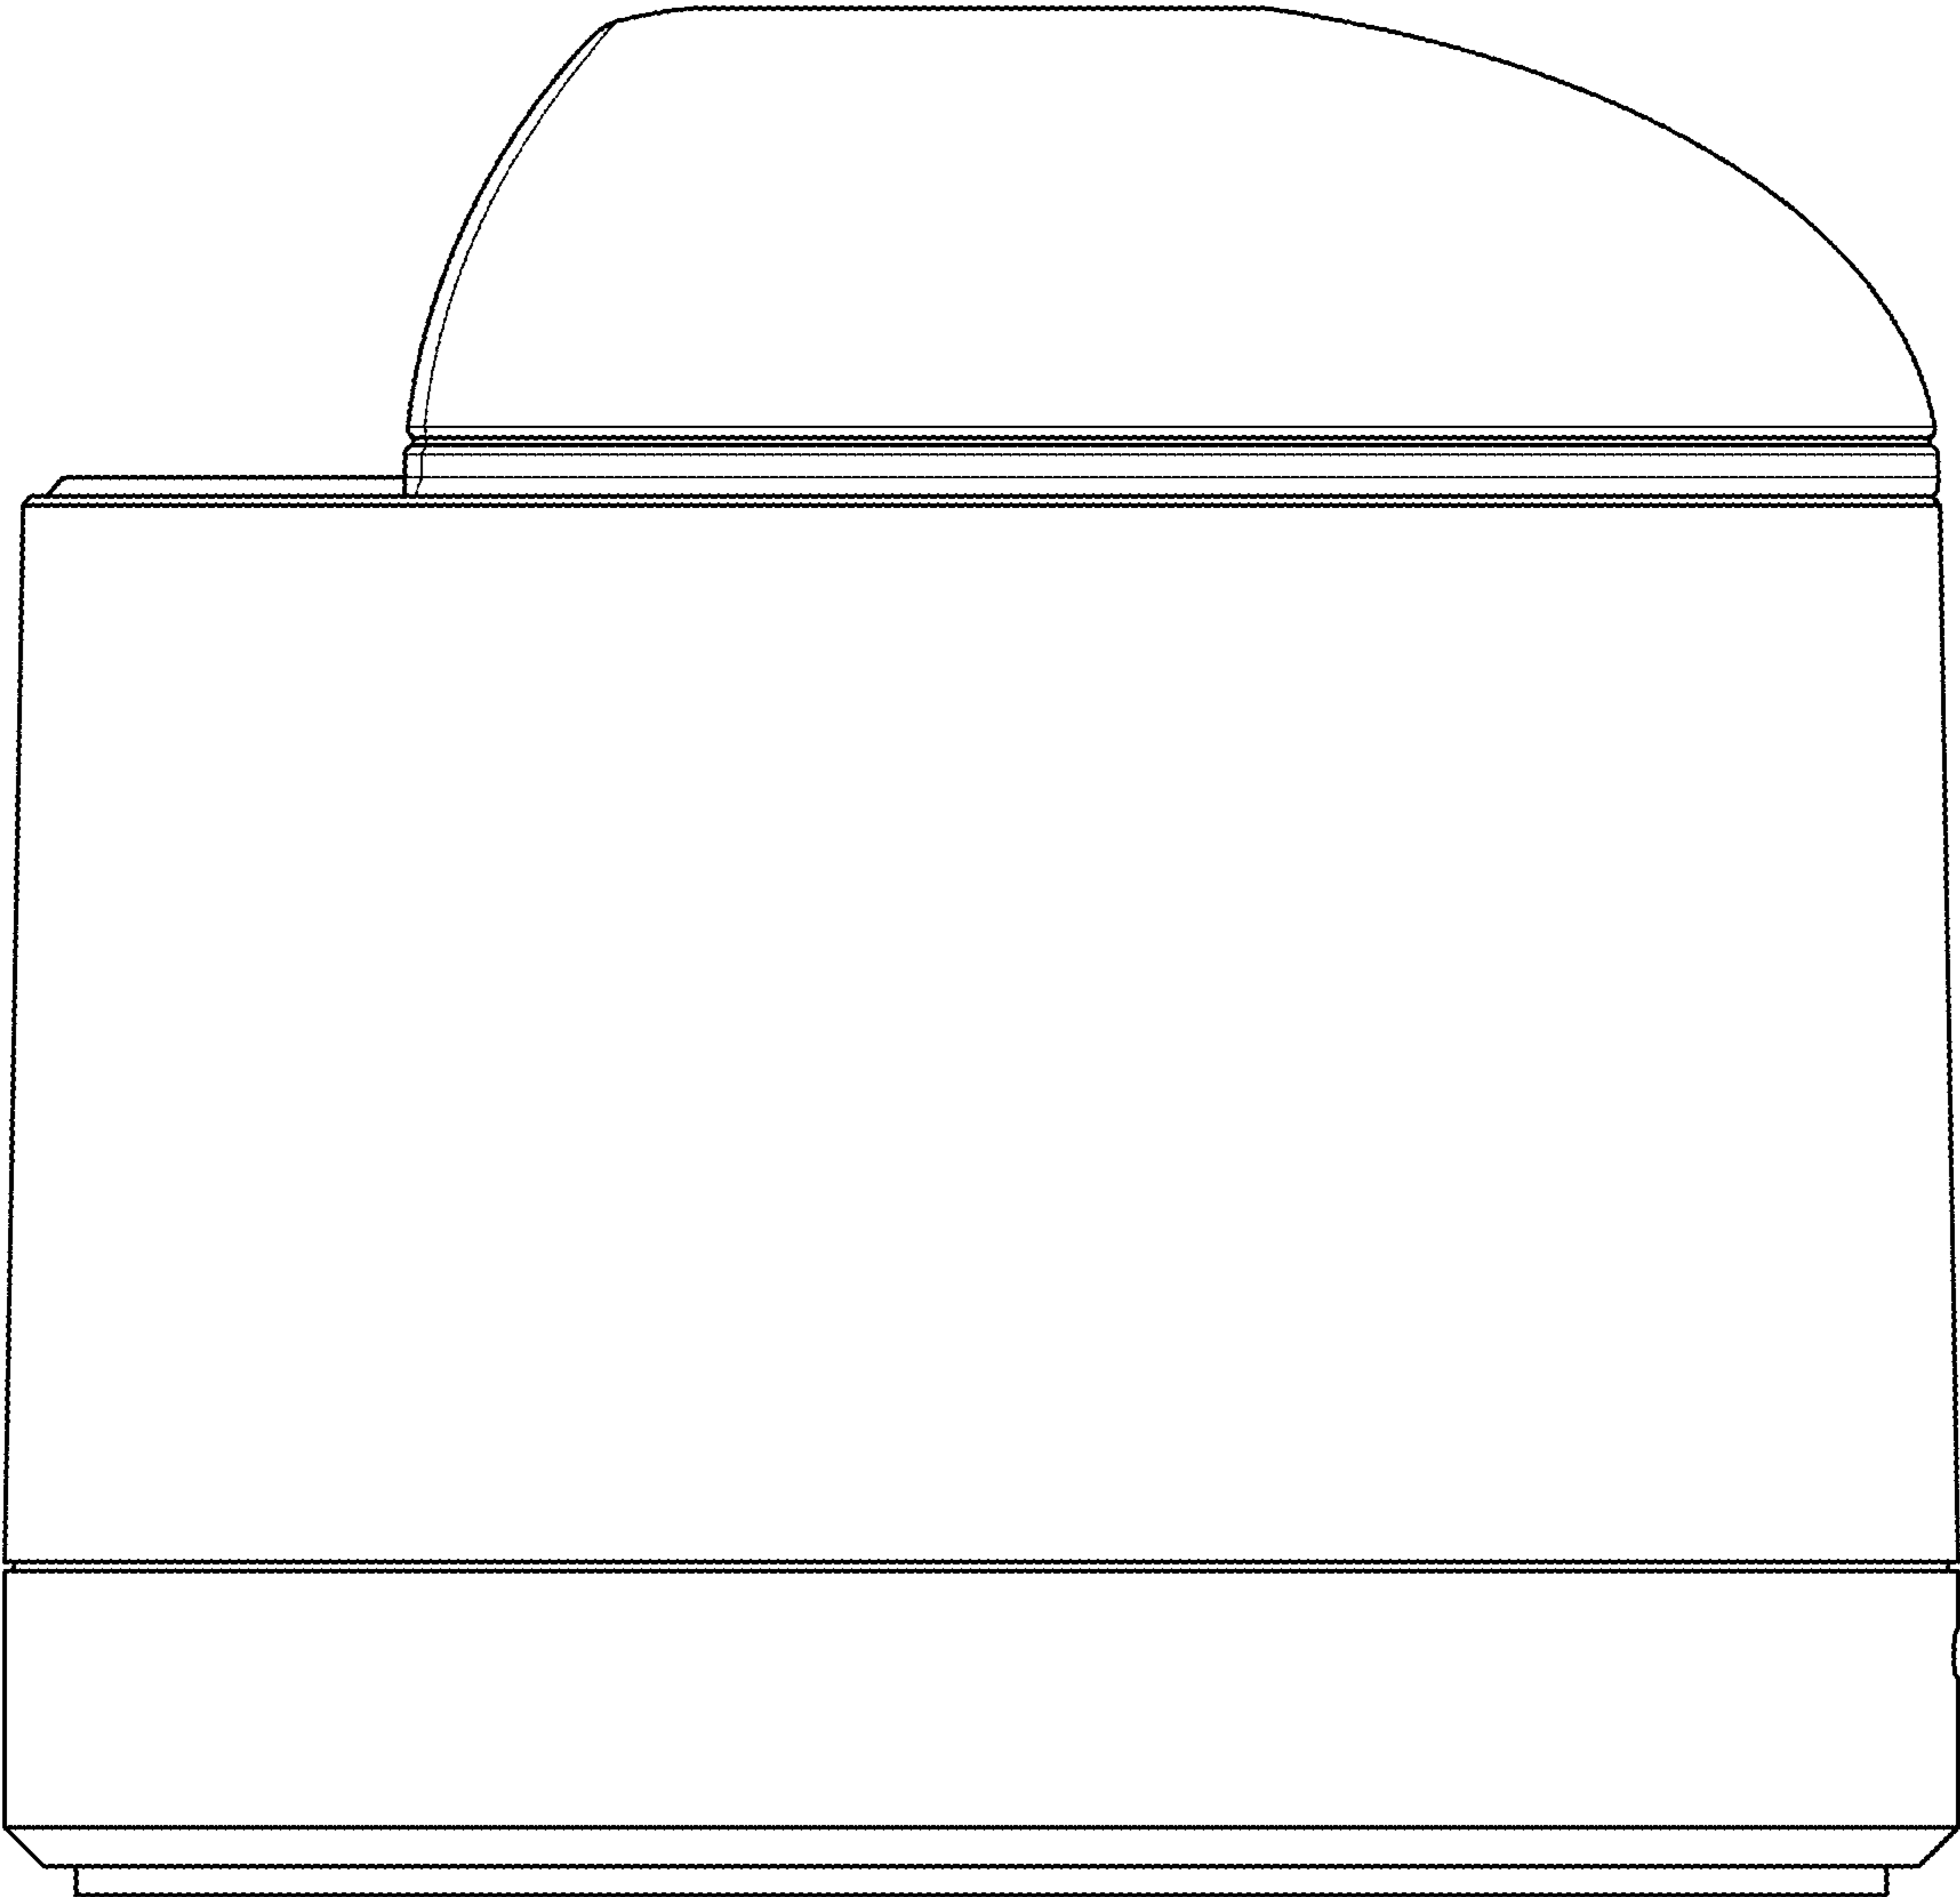


FIG. 4

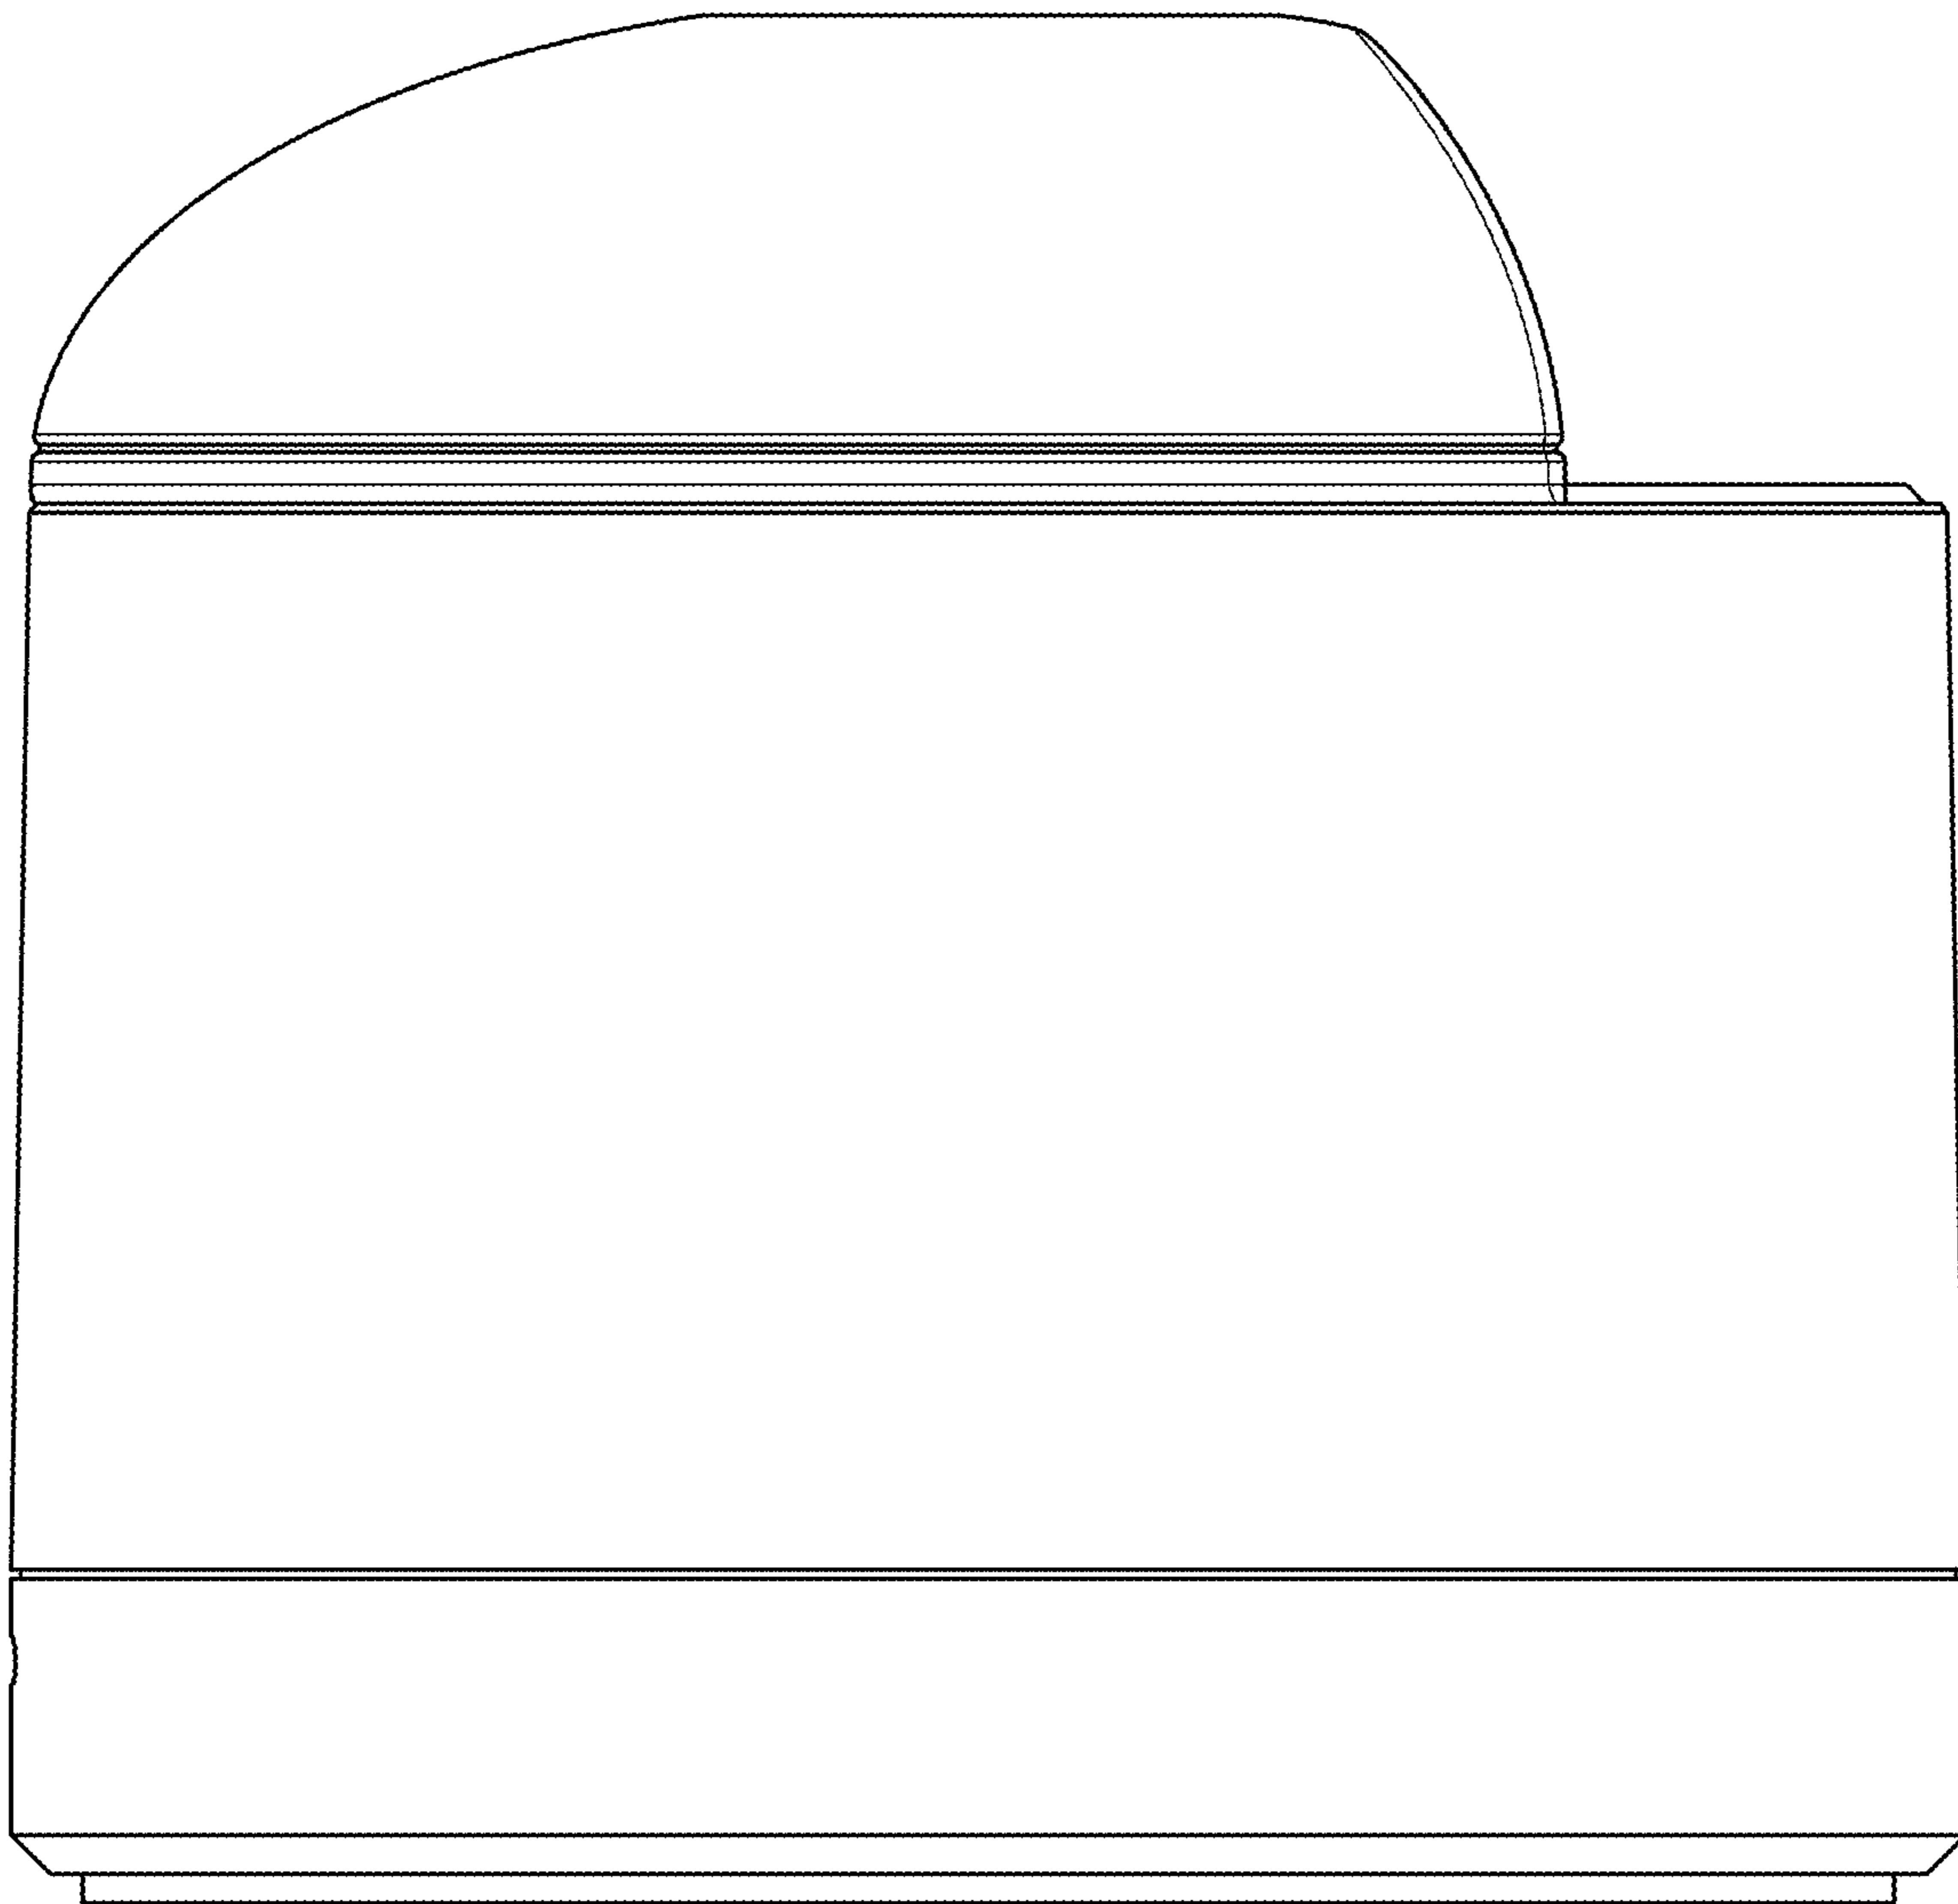


FIG. 5

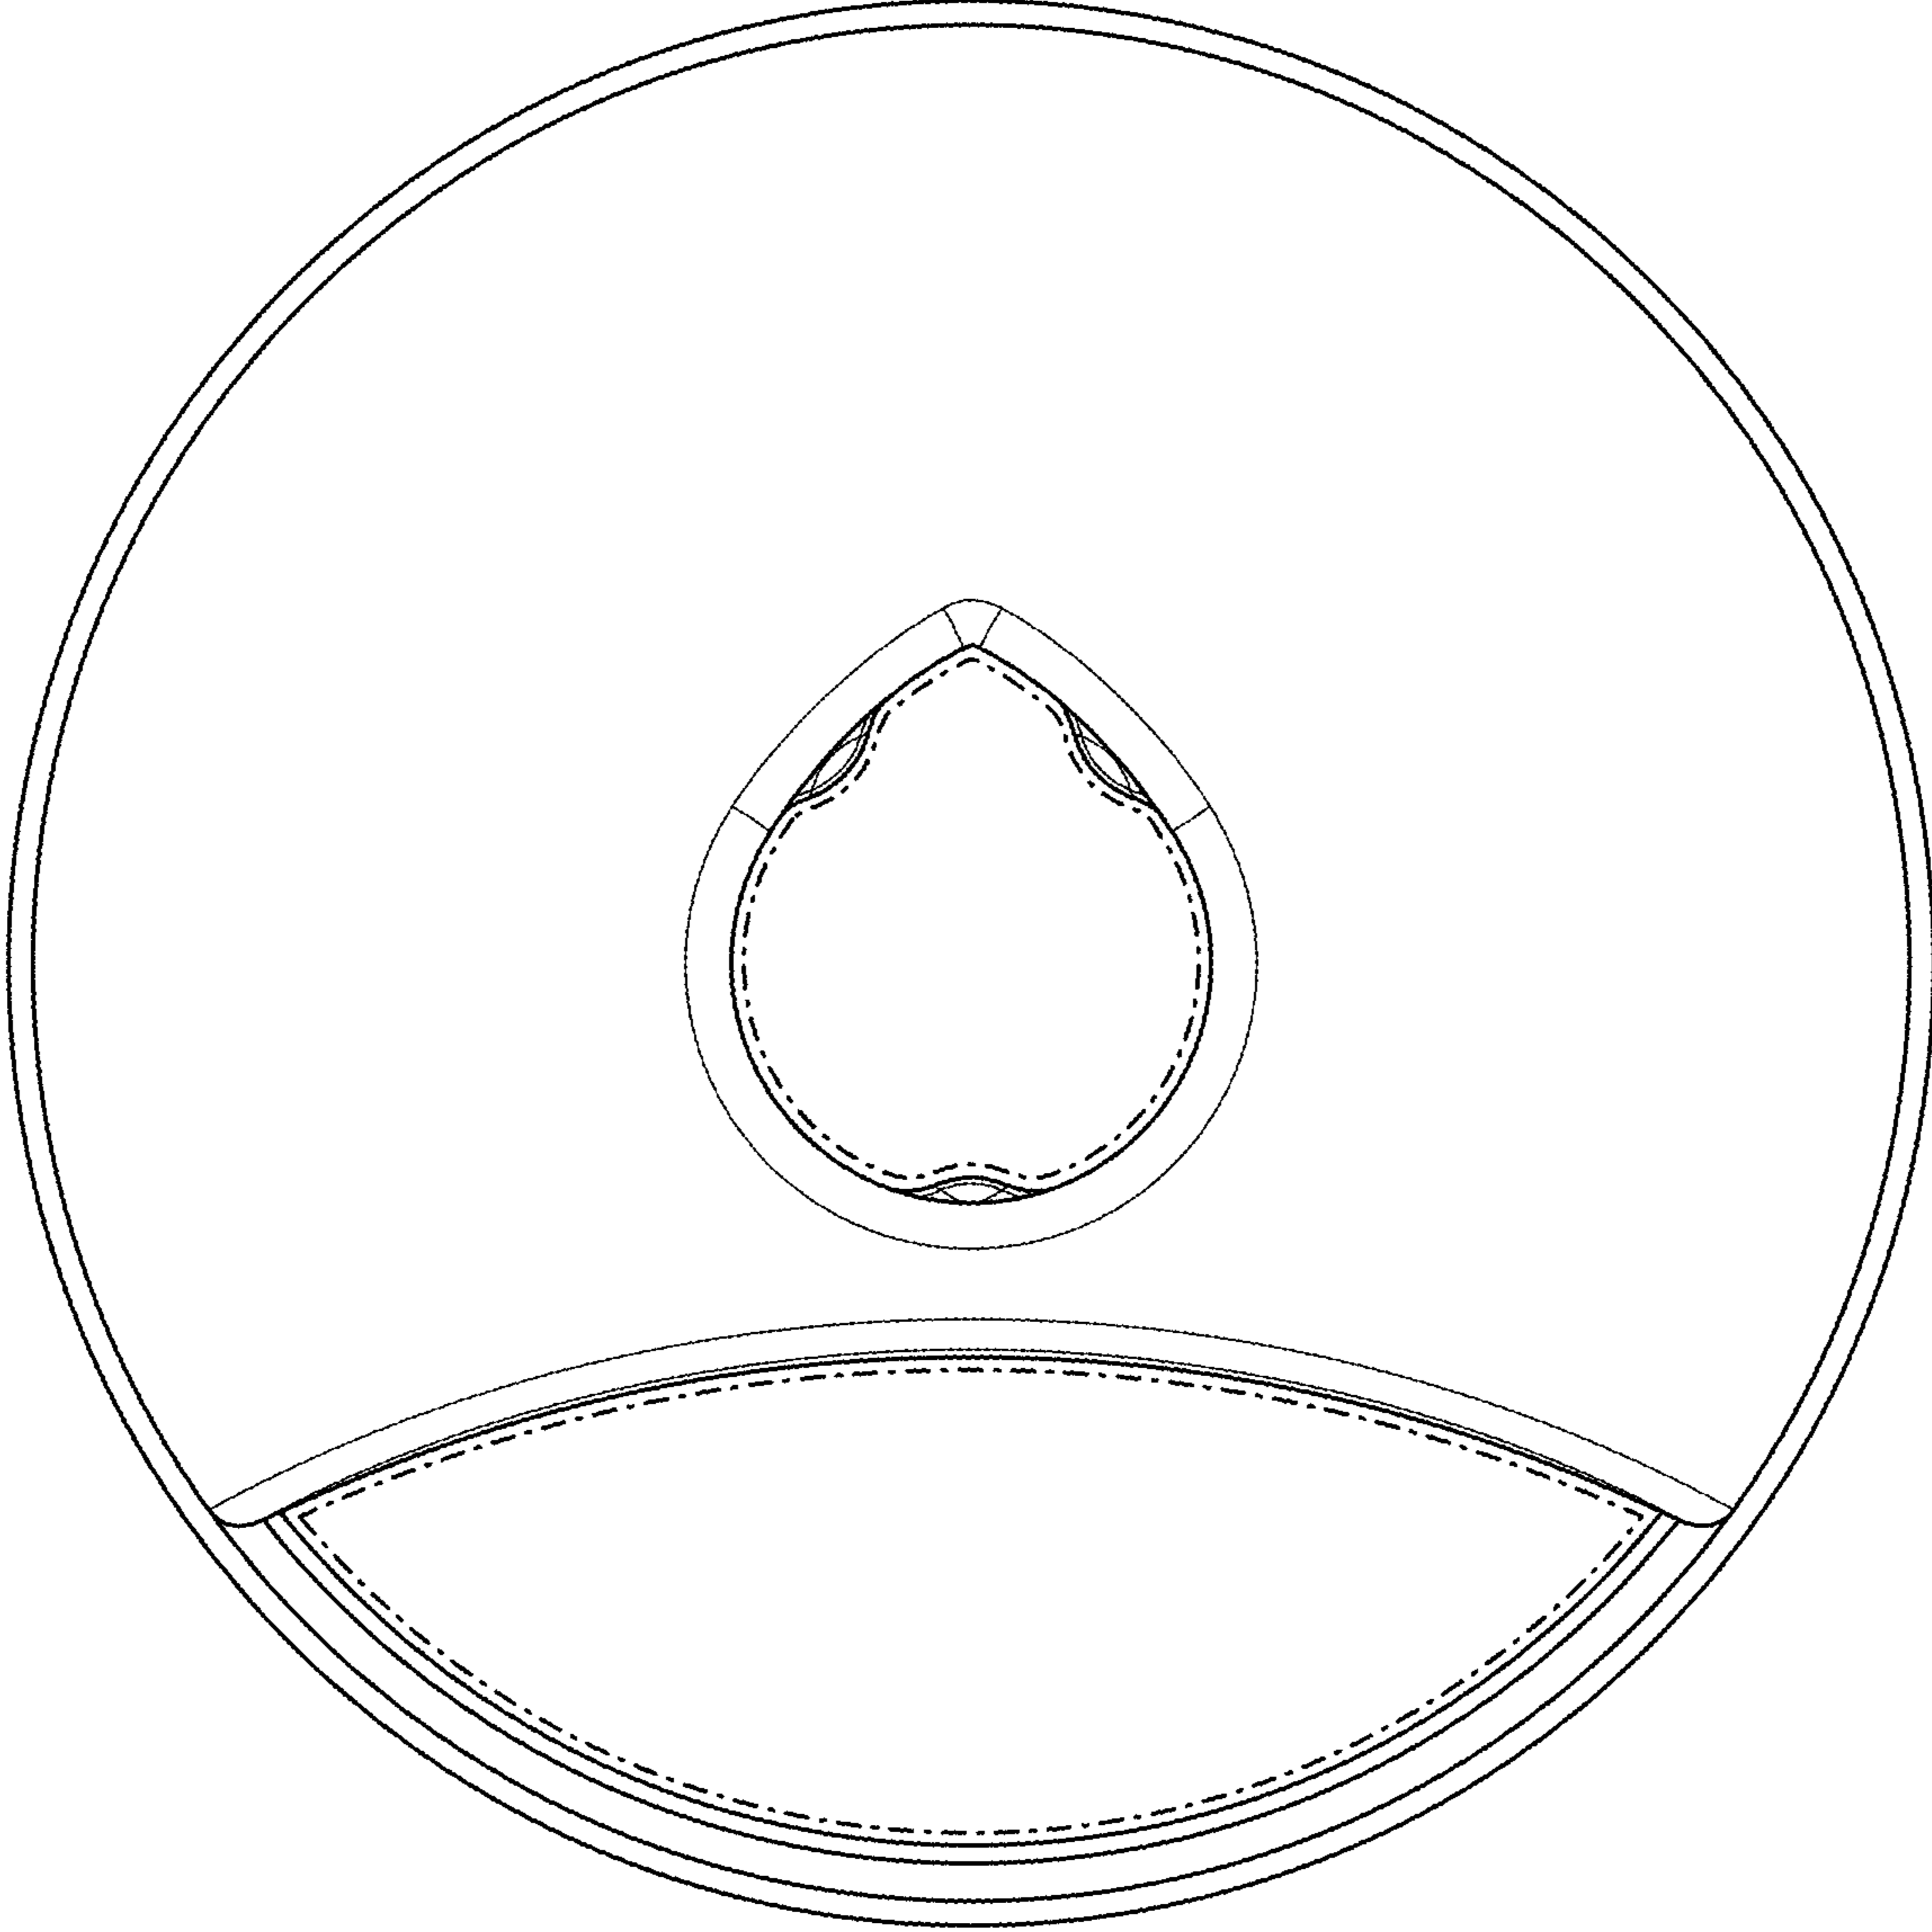


FIG. 6

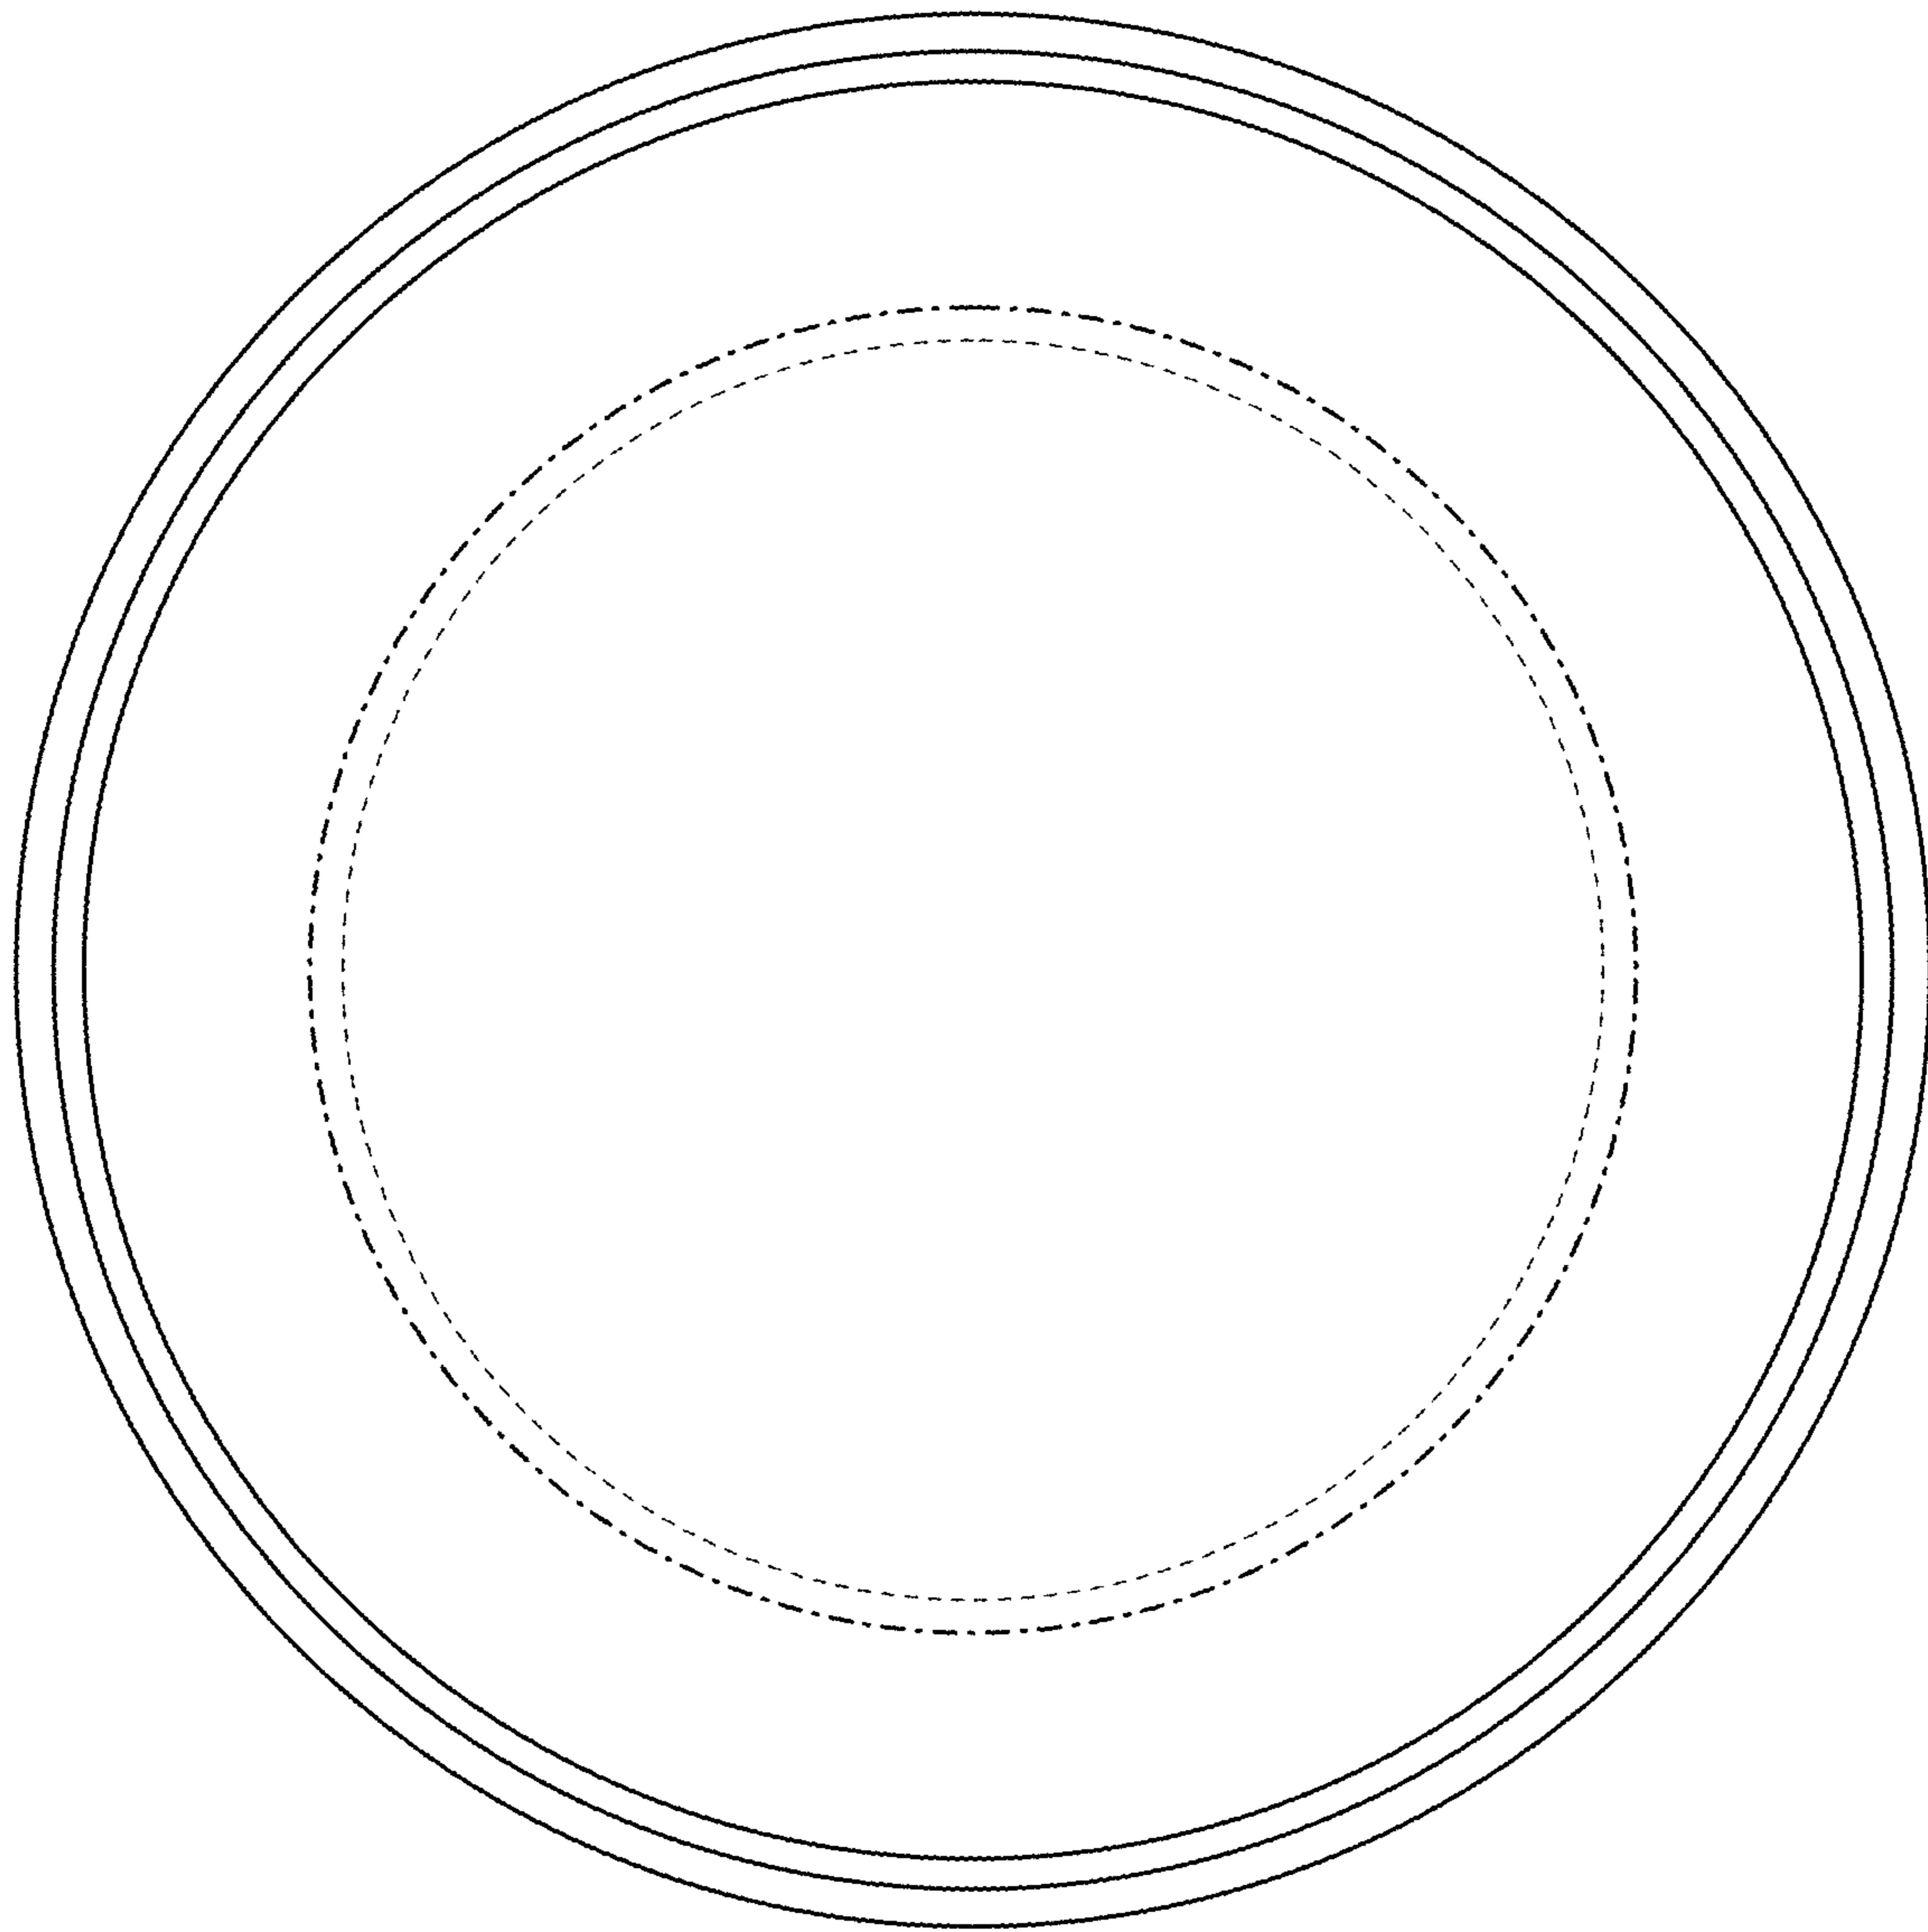


FIG. 7