



US00D923789S

(12) **United States Design Patent** (10) **Patent No.:** **US D923,789 S**
Imori (45) **Date of Patent:** **** Jun. 29, 2021**

(54) **PUNCTURE NEEDLE CARTRIDGE FOR BLOOD COLLECTING DEVICE**

(71) Applicant: **ASAHI POLYSLIDER COMPANY, LIMITED**, Osaka (JP)

(72) Inventor: **Hirokazu Imori**, Okayama (JP)

(73) Assignee: **ASAHI POLYSLIDER COMPANY, LIMITED**, Osaka (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/665,436**

(22) Filed: **Oct. 3, 2018**

(30) **Foreign Application Priority Data**

May 31, 2018 (JP) JP2018-012008

(51) **LOC (13) Cl.** **24-04**

(52) **U.S. Cl.**
USPC **D24/147**; D24/112; D24/121; D24/146

(58) **Field of Classification Search**
USPC D24/133, 128, 135, 155, 159, 183, 184,
D24/190, 121, 127, 129, 130, 131, 112,
D24/113, 114, 186; D8/71, 74, 321, 380,
D8/382, 349, 394, 499
CPC A61M 25/065; A61M 25/0612; A61M
25/00; A61M 25/0043; A61M 25/0067;
A61M 25/0097; A61M 5/42; A61M
39/00; A61M 27/00; A61F 2/958
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,358,689 A * 12/1967 Higgins A61B 5/150564
606/181
D264,378 S * 5/1982 Thomas D24/147
D351,652 S * 10/1994 Thompson D24/112
D371,195 S * 6/1996 Krebs D24/112
D376,649 S * 12/1996 Kim D24/146

D439,657 S * 3/2001 Bridle D24/113
D442,105 S * 5/2001 Lloyd D10/113.1
D445,183 S * 7/2001 McWethy D24/130
D447,566 S * 9/2001 Levaughn D24/146
D471,976 S * 3/2003 Pavlu D24/112
D499,182 S * 11/2004 Moore D24/146
D532,517 S * 11/2006 Wilkinson D24/146

(Continued)

FOREIGN PATENT DOCUMENTS

CN 303980517 * 12/2016

OTHER PUBLICATIONS

OneTouch Delica Plus Lancing Device, [site visited Apr. 20, 2021].
Available from Internet. URL: <https://www.youtube.com/watch?v=m6w2BwgAwjk> (Year: 2019).*

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) *Attorney, Agent, or Firm* — Wenderoth, Lind &
Ponack, L.L.P.



(57) **CLAIM**

The ornamental design for a puncture needle cartridge for blood collecting device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a puncture needle cartridge for blood collecting device showing my new design;
FIG. 2 is a front elevational view thereof, a rear elevational view being a mirror image thereof;
FIG. 3 is a left side view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a top plan view thereof; and,
FIG. 6 is a bottom plan view thereof.
The broken lines in the figures show portions of the puncture needle cartridge for blood collecting device that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

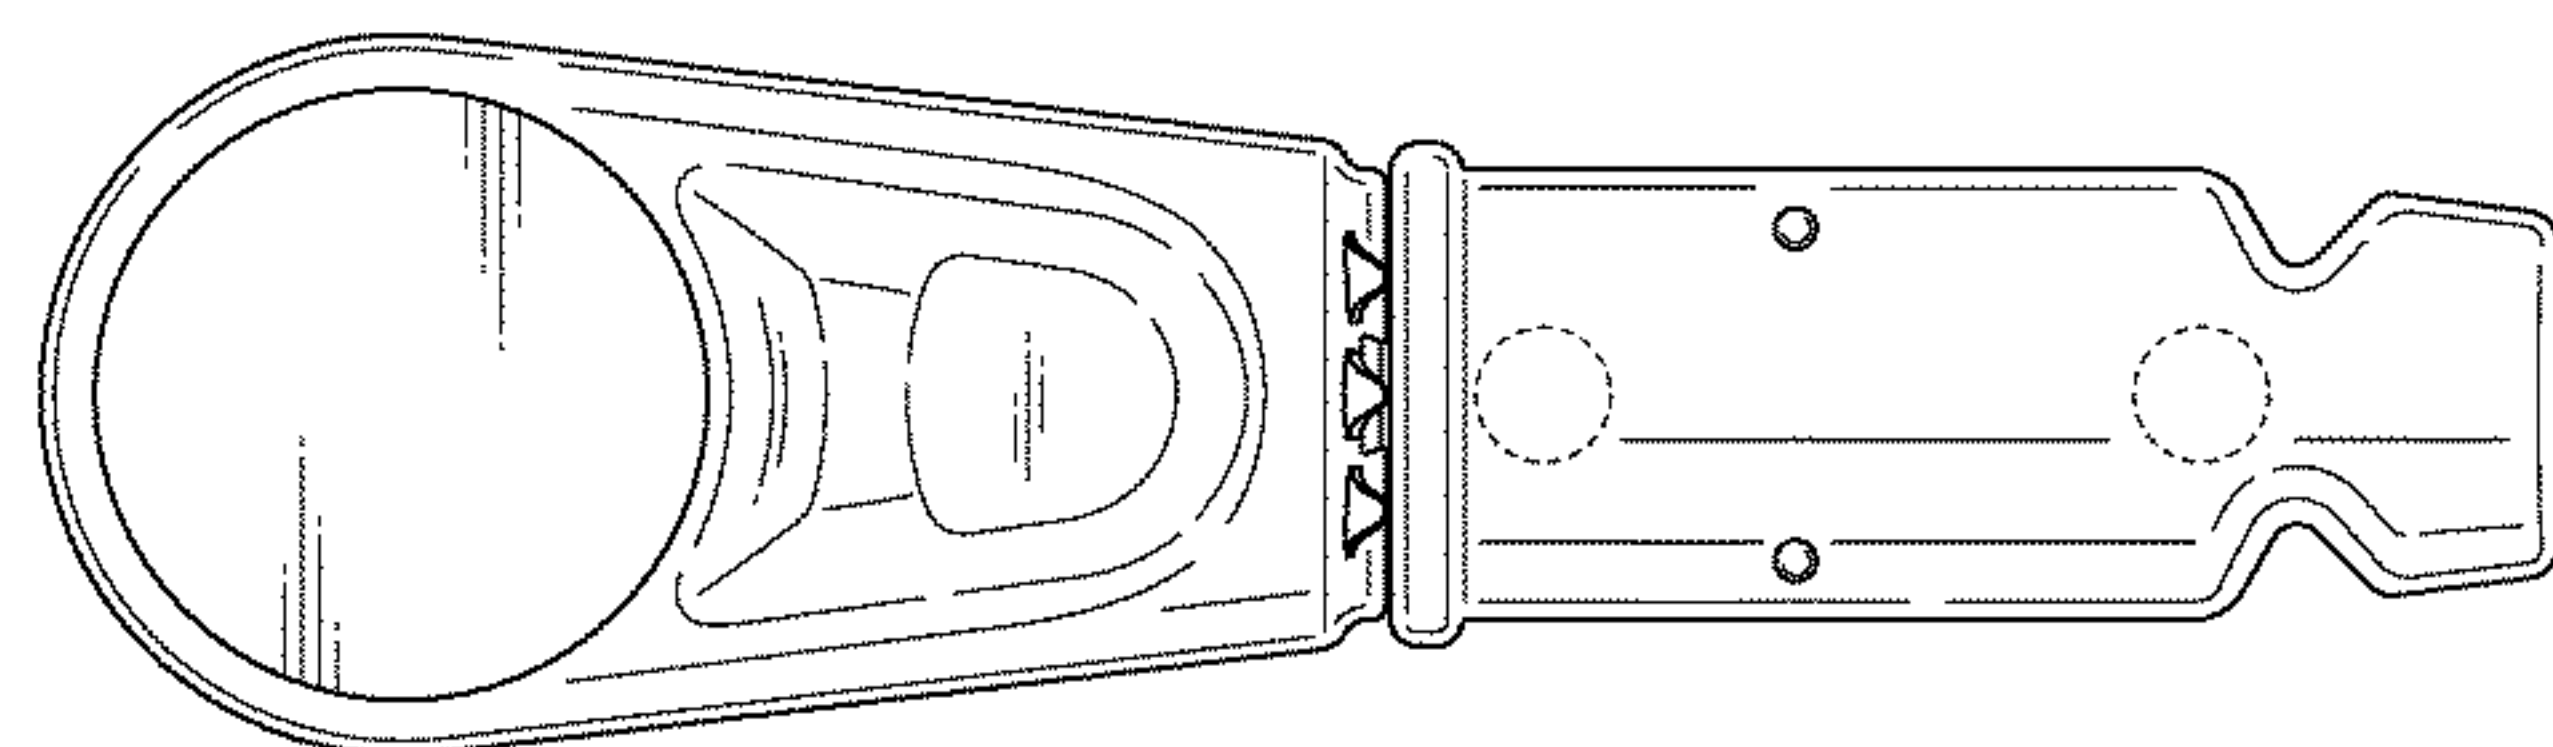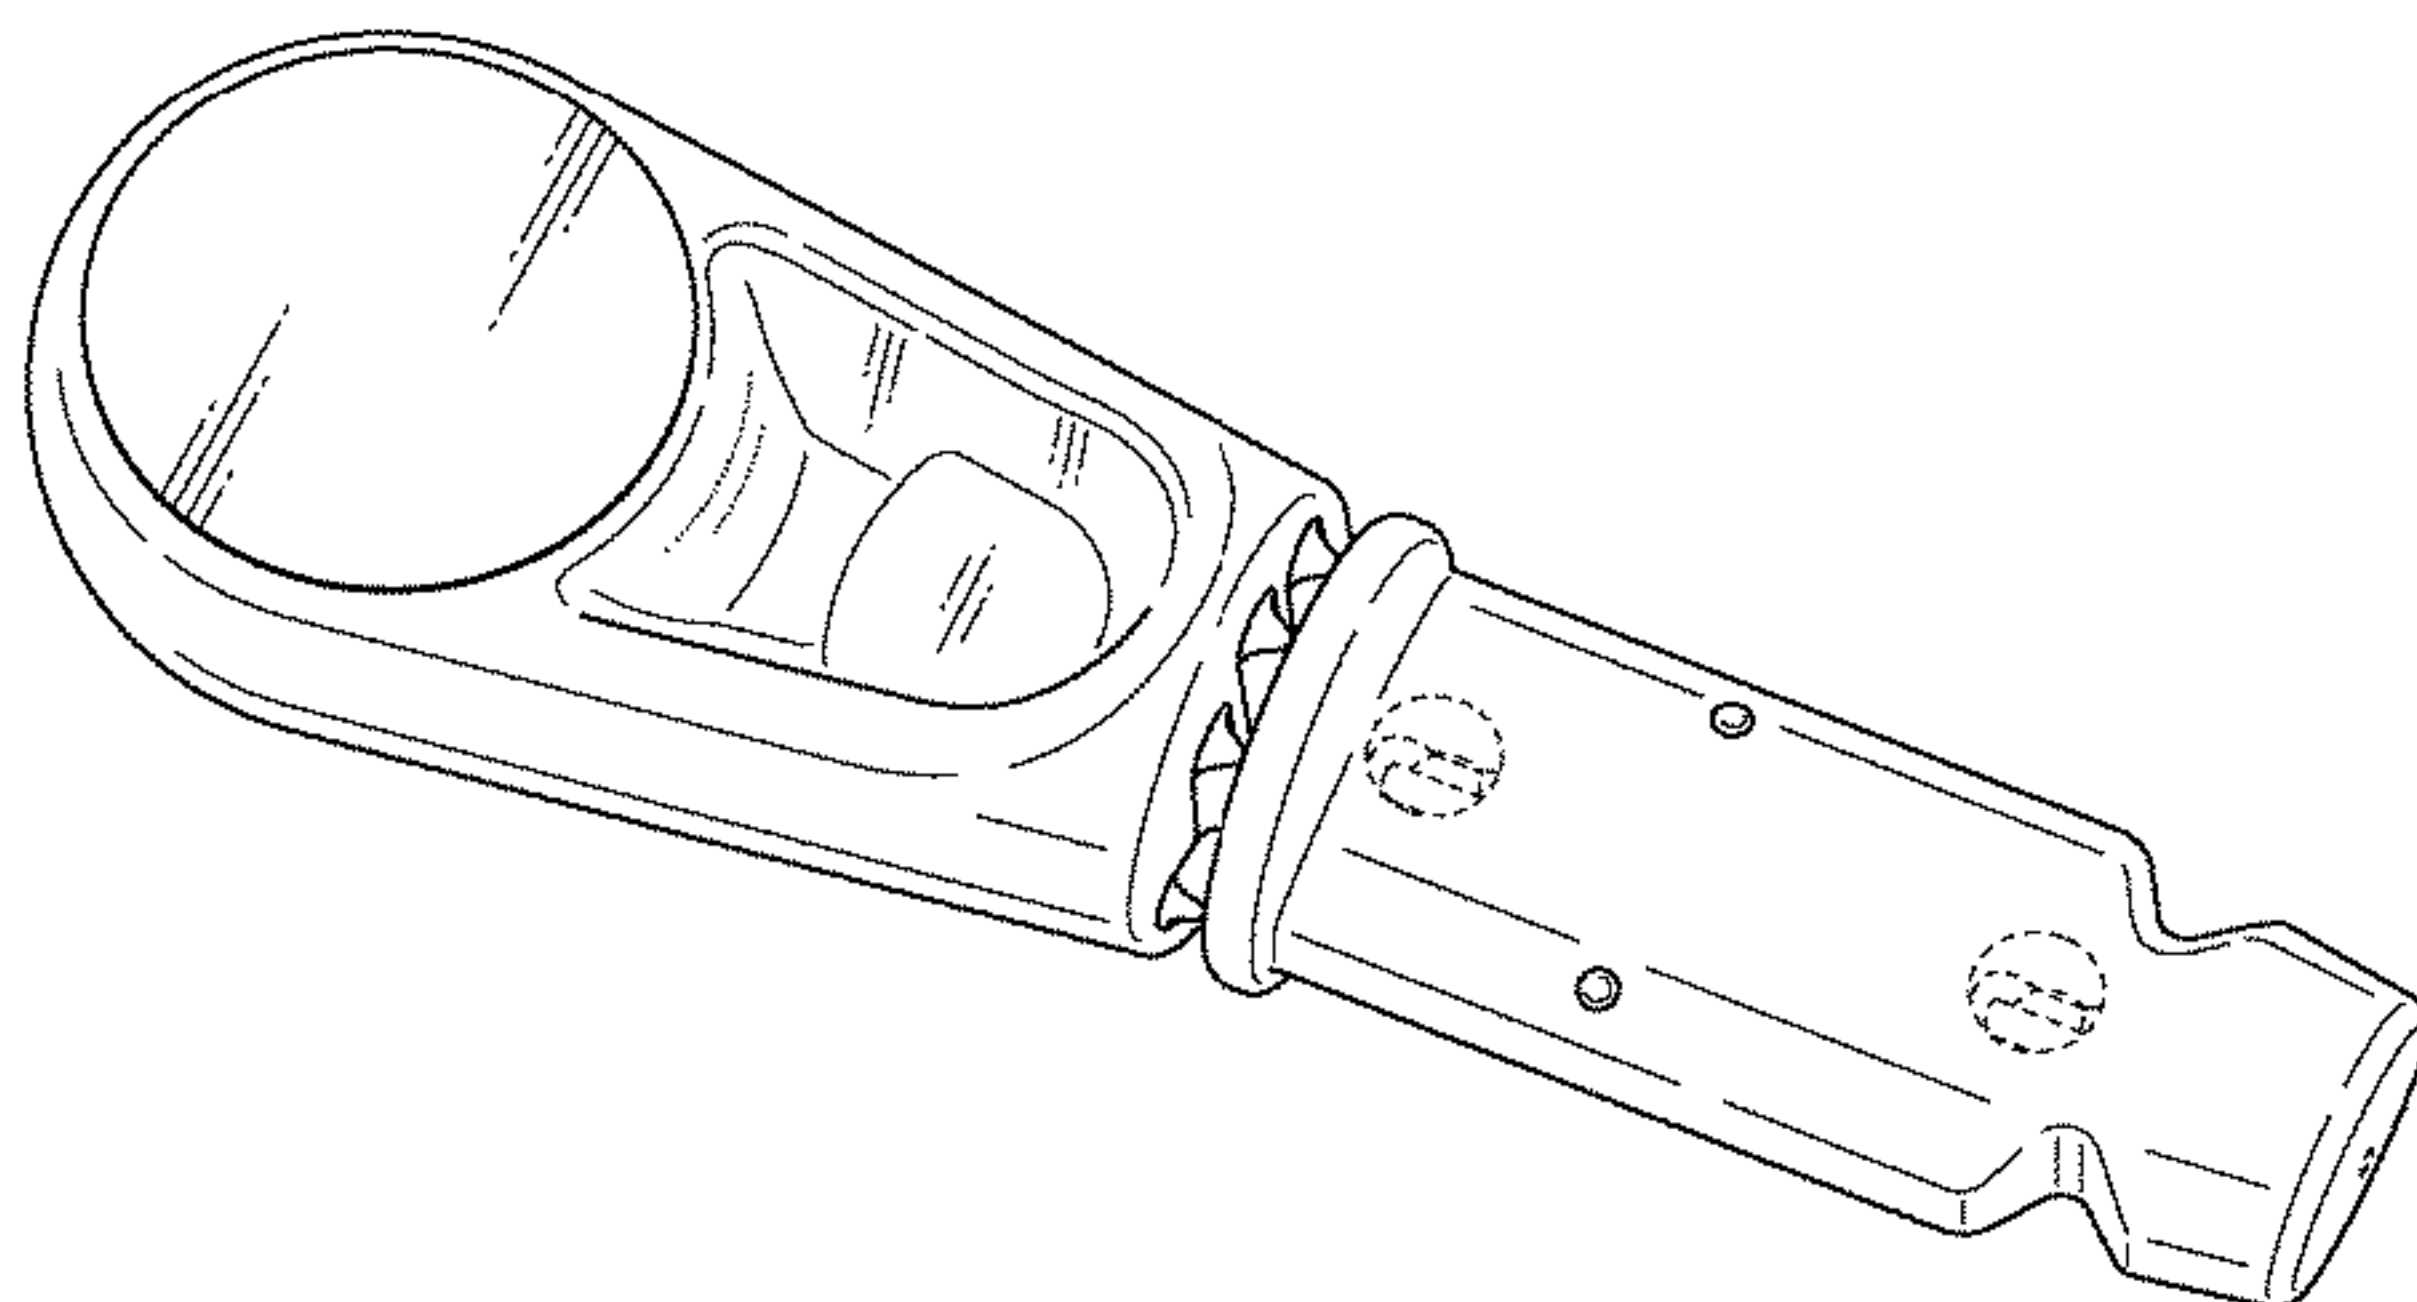

(56)

References Cited

U.S. PATENT DOCUMENTS

D538,934 S * 3/2007 Wilkinson A61B 5/150022
D24/146
D567,944 S * 4/2008 Sarna D24/146
D569,517 S * 5/2008 Wilkinson D24/146
D569,975 S * 5/2008 Wilkinson D24/146
D611,594 S * 3/2010 Ratjen D24/115
D612,051 S * 3/2010 Ruf A61B 5/150564
D24/146
D612,487 S * 3/2010 Hunter D24/114
D616,987 S * 6/2010 Brown D24/146
D621,042 S * 8/2010 Ruf D24/146
D621,044 S 8/2010 Trissel et al.
D621,045 S 8/2010 Trissel et al.
D628,293 S * 11/2010 Ruf D24/146
D628,695 S * 12/2010 Ruf D24/146
D639,421 S * 6/2011 Sano D24/118
D645,147 S * 9/2011 Ruf D24/147
D645,148 S * 9/2011 Ruf D24/147
D651,713 S * 1/2012 Shi D24/147
8,133,246 B1 * 3/2012 Starnes A61B 5/15144
606/182
D673,678 S * 1/2013 Hong D24/146
D673,679 S * 1/2013 Hong D24/146
D681,807 S * 5/2013 Niedbala D24/113
D686,724 S * 7/2013 Au D24/108
D687,320 S * 8/2013 Lee D9/723
D695,398 S * 12/2013 Solomon D24/129
D701,571 S * 3/2014 Perkins D19/163
D726,902 S * 4/2015 McLoughlin D24/113
D745,675 S * 12/2015 Jankowski D24/146
D746,457 S * 12/2015 Swick D24/146
D746,458 S * 12/2015 Imori D24/147
D749,225 S * 2/2016 Chang D24/188
D749,724 S * 2/2016 Shi D24/130
D757,267 S * 5/2016 Shi D24/147
D759,243 S * 6/2016 Molenschot D24/141
D759,303 S * 6/2016 Afridi D27/163
D768,851 S * 10/2016 Rozwadowski D24/130
D768,852 S * 10/2016 Rozwadowski D24/130
D769,443 S * 10/2016 Held D24/113
D777,918 S * 1/2017 Karbowniczek D24/146
D785,782 S * 5/2017 Chen D24/112
D785,783 S * 5/2017 Chen D24/112
D788,927 S * 6/2017 Yao D24/176
D794,790 S * 8/2017 Shi D24/146
D795,426 S * 8/2017 Shi D24/146
D799,111 S * 10/2017 Qiu D27/101

D799,743 S * 10/2017 Qiu D27/101
D808,010 S * 1/2018 Denzer D24/113
D814,019 S * 3/2018 Crosby D24/110
D817,331 S * 5/2018 Volta D14/431
D817,961 S * 5/2018 Han D14/426
D818,575 S * 5/2018 Corbin D24/113
D818,593 S * 5/2018 Kile D24/176
D819,201 S * 5/2018 Denzer D24/127
D819,262 S * 5/2018 Lin D27/101
D827,131 S * 8/2018 Hayamizu D24/129
D829,212 S * 9/2018 Bidwell D14/426
D829,890 S * 10/2018 Denzer D24/113
D838,360 S * 1/2019 Protasiewicz D24/113
D843,567 S * 3/2019 Gloria Bello D24/129
D858,753 S * 9/2019 Yosef D24/113
D864,378 S * 10/2019 Tafazoli D24/112
D865,871 S * 11/2019 Fernandez-Katz D21/333
D868,244 S * 11/2019 Cox D24/112
D875,948 S * 2/2020 Pieroni D24/176
D879,908 S * 3/2020 Nelson D22/113
D879,950 S * 3/2020 Imori D24/112
D882,072 S * 4/2020 Wills D24/117
D884,879 S * 5/2020 Hanafusa D24/121
D884,919 S * 5/2020 Parsons D24/223
D887,547 S * 6/2020 Wills D24/117
D888,941 S * 6/2020 Scrimgeour D24/113
D895,106 S * 9/2020 Patil D24/113
D898,908 S * 10/2020 Denzer D24/127
D900,309 S * 10/2020 Ono D24/112
D902,391 S * 11/2020 Scrimgeour D24/113
D902,392 S * 11/2020 Scrimgeour D24/113
D903,108 S * 11/2020 Scrimgeour D24/113
D909,204 S * 2/2021 Tempfli D9/448
D910,174 S * 2/2021 Mills D24/141
D910,849 S * 2/2021 Shi D24/146
D913,973 S * 3/2021 Georgiades D13/156
D917,064 S * 4/2021 Ribeiro D24/217
2003/0109895 A1 * 6/2003 Taylor A61B 5/150022
606/181
2012/0123459 A1 * 5/2012 Ruf A61B 5/150259
606/182
2012/0215246 A1 * 8/2012 Hyoue A61B 5/150022
606/182
2013/0158586 A1 * 6/2013 Pusey A61B 5/15117
606/173
2014/0088631 A1 * 3/2014 Saeki A61B 5/150435
606/181
2015/0313513 A1 * 11/2015 Marshall A61B 5/150465
606/182

* cited by examiner

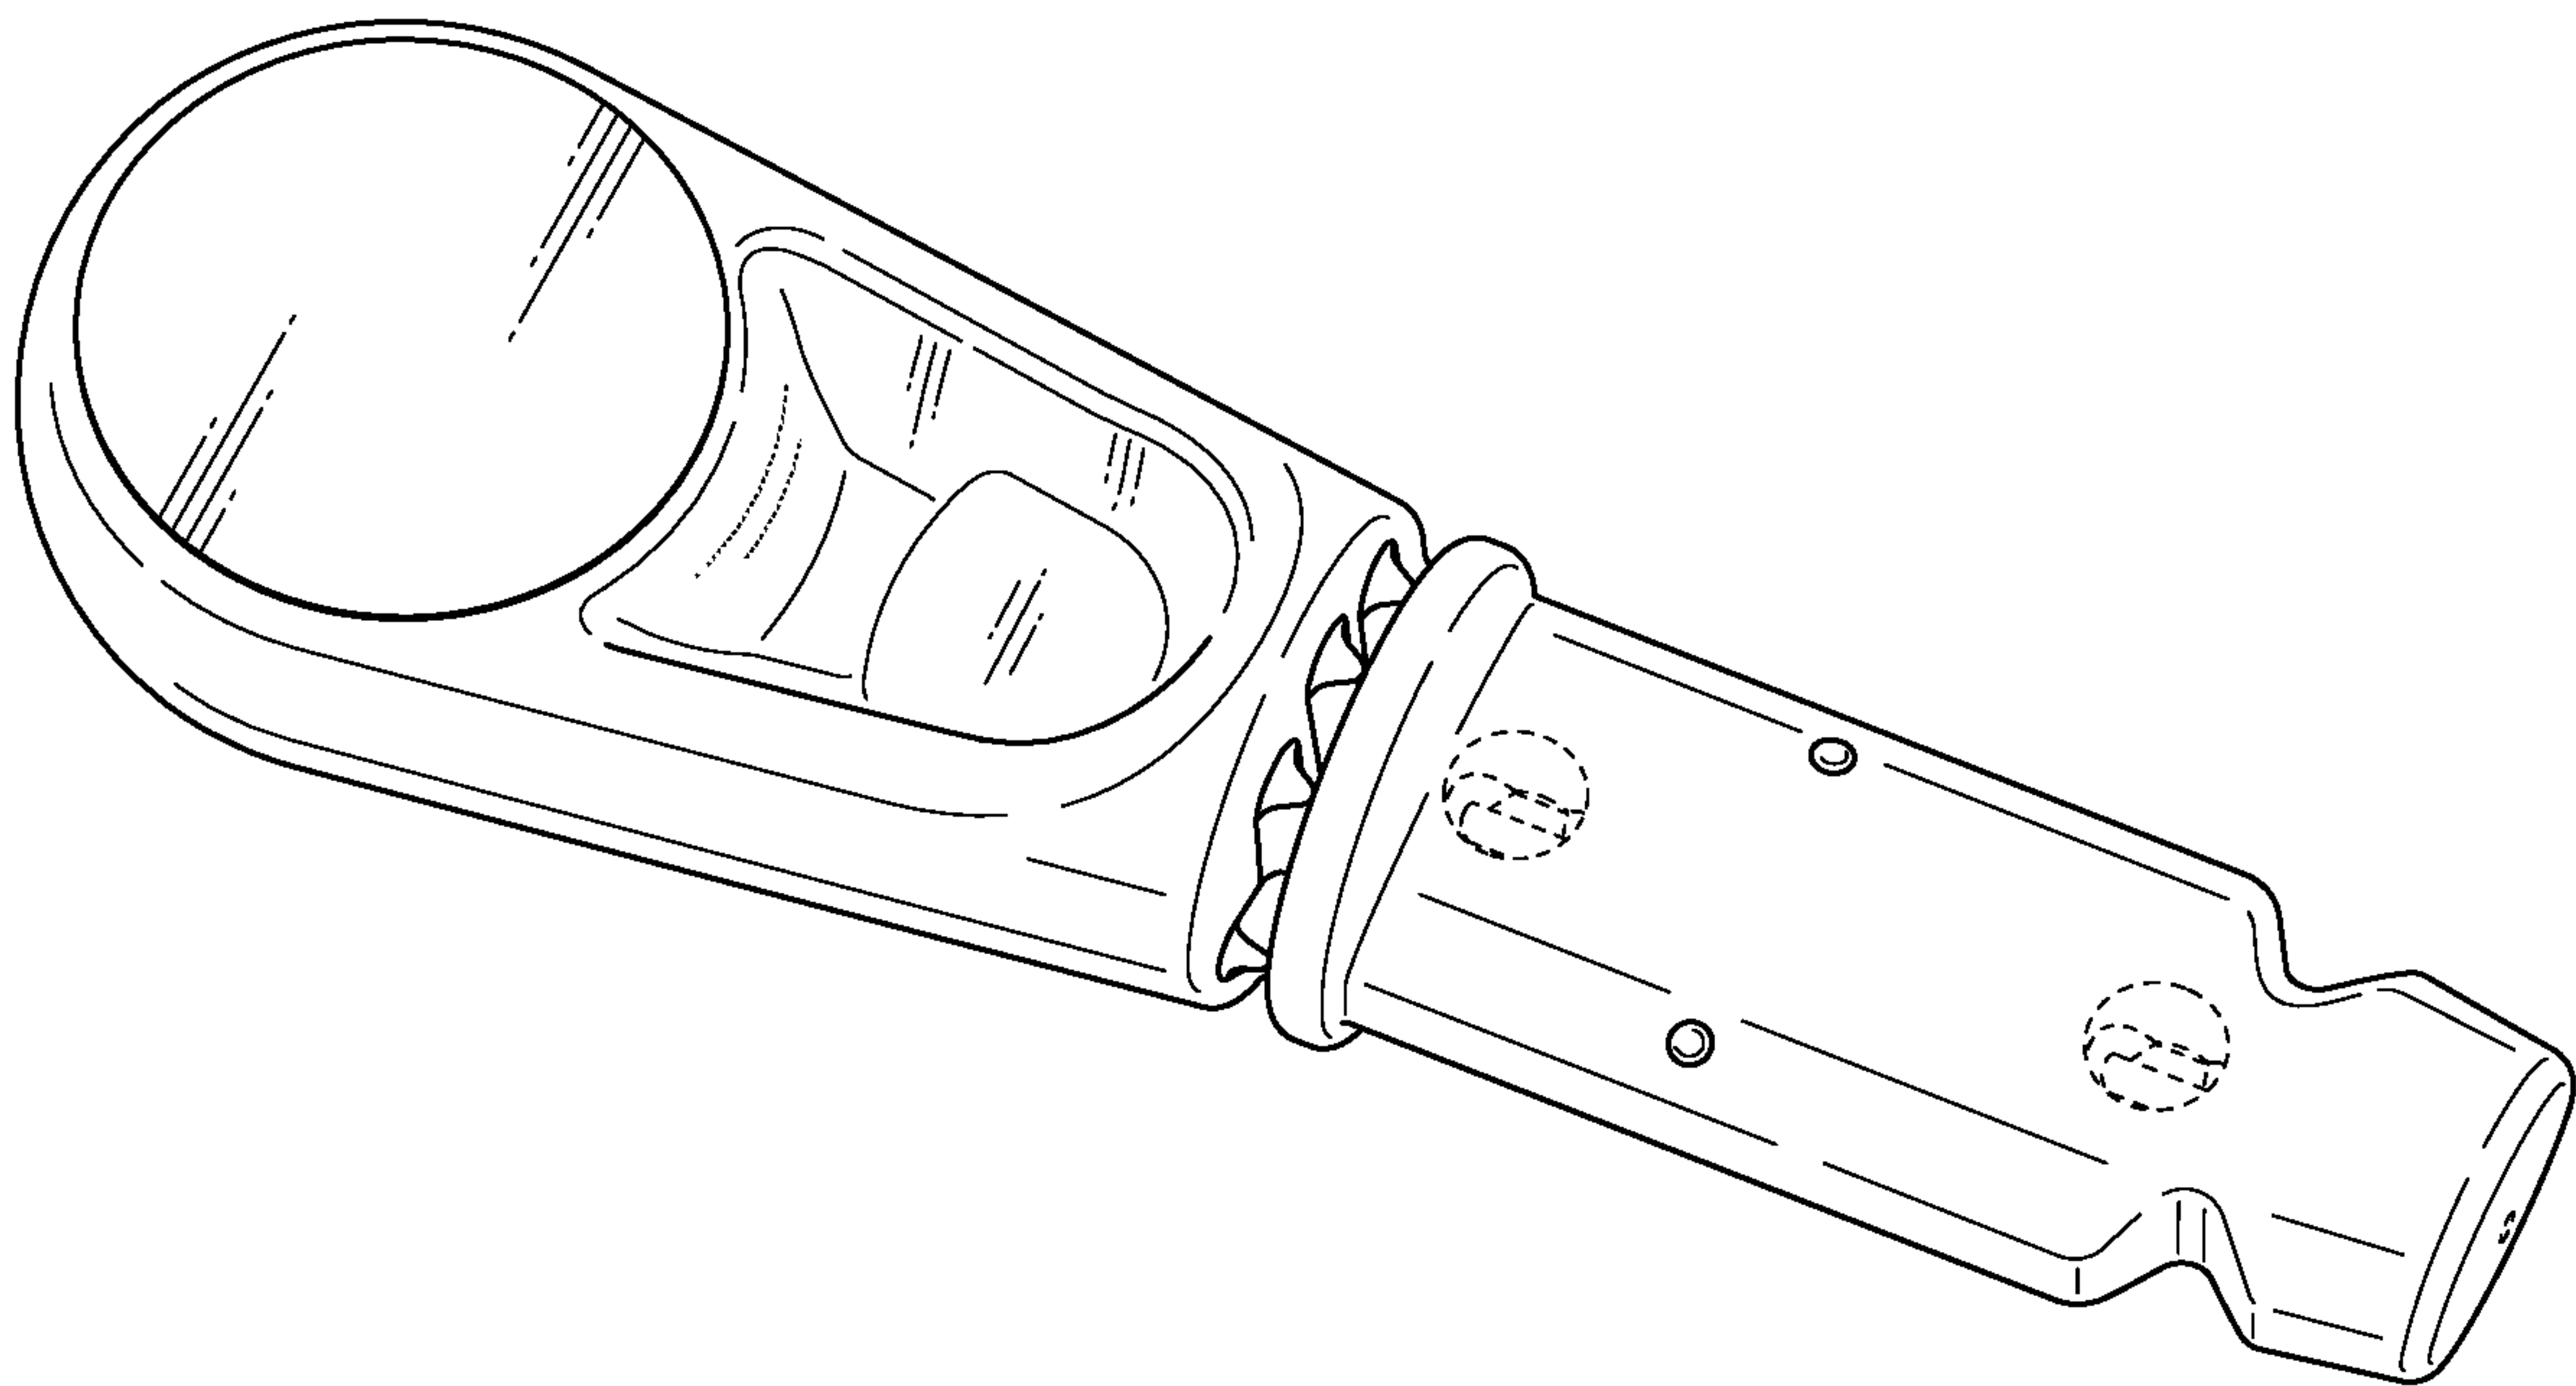


FIG. 1

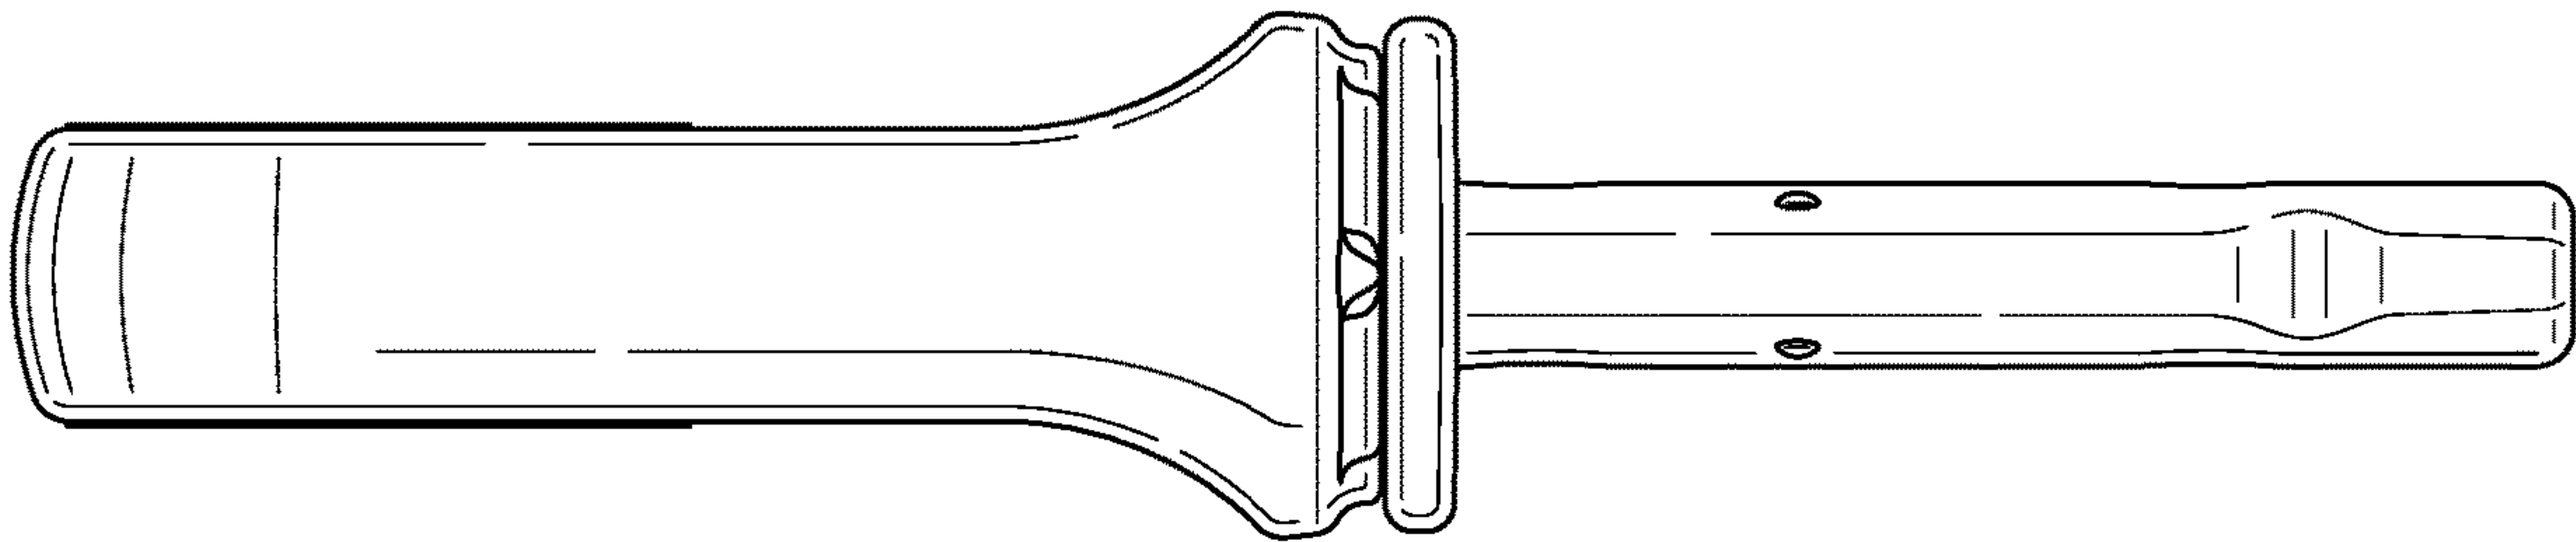


FIG. 2

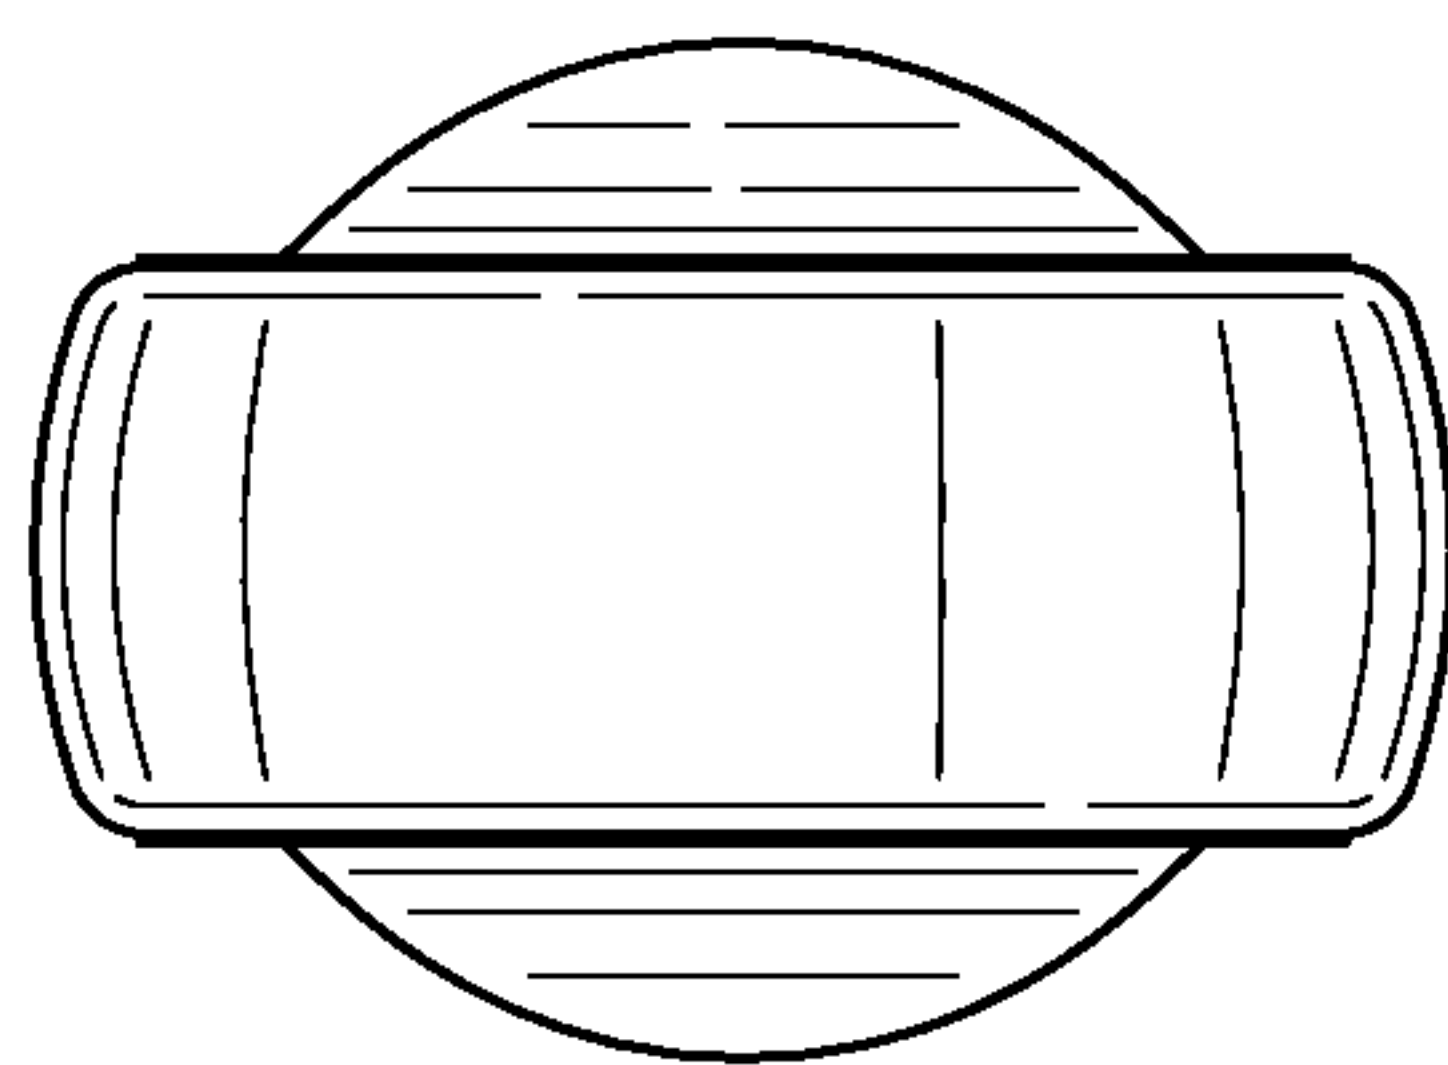


FIG. 3

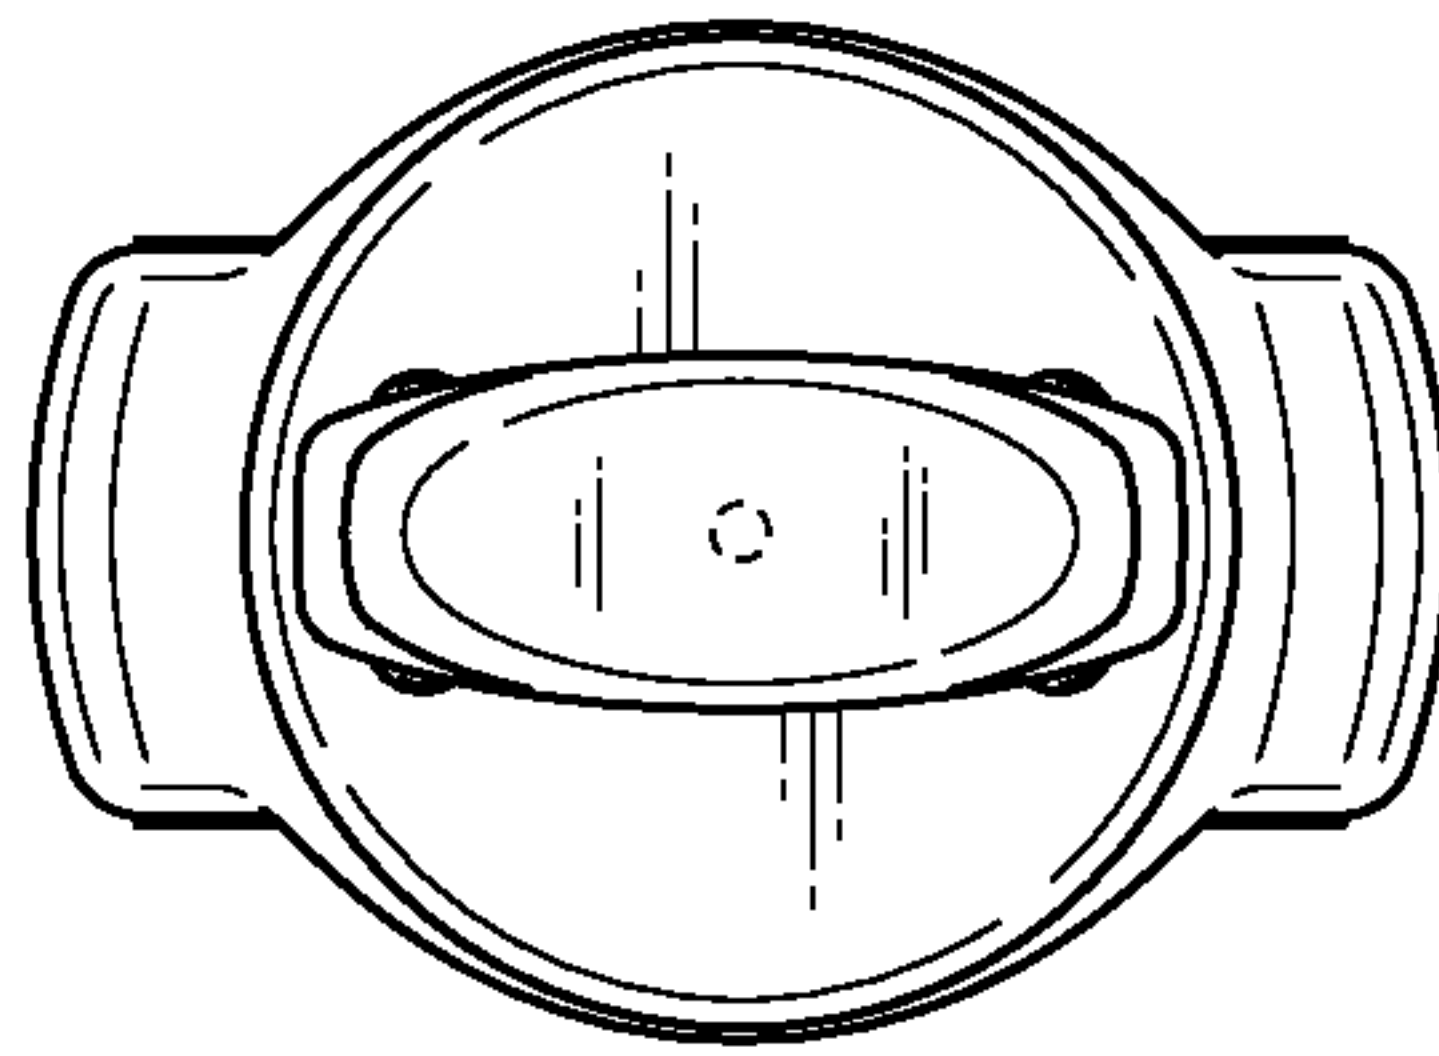


FIG. 4

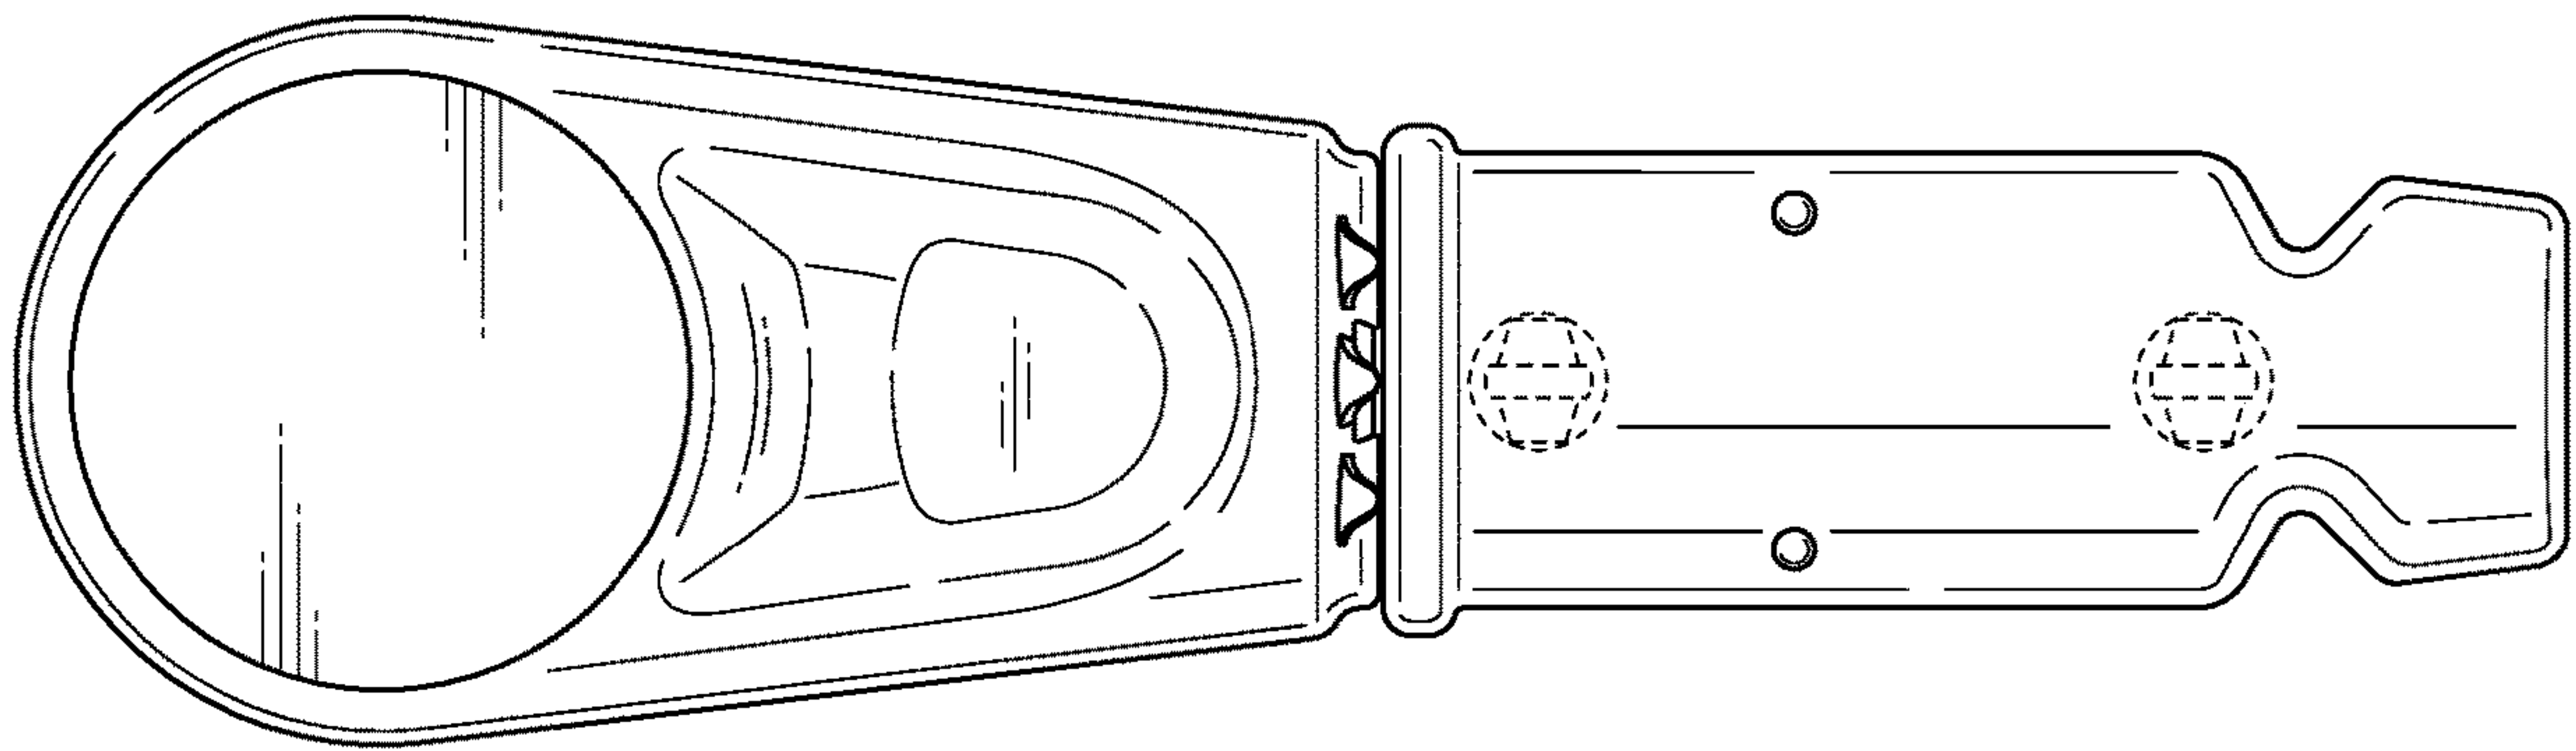


FIG. 5

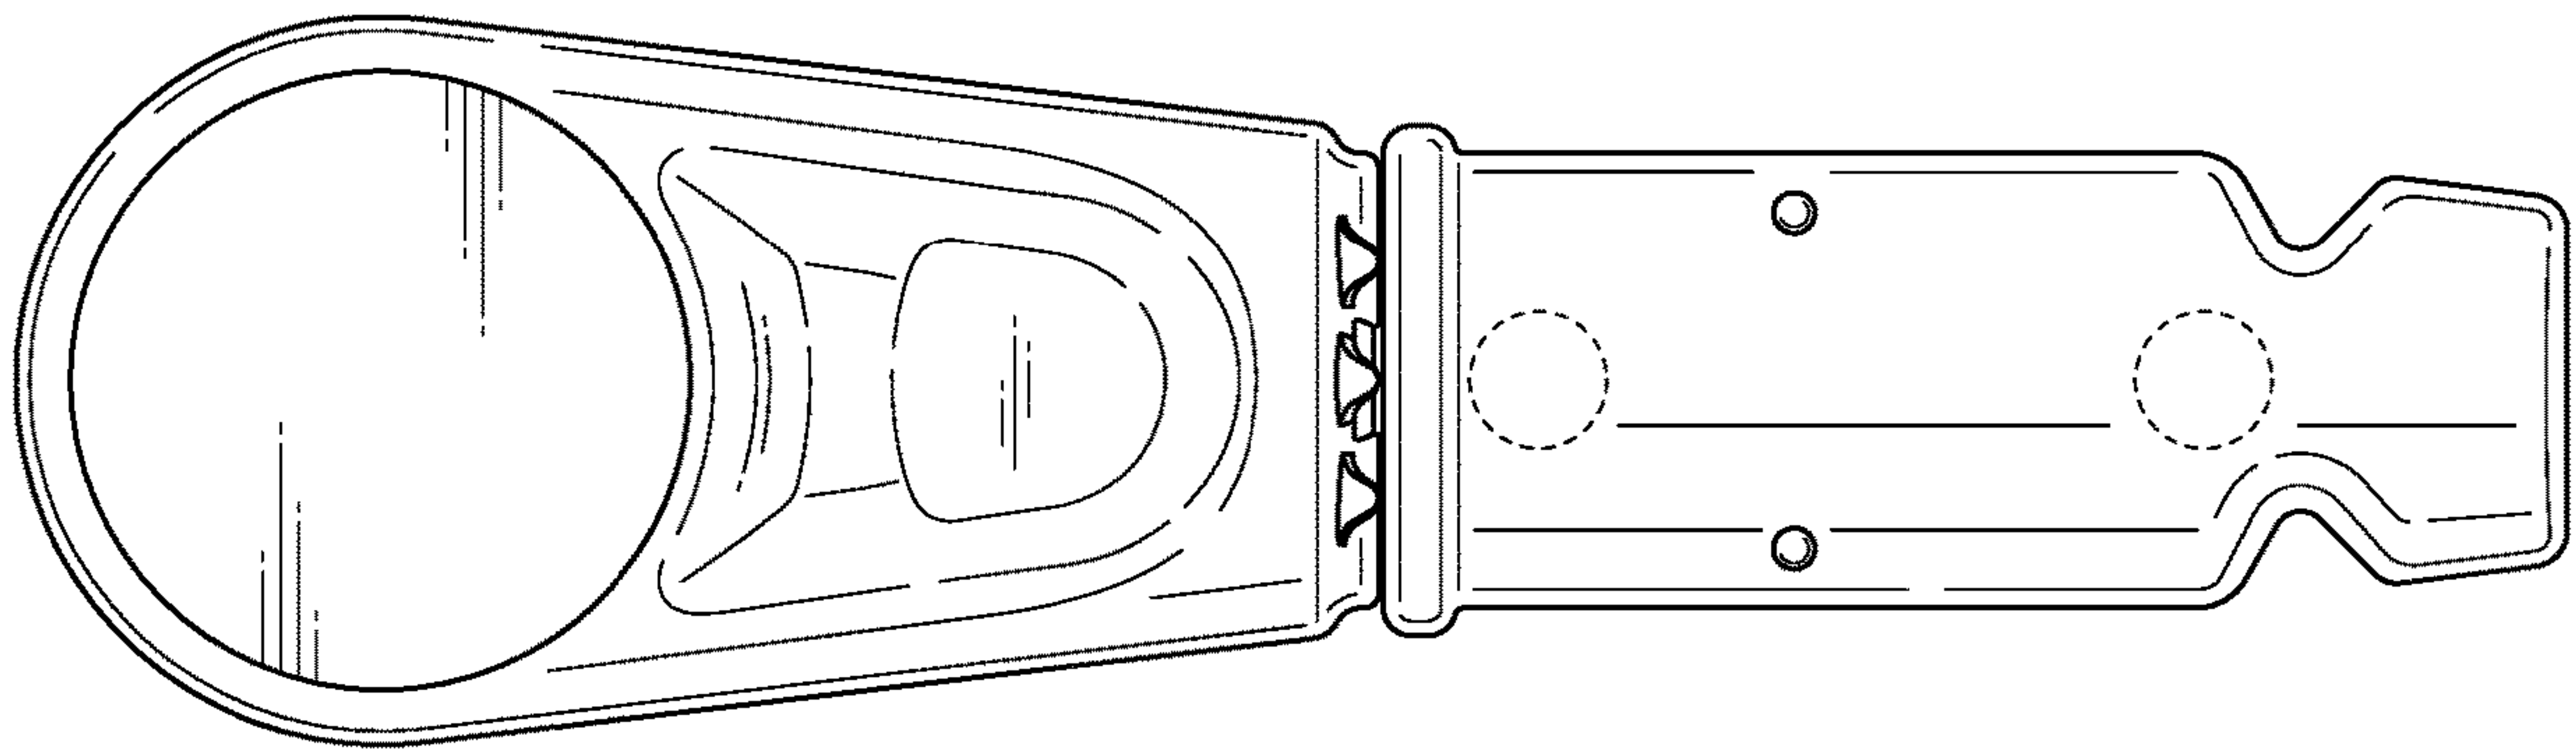


FIG. 6