



US00D926224S

(12) **United States Design Patent**
Hummel

(10) **Patent No.:** **US D926,224 S**
(45) **Date of Patent:** **** Jul. 27, 2021**

- (54) **LABORATORY DEVICE DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**
- (71) Applicant: **BRAND GMBH + CO KG**, Wertheim (DE)
- (72) Inventor: **Ursula Hummel**, Aschaffenburg (DE)
- (73) Assignee: **BRAND GMBH + CO KG**, Wertheim (DE)

6,841,129	B2	1/2005	Braun et al.	
D711,413	S *	8/2014	Yu	D14/486
8,871,157	B2	10/2014	Homberg et al.	
D721,385	S *	1/2015	Barling	D14/488
D722,324	S *	2/2015	Florence	D14/488
D745,887	S *	12/2015	Lee	D14/489
D747,728	S *	1/2016	Capela	D14/485
D759,707	S *	6/2016	You	D14/488
D762,726	S *	8/2016	Lee	D14/492
D768,158	S *	10/2016	Lee	D14/486
D769,312	S *	10/2016	Chen	D14/488
D771,661	S	11/2016	Gruner	

(Continued)

(**) Term: **15 Years**

(21) Appl. No.: **29/687,160**

(22) Filed: **Apr. 11, 2019**

(30) **Foreign Application Priority Data**

Oct. 11, 2018 (EM) 005796471

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/492**

(58) **Field of Classification Search**
 USPC D14/485-495; D20/11; D21/324, 325
 CPC G06F 1/1626; G06F 3/048; G06F 3/0481;
 G06F 3/04817; G06F 3/0482; G06F
 3/0483; G06F 3/04842; G06F 3/0485;
 G06F 3/04855; G06F 3/0486; G06F
 3/0488; G06F 3/04886; G06F 9/4443;
 G06F 17/211; G06F 17/212; G01N
 30/8651; H04L 41/22; A61B 5/14532;
 H04W 4/50; B01L 3/0227; B01L 3/0237;
 B01L 2300/027; B01L 3/0286

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,058,764	A *	5/2000	Yamada	G01N 30/8651
				422/70
6,540,964	B2	4/2003	Kohrmann et al.	
6,740,295	B2	5/2004	Braun et al.	

FOREIGN PATENT DOCUMENTS

EP 0691158 A2 1/1996

OTHER PUBLICATIONS

Hutchison, Danillellem "Titration animation" Dec. 4, 2013, posted at youtube.com, [site visited Jun. 1, 2021], <https://www.youtube.com/watch?v=sYZ-TVeYBcY> (Year: 2013).*

(Continued)

Primary Examiner — John M Otte

(74) *Attorney, Agent, or Firm* — David S. Safran; Roberts Calderon Safran & Cole, P.C.


(57) **CLAIM**

The ornamental design for a laboratory device display screen with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 shows a laboratory device display screen showing the first image in a sequence; and, FIG. 2 shows a second image thereof. The appearance of the transitional image sequentially transitions between the images shown in FIGS. 1 and 2. The process or period in which one image transitions to another image forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

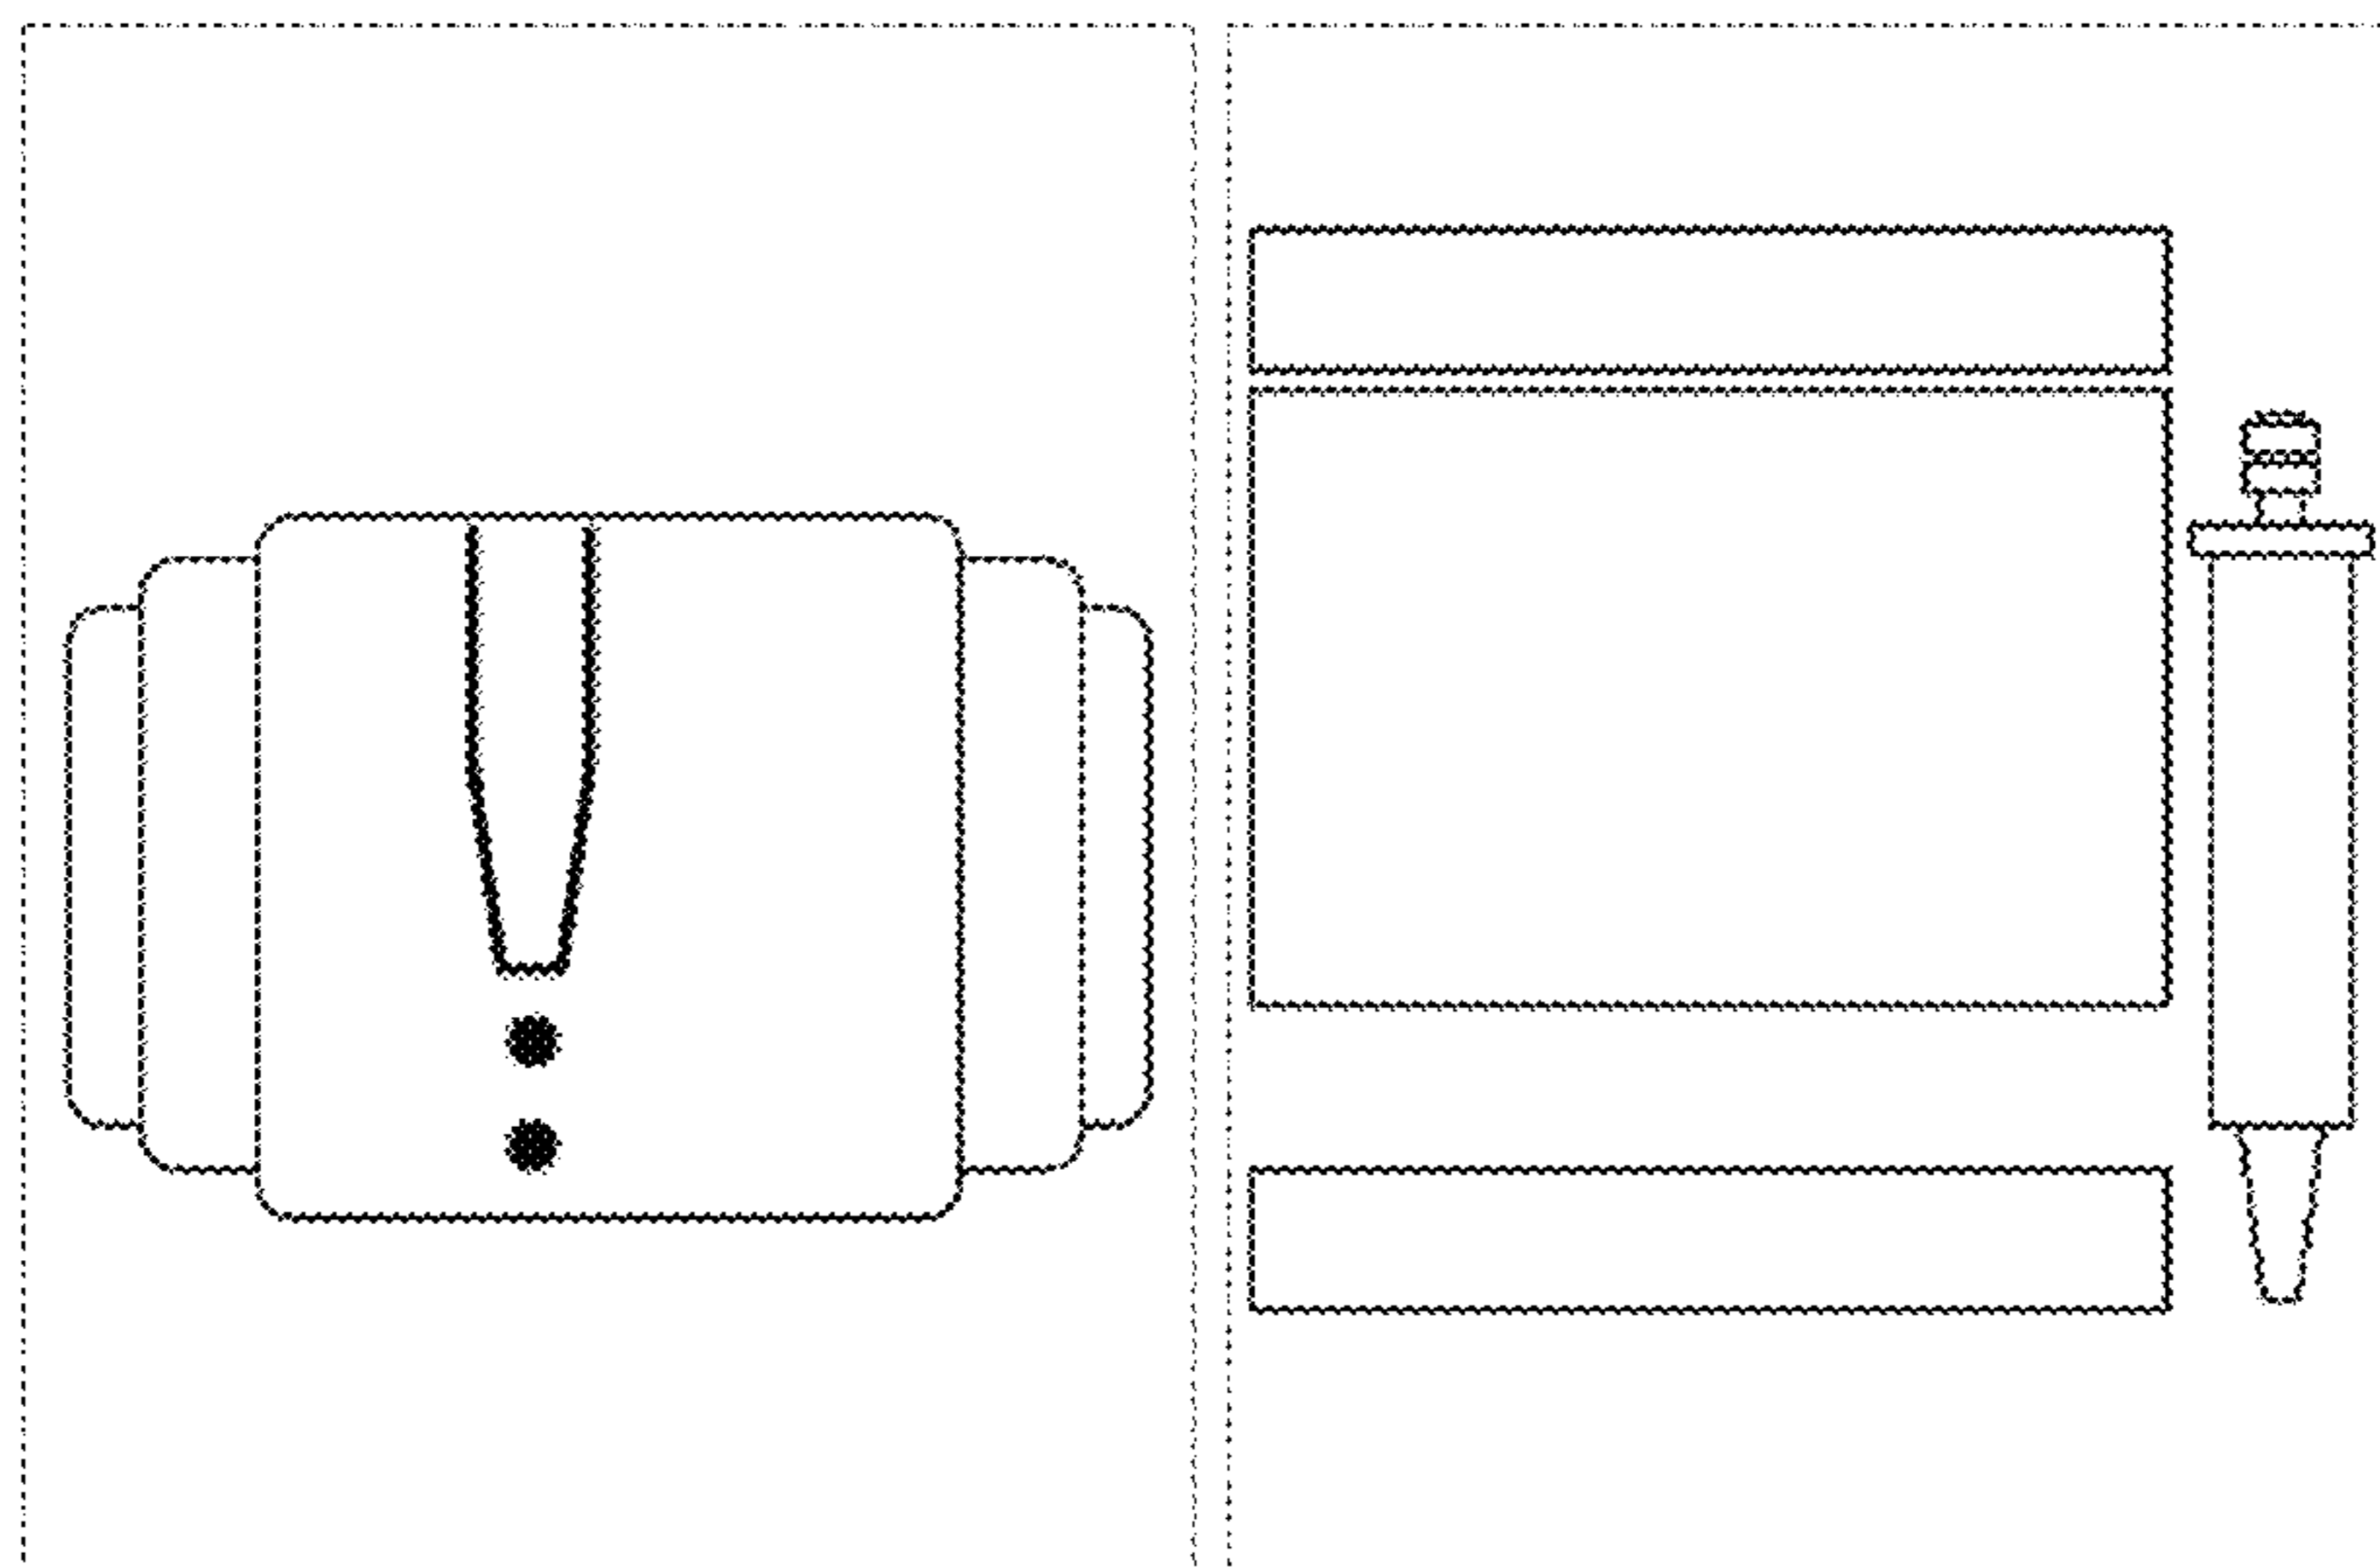

(56)

References Cited

U.S. PATENT DOCUMENTS

D791,831 S * 7/2017 Capela D14/493
 D802,003 S * 11/2017 Jeon D14/486
 D803,887 S * 11/2017 Dart D14/493
 D806,121 S * 12/2017 Jewitt D14/491
 D826,963 S * 8/2018 Guan D14/486
 D831,698 S * 10/2018 Fornoff D14/492
 D836,661 S * 12/2018 Sakata D14/486
 D878,391 S * 3/2020 Zeng D14/485
 D881,234 S * 4/2020 Capela D14/492
 2005/0137653 A1* 6/2005 Friedman H04L 41/22
 607/60
 2008/0011042 A1* 1/2008 Molitor B01L 3/0227
 73/1.74
 2009/0074622 A1* 3/2009 Kalamakis G06F 1/1626
 422/400
 2012/0245447 A1* 9/2012 Karan A61B 5/14532
 600/365

2013/0172707 A1* 7/2013 Galley H04W 4/50
 600/365
 2015/0013476 A1* 1/2015 Telimaa B01L 3/0286
 73/864.16
 2016/0364091 A1* 12/2016 Bernstein G06F 3/03545

OTHER PUBLICATIONS

“Biomedicine icons set” Sep. 27, 2018, posted at shutterstock.com, [site visited Jun. 1, 2021]. <https://www.shutterstock.com/da/image-vector/biomedicine-icons-set-cartoon-9-vector-1179148120> (Year: 2018).
 Operating Instructions: “E4 XLS+ Electronic Pipettes”; 2016; pp. 1-74; Mettler-Toledo Rainin, LLC; USA.
 Product Brochure: “HandyStep® electronic”; Jan. 2019; pp. 1-6; Issue No. 9943 22; Brand GmbH + CO KG; Germany.
 Product Brochure: “Transferpette® electronic”; Mar. 2018; pp. 1-12; Issue No. 9947 31; Brand GMBH + CO KG; Germany.

* cited by examiner

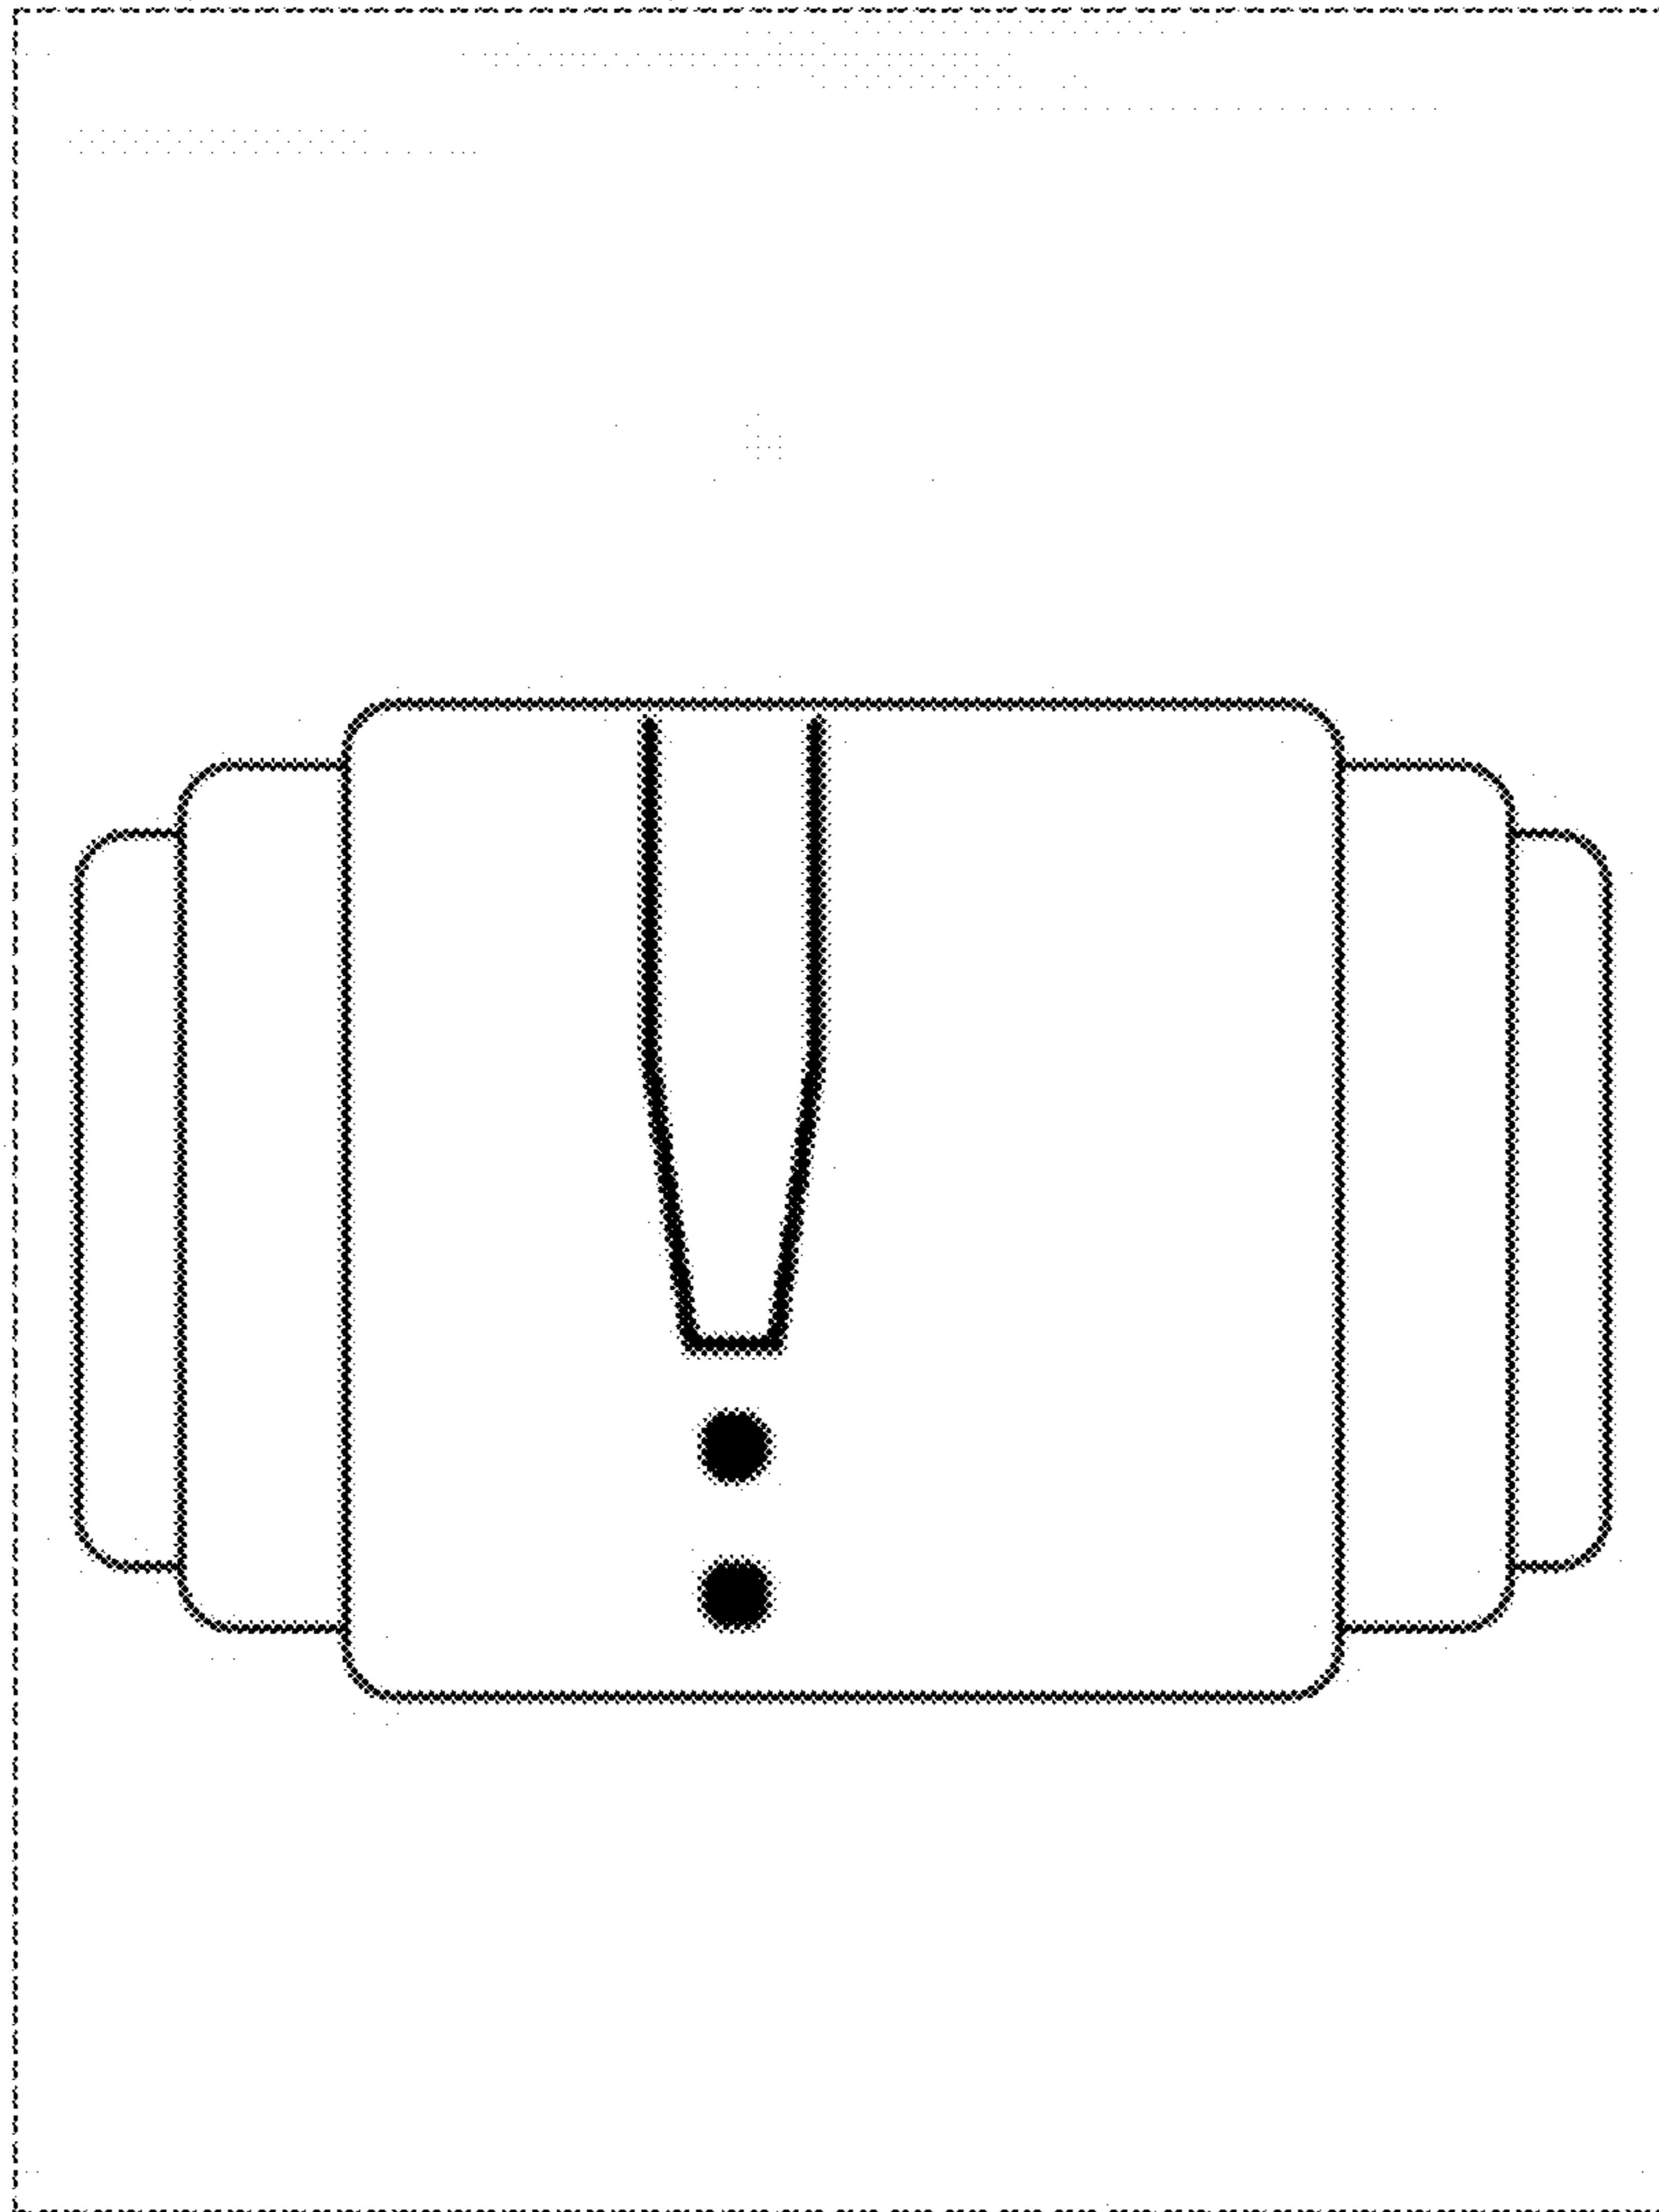


FIG. 1

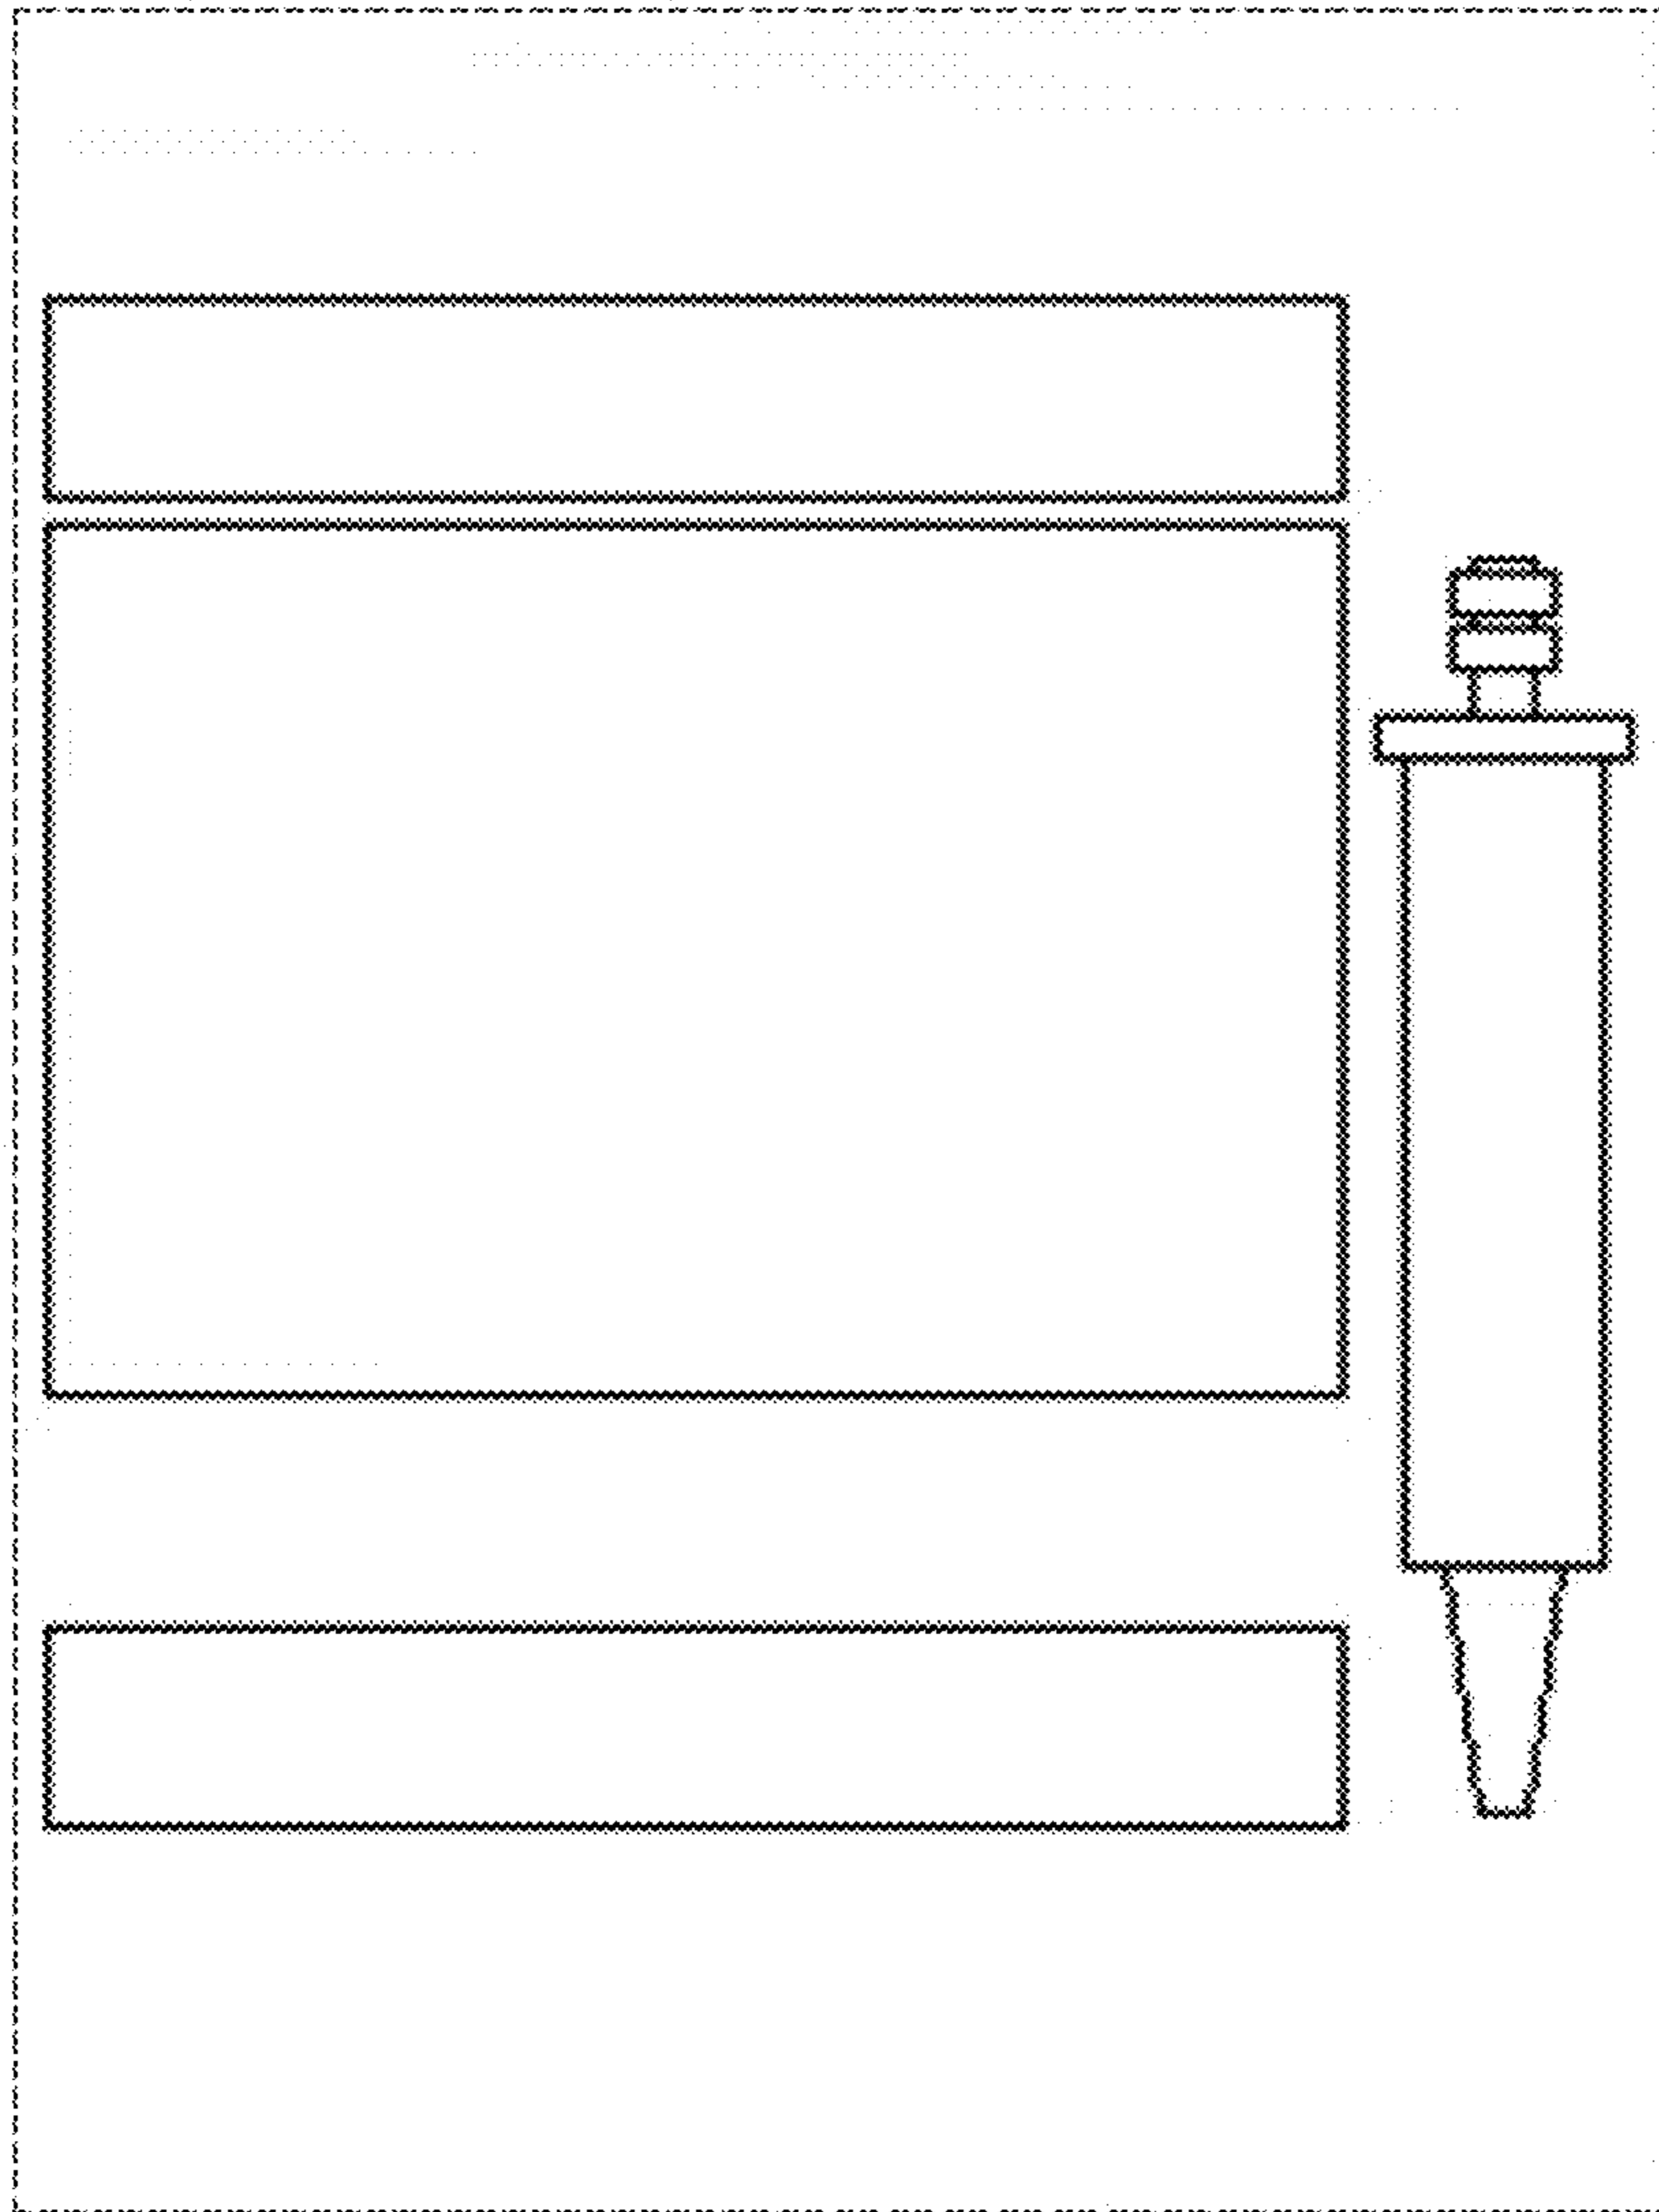


FIG. 2