

US00D926324S

(12) **United States Design Patent** (10) **Patent No.:** **US D926,324 S**
Zhang (45) **Date of Patent:** **** Jul. 27, 2021**

(54) **PULSE OXIMETER**
(71) Applicant: **HUNAN ACCURATE
BIO-MEDICAL TECHNOLOGY
CO., LTD**, Changsha (CN)
(72) Inventor: **Li Zhang**, Changsha (CN)
(73) Assignee: **HUNAN ACCURATE
BIO-MEDICAL TECHNOLOGY
CO., LTD**, Changsha (CN)

D877,339 S * 3/2020 Xian D24/165
D893,727 S * 8/2020 Zhao D24/165
D893,728 S * 8/2020 Zhao D24/165
D894,400 S * 8/2020 Wei D24/169
D895,805 S * 9/2020 Wei D24/169
D903,872 S * 12/2020 Wang D24/169
2010/0030040 A1 * 2/2010 Poeze A61B 5/14532
600/316
2019/0090795 A1 * 3/2019 Boller A61B 5/14552

(**) Term: **15 Years**
(21) Appl. No.: **29/716,240**
(22) Filed: **Dec. 9, 2019**

(30) **Foreign Application Priority Data**

Nov. 1, 2019 (EM) 007158118-0009

(51) **LOC (13) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/169; D24/167**

(58) **Field of Classification Search**
USPC D24/164-169, 107, 186-187; D14/344;
D10/75, 70, 98
CPC A61B 5/0404; A61B 5/021; A61B 5/024;
A61B 5/02438; A61B 5/681; A61B
5/0402; A61B 2560/0462; A61B 5/0205;
A61B 5/02427; A61B 5/14552; A61B
5/6626; A61B 5/6638; G01N 33/66;
G01N 33/49; G01N 33/493
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D621,516 S * 8/2010 Kiani D24/186
D670,388 S * 11/2012 Jin D24/169
D691,726 S * 10/2013 Jin D24/169

OTHER PUBLICATIONS

Fingertip Pulse Oximeter, posted at accbiomed.com, no posting date, retrieved Jan. 8, 2020, online, URL: <http://www.accbiomed.com/FingertipPulseOximeter.html> (Year: 2020).*

* cited by examiner

Primary Examiner — Lilyana Bekic
Assistant Examiner — Mary Shannon Malley


(57) **CLAIM**

The ornamental design for a pulse oximeter, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a pulse oximeter showing my new design;
FIG. 2 is another perspective view thereof;
FIG. 3 is a front elevational view thereof;
FIG. 4 is a rear elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a right side elevational view thereof;
FIG. 7 is a top plan view thereof;
FIG. 8 is a bottom plan view thereof; and,
FIG. 9 is a perspective view of the pulse oximeter where the pulse oximeter is in a configuration of use.
The broken lines in the drawings depict portions of the pulse oximeter that form no part of the claimed design.

1 Claim, 9 Drawing Sheets

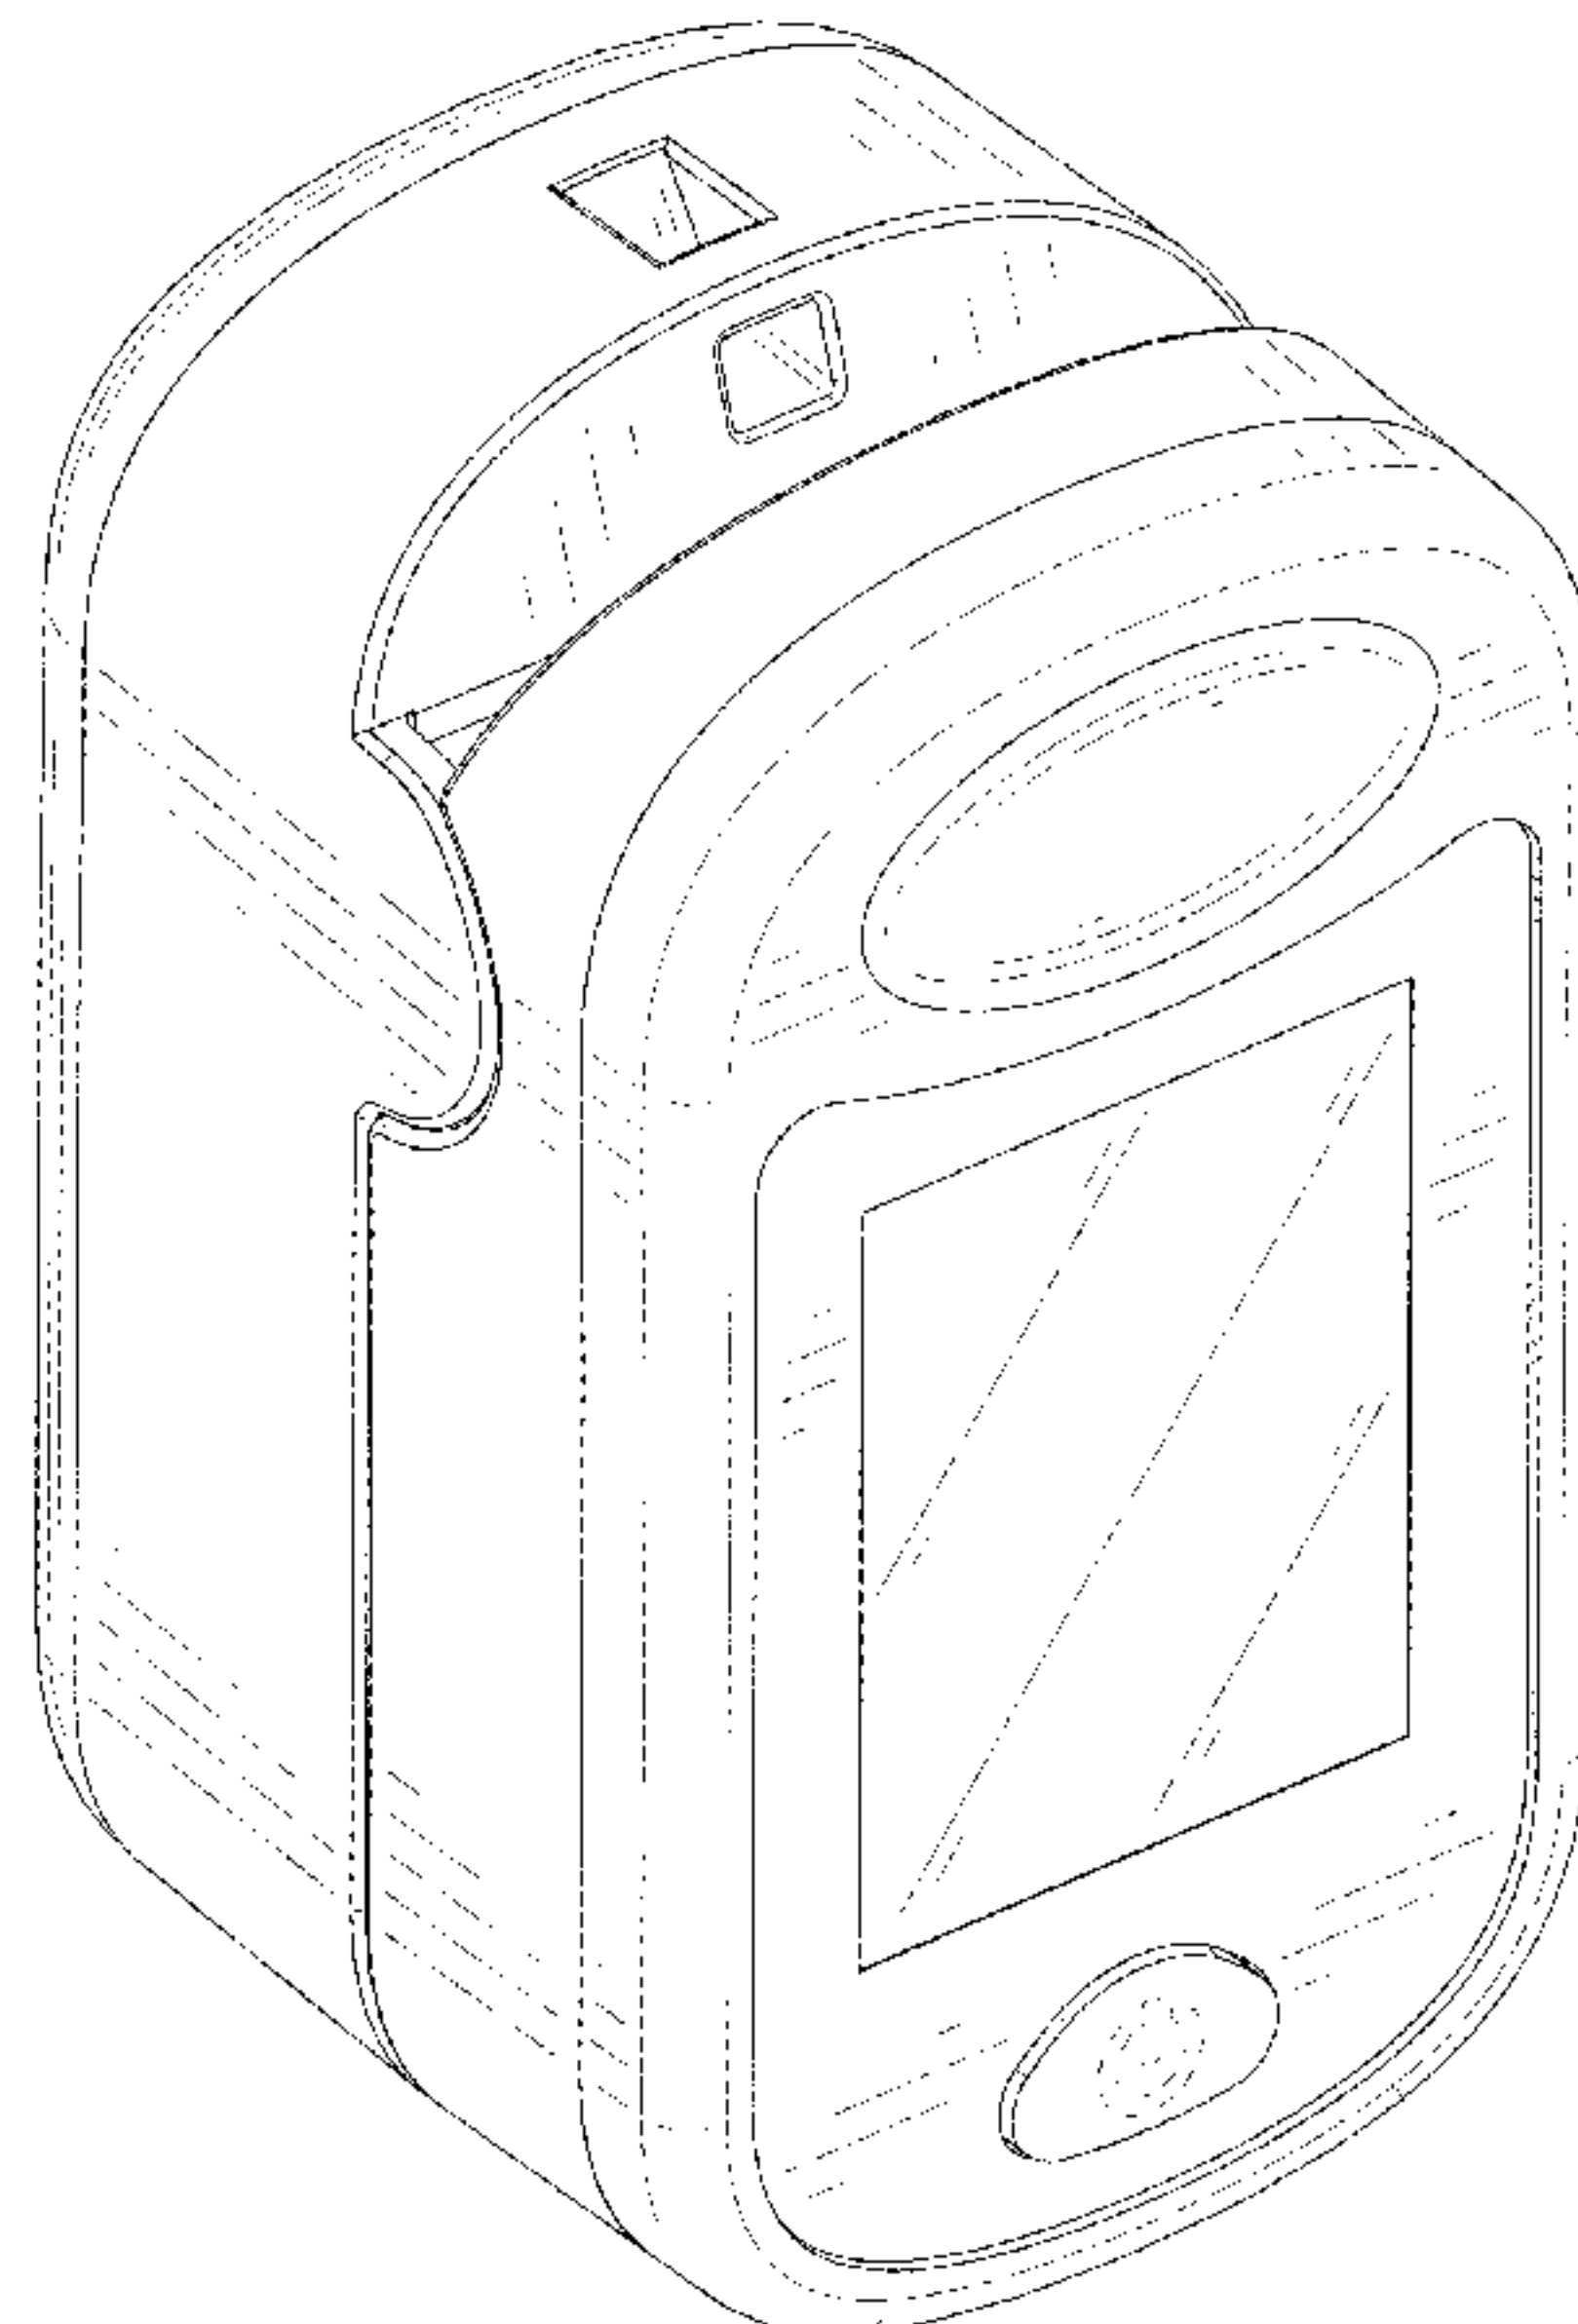

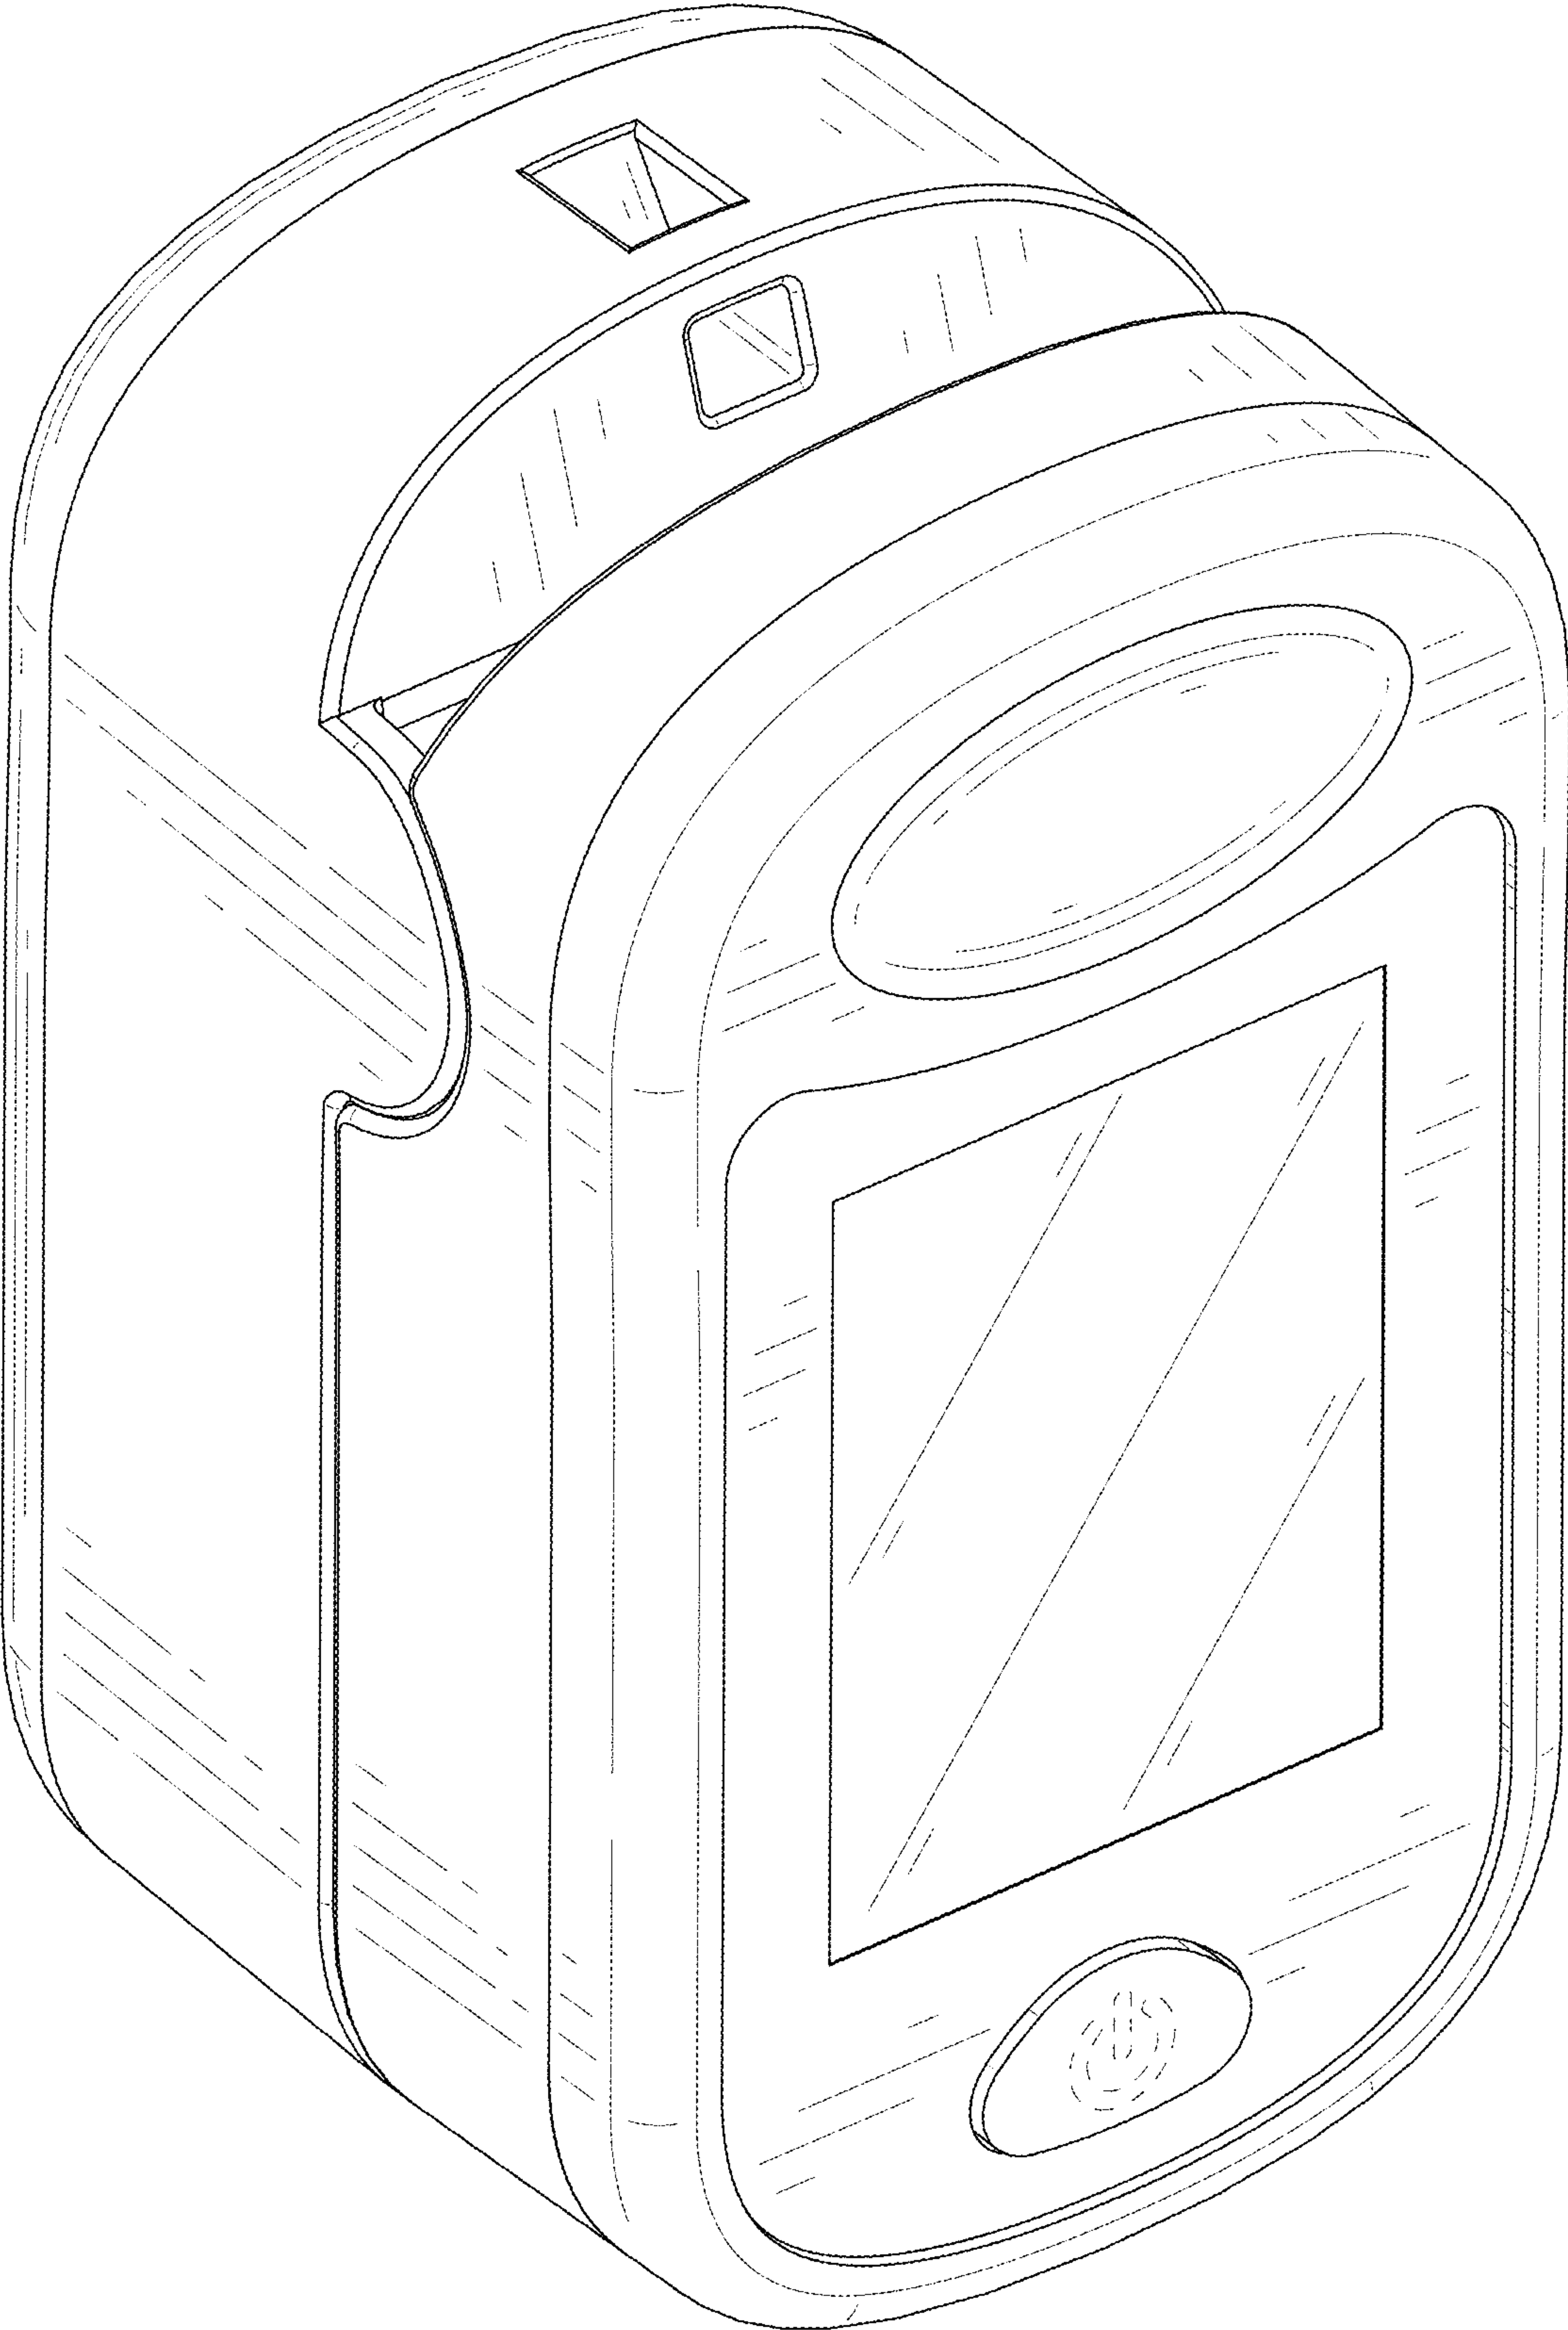


FIG. 1

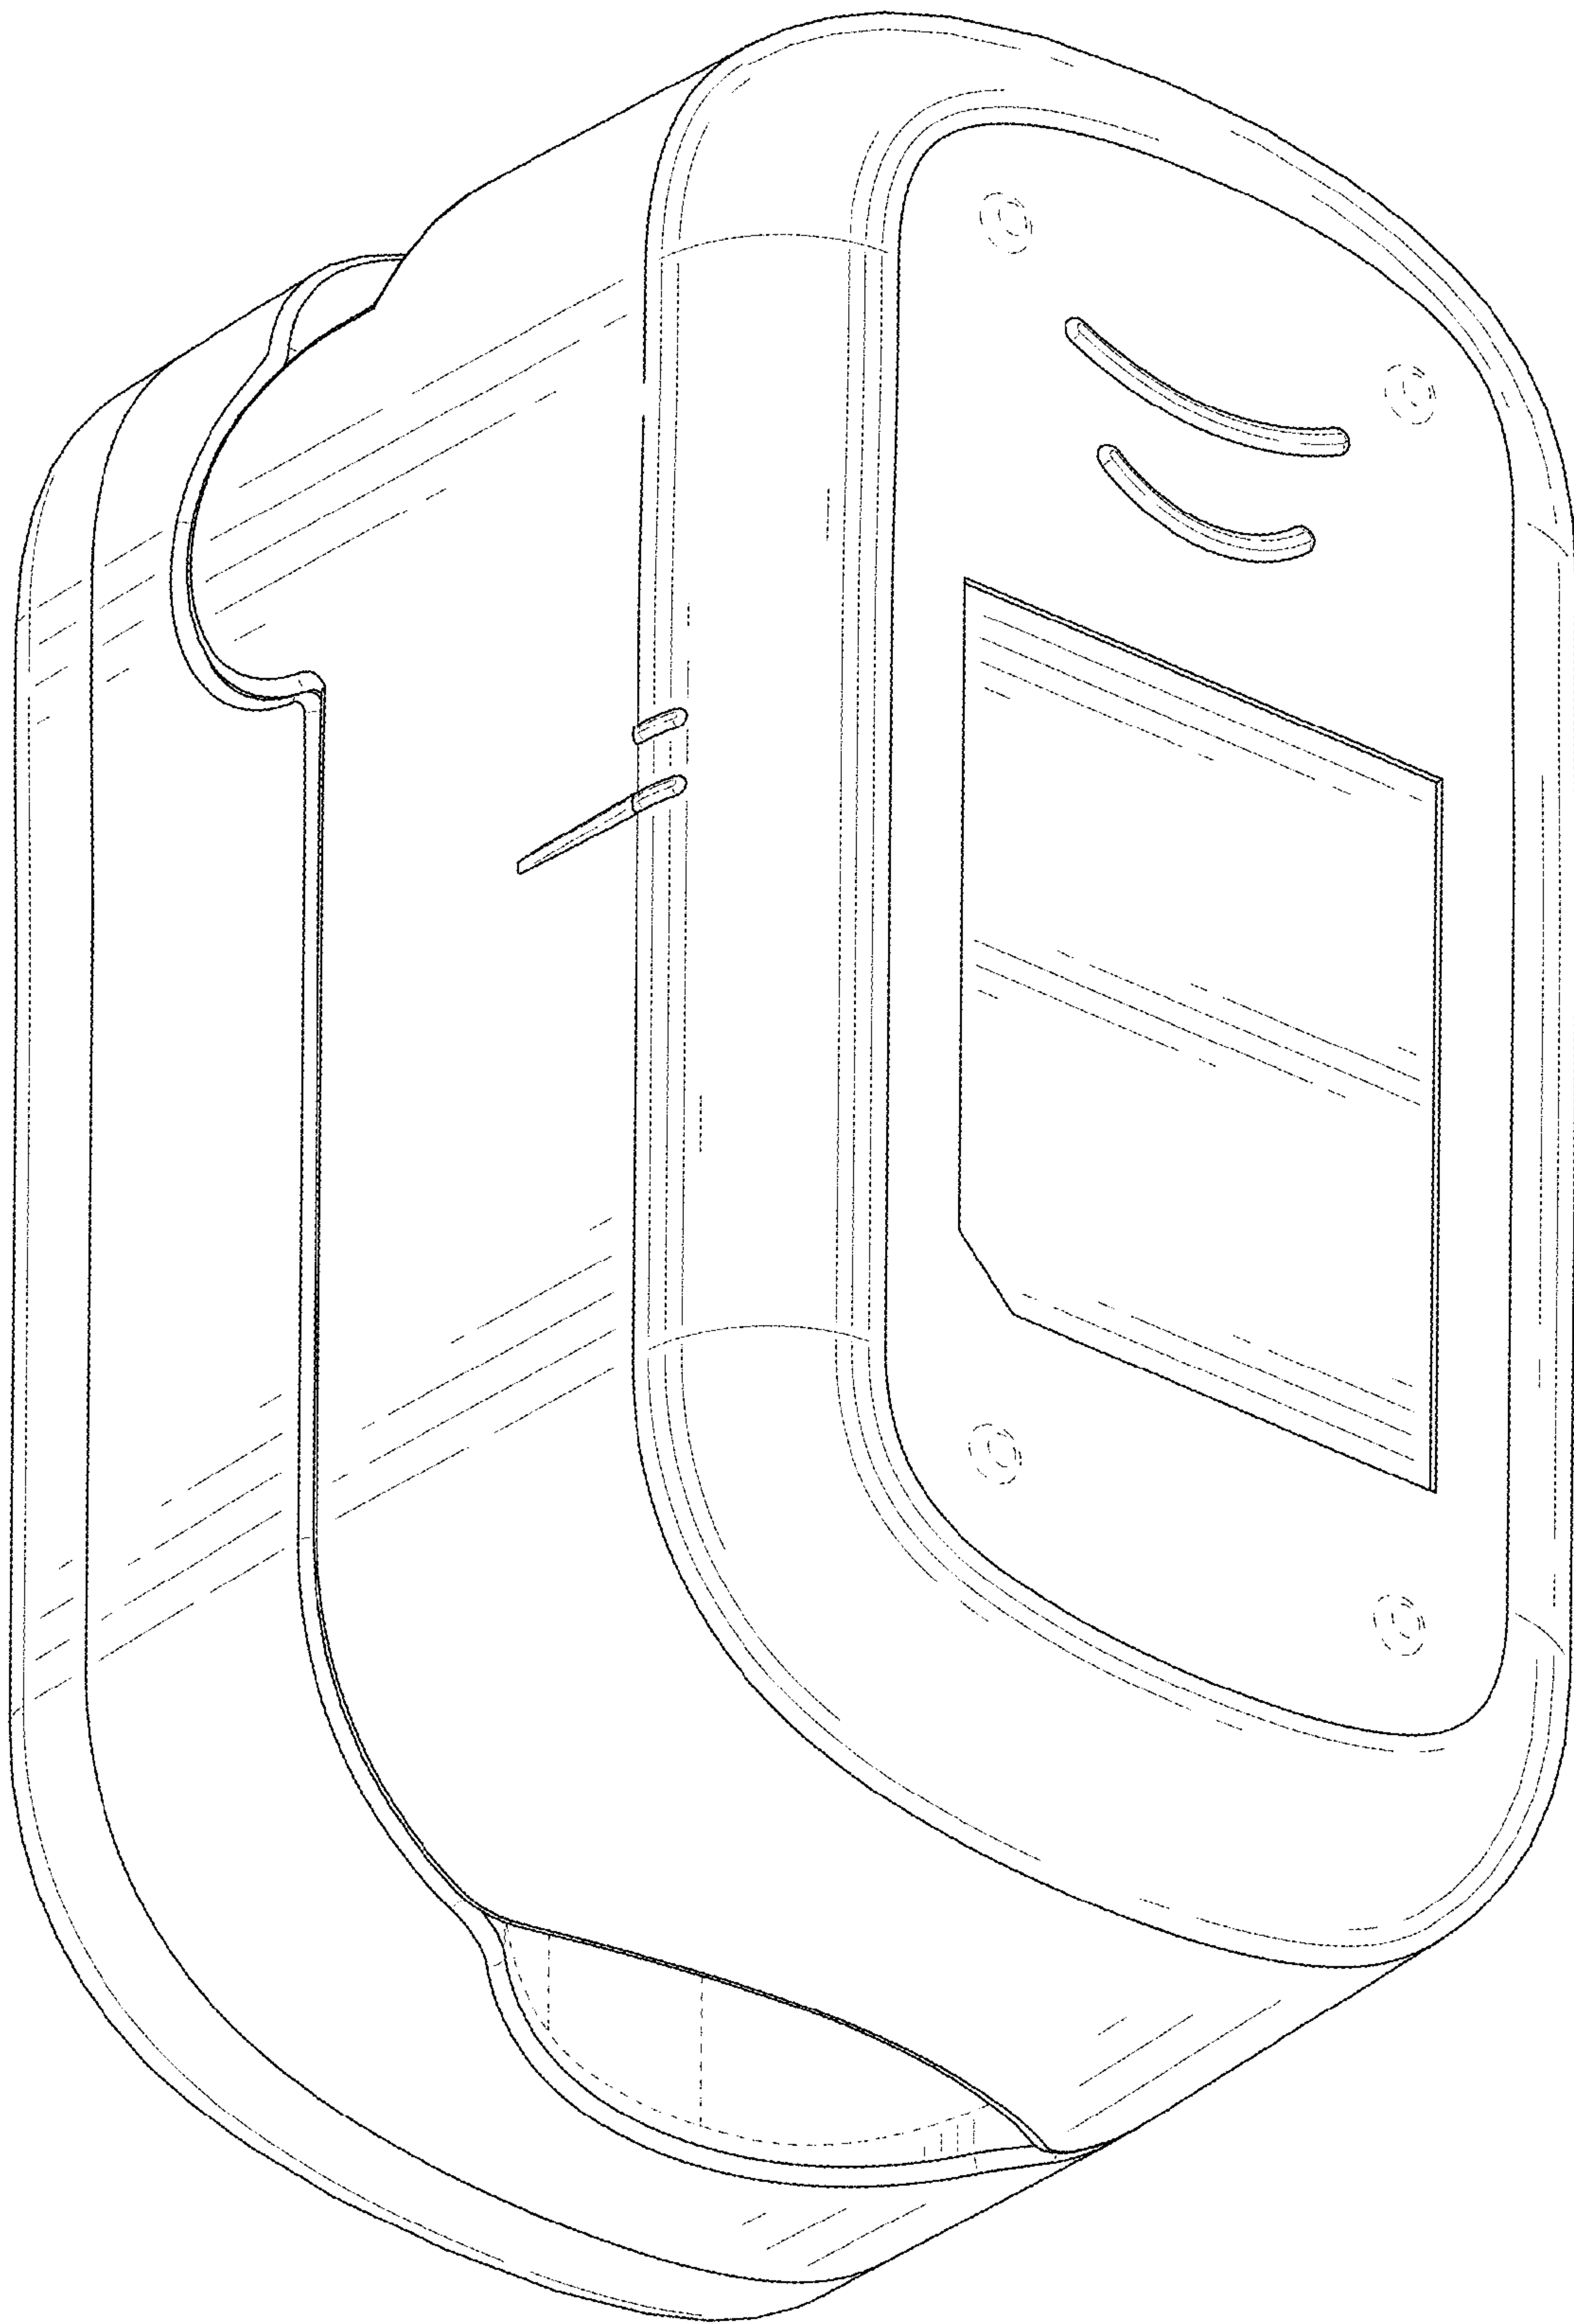


FIG. 2

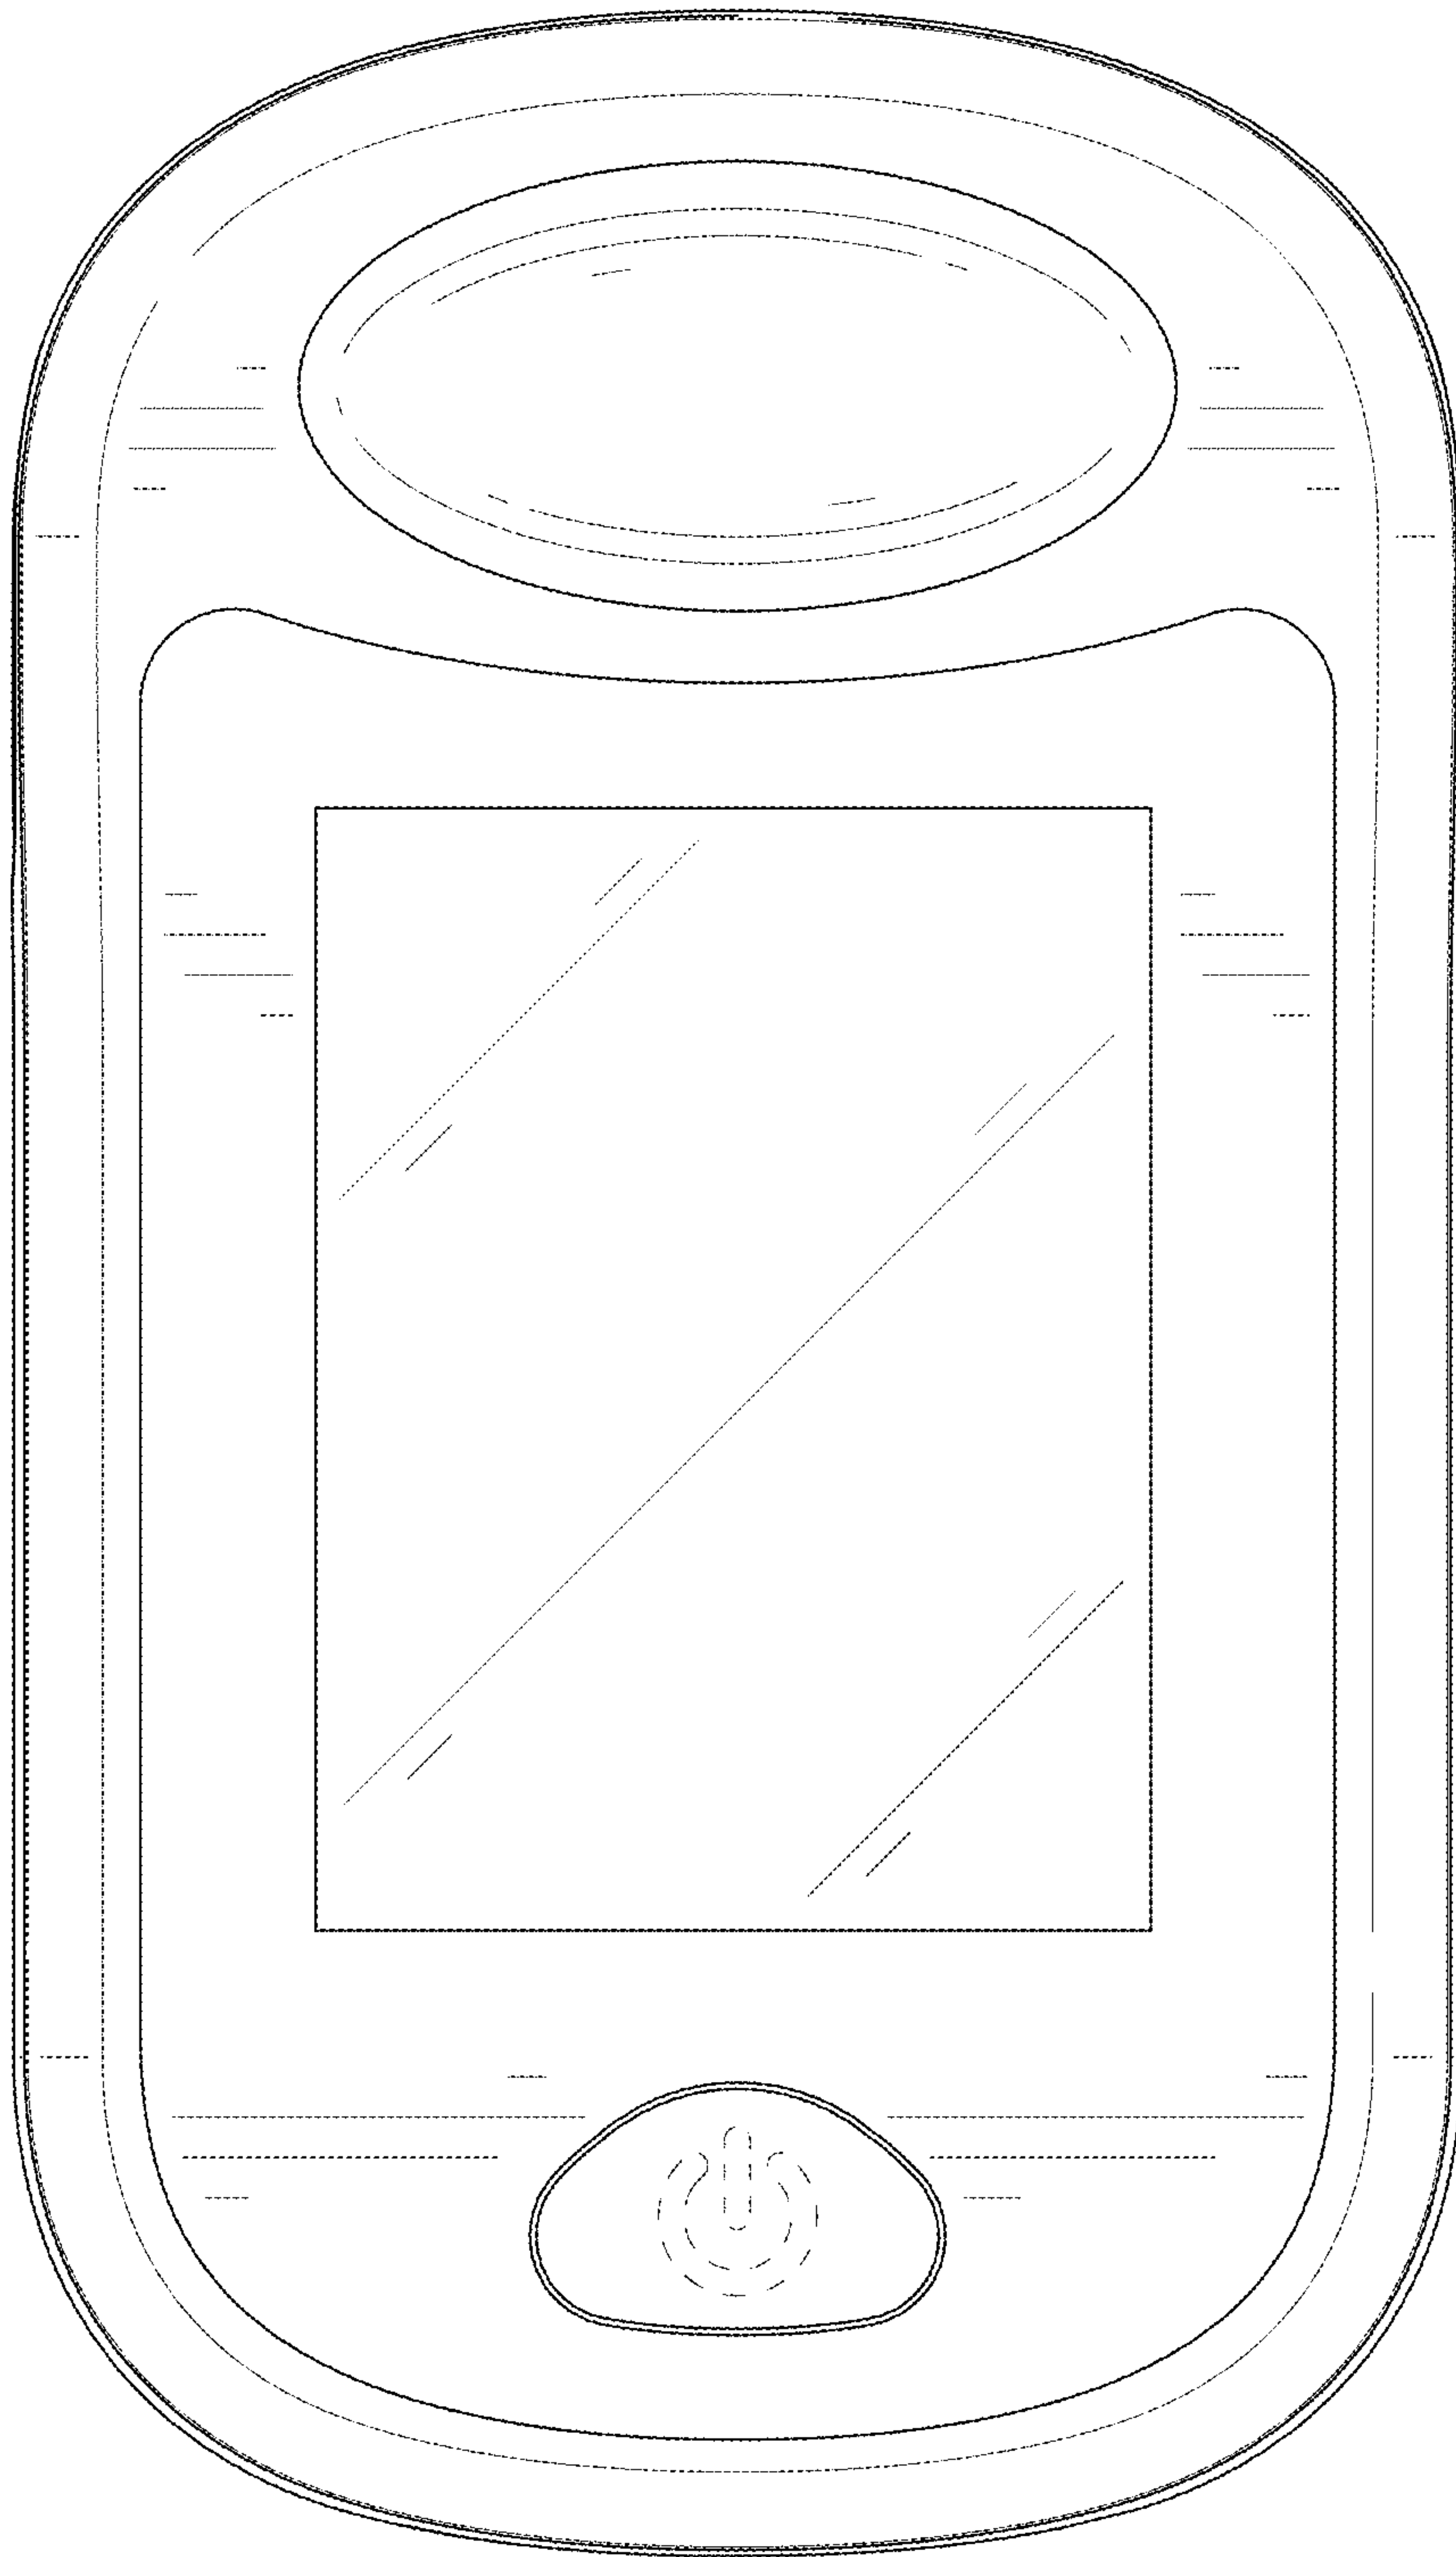


FIG. 3

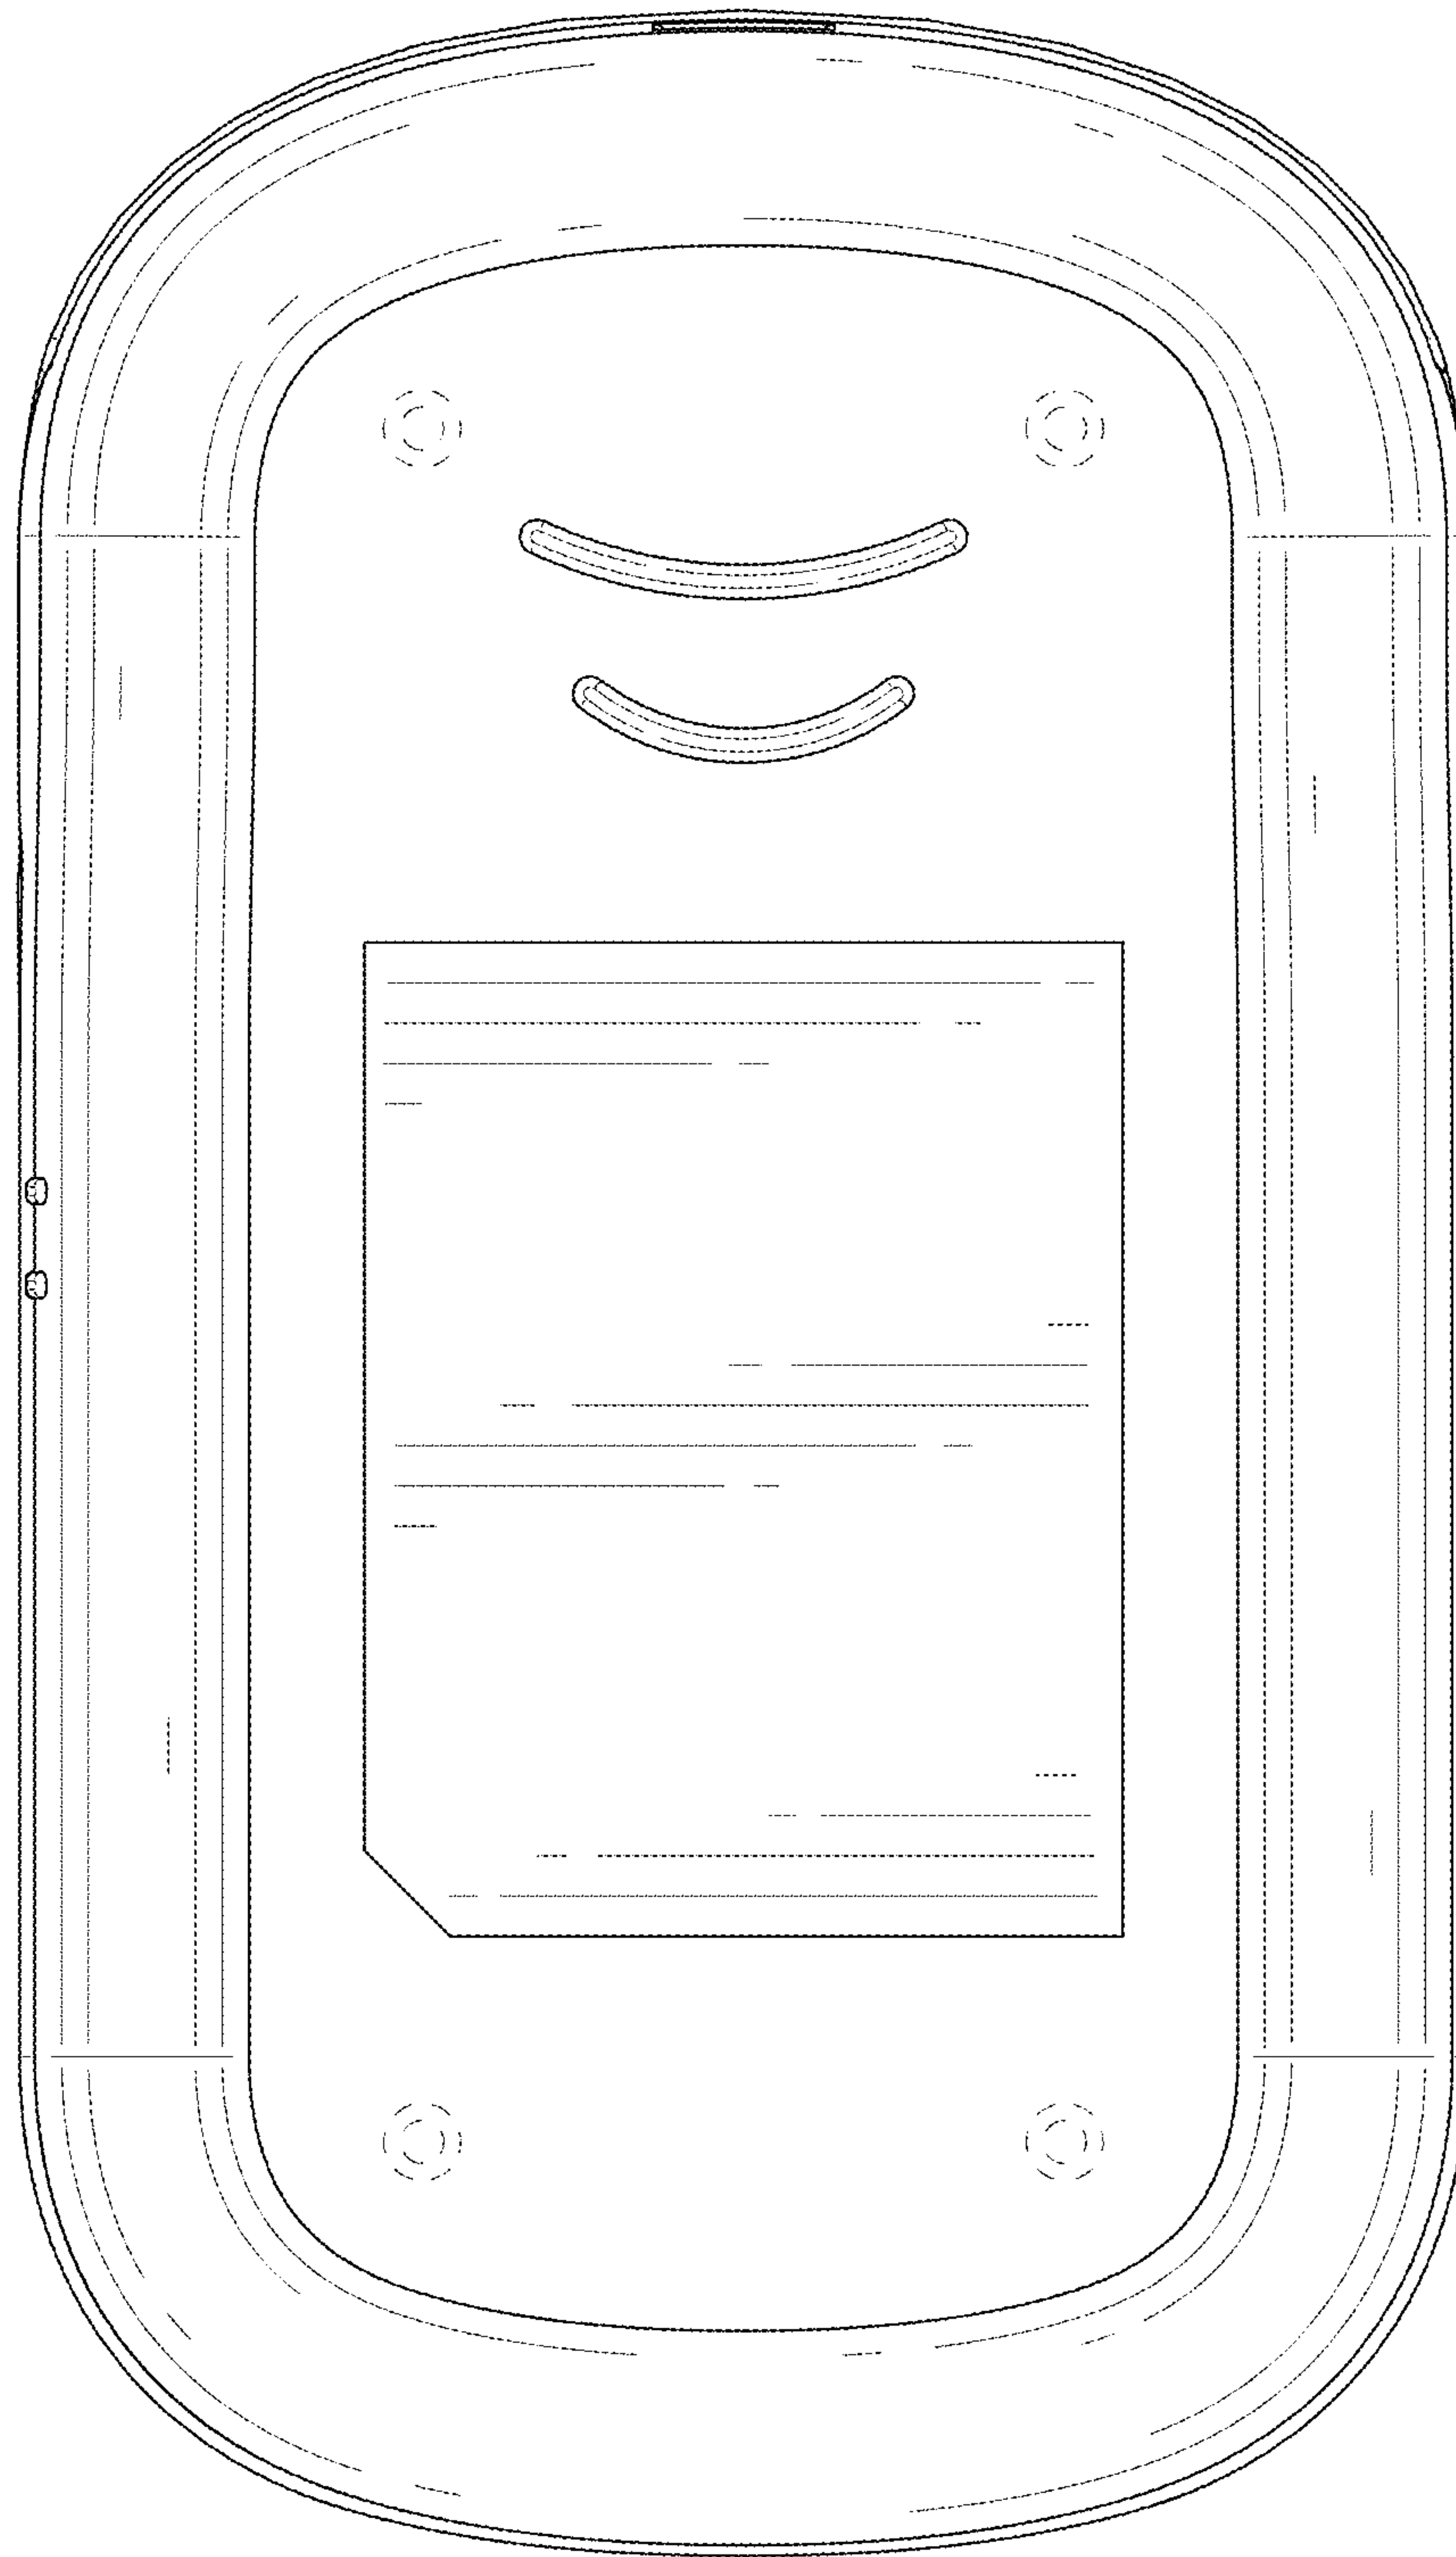


FIG. 4

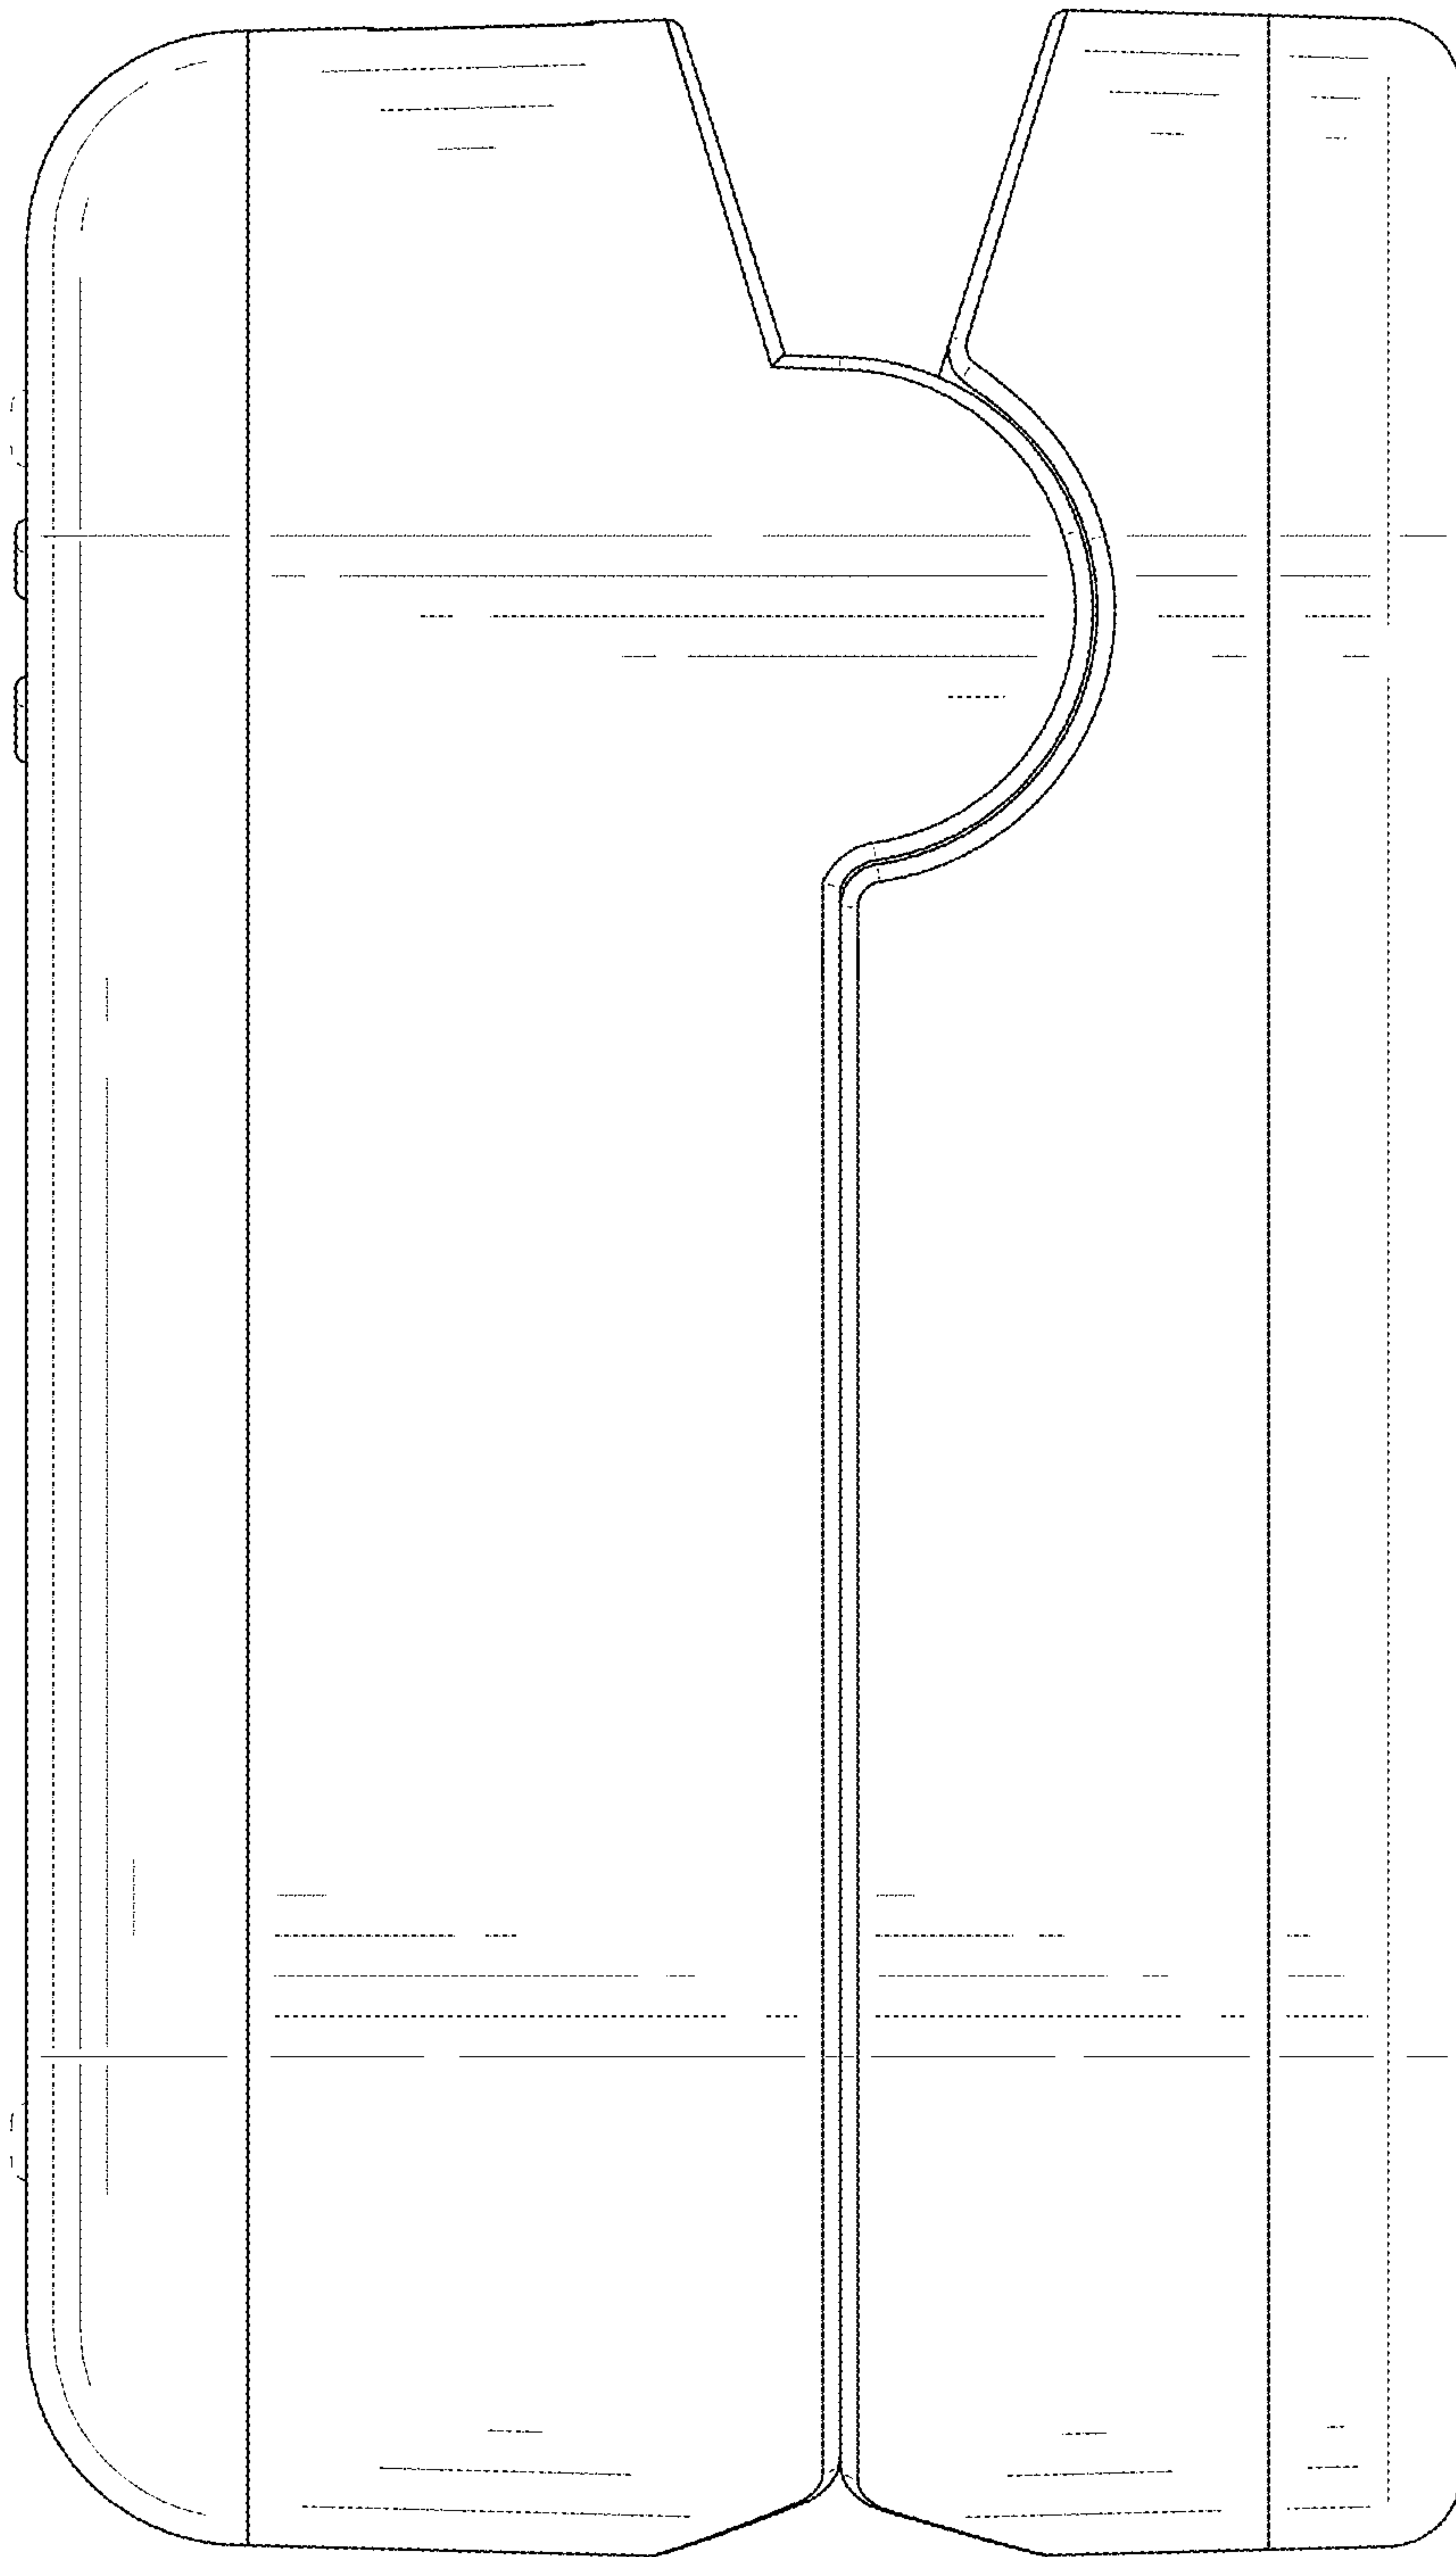


FIG. 5

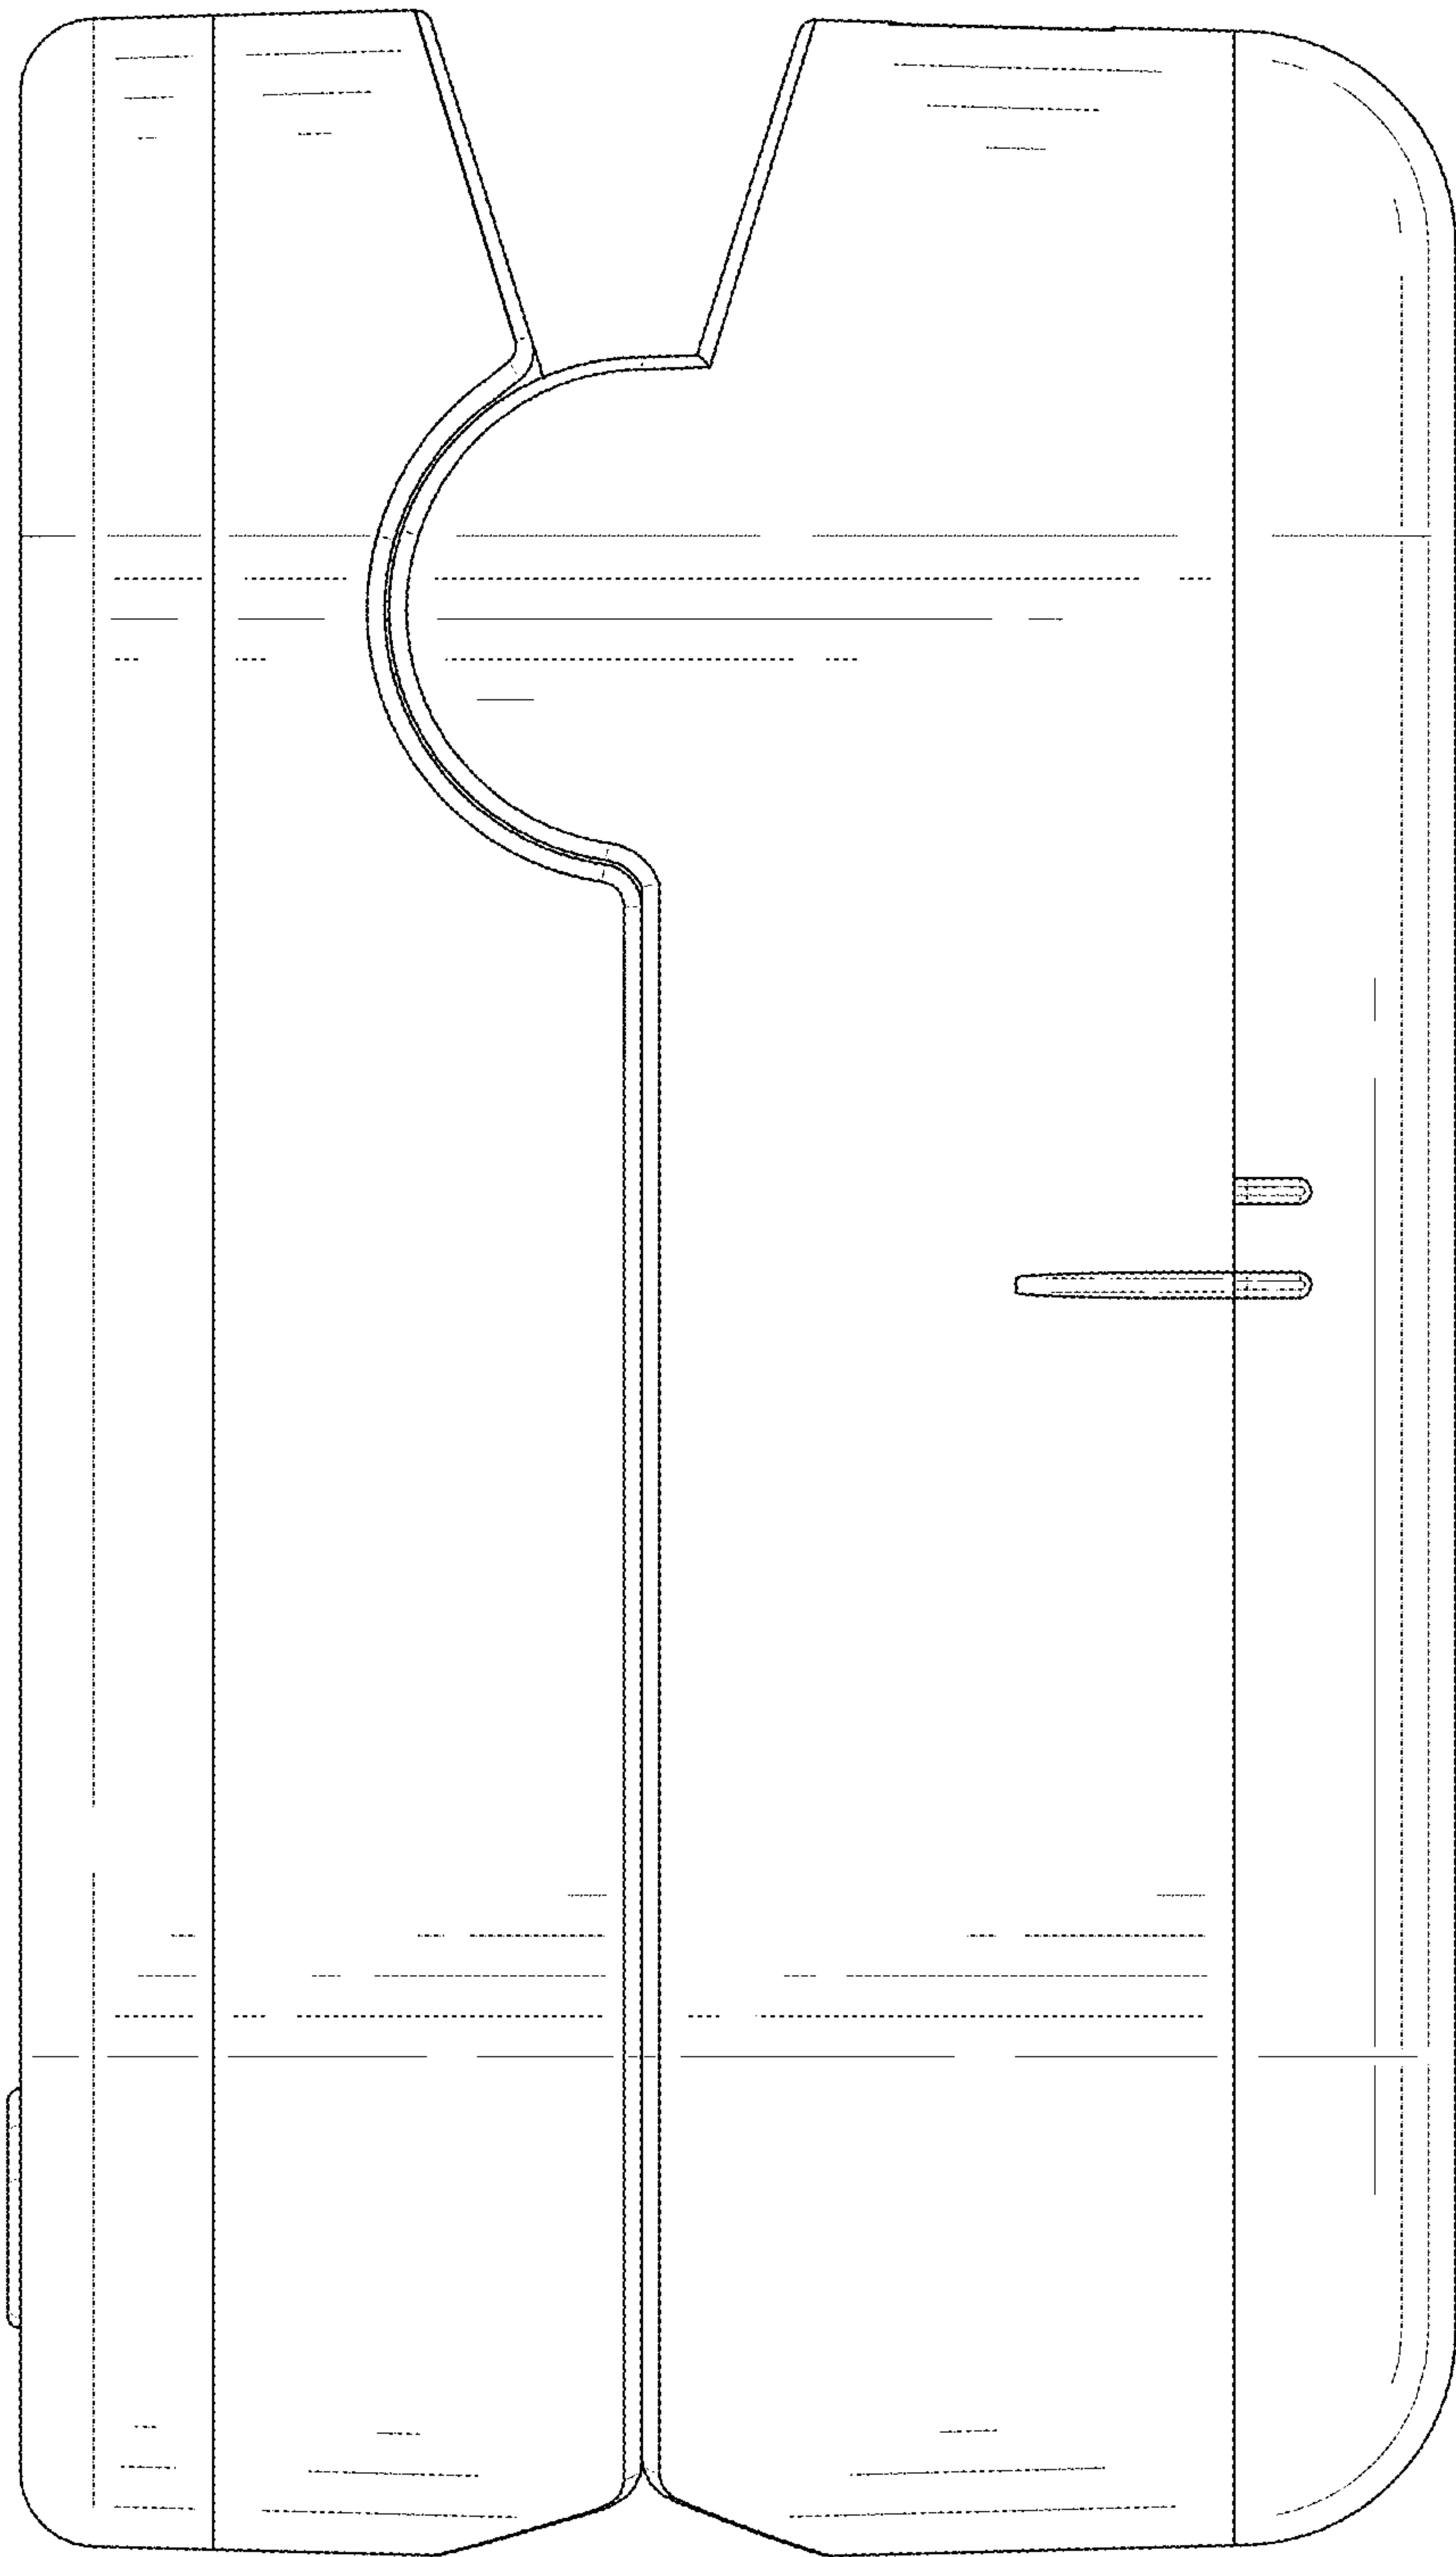


FIG. 6

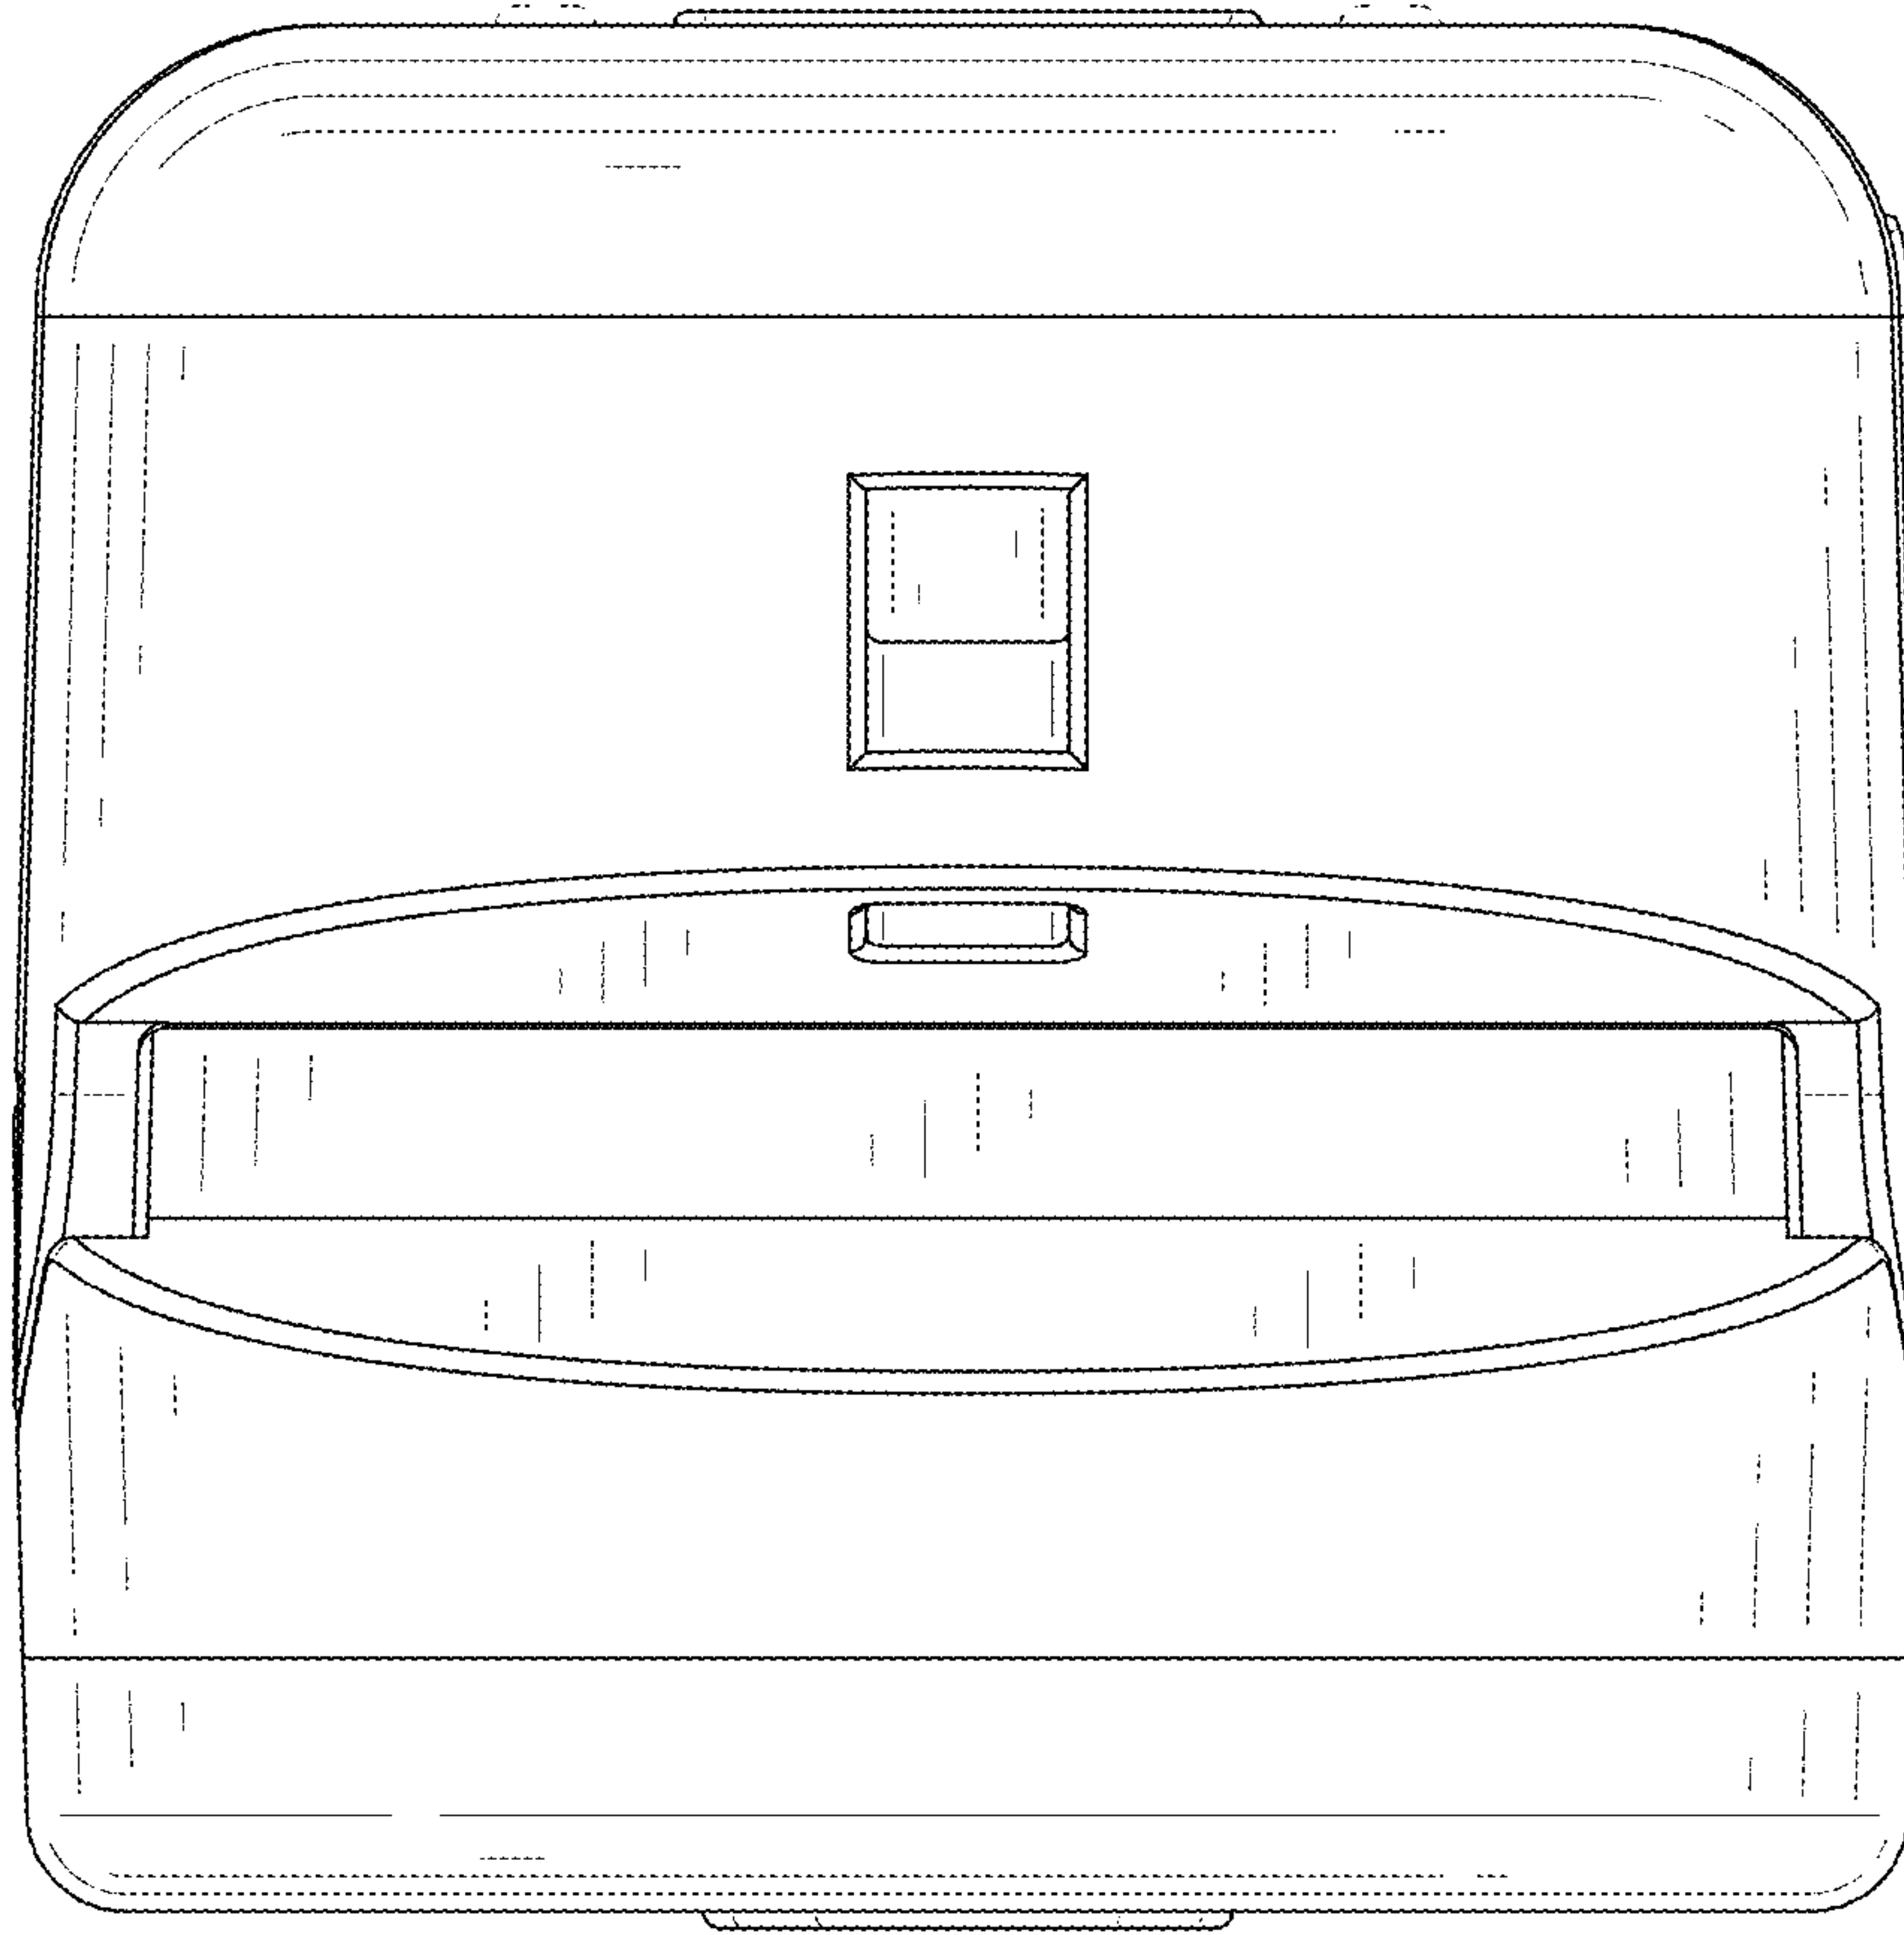


FIG. 7

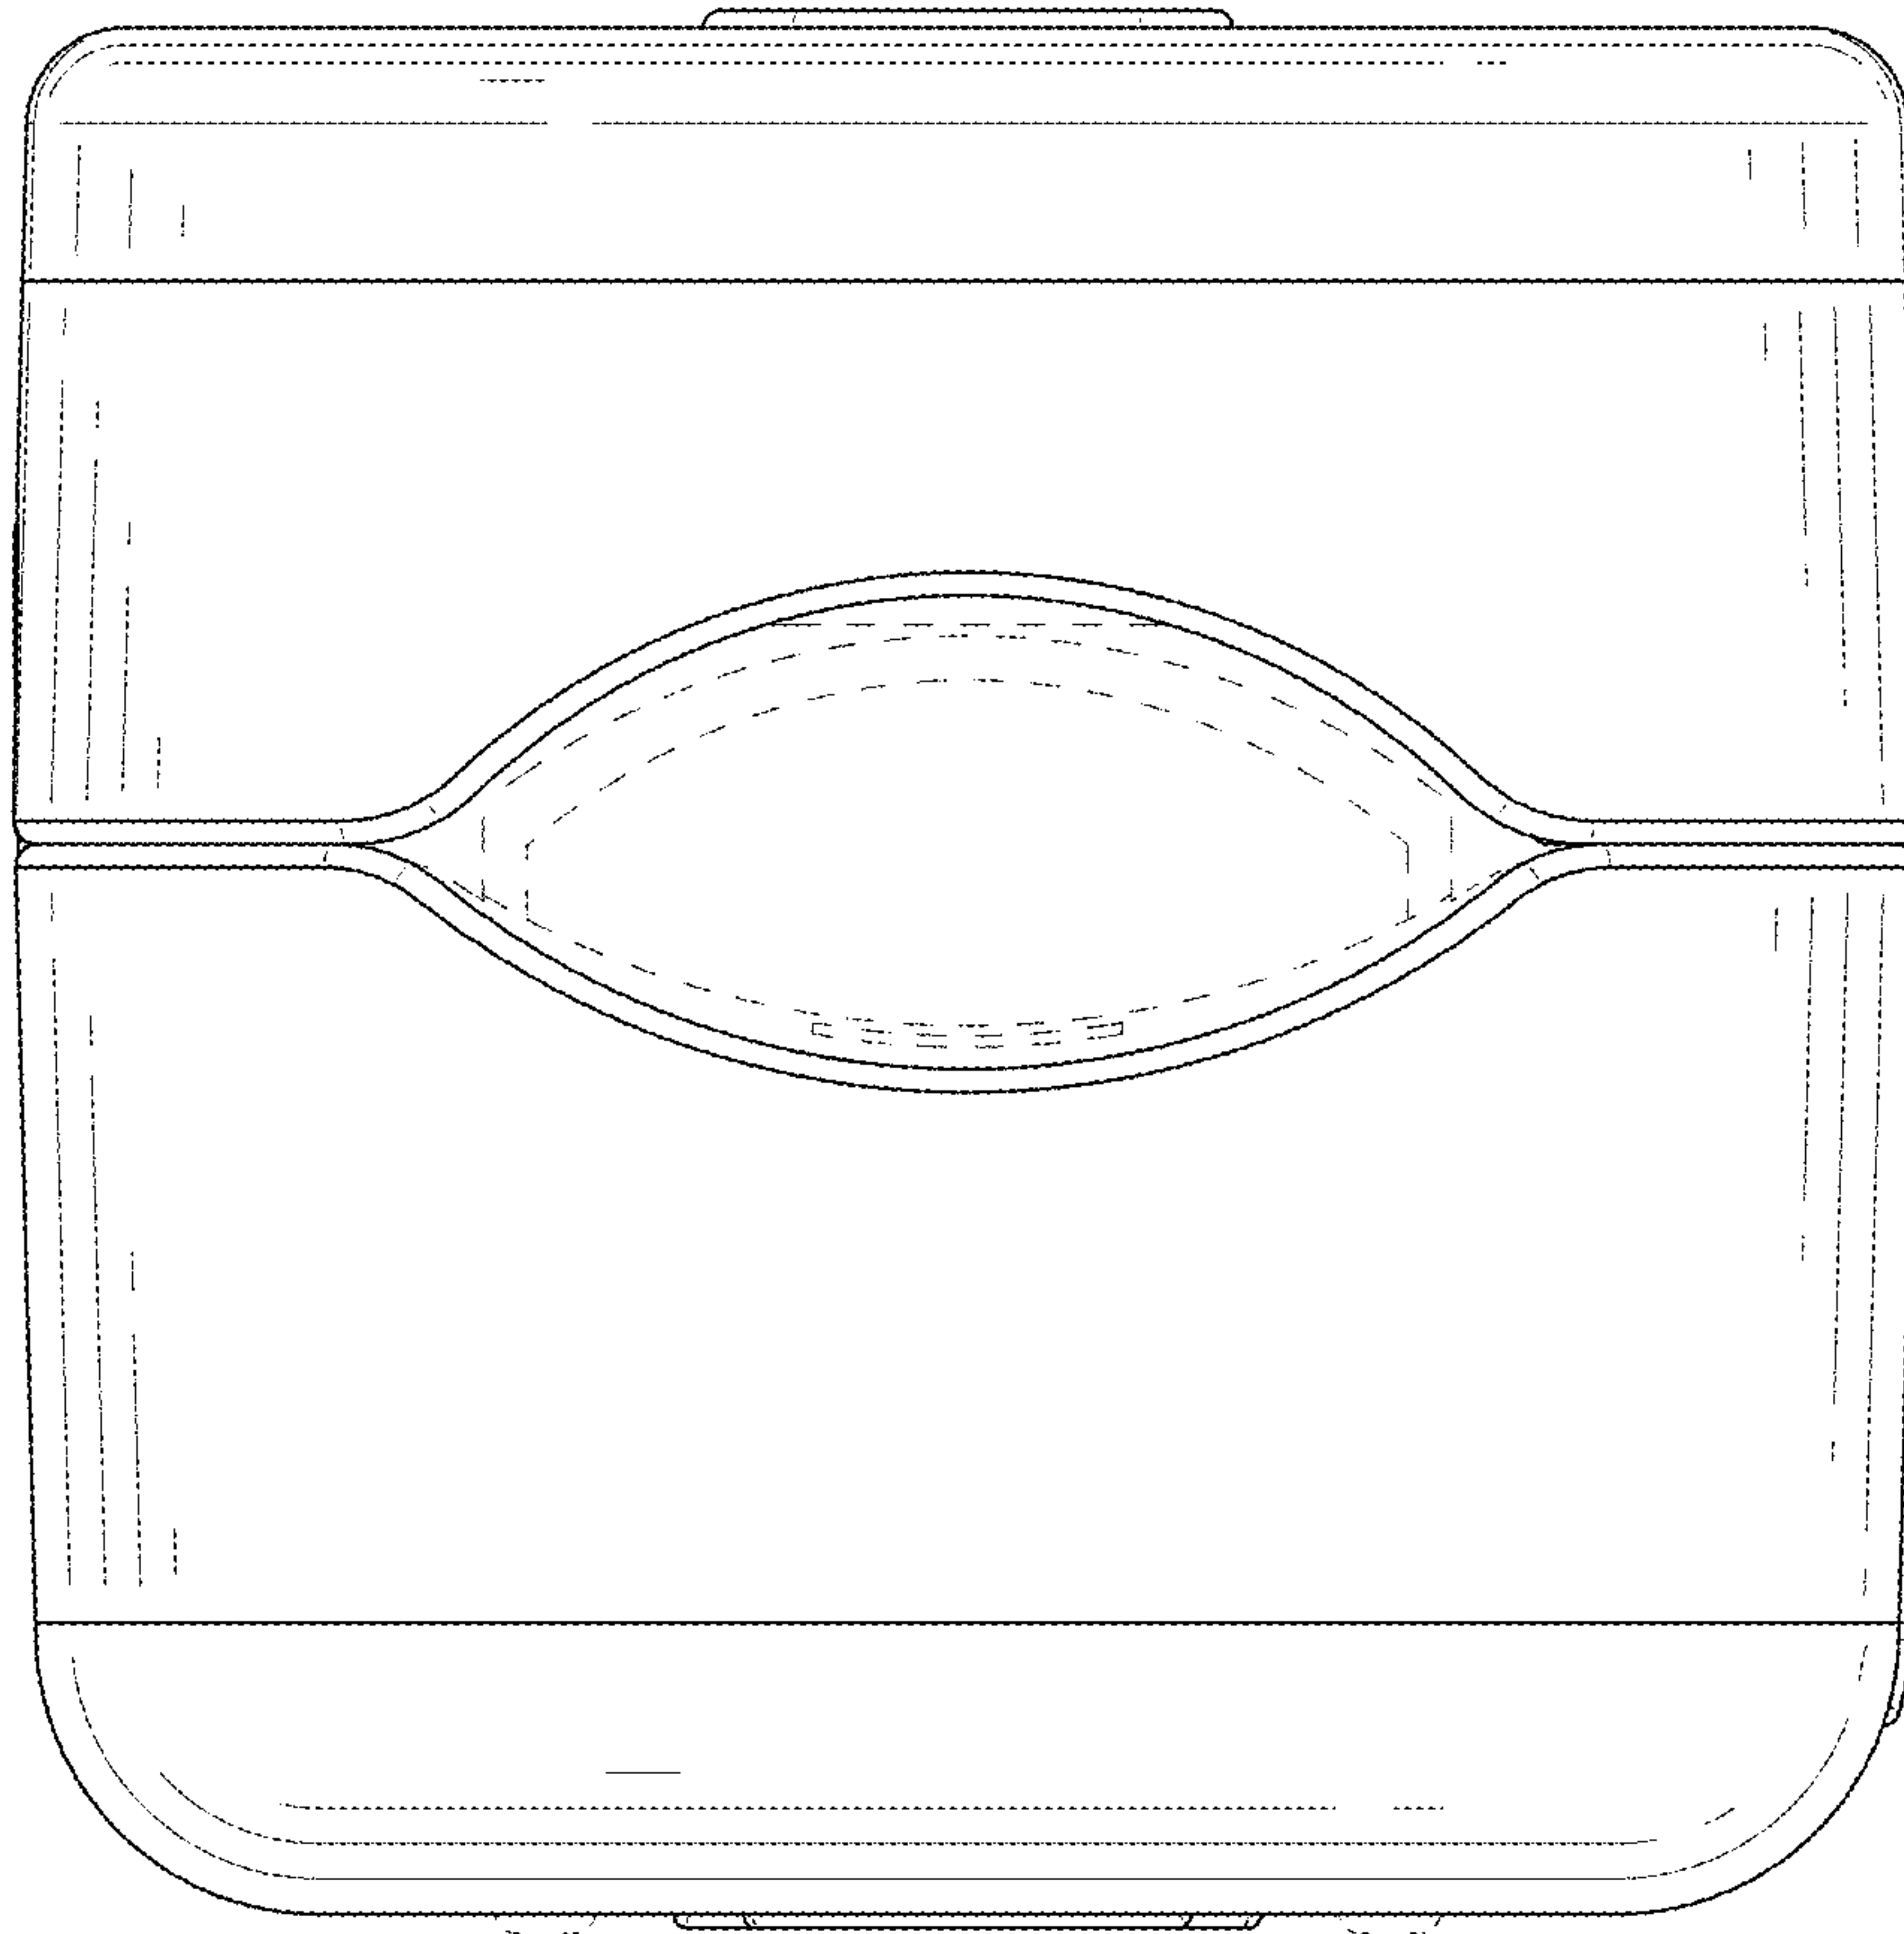


FIG. 8

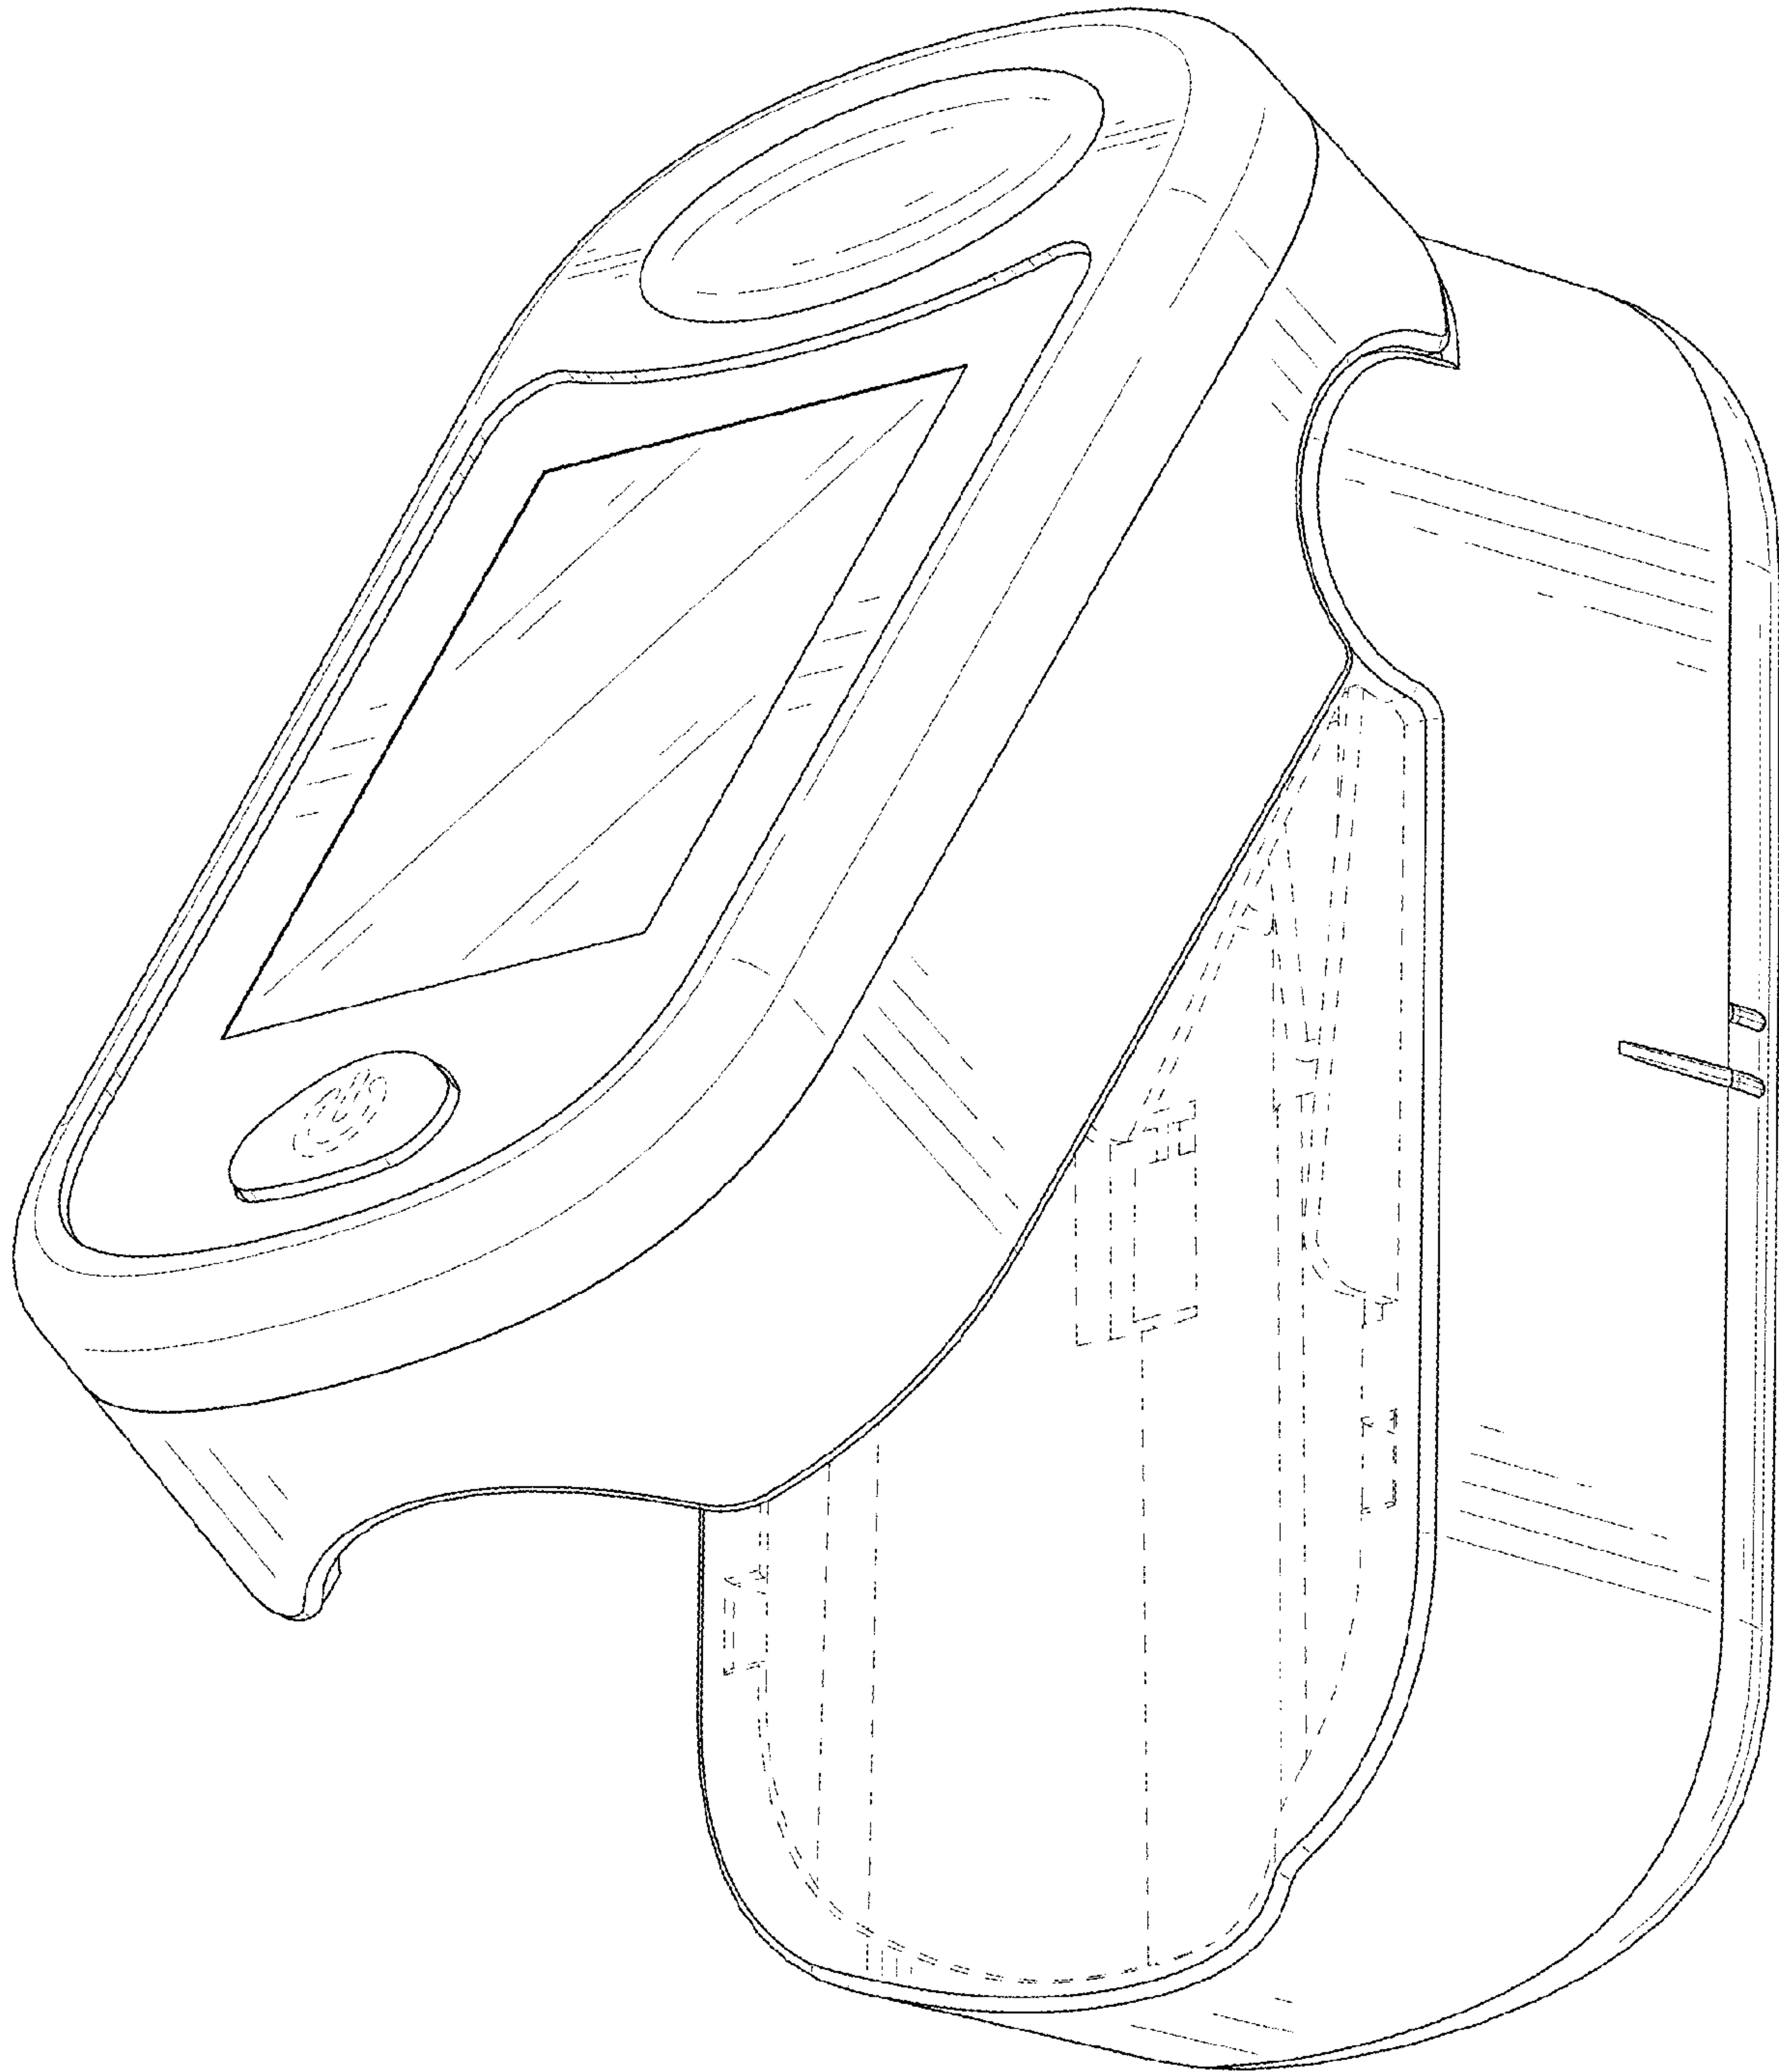


FIG. 9