



US00D926798S

(12) **United States Design Patent** (10) **Patent No.:** **US D926,798 S**
Gaultieri et al. (45) **Date of Patent:** **** Aug. 3, 2021**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE**

D717,312 S * 11/2014 Matas G06F 3/0483
D14/485
D726,760 S * 4/2015 Yokota D14/488
D731,510 S * 6/2015 Kiruluta D14/486

(71) Applicant: **GE Precision Healthcare LLC**,
Wauwatosa, WI (US)

(Continued)

(72) Inventors: **James Gaultieri**, Pittsburgh, PA (US);
Axel Crasemann, Munich (DE)

OTHER PUBLICATIONS

Infinitt, "Infinitt Pacs," 6 pages. Retrieved Aug. 29, 2019, from
<https://www.infinittna.com/solutions/radiology/infinitt-pacs/>.

(73) Assignee: **GE Precision Healthcare LLC**,
Wauwatosa, WI (US)

(Continued)

(**) Term: **15 Years**

Primary Examiner — Cary M Robinson

(21) Appl. No.: **29/694,194**

(74) Attorney, Agent, or Firm — Hanley, Flight &
Zimmerman, LLC

(22) Filed: **Jun. 7, 2019**

(57) **CLAIM**

(51) **LOC (13) Cl.** **14-04**

The ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.

(52) **U.S. Cl.**

USPC **D14/486**; D14/490

(58) **Field of Classification Search**

USPC 345/1.1, 1.2, 2.1–2.3, 3.1, 902; 715/763,
715/810, 836, 837, 846, 847, 977;
D14/485–495

CPC B60K 37/00; G06F 3/048–04897; G06F
3/013; G06F 3/017; G06F 3/165; G06F
3/197; G06F 17/212; G06T 13/80; G06T
15/02; H04M 1/6075; H04M 3/567;
H04M 1/2477; H04M 1/26; H04M
1/274582; H04L 12/581; H04L 12/813;
H04L 12/1813; G06Q 10/10; H04N 7/16

See application file for complete search history.

DESCRIPTION

A portion of the disclosure of this patent document contains material for which a claim for copyright is made. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the US Patent and Trademark Office patent file or records, but reserves all other copyrights whatsoever.

FIG. 1 is a front view of a display screen or portion thereof with a graphical user interface showing a first embodiment of the claimed design; and,

FIG. 2 is another front view of FIG. 1, but showing alternative broken line subject matter.


The outer broken line illustrates the display screen or portion thereof and the inner broken lines and dotted lines (including the selection of the thumbnail images appearing in dotted lines, as shown in FIG. 2) illustrate portions of the graphical user interface. None of the broken lines form part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,706,097 A * 1/1998 Schelling G03B 31/06
355/40
6,711,297 B1 * 3/2004 Chang G06T 1/00
382/240
D546,335 S * 7/2007 Vong D14/485
D688,687 S * 8/2013 Smith D14/486

1 Claim, 2 Drawing Sheets

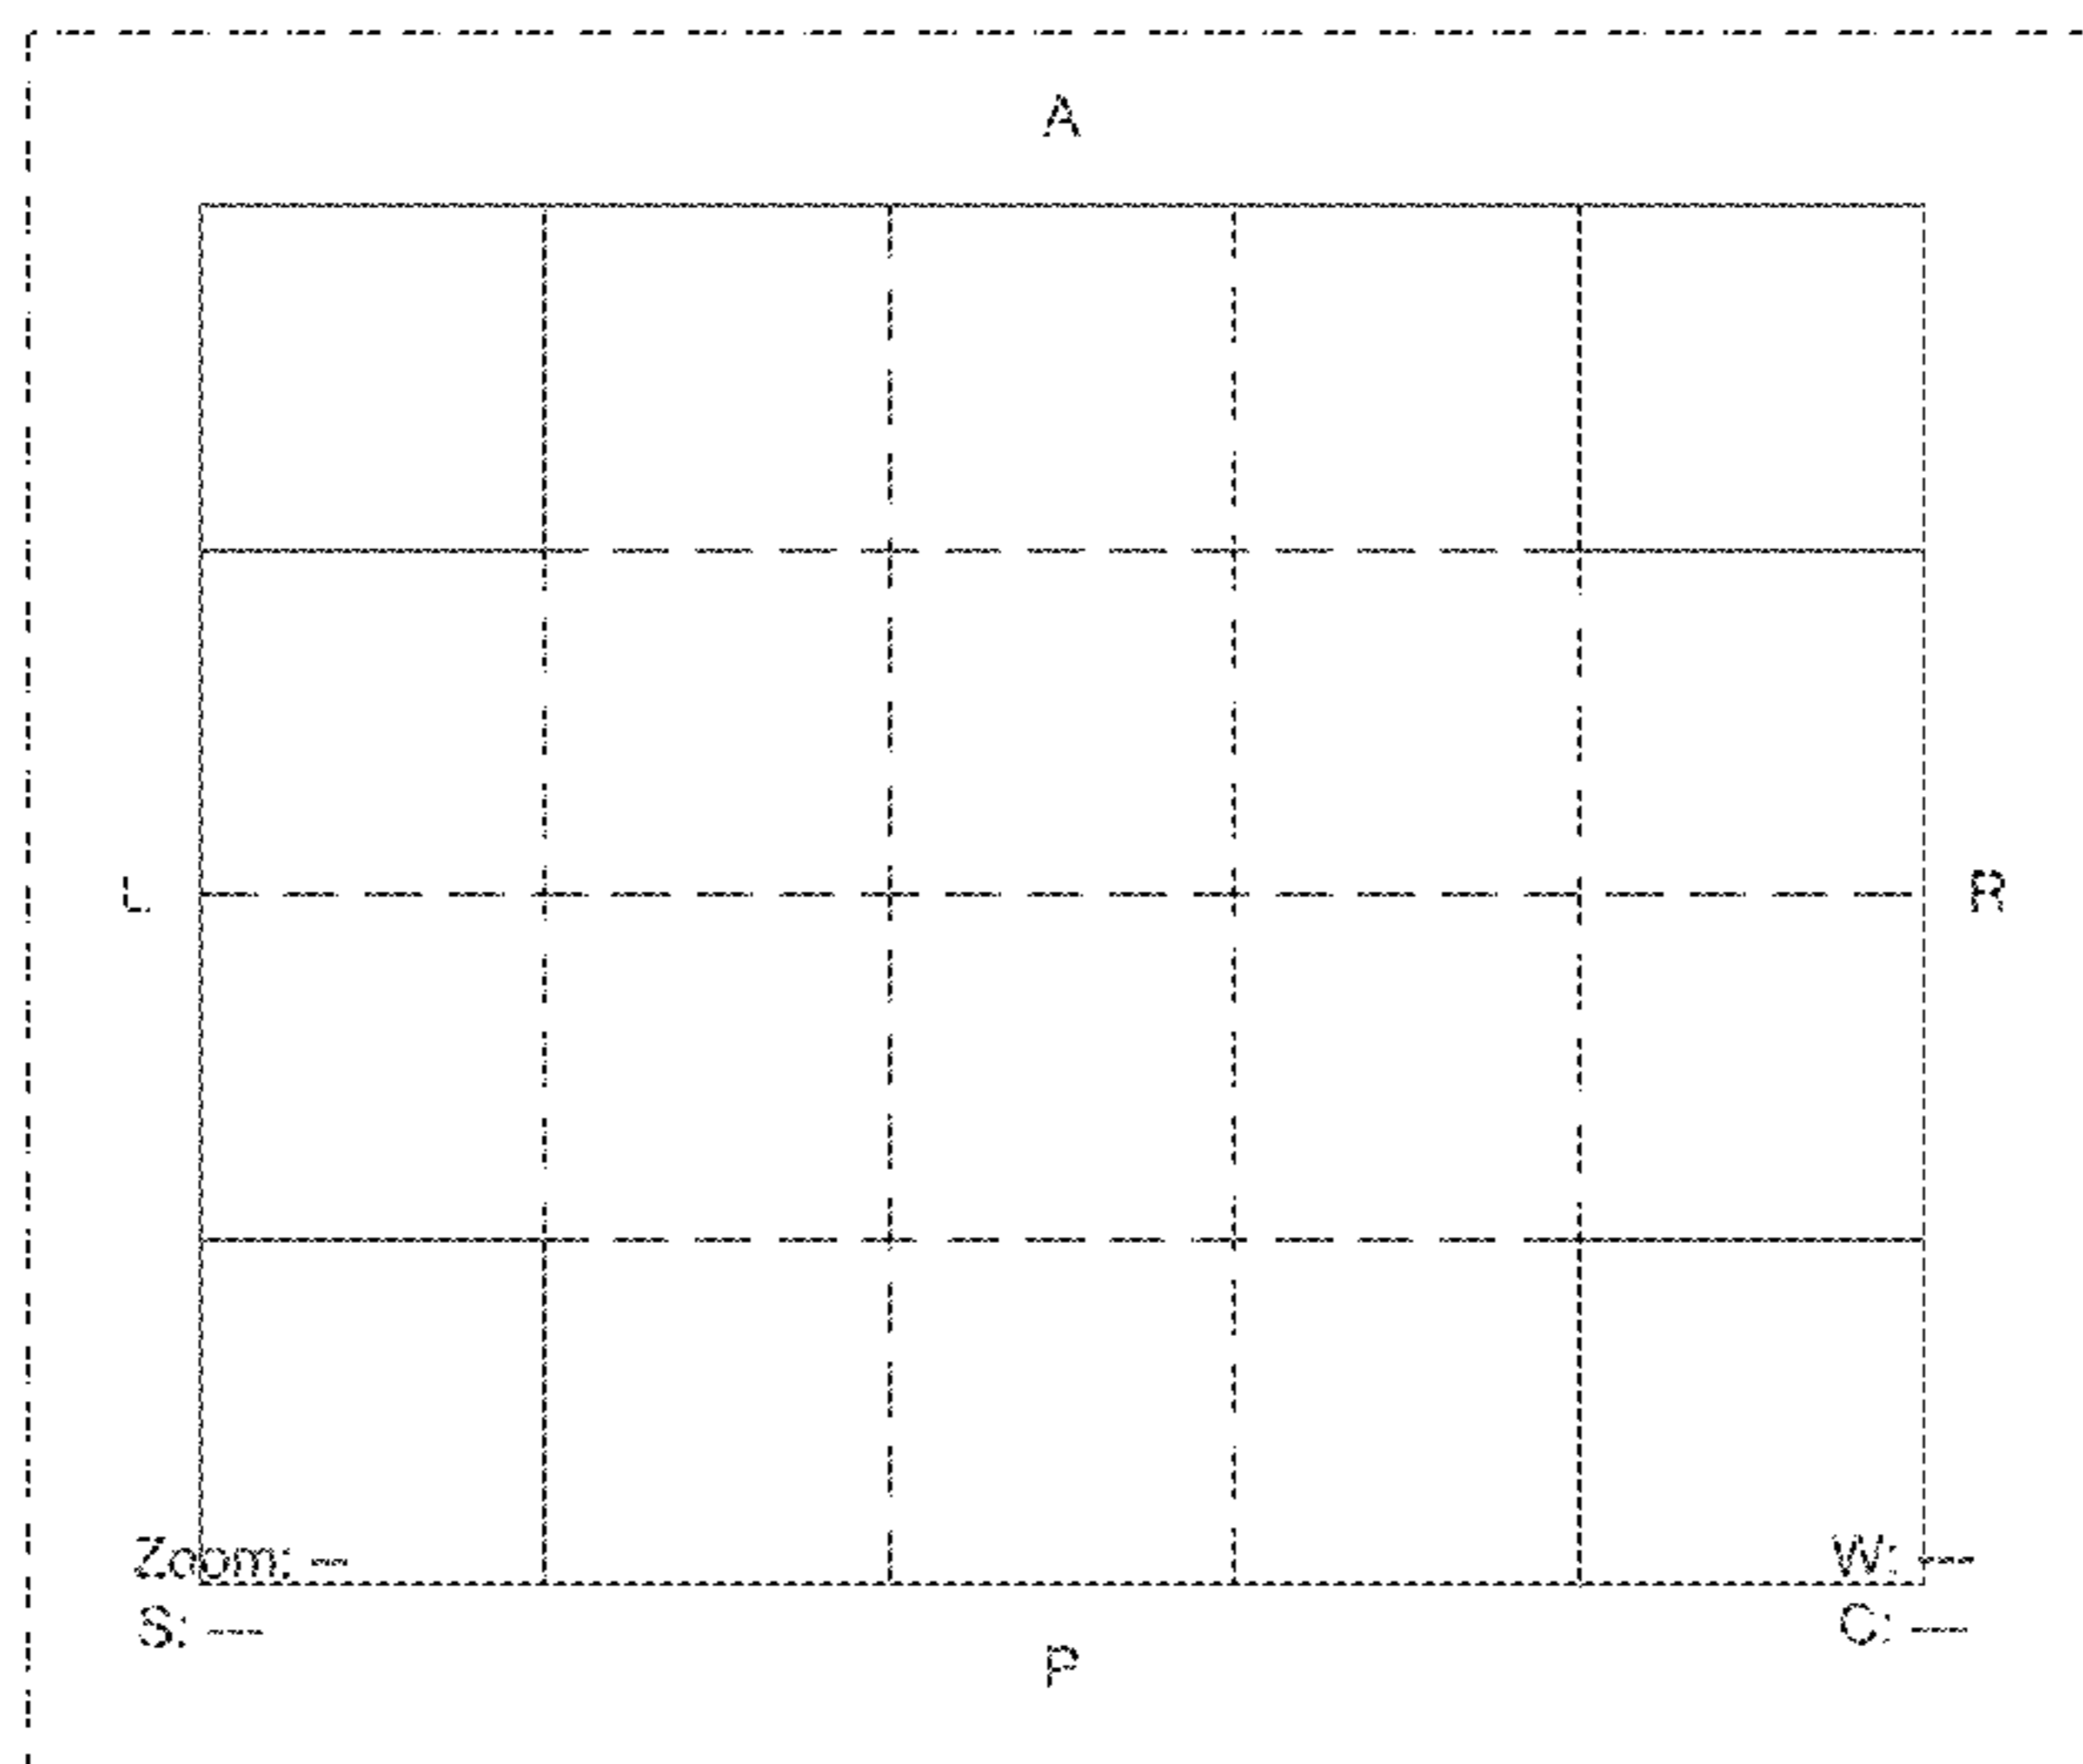

(56)

References Cited


U.S. PATENT DOCUMENTS

D750,651 S * 3/2016 Seo D14/486
 D756,910 S * 5/2016 Gupta D13/103
 D760,238 S * 6/2016 Evans D14/485
 D763,879 S * 8/2016 Worrell D14/486
 D786,910 S * 5/2017 Higuchi D14/486
 D817,980 S * 5/2018 Sagrillo
 2003/0197724 A1 * 10/2003 Reed G06F 3/0481
 715/738
 2006/0212811 A1 * 9/2006 Gottfurcht G06F 3/04892
 715/201
 2010/0023865 A1 * 1/2010 Fulker H04L 12/2809
 715/734
 2011/0317192 A1 * 12/2011 Fukuoka H04N 1/00411
 358/1.13
 2016/0248900 A1 * 8/2016 Kim G06F 3/04845
 2016/0300172 A1 * 10/2016 Bangalore G01W 1/14
 2016/0307274 A1 * 10/2016 Sweeney G06Q 40/08
 2020/0315589 A1 * 10/2020 Stavros A61B 5/7275

OTHER PUBLICATIONS


“Visage Imaging to Present Visage 7.1.4, Work-in-Progress Products at RSNA 2013,” Imaging Technology News, Nov. 27, 2013, 2 pages. Retrieved Aug. 29, 2019, from <https://www.itnonline.com/content/visage-imaging-present-visage-714-work-progress-products-rsna-2013>.
 Siemens, “syngo DynaCT Smart: Reduce Metal Artifacts to See the Unseen,” 5 pages. Retrieved Aug. 29, 2019, from <https://www.siemens-healthineers.com/angio/options-and-upgrades/clinical-software-applications/syngo-dynact-smart>.
 Konica Minolta, “Direct Digitizer CS-7, Version 1.30 Operation Manual,” Jan. 12, 2017, 424 pages.
 GE Healthcare, “Centricity Cardio Enterprise,” 10 pages. Retrieved Aug. 29, 2019, from <http://www3.gehealthcare.in/en/products/categories/healthcare-it/medical-imaging-informatics-ris-pacs-cvis/centricity-cardio-enterprise#tabs/tab92A16C6F957047F6A42FC5B8431F3BBE>.

* cited by examiner

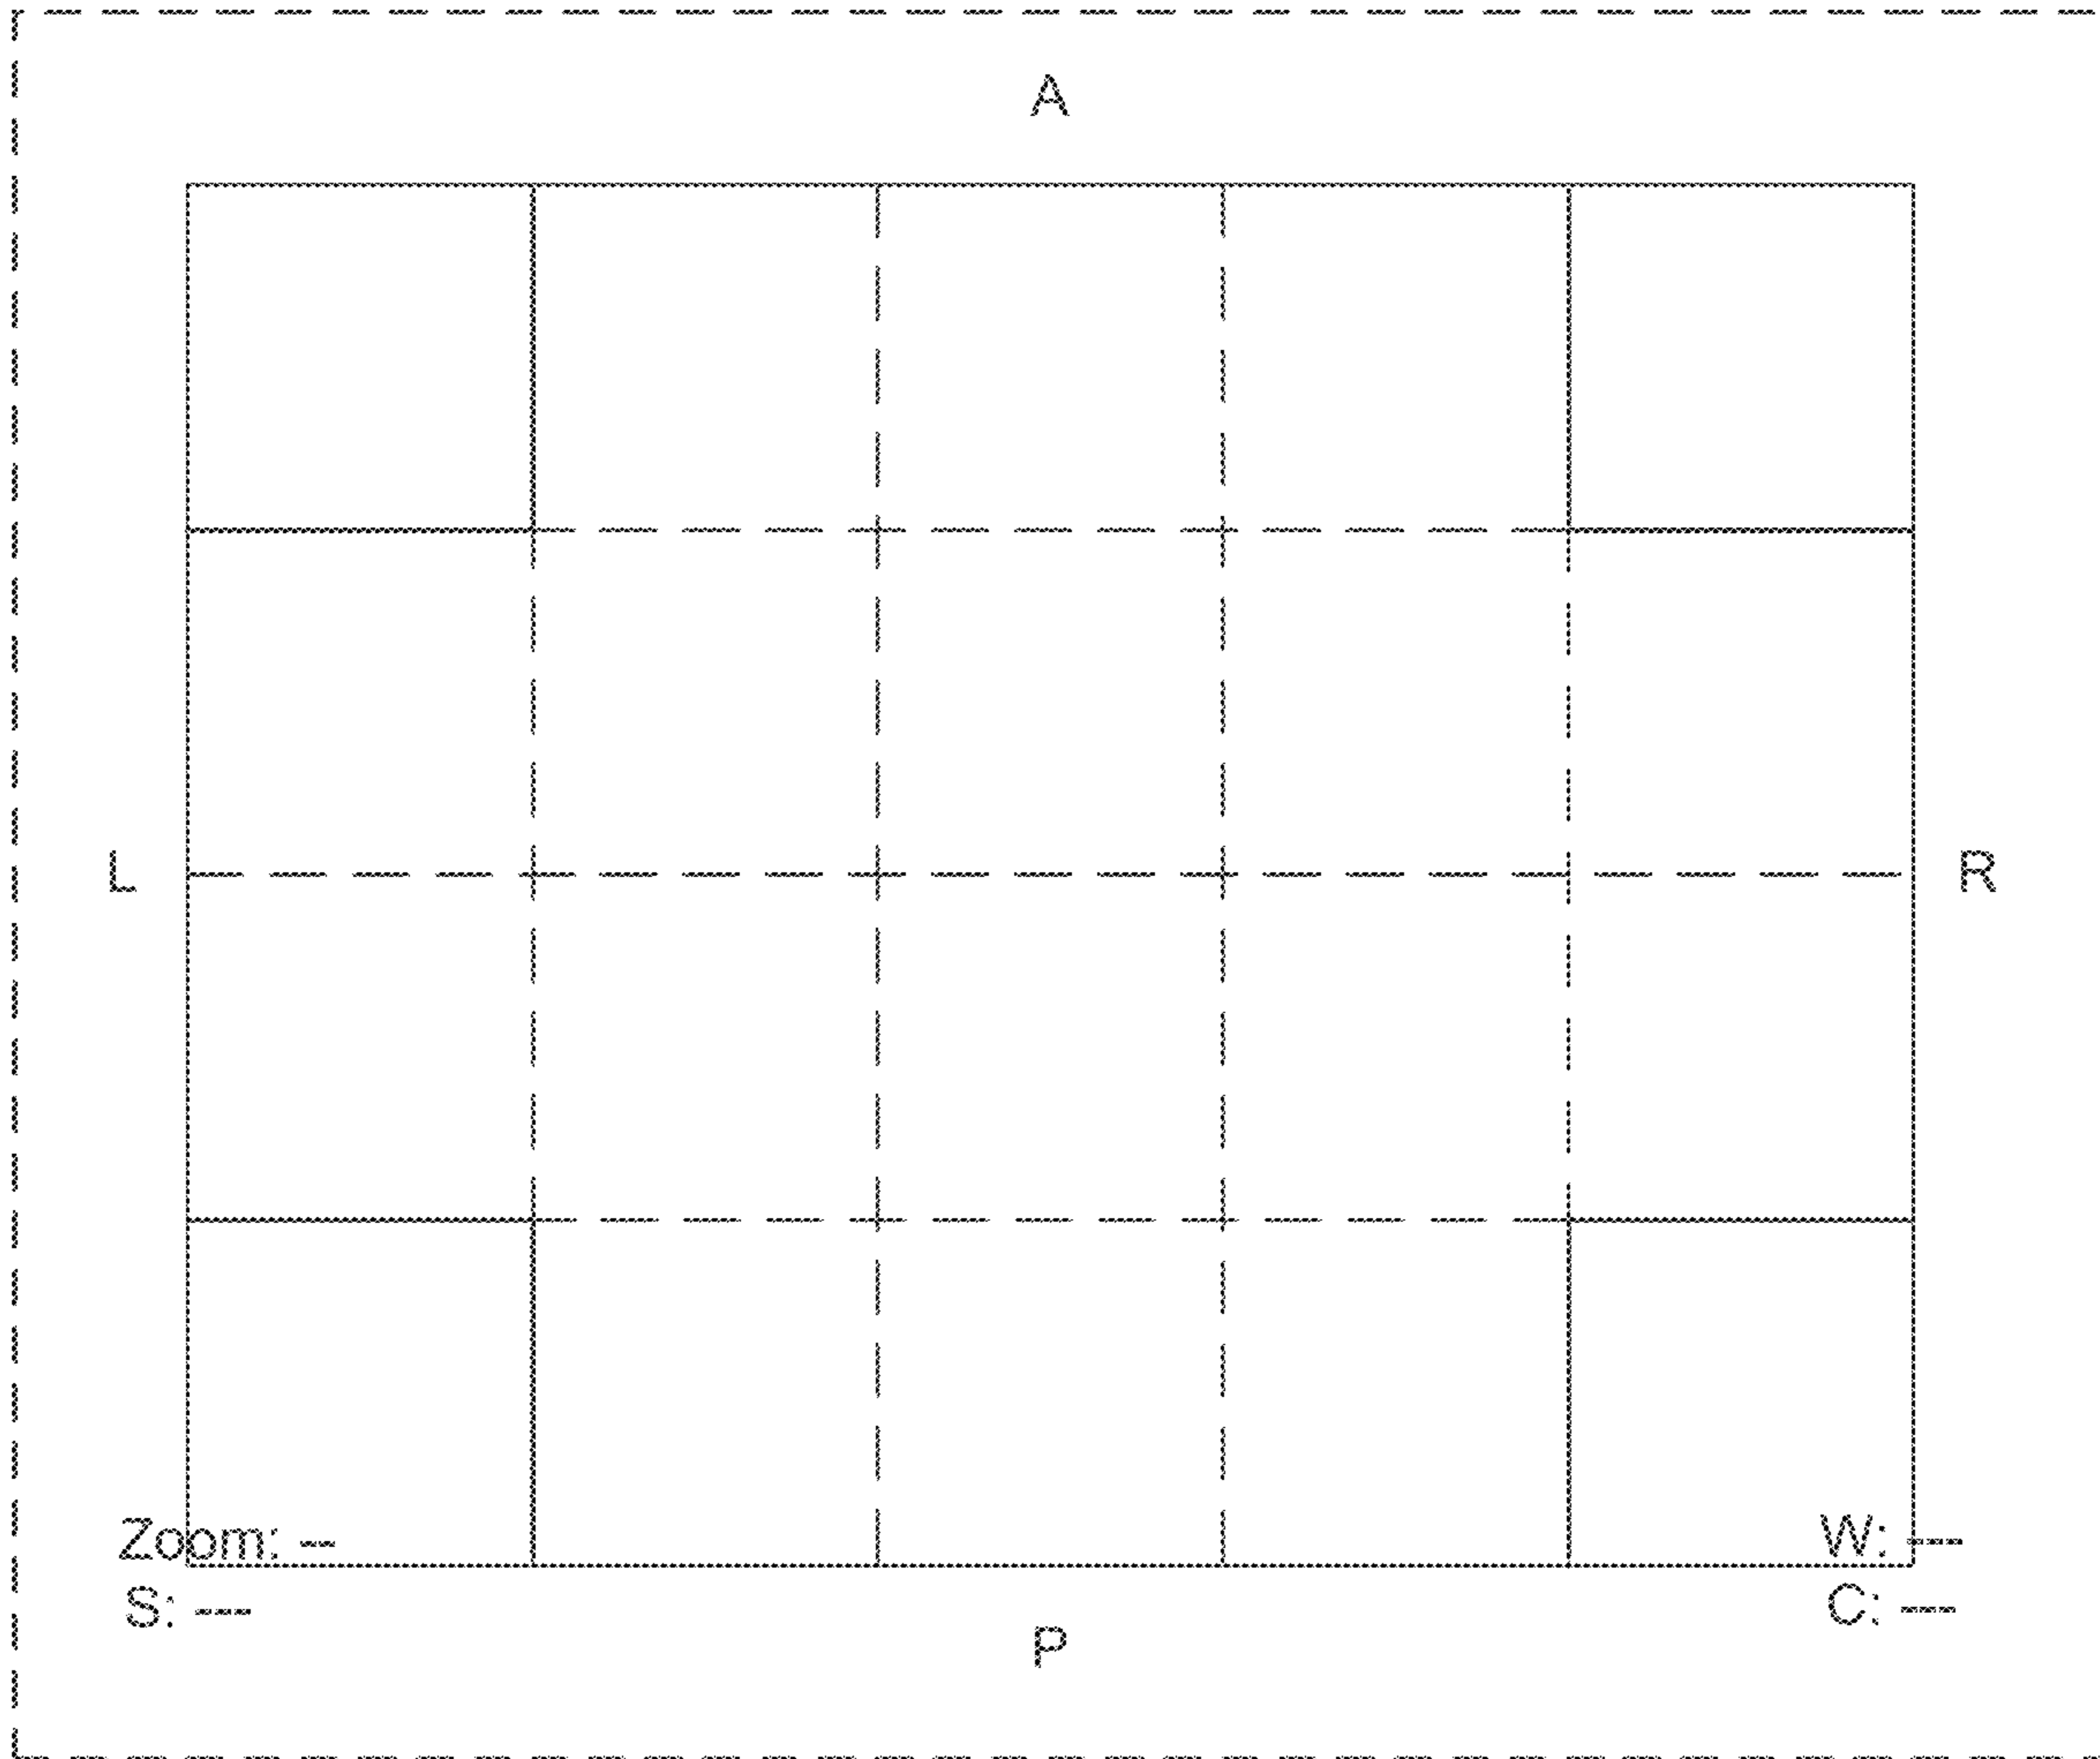

© 2019 GE Precision Healthcare LLC

FIG. 1

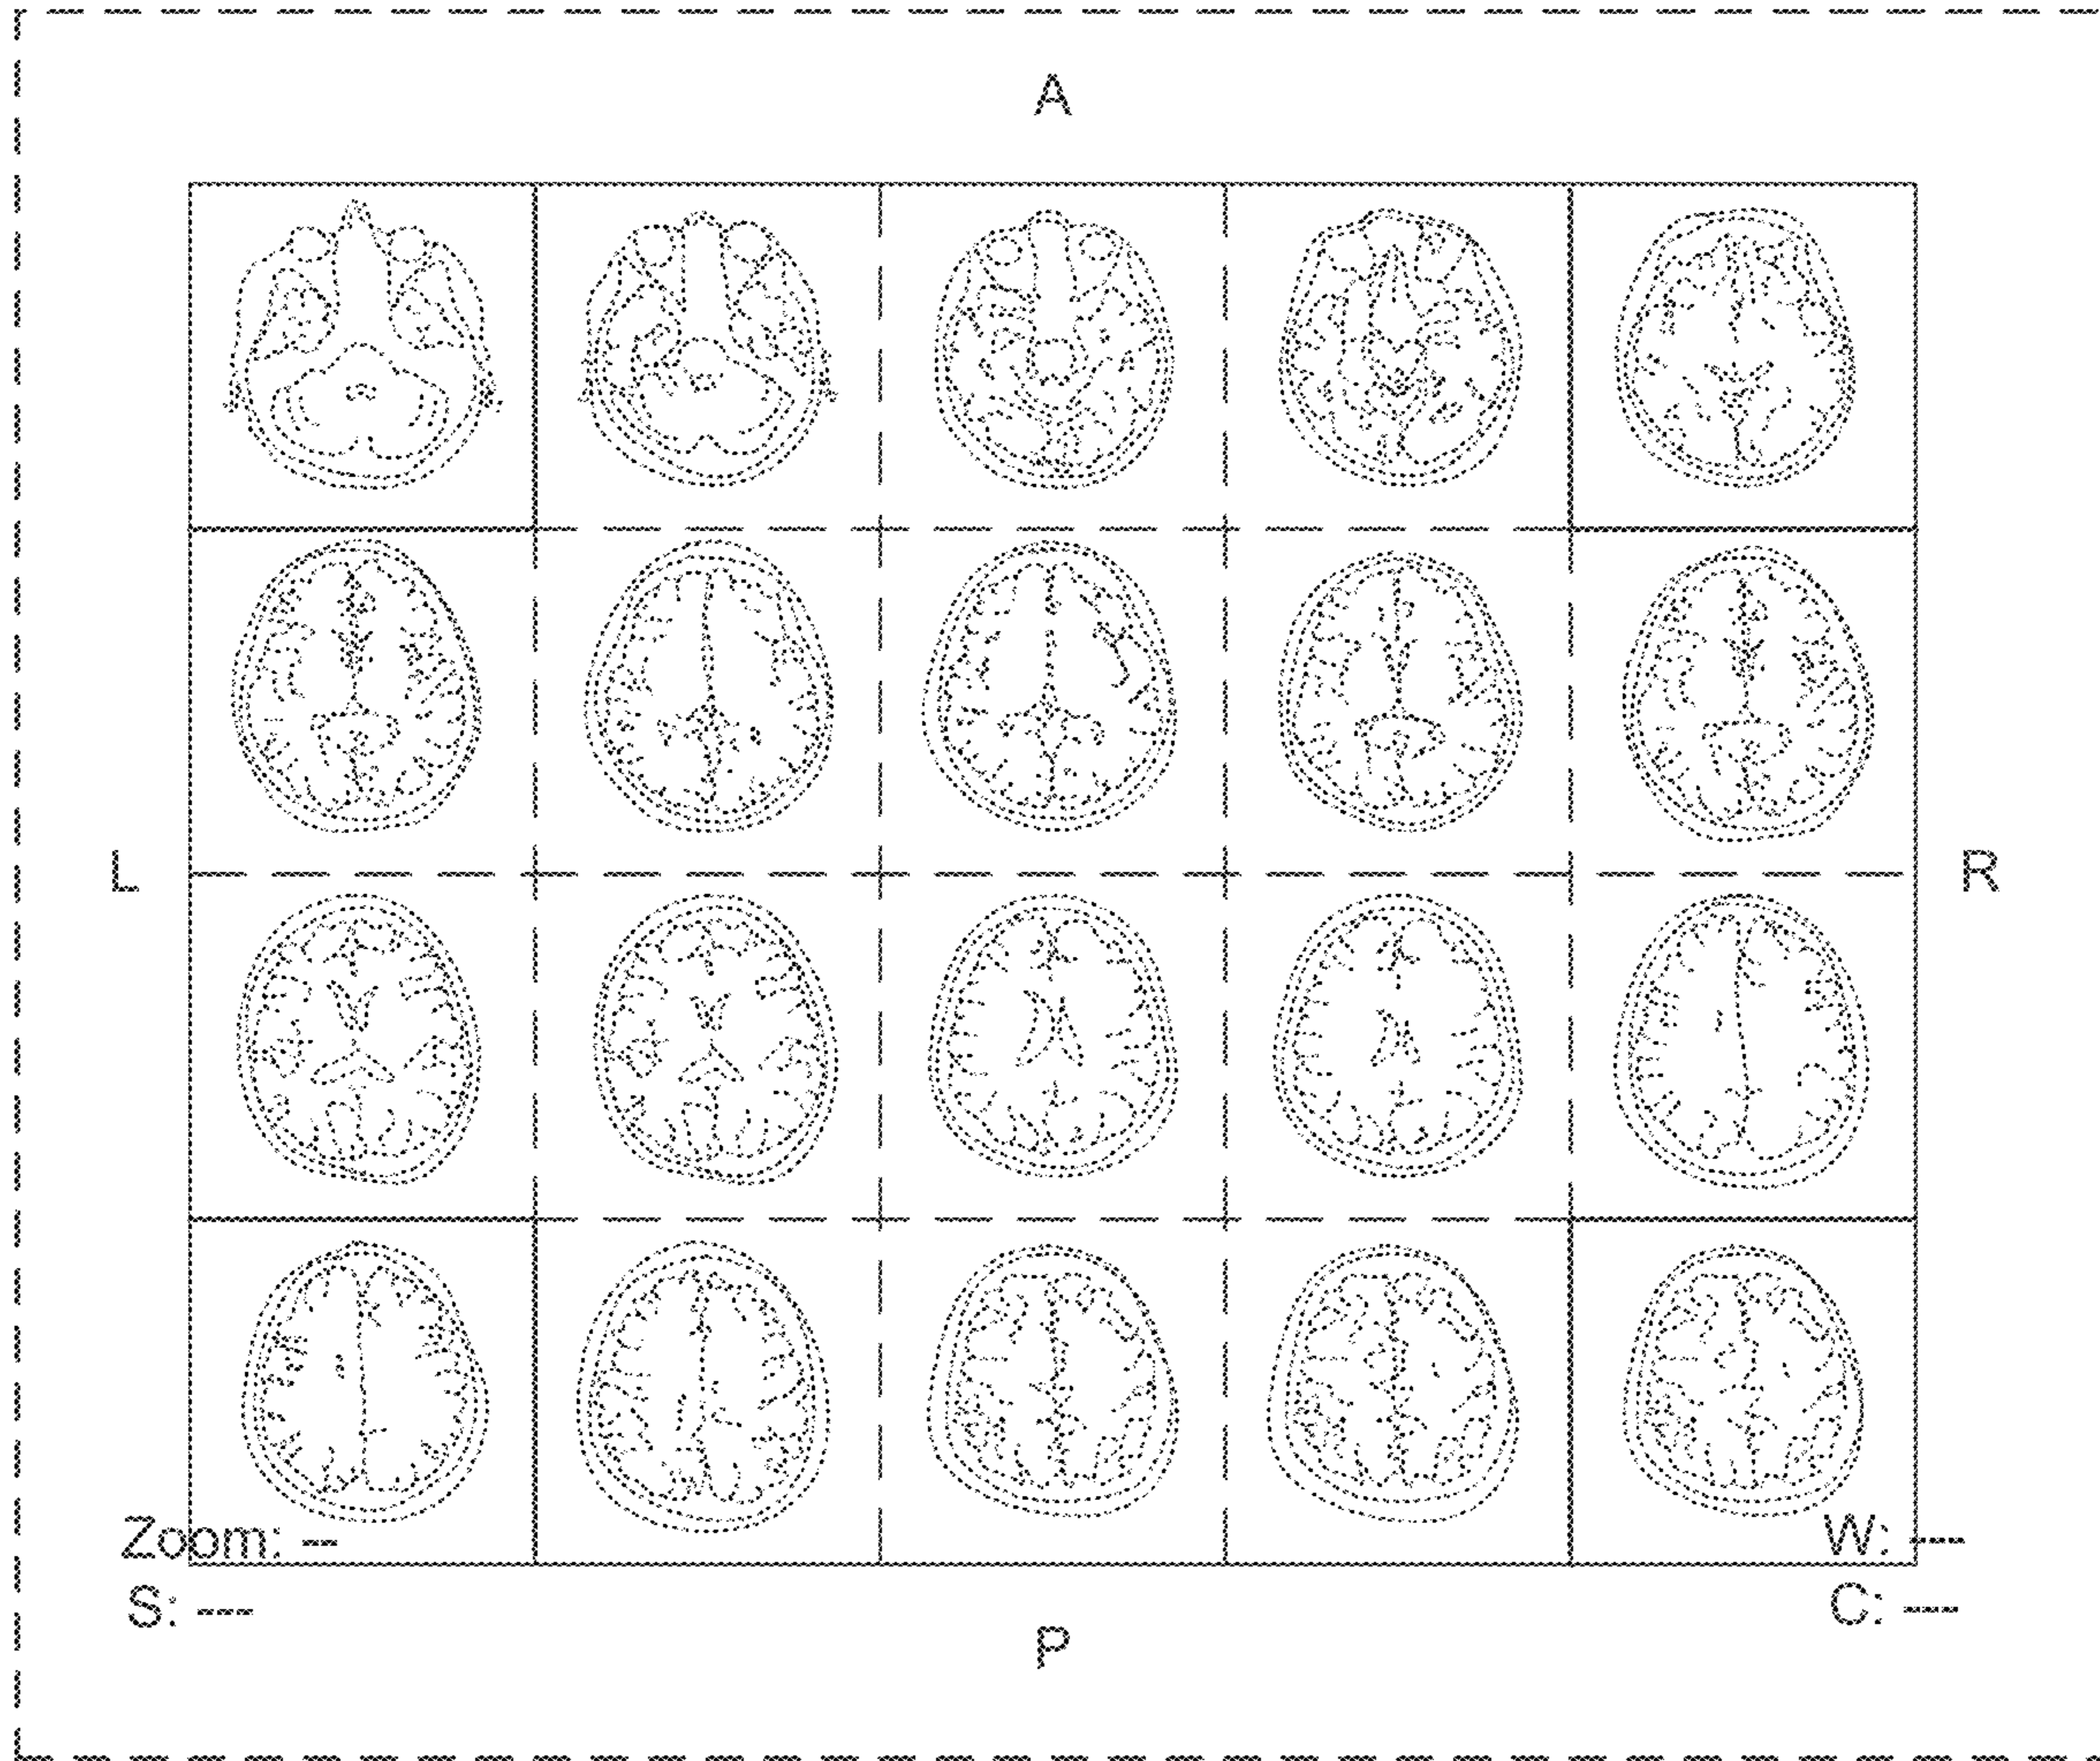

© 2019 GE Precision Healthcare LLC

FIG. 2