



US00D926986S

(12) **United States Design Patent** (10) **Patent No.:** **US D926,986 S**
Roman et al. (45) **Date of Patent:** **** Aug. 3, 2021**

(54) **IMPLANT**

(71) Applicant: **ARROWHEAD MEDICAL DEVICE TECHNOLOGIES, LLC**, Collierville, TN (US)

(72) Inventors: **Scott R. Roman**, Hampton, GA (US); **Thomas J. Twardzik**, Germantown, TN (US)

(73) Assignee: **ARROWHEAD MEDICAL DEVICE TECHNOLOGIES, LLC**, Collierville, TN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/768,505**

(22) Filed: **Jan. 29, 2021**

Related U.S. Application Data

(63) Continuation of application No. 29/637,532, filed on Feb. 20, 2018, now Pat. No. Des. 910,177, which is a continuation of application No. 15/619,831, filed on Jun. 12, 2017, now Pat. No. 9,924,985, which is a continuation of application No. 14/776,066, filed as application No. PCT/US2014/024485 on Mar. 12, 2014, now Pat. No. 9,675,391.

(51) **LOC (13) Cl.** **24-03**

(52) **U.S. Cl.**
USPC **D24/155**

(58) **Field of Classification Search**
USPC D24/155
CPC A61F 6/04; A61F 6/065; A61F 2/4225; A61F 2/4241; A61F 2002/4233; A61F 2002/4235; A61F 2002/4228; A61F 2002/30205; A61F 2002/30224
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,053,035 A 10/1991 McLaren
5,893,850 A 4/1999 Cachia
6,695,499 B2 2/2004 Tormala et al.
6,736,818 B2 5/2004 Perren et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2011130229 10/2011

OTHER PUBLICATIONS

Extended European Search Report issued in European Patent Application 14780322.5 dated Nov. 16, 2016.

(Continued)

Primary Examiner — Charles D Hanson

(74) *Attorney, Agent, or Firm* — Heslin Rothenberg Farley & Mesiti P.C.


(57) **CLAIM**

The ornamental design for an implant, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the implant comprising the new design;
FIG. 2 is a back perspective view of the design of FIG. 1;
FIG. 3 is a right elevational view of the design of FIG. 1, wherein the left elevational view is a mirror image thereof;
FIG. 4 is a top view of the design of FIG. 1, wherein the bottom view is a mirror image thereof;
FIG. 5 is a front elevational view of the design of FIG. 1; and,
FIG. 6 is a back elevational view of the design of FIG. 1. The broken lines shown in the figures are directed to the environment and are for illustrative purposes only; the broken lines form no part of the claimed implant invention. The relatively light uneven broken lines shown in the figures represent contour, not surface decoration.

1 Claim, 3 Drawing Sheets

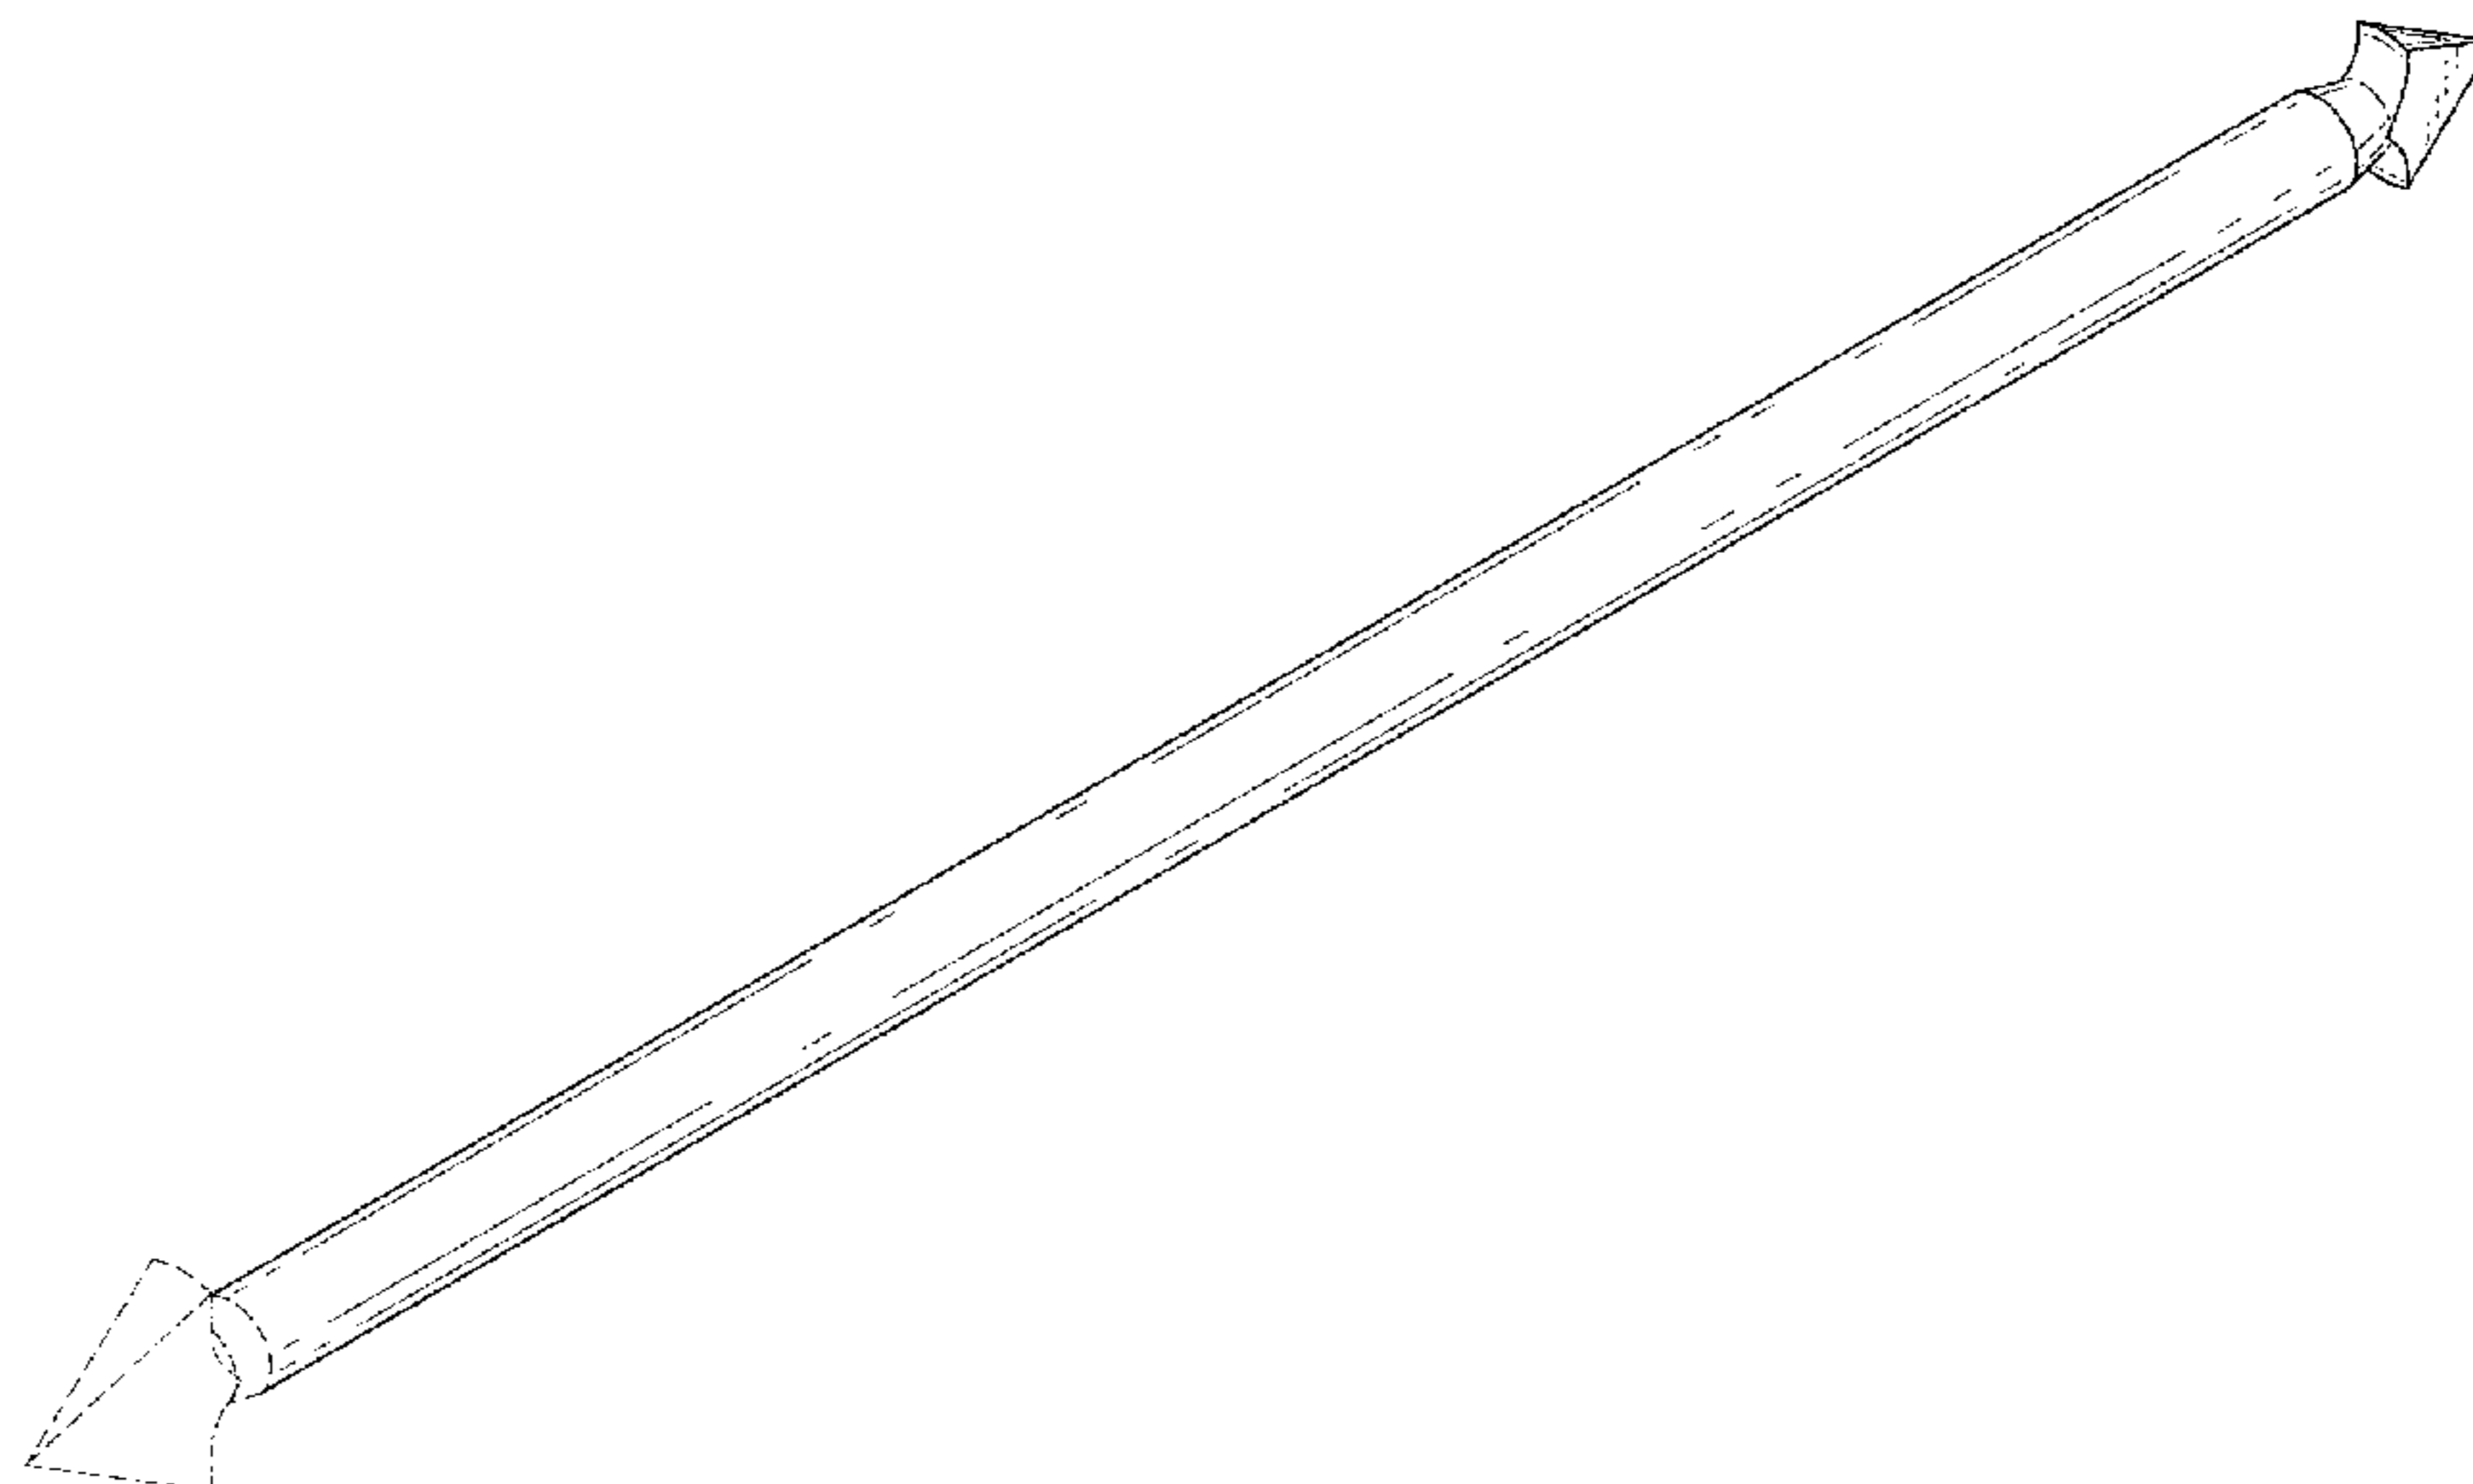

(56)

References Cited

U.S. PATENT DOCUMENTS

9,675,391 B2 6/2017 Roman et al.
 10,080,597 B2* 9/2018 Shemwell A61B 17/7291
 2004/0220574 A1 11/2004 Pelo et al.
 2006/0129153 A1 6/2006 Klaue et al.
 2007/0083202 A1 4/2007 Running et al.
 2008/0132894 A1 6/2008 Coillard-Lavirotte et al.
 2008/0177262 A1 7/2008 Augoyard et al.
 2009/0005782 A1 1/2009 Chirico et al.
 2009/0036893 A1 2/2009 Kartalian et al.
 2010/0324556 A1 12/2010 Tyber et al.
 2011/0172668 A1 7/2011 Frake
 2011/0257652 A1* 10/2011 Roman A61B 17/16
 606/62
 2011/0276099 A1 11/2011 Champagne et al.
 2011/0301652 A1 12/2011 Reed et al.
 2012/0089197 A1 4/2012 Anderson

2014/0276825 A1* 9/2014 Brown A61B 17/88
 606/62
 2014/0276827 A1* 9/2014 Roman A61B 17/7291
 606/64
 2014/0277554 A1* 9/2014 Roman A61B 17/7233
 623/21.19
 2016/0030096 A1 2/2016 Roman et al.
 2018/0168703 A1* 6/2018 Roman A61F 2/4225

OTHER PUBLICATIONS

International Search Report for PCT/US2014/024485 dated Jul. 10, 2014.
 International Search Report and Written Opinion issued for PCT/US2014/022058 dated Jun. 25, 2014.
 International Search Report and Written Opinion issued for PCT/US2014/024599 dated Aug. 3, 2014.

* cited by examiner

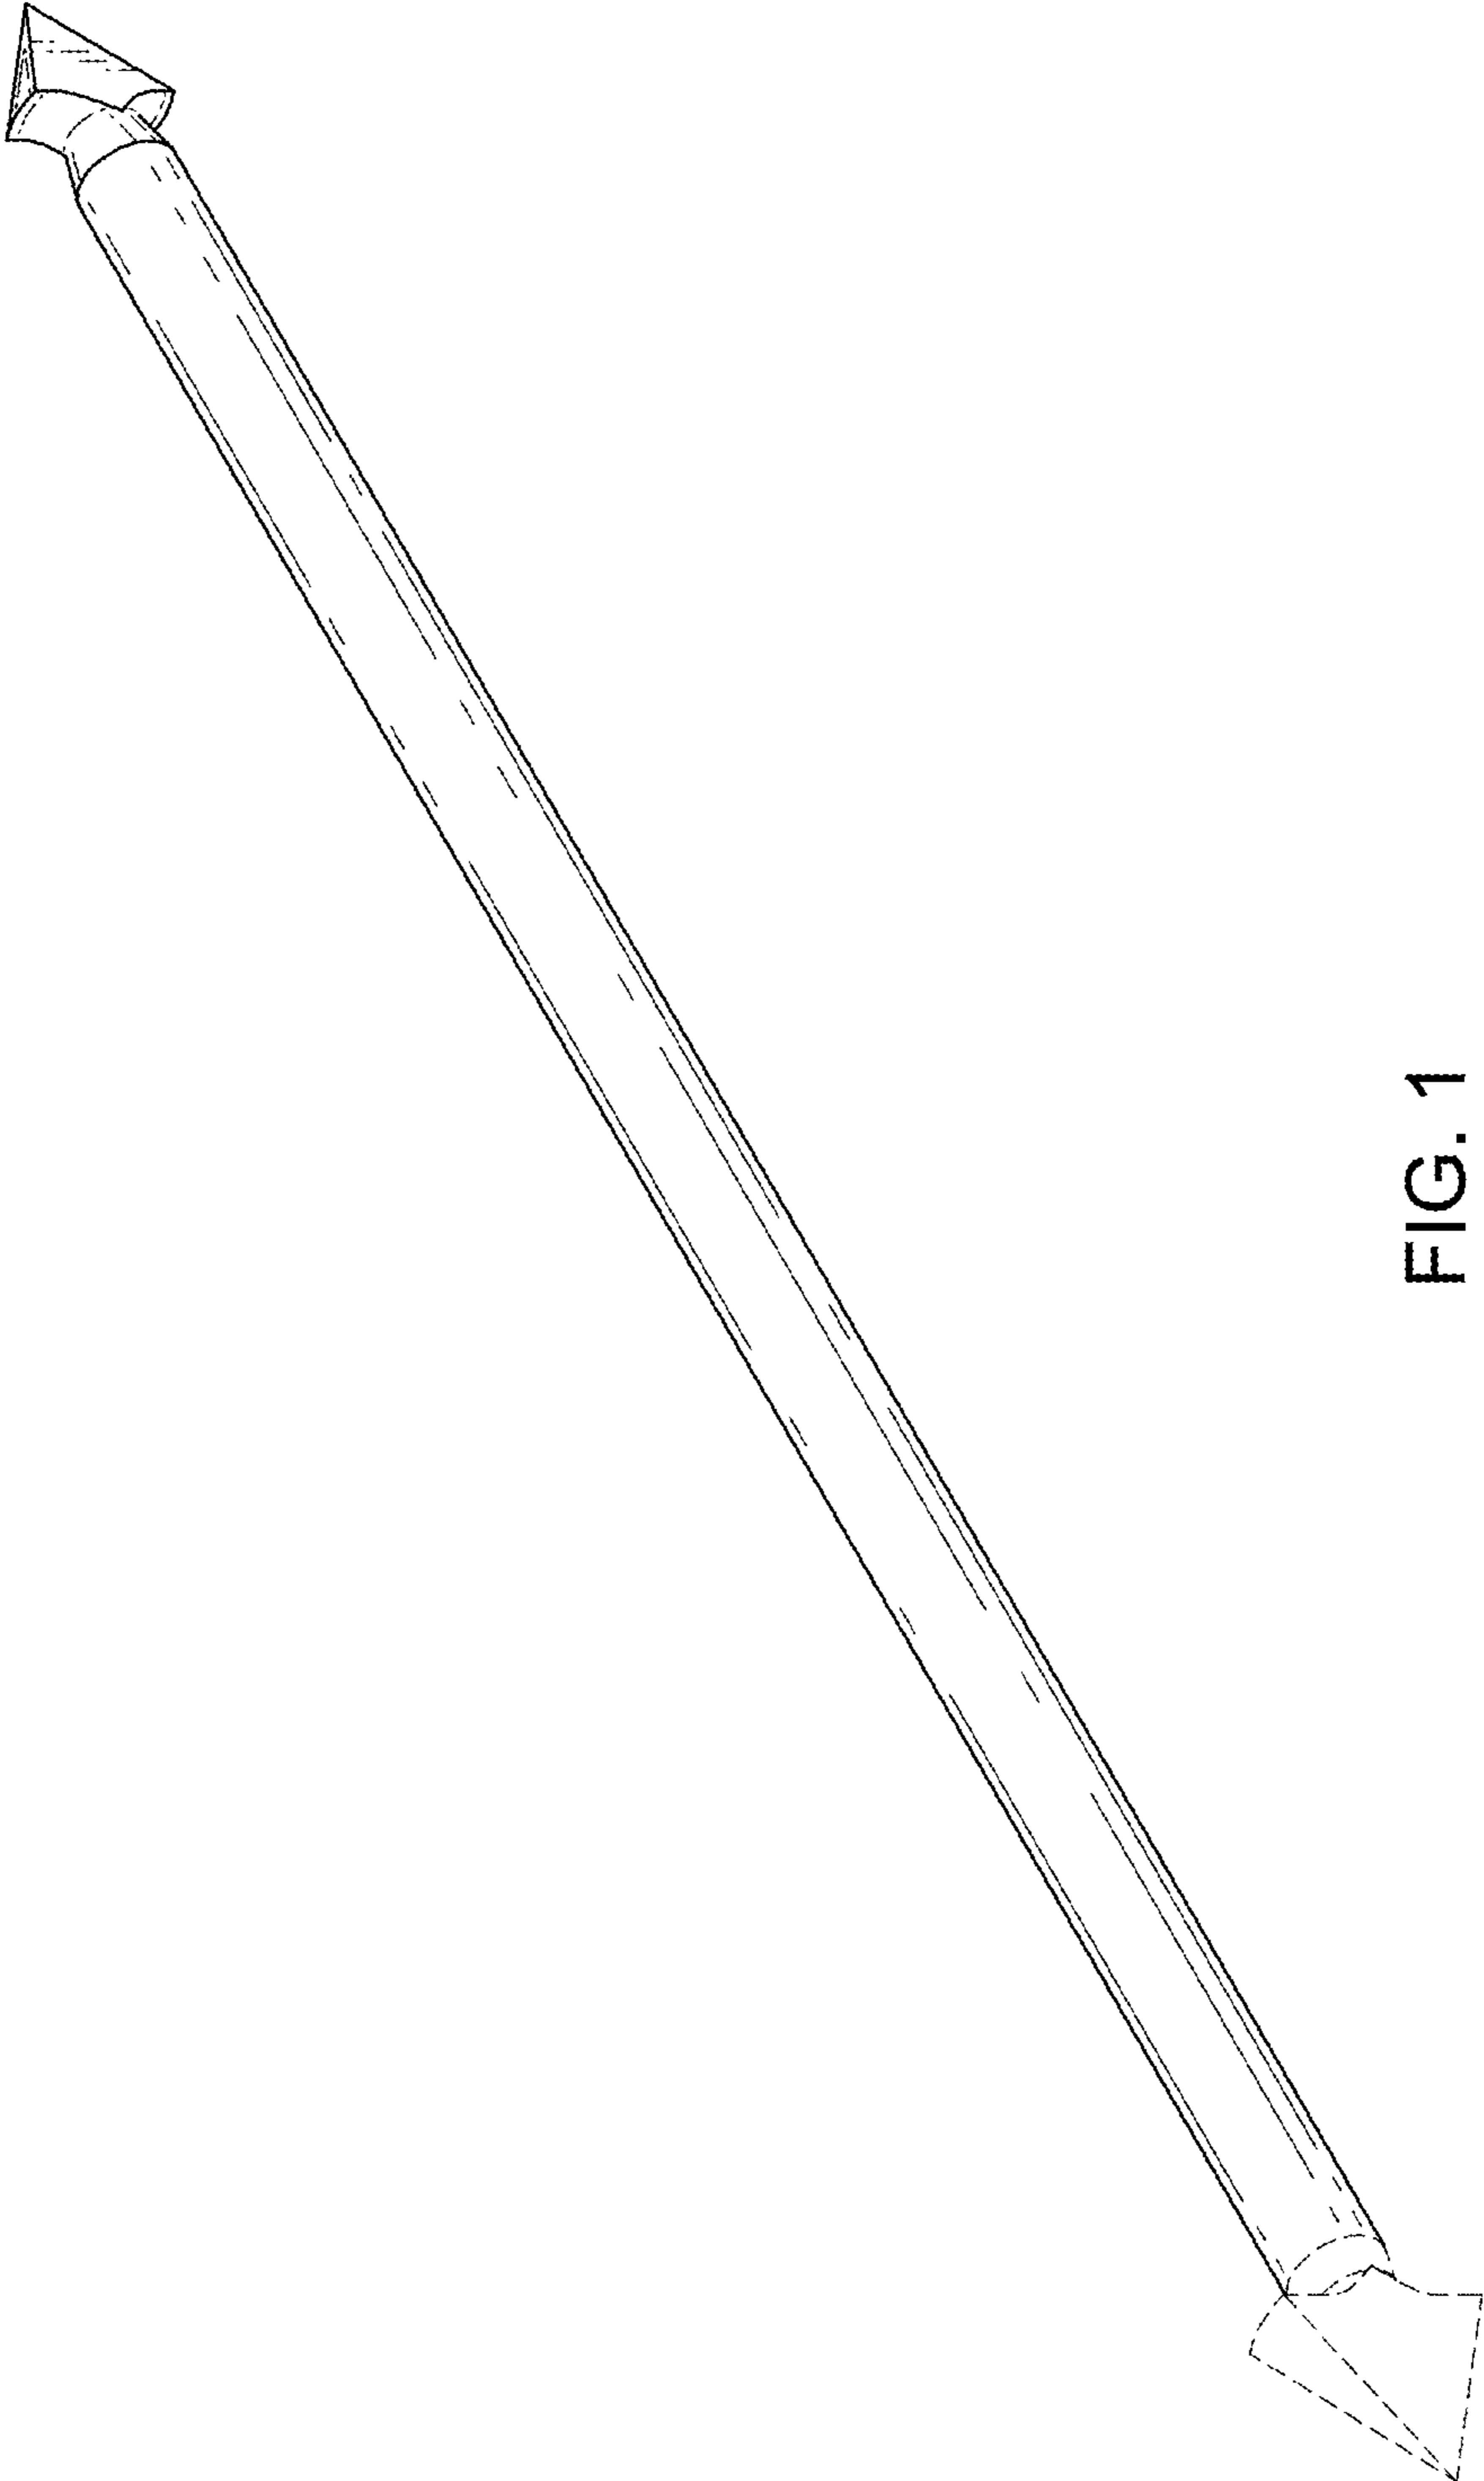


FIG. 1

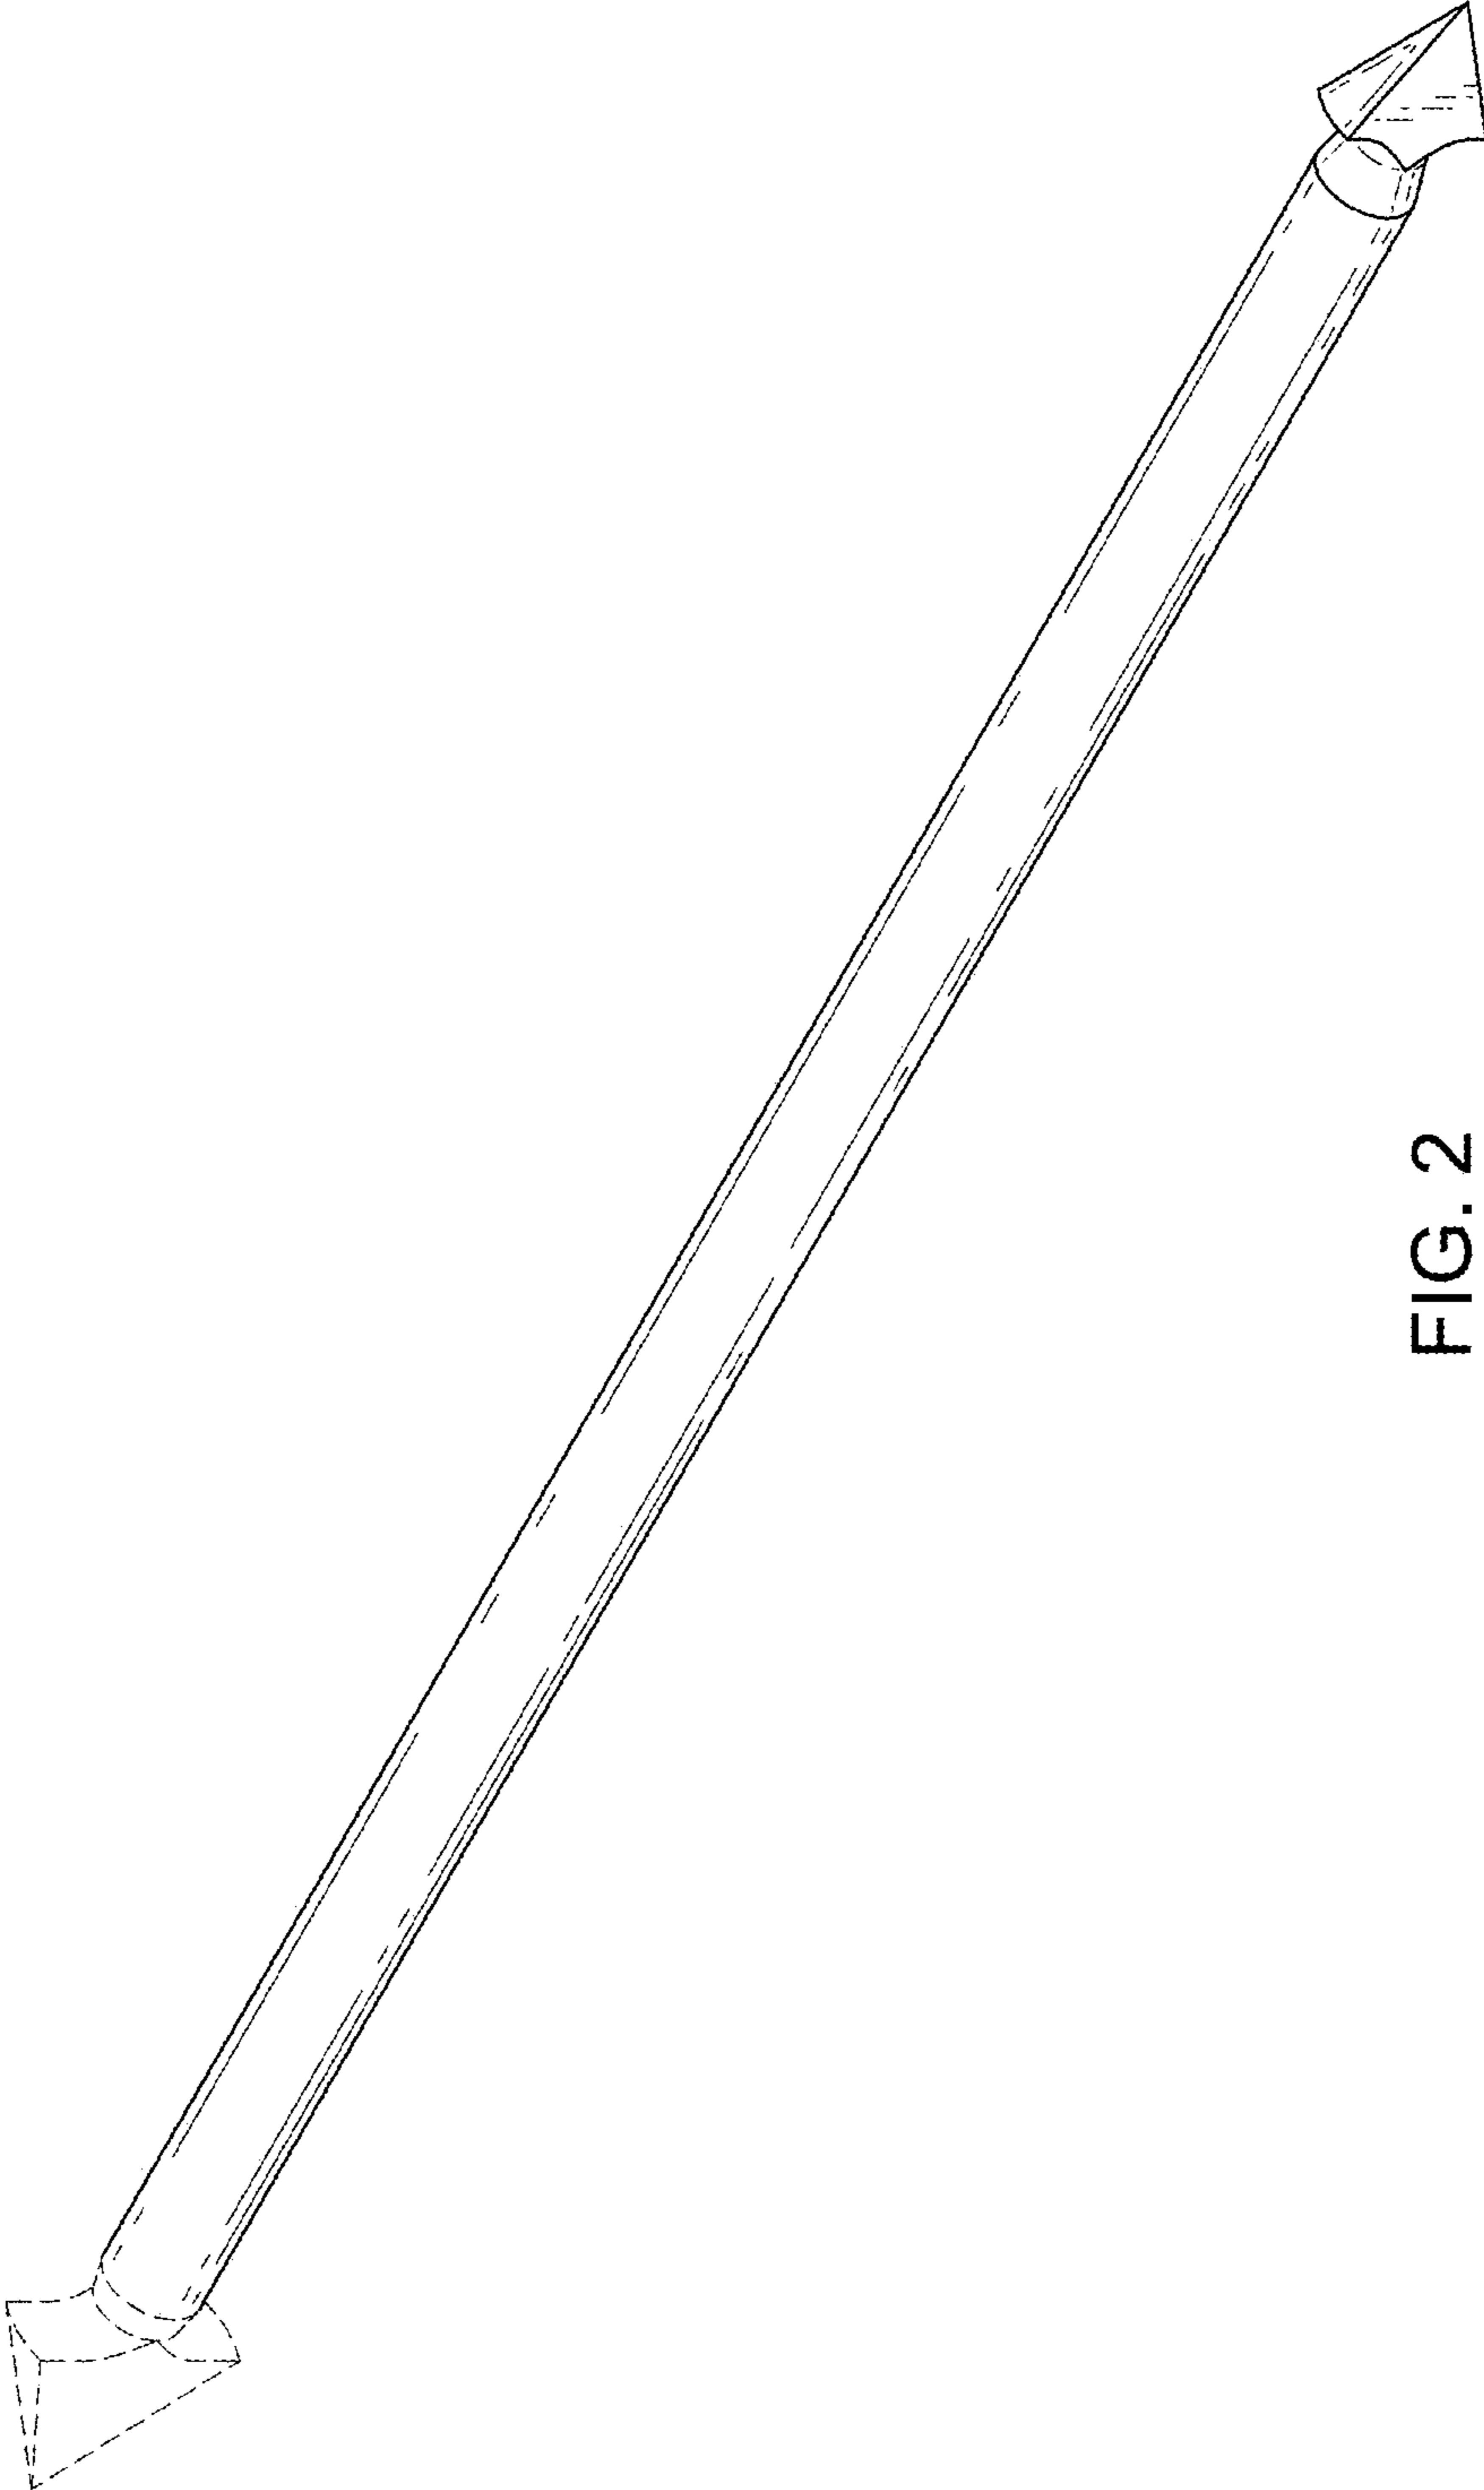


FIG. 2

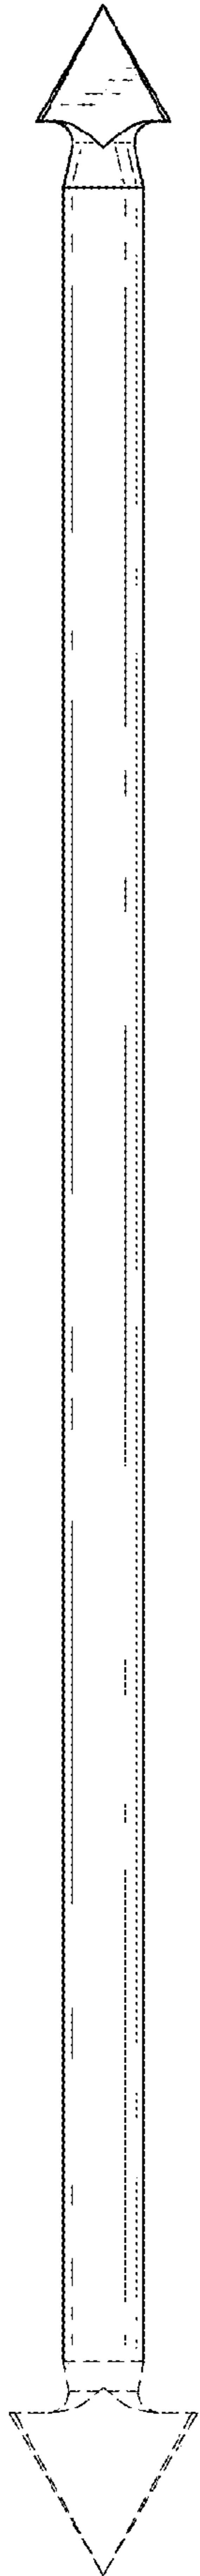


FIG. 3

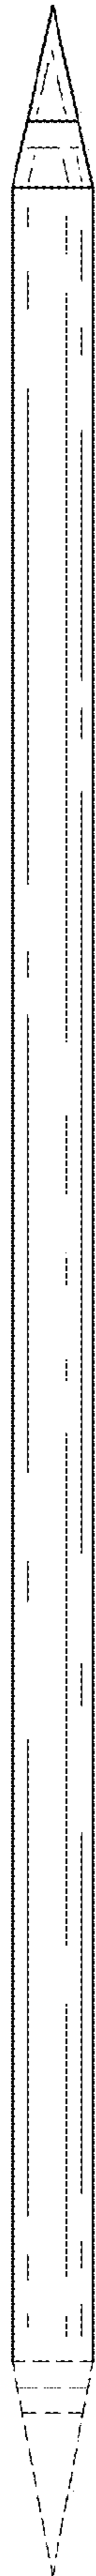


FIG. 4

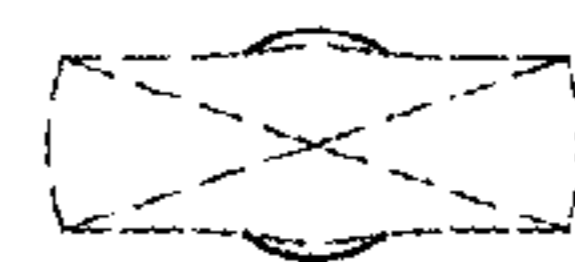


FIG. 5



FIG. 6