



US00D926995S

(12) **United States Design Patent**
He et al.

(10) **Patent No.:** **US D926,995 S**

(45) **Date of Patent:** **** Aug. 3, 2021**

(54) **PATIENT MONITOR**

(71) Applicant: **Shenzhen Mindray Bio-Medical Electronics Co., Ltd.**, Shenzhen (CN)

(72) Inventors: **Lijuan He**, Shenzhen (CN); **Zedong Li**, Shenzhen (CN); **Wenhui Zhou**, Shenzhen (CN); **Huan Zou**, Shenzhen (CN); **Xiang Zhou**, Shenzhen (CN); **Haibo Chai**, Shenzhen (CN)

(73) Assignee: **Shenzhen Mindray Bio-Medical Electronics Co., Ltd.**, Shenzhen (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/762,251**

(22) Filed: **Dec. 15, 2020**

Related U.S. Application Data

(62) Division of application No. 29/656,852, filed on Jul. 17, 2018, now Pat. No. Des. 905,249.

(30) **Foreign Application Priority Data**

Jan. 31, 2018 (CN) 201830046600.0

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/185**

(58) **Field of Classification Search**

USPC D24/185, 186, 177, 108, 216, 107, 160,
D24/165, 232, 167, 200; D14/186, 129;
D23/360; D18/4.6

CPC B25J 15/0028

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D238,887 S * 2/1976 O'Neal et al. D24/232

D281,196 S * 10/1985 Knight D24/167

D330,424 S * 10/1992 Davis D24/160
D340,769 S * 10/1993 Bloom D24/165
D400,249 S * 10/1998 Holubar D24/107
D508,998 S * 8/2005 Ryan D24/200
D552,741 S * 10/2007 Zhou D24/186
D592,754 S 5/2009 Koike
D612,503 S * 3/2010 Johnston D24/186
D624,654 S 9/2010 Shimizu
D649,644 S * 11/2011 Chai D24/167
D680,653 S 4/2013 Fullerton
D682,414 S 5/2013 Chen
D683,034 S 5/2013 Shigeno

(Continued)

OTHER PUBLICATIONS

“Compact Patient Monitor” found on the internet by RMS at:
<http://mindray.sy/patient-monitors/mid-low-acuity/epm-15-12-10/>
reference found Mar. 23, 2021.*

(Continued)

Primary Examiner — Rhea Shields

(74) *Attorney, Agent, or Firm* — Kory D. Christensen

(57) **CLAIM**

We claim the ornamental design for a patient monitor, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a patient monitor, showing our new design;

FIG. 2 is a rear perspective view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof;


FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

Broken lines are for illustrating unclaimed portions of the patient monitor; the broken lines form no part of the claimed design.

1 Claim, 6 Drawing Sheets

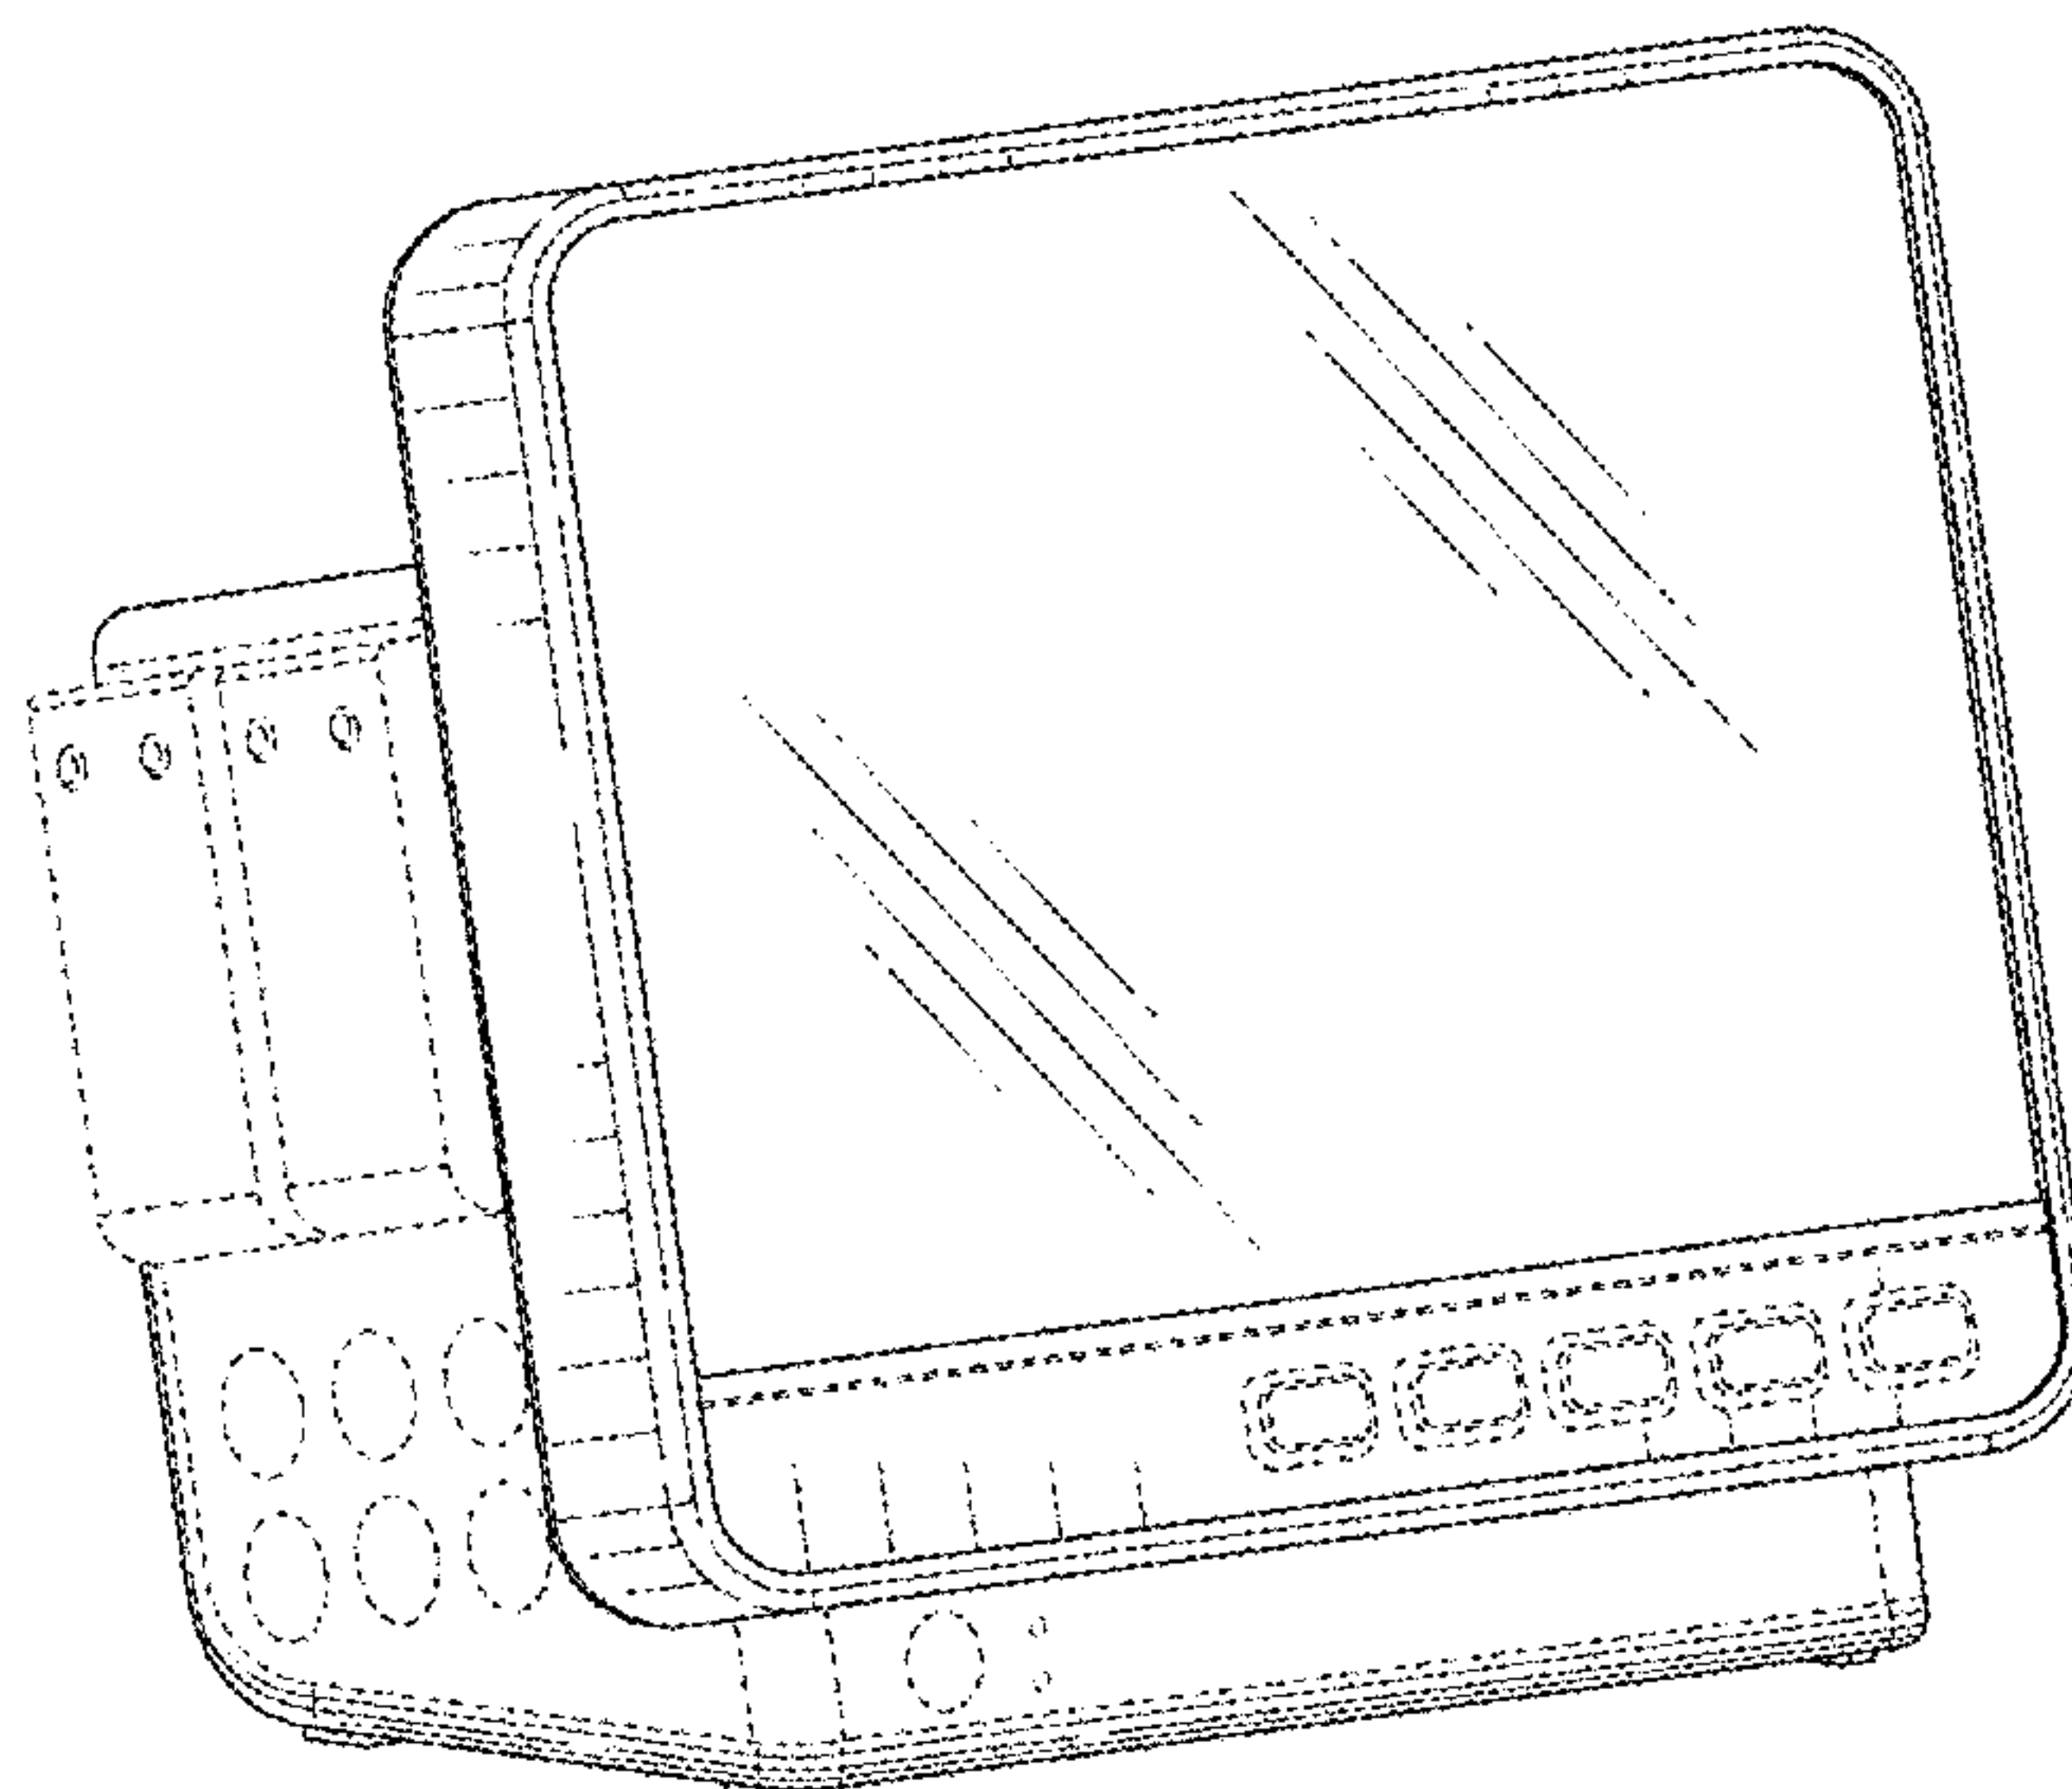

(56)

References Cited

U.S. PATENT DOCUMENTS

D690,293 S 9/2013 Wilson
 D697,214 S * 1/2014 Rosenfeldt D24/186
 D706,239 S * 6/2014 Chen D14/186
 D711,003 S * 8/2014 Chen D24/186
 D717,446 S * 11/2014 Lu D24/167
 D724,737 S 3/2015 Kawamura
 D734,475 S 7/2015 Ross
 D734,858 S * 7/2015 Weichert D24/186
 D739,031 S 9/2015 Golden
 D800,108 S 10/2017 Chen
 D801,519 S 10/2017 Sabin
 D802,768 S 11/2017 Rider
 D822,214 S 7/2018 Iles
 D827,859 S 9/2018 Mathers
 D834,724 S 11/2018 Mathers
 D835,100 S 12/2018 Zhan
 D861,147 S * 9/2019 He D23/360
 D868,957 S 12/2019 Chase
 D871,604 S 12/2019 Rein
 D874,017 S * 1/2020 Jenoski D24/216
 D877,925 S 3/2020 Tanaka
 D878,619 S * 3/2020 Tanaka D24/216
 D879,059 S 3/2020 Saito

D882,802 S 4/2020 Remedios
 D887,559 S * 6/2020 Esfandiari D24/186
 D890,345 S 7/2020 Mathers
 D890,351 S 7/2020 Sung
 D891,607 S * 7/2020 Bjelovuk D24/108
 D895,122 S * 9/2020 Benedikter D24/177
 D902,412 S * 11/2020 Angeles D24/185
 D905,249 S * 12/2020 He D24/185
 D908,893 S * 1/2021 Xia D24/186
 D909,469 S * 2/2021 Watanabe D18/4.6
 D909,589 S * 2/2021 Kohno D24/186
 D912,639 S * 3/2021 Chang D14/129
 D913,505 S * 3/2021 Henderson D24/186
 D913,519 S * 3/2021 Raghu D24/216
 2015/0374571 A1 12/2015 Denson
 2019/0254614 A1 8/2019 Remedios
 2020/0360102 A1 * 11/2020 Lu B25J 15/0028

OTHER PUBLICATIONS

“Patient Monitor” found on the internet by RMS at: <https://concordiamyanmar.com/shop/default-products/medical-product/patient-monitor-system/patient-monitors/epm-10-12-15/> reference found Mar. 23, 2021.*

* cited by examiner

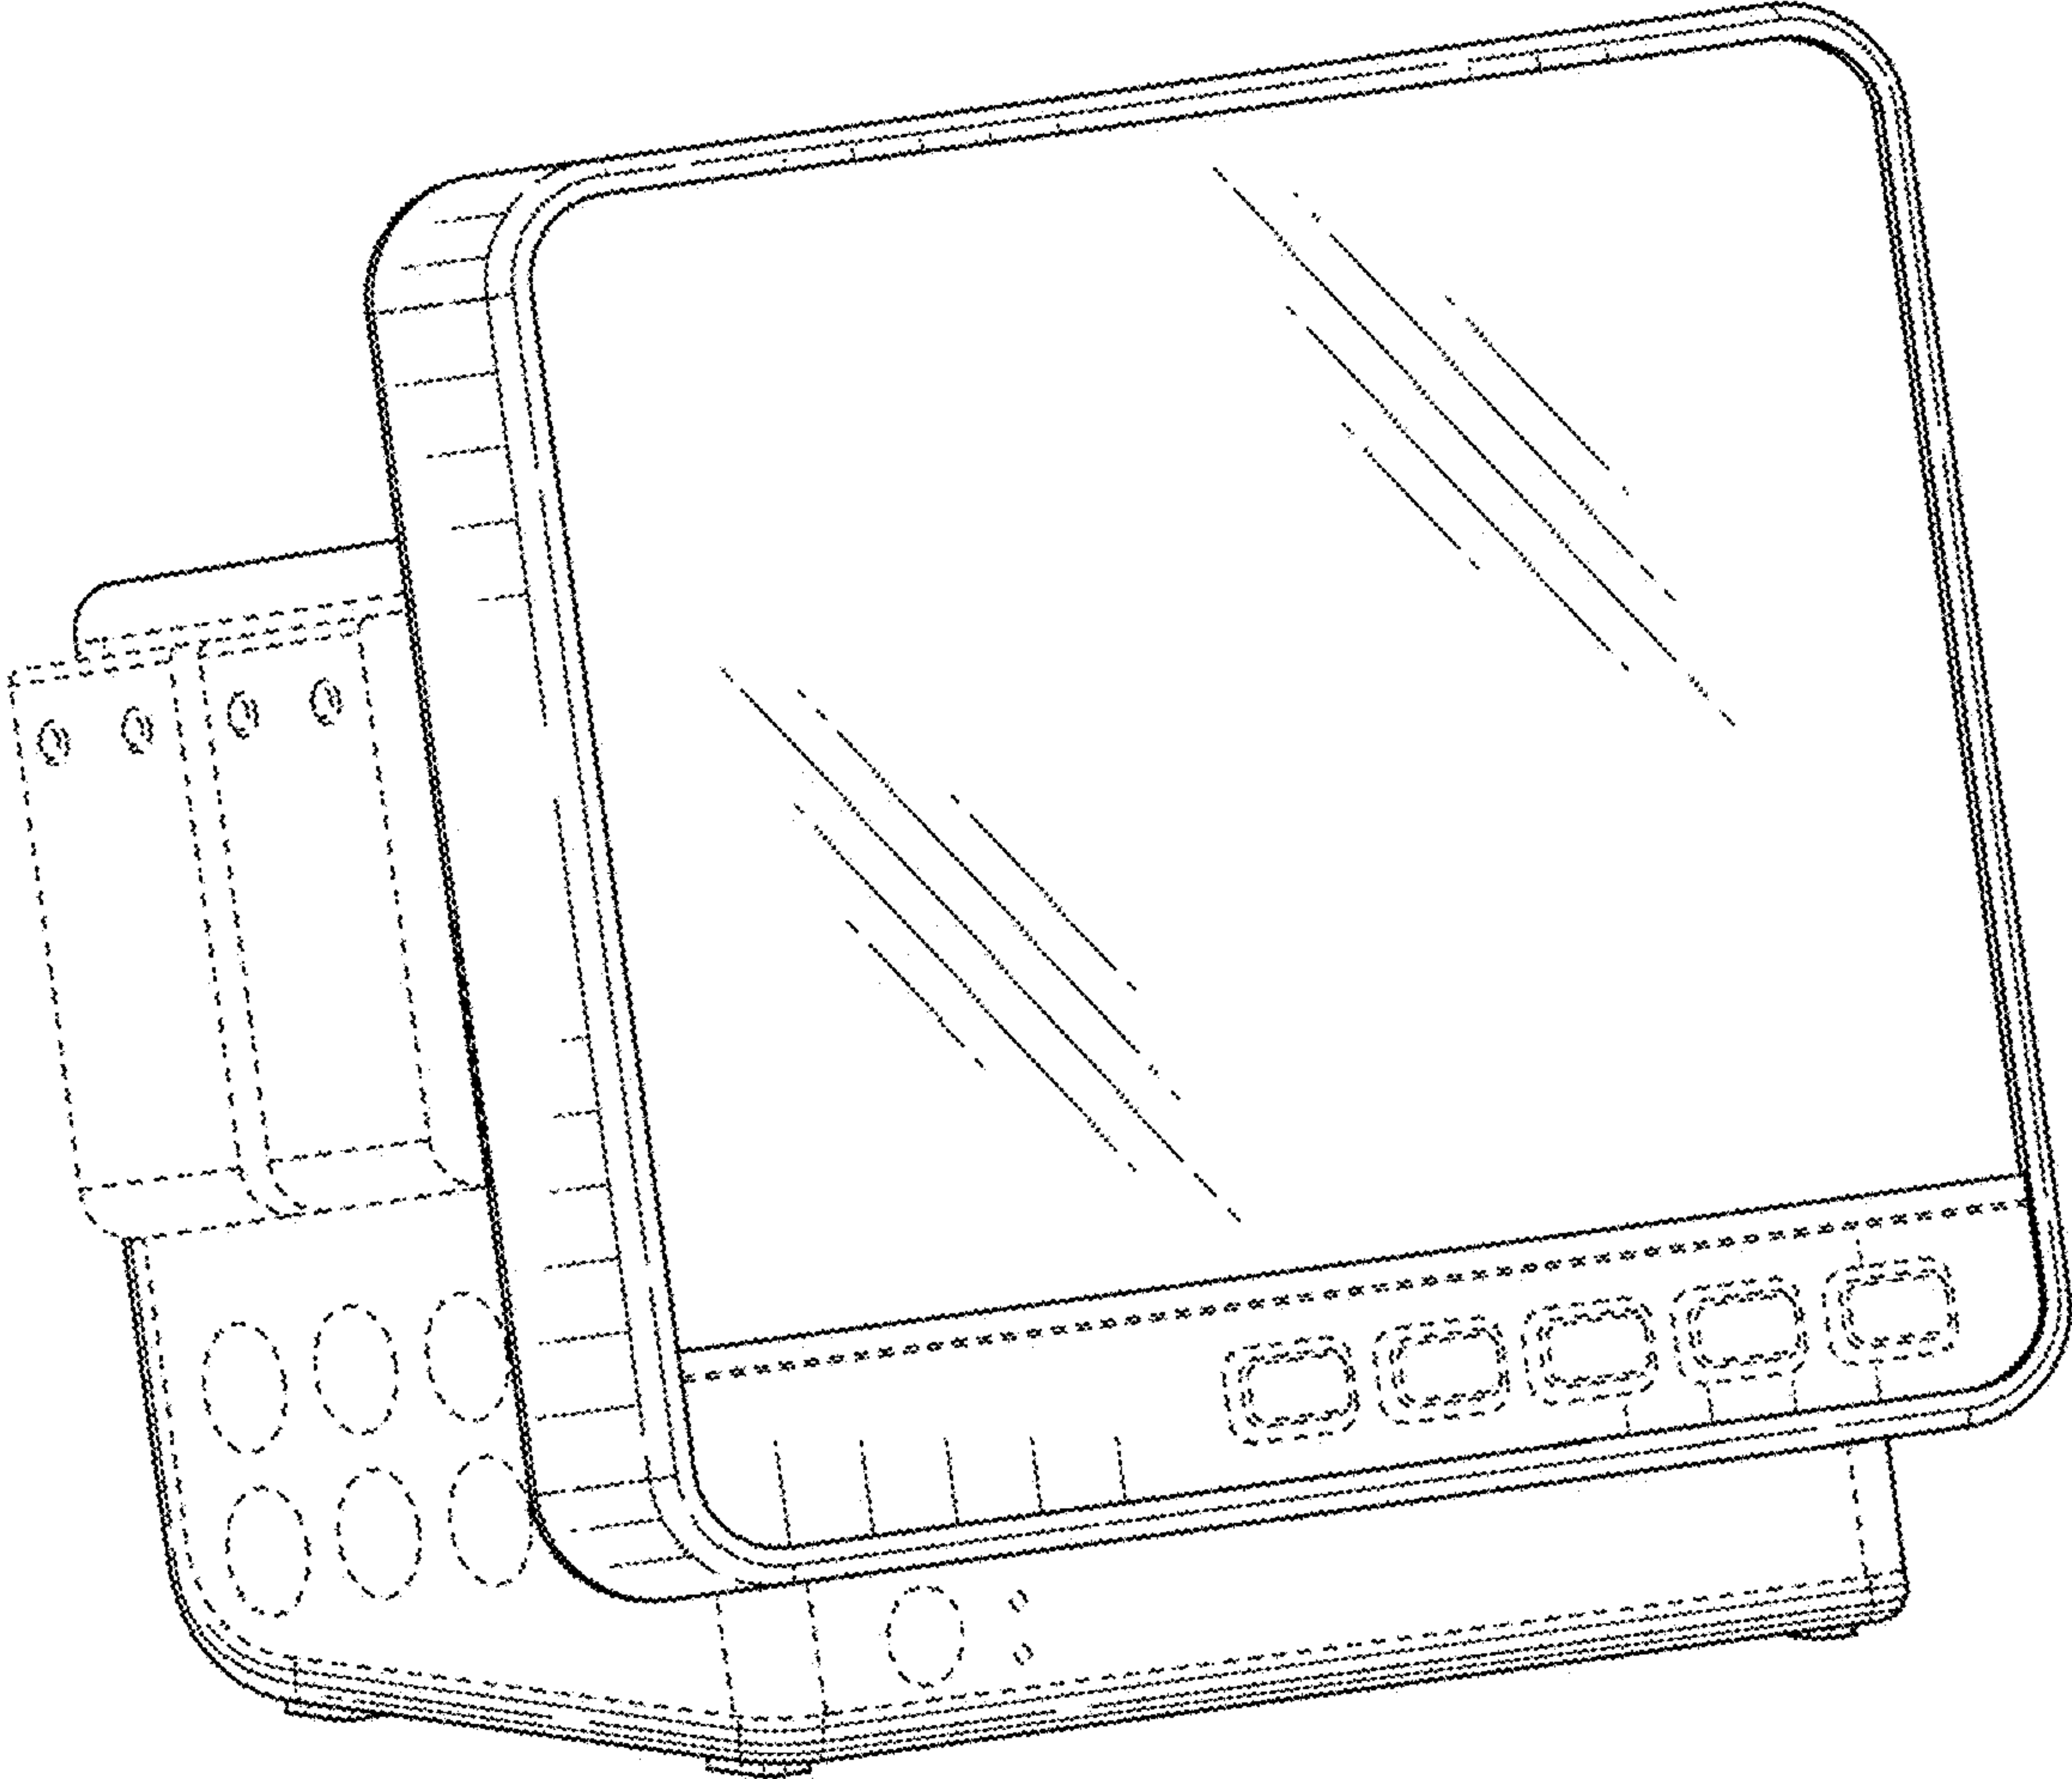


FIG. 1

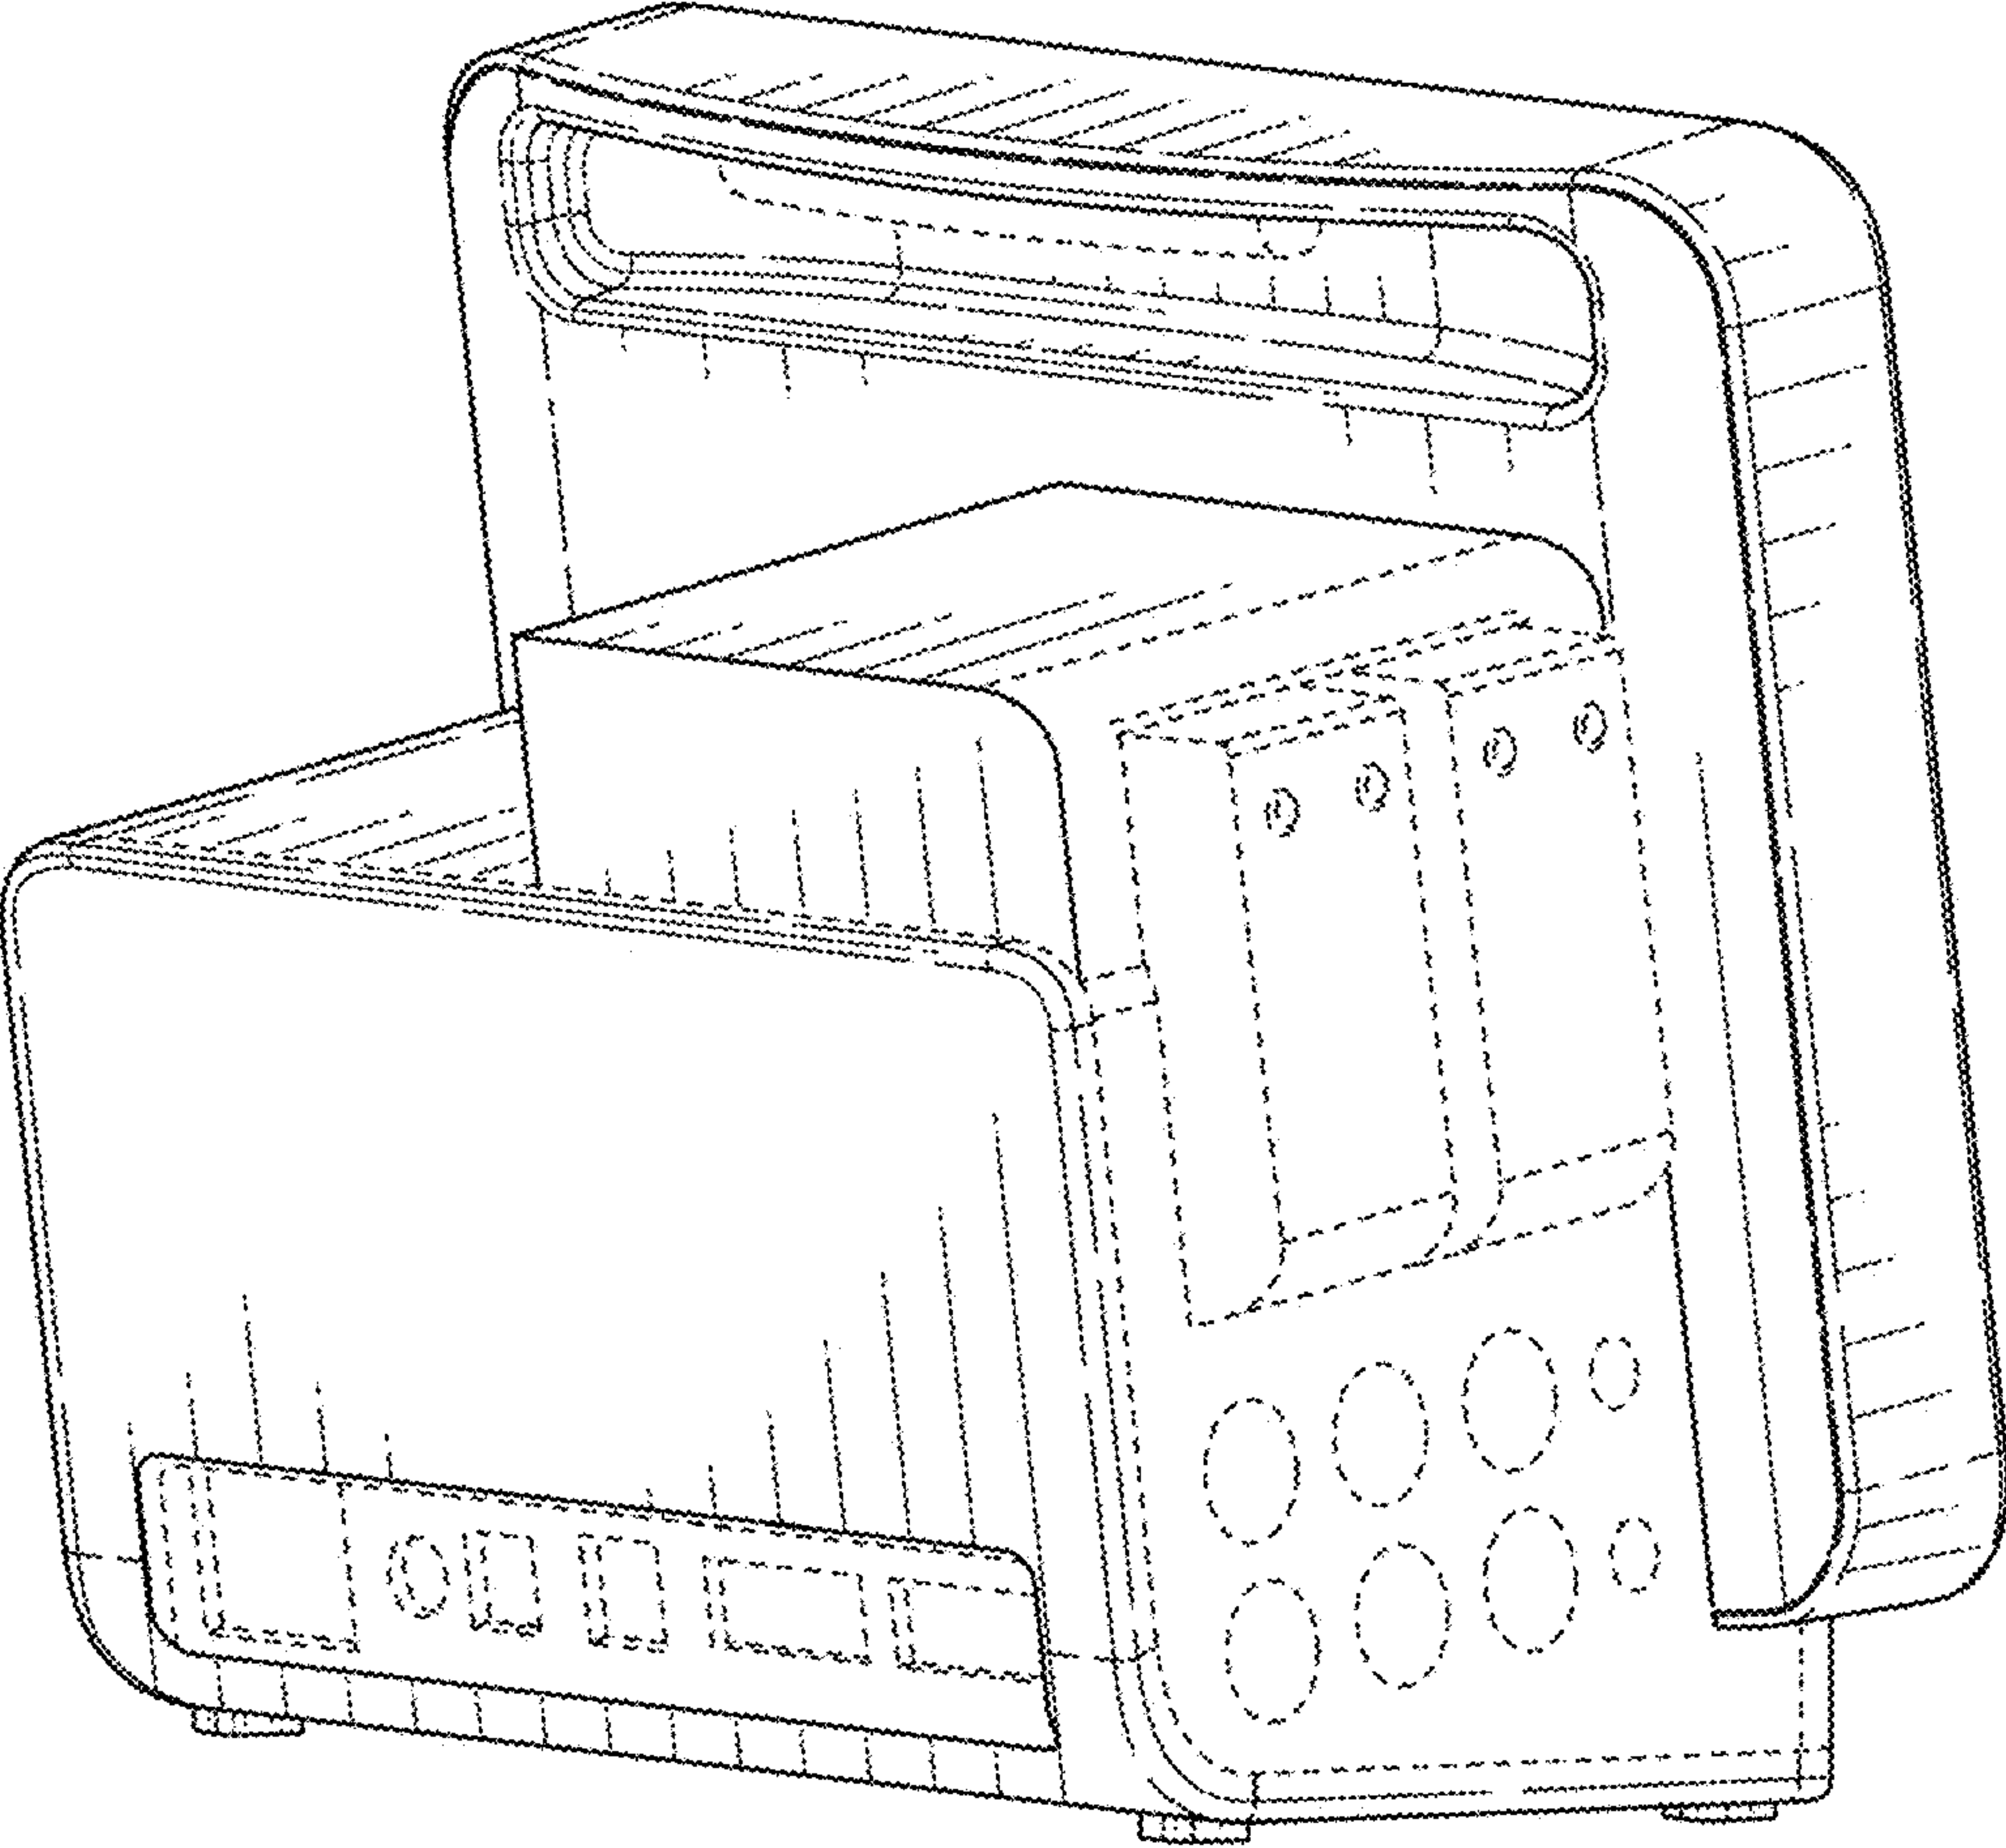


FIG. 2

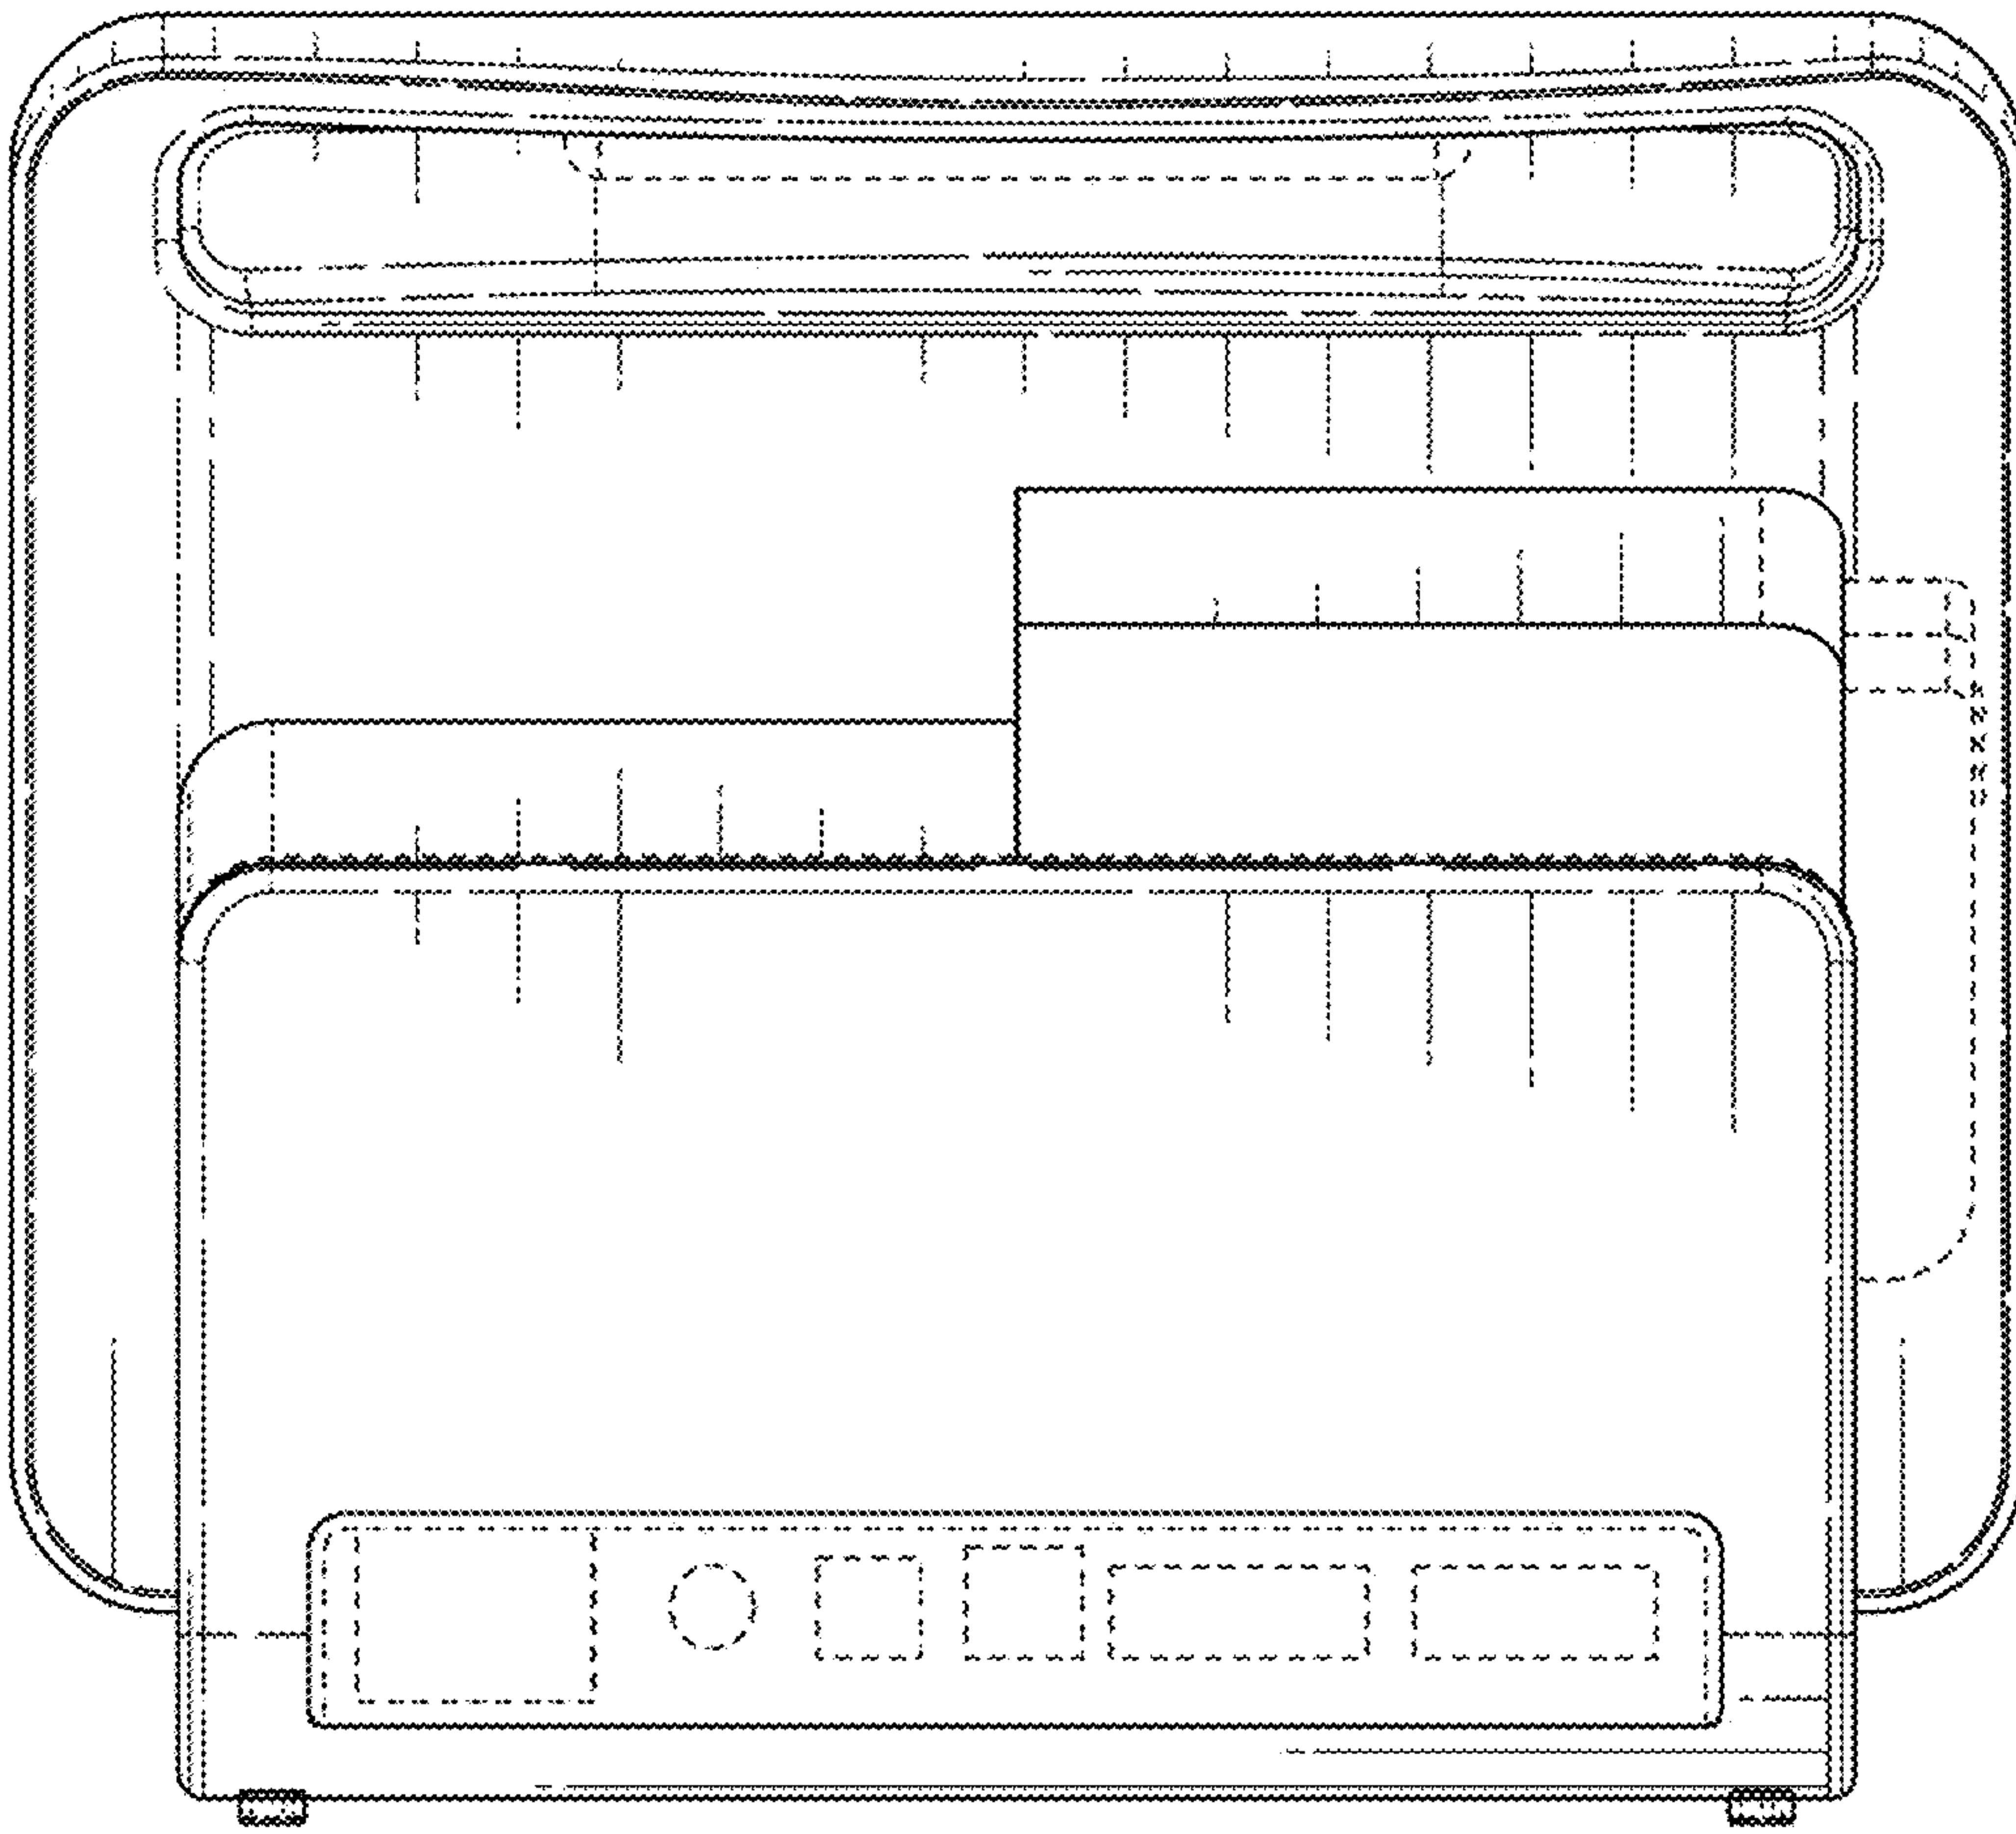


FIG. 3

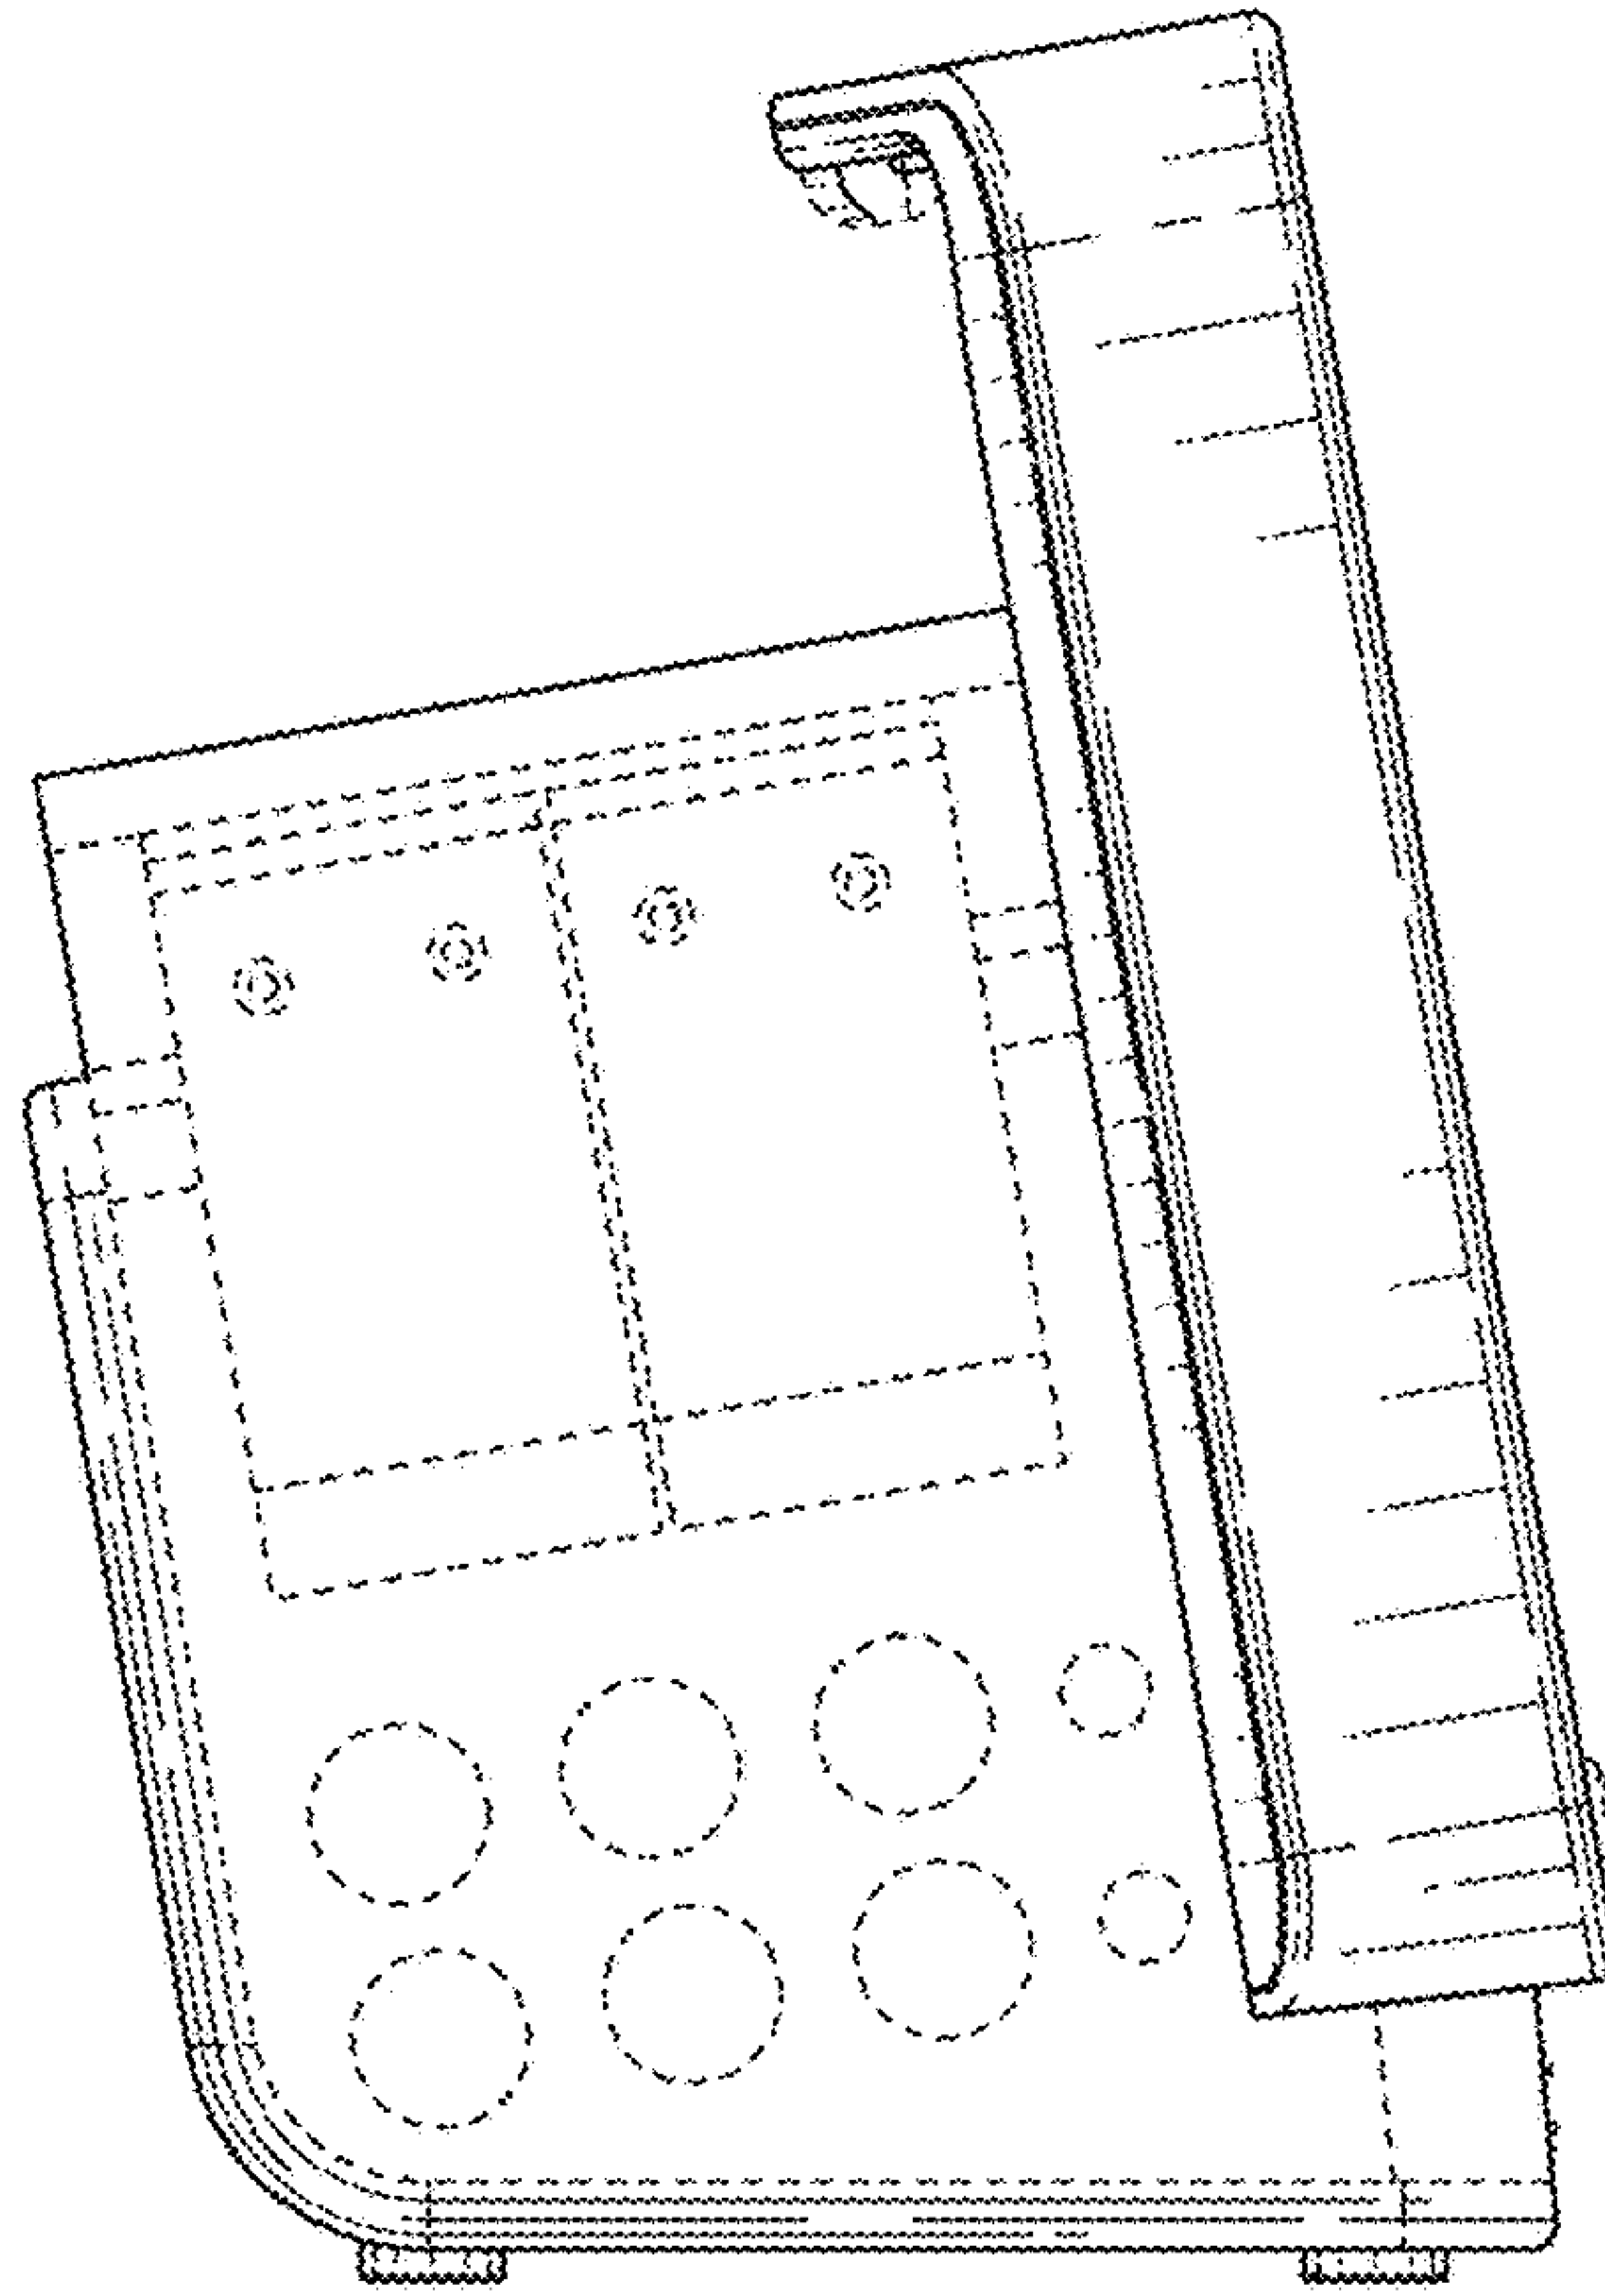


FIG. 4

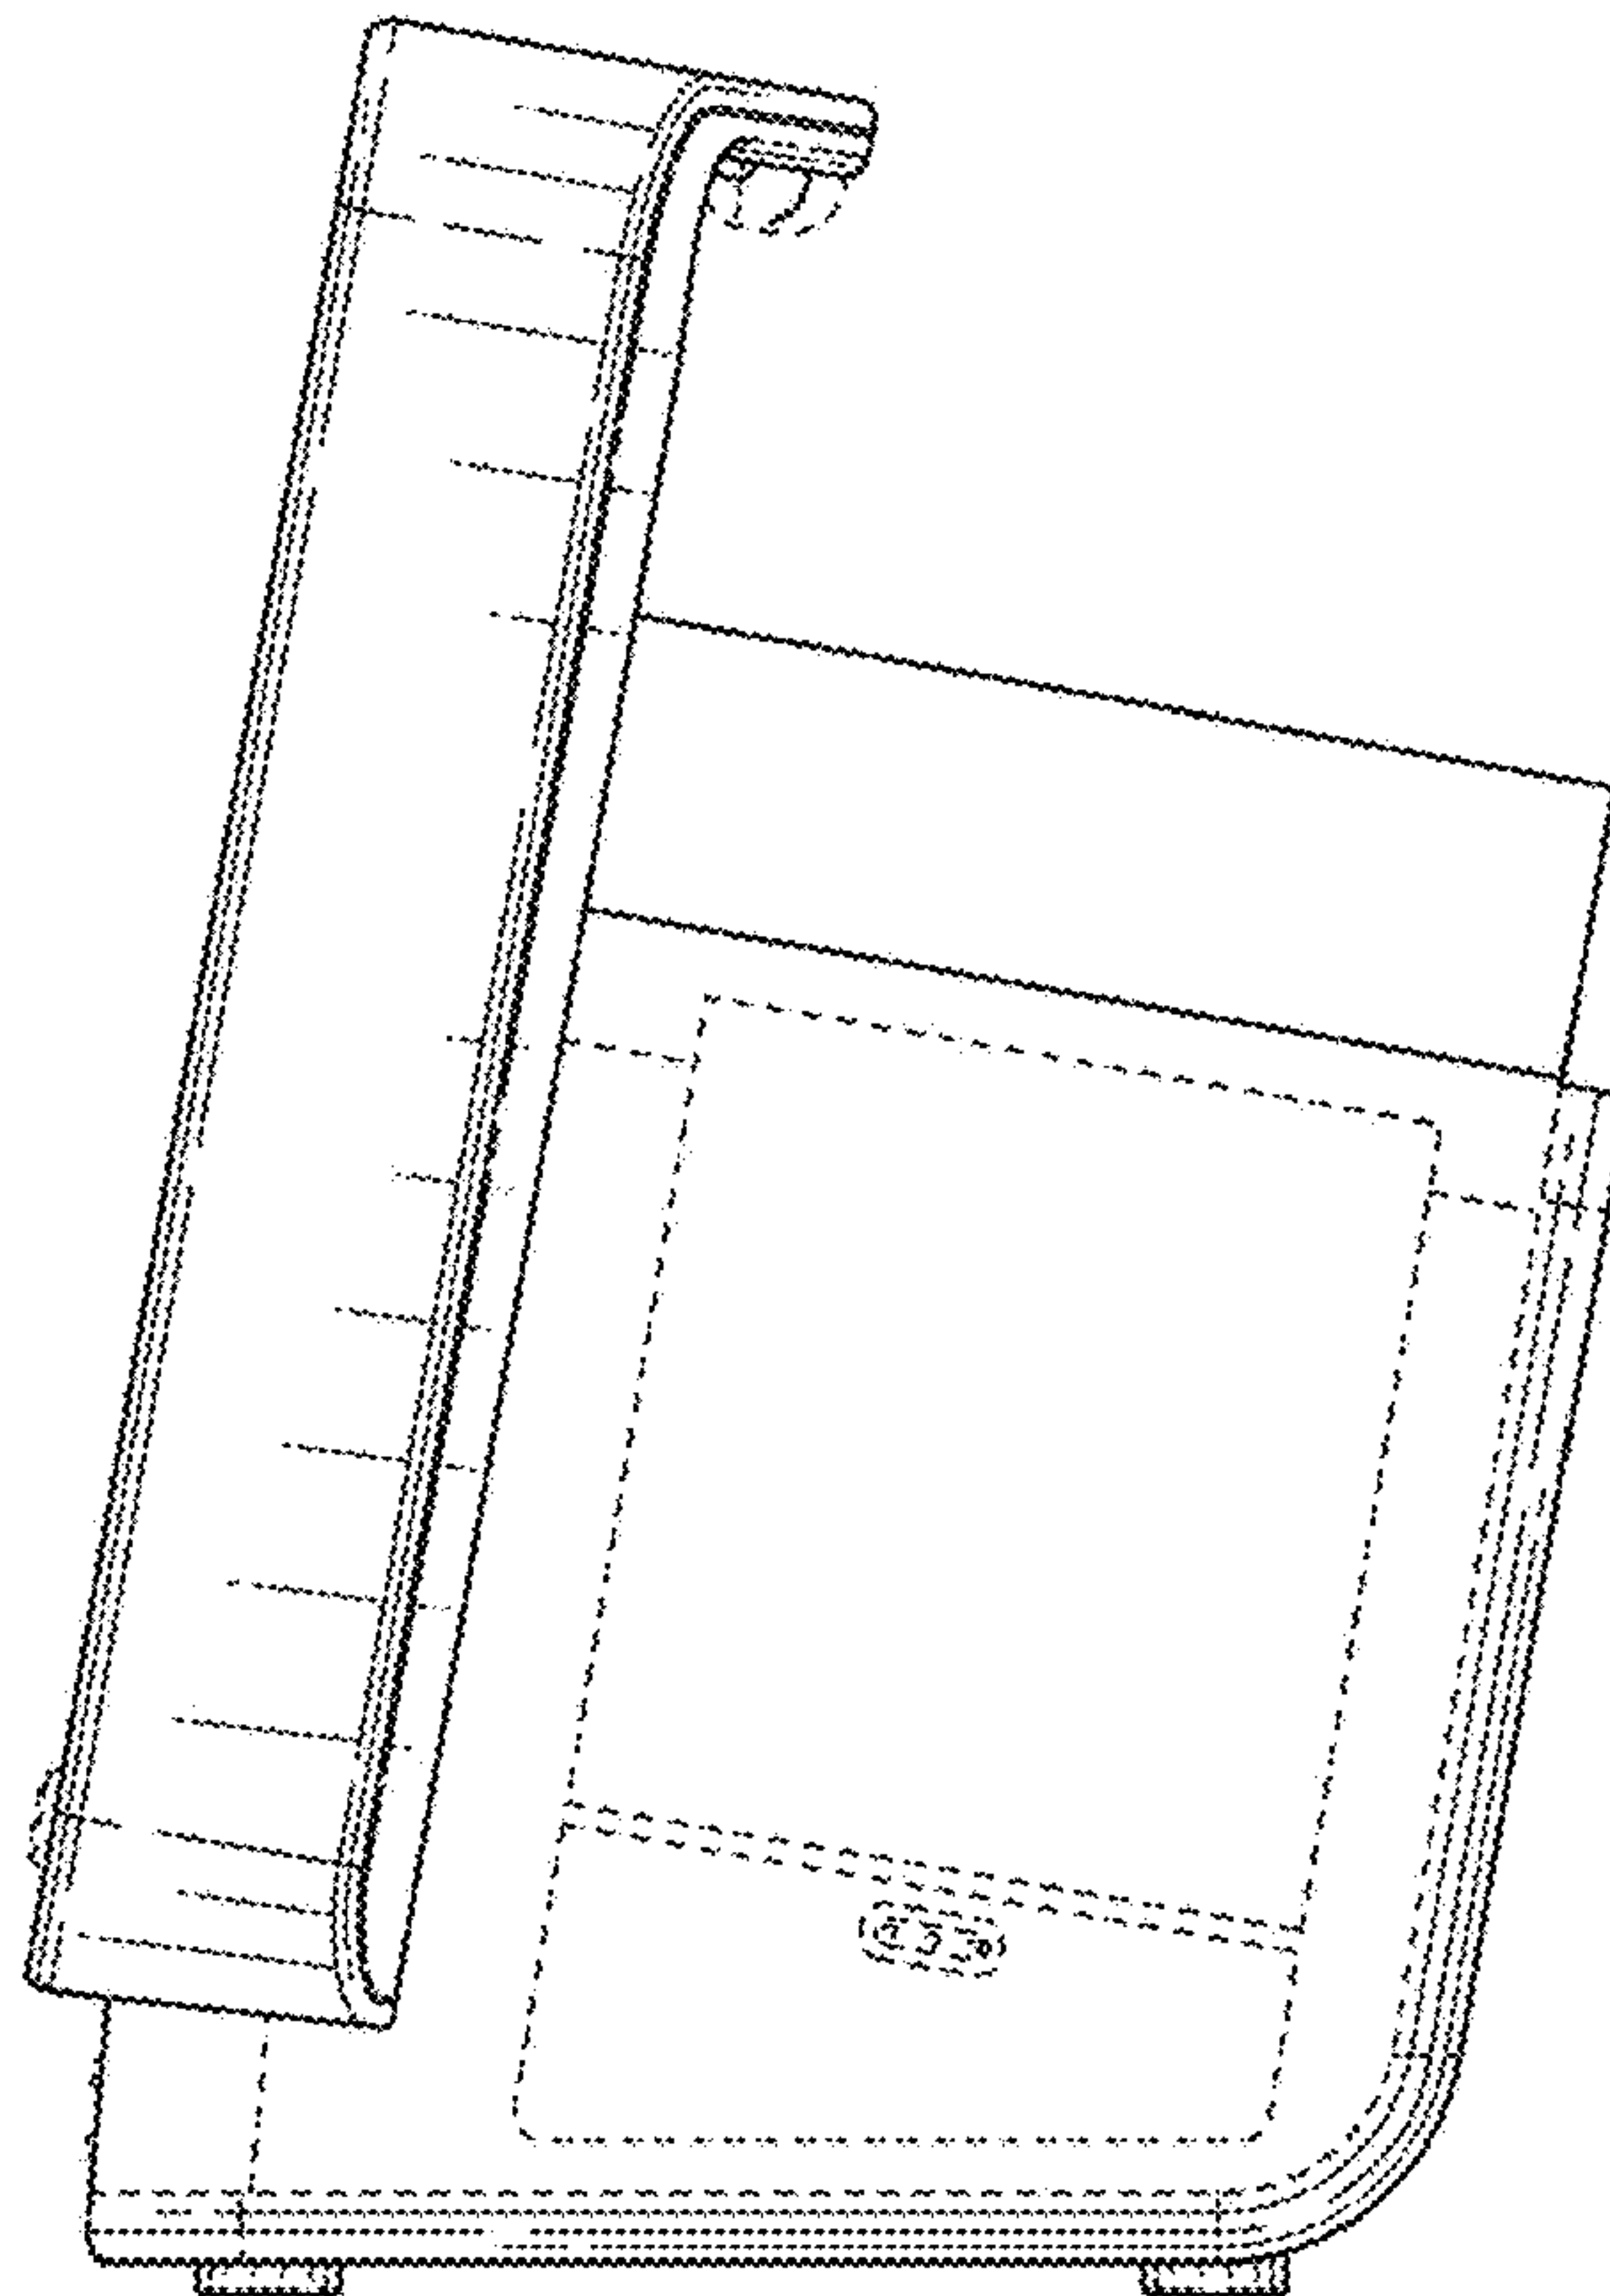


FIG. 5

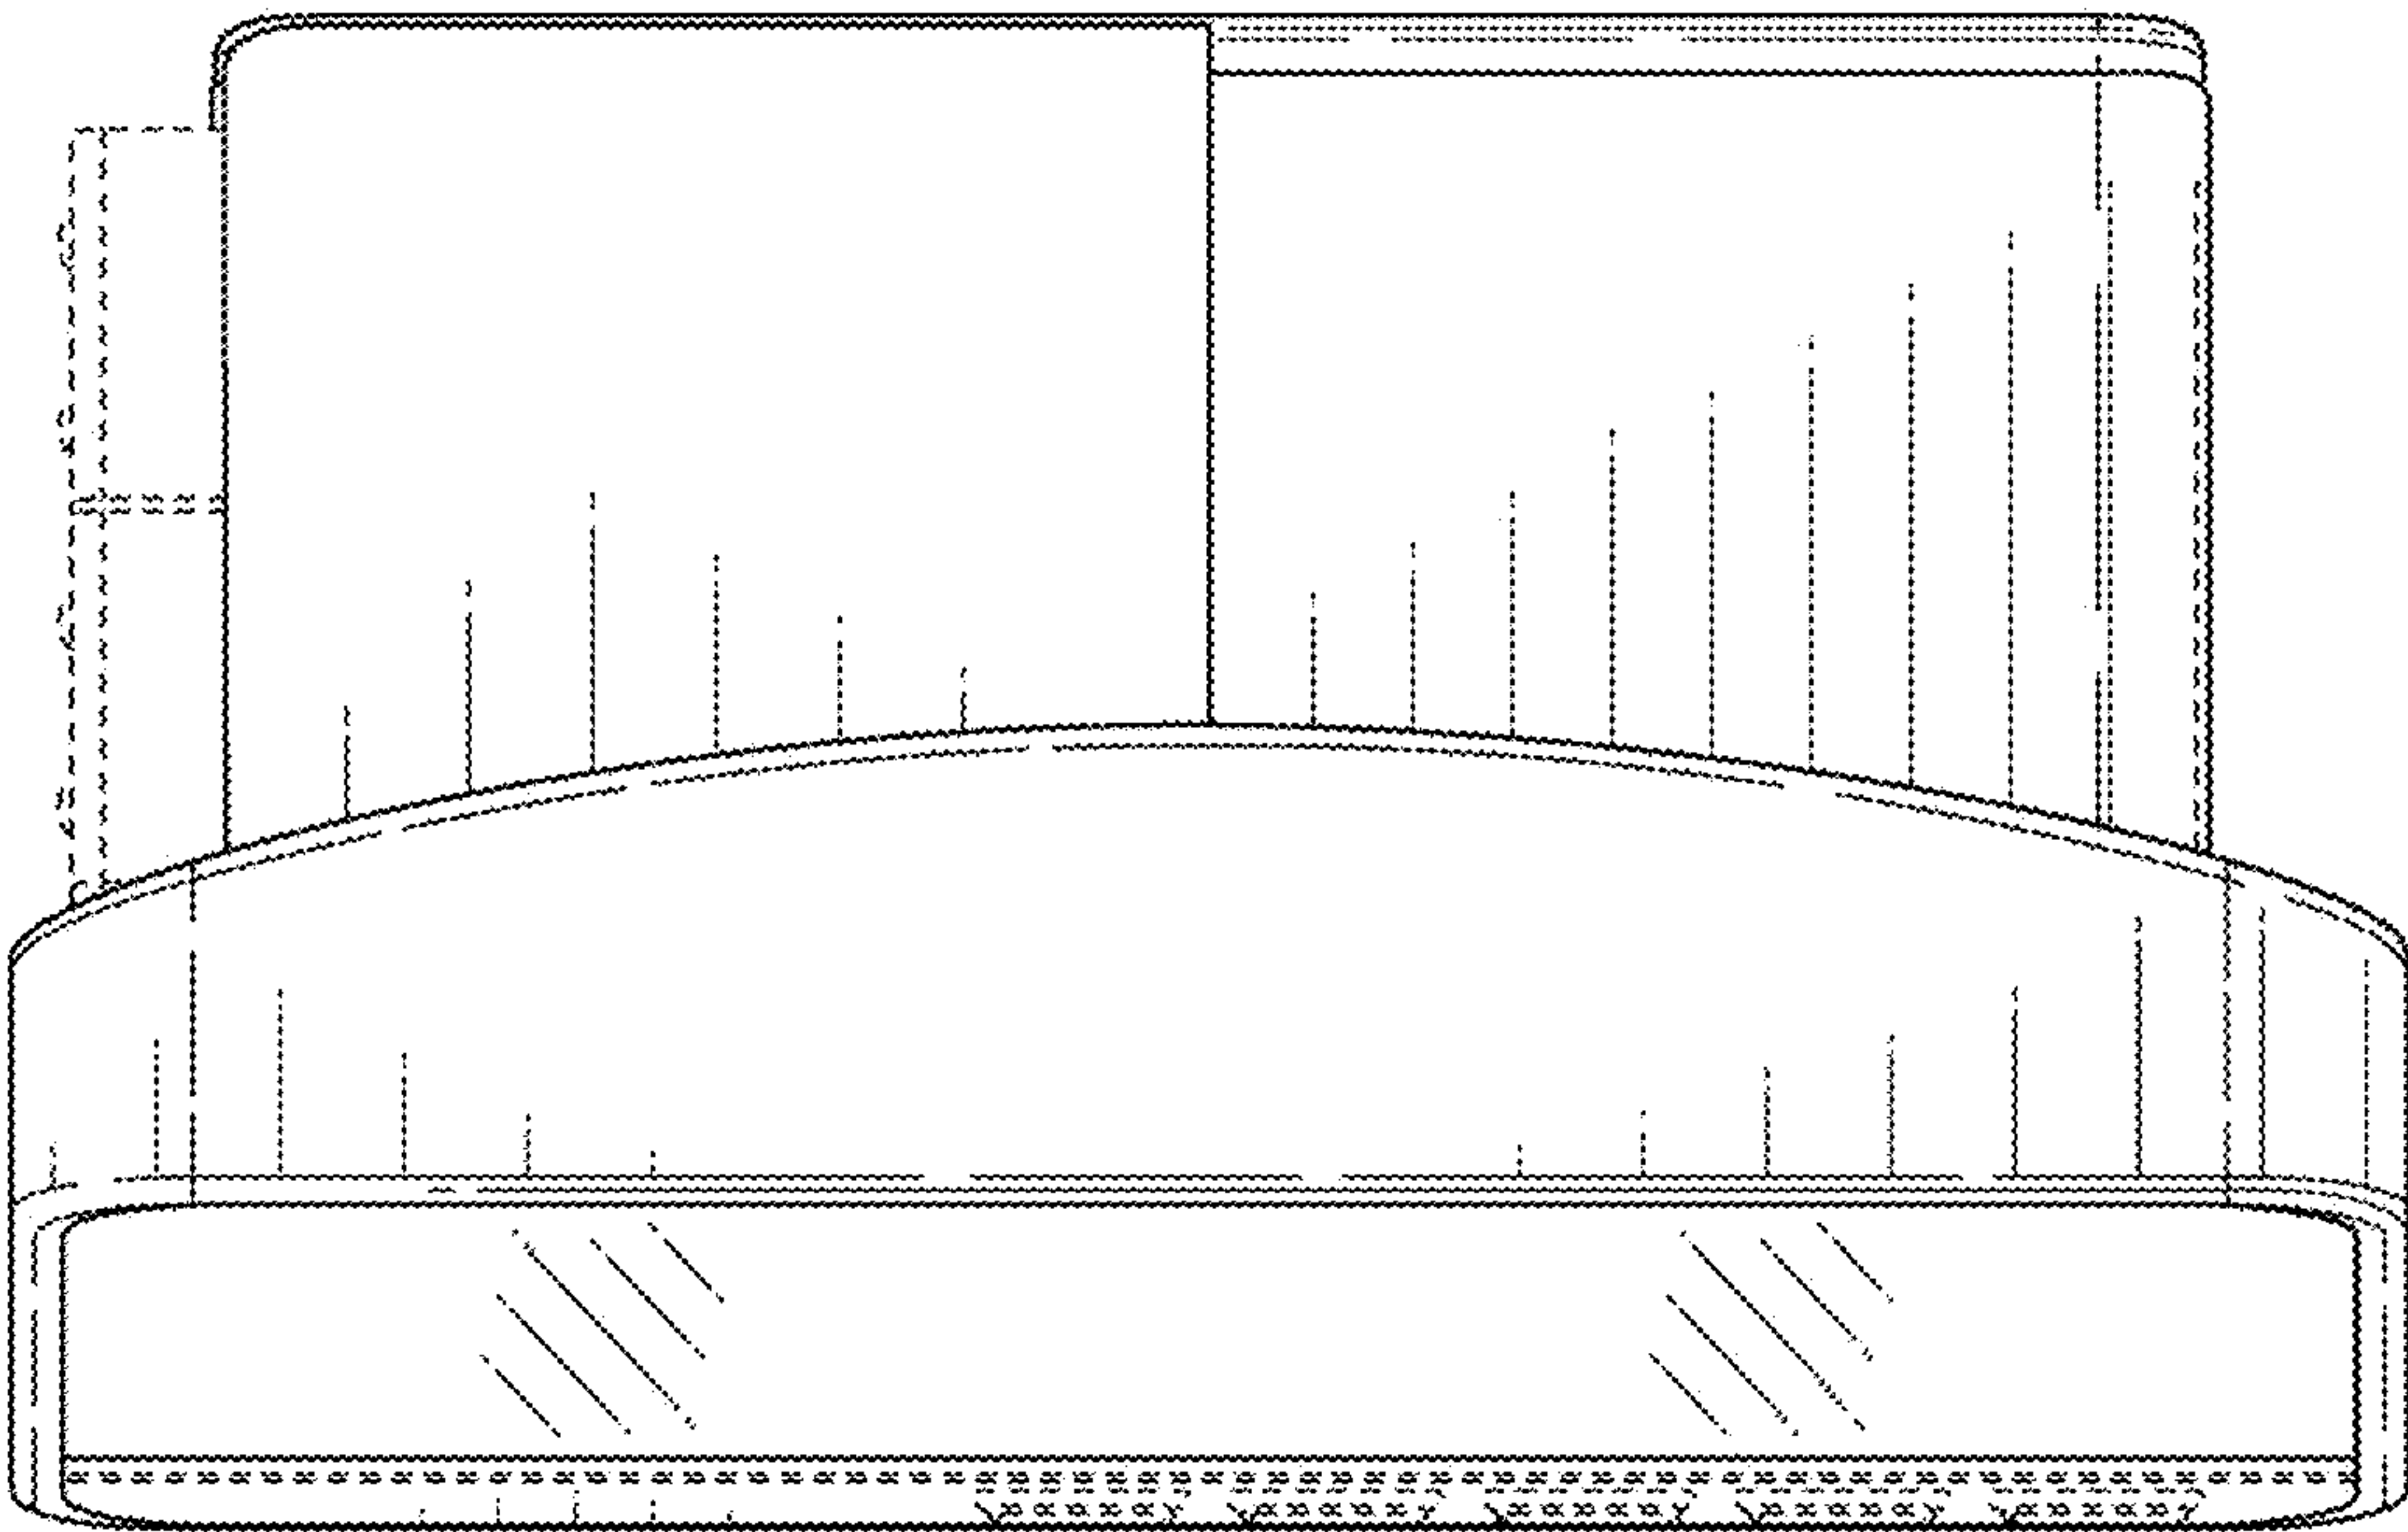


FIG. 6

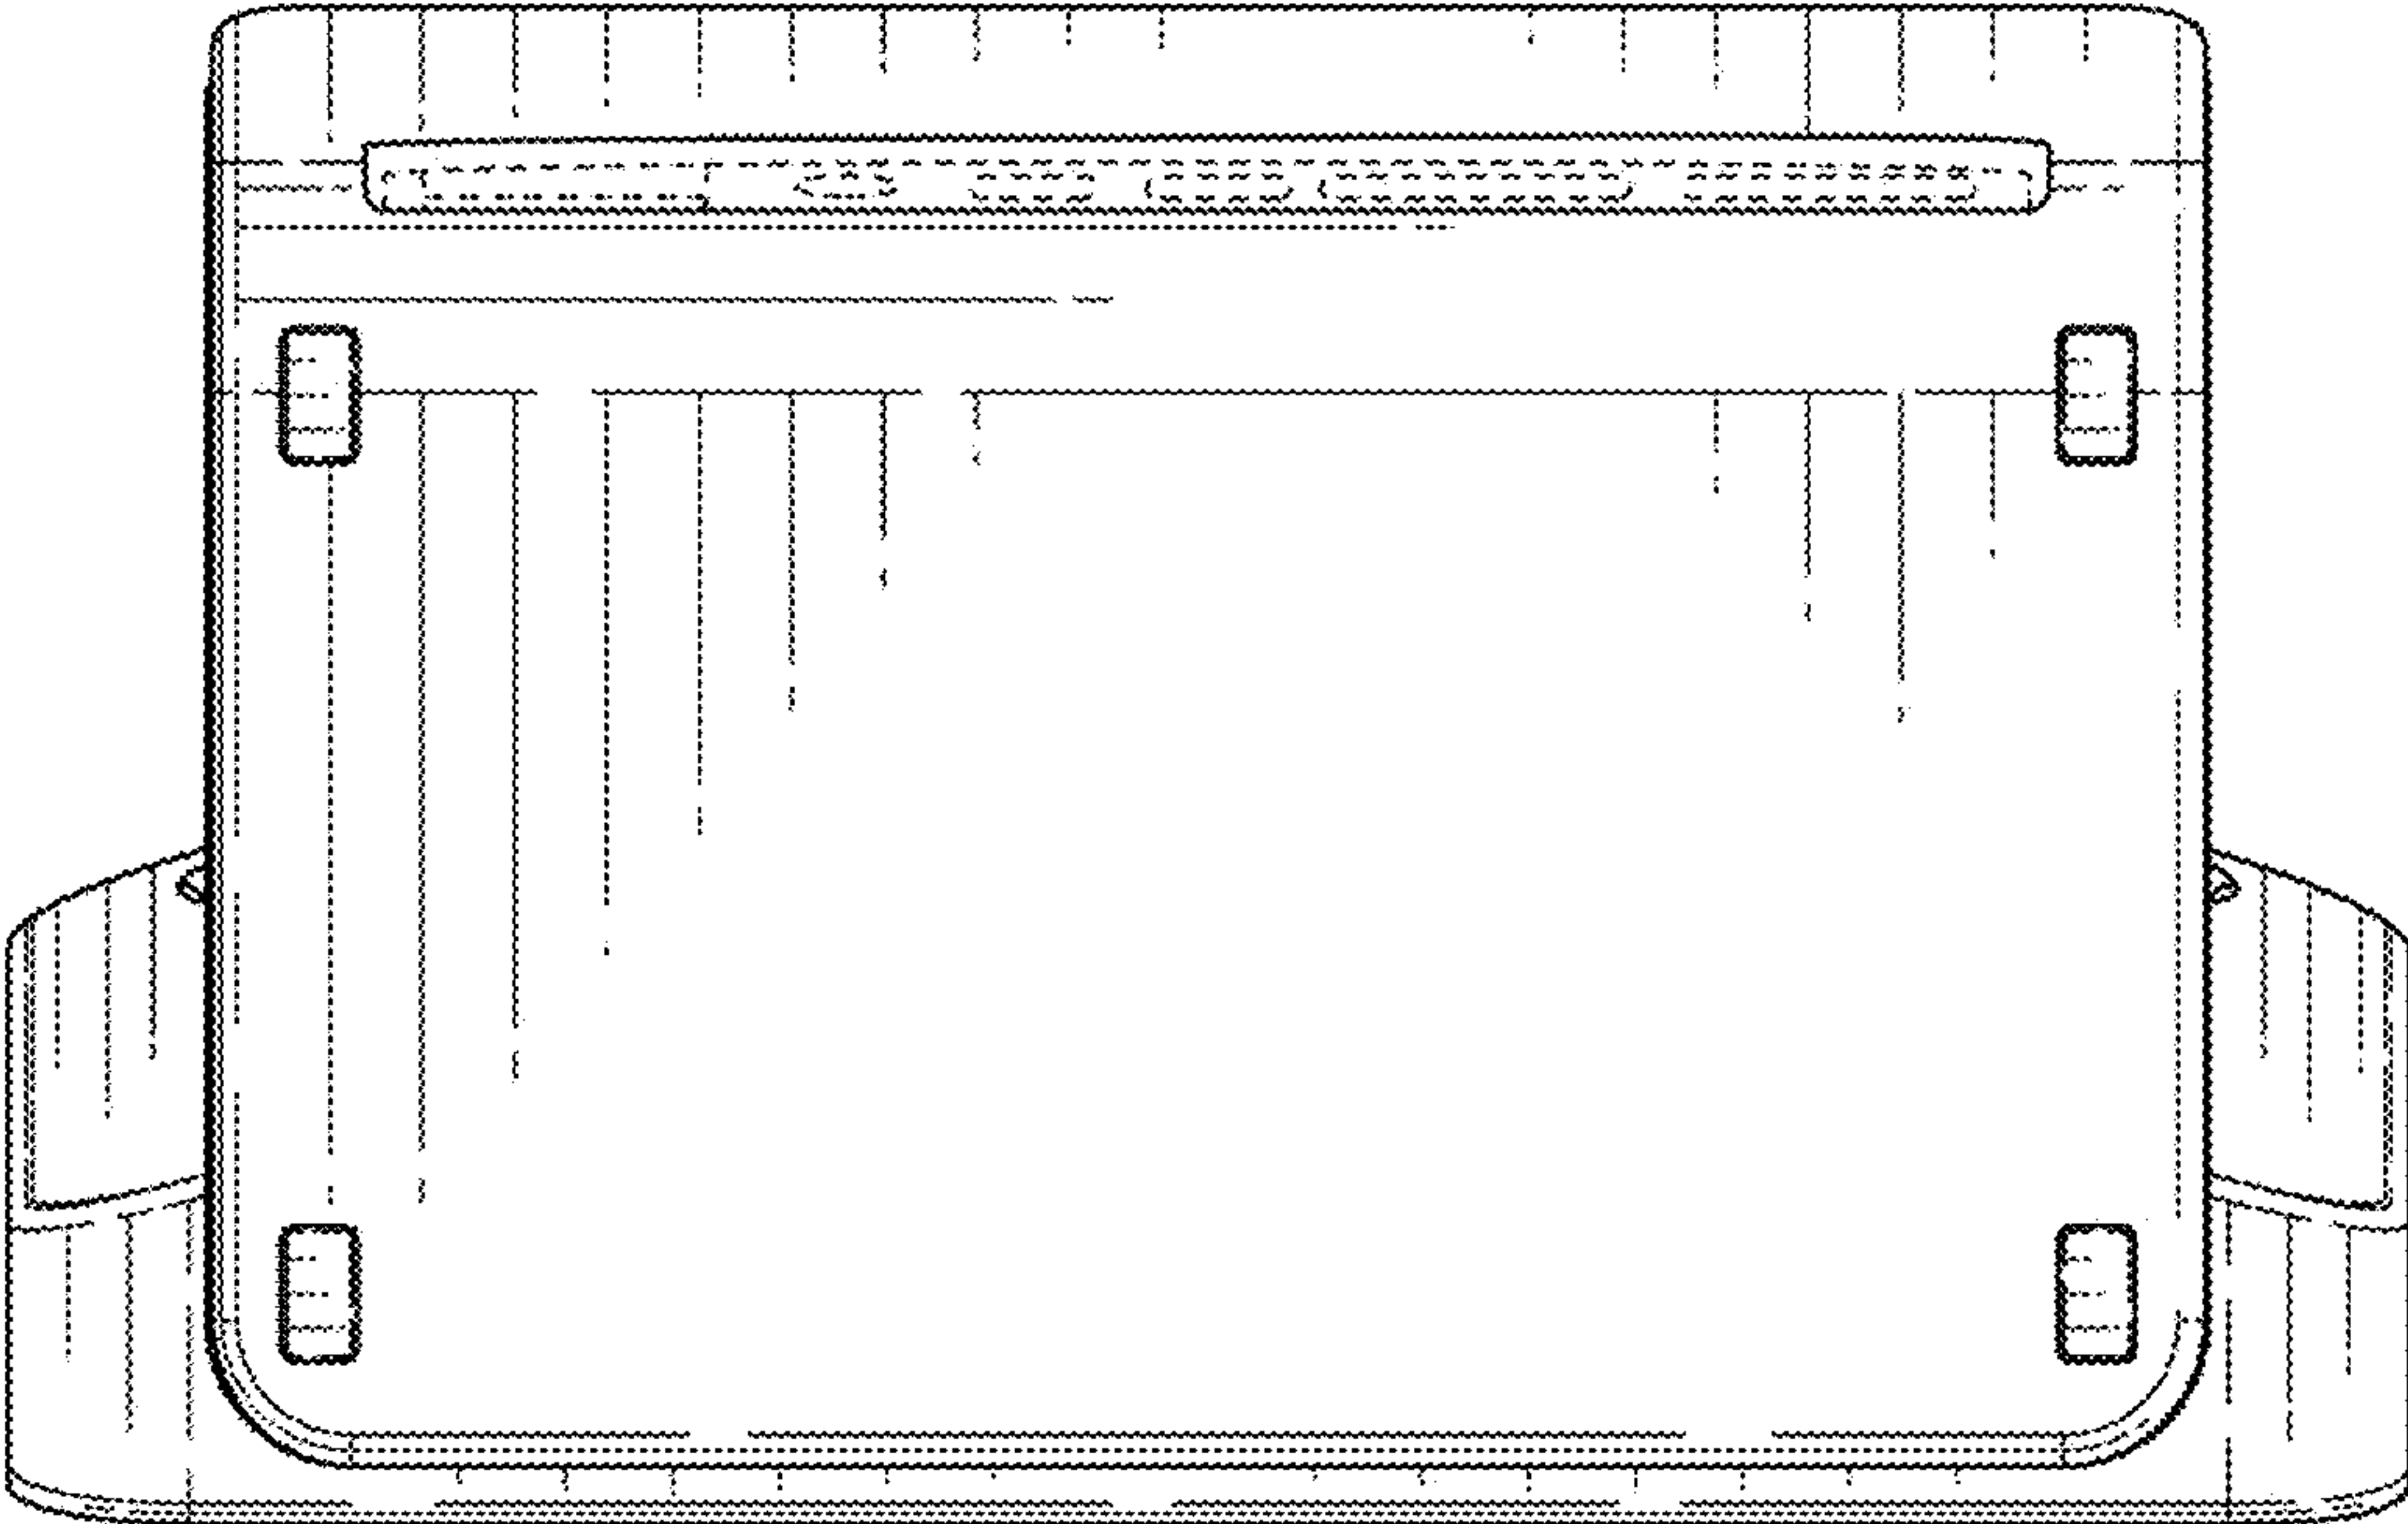


FIG. 7