



US00D927426S

(12) **United States Design Patent** (10) **Patent No.:** **US D927,426 S**
Bowman et al. (45) **Date of Patent:** **** *Aug. 10, 2021**

(54) **MEDICAL DEVICE CONNECTOR**

(71) Applicant: **Physio-Control, Inc.**, Redmond, WA (US)

(72) Inventors: **Ryan Bowman**, Redmond, WA (US);
Zack Pahlman, Redmond, WA (US);
Jeremy Wong, Redmond, WA (US)

(73) Assignee: **Physio-Control, Inc.**, Redmond, WA (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

(21) Appl. No.: **29/708,317**

(22) Filed: **Oct. 4, 2019**

(51) **LOC (13) Cl.** **13-03**

(52) **U.S. Cl.**
USPC **D13/133; D13/146**

(58) **Field of Classification Search**
USPC D13/107, 108, 123, 133, 146, 147, 154,
D13/184, 199; D24/107, 127, 129, 167,
D24/168, 187
CPC A61N 1/39; A61B 5/00; A61B 5/04; A61B
5/0408; A61B 5/0416; A61B 6/03; H01R
9/00; H01R 9/03; H01R 13/00; H01R
13/46; H01R 13/627; H01R 13/64; H01R
13/73; H01R 24/00
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 2,384,267 A * 9/1945 Andersen H01R 24/84
439/293
- D250,719 S 1/1979 Jacobson et al.
- D263,794 S 4/1982 Yoshizawa
- D290,458 S 6/1987 O'Leary
- D319,312 S * 8/1991 Schneider D24/129

- D395,282 S 6/1998 Rudoy et al.
- D410,625 S * 6/1999 Kerek D13/133
- D434,377 S 11/2000 Bussett et al.
- D475,014 S 5/2003 Kano
- D523,815 S 6/2006 Lai
- D588,990 S 3/2009 Kok et al.
- D589,444 S 3/2009 Kok et al.
- D589,881 S 4/2009 Kok et al.
- D645,406 S 9/2011 Chartrand et al.
- D668,611 S * 10/2012 Byrne D13/146
- 8,647,147 B2 2/2014 Chartrand et al.
- D730,839 S * 6/2015 Sasano D13/147
- D743,342 S * 11/2015 Sasano D13/147

(Continued)

OTHER PUBLICATIONS

Aedsuperstore.com, "Physio-Control Lifepak 500 Data Transfer USB to Quik-Combo Cable", retrieved on Oct. 7, 2020 from <https://www.aedsuperstore.com/physio-control-lifepak-500-data-transfer-usb-to-quick-combo-cable.html>, Dec. 1, 2010, 3 pages.

(Continued)

Primary Examiner — Shawn T Gingrich
(74) *Attorney, Agent, or Firm* — Lee & Hayes, P.C.


(57) **CLAIM**

The ornamental design for a medical device connector, as shown and described.

DESCRIPTION

FIG. 1 is a back perspective view of a medical device connector;
FIG. 2 is a front view thereof;
FIG. 3 is a back view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a left side view thereof; and,
FIG. 6 is a right side view thereof.
The dashed-lines represent the remainder of the article and do not form part of the claimed design, are directed to environment, and represent unclaimed subject matter.

1 Claim, 3 Drawing Sheets

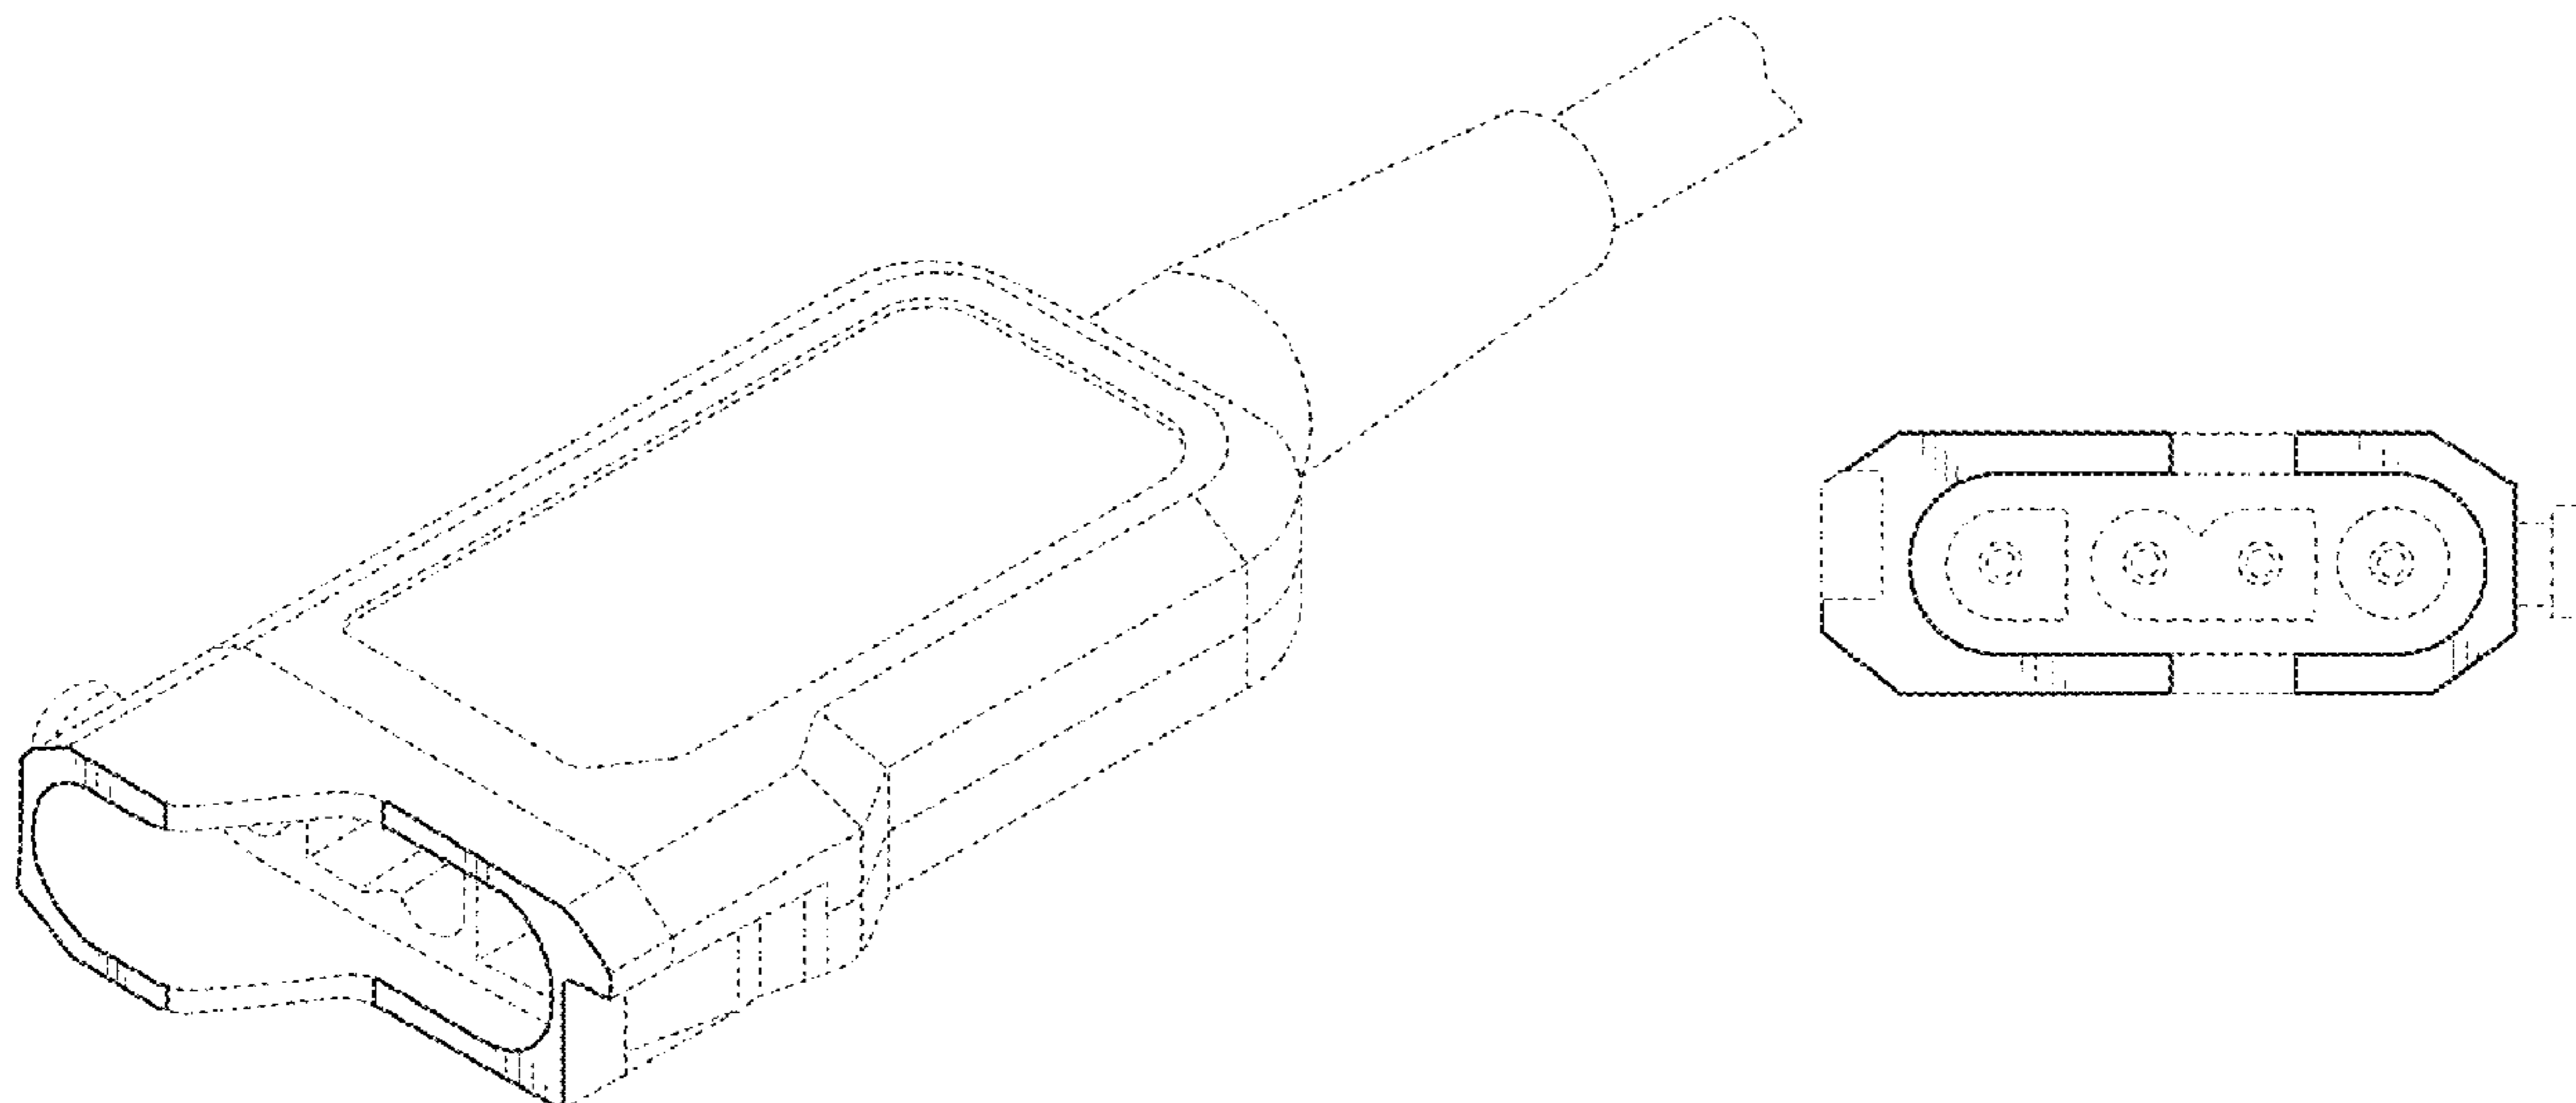

(56)

References Cited

U.S. PATENT DOCUMENTS

D743,906	S	*	11/2015	Sasano	D13/147
D851,595	S	*	6/2019	Chen	D13/133
D864,870	S		10/2019	Payne	
D887,987	S		6/2020	Ganamukhi et al.	
D896,175	S		9/2020	Staffl et al.	
2005/0227529	A1		10/2005	Mrakovich et al.	
2011/0014821	A1		1/2011	Ko	
2012/0178270	A1		7/2012	McElroy et al.	
2014/0073180	A1*		3/2014	Knight	H01R 13/5221 439/588
2015/0017841	A1		1/2015	Chen et al.	
2016/0028169	A1		1/2016	Glick et al.	
2018/0159274	A1		6/2018	Eriksson et al.	
2021/0011235	A1*		1/2021	Wimmer	G02B 6/3831

OTHER PUBLICATIONS

Amazon.com, “Physio-Control 11113-000002 Quik-Combo Test Plug for Testing QC Cable”, retrieved on Oct. 7, 2020 from <<https://www.amazon.com/physio-control-11113-000002-quik-combo-testing-cable/dp/B085D4M7B3>>, Nov. 27, 2009, 2 pages.

DHGate.com, “T4 T5 T8 Bracket Light Male and Female Plug Connector”, retrieved on Oct. 7, 2020 from <https://www.dhgate.com/product/t4-t5-t8-bracket-light-male-and-femal-plug/410219373.html#redirect_detail=WAP2PC>, Nov. 20, 2019.

Non Final Office Action dated Oct. 28, 2020 for U.S. Appl. No. 29/708,366, “Medical Device Connector”, Bowman, 9 pages.

Non Final Office Action dated Oct. 28, 2020 for U.S. Appl. No. 29/708,367, “Medical Device Connector”, Bowman, 7 pages.

Non Final Office Action dated Dec. 8, 2020 for U.S. Appl. No. 29/708,322, “Medical Device Connector”, Bowman, 10 pages.

Non Final Office Action dated Dec. 8, 2020 for U.S. Appl. No. 29/708,355, “Medical Device Connector”, Bowman, 8 pages.

* cited by examiner

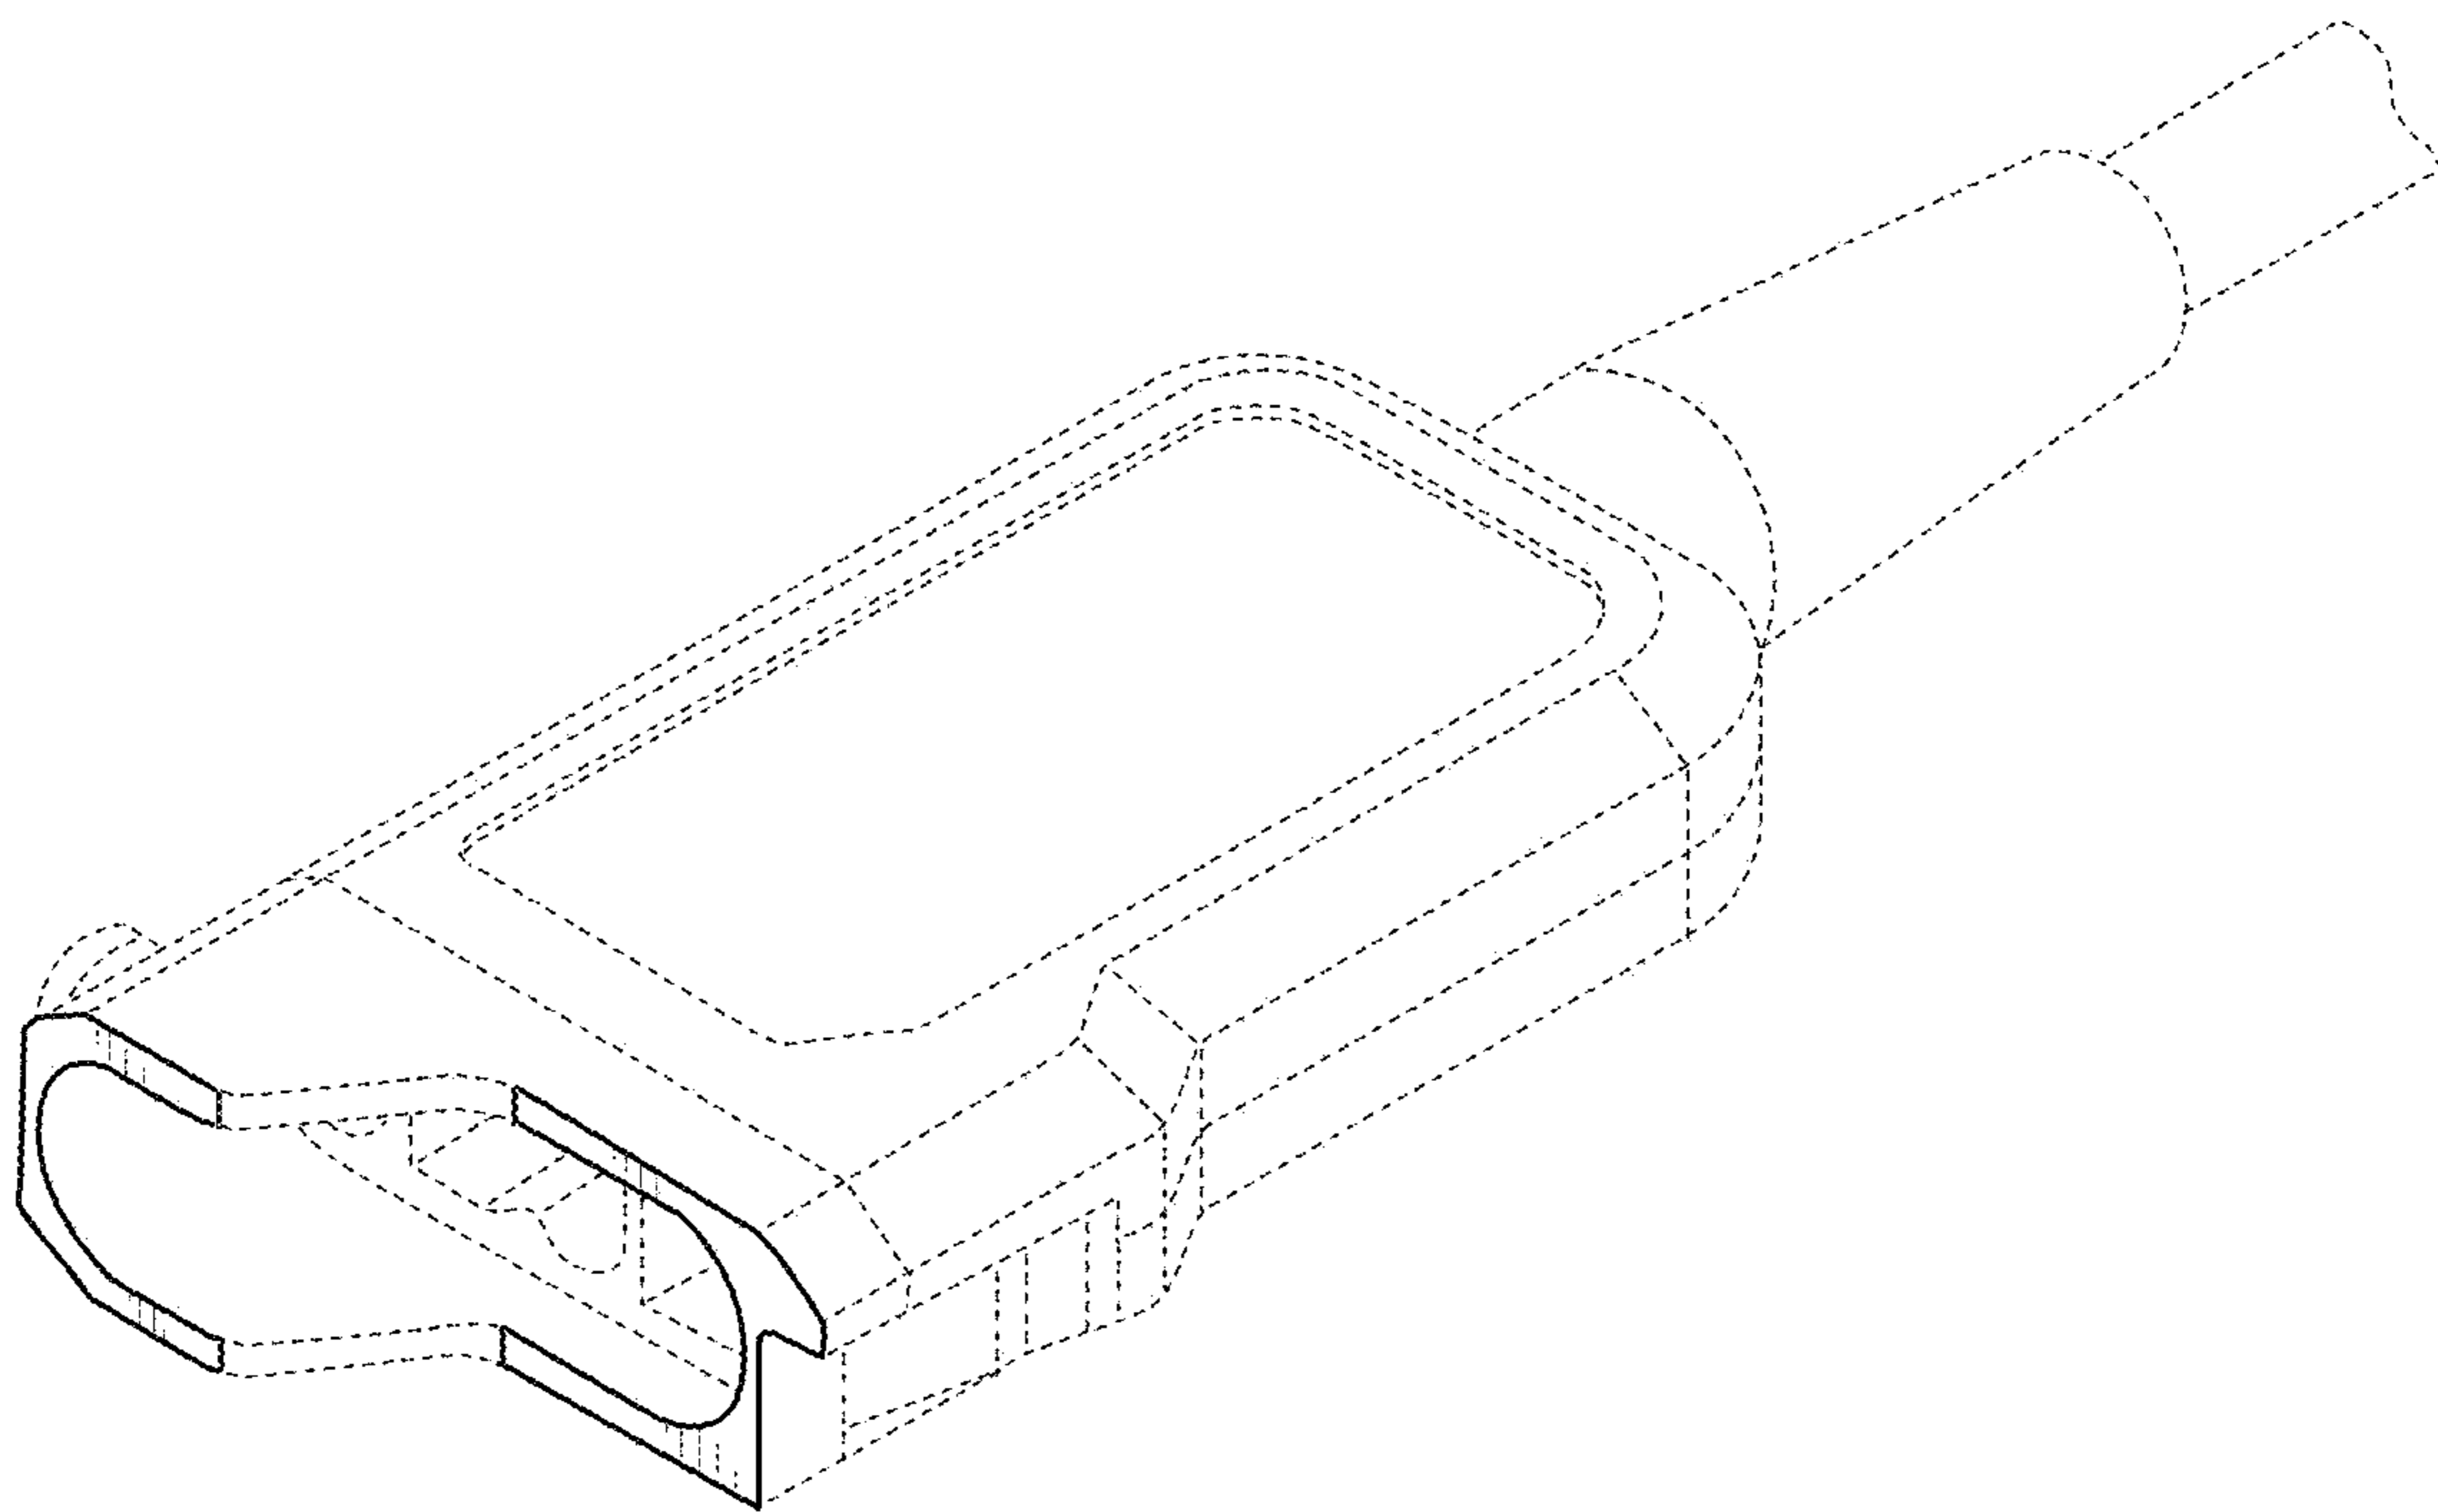


FIG. 1

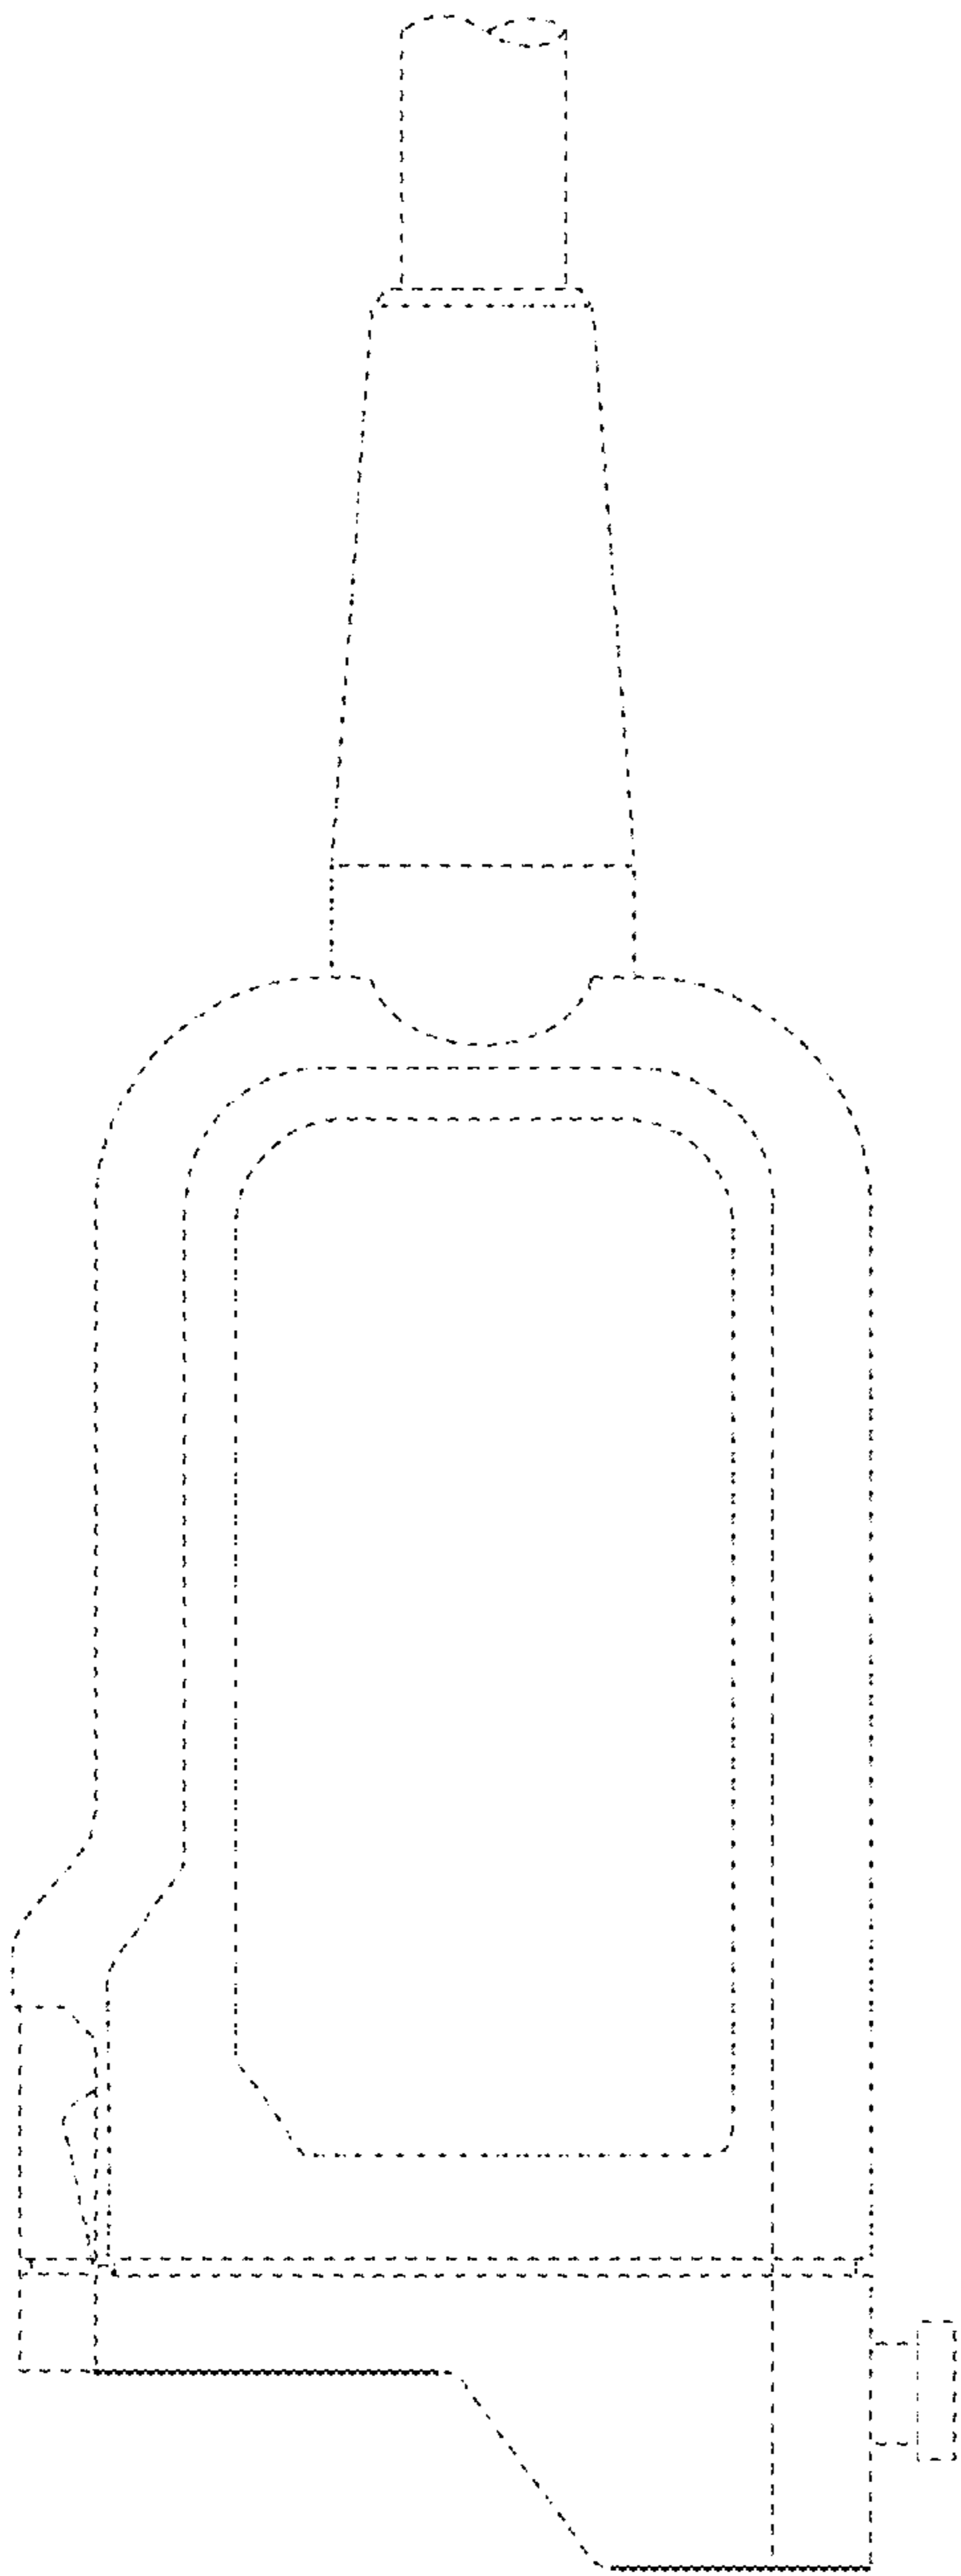


FIG. 2

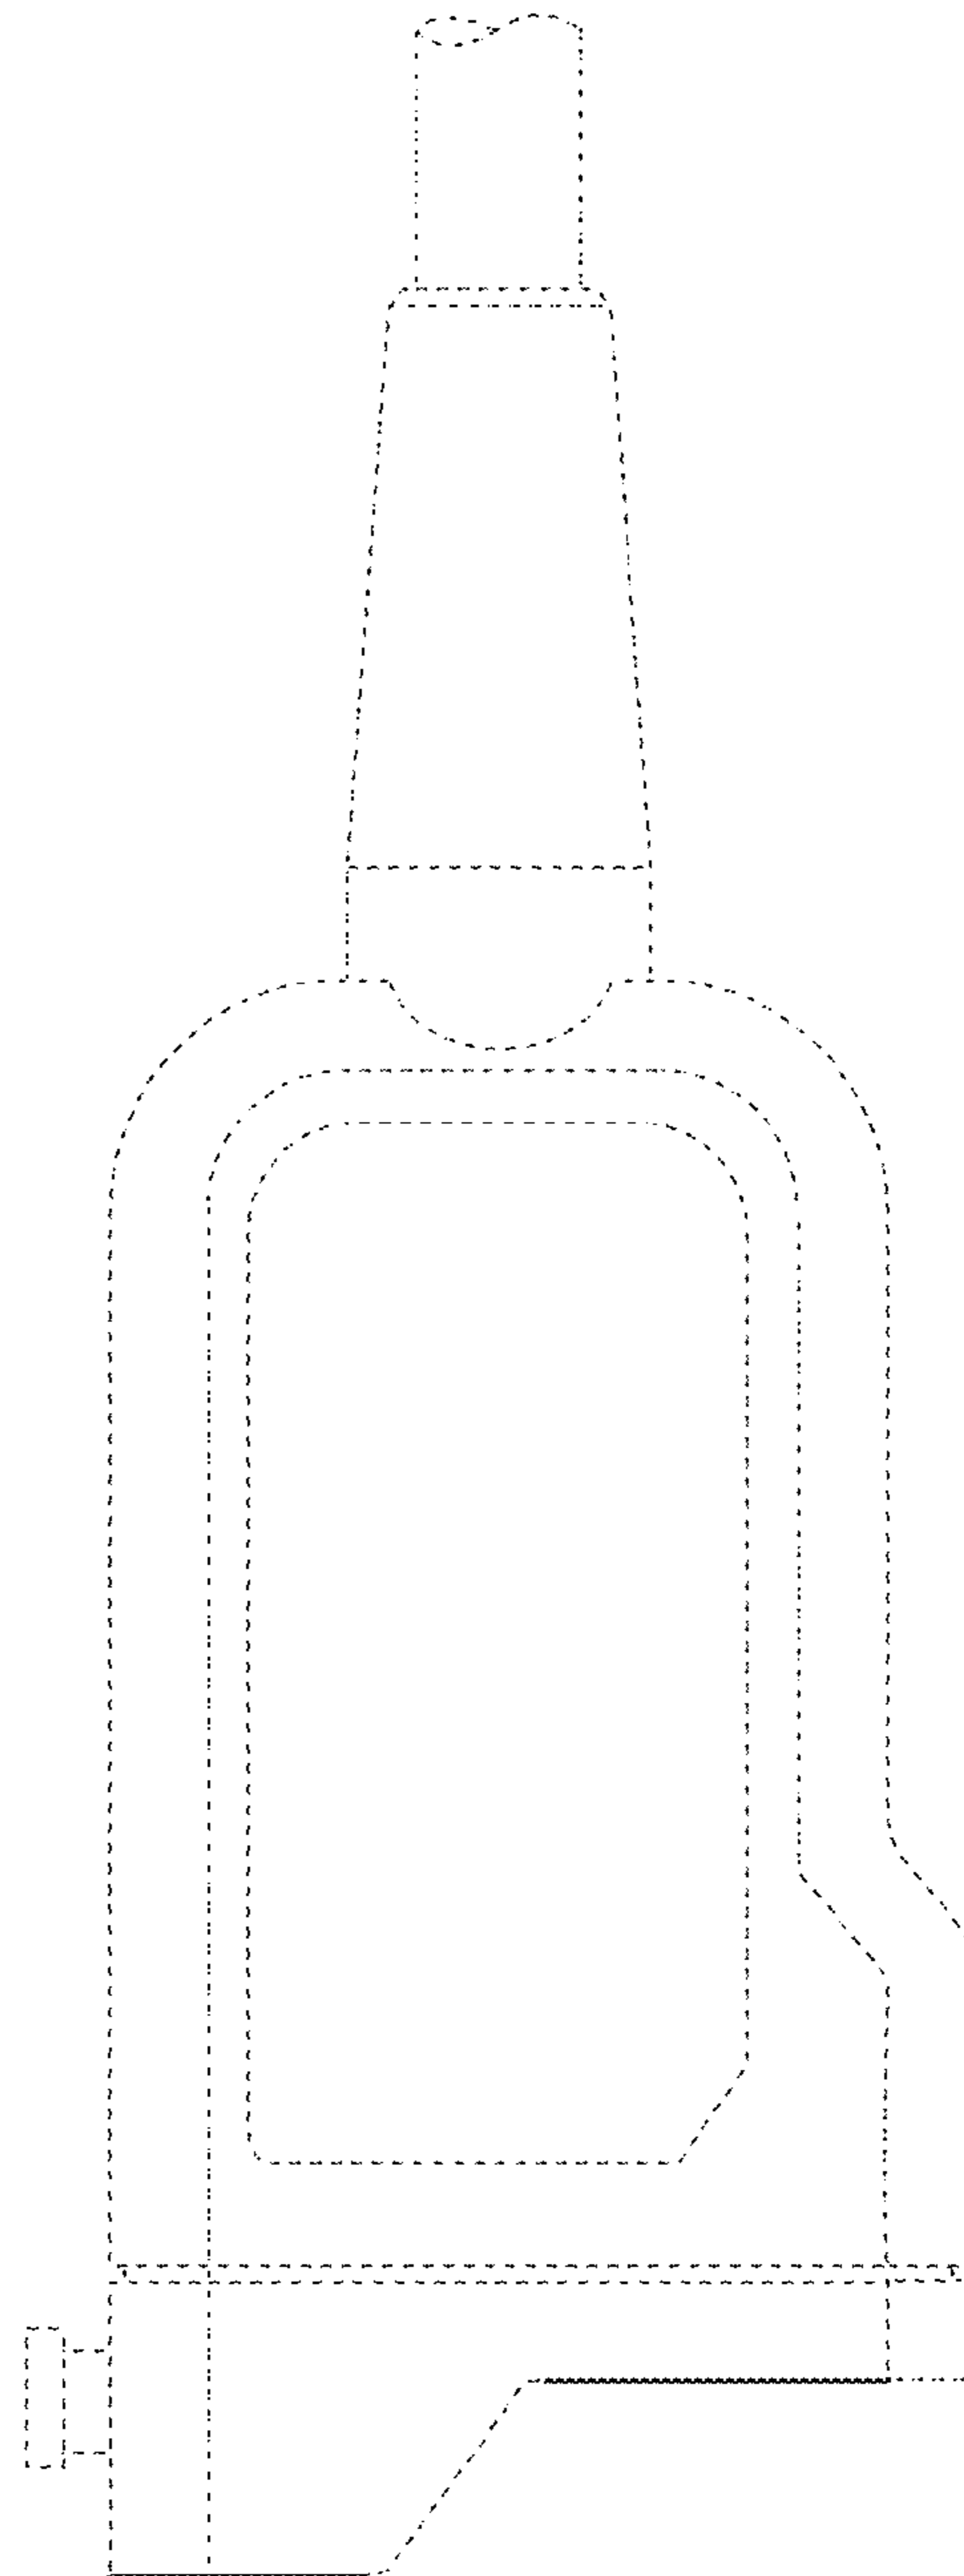


FIG. 3

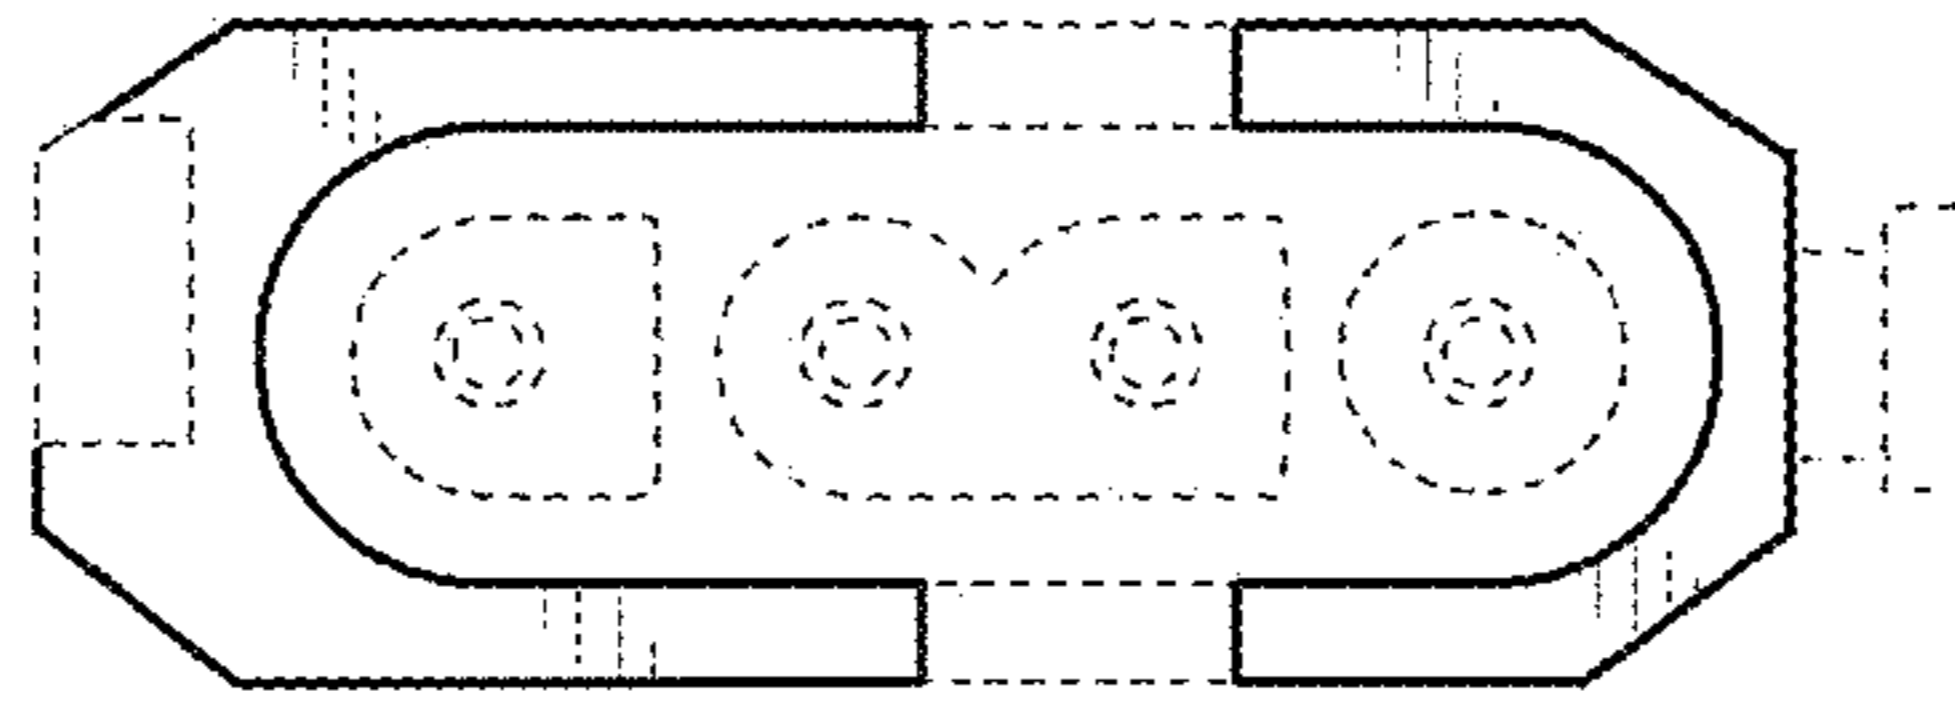


FIG. 4

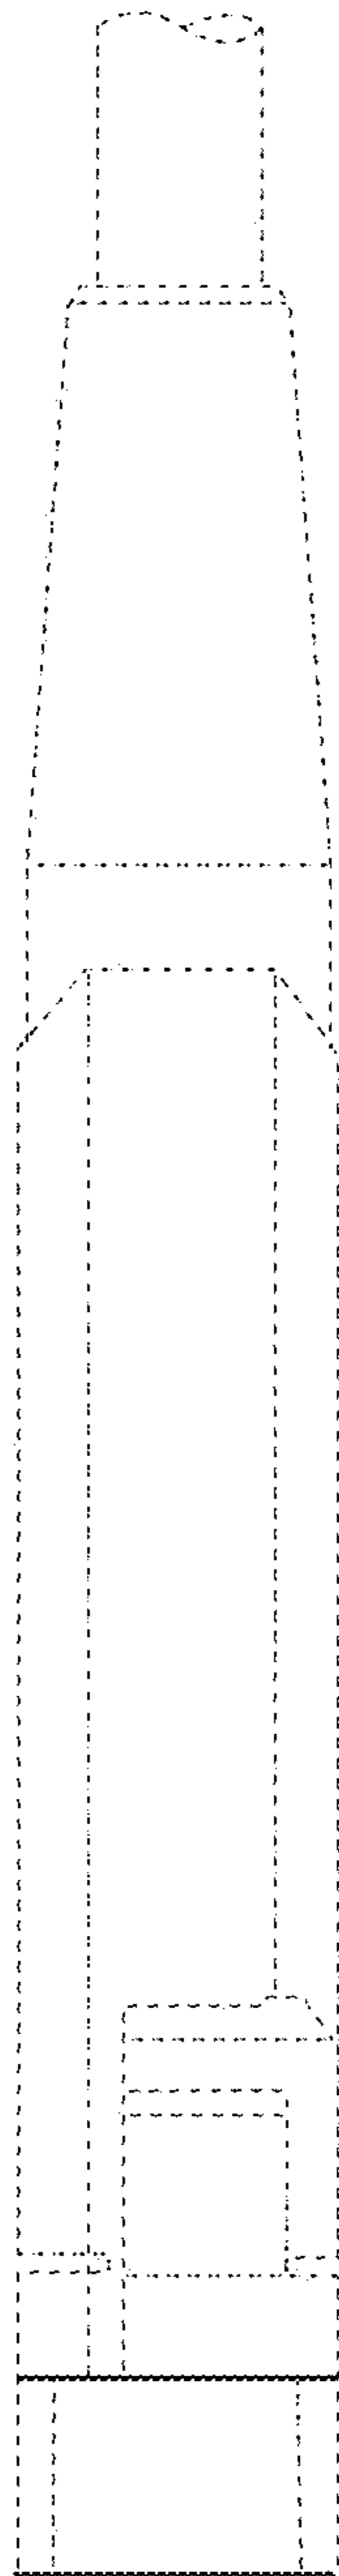


FIG. 5

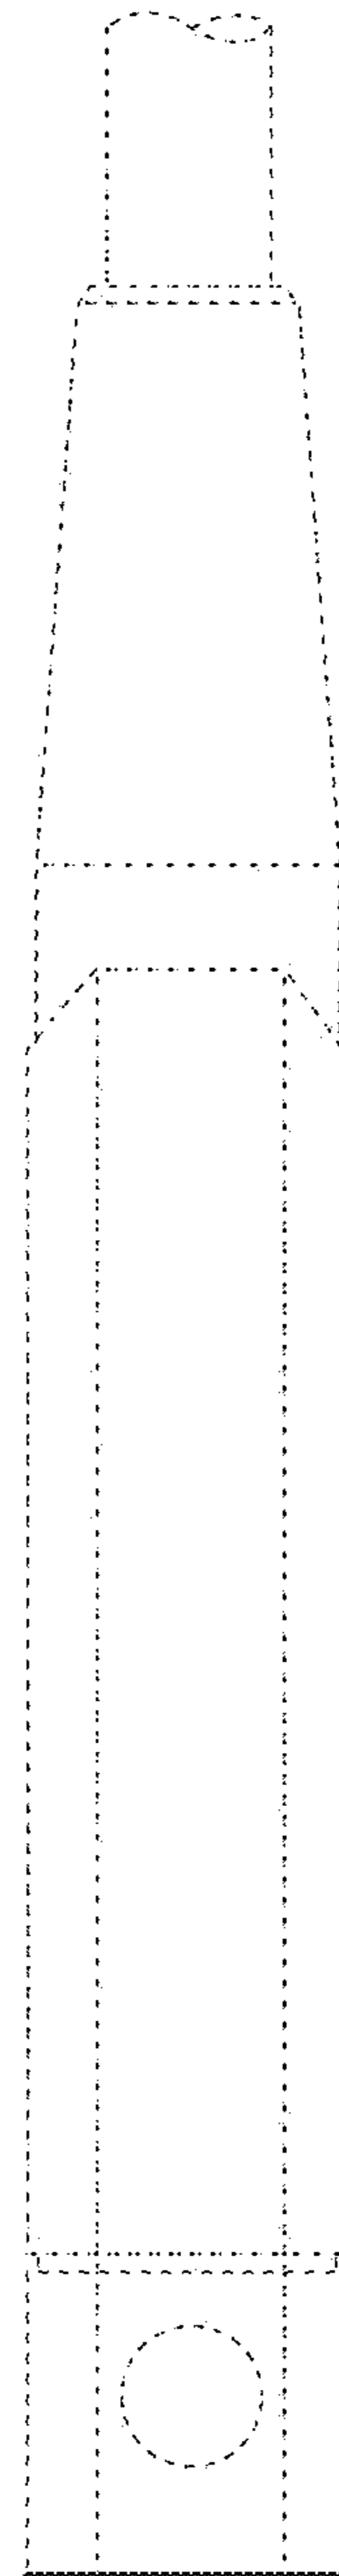


FIG. 6