



US00D927689S

(12) **United States Design Patent** (10) **Patent No.:** **US D927,689 S**
Limem et al. (45) **Date of Patent:** **** Aug. 10, 2021**

(54) **THREE DIMENSIONAL MASTOPEXY IMPLANT**

4,388,735 A 6/1983 Ionescu et al.
4,936,858 A 6/1990 O'Keefe
5,217,494 A 6/1993 Coggins et al.
5,356,429 A 10/1994 Seare
5,383,929 A 1/1995 Ledergerber

(71) Applicant: **Tepha, Inc.**, Lexington, MA (US)

(Continued)

(72) Inventors: **Skander Limem**, Melrose, MA (US);
Emily Stires, Boston, MA (US);
Rebecca Marciante, North Reading, MA (US); **Said Rizk**, Windham, NH (US); **Arikha Moses**, Summit, NJ (US); **Fabio Felix**, Foxborough, MA (US); **Bruce Van Natta**, Westfield, IN (US)

FOREIGN PATENT DOCUMENTS

WO 2004096098 A1 11/2004
WO 2006117622 A1 11/2006

(Continued)

(73) Assignee: **Tepha, Inc.**, Lexington, MA (US)

OTHER PUBLICATIONS

(**) Term: **15 Years**

U.S. Appl. No. 16/587,903, Sep. 30, 2019, Skander Limem.

(Continued)

(21) Appl. No.: **29/735,098**

Primary Examiner — Charles D Hanson

(22) Filed: **May 18, 2020**

(74) *Attorney, Agent, or Firm* — Richard Batt

Related U.S. Application Data

(62) Division of application No. 29/668,175, filed on Oct. 29, 2018, now Pat. No. Des. 888,244, which is a division of application No. 29/542,048, filed on Oct. 9, 2015, now Pat. No. Des. 836,778.

(51) **LOC (13) Cl.** **24-03**

(52) **U.S. Cl.**
USPC **D24/155**

(58) **Field of Classification Search**
USPC D24/155
CPC A61F 2/12
See application file for complete search history.

(57) **CLAIM**

The ornamental design for a three dimensional mastopexy implant, as shown and described.

DESCRIPTION


FIG. 1 is a front view of a three dimensional mastopexy implant showing our new design;
FIG. 2 is a top view of the three dimensional mastopexy implant shown in FIG. 1;
FIG. 3 is a side view of the three dimensional mastopexy implant shown in FIG. 1;
FIG. 4 is a bottom view of the three dimensional mastopexy implant shown in FIG. 1;
FIG. 5 is another side view of the three dimensional mastopexy implant shown in FIG. 1;
FIG. 6 is a rear view of the three dimensional mastopexy implant shown in FIG. 1; and,
FIG. 7 is a top, front, side perspective view of the three dimensional mastopexy implant shown in FIG. 1.

1 Claim, 4 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,701,879 A 2/1955 Bennett
3,280,818 A 10/1966 Pankey et al.
3,934,593 A 1/1976 Mellinger
4,372,293 A 2/1983 Vijil-Rosales

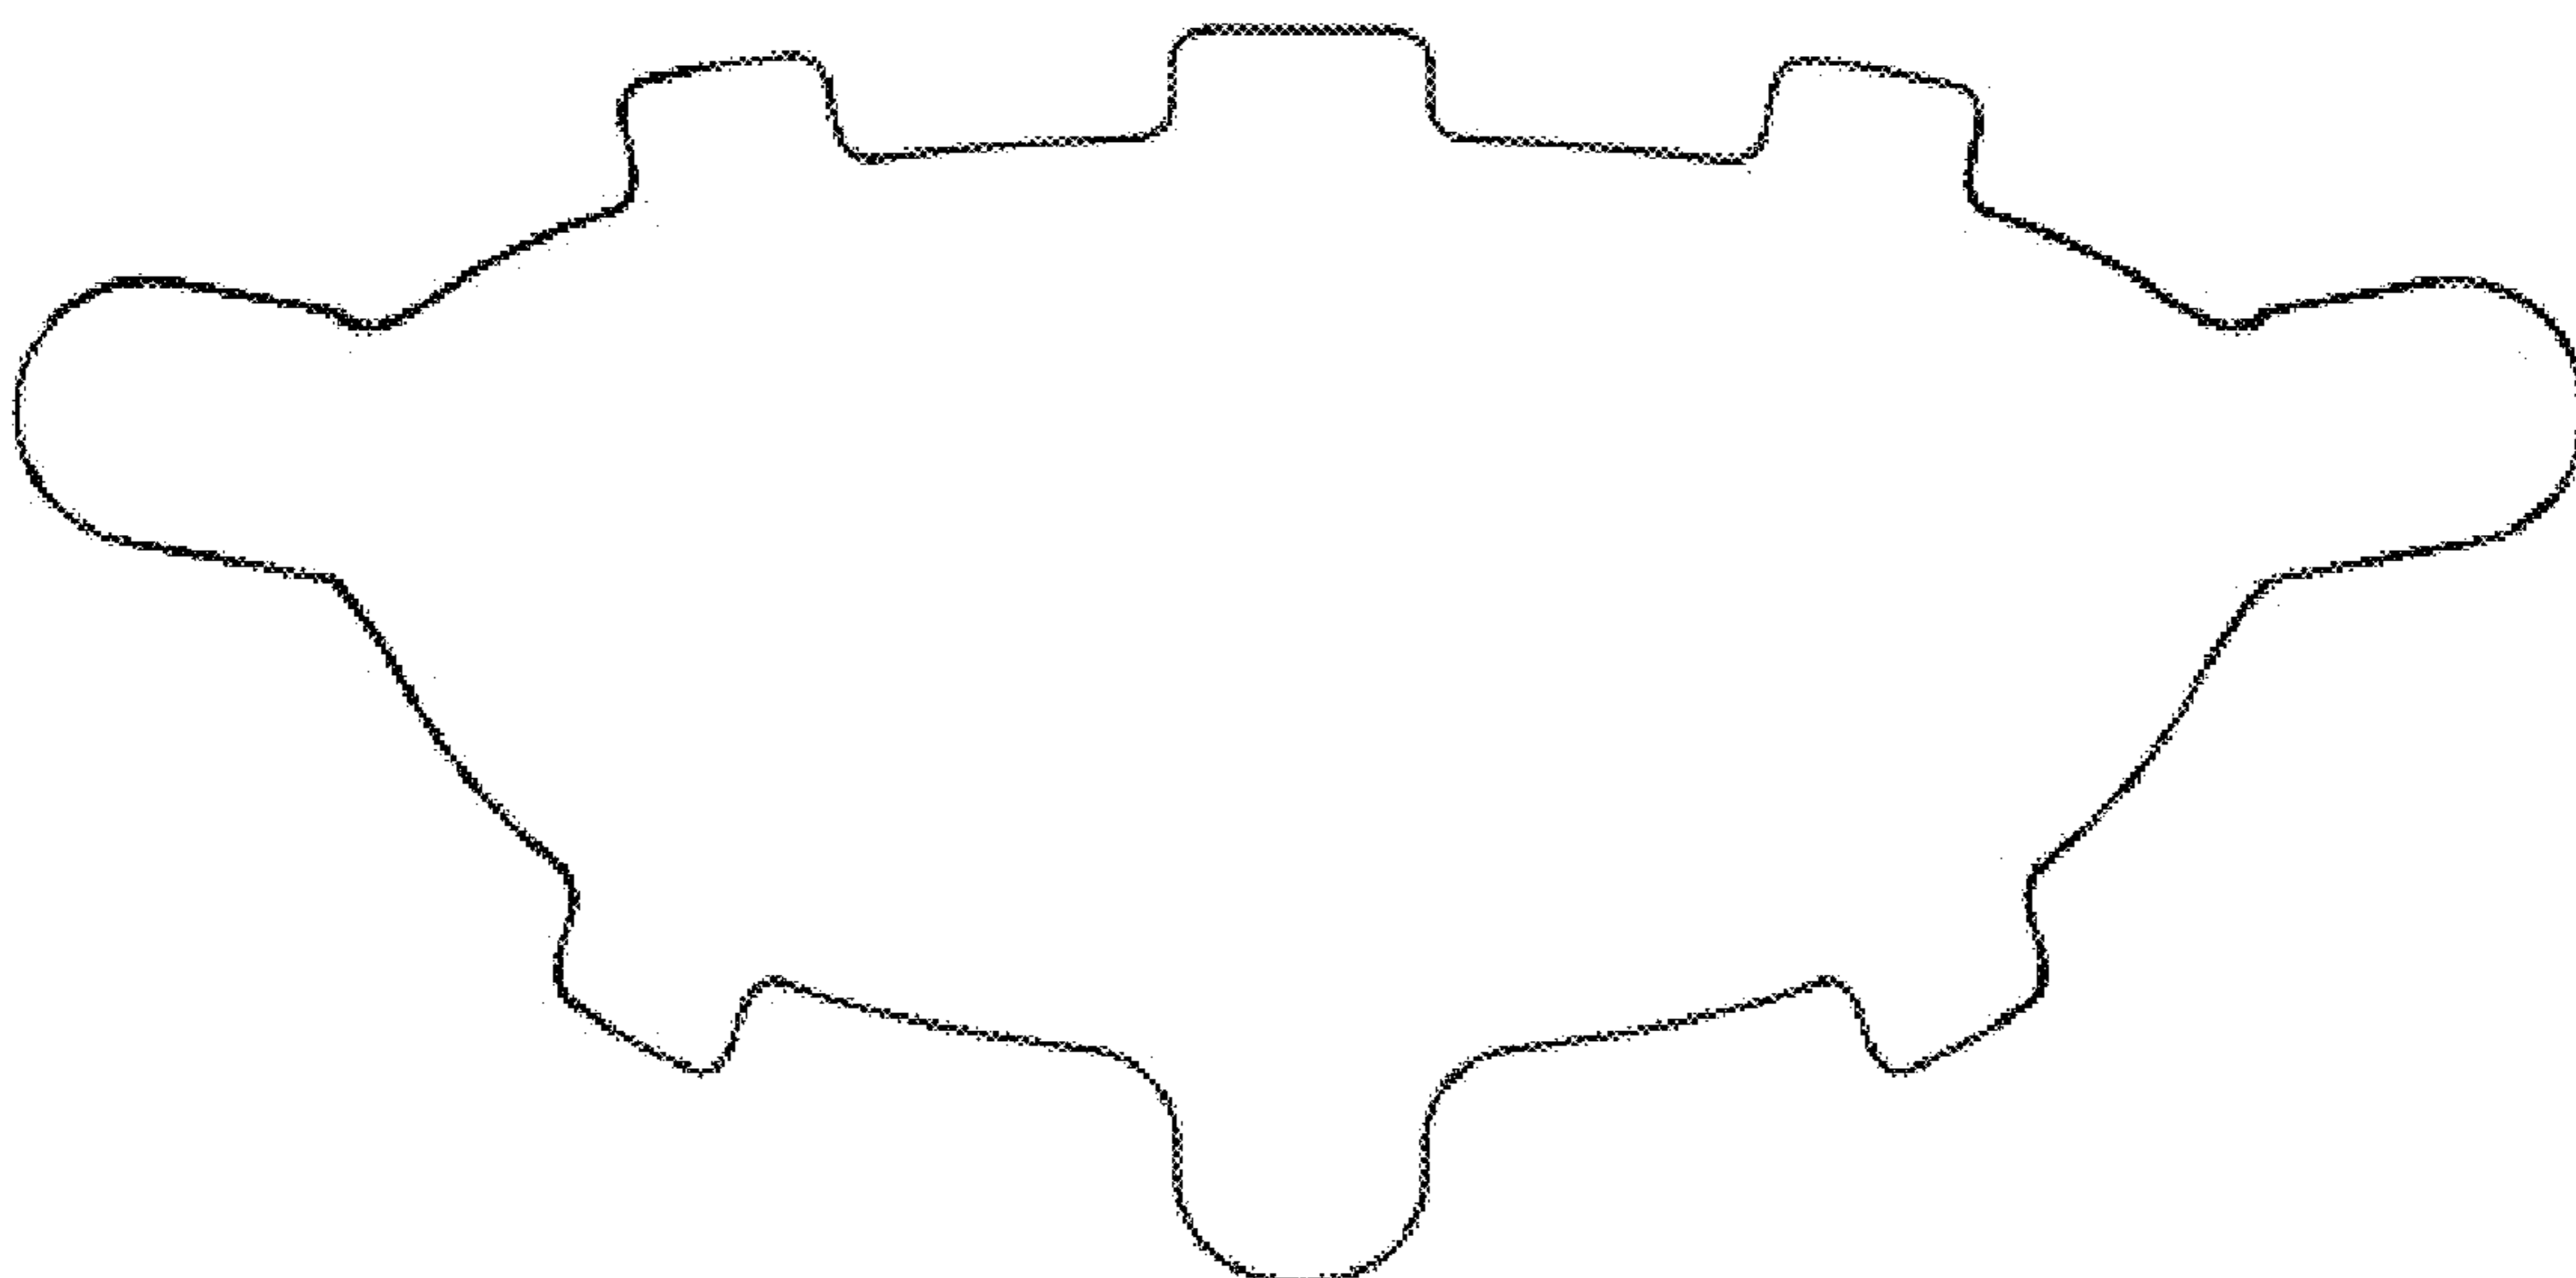

(56)

References Cited

OTHER PUBLICATIONS

DeBruijn, et al, "Mastopexy with Mesh Reinforcement: The Mechanical Characteristics of Polyester Mesh in the Female Breast," *Plast. Reconstr. Surg.* 124: 364, 2009.

European Search and Opinion dated Jul. 3, 2017, for 12754773.5-1666.

Goes, "Periareolar mammoplasty: double skin technique with application of polyglactine or mixed mesh," *Plast. Reconstr. Surg.* 97-959-68 (1996).

Goes, "Periareolar mammoplasty: double-skin technique with application of mesh support," *Clin Plastic Surg* 29 (2002) 349-364.

Goes, "Periareolar Mastopexy with FortaPerm," *Aesth. Plast. Surg.*, 34-350-8, 2010.

Hans De Bruijn, et al, "Mastopexy with Mesh Reinforcement: The Mechanical Characteristics of Polyester Mesh in the Female Breast," *Plast. Reconstr. Surg.* 124: 364, 2009.

Hans de Bruijn, Siegmund Johannes, "Mastopexy with 3D Preshaped Mesh for Long Term Results: Development of the Internal Bra System," *Aesth Plast Surg.*, 32:757-765, DOI 10.1007/s00266-008-9186-y, 2008.

International Search Report for PCT/US2019/015849, dated Apr. 23, 2019.

Johnson, Gerald W., "Central core reduction mammoplasties and Marlex suspension of breast tissue," *Aesthetic Plastic Surgery* 5:77-84, 1981.

Malluci, Concepts in aesthetic breast dimensions: Analysis of the ideal breast, *Journal of Plastic, Reconstructive & Aesthetic Surgery* (2012) 65, p. 8-16.

Malluci, Design for Natural Breast Augmentation: The Ice Principle, *Plastic and Reconstructive Surgery*, Jun. 2016, vol. 137 No. 6, 1728-1737.

Malluci, Population Analysis of the Perfect Breast: A Morphometric Analysis, (2014), *www.PRSJournal.com*, vol. 134, No. 3 • The Perfect Breast, p. 436- 447.

P. van Deventer, Improving the Longevity and Results of Mastopexy and Breast Reduction Procedures: Reconstructing an Internal Breast Support System with Biocompatible Mesh to Replace the Supporting Function of the Ligamentous Suspension, *Aesth Plast Surg* (2012) 36:578-589, DOI 10.1007/s00266-011-9845-2.

PCT International Search Report and Written Opinion of the International Searching Authority, dated Nov. 5, 2012 application No. PCT/US2012/027975.

Ray, J.A. et al., "Polydioxanone (PDS), a Novel Monofilament Synthetic Absorbable Suture", *Surgery, Gynecology & Obstetrics*, Oct. 1981, vol. 153, 497-507.

Supplementary European Search Report of the EPO dated Jul. 30, 2014, EP 12754773.5 from PCT/US2012/027075.

Williams "Poly-4-hydroxybutyrate (P4HB): a new generation of resorbable medical devices for tissue repair and regeneration," DOI 10.1515/bmt-2013-0009 *Biomed Tech* 2013; 58(5): 439-452.

Written Opinion of IPEA dated Jun. 15, 2015 for PCT/US2014/046420.

Written Opinion of ISR dated Nov. 5, 2012 for PCT/US2012/027975.

* cited by examiner

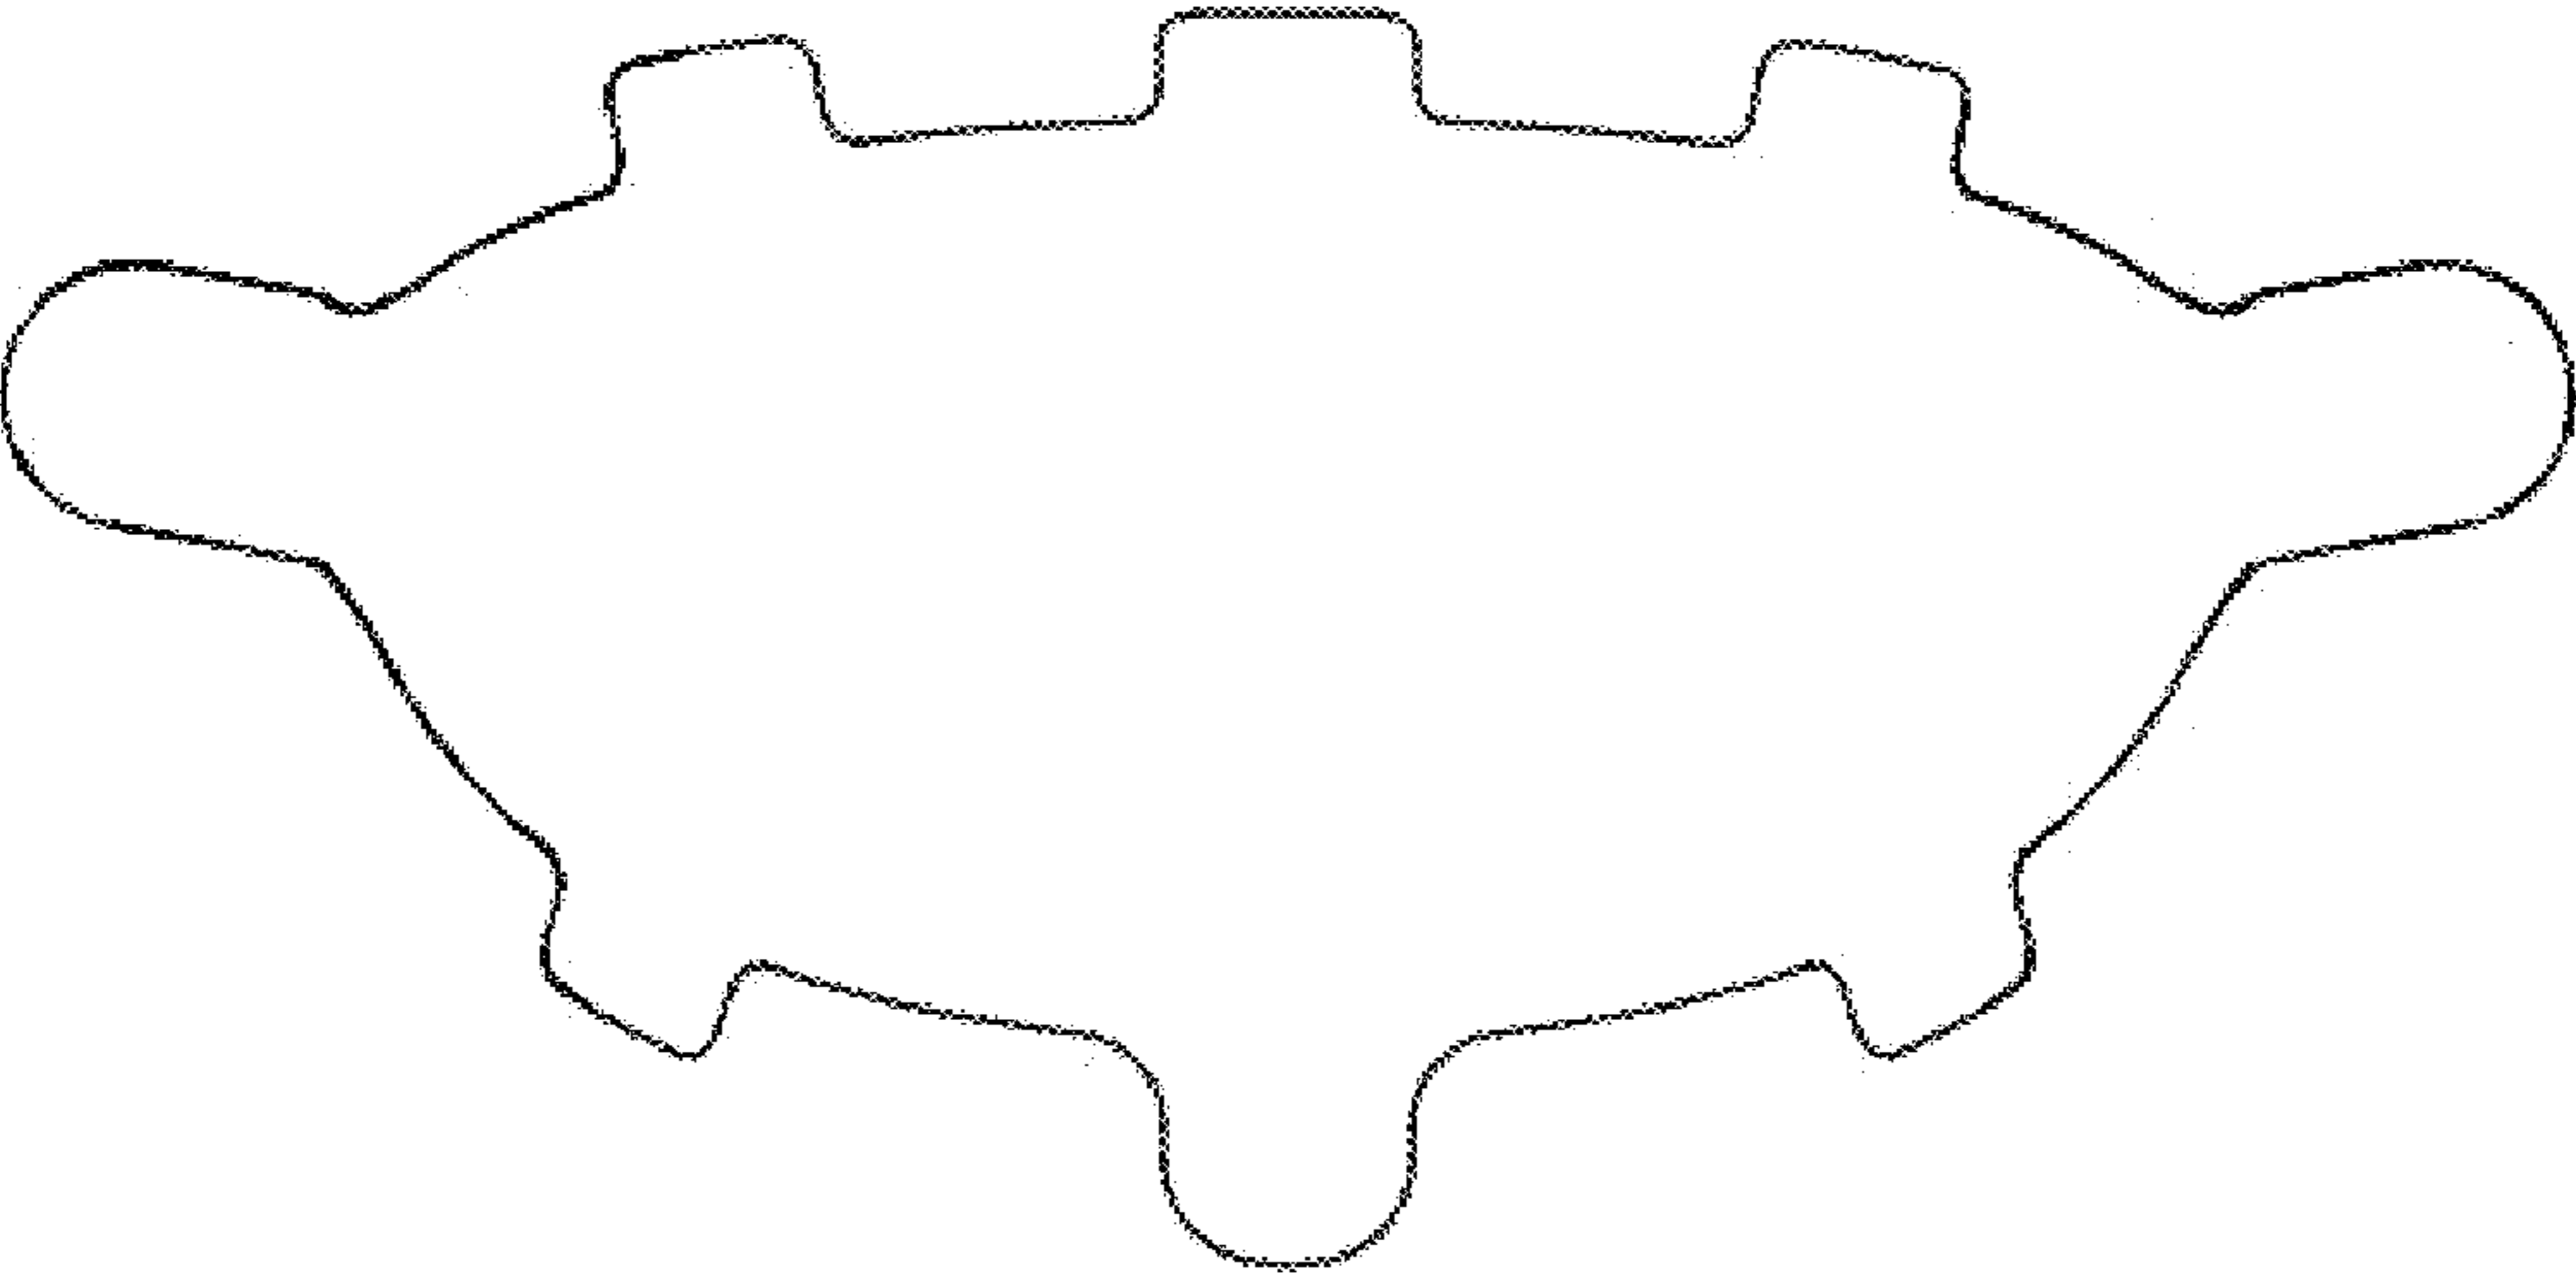


Figure 1

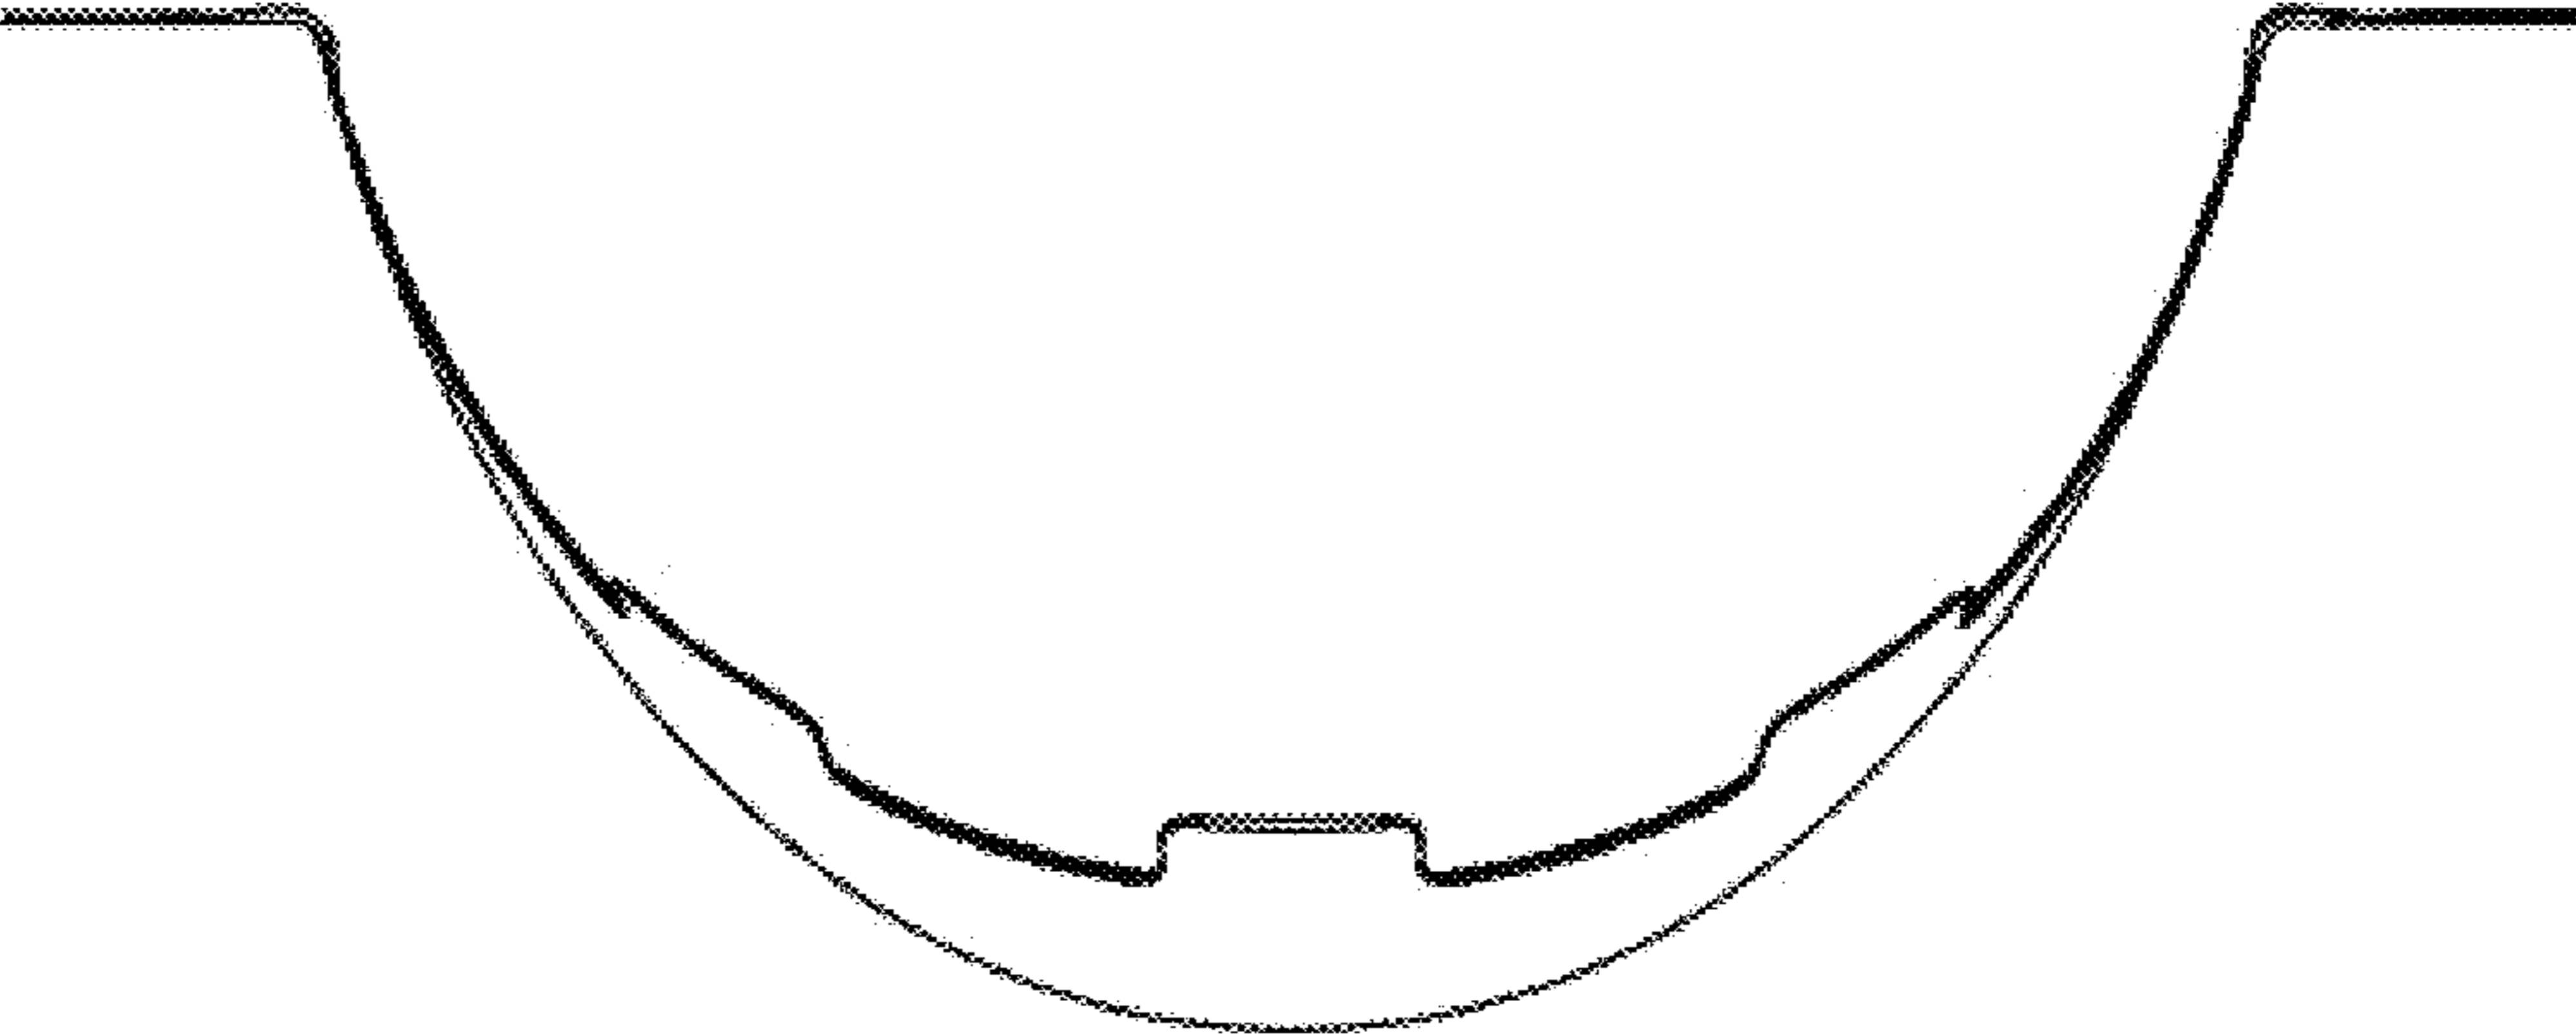


Figure 2

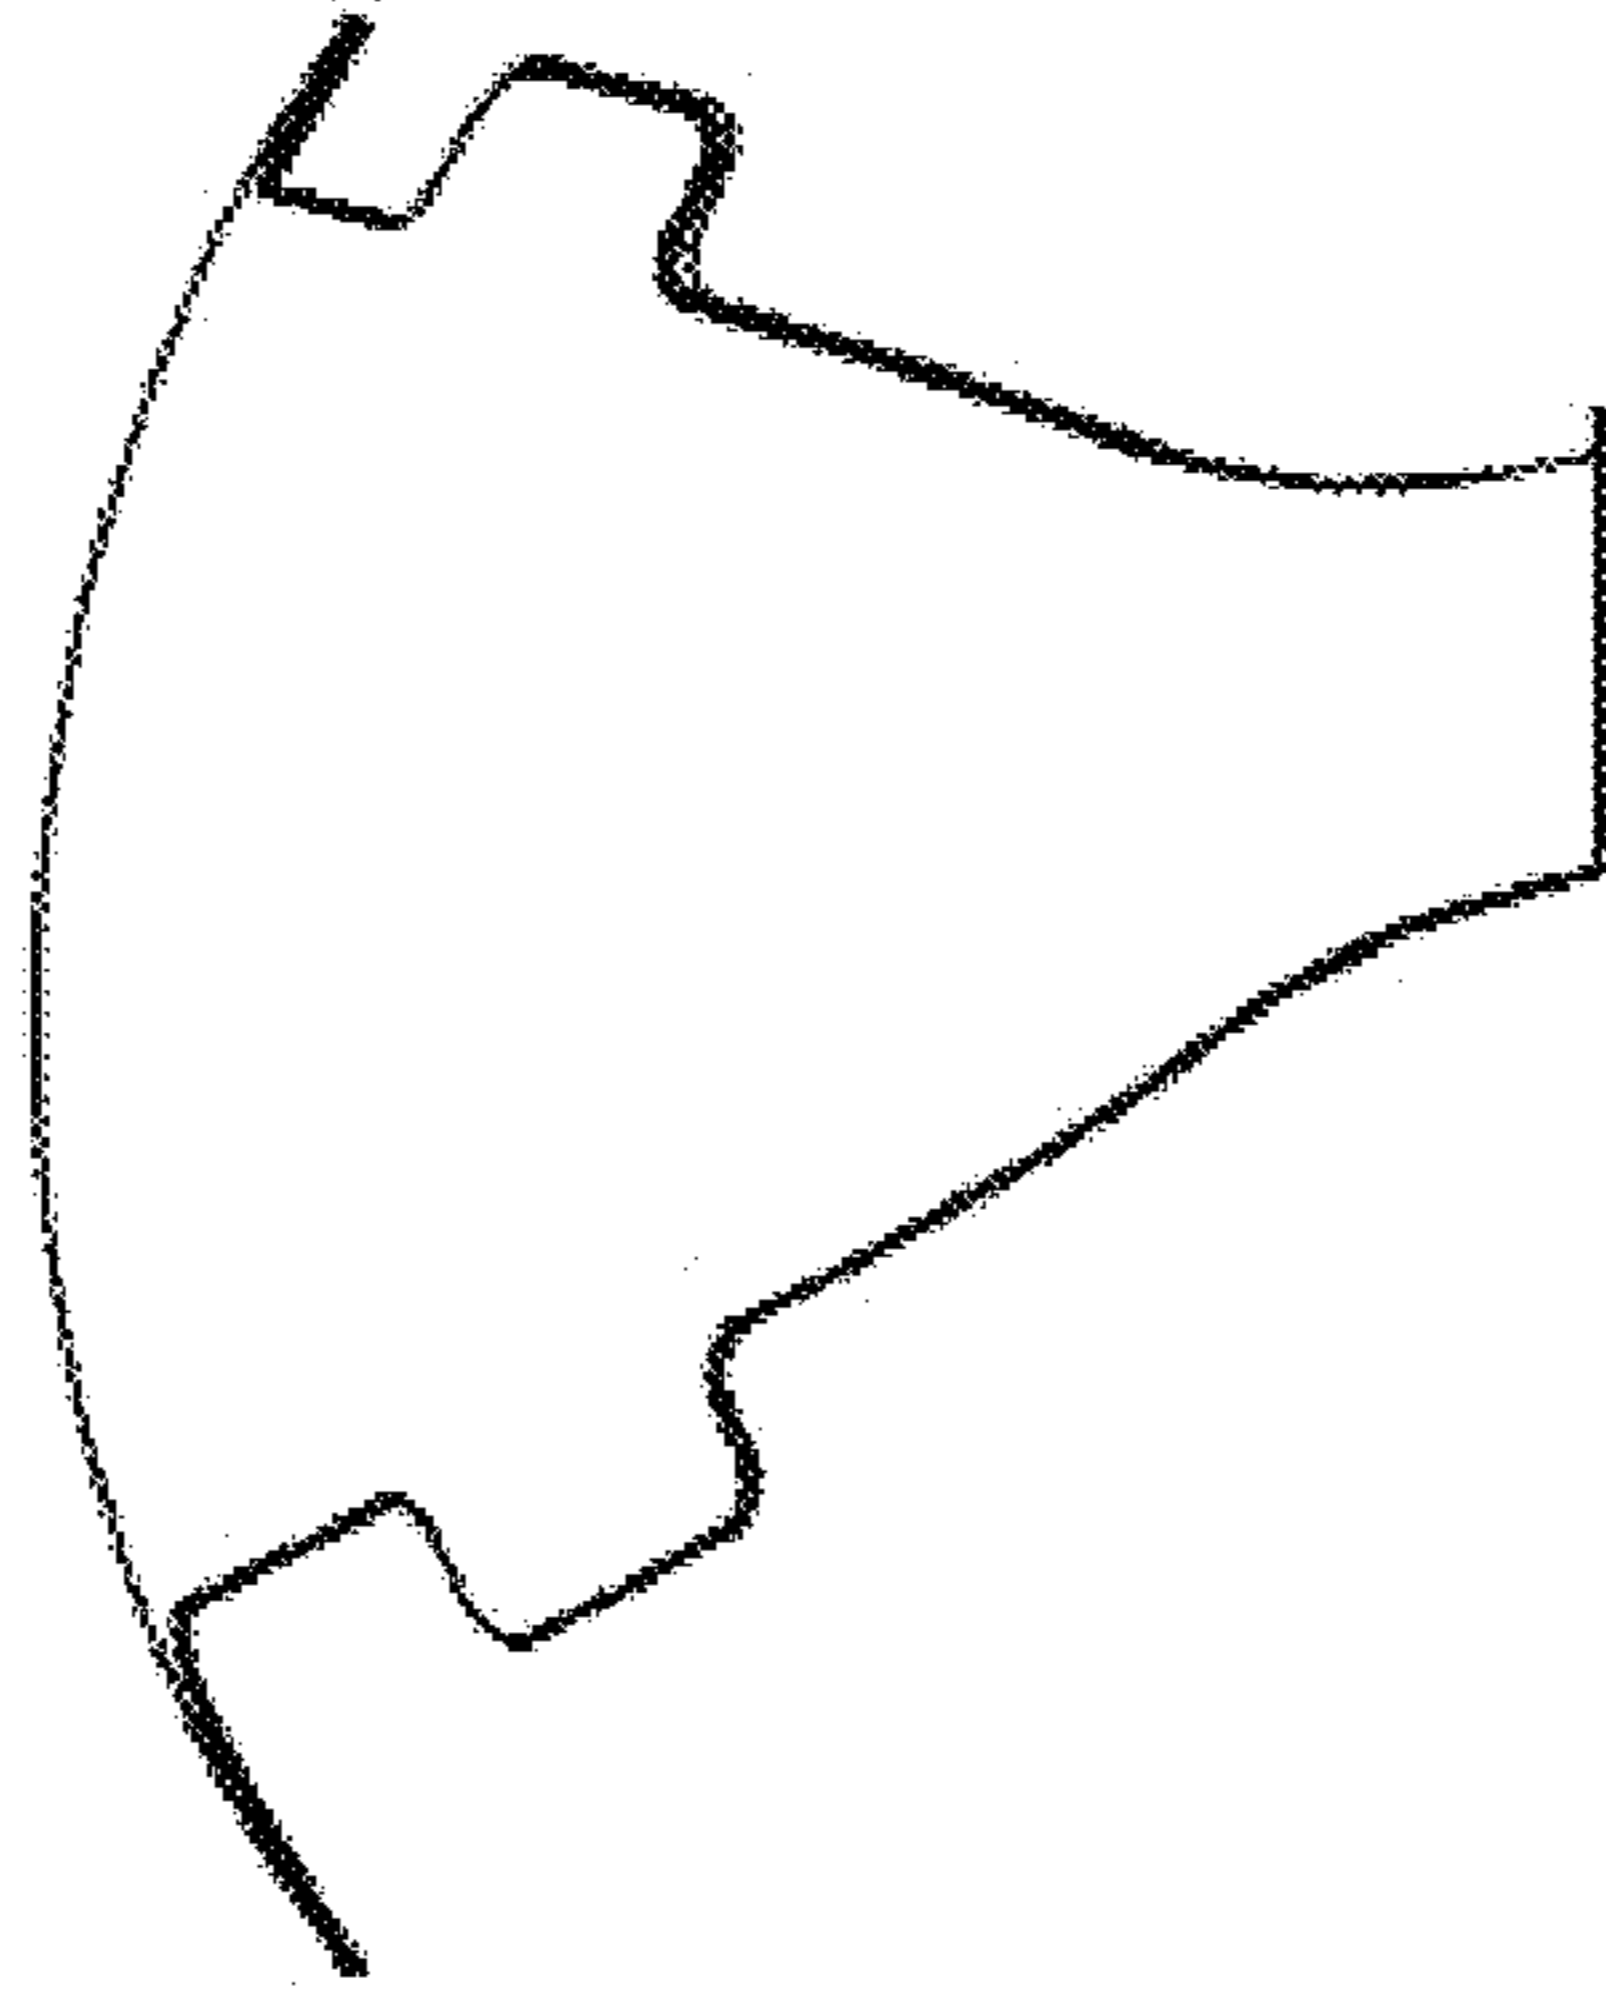


Figure 3

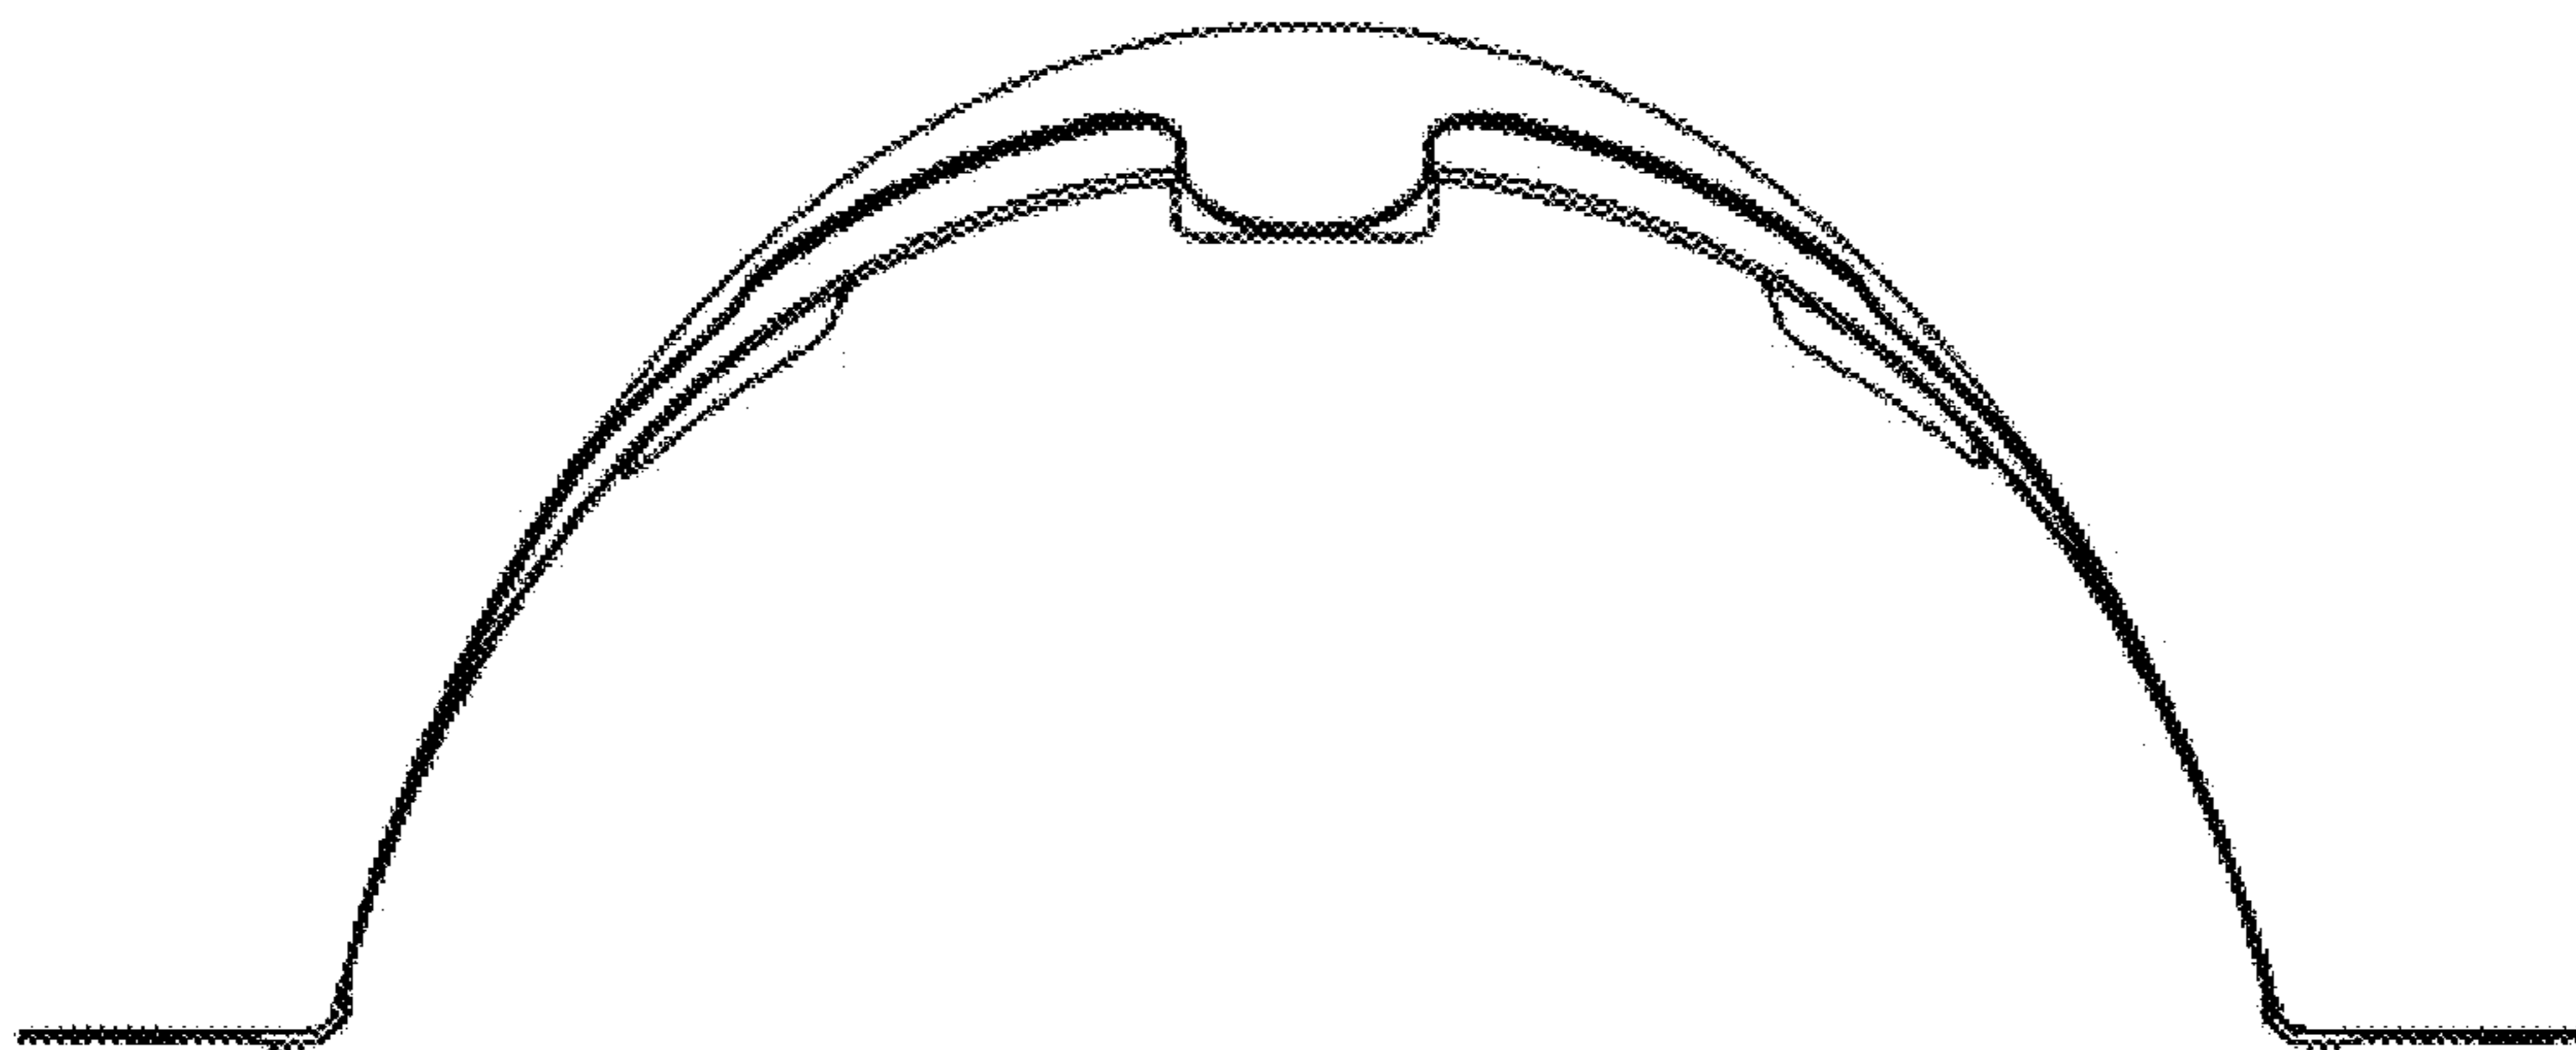


Figure 4

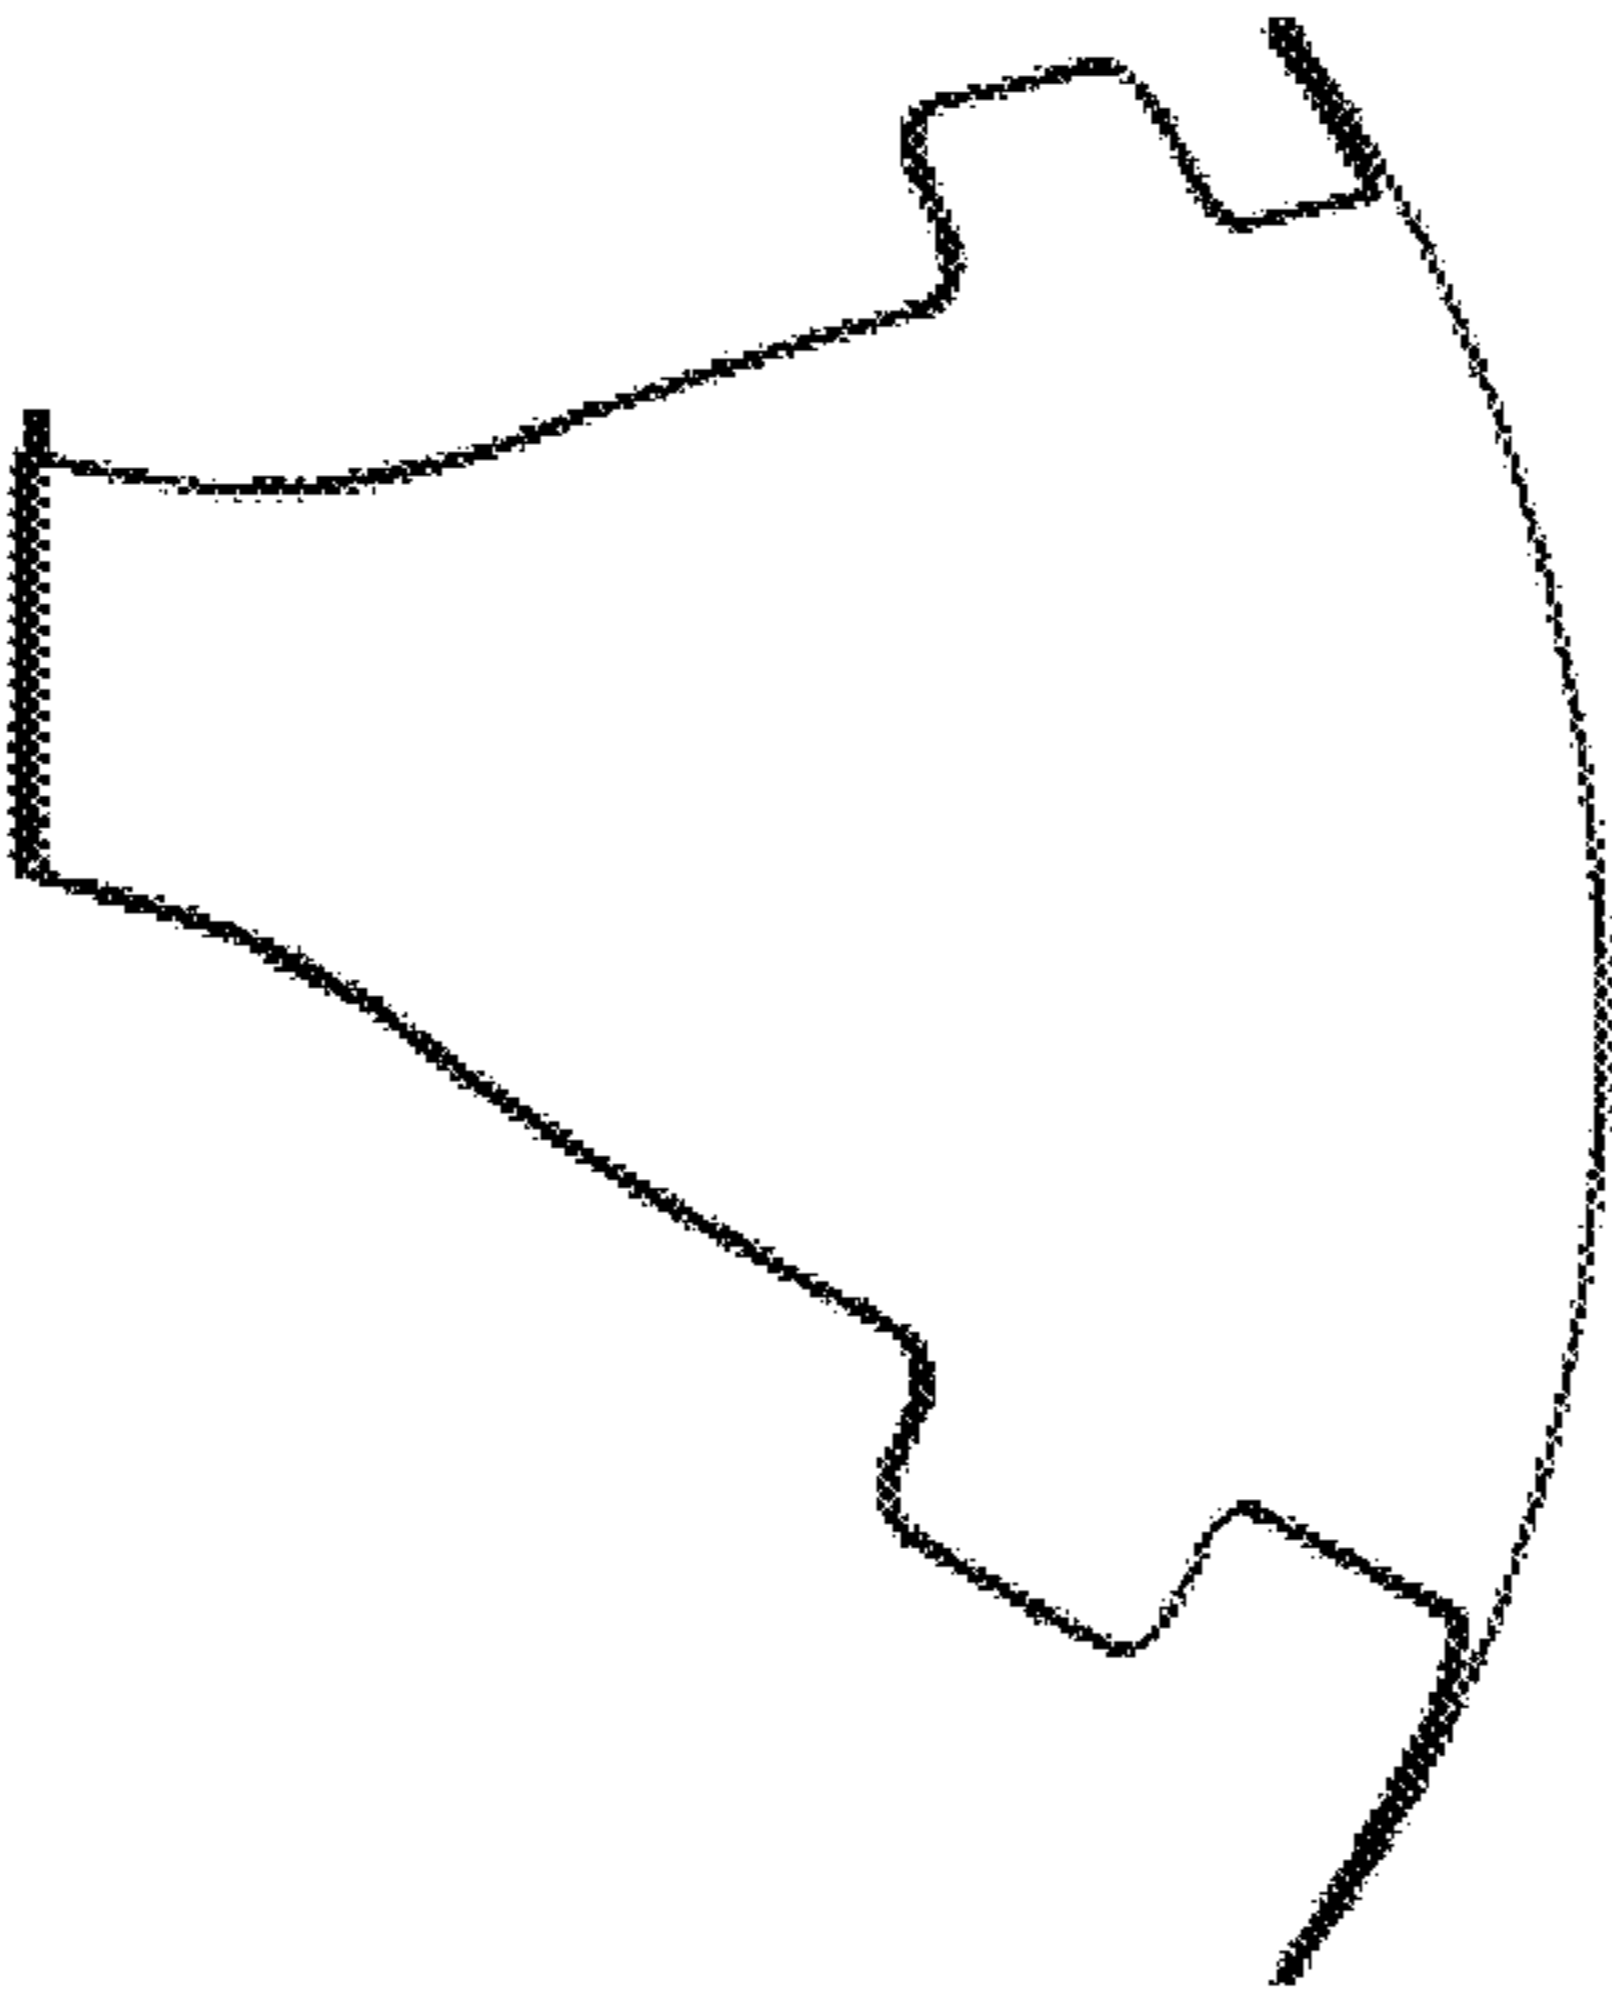


Figure 5

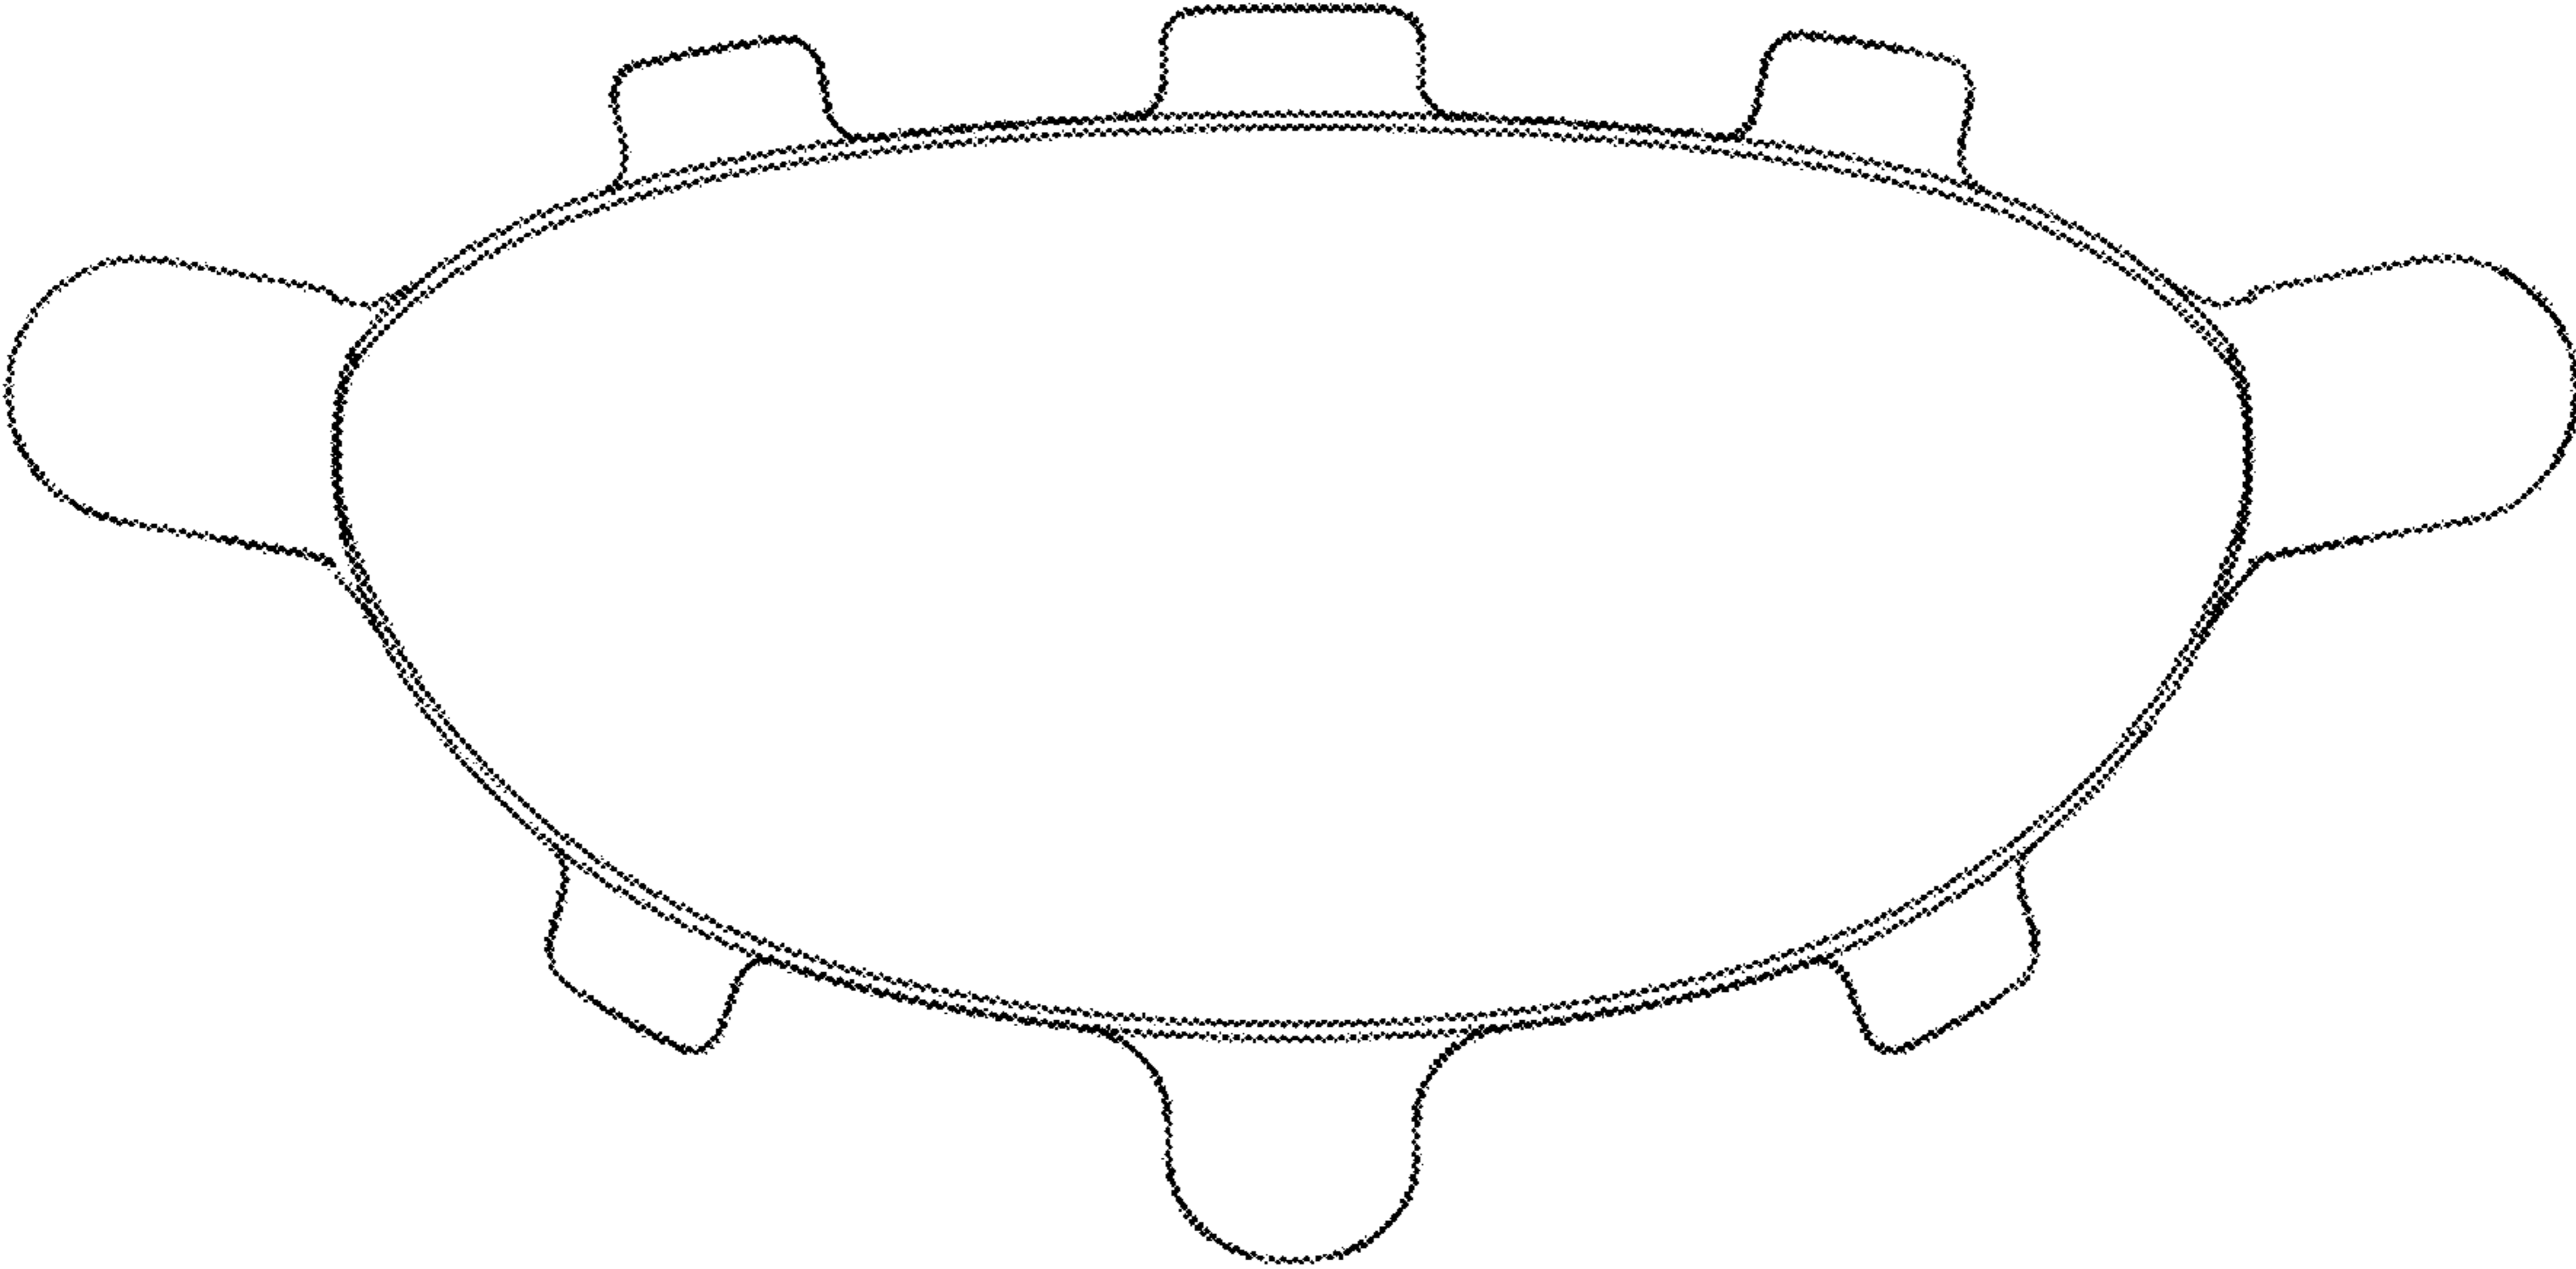


Figure 6

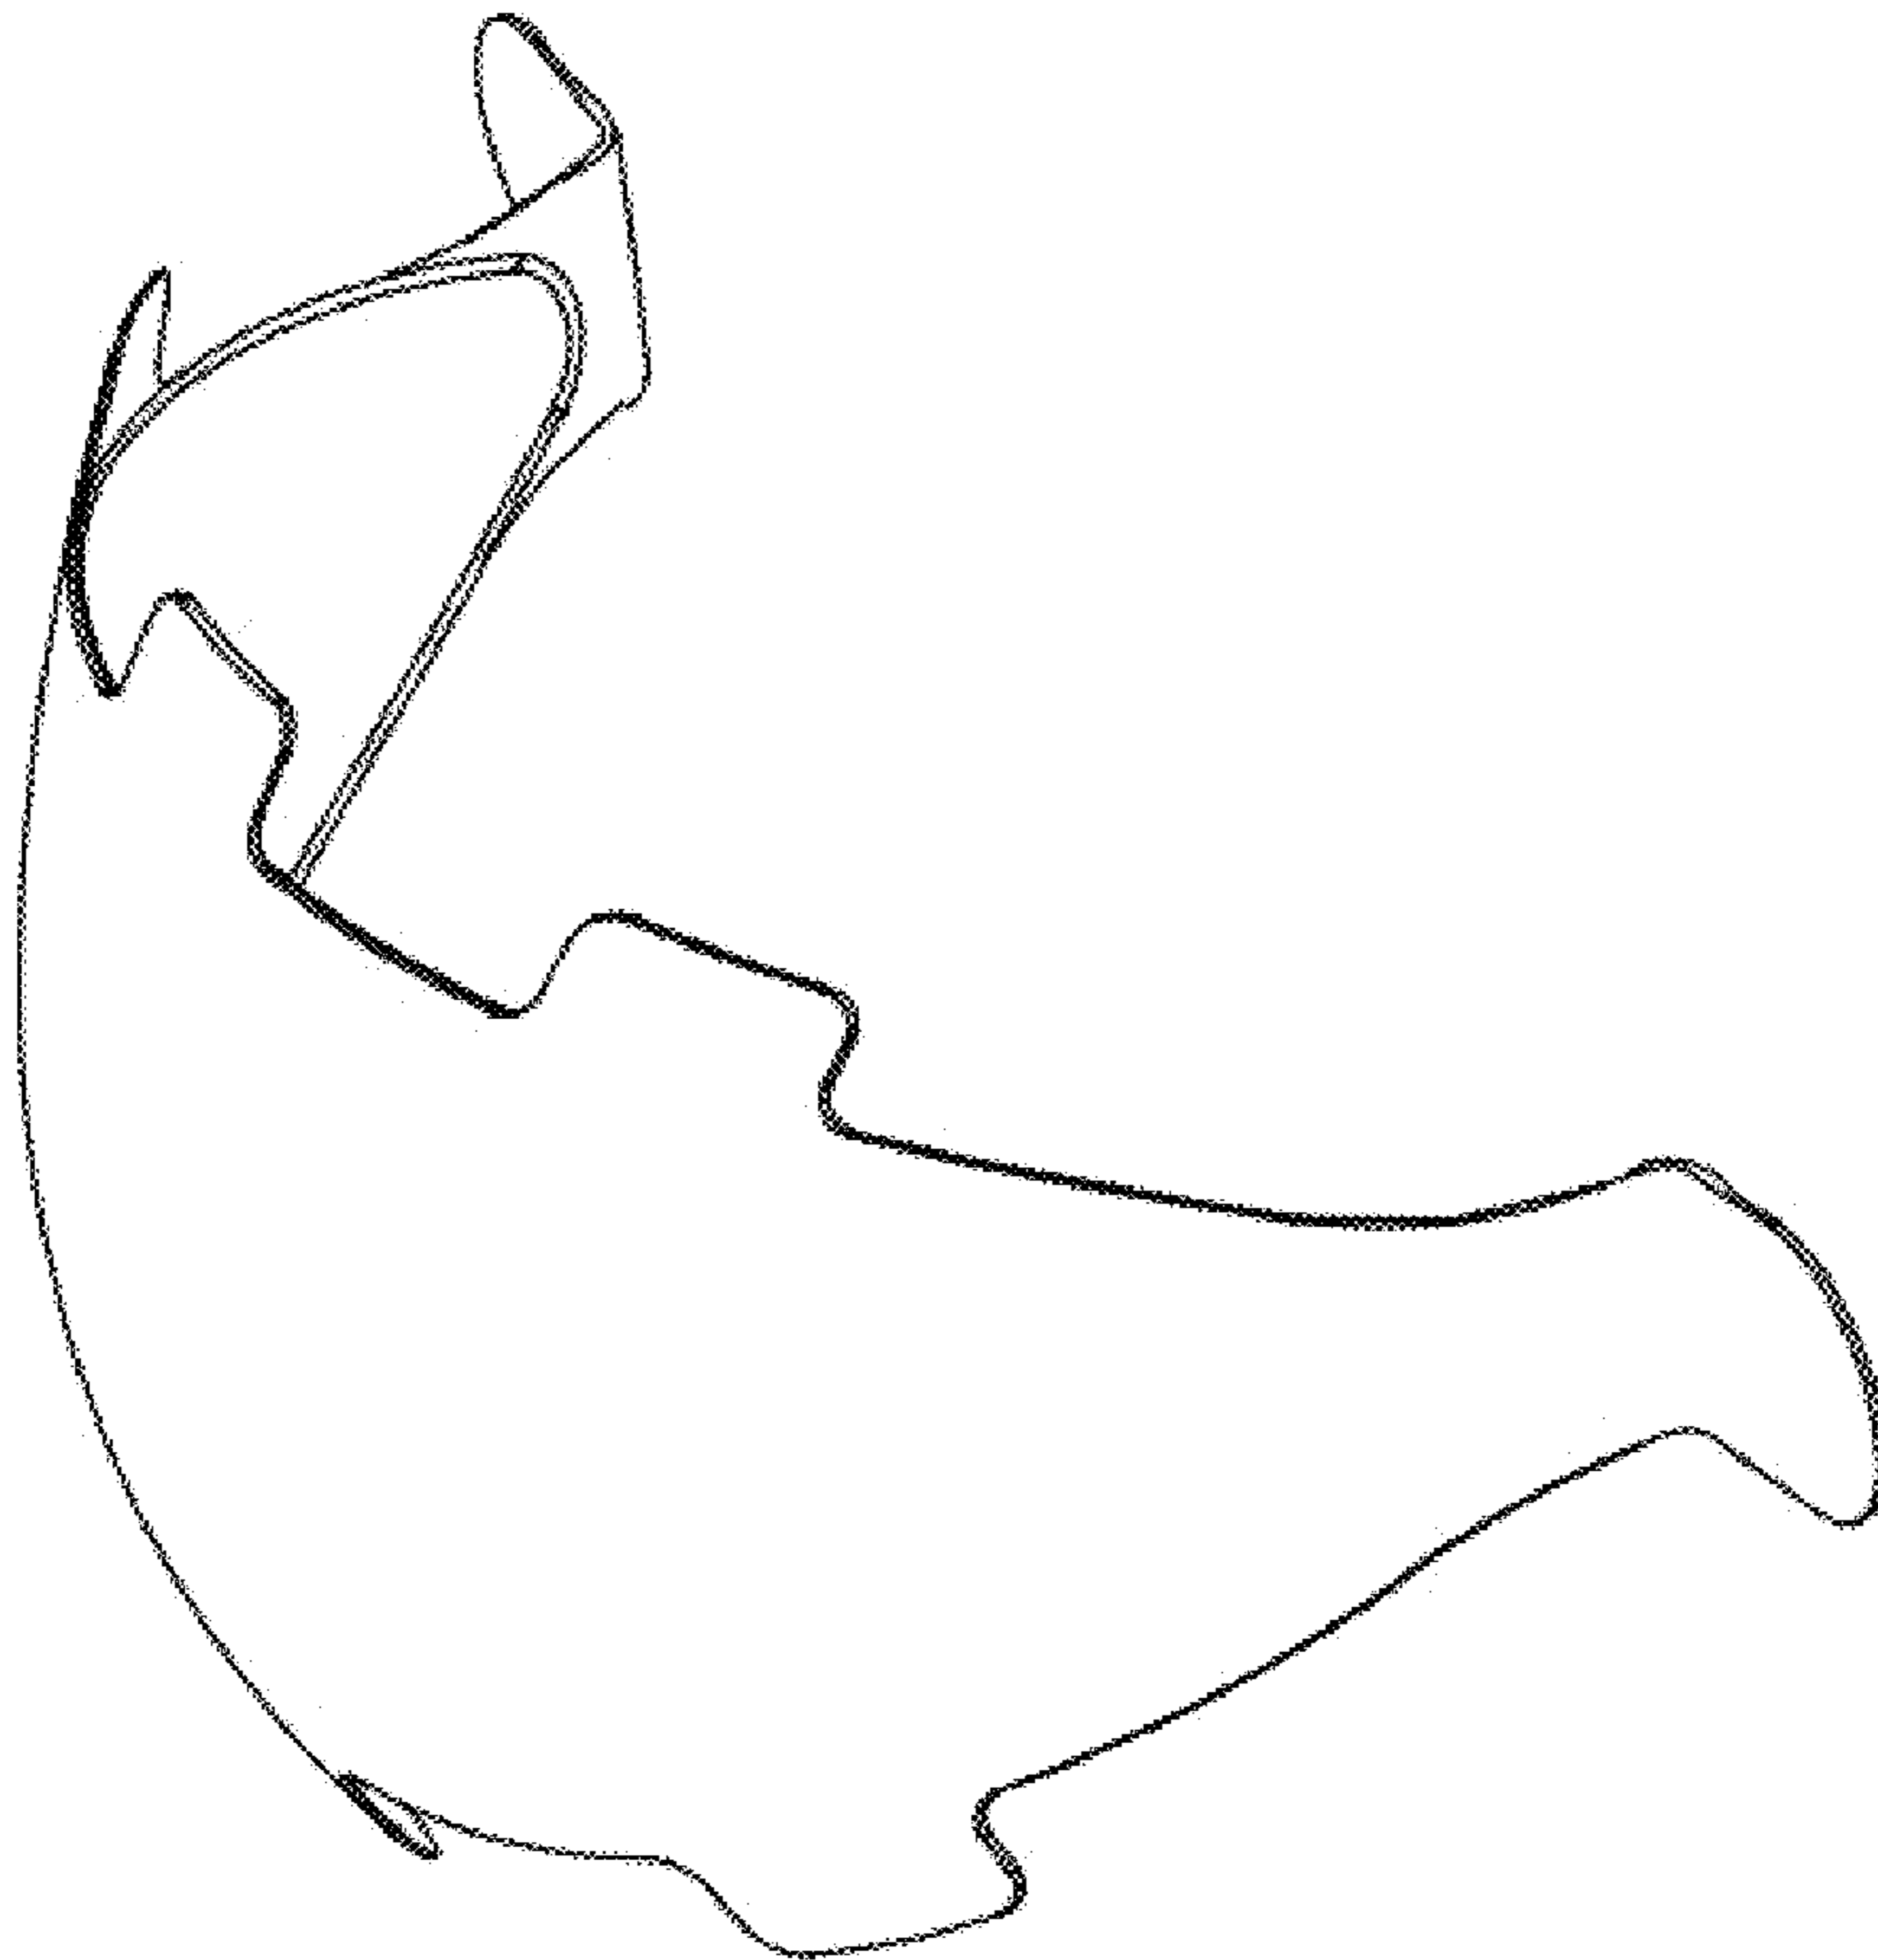


Figure 7