



US00D928931S

(12) **United States Design Patent** (10) **Patent No.:** **US D928,931 S**
Lyu et al. (45) **Date of Patent:** **** Aug. 24, 2021**

(54) **FILTRATION AND STERILIZATION DEVICE FOR RESPIRATORY DROPLET**

(71) Applicant: **Guangzhou Ajax Medical Equipment Co., Ltd.**, Guangzhou (CN)

(72) Inventors: **Bing Lyu**, Guangzhou (CN); **Yuansheng Zhou**, Guangzhou (CN); **Xuehua Huang**, Guangzhou (CN); **Qing Xiang**, Guangzhou (CN); **Zhijie Li**, Guangzhou (CN)

(73) Assignee: **GUANGZHOU AJAX MEDICAL EQUIPMENT CO., LTD.**, Guangzhou (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/733,140**

(22) Filed: **Apr. 29, 2020**

(30) **Foreign Application Priority Data**

Mar. 6, 2020 (CN) 202030072773.7

(51) **LOC (13) Cl.** **23-04**

(52) **U.S. Cl.**
USPC **D23/364**

(58) **Field of Classification Search**
USPC D23/355–366, 352, 369, 332, 333, 335, D23/336, 342, 351; 422/120, 122; 55/356, 473, 504; 96/97; 261/DIG. 17, 261/DIG. 65, DIG. 88, DIG. 31
CPC .. A61L 9/16; A61L 9/22; B01D 47/00; B01D 47/027; B01D 2221/02; B01D 2259/4508; B03C 3/155; B03C 3/368; F24F 3/16; F24F 13/20; F24F 13/28

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | |
|-----------|------|---------|----------|-------|--------------|
| 5,154,893 | A * | 10/1992 | Nakade | | A61L 9/122 |
| | | | | | 422/122 |
| 5,188,644 | A * | 2/1993 | Landy | | B01D 46/2411 |
| | | | | | 422/122 |
| 5,267,371 | A * | 12/1993 | Soler | | A47L 5/36 |
| | | | | | 15/327.5 |
| 5,281,246 | A * | 1/1994 | Ray | | B01D 46/002 |
| | | | | | 55/302 |
| 6,143,048 | A * | 11/2000 | Comproni | | B01D 46/0036 |
| | | | | | 118/326 |
| 6,663,698 | B2 * | 12/2003 | Mishin | | B01D 46/0005 |
| | | | | | 55/320 |
| 8,460,417 | B2 * | 6/2013 | Reid | | B08B 15/04 |
| | | | | | 55/356 |
| D771,786 | S * | 11/2016 | Canipe | | D23/333 |
| D780,898 | S * | 3/2017 | Canipe | | D23/333 |

(Continued)

Primary Examiner — David G Muller

(74) *Attorney, Agent, or Firm* — Bayramoglu Law Offices LLC


(57) **CLAIM**

The ornamental design for a filtration and sterilization device for respiratory droplet, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a filtration and sterilization device for respiratory droplet showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a left side elevational view thereof; FIG. 5 is a right side elevational view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof. The broken lines depict portions of the filtration and sterilization device for respiratory droplet in which the design is embodied that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

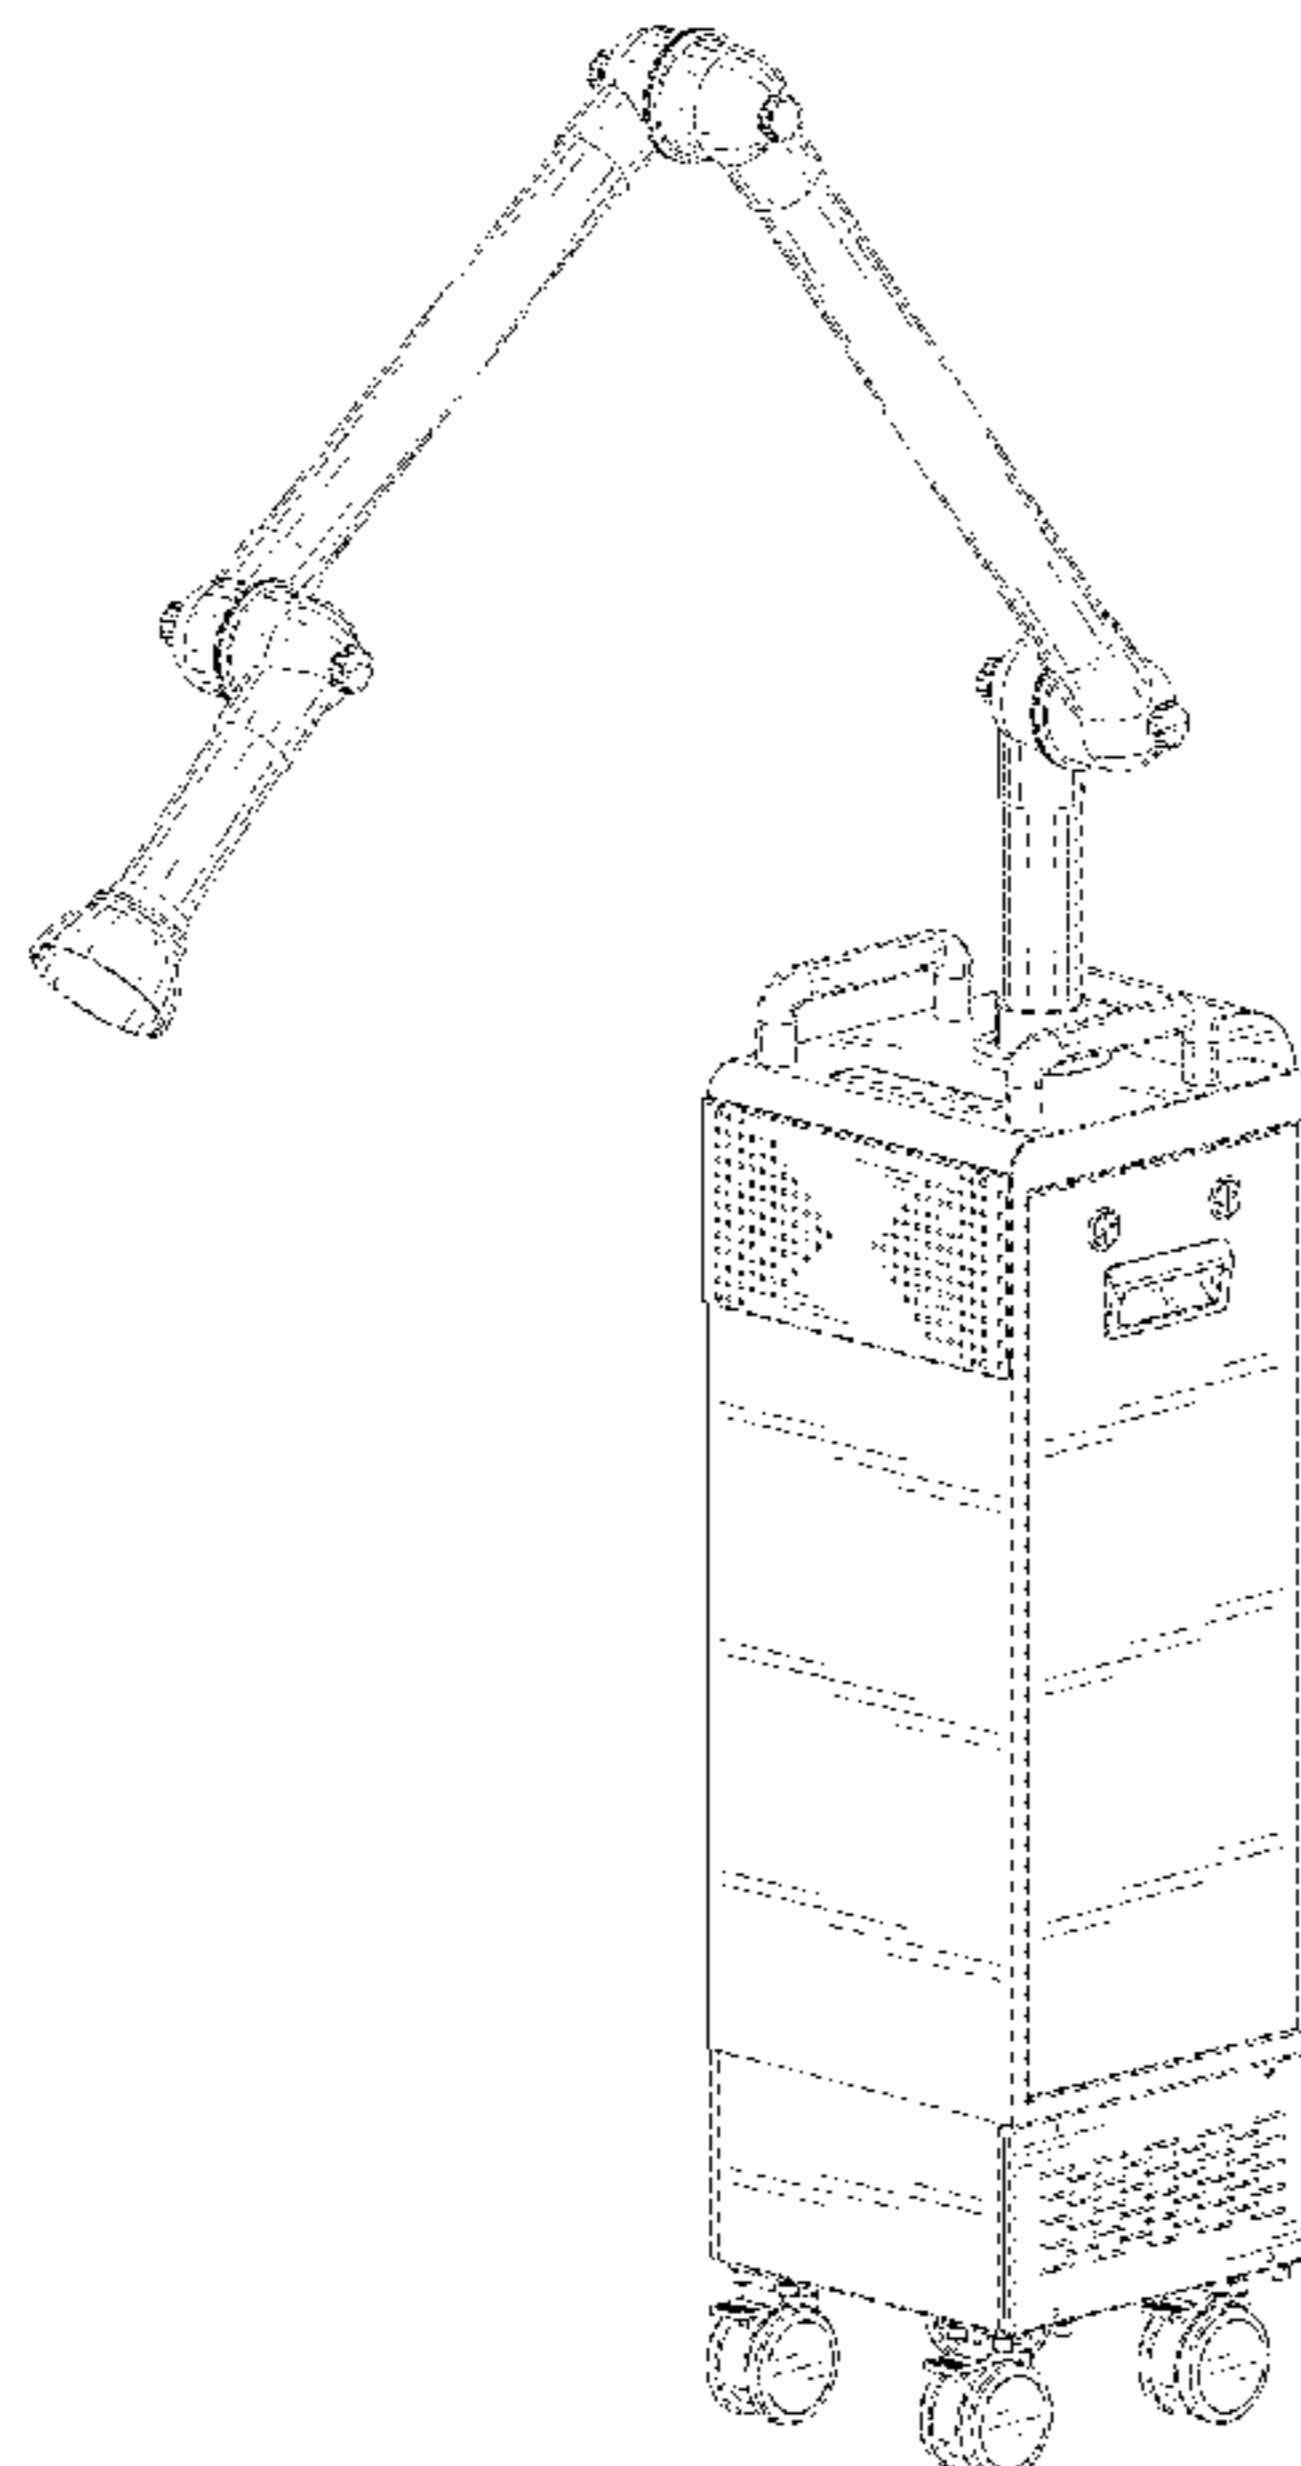

(56)

References Cited

U.S. PATENT DOCUMENTS

D918,360 S * 5/2021 Francis D23/335
2011/0223071 A1* 9/2011 Kang B01D 46/0036
422/169
2018/0133084 A1* 5/2018 Kirschman B01D 46/0028
2021/0128769 A1* 5/2021 Zhang B01D 46/4245

* cited by examiner

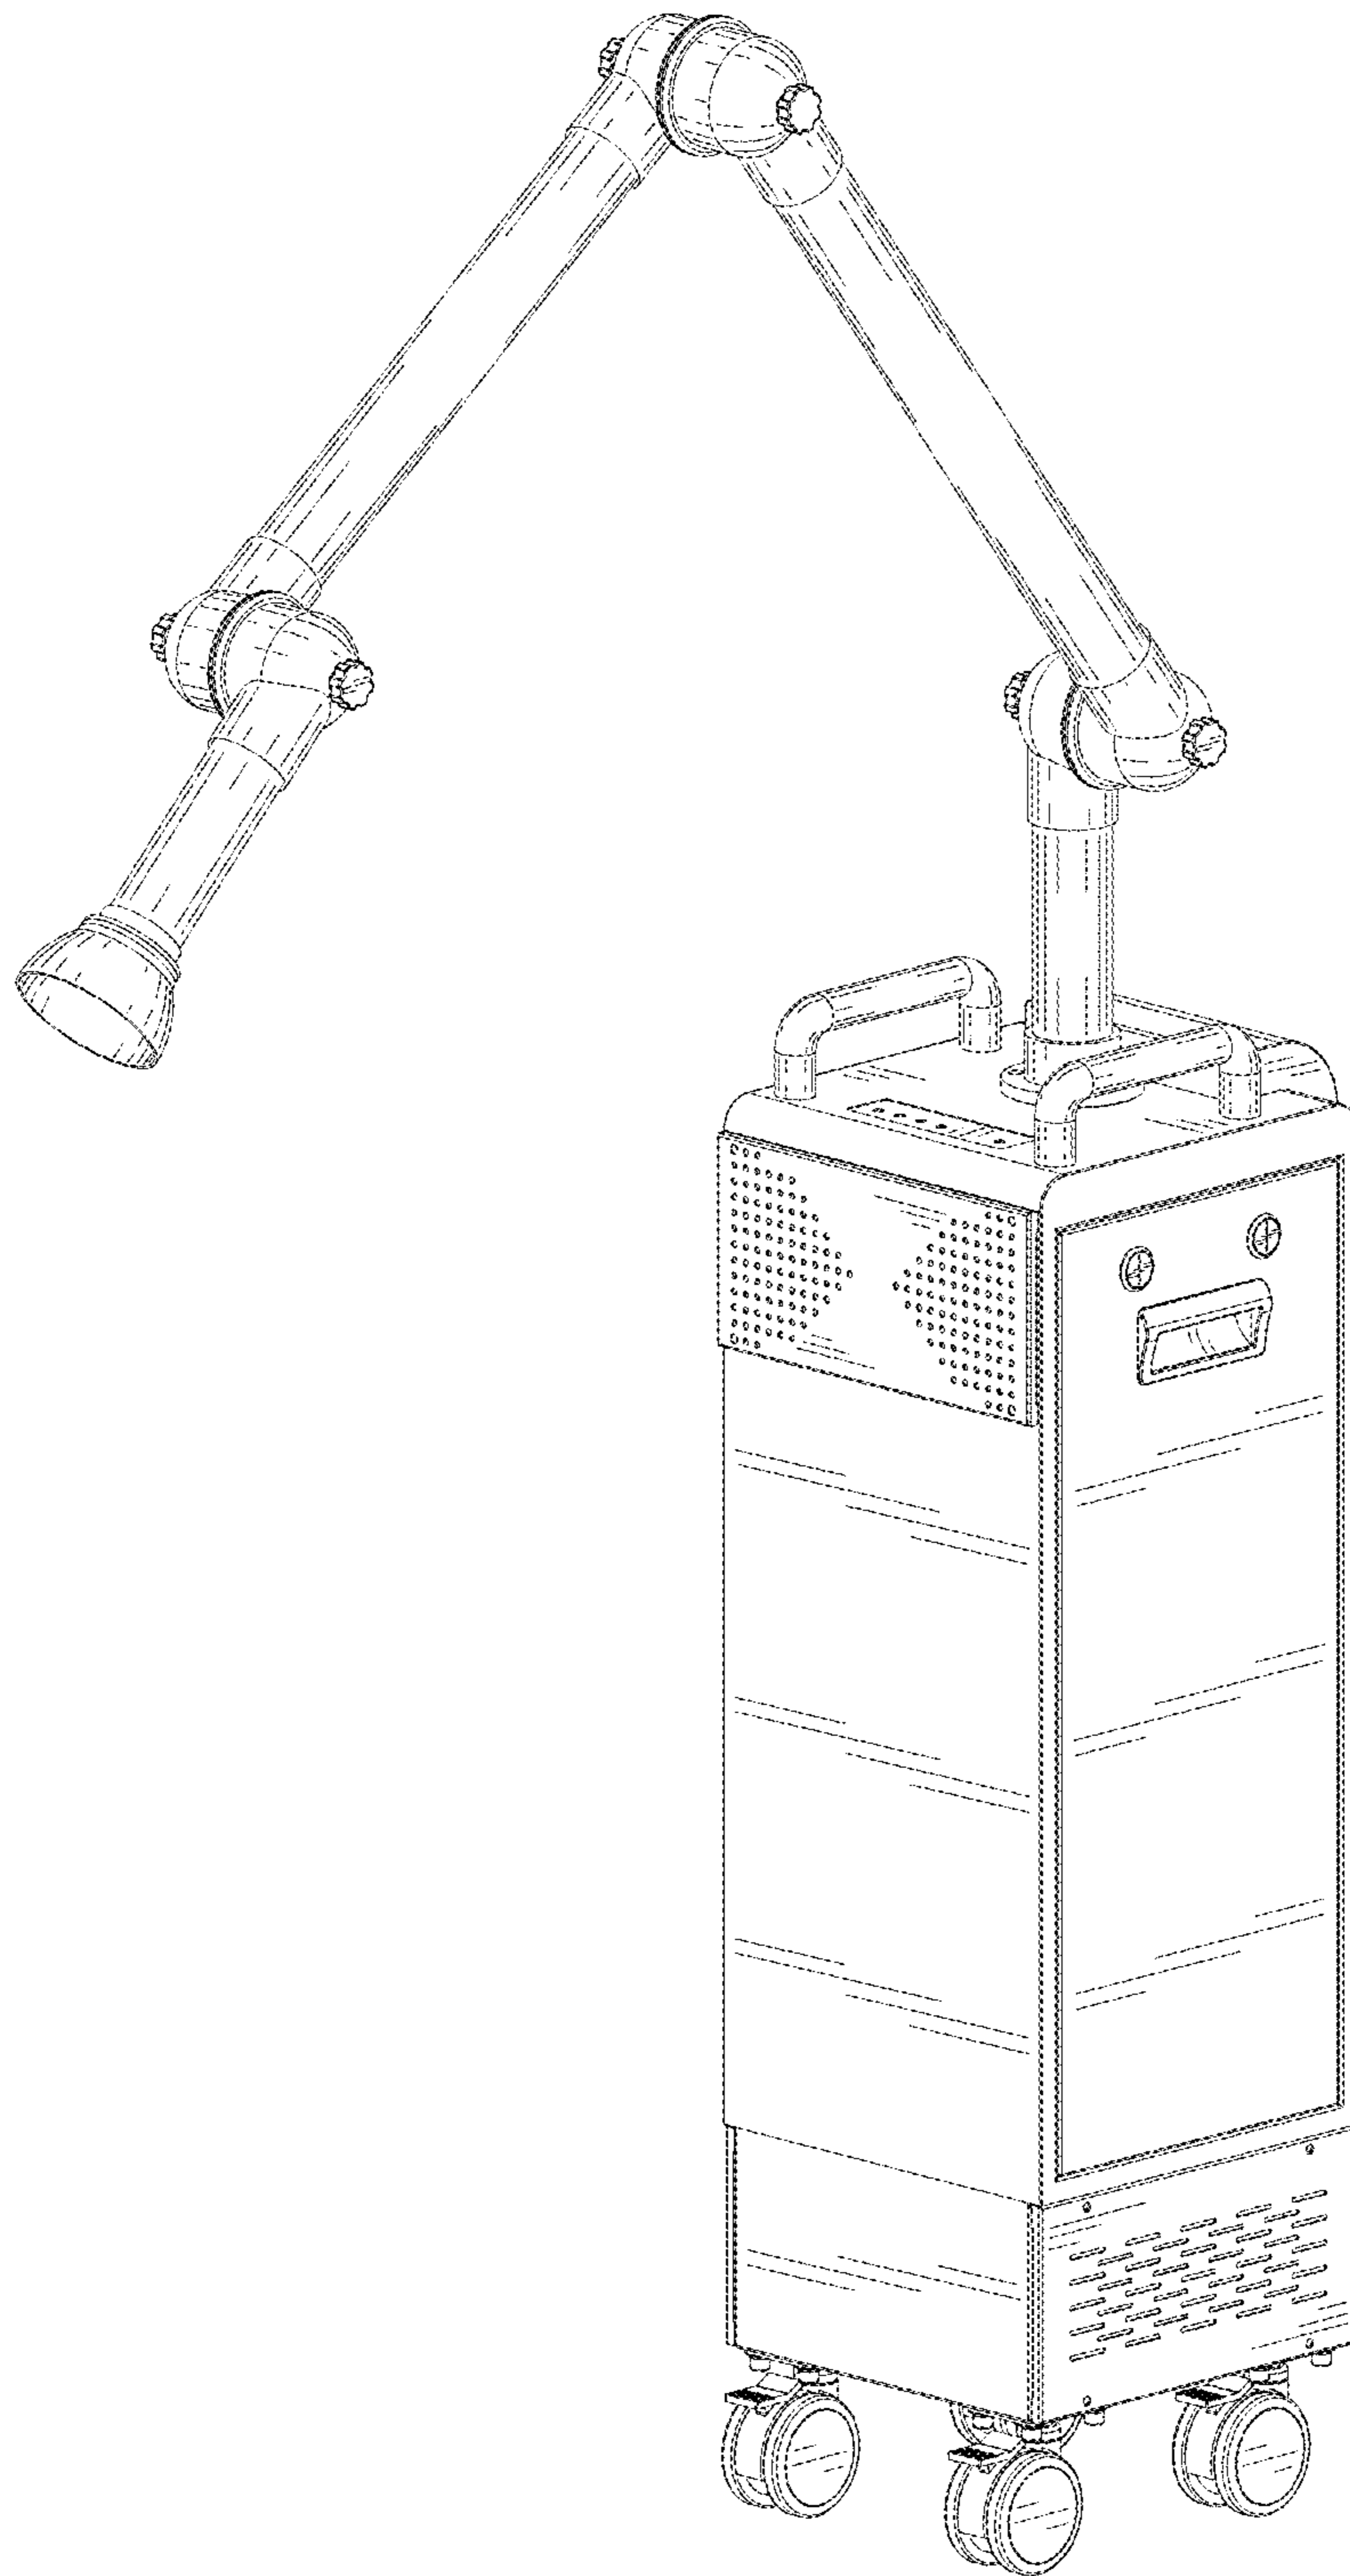


FIG. 1

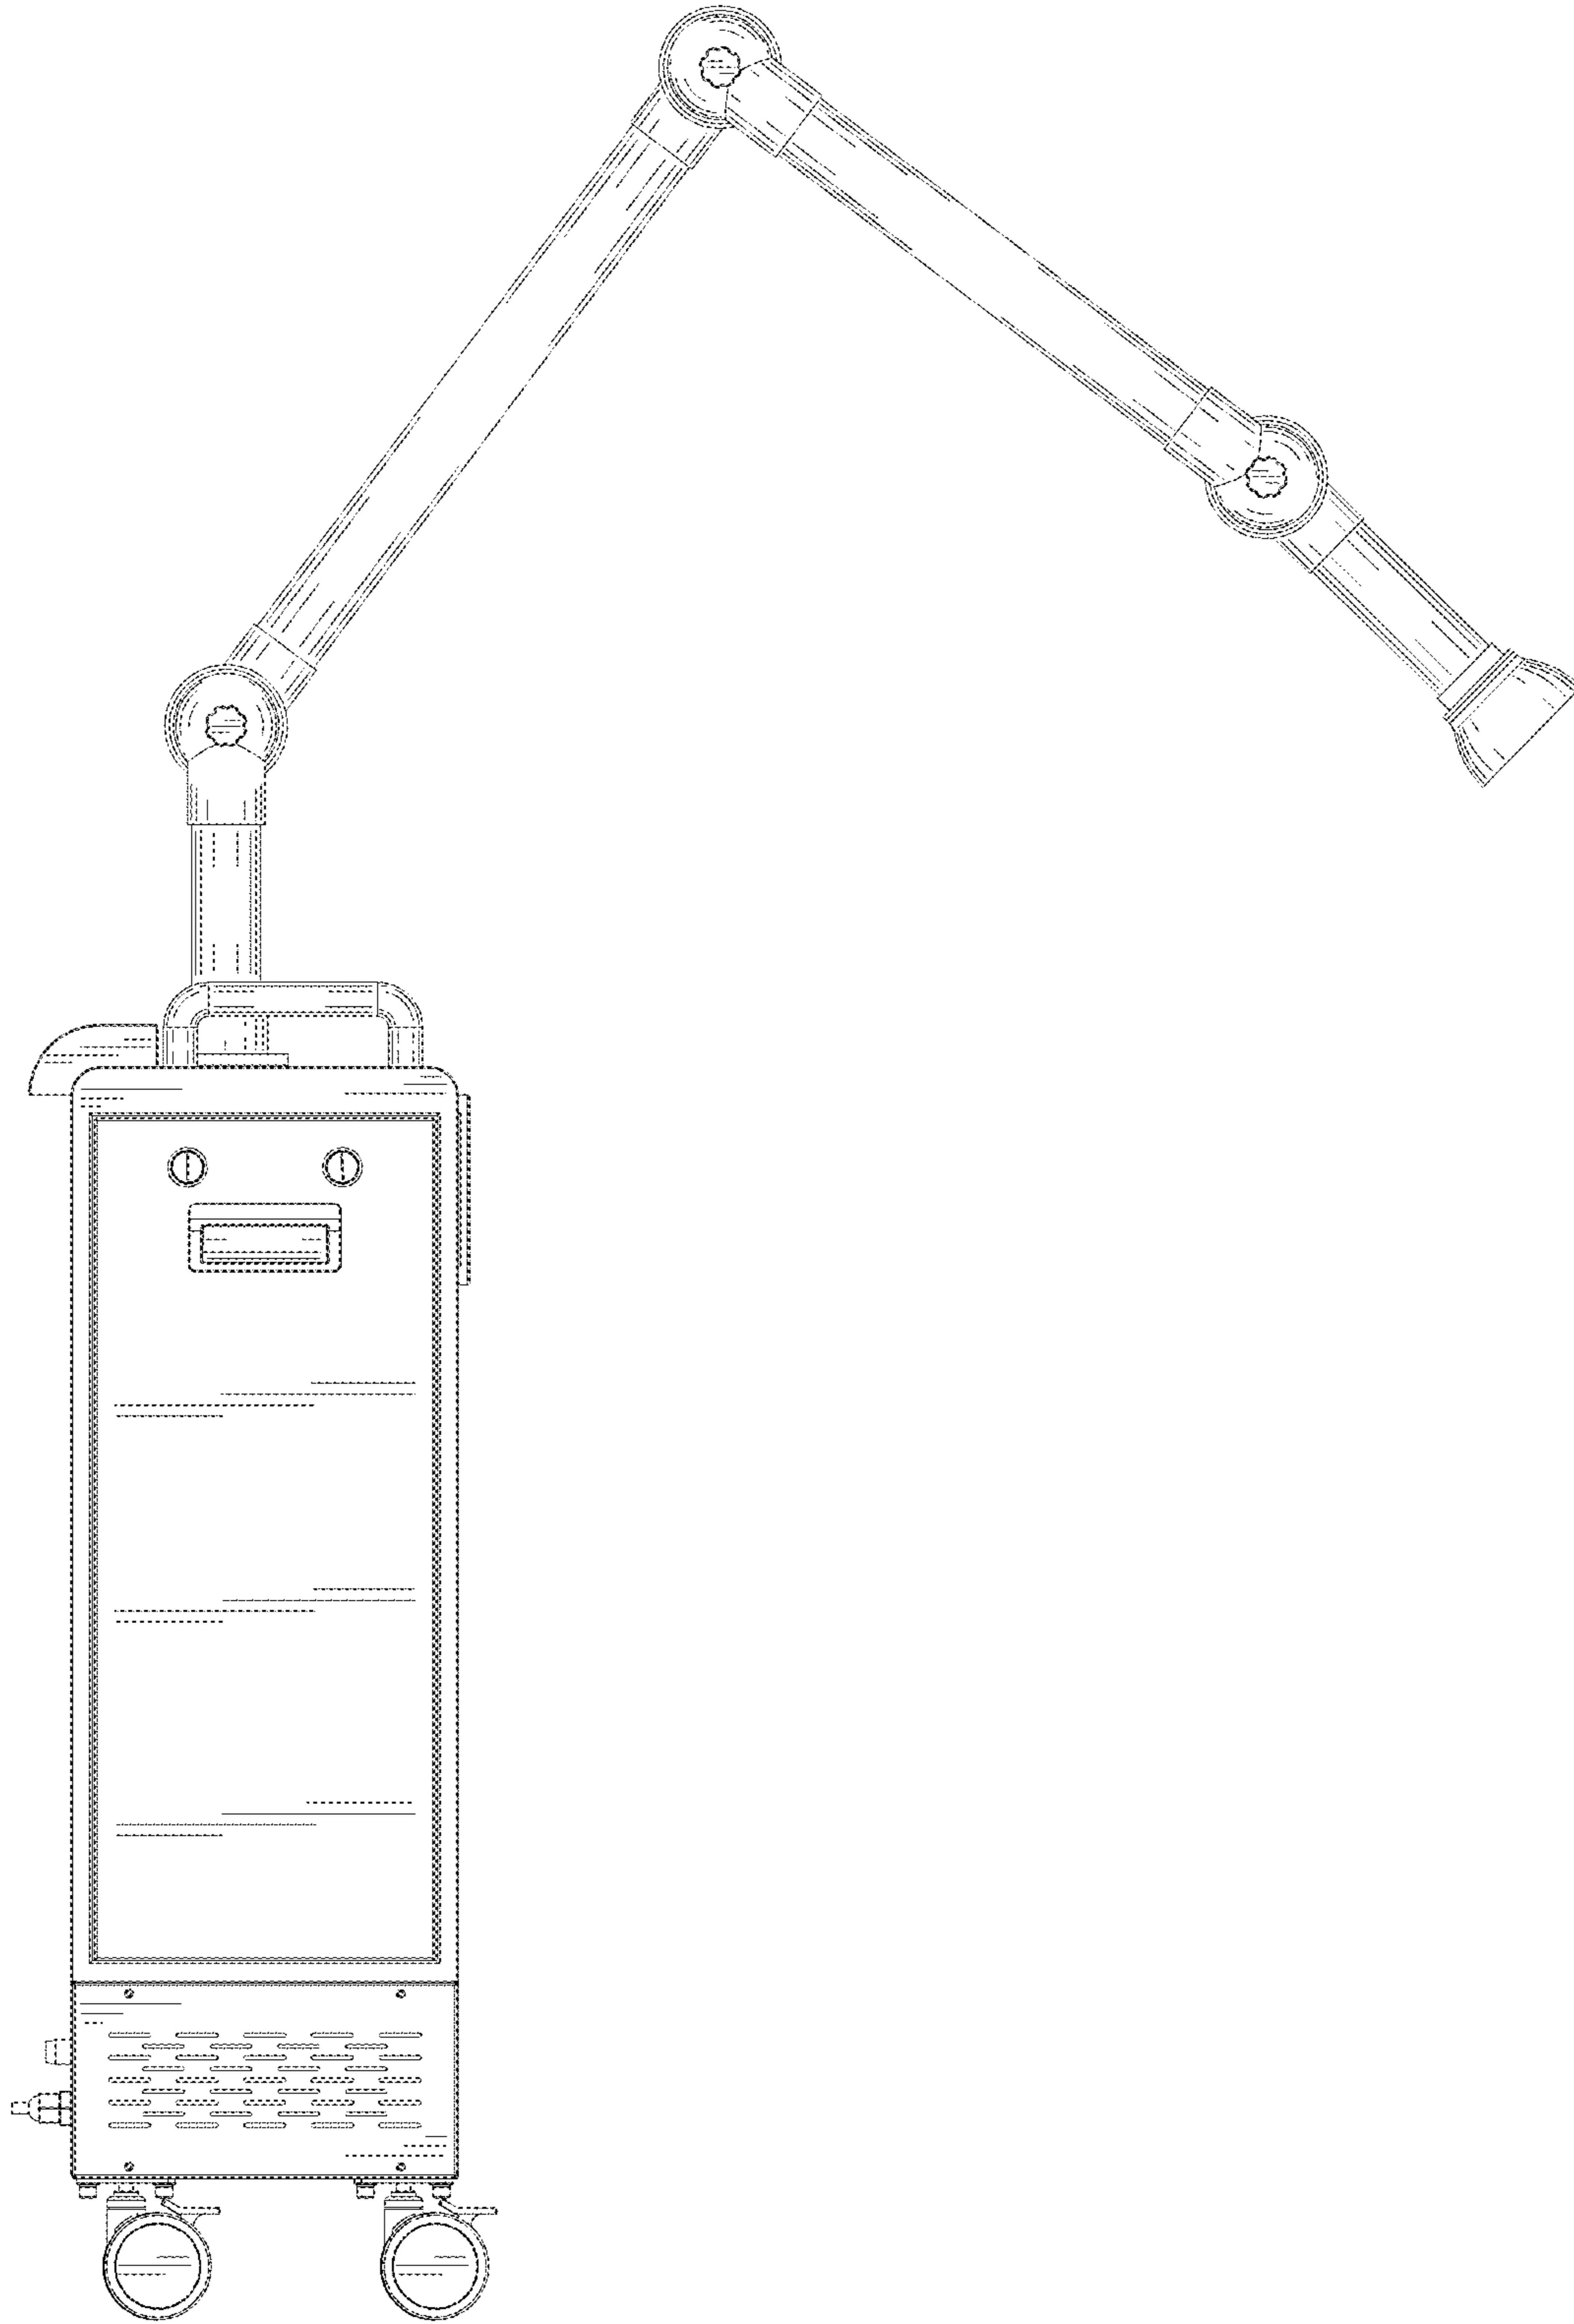


FIG. 2

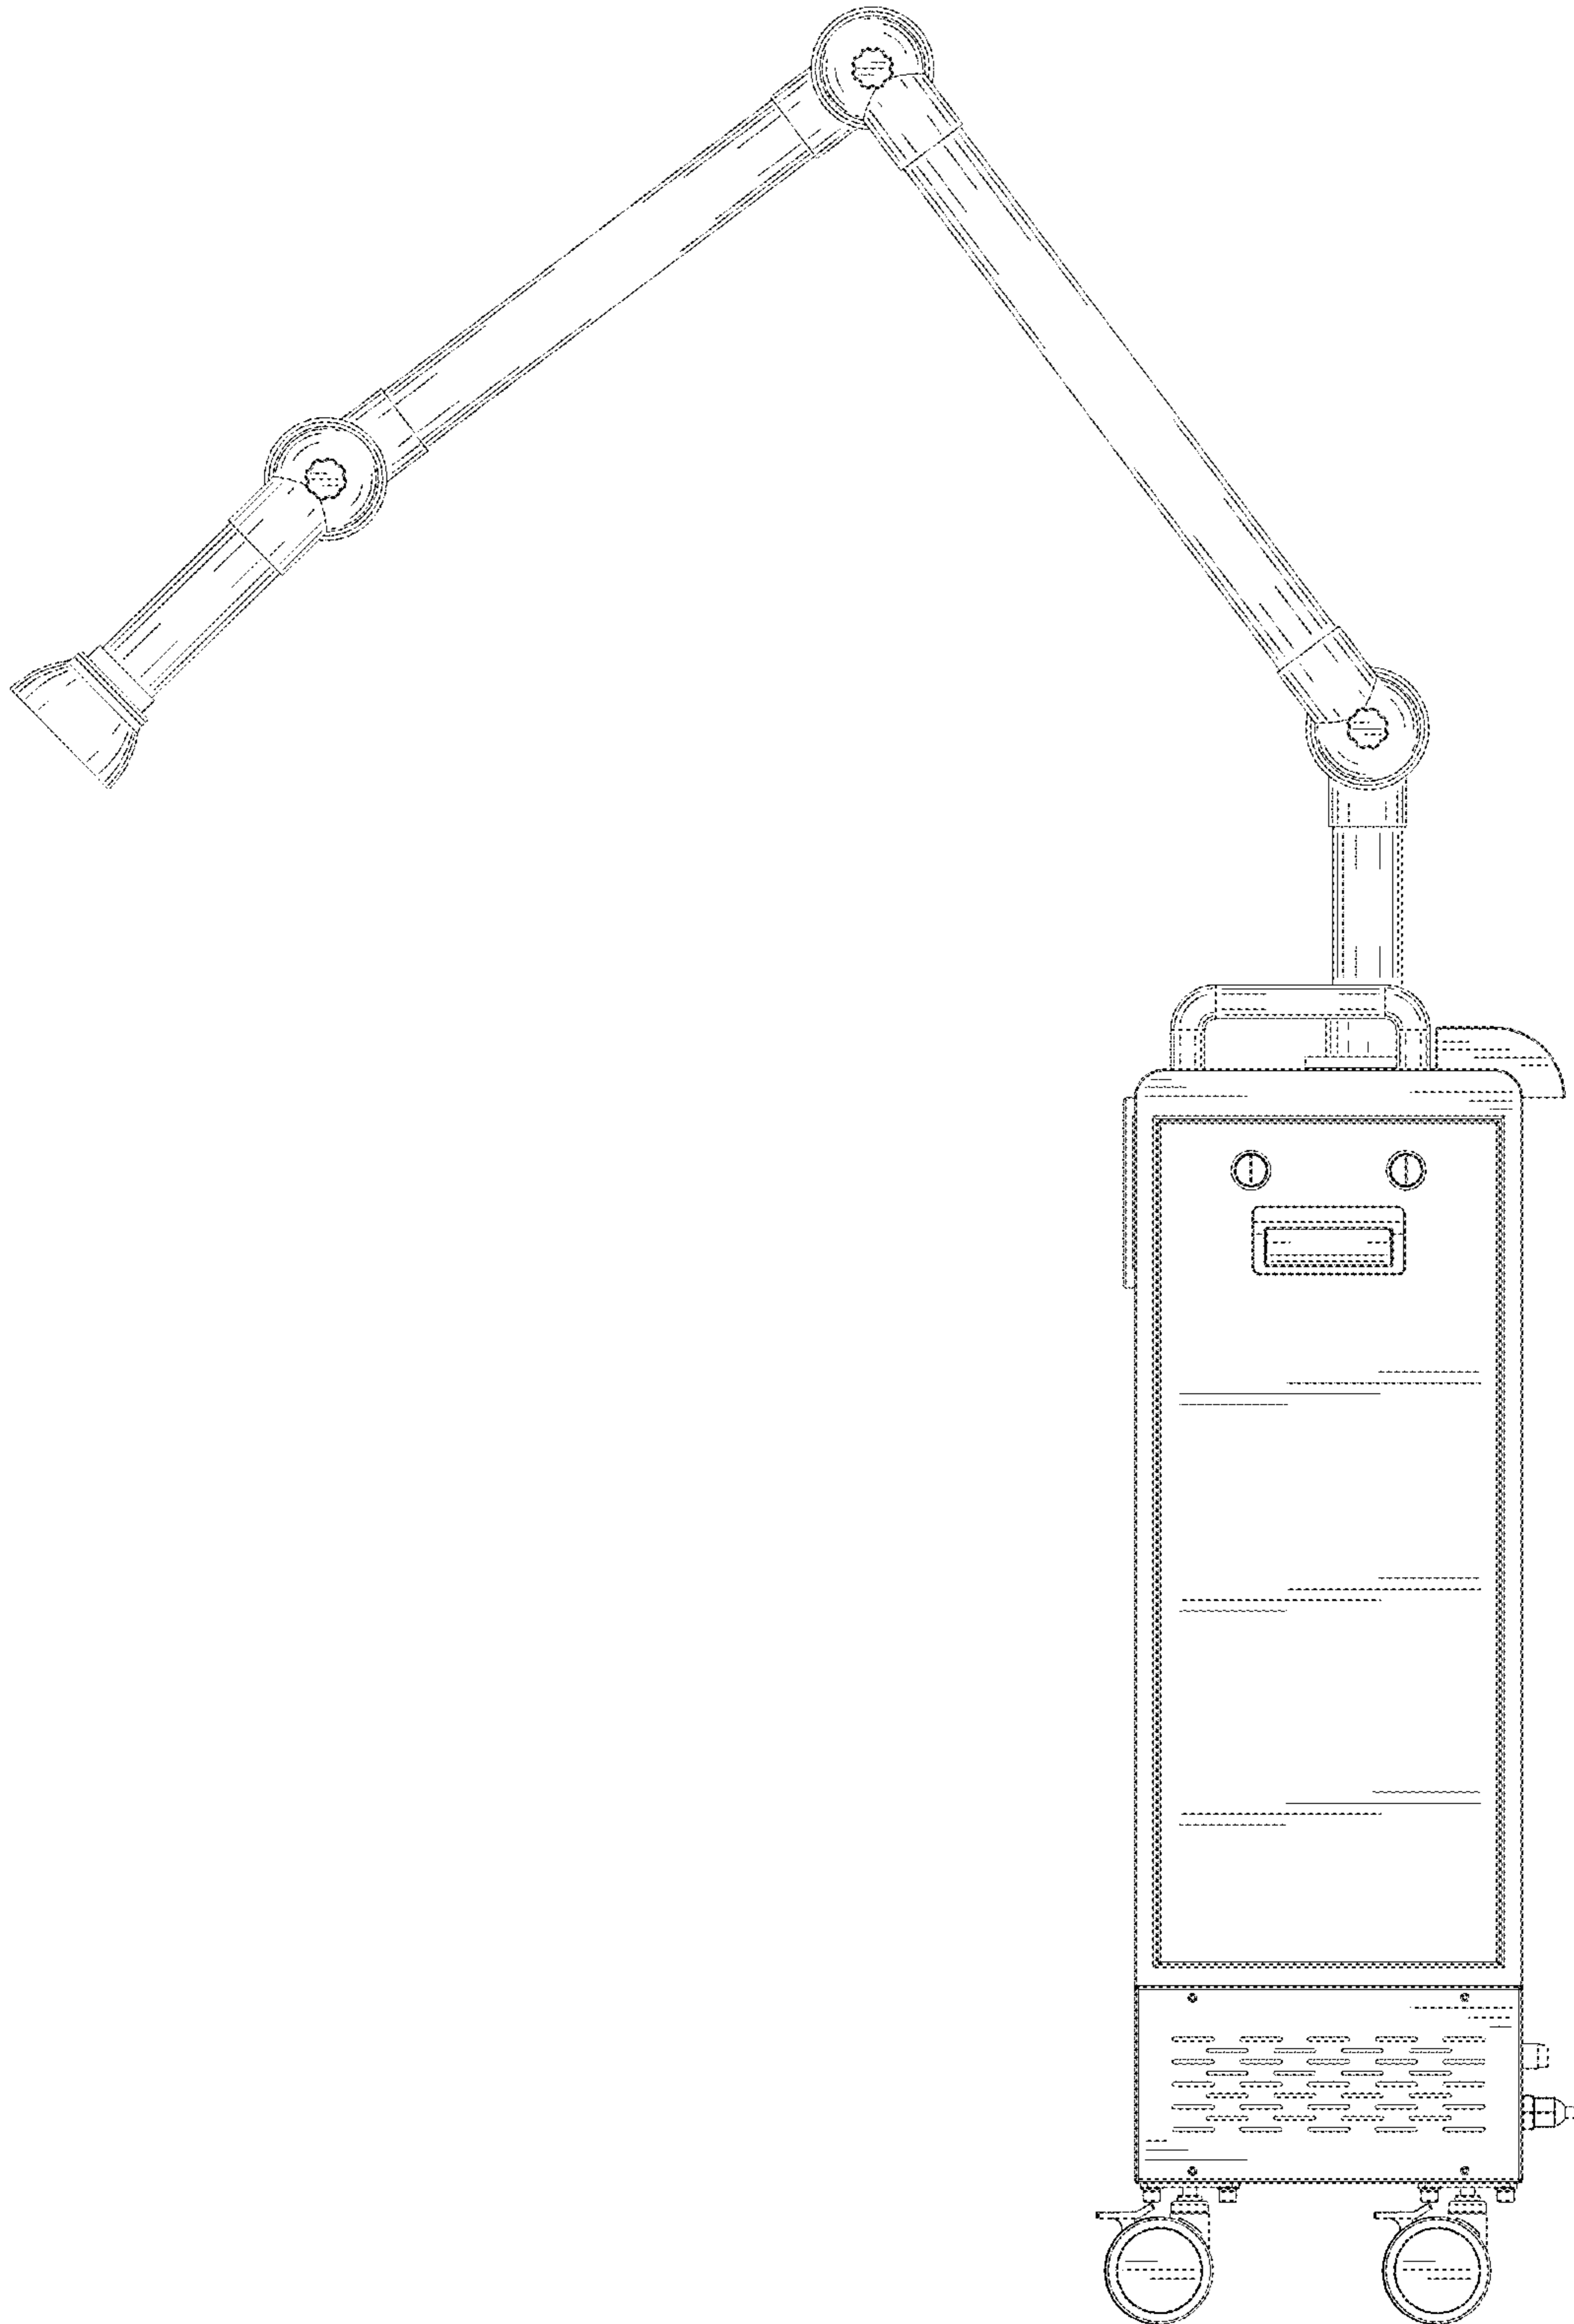


FIG. 3

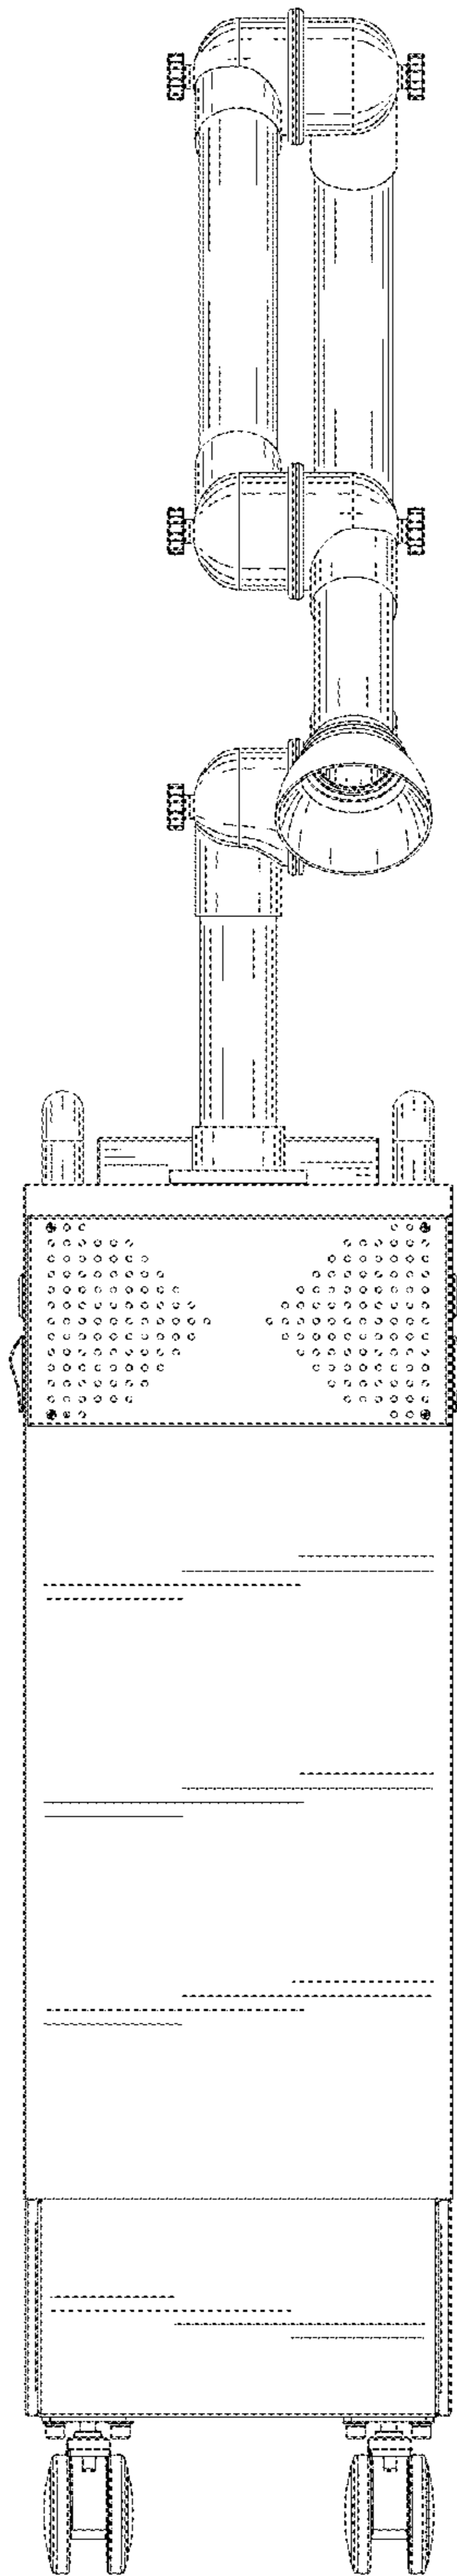


FIG. 4

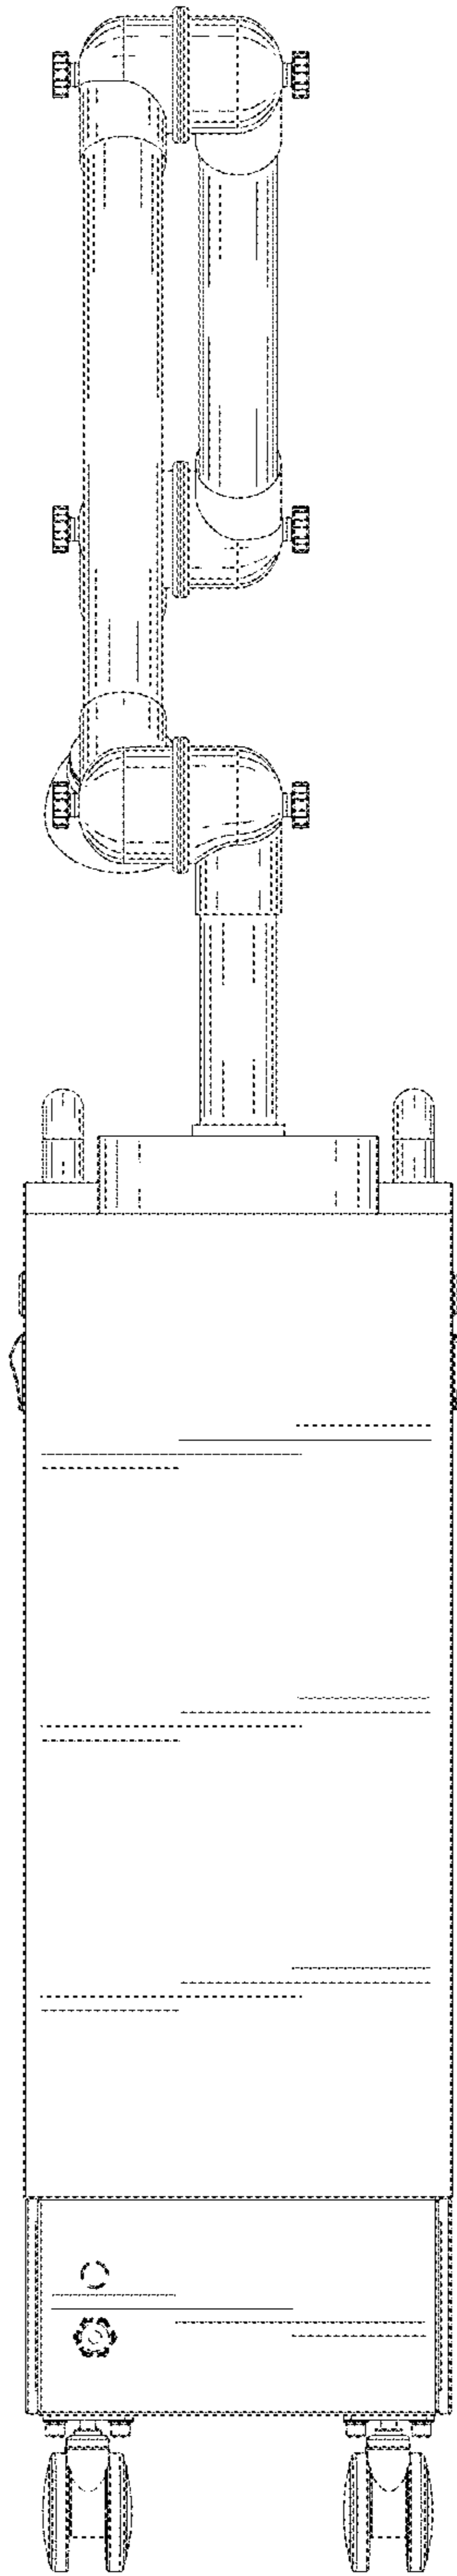


FIG. 5

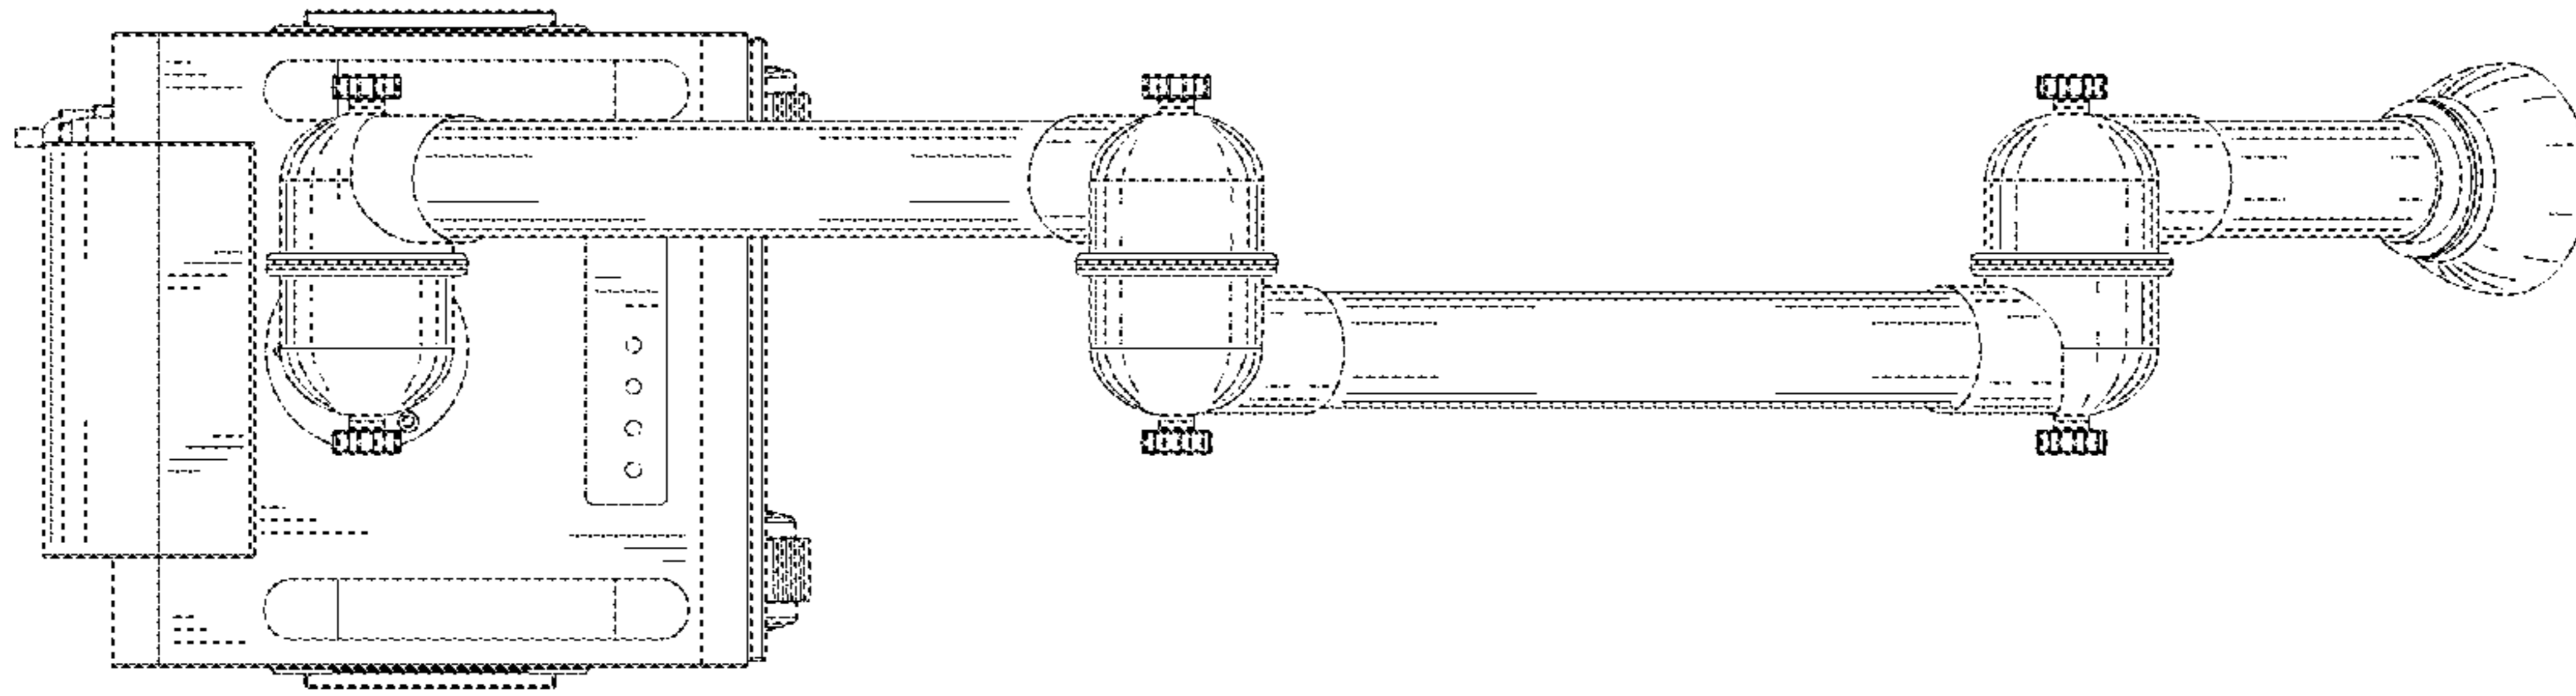


FIG. 6

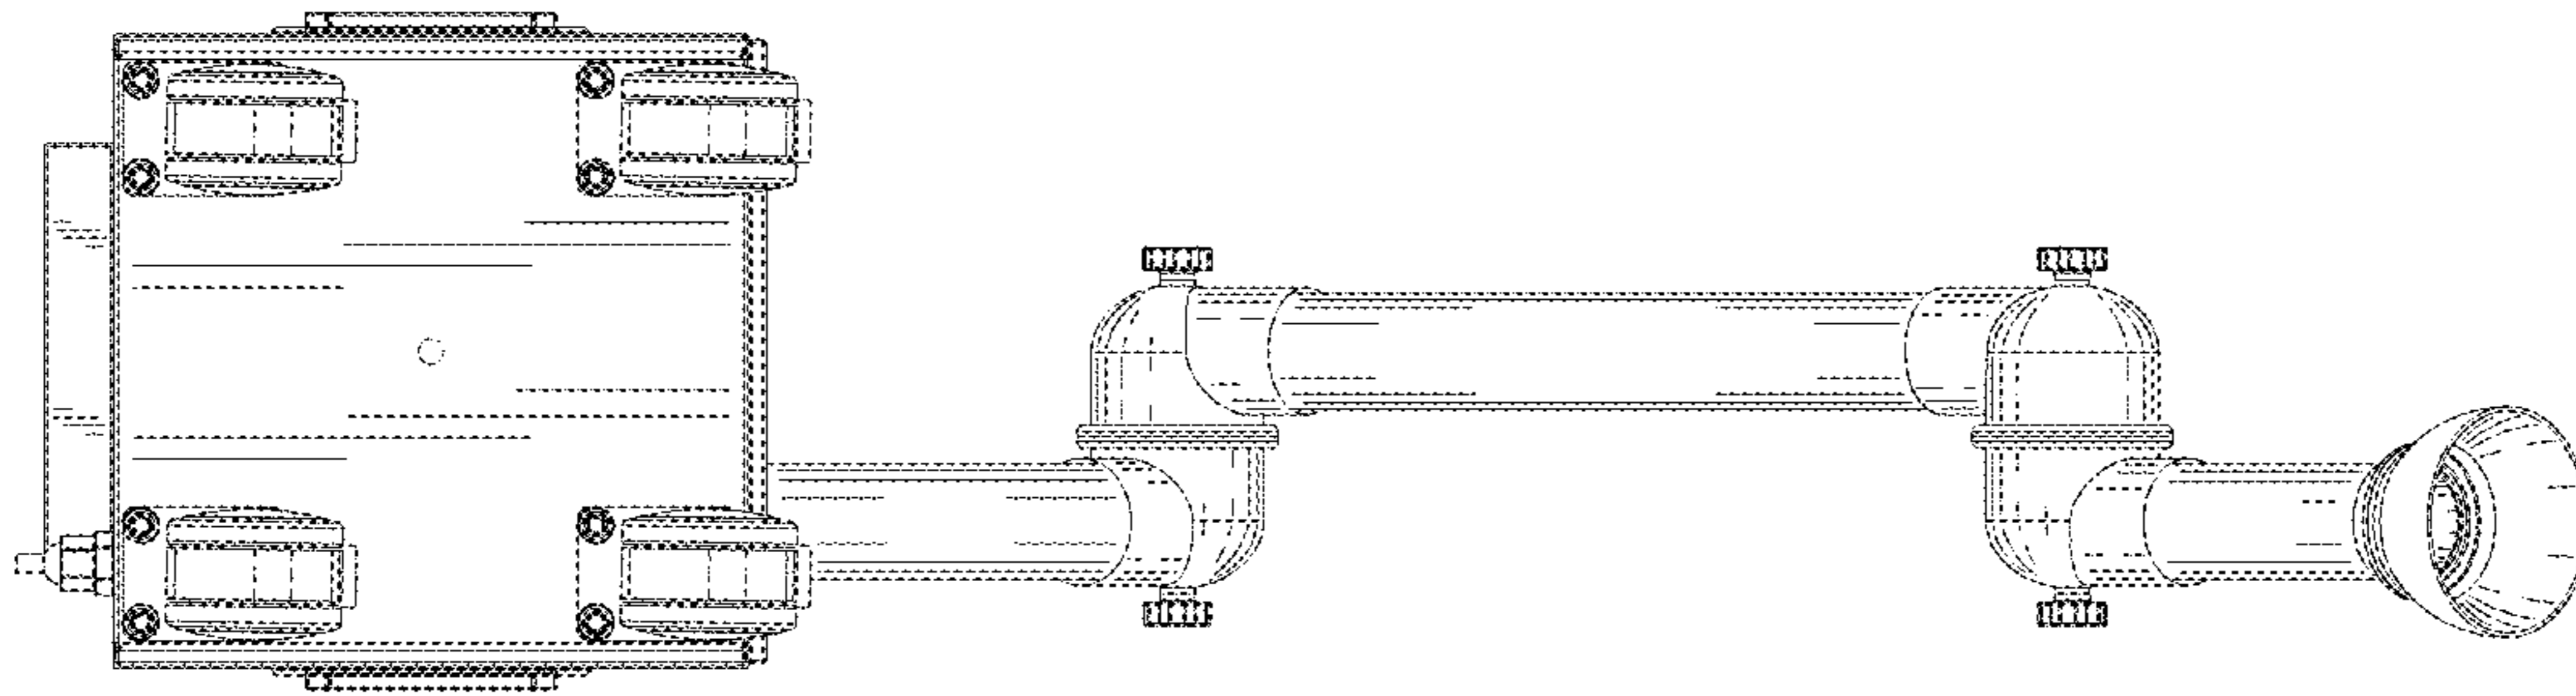


FIG. 7