



US00D928961S

(12) **United States Design Patent** (10) **Patent No.:** **US D928,961 S**
Zhang et al. (45) **Date of Patent:** **** Aug. 24, 2021**

(54) **IMAGING APPARATUS**

D874,005 S * 1/2020 Zhang D24/158
D895,804 S * 9/2020 Zhuang D24/158
D898,917 S * 10/2020 Stalter D24/158

(71) Applicant: **GE Precision Healthcare LLC**,
Milwaukee, WI (US)

(72) Inventors: **Wei Zhang**, Beijing (CN); **Jun Hou**,
Shanghai (CN)

(73) Assignee: **GE PRECISION HEALTHCARE**
LLC, Milwaukee, WI (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/698,209**

(22) Filed: **Jul. 15, 2019**

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/107, 158-160, 185-187
CPC A61B 5/055; G01N 2223/1016; G01N
2223/301; G01N 2223/031; G01N
2223/419; G01N 23/046; G01R 33/48
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D417,734 S * 12/1999 Benders D24/158
D503,804 S * 4/2005 Phleps D24/158
D580,471 S * 11/2008 Tena Comadran D16/200
D715,444 S * 10/2014 Zhi D24/159
D725,275 S * 3/2015 Matsumura D24/158
D751,205 S * 3/2016 Tan D24/158
D753,828 S * 4/2016 Baba D24/158
D849,949 S * 5/2019 Stalter D24/158

OTHER PUBLICATIONS

Revolution™ Maxima | GE Healthcare | GE Healthcare. Retrieved
from GE health care's website on 0/12/2021. No available posting
date.*

Zhang, W. et al., "An Ornamental Design for a Ceiling-Mount
Camera," U.S. Appl. No. 29/698,210, filed Jul. 15, 2019, 19 pages.
Zhang, W. et al., "An Ornamental Design for an Imaging Appara-
tus," U.S. Appl. No. 29/698,208, filed Jul. 15, 2019, 19 pages.

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — McCoy Russell LLP

(57) **CLAIM**

The ornamental design for an imaging apparatus, as shown
and described.

DESCRIPTION

FIG. 1 is a front-left perspective view of an imaging
apparatus according to the claimed design.

FIG. 2 is a front view of the imaging apparatus.

FIG. 3 is a rear view of the imaging apparatus.

FIG. 4 is a top view of the imaging apparatus.


FIG. 5 is a bottom view of the imaging apparatus.

FIG. 6 is a left side view of the imaging apparatus; and,

FIG. 7 is a right side view of the imaging apparatus.

The broken lines in the drawings illustrate portions of the
imaging apparatus that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

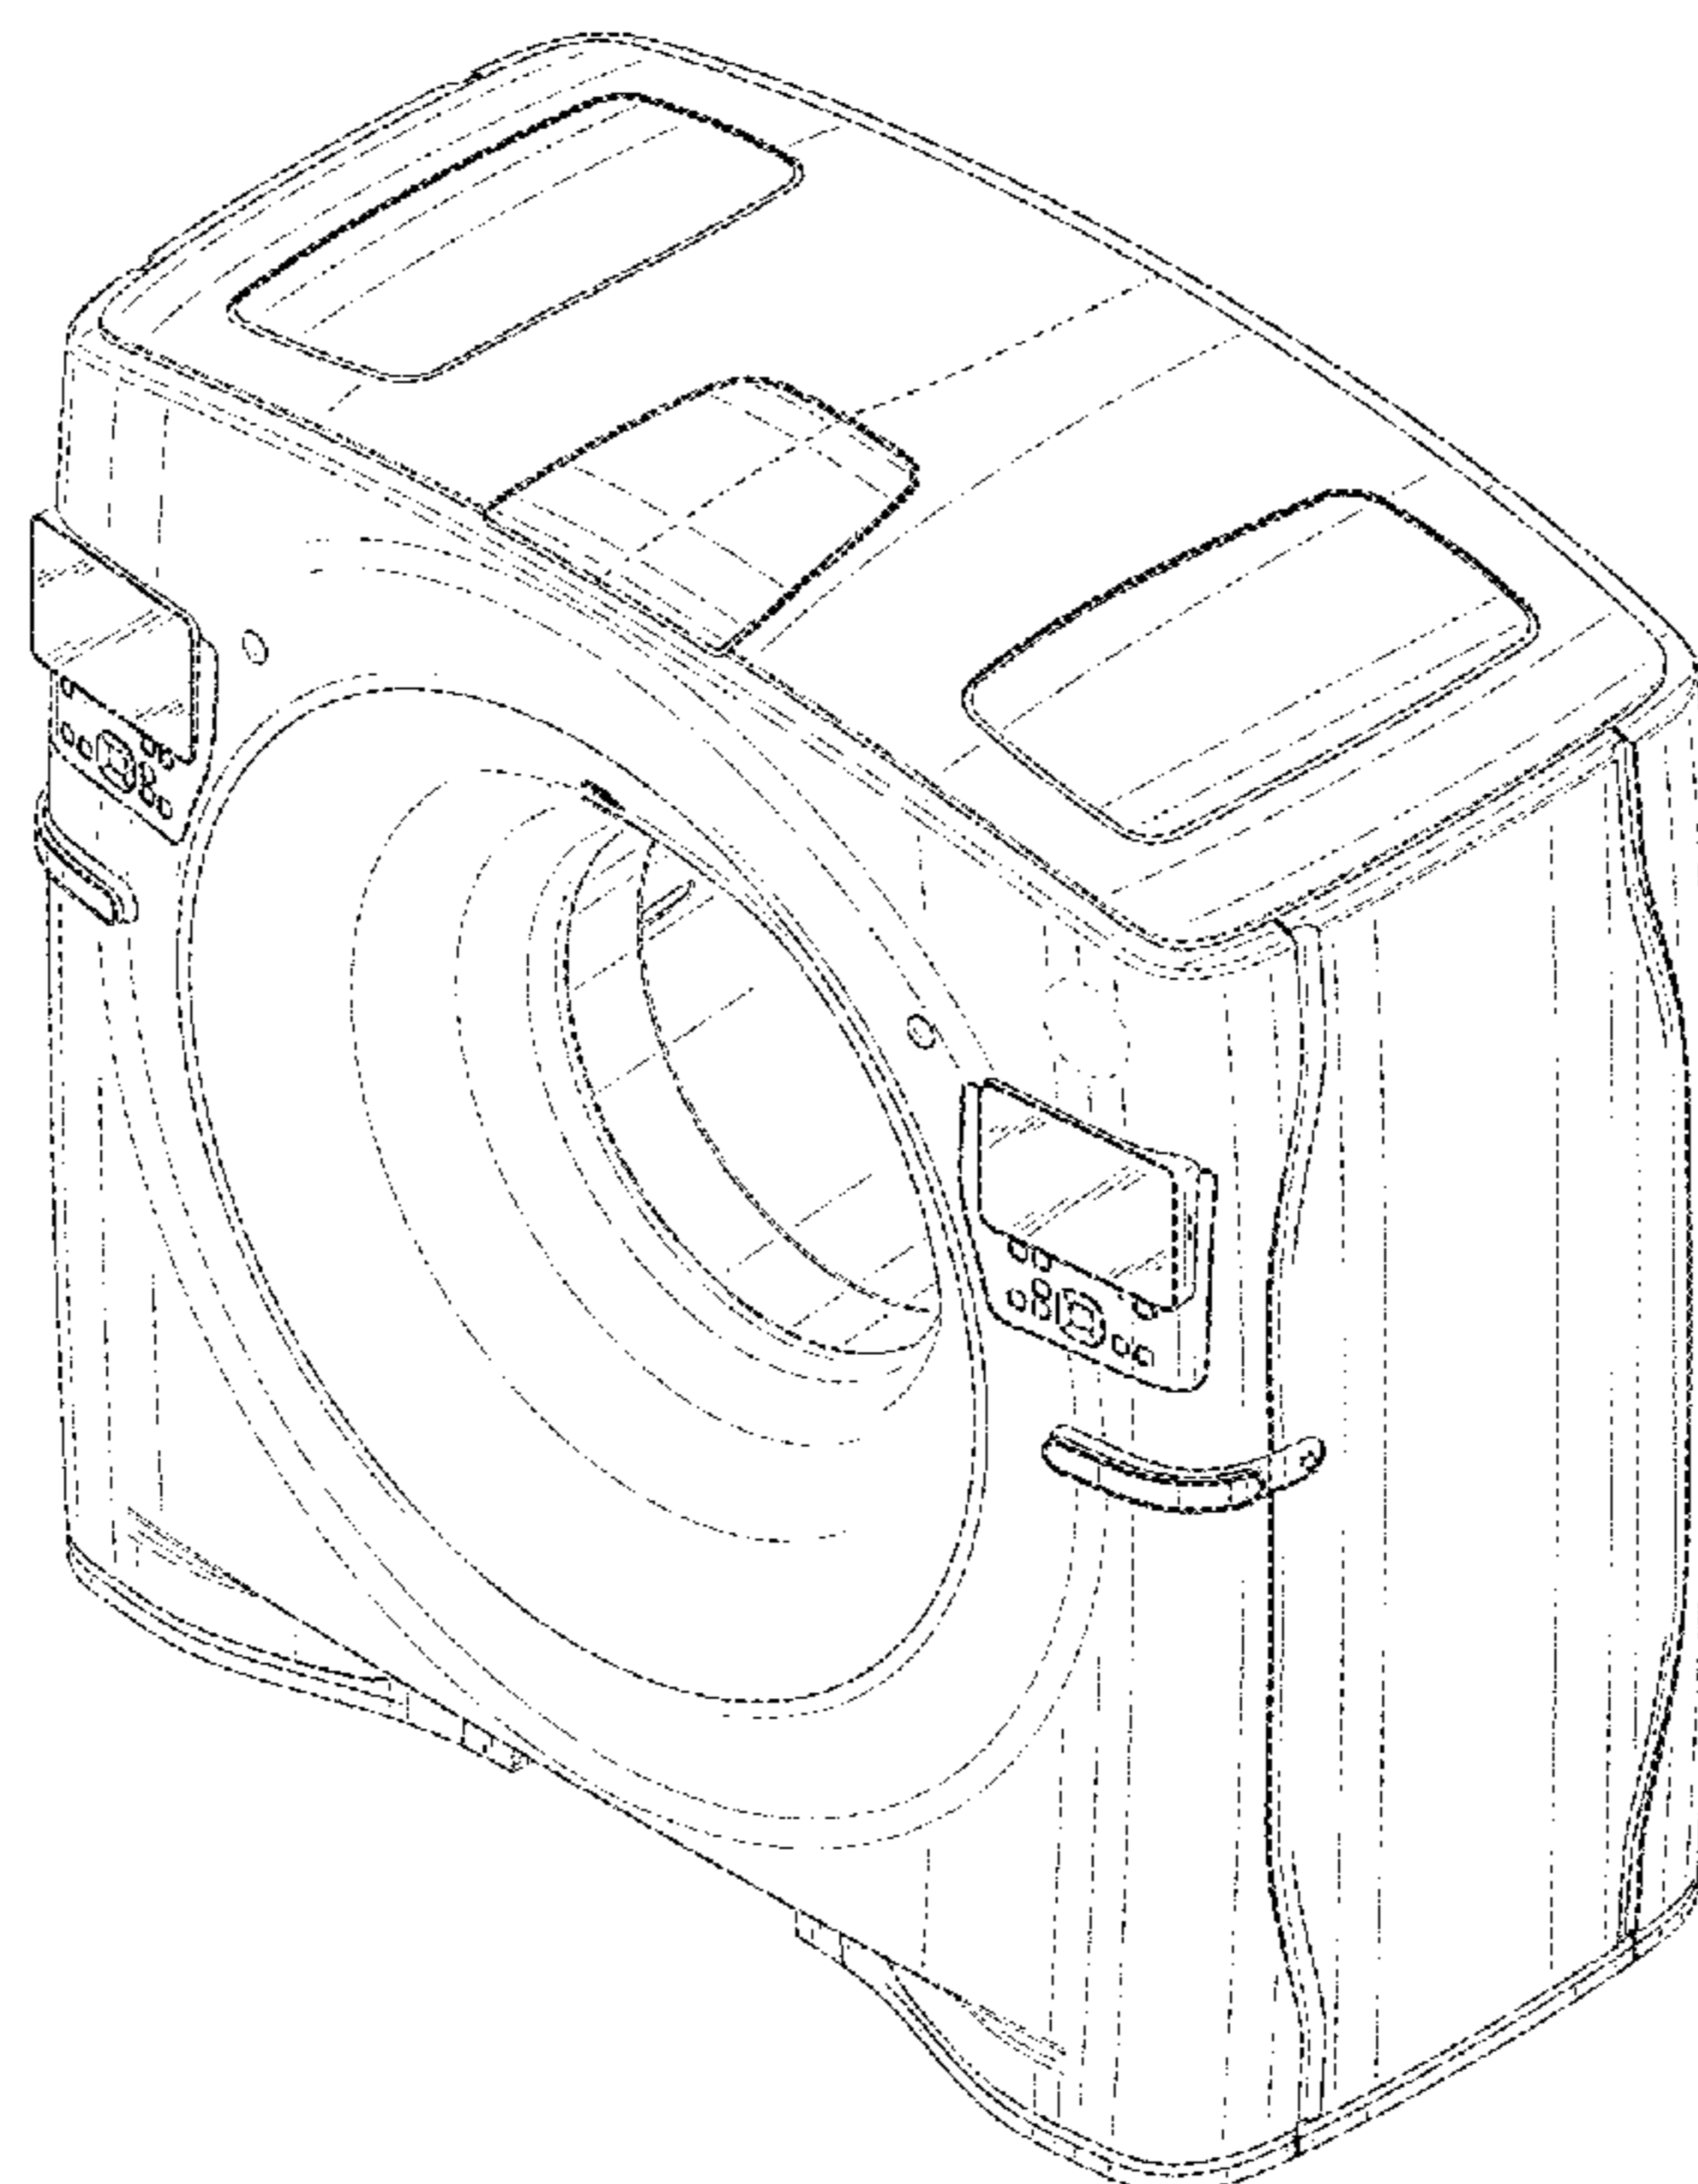

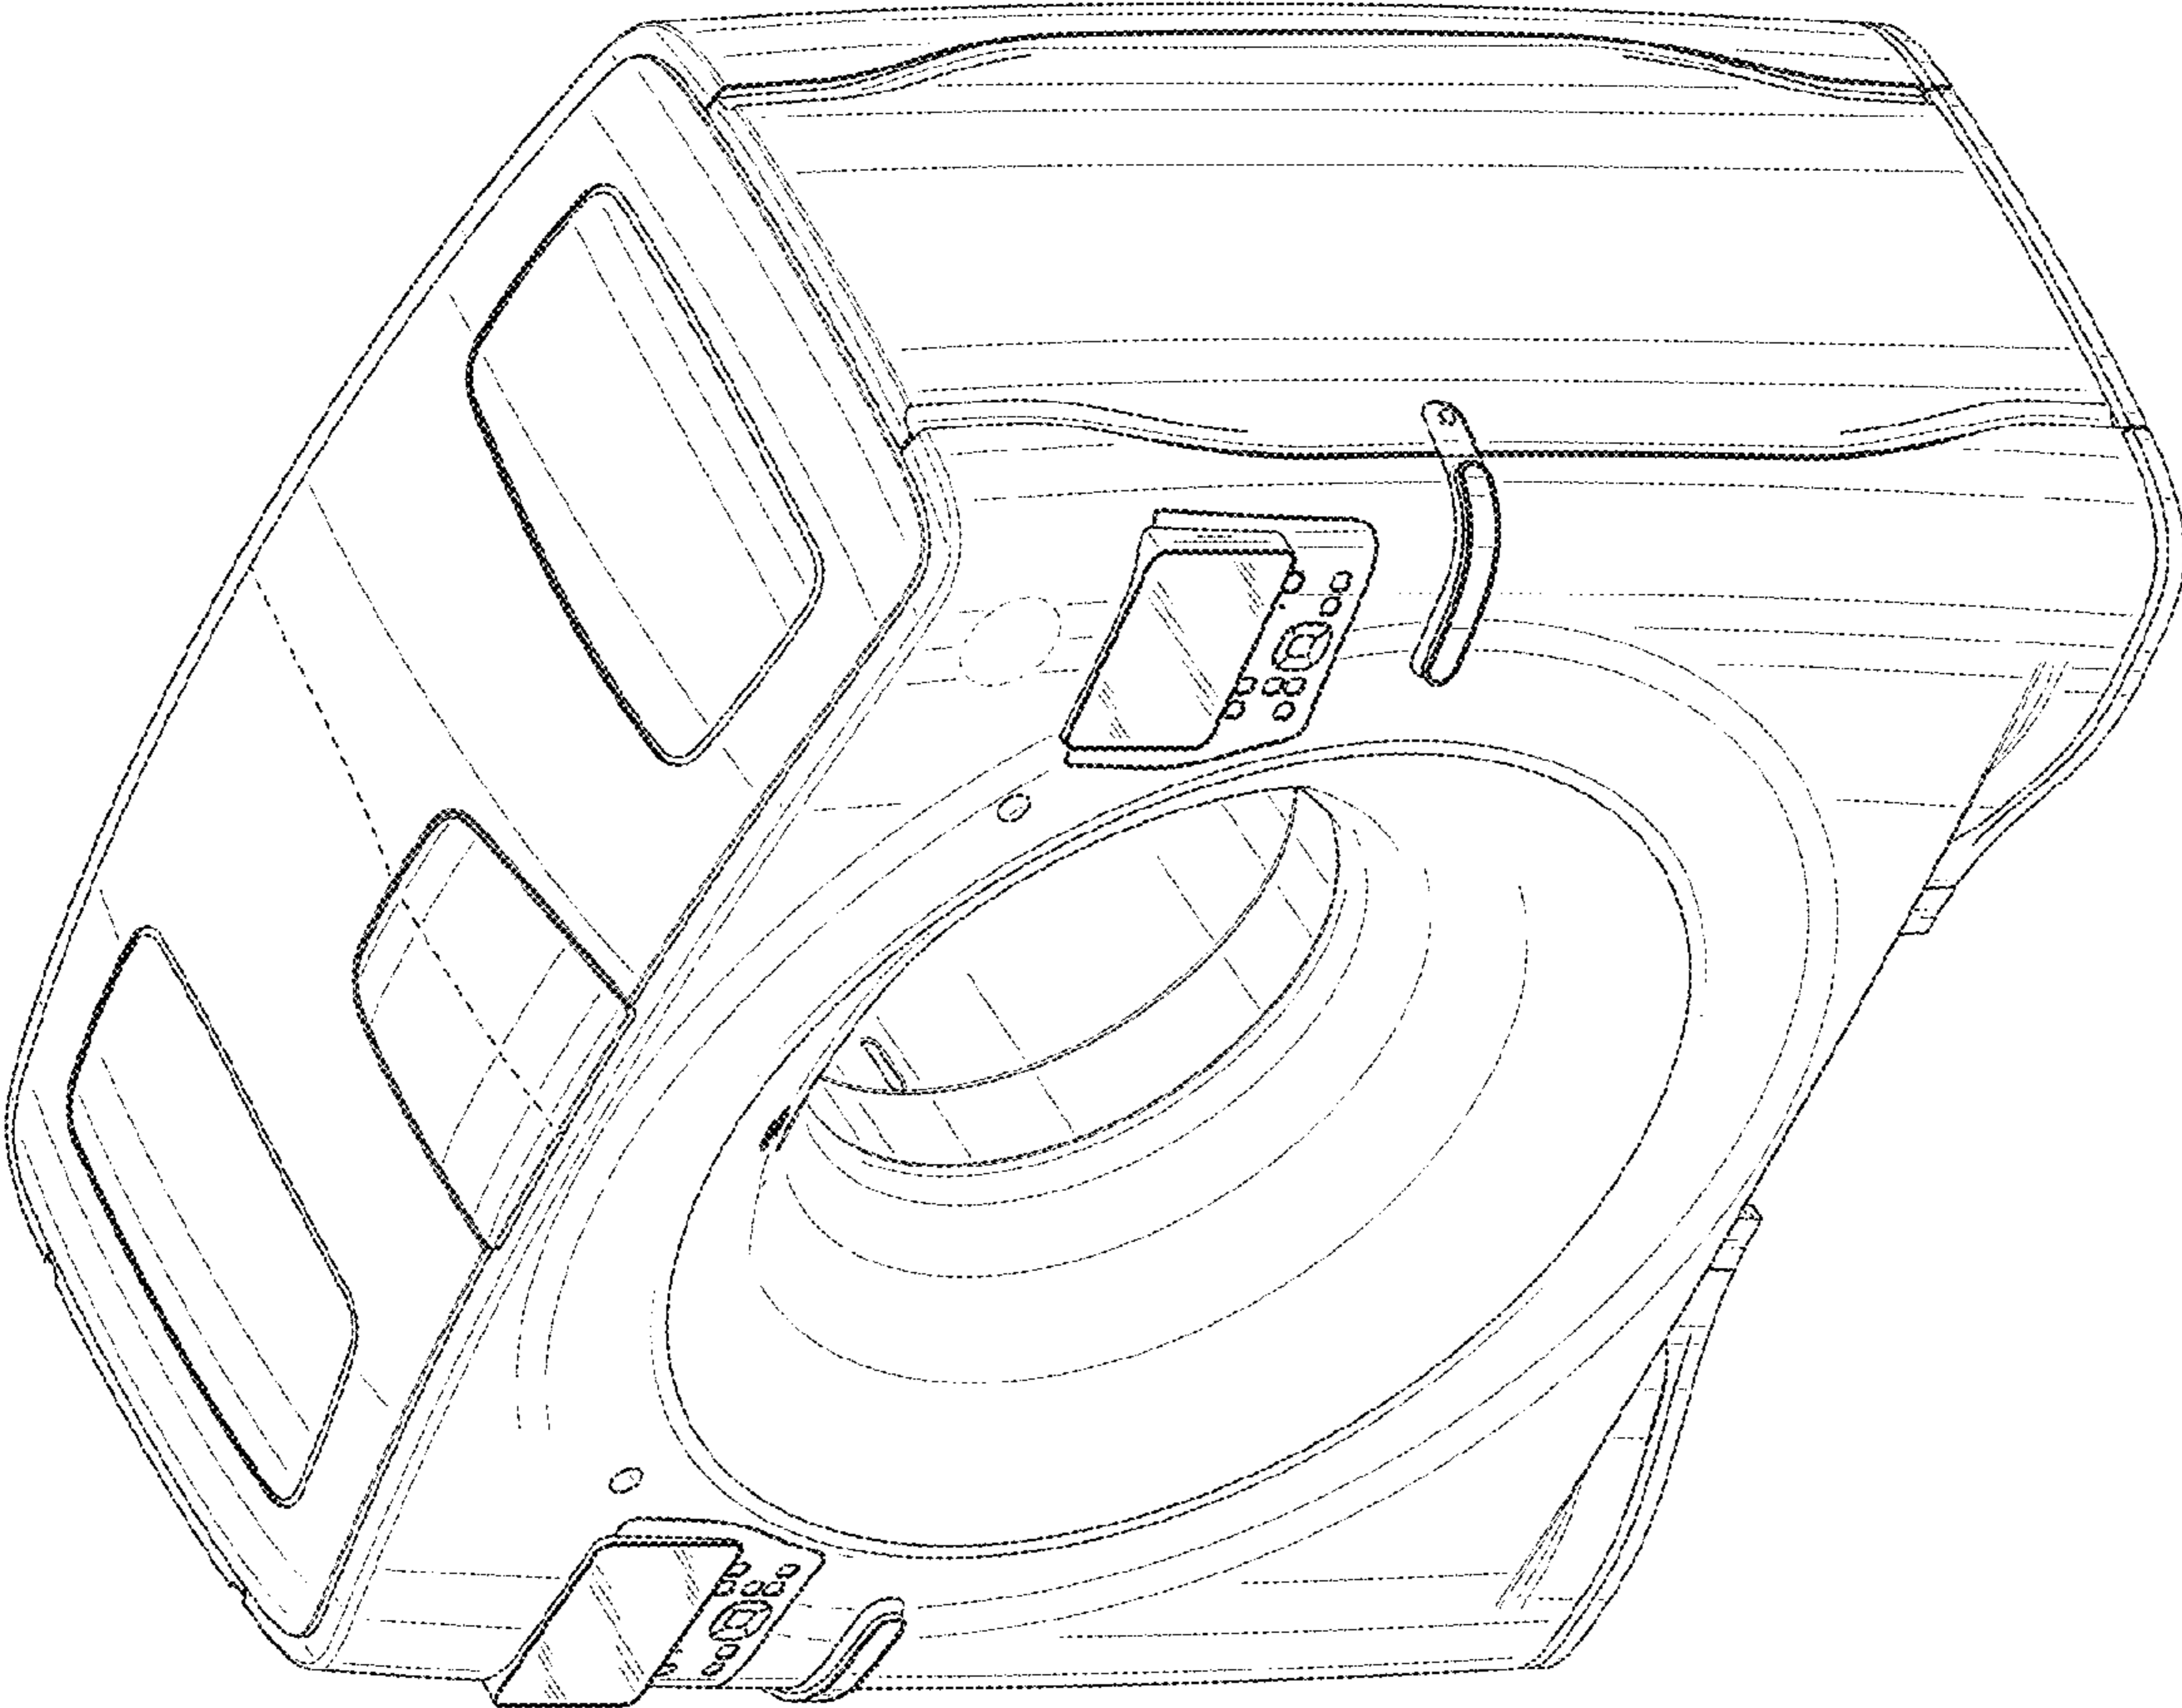


FIG. 1

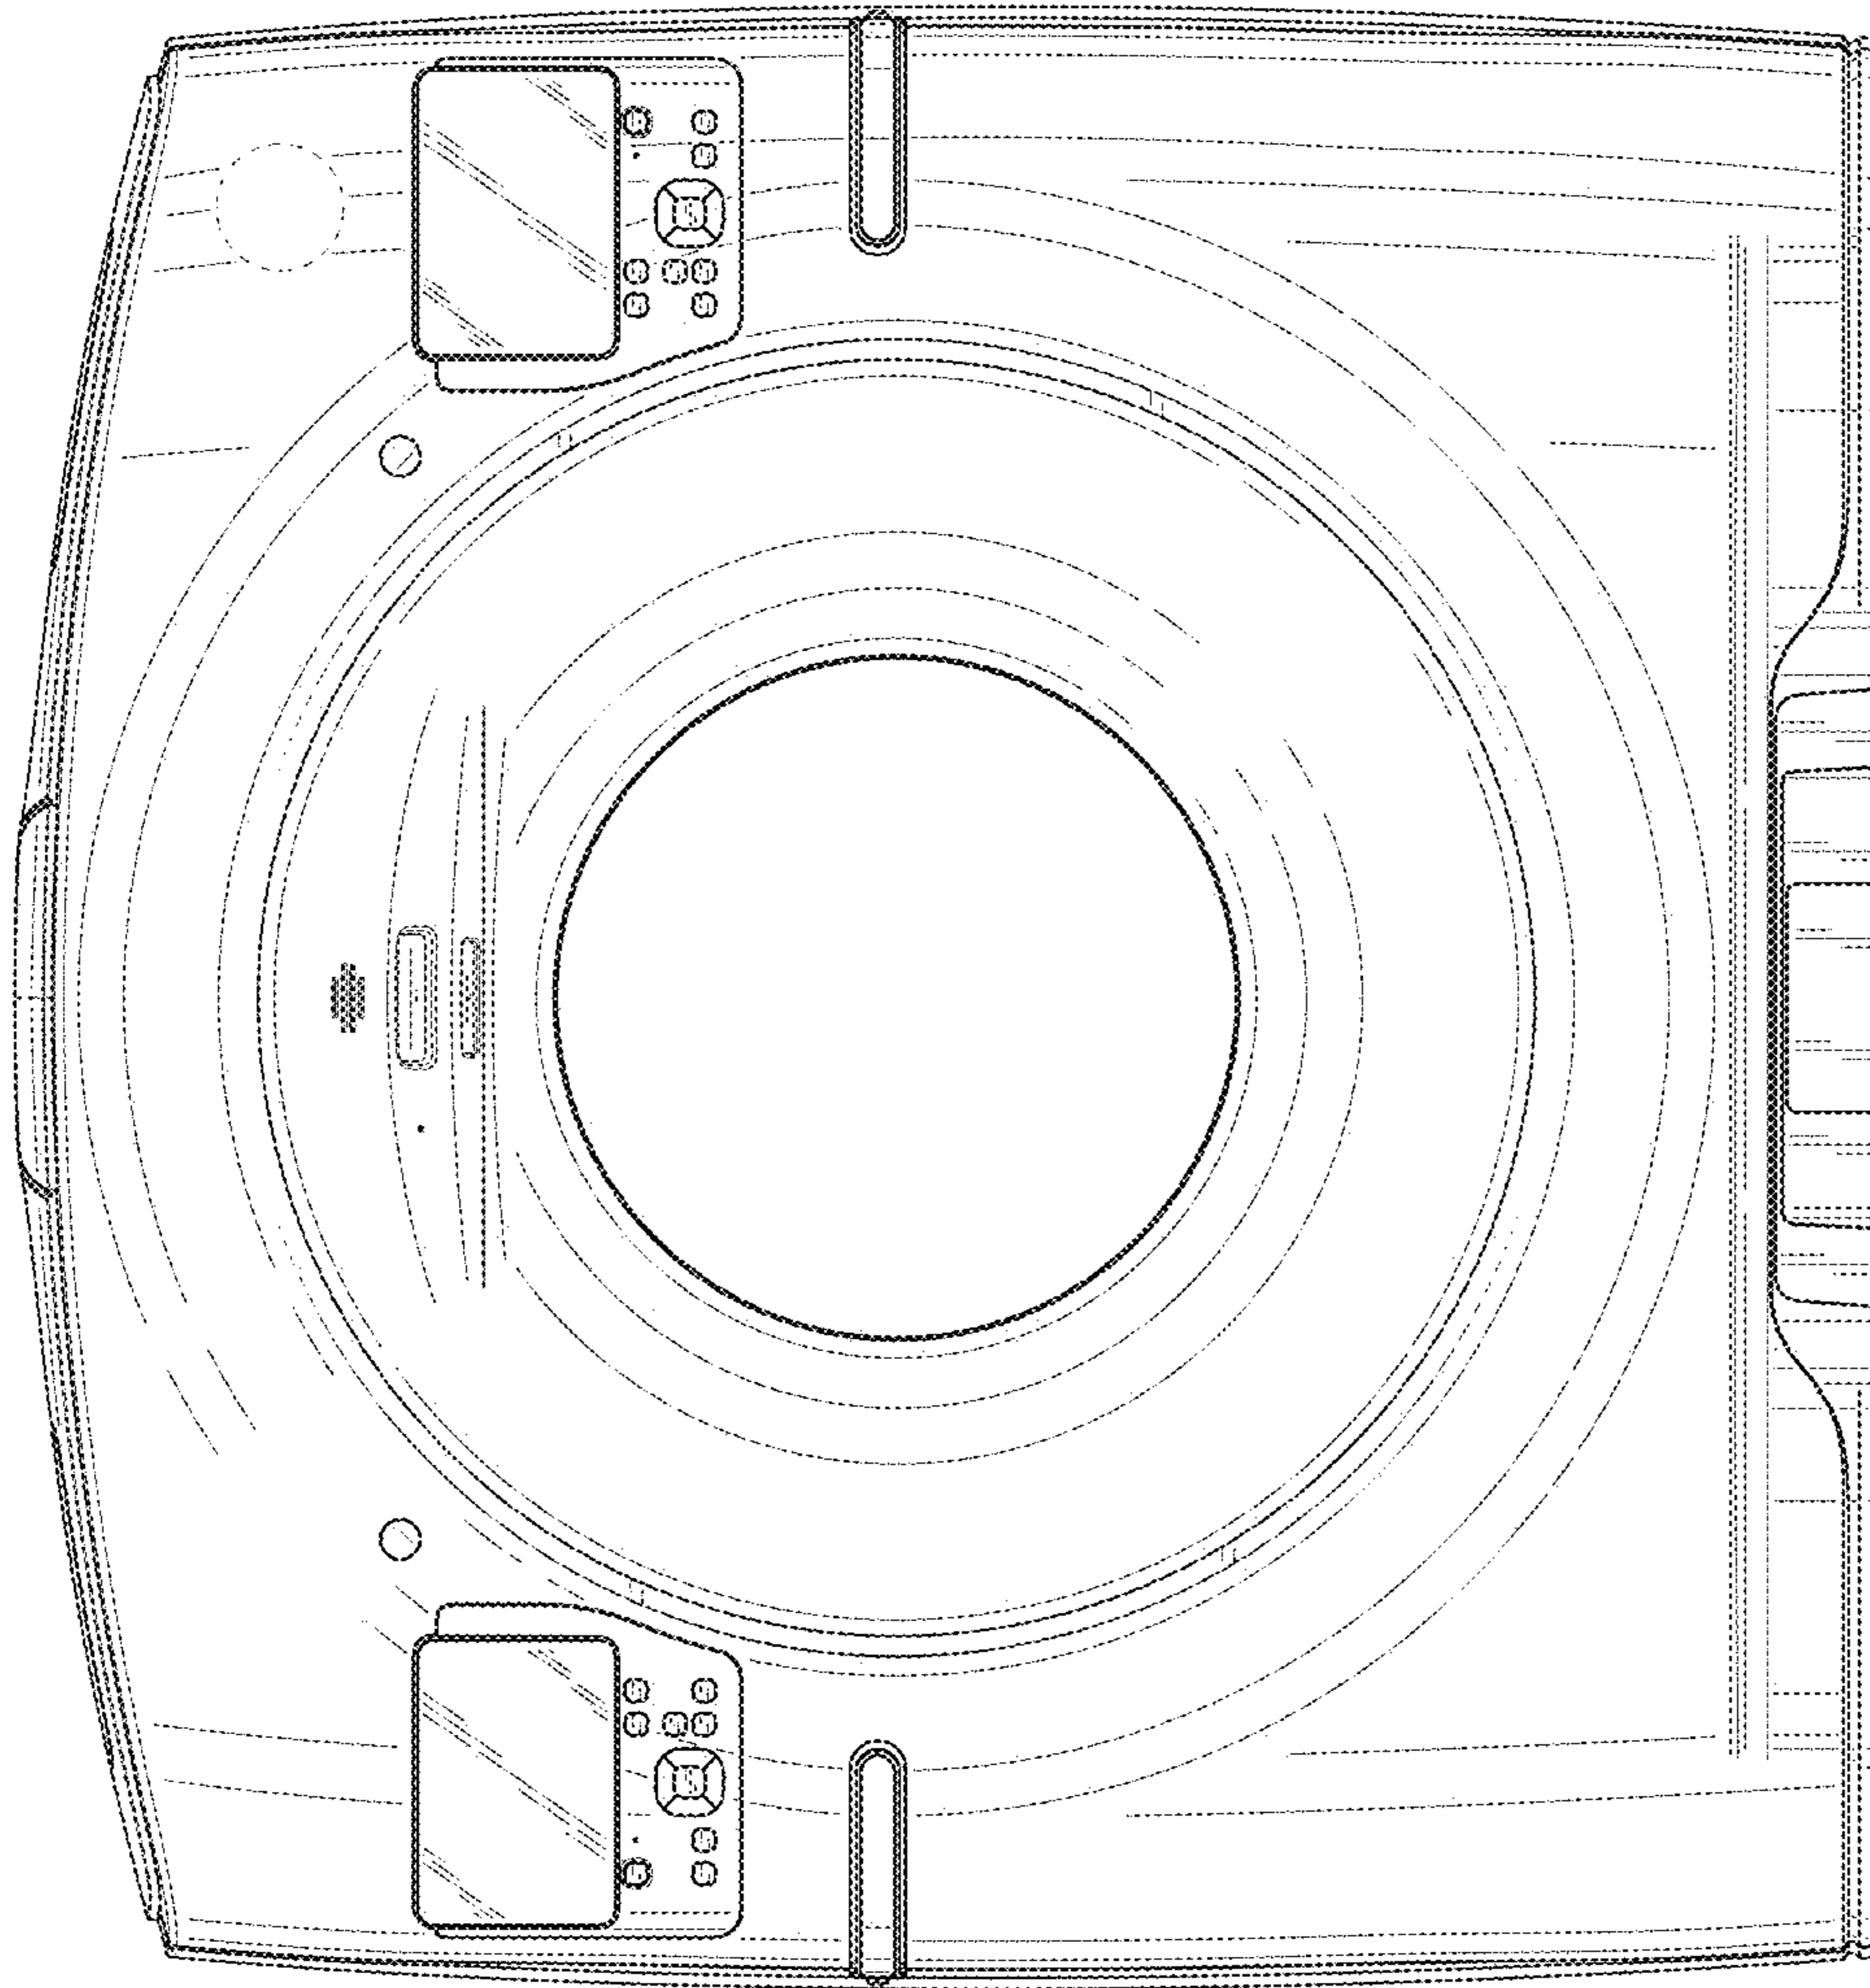


FIG. 2

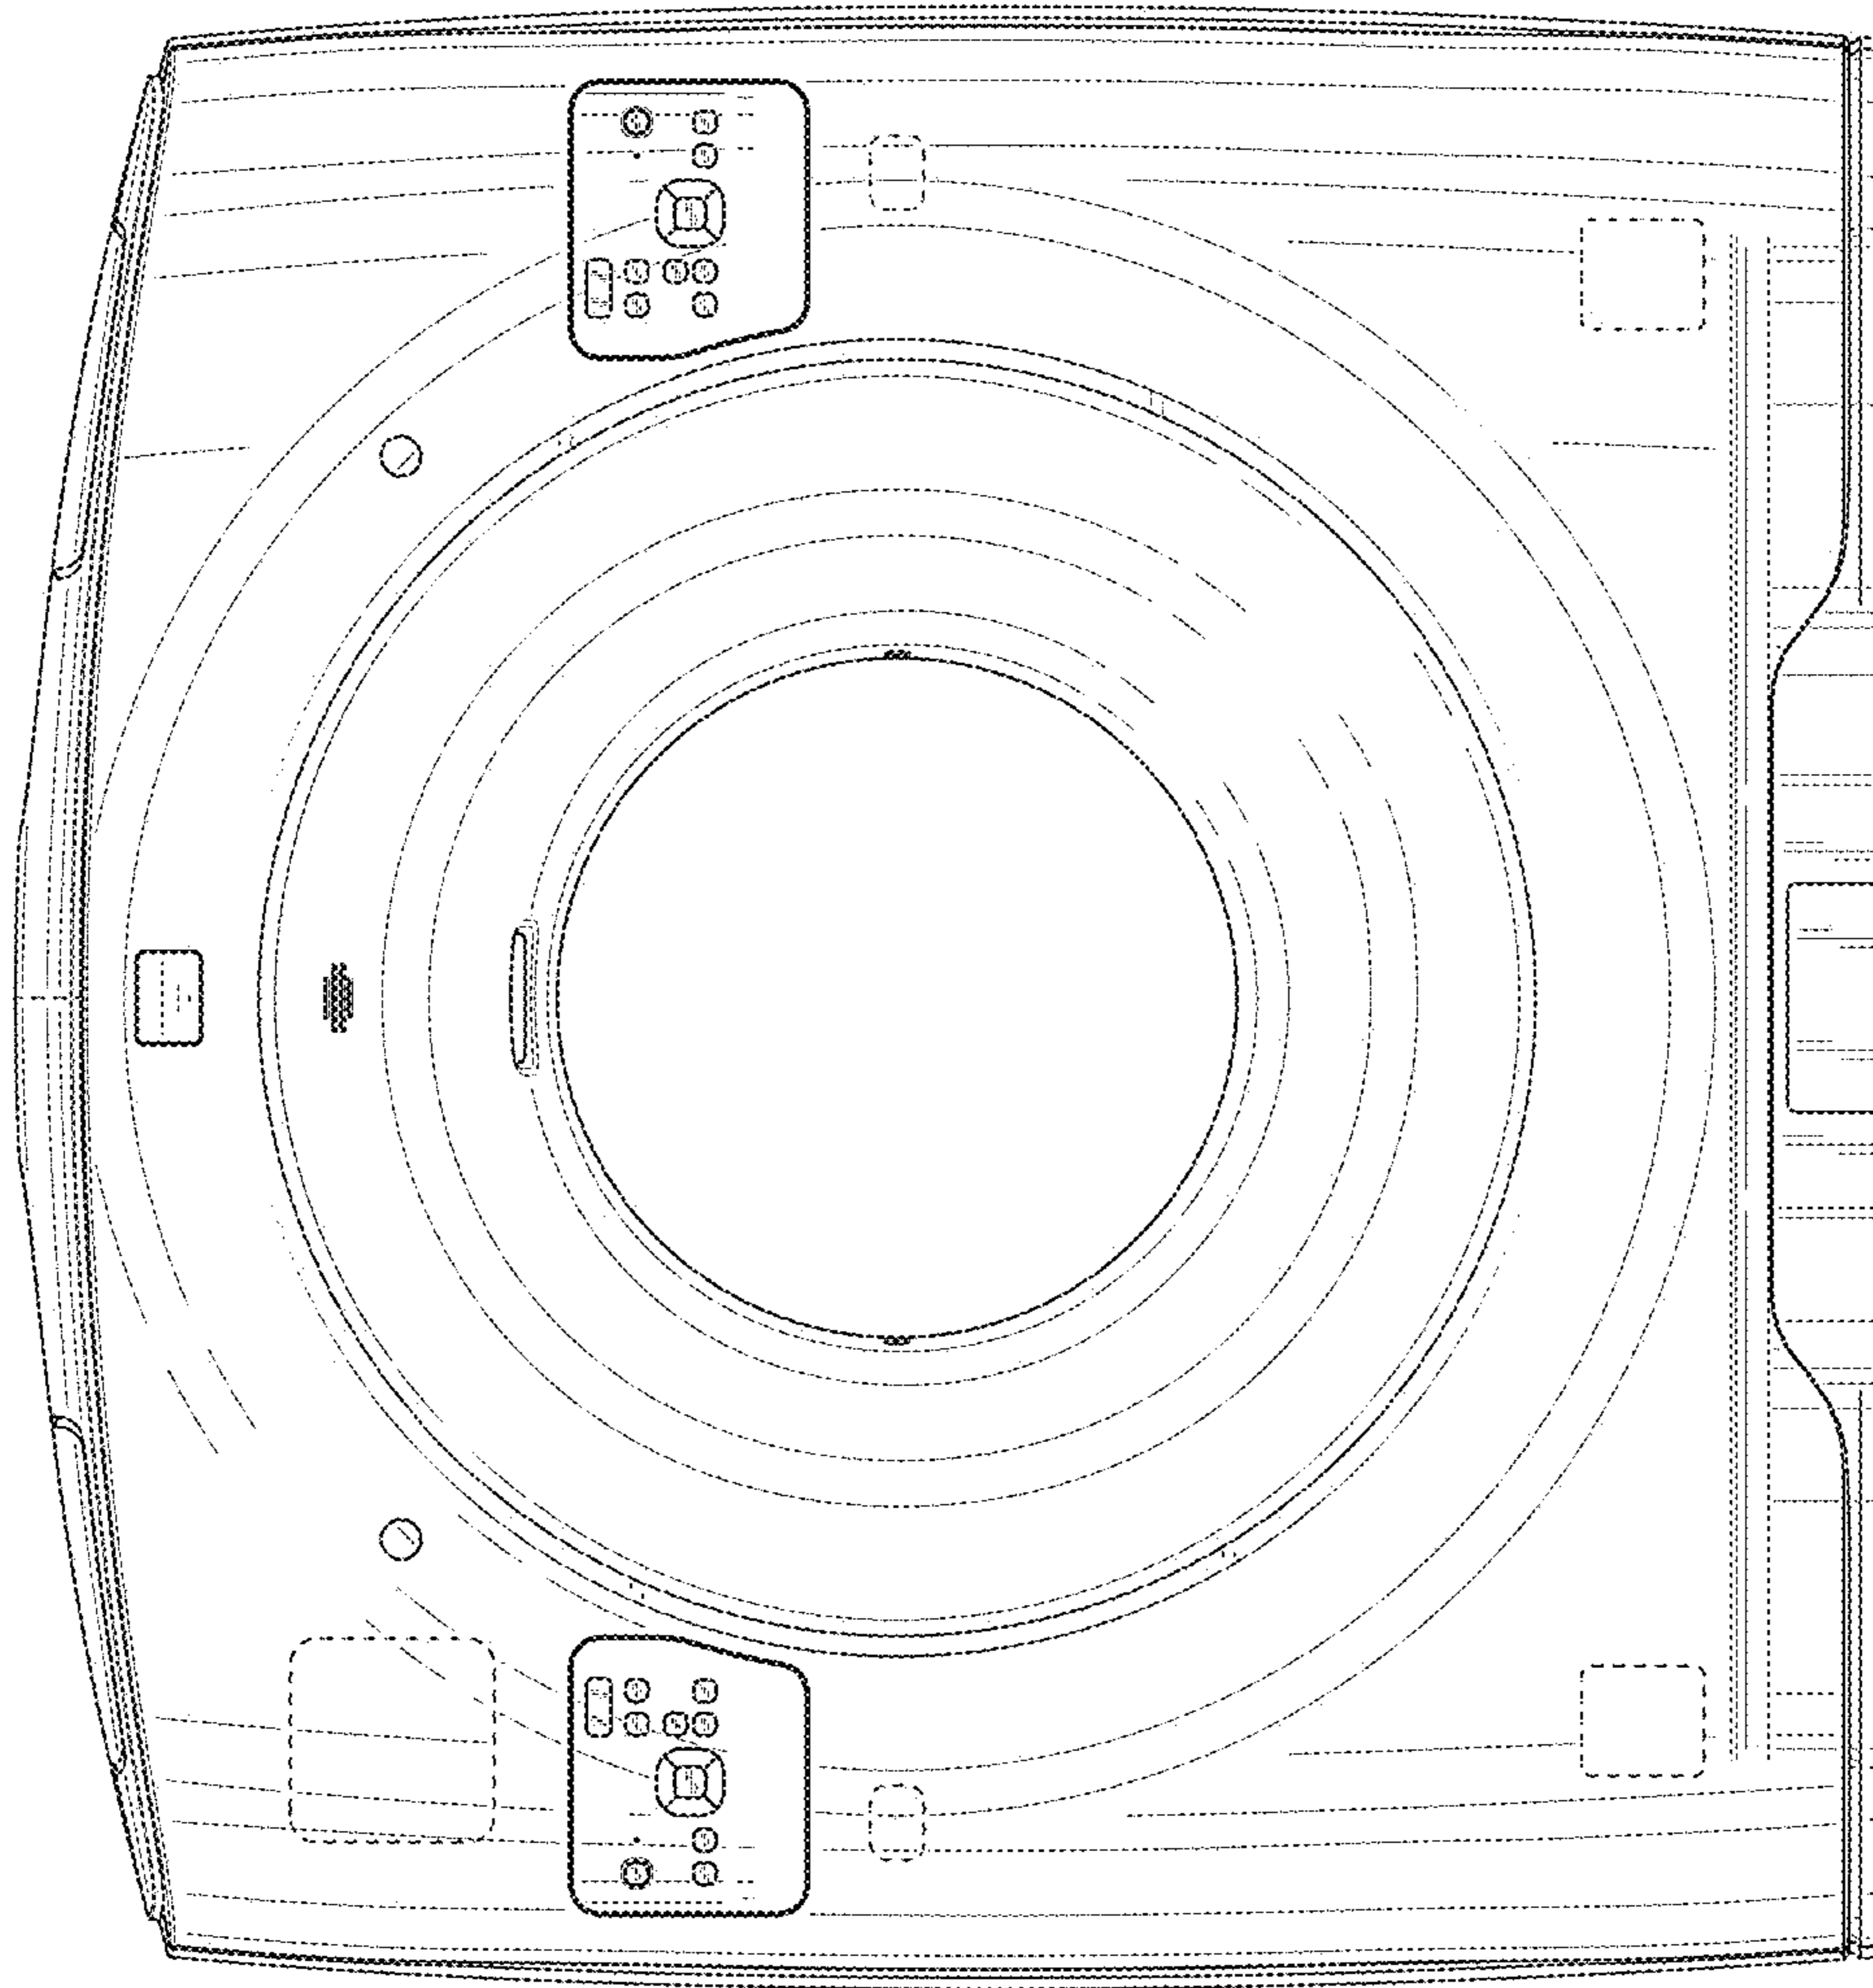


FIG. 3

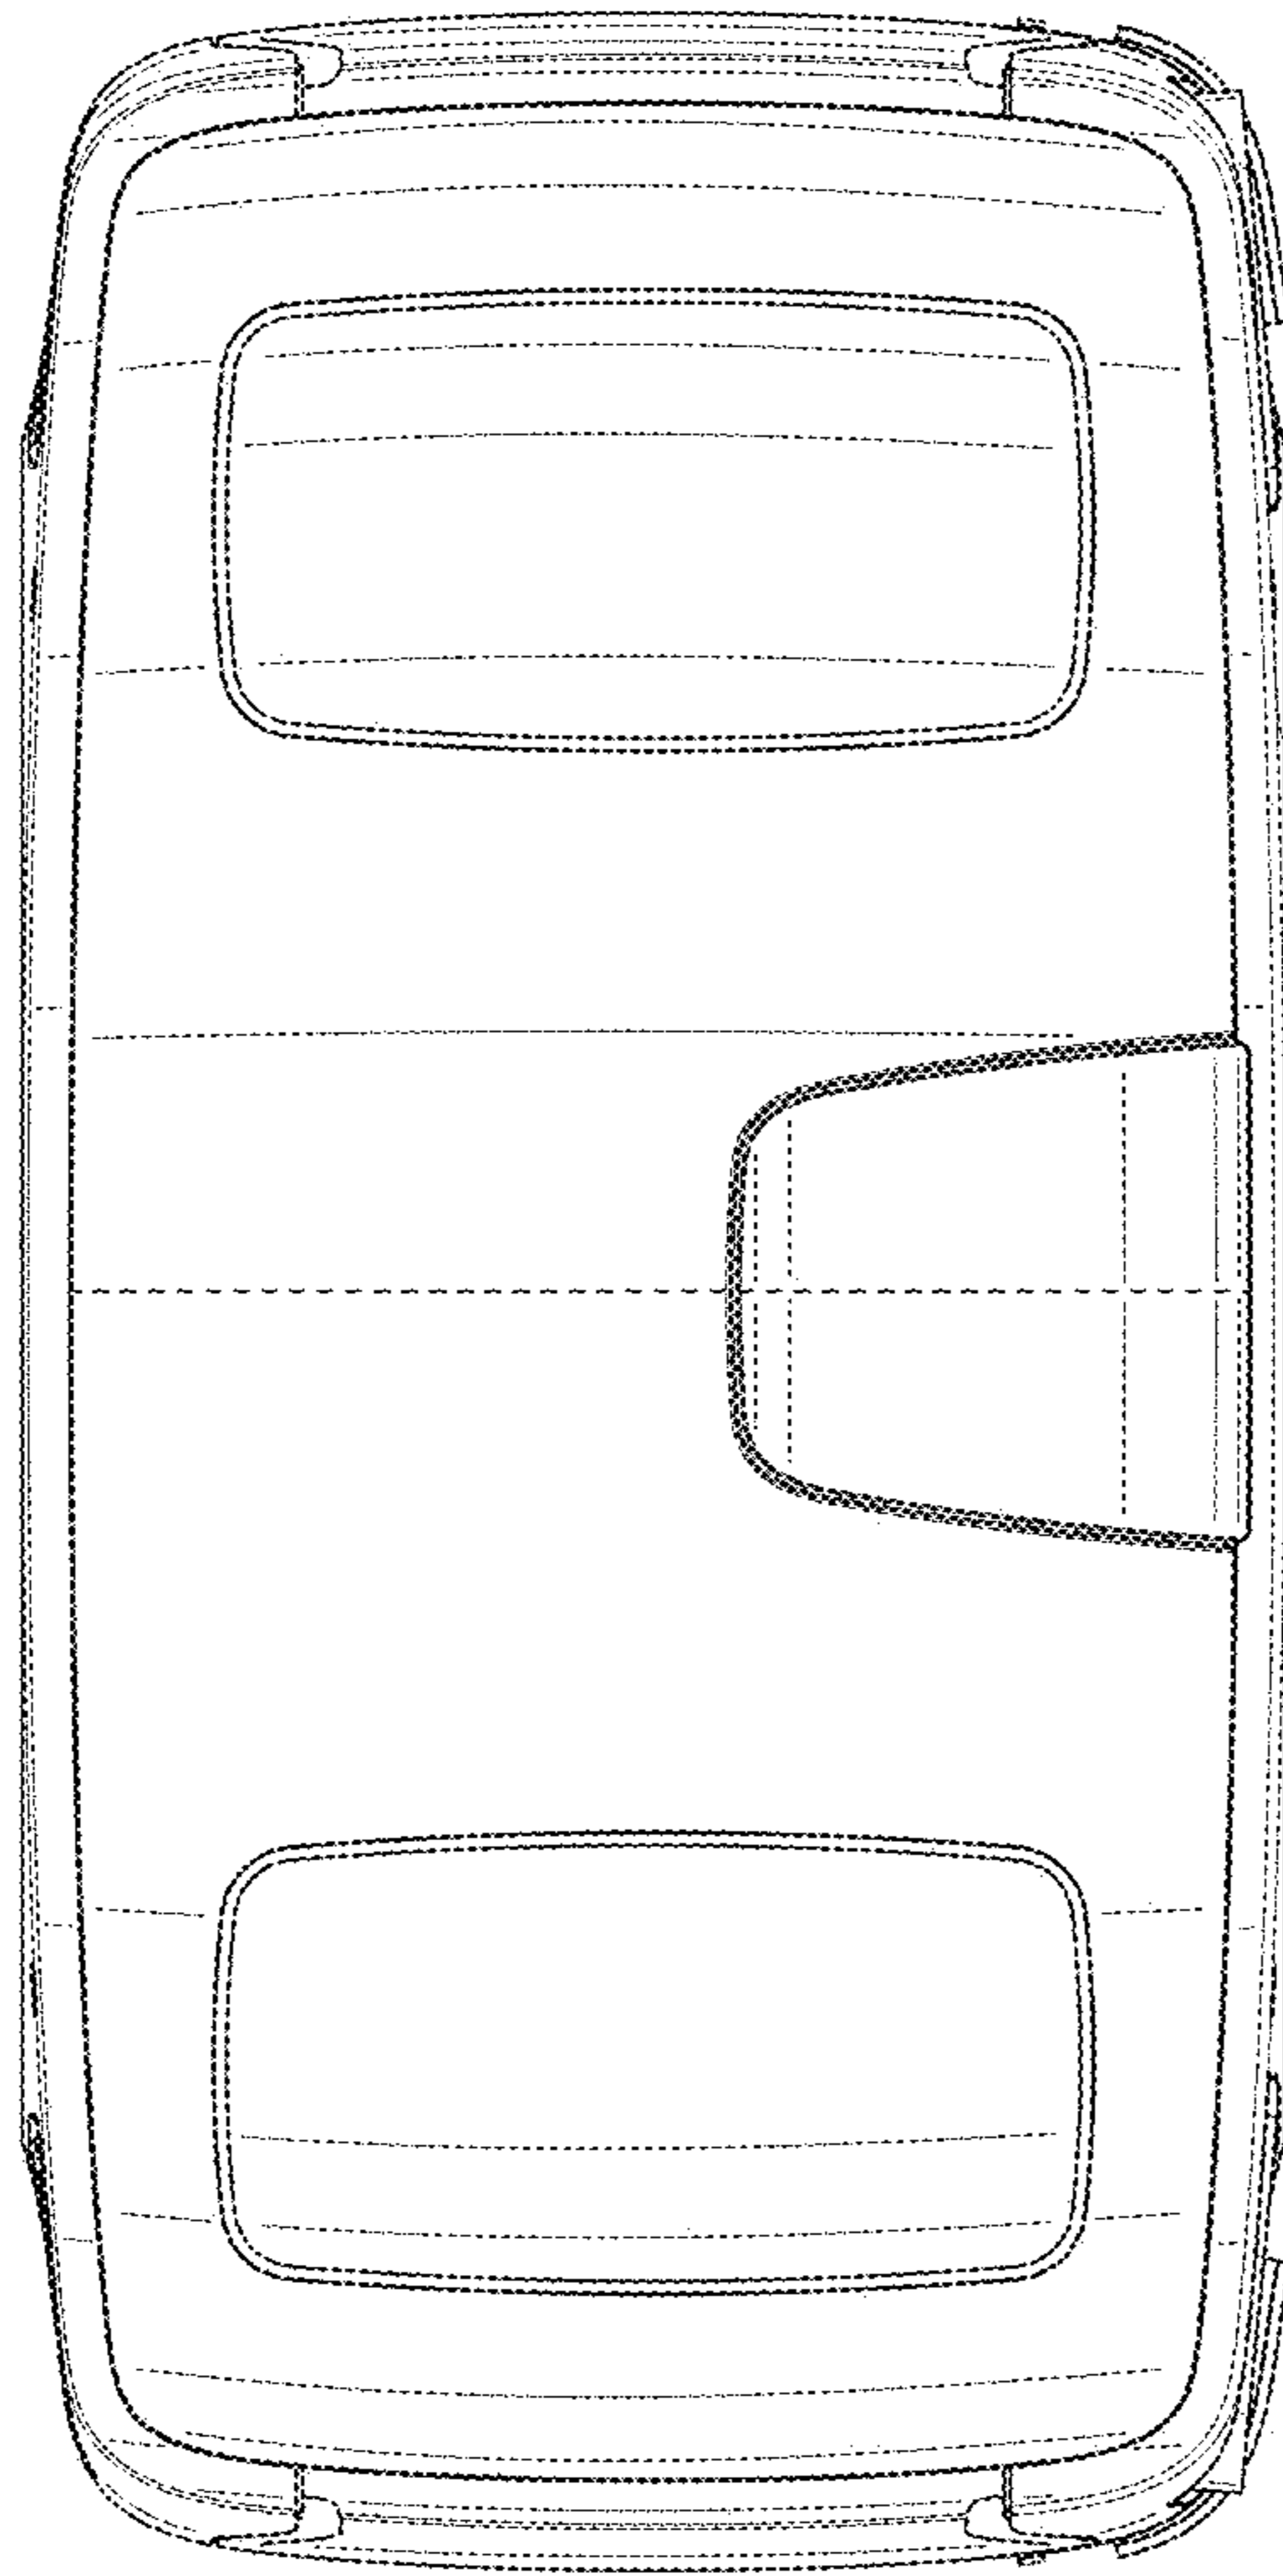


FIG. 4

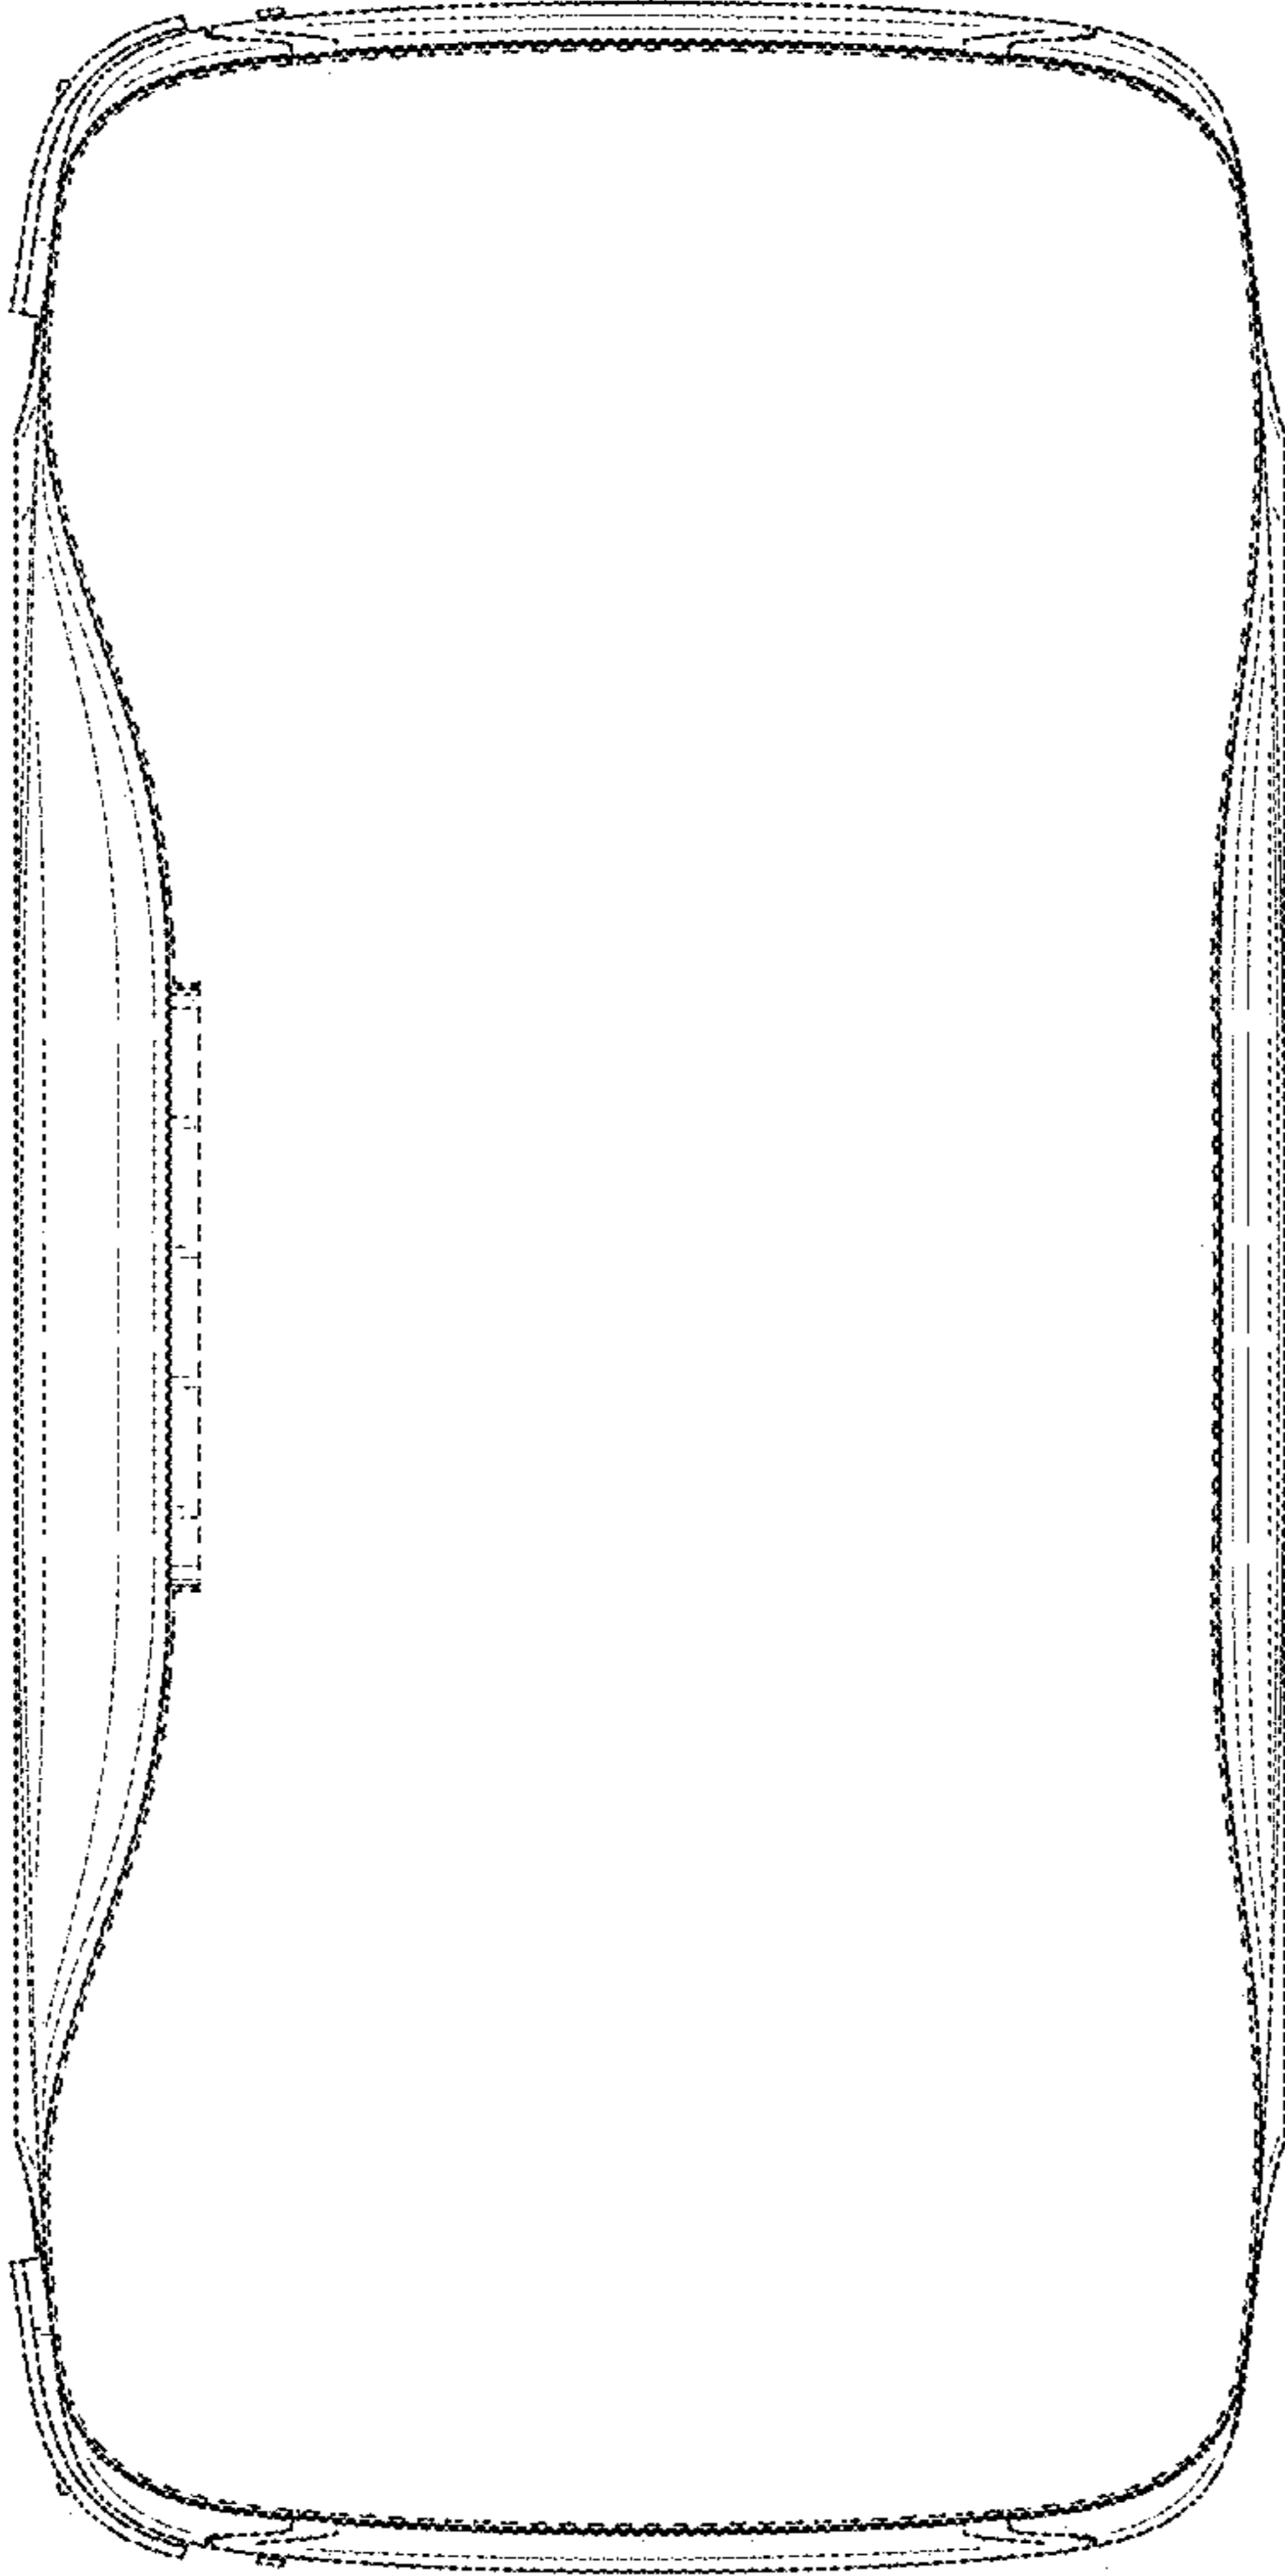


FIG. 5

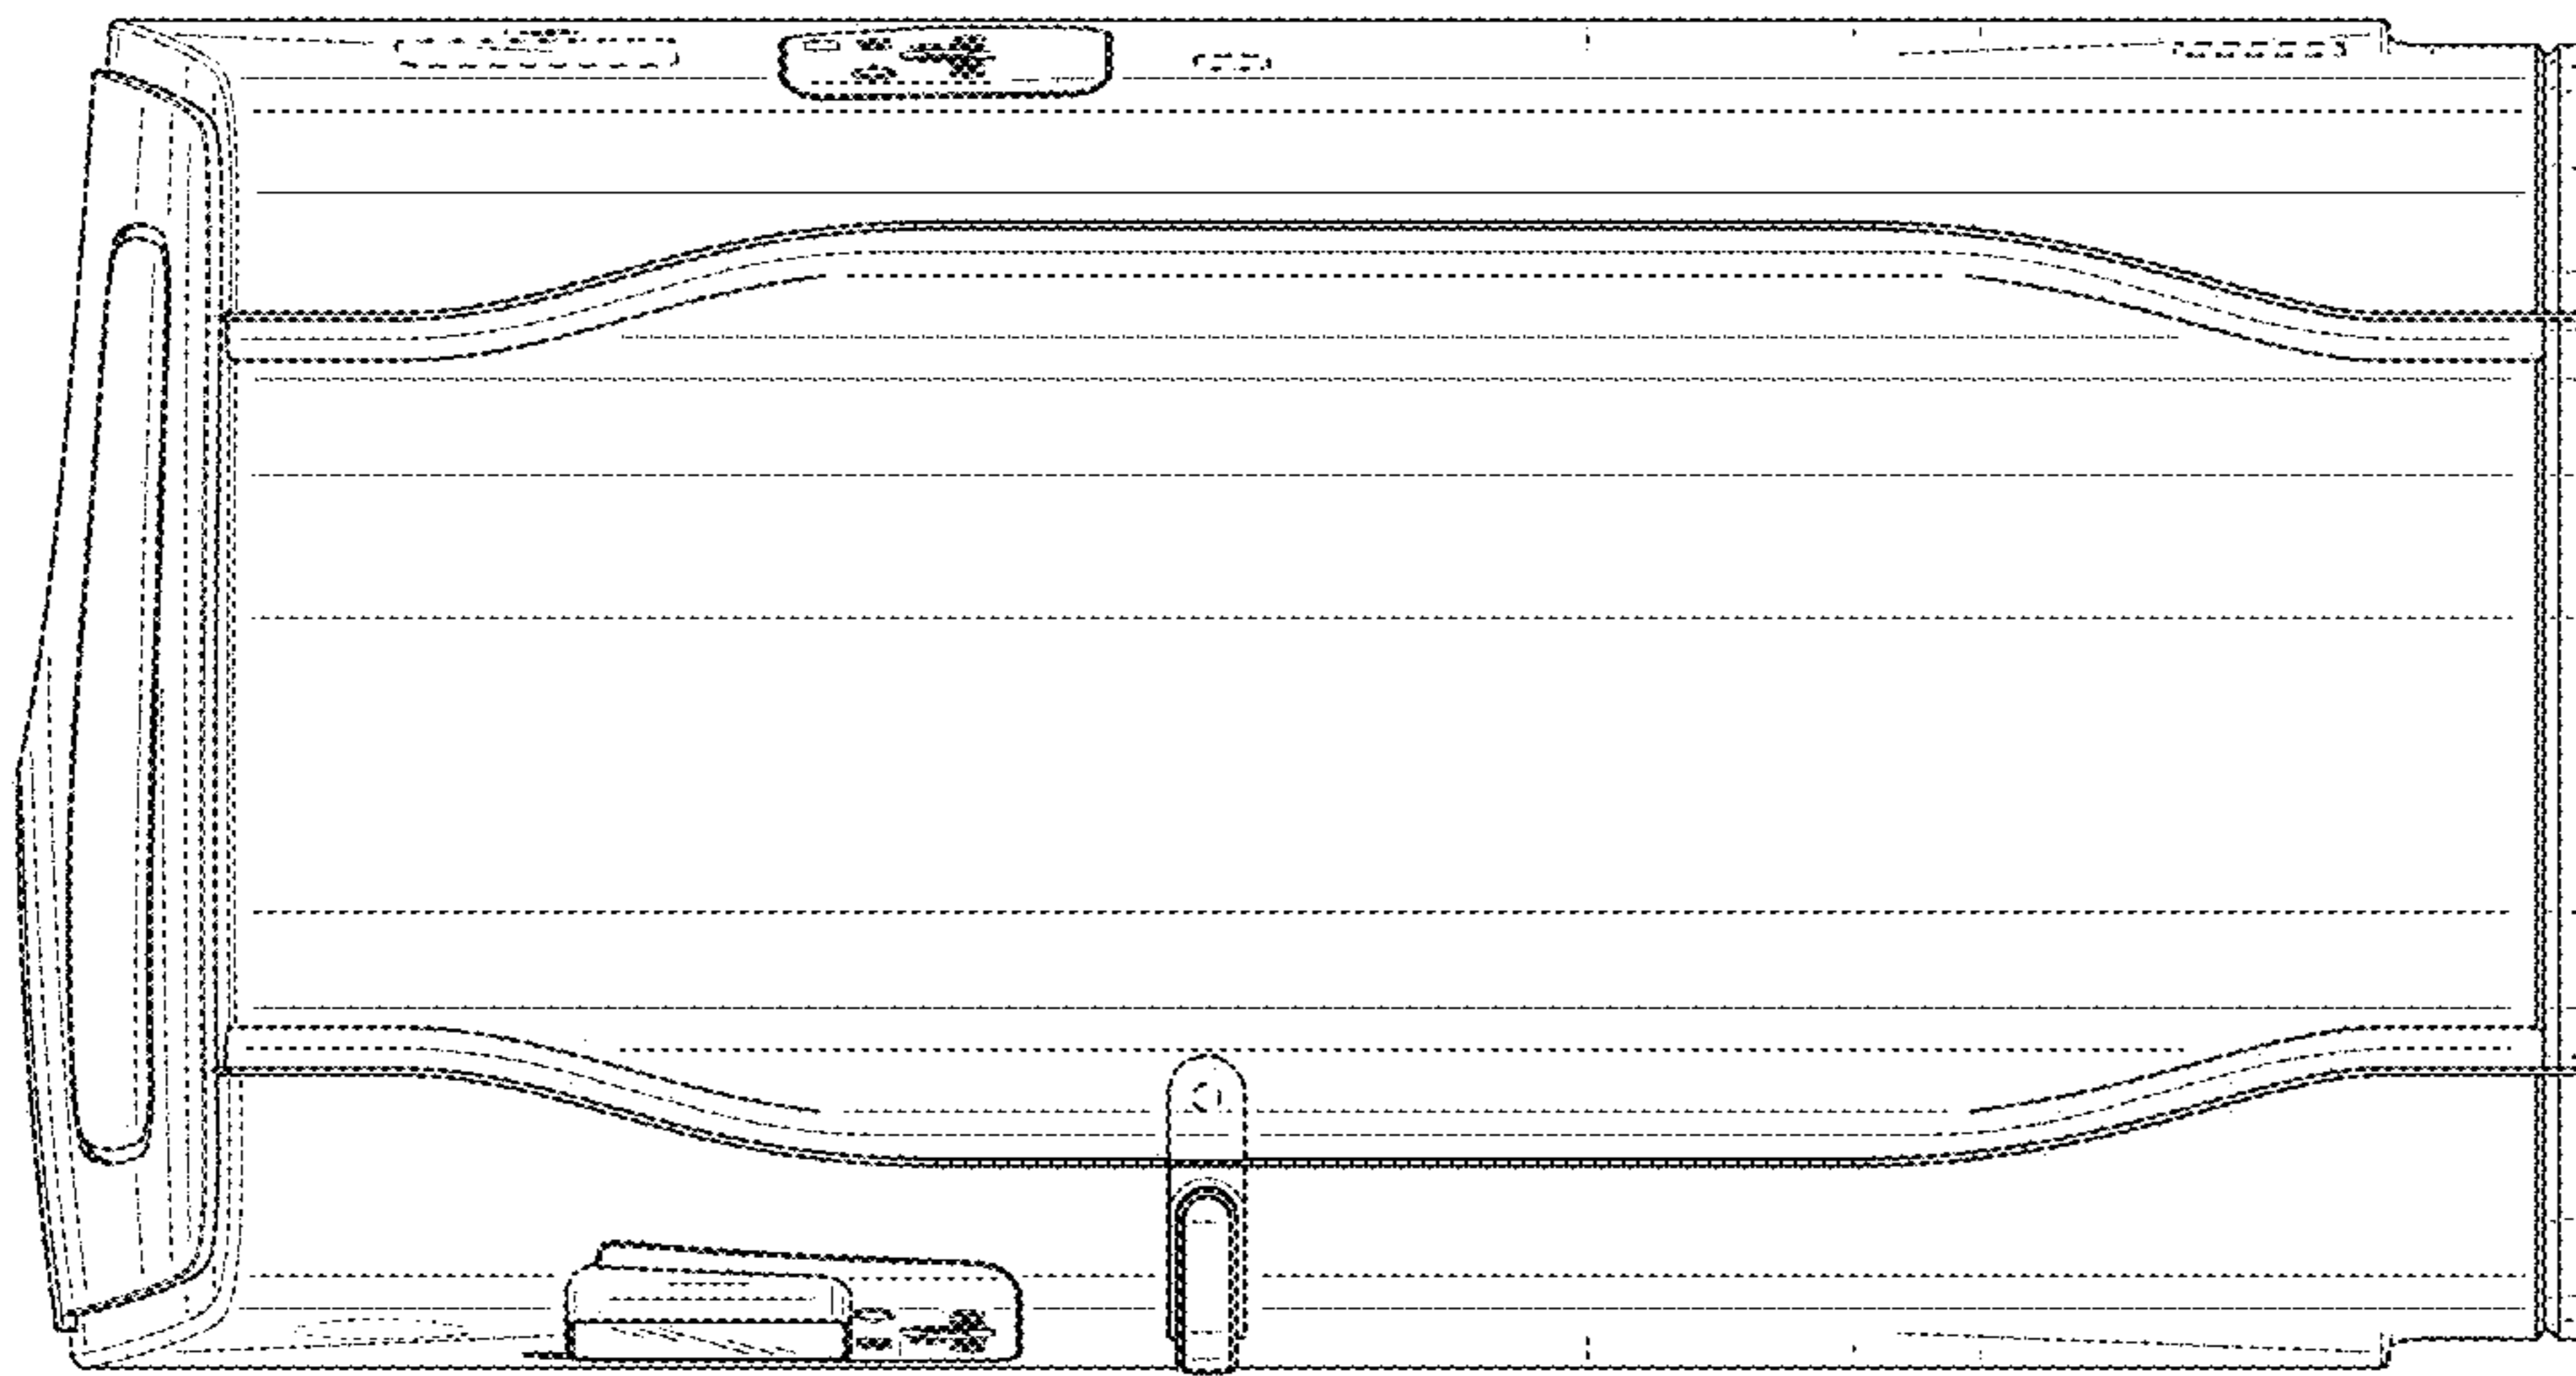


FIG. 6

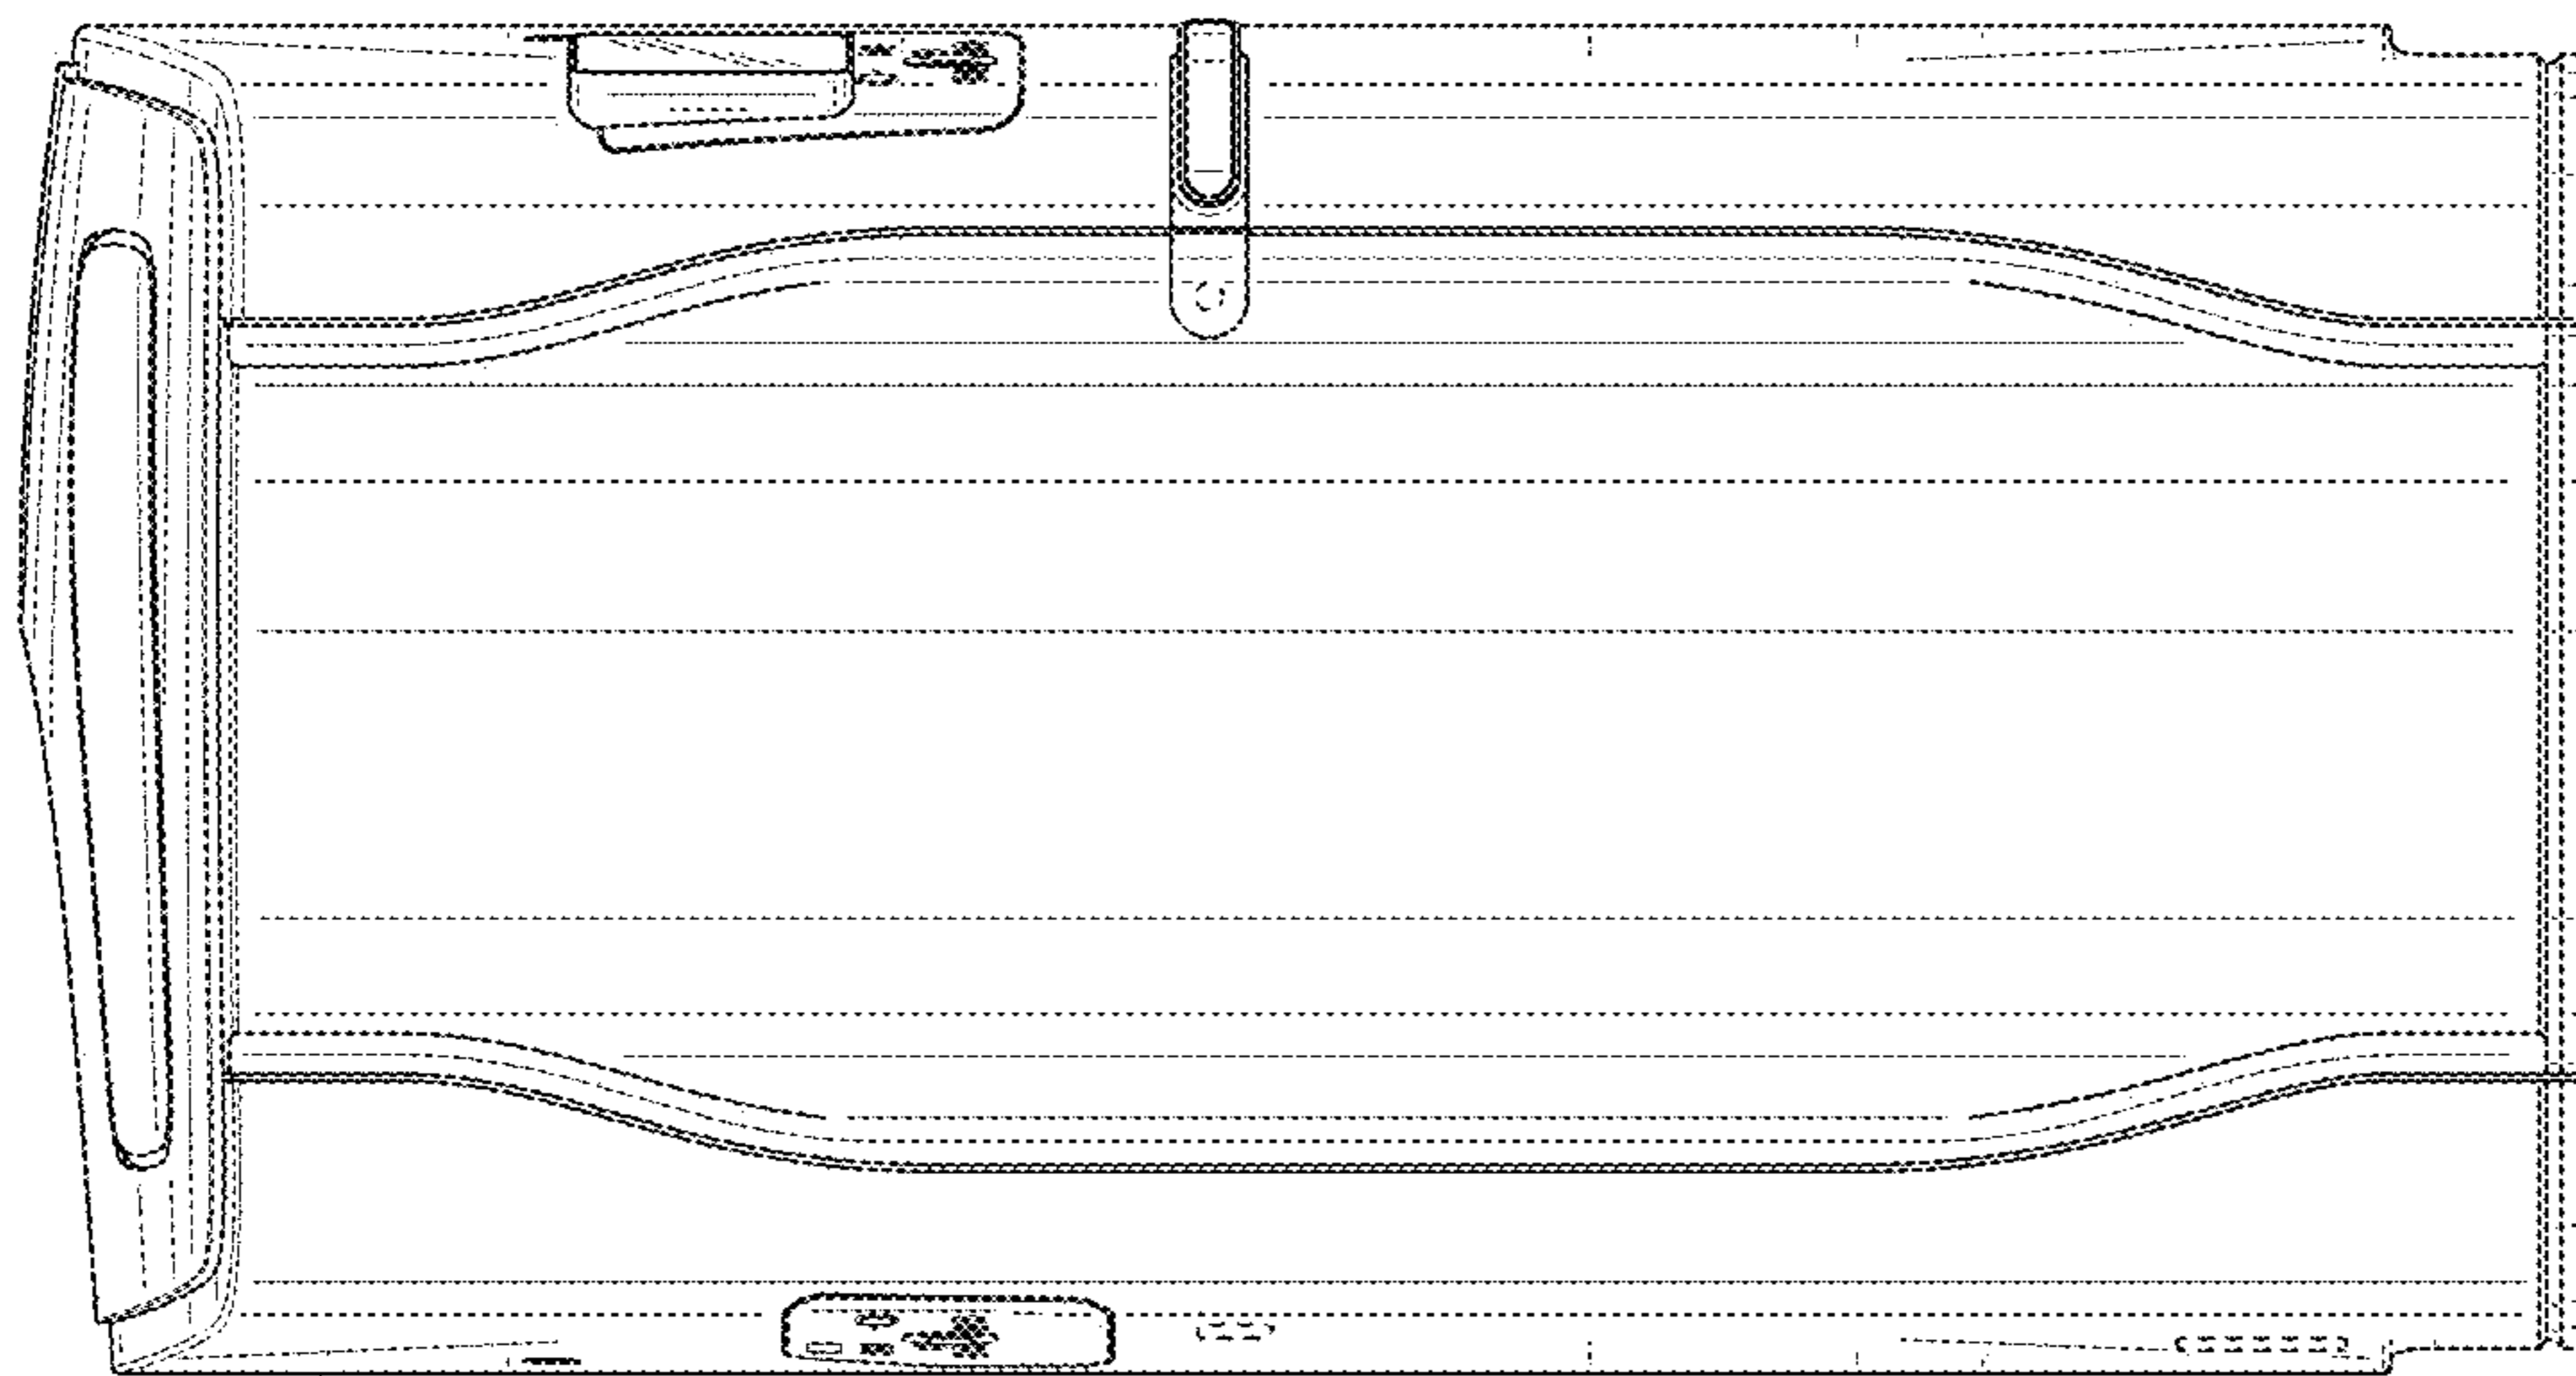


FIG. 7