



US00D930849S

(12) **United States Design Patent** (10) **Patent No.:** **US D930,849 S**  
**Liping et al.** (45) **Date of Patent:** **\*\* Sep. 14, 2021**

- (54) **DIAGNOSTIC TESTING KIT**
- (71) Applicant: **LEADWAY (HK) LIMITED**, Hong Kong (CN)
- (72) Inventors: **Tao Liping**, Hangzhou (CN); **Li Tianhao**, Hangzhou (CN)
- (73) Assignee: **LEADWAY (HK) LIMITED**, Hong Kong (CN)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/655,363**
- (22) Filed: **Jul. 2, 2018**
- (30) **Foreign Application Priority Data**  
Dec. 4, 2017 (CN) ..... 201730610293.X
- (51) **LOC (13) Cl.** ..... **24-02**
- (52) **U.S. Cl.**  
USPC ..... **D24/223**
- (58) **Field of Classification Search**  
USPC ..... D24/107, 108, 112–114, 127, 130, 133, D24/169, 186, 216–217, 219, 222–226, D24/227, 231, 232; D10/81  
(Continued)
- (56) **References Cited**  
**U.S. PATENT DOCUMENTS**  
D491,274 S \* 6/2004 Dubniczki ..... D24/223  
D499,812 S \* 12/2004 Wu ..... D24/223  
(Continued)  
**FOREIGN PATENT DOCUMENTS**  
CN 201130305528 \* 9/2011  
**OTHER PUBLICATIONS**

Global Ovulation Test Kit Market2019—Clearblue, Wondfu, Fertile Focus, Premom. Online, published date Apr. 30, 2019. Retrieved on

Jul. 25, 2019 from URL: <https://newsstockexchange.com/32357/global-ovulation-test-kit-market-2019-clearblue-wondfu-fertile-focus-premom/>.\*

*Primary Examiner* — Susan Bennett Hattan  
*Assistant Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Acuity Law Group, PC; Michael A. Whittaker


(57) **CLAIM**

The ornamental design for a diagnostic testing kit, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan view of a first embodiment of a diagnostic testing kit;  
 FIG. 2 is a front elevation view of the first embodiment;  
 FIG. 3 is a rear elevation view of the first embodiment;  
 FIG. 4 is a first side elevation view of the first embodiment;  
 FIG. 5 is a bottom plan view of the first embodiment;  
 FIG. 6 is a second side elevation of the first embodiment;  
 FIG. 7 is a front perspective view of the top and first side of the first embodiment.  
 FIG. 8 is a front perspective view of the bottom and second side of the first embodiment;  
 FIG. 9 is a top plan view of a second embodiment of a diagnostic testing apparatus design;  
 FIG. 10 is a front elevation view of the second embodiment;  
 FIG. 11 is a rear elevation view of the second embodiment;  
 FIG. 12 is a first side elevation view of the second embodiment;  
 FIG. 13 is a bottom plan view of the second embodiment;  
 FIG. 14 is a second side elevation of the second embodiment;  
 FIG. 15 is a front perspective view of the top and first side of the second embodiment; and,  
 FIG. 16 is a front perspective view of the bottom and second side of the second embodiment.  
 The broken lines in the drawings depict portions of the diagnostic testing kit that form no part of the claimed design.

**1 Claim, 16 Drawing Sheets**

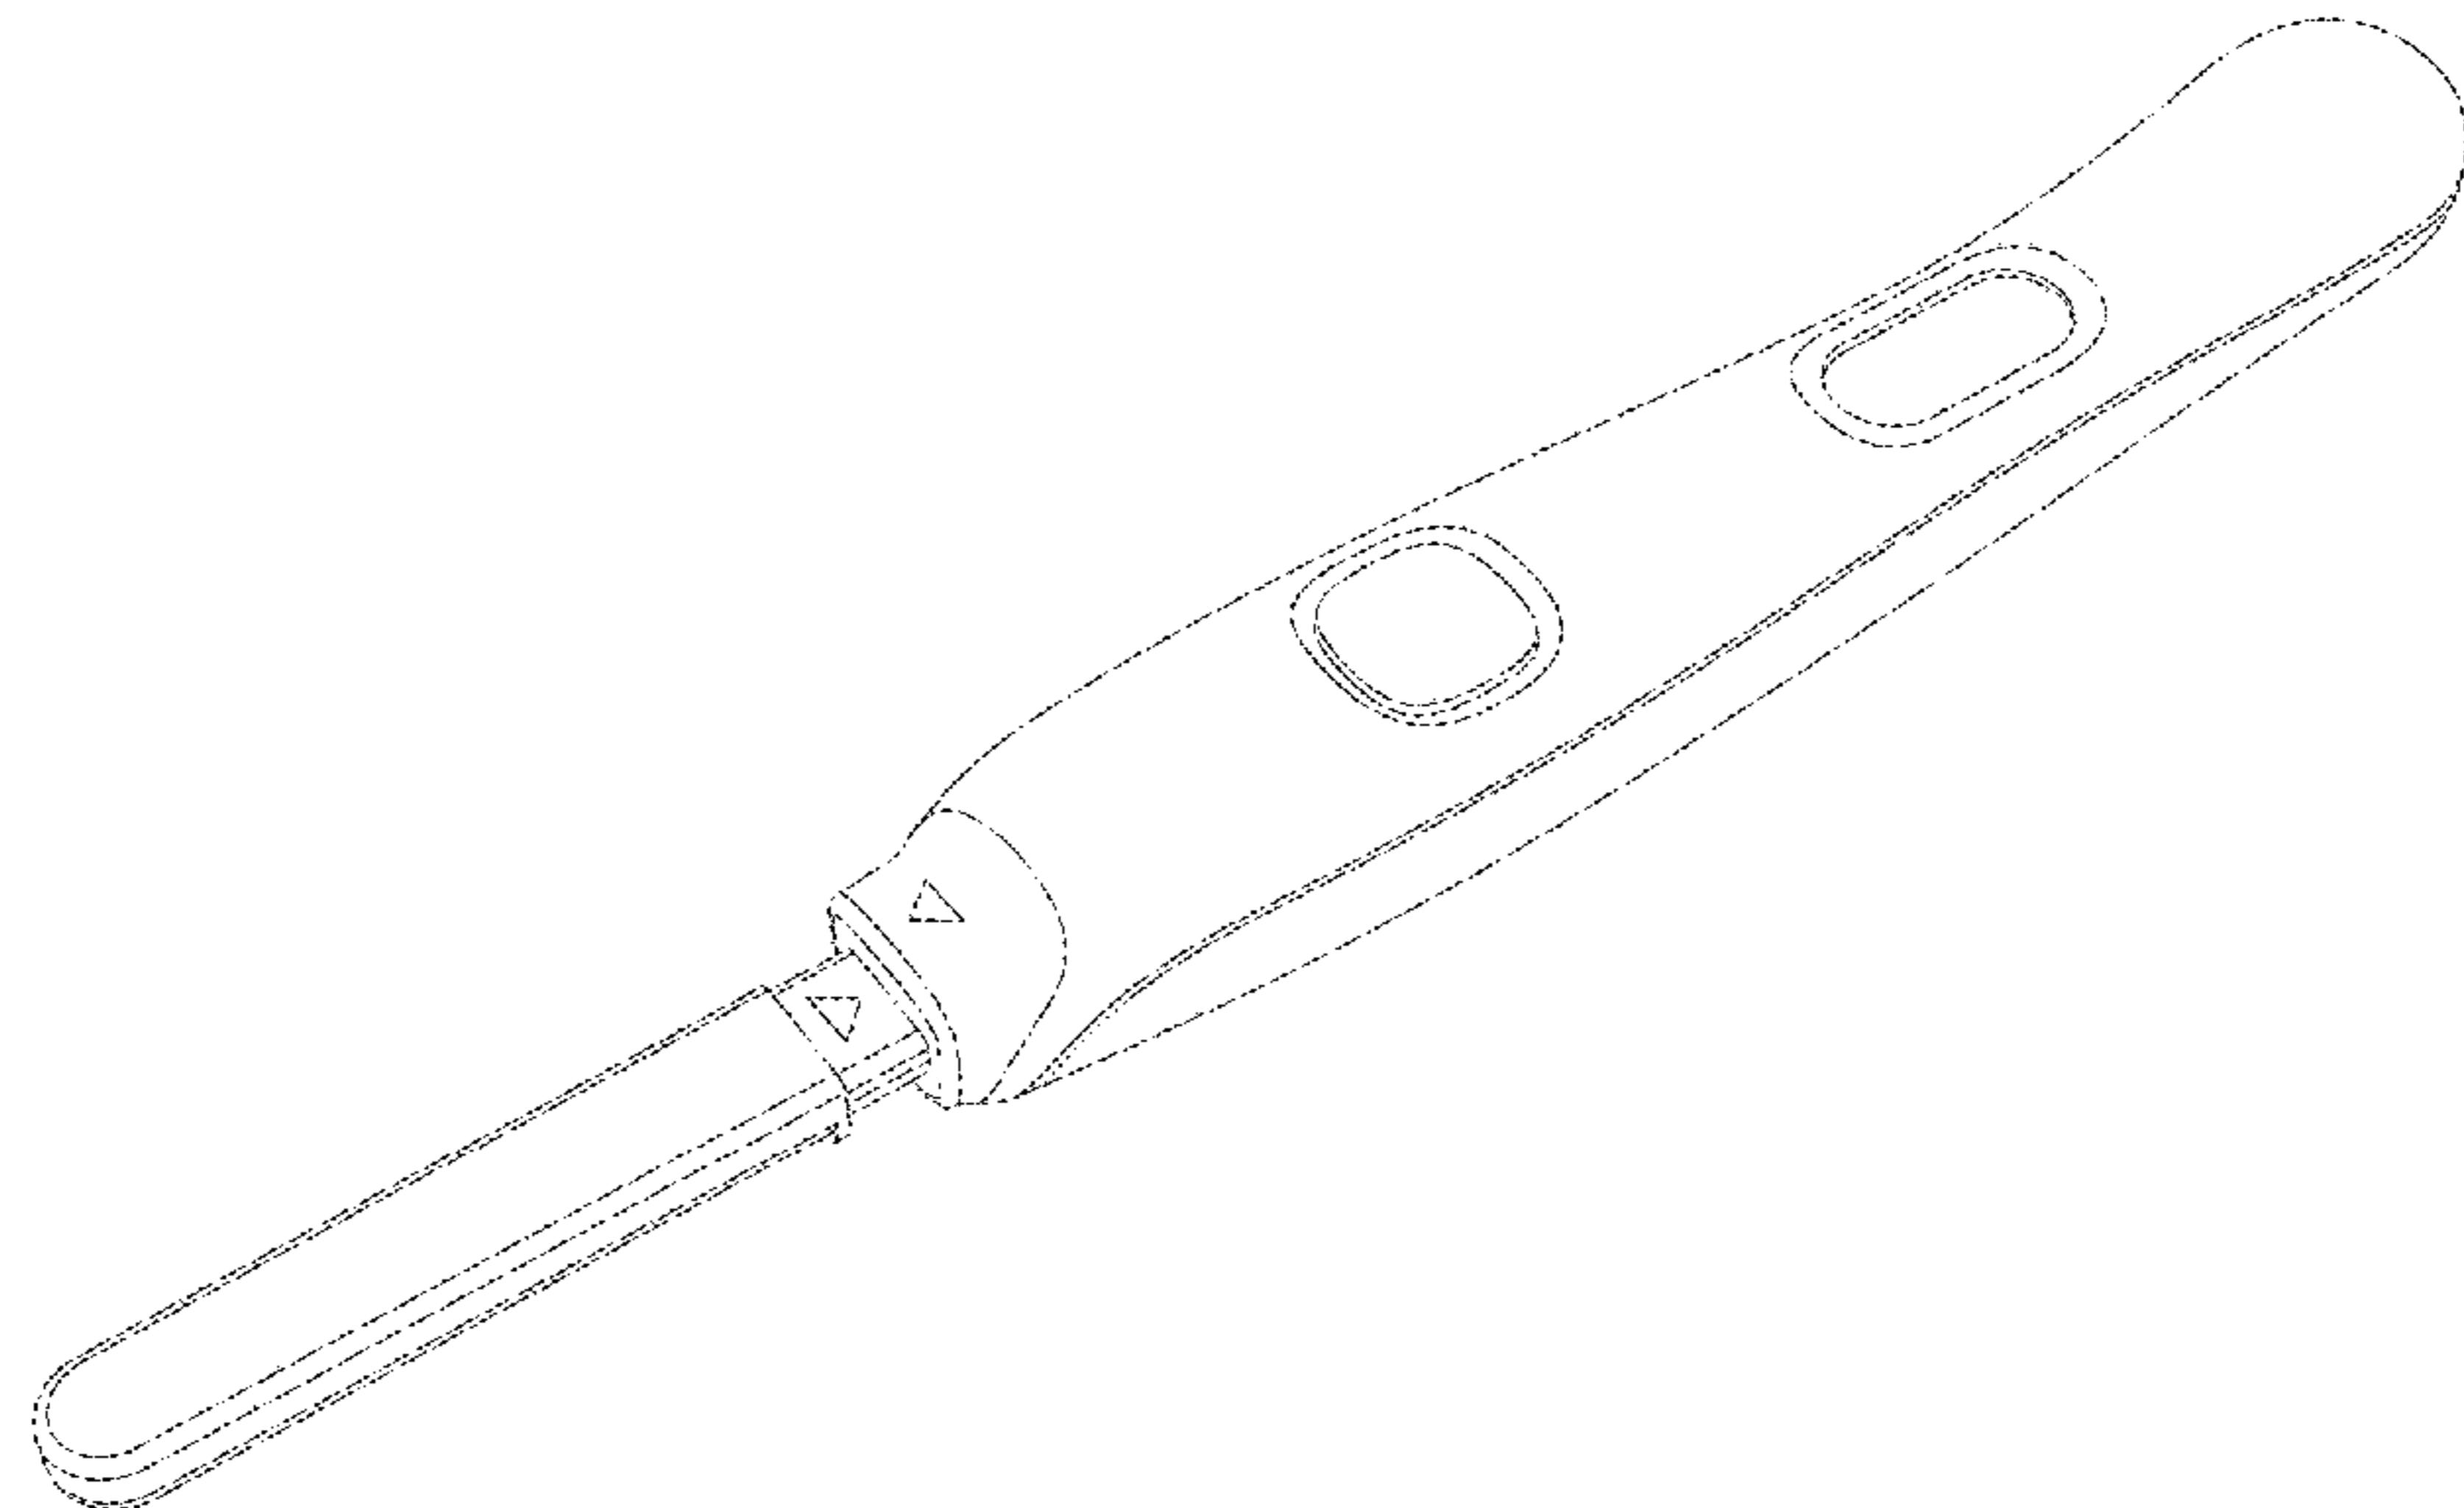

(58) **Field of Classification Search**

CPC ..... G01N 33/76; G01N 33/558; G01N  
33/54386; G01N 21/8483

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D523,964	S	6/2006	Phelan et al.	
D537,167	S *	2/2007	Sigel .....	D24/223
D537,169	S	2/2007	Sigel et al.	
D537,531	S	2/2007	Sigel et al.	
D557,815	S *	12/2007	Lee .....	D24/223
D570,490	S *	6/2008	Laverack .....	D24/225
D571,019	S *	6/2008	Laverack .....	D24/225
D571,020	S *	6/2008	Laverack .....	D24/225
D574,966	S *	8/2008	Laverack .....	D24/225
D575,876	S *	8/2008	Laverack .....	D24/225
D575,877	S *	8/2008	Laverack .....	D24/225
D576,737	S *	9/2008	Lee .....	D24/216
D592,759	S *	5/2009	Laverack .....	D24/225
D672,880	S	12/2012	Laverack et al.	
D676,144	S	2/2013	Laverack et al.	
D676,569	S	2/2013	Laverack et al.	
D694,903	S	12/2013	Laverack et al.	
D698,937	S	2/2014	Laverack et al.	
D735,351	S *	7/2015	Laverack .....	D24/223
9,151,754	B2	10/2015	Snowden et al.	
D825,075	S *	8/2018	Alderete .....	D24/224
2008/0124244	A1	5/2008	Sigel et al.	
2009/0208371	A1	8/2009	Hannant et al.	
2016/0195553	A1 *	7/2016	Wang .....	G01N 33/76 436/65

\* cited by examiner

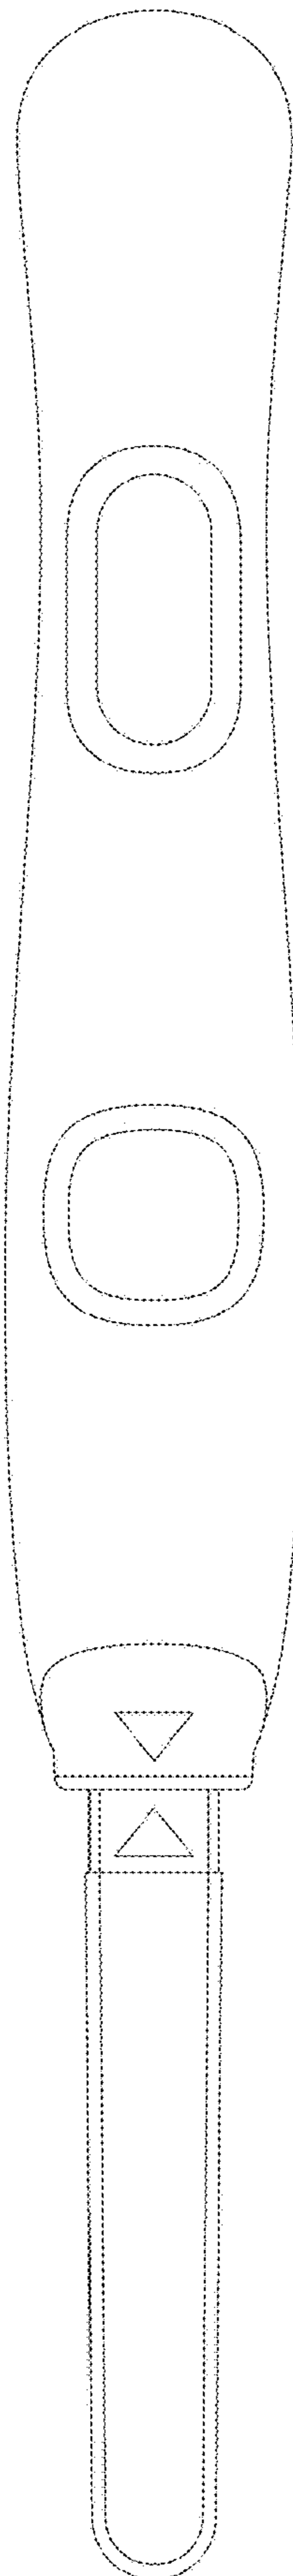


FIG. 1

FIG. 2

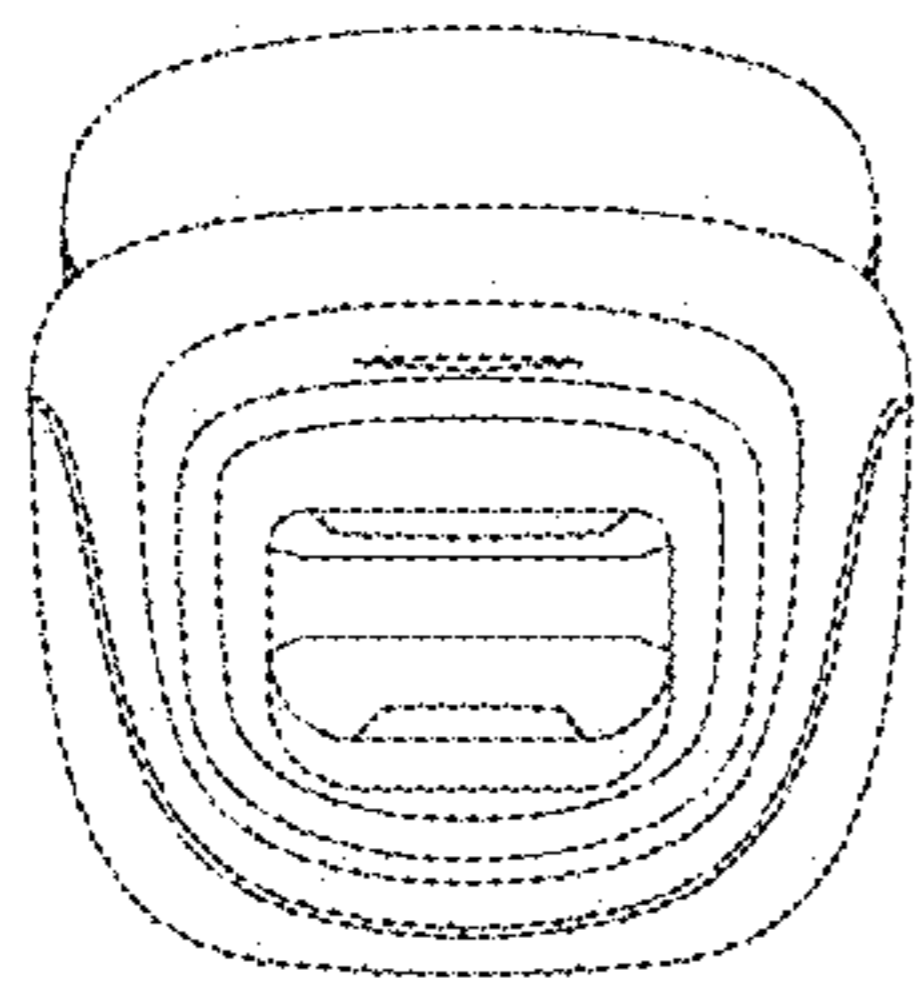
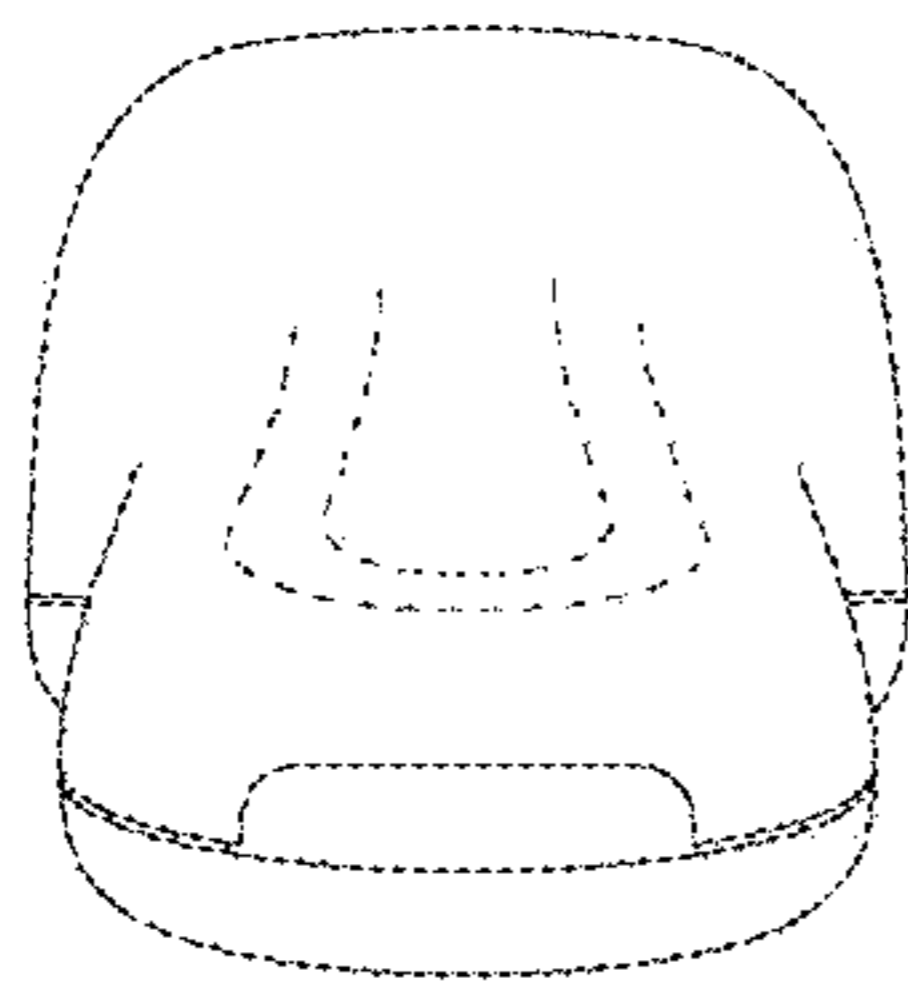


FIG. 3



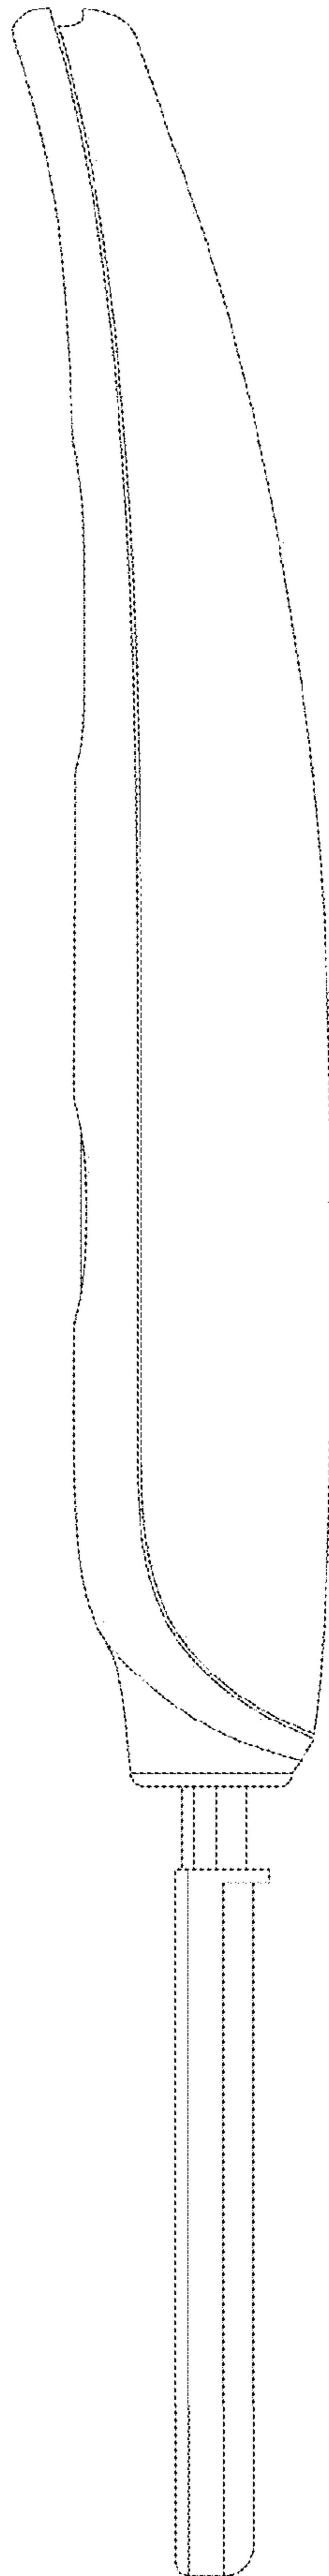


FIG. 4

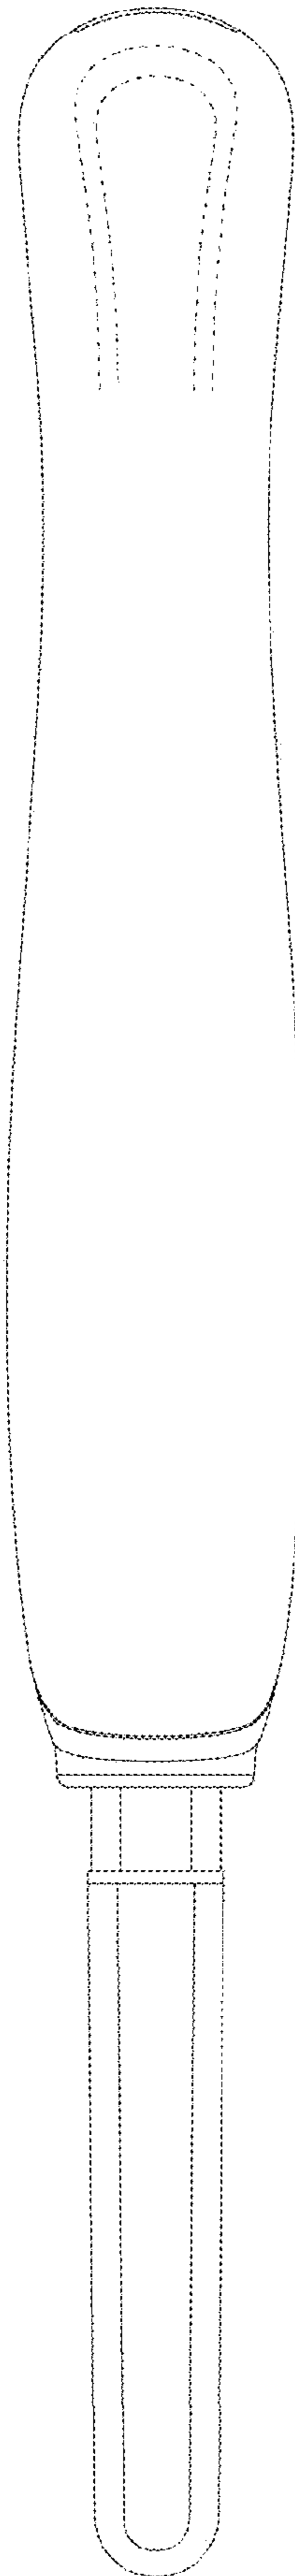


FIG. 5

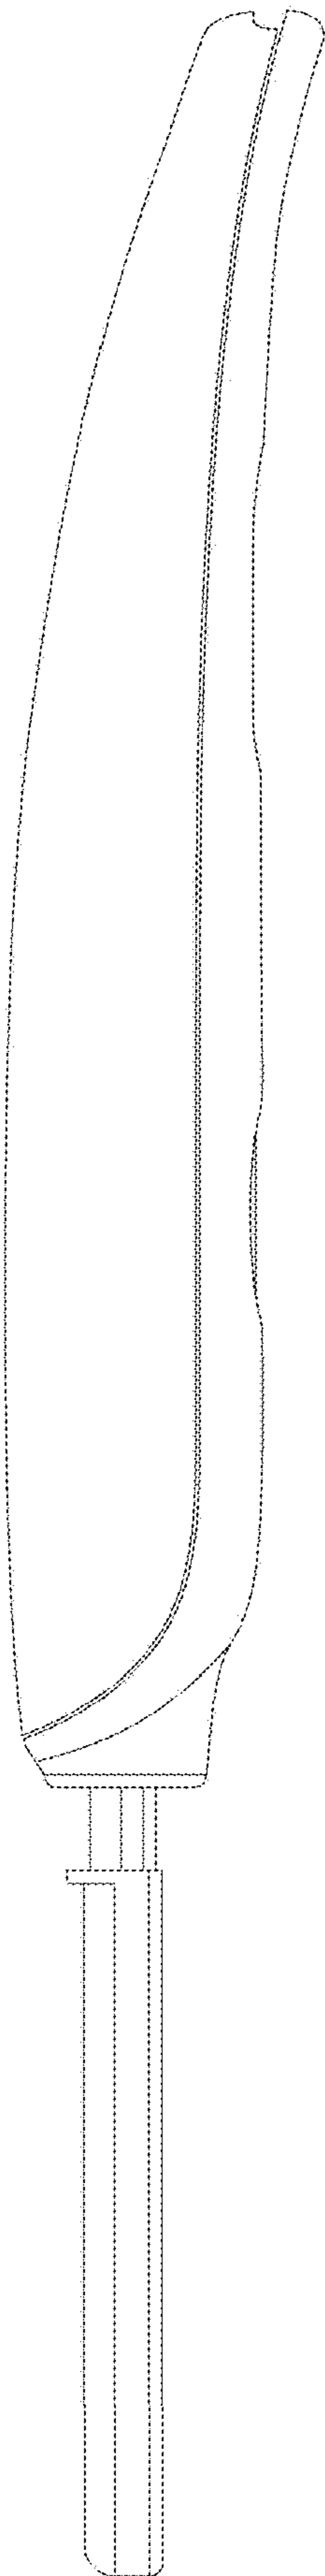


FIG. 6



FIG. 7

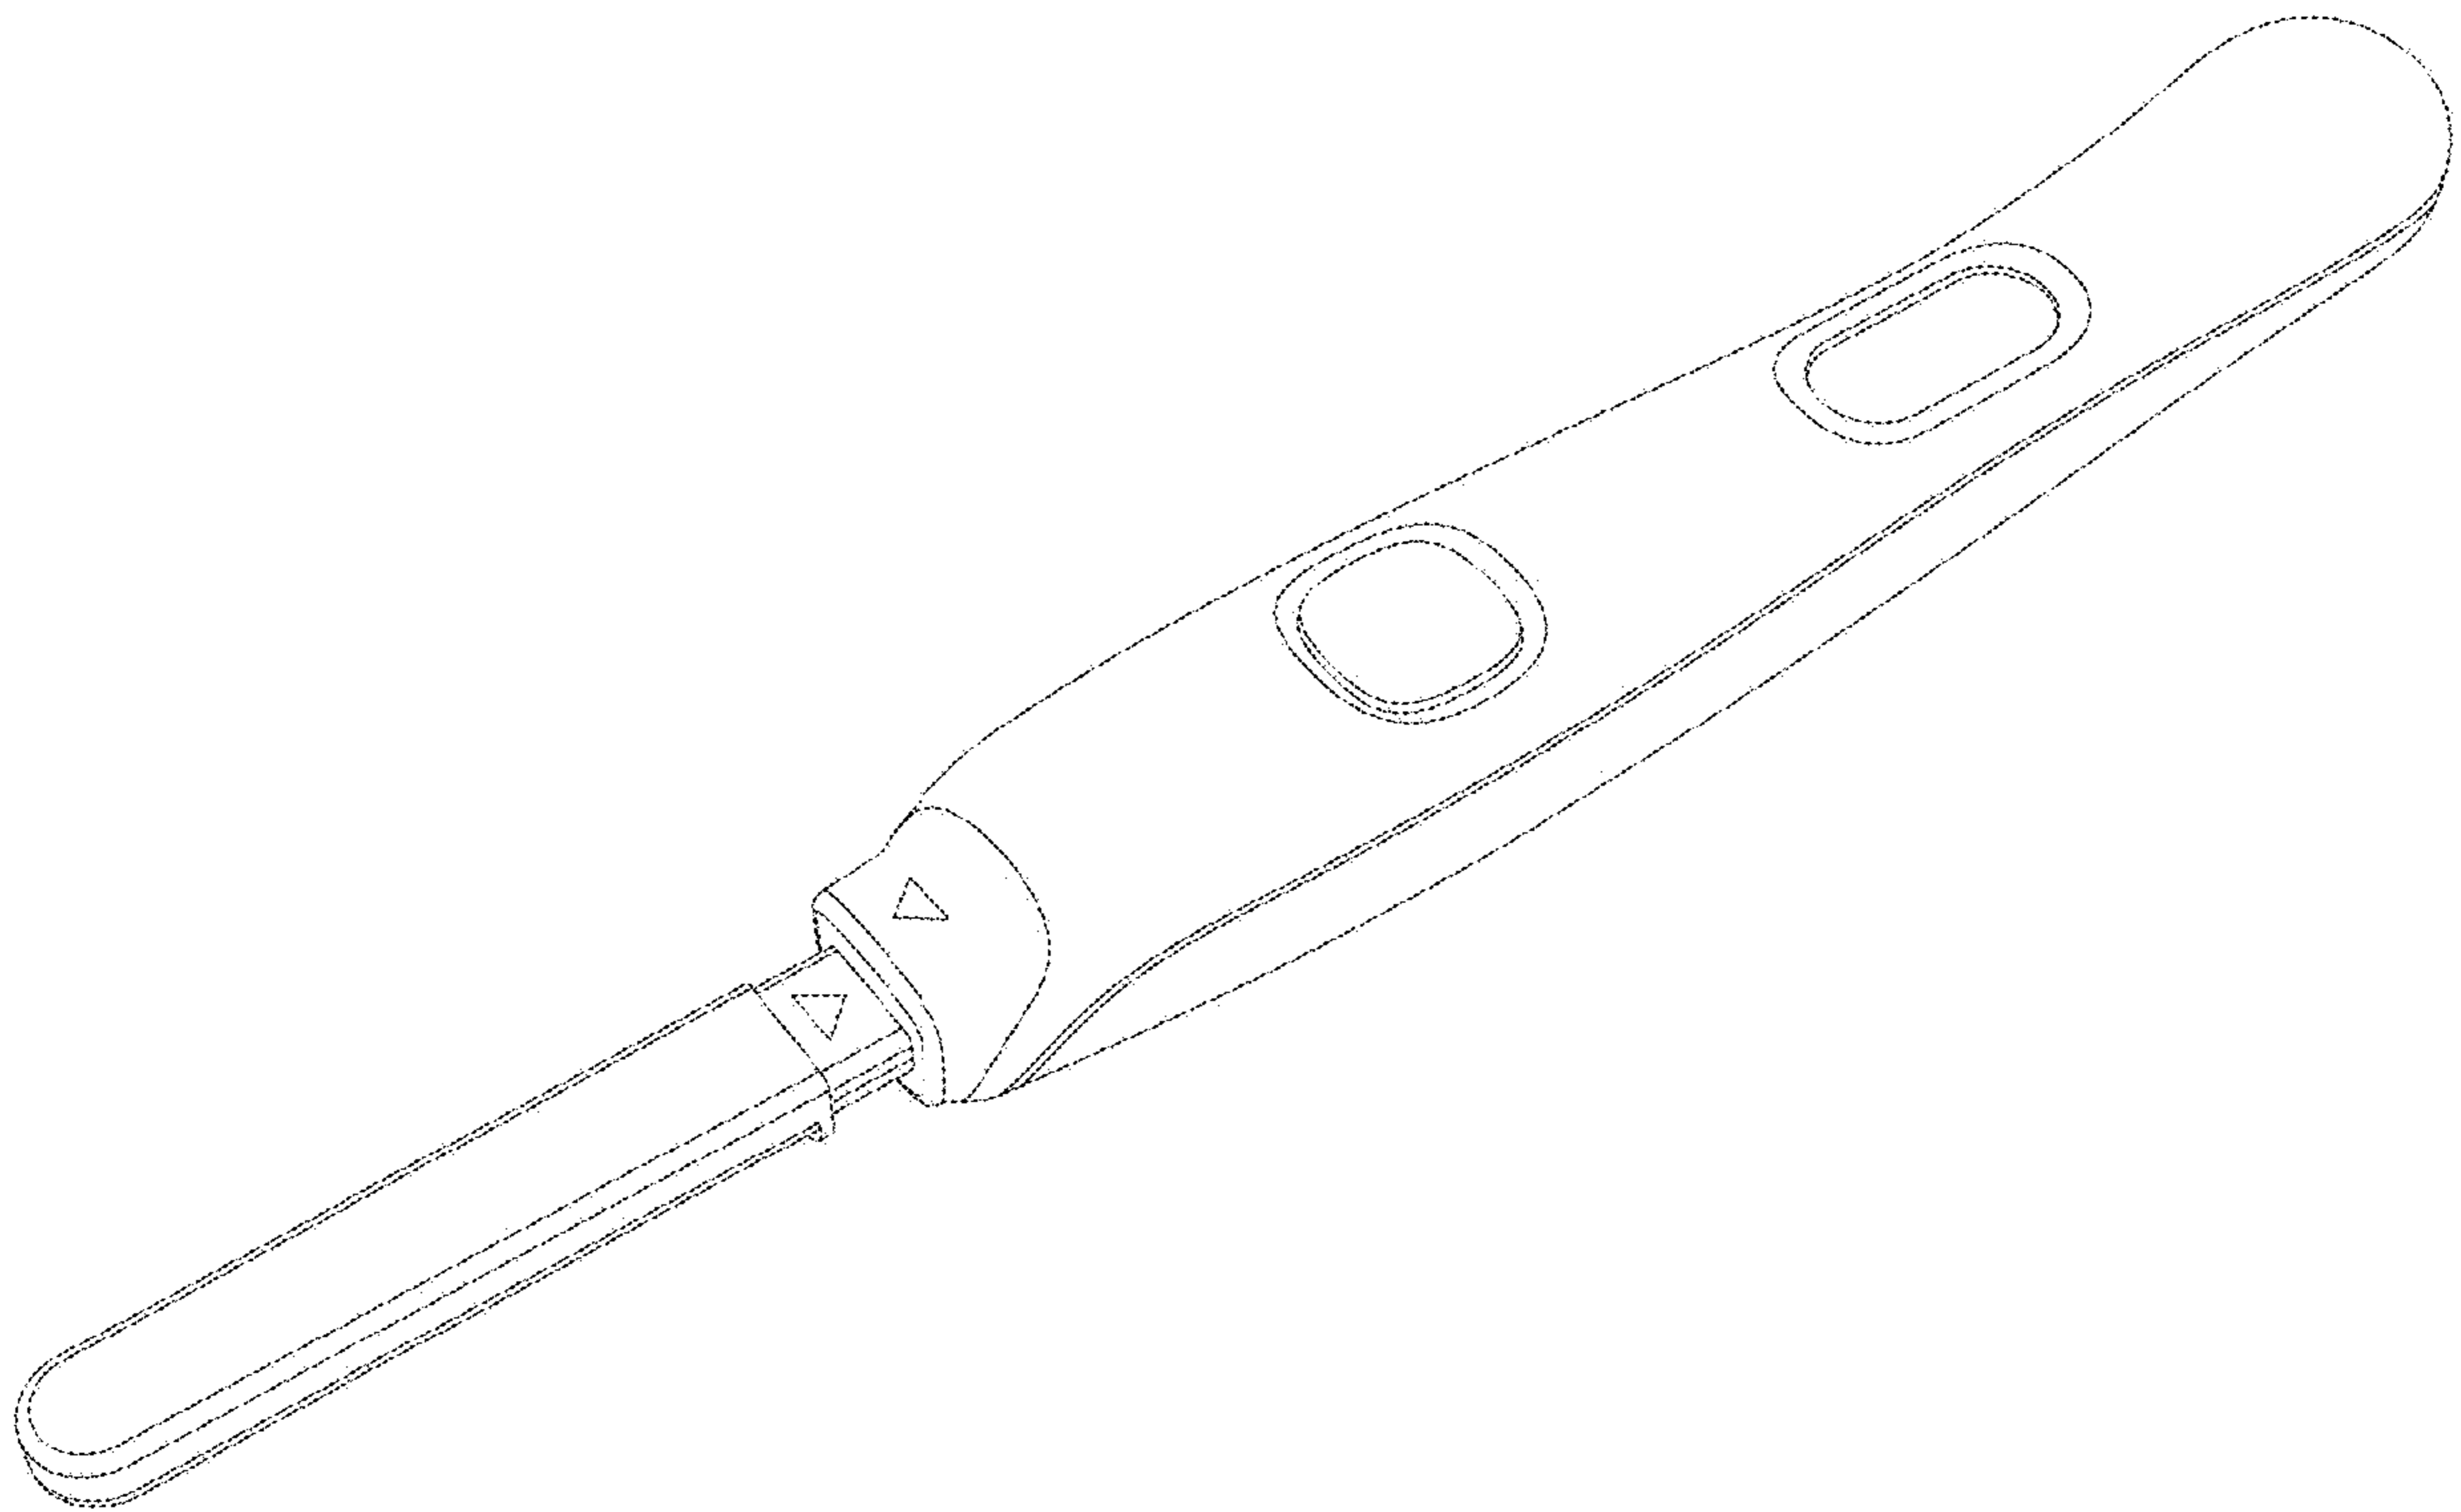


FIG. 8

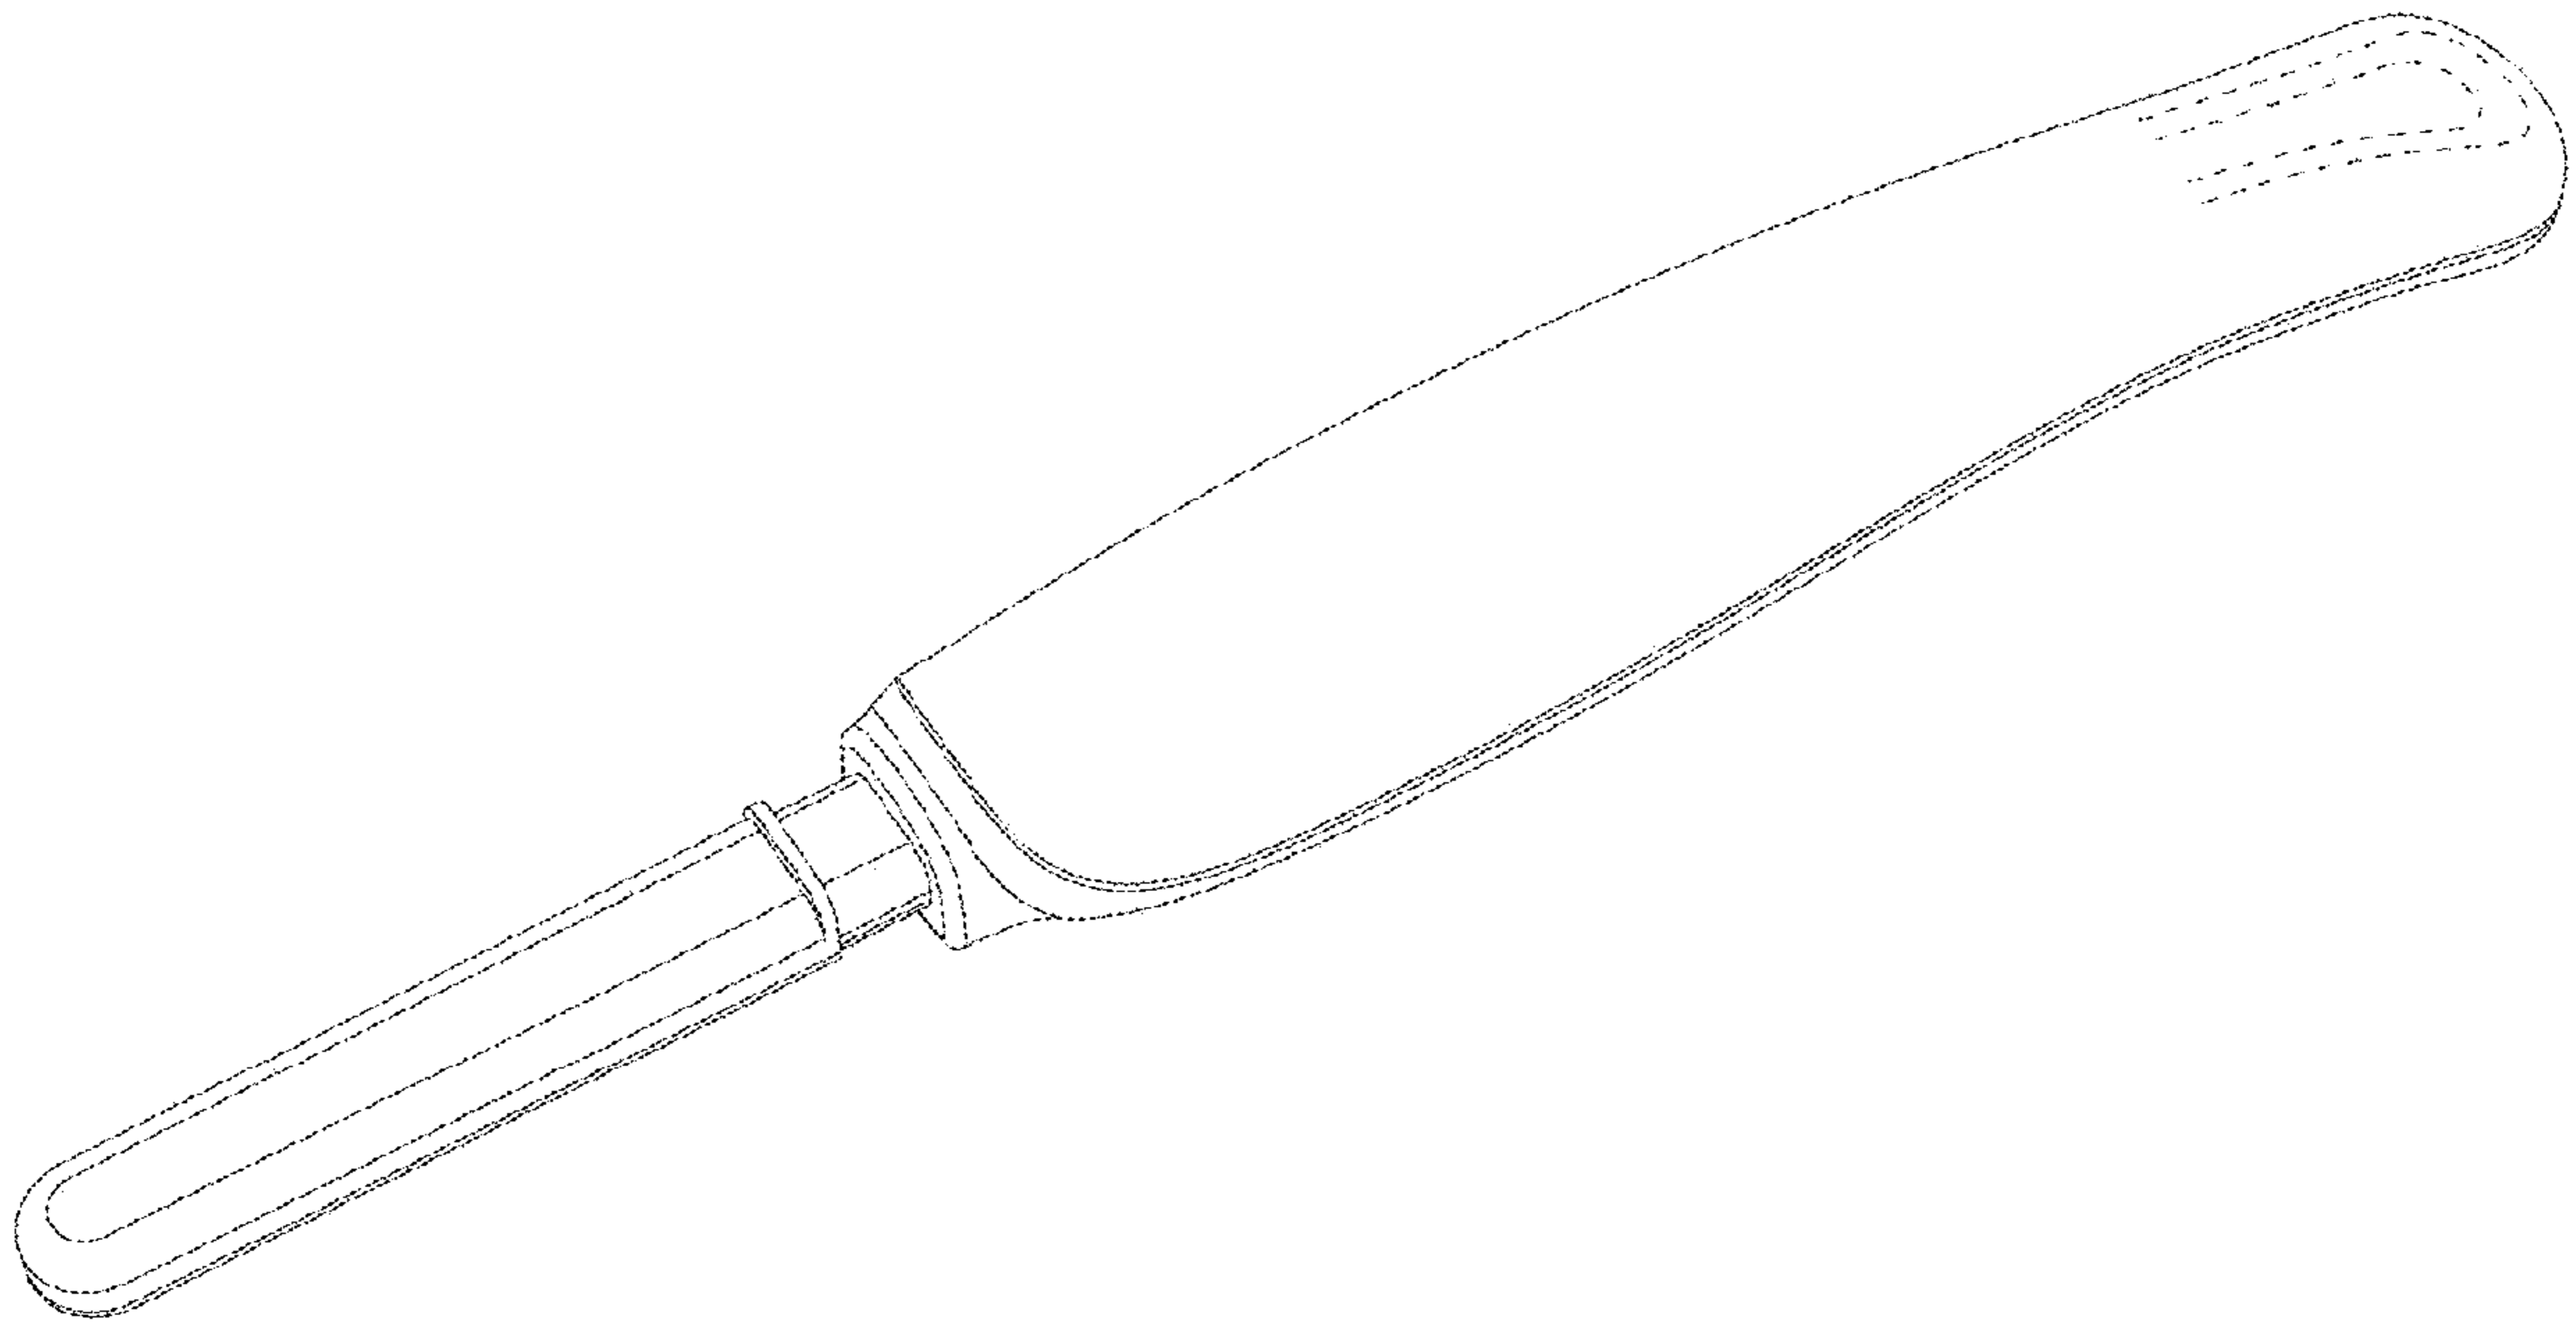


FIG. 9

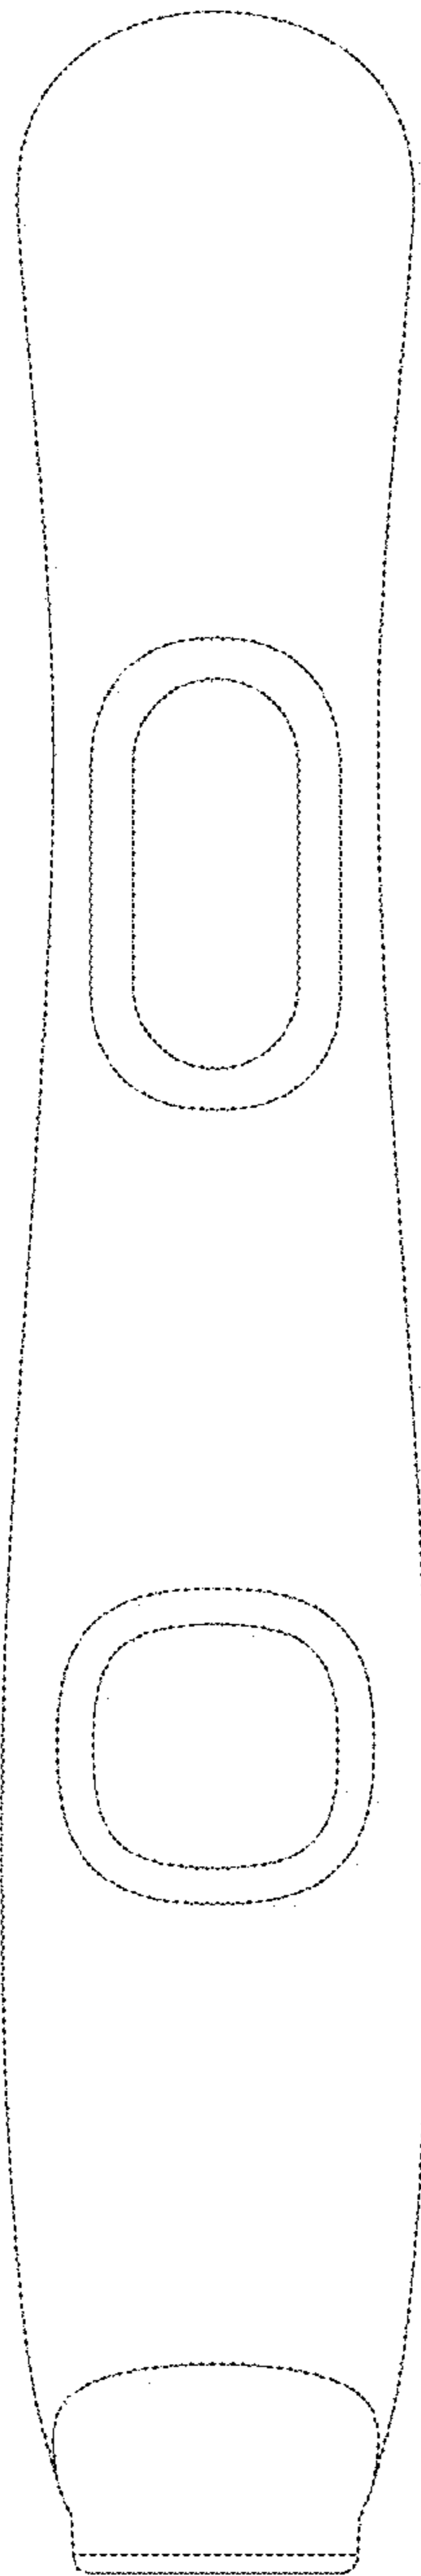


FIG. 10

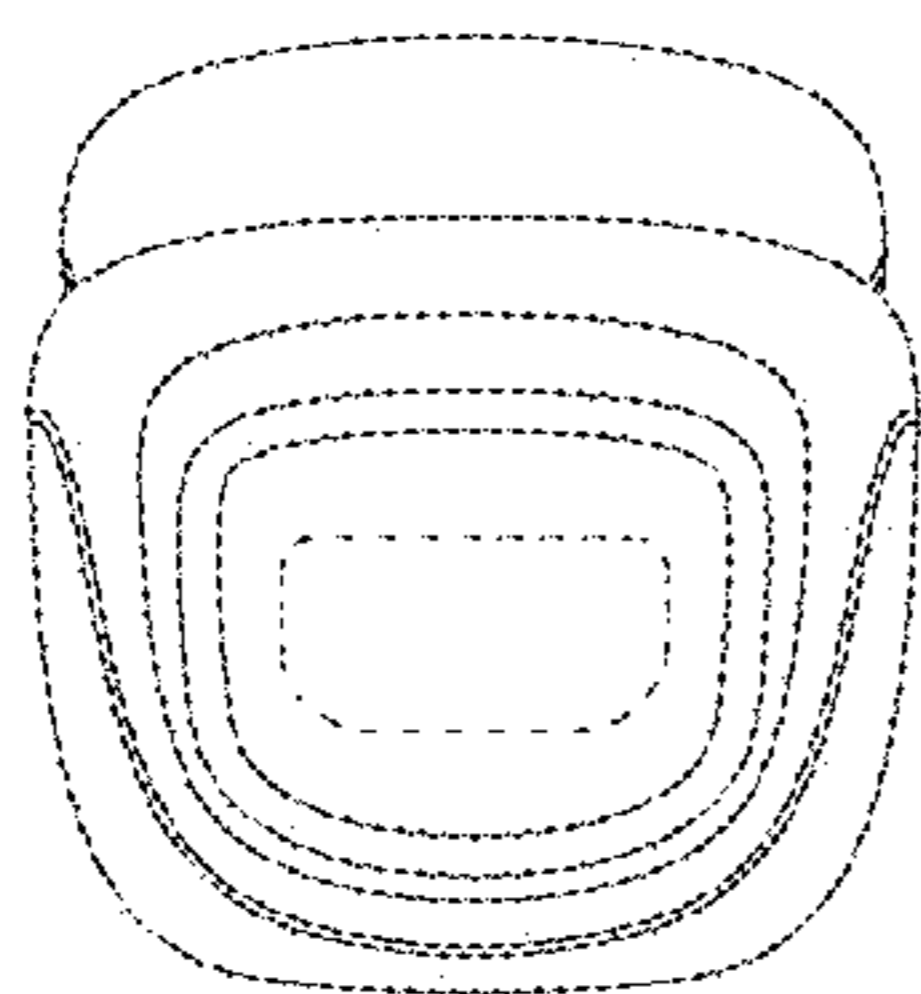


FIG. 11

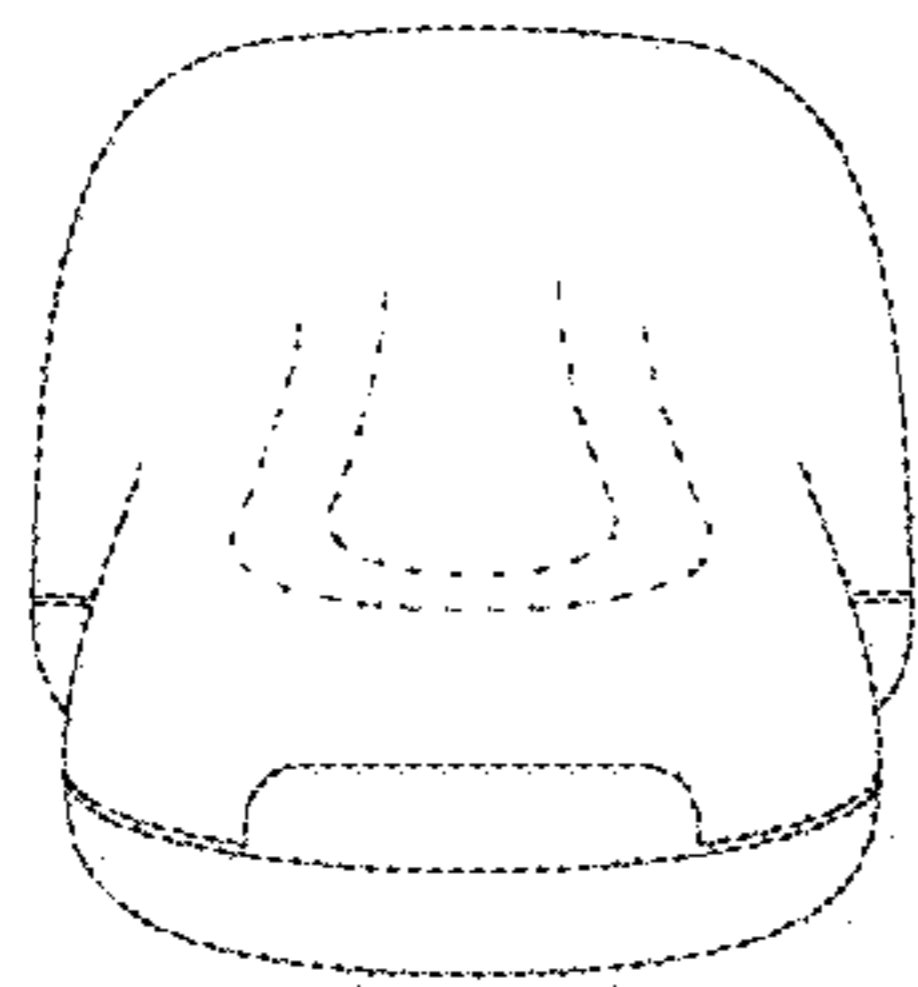


FIG. 12

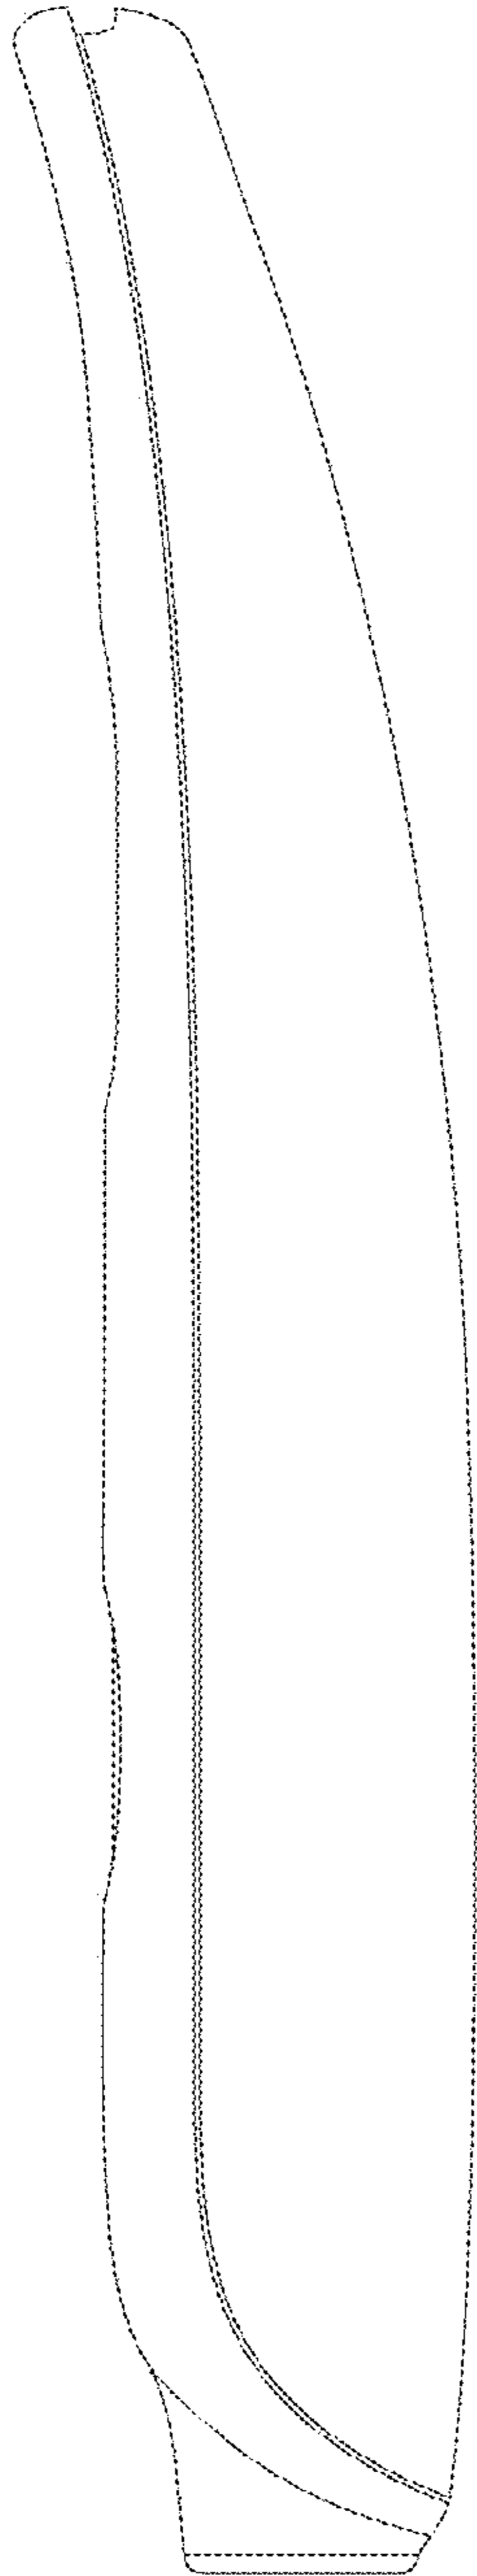


FIG. 13

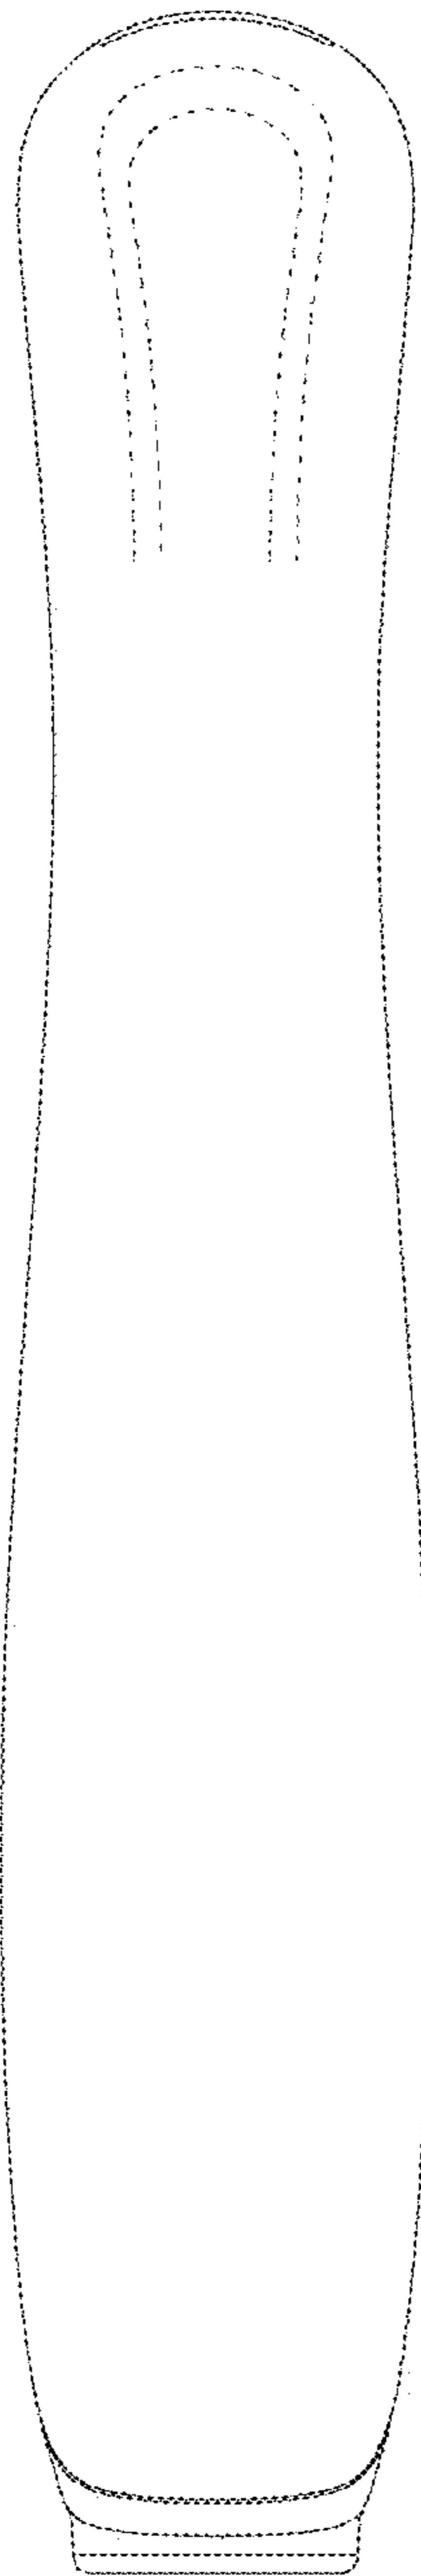


FIG. 14

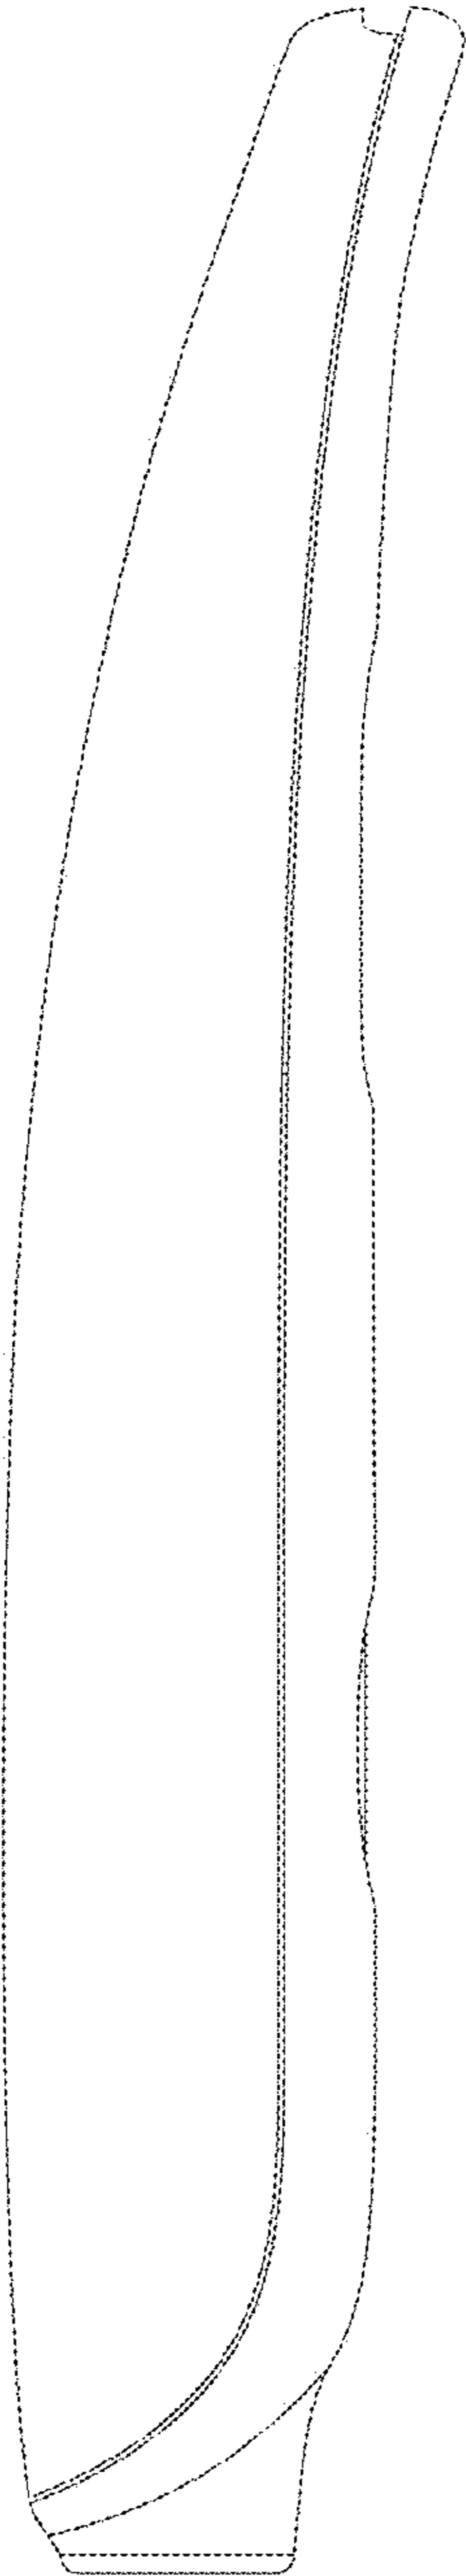




FIG. 15

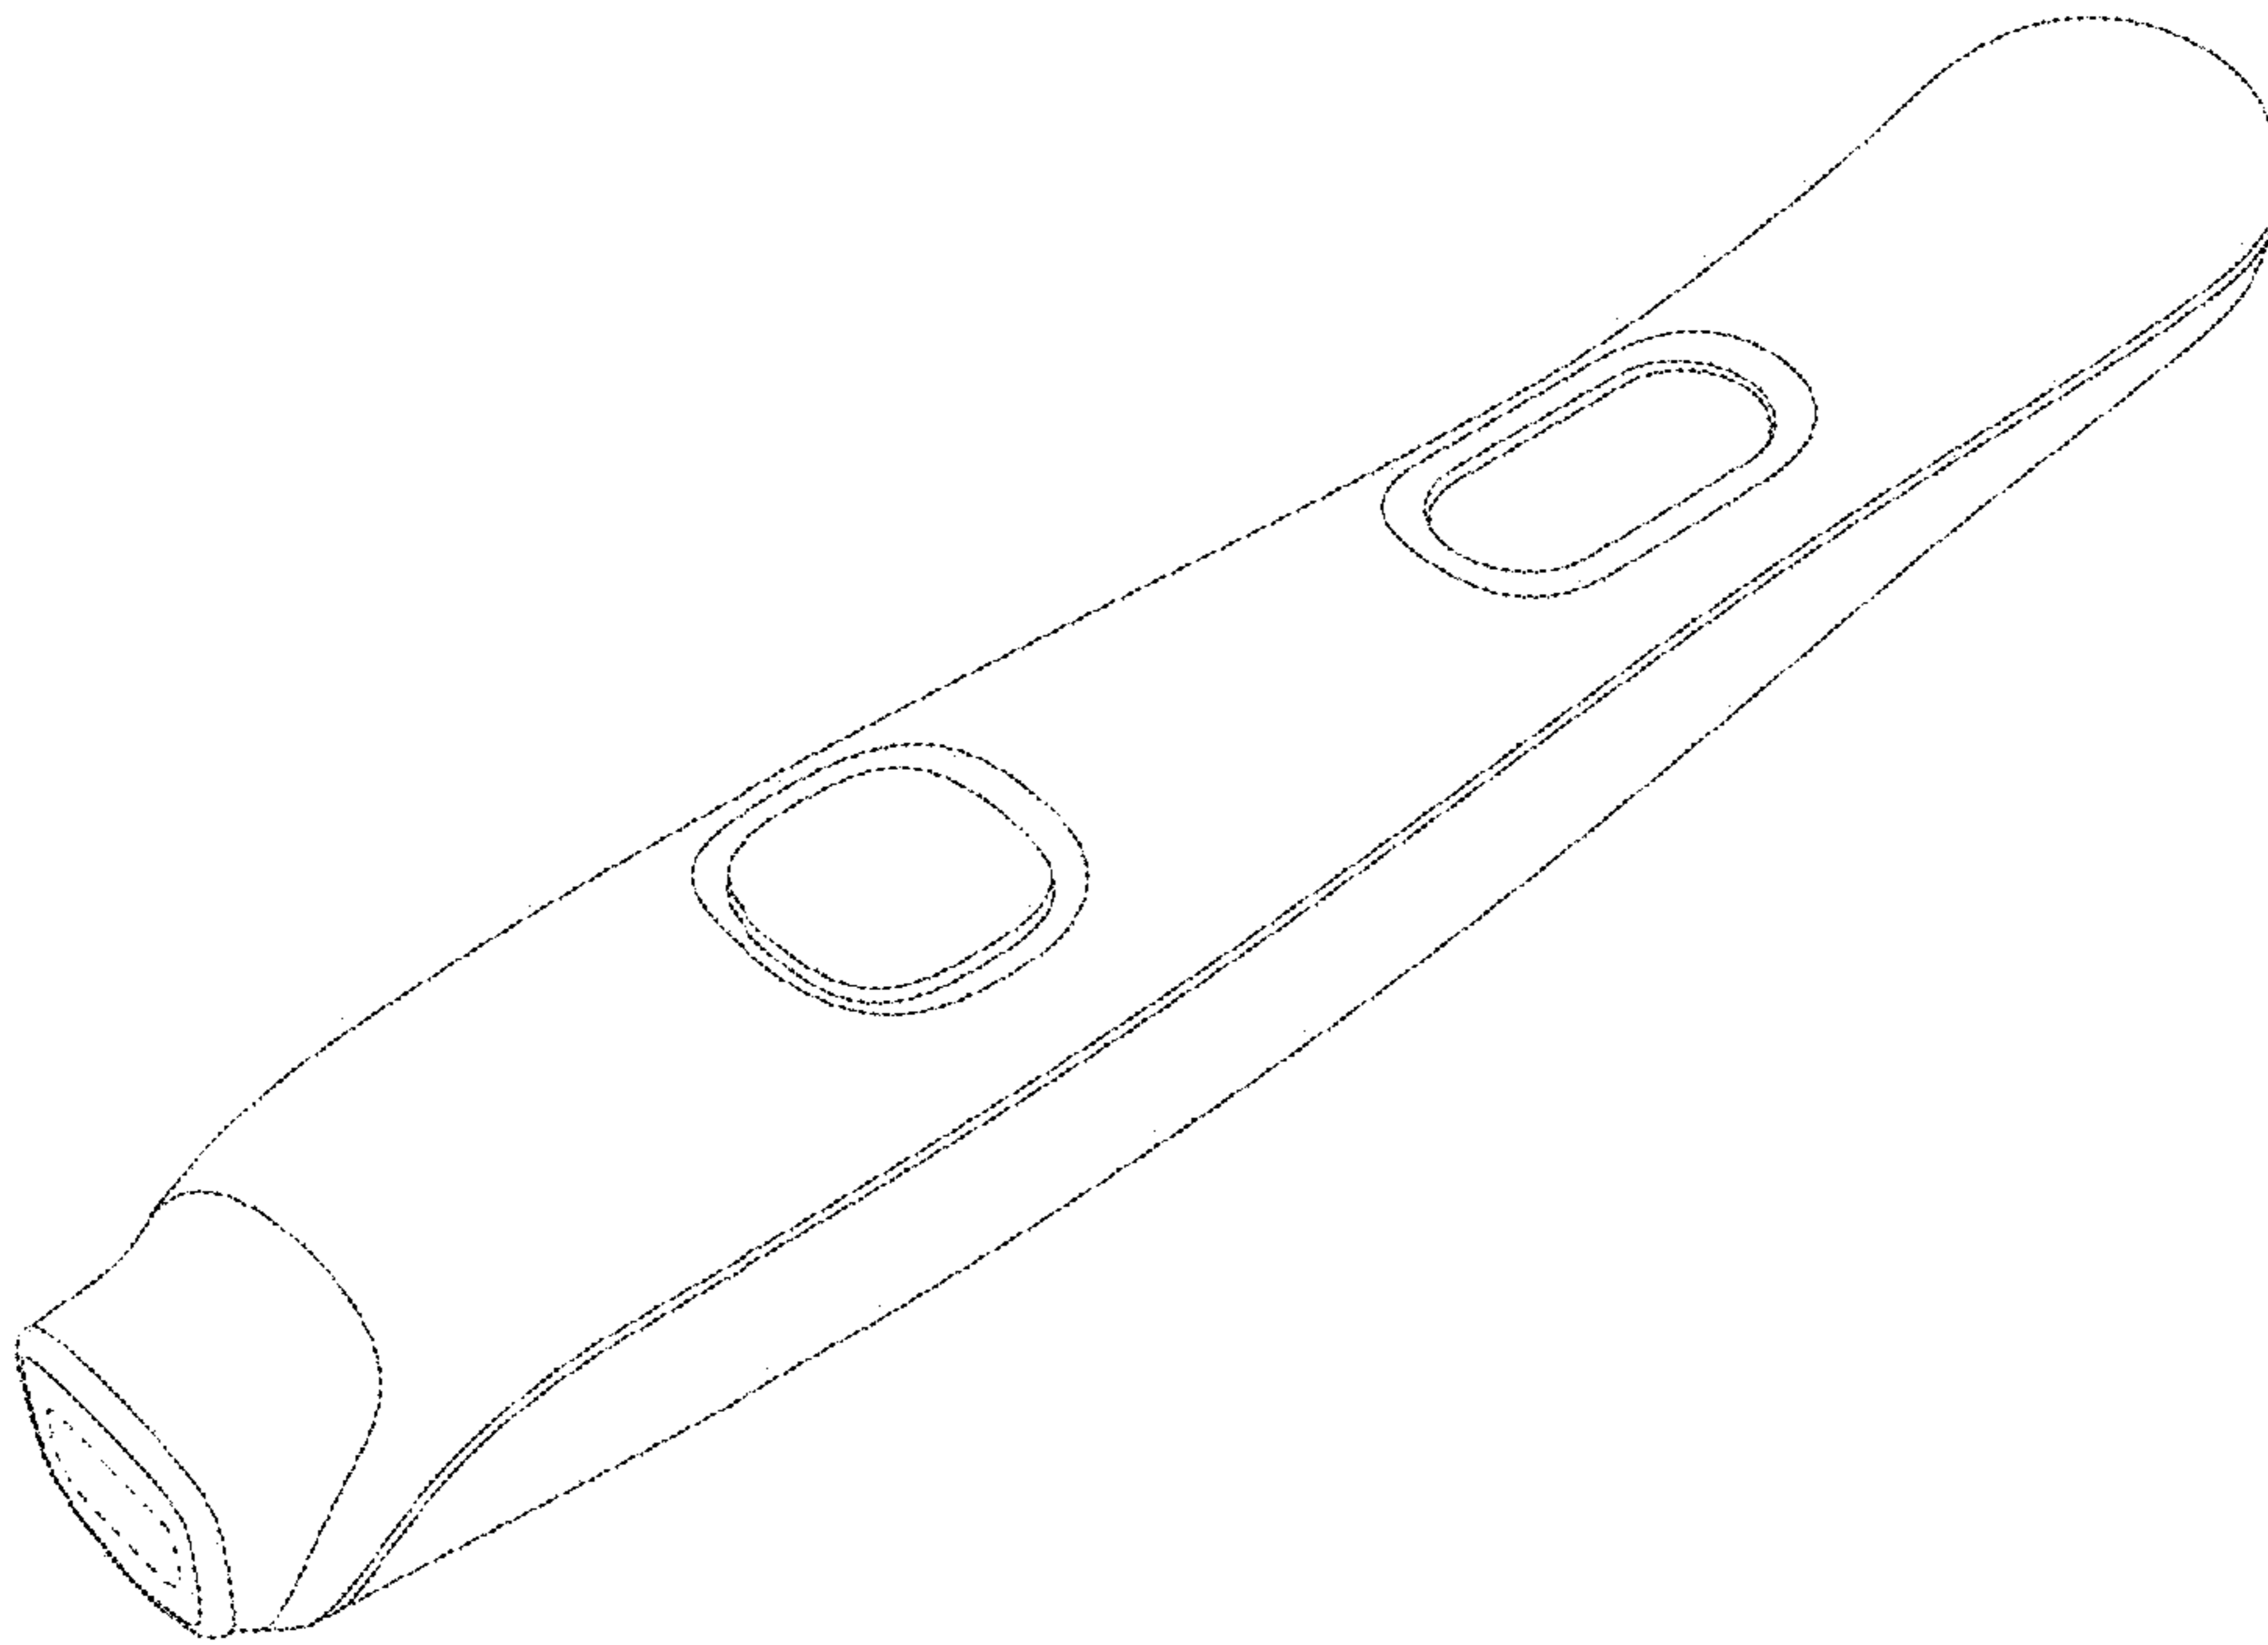


FIG. 16

