

US00D932632S

(12) **United States Design Patent**
Laing et al.

(10) **Patent No.:** **US D932,632 S**

(45) **Date of Patent:** **** Oct. 5, 2021**

(54) **UROFLOWMETER**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **ClearTrac Technologies, LLC**,
Elizabethton, TN (US)

CN 2221776 Y 3/1996
CN 105769223 A 7/2016

(Continued)

(72) Inventors: **Brent Laing**, Greenwood Village, CO (US); **John Green**, Elizabethton, TN (US); **Paul R. Johnson**, Boulder, CO (US); **Robert John Smith**, Louisville, CO (US); **Robert Edwin Schneider**, Erie, CO (US); **Magnus Hargis**, Hudson, CO (US); **Elise Geolat Edson**, Boulder, CO (US); **Elizabeth A. O'Brien**, Louisville, CO (US)

OTHER PUBLICATIONS

Drive Medical. "Drive Medical Folding Steel Bedside Commode, Grey." obtained Nov. 12, 2018 from <https://www.amazon.com/Drive-Medical-Folding-Bedside-Commode/dp/B001HP7AQE/ref=sr_1_3?s=industrial&ie=UTF8&qid=1539732631&sr=1-3&keywords=commode>, 8 pages.

(Continued)

(73) Assignee: **CLEARTRAC TECHNOLOGIES, LLC**, Elizabethton, TN (US)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(**) Term: **15 Years**

(57) **CLAIM**

The ornamental design for a uroflowmeter, as shown and described.

(21) Appl. No.: **29/656,567**

DESCRIPTION

(22) Filed: **Jul. 13, 2018**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**; D24/122

(58) **Field of Classification Search**
USPC D24/107, 121, 122, 129, 186, 216, 223,
D24/224, 231; D10/96, 102; D7/691
CPC A61B 10/007; A61B 5/205; A61B 5/207;
A61B 5/208
See application file for complete search history.

FIG. 1 shows a front perspective view of a uroflowmeter; FIG. 2 shows a rear perspective view of the uroflowmeter of FIG. 1; FIG. 3 shows a right elevation view of the uroflowmeter of FIG. 1; FIG. 4 shows a left elevation view of the uroflowmeter of FIG. 1; FIG. 5 shows a front elevation view of the uroflowmeter of FIG. 1; FIG. 6 shows a rear elevation view of the uroflowmeter of FIG. 1; FIG. 7 shows a top view of the piece of the uroflowmeter of FIG. 1; and, FIG. 8 shows a bottom view of the uroflowmeter of FIG. 1. The broken lines illustrate portions of the uroflowmeter that form no part of the claimed design; the broken lines and the unshaded surfaces form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

2,648,981 A 8/1953 Drake, Jr.
3,172,130 A 3/1965 Lange
3,219,276 A 11/1965 Norris
3,859,854 A 1/1975 Dye et al.

(Continued)

1 Claim, 4 Drawing Sheets

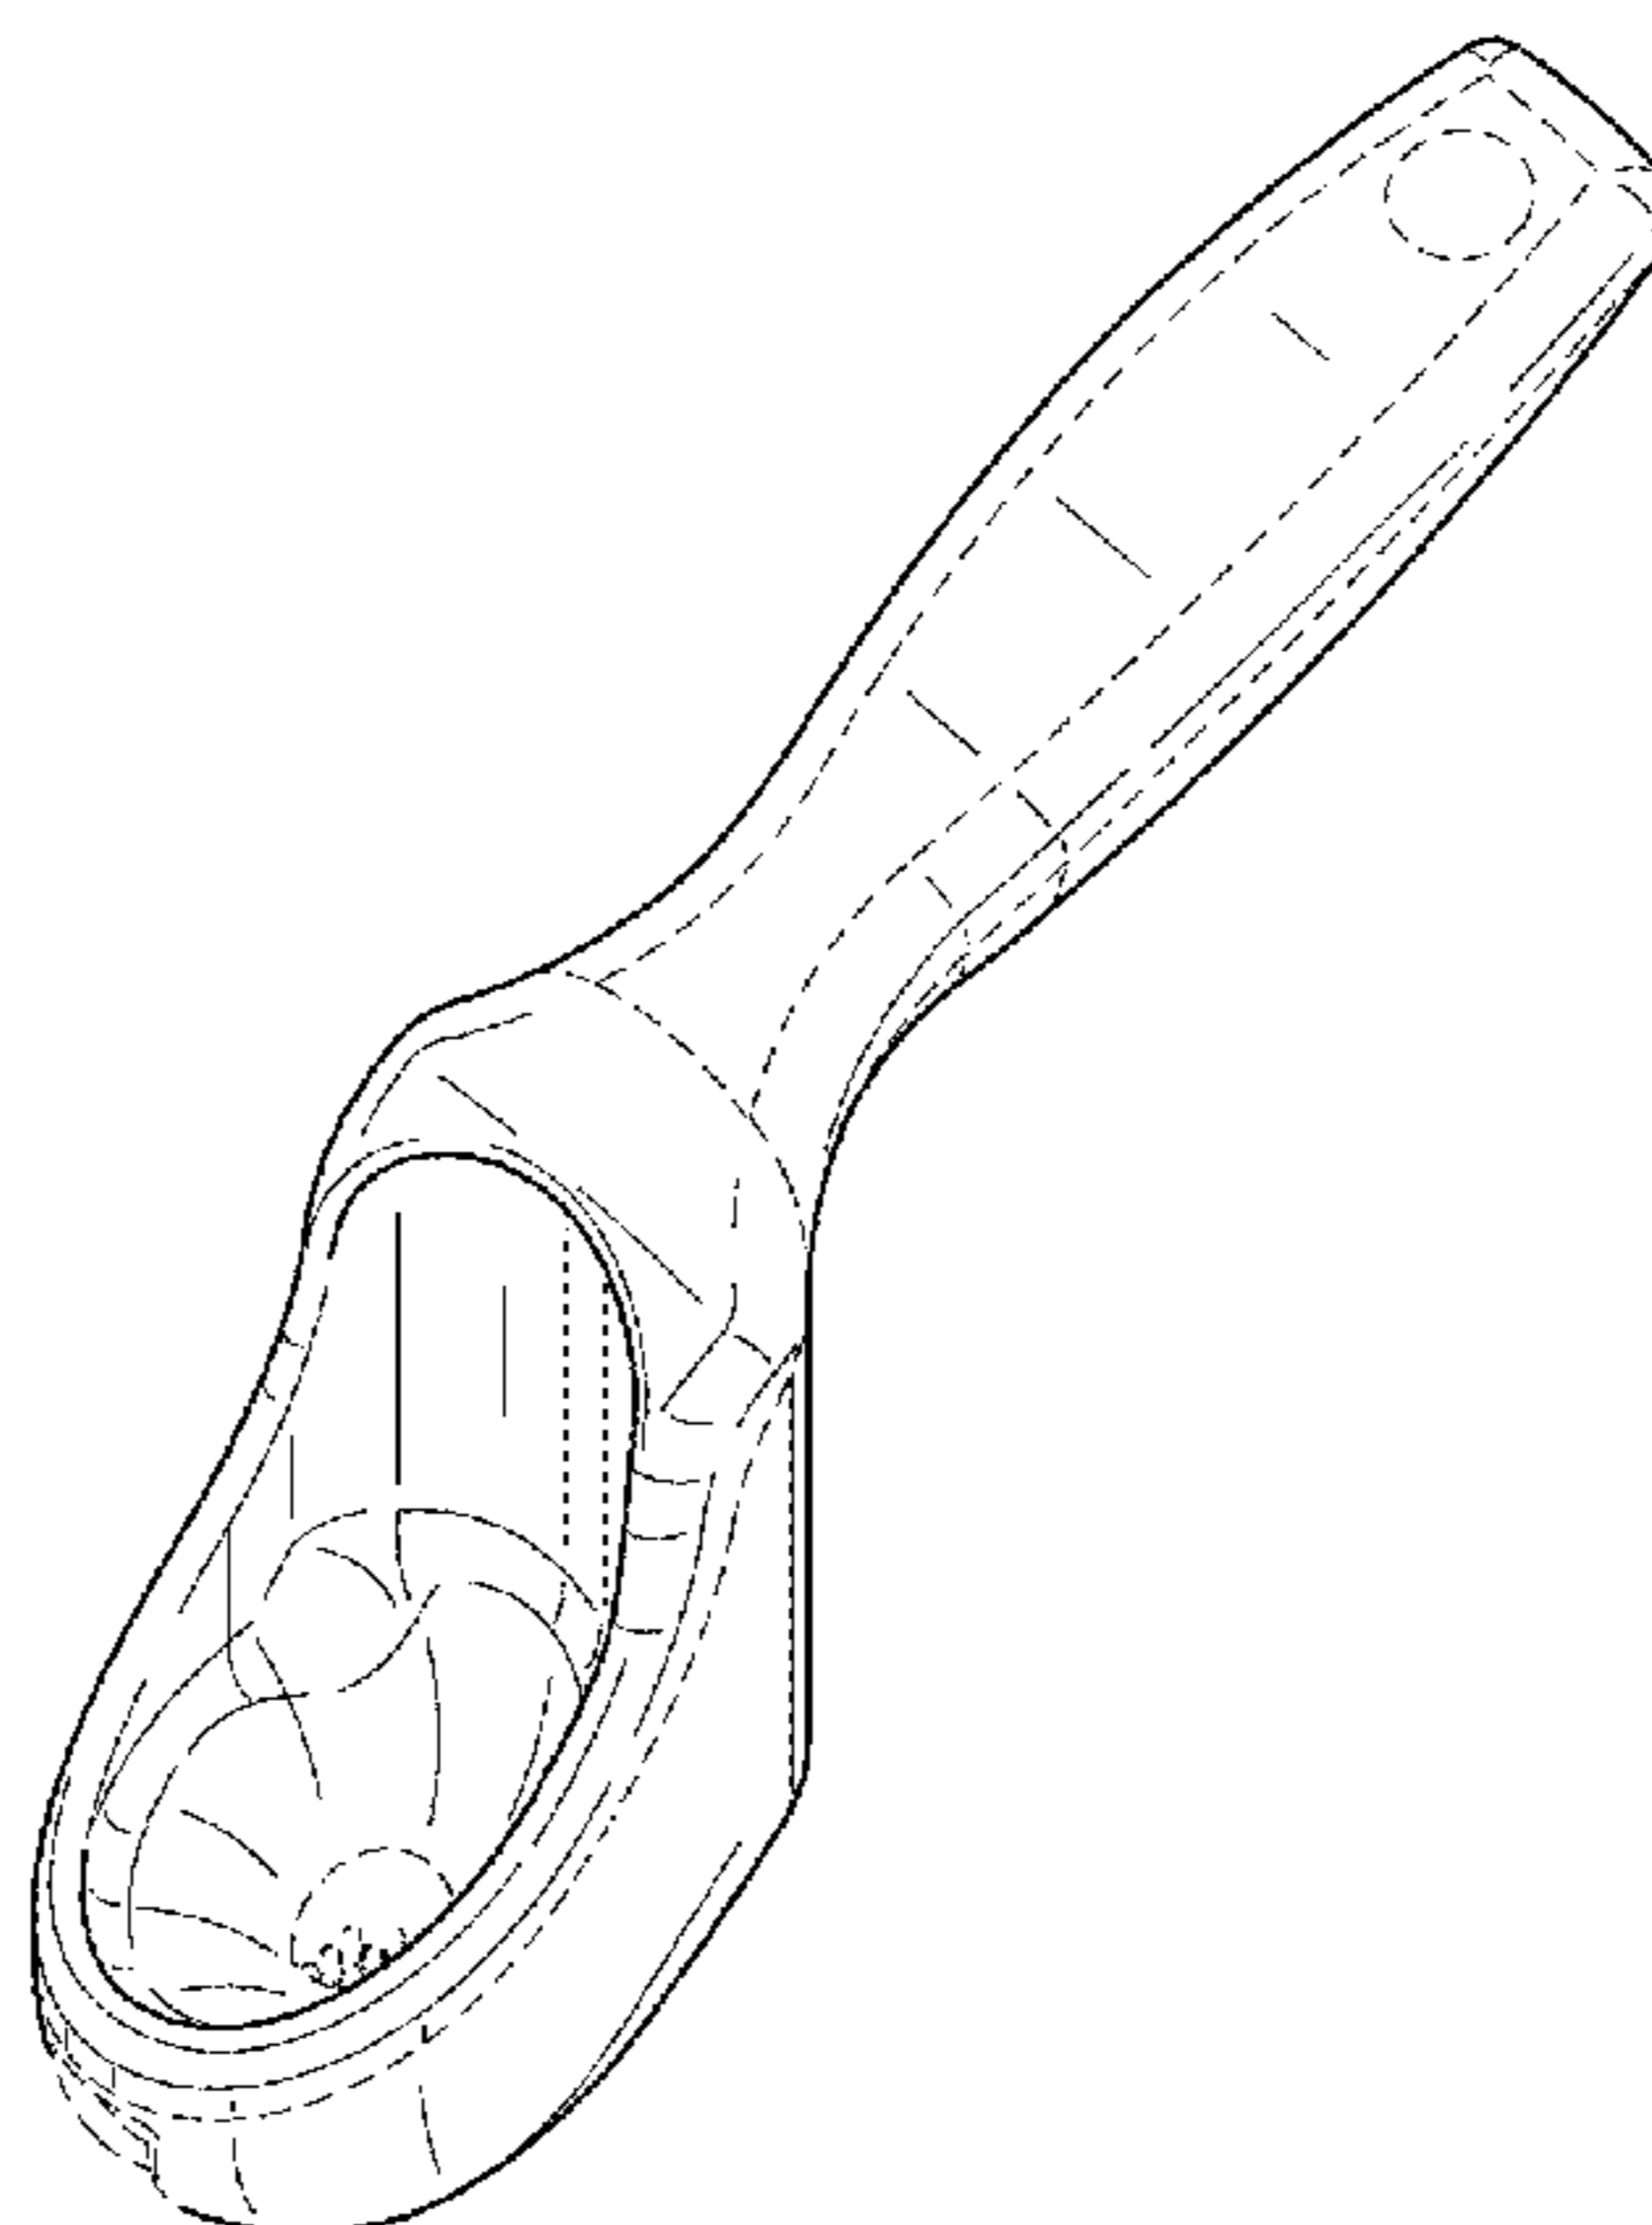

(56)

References Cited

U.S. PATENT DOCUMENTS

3,871,230 A 3/1975 Dye et al.
 3,884,072 A 5/1975 Cheng
 3,929,412 A 12/1975 Villari
 3,931,972 A 1/1976 Fabian
 4,051,431 A 9/1977 Wurster
 4,085,616 A 4/1978 Patel et al.
 4,131,016 A 12/1978 Layton
 4,238,448 A 12/1980 Layton et al.
 4,343,316 A 8/1982 Jespersen
 4,554,687 A 11/1985 Carter et al.
 4,619,273 A 10/1986 Iosif
 D296,360 S * 6/1988 Oelberg D24/186
 4,832,046 A 5/1989 Parrish
 4,891,993 A 1/1990 Barker
 5,046,510 A 9/1991 Ams et al.
 5,062,304 A 11/1991 Van et al.
 5,176,148 A 1/1993 Wiest et al.
 D340,768 S 10/1993 Jabour
 5,377,101 A 12/1994 Rollema
 5,422,076 A 6/1995 Jones
 D378,129 S * 2/1997 Wexler D24/122
 D422,851 S 4/2000 Joergensen
 D425,365 S 5/2000 Chien
 D436,801 S 1/2001 Wonderley
 6,398,742 B1 6/2002 Kim
 D460,328 S 7/2002 Groote et al.
 D461,105 S 8/2002 Law
 6,651,259 B1 11/2003 Hartman et al.
 D492,995 S 7/2004 Rue et al.
 D494,279 S * 8/2004 Cogan D24/216
 6,889,563 B2 5/2005 Tomita et al.
 6,904,809 B1 6/2005 Aundal
 6,931,943 B1 8/2005 Aundal
 D545,621 S 7/2007 Hood
 D551,032 S 9/2007 Lion et al.
 D552,431 S 10/2007 Chou
 D572,089 S 7/2008 Teys et al.
 7,416,542 B2 8/2008 Aundal
 D598,251 S 8/2009 Ikoma et al.
 7,606,617 B2 10/2009 Wariar
 7,739,907 B2 6/2010 Boiarski
 D619,246 S 7/2010 Hazeres
 7,819,020 B2 10/2010 Jacobi et al.
 7,892,217 B2 2/2011 Boiarski
 8,141,420 B2 3/2012 Hirao
 D659,558 S 5/2012 Johnson et al.
 8,231,552 B2 7/2012 Shahar et al.
 8,424,376 B2 4/2013 Boiarski
 D681,392 S 5/2013 Dichraff et al.
 D688,370 S * 8/2013 Desai D24/122
 8,500,705 B2 8/2013 Kim
 8,544,341 B2 10/2013 Grumbles et al.
 D709,185 S * 7/2014 Queiroli D24/122
 8,813,551 B2 8/2014 Boiarski
 9,021,878 B2 5/2015 Grinstein et al.
 D736,043 S 8/2015 Lee et al.
 D770,613 S * 11/2016 Roberts D24/122
 9,642,737 B2 5/2017 Seres et al.
 9,775,556 B2 10/2017 Dimino et al.
 D823,652 S 7/2018 Dooley et al.
 10,034,659 B2 7/2018 Siller Gonzalez et al.
 D842,985 S * 3/2019 Heckerman D24/122
 D862,999 S 10/2019 Riedel et al.
 D871,137 S 12/2019 Brouillac
 D876,183 S 2/2020 Yee
 D889,918 S 7/2020 Hubert
 D893,947 S 8/2020 Pulk
 2005/0261605 A1 11/2005 Shemer et al.
 2008/0312556 A1 12/2008 Dijkman
 2008/0312557 A1 12/2008 Cho et al.
 2011/0000309 A1 1/2011 Griffiths et al.
 2012/0109008 A1 5/2012 Charlez et al.

2016/0029942 A1 2/2016 Paulsen et al.
 2016/0051176 A1 2/2016 Ramos et al.
 2017/0020433 A1 1/2017 Hotaling et al.
 2017/0086728 A1 3/2017 Hidas
 2017/0105670 A1 4/2017 Holt et al.
 2017/0135622 A1 5/2017 Shimokawa et al.
 2017/0307423 A1 10/2017 Pahwa et al.
 2018/0085008 A1 3/2018 Hall et al.
 2018/0303465 A1 * 10/2018 Lyon B01D 29/13
 2019/0365306 A1 12/2019 Laing et al.
 2019/0365307 A1 * 12/2019 Laing G06F 9/542
 2019/0365308 A1 * 12/2019 Laing A61B 5/208

FOREIGN PATENT DOCUMENTS

CN 106037766 A 10/2016
 DE 3007855 A1 9/1981
 DE 19733630 A1 2/1999
 DE 102014008760 A1 1/2015
 EM 005840378-0001 3/2019
 EM 005840378-0002 3/2019
 EM 005840378-0003 3/2019
 EM 006821633-0001 10/2019
 EM 006821633-0002 10/2019
 EM 006821633-0003 10/2019
 EM 006821633-0004 10/2019
 EP 2303124 B1 8/2012
 EP 2741671 B1 1/2016
 EP 2716219 B1 3/2017
 EP 2564778 B1 4/2018
 JP 3729732 B2 10/2005
 KR 20110030826 A 3/2011
 RU 2034516 C1 5/1995
 RU 2071724 C1 1/1997
 RU 2643110 C1 1/2018
 WO 9925246 A1 5/1999
 WO 2009035599 A1 3/2009
 WO 2009142508 A1 11/2009
 WO 2014141234 A1 9/2014
 WO 2016056571 A1 4/2016
 WO 2017036952 A1 3/2017
 WO 2017149272 A1 9/2017
 WO 2018036664 A1 3/2018
 WO 2018051244 A1 3/2018

OTHER PUBLICATIONS

Specimen Collection Unit. "Specimen Collection Unit, QTY of 1." obtained Nov. 12, 2018 from <<https://www.amazon.com/Specimen-Collection-Unit-QTY-1/dp/B002ZUCVP0#feature-bullets-btf>>, 6 pages.
 Bestmedical. "Uroflowmeter: Portable & wireless." obtained Nov. 12, 2018 from <<http://www.best-medical.nl/uroflowmeter/>>, 6 pages.
 MDTI. "Uflow meter Male Urine Peak Flow Device." obtained Nov. 12, 2018 from <<https://www.mdti.co.uk/uflow->>, 2 pages.
 Albyn Medical Product Detail. "SmartFlow: SmartFlow brings together high specifications and ease-of-use." Obtained Nov. 12, 2018 from <<http://www.albynmedical.com/products/ProductDetail.aspx?ID=8>>, 2 pages.
 Laborie. "Uroflowmetry: Uroflowmeters designed for practical, everyday studies, available in a range of configurations to meet different demands." obtained Nov. 12, 2018 from <<https://www.laborie.com/category/urology-urogynecology/uroflowmetry/>>, 6 pages.
 Minze Health. "Homeflow." obtained Nov. 12, 2018 from <<https://minzehealth.com/products/homeflow/>>, 8 pages.
 Chun, Kwonsoo et al. "Noninvasive Medical Tools for Evaluating Voiding Pattern in Real Life." International Neurology Journal, 2017, S10-16.
 PCT, "International Search Report and Written Opinion", Application No. PCT/US2019/021292, dated May 8, 2019, 11 pages.
 PCT, "International Search Report and Written Opinion", Application No. PCT/US19/21421, May 31, 2019, 16 pages.

* cited by examiner

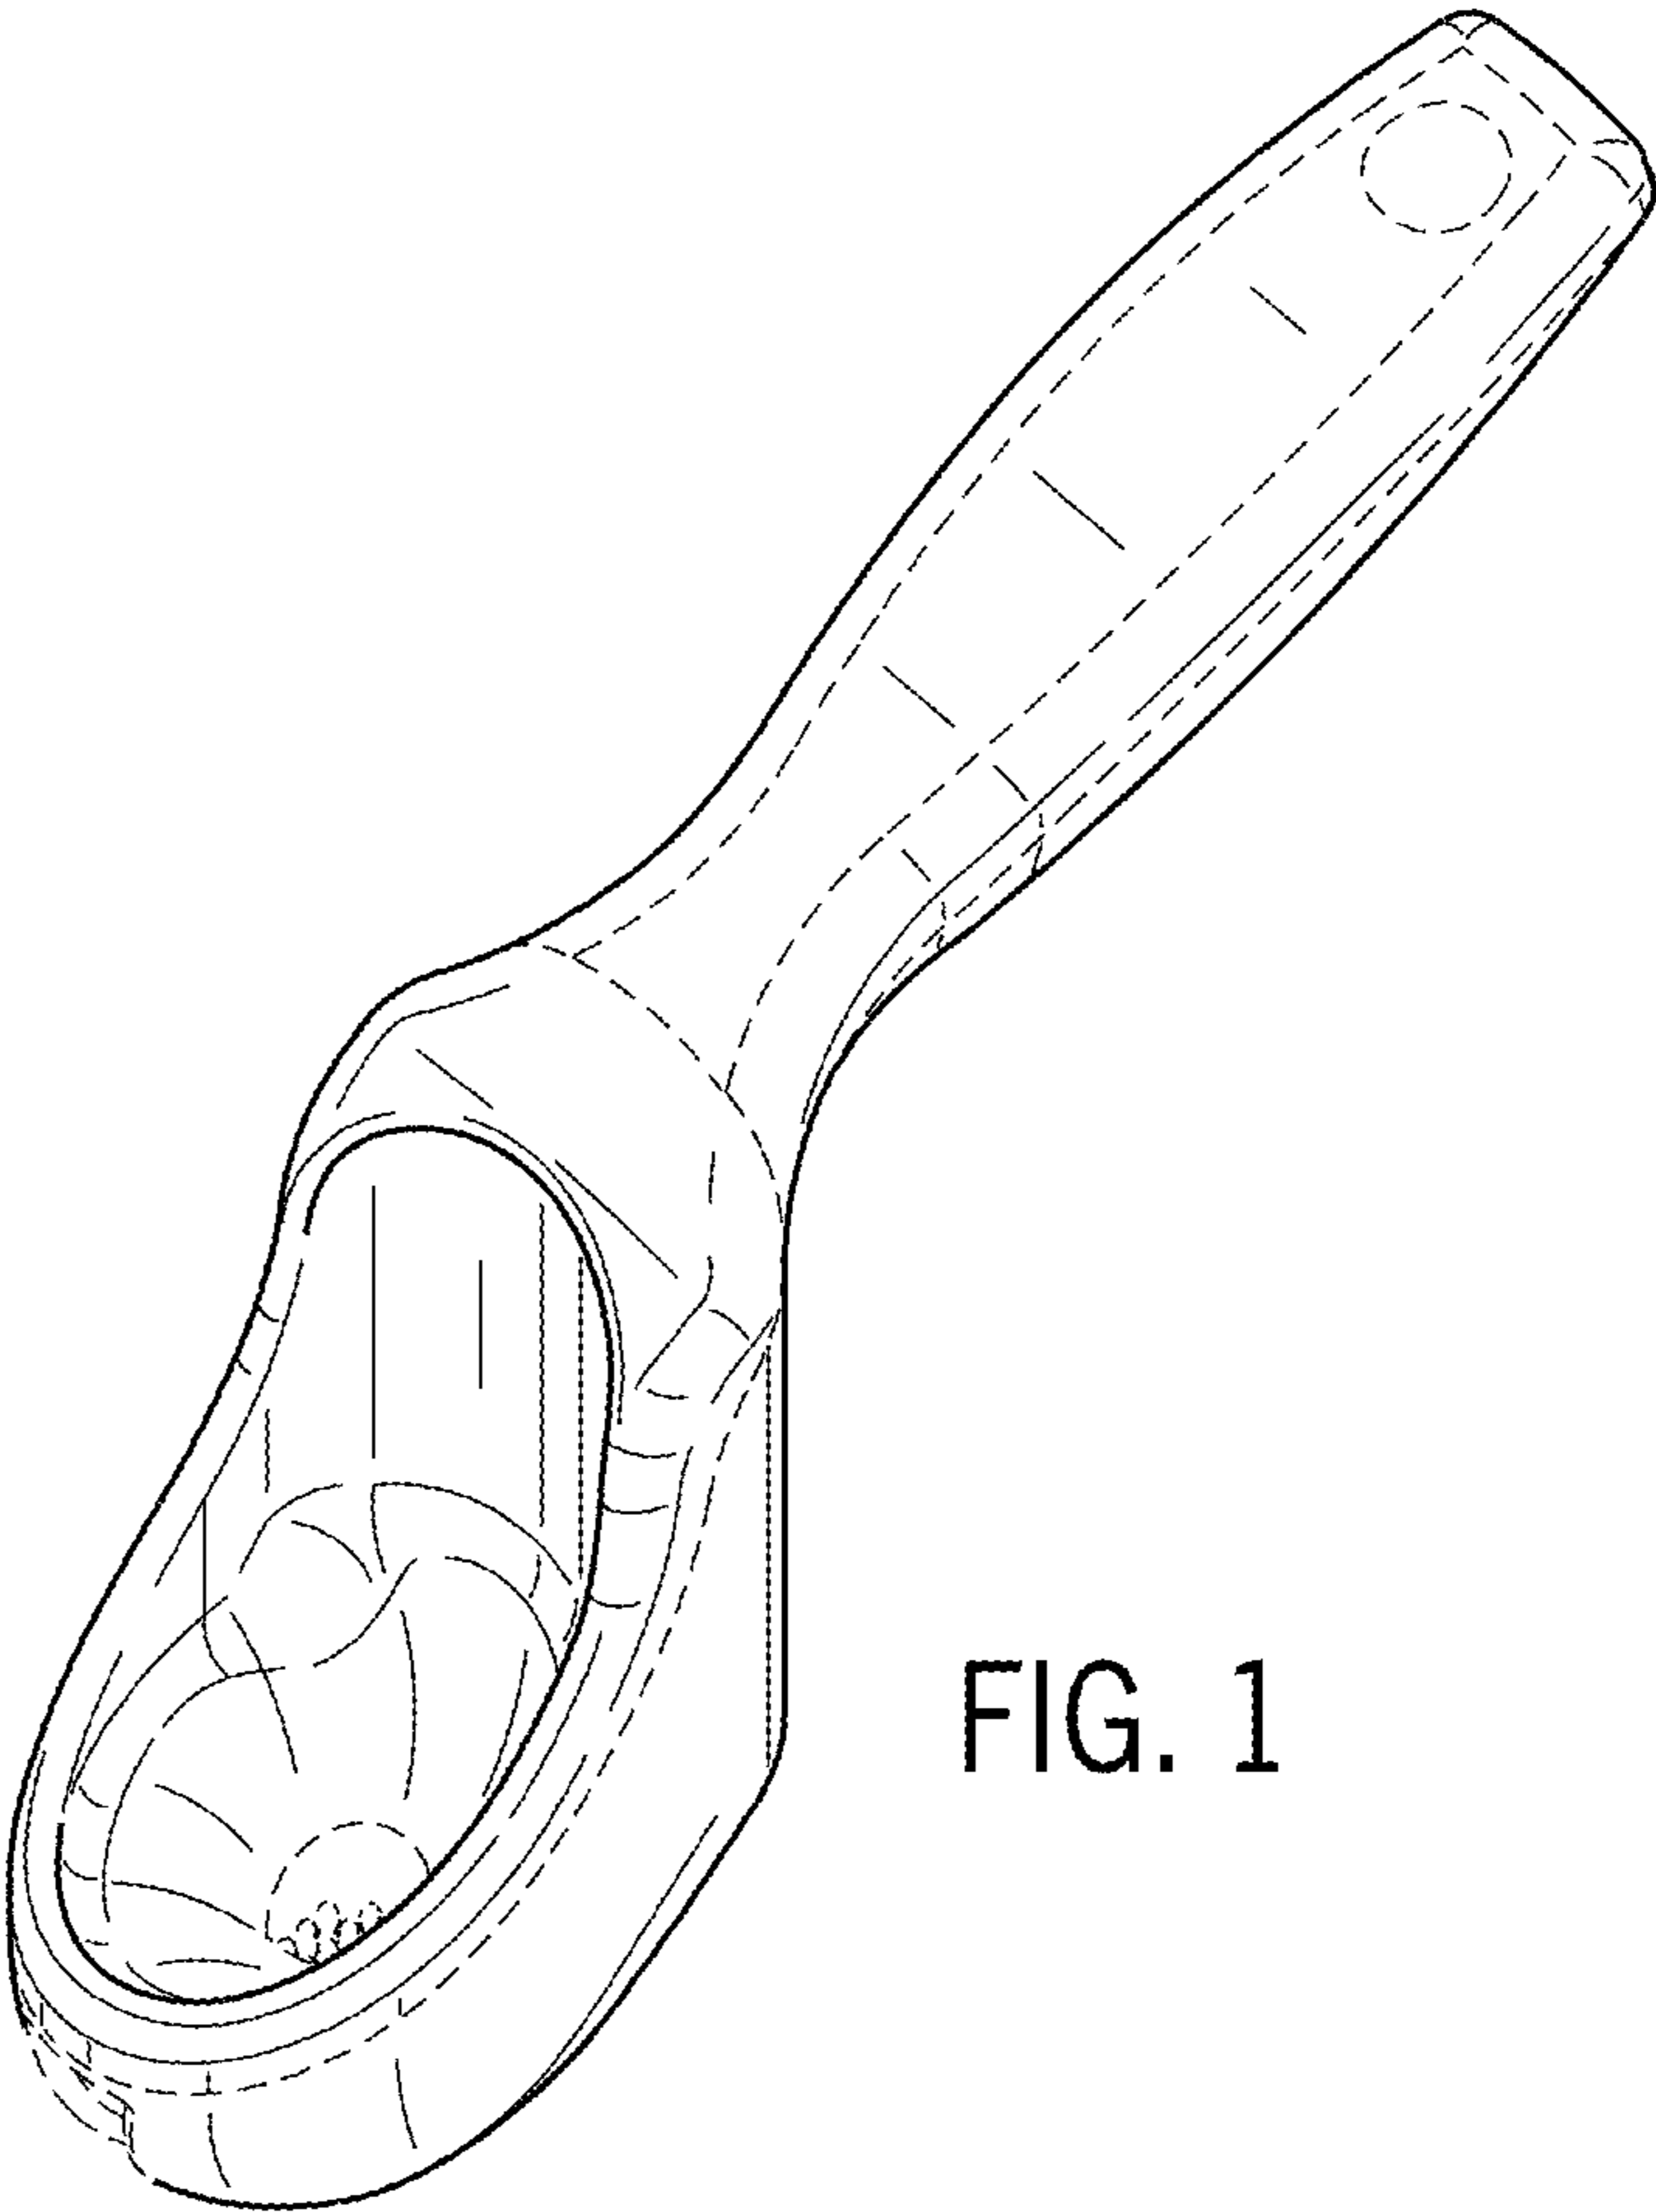


FIG. 1

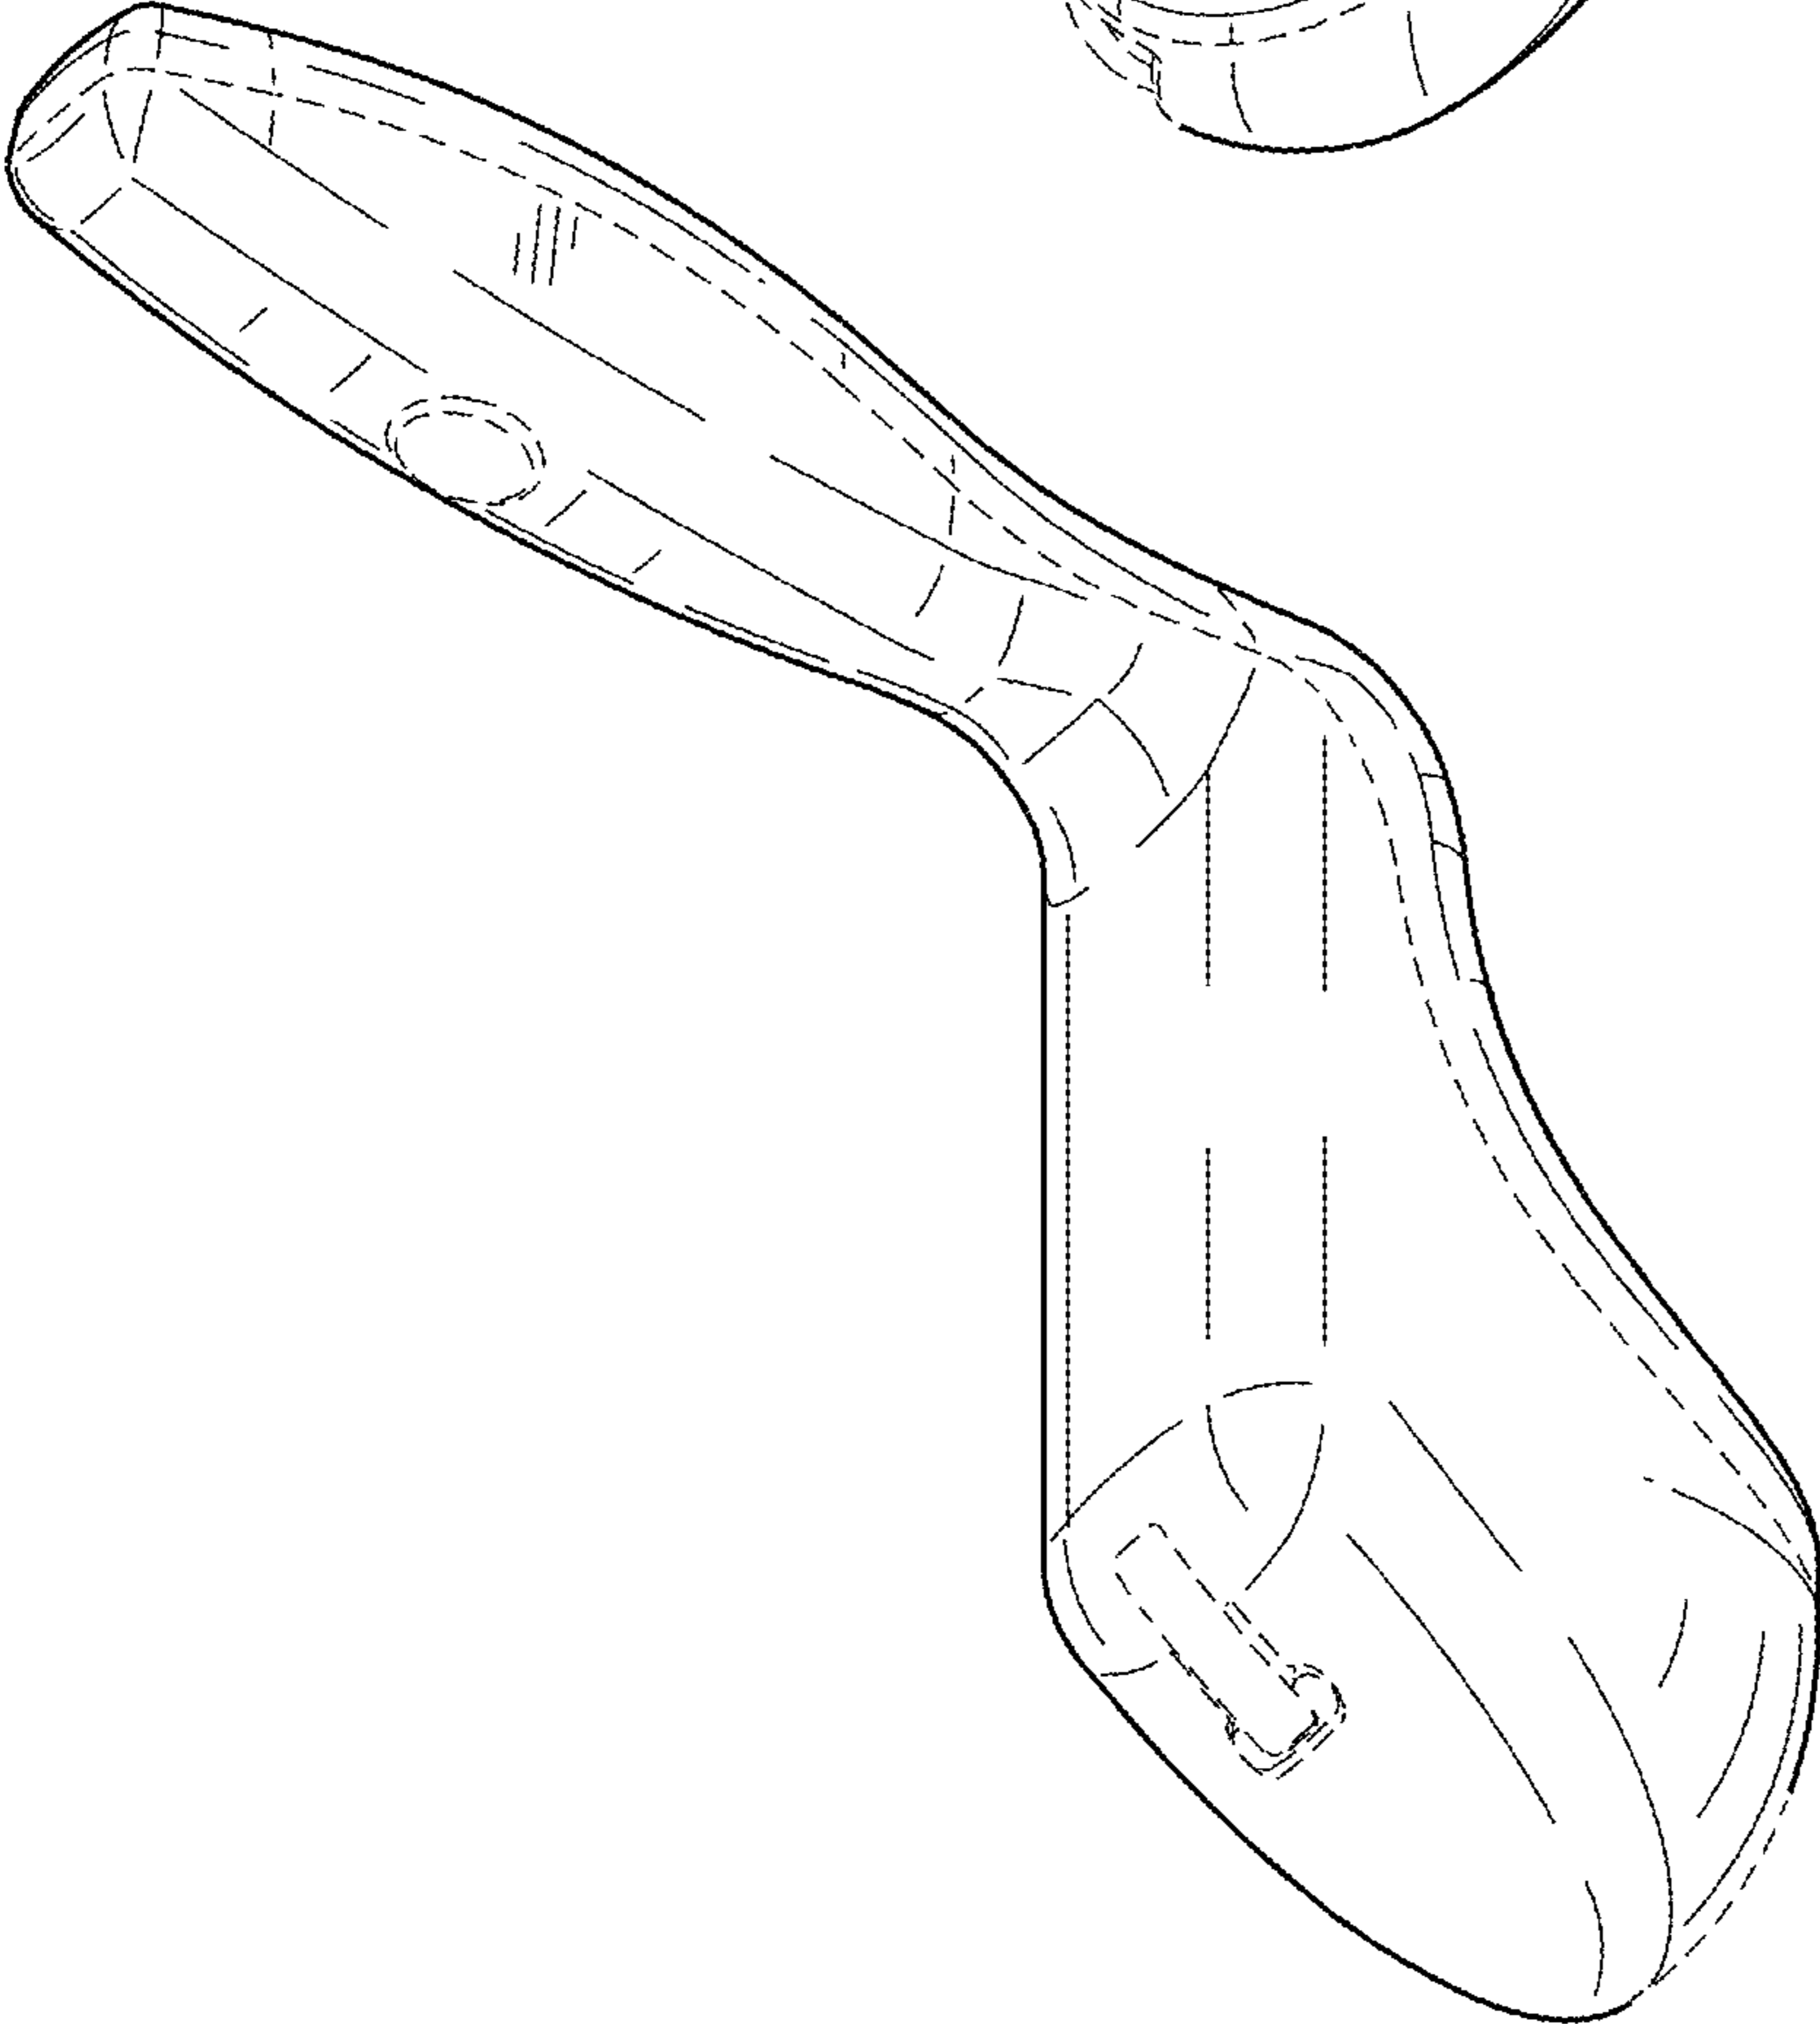


FIG. 2

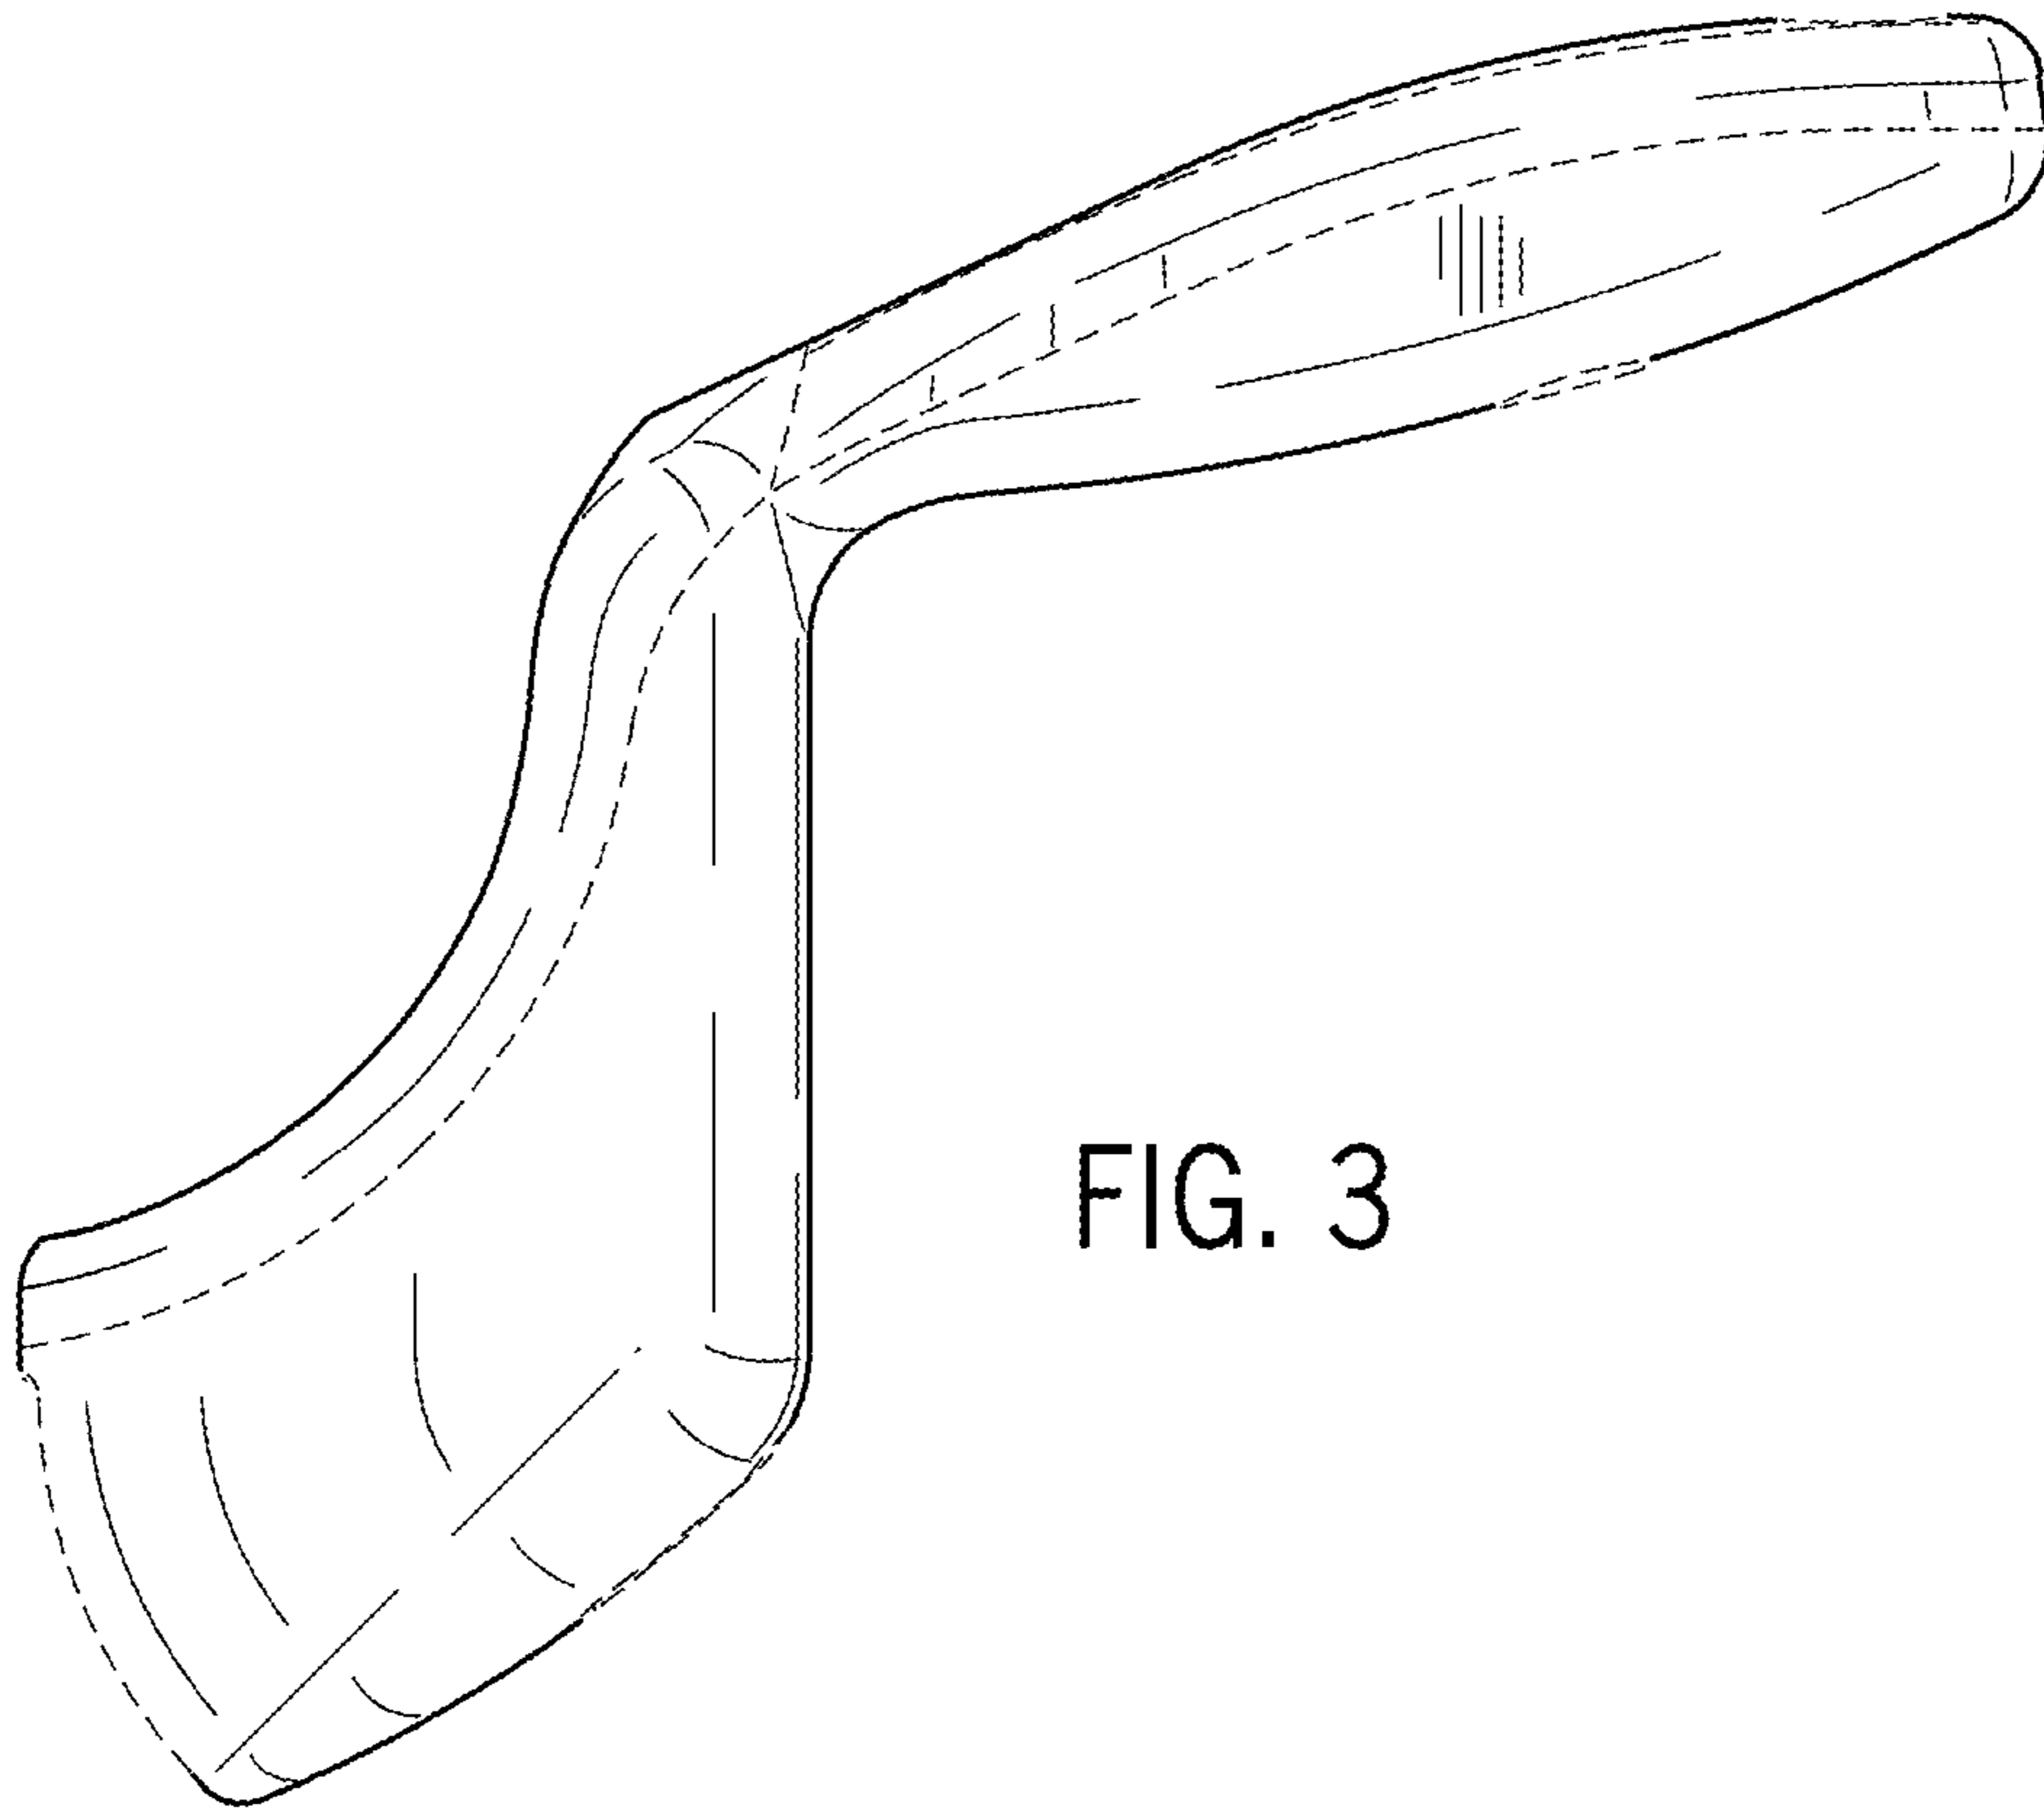


FIG. 3

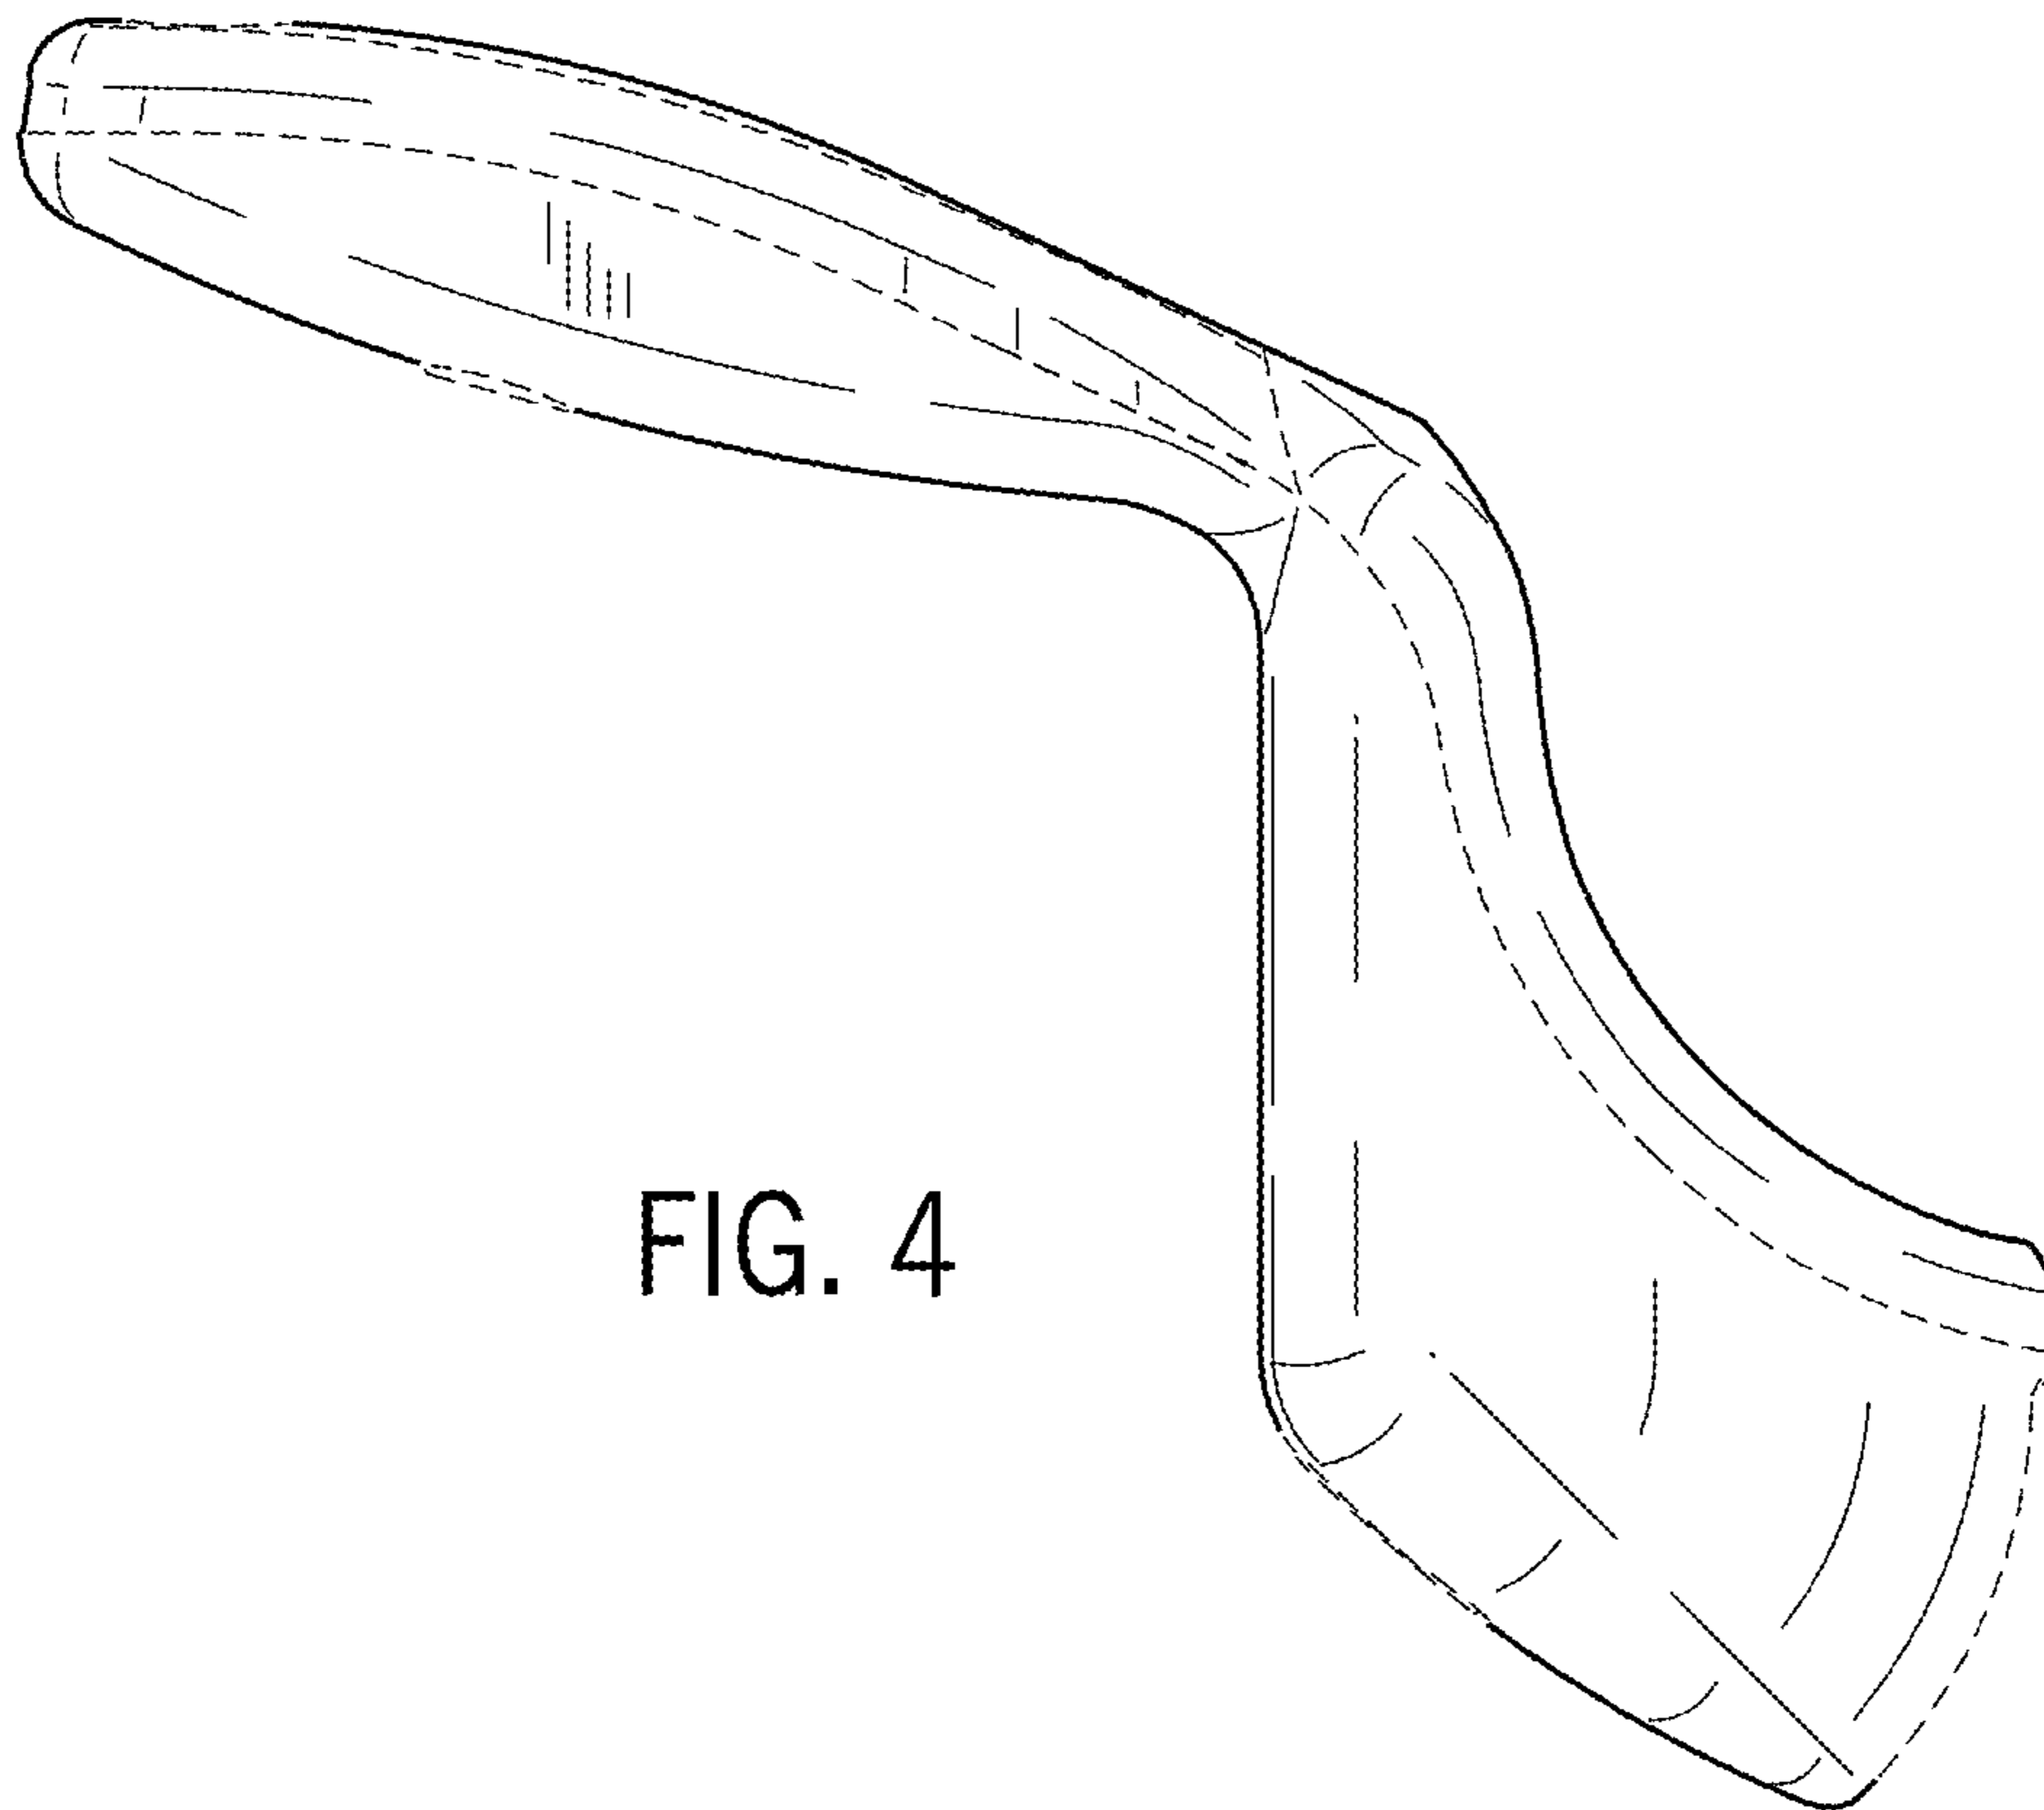


FIG. 4

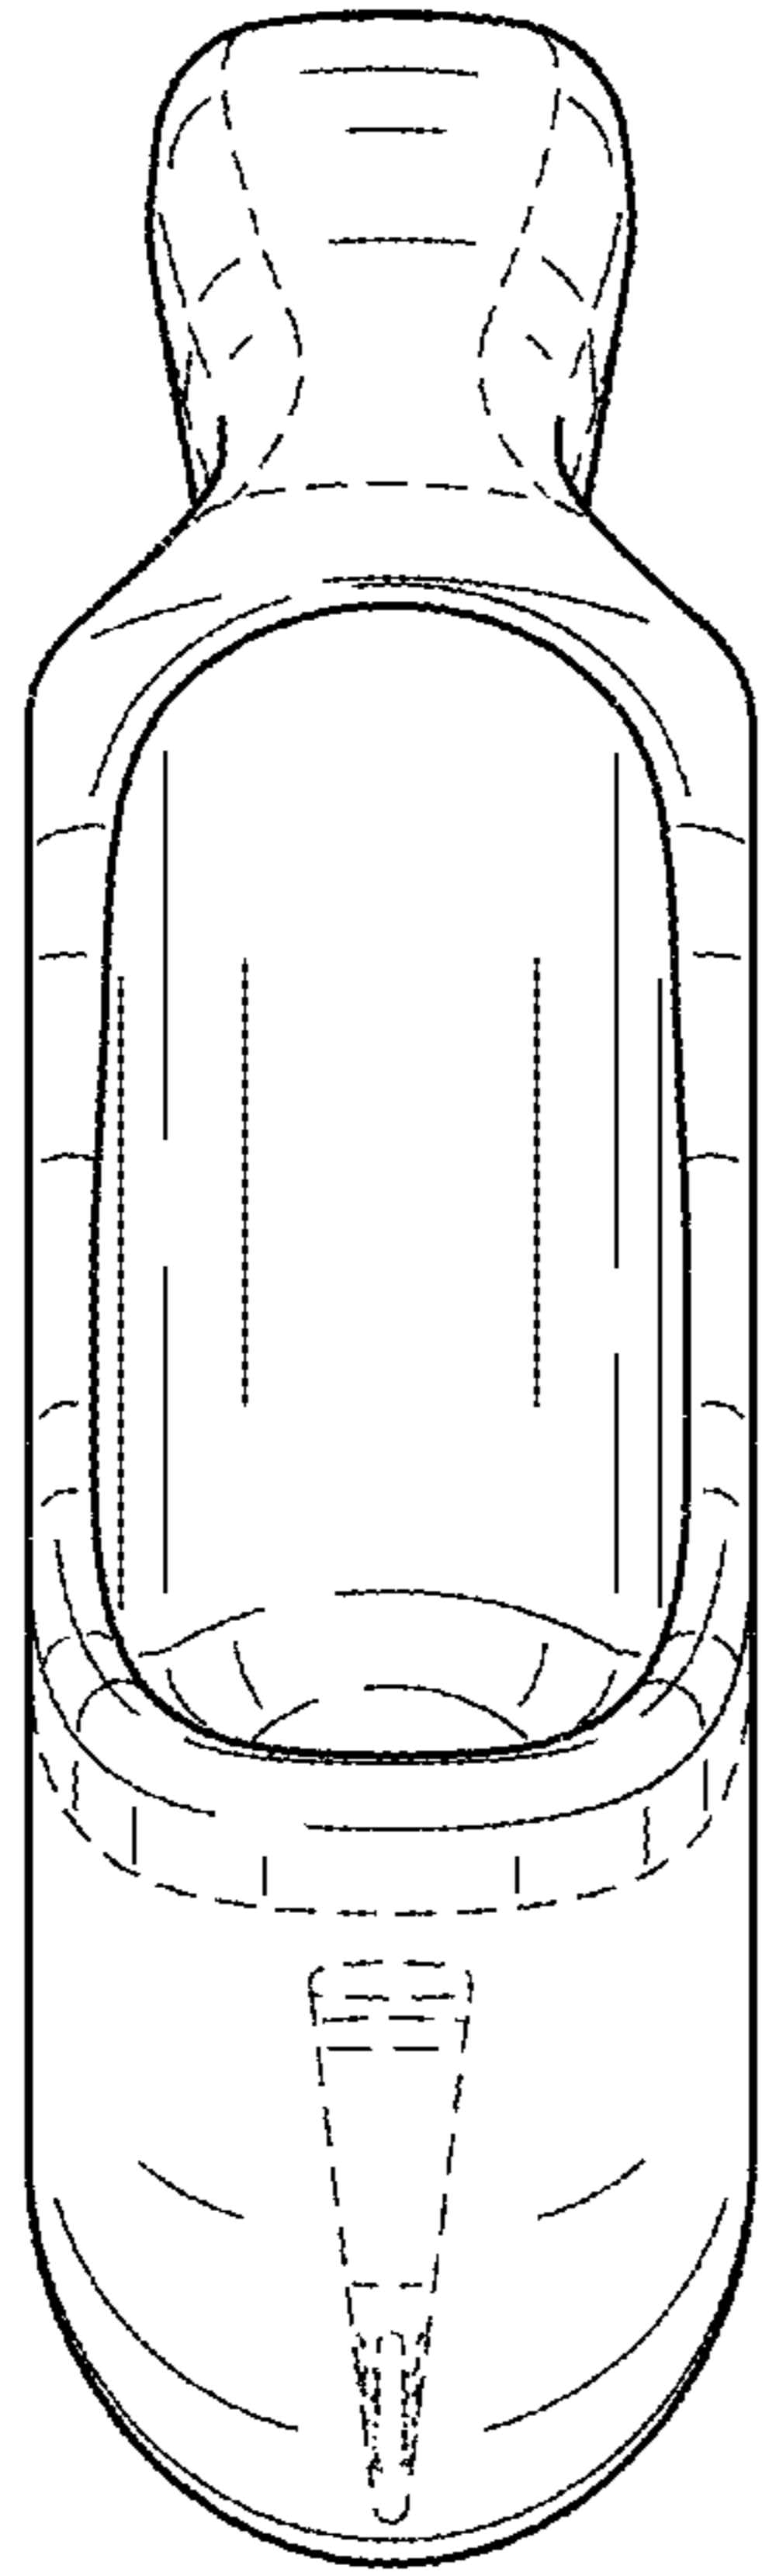


FIG. 5

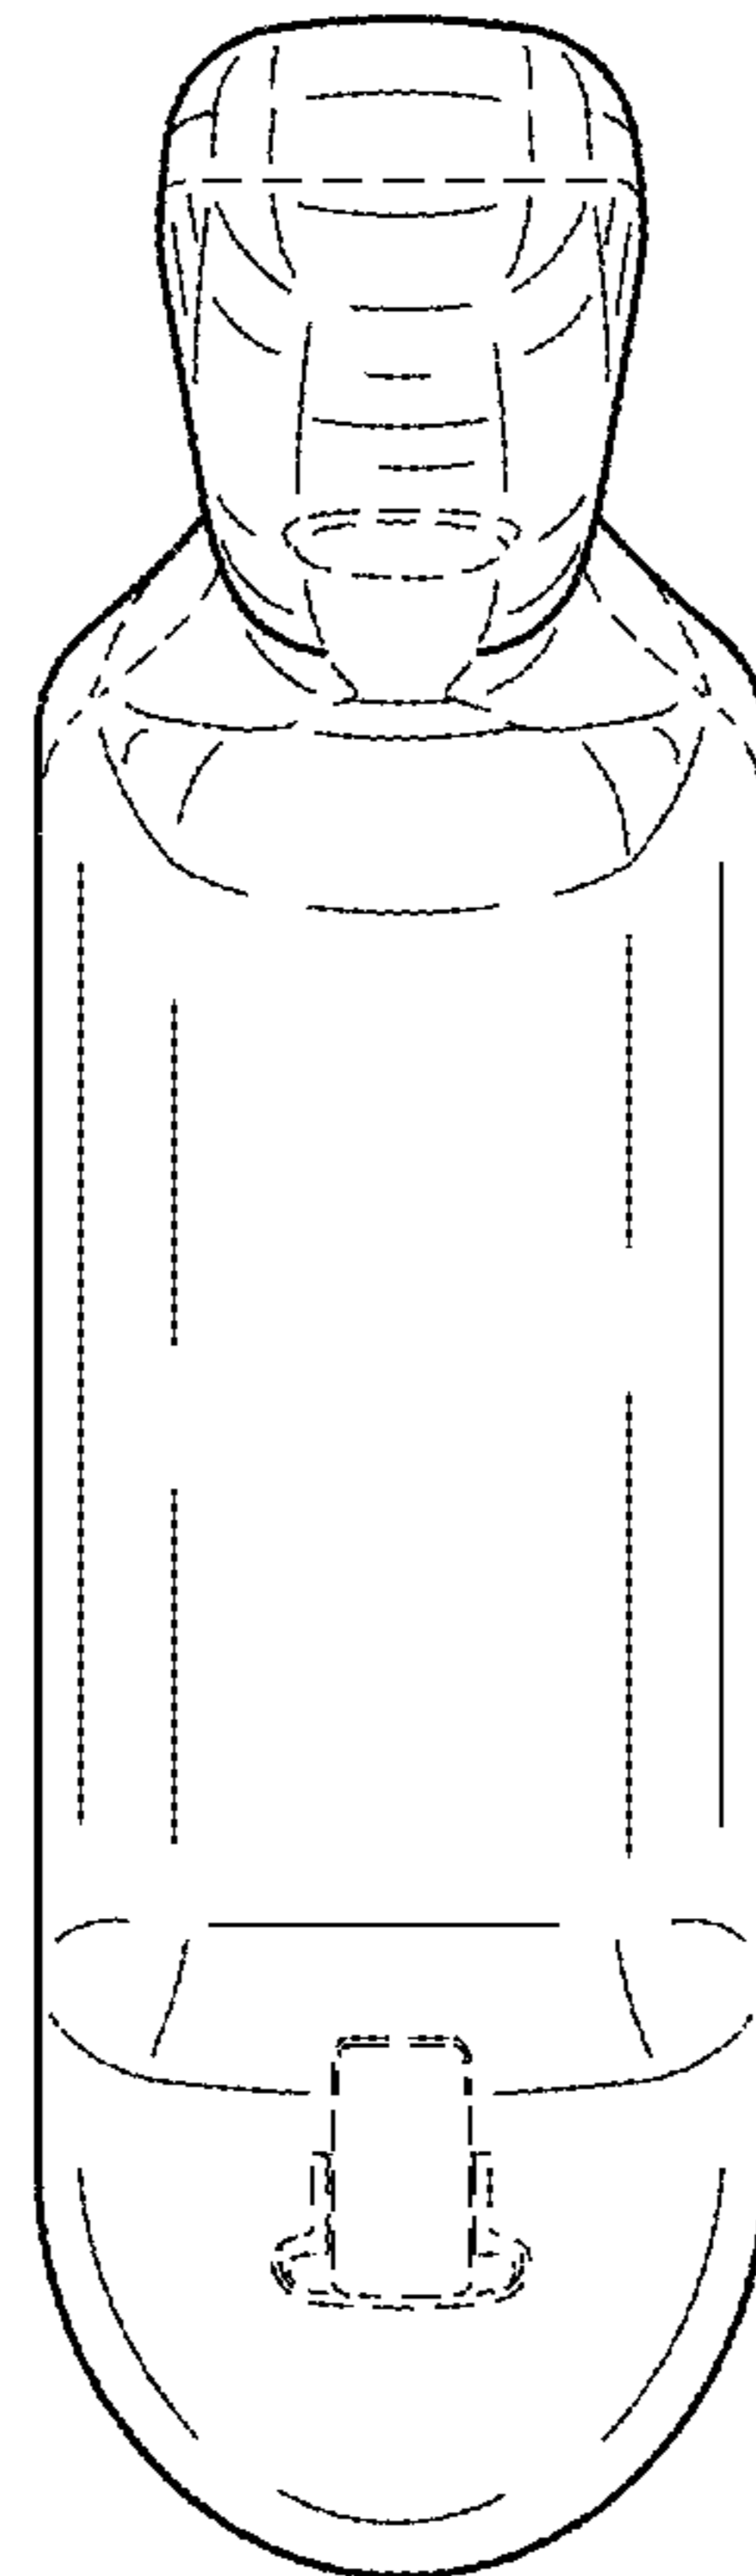


FIG. 6

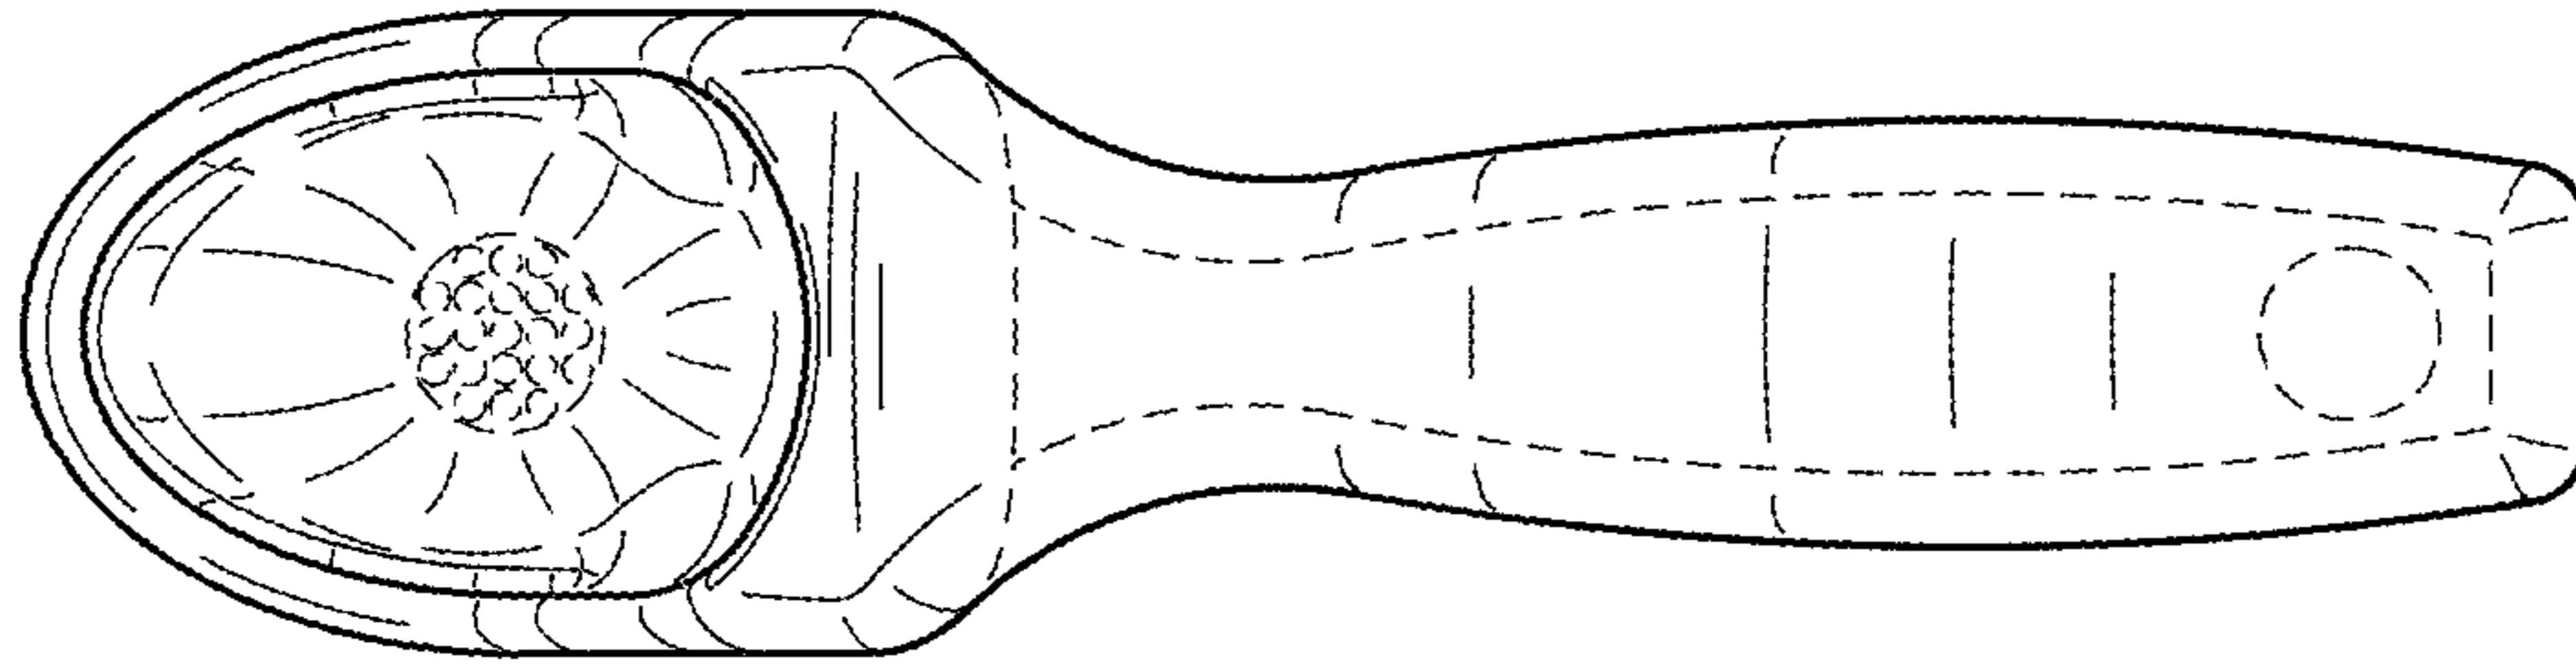


FIG. 7

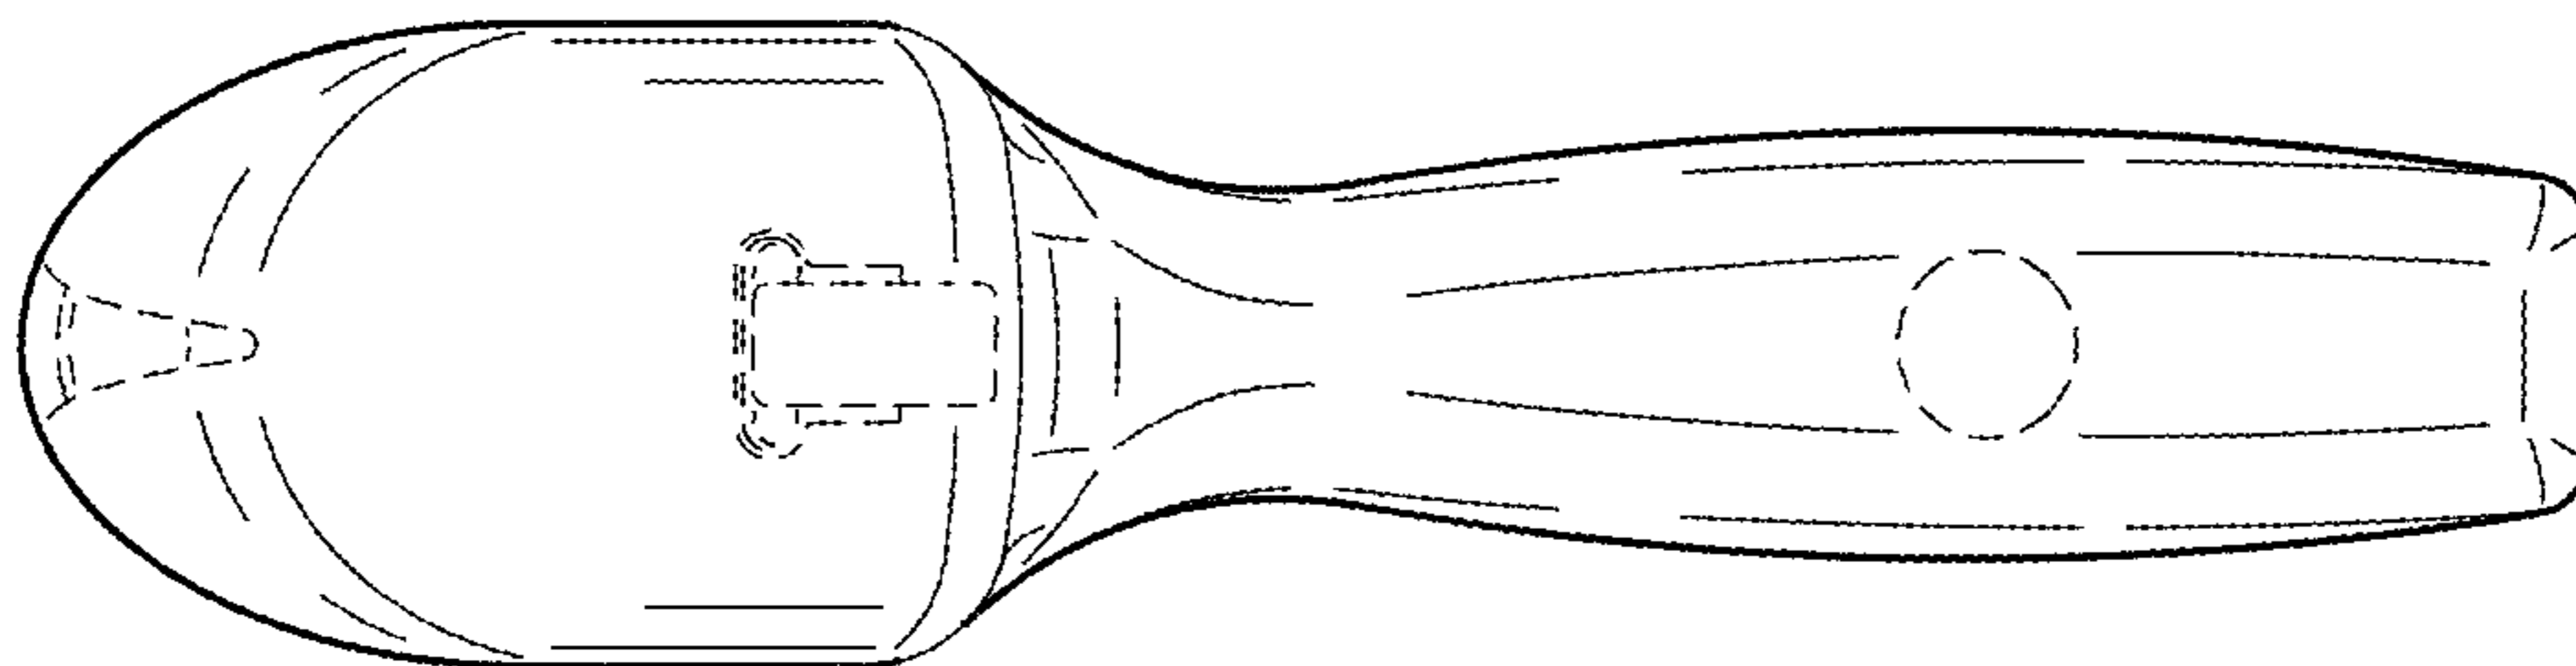


FIG. 8