



US00D933214S

(12) **United States Design Patent** (10) **Patent No.:** **US D933,214 S**  
**Garell** (45) **Date of Patent:** **\*\* Oct. 12, 2021**

(54) **PASSING ELEVATOR**

(71) Applicant: **Paul Charles Garell**, Chappaqua, NY  
(US)

(72) Inventor: **Paul Charles Garell**, Chappaqua, NY  
(US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/730,733**

(22) Filed: **Apr. 8, 2020**

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/133; D24/167**

(58) **Field of Classification Search**  
USPC .... D24/133, 135, 146, 147; D8/14, 45, 6, 7;  
D32/49  
CPC ..... A61B 17/02; A61B 17/0206; A61B  
2017/0237; A61B 2017/0243; A61B  
2017/0256  
See application file for complete search history.

8,805,544 B2 8/2014 Pianca et al.  
D742,007 S \* 10/2015 Schuetz ..... D24/152  
D758,565 S \* 6/2016 Efinger ..... D24/112  
D776,276 S \* 1/2017 Witt ..... D24/146

(Continued)

**FOREIGN PATENT DOCUMENTS**

DE 60032052 T2 7/2007  
EP 1048271 B1 11/2006

**OTHER PUBLICATIONS**

Medtronic—Surgical Lead Implantation Guide, 2010.  
(Continued)

*Primary Examiner* — Philip S Hyder  
(74) *Attorney, Agent, or Firm* — Brian K. Johnson, Esq.,  
LLC

(57) **CLAIM**

The ornamental design for a passing elevator, as shown and described.

**DESCRIPTION**


A portion of the disclosure of this patent document may contain material, which is subject to copyright protection. The owner has no objection to the facsimile reproduction by any one of the patent documents or the patent disclosure, as it appears in the Patent and Trademark Office patent file or records, but otherwise reserves all copyrights whatsoever. FIG. 1 is a perspective view of the passing elevator showing the new design; FIG. 2 is a front view thereof; FIG. 3 is a back view thereof; FIG. 4 is a right side view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a top view thereof; and, FIG. 7 is a bottom view thereof.

**1 Claim, 5 Drawing Sheets**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D318,116 S \* 7/1991 Michelson ..... D24/147  
5,827,311 A 10/1998 Berelsman et al.  
6,249,707 B1 6/2001 Kohnen et al.  
D522,110 S \* 5/2006 Lanius ..... D23/283  
D535,744 S \* 1/2007 Wright ..... D24/135  
D571,008 S 6/2008 Wu  
D571,467 S 6/2008 Wu  
D571,468 S 6/2008 Wu  
D571,913 S 6/2008 Wu  
D575,396 S 8/2008 Wu  
D577,120 S 9/2008 Wu  
D593,201 S \* 5/2009 Lash ..... D24/135  
D658,285 S \* 4/2012 Ryshkus ..... D24/135  
D658,286 S \* 4/2012 Ryshkus ..... D24/135  
D691,274 S \* 10/2013 Buckels ..... D24/167  
8,588,936 B2 11/2013 MacDonald et al.  
D706,924 S \* 6/2014 Ryshkus ..... D24/135

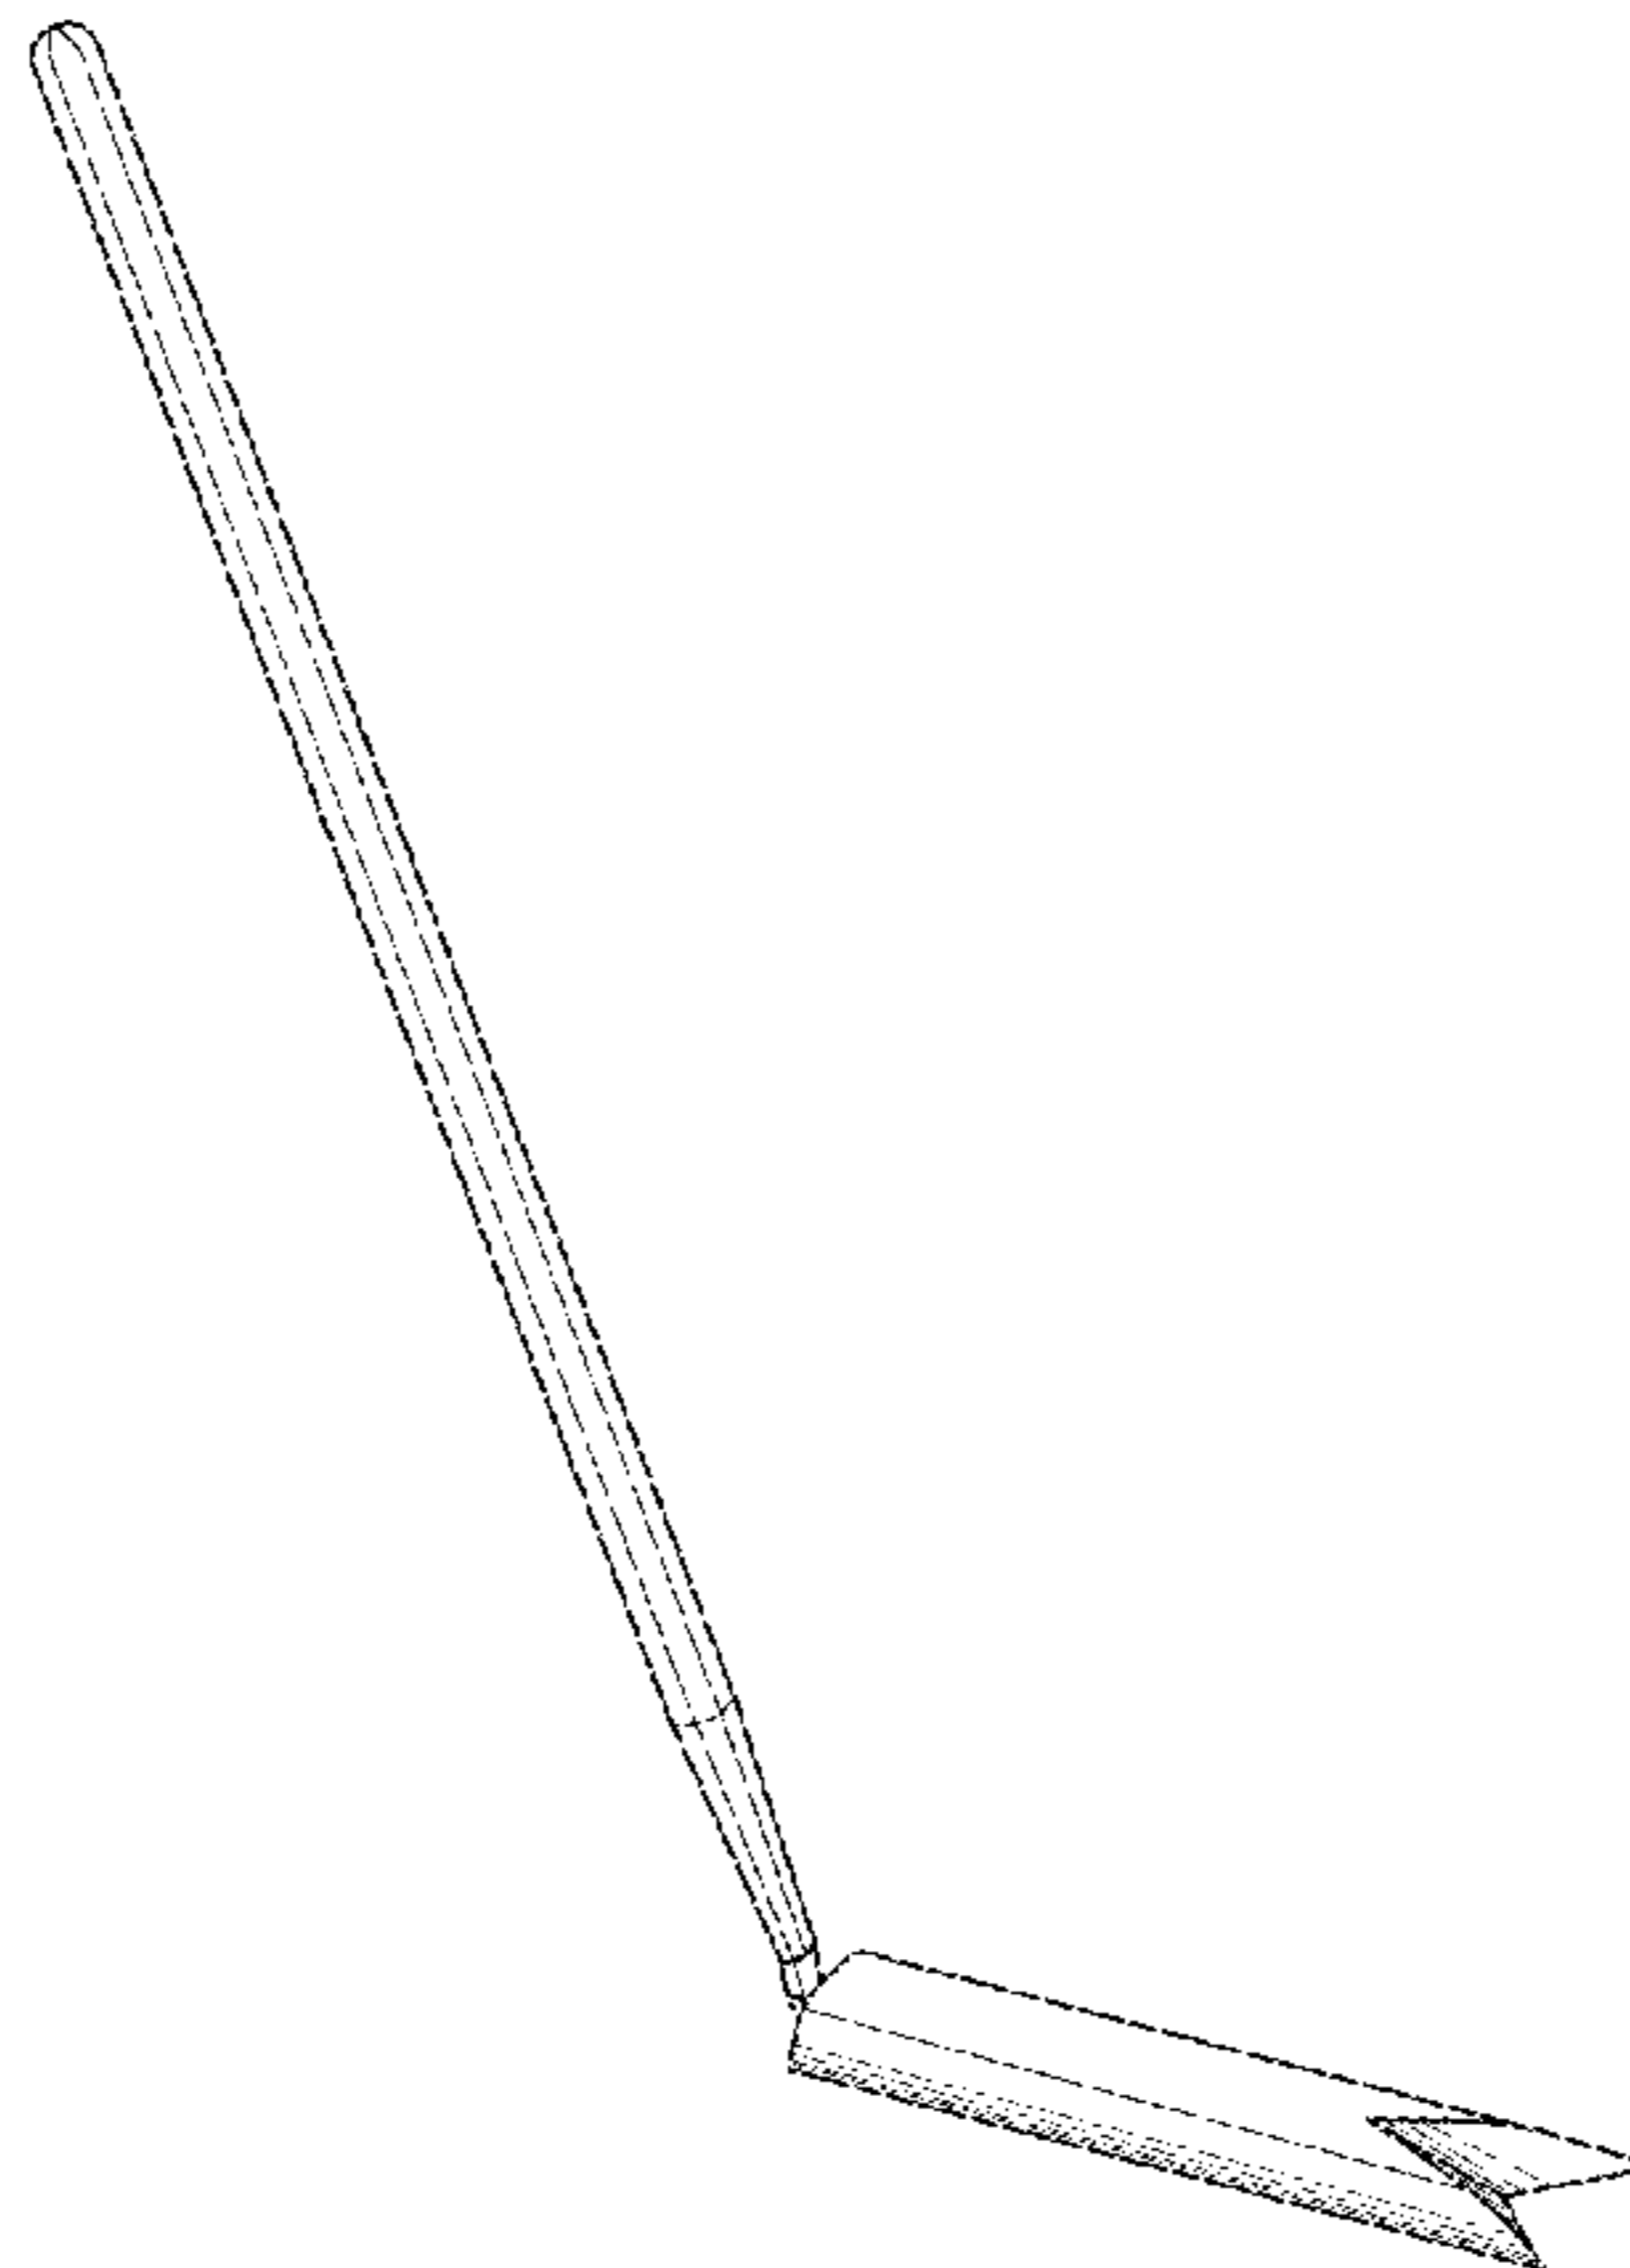

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D786,166 S \* 5/2017 Henderson ..... D12/213  
D833,607 S \* 11/2018 Aradono ..... D24/135  
2009/0149715 A1\* 6/2009 Mao ..... A61B 5/14542  
600/202  
2013/0204270 A1 8/2013 Howard et al.  
2014/0277266 A1 9/2014 Khalil et al.  
2016/0206302 A1\* 7/2016 Eckermann ..... A61B 17/02  
2017/0172555 A1\* 6/2017 Shimizu ..... A61B 17/02  
2017/0304631 A1 10/2017 Biele et al.

OTHER PUBLICATIONS

Boston Scientific—Precision Spinal Cord Simulator System Clinician Manual, 2017.  
Boston Scientific—Surgical Leads, 2017.  
Medtronic model 3550P4—accessory kit—Jul. 2009.

\* cited by examiner

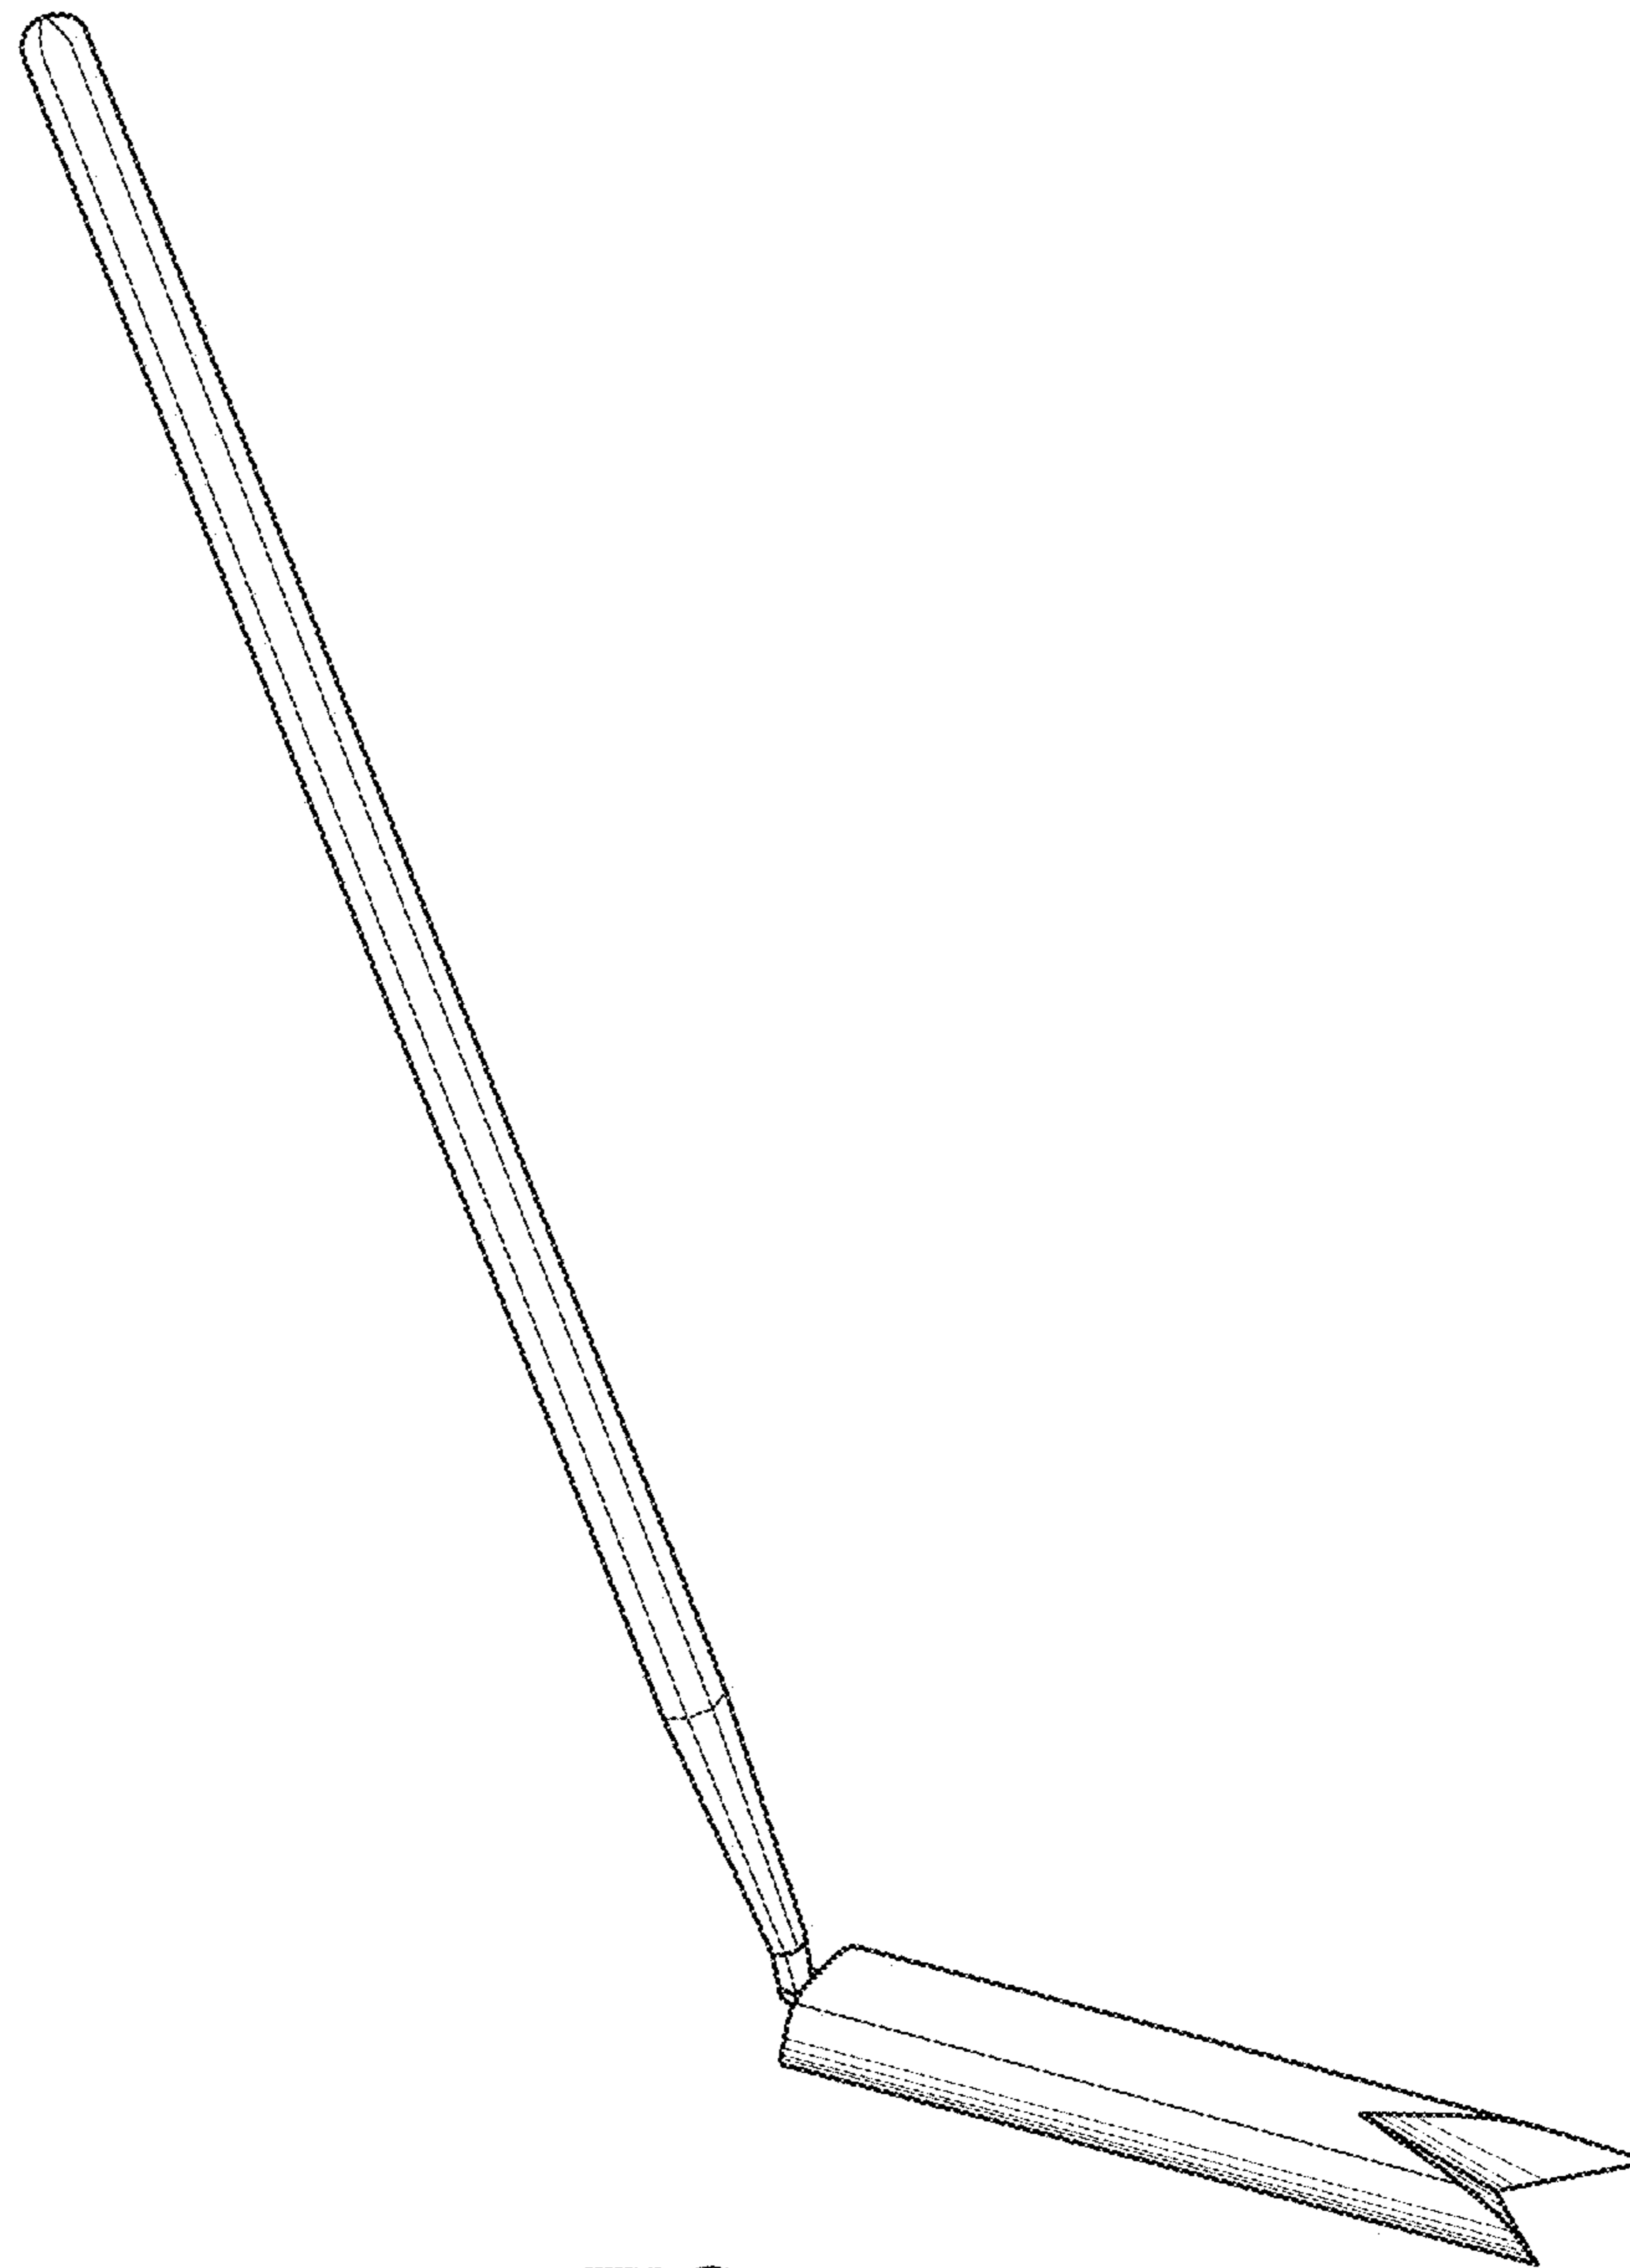


FIG. 1

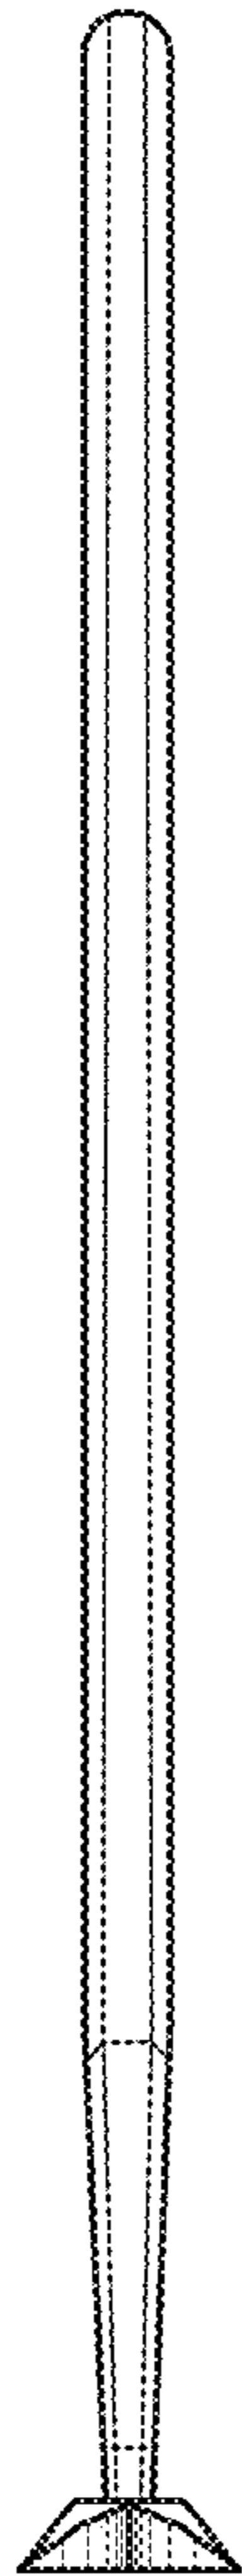


FIG. 2

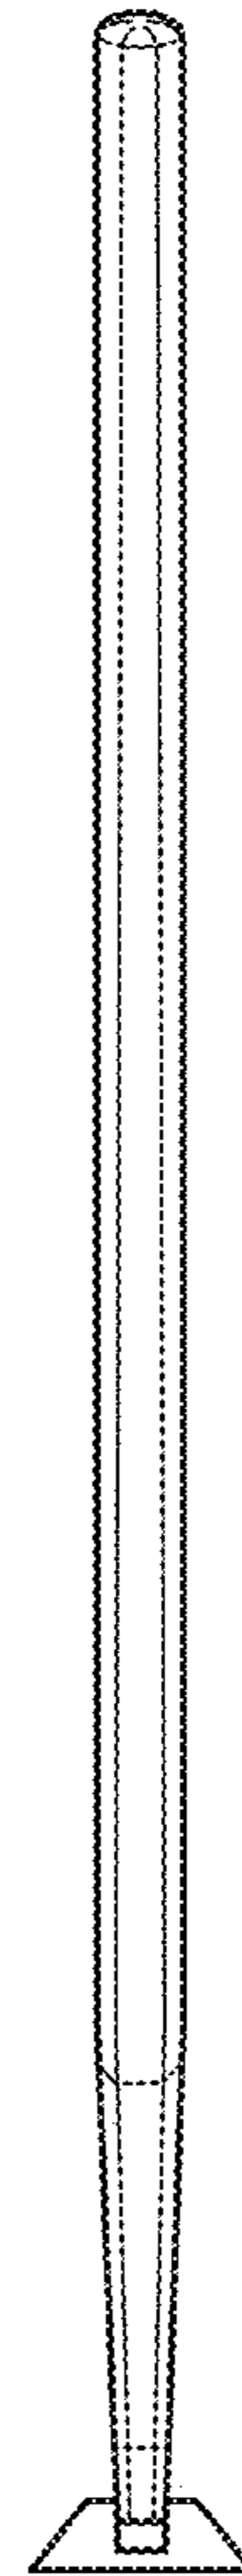


FIG. 3

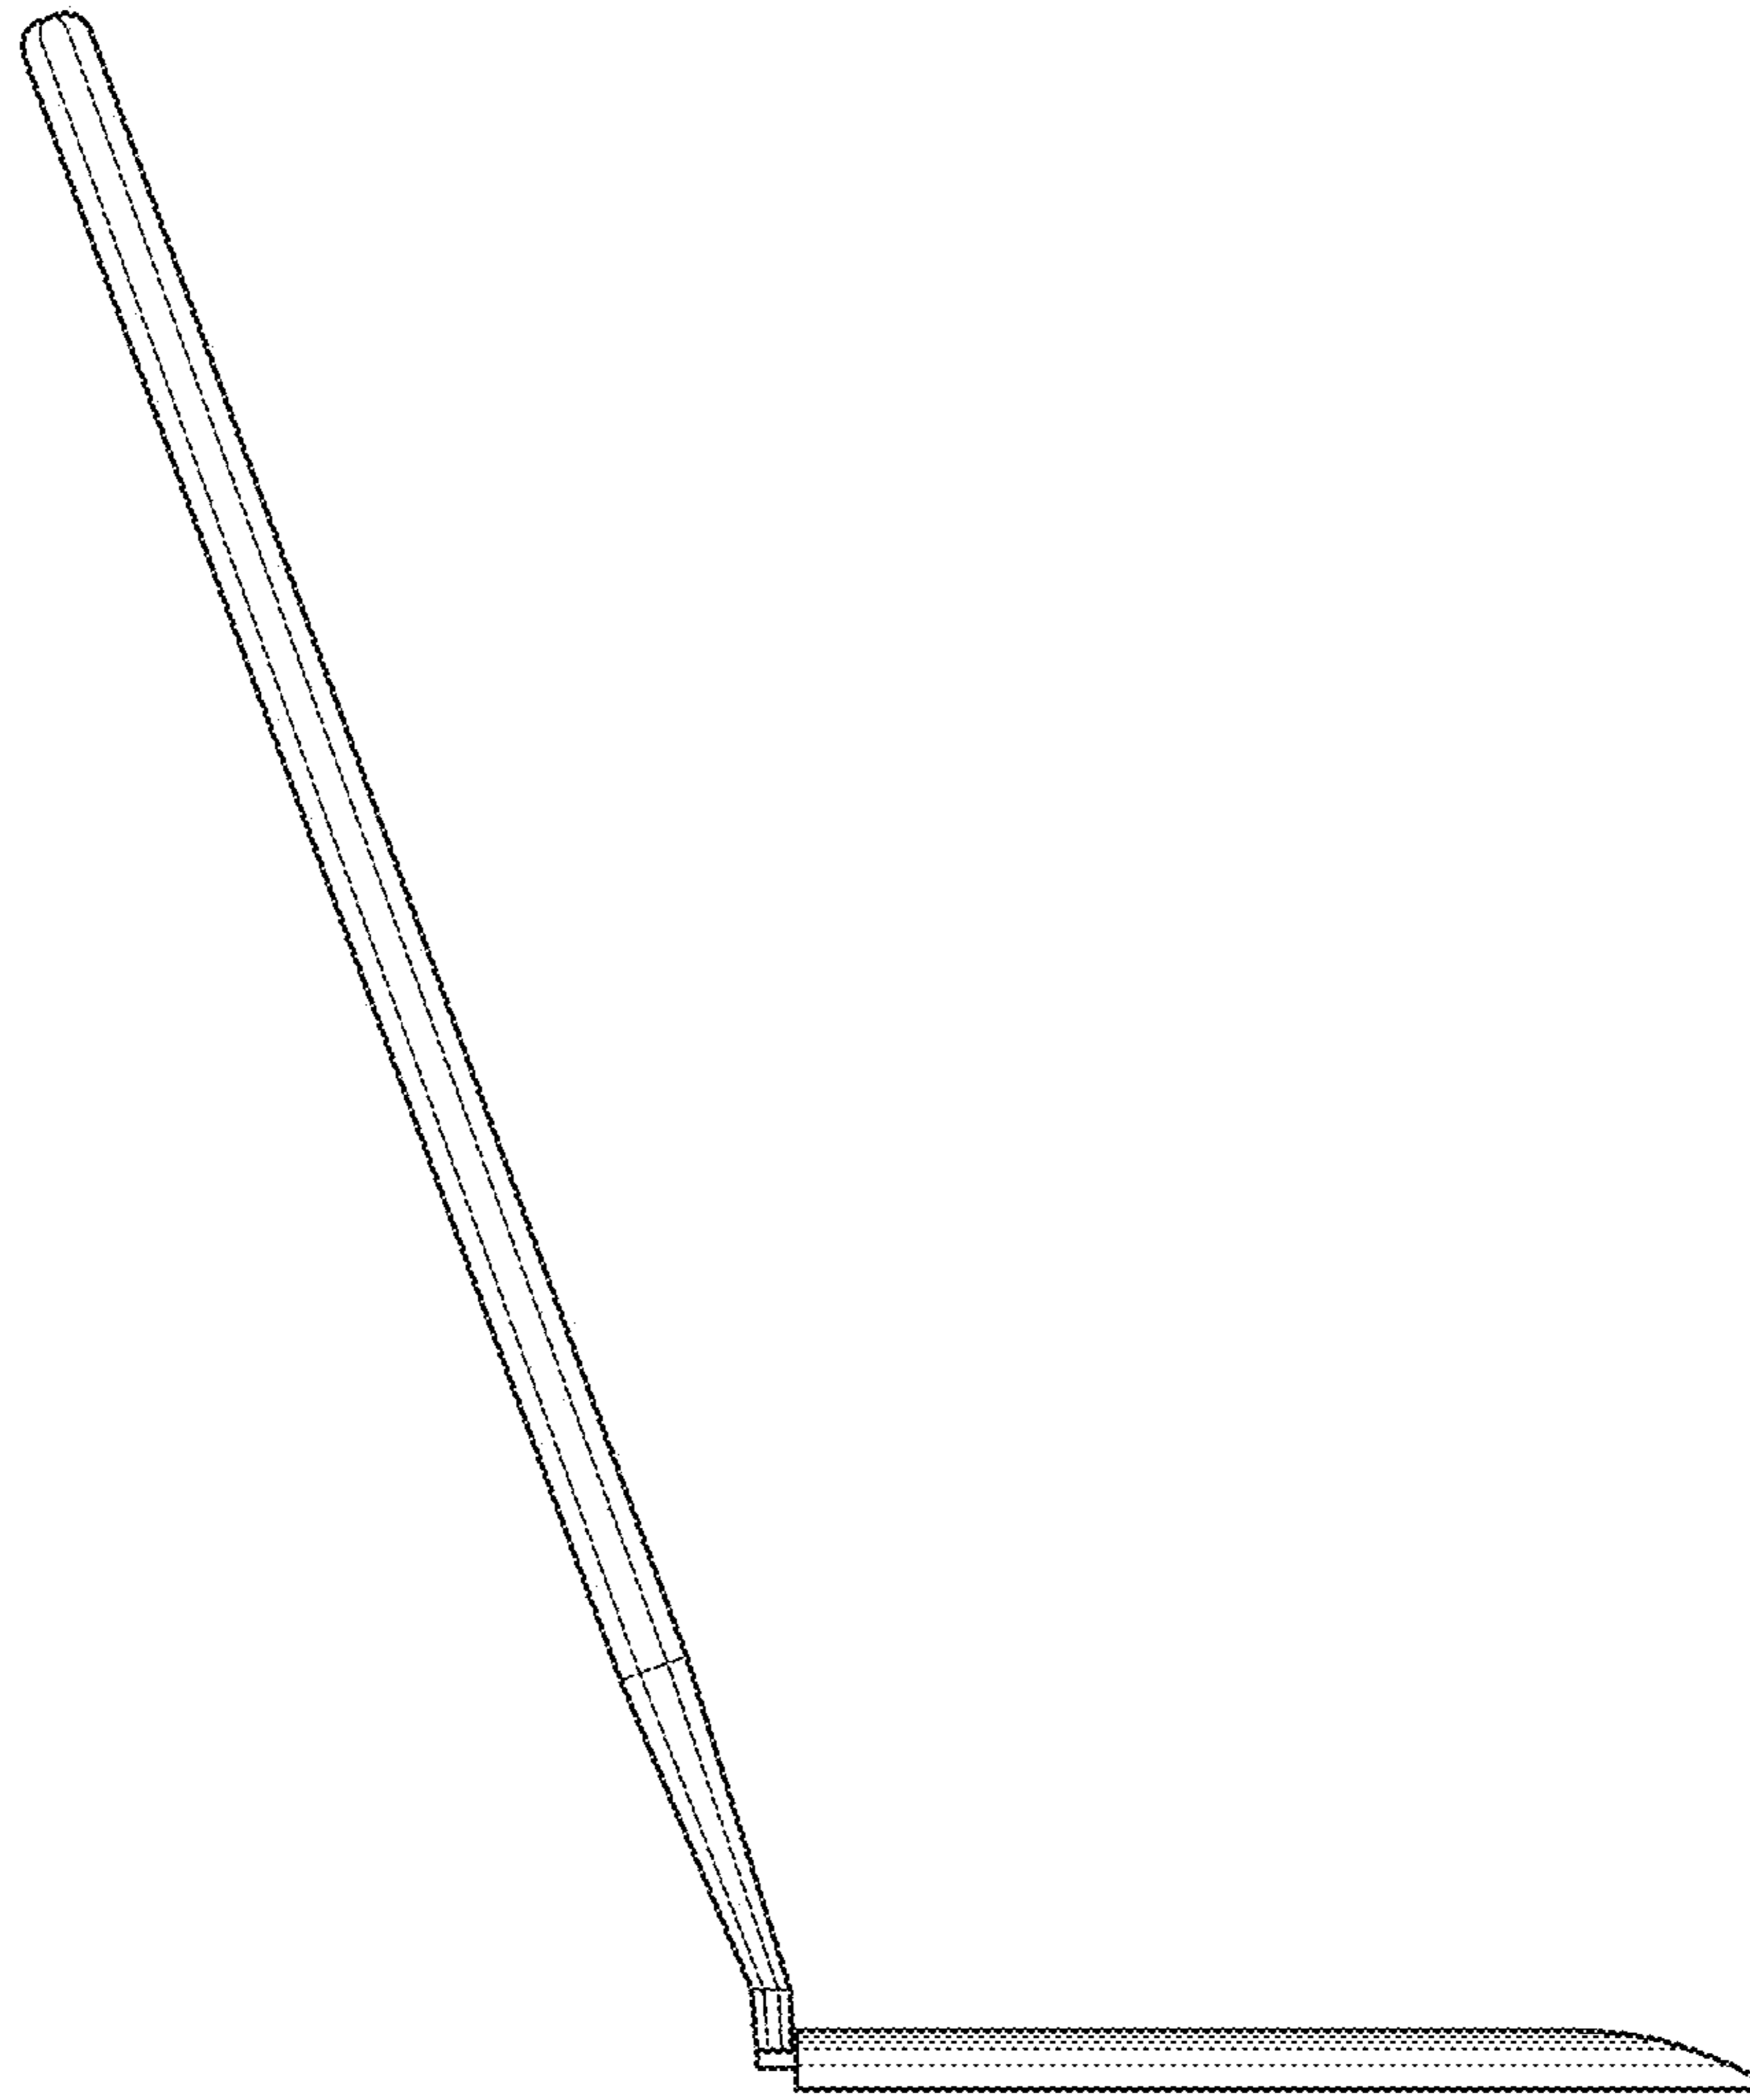


FIG. 4

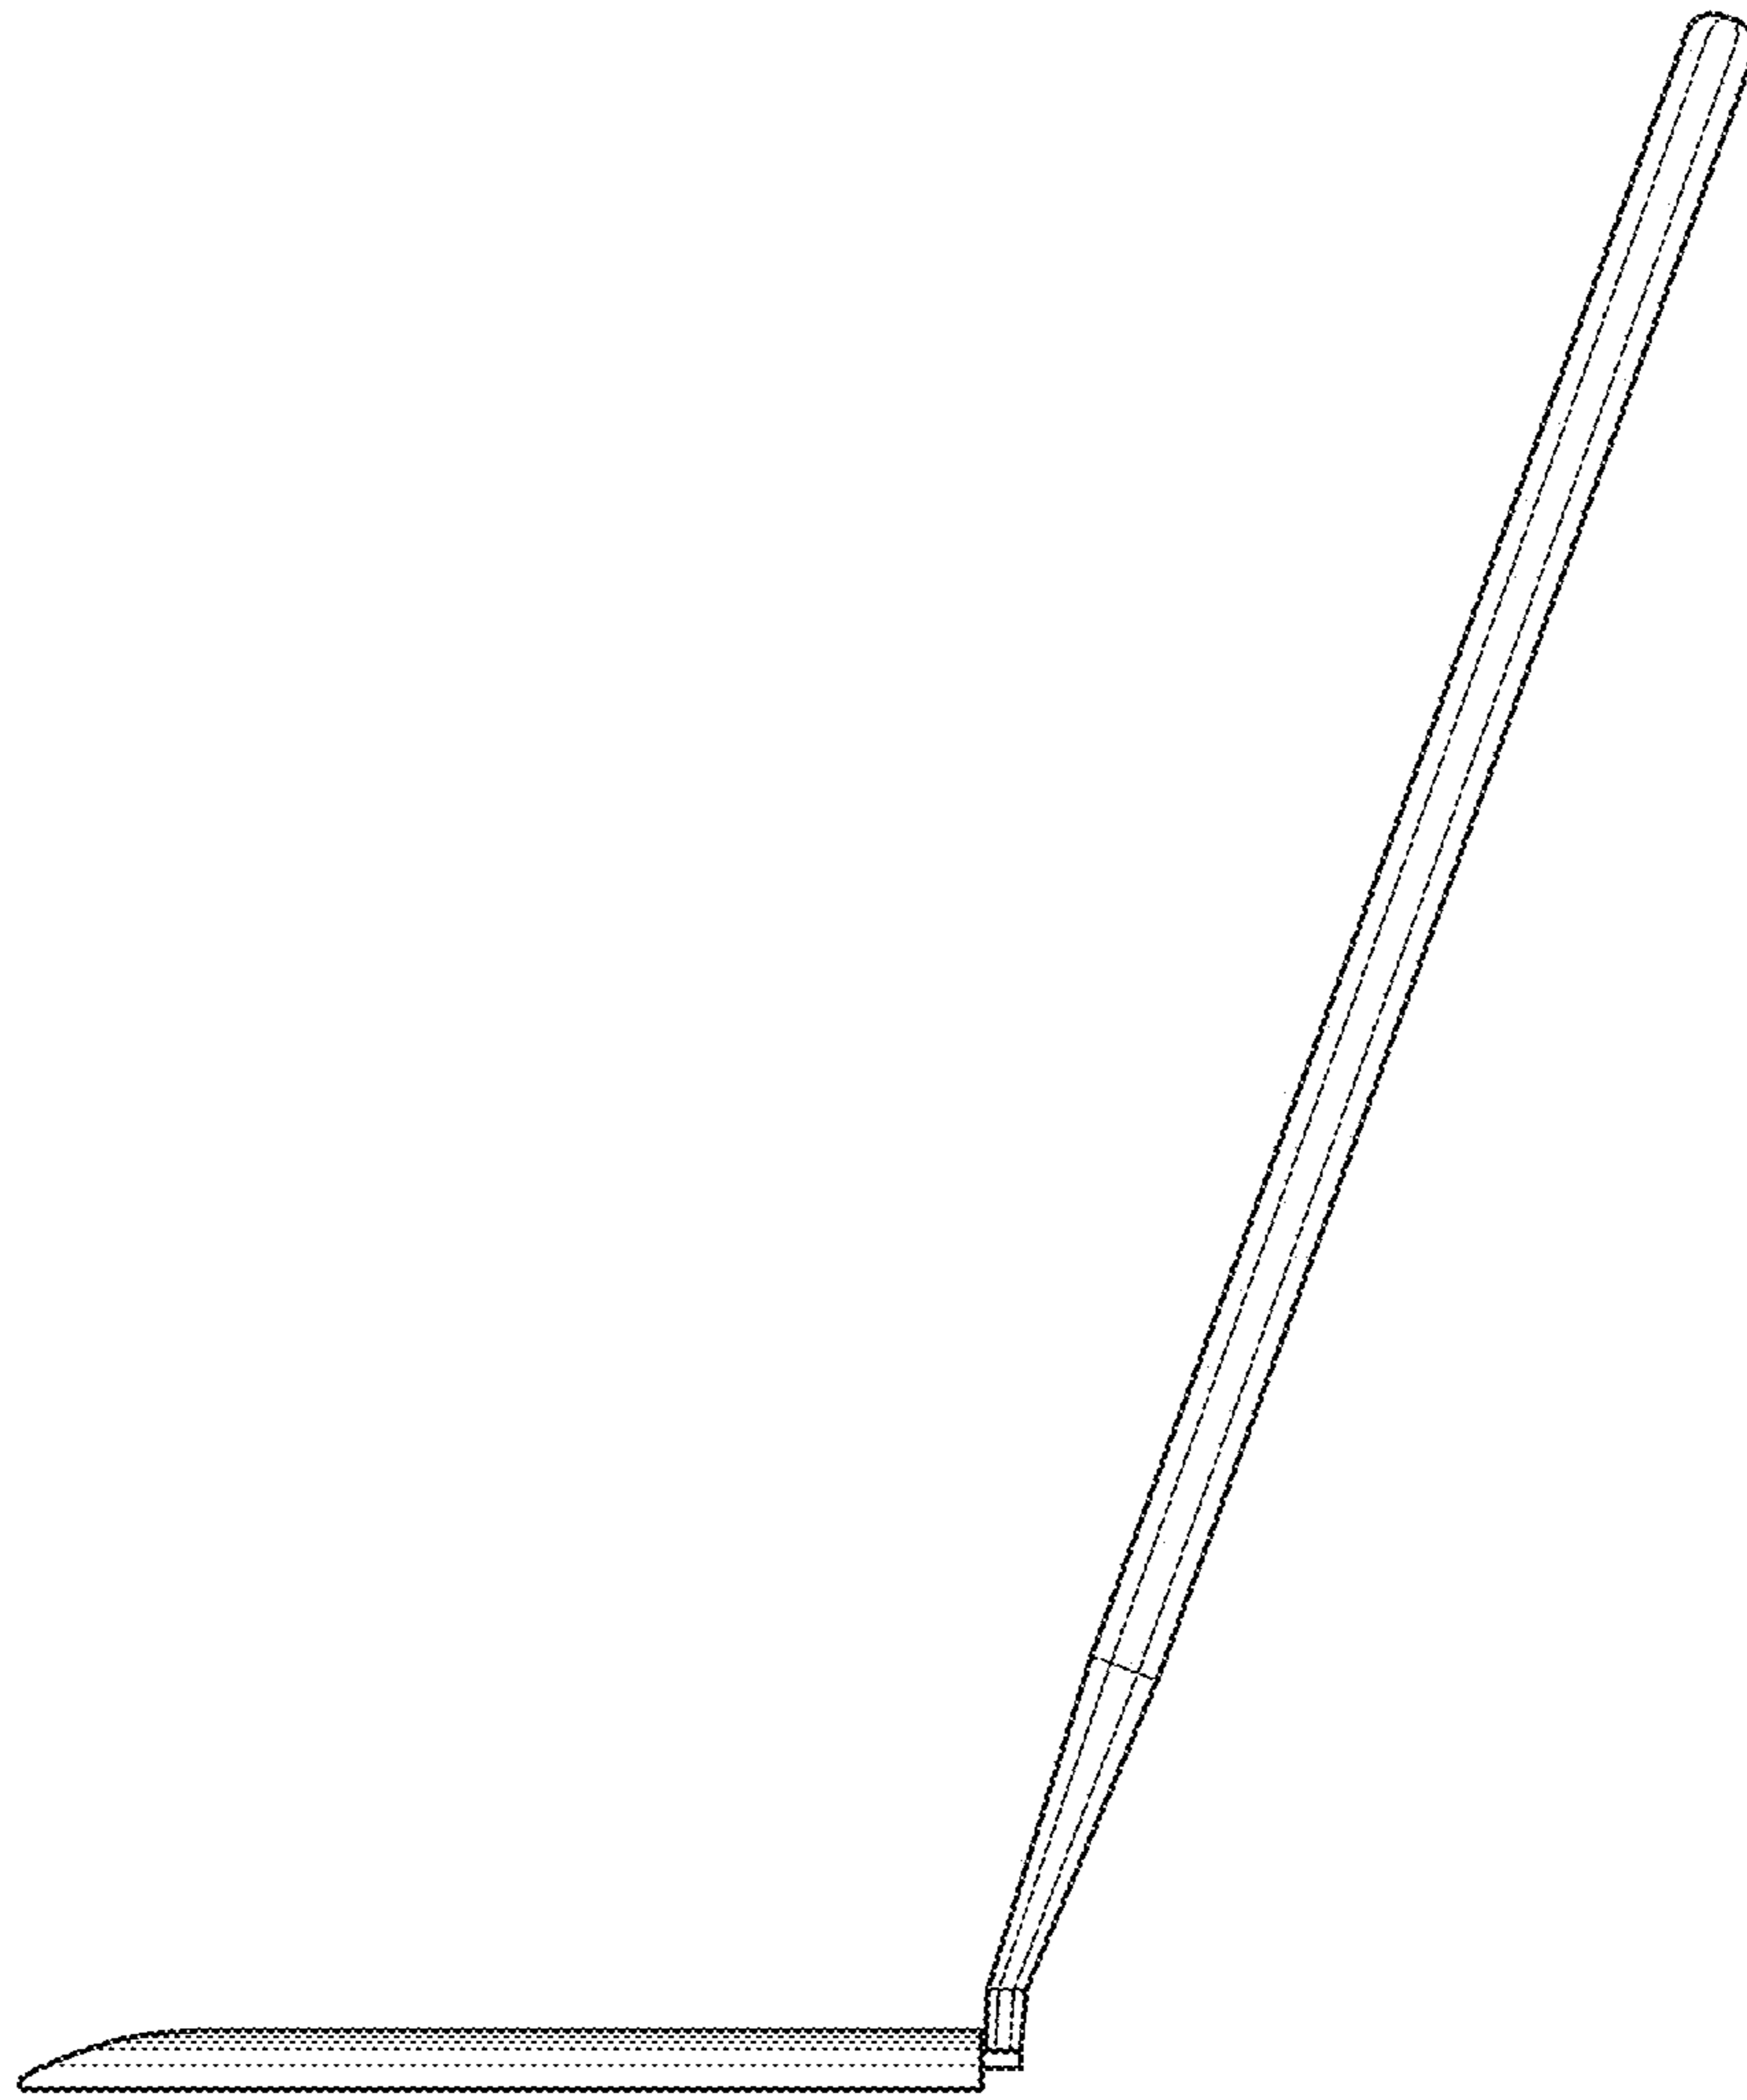


FIG. 5

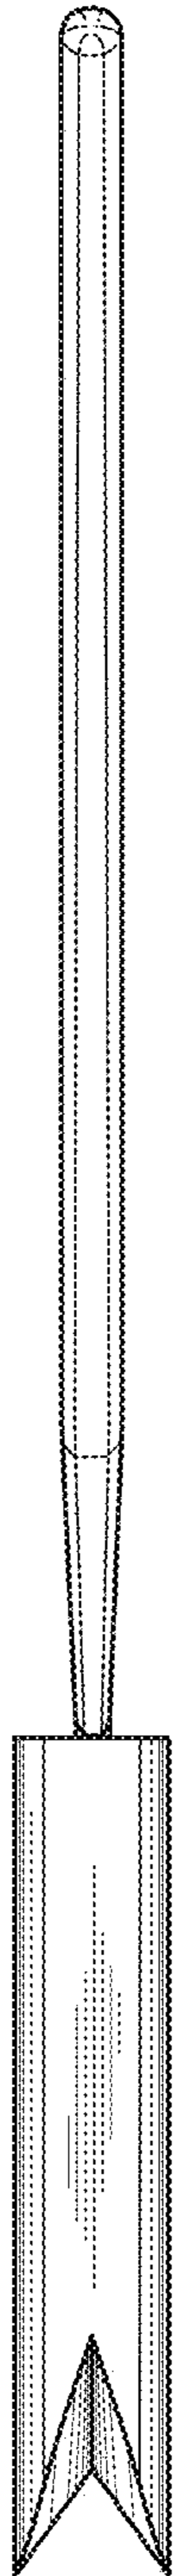


FIG. 6

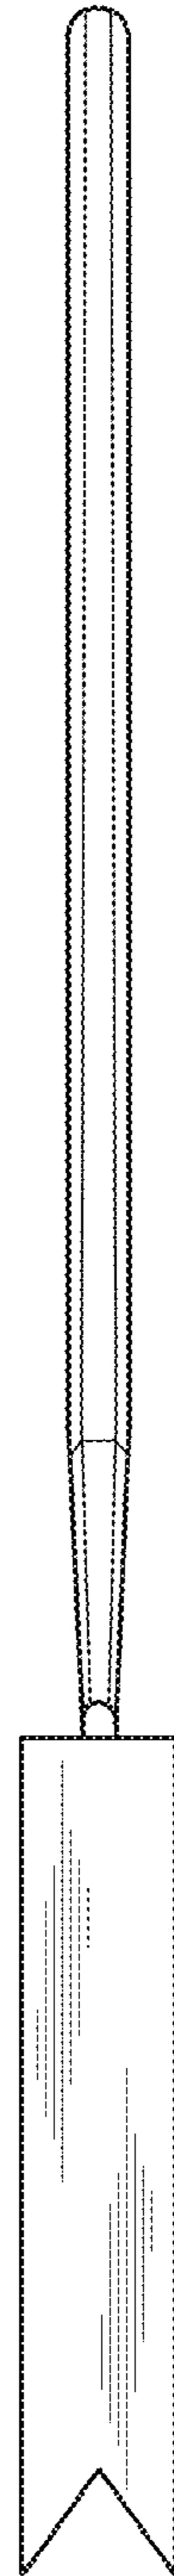


FIG. 7