



US00D933238S

(12) **United States Design Patent** (10) **Patent No.:** **US D933,238 S**
Laing et al. (45) **Date of Patent:** **** Oct. 12, 2021**

(54) **UROFLOWMETER**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **ClearTrac Technologies, LLC**,
Elizabethton, TN (US)

CN 2221776 Y 3/1996
CN 105769223 A 7/2016

(Continued)

(72) Inventors: **Brent Laing**, Greenwood Village, CO (US); **John Green**, Elizabethton, TN (US); **Paul R. Johnson**, Boulder, CO (US); **Robert John Smith**, Louisville, CO (US); **Robert Edwin Schneider**, Erie, CO (US); **Magnus Hargis**, Hudson, CO (US); **Elise Geolat Edson**, Boulder, CO (US); **Elizabeth A. O'Brien**, Louisville, CO (US); **Joseph L. Kapushion**, Westminster, CO (US)

OTHER PUBLICATIONS

Drive Medical. "Drive Medical Folding Steel Bedside Commode, Grey." obtained Nov. 12, 2018 from <https://www.amazon.com/Drive-Medical-Folding-Bedside-Commode/dp/B001HP7AQE/ref=sr_1_3?s=industrial&ie=UTF8&qid=1539732631&sr=1-3&keywords=commode>, 8 pages.

(Continued)

(73) Assignee: **CLEARTRAC TECHNOLOGIES, LLC**, Elizabethton, TN (US)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(**) Term: **15 Years**

(57) **CLAIM**

(21) Appl. No.: **29/707,600**

The ornamental design for a uroflowmeter, as shown and described.

(22) Filed: **Sep. 30, 2019**

DESCRIPTION

Related U.S. Application Data

(63) Continuation of application No. 29/682,876, filed on Mar. 8, 2019.

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186; D24/122**

(58) **Field of Classification Search**
USPC D24/107, 121, 122, 129, 186, 216, 223, D24/224, 231; D10/96, 102; D7/691
(Continued)

FIG. 1 shows a front perspective view of a uroflowmeter; FIG. 2 shows a right elevation view of the uroflowmeter of FIG. 1; FIG. 3 shows a left elevation view of the uroflowmeter of FIG. 1; FIG. 4 shows a front elevation view of the uroflowmeter of FIG. 1; FIG. 5 shows a rear elevation view of the uroflowmeter of FIG. 1; FIG. 6 shows a top view of the uroflowmeter of FIG. 1; and, FIG. 7 shows a bottom view of the uroflowmeter of FIG. 1. The dash-dot-dash lines represent the bounds of the claim, and the remaining broken lines illustrate portions of the uroflowmeter that form no part of the claimed design; none of the broken lines form a part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

2,648,981 A 8/1953 Drake
3,172,130 A 3/1965 Lange

(Continued)

1 Claim, 4 Drawing Sheets

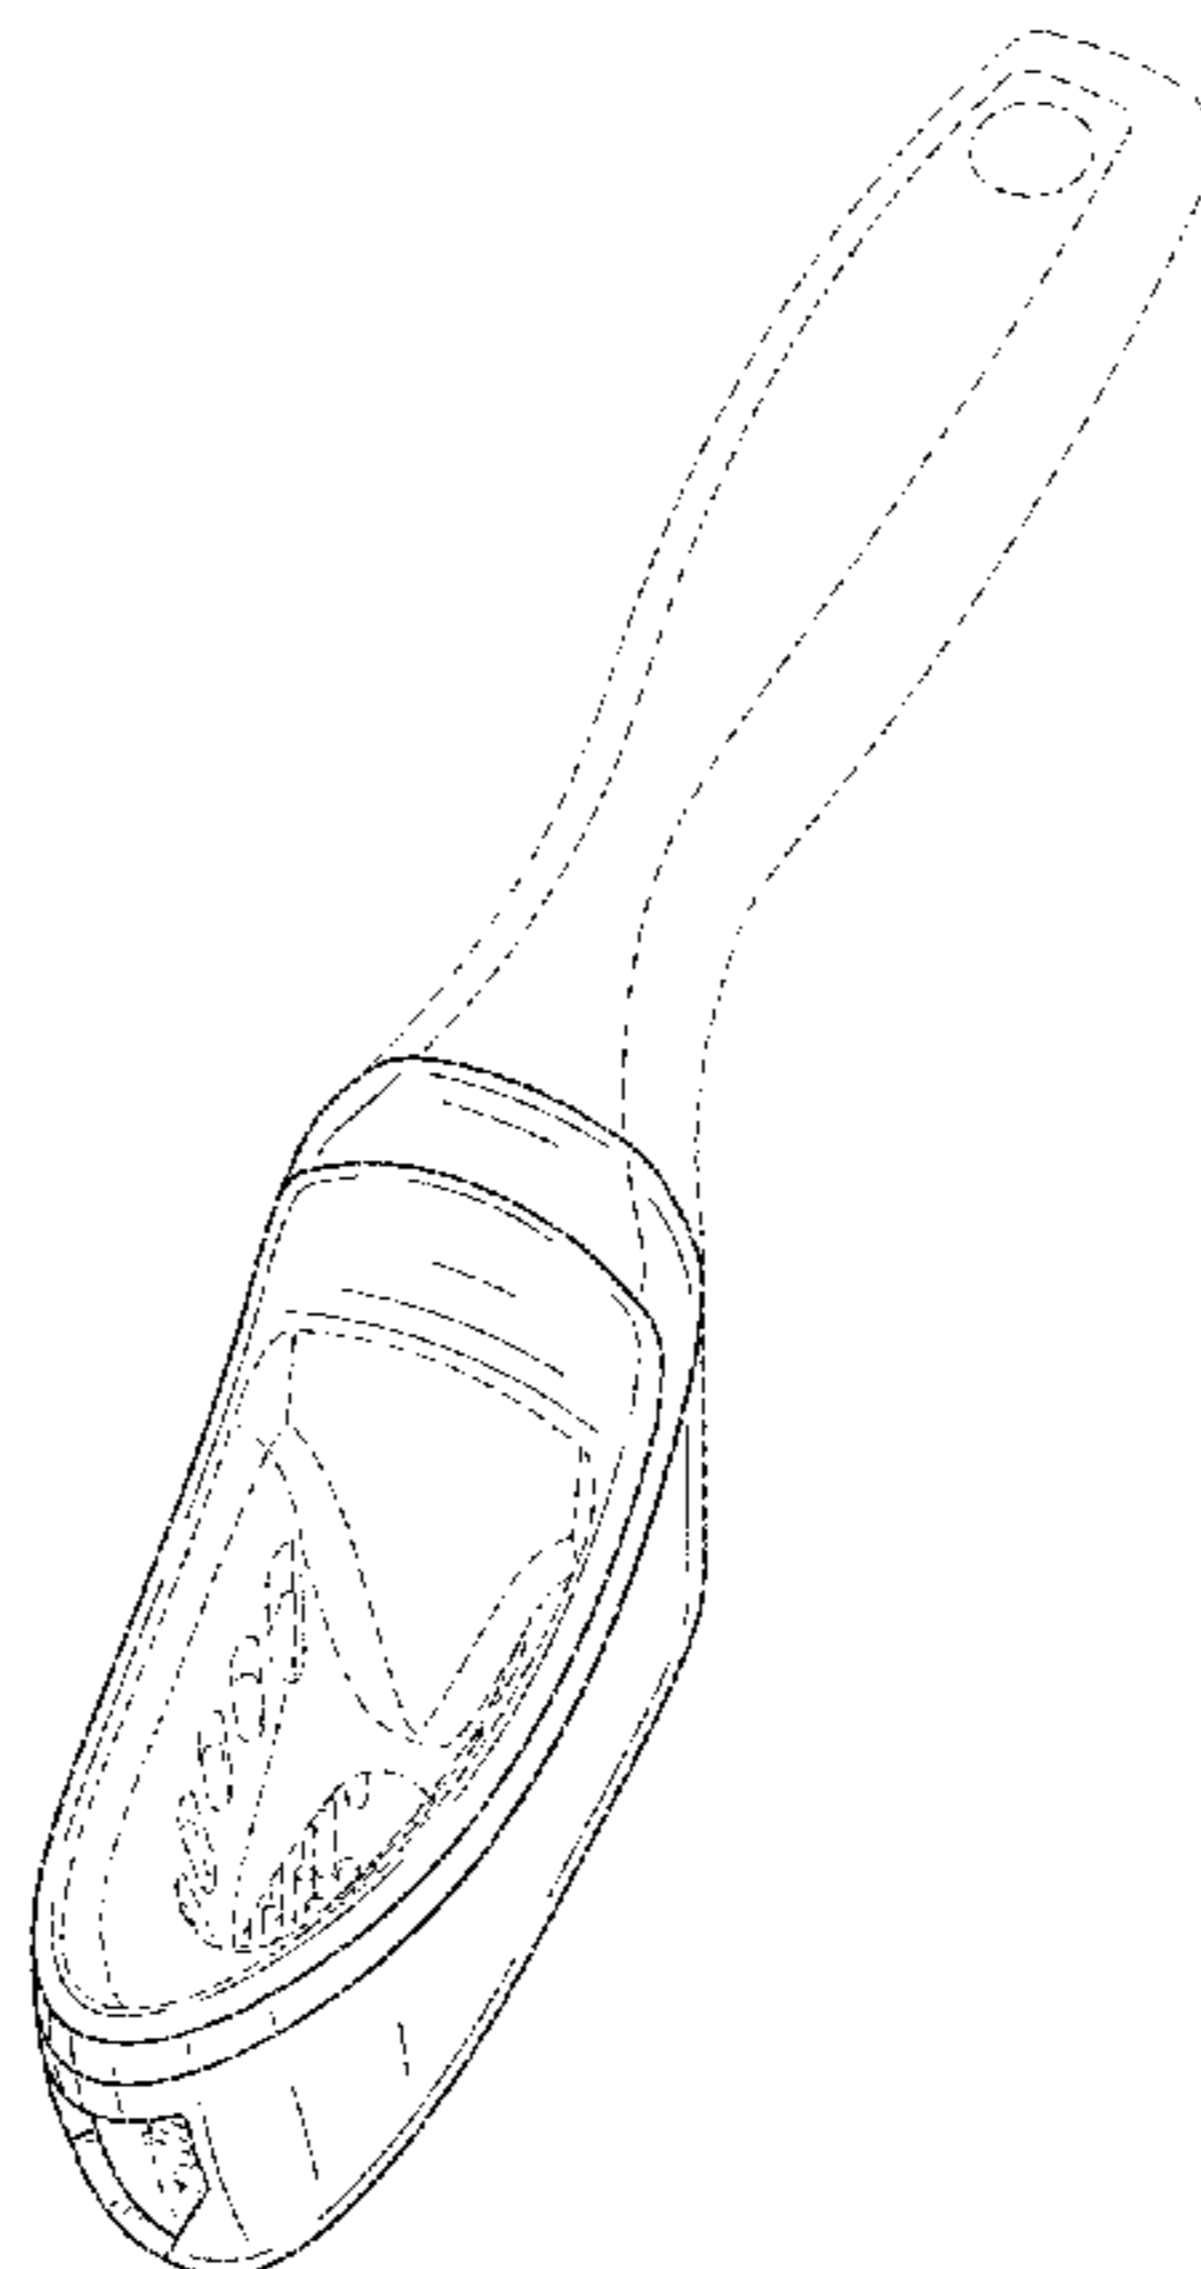

(56)

References Cited

OTHER PUBLICATIONS

PCT, "International Search Report and Written Opinion", Application No. PCT/US19/21421, dated May 31, 2019, 16 pages.

* cited by examiner

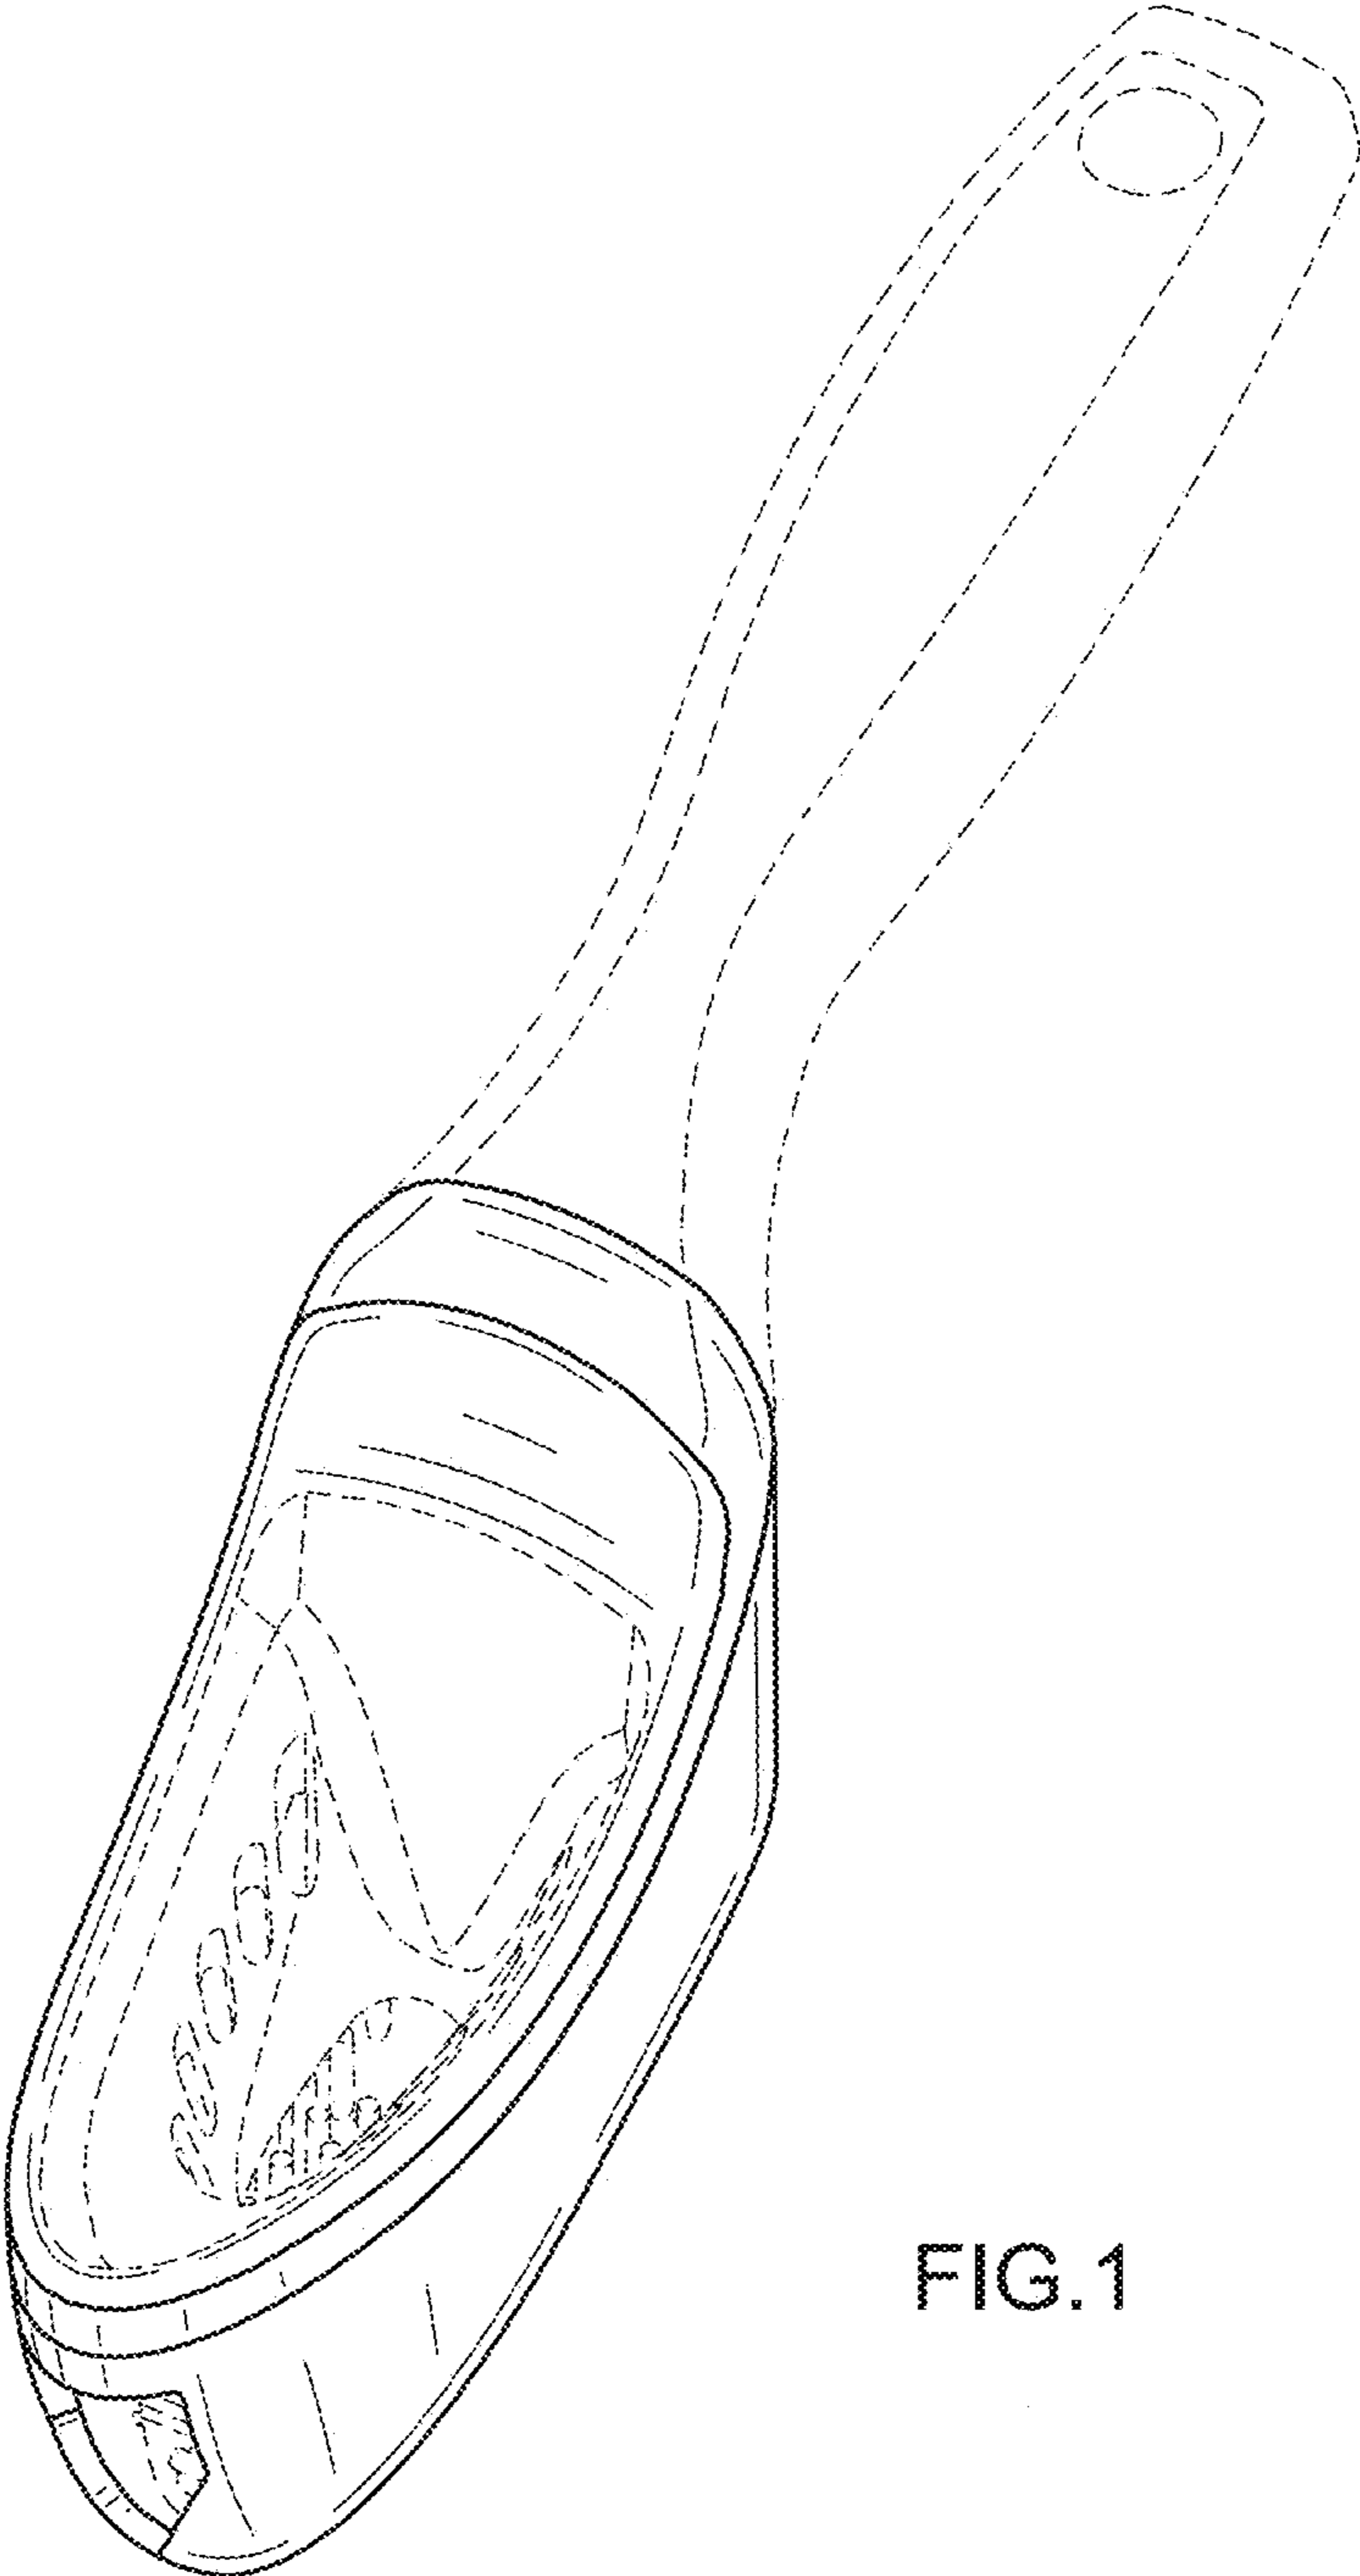


FIG.1

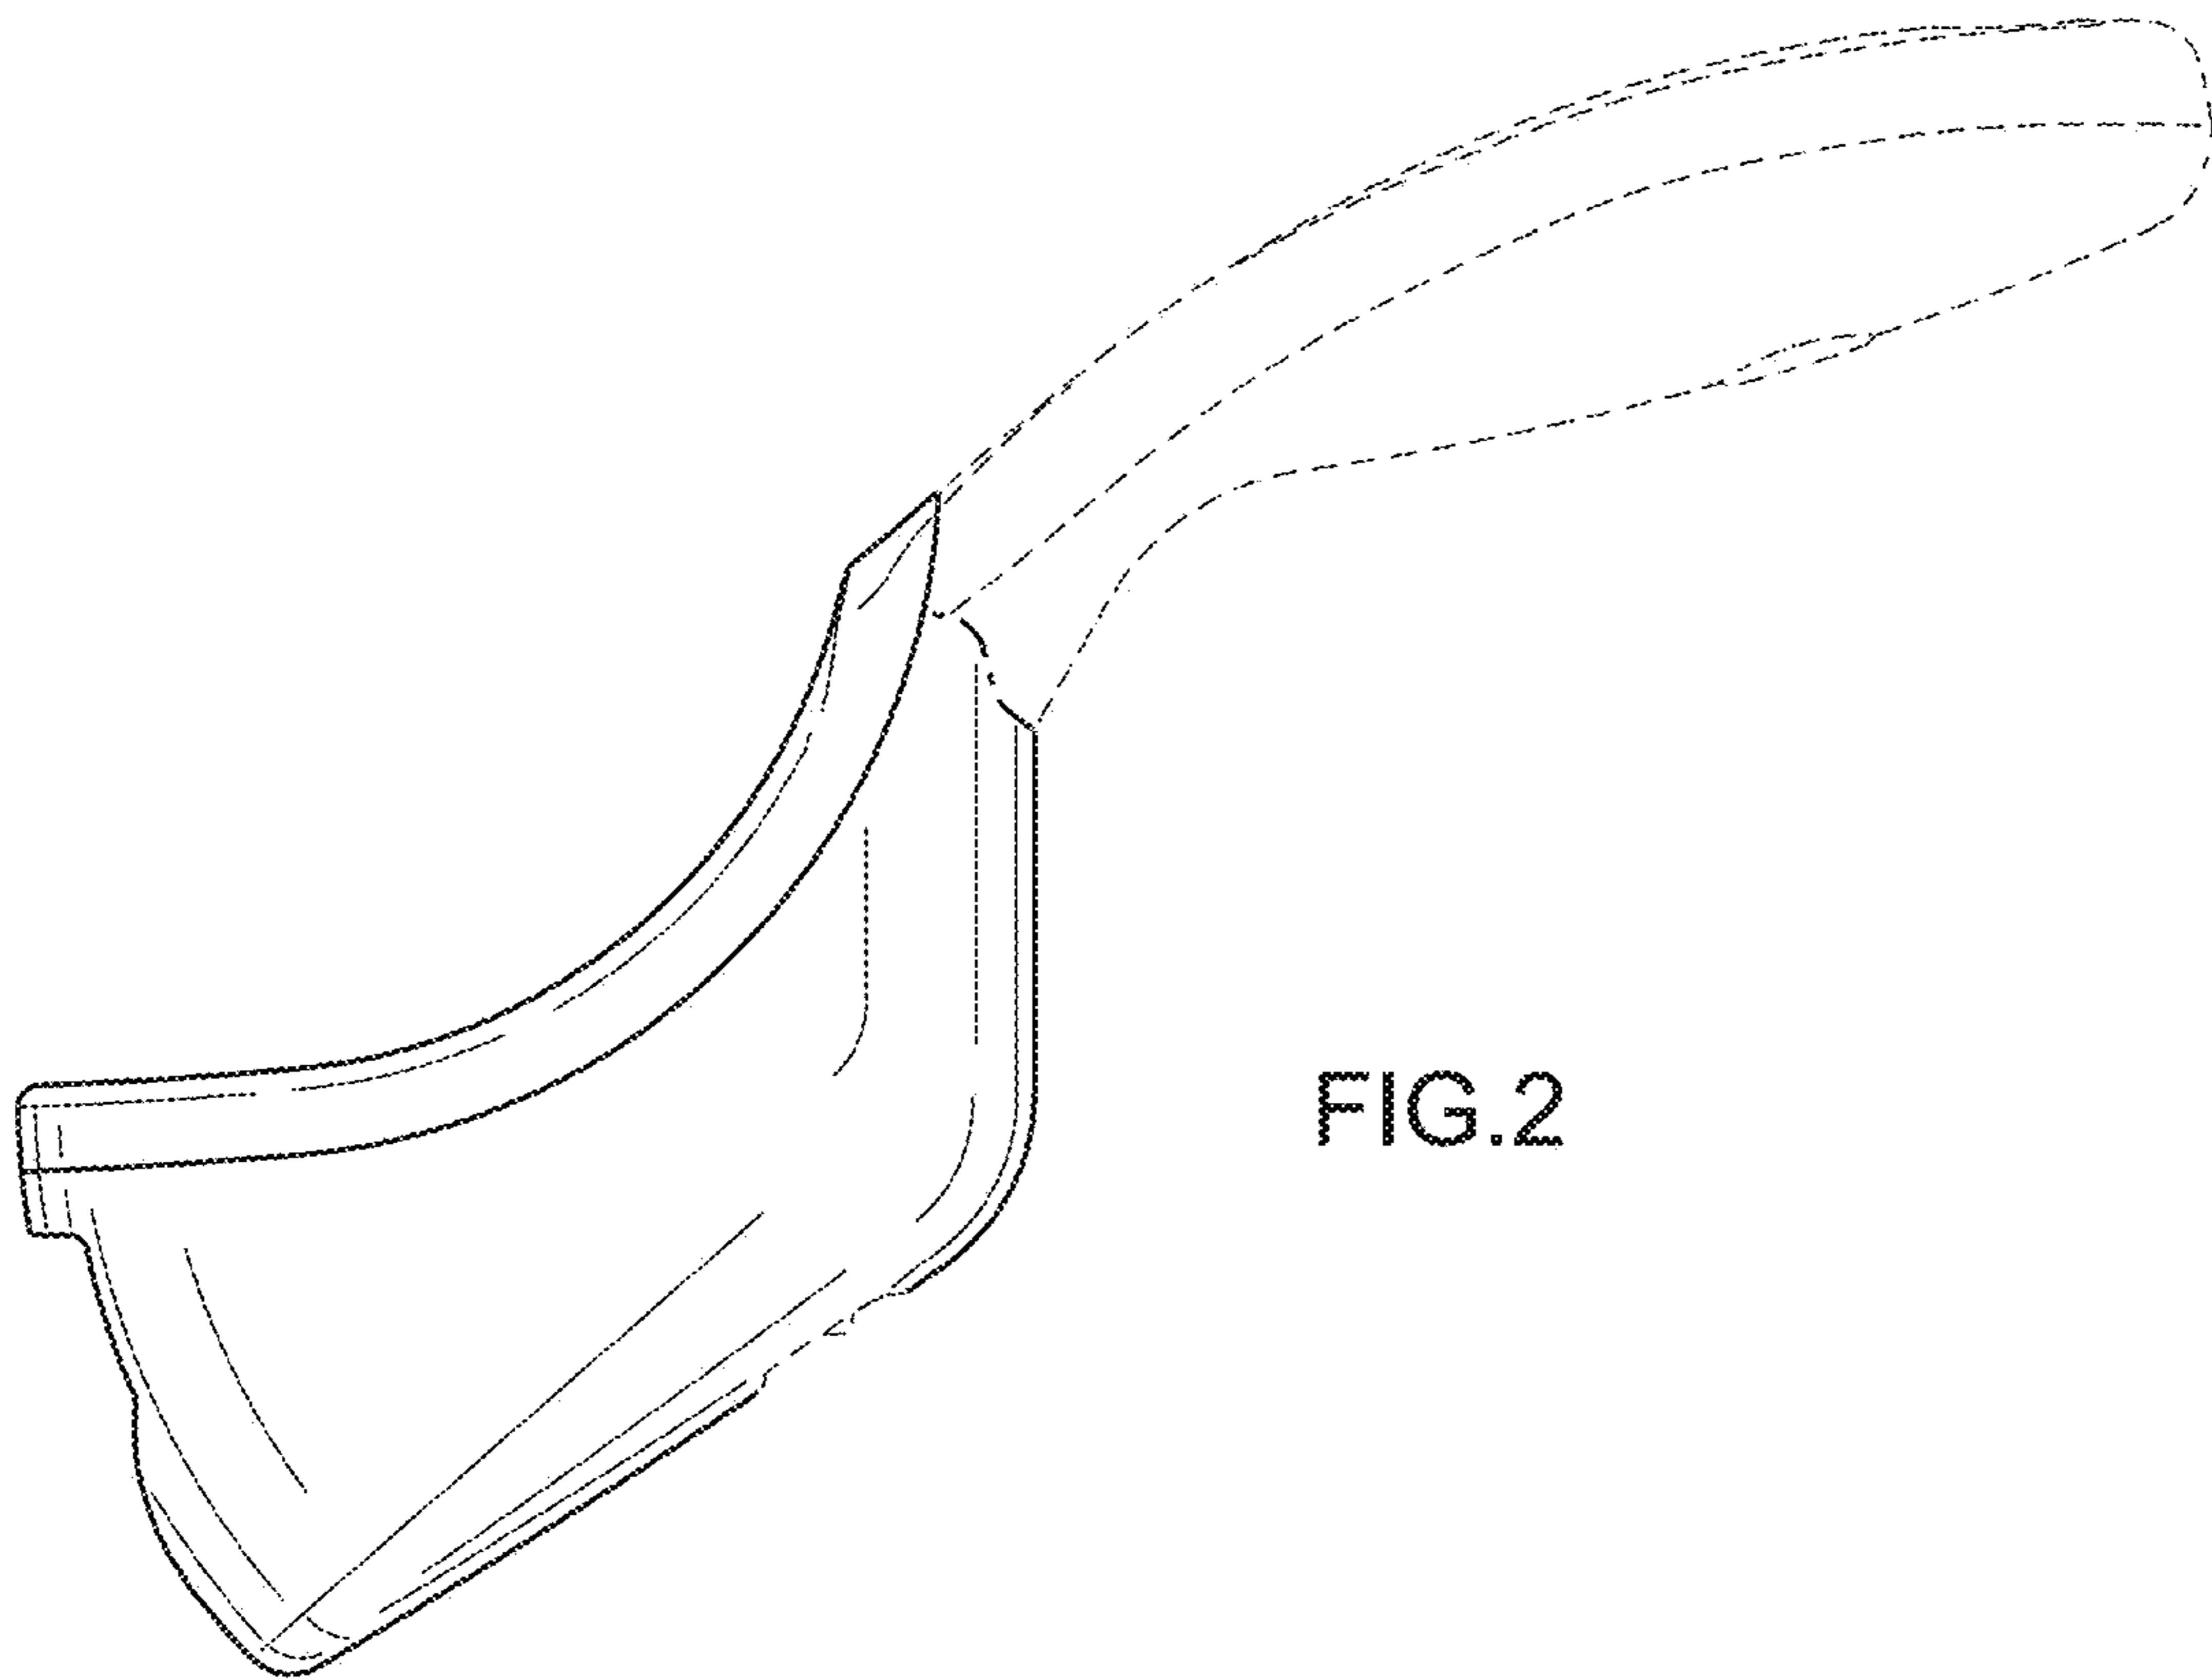


FIG. 2

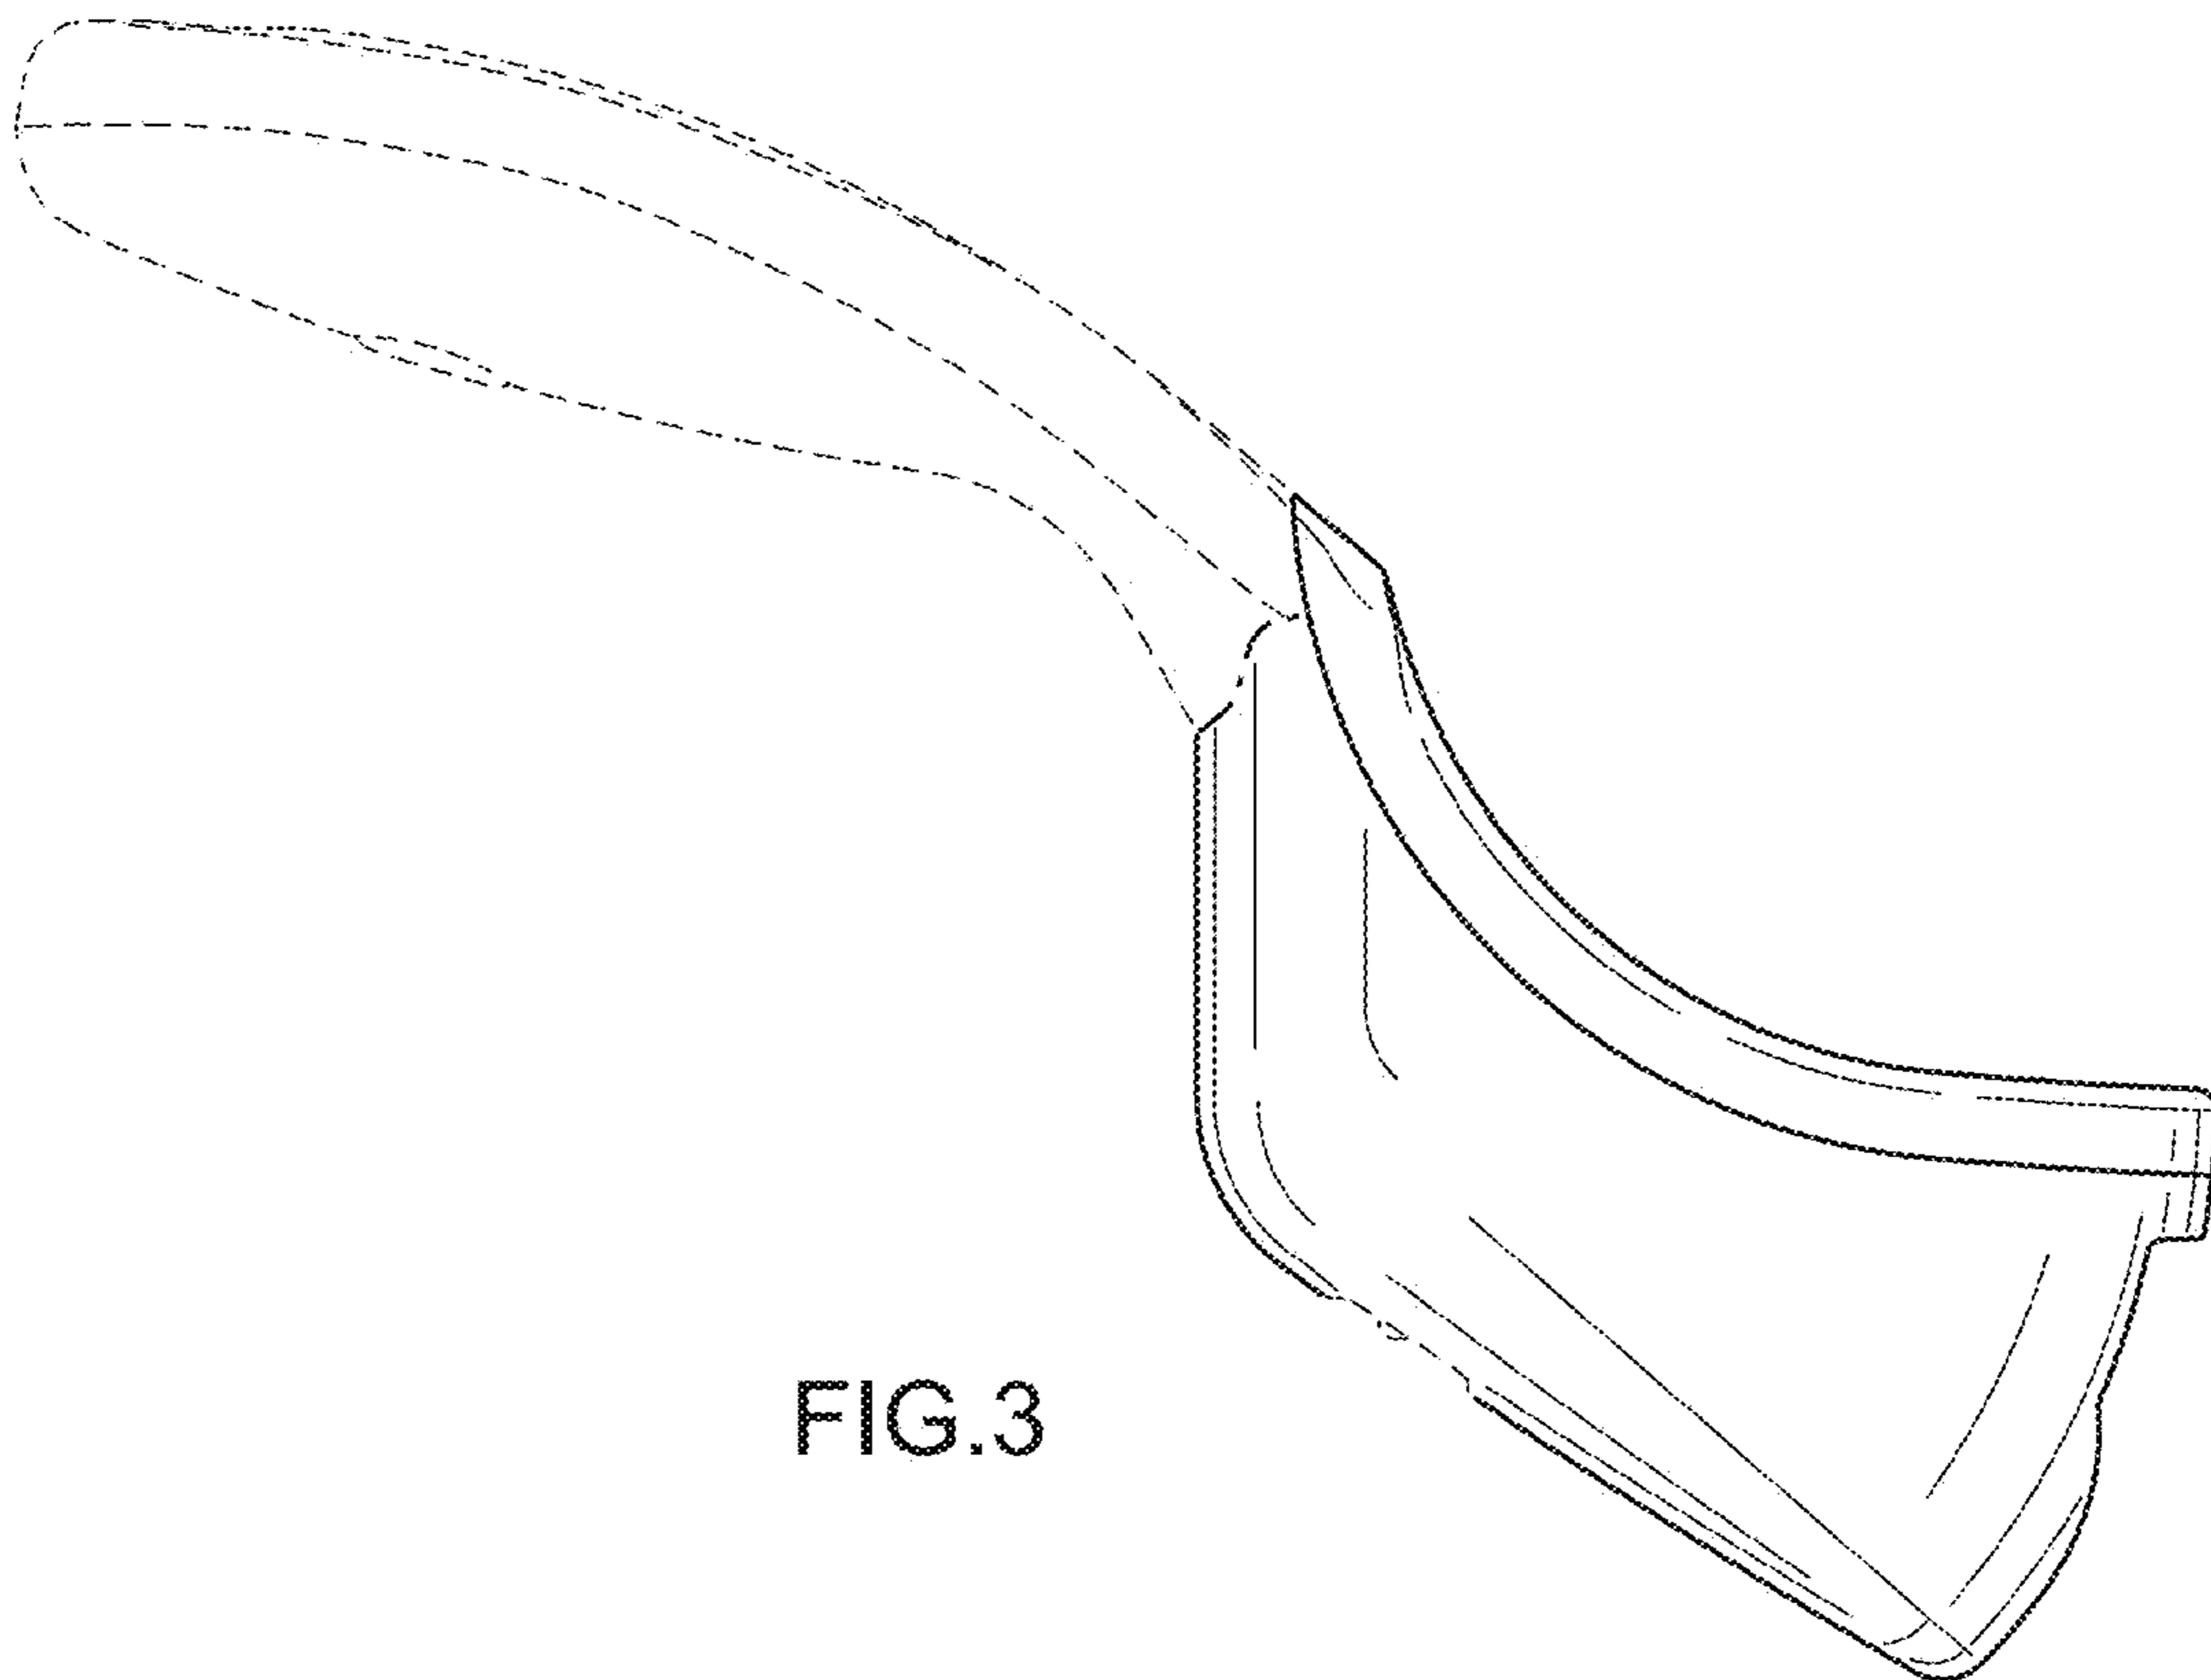


FIG. 3

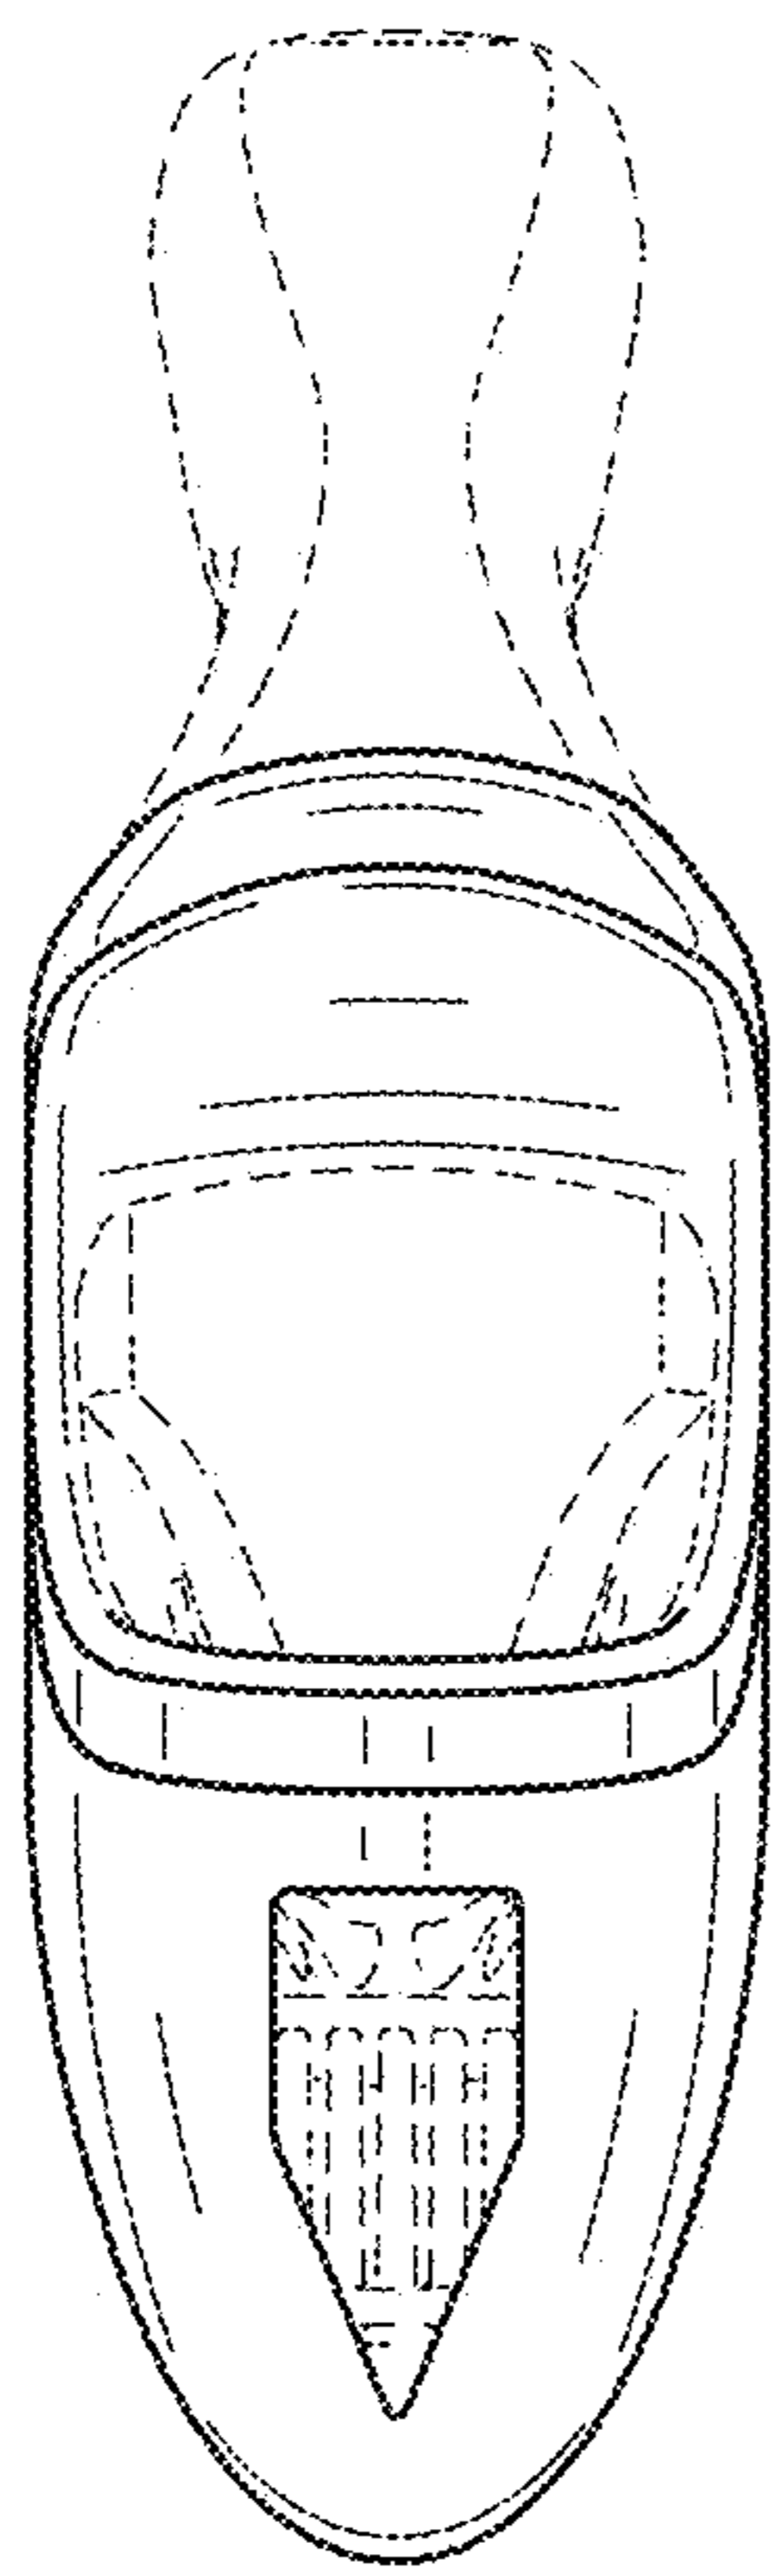


FIG. 4

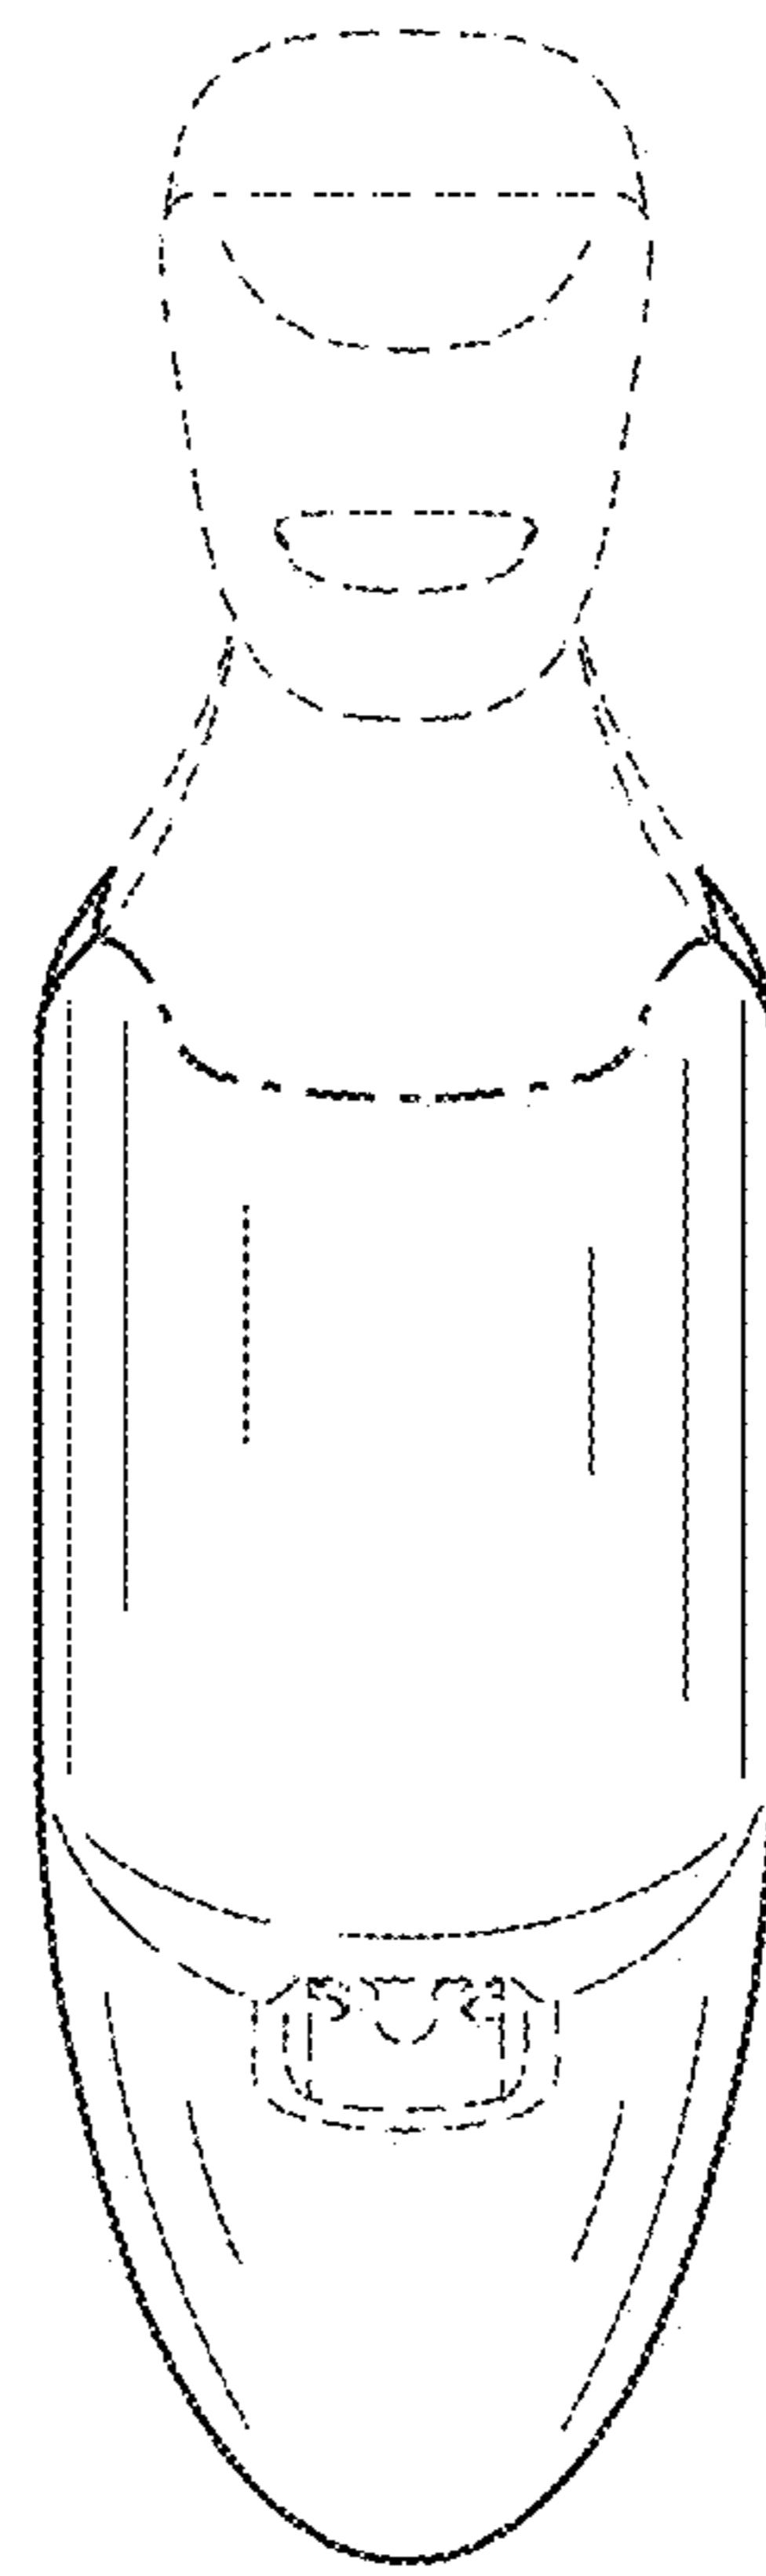


FIG. 5

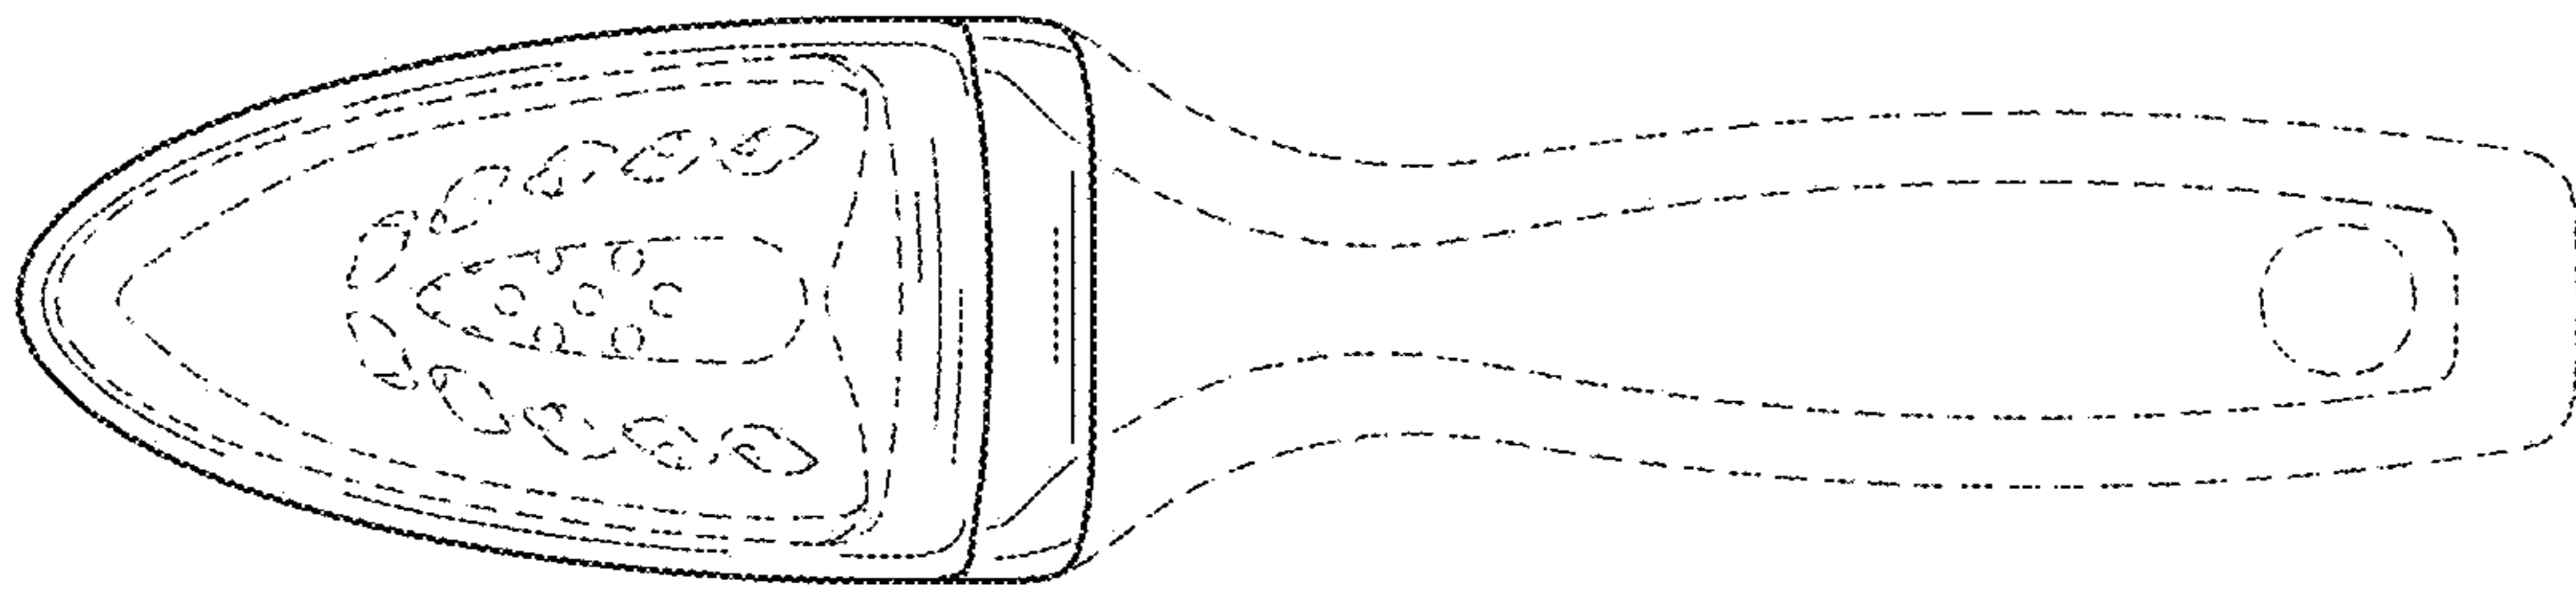


FIG. 6

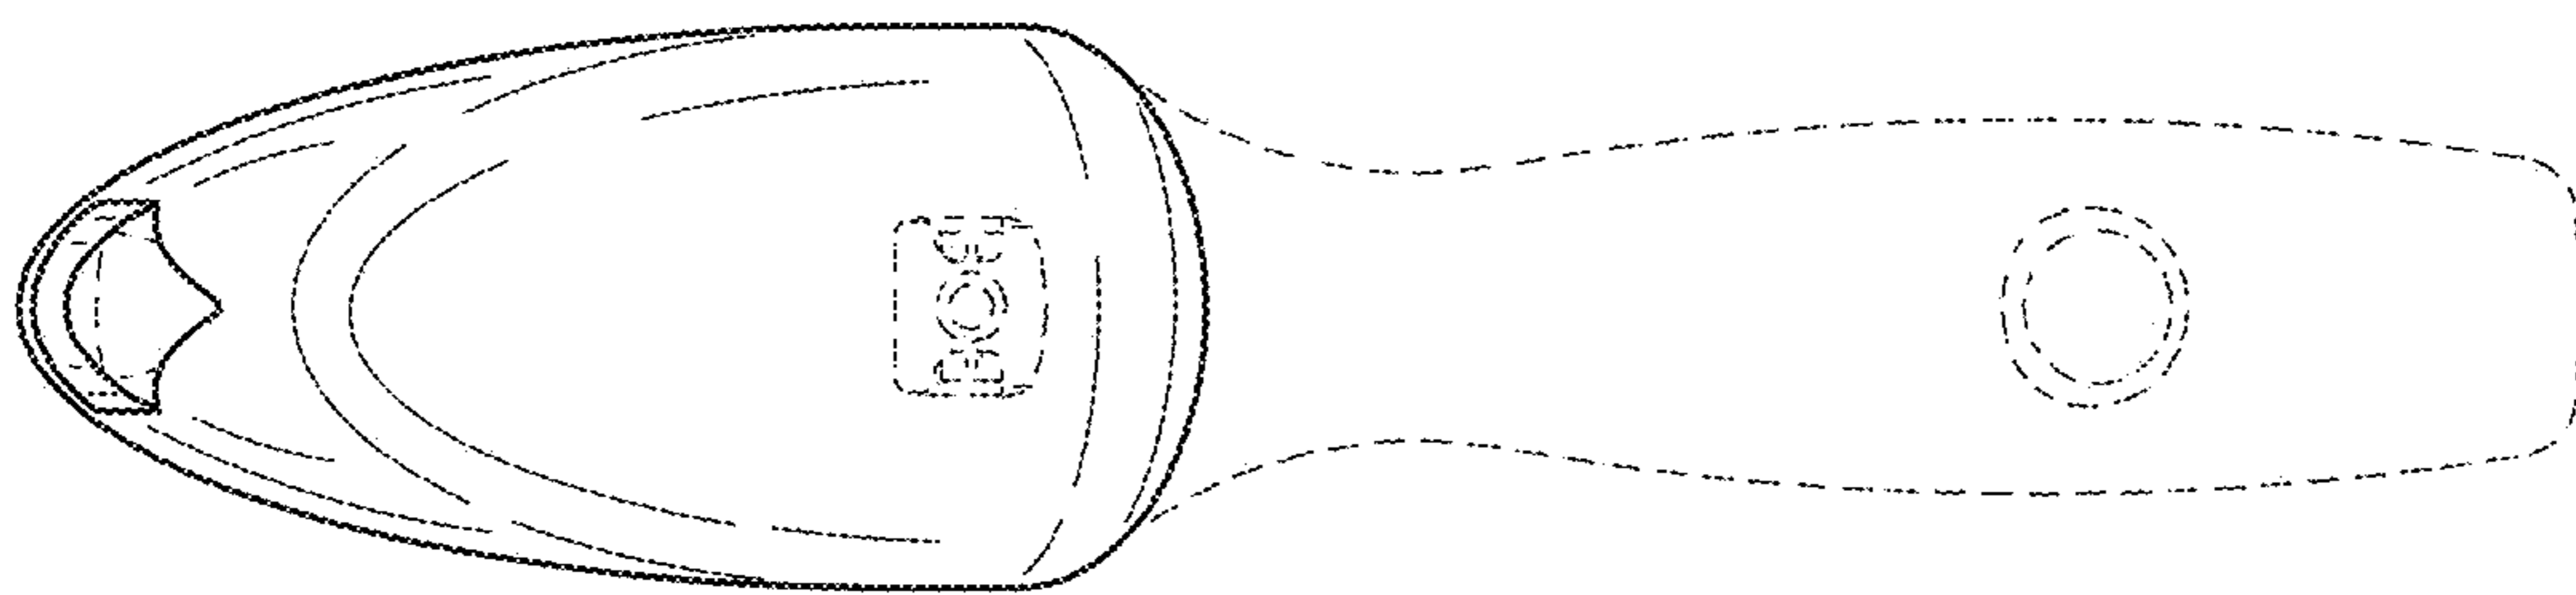


FIG. 7