



US00D933242S

(12) **United States Design Patent** (10) **Patent No.:** **US D933,242 S**
Ito et al. (45) **Date of Patent:** **** Oct. 12, 2021**

(54) **PAD FOR NERVE STIMULATOR DEVICE**

(71) Applicant: **OMRON HEALTHCARE Co., Ltd.**,
Kyoto (JP)

(72) Inventors: **Tamaki Ito**, Kyoto (JP); **Tsuyoshi Ogihara**, Kyoto (JP); **Kosuke Inoue**, Kyoto (JP); **Takashi Shigeno**, Tokyo (JP); **Kazuya Andachi**, Tokyo (JP)

(73) Assignee: **OMRON HEALTHCARE Co., Ltd.**

(**) Term: **15 Years**

(21) Appl. No.: **29/722,285**

(22) Filed: **Jan. 28, 2020**

(30) **Foreign Application Priority Data**

Jul. 29, 2019 (JP) 2019-016884

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/187, 186, 165-168, 200; D13/120,
D13/121; D10/75, 78, 97, 98, 103
CPC A61N 1/04; A61N 1/0404; A61N 1/0452;
A61N 1/0456; A61N 1/0476; A61N
1/048; A61N 1/0484; A61N 1/0492;
A61N 1/18; A61N 1/36014; A61N
1/36021

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D366,317 S * 1/1996 Axelgaard D24/168
D456,907 S * 5/2002 Sanfilippo D24/187
D471,281 S * 3/2003 Baura D24/187
D495,055 S * 8/2004 Silber D24/187
D558,352 S * 12/2007 Sanfilippo D24/187
D665,085 S * 8/2012 Strother D24/187

D831,830 S * 10/2018 Lemons D24/168
D889,662 S * 7/2020 Hubelbank D24/168
2013/0096641 A1 * 4/2013 Strother A61N 1/36021
607/46
2013/0226275 A1 * 8/2013 Duncan A61N 1/0492
607/152
2016/0008609 A1 * 1/2016 Chen A61N 1/37217
607/59

FOREIGN PATENT DOCUMENTS

CN 305906865 * 7/2020
KR 301085560.0000 * 12/2020

OTHER PUBLICATIONS

TENS Electrodes by Discount TENS store. Amazon. Oldest review date: Oct. 9, 2019. Date retrieved: Jan. 13, 2021. Retrieved from internet: <https://www.amazon.com/TENS-Electrodes-Adhesive-Butterfly-Discount/dp/B07QPW8P3M> (Year: 2019).*

(Continued)

Primary Examiner — Lilyana Bekic

Assistant Examiner — Lee D. Starr

(74) *Attorney, Agent, or Firm* — Saidman DesignLaw Group, LLC


(57) **CLAIM**

The ornamental design for a pad for nerve stimulator device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a pad for nerve stimulator device showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a bottom view thereof;
FIG. 6 is a right side view thereof; and,
FIG. 7 is a left side view thereof.

1 Claim, 5 Drawing Sheets

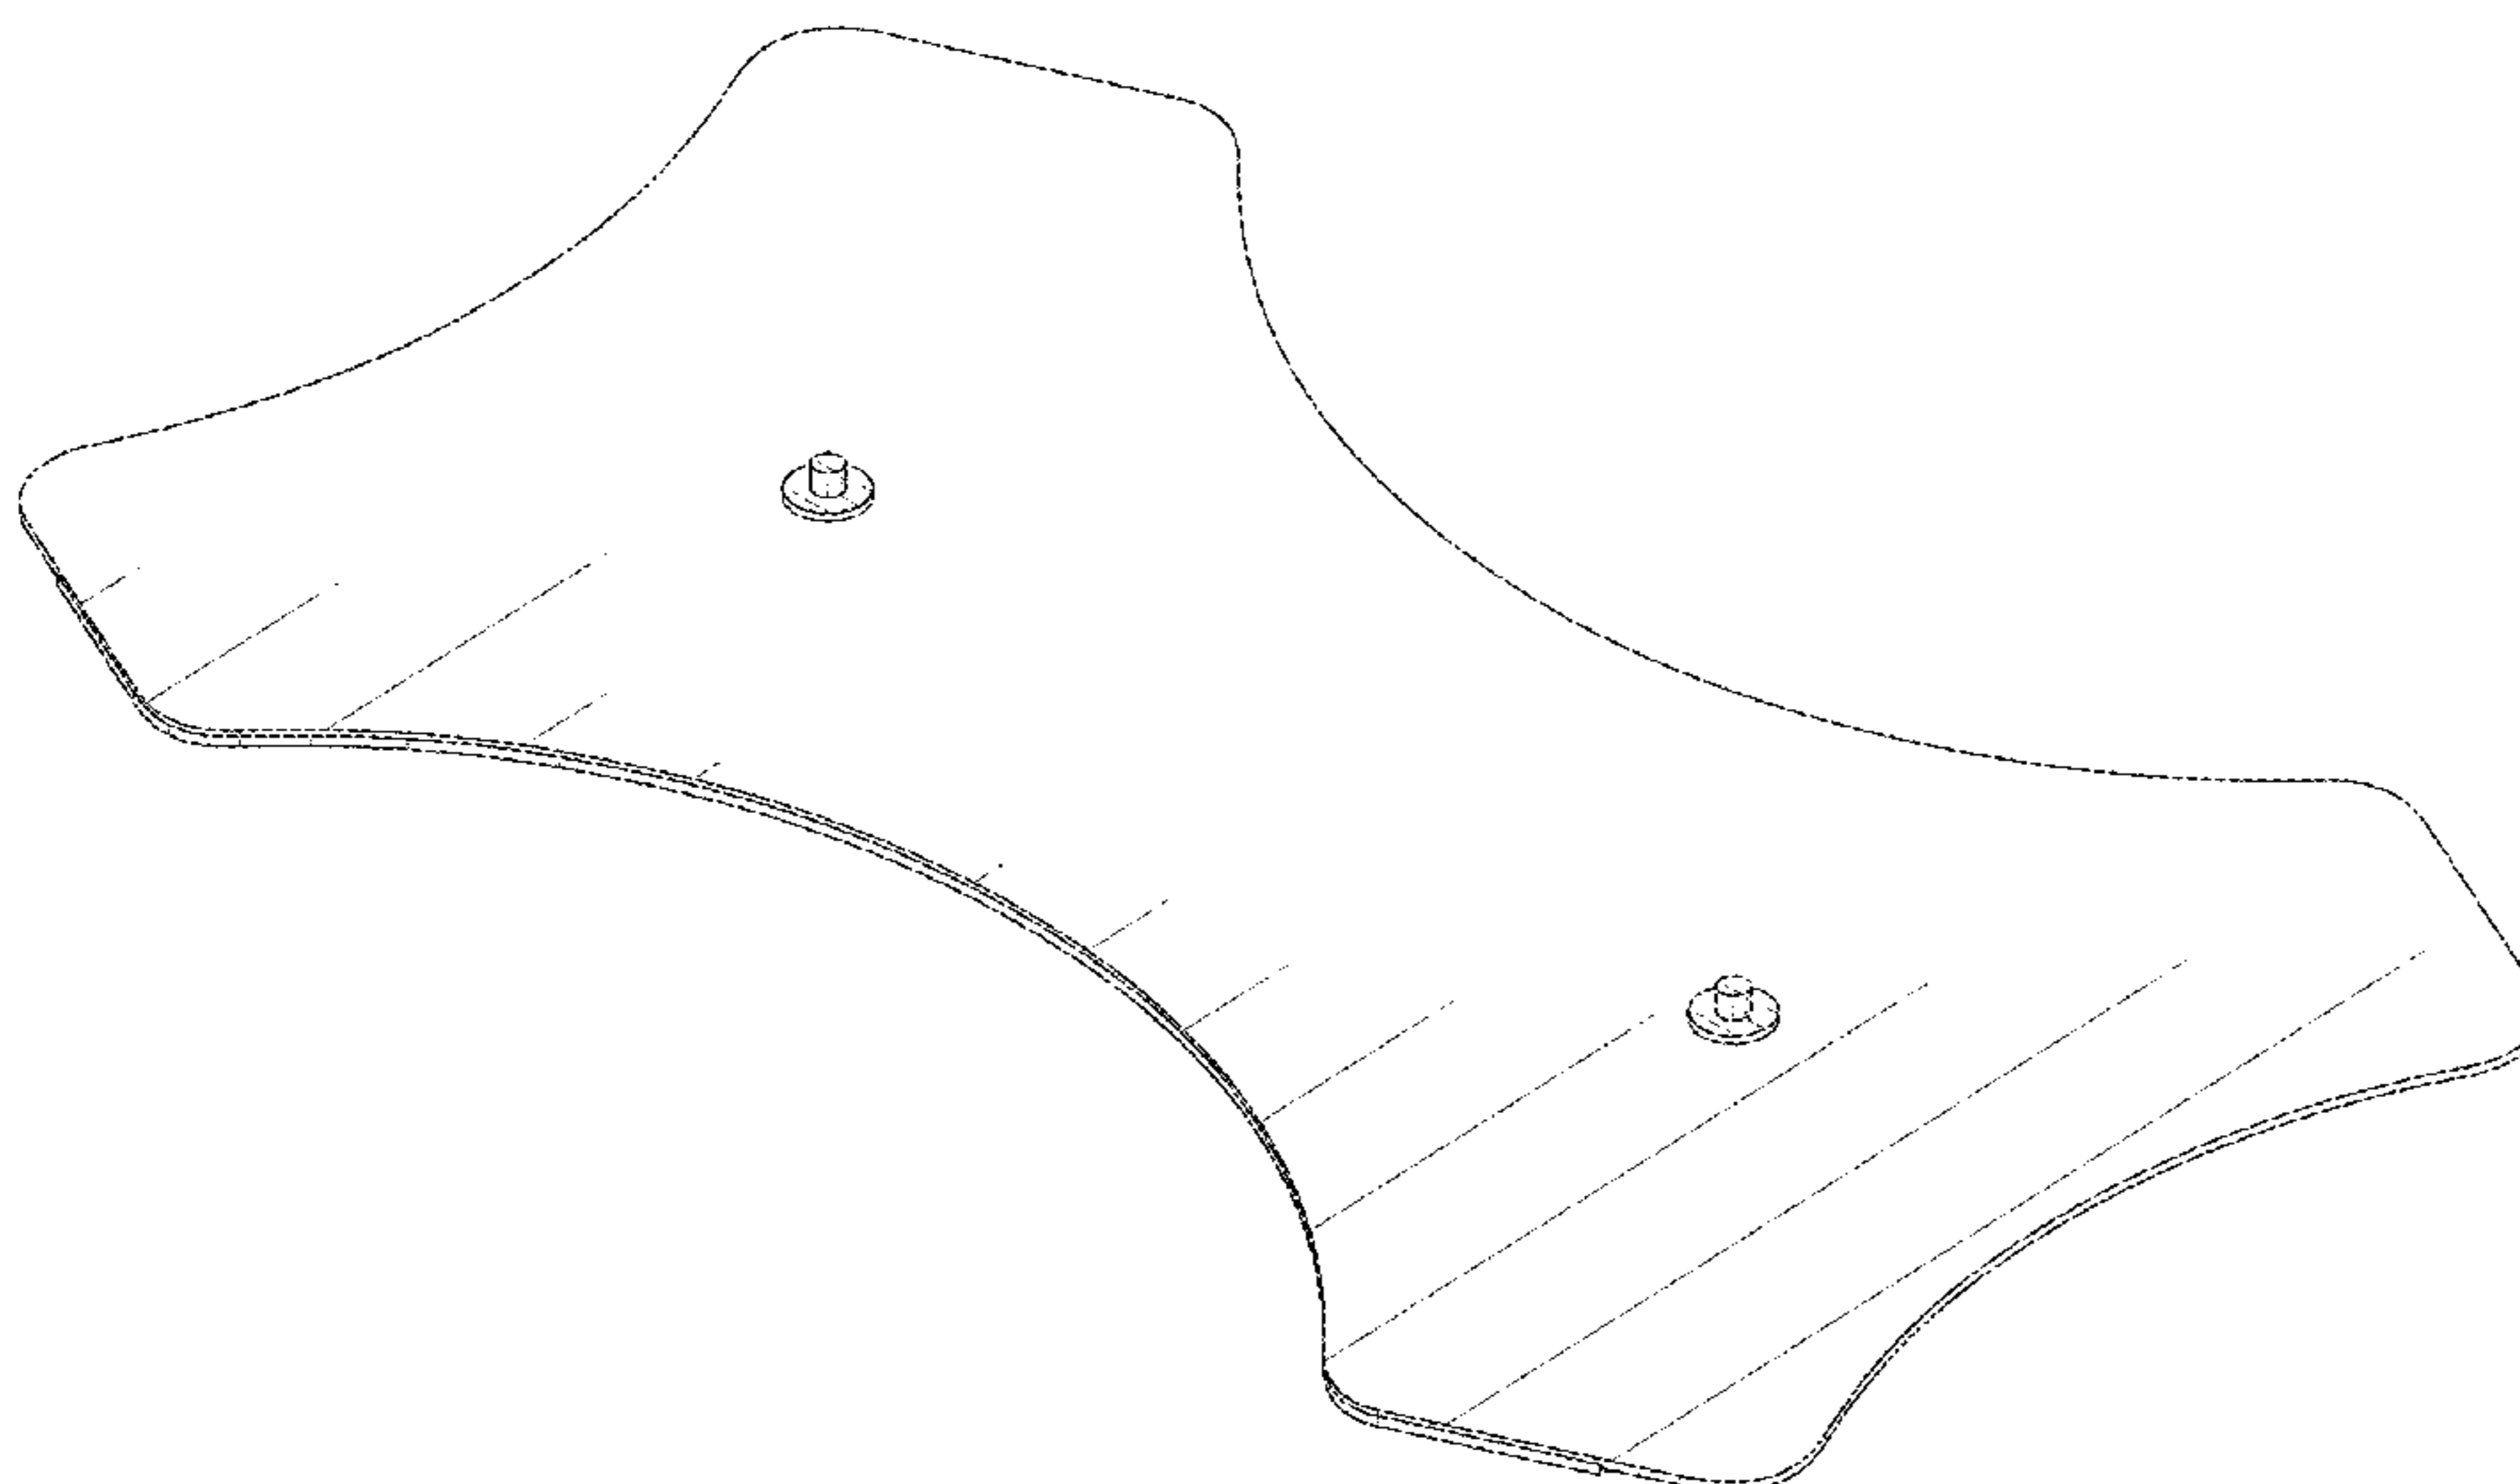

(56)

References Cited

OTHER PUBLICATIONS

Mini Wireless Electrode Pads by iReliev. ireliev.com. Oldest review date: Dec. 10, 2018. Date retrieved: Jan. 13, 2021. Retrieved from internet: <https://staging.ireliev.com/product/mini-tens-electrode-pads/> (Year: 2018).*

* cited by examiner

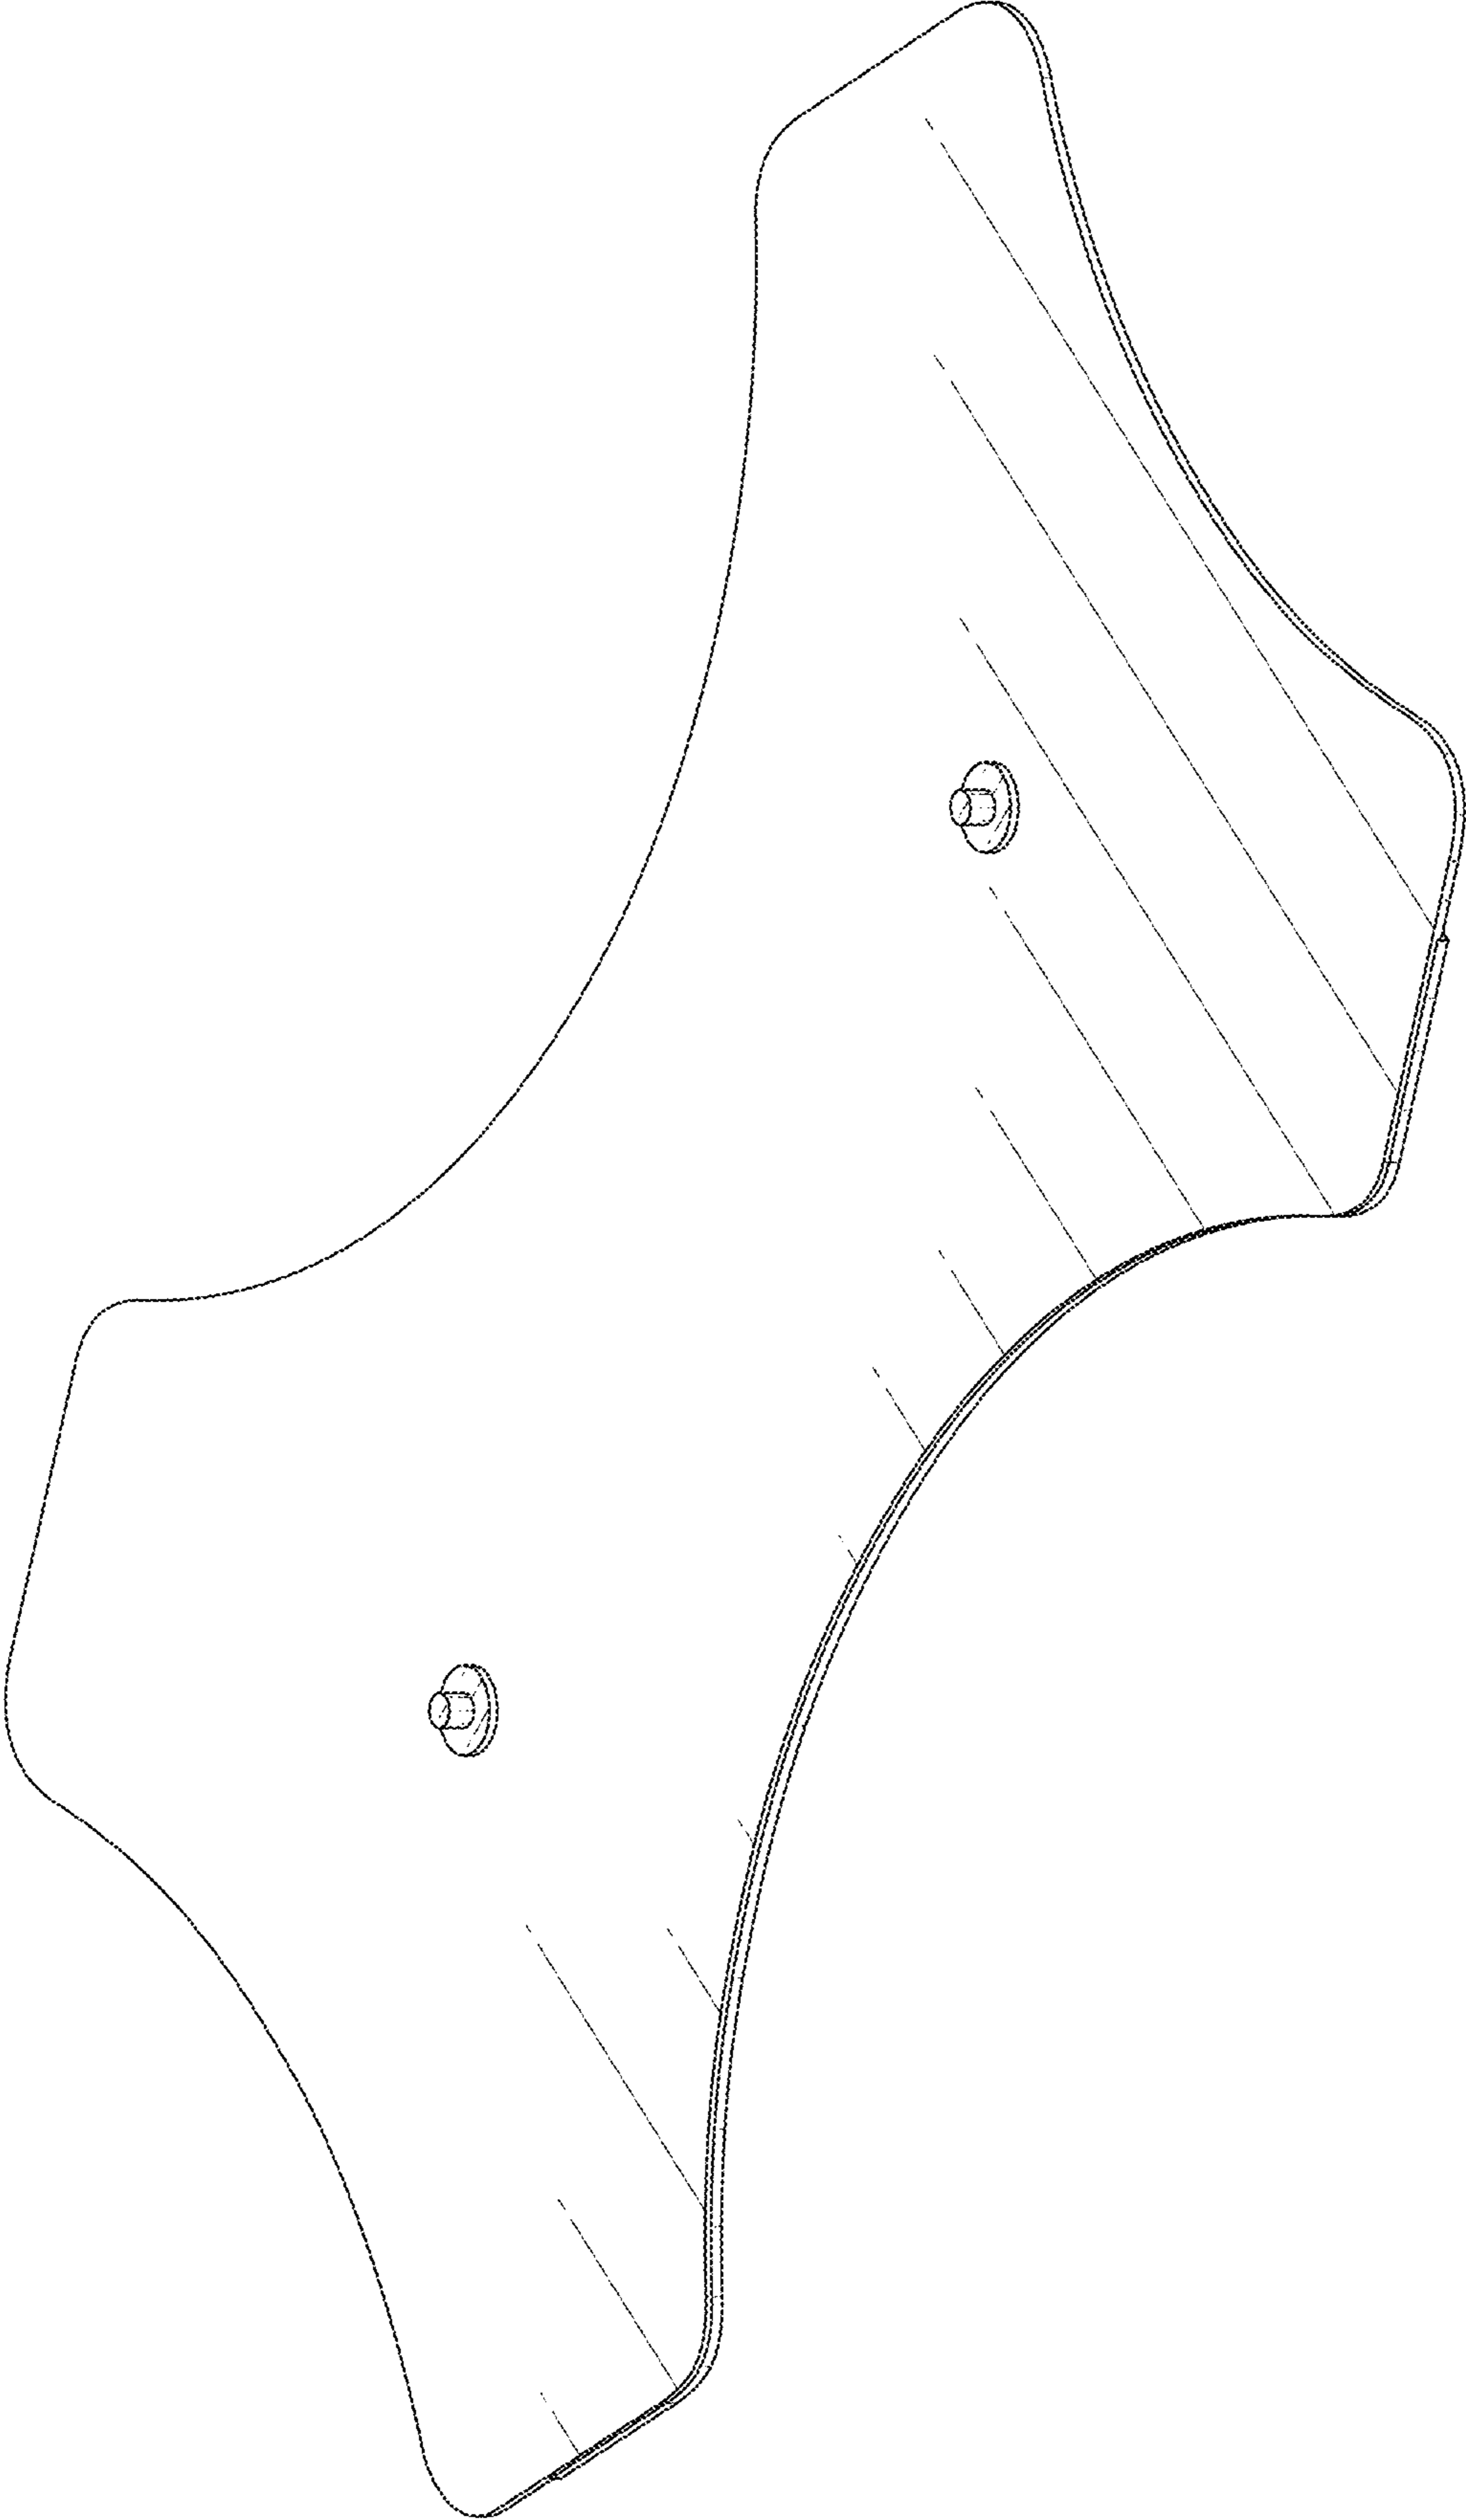


FIG. 1

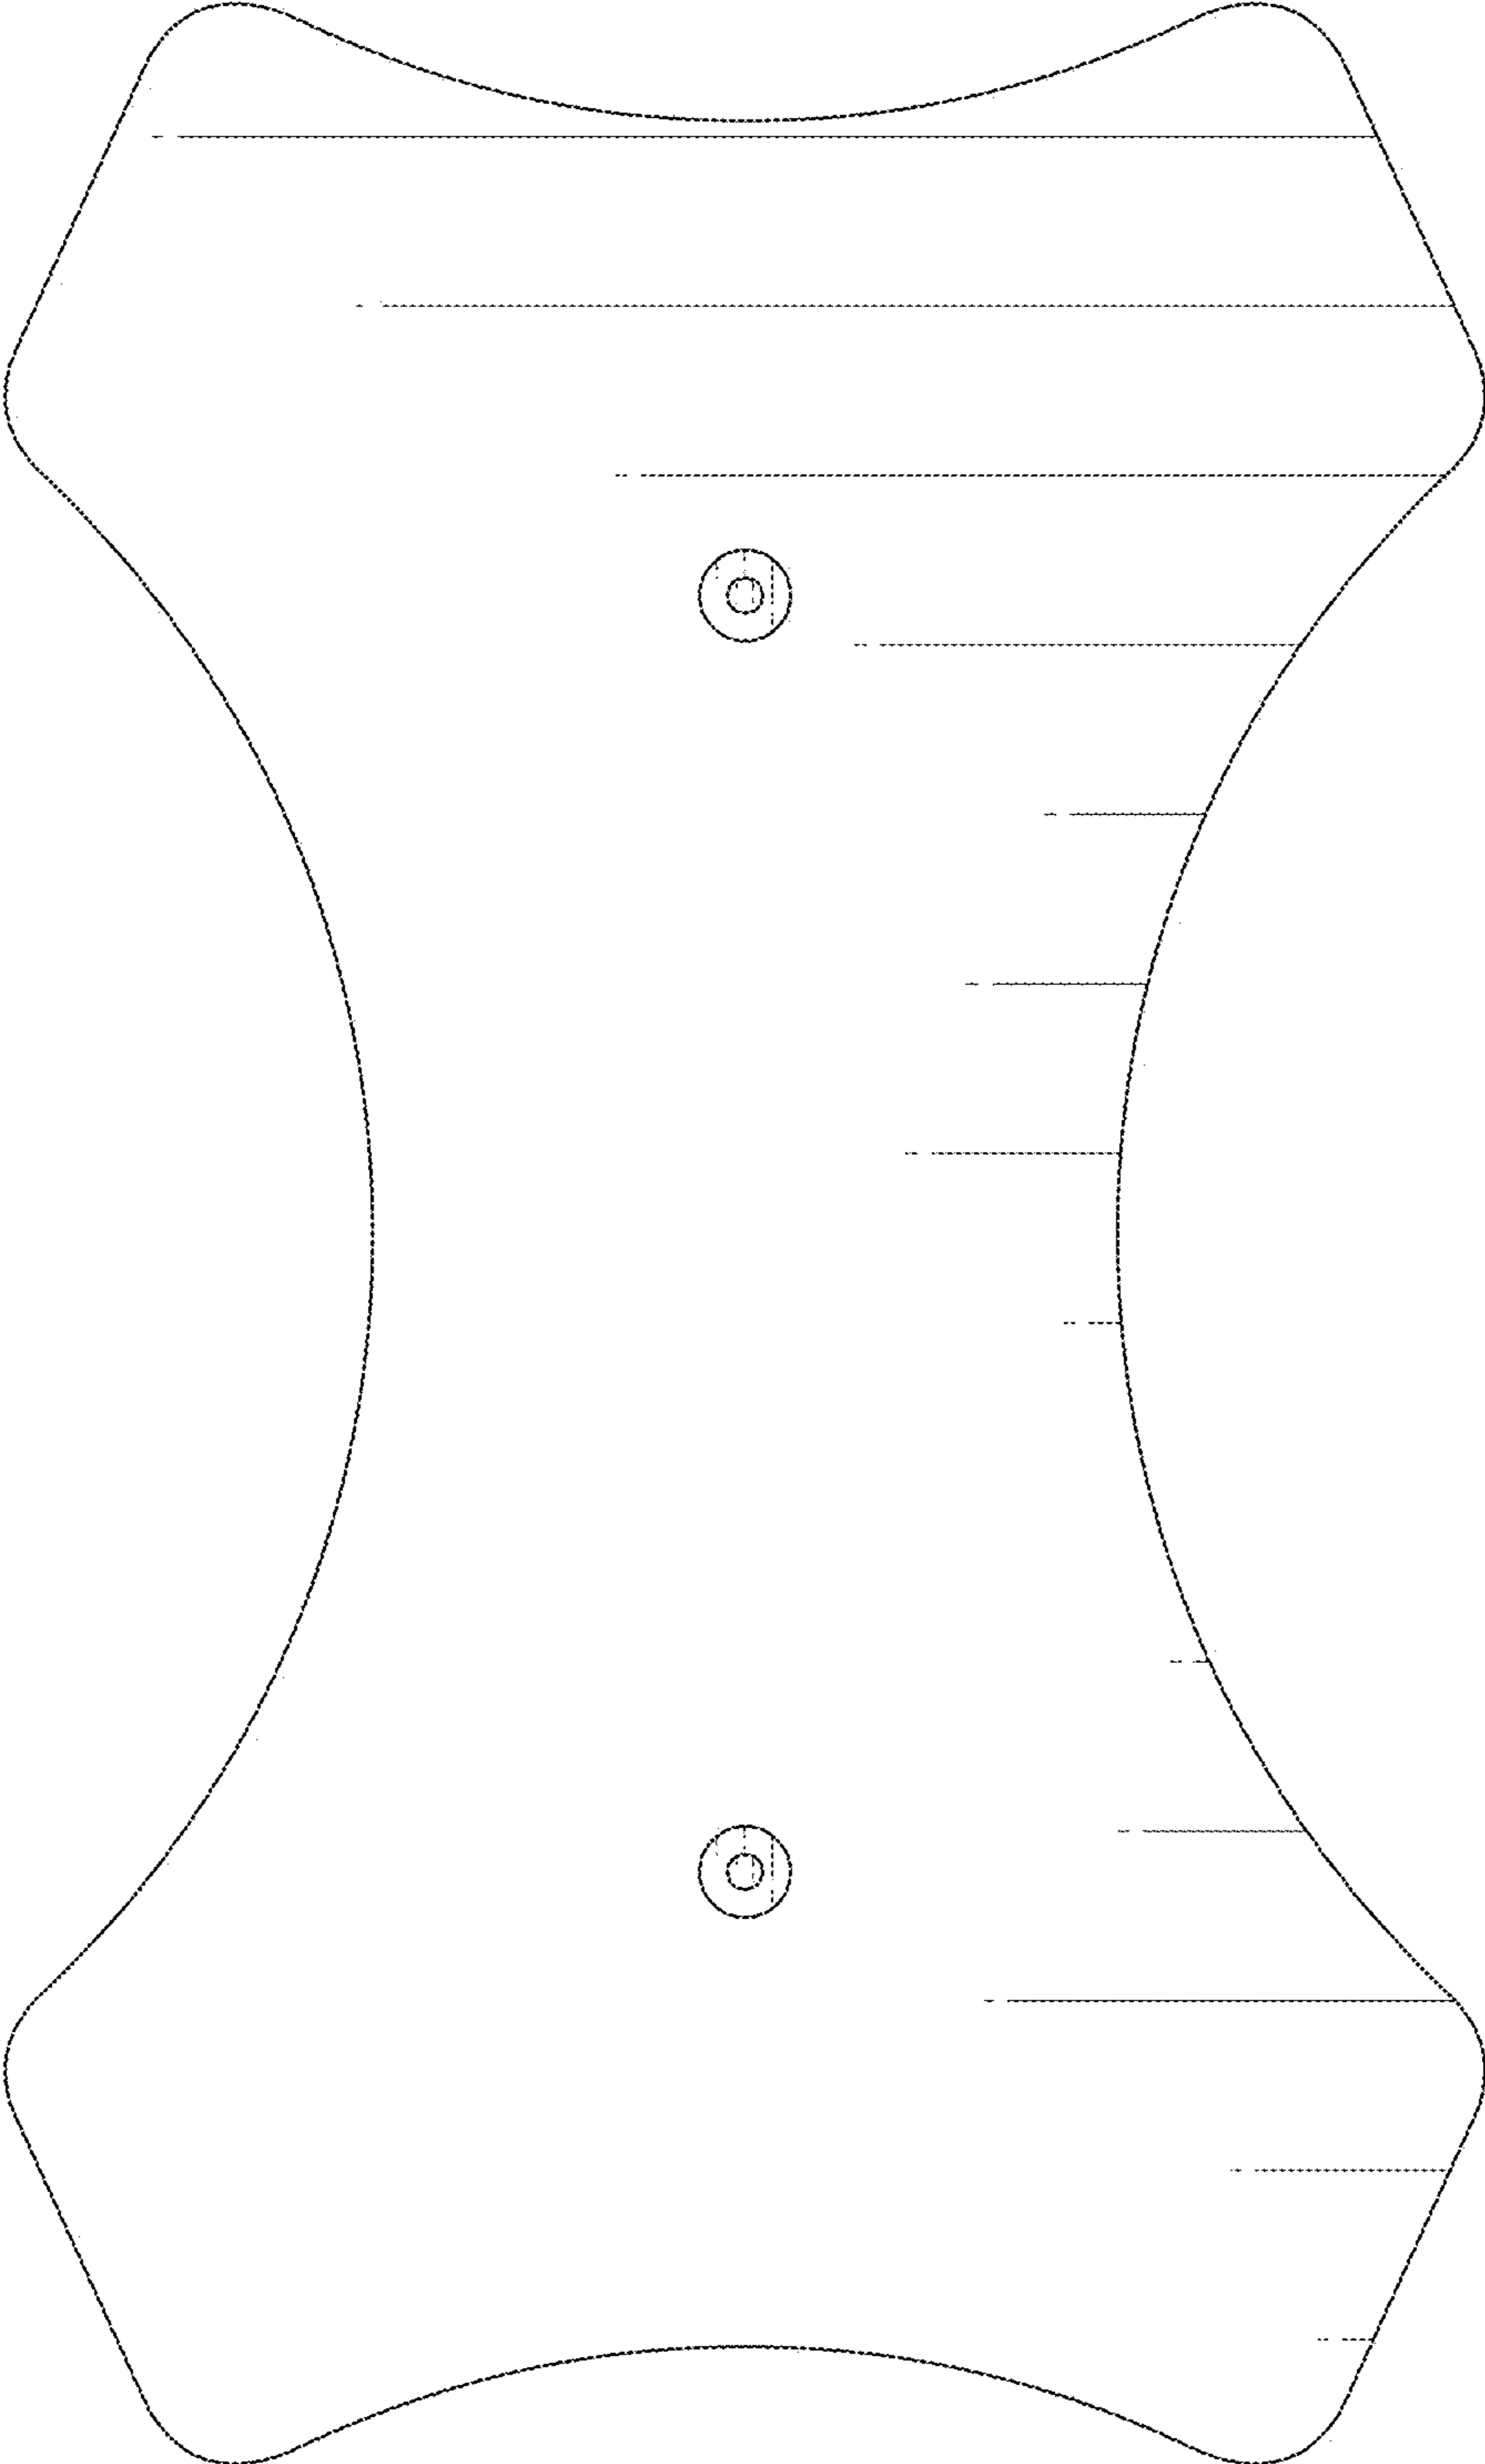


FIG. 2

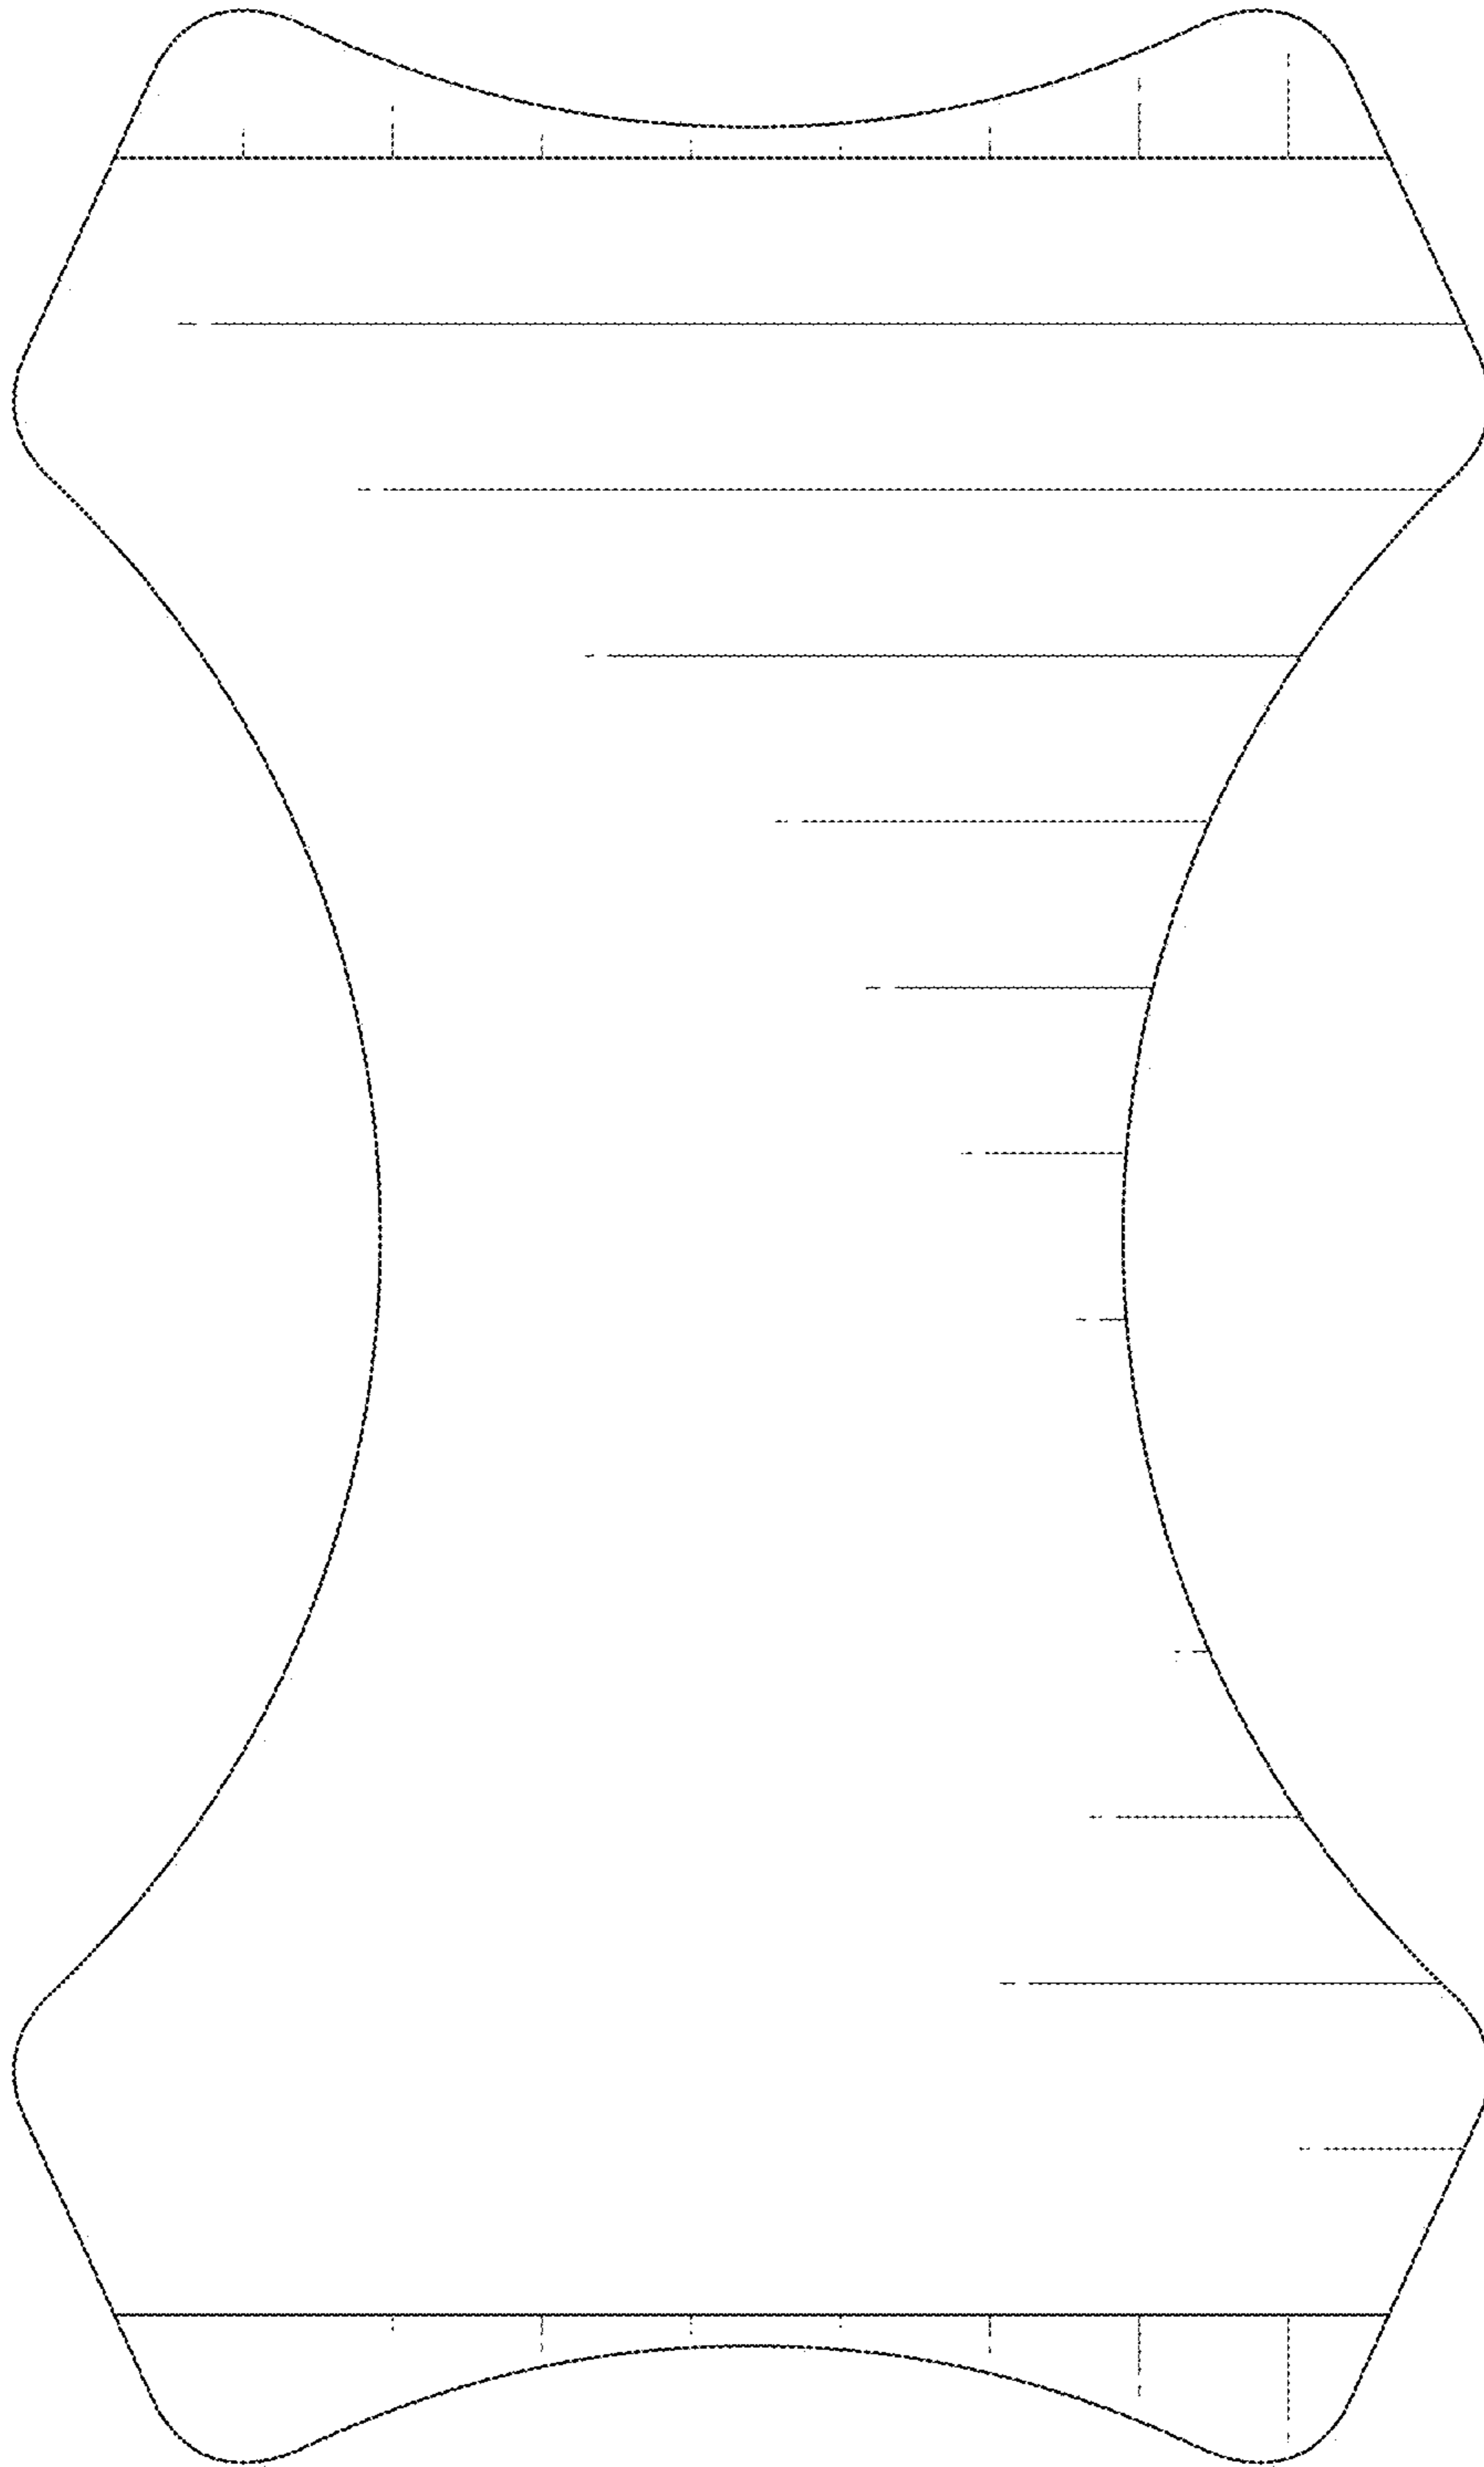


FIG. 3

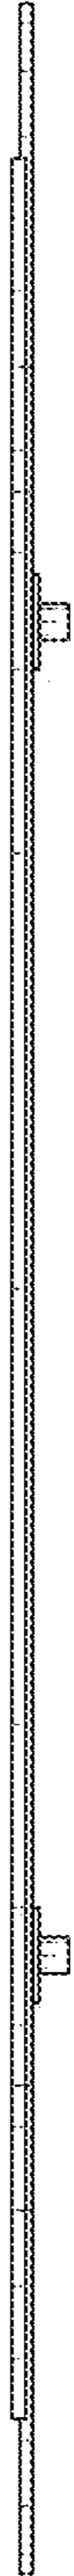


FIG. 4



FIG. 5

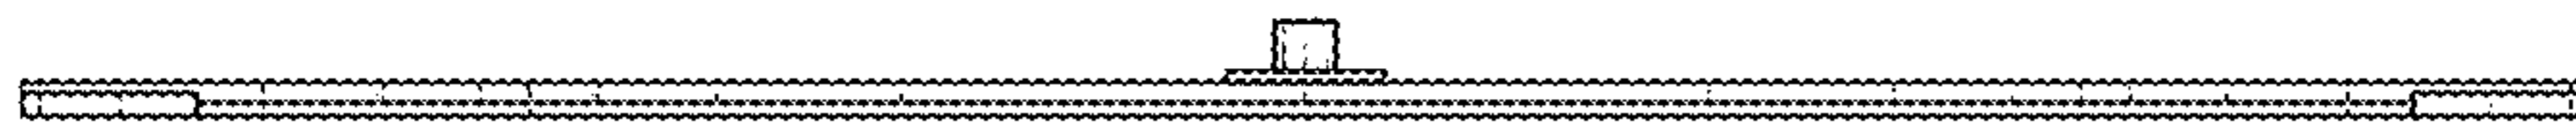


FIG. 7



FIG. 6