

US00D936843S

(12) **United States Design Patent** (10) **Patent No.:** **US D936,843 S**  
**Besko et al.** (45) **Date of Patent:** **\*\* Nov. 23, 2021**

(54) **MEDICAL SENSOR**

FOREIGN PATENT DOCUMENTS

- (71) Applicant: **Covidien LP**, Mansfield, MA (US)
- (72) Inventors: **David P. Besko**, Thornton, CO (US);  
**Timothy W. Fries**, Louisville, CO (US)
- (73) Assignee: **COVIDIEN LP**, Mansfield, MA (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/704,952**
- (22) Filed: **Sep. 9, 2019**

- EP 1945099 A1 7/2008
- JP H0616774 A 1/1994
- (Continued)

OTHER PUBLICATIONS

Nellcor Oximax DS100A Adult Neonatal Disposable oxygen sensor. Online, published date unknown. Retrieved on 12/21/218 from URL: <https://www.alibaba.com/product-detail/Nellcor-Oximax-DS-100A-Adult-Neonatal-Disposable-60609345689.html> (1 pp.).

(Continued)

**Related U.S. Application Data**

- (62) Division of application No. 29/618,332, filed on Sep. 20, 2017, now Pat. No. Des. 862,709.
- (51) **LOC (13) Cl.** ..... **24-02**
- (52) **U.S. Cl.**  
USPC ..... **D24/187**
- (58) **Field of Classification Search**  
USPC ..... D24/165, 167, 168, 186, 187; D13/133,  
D13/147; D10/56, 60, 97  
CPC ... A61B 5/1455; A61B 5/6833; A61B 5/6843;  
A61B 5/14552; A61B 5/02438; A61M  
25/0127; A42B 1/242  
See application file for complete search history.

*Primary Examiner* — Michael C Stout  
*Assistant Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

(57) **CLAIM**

We claim the ornamental design for a medical sensor, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the medical sensor of the present invention;  
FIG. 2 is a top view of the medical sensor of FIG. 1;  
FIG. 3 is a bottom view of the medical sensor of FIG. 1;  
FIG. 4 is a right side view of the medical sensor of FIG. 1;  
FIG. 5 is a left side view of the medical sensor of FIG. 1;  
FIG. 6 is a front view of the medical sensor of FIG. 1; and,  
FIG. 7 is a rear view of the medical sensor of FIG. 1.  
The broken away symbols in the drawings indicate that any portion of the article beyond what is shown forms no part of the claimed design.  
The thick broken lines in the figures are claimed features of the design. The thin broken lines in FIGS. 2 and 3 depict portions of the medical sensor that form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,825,879 A 5/1989 Tan et al.
- 4,865,038 A 9/1989 Rich et al.
- 4,964,408 A 10/1990 Hink et al.
- 5,069,213 A 12/1991 Polczynski
- 5,154,175 A 10/1992 Gunther
- 5,228,440 A 7/1993 Chung et al.
- 5,249,576 A 10/1993 Goldberger
- 5,287,853 A 2/1994 Wester et al.

(Continued)

**1 Claim, 5 Drawing Sheets**

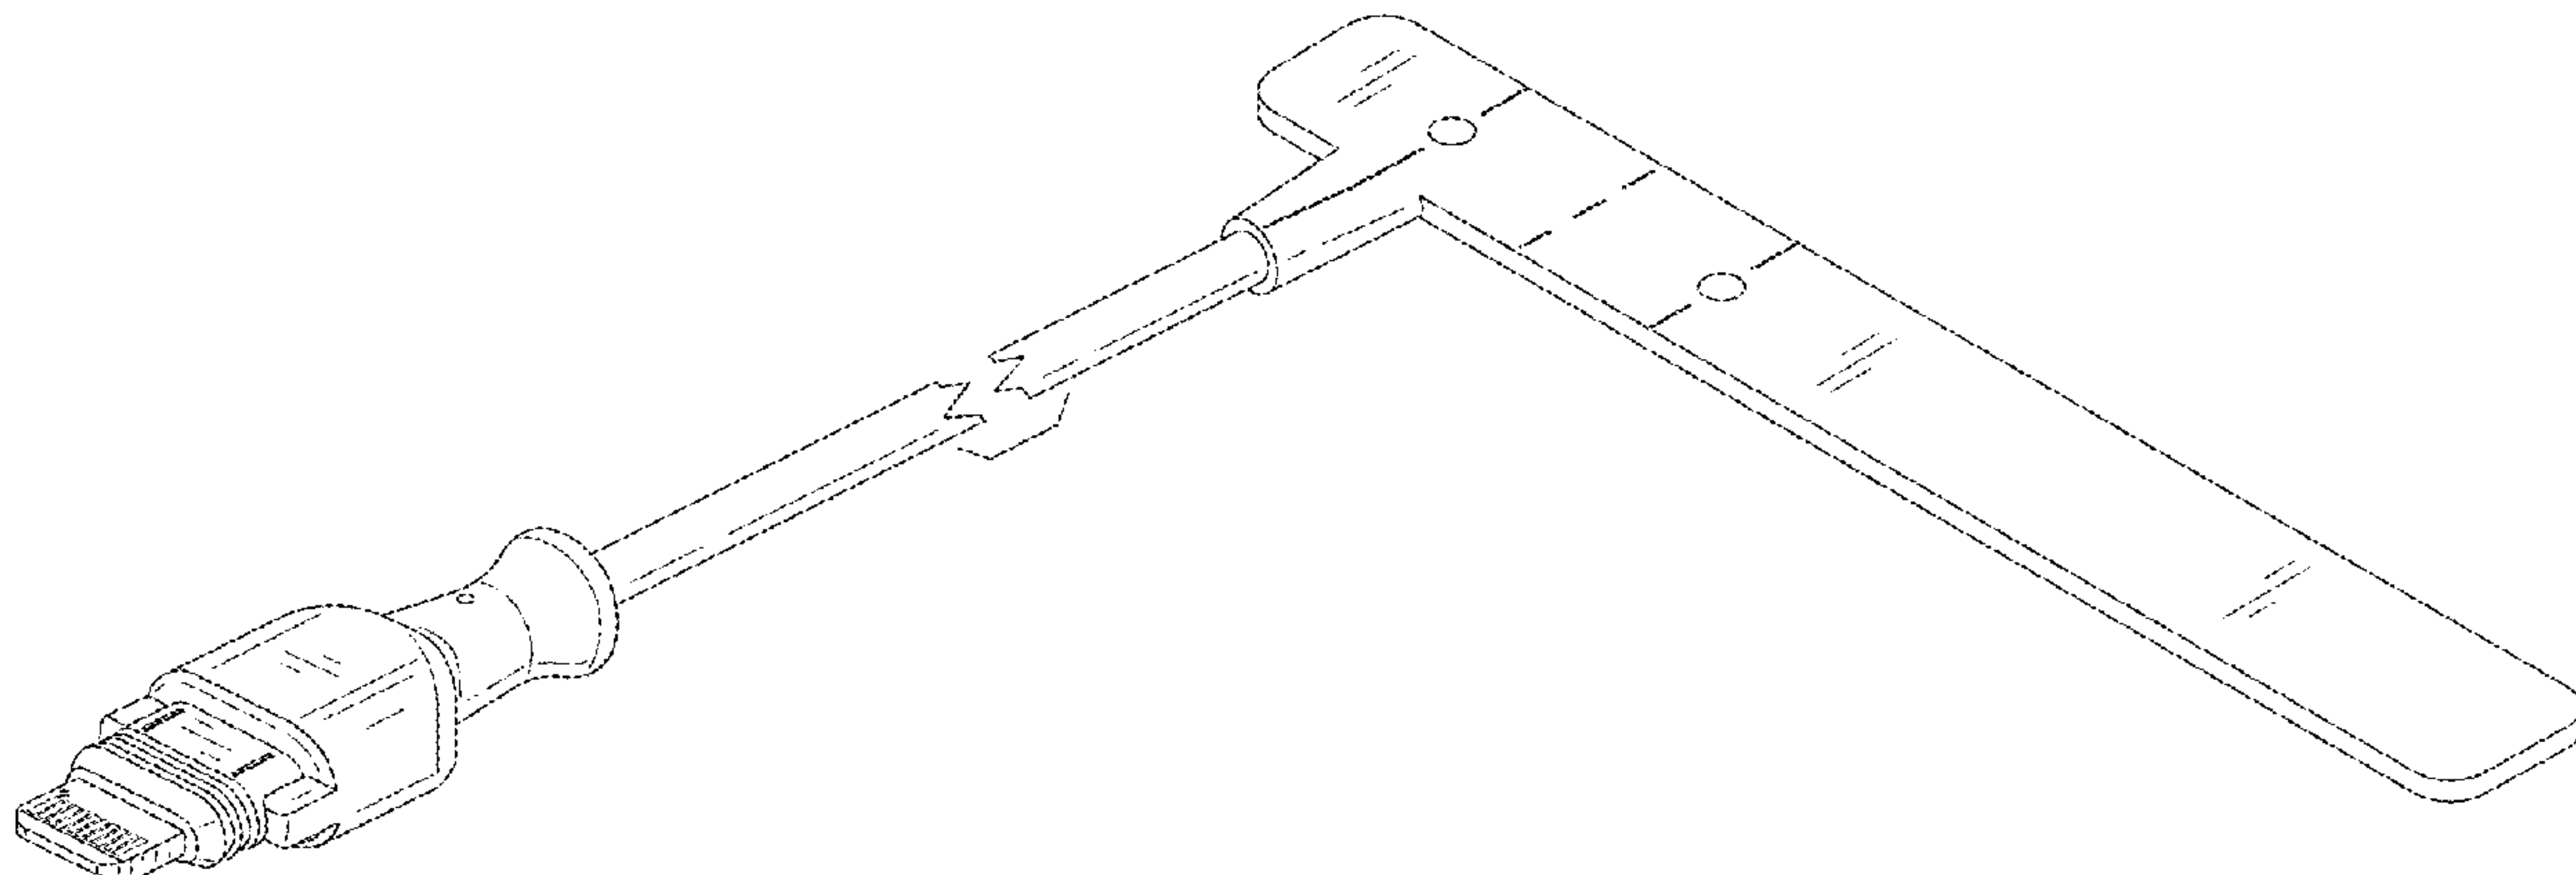

(56)

References Cited

U.S. PATENT DOCUMENTS

5,343,869 A 9/1994 Pross et al.  
 5,387,122 A 2/1995 Goldberger et al.  
 5,425,362 A 6/1995 Siker et al.  
 D366,528 S 1/1996 Crouse et al.  
 5,491,299 A 2/1996 Naylor  
 5,645,440 A 7/1997 Tobler et al.  
 5,660,567 A 8/1997 Nierlich et al.  
 5,743,260 A 8/1998 Chung et al.  
 5,790,729 A 8/1998 Pologe et al.  
 5,851,178 A 12/1998 Aronow  
 5,890,929 A 4/1999 Mills et al.  
 5,934,925 A 8/1999 Tobler et al.  
 5,961,452 A 10/1999 Chung et al.  
 5,997,343 A 12/1999 Mills et al.  
 6,014,576 A 1/2000 Raley  
 6,026,312 A 2/2000 Shemwell et al.  
 6,112,107 A 8/2000 Hannula  
 6,152,754 A 11/2000 Gerhardt et al.  
 6,165,005 A 12/2000 Mills et al.  
 6,253,097 B1 6/2001 Aronow et al.  
 6,280,213 B1 8/2001 Tobler et al.  
 6,298,255 B1 10/2001 Cordero et al.  
 6,370,409 B1 4/2002 Chung et al.  
 6,541,756 B2 4/2003 Schulz et al.  
 6,678,543 B2 1/2004 Diab et al.  
 6,850,788 B2 2/2005 Al-Ali  
 7,117,590 B2 10/2006 Koenig et al.  
 7,132,641 B2 11/2006 Schulz et al.  
 7,210,959 B1 5/2007 Teves  
 7,225,006 B2 5/2007 Al-Ali et al.  
 7,248,910 B2 7/2007 Li et al.  
 7,371,981 B2 5/2008 Abdul-Hafiz  
 7,377,794 B2 5/2008 Al-Ali et al.  
 7,427,165 B2 9/2008 Benaron et al.  
 D615,657 S 5/2010 Anderson et al.  
 D615,658 S 5/2010 Anderson et al.  
 D615,659 S 5/2010 Anderson et al.  
 D615,660 S 5/2010 Anderson et al.  
 D629,521 S 12/2010 Lash et al.  
 8,188,433 B2 5/2012 Gonopolskiy et al.  
 8,428,967 B2 4/2013 Olsen et al.  
 8,483,790 B2 7/2013 Hannula et al.  
 D705,429 S 5/2014 Cheney et al.  
 8,726,496 B2 5/2014 Besko  
 8,764,671 B2 7/2014 Kiani  
 9,138,182 B2 9/2015 Al-Ali et al.  
 D741,808 S 10/2015 Shim  
 9,211,072 B2 12/2015 Kiani  
 D756,817 S 5/2016 Fries et al.  
 D758,594 S \* 6/2016 Winters ..... D24/187  
 D761,435 S \* 7/2016 Mizuno ..... D24/187  
 D779,432 S 2/2017 Wong et al.  
 D779,433 S 2/2017 Fries et al.

D790,069 S 6/2017 Wong et al.  
 D794,567 S \* 8/2017 Fries ..... D13/133  
 D794,568 S 8/2017 Wardenburg  
 D800,583 S 10/2017 Ahong et al.  
 D806,256 S 12/2017 Allen et al.  
 D813,498 S 3/2018 Lavin et al.  
 D826,173 S 8/2018 Chen et al.  
 D860,465 S \* 9/2019 Lovell ..... D24/187  
 D862,709 S \* 10/2019 Besko ..... D24/187  
 D905,250 S \* 12/2020 Lovell ..... D24/187  
 D905,858 S \* 12/2020 Lovell ..... D24/187  
 2002/0103423 A1 8/2002 Chin et al.  
 2003/0135099 A1 7/2003 Al-Ali  
 2003/0162414 A1 8/2003 Schulz et al.  
 2004/0267103 A1 12/2004 Li et al.  
 2005/0113704 A1 5/2005 Lawson et al.  
 2006/0149149 A1 7/2006 Schmid  
 2006/0241363 A1 10/2006 Al-Ali et al.  
 2007/0073121 A1 3/2007 Hoarau et al.  
 2007/0123783 A1 5/2007 Chang  
 2008/0064940 A1 3/2008 Raridan  
 2008/0071153 A1 3/2008 Al-Ali et al.  
 2008/0076980 A1 3/2008 Hoarau  
 2008/0076995 A1 3/2008 Hoarau  
 2008/0076996 A1 3/2008 Hoarau  
 2008/0081954 A1 4/2008 Meyer et al.  
 2008/0220633 A1 9/2008 Al-Ali et al.  
 2008/0255435 A1 10/2008 Al-Ali et al.  
 2008/0316488 A1 12/2008 Mao et al.  
 2010/0076282 A1 3/2010 Sandmore  
 2014/0228659 A1 8/2014 Besko  
 2015/0216459 A1 8/2015 Al-Ali et al.

FOREIGN PATENT DOCUMENTS

JP 2004329406 A 11/2004  
 JP 2005052385 A 3/2005  
 JP 2005110816 A 4/2005  
 JP 2006061566 A 3/2006  
 JP 2007117641 A 5/2007  
 JP 2007167183 A 7/2007  
 JP 2007167184 A 7/2007  
 JP 2007190122 A 8/2007

OTHER PUBLICATIONS

SpO2\_Sensors\_and\_Adapter\_Cables\_for\_IntelliVue Aug. 1, 2008 (6 pp.).  
 AdultO2\_Manual\_Multi\_Jan. 1, 2011 (62 pp.).  
 Nellcor-adult-reusable-spo2-sensor-application-guide Jan. 1, 2012 (1 pp.).  
 883-11-PM-0258BRC\_INVOSNeonatalBrochure\_singles-1320864559 (5 pp.).  
 12673-DesignedtoTreat-1402592390\_INVOS\_brochure (2 pp.).

\* cited by examiner

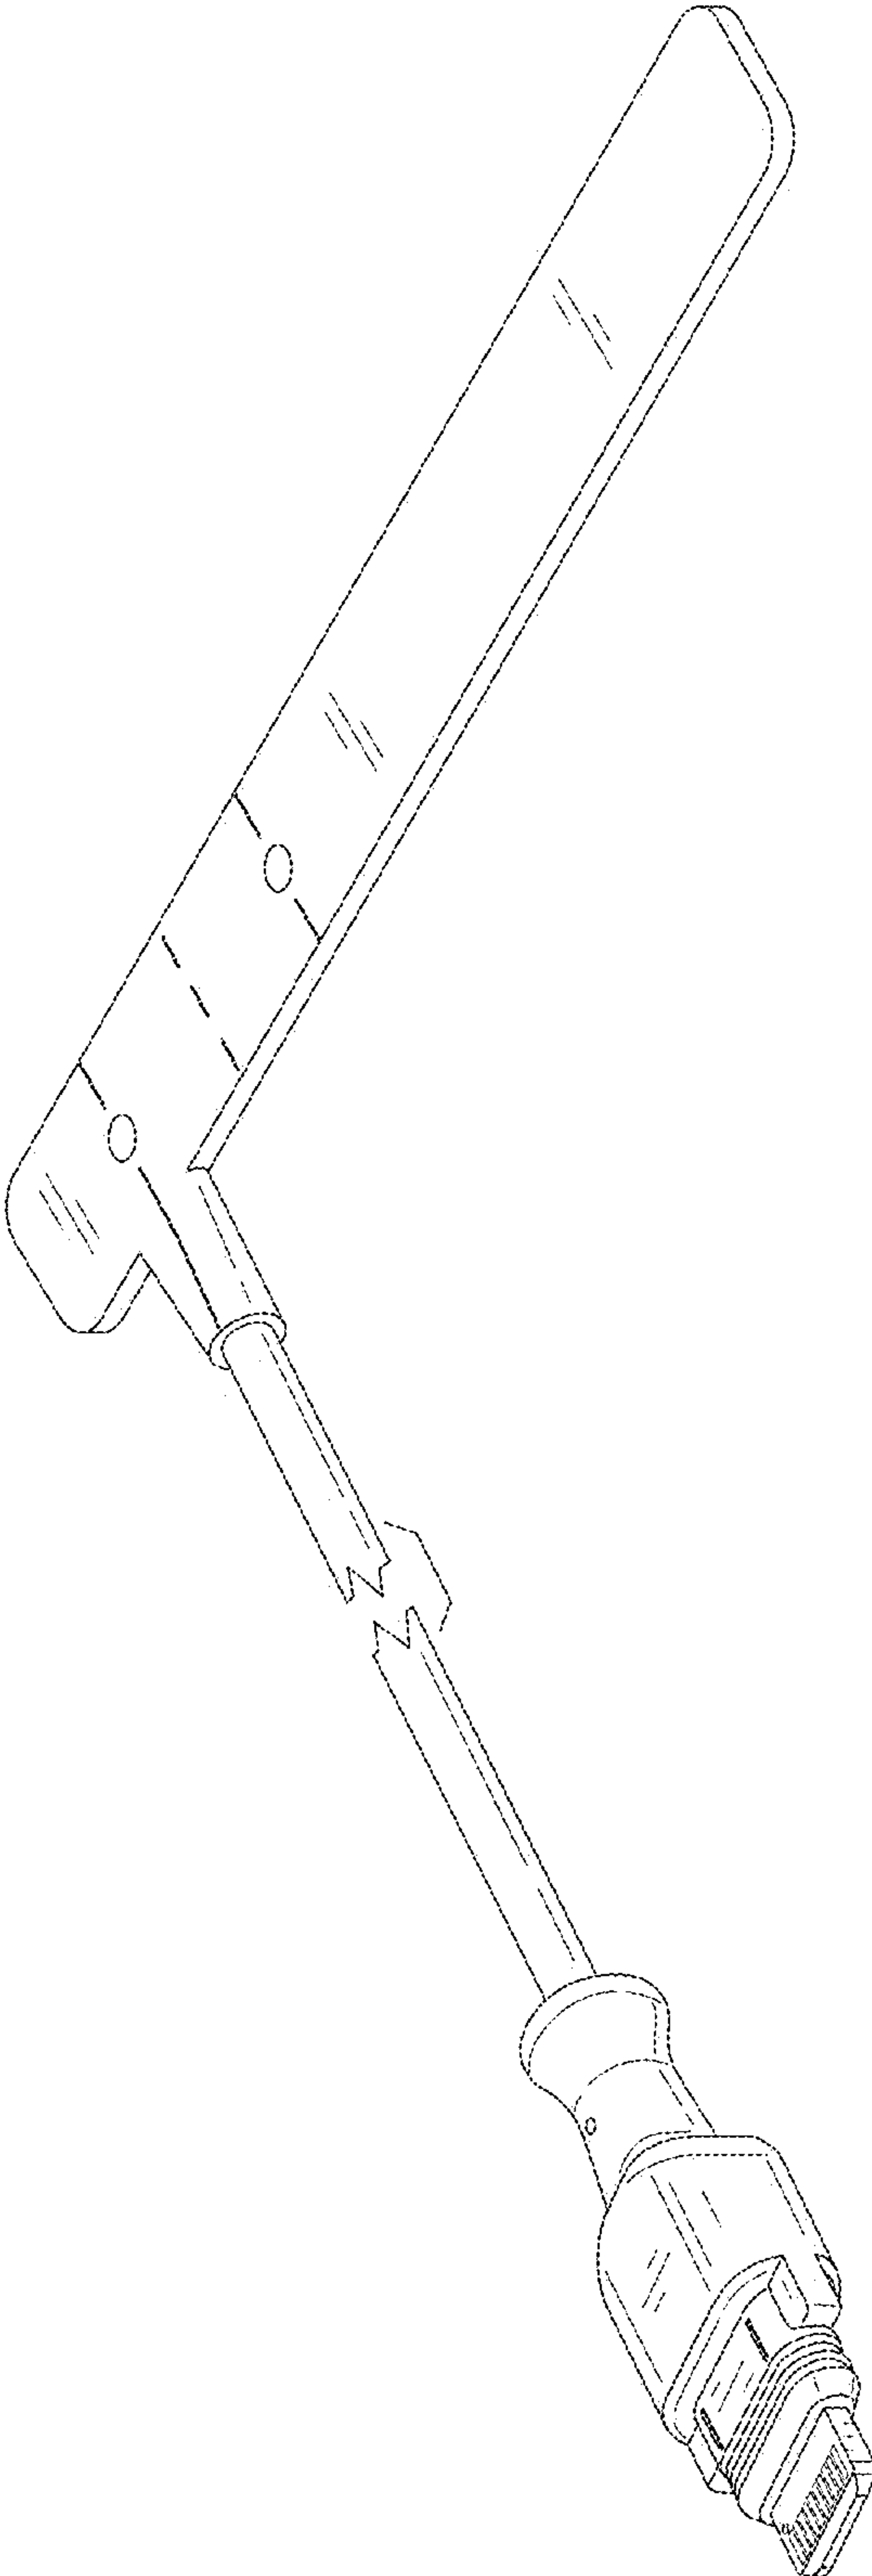


FIG. 1

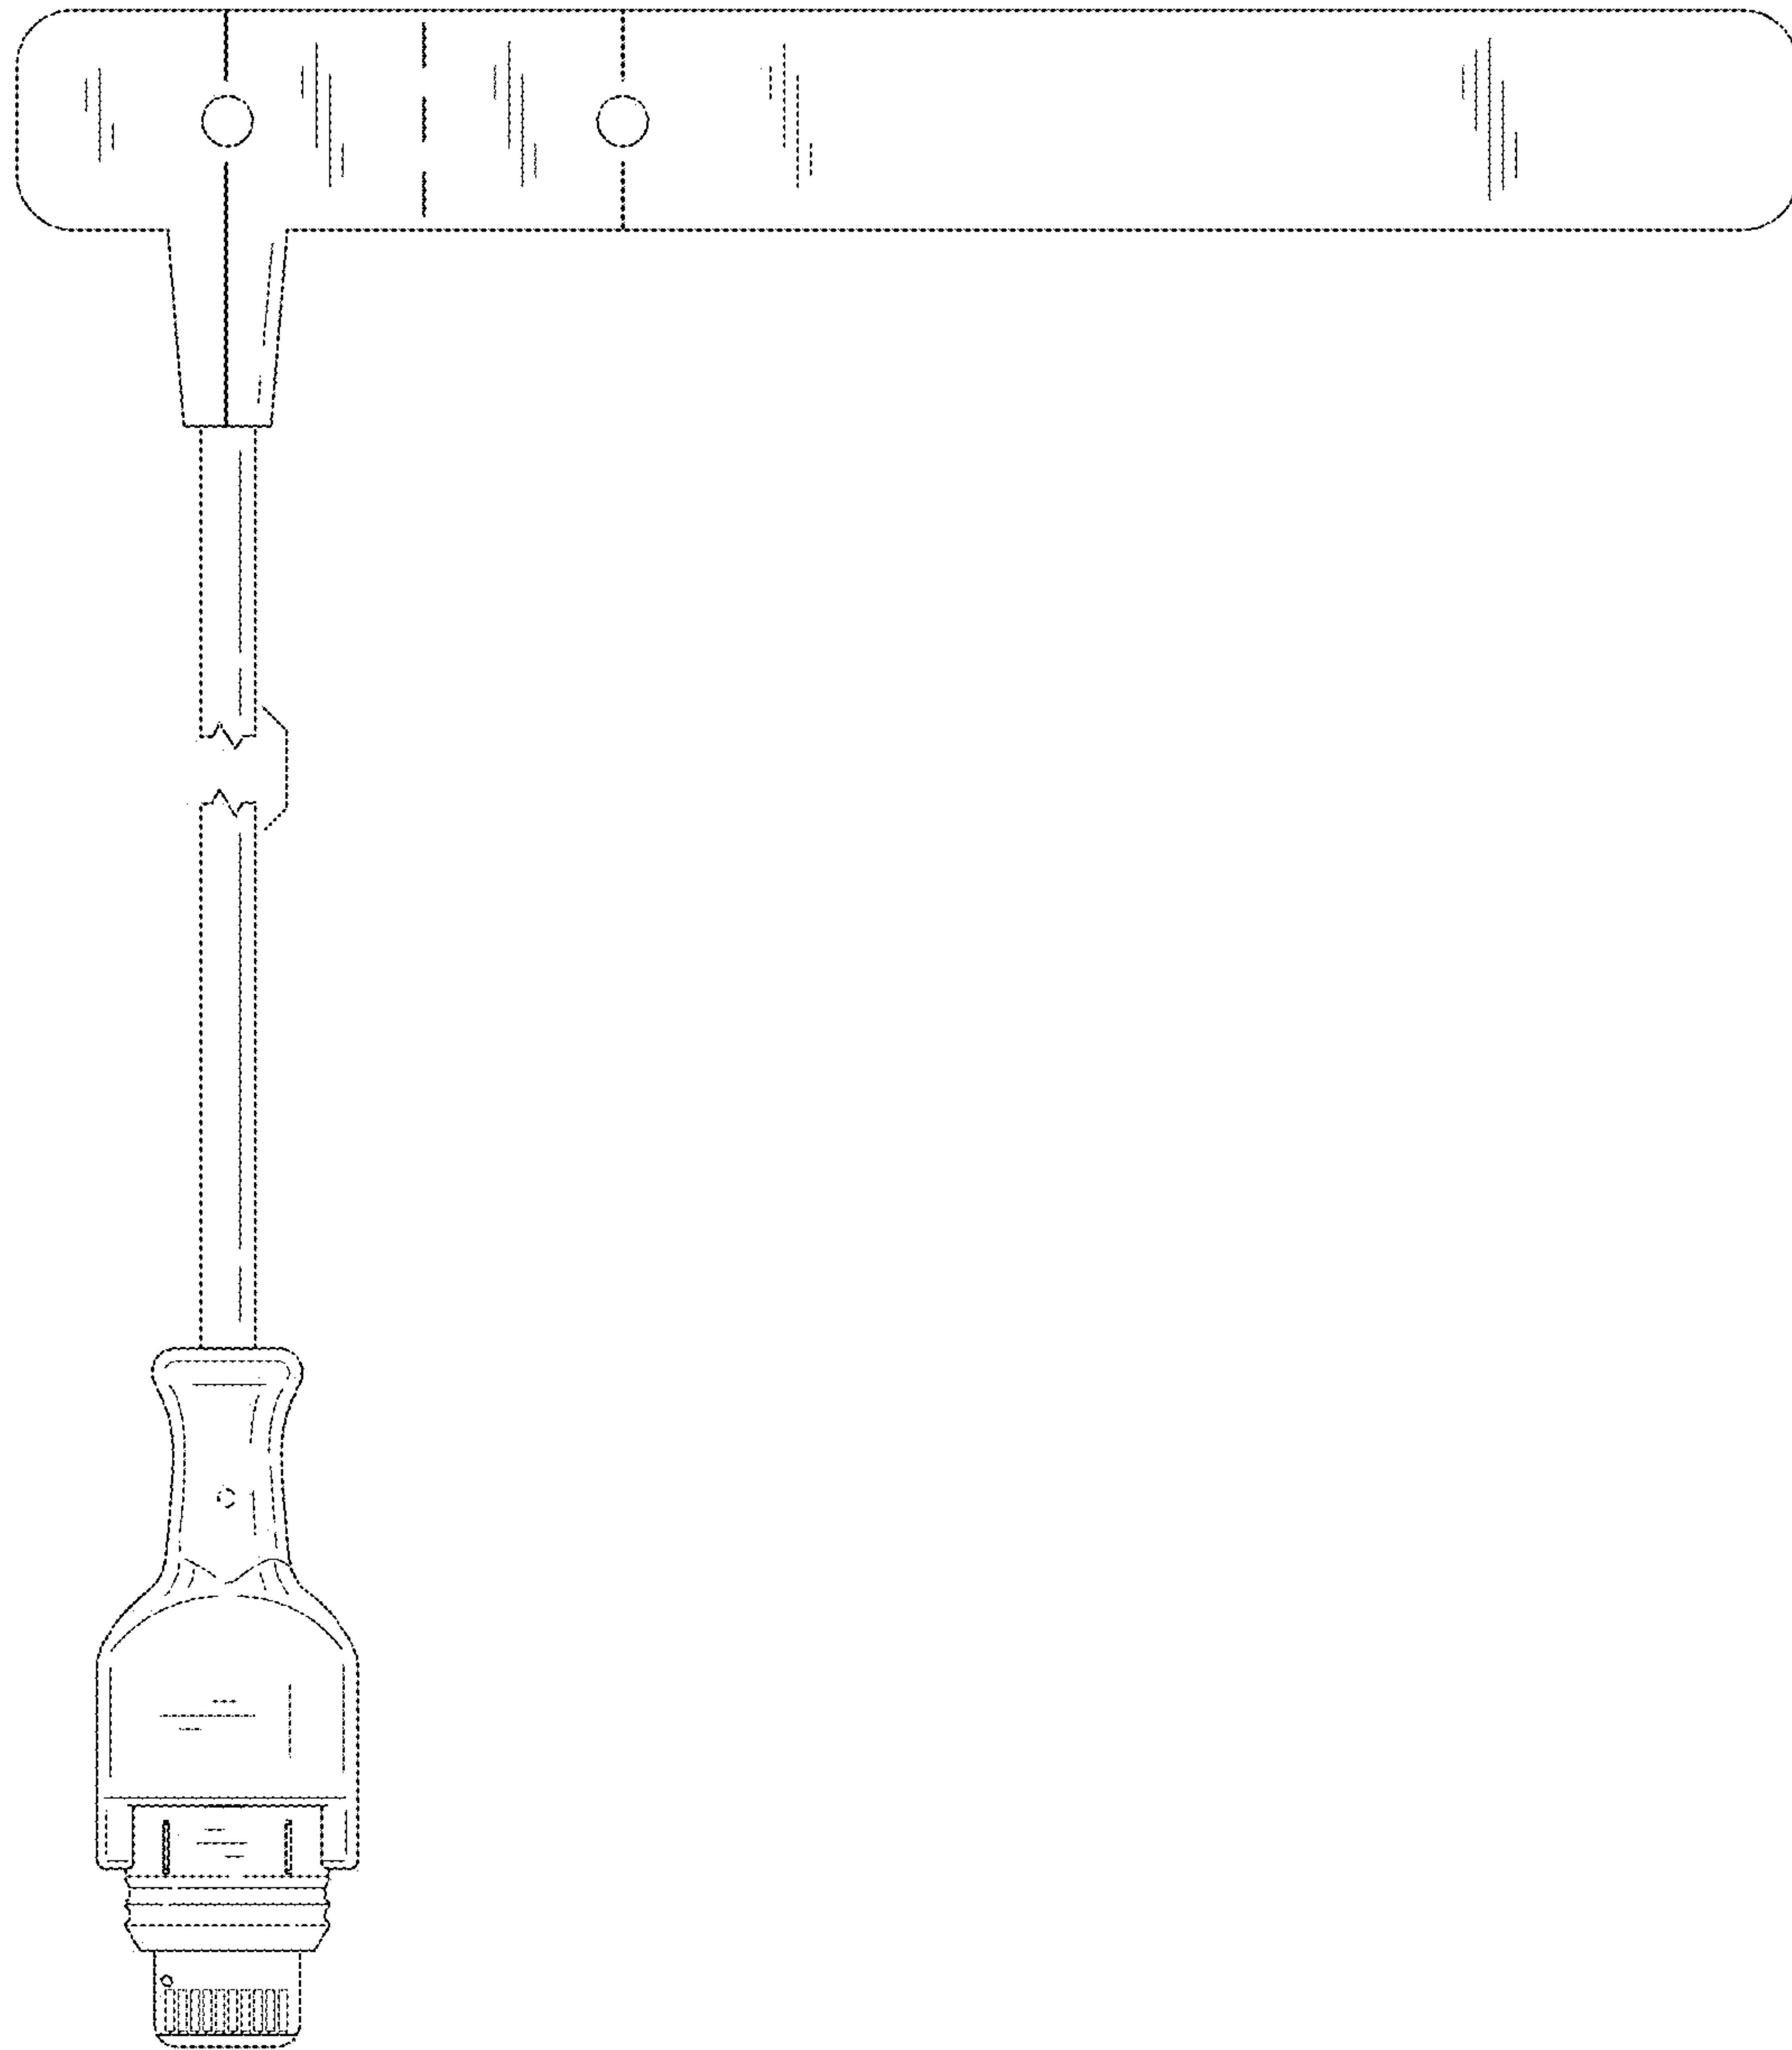


FIG. 2



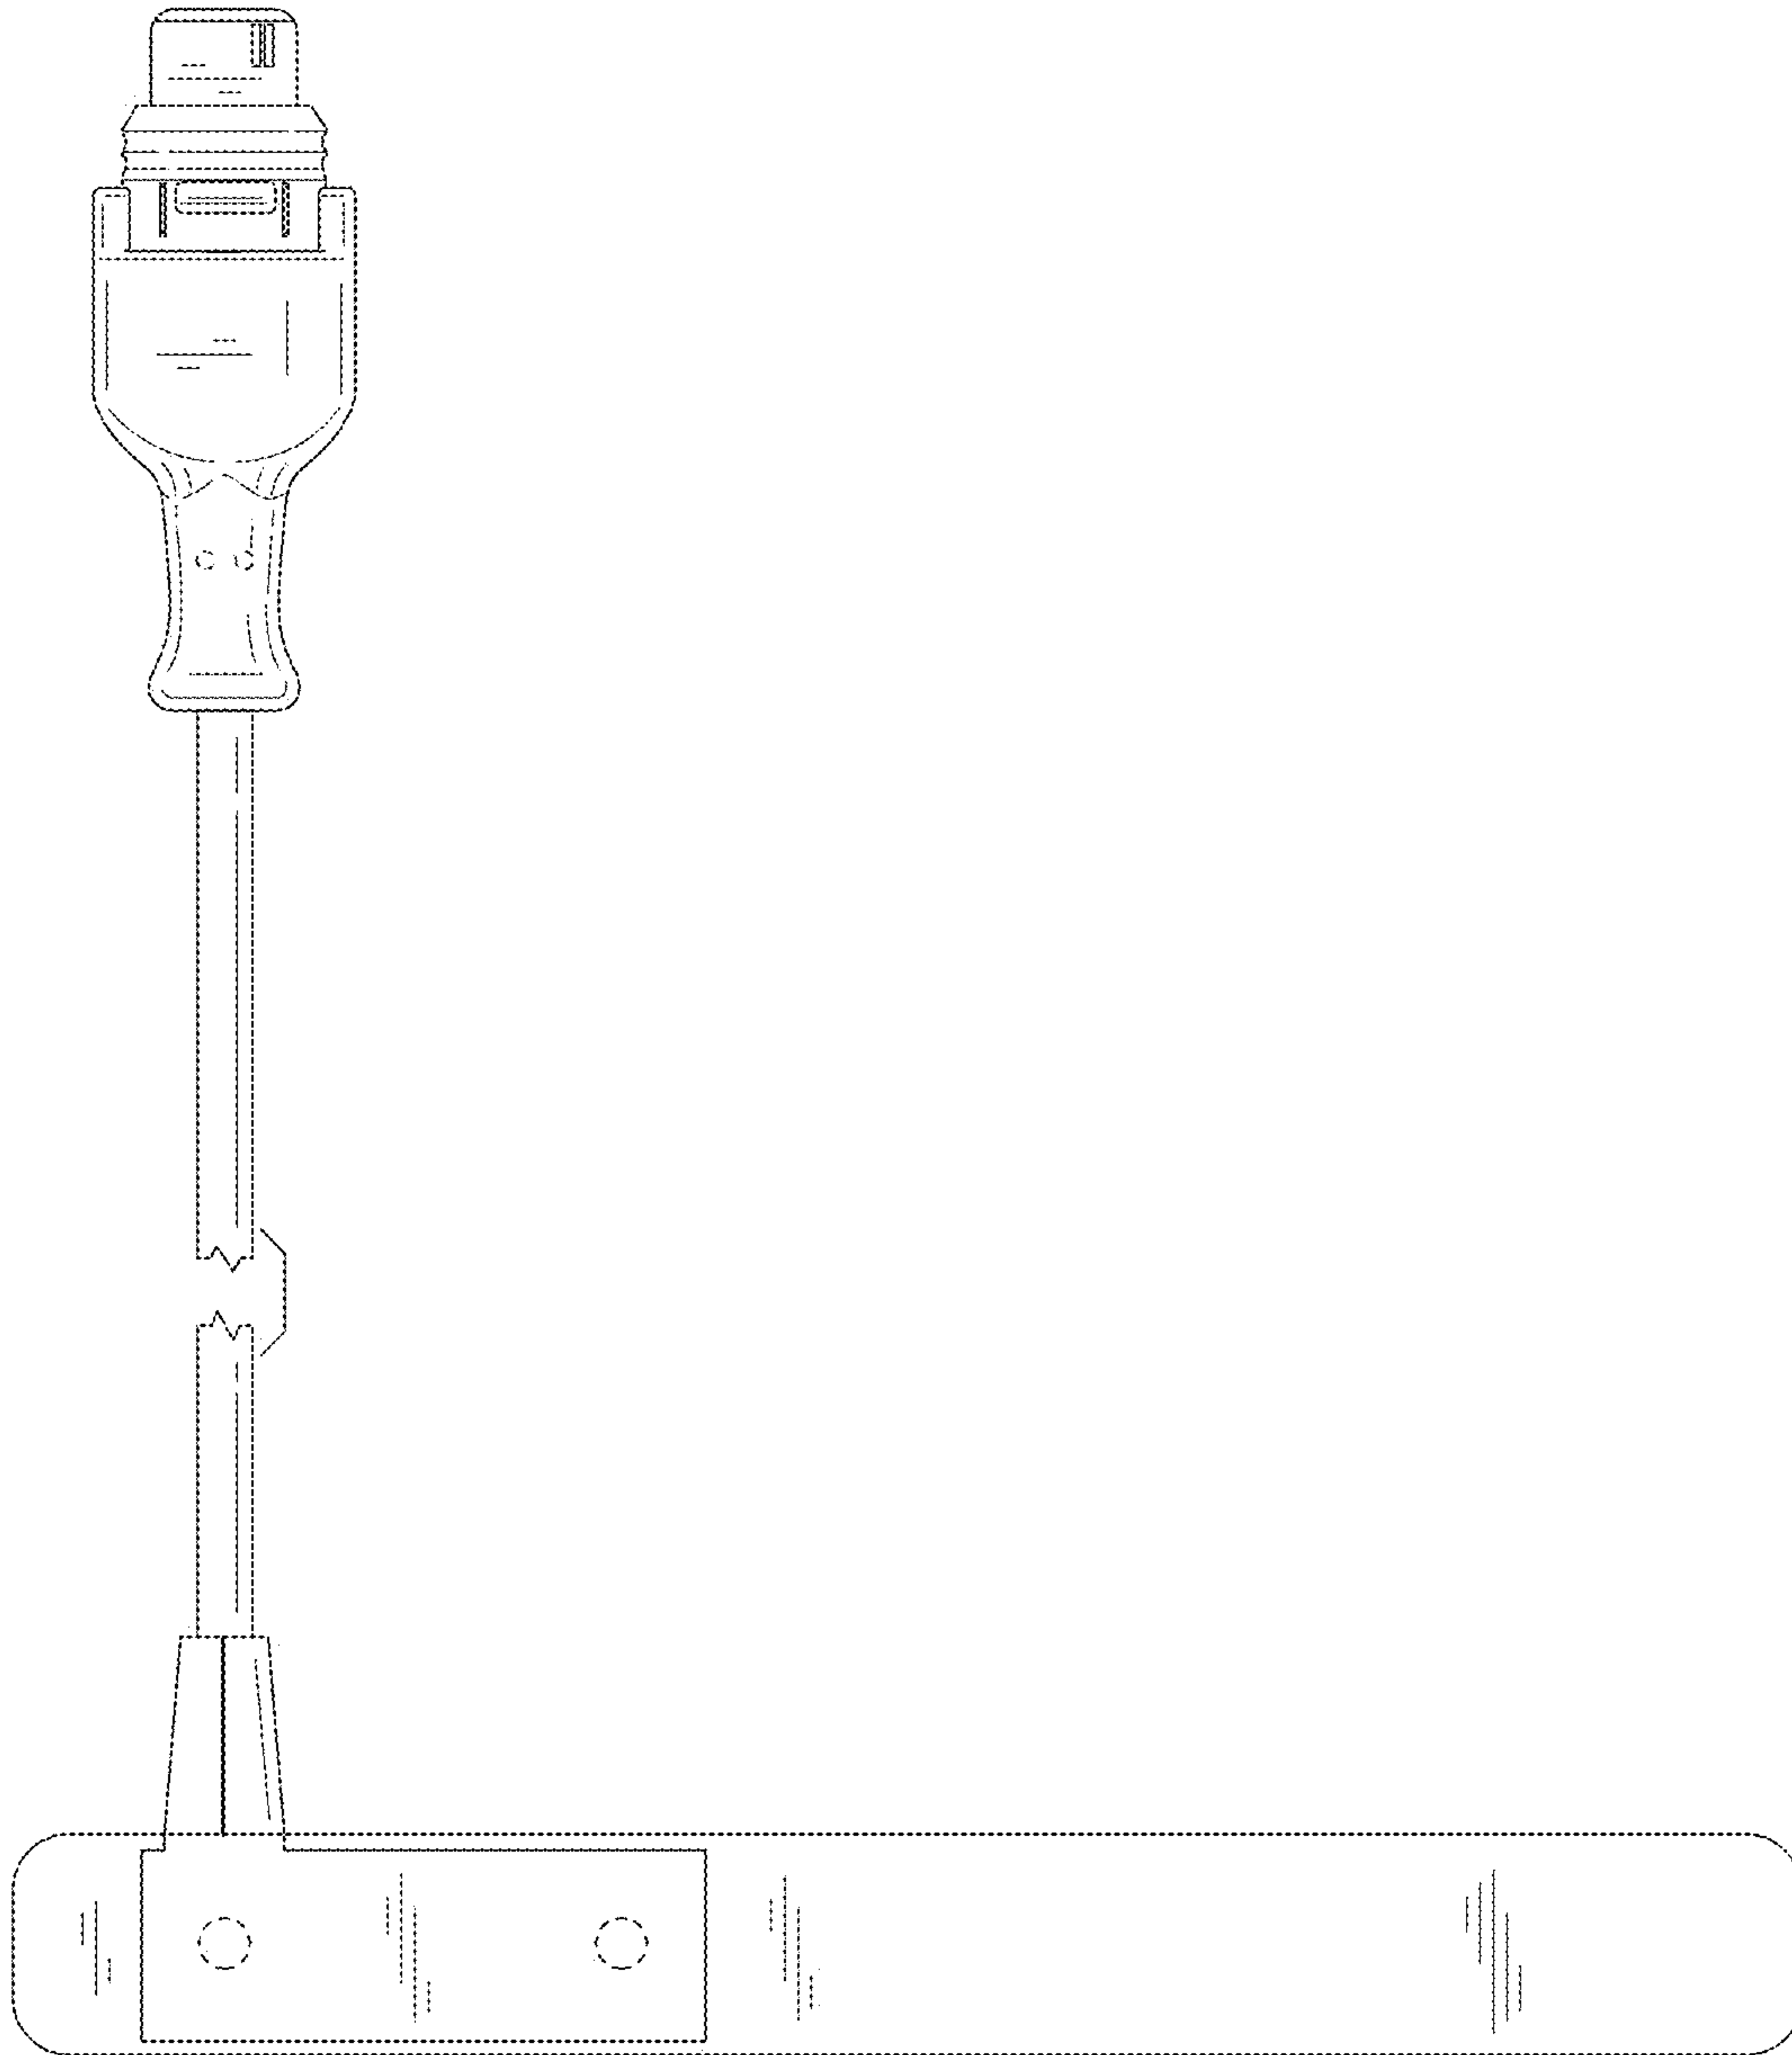


FIG. 3

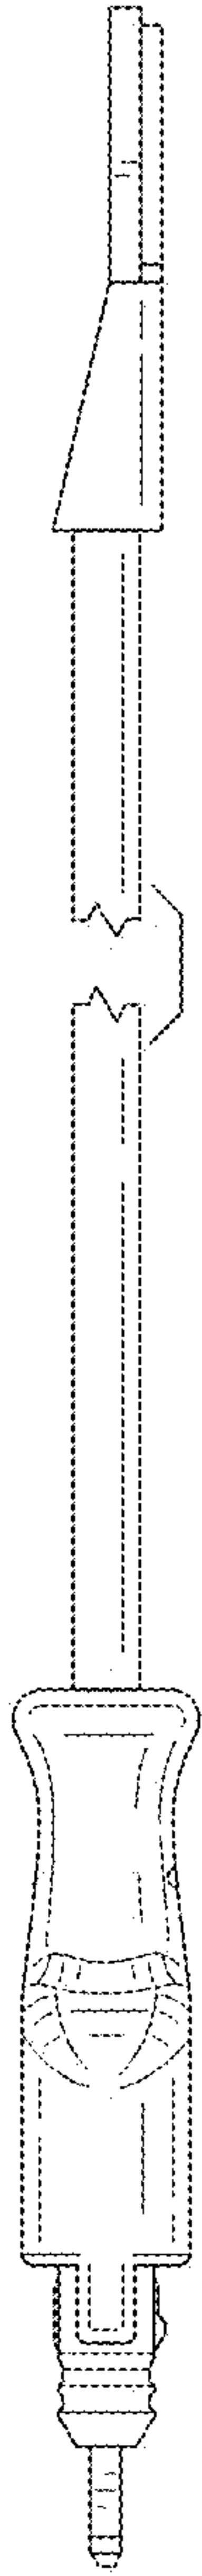


FIG. 4

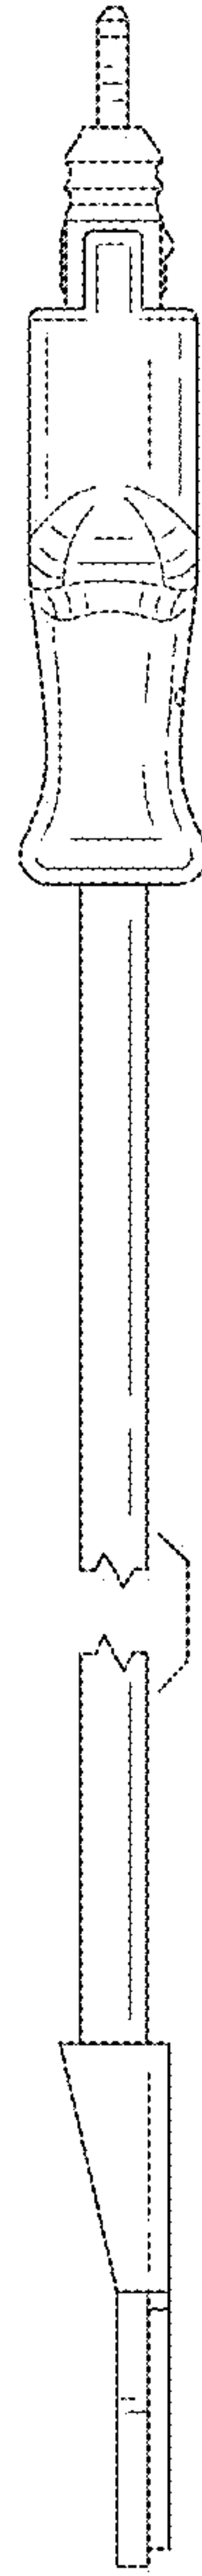


FIG. 5

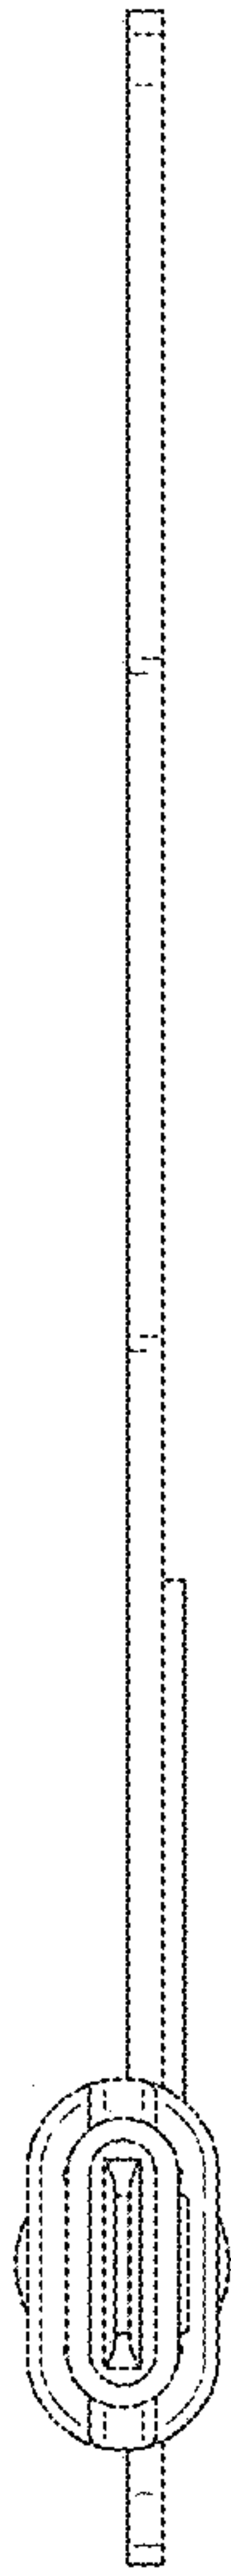


FIG. 6

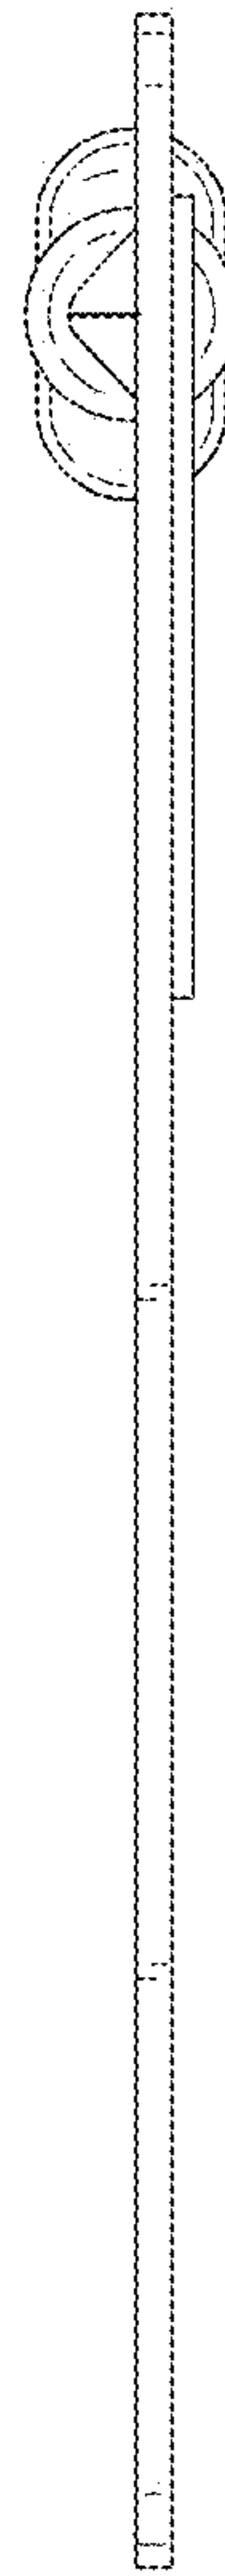


FIG. 7