



US00D937409S

(12) **United States Design Patent**  
**Ooshima et al.**

(10) **Patent No.:** **US D937,409 S**

(45) **Date of Patent:** **\*\* Nov. 30, 2021**

(54) **HOLDER FOR AN X-RAY TOMOGRAPHY  
DIAGNOSIS APPARATUS**

(71) Applicant: **Canon Medical Systems Corporation,**  
Otawara (JP)

(72) Inventors: **Jun Ooshima,** Nasushiobara (JP);  
**Kana Nishimura,** Tokyo (JP); **Rika  
Harada,** Tokyo (JP)

(73) Assignee: **Canon Medical Systems Corporation,**  
Otawara (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/714,905**

(22) Filed: **Nov. 26, 2019**

(30) **Foreign Application Priority Data**

Jun. 14, 2019 (JP) ..... 2019-013097

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/128; D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/128, 127, 189-192, 158; 604/179,  
604/180; 600/391, 392; 128/DIG. 26  
CPC ..... A61M 25/02; A61M 16/0666; A61M  
2210/0618; A61M 2025/0253; A61M  
2025/0226

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D527,822 S 9/2006 Trevino  
D554,257 S \* 10/2007 Ogiwara ..... D24/158  
D601,261 S 9/2009 Levan  
D642,278 S 7/2011 Sharps et al.  
D663,798 S \* 7/2012 Duncan ..... D21/789

D669,990 S \* 10/2012 Degruytere ..... D24/158  
D683,024 S \* 5/2013 Baba ..... D24/158  
D695,405 S \* 12/2013 Moon ..... D24/158  
D715,941 S \* 10/2014 Li ..... D24/158  
D725,779 S \* 3/2015 Braswell, Jr. .... D24/158  
D766,440 S \* 9/2016 Kim ..... D24/158  
D797,945 S \* 9/2017 Kim ..... D24/191  
D799,052 S 10/2017 Rossouw  
D800,911 S \* 10/2017 Diemer ..... D24/192  
D828,551 S \* 9/2018 Zou ..... D24/130  
D829,913 S \* 10/2018 Kitayama ..... D24/159  
D835,783 S \* 12/2018 Smith ..... D24/140  
D837,385 S 1/2019 He et al.  
D890,344 S \* 7/2020 Wells ..... D24/158  
D905,234 S \* 12/2020 Nock ..... D24/127  
D908,229 S \* 1/2021 Wagner ..... D24/191

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 303128501 3/2015  
CN 303980459 12/2016  
JP 1091161 11/2000

(Continued)

*Primary Examiner* — David G Muller

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,  
Farabow, Garrett & Dunner, L.L.P.


(57) **CLAIM**

The ornamental design for a holder for an X-ray tomography  
diagnosis apparatus, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a holder for an X-ray  
tomography diagnosis apparatus showing our new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a rear elevational view thereof;  
FIG. 4 is a top plan view thereof;  
FIG. 5 is a bottom plan view thereof; and,  
FIG. 6 is a left side elevational view thereof.

**1 Claim, 6 Drawing Sheets**

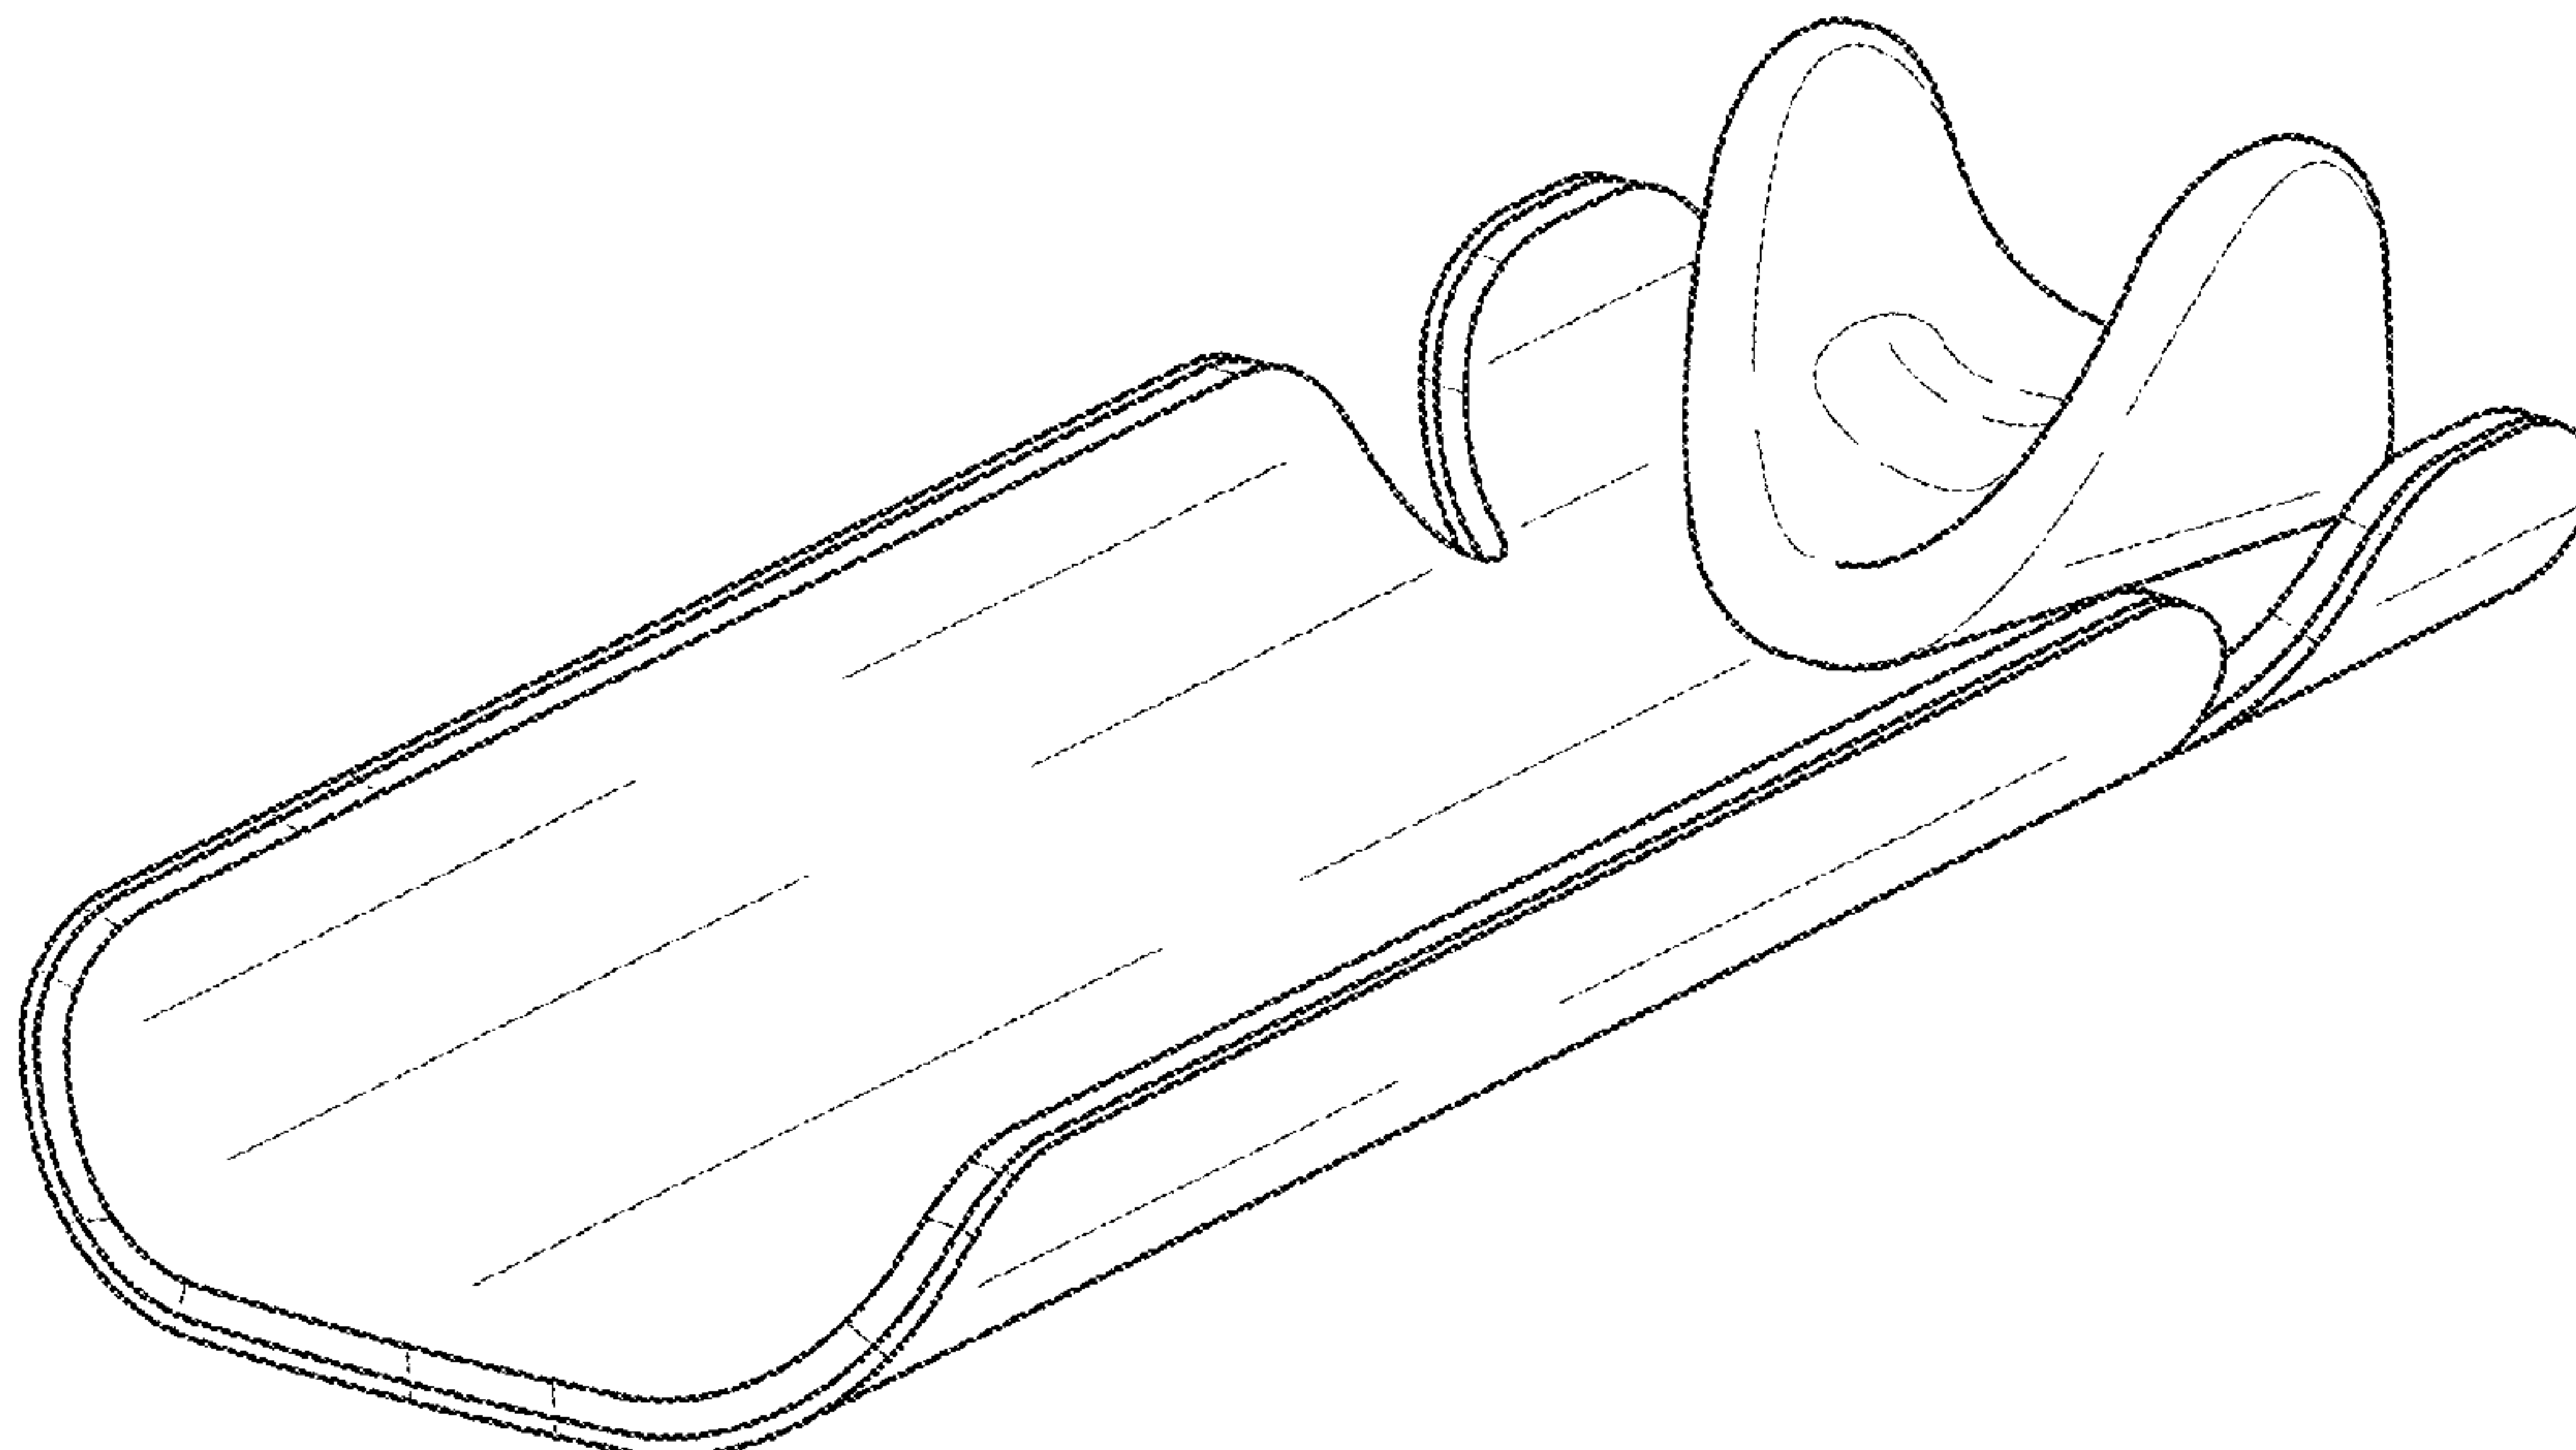

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D919,100 S \* 5/2021 Al-Ali ..... D24/186

FOREIGN PATENT DOCUMENTS

JP	1161361	12/2002
JP	1161362	12/2002
JP	1187079	10/2003
JP	1390819	6/2010
JP	1617186	11/2018

\* cited by examiner

Fig. 1

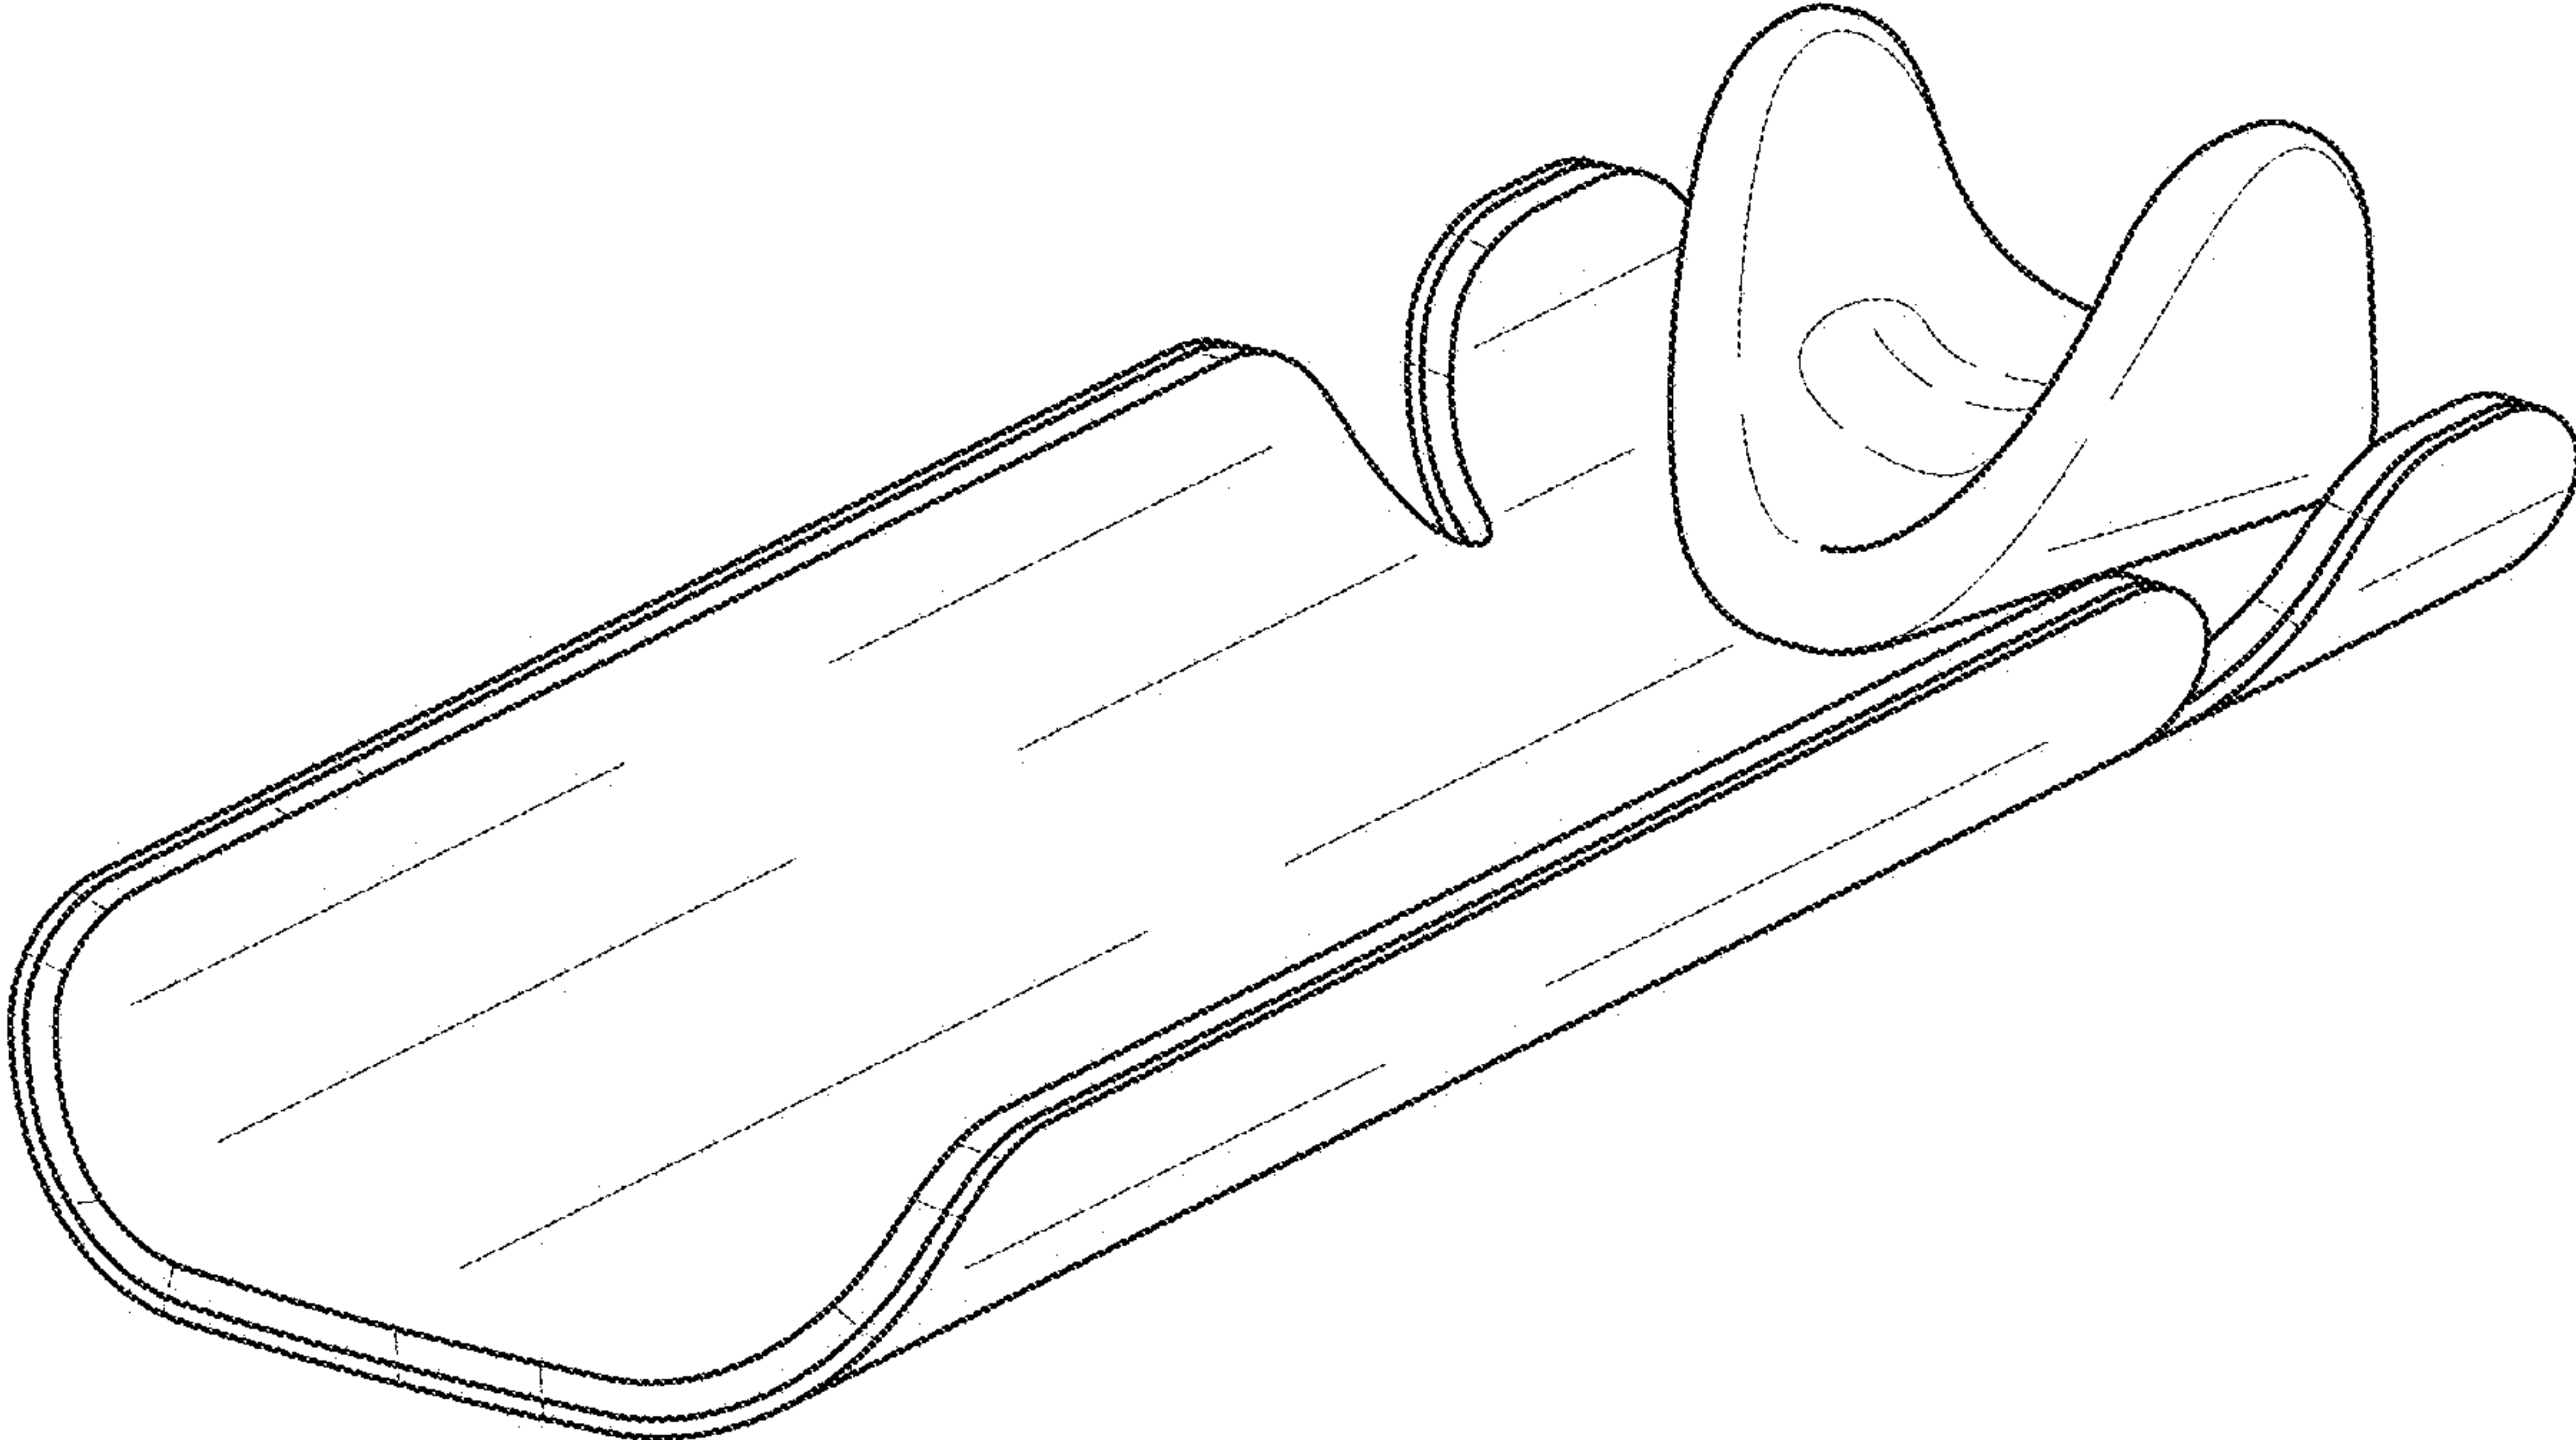


Fig. 2

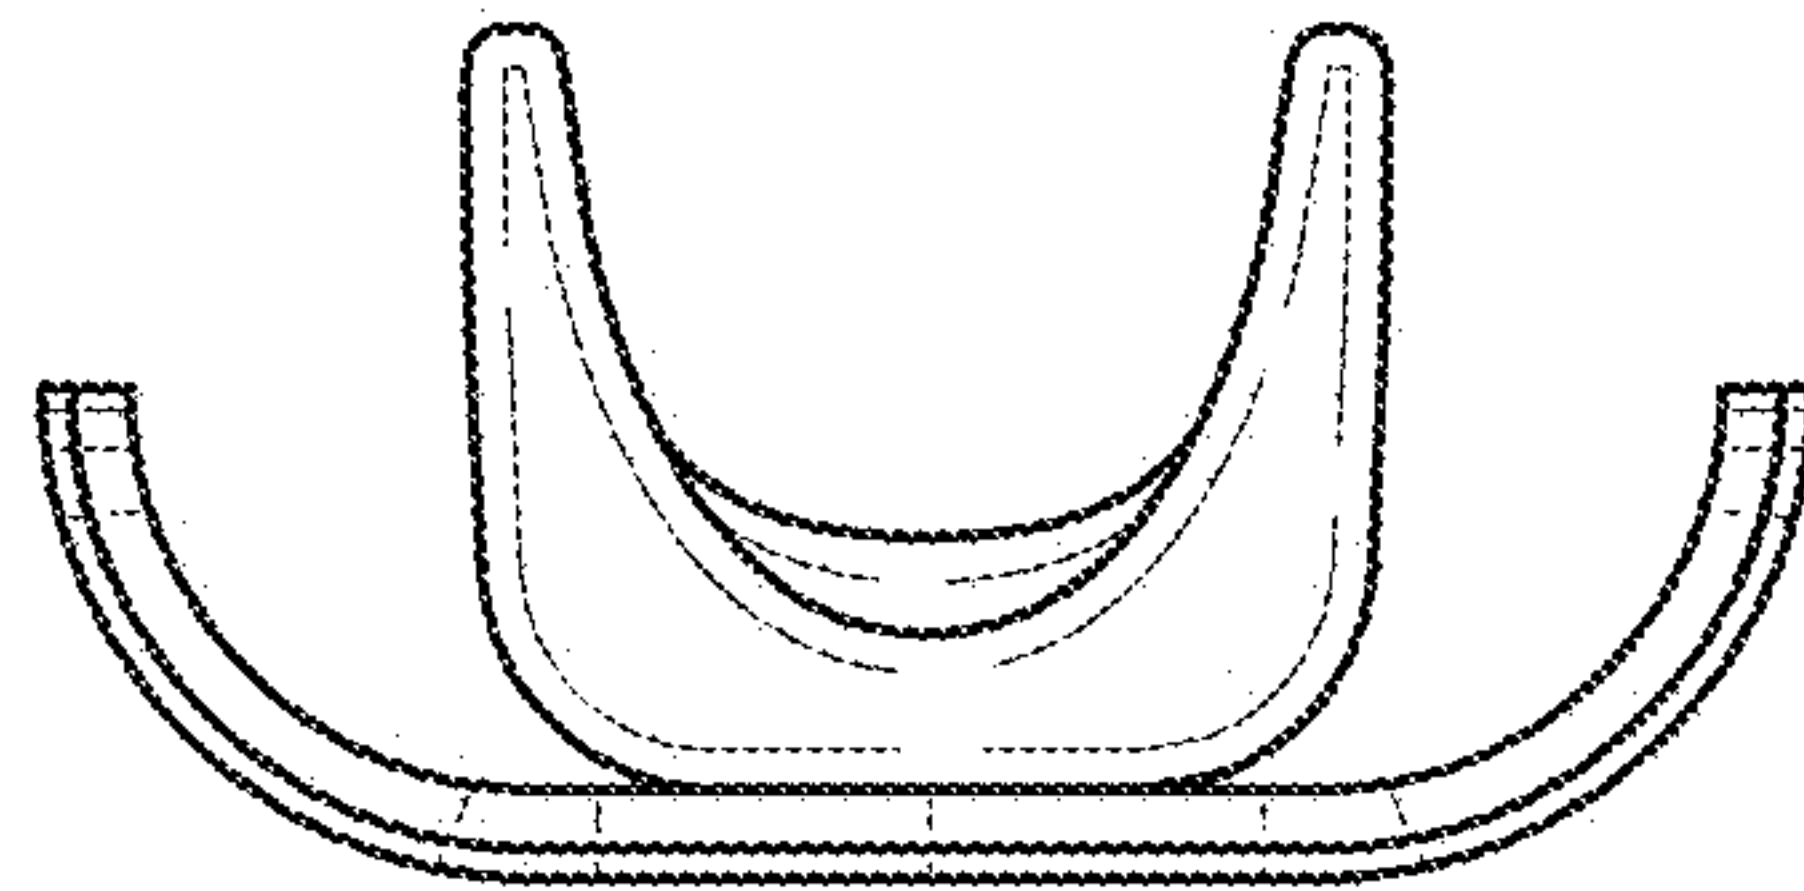


Fig. 3

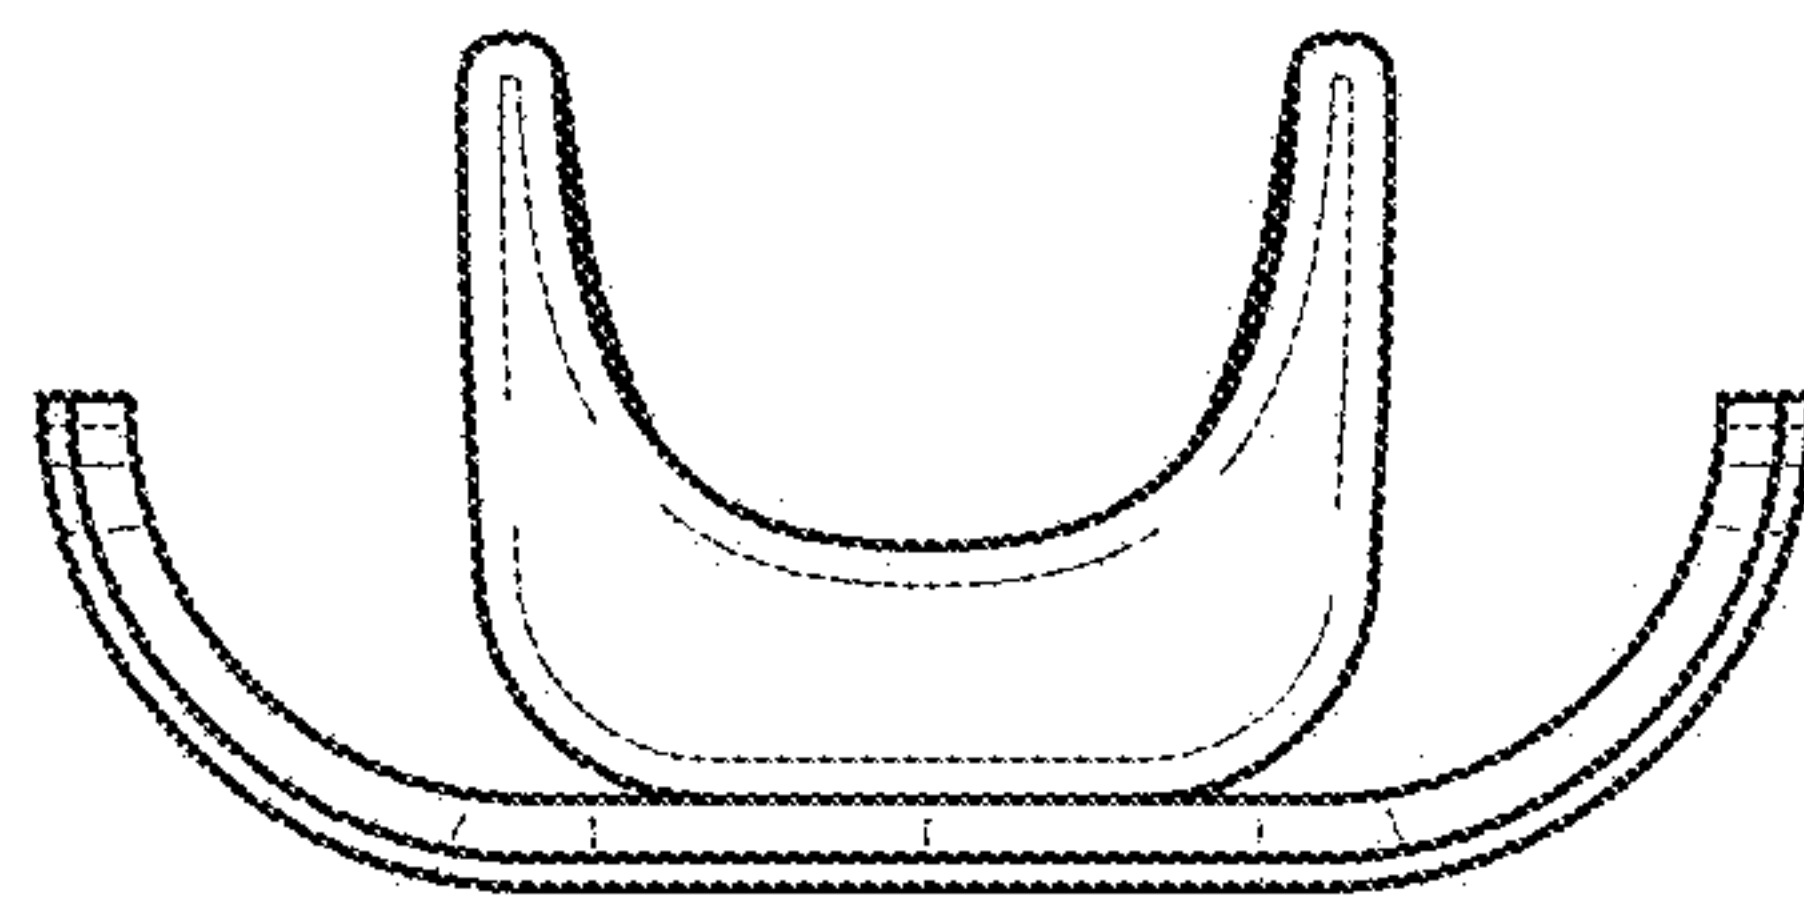


Fig. 4

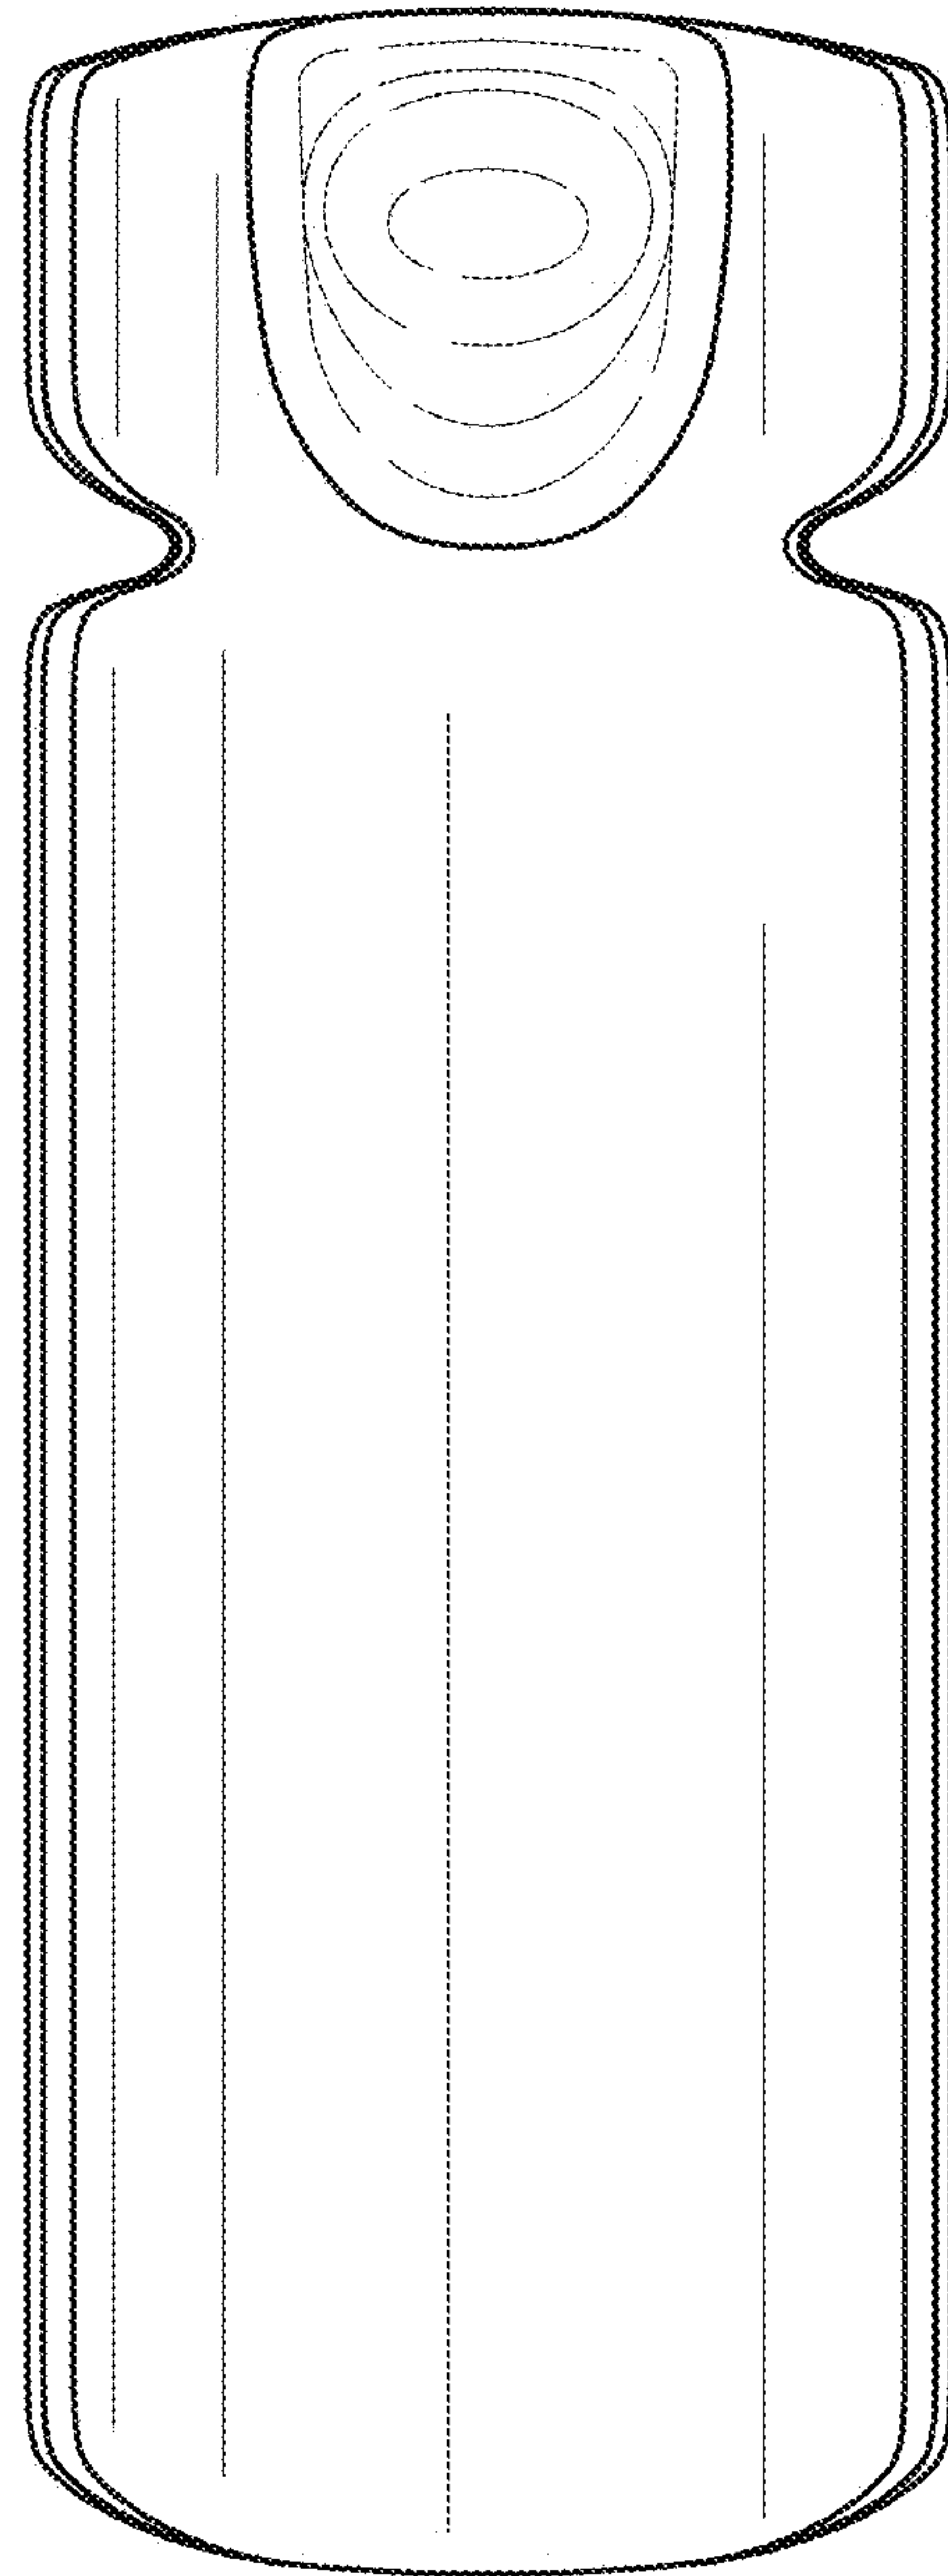


Fig. 5

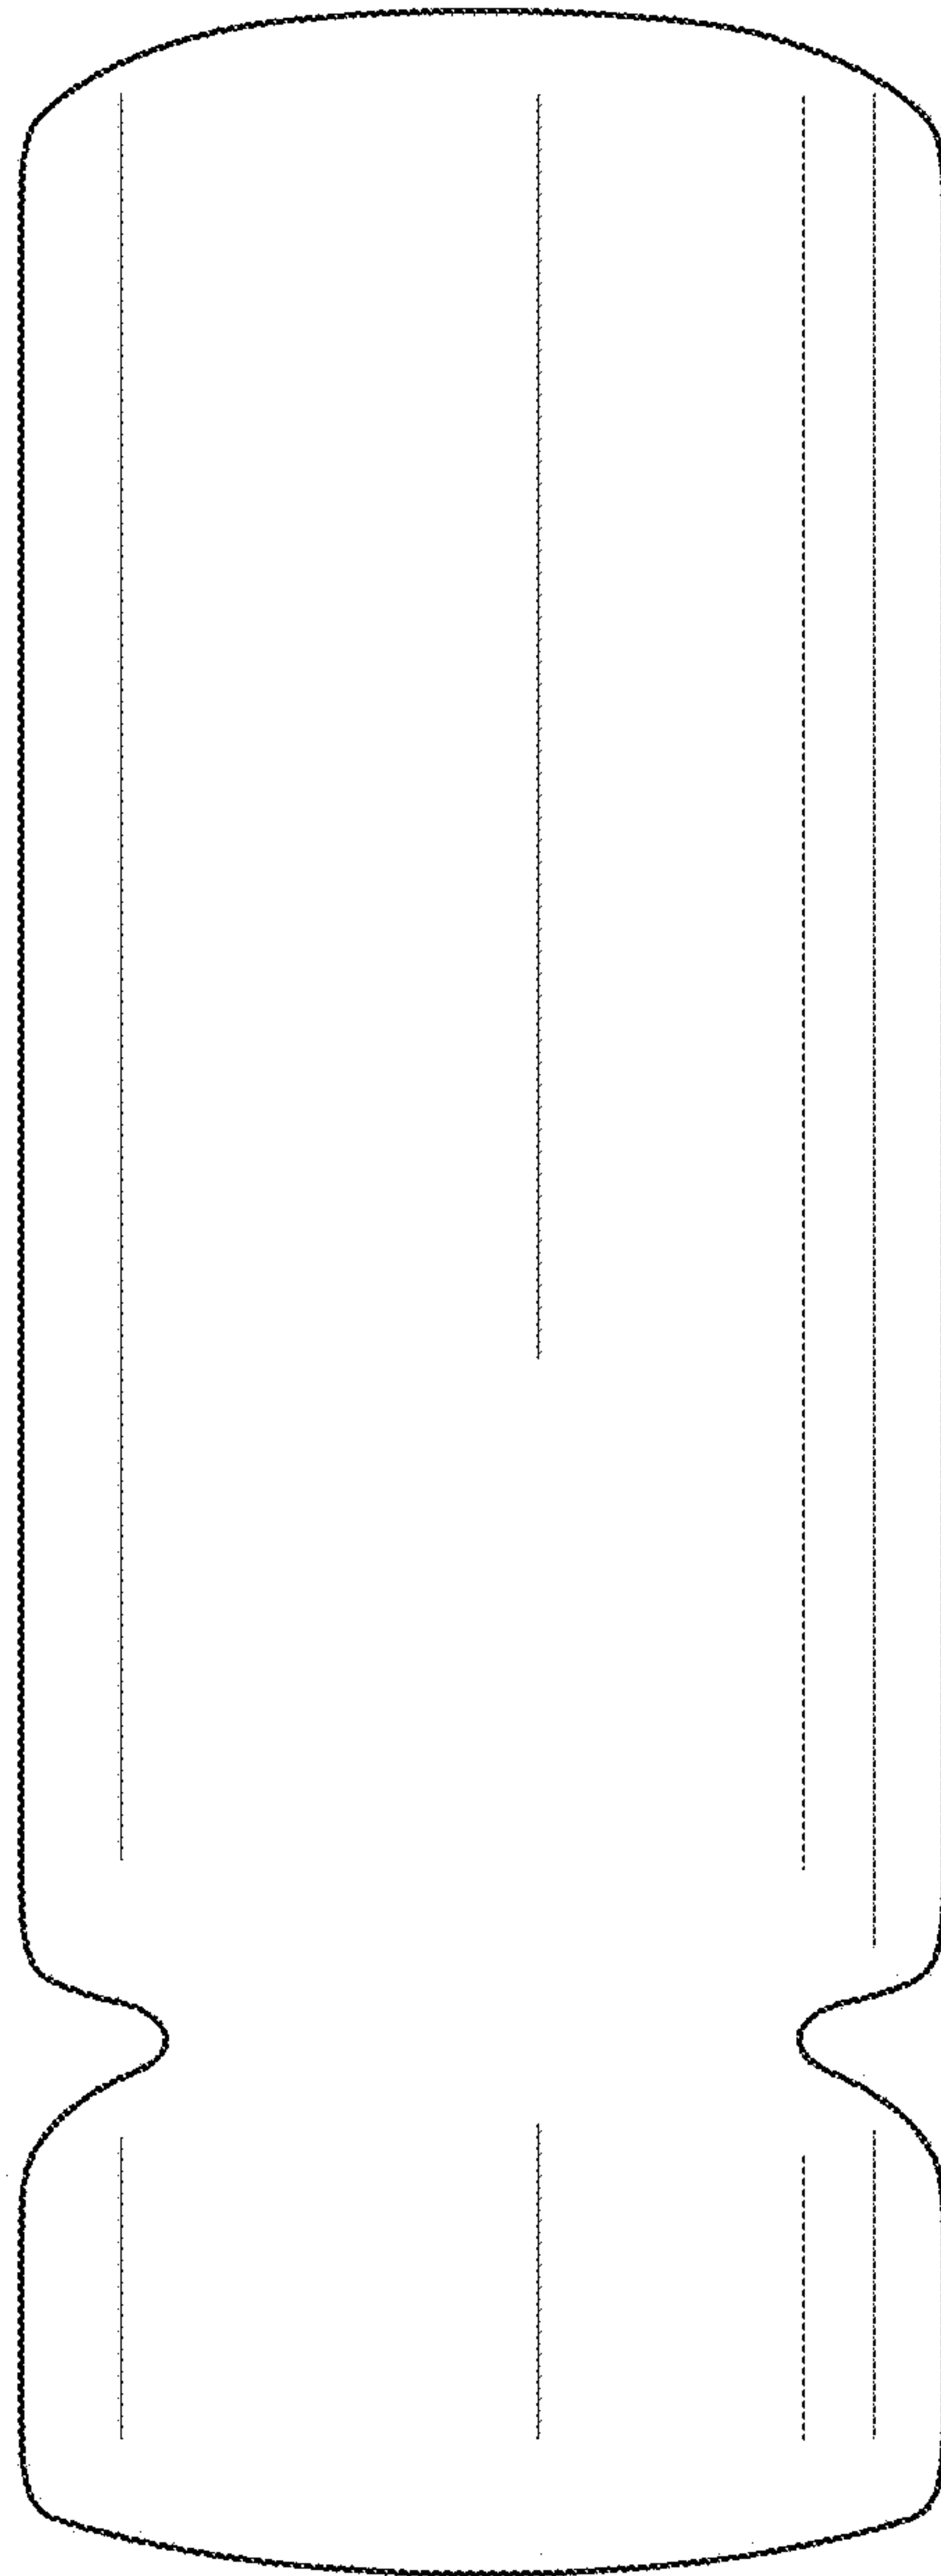


Fig. 6

