



US00D937429S

(12) **United States Design Patent** (10) **Patent No.:** **US D937,429 S**  
**Bobey et al.** (45) **Date of Patent:** **\*\* Nov. 30, 2021**

(54) **OUTER COVERING FOR A PERCUSSIVE HIGH FREQUENCY CHEST WALL OSCILLATION SYSTEM**

(71) Applicant: **HILL-ROM SERVICES PTE. LTD.**, Singapore (SG)

(72) Inventors: **John A. Bobey**, Daniel Island, SC (US); **Deny D. Barilea**, Singapore (SG); **Suresha Venkataraya**, Singapore (SG); **Wei T. Tan**, Singapore (SG); **Clementine Pirio**, Nantes (FR); **Bryan Chng**, Singapore (SG); **Scott Saunders**, Portland, OR (US); **Damon Clegg**, Portland, OR (US)

(73) Assignee: **HILL-ROM SERVICES PTE. LTD.**, Singapore (SG)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/768,246**

(22) Filed: **Jan. 28, 2021**

**Related U.S. Application Data**

(62) Division of application No. 29/714,001, filed on Nov. 20, 2019, now Pat. No. Des. 912,259, which is a division of application No. 29/665,615, filed on Oct. 5, 2018, now Pat. No. Des. 870,904, which is a division of application No. 29/594,780, filed on Feb. 22, 2017, now Pat. No. Des. 834,718.

(51) **LOC (13) Cl.** ..... **28-03**

(52) **U.S. Cl.**  
USPC ..... **D24/200**

(58) **Field of Classification Search**  
USPC ..... D24/200, 107, 164, 215; D2/828-829  
CPC ..... A61H 9/00; A61H 9/005; A61H 9/0071; A61H 9/0007; A61H 9/0078; A61H 7/004; A61H 23/00; A61H 23/006; A61H 23/02; A61H 23/0218; A61H 23/04; A61H 2023/045; A41D 13/0518

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,869,537 A 1/1959 Chu  
3,053,250 A 9/1962 Stubbs  
5,235,967 A 8/1993 Arbisi et al.

(Continued)

OTHER PUBLICATIONS

Medgadget, "Hill-Rom's New Monarch Battery Powered Airway Clearance System." Apr. 27, 2017. [On line], [site visited Aug. 17, 2021]. Retrieved from internet: <URL: <https://www.medgadget.com/2017/04/hill-roms-new-monarch-battery-powered-airway-clearance-system.html>>.\*

(Continued)

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP


(57) **CLAIM**

The ornamental design for an outer covering for a percussive high frequency chest wall oscillation system, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of an outer covering for a percussive high frequency chest wall oscillation system in accordance with the present design; FIG. 2 is a front elevation view thereof; FIG. 3 is a rear elevation view thereof; FIG. 4 is right side elevation view thereof; FIG. 5 is a left side elevation view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof. The broken lines showing the remainder of the outer covering for a percussive high frequency chest wall oscillation system are directed to environment. None of the broken lines form a part of the claimed design.

**1 Claim, 7 Drawing Sheets**

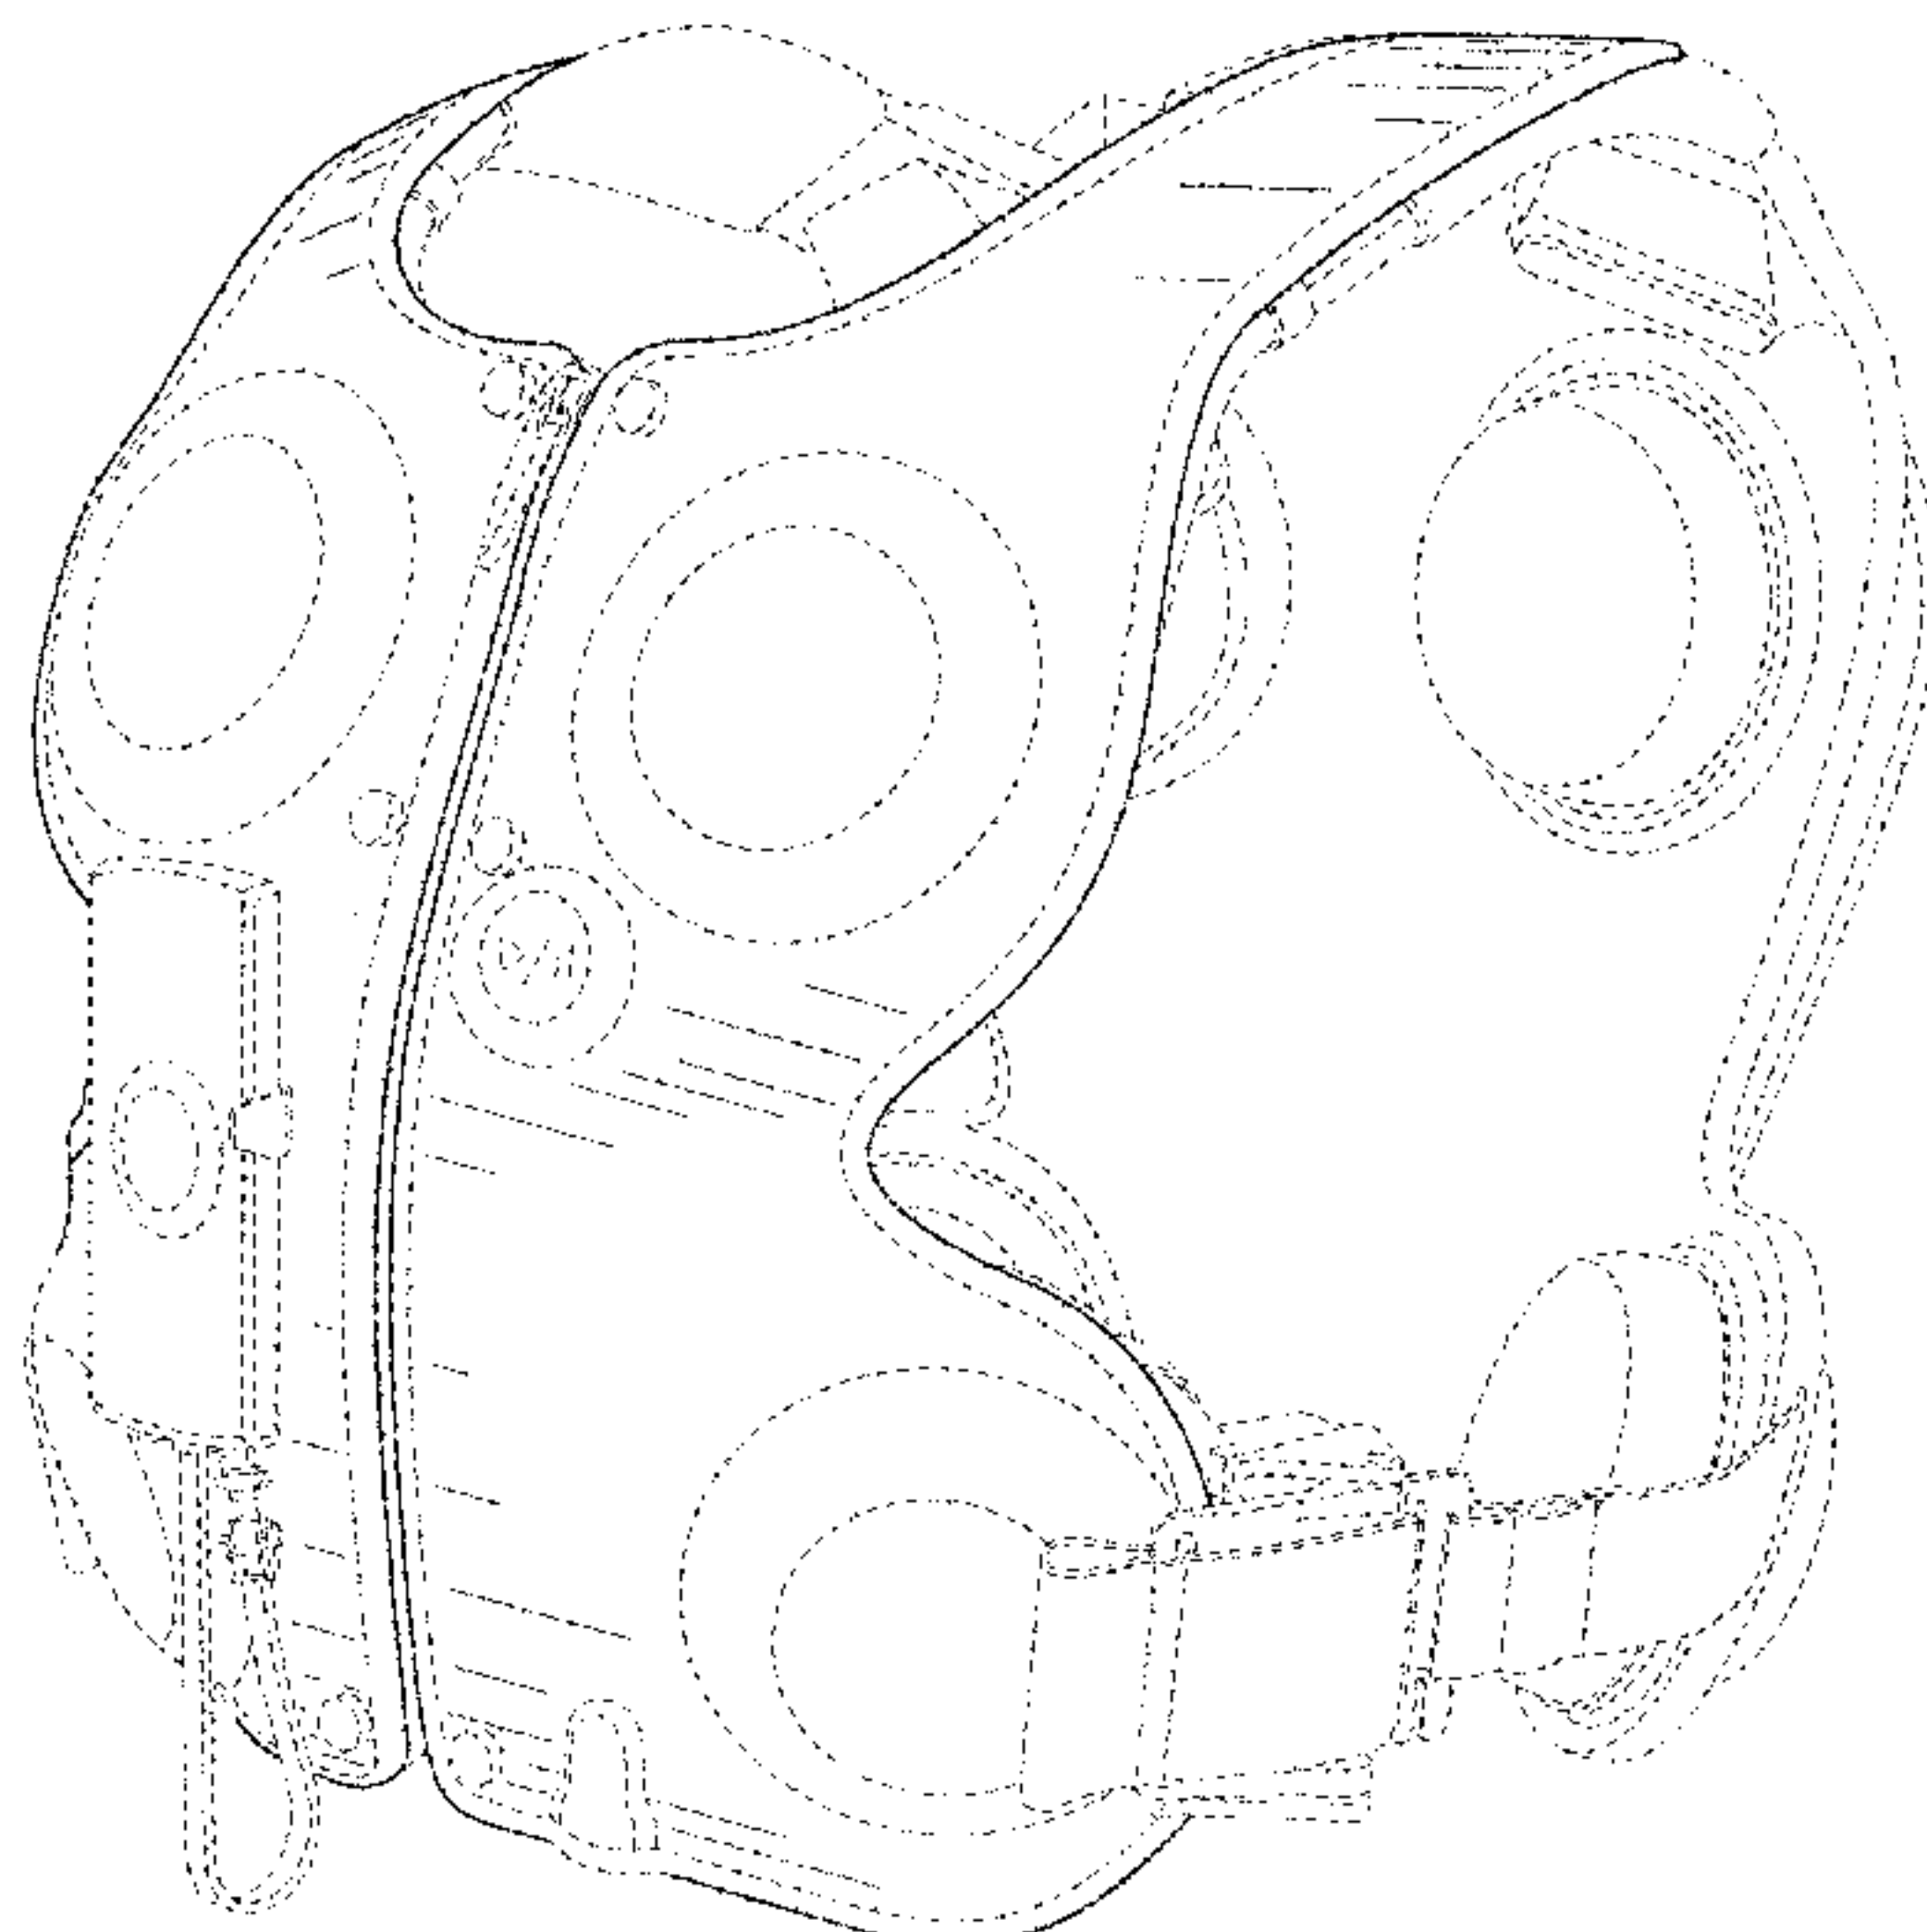

(56)

References Cited

U.S. PATENT DOCUMENTS


6,254,556 B1 7/2001 Hansen et al.  
 D456,591 S 5/2002 Hansen  
 D461,897 S 8/2002 Hansen  
 D469,876 S 2/2003 Hansen et al.  
 D478,989 S 8/2003 Hansen et al.  
 6,676,614 B1 1/2004 Hansen et al.  
 7,115,104 B2 10/2006 Van Brunt et al.  
 7,232,417 B2 6/2007 Plante  
 7,374,550 B2 5/2008 Hansen et al.  
 7,582,065 B2 9/2009 Van Brunt et al.  
 7,931,607 B2 4/2011 Biondo et al.  
 D639,954 S 6/2011 Helgeson et al.  
 8,460,223 B2 6/2013 Huster et al.  
 D704,849 S 5/2014 Hunter  
 9,237,982 B2 1/2016 Van Brunt  
 9,549,869 B2 1/2017 DeVliger et al.  
 9,895,287 B2 2/2018 Shockley, Jr. et al.  
 9,907,725 B2 \* 3/2018 Shockley, Jr. .... A61H 23/02  
 9,968,511 B2 5/2018 Huster et al.  
 D834,718 S 11/2018 Bobey et al.  
 10,251,810 B2 4/2019 Shockley, Jr. et al.  
 D852,969 S 7/2019 Bobey et al.  
 D870,904 S 12/2019 Bobey et al.  
 10,610,446 B2 4/2020 Shockley, Jr. et al.  
 D898,926 S \* 10/2020 Bobey ..... D24/200

D912,259 S 3/2021 Bobey et al.  
 2004/0133133 A1 7/2004 Dreimann et al.  
 2006/0005306 A1 1/2006 Call et al.  
 2008/0108914 A1 5/2008 Brouqueyre et al.  
 2009/0192421 A1 7/2009 Huster et al.  
 2011/0087143 A1 4/2011 Bobey et al.  
 2012/0291798 A1 11/2012 Park et al.  
 2014/0005579 A1 1/2014 Drlik et al.  
 2014/0276271 A1 9/2014 Stryker et al.  
 2016/0095790 A1 4/2016 Shockley, Jr. et al.  
 2018/0049939 A1 2/2018 Bobey et al.

OTHER PUBLICATIONS

Hodsdon, Suzanne, "Hill-Rom Unveils Mobile, Connected Airway Clearance System for Patients on the Move" May 2, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL:https://www.meddeviceonline.com/doc/hill-rom/unveils-mobile-connected-airway-clearance-system-for-patients-on-the-move-0001 >.  
 Hill-Rom | Respiratory Care | Monarch™ Airway Clearance System 3D Animation Video, published on Jun. 26, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL:https://www.youtube.com/results?search\_query=monarch+airways+clearance+system>.

\* cited by examiner

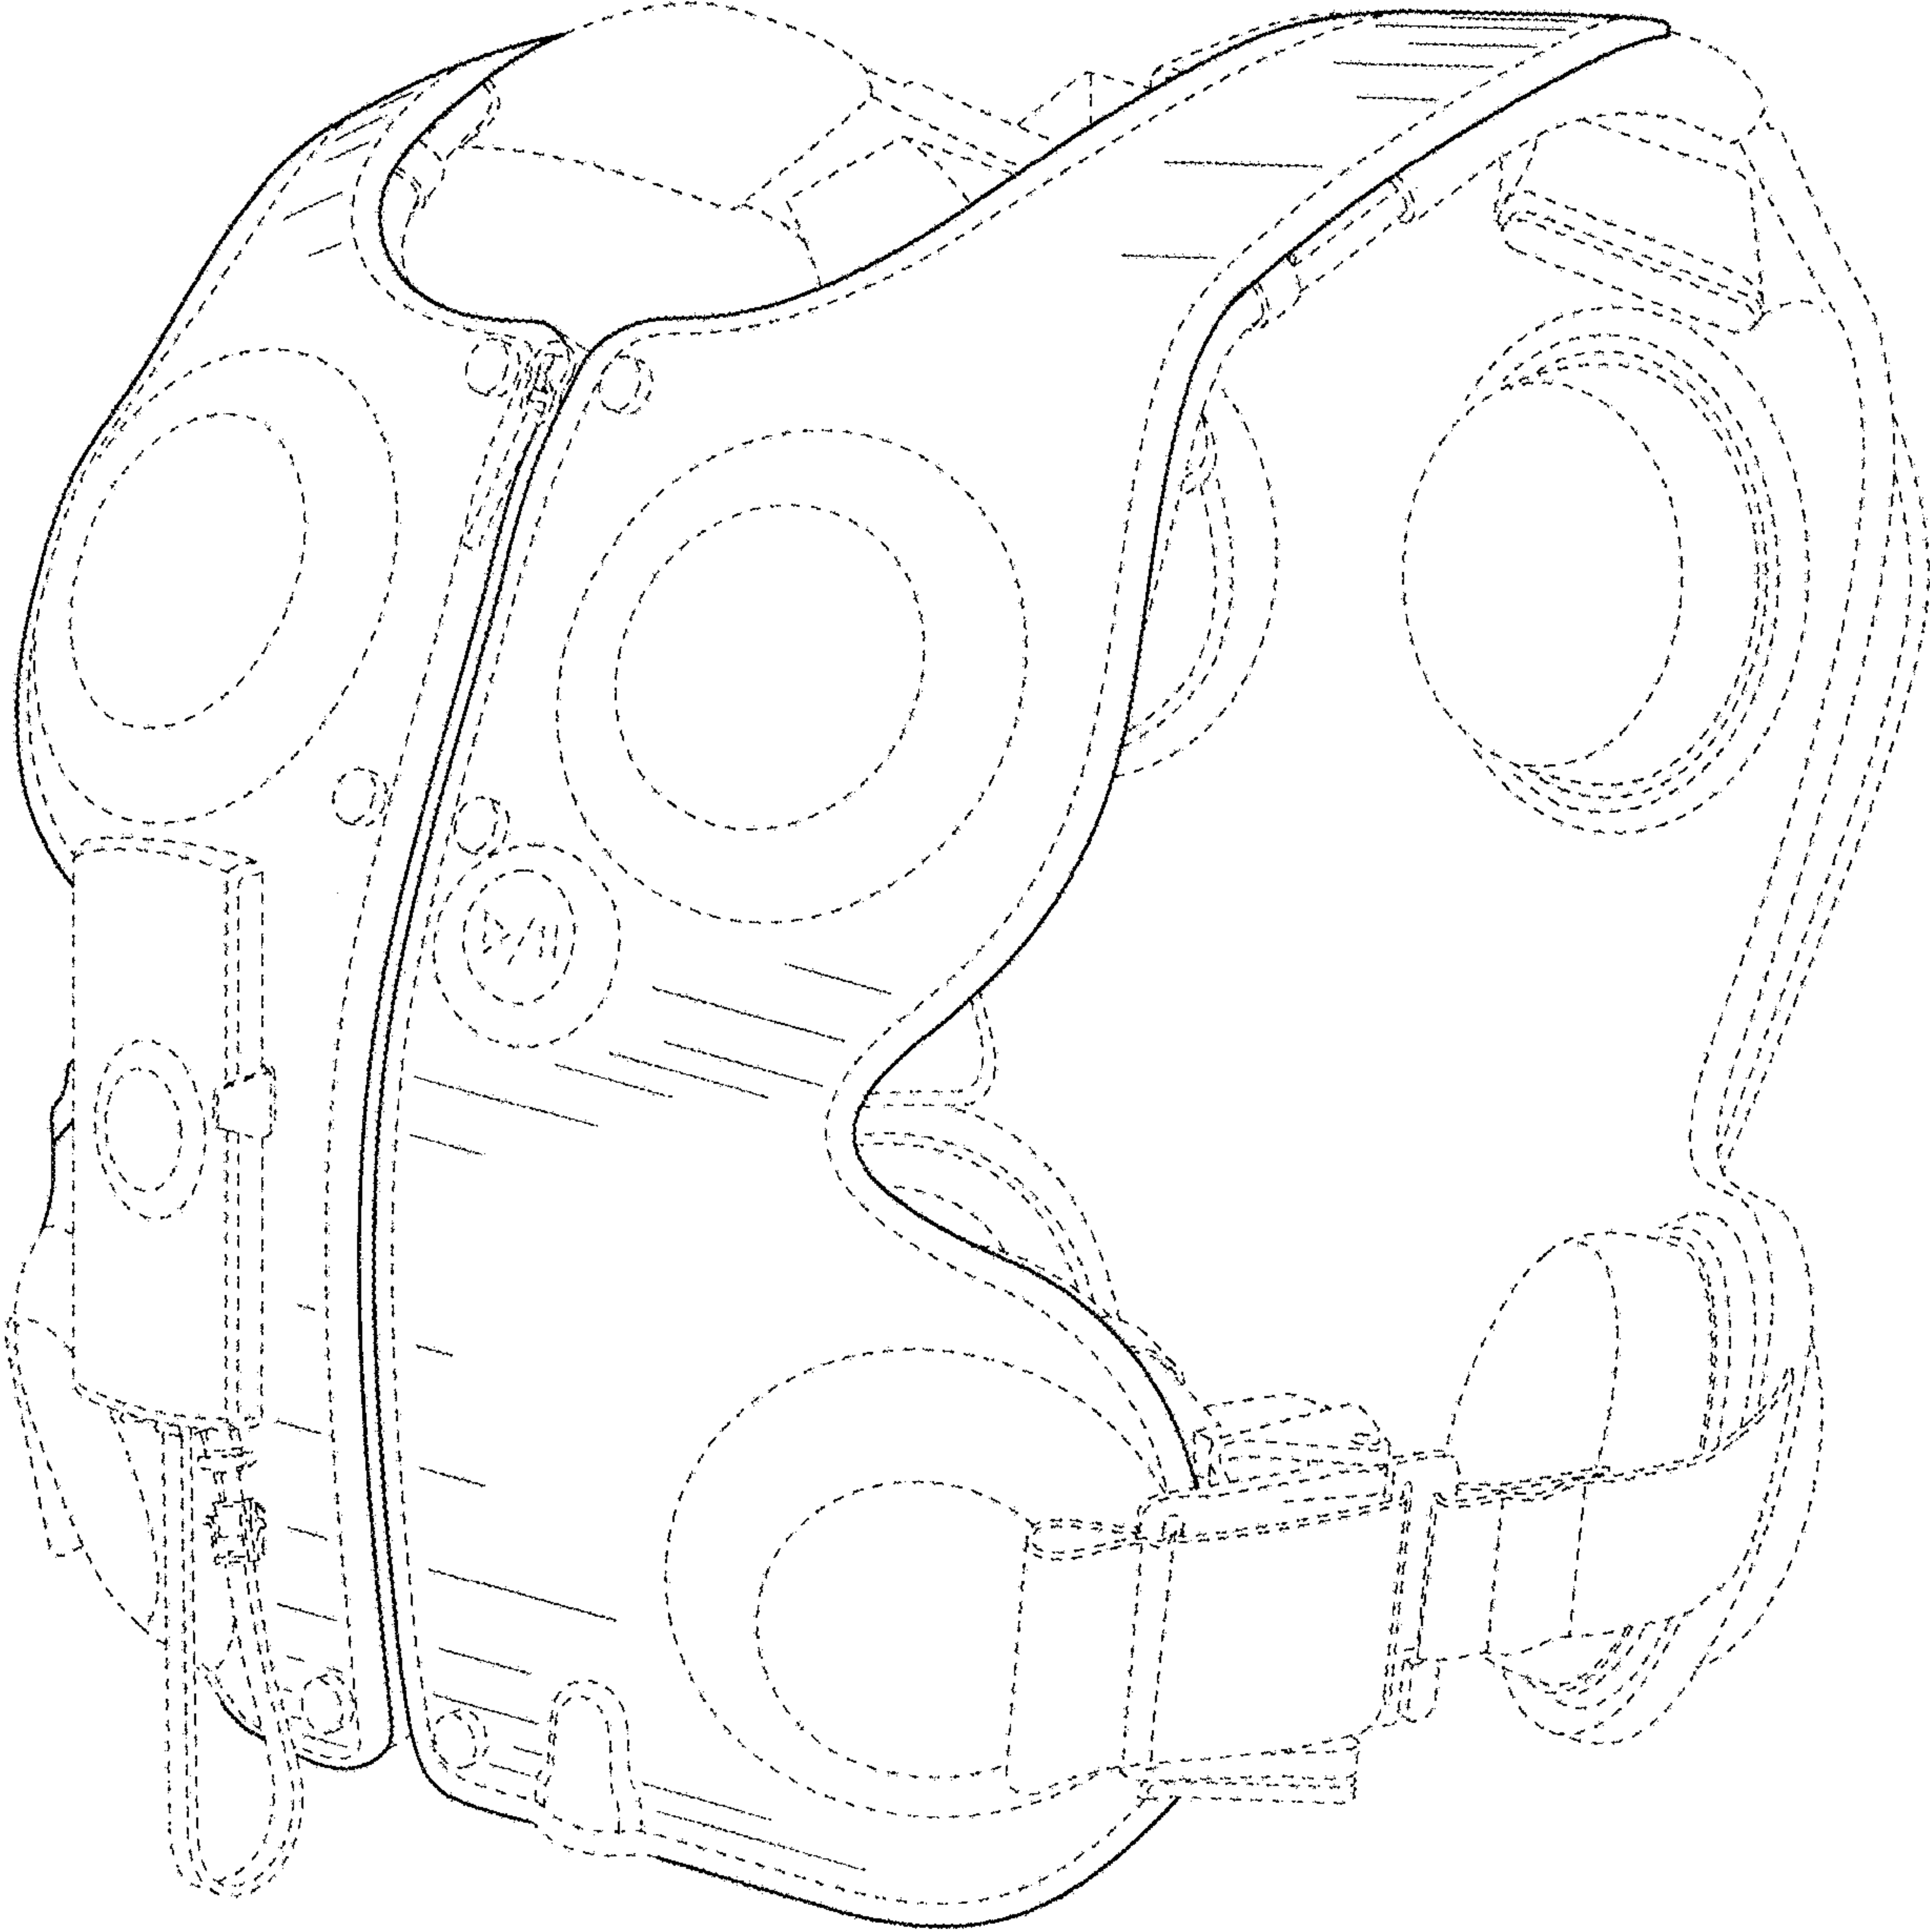

*FIG. 1*




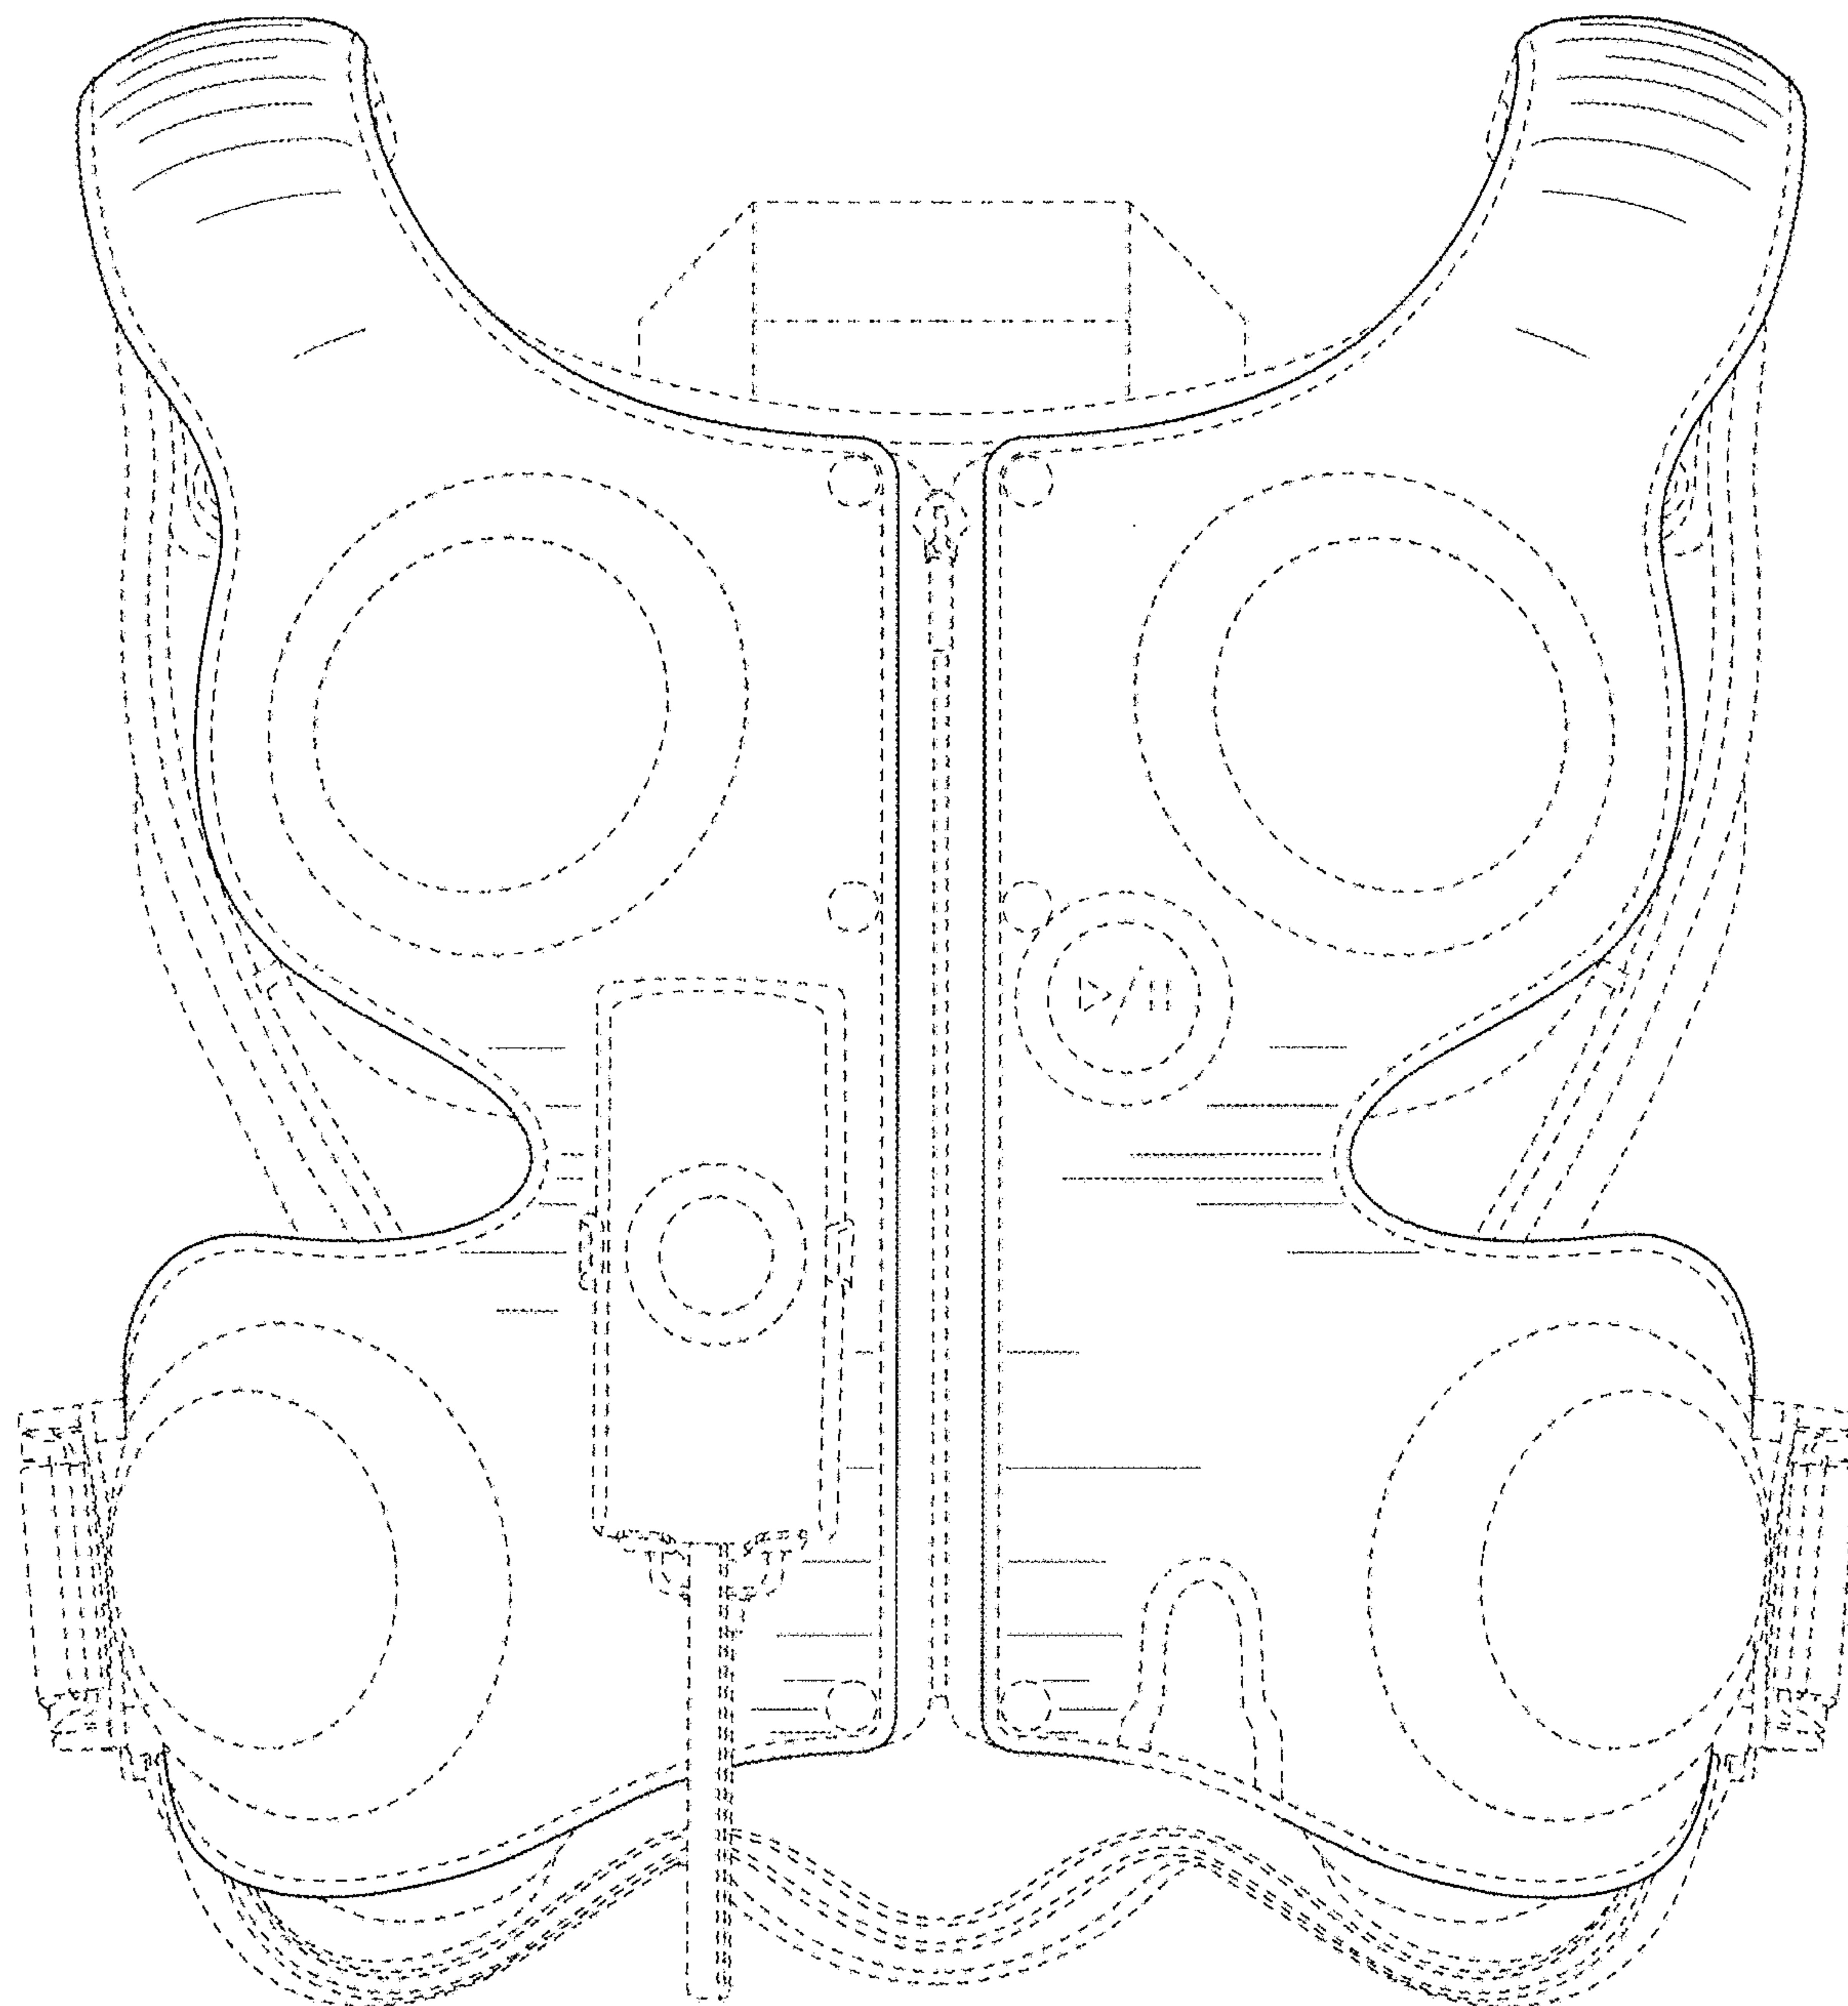


FIG. 2

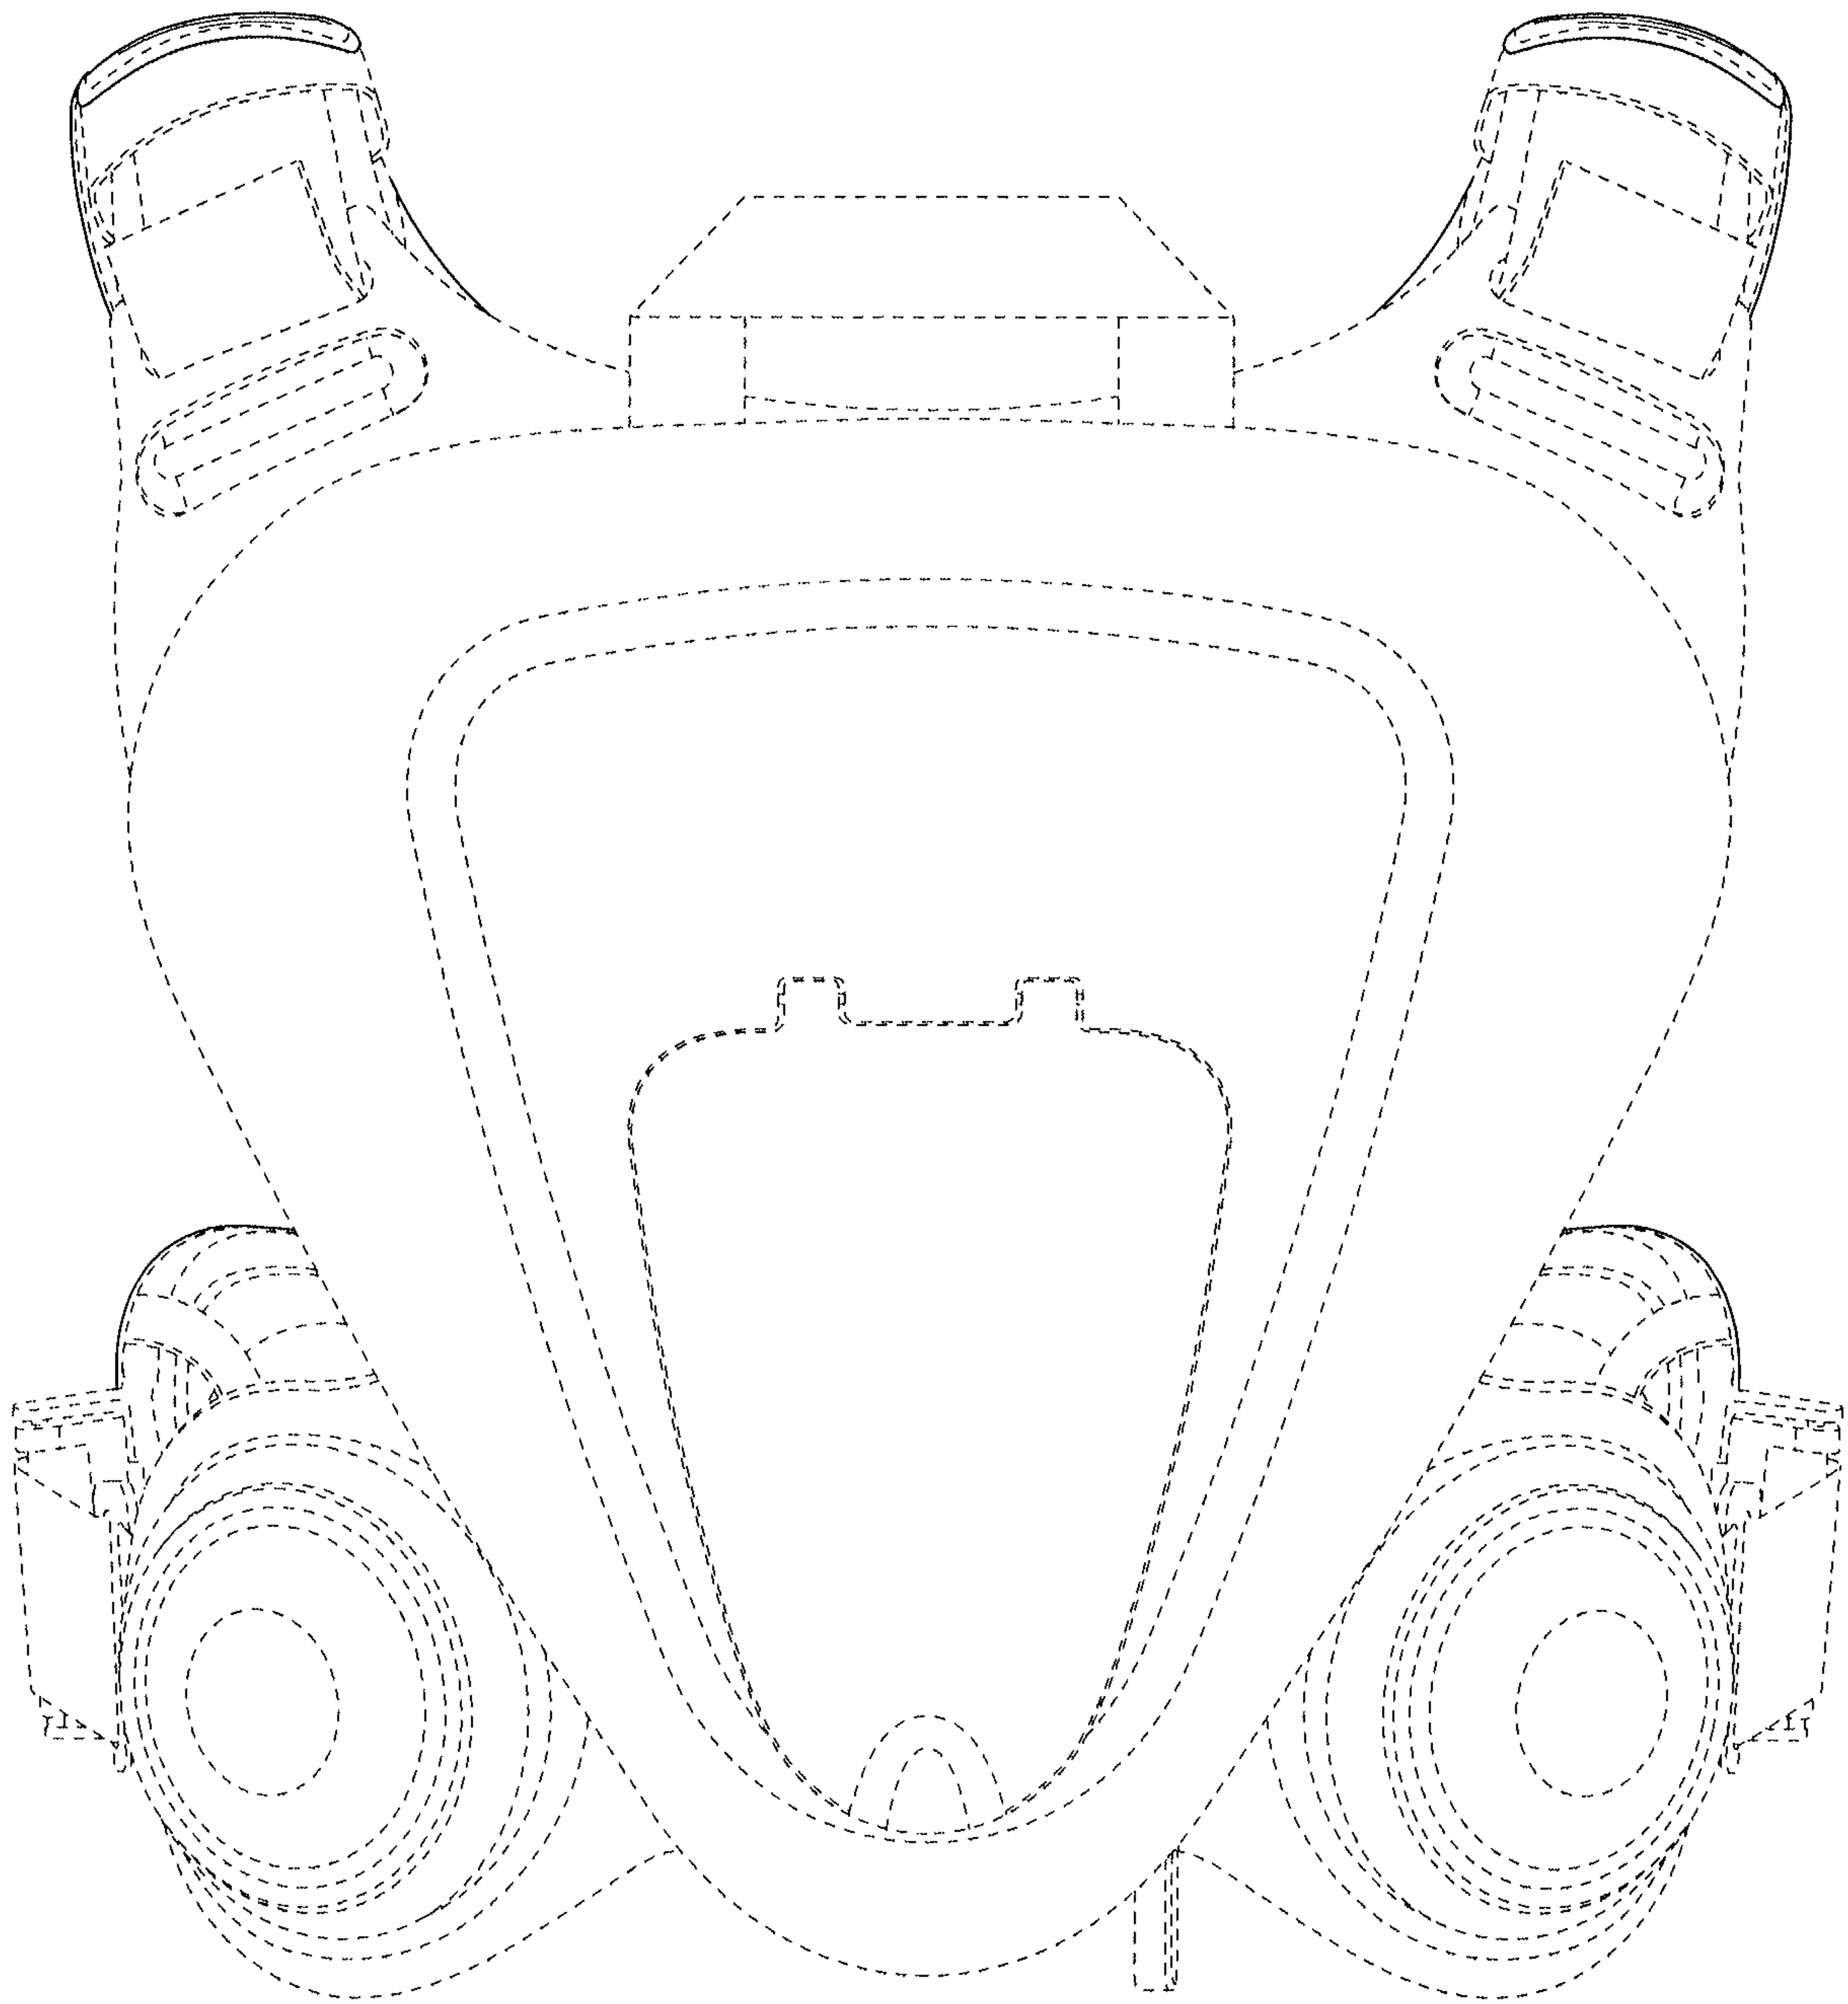

*FIG. 3*



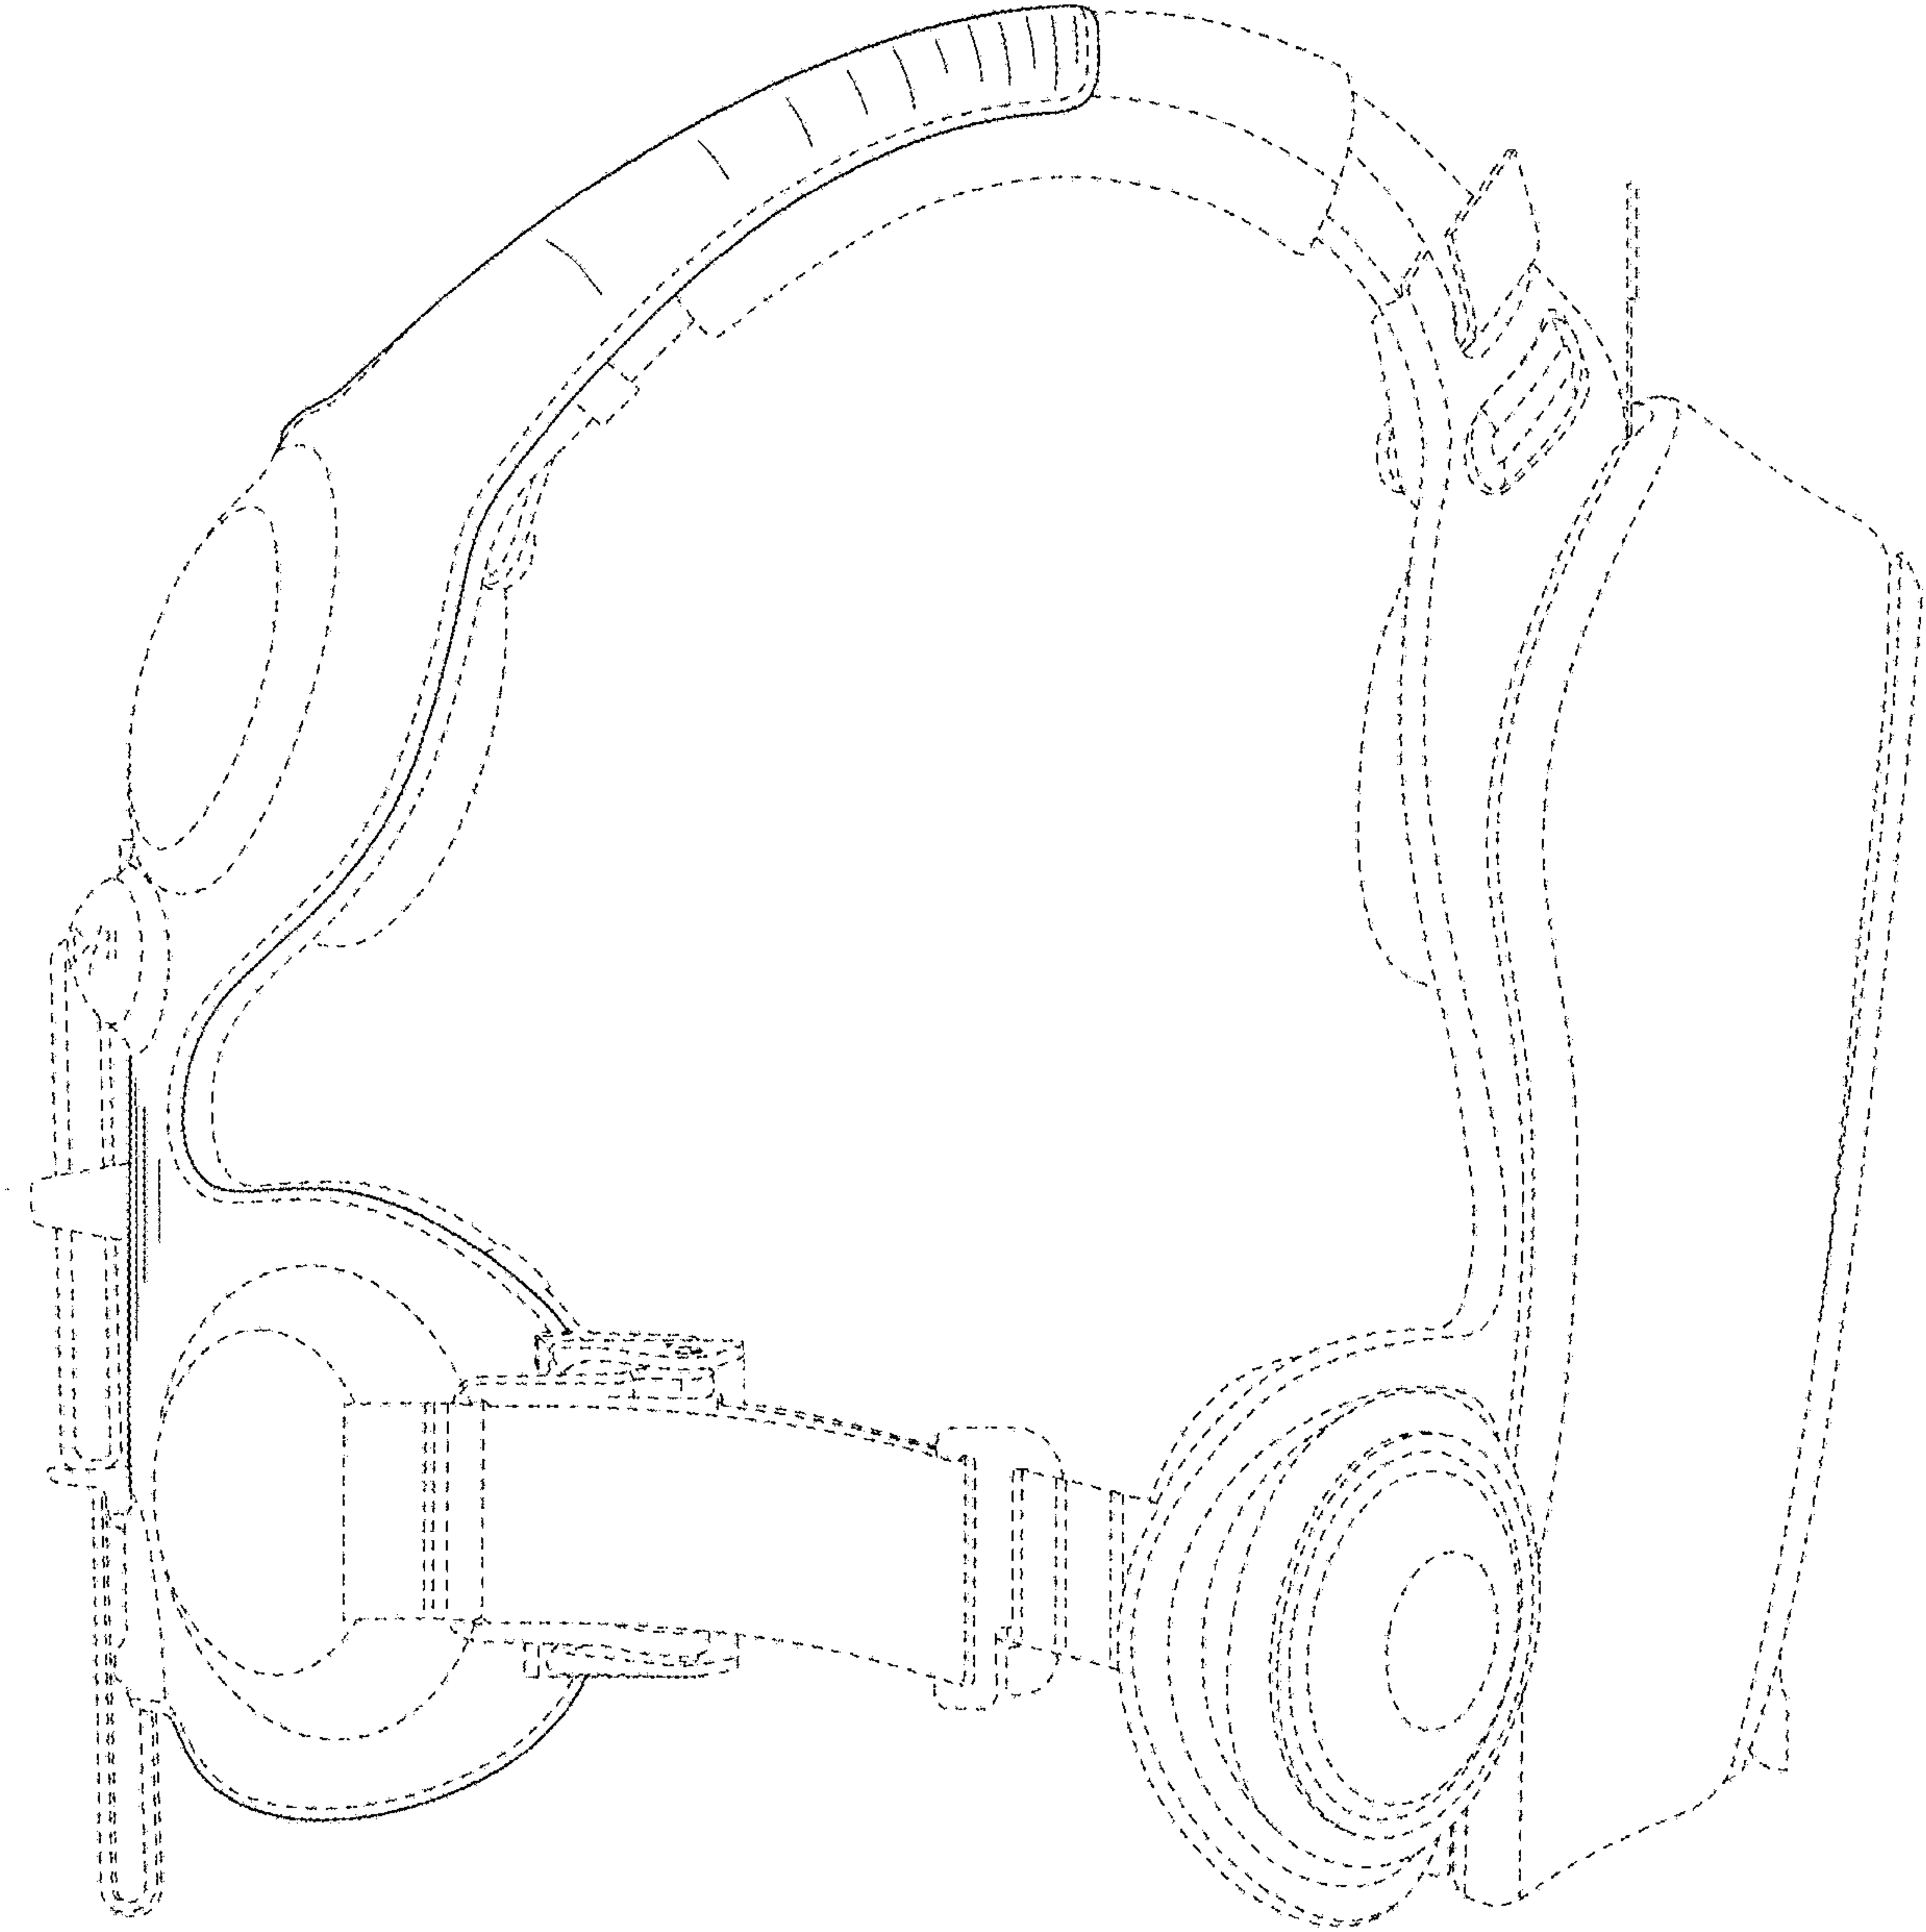


FIG. 4




*FIG. 5*

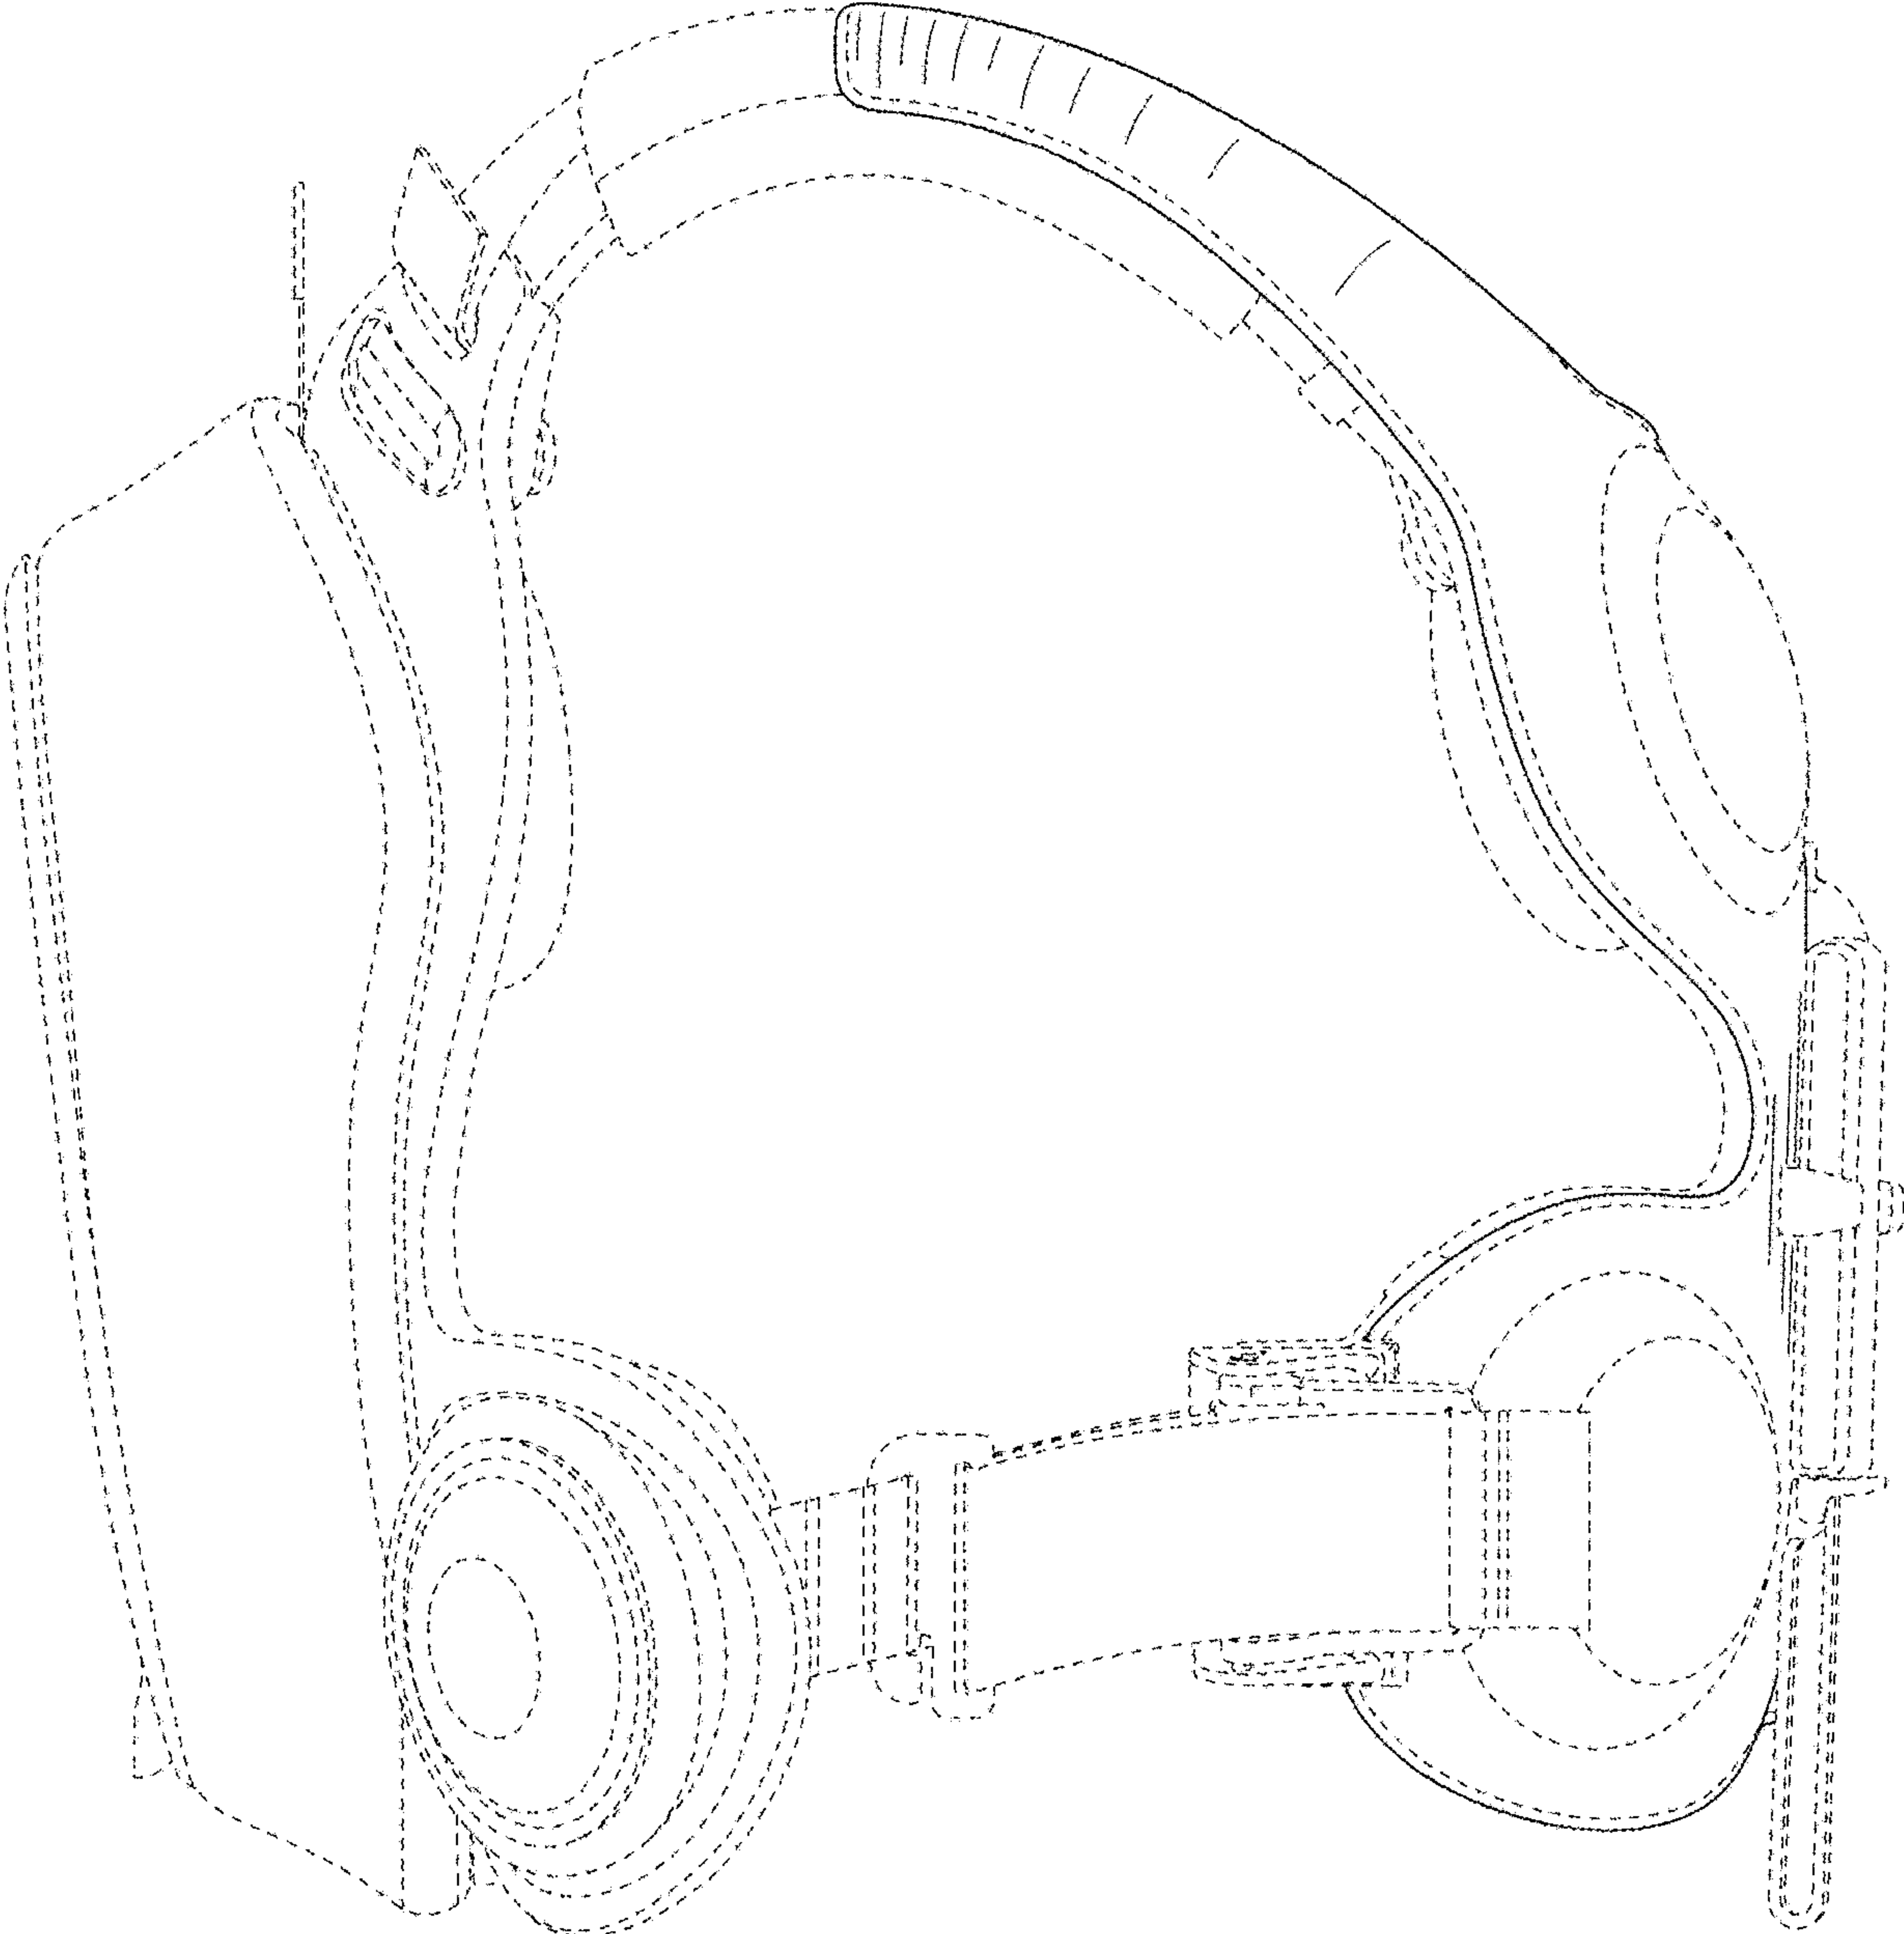

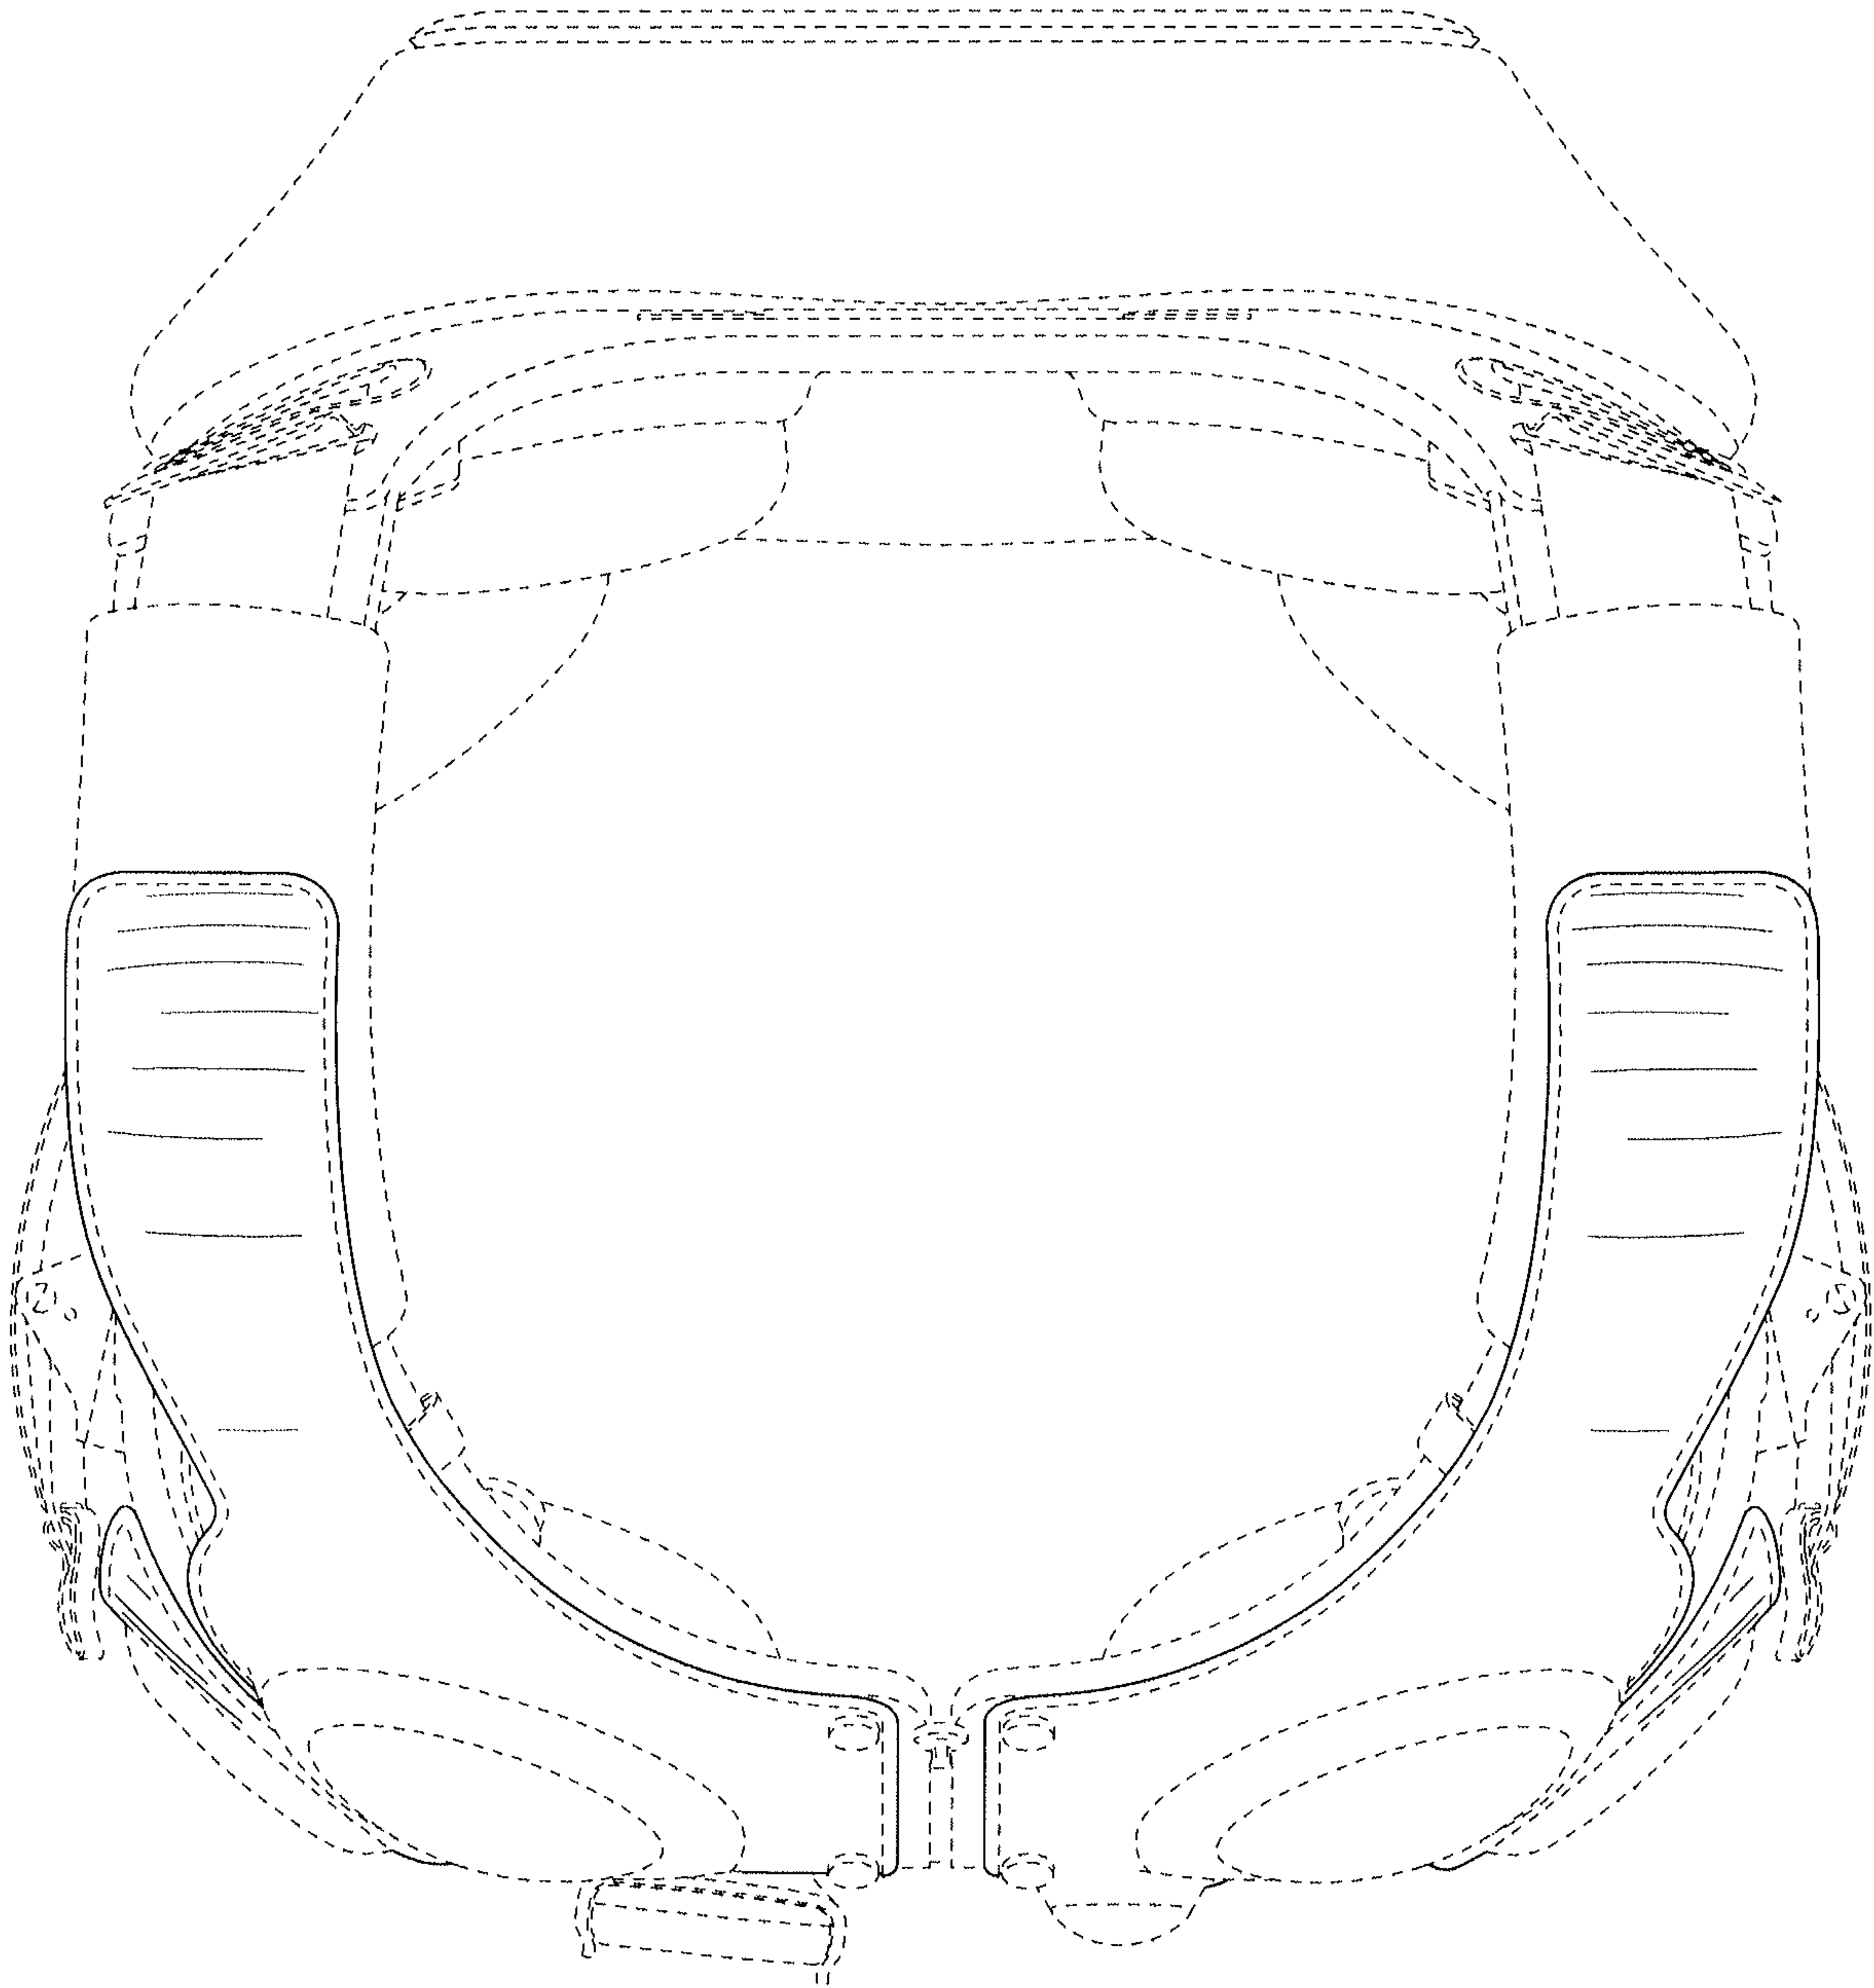

*FIG. 6*



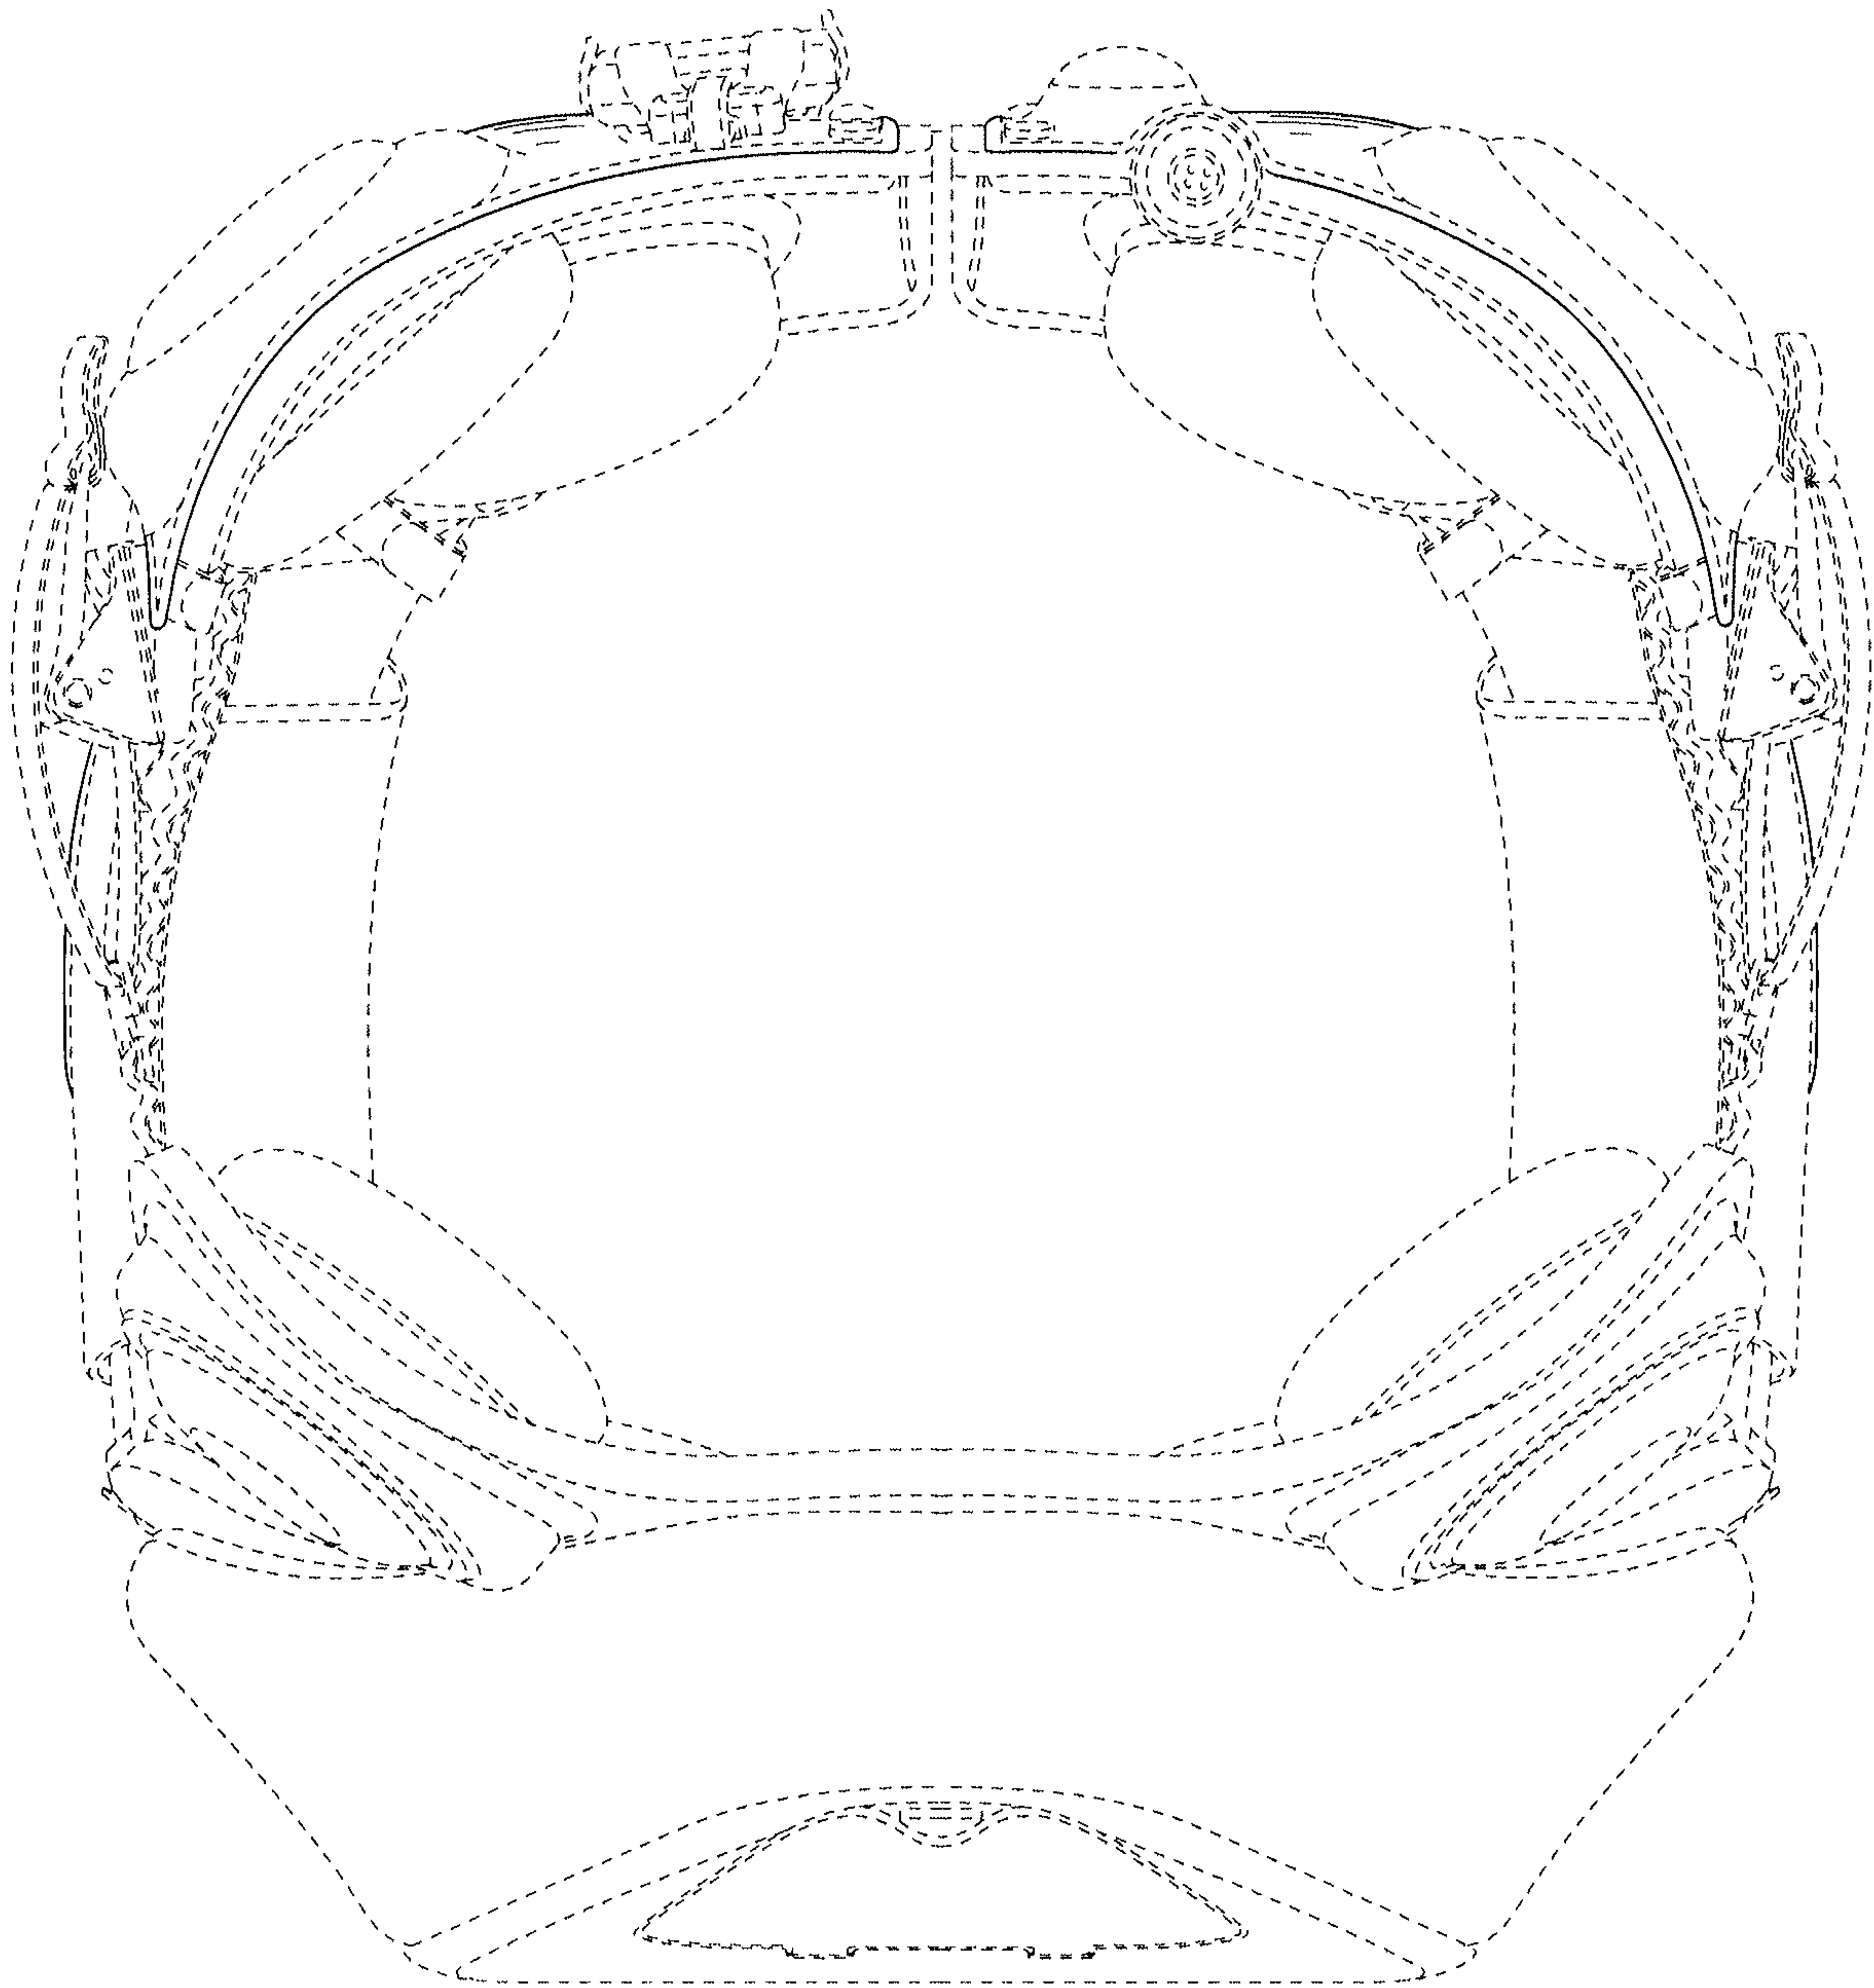

*FIG. 7*