



US00D937435S

(12) **United States Design Patent**
Rai et al.

(10) **Patent No.:** **US D937,435 S**

(45) **Date of Patent:** **** Nov. 30, 2021**

(54) **CARRIER FOR USE IN A DIAGNOSTIC ANALYZER**

https://pt.dotmed.com/listing/chemistry-analyzer/abbott-labs/architect/78850.102/1882008.*

(Continued)

(71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(72) Inventors: **Surya Pratap Rai**, Gurnee, IL (US);
Tingting Yu, Grayslake, IL (US);
Lauren Gerardi, San Francisco, CA (US);
Jose Pioquinto, Round Lake, IL (US);
Vincent A Ciriello, Denton, TX (US)

(74) *Attorney, Agent, or Firm* — Hanley, Flight & Zimmerman, LLC

(57) **CLAIM**

The ornamental design for a carrier for use in a diagnostic analyzer, as shown and described.

DESCRIPTION

(73) Assignee: **Abbott Laboratories**, Abbott Park, IL (US)

FIG. 1 is a front, right, top perspective view of a carrier for use in a diagnostic analyzer.

(**) Term: **15 Years**

FIG. 2 is a rear, left, top perspective view of the carrier of FIG. 1.

(21) Appl. No.: **29/690,282**

FIG. 3 is a rear, right, bottom perspective view of the carrier of FIG. 1.

(22) Filed: **May 7, 2019**

FIG. 4 is a front, left, bottom perspective view of the carrier of FIG. 1.

(51) **LOC (13) Cl.** **24-02**

FIG. 5 is a front view of the carrier of FIG. 1.

(52) **U.S. Cl.**

FIG. 6 is a rear view of the carrier of FIG. 1.

USPC **D24/230**

FIG. 7 is a right side view of the carrier of FIG. 1.

(58) **Field of Classification Search**

USPC D24/107, 108, 127, 128, 216, 217, 219,
D24/224, 227–232, 226; D10/81

FIG. 8 is a left side view of the carrier of FIG. 1.

FIG. 9 is a top view of the carrier of FIG. 1.

FIG. 10 is a bottom view of the carrier of FIG. 1.

(Continued)

FIG. 11 is a front, right, top perspective view of a carrier for use in a diagnostic analyzer.

(56) **References Cited**

FIG. 12 is a rear, left, top perspective view of the carrier of FIG. 11.

U.S. PATENT DOCUMENTS

FIG. 13 is a rear, right, bottom perspective view of the carrier of FIG. 11.

D333,522 S 2/1993 Gianino
D368,532 S * 4/1996 Jonkman D24/227

(Continued)

FIG. 14 is a front, left, bottom perspective view of the carrier of FIG. 11.

FOREIGN PATENT DOCUMENTS

JP D2015-12159 * 6/2015
JP D2018-15359 * 6/2017

FIG. 15 is a front view of the carrier of FIG. 11.

FIG. 16 is a rear view of the carrier of FIG. 11.

FIG. 17 is a right side view of the carrier of FIG. 11.

FIG. 18 is a left side view of the carrier of FIG. 11.

FIG. 19 is a top view of the carrier of FIG. 11; and,



FIG. 20 is a bottom view of the carrier of FIG. 11.

OTHER PUBLICATIONS

Vende Se Abbott Labs Architect Chemistry Analyzer. Online, published date unknown. Retrieved on Sep. 22, 2020 from URL:

The broken lines depict portions of the carrier for use in a diagnostic analyzer that form no part of the claimed design. The dash-dot lines indicate boundaries of the claim design, and form no part thereof.

1 Claim, 16 Drawing Sheets

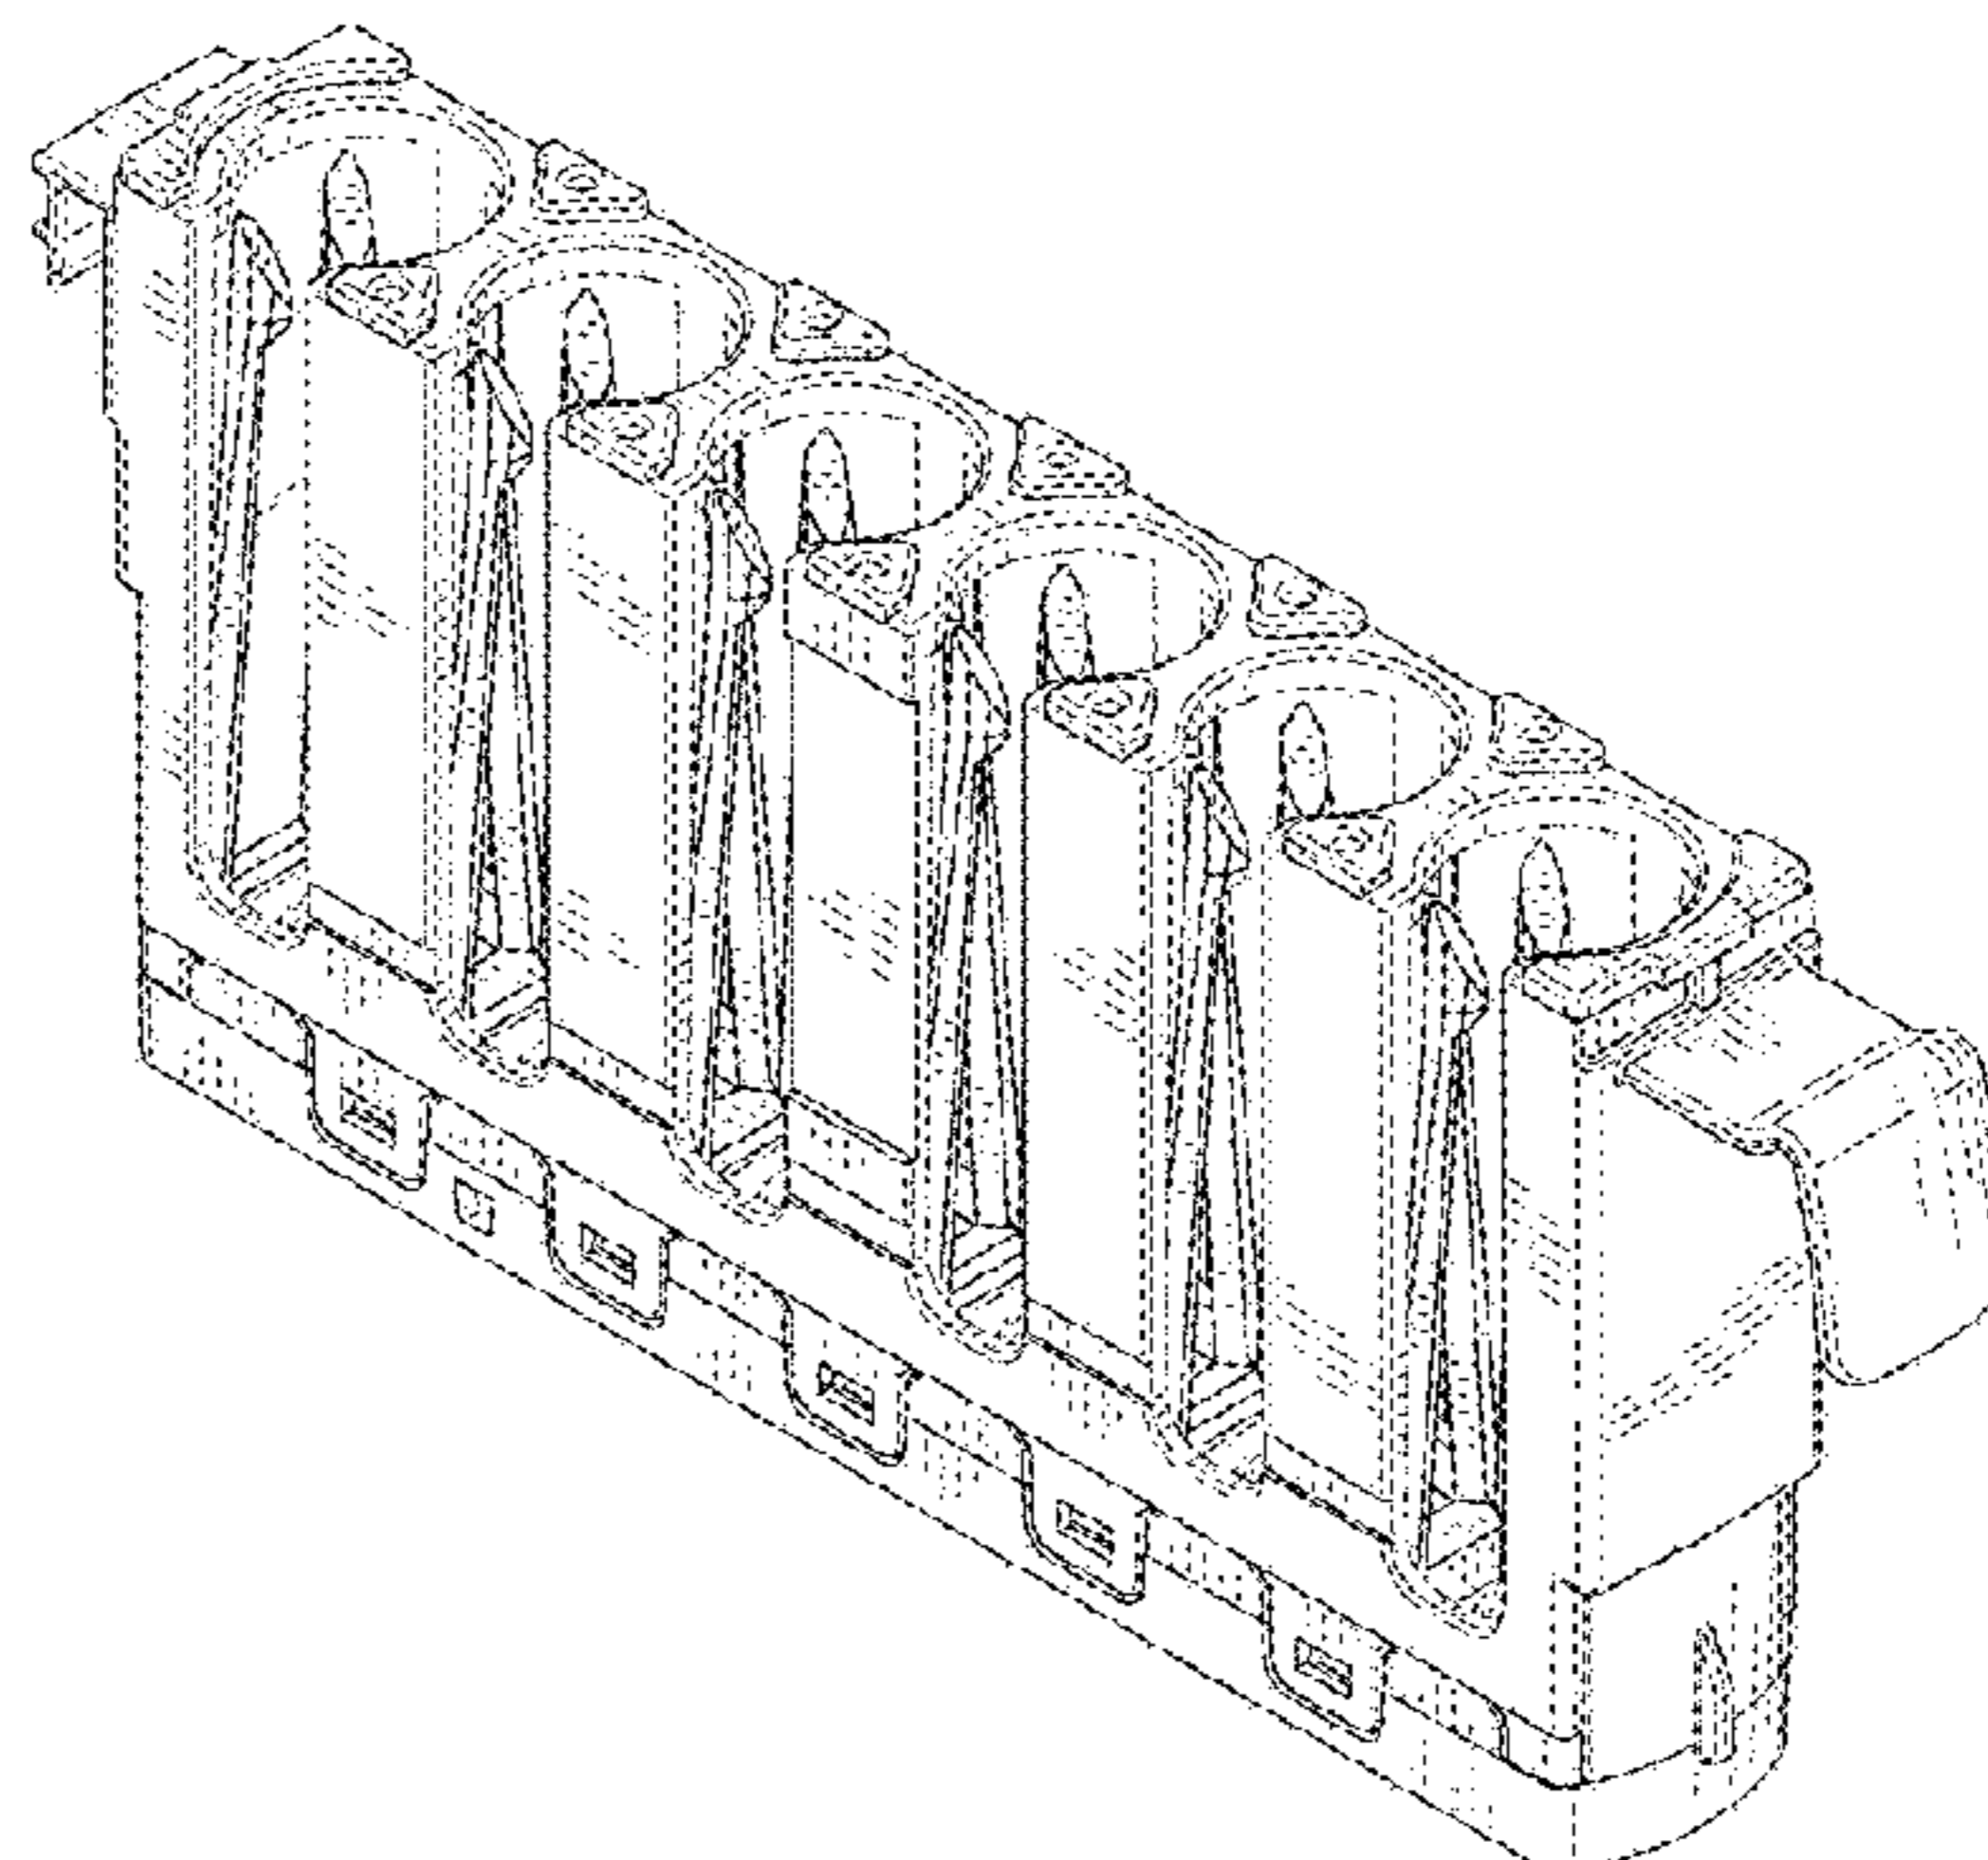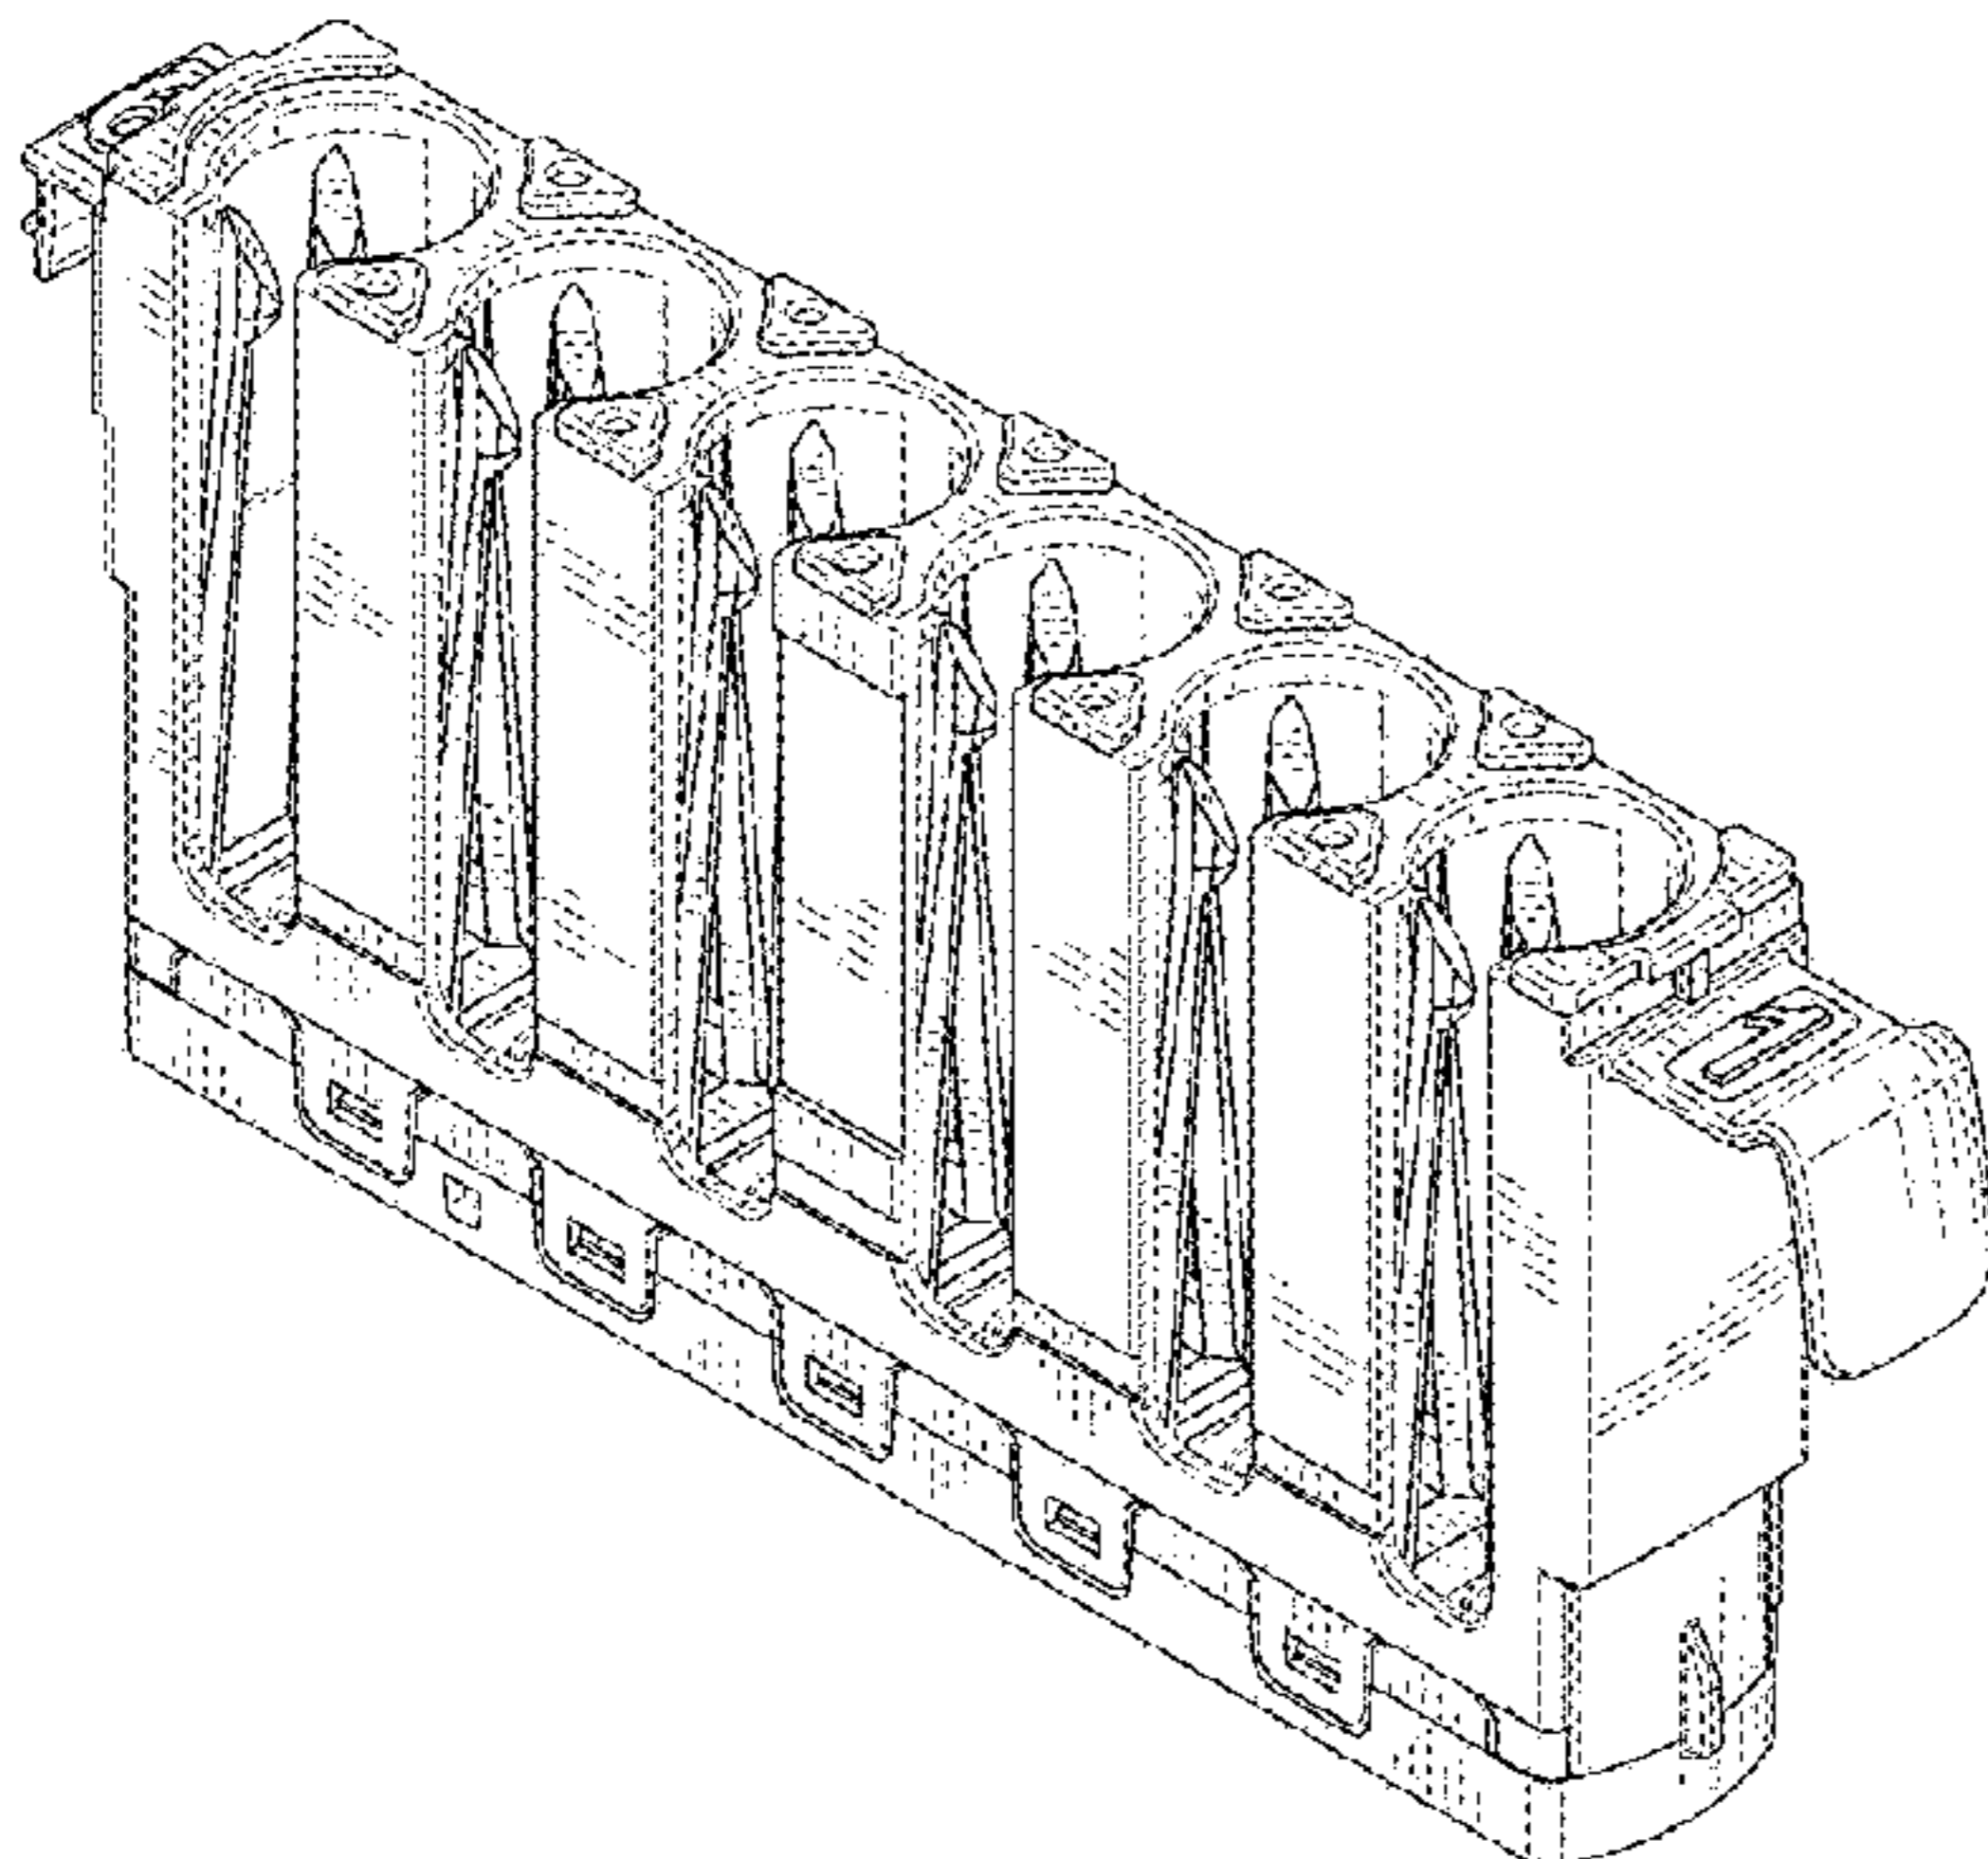

(58) **Field of Classification Search**
 CPC A61J 1/00; A61J 1/12; A61J 1/065; A61J
 1/067; B01L 9/00
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,589,137 A 12/1996 Markin et al.
 D382,346 S 8/1997 Buhler et al.
 5,700,429 A 12/1997 Buhler et al.
 5,861,563 A 1/1999 Boyd et al.
 D413,391 S 8/1999 Lapeus et al.
 D413,677 S 9/1999 Dumitrescu et al.
 5,948,360 A 9/1999 Rao et al.
 D417,009 S * 11/1999 Boyd D24/227
 D420,747 S * 2/2000 Dumitrescu D24/227
 D421,130 S 2/2000 Cohen et al.
 D428,497 S 7/2000 Lapeus et al.
 6,123,205 A 9/2000 Dumitrescu et al.
 6,588,625 B2 7/2003 Luoma, II et al.
 6,669,910 B1 12/2003 Bienhaus et al.
 D500,363 S 12/2004 Fanning et al.
 7,000,785 B2 2/2006 Jafari et al.
 7,132,082 B2 11/2006 Aviles et al.
 7,276,208 B2 10/2007 Sevigny et al.
 7,282,182 B2 10/2007 Dale et al.
 7,458,483 B2 12/2008 Luoma, II
 D595,423 S 6/2009 Johansson et al.
 D603,524 S 11/2009 Suzuki et al.
 7,628,954 B2 12/2009 Gomm et al.
 7,682,565 B2 3/2010 Linton et al.
 7,688,207 B2 3/2010 Fritchie et al.
 7,858,031 B2 12/2010 Schutt et al.
 D630,317 S * 1/2011 Wung D24/128

7,947,225 B2 5/2011 Itoh
 8,035,485 B2 10/2011 Fritchie
 8,147,777 B2 4/2012 Schacher et al.
 8,309,036 B2 11/2012 Clark et al.
 D674,507 S 1/2013 Suzuki et al.
 D675,338 S 1/2013 Suzuki et al.
 D686,337 S * 7/2013 Tarunina D24/224
 8,906,321 B2 12/2014 Arras et al.
 8,939,364 B2 1/2015 Clark et al.
 9,011,802 B2 4/2015 Hagen
 9,117,192 B2 8/2015 Clark et al.
 9,144,801 B2 9/2015 Johnson et al.
 9,149,979 B2 10/2015 Sattler et al.
 D782,062 S * 3/2017 Luoma, II D24/224
 D782,063 S * 3/2017 Luoma, II D24/224
 D793,088 S * 8/2017 Ou D3/315
 D812,244 S * 3/2018 Shanafelter D24/230
 D837,401 S 1/2019 Gardner et al.
 D855,211 S * 7/2019 Ziegler D24/229
 D883,513 S * 5/2020 Jenoski D24/227
 D888,278 S * 6/2020 Madigan D24/227
 2005/0249634 A1 11/2005 Devlin, Sr.
 2009/0129990 A1 5/2009 Kokawa et al.
 2012/0051987 A1 3/2012 Johnson et al.
 2013/0078617 A1 3/2013 Ueda et al.
 2014/0273241 A1 9/2014 Ochraneck et al.
 2015/0338429 A1 11/2015 Rousseau et al.

OTHER PUBLICATIONS

Roche Cobas E411 Immunology Individual Sample Rack. Online, published date unknown. Retrieved on Sep. 22, 2020 from URL: <https://wytec.com.pt/roche/20-roche-cobas-e411-immunology-individual-sample-rack.html>.*

* cited by examiner

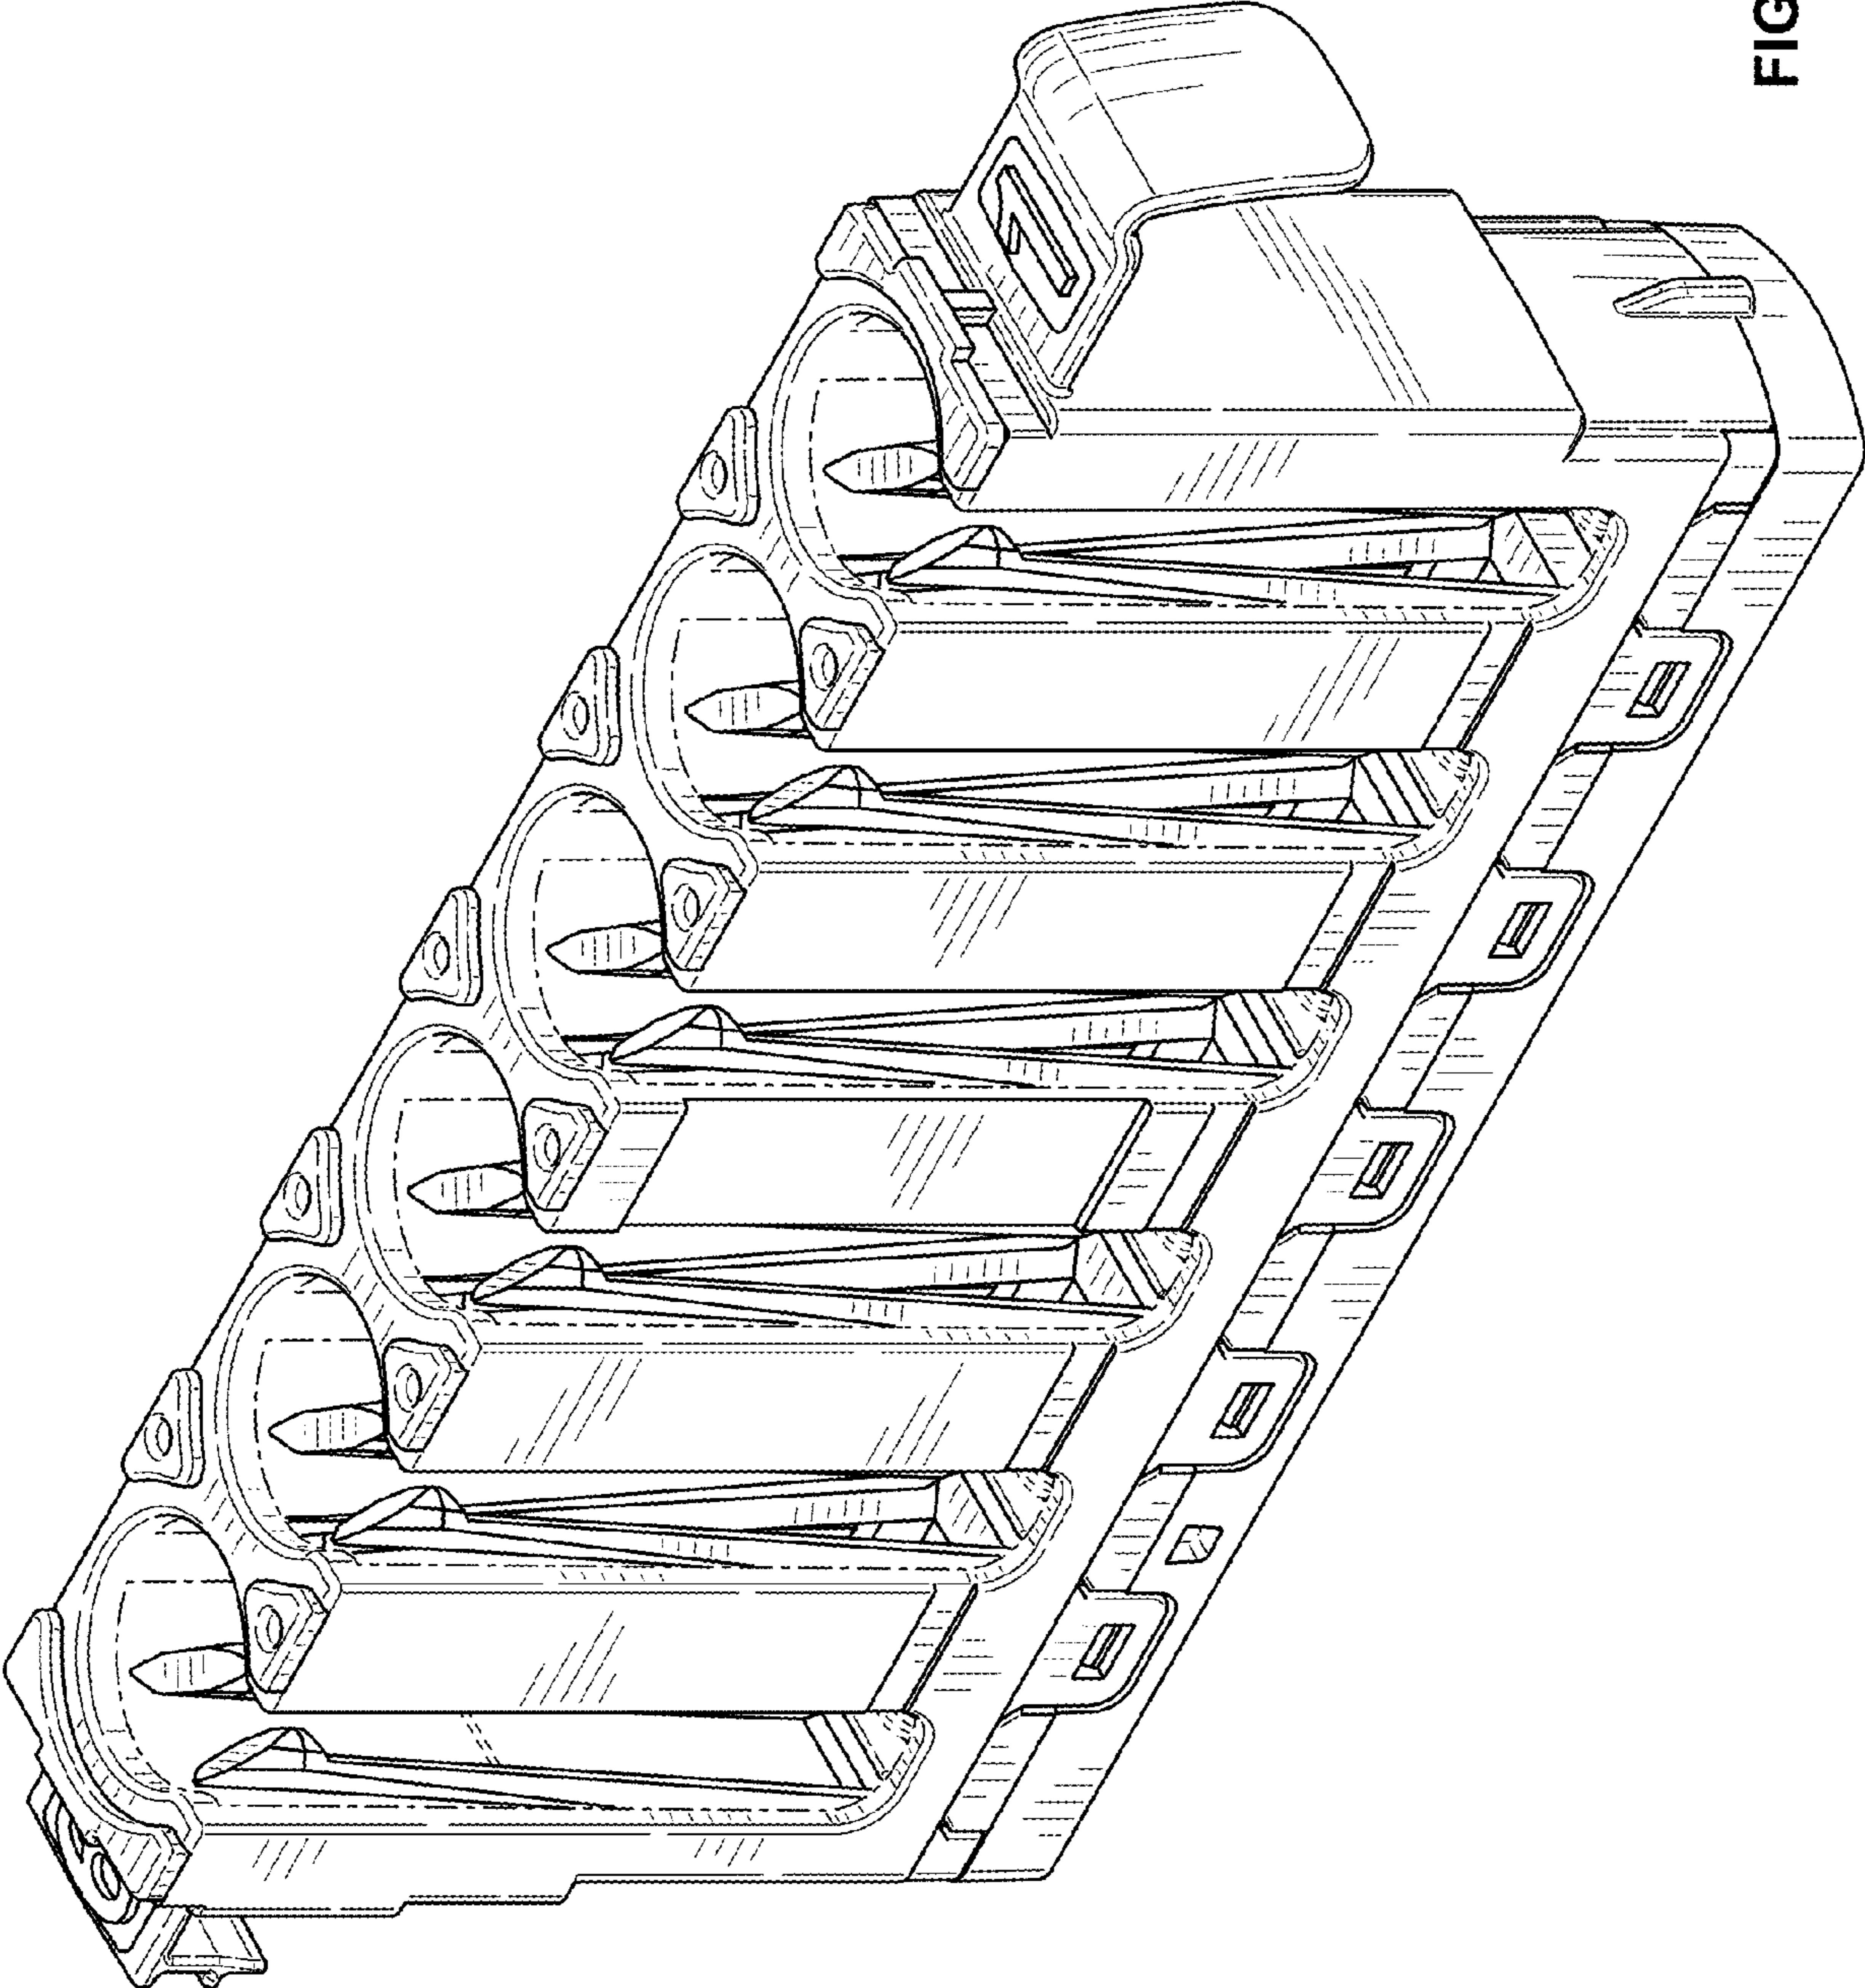


FIG. 1

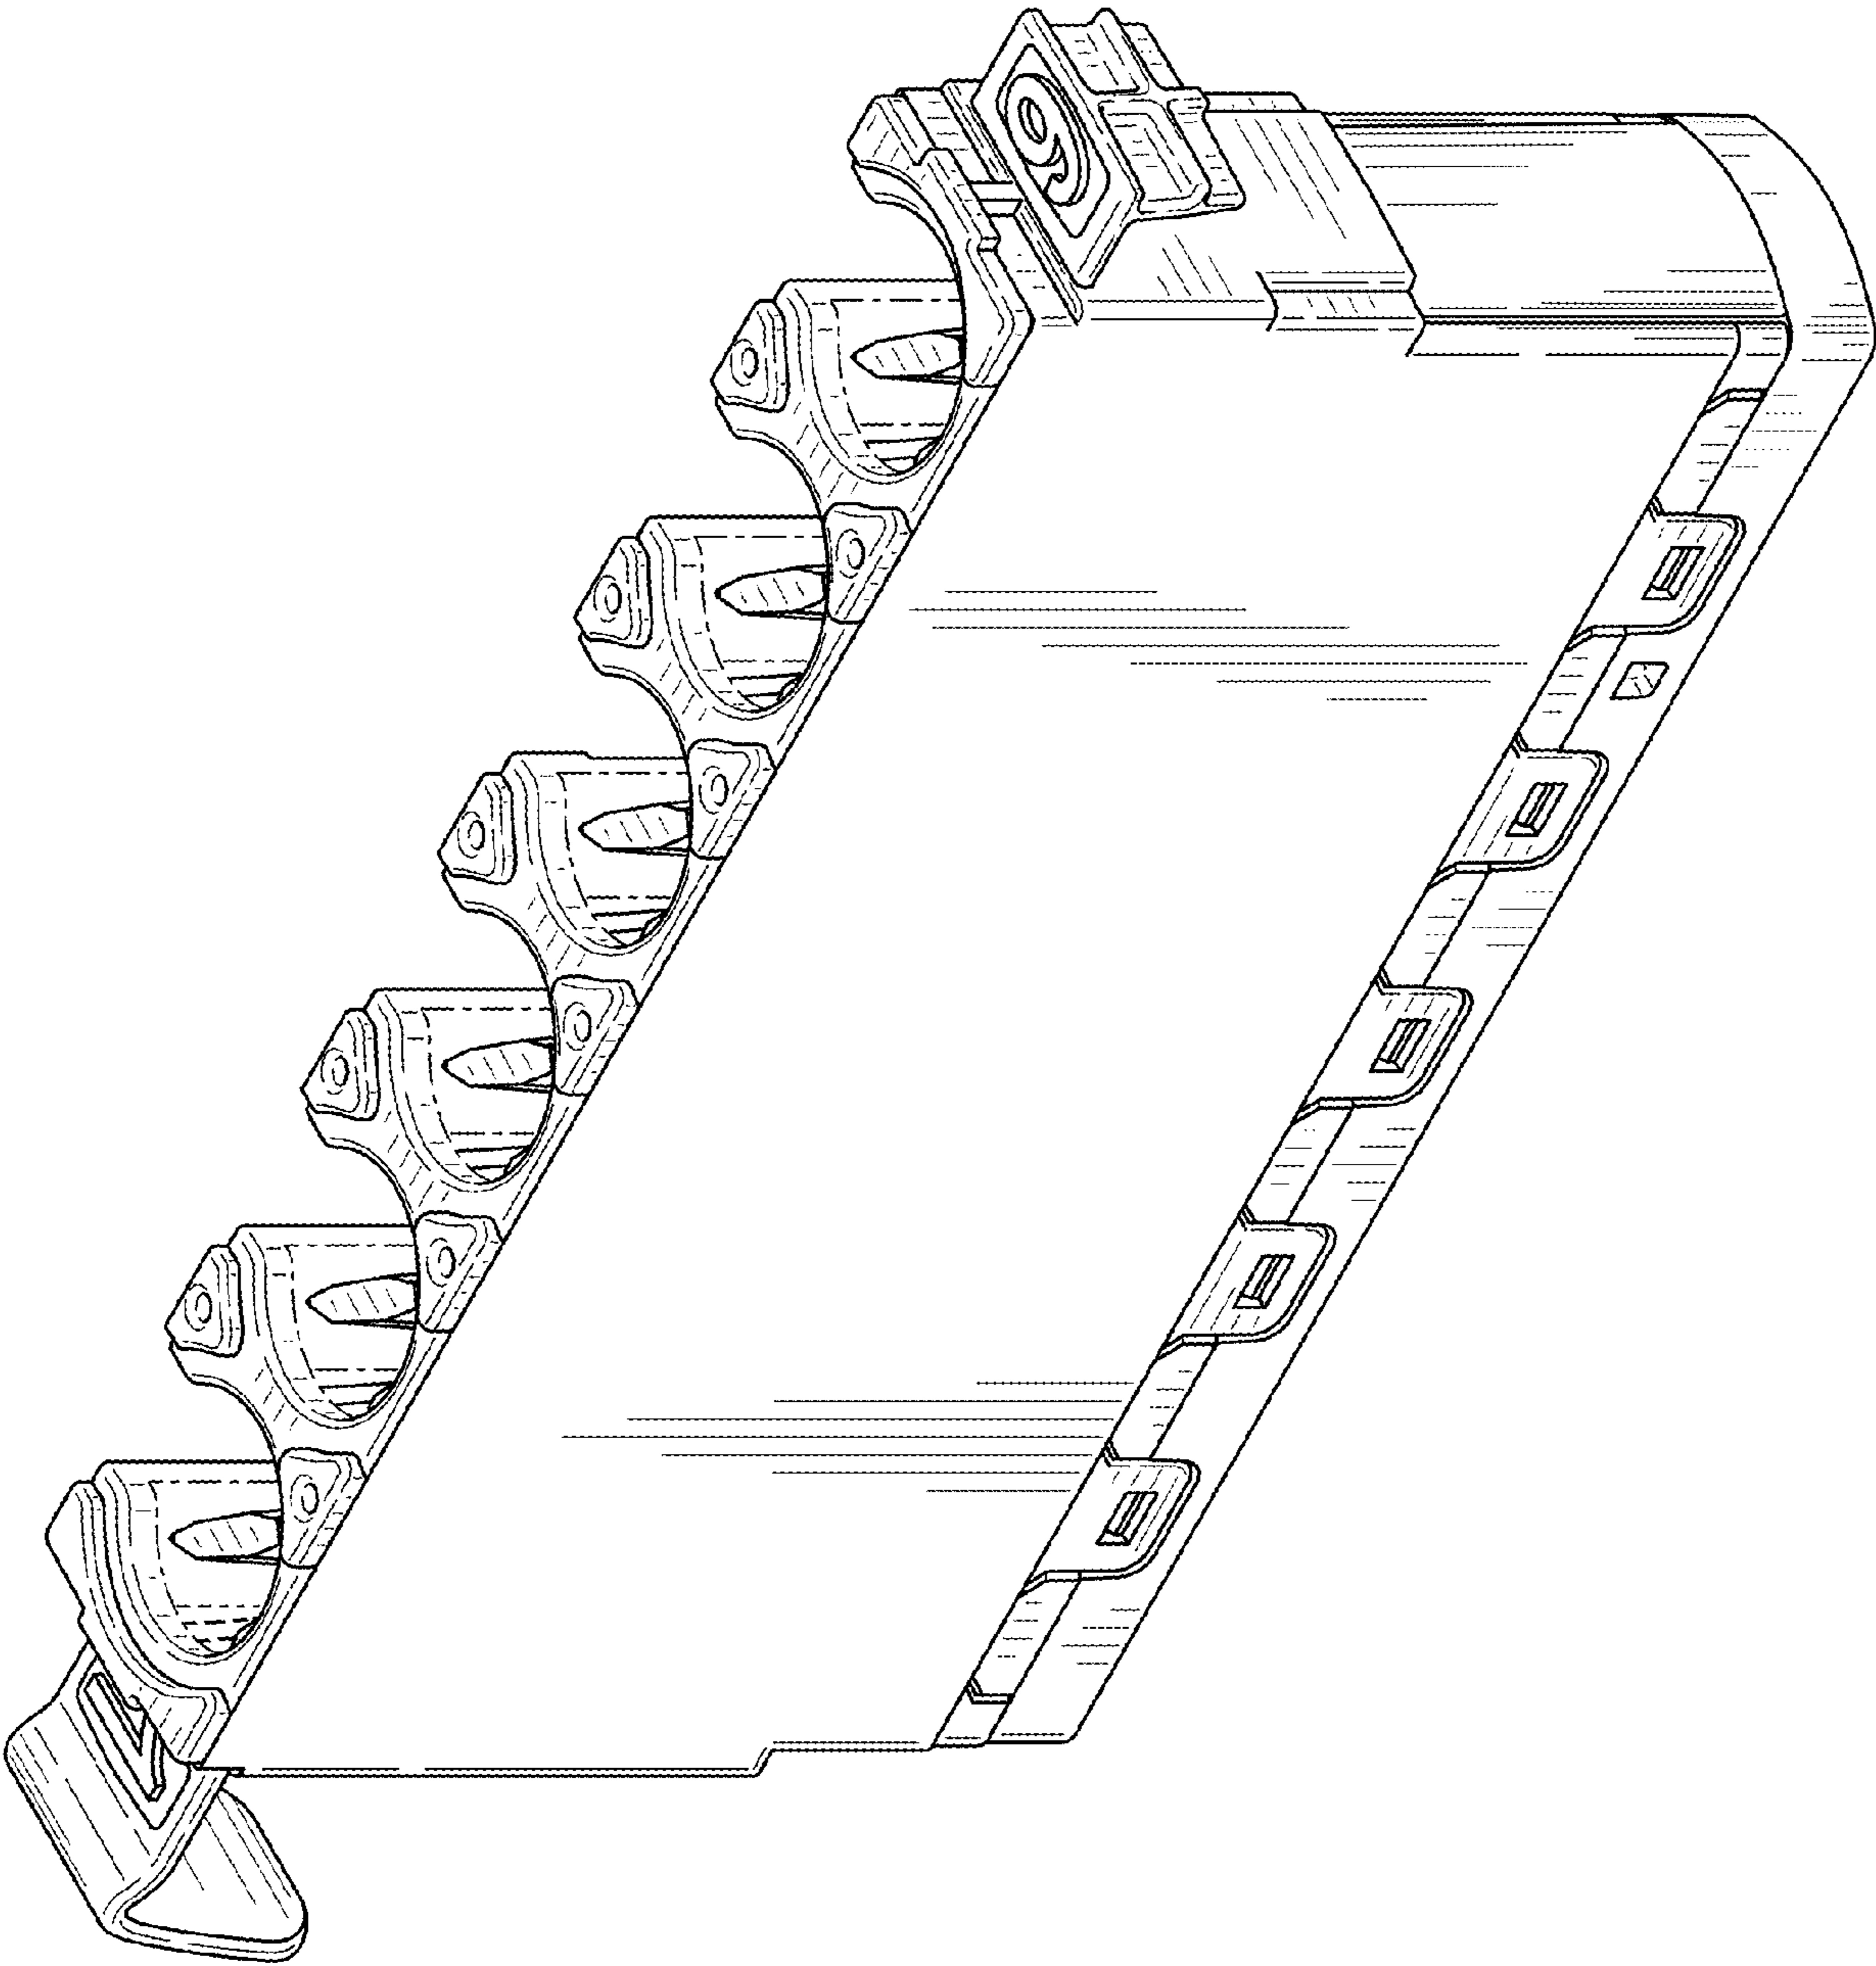


FIG. 2

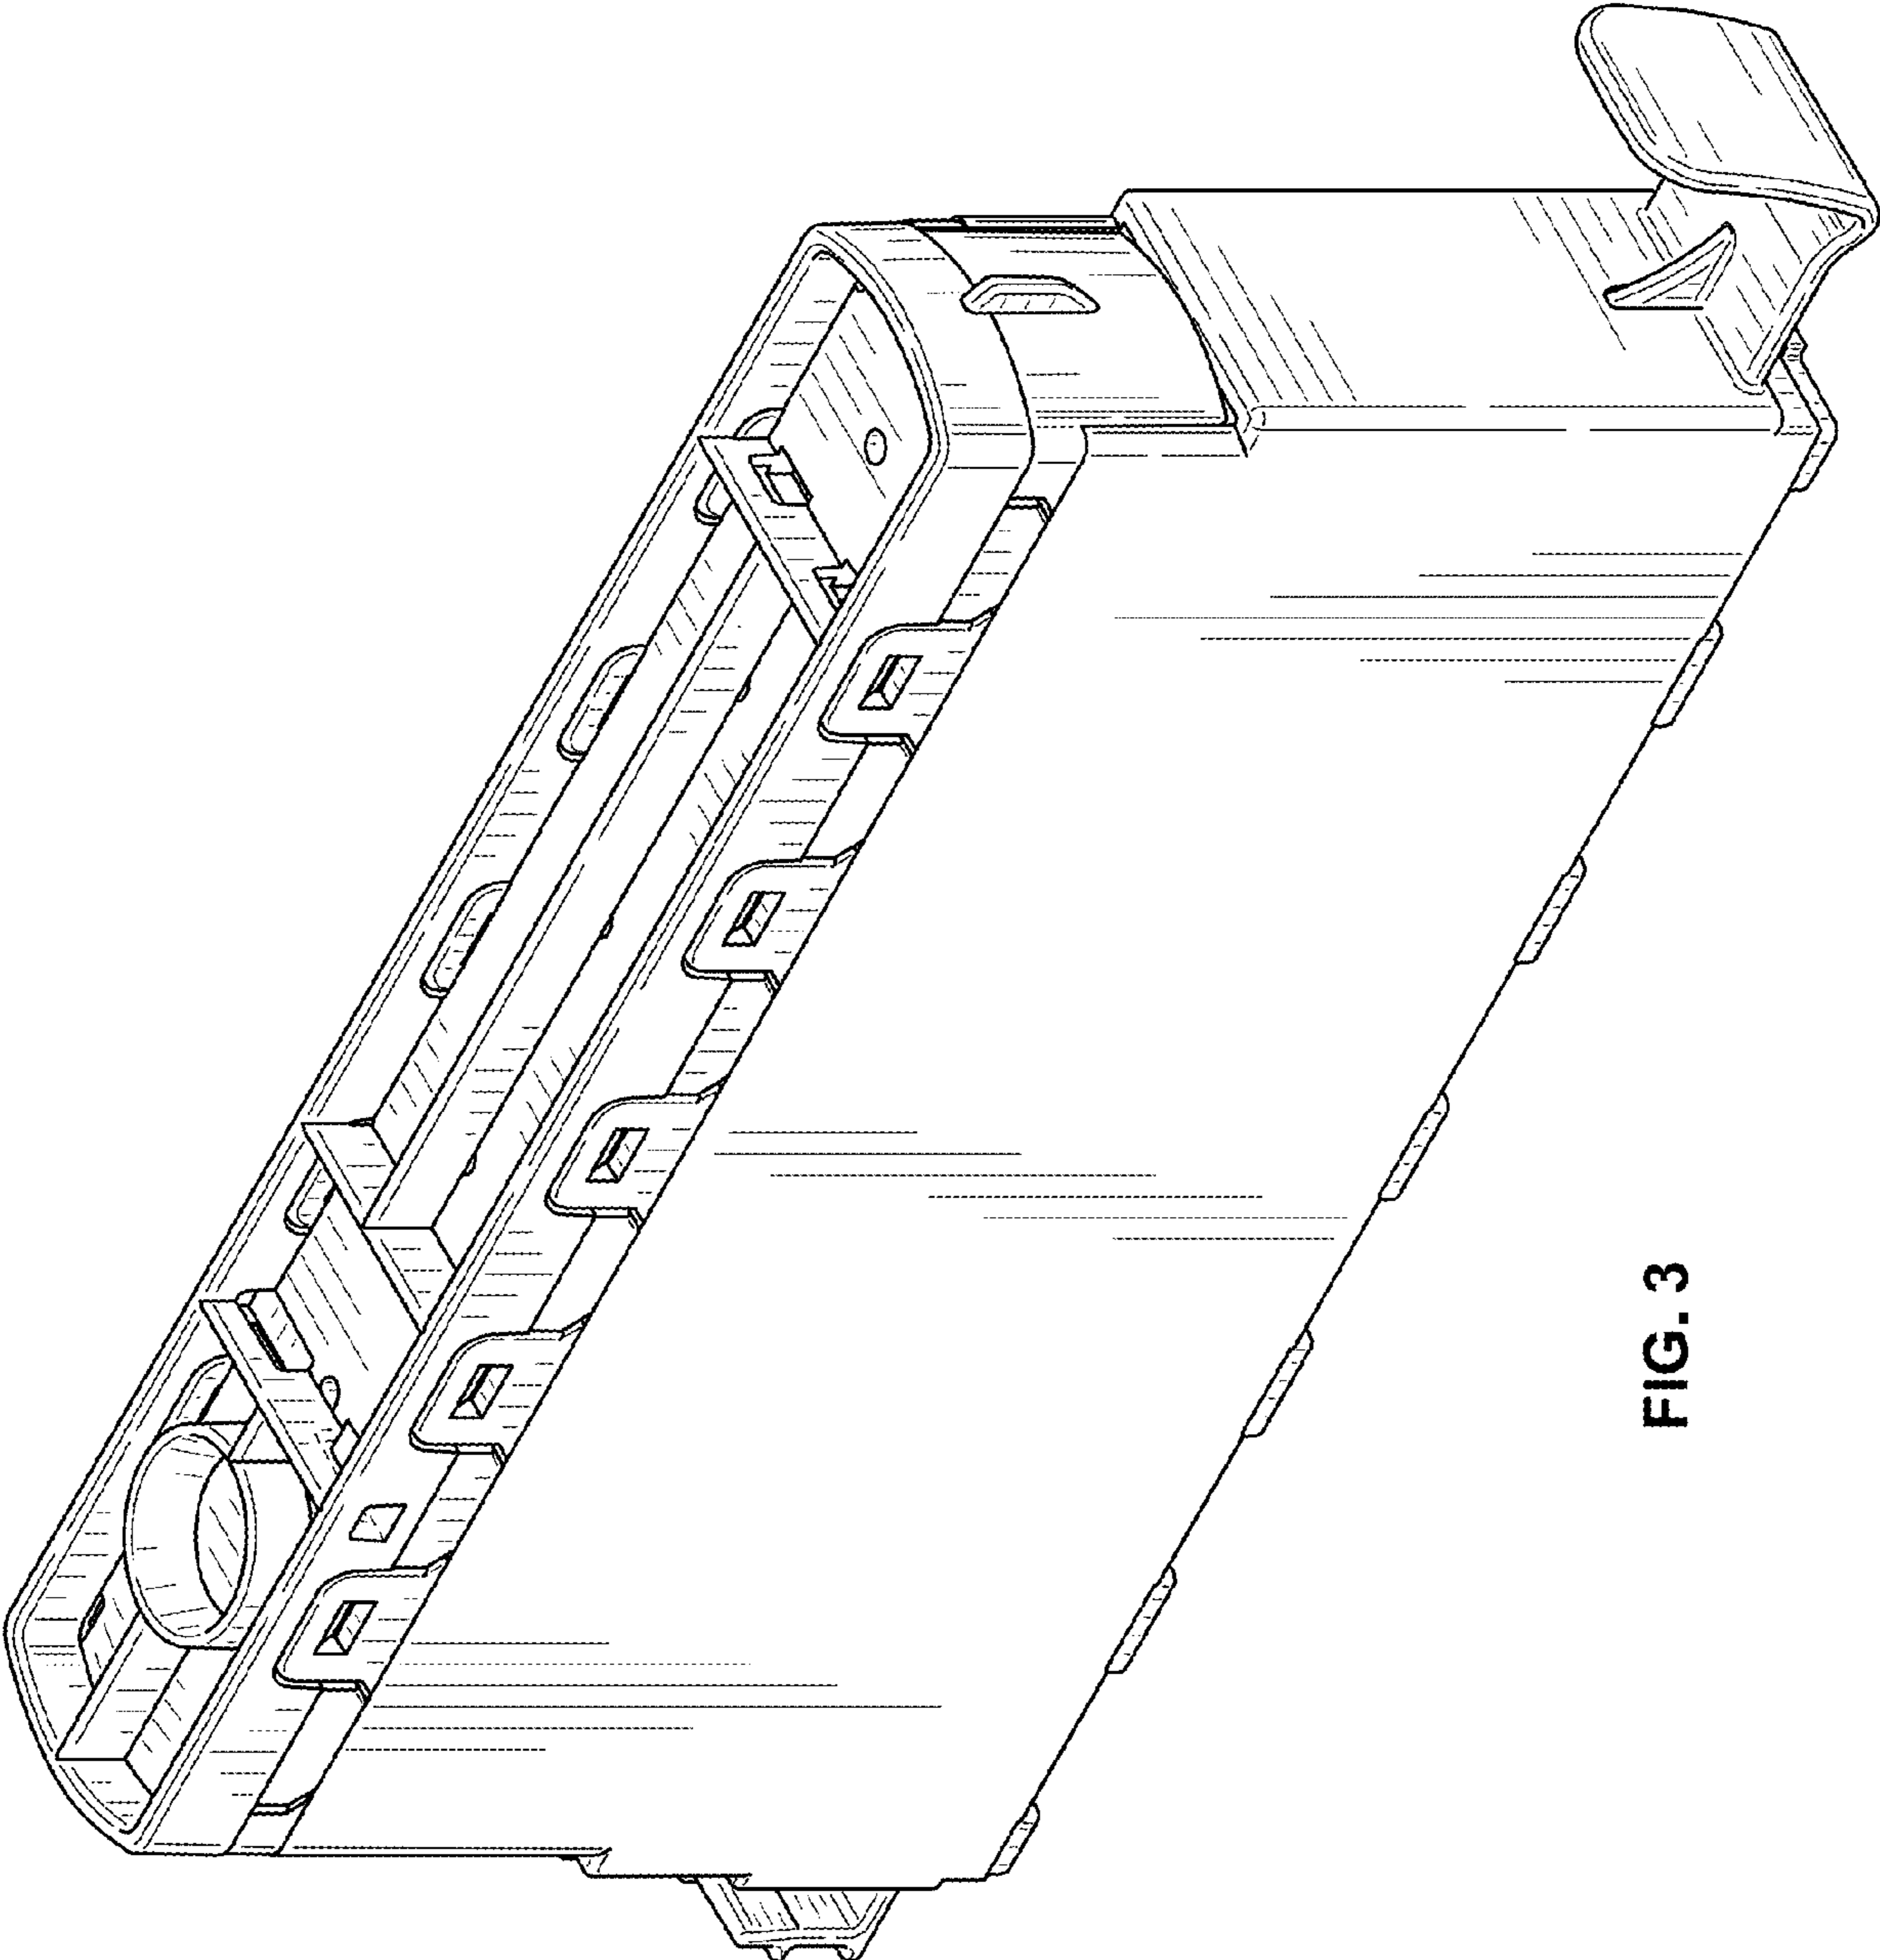


FIG. 3

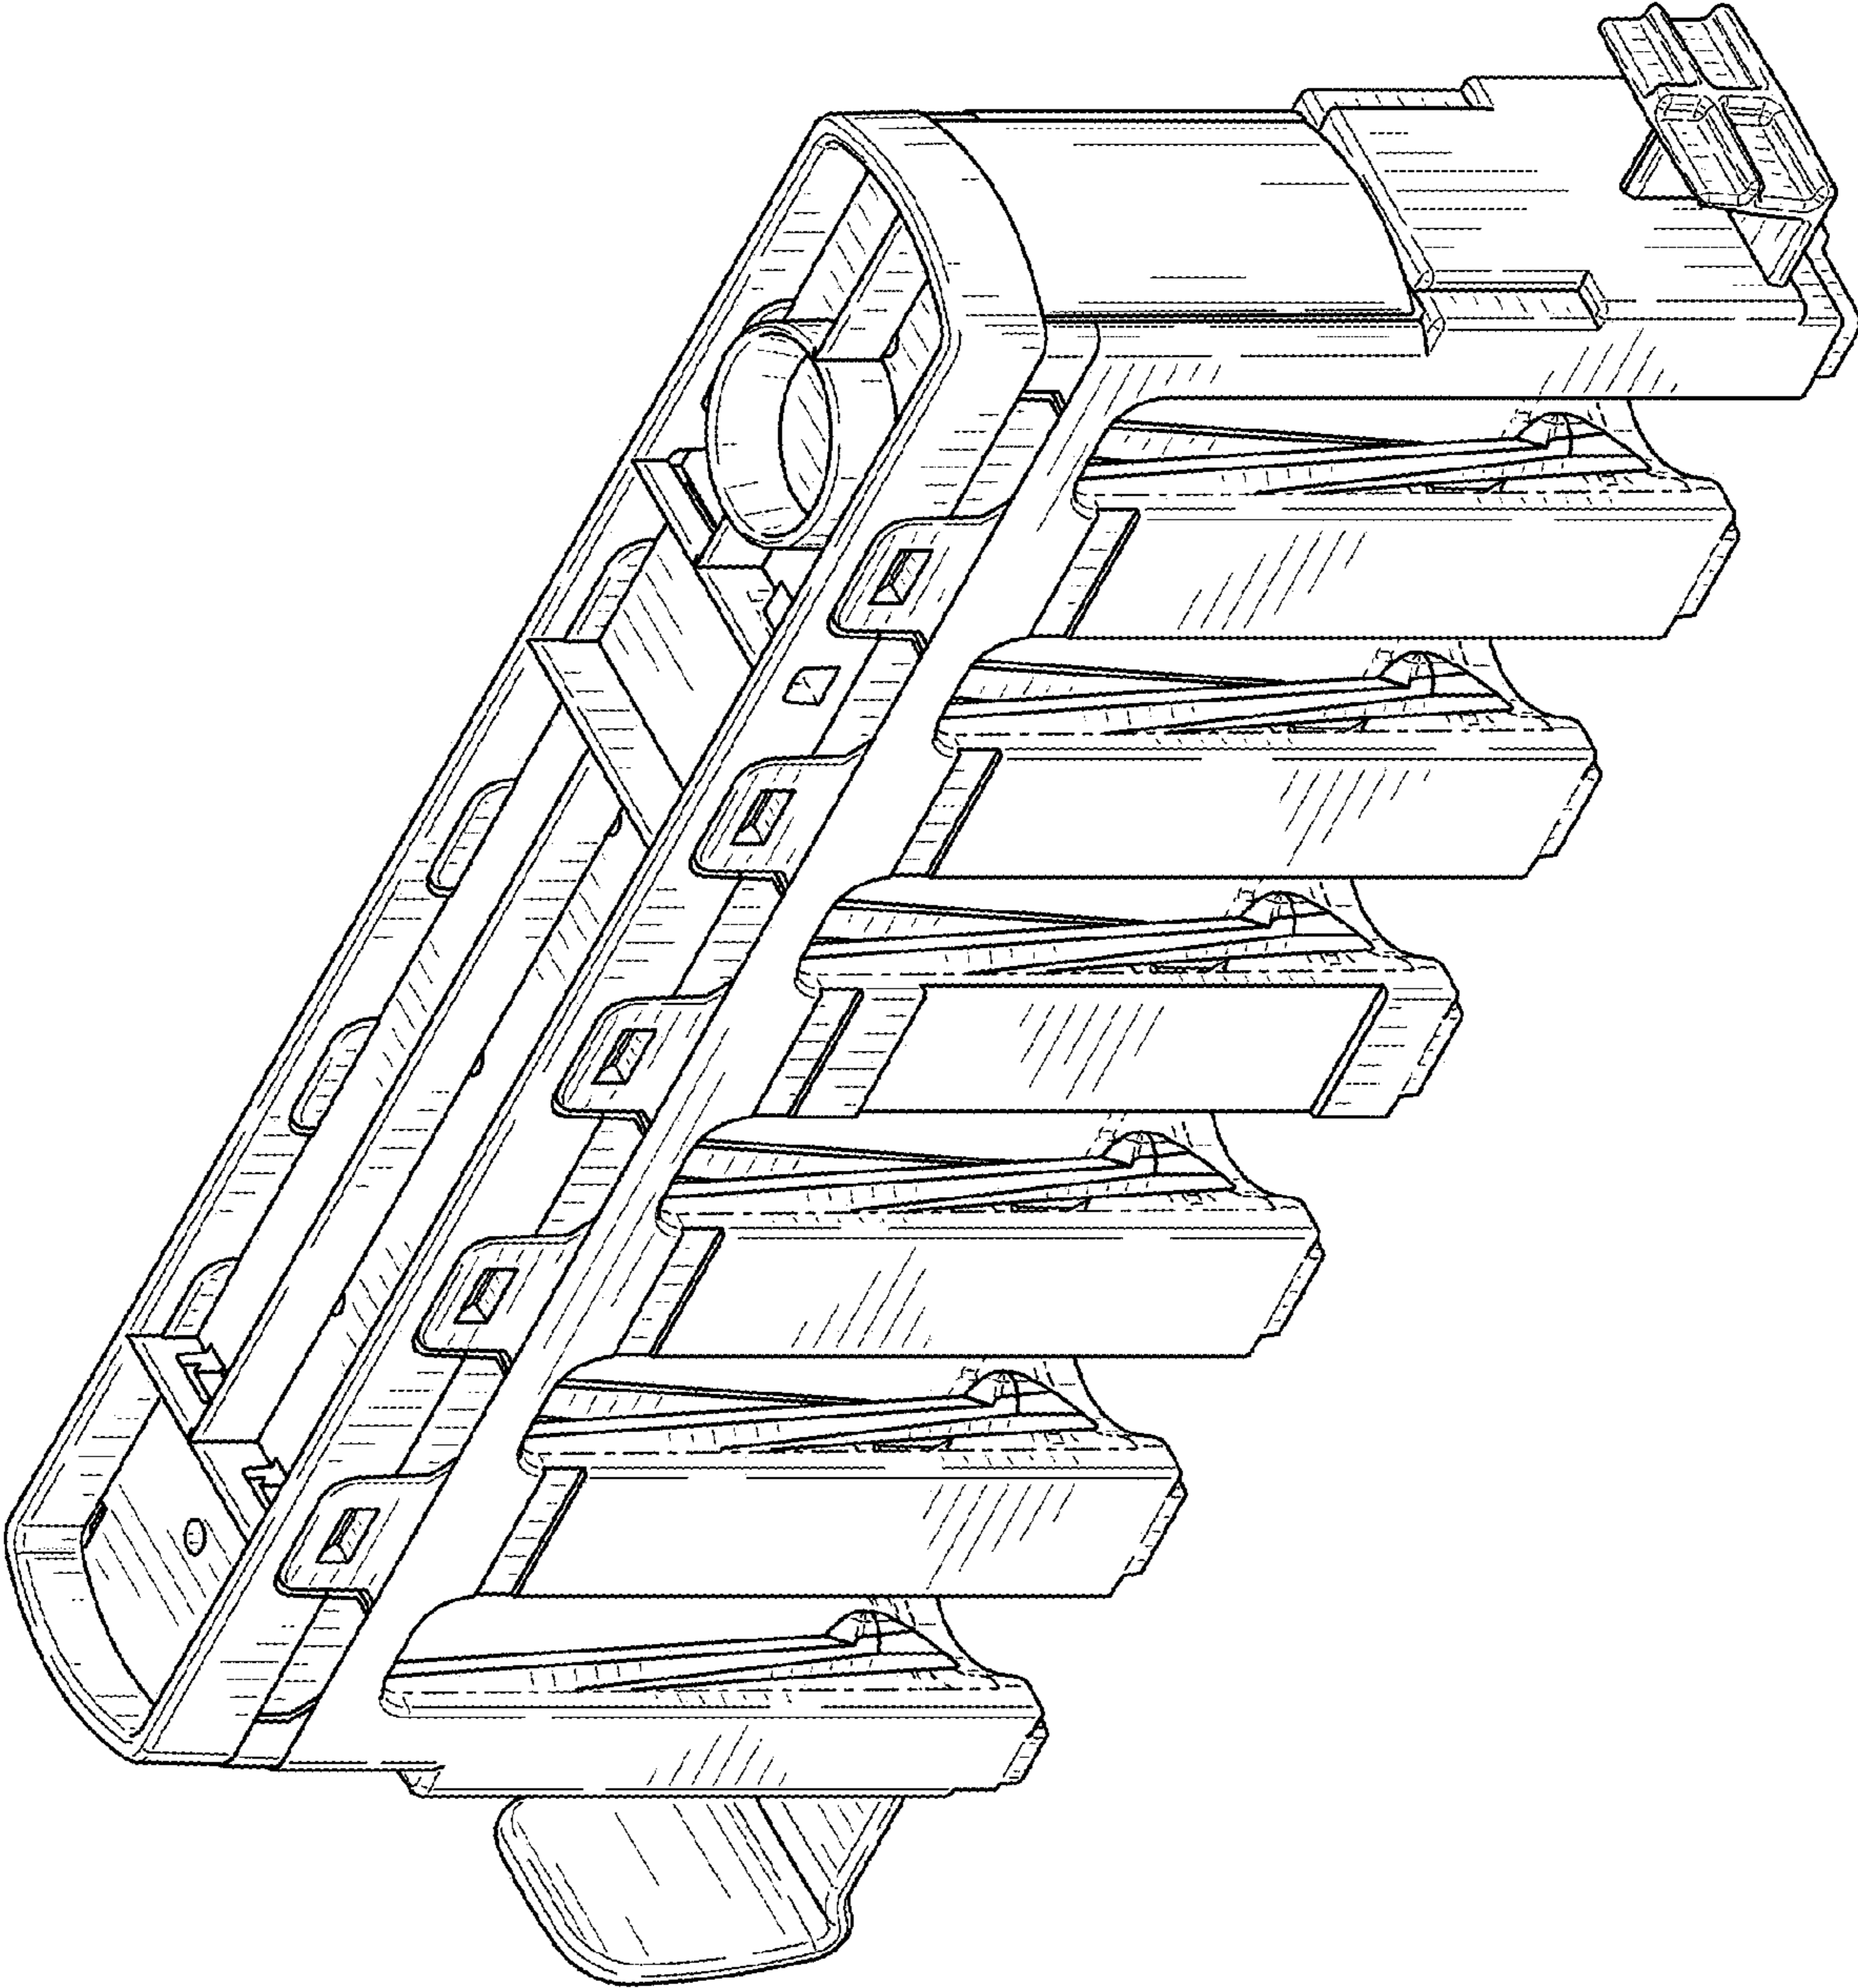


FIG. 4

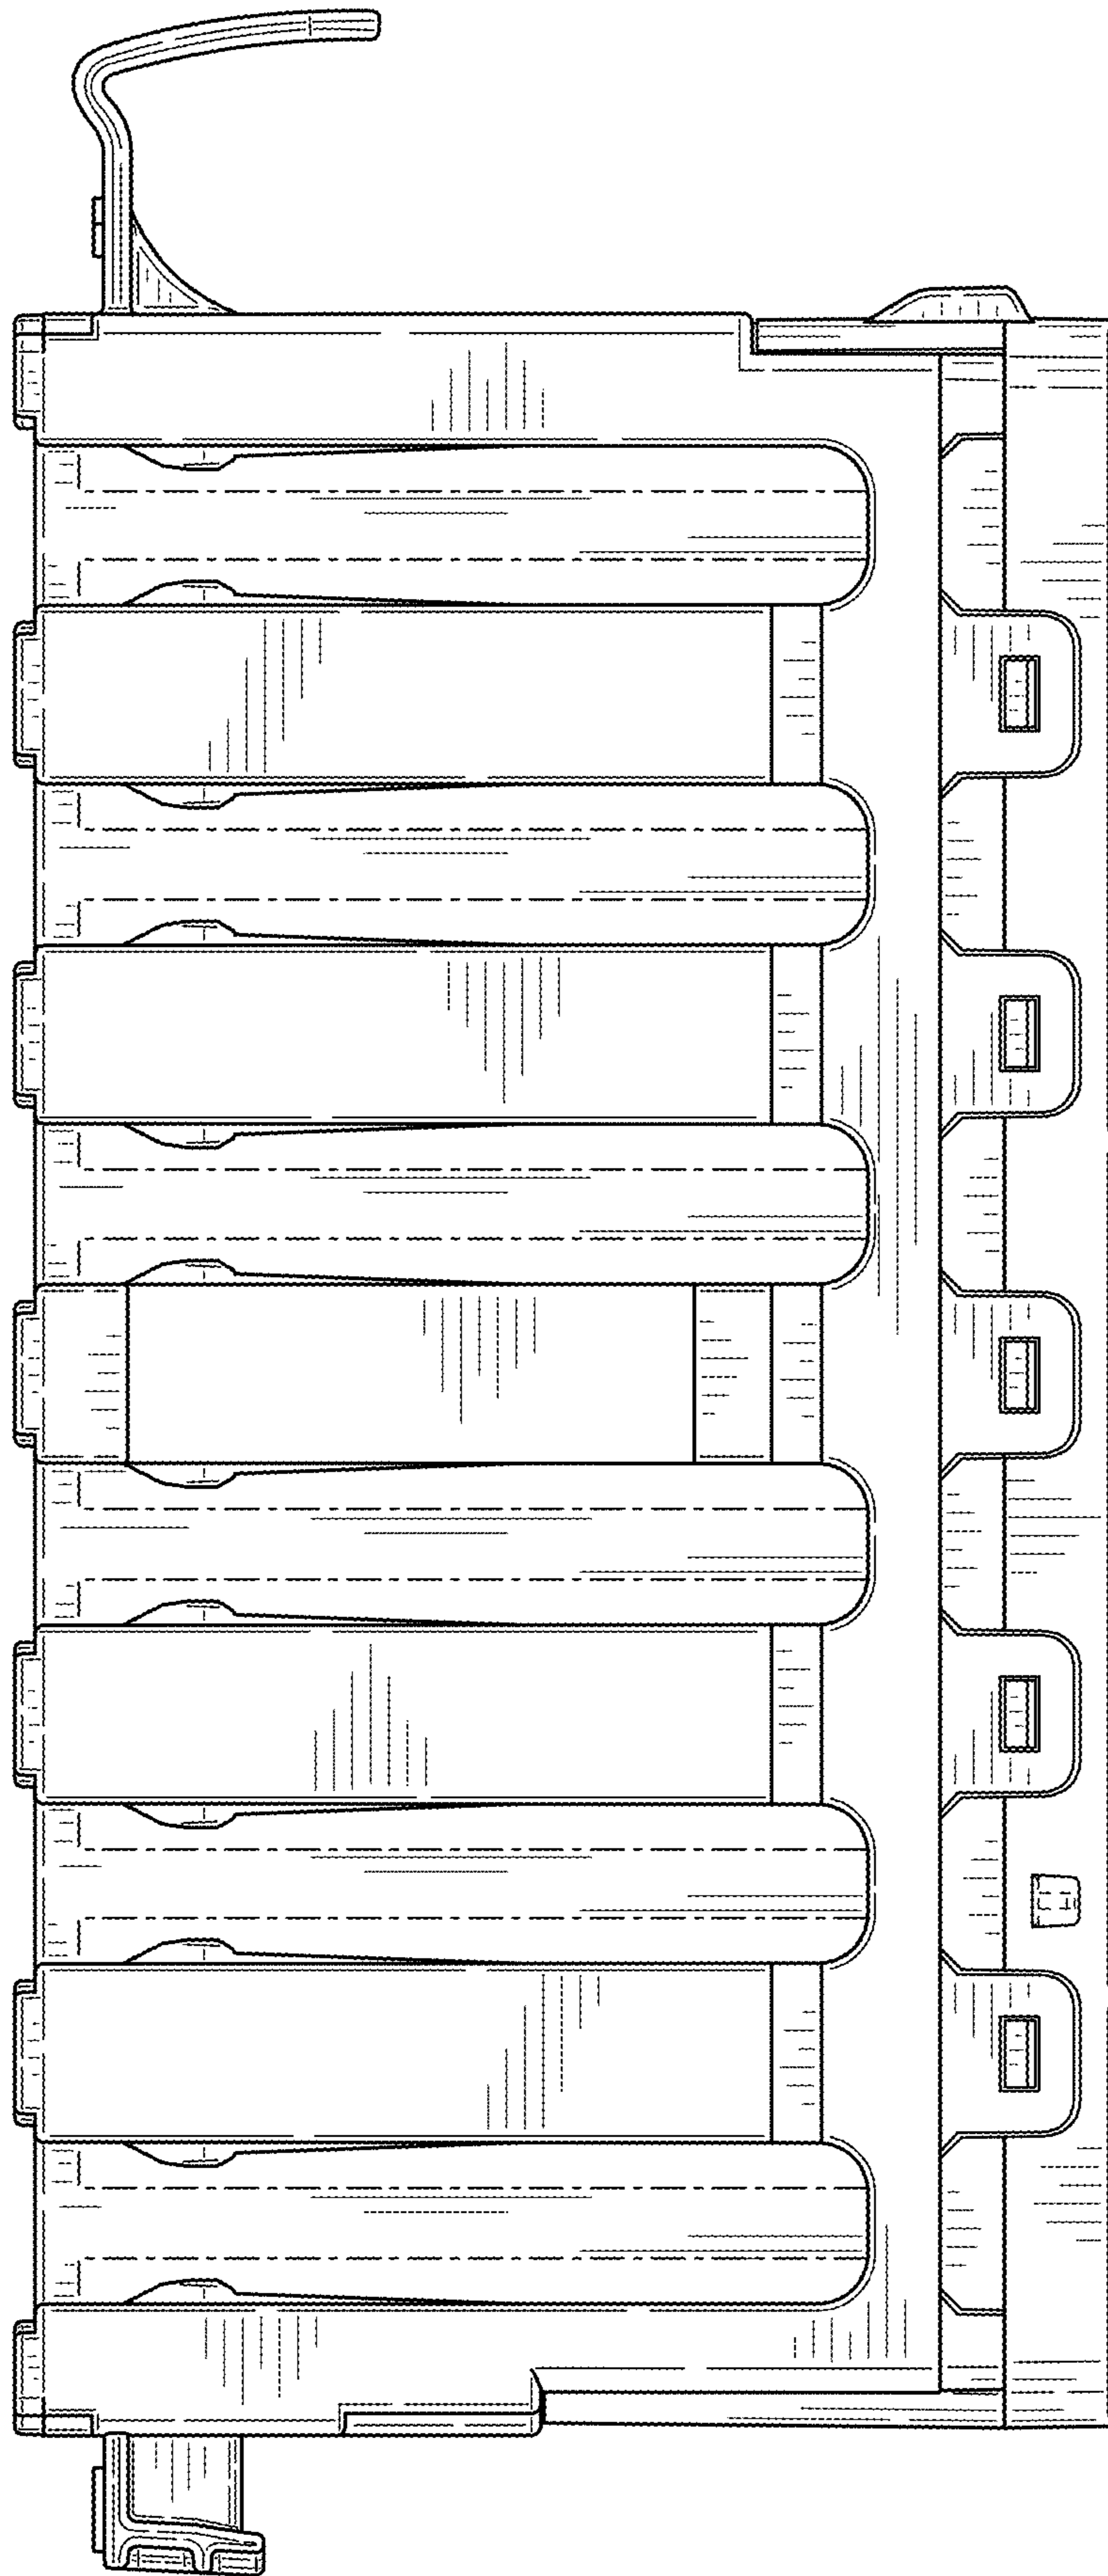


FIG. 5

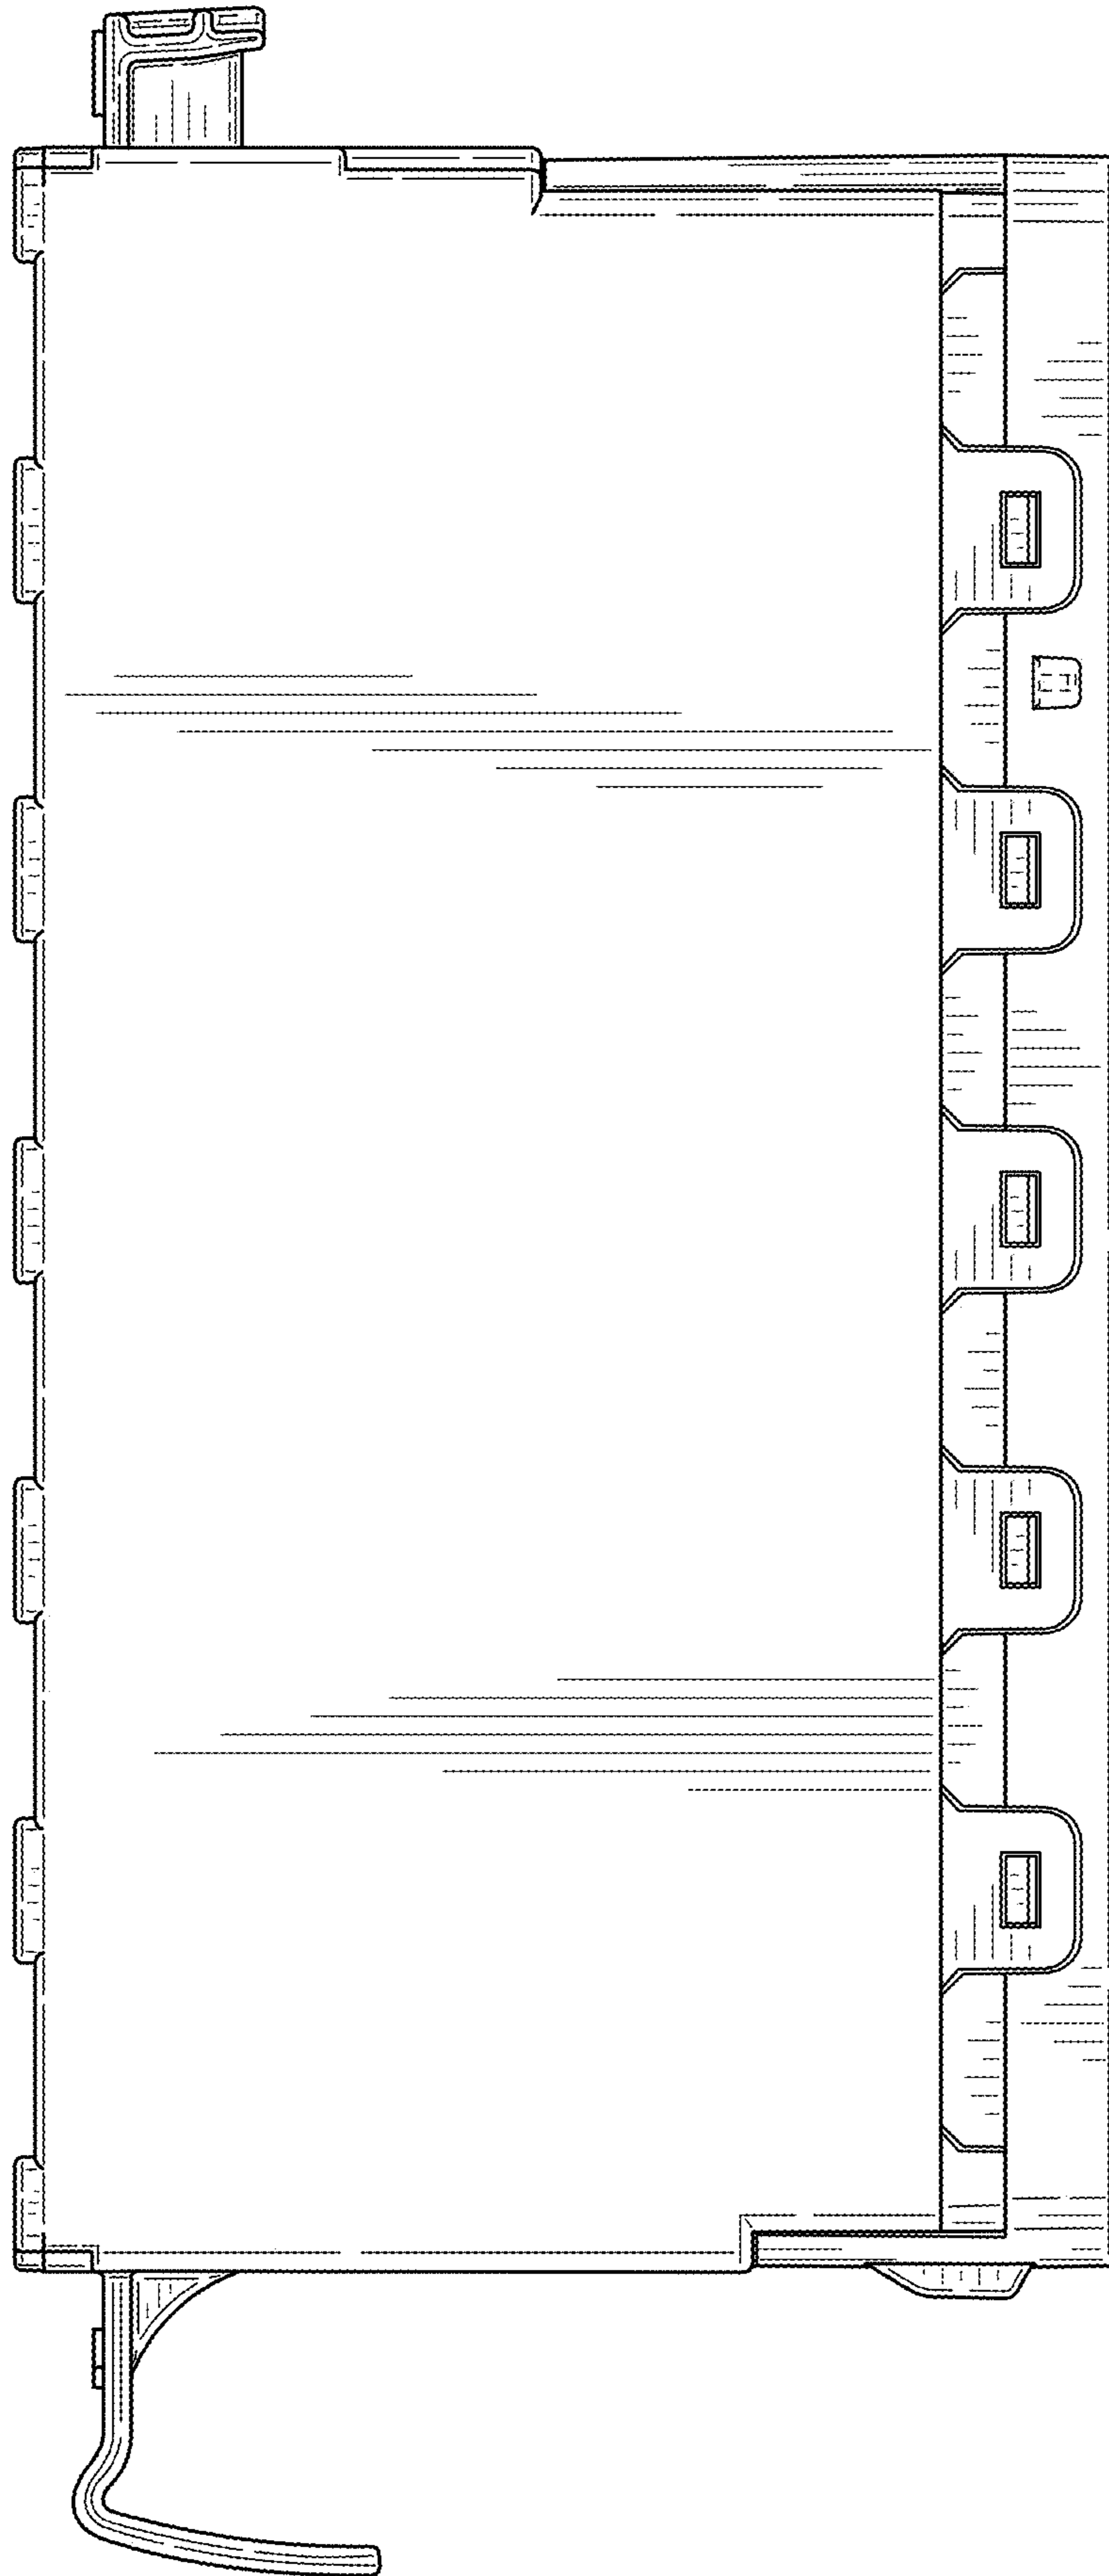


FIG. 6

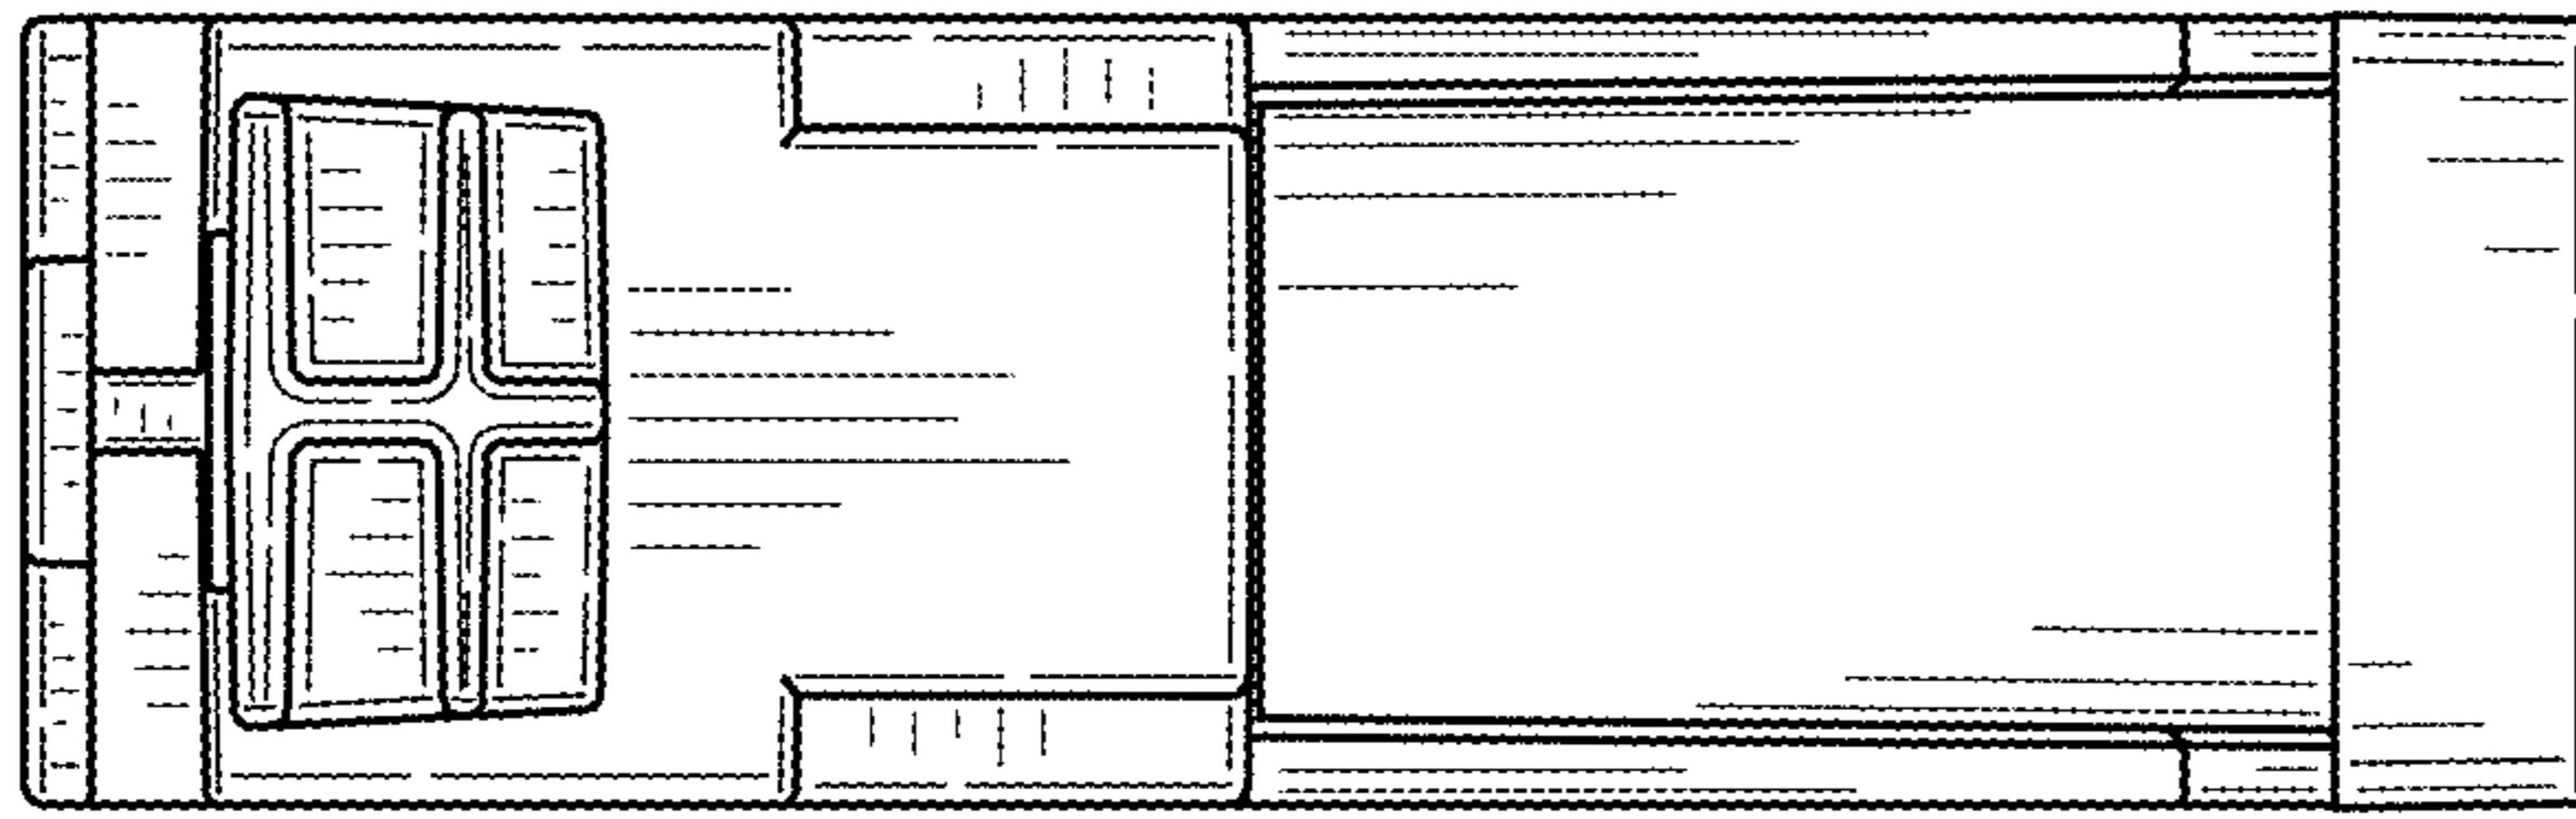


FIG. 8

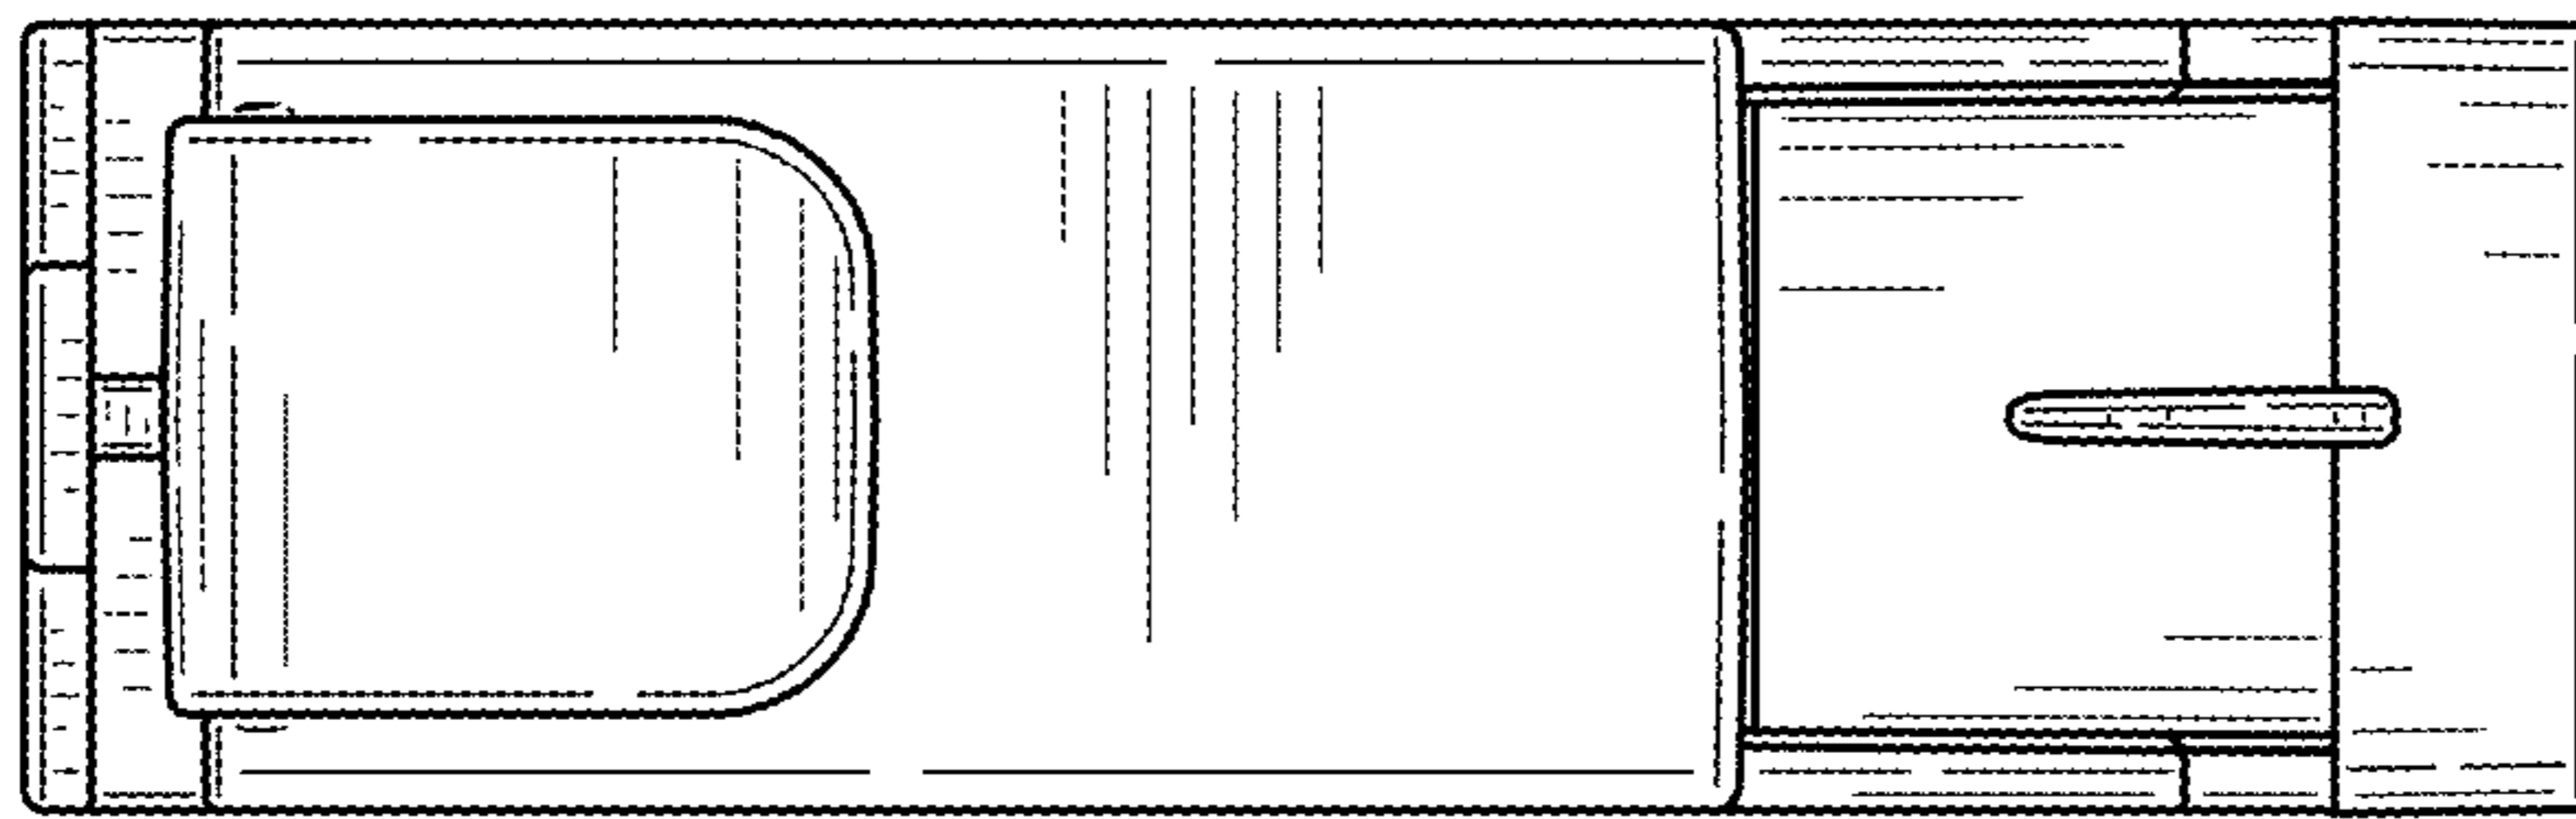


FIG. 7

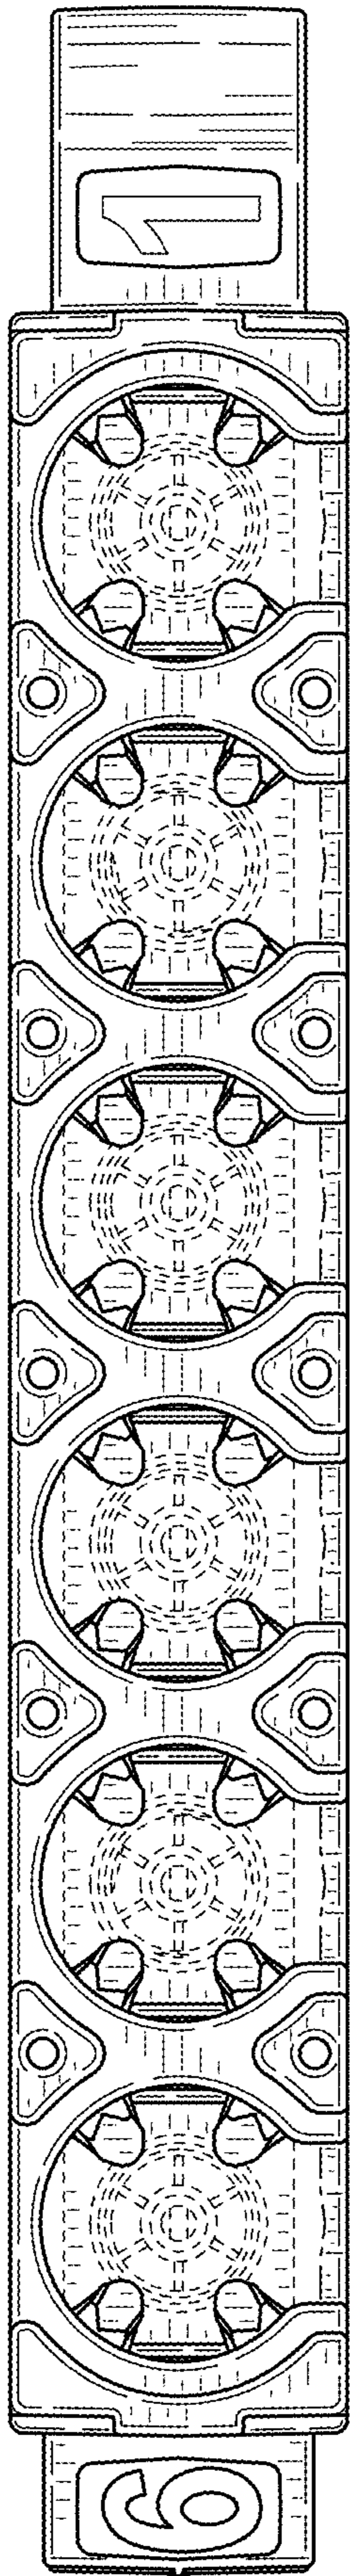


FIG. 9

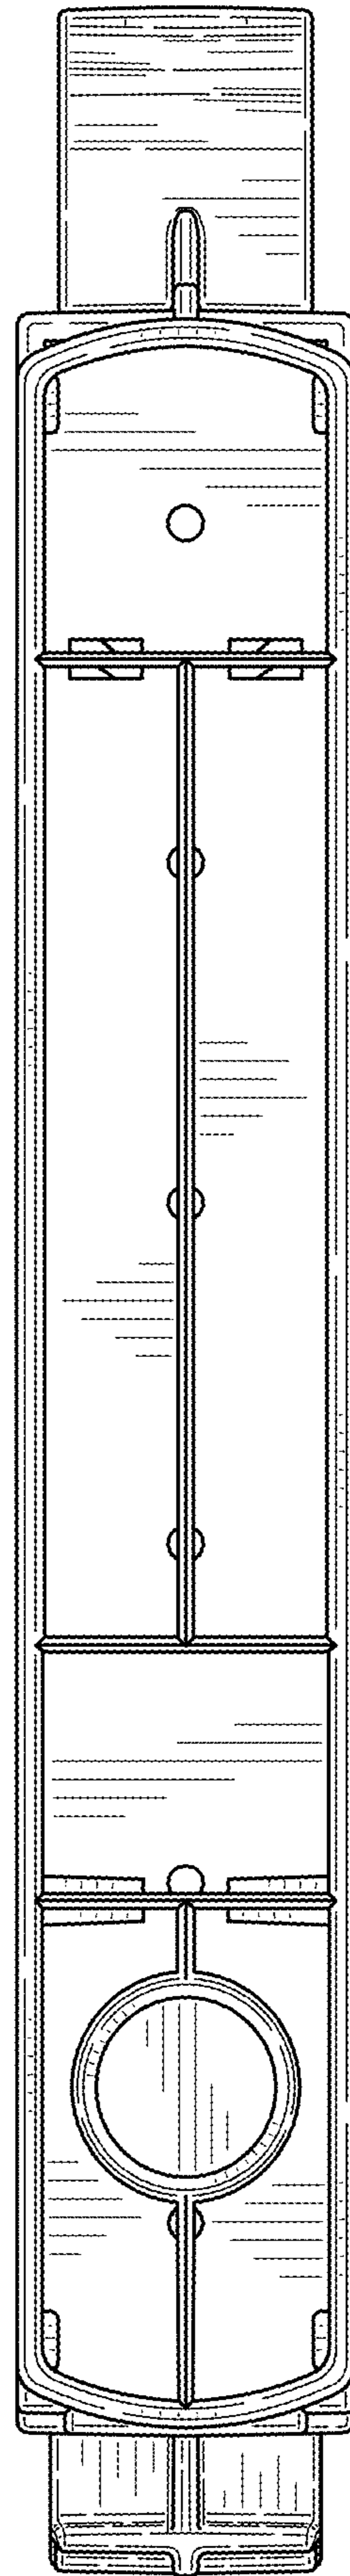


FIG. 10

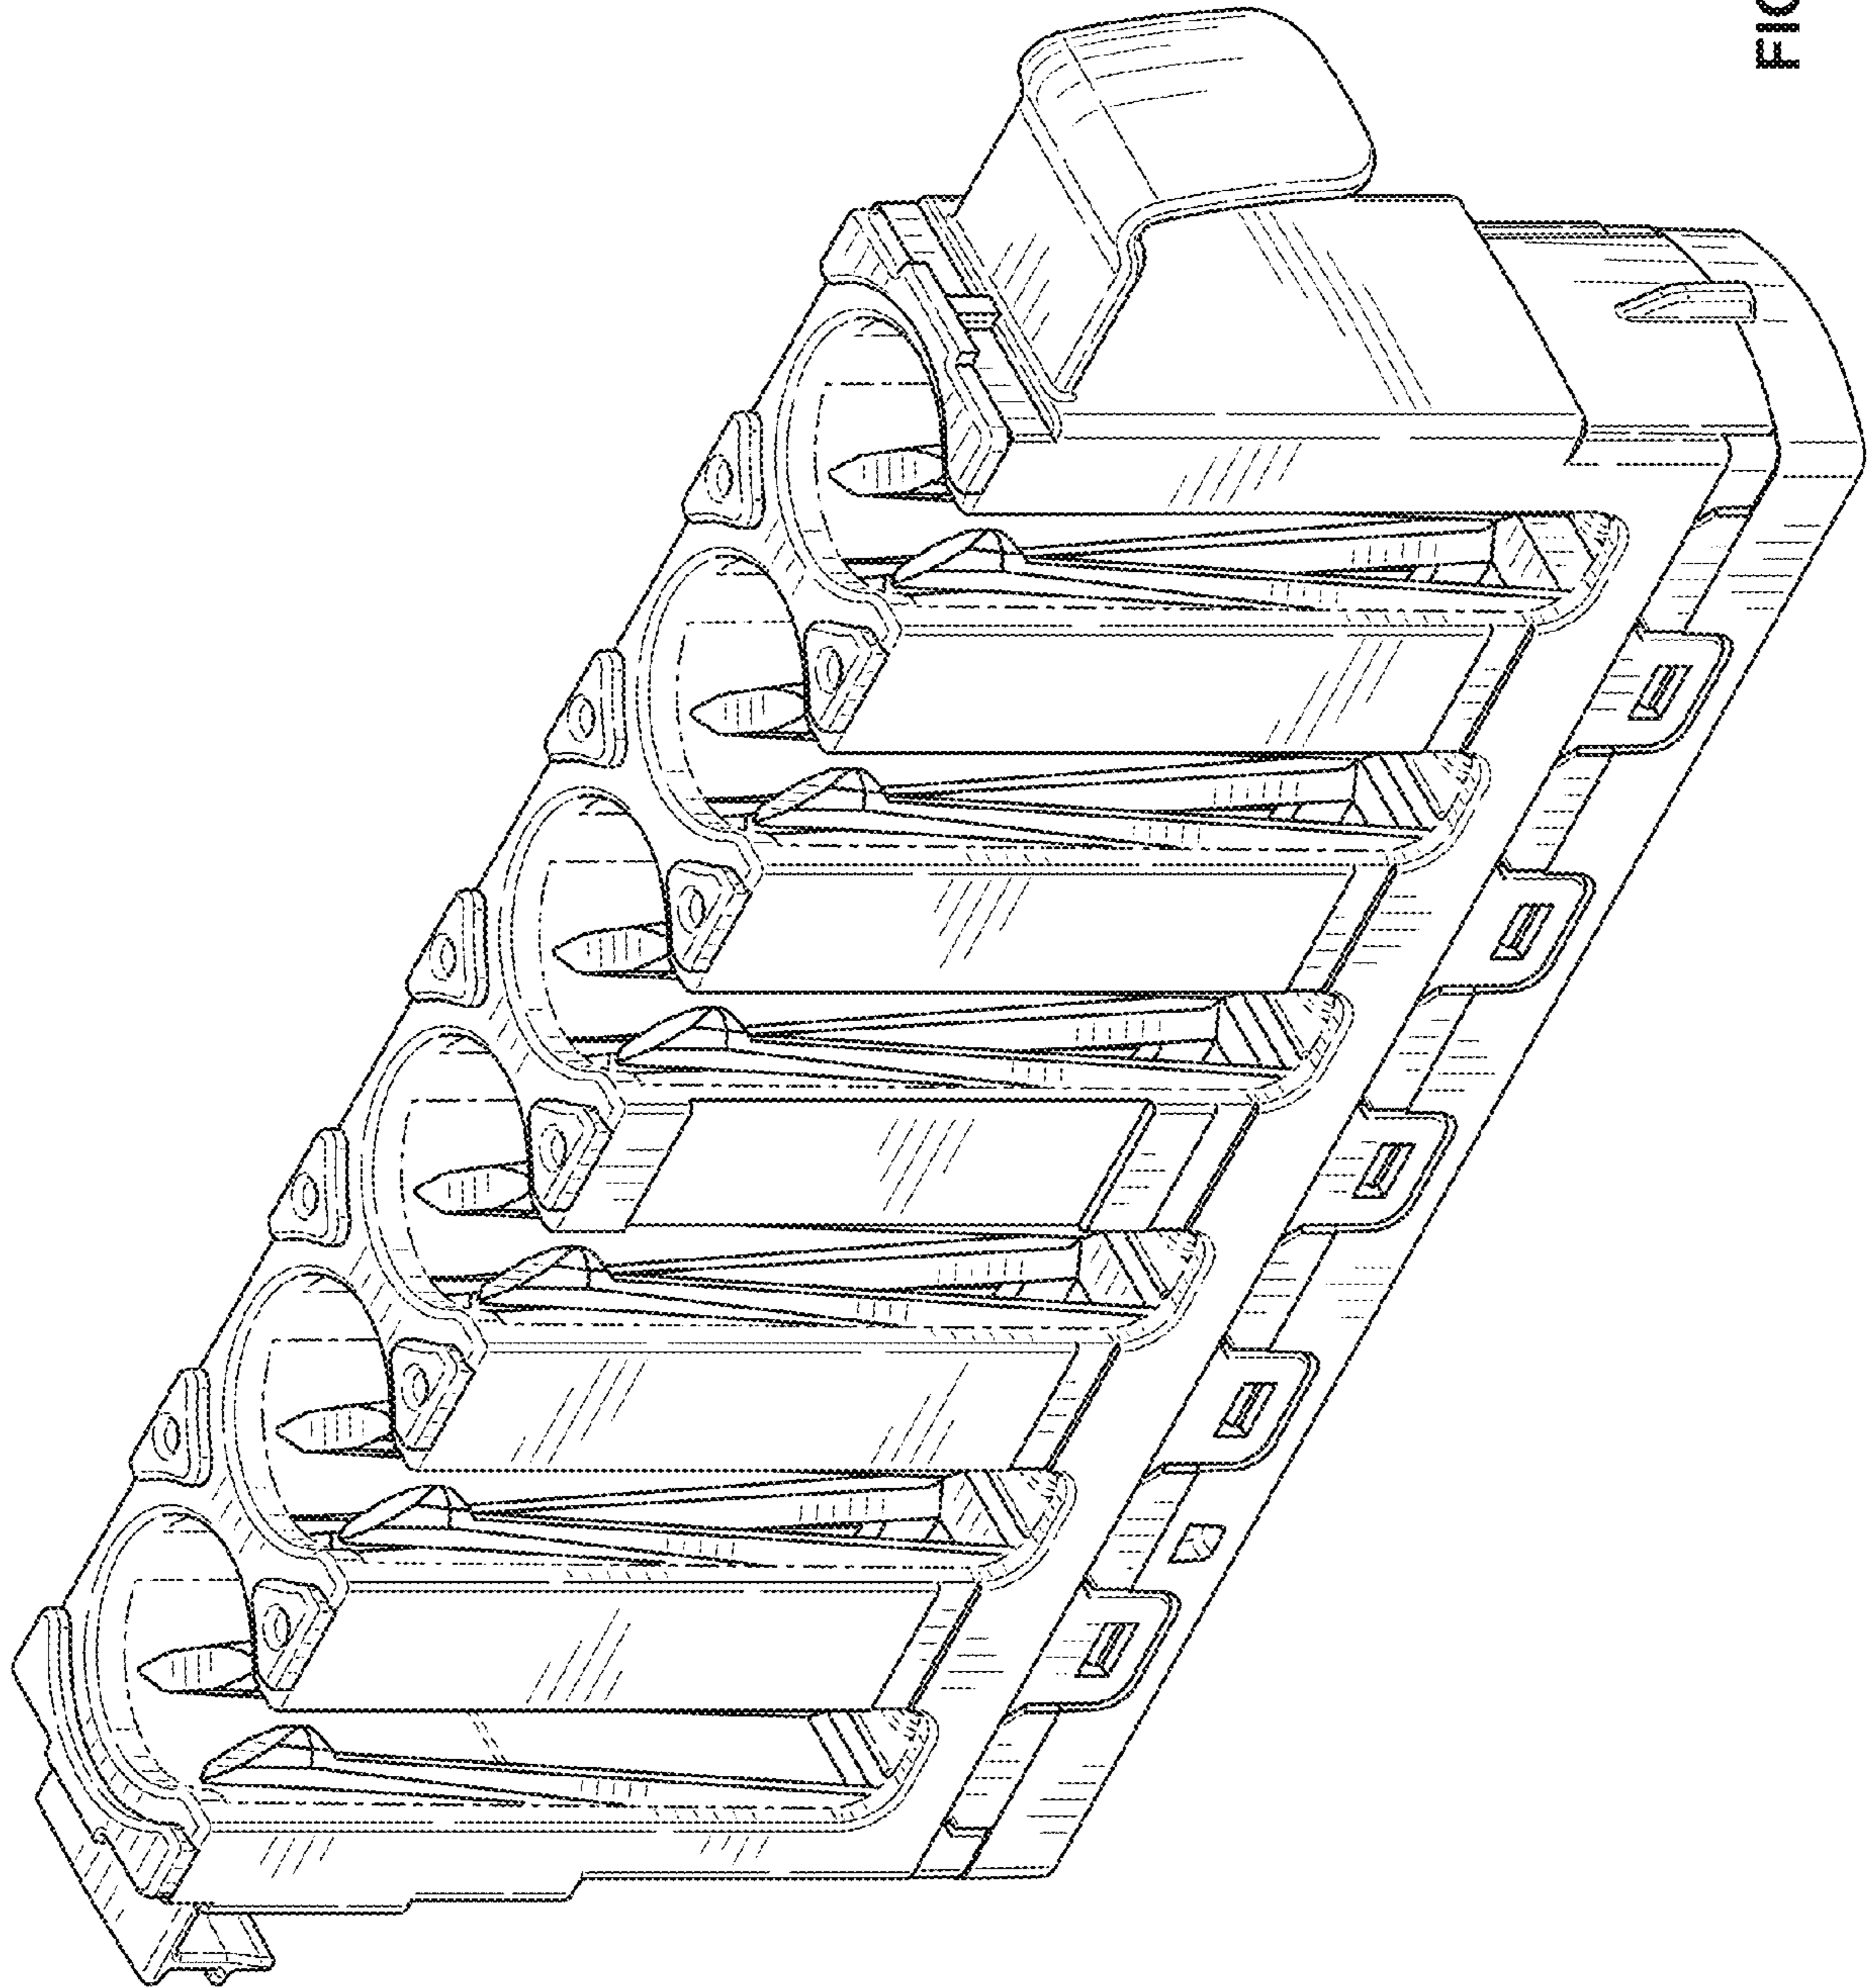


FIG. 11

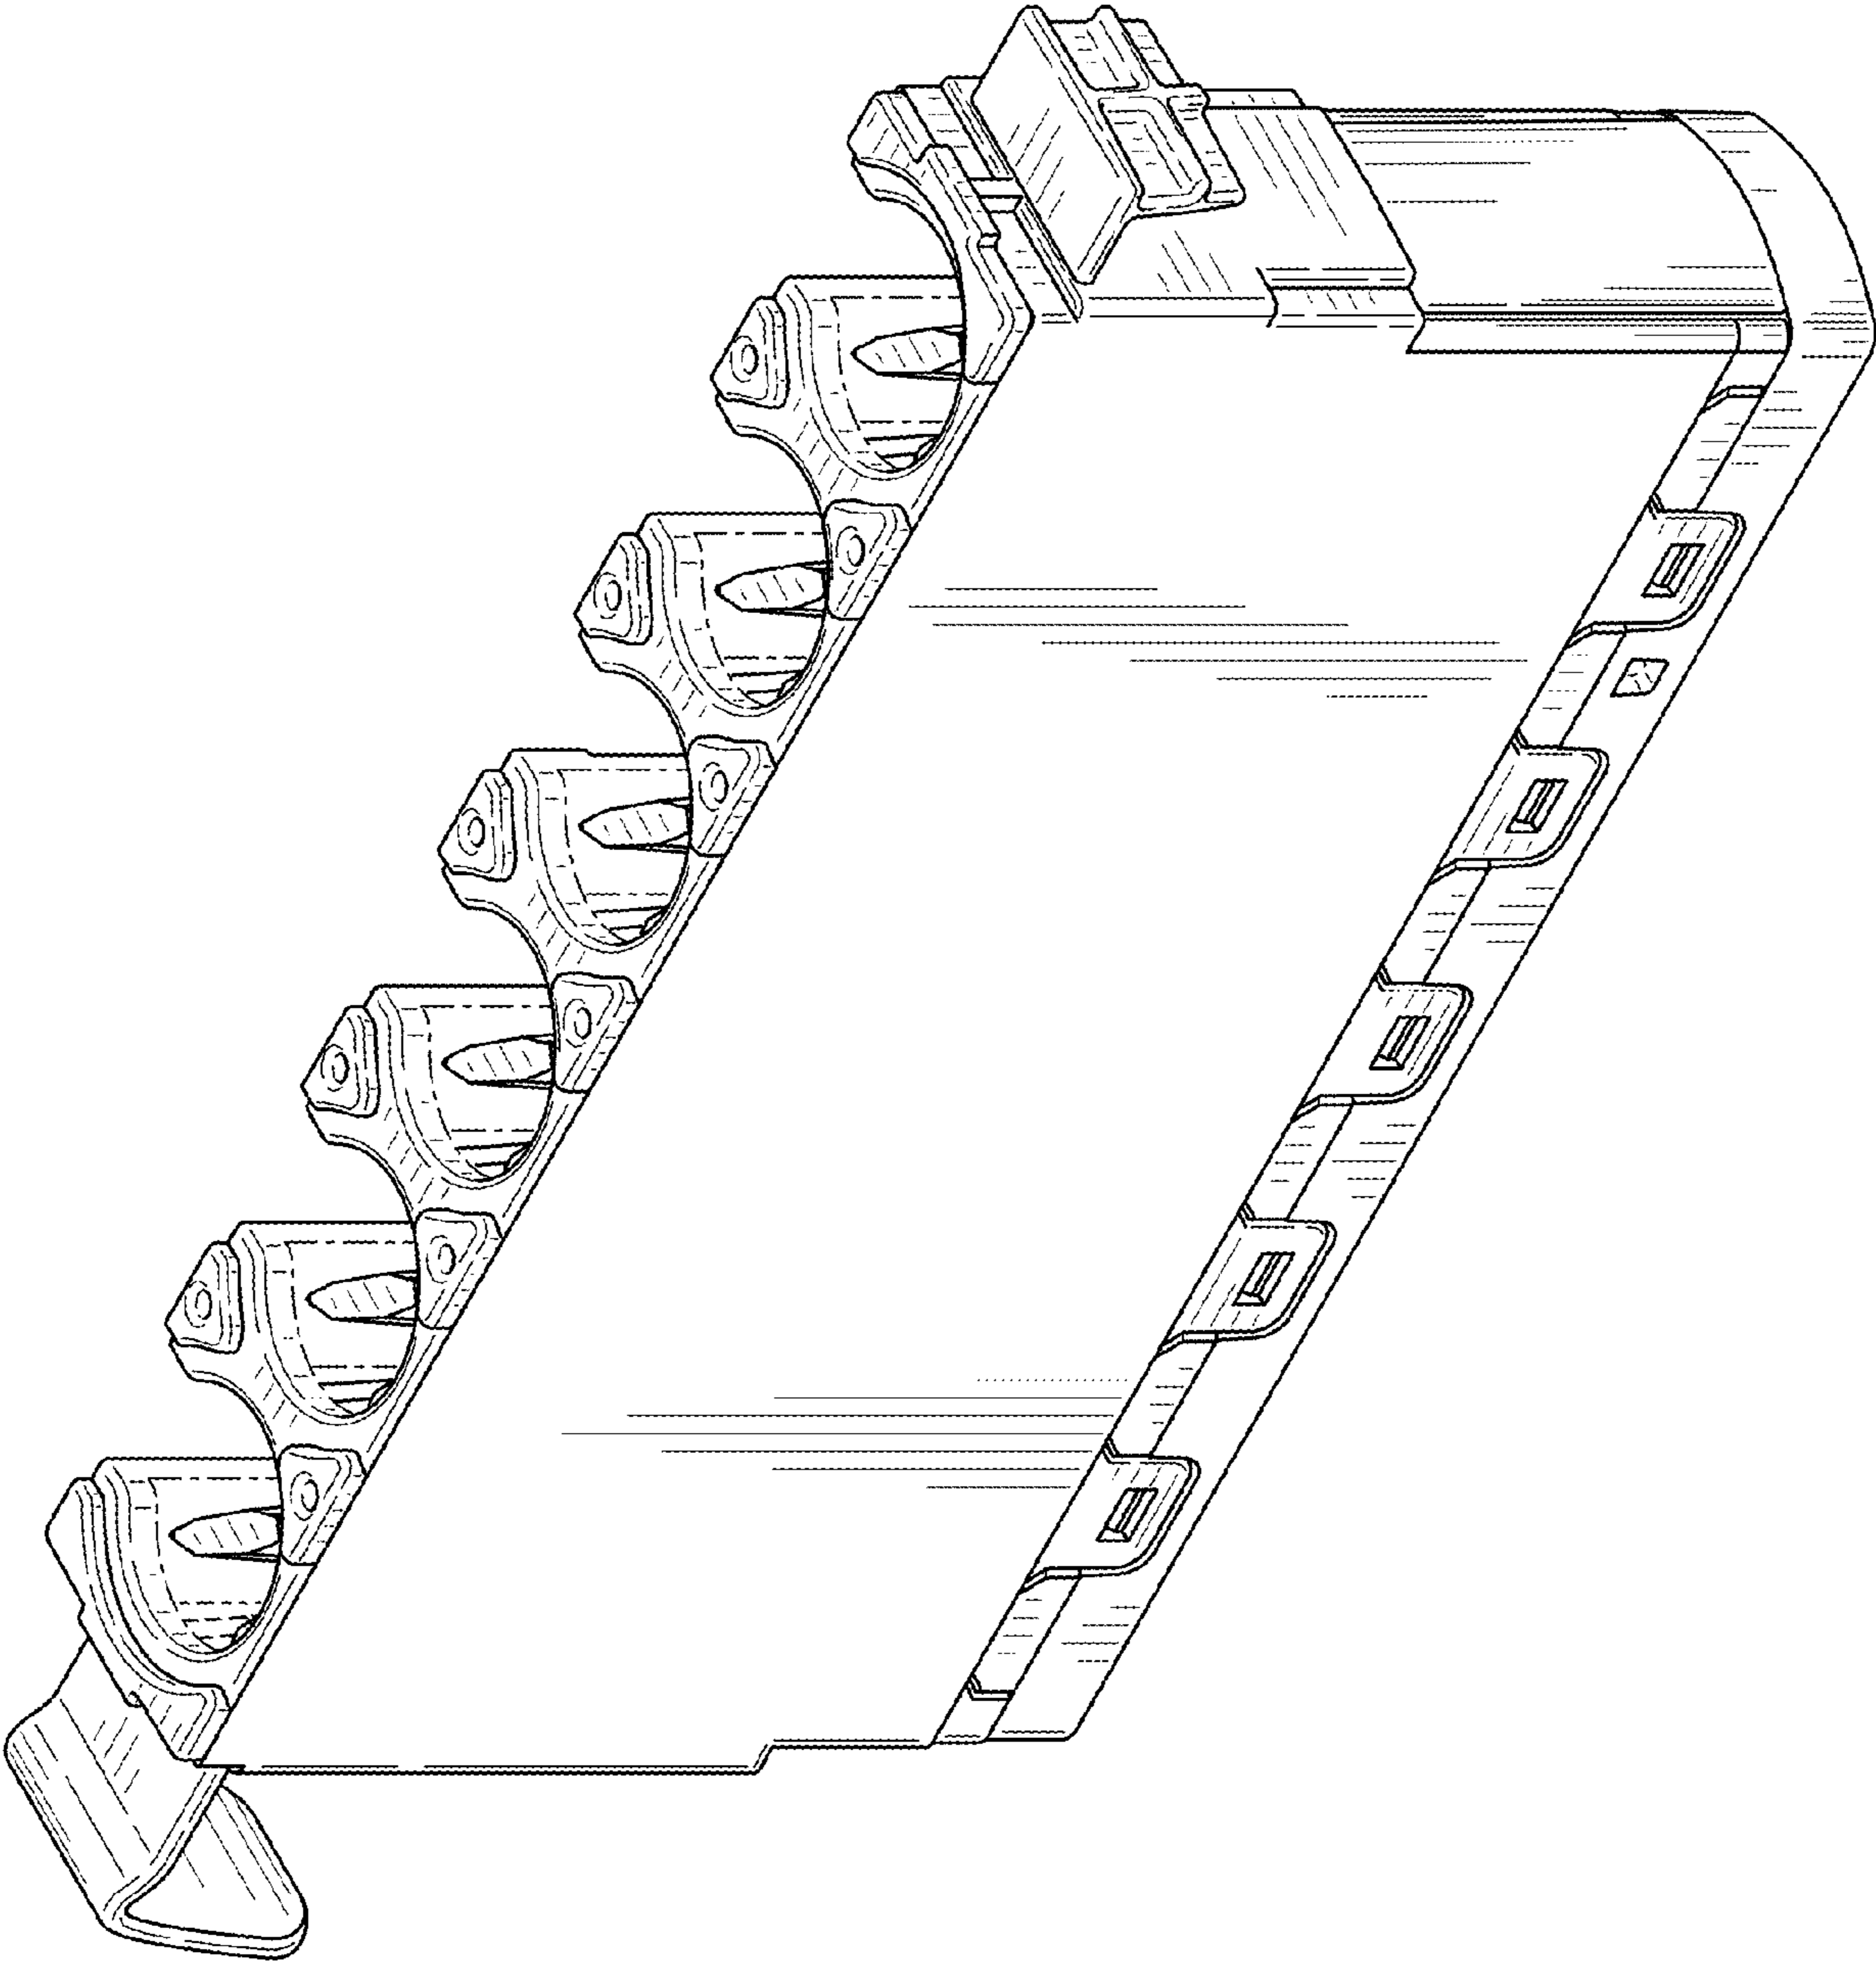


FIG. 12

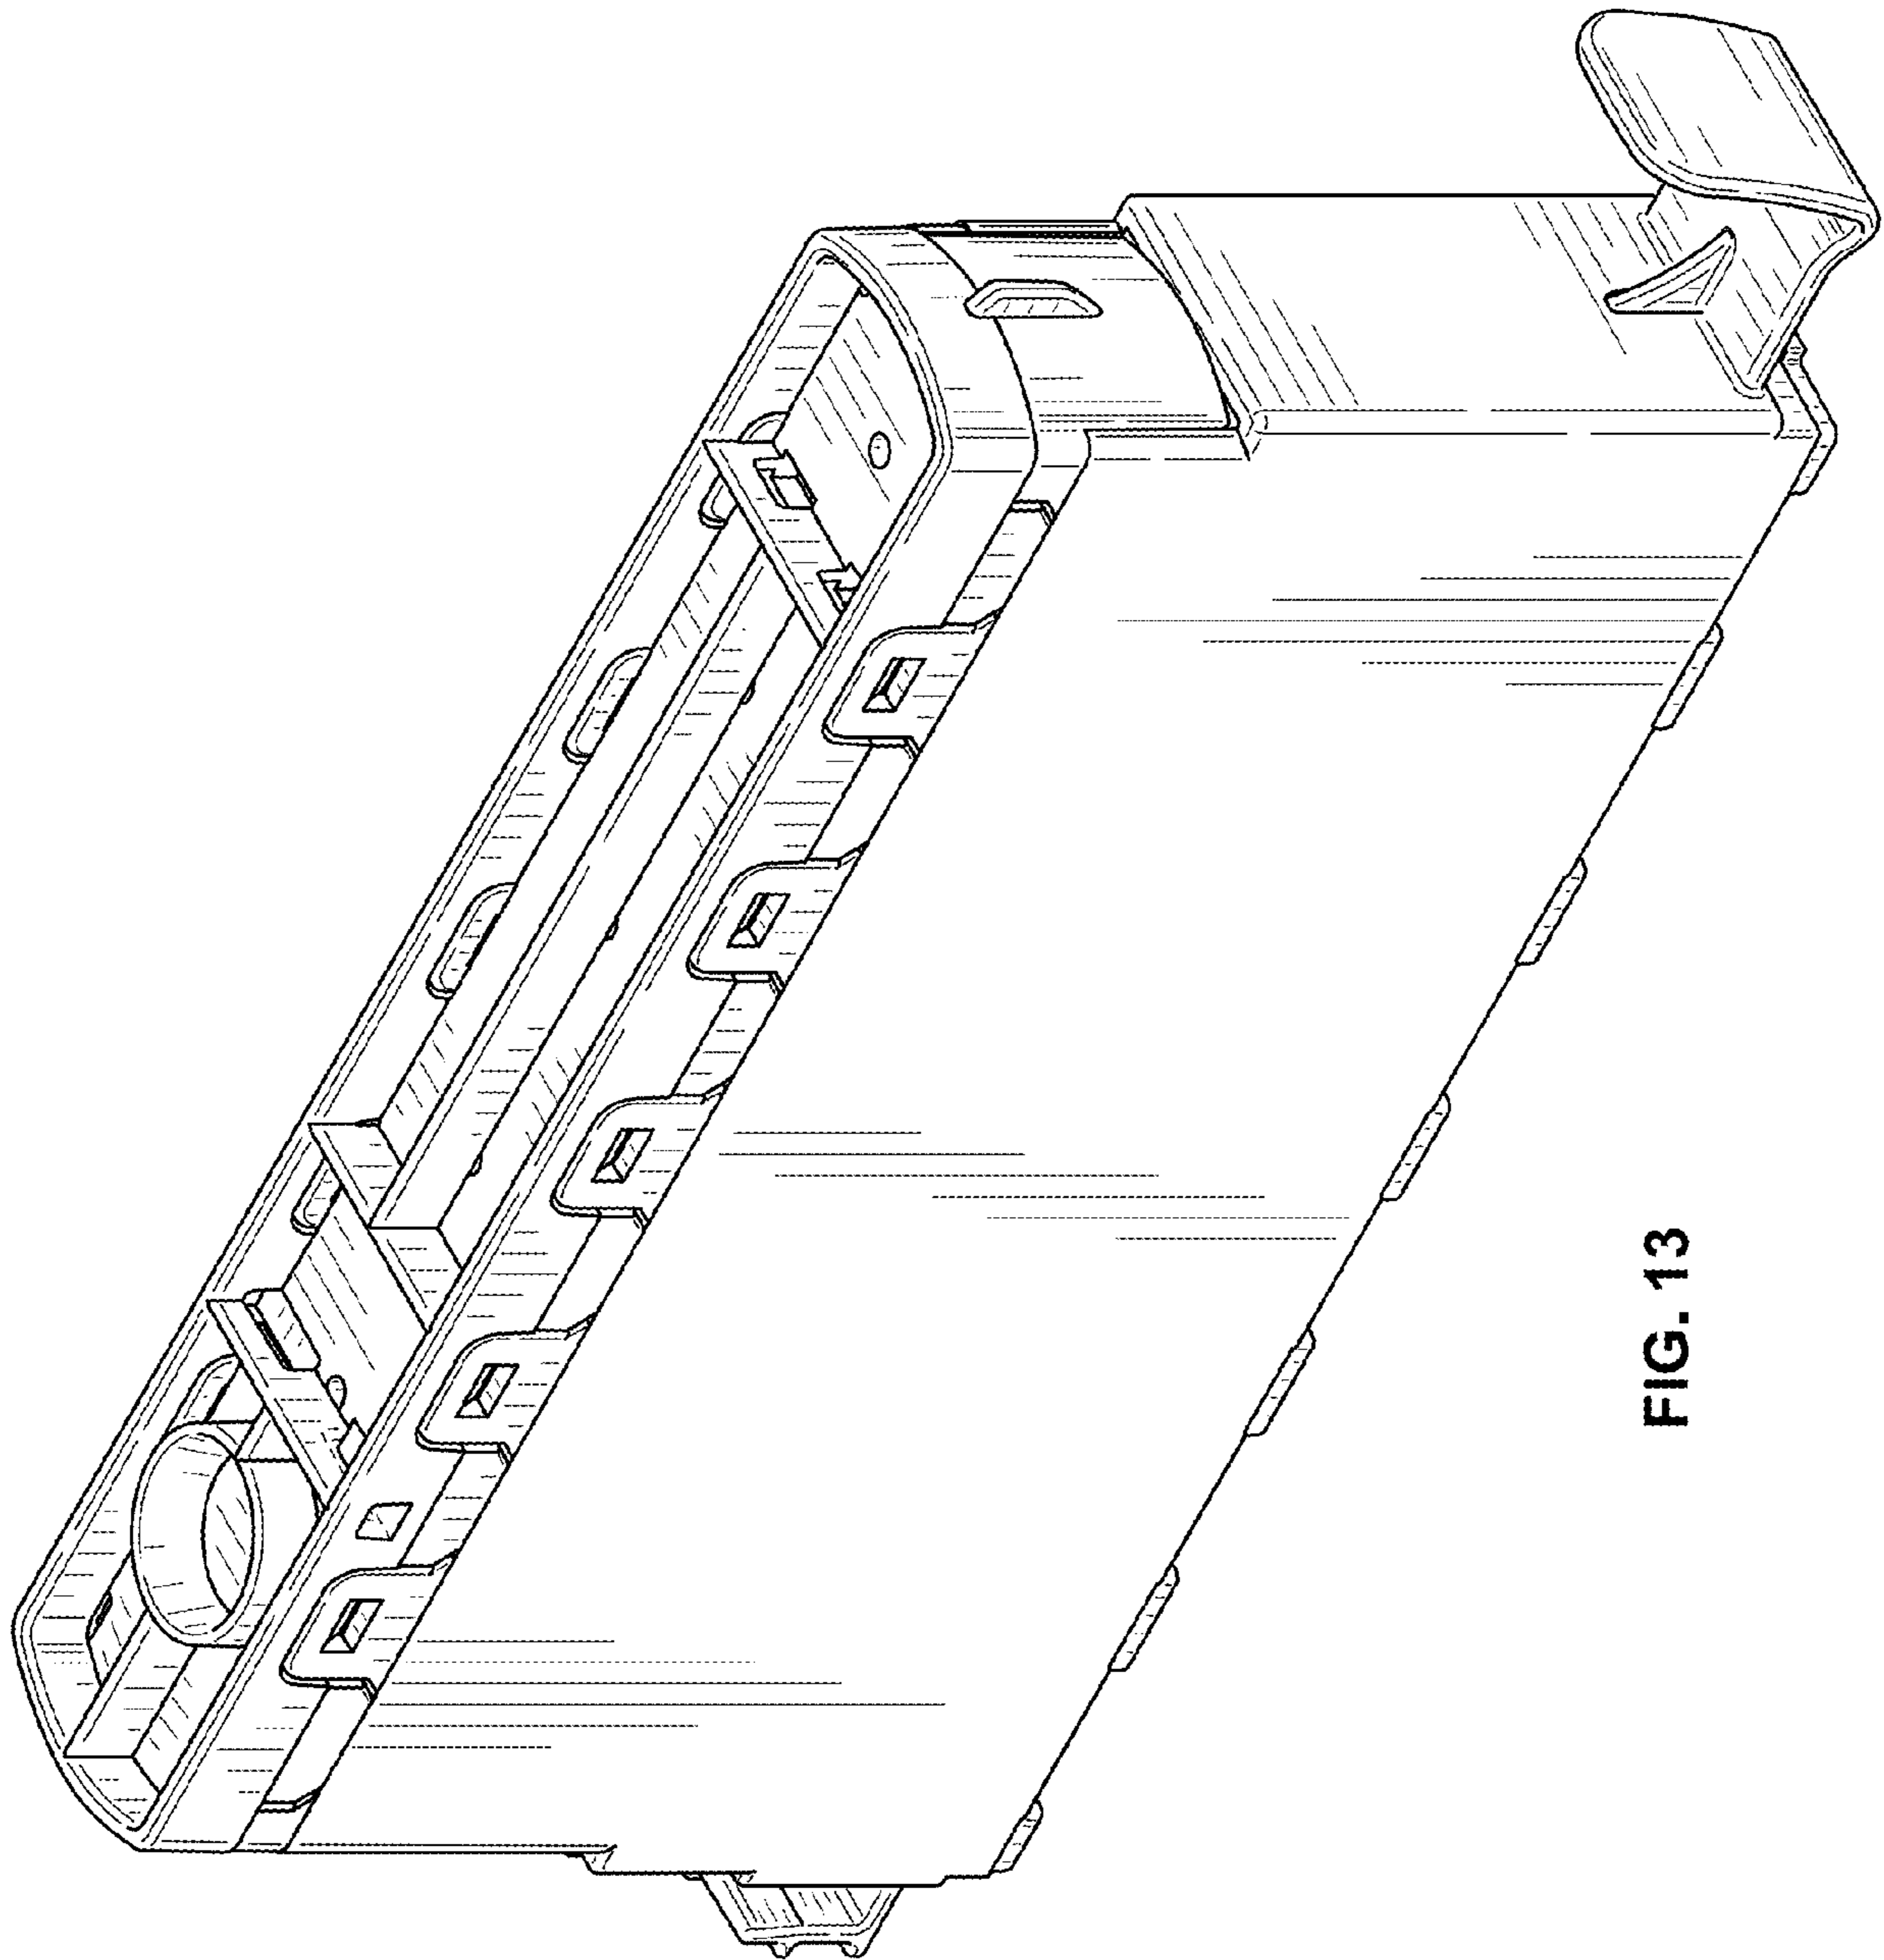


FIG. 13

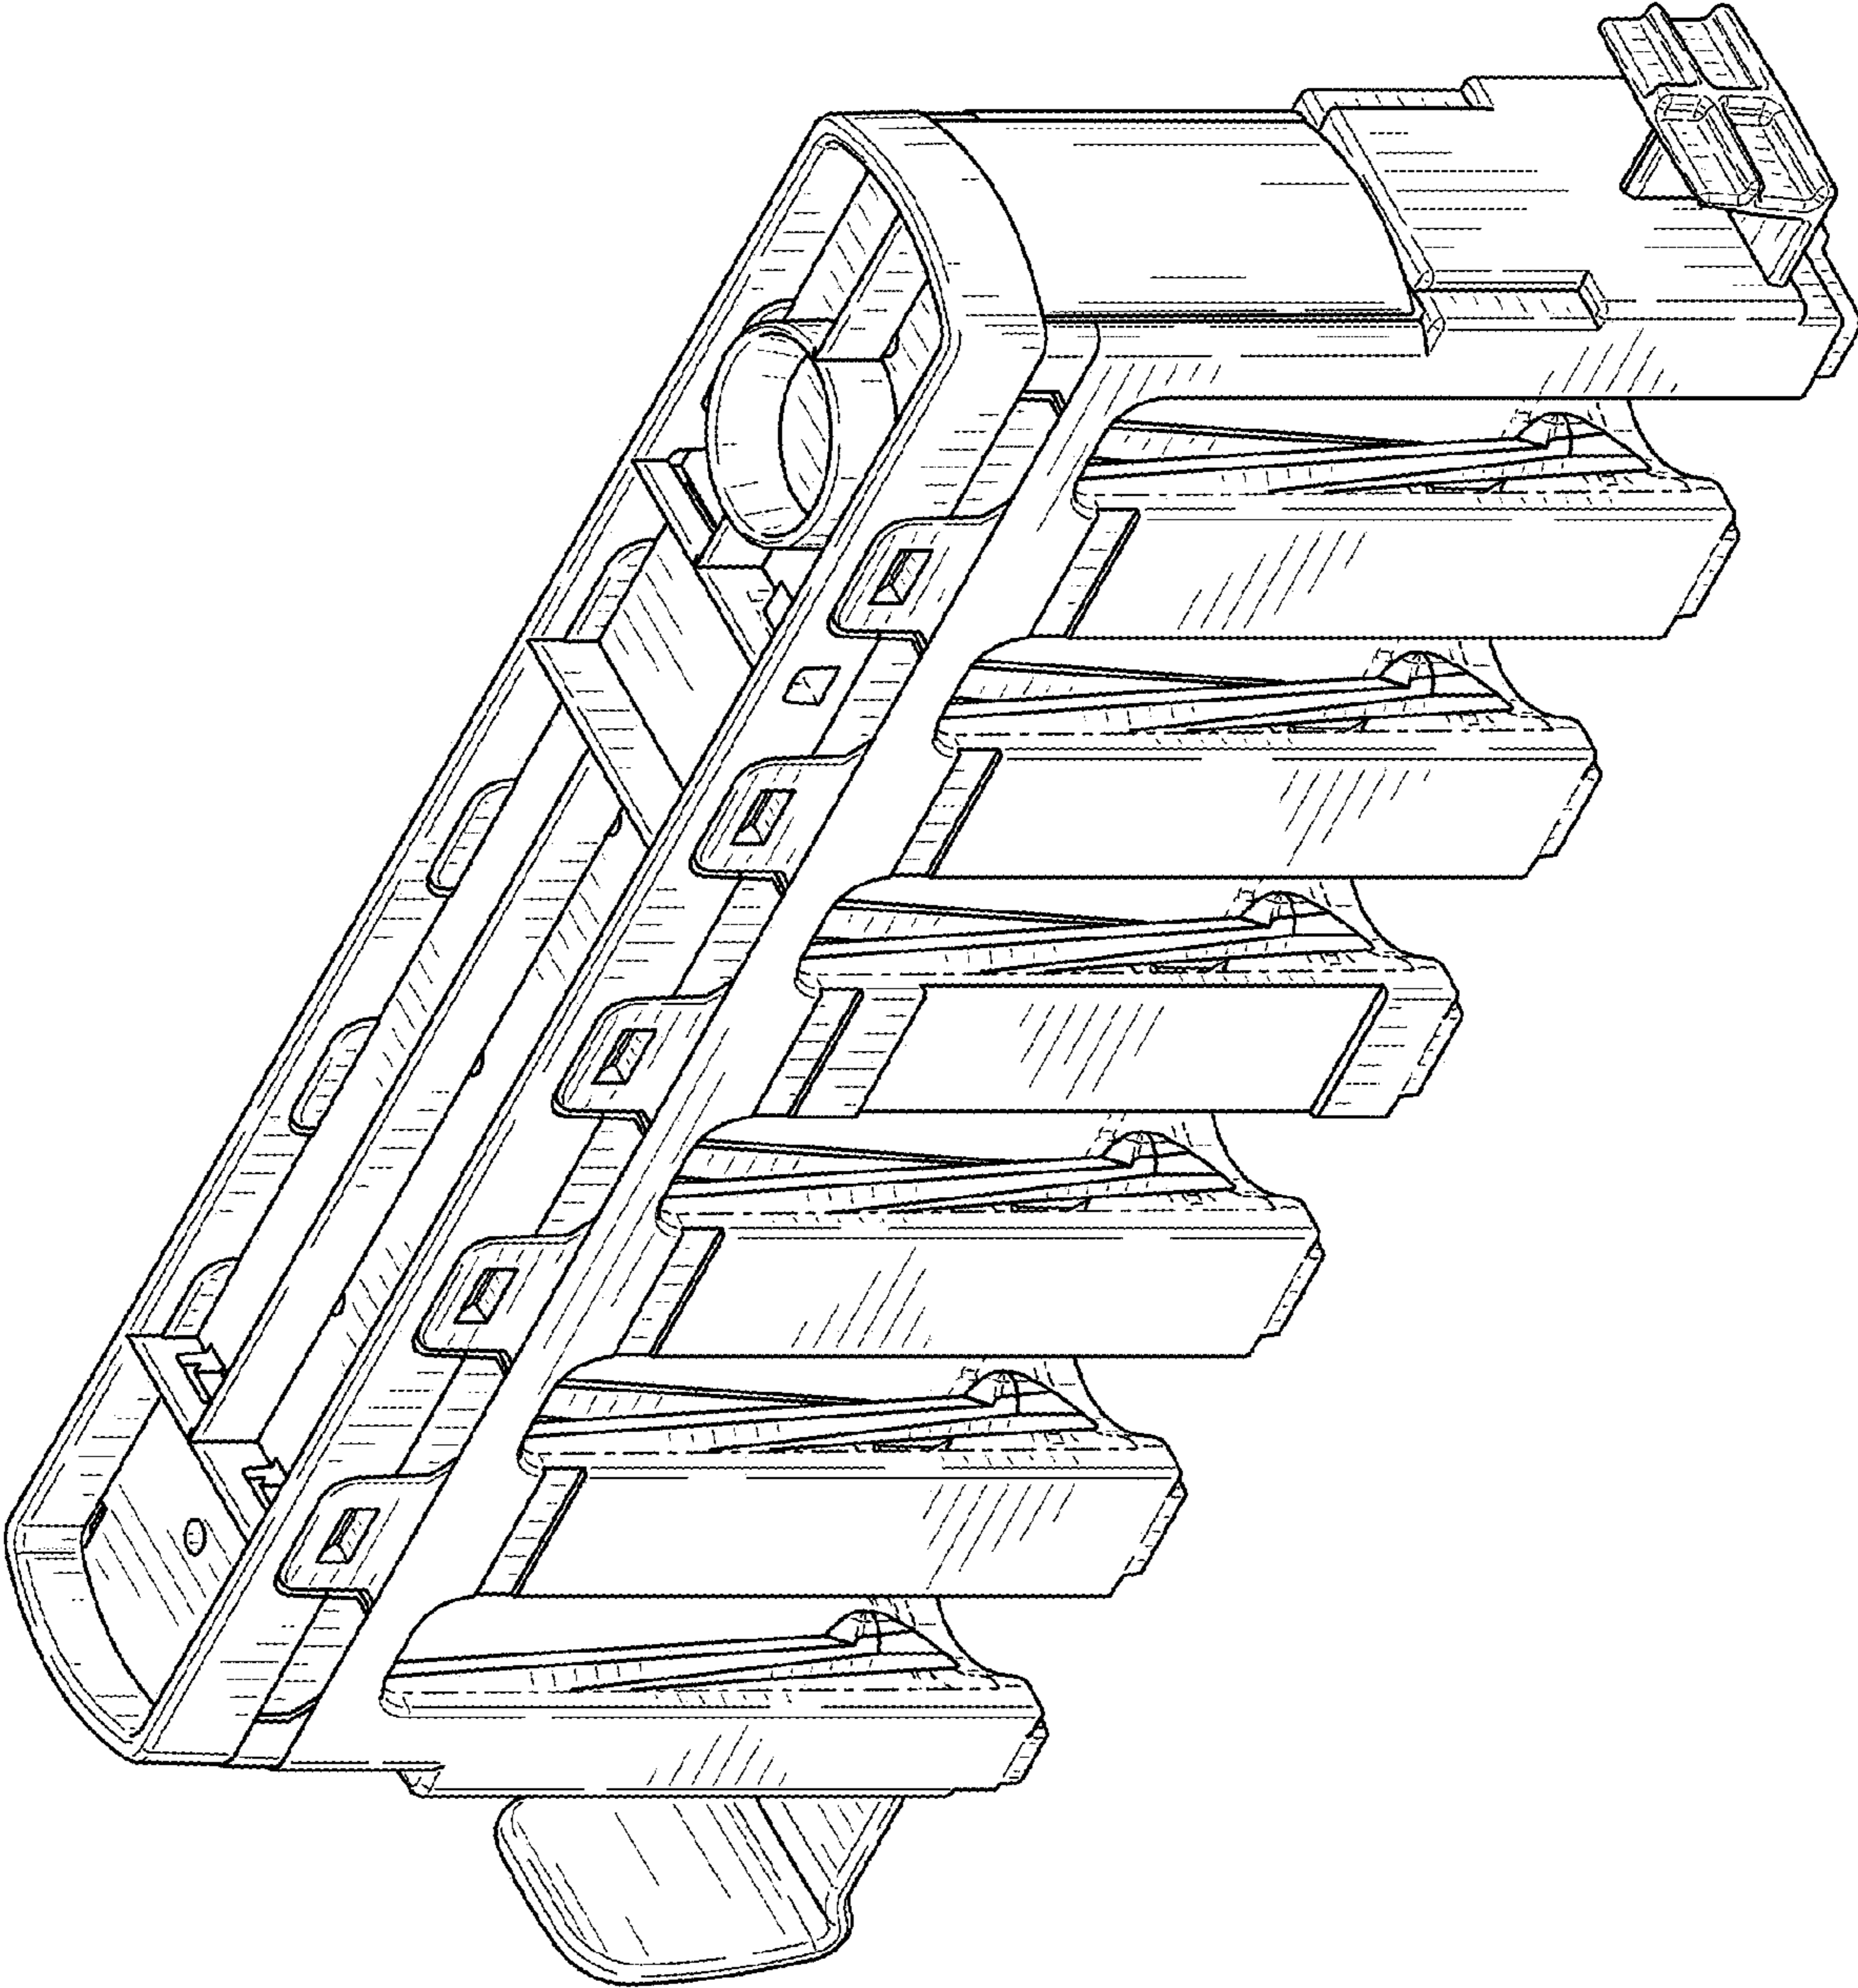


FIG. 14

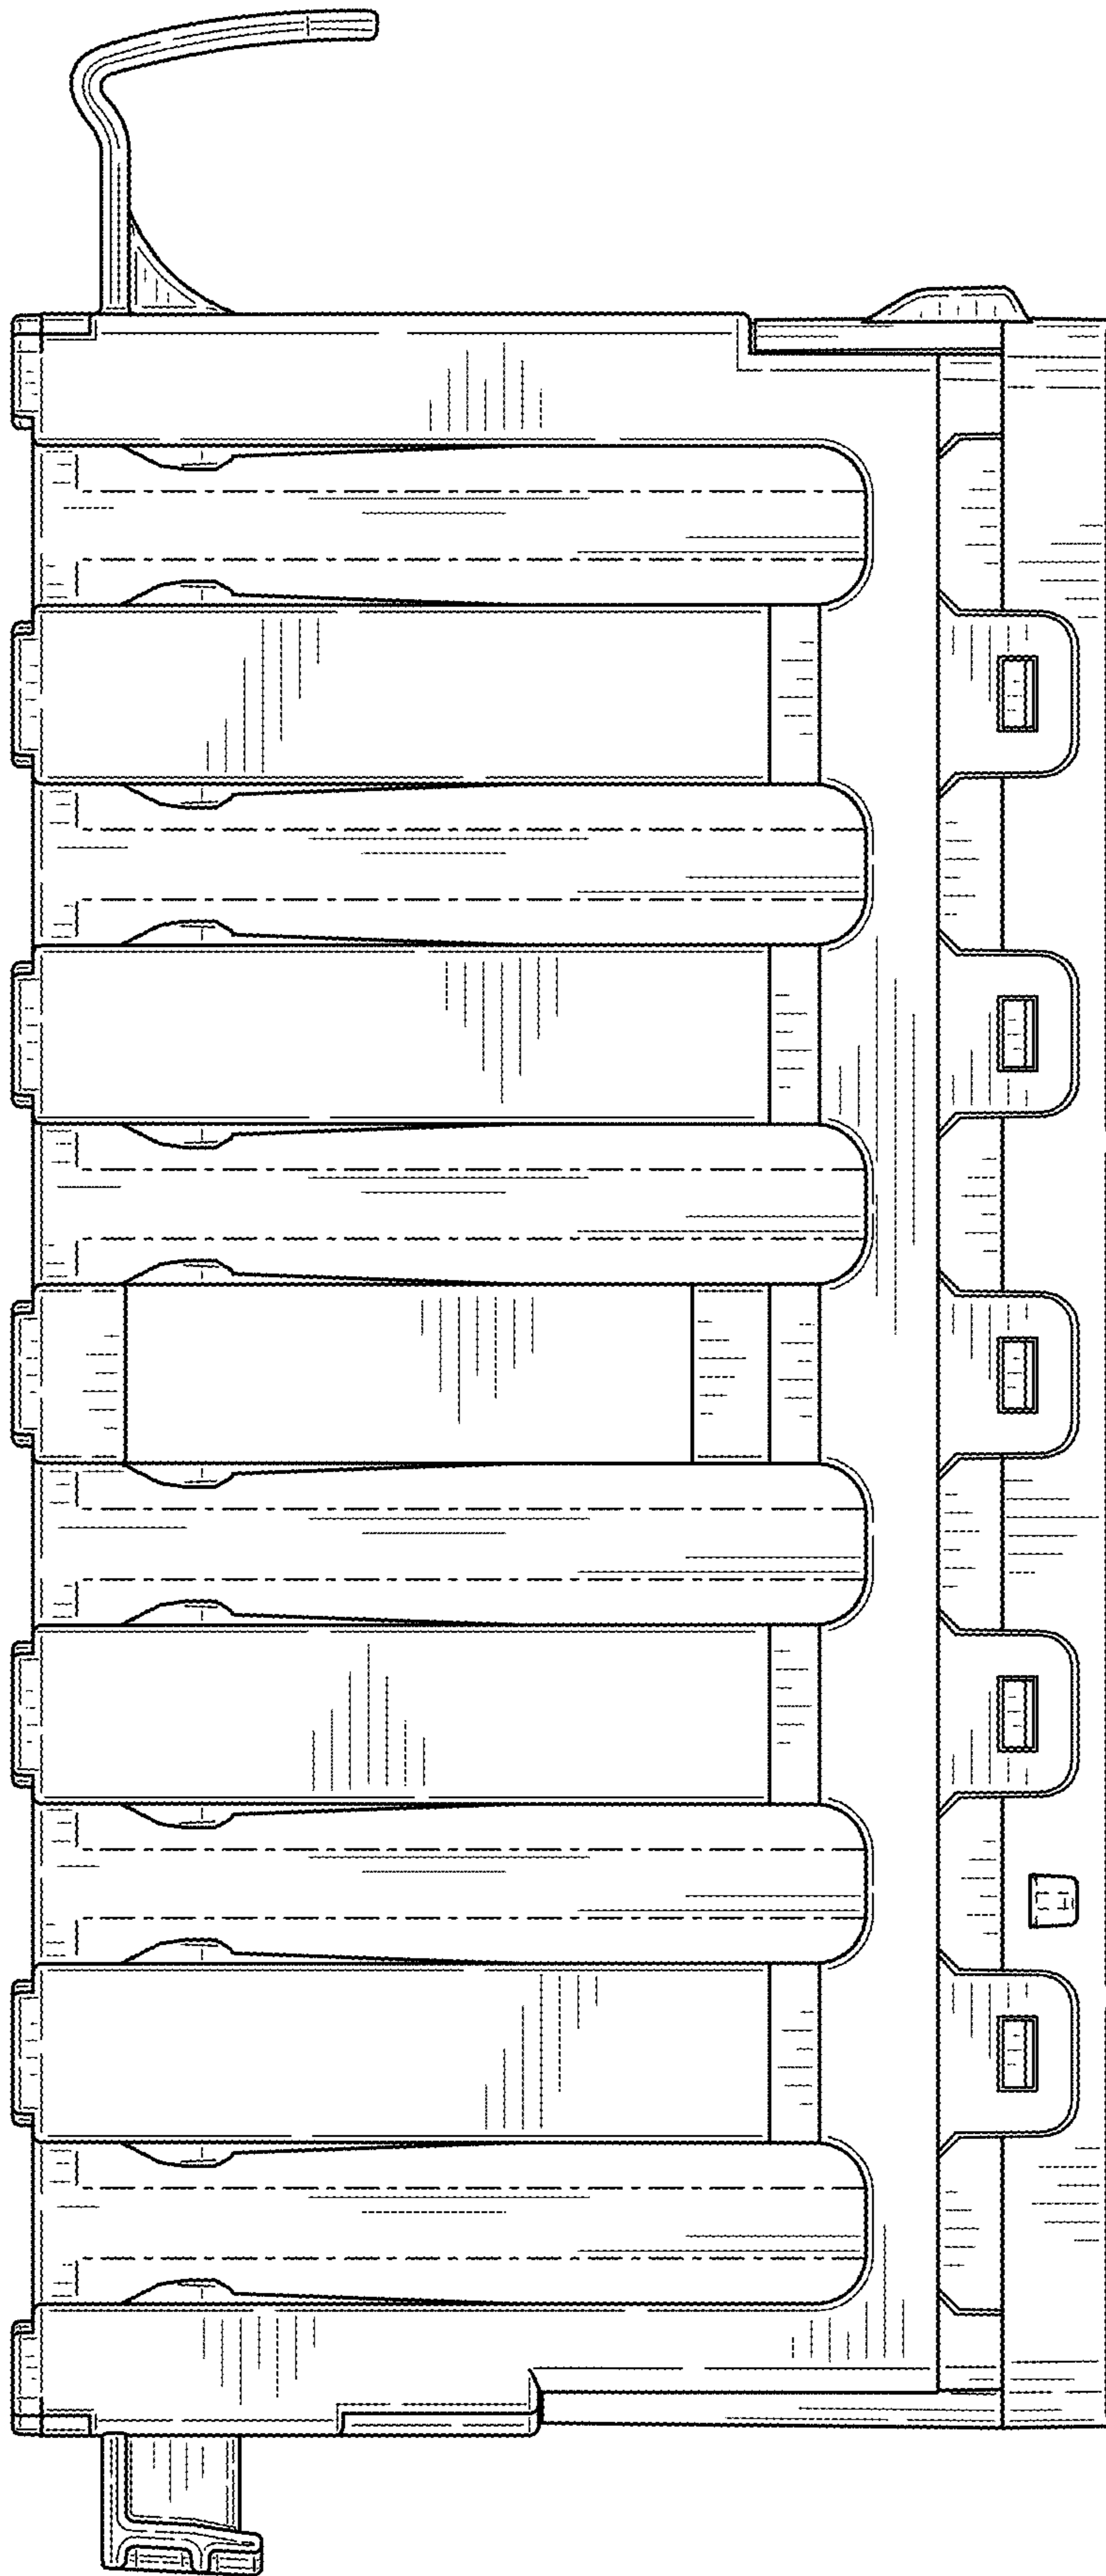


FIG. 15

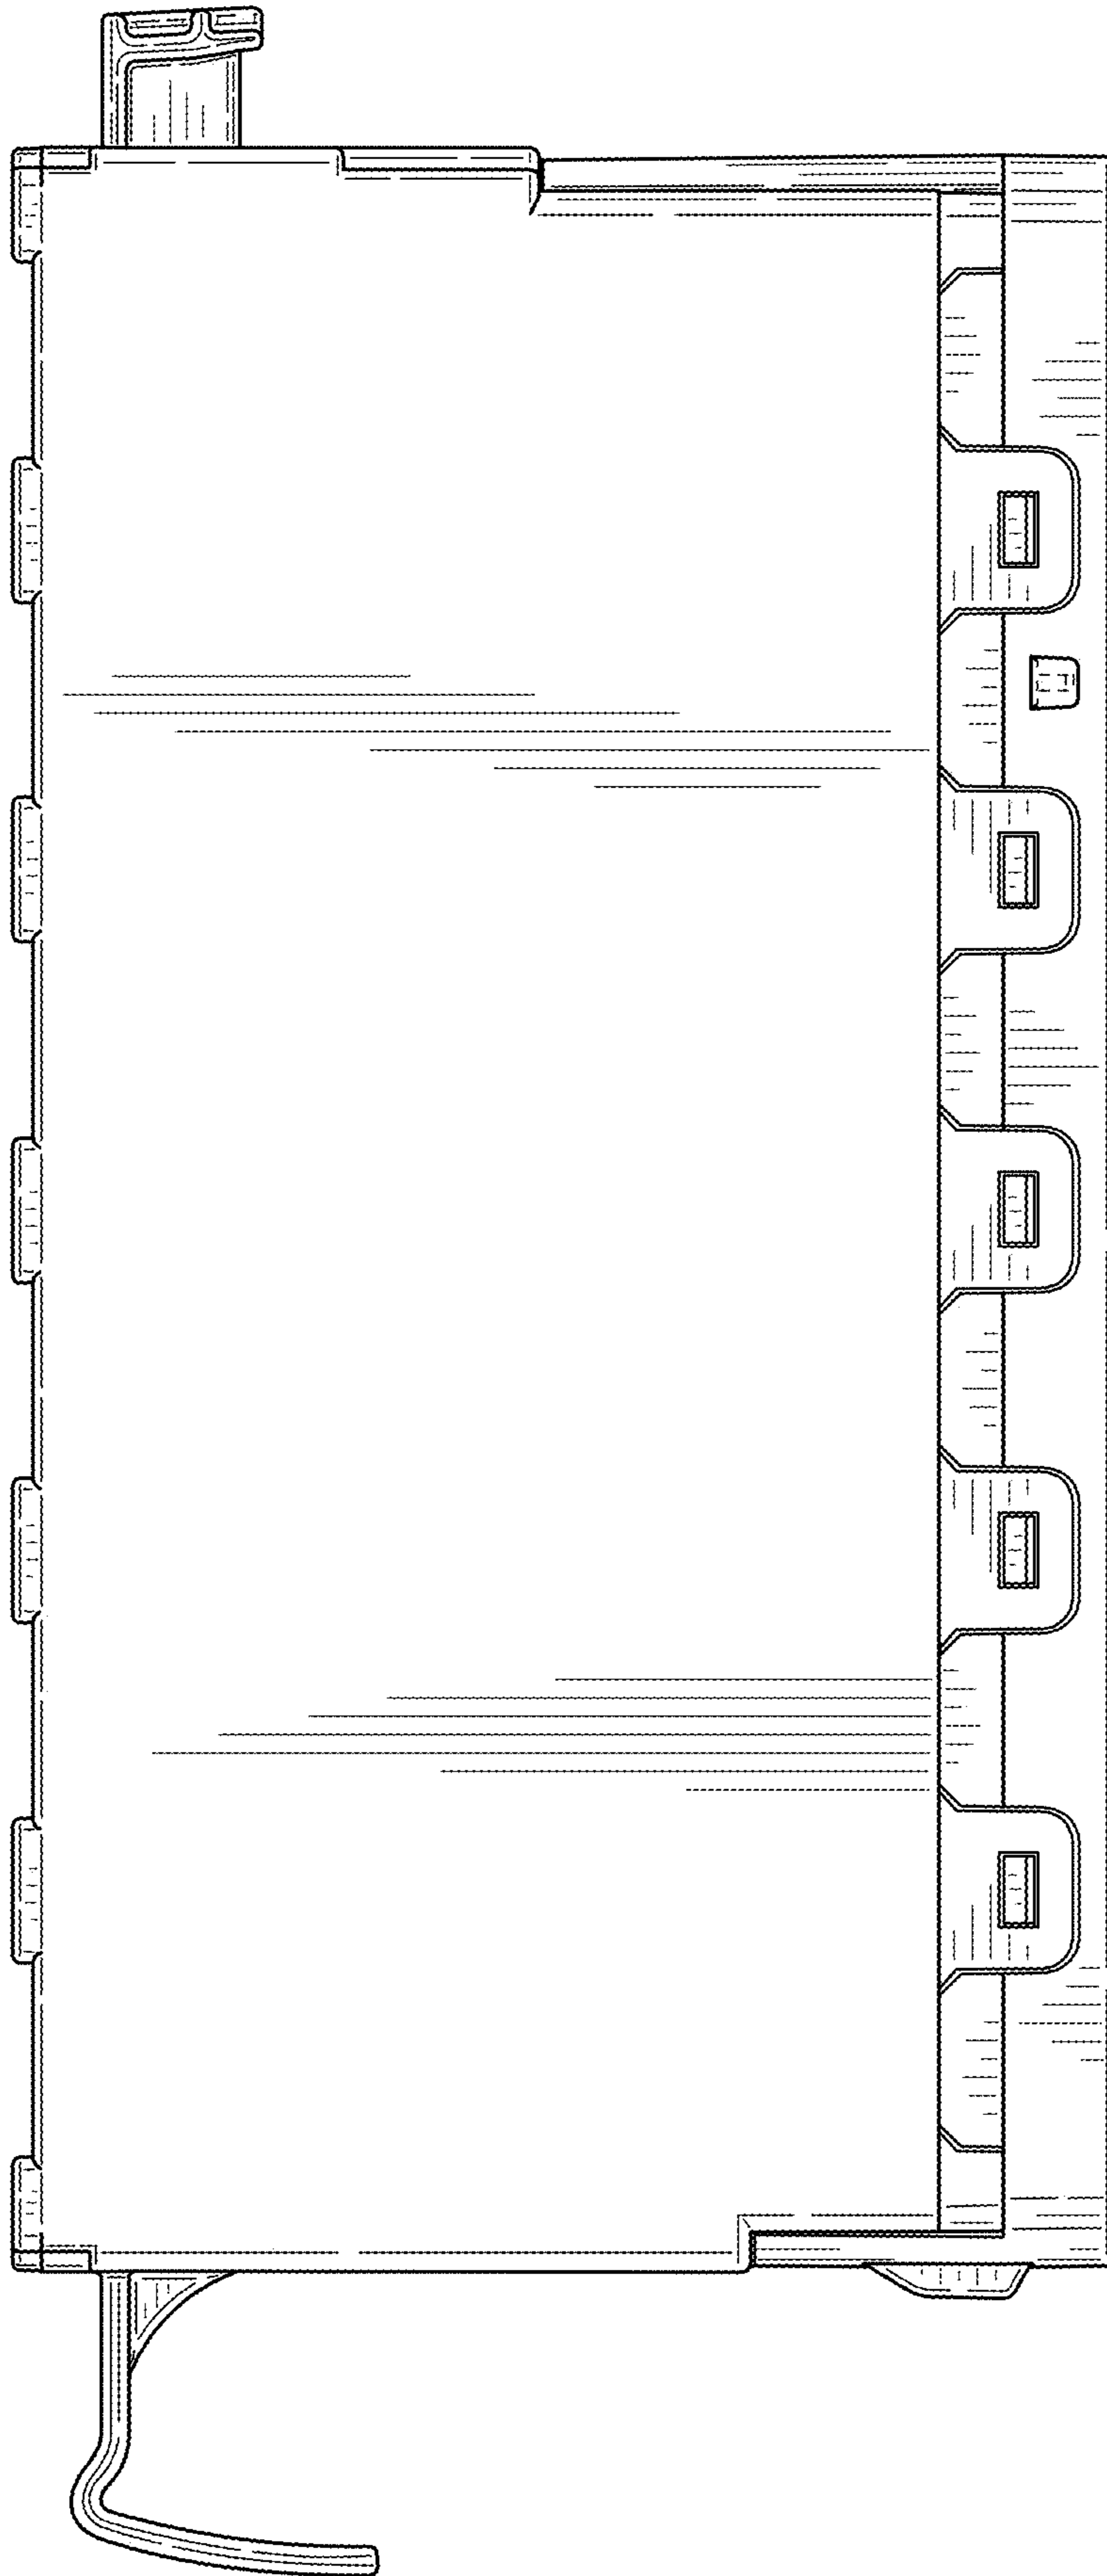


FIG. 16

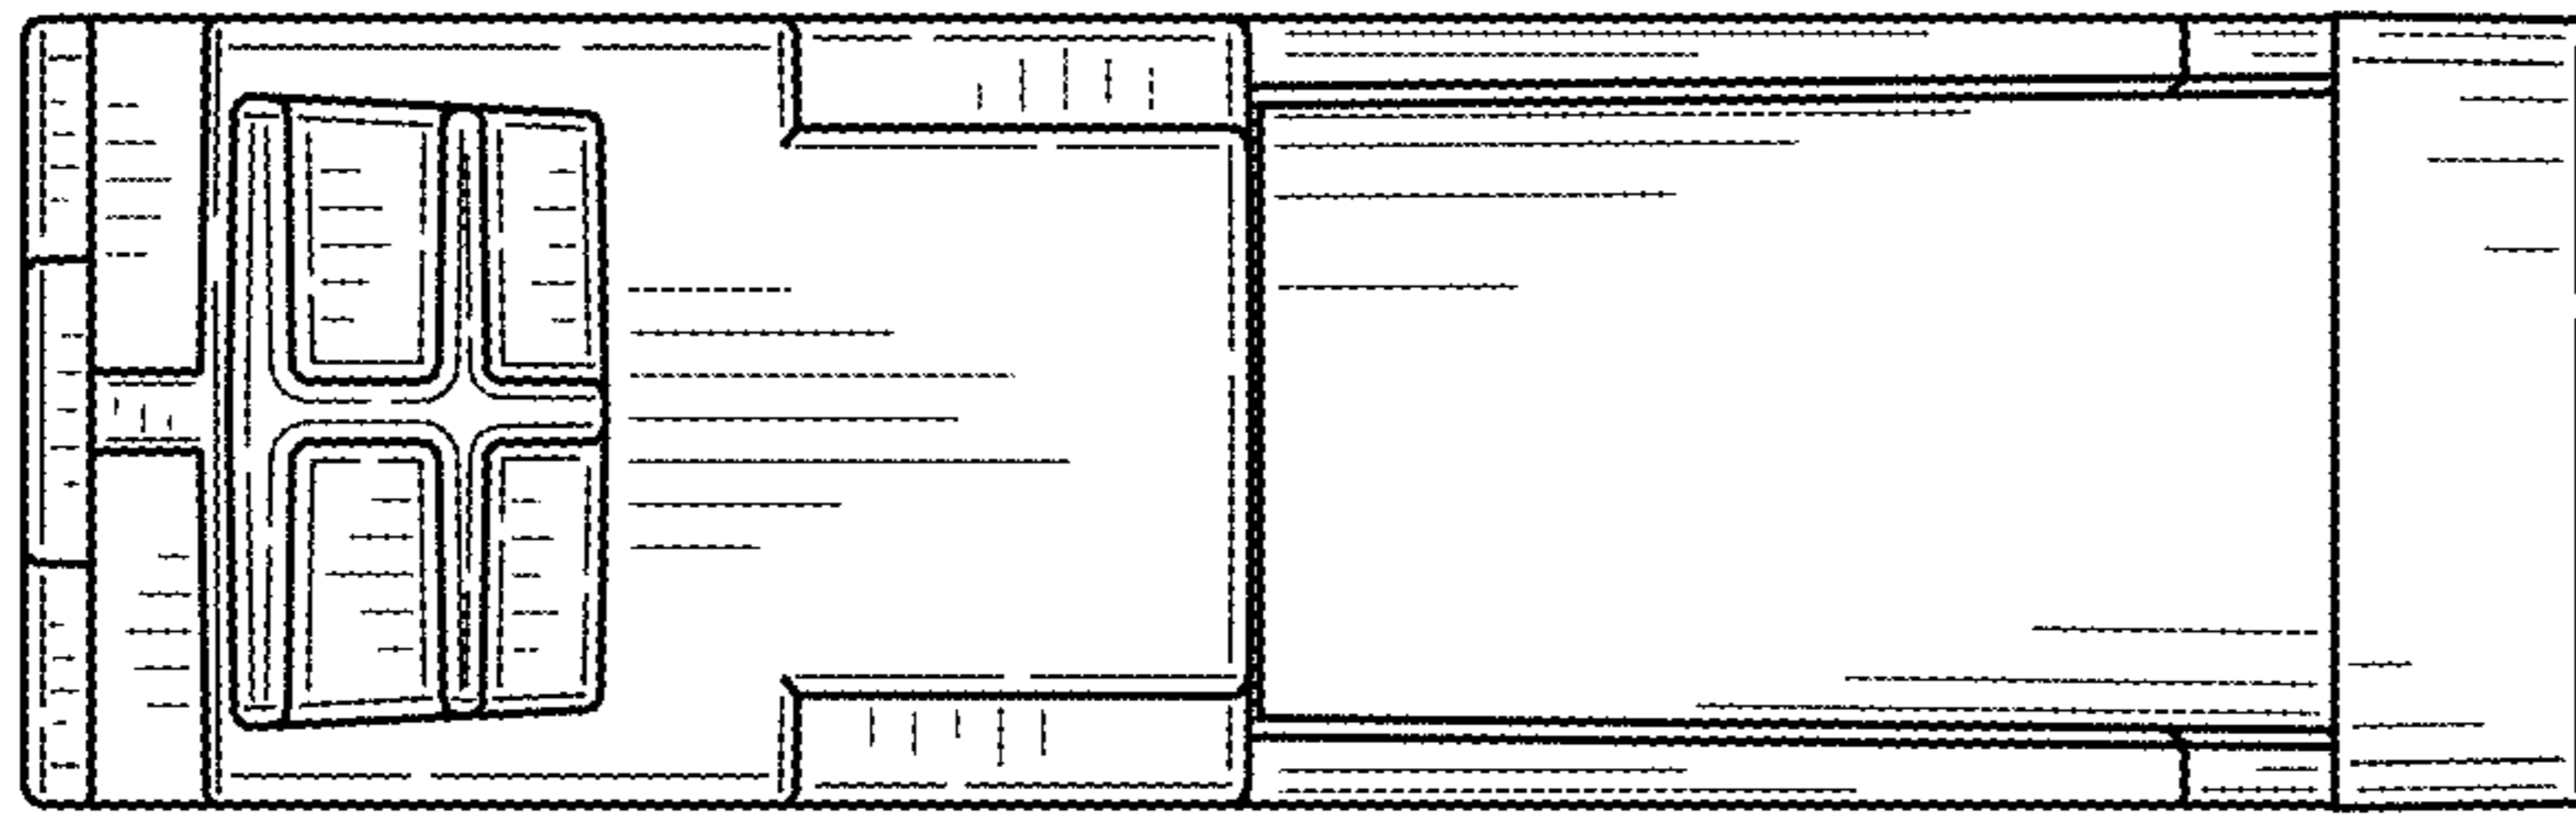


FIG. 18

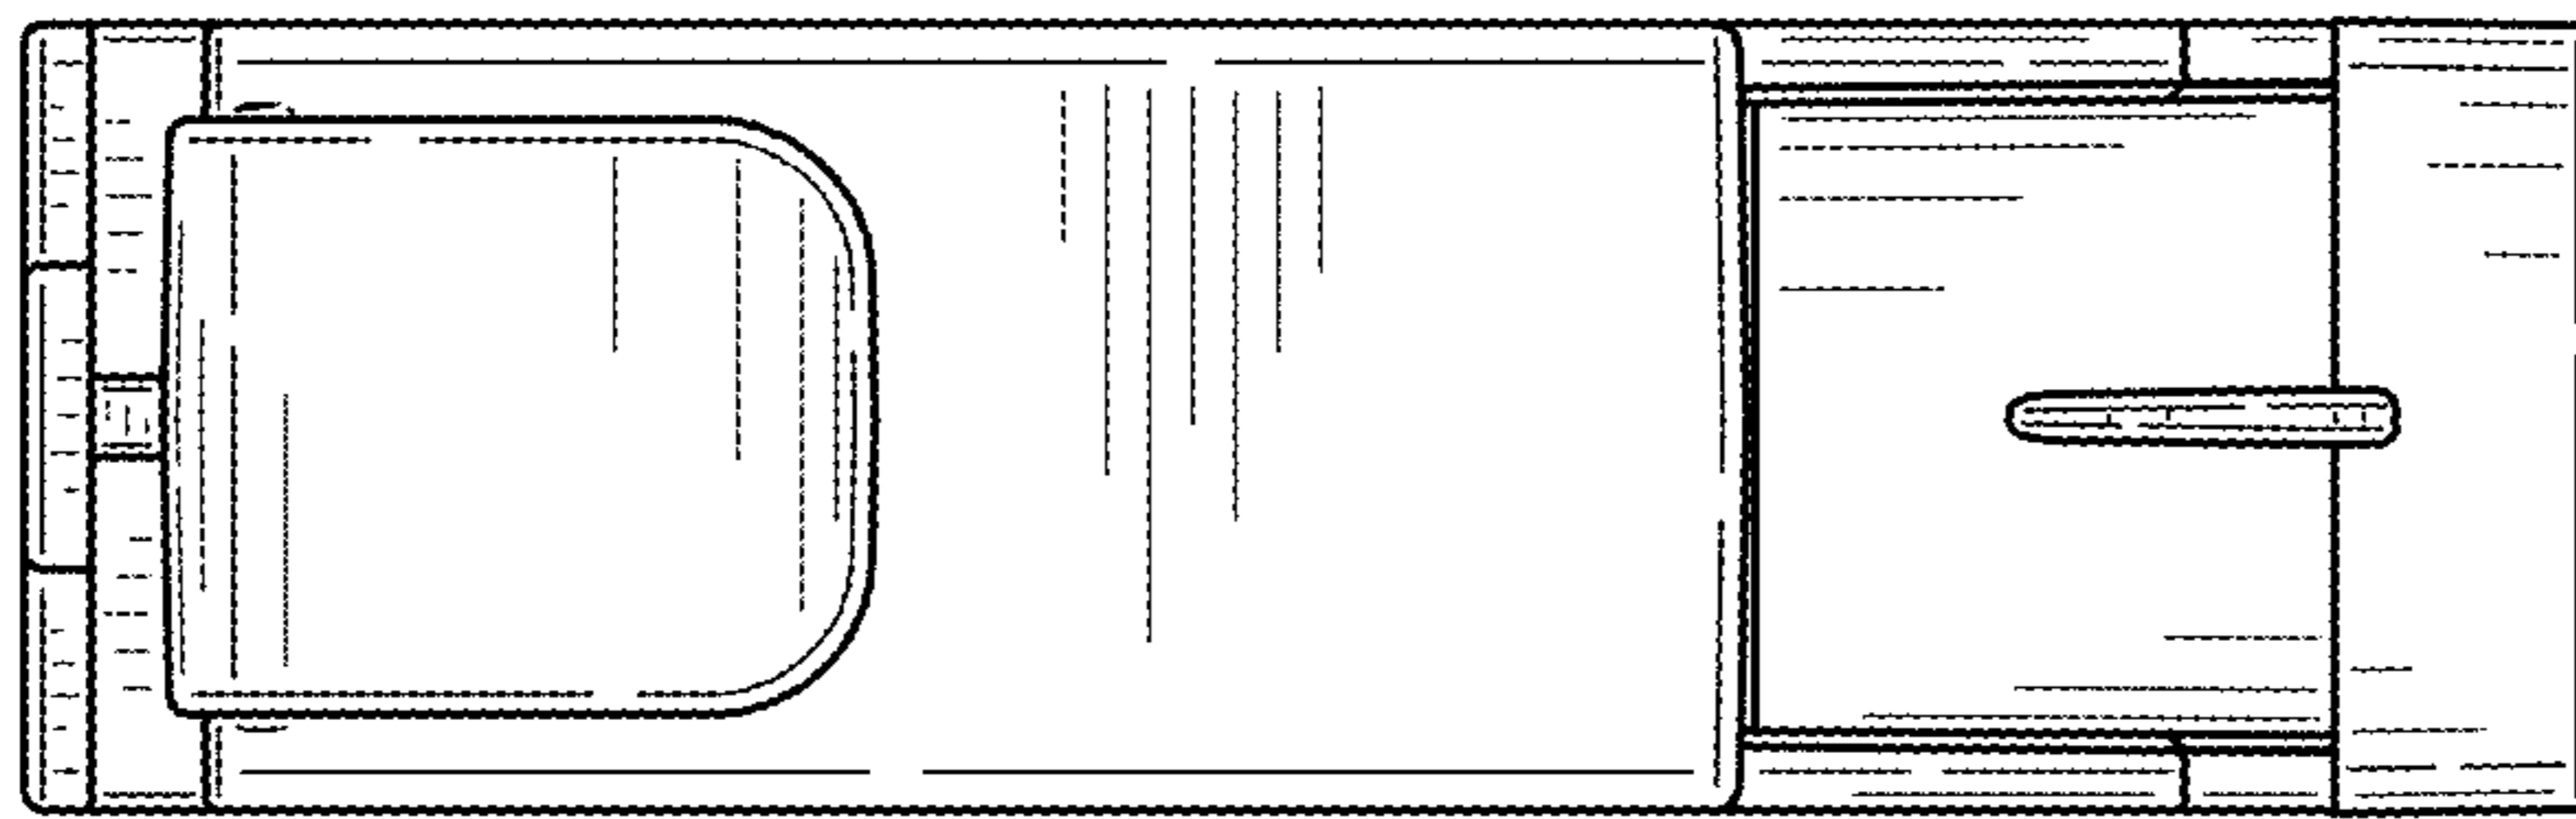


FIG. 17

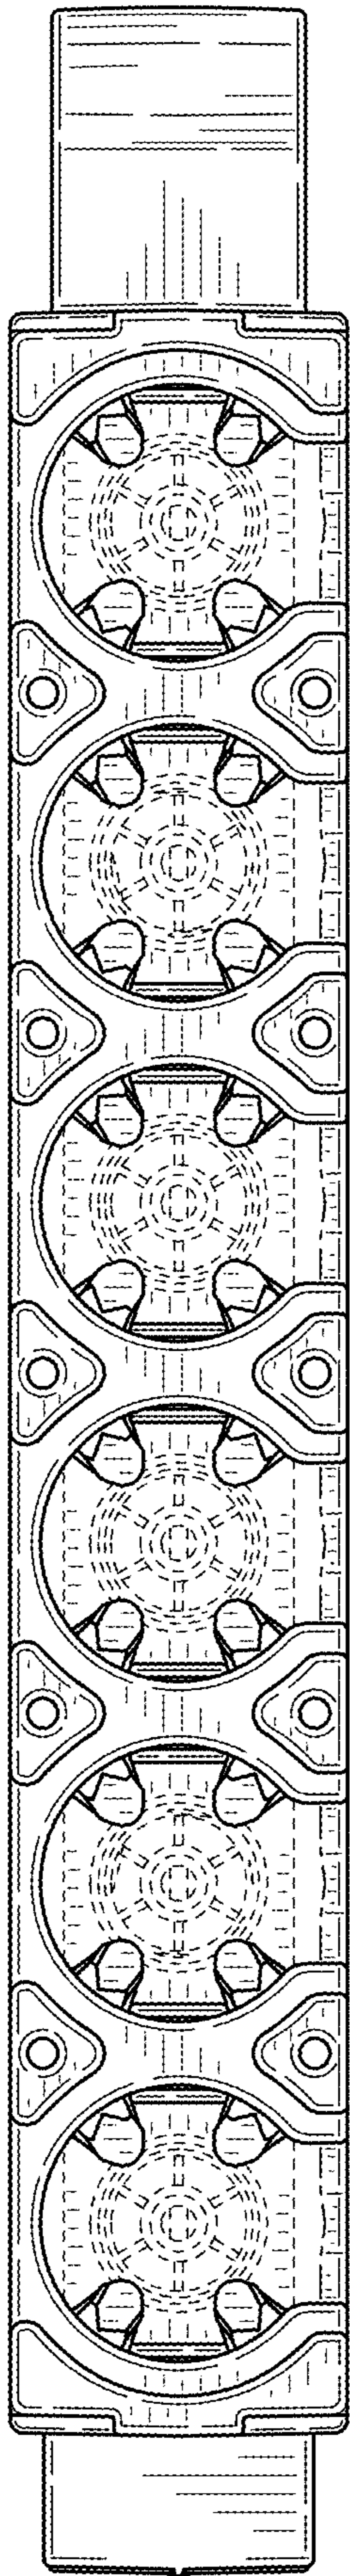


FIG. 19

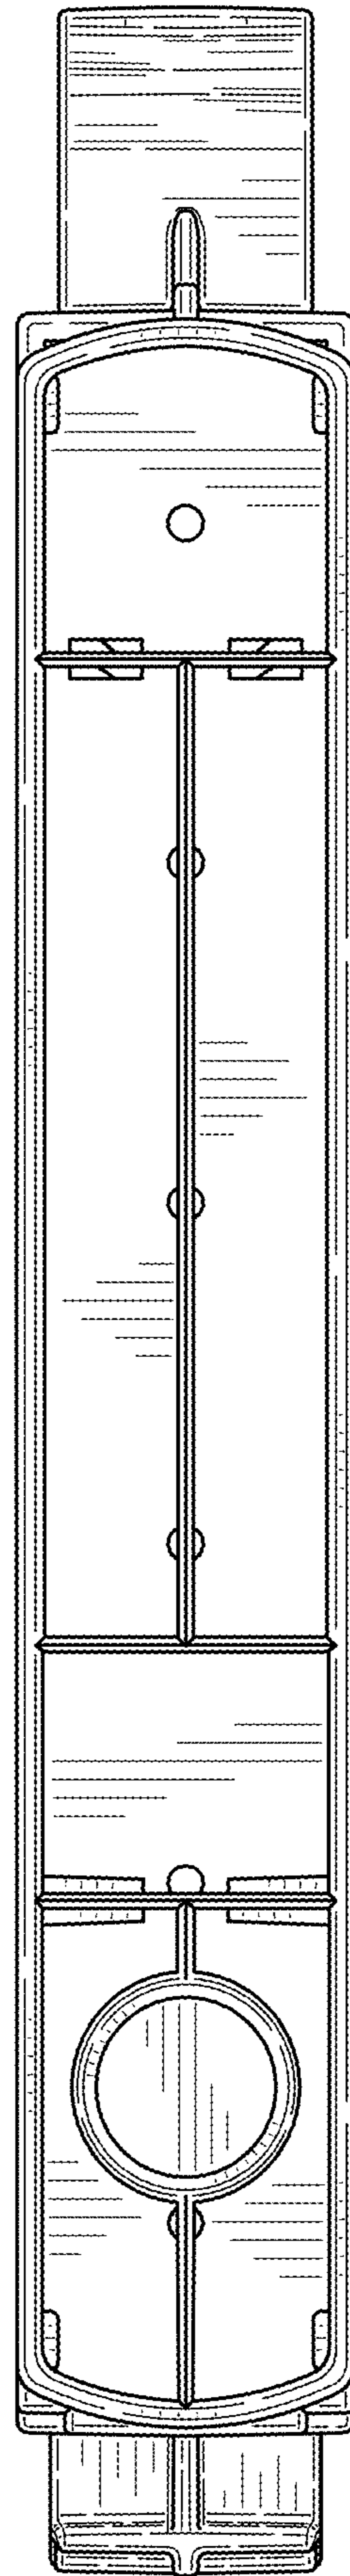


FIG. 20