



US00D938026S

(12) **United States Design Patent** (10) **Patent No.:** **US D938,026 S**
Pendleton et al. (45) **Date of Patent:** **** Dec. 7, 2021**

(54) **SURGICAL STRIKE PLATE HANDLE FOR IMPLANT REMOVAL**
(71) Applicant: **Tightline Development, LLC**, Atlanta, GA (US)
(72) Inventors: **John E. Pendleton**, Atlanta, GA (US); **Daniel H. Hursh**, Roswell, GA (US); **Benjamin M. Stronach**, Madison, MS (US)
(73) Assignee: **TIGHTLINE DEVELOPMENT, LLC.**, Atlanta, GA (US)
(**) Term: **15 Years**

D613,144 S * 4/2010 Lin D8/107
D646,783 S * 10/2011 Bast D24/133
D649,635 S * 11/2011 Cronin D24/133
D663,025 S * 7/2012 Bast D24/133
D687,690 S * 8/2013 Chen D8/105
D707,356 S * 6/2014 Vonck D24/133
8,834,480 B2 9/2014 Hudak, Jr. et al.
D715,431 S * 10/2014 Vonck D24/133
D724,410 S * 3/2015 Han D8/307
9,089,440 B2 7/2015 Mueller
D771,249 S * 11/2016 Heath D24/133
D799,302 S * 10/2017 Bast D8/107
D803,025 S * 11/2017 Larose D8/300
D839,066 S * 1/2019 Bast D8/14
D845,740 S * 4/2019 Bast D8/107
D856,513 S * 8/2019 Taylor D24/133
2010/0288087 A1* 11/2010 Lai B25G 1/085
81/490

(21) Appl. No.: **29/674,291**
(22) Filed: **Dec. 20, 2018**
(51) **LOC (13) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/133**
(58) **Field of Classification Search**
USPC D24/133, 134, 137, 138, 172, 173, 174,
D24/187, 143, 200, 145; D8/14, 21, 82,
D8/83, 84, 85, 86, 107, 34; D6/540, 546,
D6/554, 556
CPC A61B 17/64; A61B 17/62; A61B 17/00;
A61B 7/70; A61B 7/02; A61B 7/003;
A61B 7/04; H04R 1/46
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
6,151,998 A * 11/2000 Fu-Hui B25G 1/085
81/177.1
6,565,575 B2 5/2003 Lewis
7,272,999 B2* 9/2007 Cutler B25B 15/02
81/467
D557,584 S * 12/2007 Gao D8/107

(Continued)

Primary Examiner — Manpreet S Matharu
Assistant Examiner — Yolanda Robinson
(74) *Attorney, Agent, or Firm* — Fisherbroyles, LLP;
Anthony J DoVale


(57) **CLAIM**

The ornamental design for a surgical strike plate handle for implant removal, as shown and described.

DESCRIPTION

FIG. 1 is a front side view of a strike plate handle for implant removal showing our new design; FIG. 2 is a back side view thereof; FIG. 3 is a left, side view thereof; FIG. 4 is a right, side view thereof; FIG. 5 is a top plan view thereof; and, FIG. 6 is a bottom plan view thereof. The broken lines shown in the surgical strike plate handle for implant removal are for portions that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

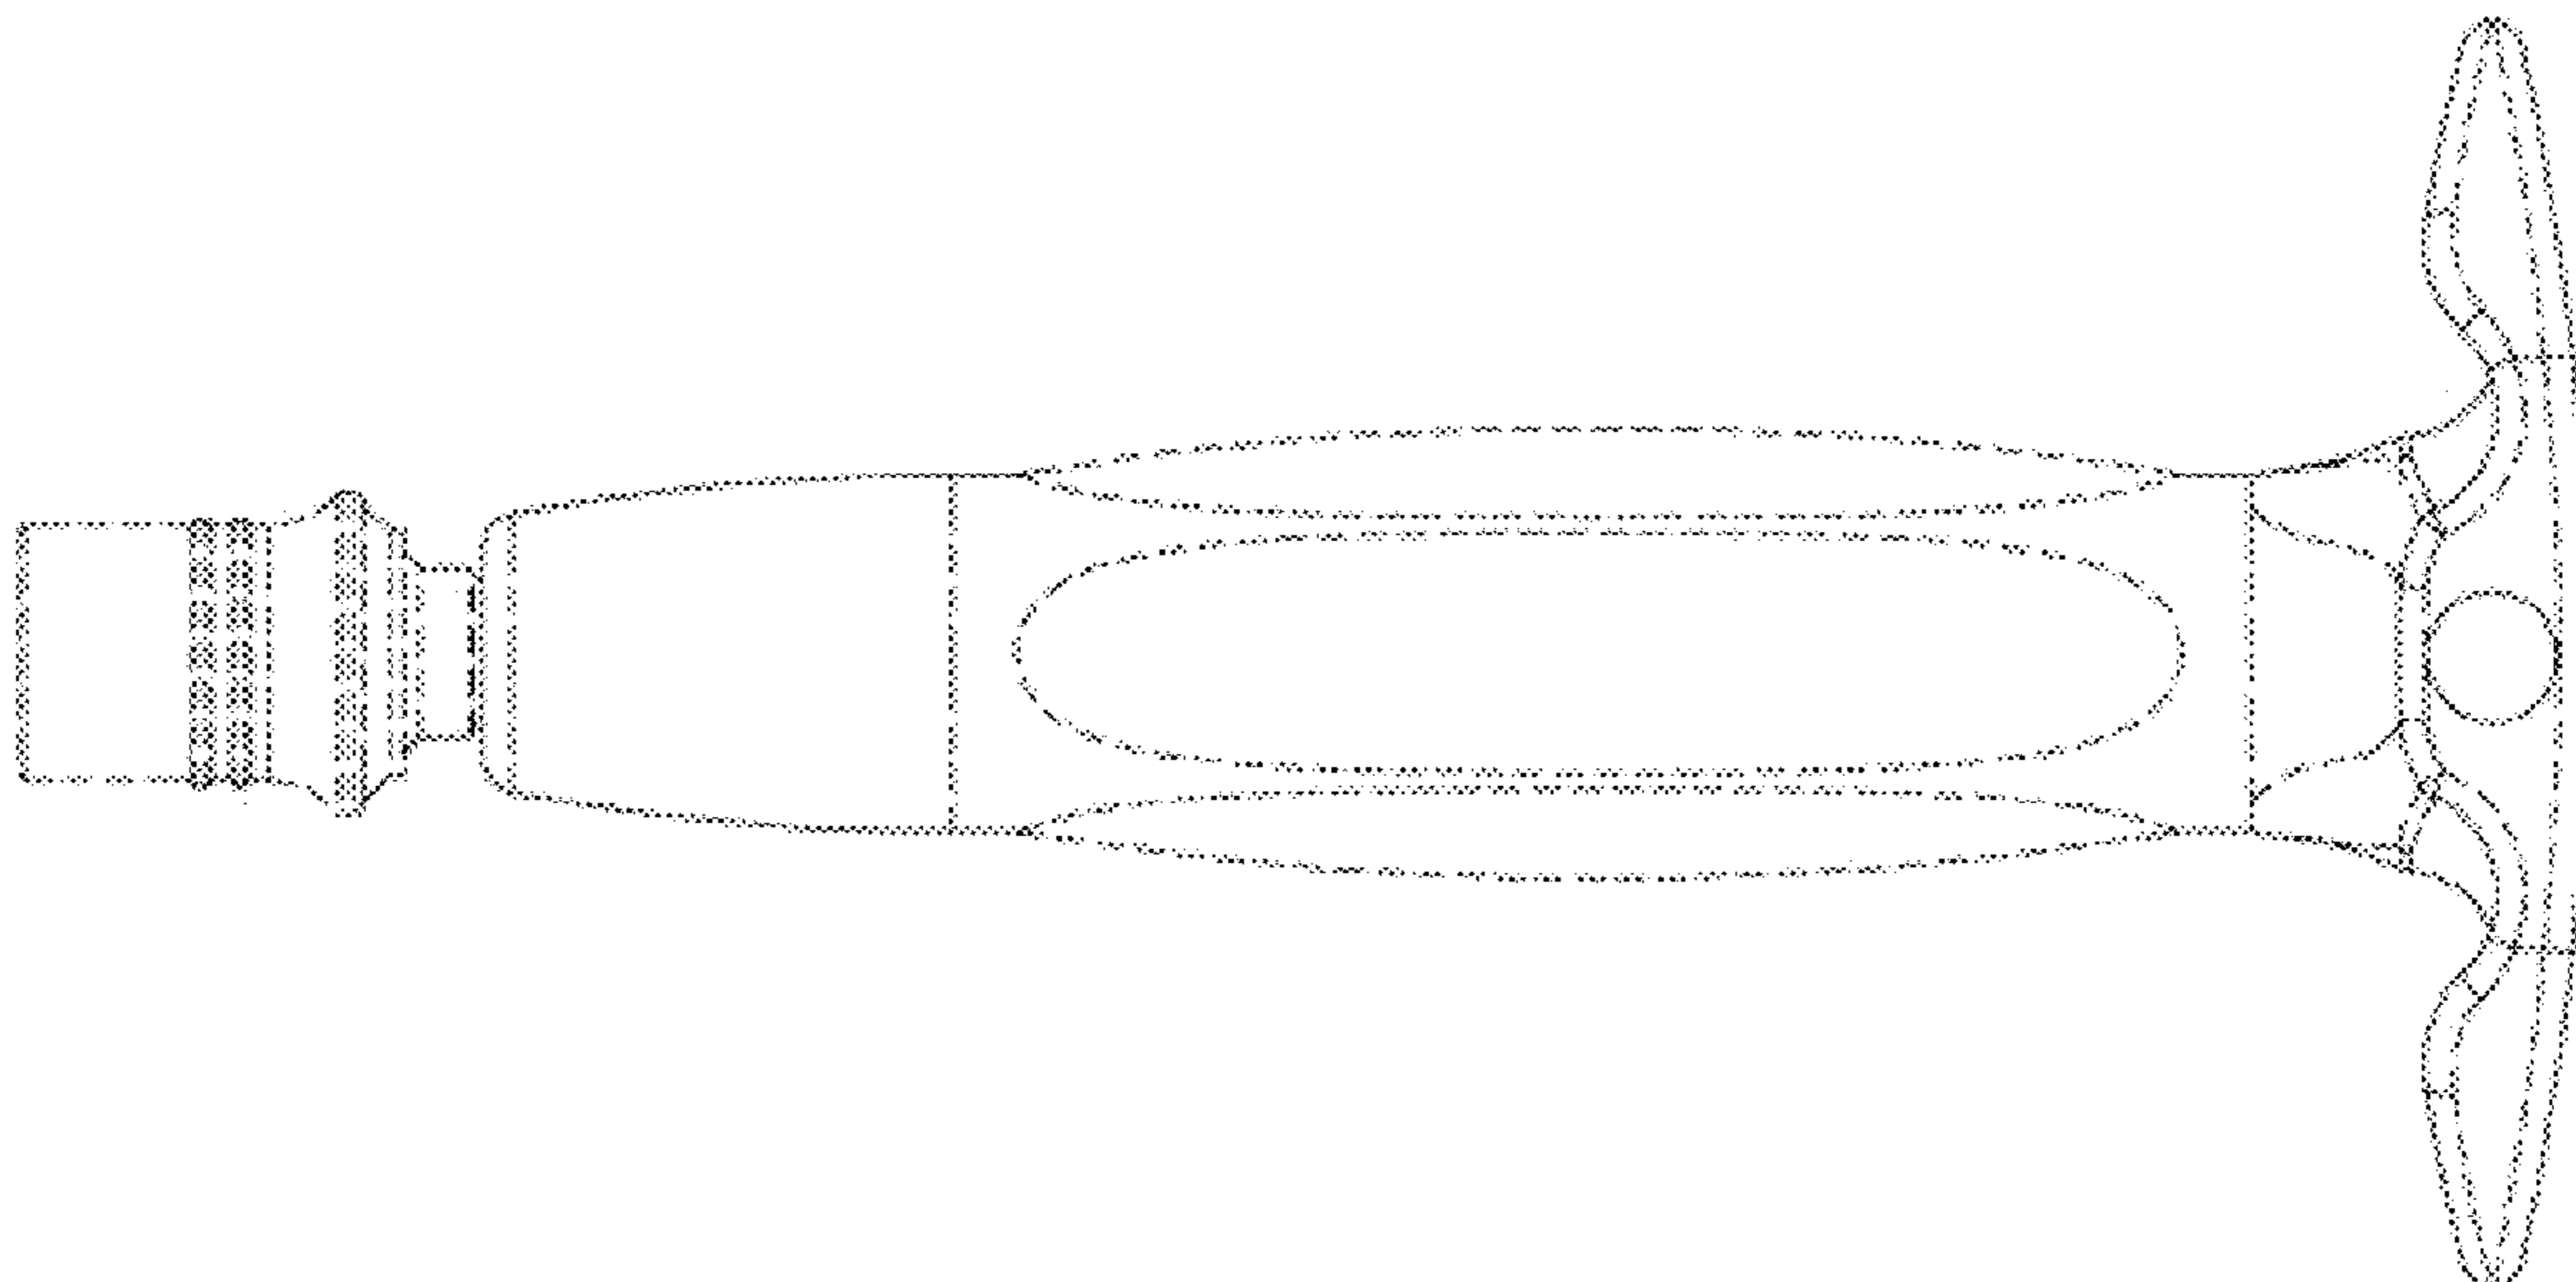

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0100957 A1 4/2016 Lewis
2018/0206859 A1 7/2018 Pendleton et al.

* cited by examiner

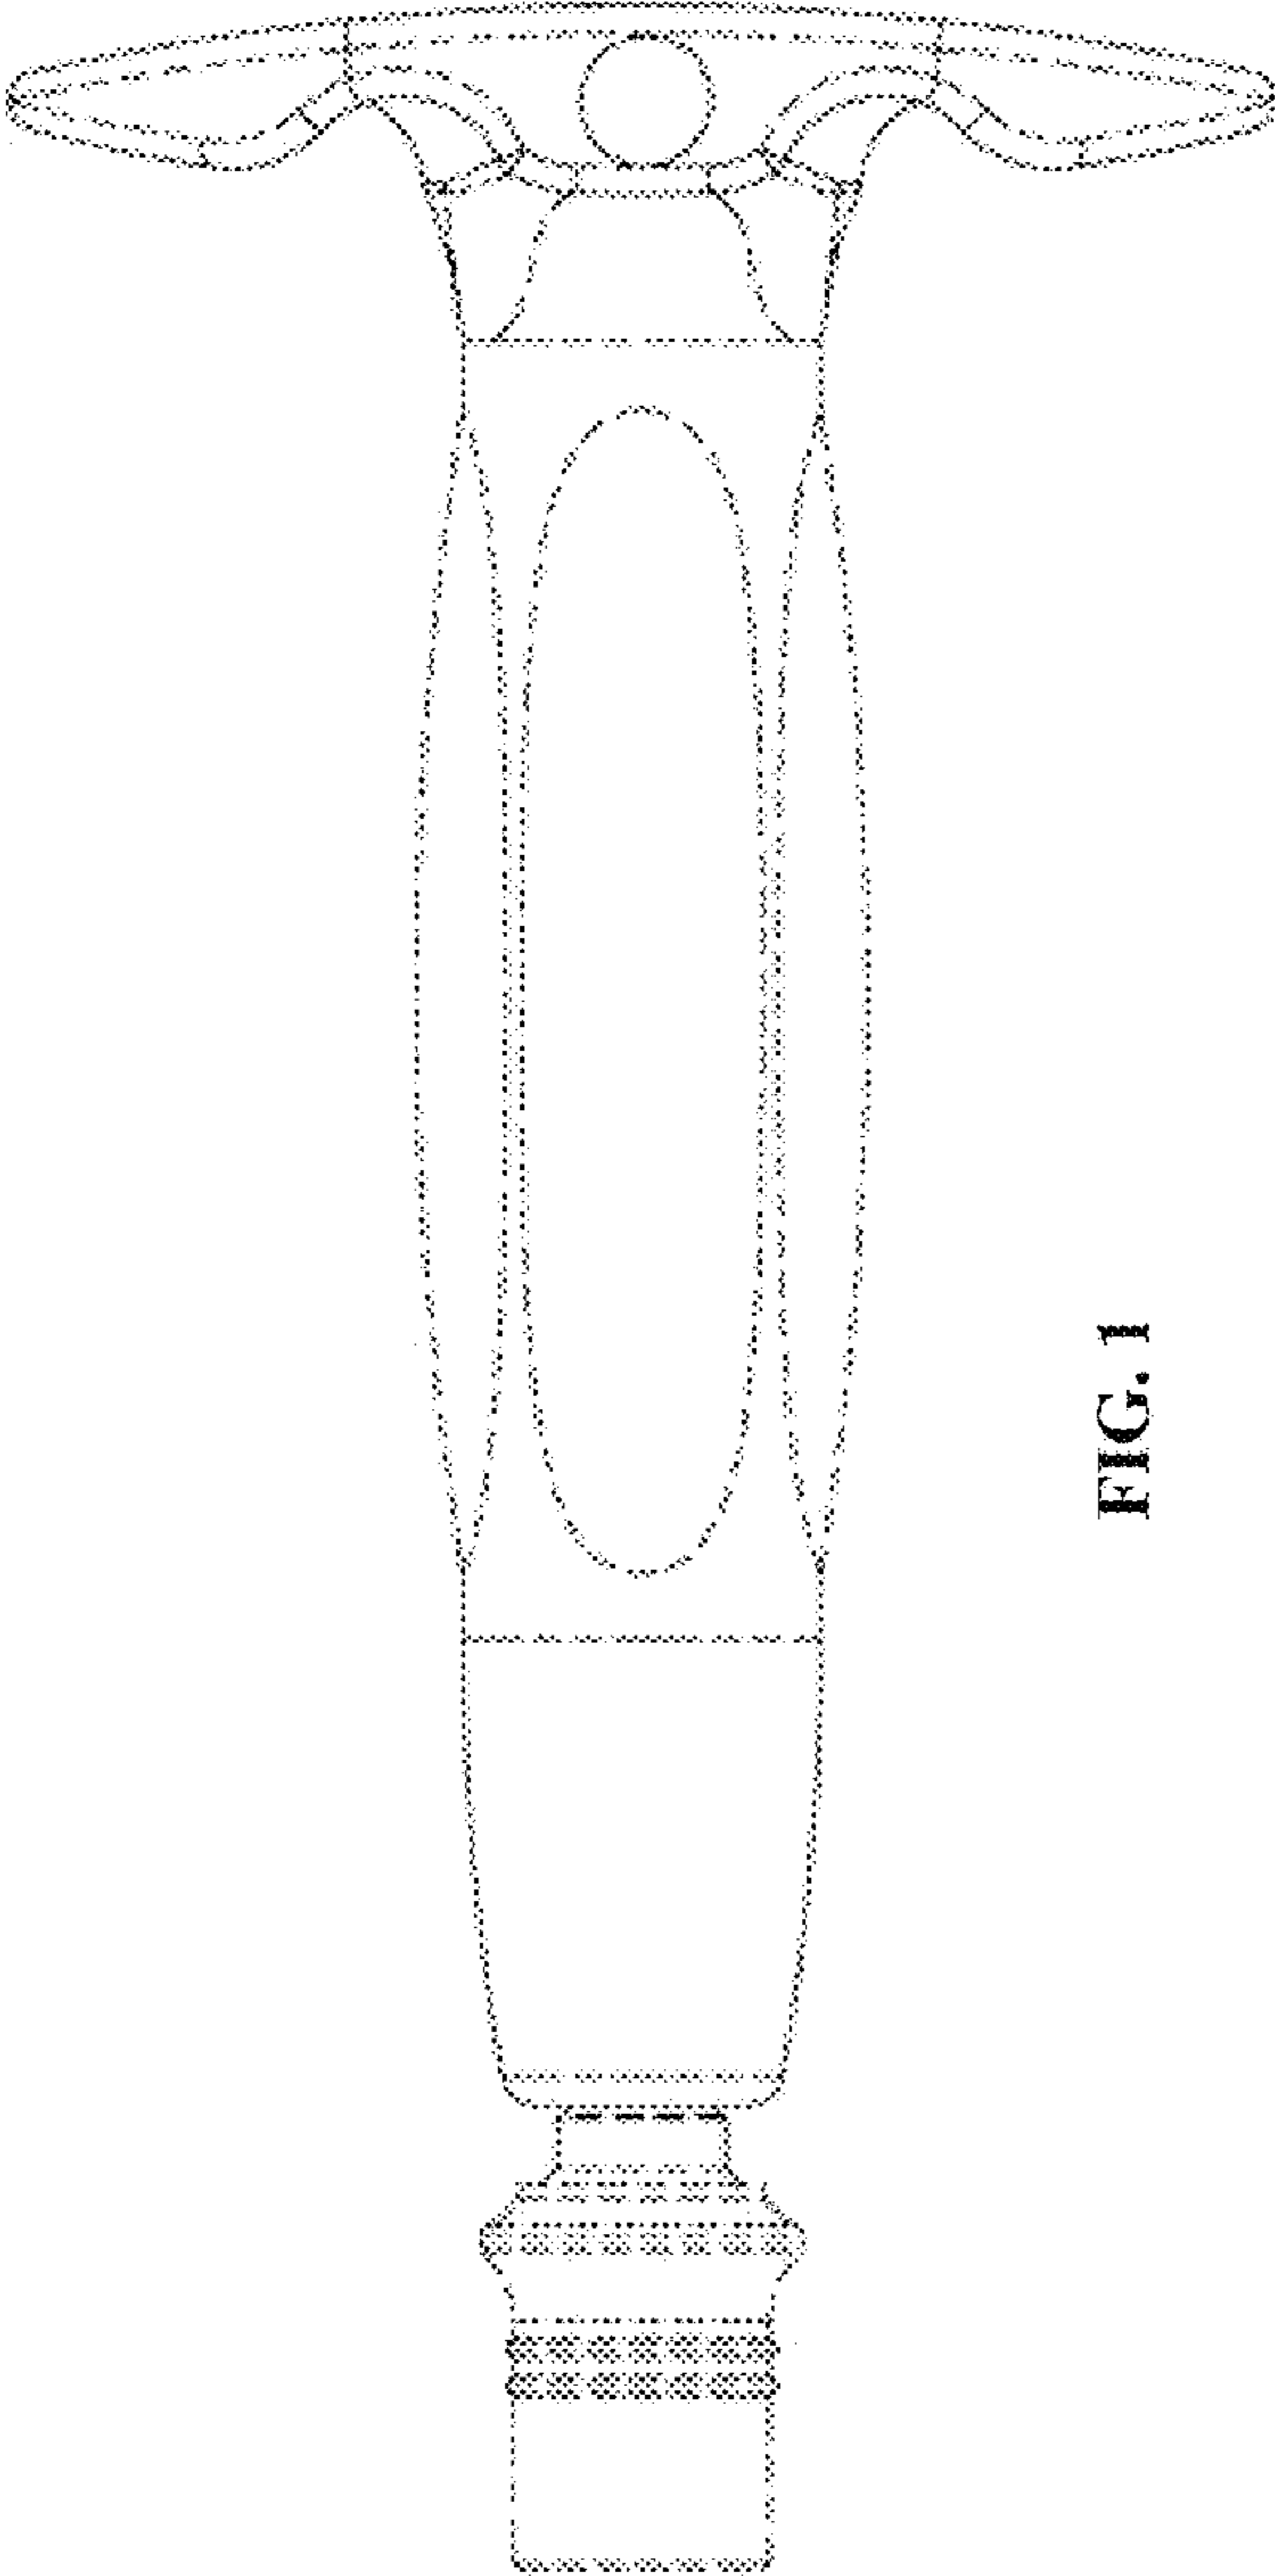


FIG. 1

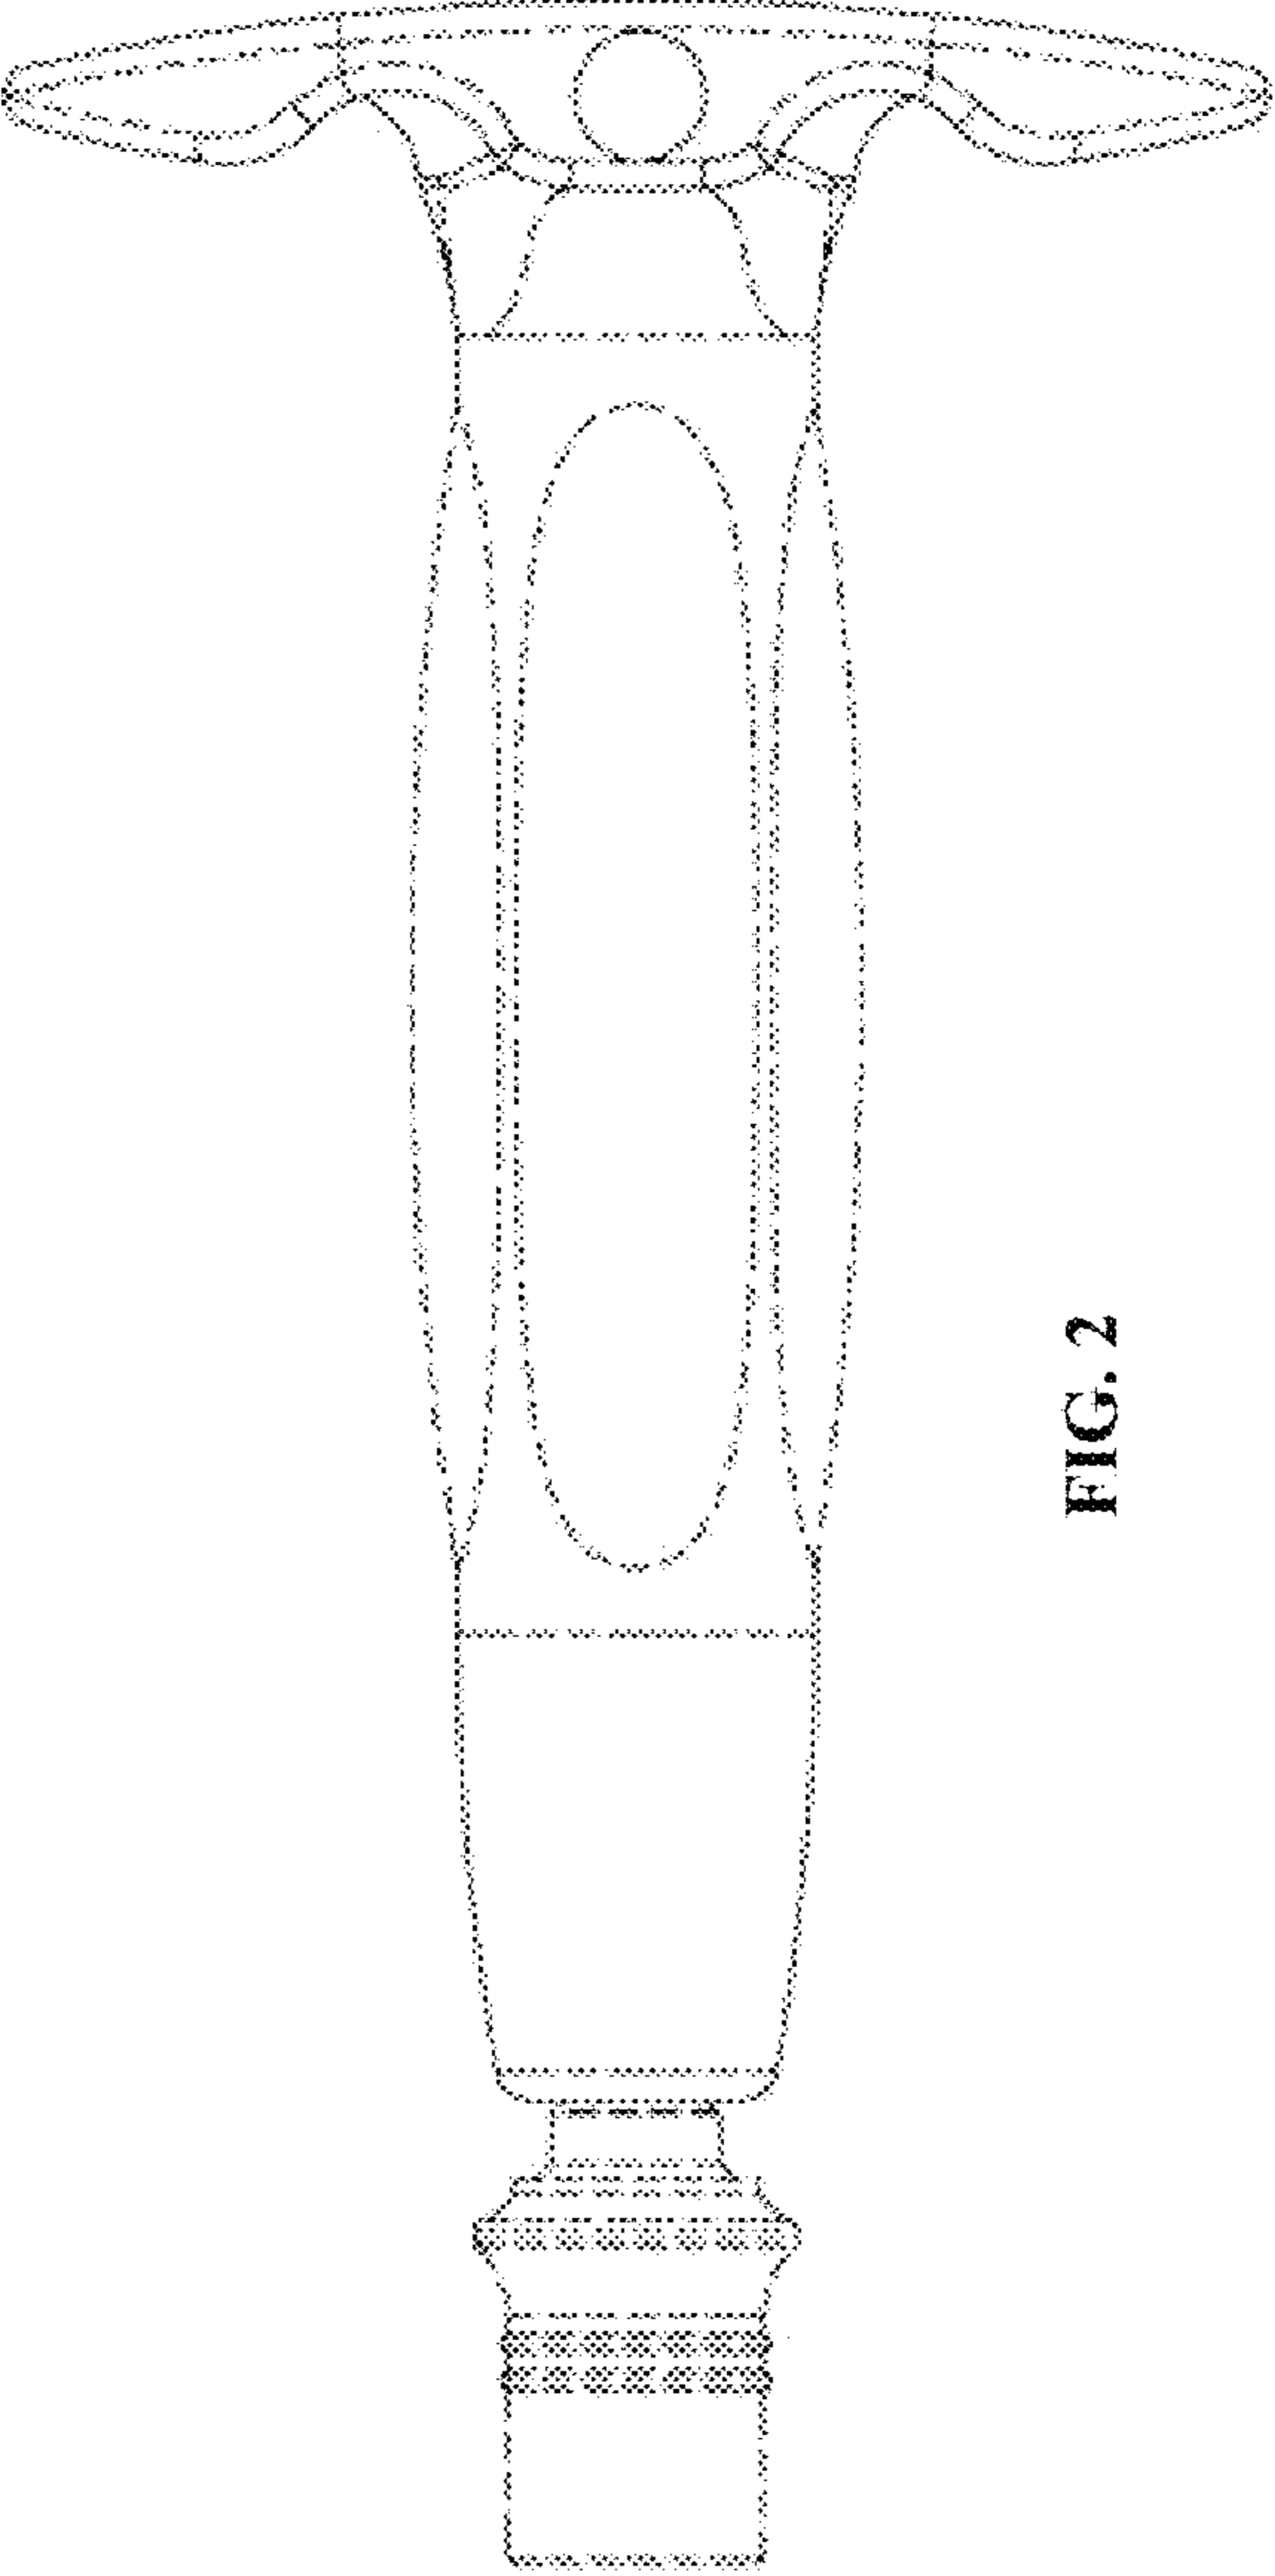


FIG. 2

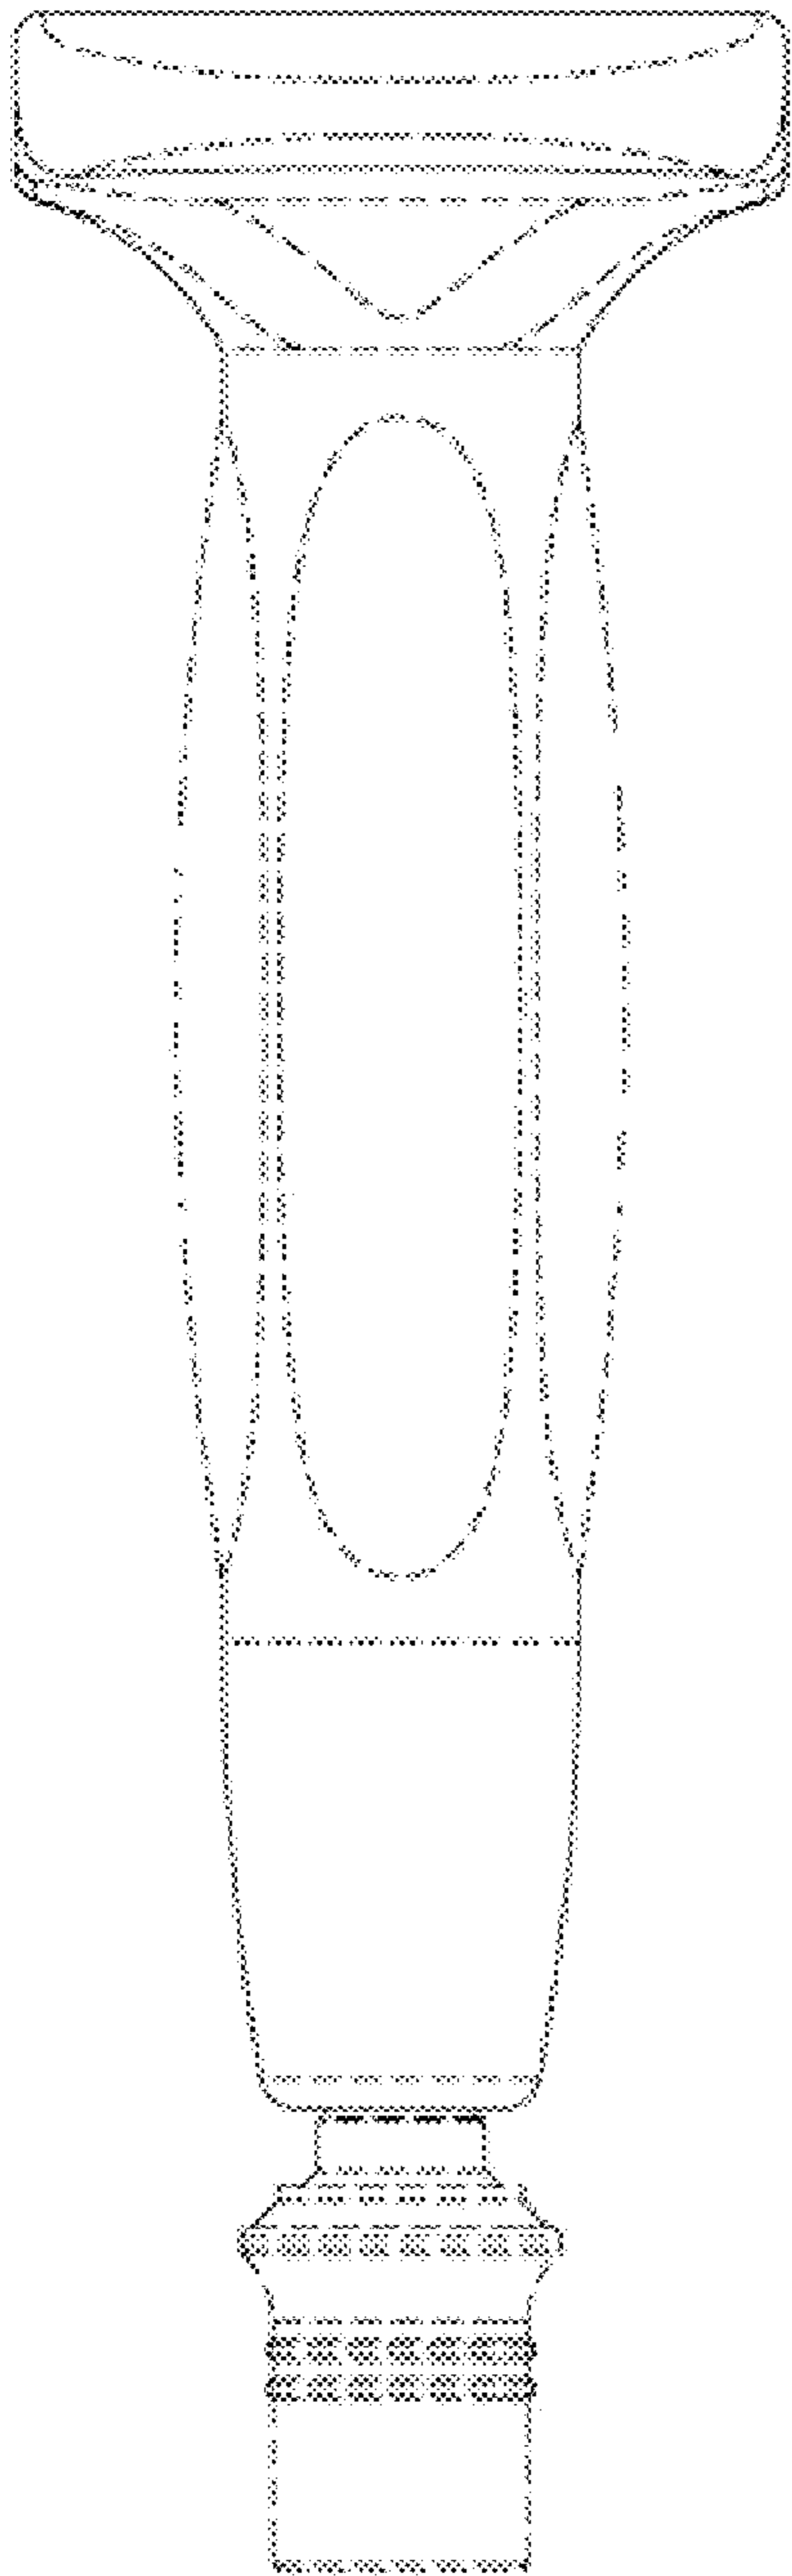


FIG. 3

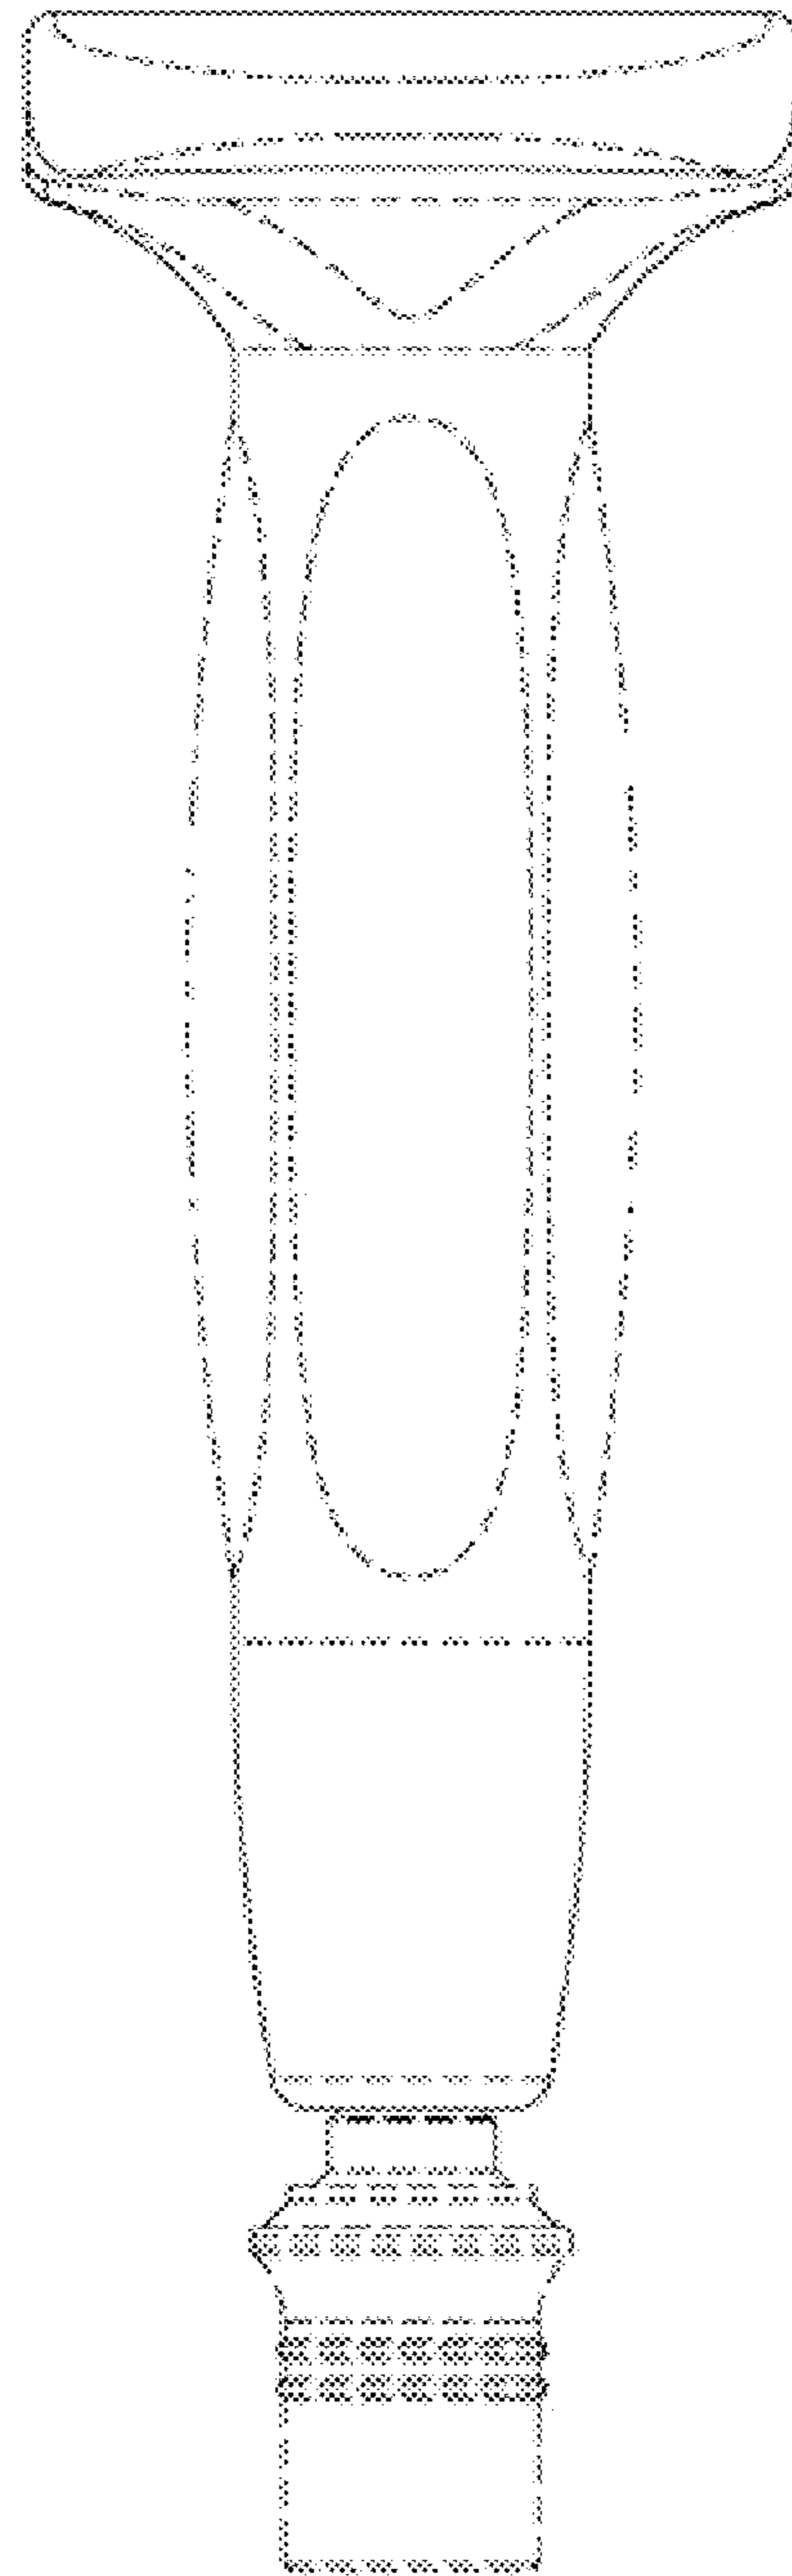


FIG. 4

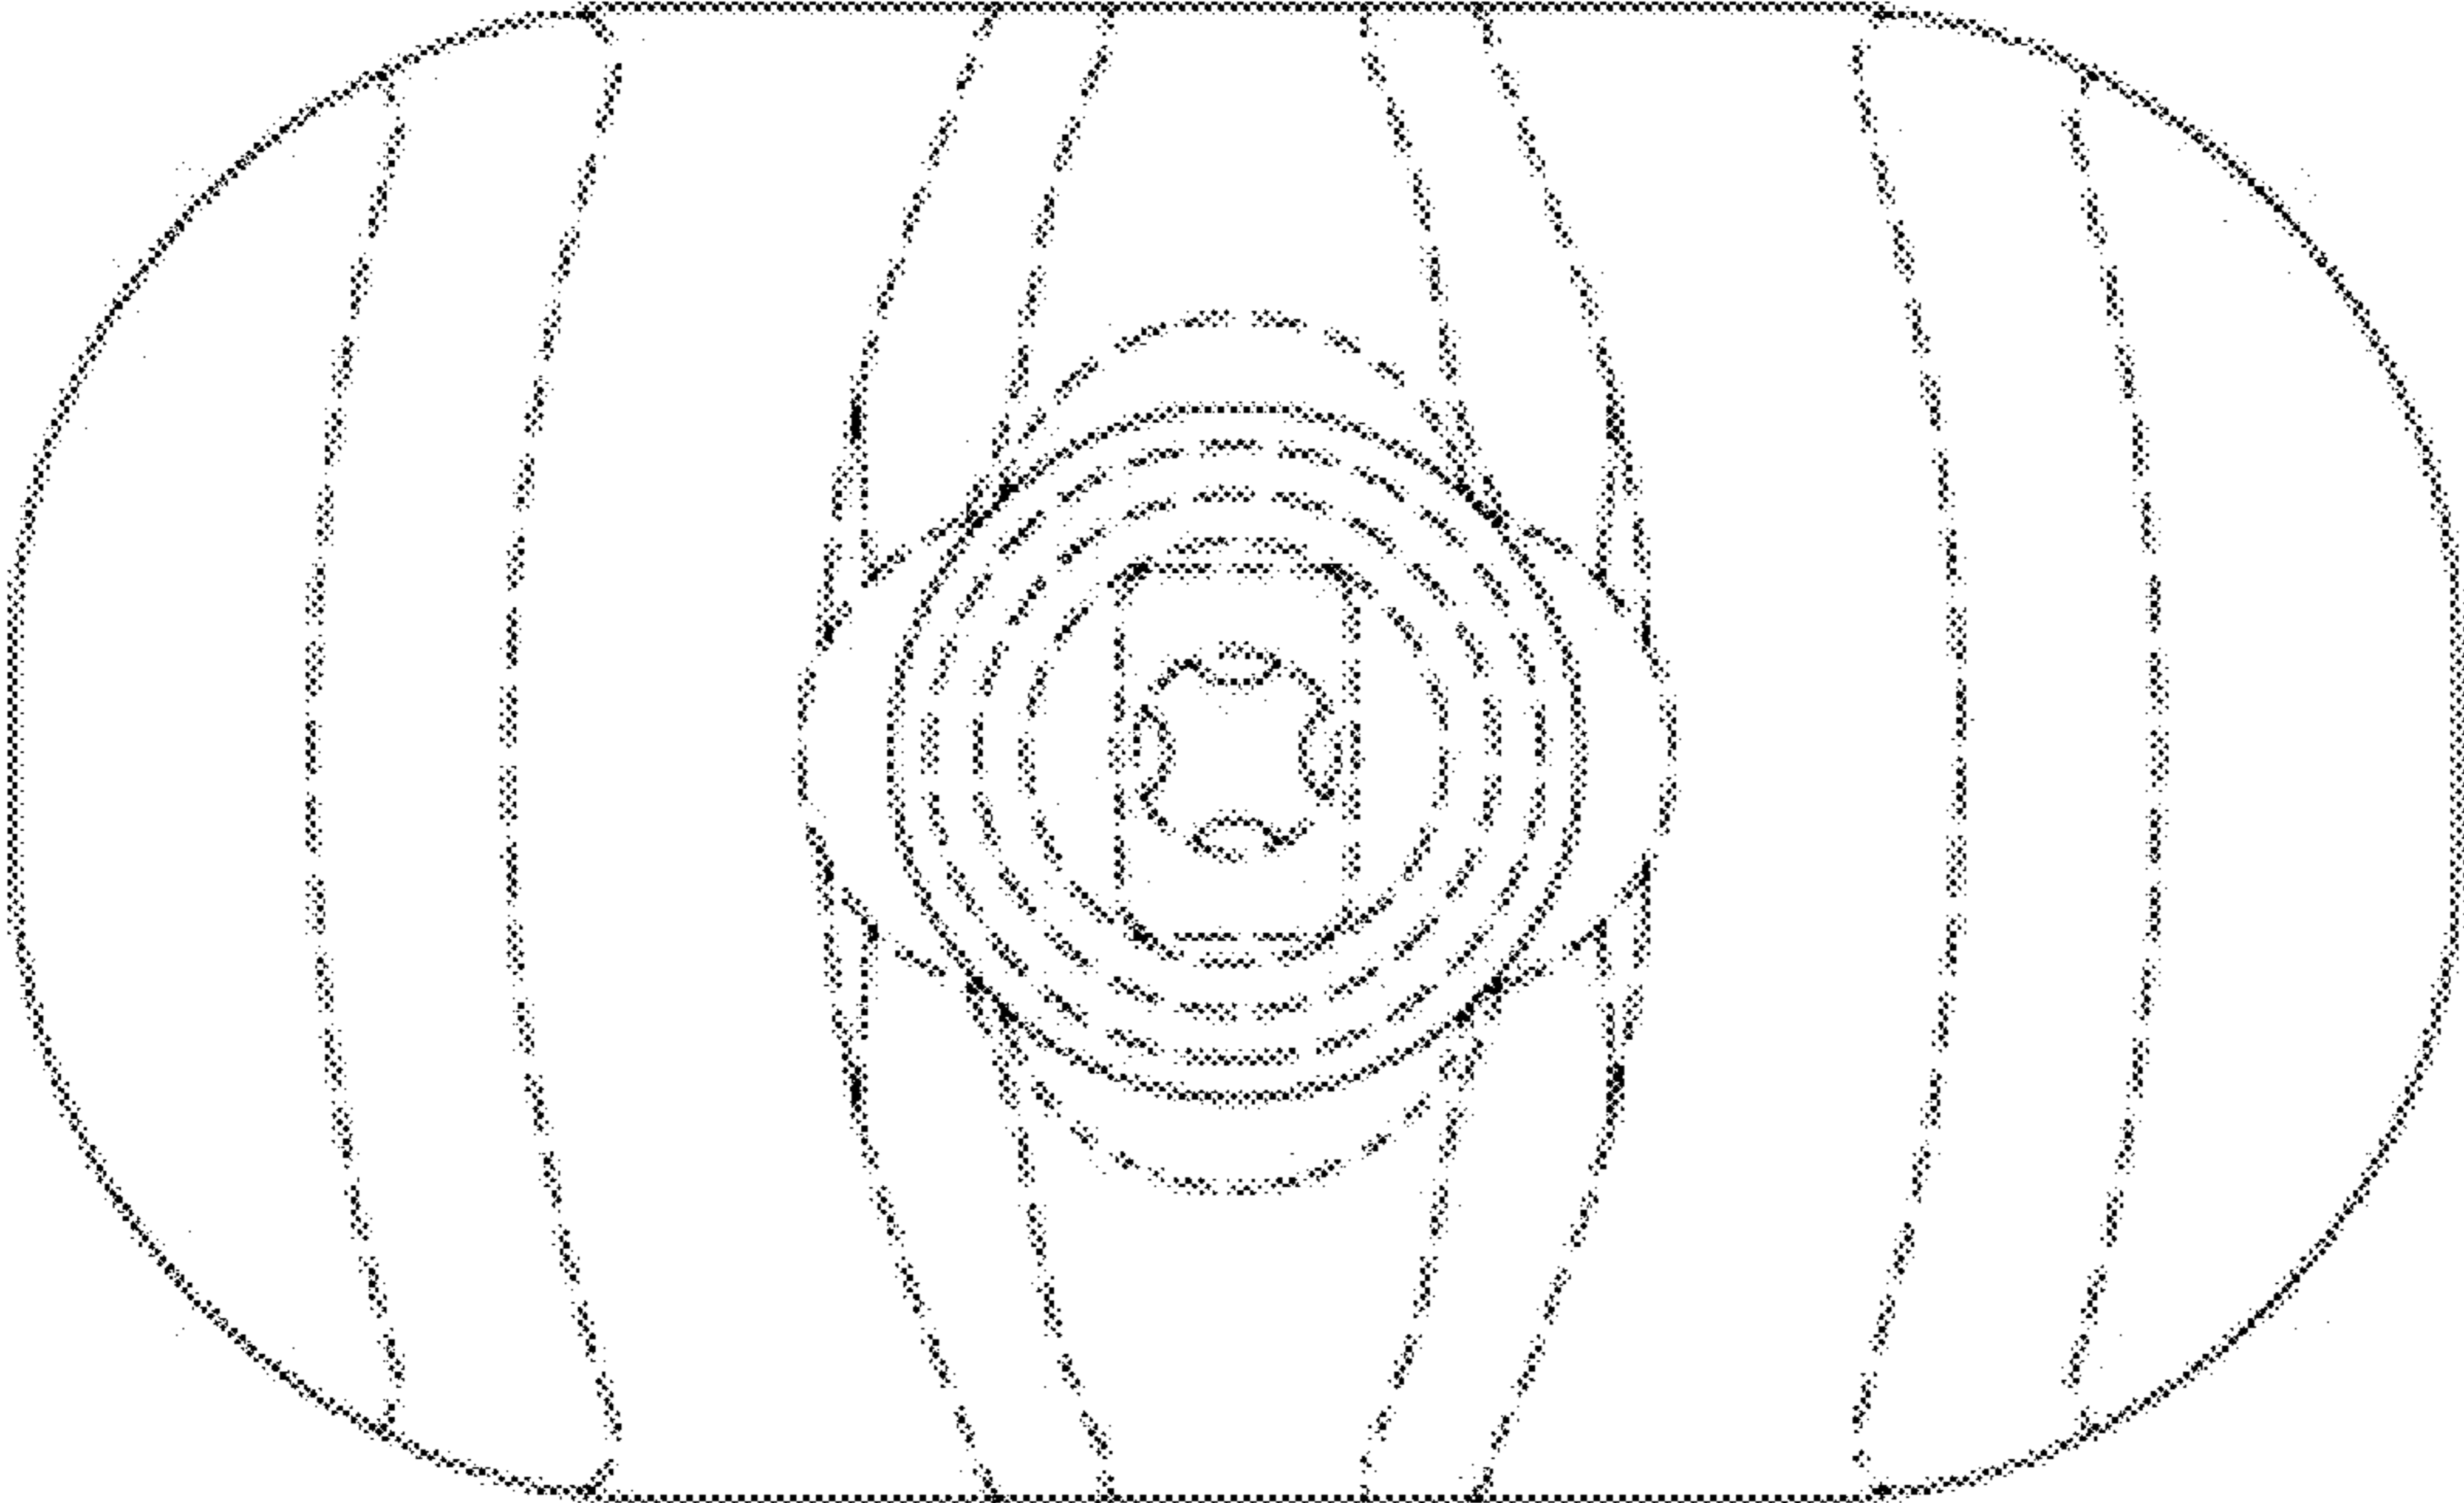


FIG. 6

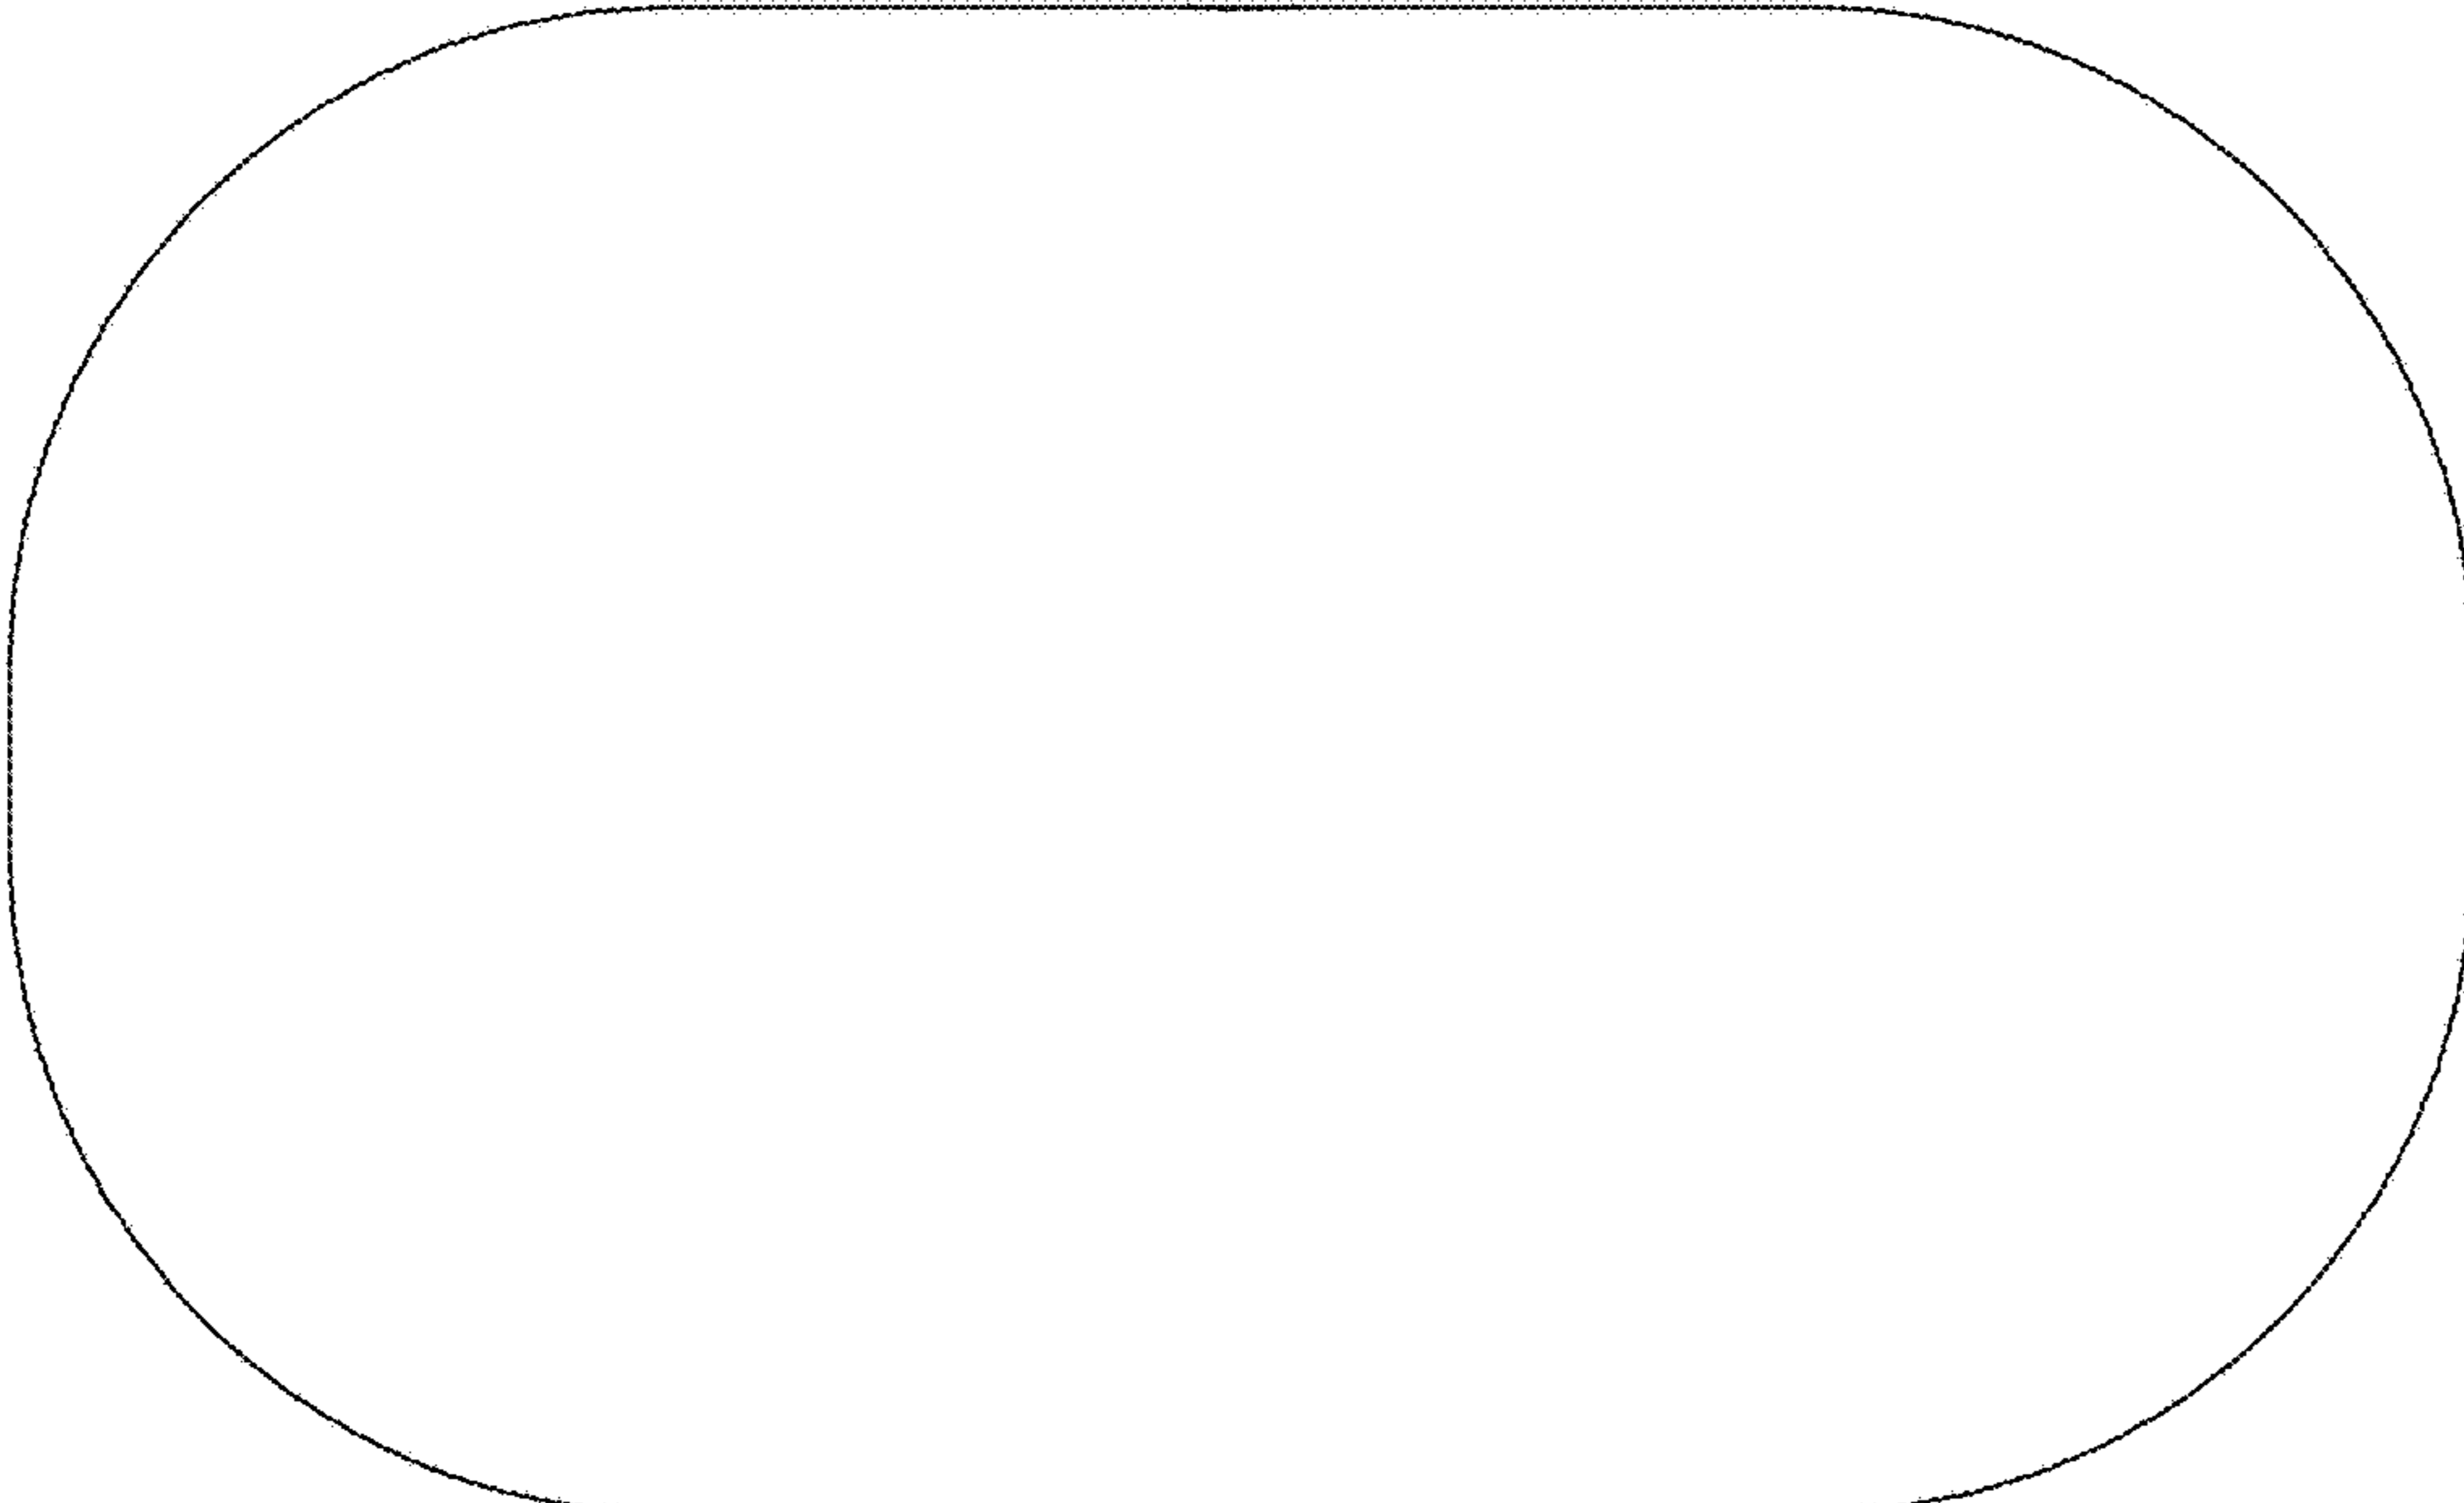


FIG. 5