



US00D938026S

(12) **United States Design Patent** (10) **Patent No.:** **US D938,026 S**  
**Pendleton et al.** (45) **Date of Patent:** **\*\* Dec. 7, 2021**

(54) **SURGICAL STRIKE PLATE HANDLE FOR IMPLANT REMOVAL**  
(71) Applicant: **Tightline Development, LLC**, Atlanta, GA (US)  
(72) Inventors: **John E. Pendleton**, Atlanta, GA (US); **Daniel H. Hursh**, Roswell, GA (US); **Benjamin M. Stronach**, Madison, MS (US)  
(73) Assignee: **TIGHTLINE DEVELOPMENT, LLC.**, Atlanta, GA (US)  
(\*\*) Term: **15 Years**

D613,144 S \* 4/2010 Lin ..... D8/107  
D646,783 S \* 10/2011 Bast ..... D24/133  
D649,635 S \* 11/2011 Cronin ..... D24/133  
D663,025 S \* 7/2012 Bast ..... D24/133  
D687,690 S \* 8/2013 Chen ..... D8/105  
D707,356 S \* 6/2014 Vonck ..... D24/133  
8,834,480 B2 9/2014 Hudak, Jr. et al.  
D715,431 S \* 10/2014 Vonck ..... D24/133  
D724,410 S \* 3/2015 Han ..... D8/307  
9,089,440 B2 7/2015 Mueller  
D771,249 S \* 11/2016 Heath ..... D24/133  
D799,302 S \* 10/2017 Bast ..... D8/107  
D803,025 S \* 11/2017 Larose ..... D8/300  
D839,066 S \* 1/2019 Bast ..... D8/14  
D845,740 S \* 4/2019 Bast ..... D8/107  
D856,513 S \* 8/2019 Taylor ..... D24/133  
2010/0288087 A1\* 11/2010 Lai ..... B25G 1/085  
81/490

(21) Appl. No.: **29/674,291**  
(22) Filed: **Dec. 20, 2018**  
(51) **LOC (13) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/133**  
(58) **Field of Classification Search**  
USPC ..... D24/133, 134, 137, 138, 172, 173, 174, D24/187, 143, 200, 145; D8/14, 21, 82, D8/83, 84, 85, 86, 107, 34; D6/540, 546, D6/554, 556  
CPC ..... A61B 17/64; A61B 17/62; A61B 17/00; A61B 7/70; A61B 7/02; A61B 7/003; A61B 7/04; H04R 1/46  
See application file for complete search history.

(Continued)

*Primary Examiner* — Manpreet S Matharu  
*Assistant Examiner* — Yolanda Robinson  
(74) *Attorney, Agent, or Firm* — Fisherbroyles, LLP; Anthony J DeVale

(57) **CLAIM**


The ornamental design for a surgical strike plate handle for implant removal, as shown and described.

**DESCRIPTION**

FIG. 1 is a front side view of a strike plate handle for implant removal showing our new design; FIG. 2 is a back side view thereof; FIG. 3 is a left, side view thereof; FIG. 4 is a right, side view thereof; FIG. 5 is a top plan view thereof; and, FIG. 6 is a bottom plan view thereof. The broken lines shown in the surgical strike plate handle for implant removal are for portions that form no part of the claimed design.

(56) **References Cited**  
U.S. PATENT DOCUMENTS  
6,151,998 A \* 11/2000 Fu-Hui ..... B25G 1/085  
81/177.1  
6,565,575 B2 5/2003 Lewis  
7,272,999 B2\* 9/2007 Cutler ..... B25B 15/02  
81/467  
D557,584 S \* 12/2007 Gao ..... D8/107

**1 Claim, 3 Drawing Sheets**

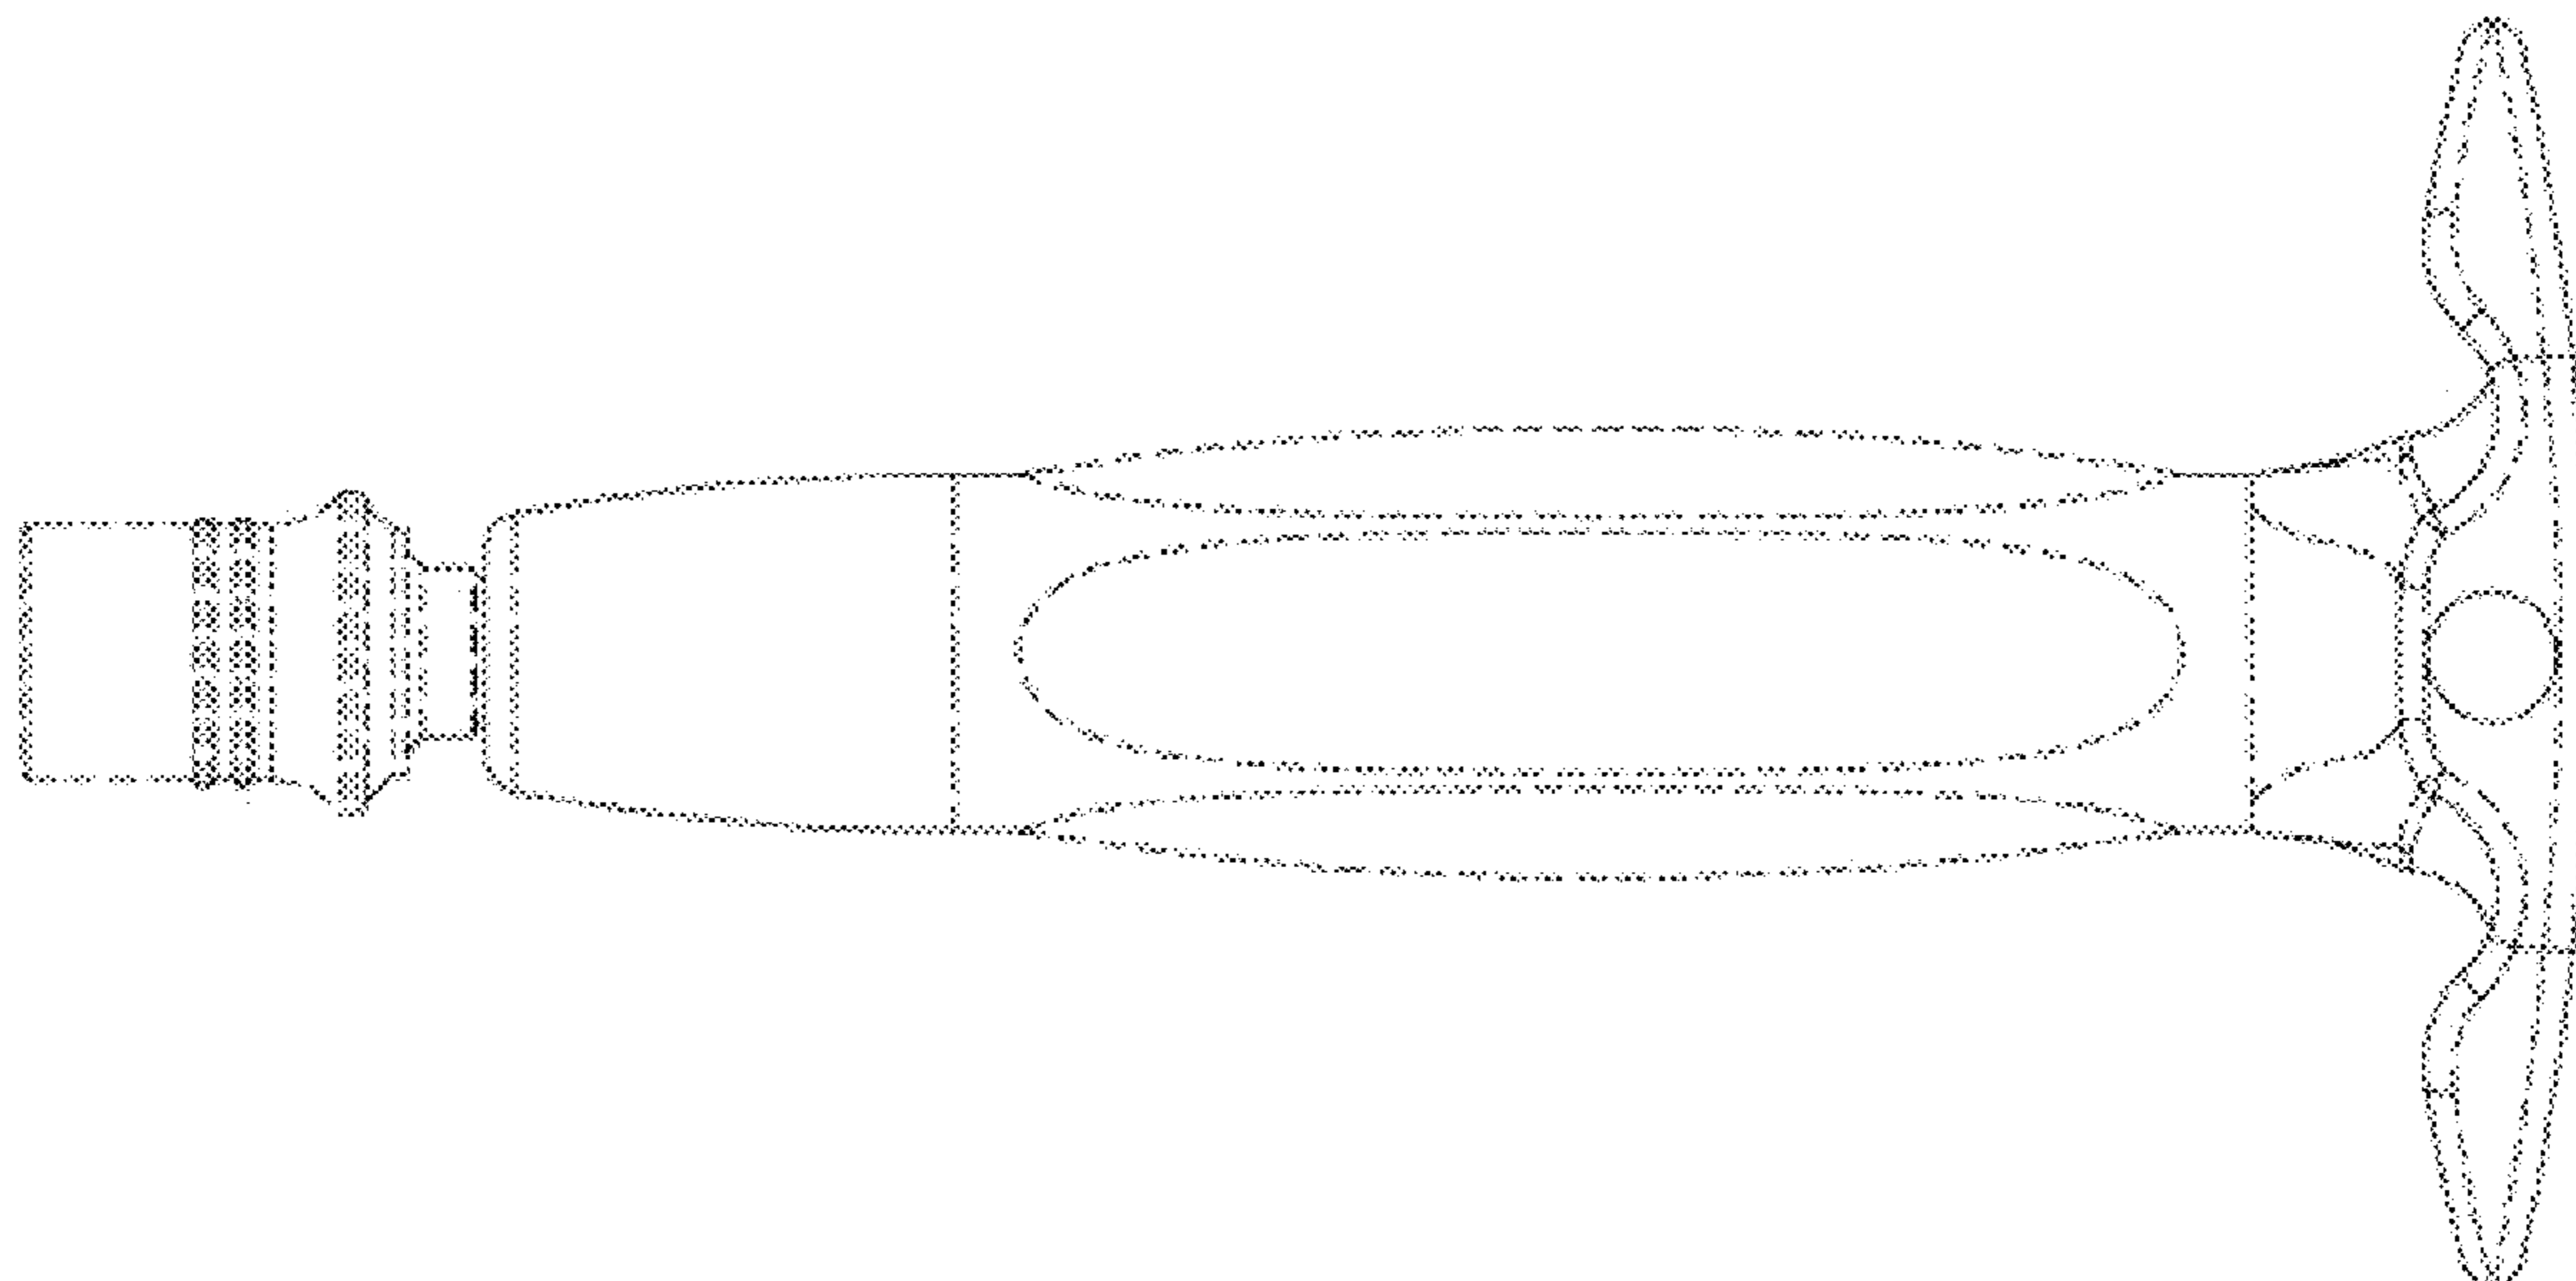

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2016/0100957 A1 4/2016 Lewis  
2018/0206859 A1 7/2018 Pendleton et al.

\* cited by examiner

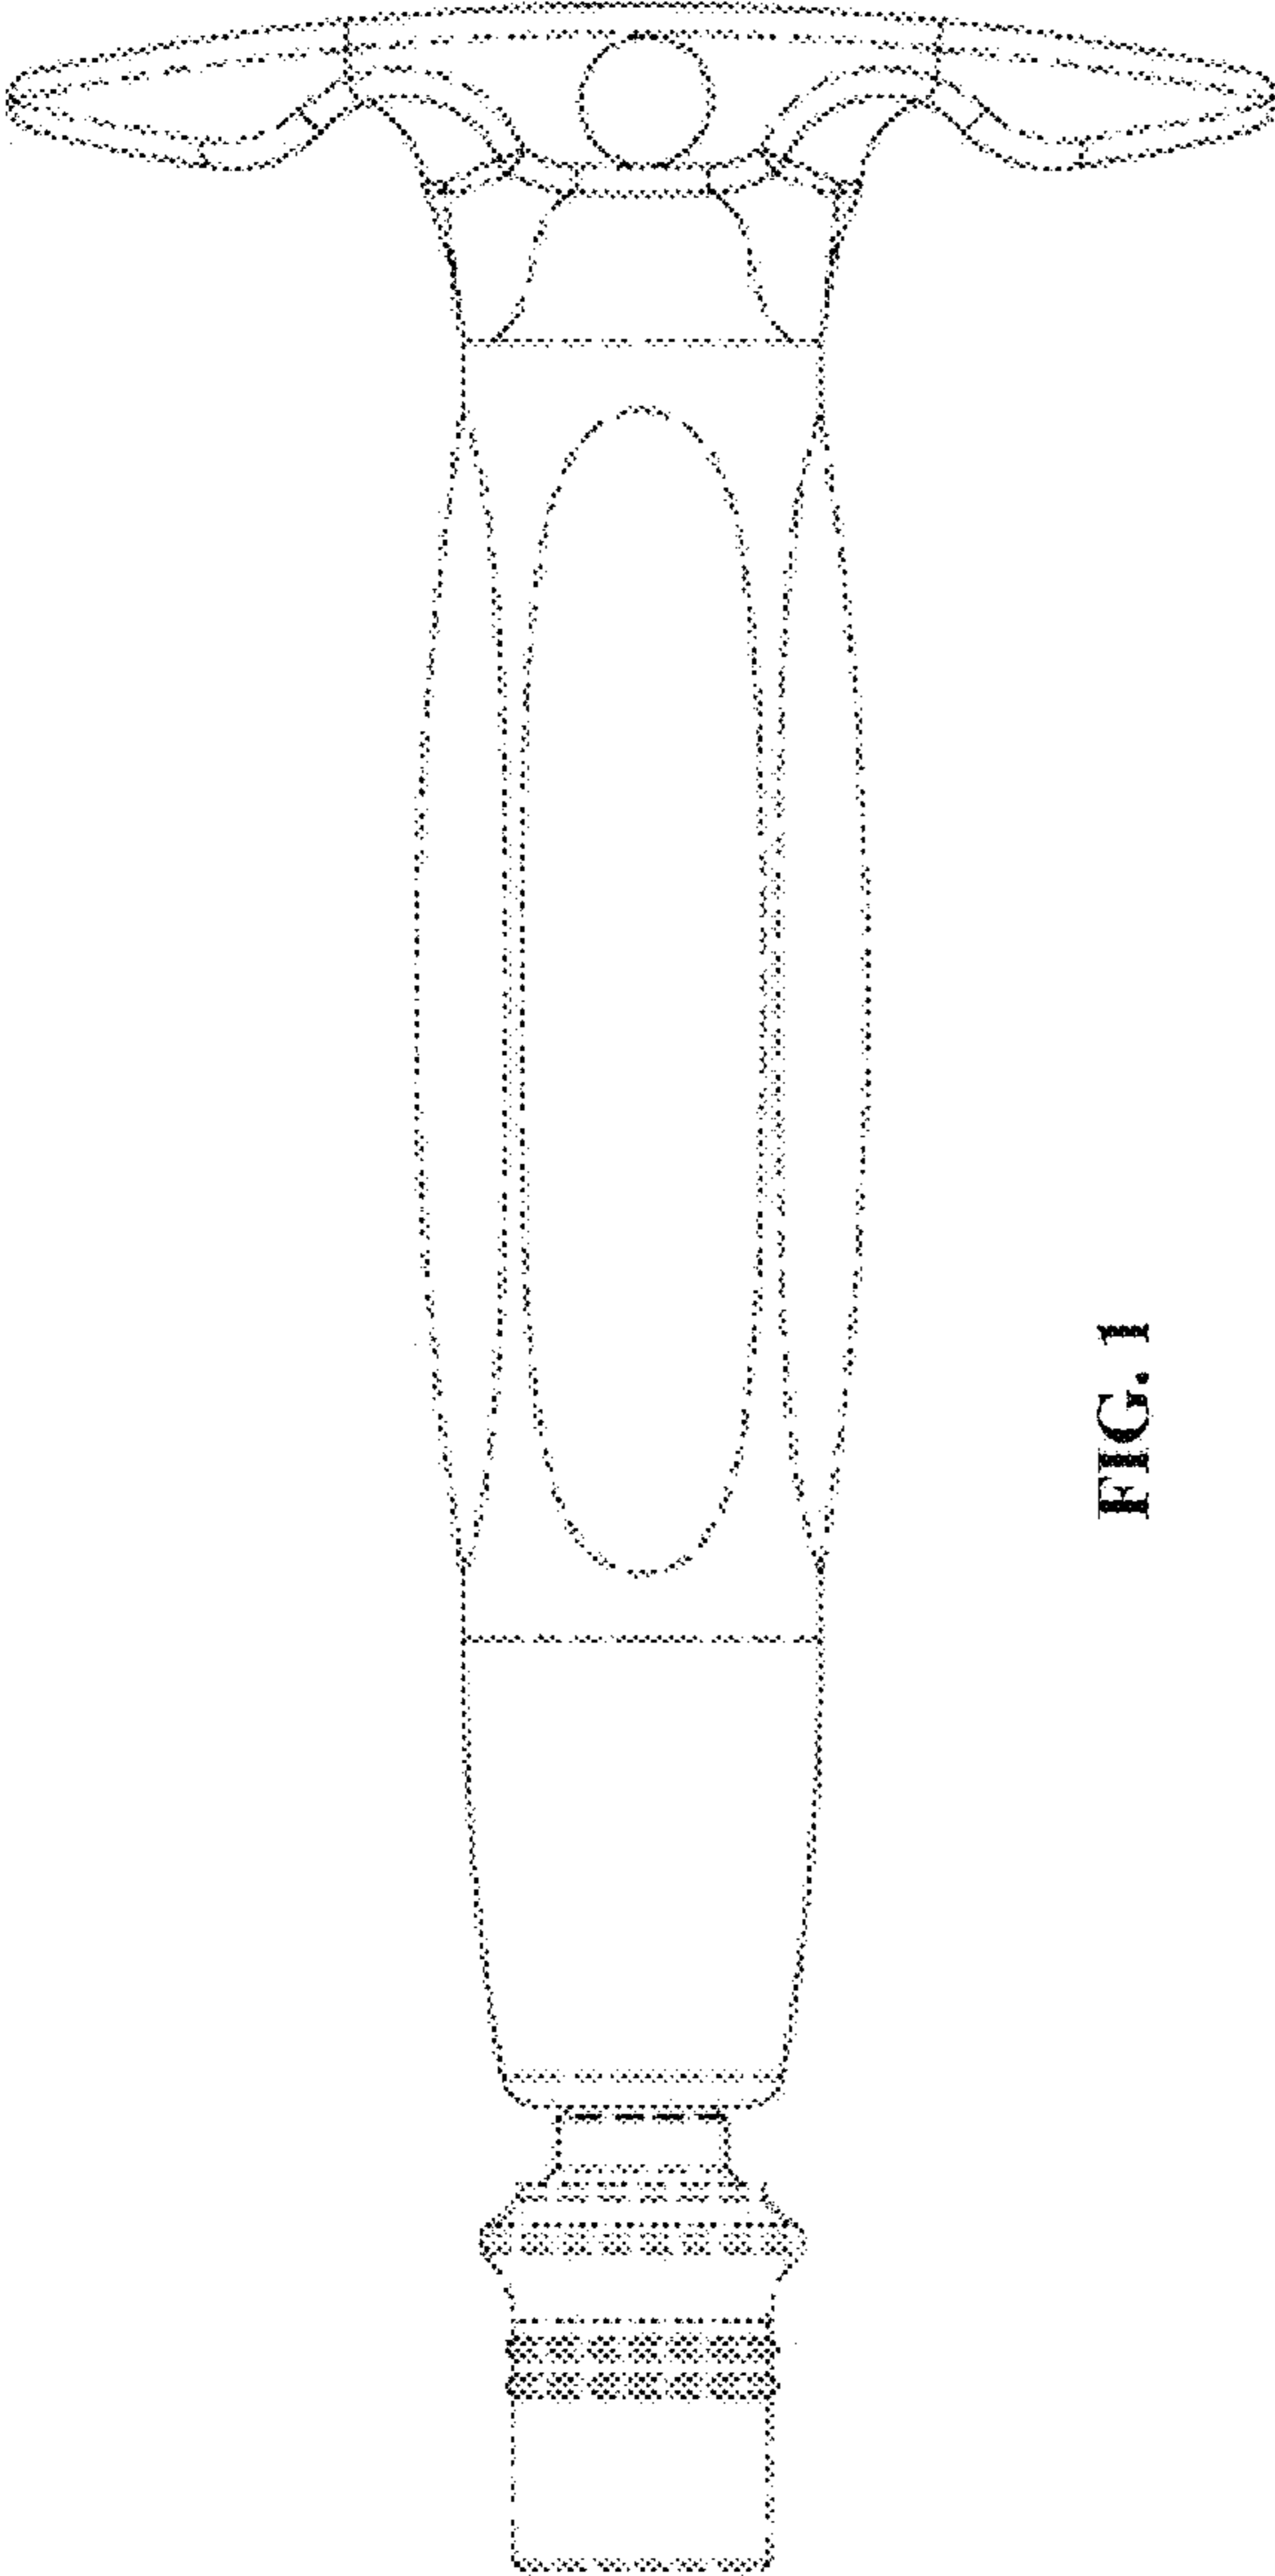


FIG. 1

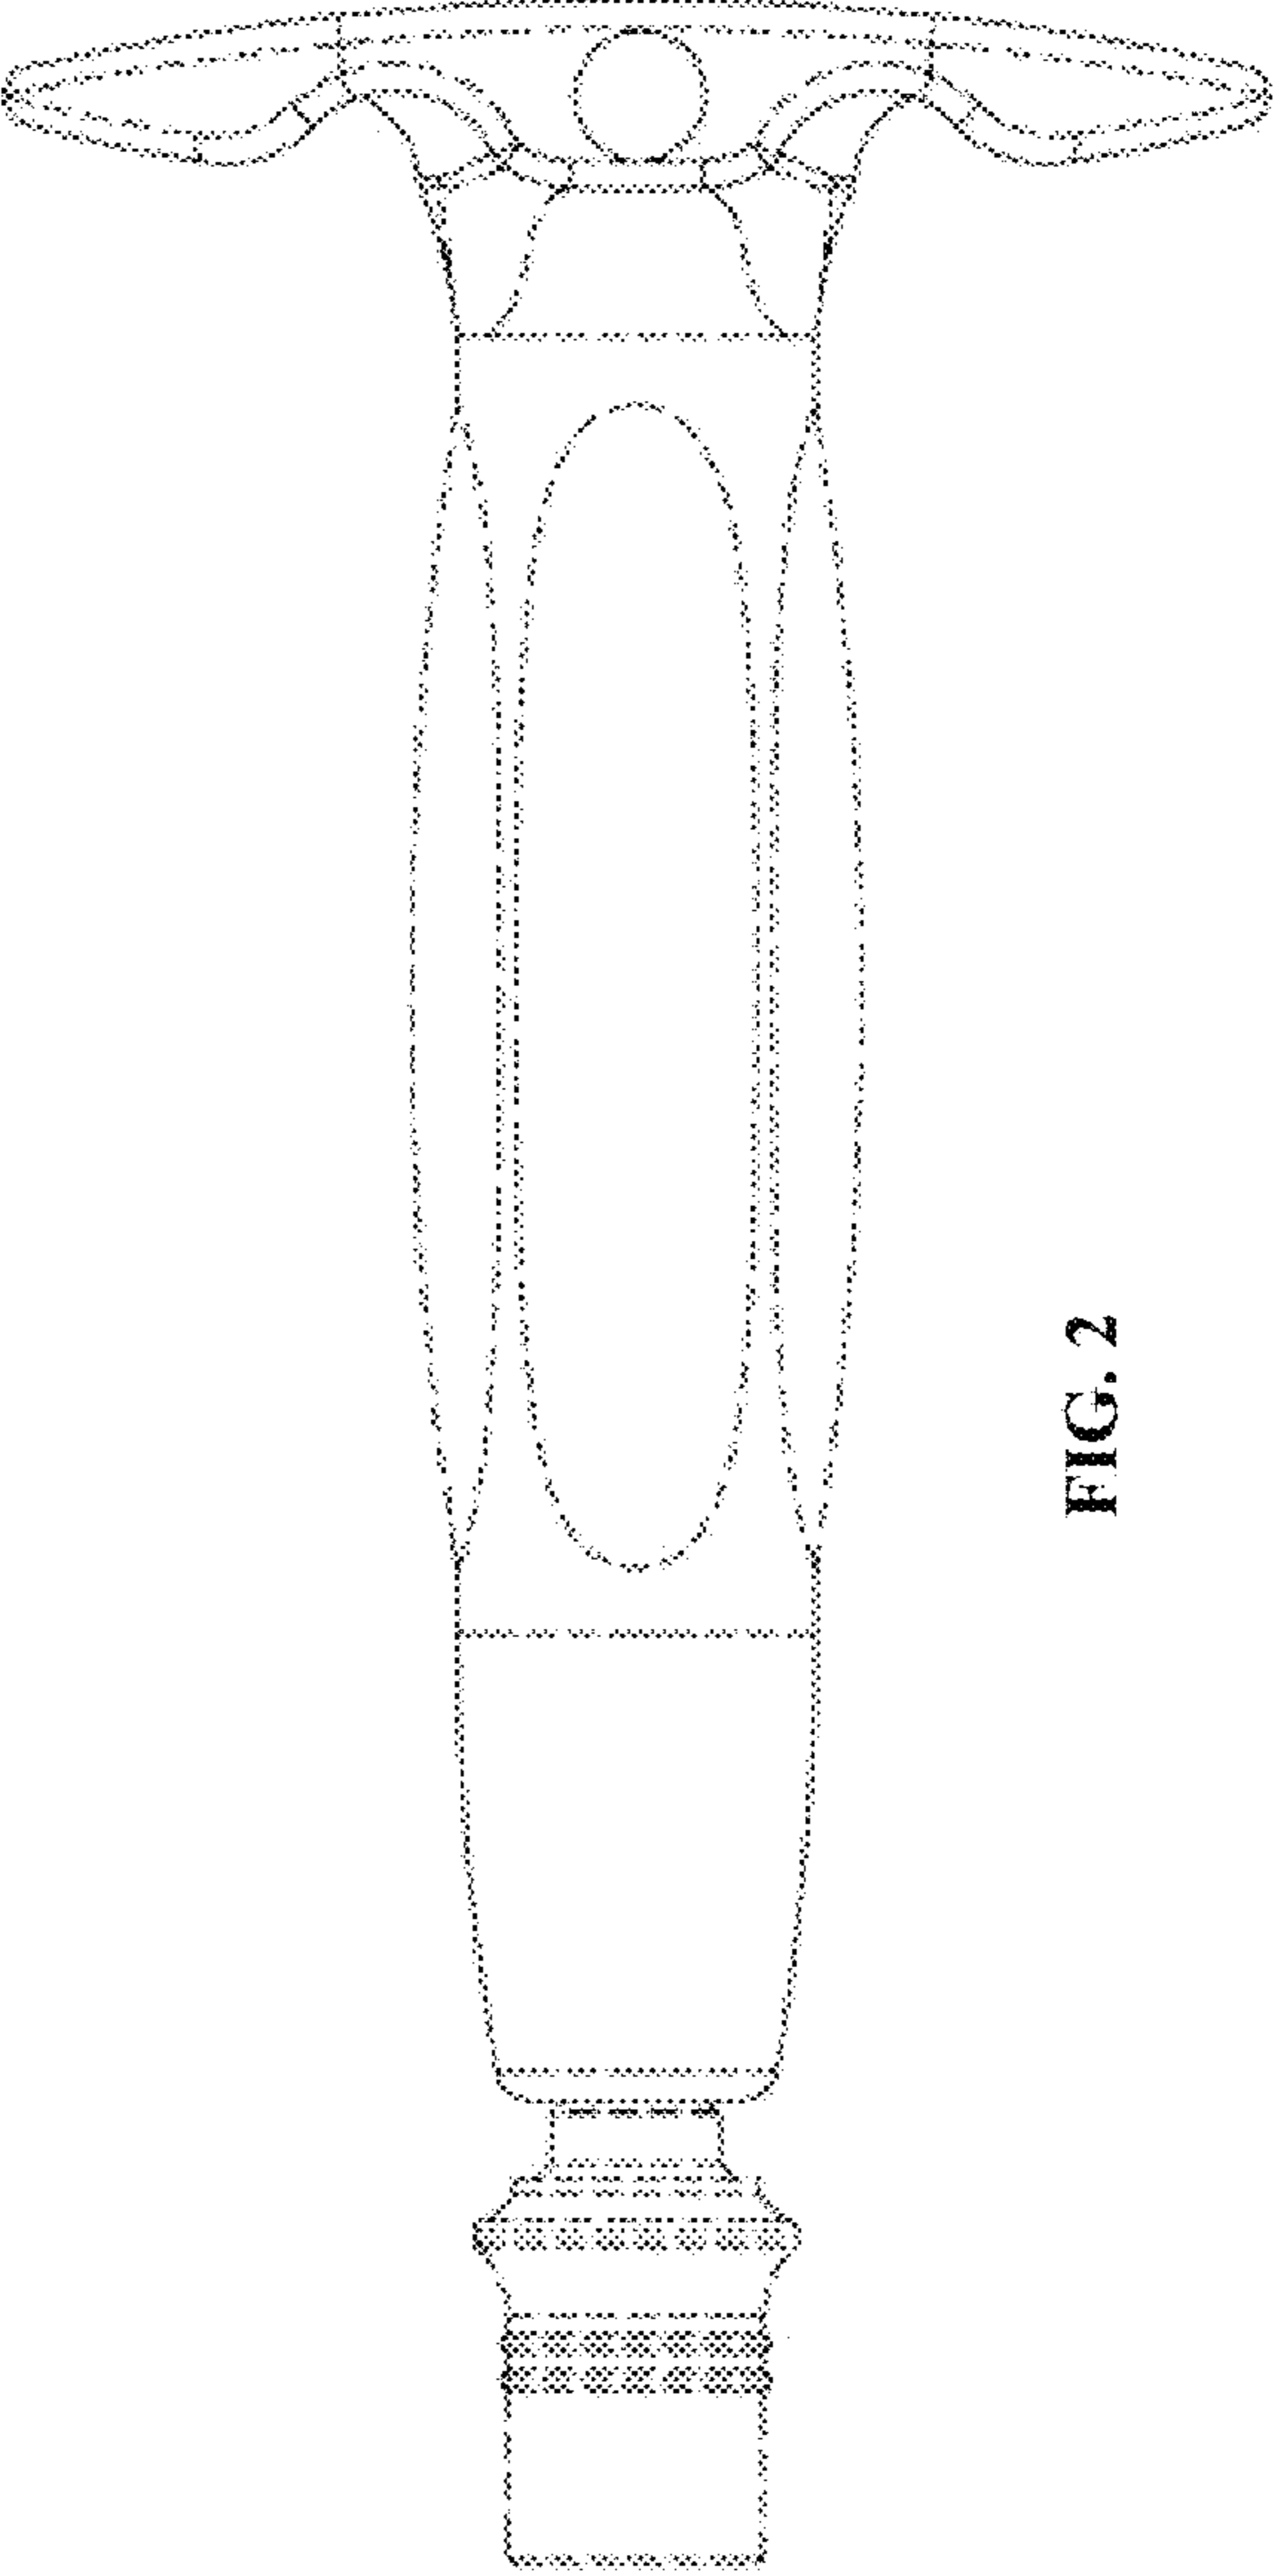


FIG. 2

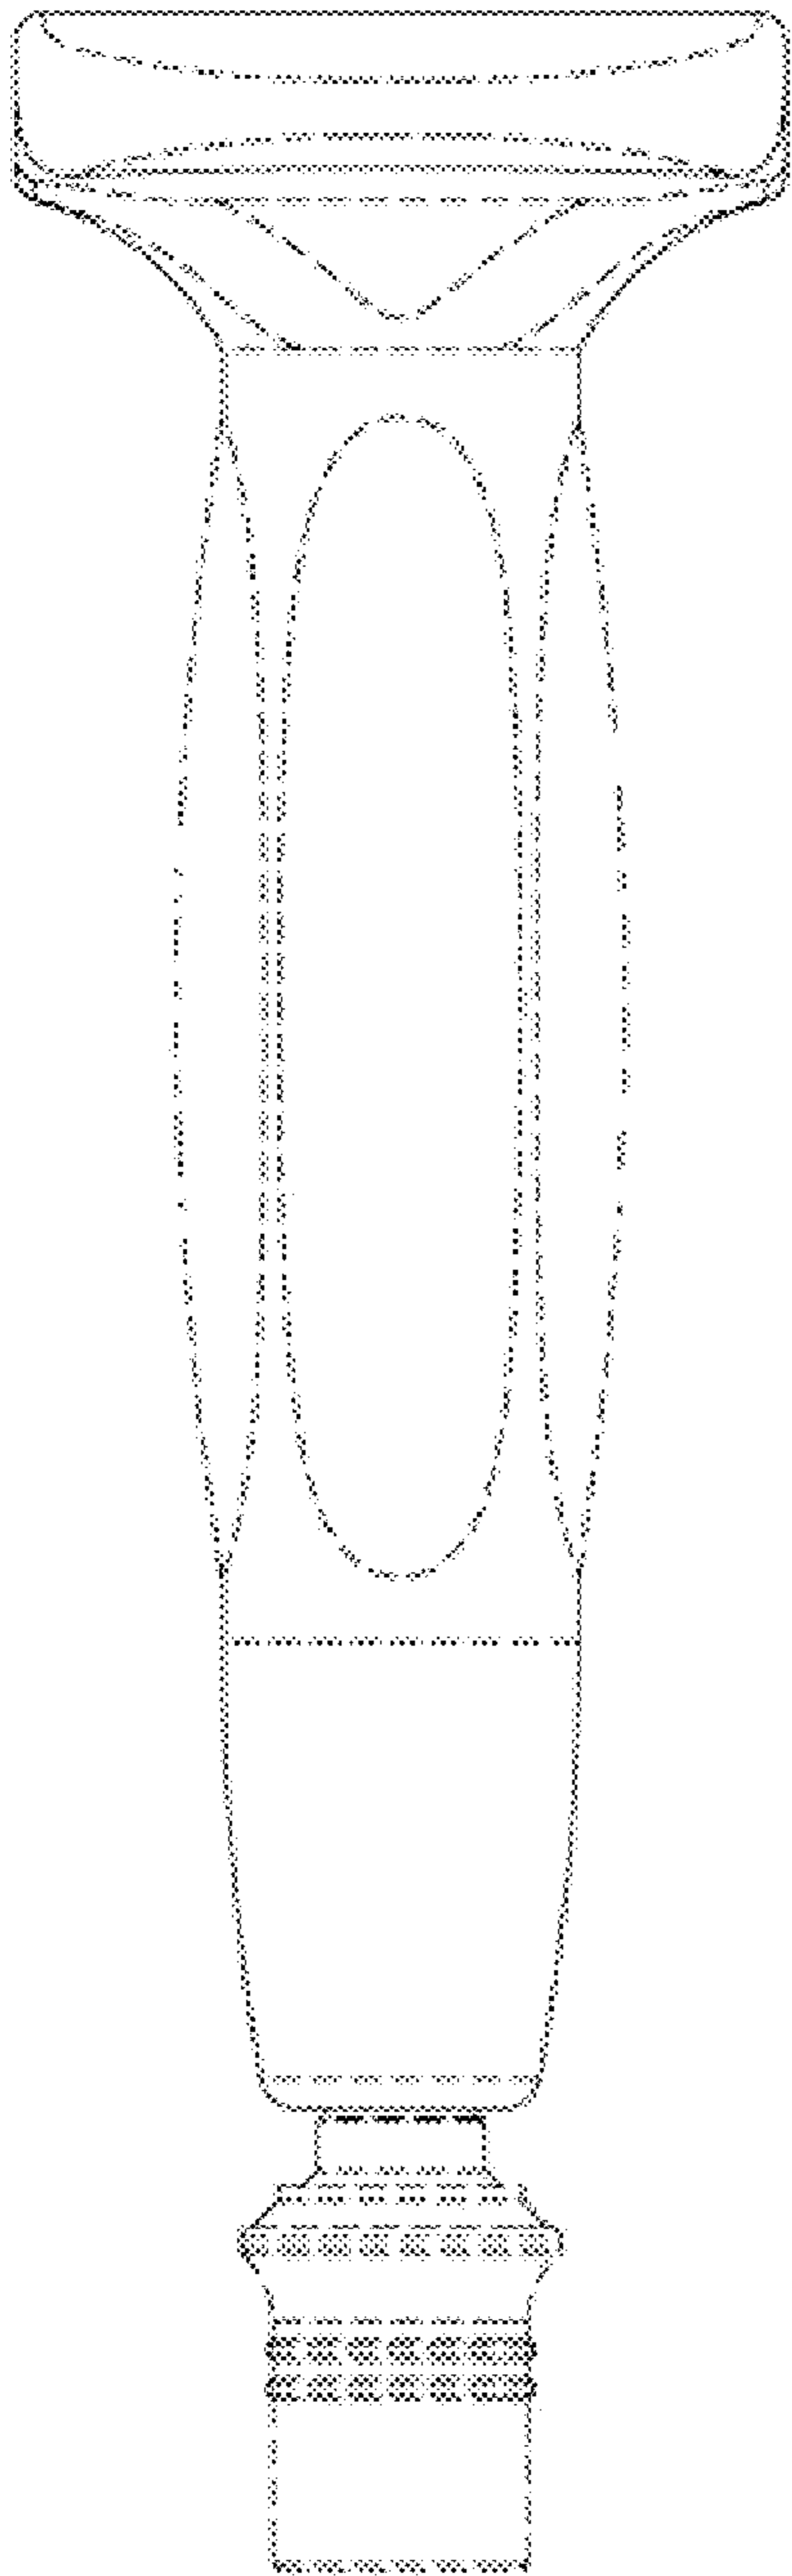


FIG. 3

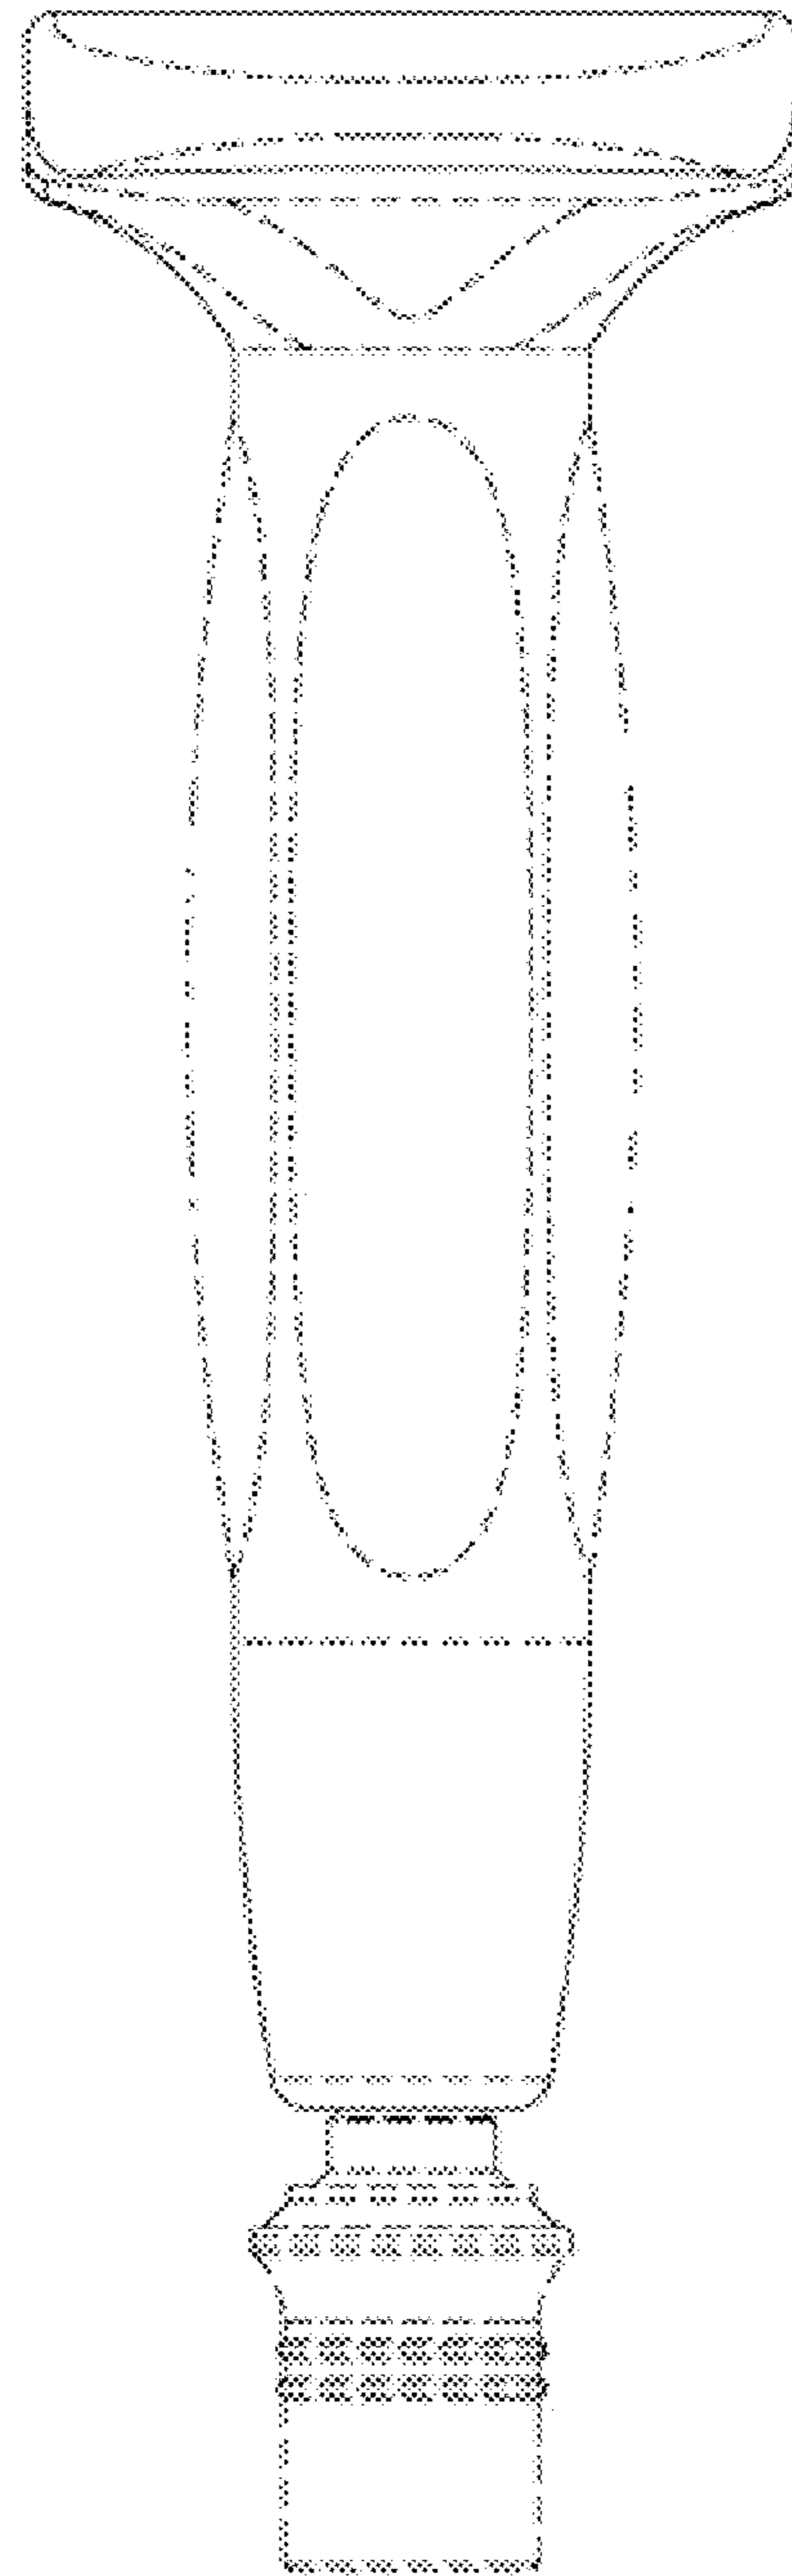


FIG. 4

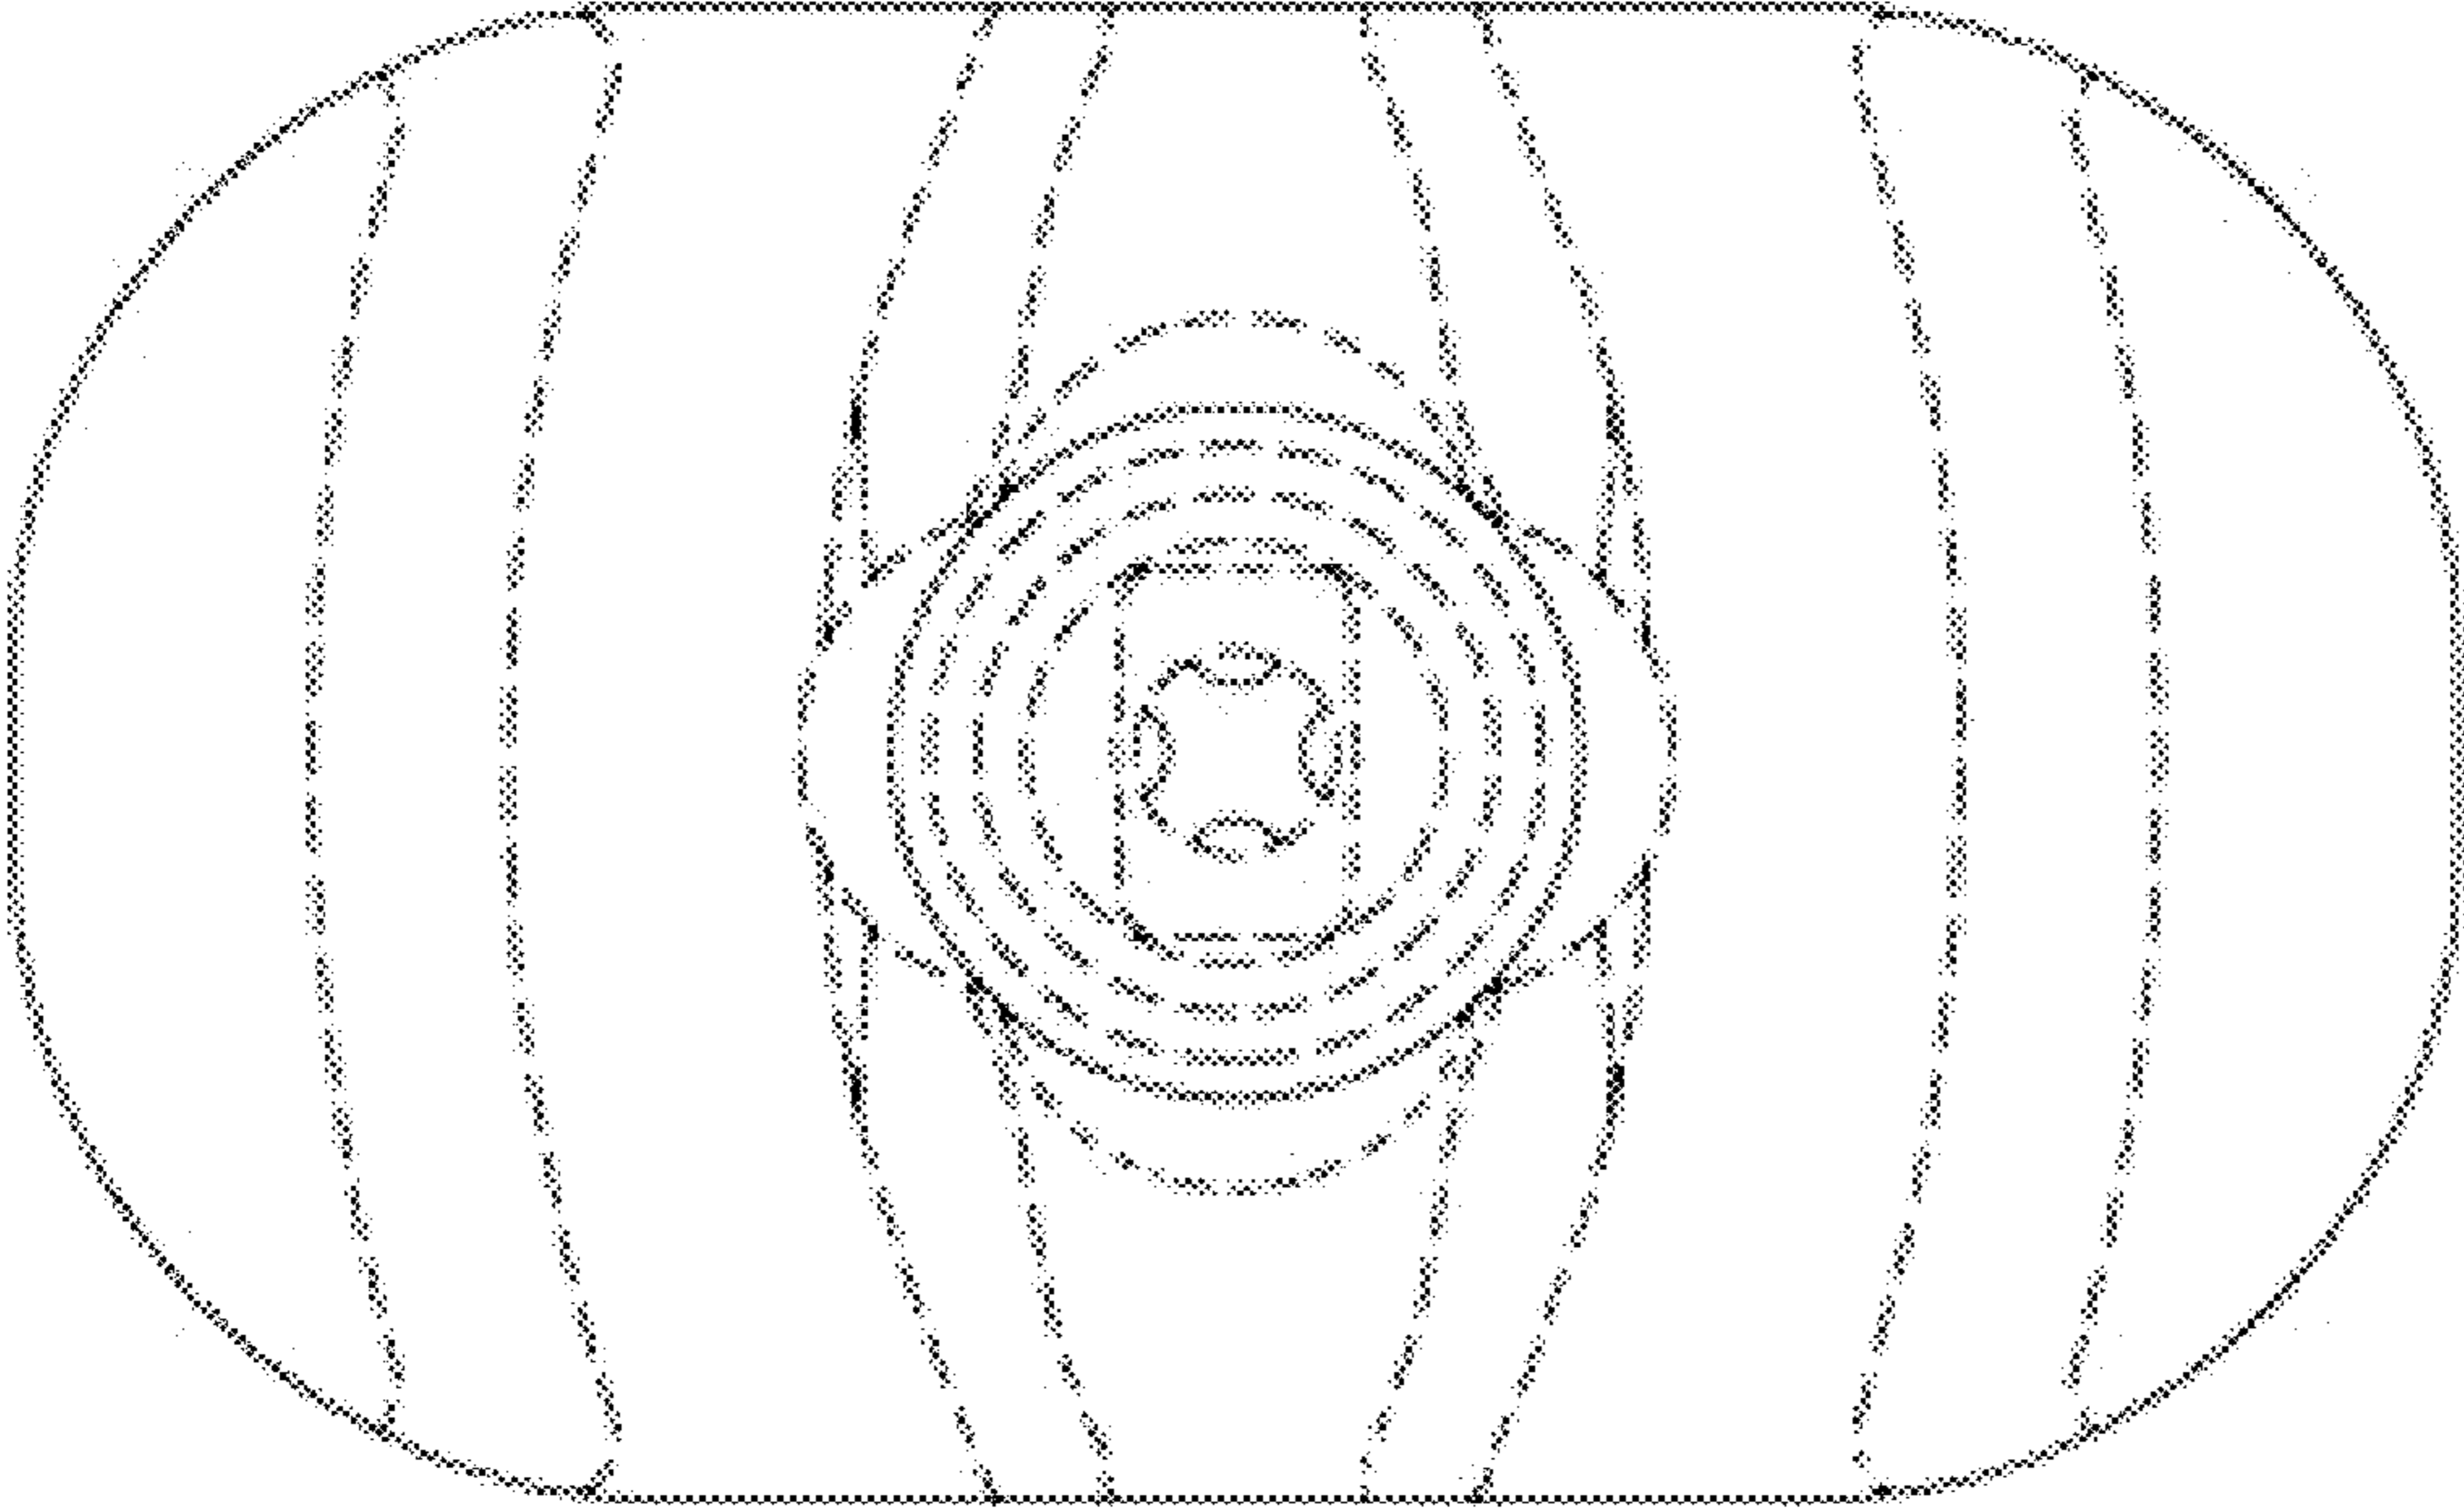


FIG. 6

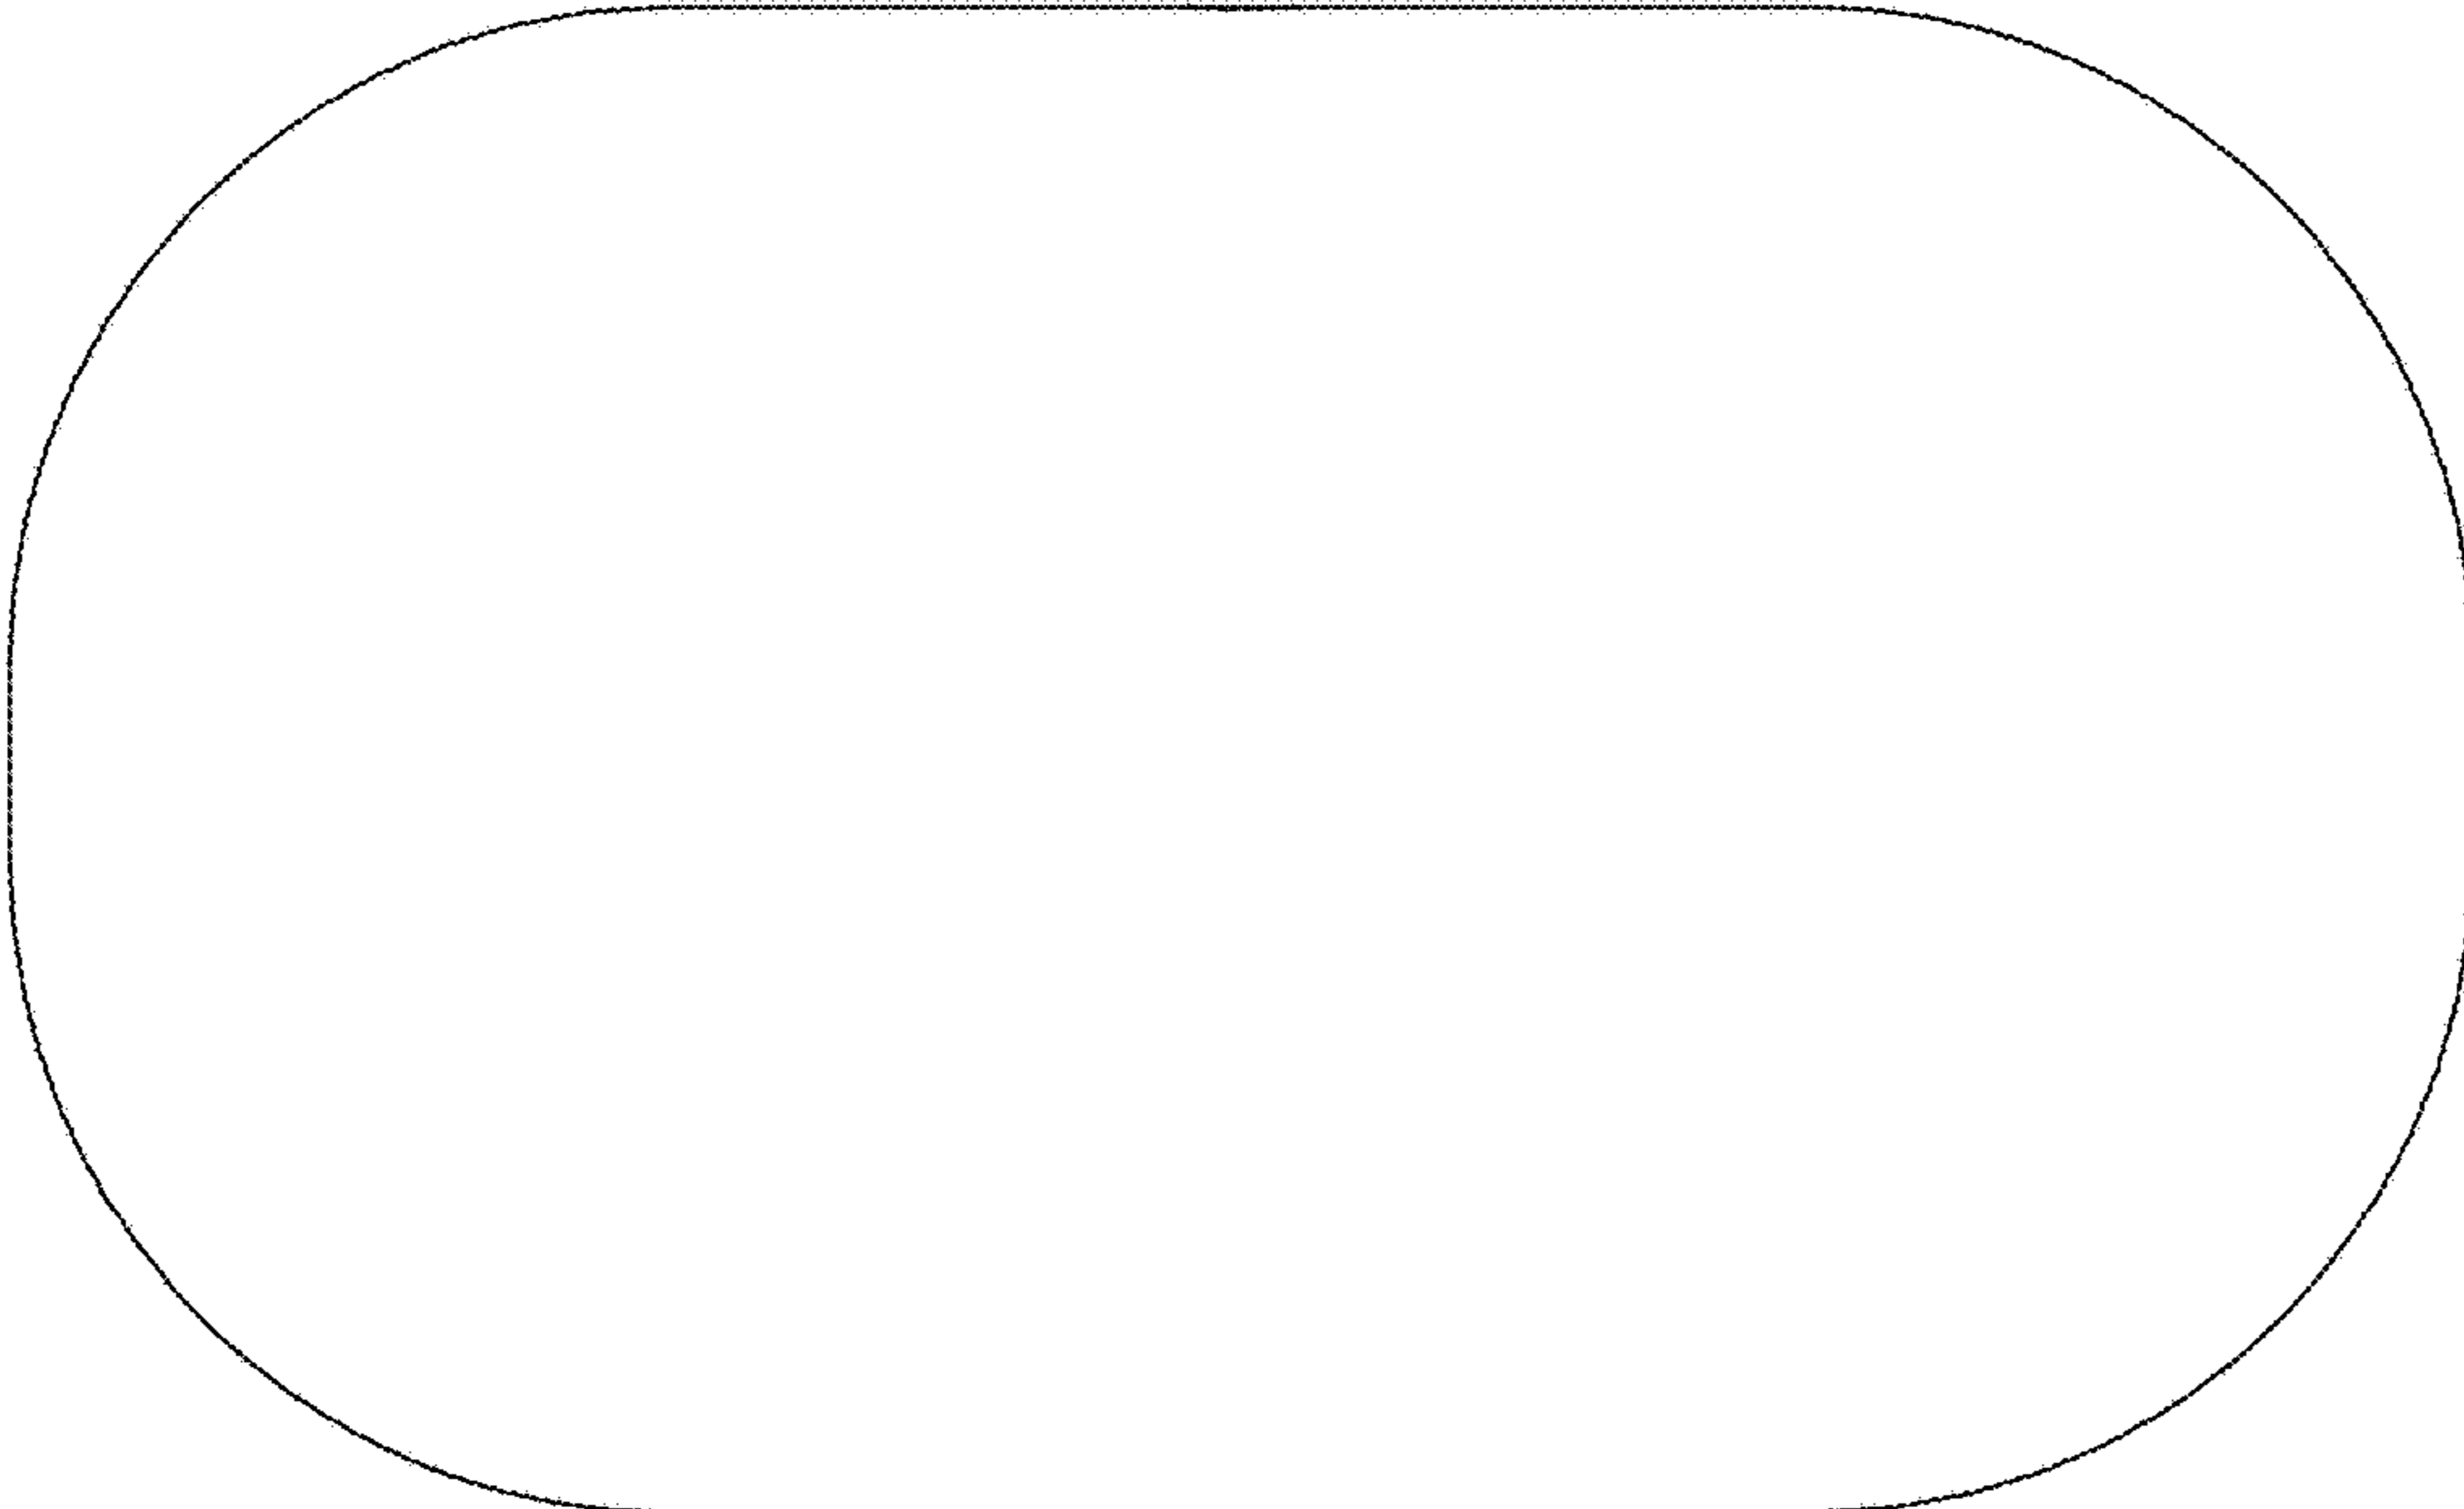


FIG. 5