



US00D938047S

(12) **United States Design Patent** (10) **Patent No.:** **US D938,047 S**
Denis (45) **Date of Patent:** **** Dec. 7, 2021**

(54) **DIAGNOSTIC INSTRUMENT**

(71) Applicant: **AMINOGRAM**, La Ciotat (FR)

(72) Inventor: **Eric Denis**, Lyons (FR)

(73) Assignee: **AMINOGRAM**, La Ciotat (FR)

(**) Term: **15 Years**

(21) Appl. No.: **29/744,032**

(22) Filed: **Jul. 27, 2020**

(30) **Foreign Application Priority Data**

Jan. 27, 2020 (EM) 007561675

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search**
USPC D24/107, 165–169, 186, 187, 231, 232,
D24/128, 133; D10/79
CPC ... A61B 5/0064; A61B 5/0066; A61B 5/0205;
A61B 5/0053; A61B 5/015; A61B
2560/0431; A61B 2562/0247; A61B
8/485

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D463,546 S * 9/2002 Jansen D24/128
D604,855 S * 11/2009 Shearlaw D24/186
D767,770 S * 9/2016 Purfey D24/186
D782,684 S * 3/2017 Pippel D24/186
D783,838 S * 4/2017 Zhao D24/186
D815,292 S * 4/2018 Goldman D24/186
D870,294 S * 12/2019 Bechtel D24/186

D903,880 S * 12/2020 Roy D24/187
D916,294 S * 4/2021 Murray D24/186
2009/0270728 A1 * 10/2009 Da Silva A61B 8/0858
600/437
2015/0320385 A1 * 11/2015 Wright A61B 8/485
600/474

FOREIGN PATENT DOCUMENTS

EM 002856500-0001 * 11/2015

OTHER PUBLICATIONS

TriaMedical Inc. Aminogram—the BIODY XPERT ZM released in 2014. Retrieved on Sep. 3, 2021 from website: <https://www.triamedical.ca/en/aminogram/>.*

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Oliff PLC


(57) **CLAIM**

The ornamental design for a diagnostic instrument, as shown and described.

DESCRIPTION

FIG. 1 is a rear, right-side, top perspective view of the diagnostic instrument, showing the new design;
FIG. 2 is a top plan view thereof;
FIG. 3 is a bottom plan view thereof;
FIG. 4 is a right-side elevational view thereof;
FIG. 5 is a left-side elevational view thereof;
FIG. 6 is a front, right-side, top perspective view thereof;
and,
FIG. 7 is a front, bottom, right-side perspective view thereof.
The broken lines depict parts of the diagnostic instrument that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

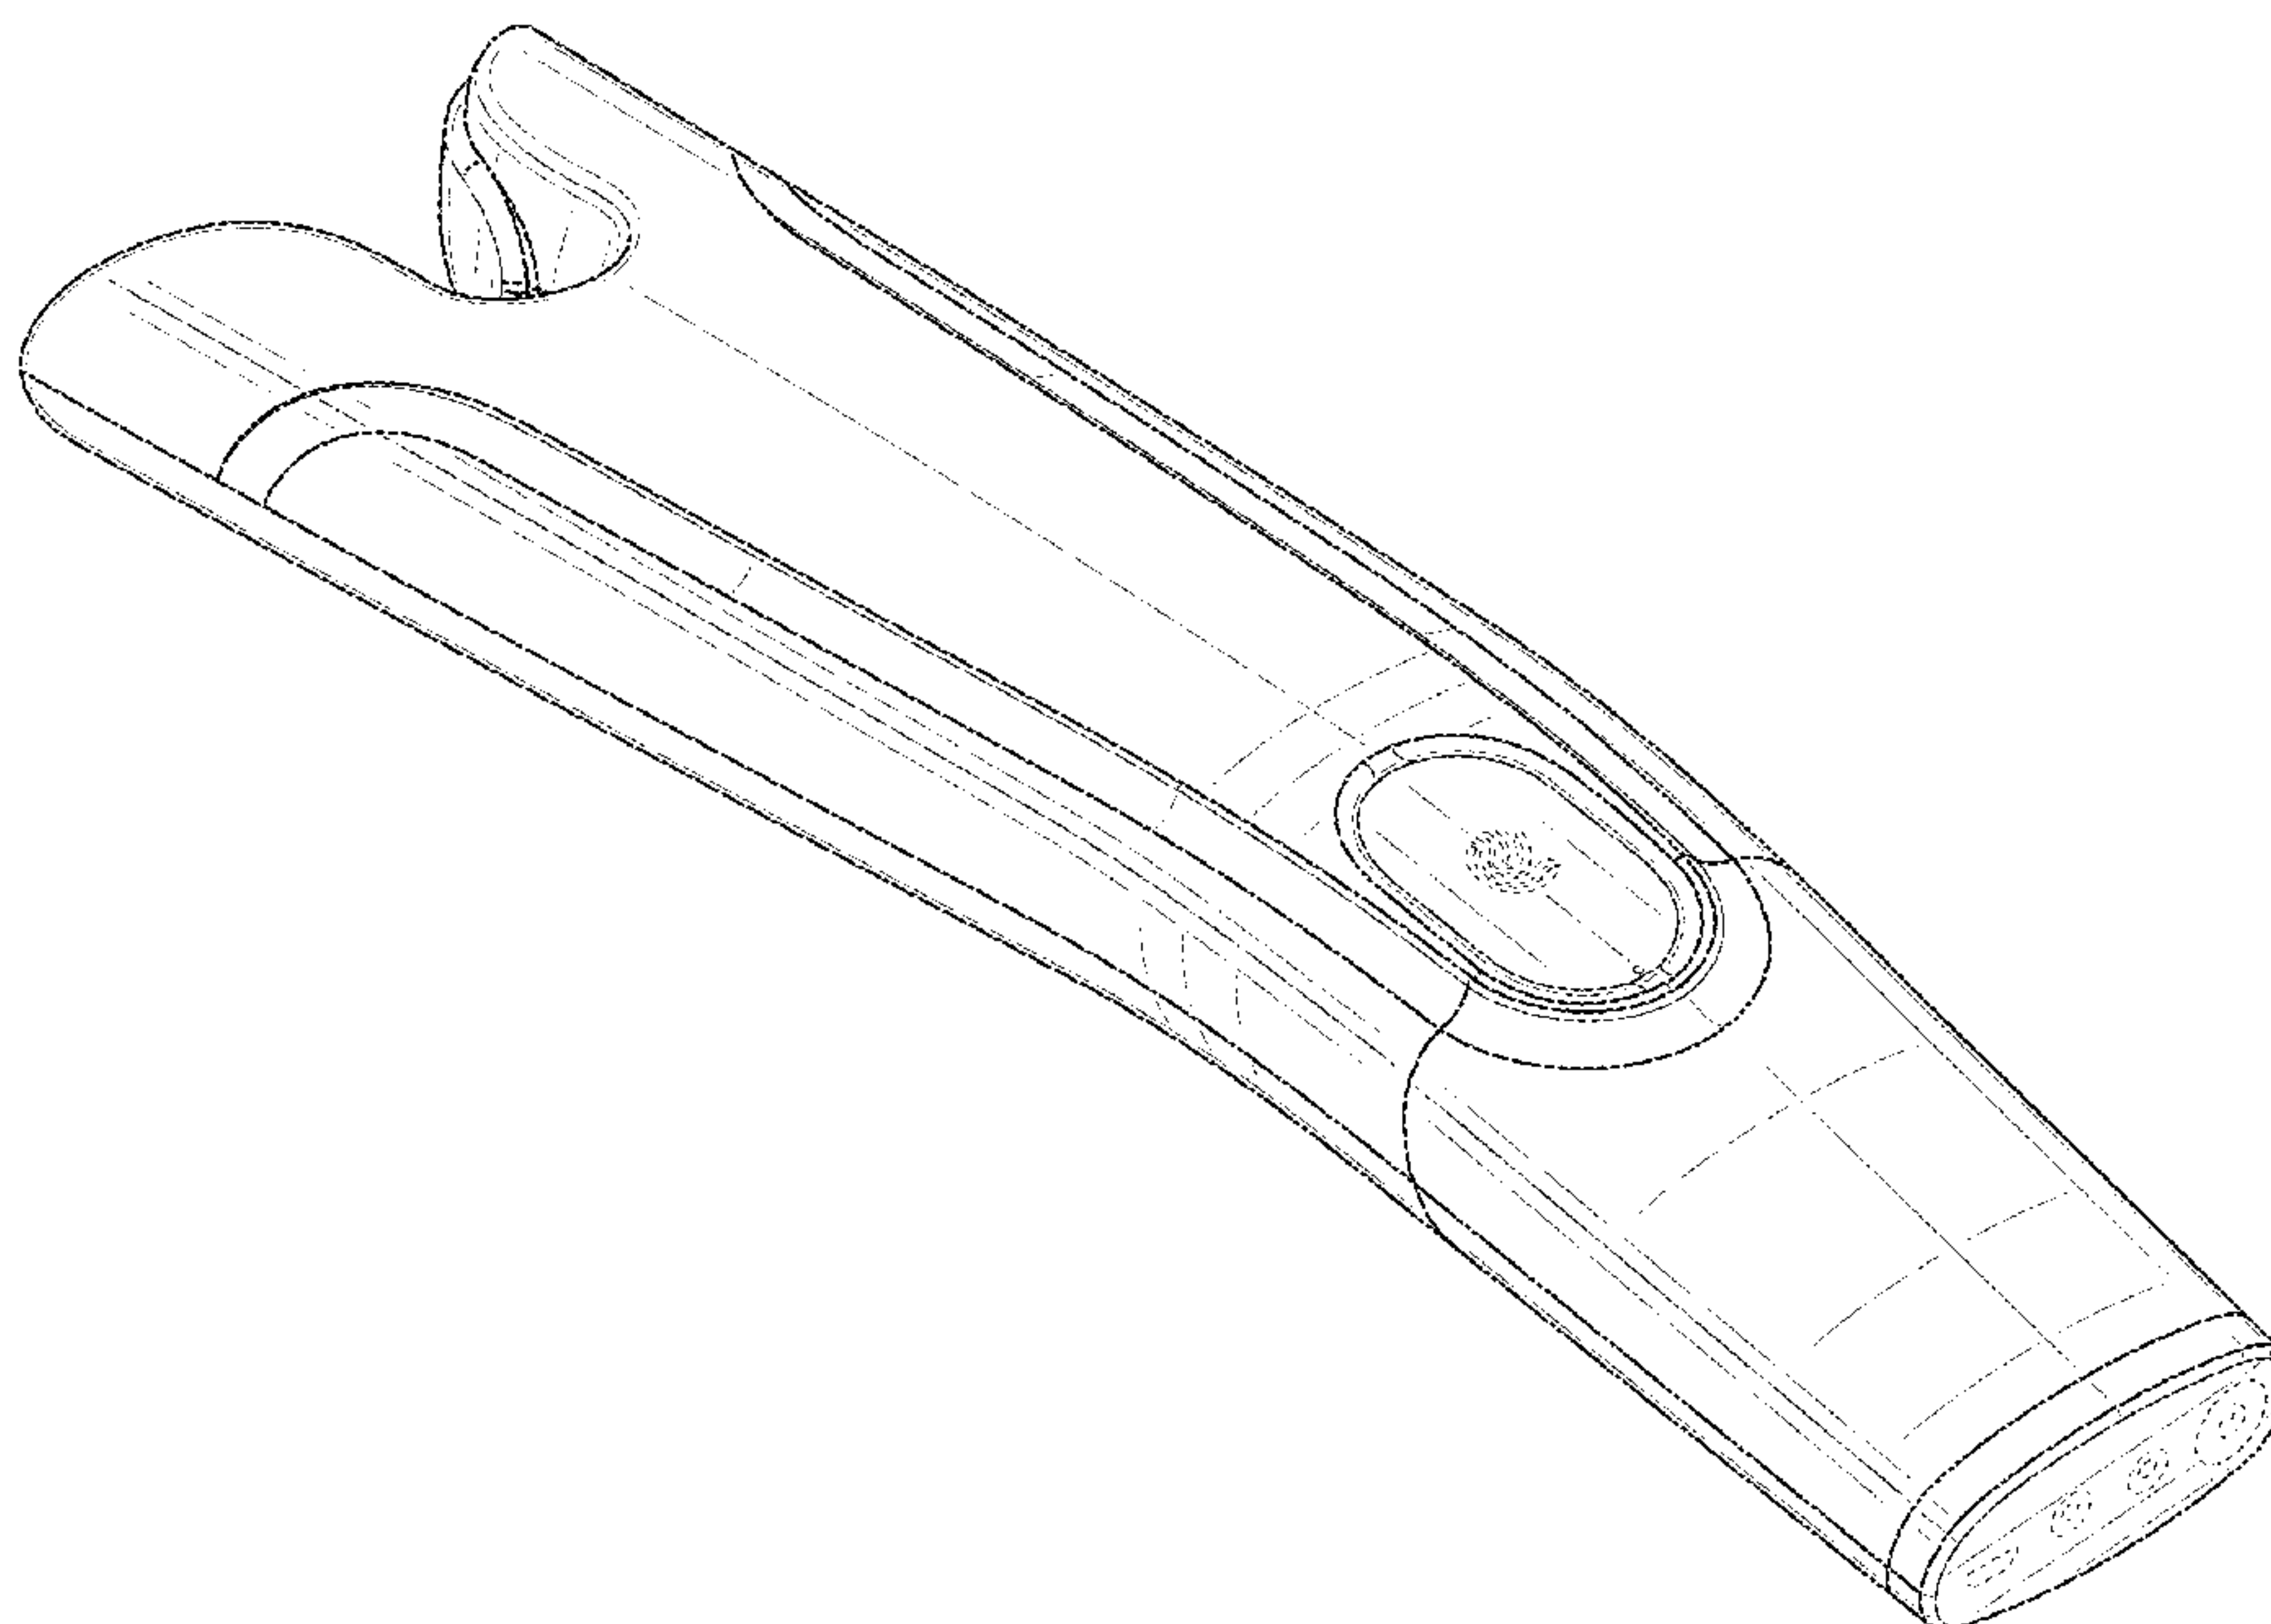

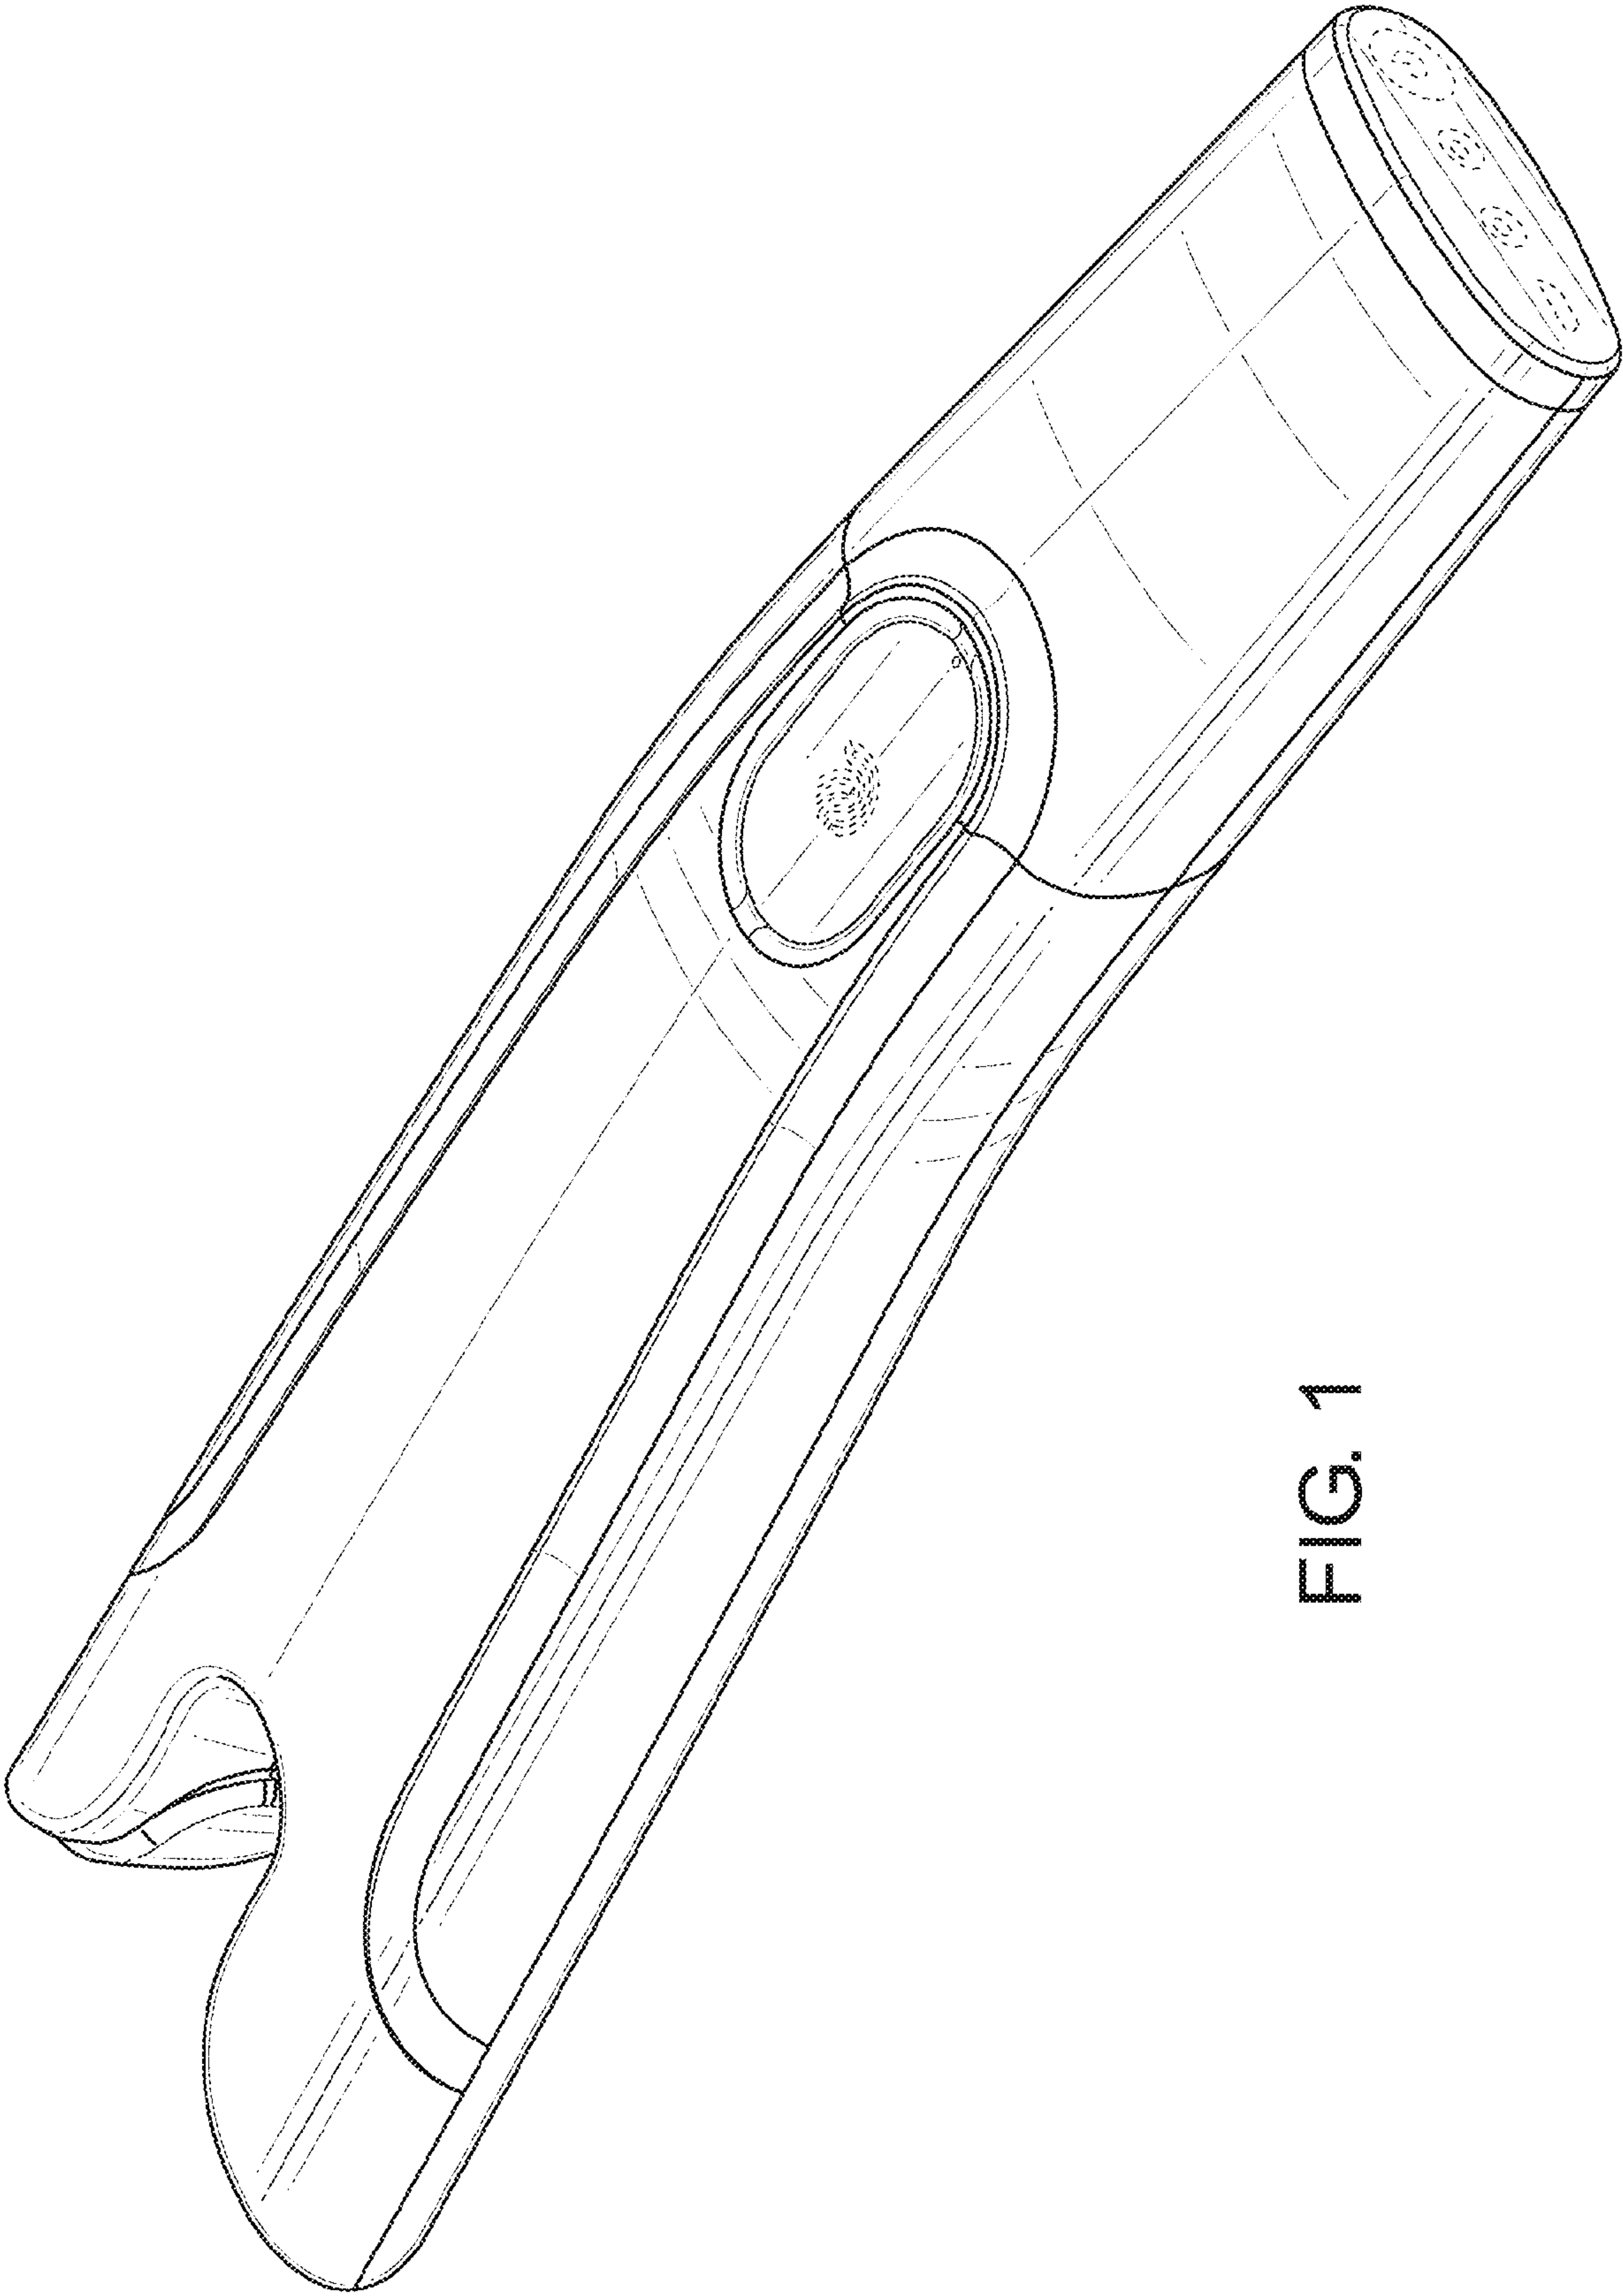


FIG. 1

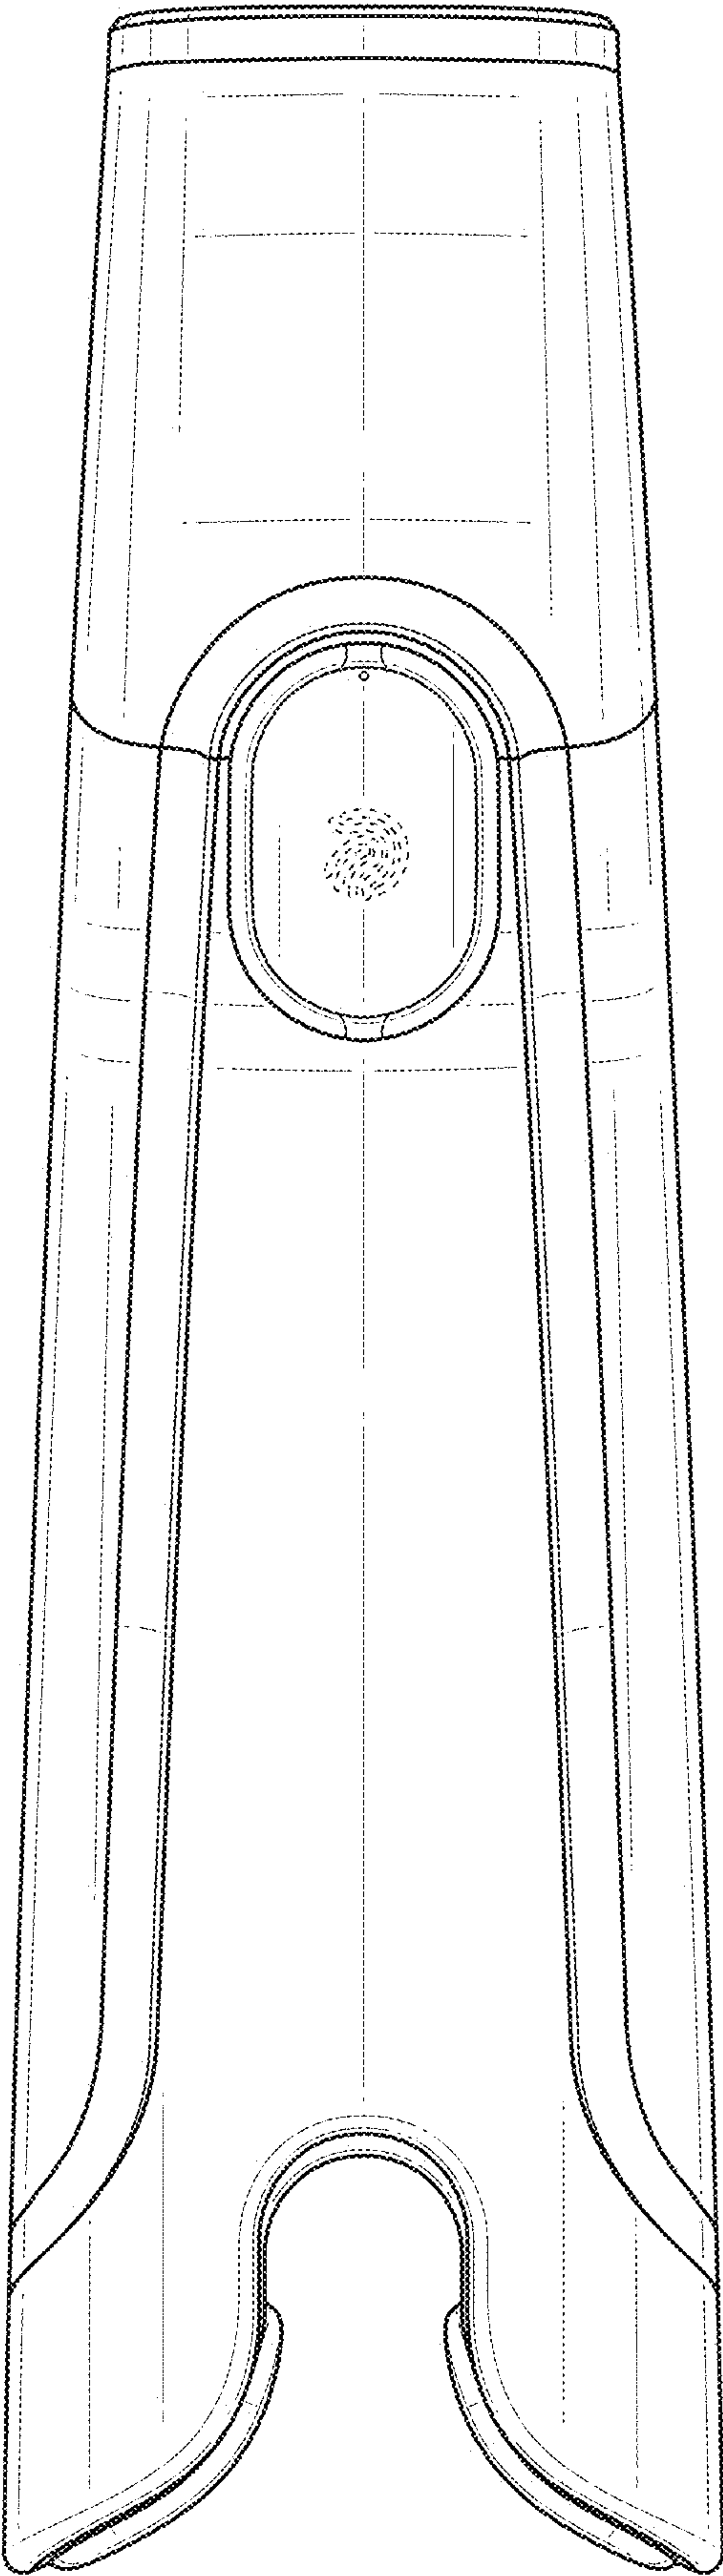


FIG. 2

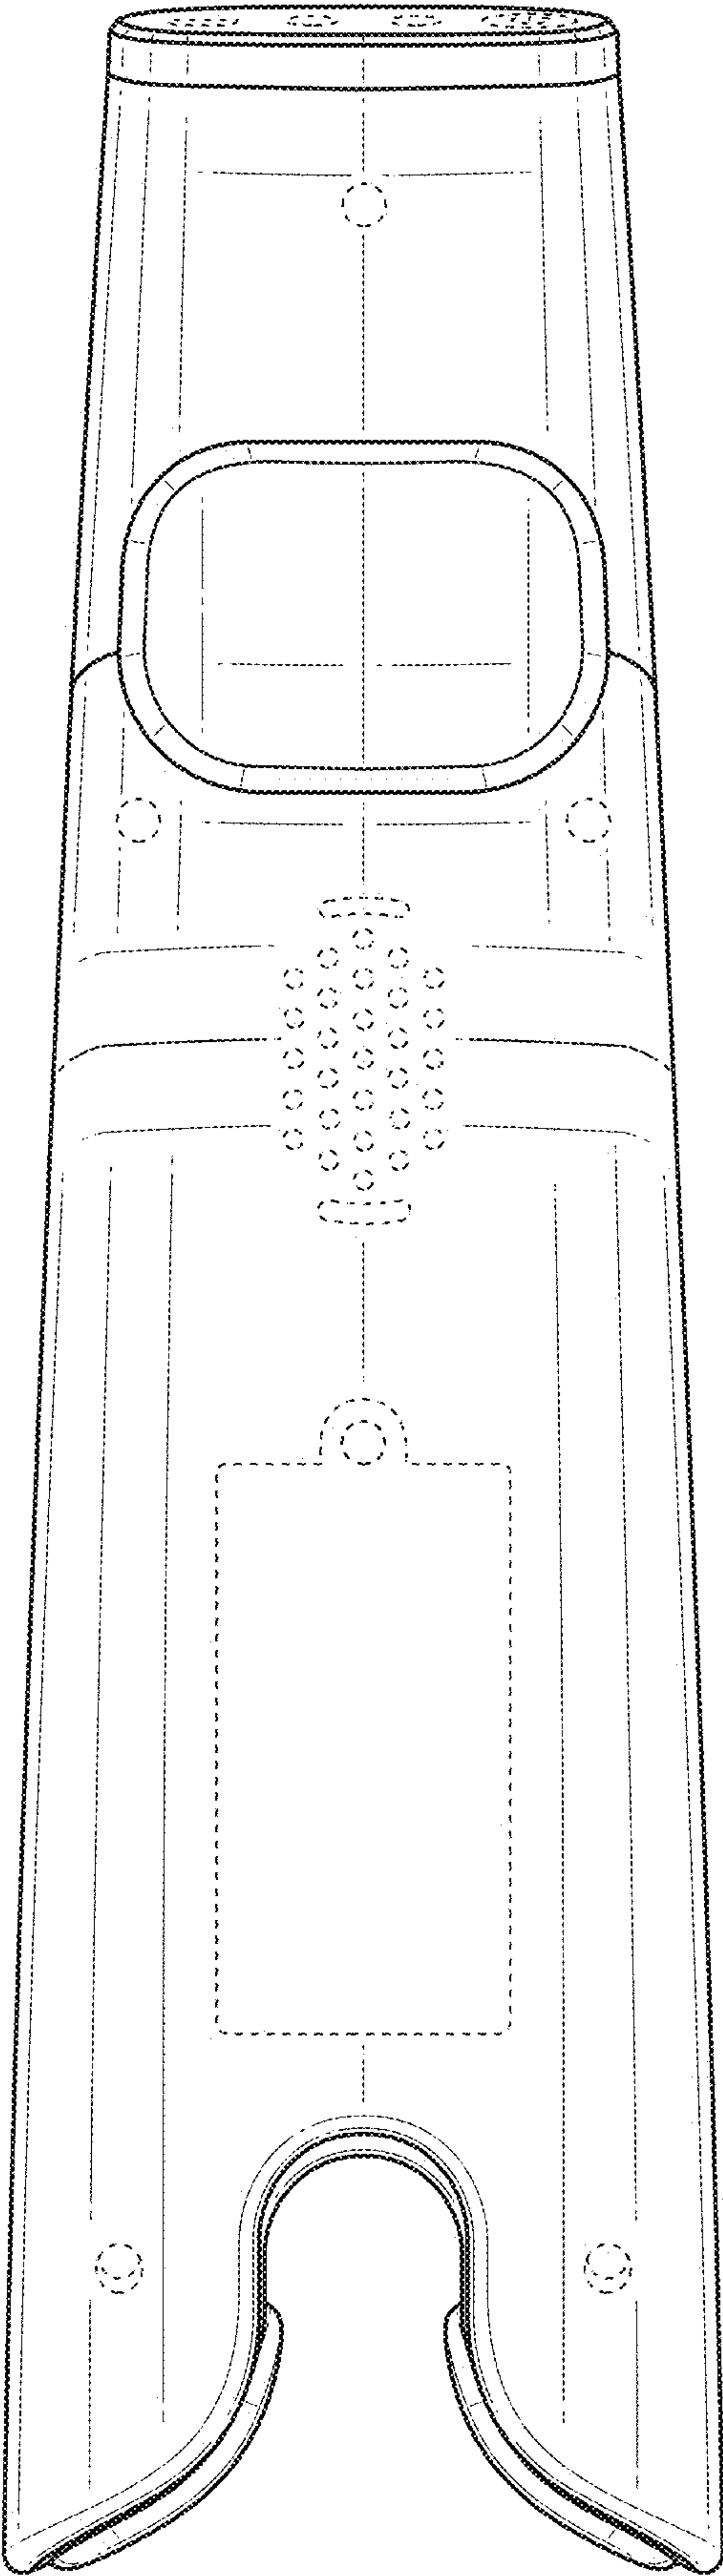


FIG. 3

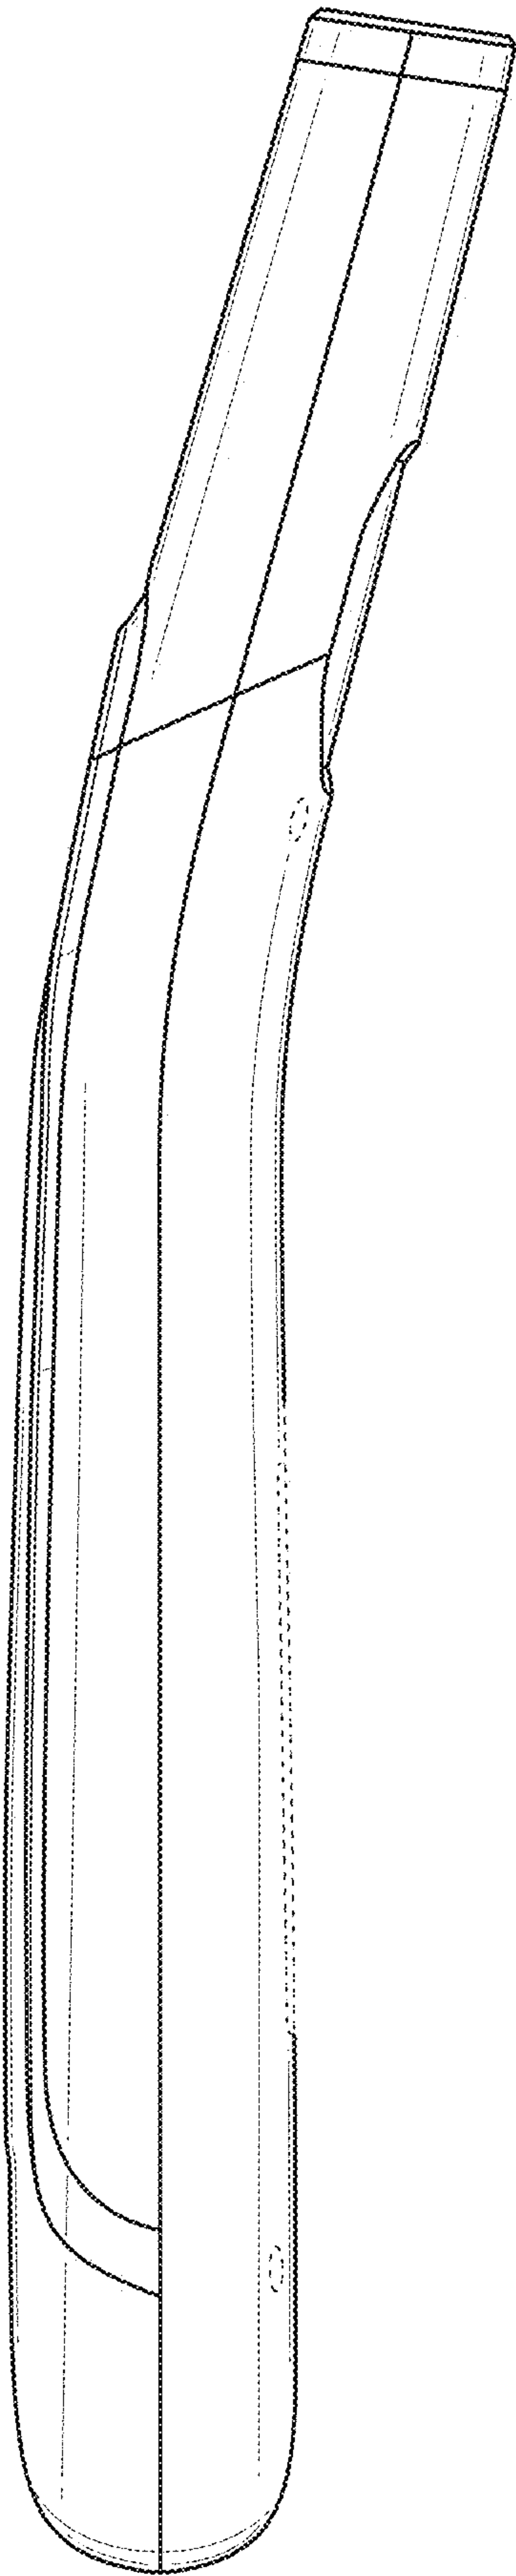


FIG. 4

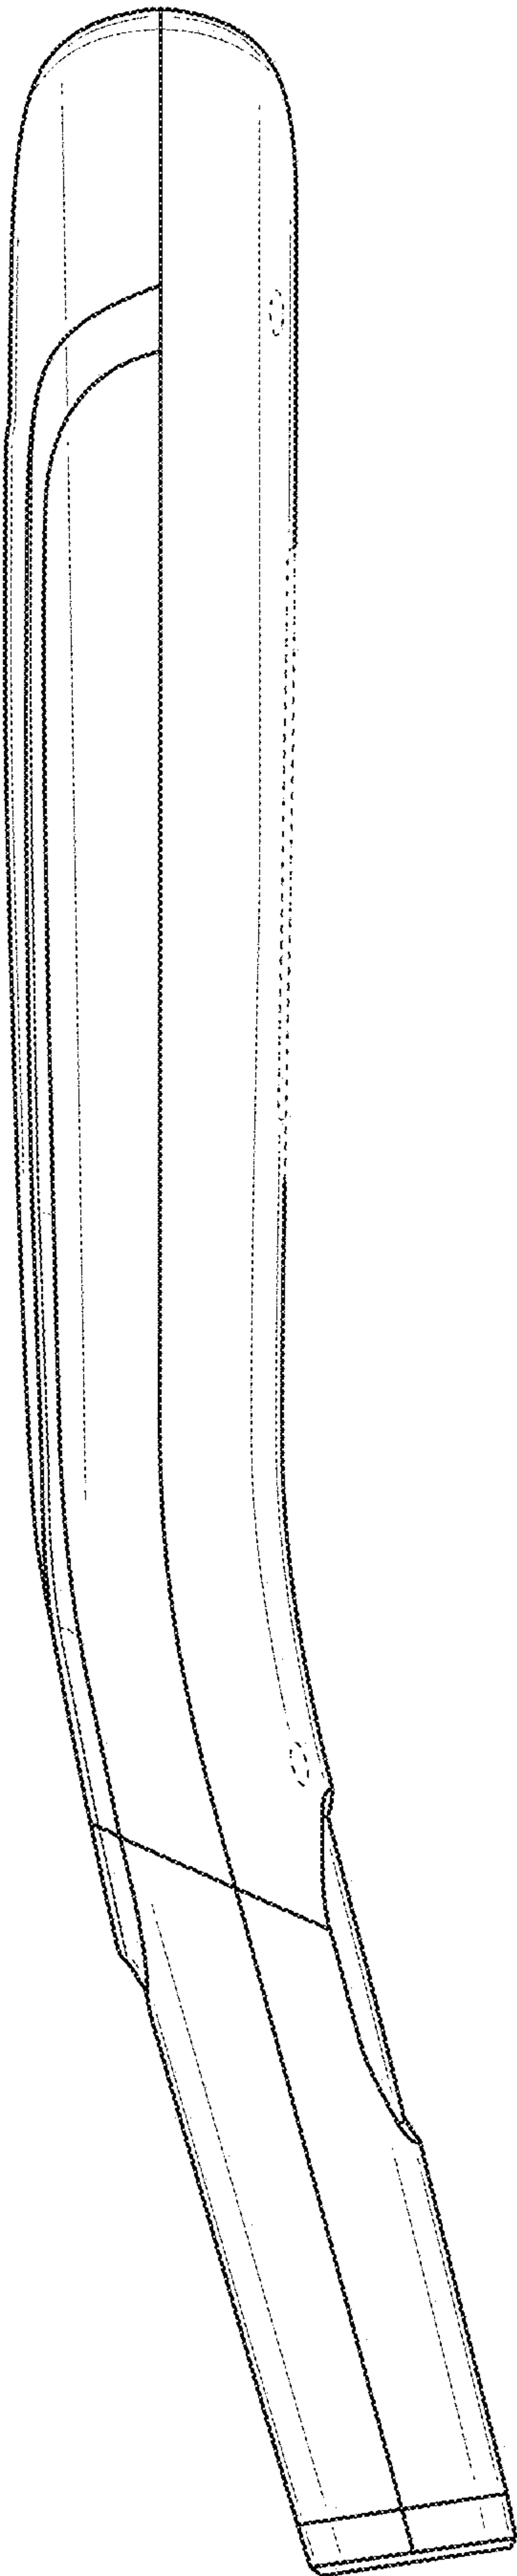


FIG. 5

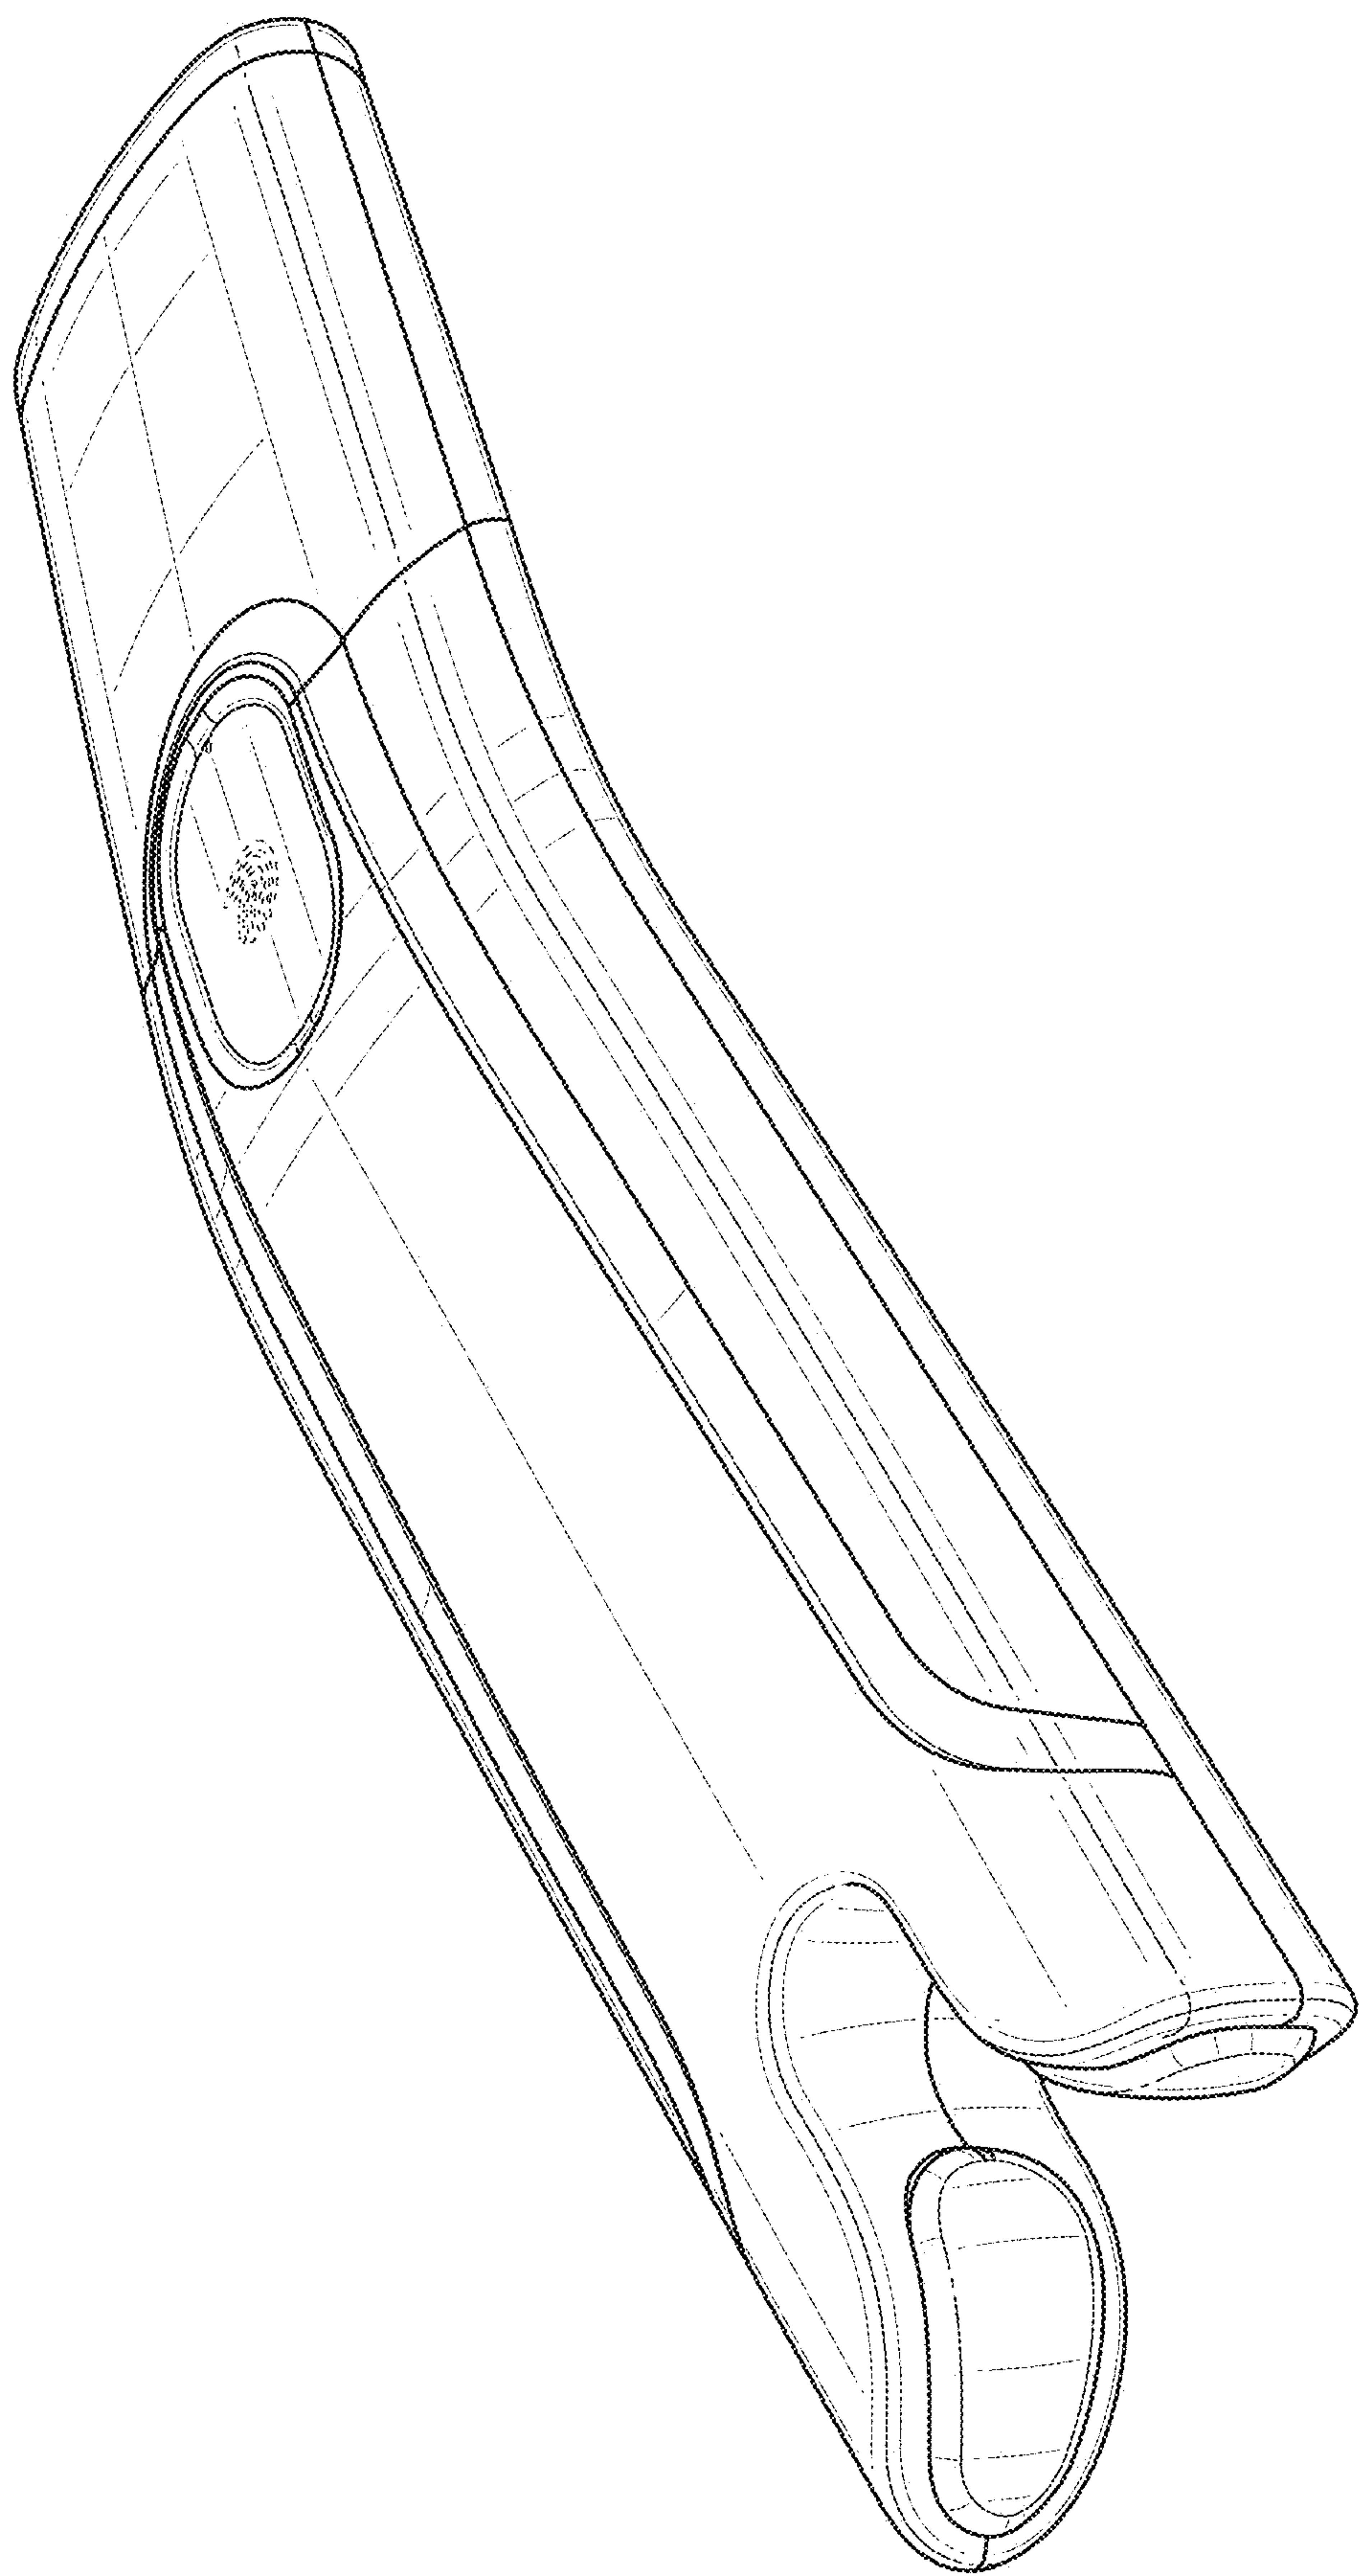


FIG. 6

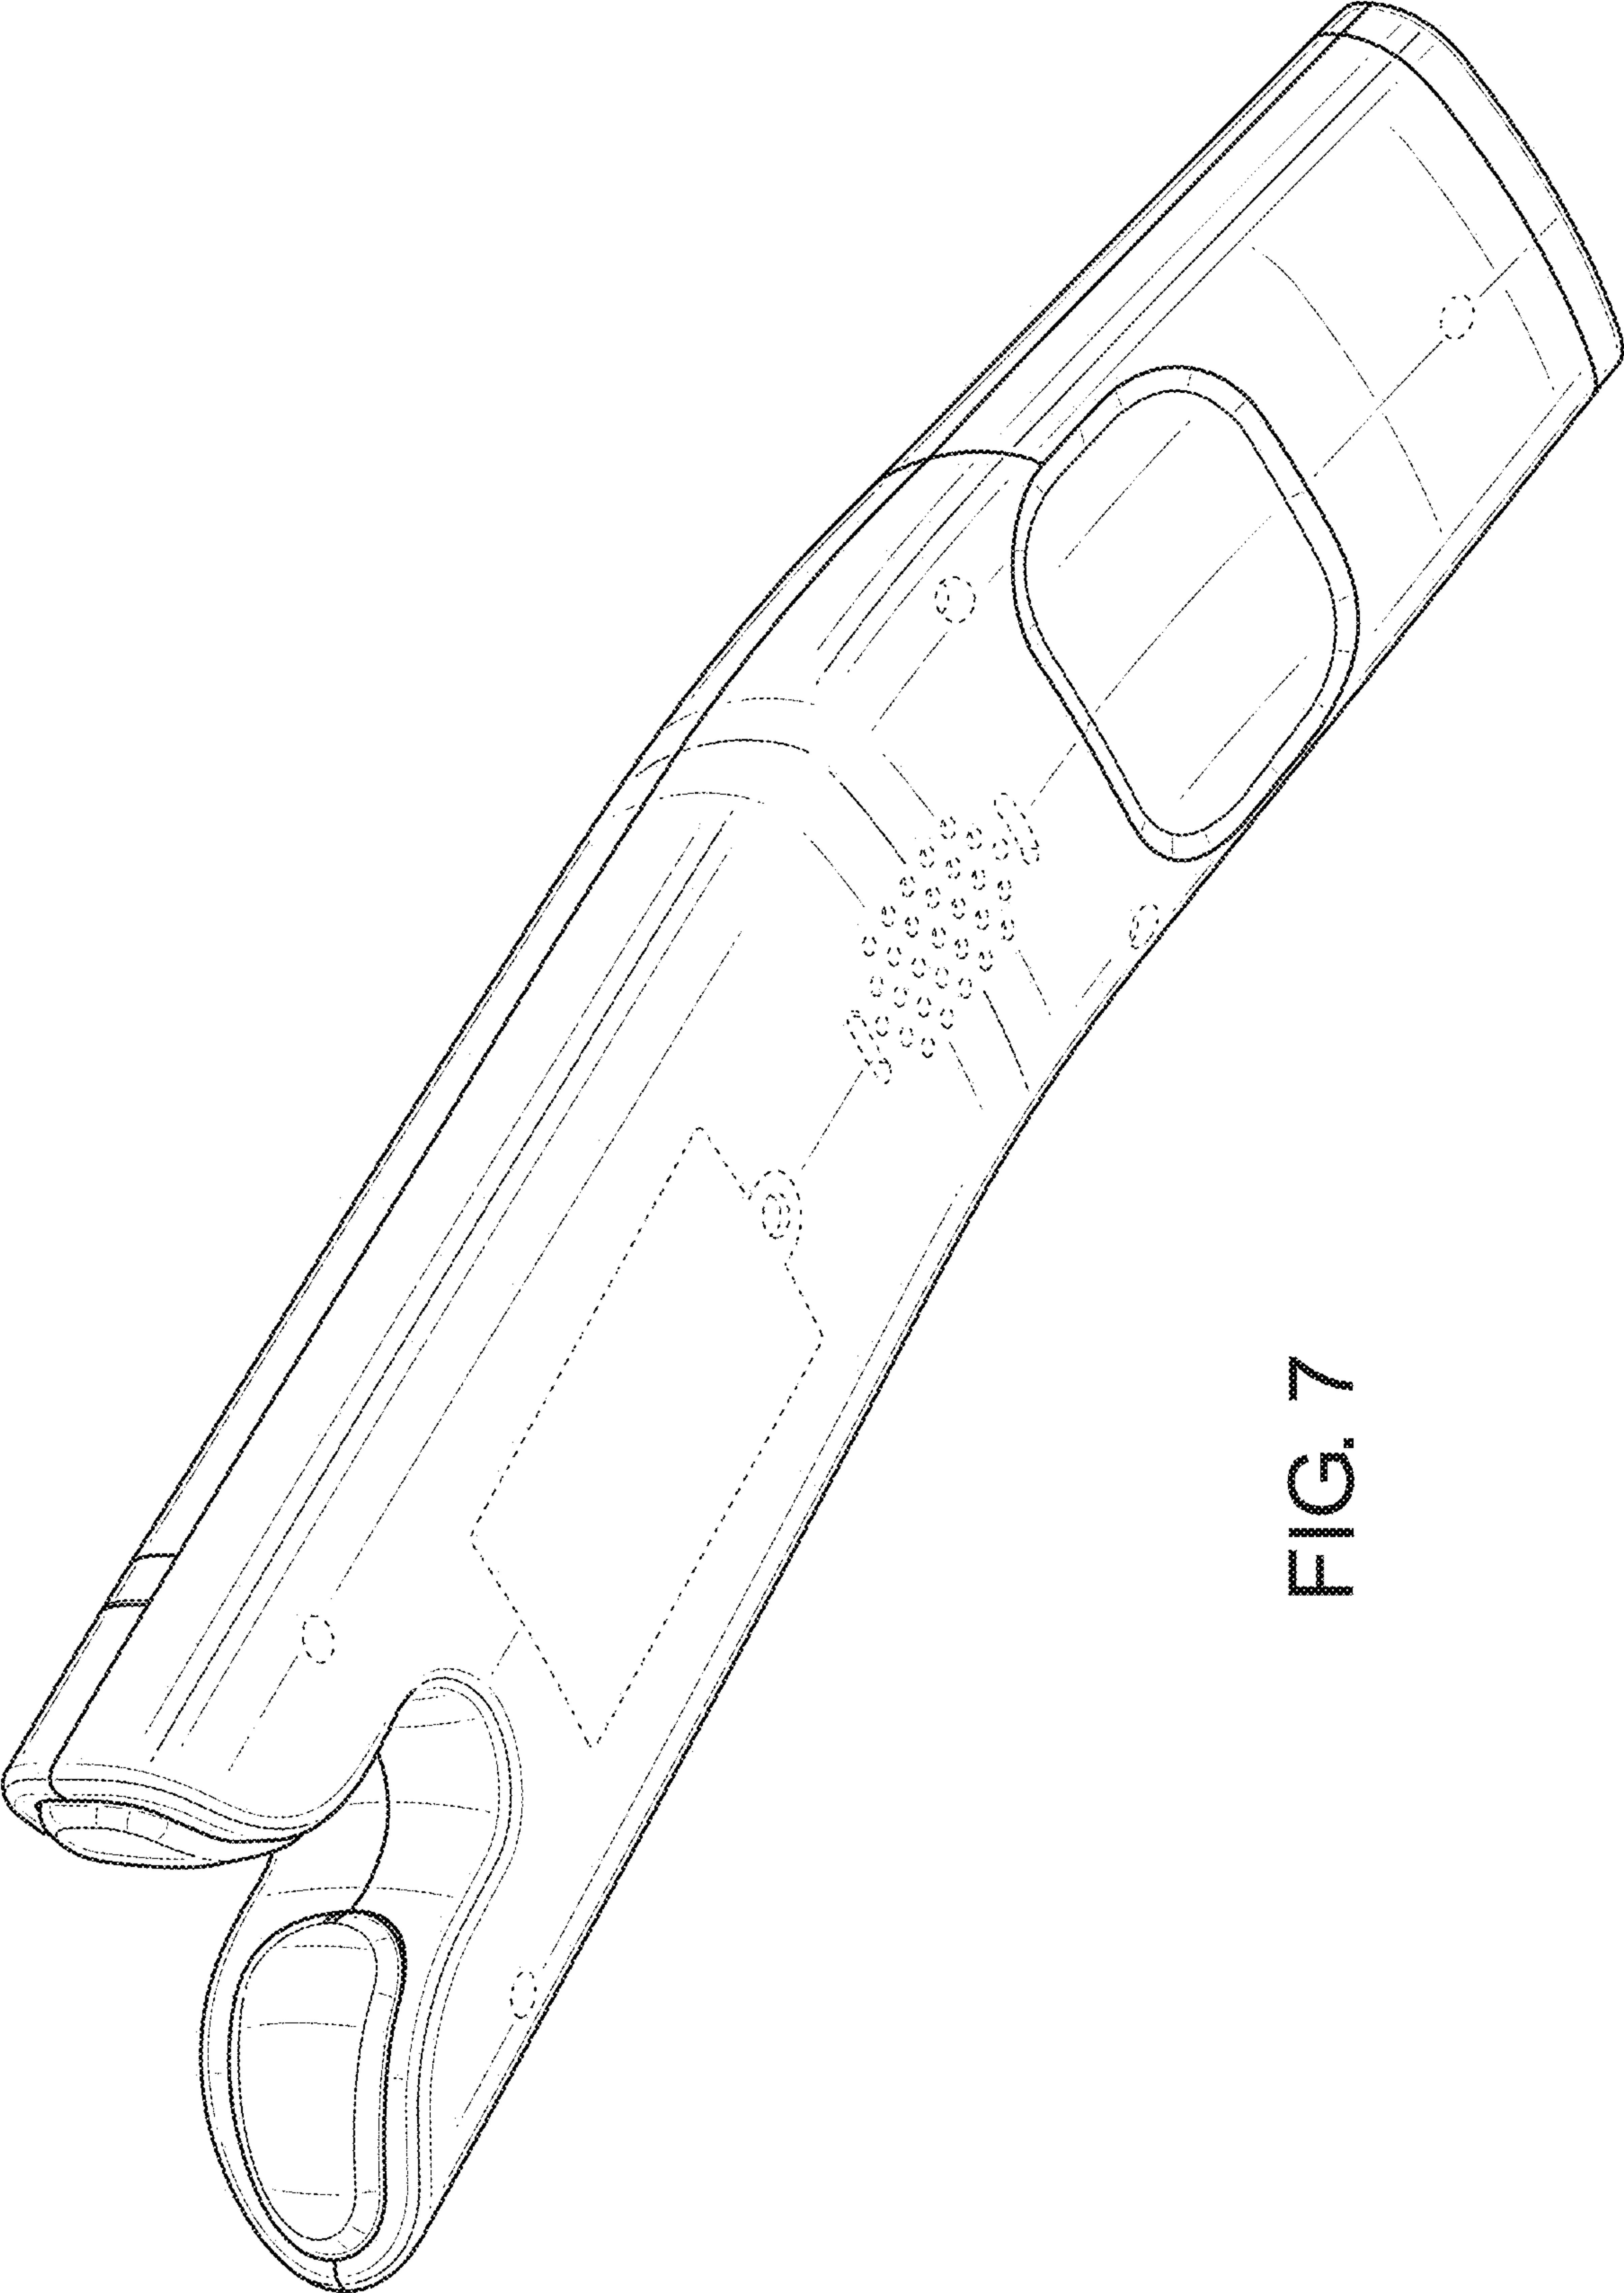


FIG. 7