



US00D938466S

(12) **United States Design Patent**
Wheeler et al.

(10) **Patent No.:** **US D938,466 S**

(45) **Date of Patent:** **** Dec. 14, 2021**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **Smiths Medical ASD, Inc.**, Plymouth, MN (US)

(72) Inventors: **Douglas Wheeler**, Eden Prairie, MN (US); **Joel Paulson**, Minneapolis, MN (US); **Lisa Hoh**, St. Paul, MN (US); **Ryan Heilman**, Andover, MN (US)

(73) Assignee: **Smiths Medical ASD, Inc.**, Plymouth, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/726,013**

(22) Filed: **Feb. 28, 2020**

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048-04897
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,681,285	A	10/1997	Ford et al.	
7,072,725	B2	7/2006	Bristol et al.	
7,324,949	B2	1/2008	Bristol	
D589,527	S *	3/2009	Shamma	D14/486
D640,264	S *	6/2011	Fujii	D14/486
7,970,620	B2	6/2011	Brown	
8,065,161	B2	11/2011	Howard et al.	
8,380,536	B2	2/2013	Howard et al.	
8,543,416	B2	9/2013	Palmroos et al.	
D694,259	S *	11/2013	Klein	D14/486
8,660,860	B2	2/2014	Wehba et al.	

8,983,616	B2	3/2015	Kaula et al.	
8,990,722	B2	3/2015	Gannon et al.	
9,177,108	B2	11/2015	Garibaldi et al.	
9,393,366	B2	7/2016	Gannon et al.	
9,440,023	B2	9/2016	Villegas et al.	
9,483,614	B2	11/2016	Ash et al.	
9,492,341	B2	11/2016	Huster et al.	
9,572,923	B2	2/2017	Howard et al.	
10,009,391	B1 *	6/2018	Smith	G06F 16/2423
D822,035	S *	7/2018	Wu	D14/485
D822,678	S *	7/2018	Wu	D14/485
D823,860	S *	7/2018	Wiffen	D14/485
D841,665	S *	2/2019	Matheson	D14/485
D874,474	S *	2/2020	Rognlie	D14/485
D874,481	S *	2/2020	Kumar	D14/485
D876,453	S *	2/2020	Knowles	D14/485
D876,454	S *	2/2020	Knowles	D14/485
D881,205	S *	4/2020	Tappan	D14/485
D888,082	S *	6/2020	Weick	D14/486
D922,421	S *	6/2021	Widmer	D14/486
D923,027	S *	6/2021	Anderson	D14/485
D924,909	S *	7/2021	Nasu	D14/486

(Continued)

Primary Examiner — Andrew T Nemeth

(74) Attorney, Agent, or Firm — Patterson Thuent Pedersen, P.A.

(57) **CLAIM**


We claim the ornamental design for a display screen or portion thereof with graphical user interface, as shown and described.

DESCRIPTION

The FIGURE is a front view of a display screen or portion thereof with graphical user interface.

The outer broken line showing the display screen or portion thereof and all other broken lines showing portions of the graphical user interface illustrate portions of the article of manufacture. None of the aforementioned broken line subject matters form part of the claimed design.

1 Claim, 1 Drawing Sheet

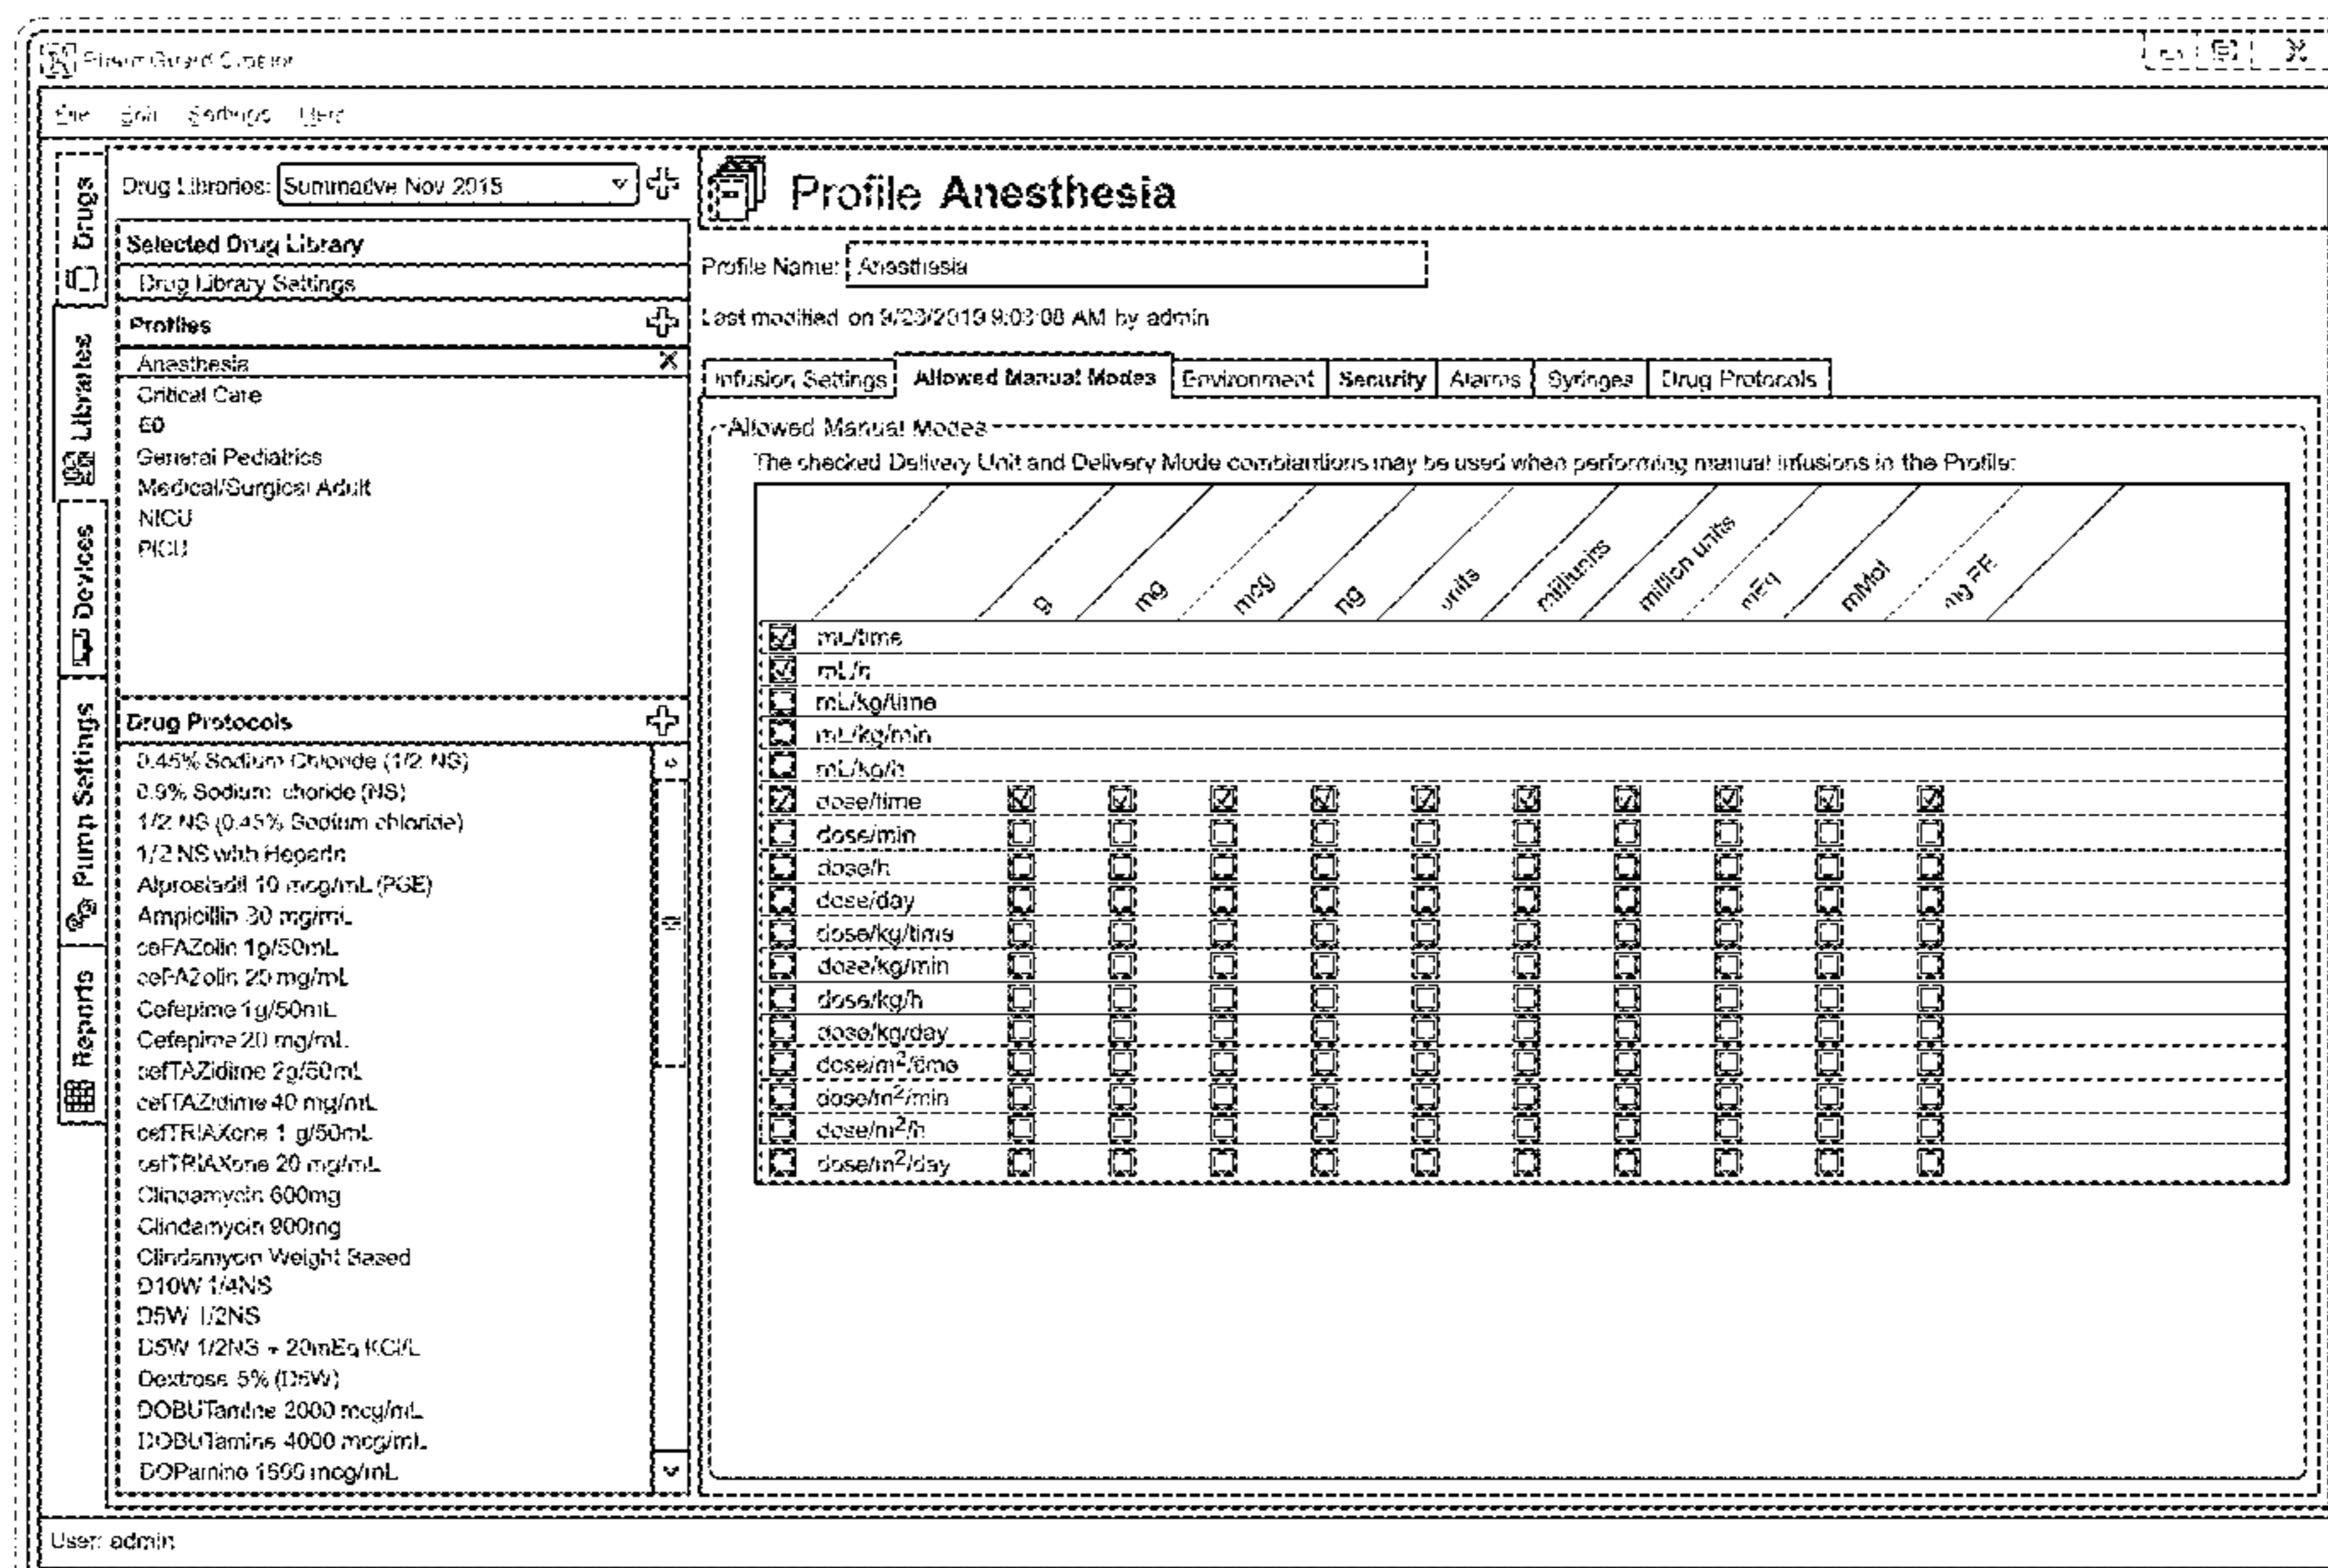

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0172455 A1* 9/2004 Green H04L 51/24
709/207
2007/0233692 A1* 10/2007 Lisa G06F 16/248
2008/0046803 A1* 2/2008 Beauchamp G06F 16/957
715/212
2011/0106669 A1* 5/2011 Baghdassarian G06Q 30/08
705/30
2013/0055244 A1* 2/2013 Cannon, III G06F 3/0483
718/1
2013/0212507 A1* 8/2013 Fedoseyeva G06Q 10/00
715/765
2015/0213211 A1* 7/2015 Zaleski G16H 10/60
715/753
2020/0105107 A1* 4/2020 McKeever G07F 17/3211
2021/0233365 A1* 7/2021 McKeever G07F 17/3211

* cited by examiner

File Edit Settings Help

Labels X

Drug Libraries: Summative Nov 2018

Selected Drug Library

Drug Library Settings

Profiles

- Anesthesia
- Critical Care
- ED
- General Pediatrics
- Medical/Surgical Adult
- NICU
- PICU

Profile Anesthesia

Profile Name: Anesthesia

Last modified on 9/23/2019 9:03:06 AM by admin

Infusion Settings
Allowed Manual Modes
Environment
Security
Alarms
Syringes
Drug Protocols

Allowed Manual Modes

The checked Delivery Unit and Delivery Mode combinations may be used when performing manual infusions in the Profile:

	g	mg	mcg	ng	units	milliunits	million units	mcg	mmol	mg PE
<input checked="" type="checkbox"/> mL/time										
<input checked="" type="checkbox"/> mL/h										
<input type="checkbox"/> mL/kg/time										
<input type="checkbox"/> mL/kg/min										
<input type="checkbox"/> mL/kg/h										
<input checked="" type="checkbox"/> dose/time										
<input type="checkbox"/> dose/min										
<input type="checkbox"/> dose/h										
<input type="checkbox"/> dose/day										
<input type="checkbox"/> dose/kg/time										
<input type="checkbox"/> dose/kg/min										
<input type="checkbox"/> dose/kg/h										
<input type="checkbox"/> dose/kg/day										
<input type="checkbox"/> dose/m ² /time										
<input type="checkbox"/> dose/m ² /min										
<input type="checkbox"/> dose/m ² /h										
<input type="checkbox"/> dose/m ² /day										

Drug Protocols

- 0.45% Sodium Chloride (1/2 NS)
- 0.9% Sodium chloride (NS)
- 1/2 NS (0.45% Sodium chloride)
- 1/2 NS with Heparin
- Alprostadil 10 mcg/mL (POE)
- Ampicillin 30 mg/mL
- ceFAZolin 1g/50mL
- ceFAZolin 20 mg/mL
- Cefepime 1g/50mL
- Cefepime 20 mg/mL
- cefTAZidime 2g/50mL
- cefTAZidime 40 mg/mL
- cefTRIAxone 1 g/50mL
- cefTRIAxone 20 mg/mL
- Clindamycin 600mg
- Clindamycin 900mg
- Clindamycin Weight Based
- D10W 1/4NS
- D5W 1/2NS
- D5W 1/2NS + 20mEq KCl/L
- Dextrose 5% (D5W)
- DOBUTamine 2000 mcg/mL
- DOBUTamine 4000 mcg/mL
- DOPamine 1600 mcg/mL

Drugs Libraries Devices Pump Settings Reports

User: admin