



US00D938522S

(12) **United States Design Patent**
Flatt et al.

(10) **Patent No.:** **US D938,522 S**

(45) **Date of Patent:** **** Dec. 14, 2021**

(54) **LABEL**

(71) Applicants: **Alexander Flatt**, Norwich (GB);
Samuel John Mortimer, Hull (GB);
Mark Parling, Hull (GB); **Richard Thorpe**, Hull (GB)

(72) Inventors: **Alexander Flatt**, Norwich (GB);
Samuel John Mortimer, Hull (GB);
Mark Parling, Hull (GB); **Richard Thorpe**, Hull (GB)

(**) Term: **15 Years**

(21) Appl. No.: **29/661,666**

(22) Filed: **Aug. 29, 2018**

(51) **LOC (13) Cl.** **19-08**

(52) **U.S. Cl.**
USPC **D20/27**

(58) **Field of Classification Search**
USPC D9/550, 563; D10/46, 47, 52, 104.1,
D10/104.2; D14/490, 491; D19/1, 2, 3,
D19/4, 5, 6, 7, 8, 9, 10, 11, 12; D20/10,
D20/11, 18, 22, 23, 24, 25, 26, 27, 28,
D20/29, 40, 43, 44, 49
CPC G09F 1/00; G09F 1/04; G09F 3/00; G09F
3/005; G09F 3/0288; G09F 3/0289; G09F
3/02; G09F 3/04; G09F 3/06; G09F 3/08;
G09F 3/10; G06K 19/0776

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D425,934 S * 5/2000 Kunkler D19/11
D445,445 S * 7/2001 Kane D17/20
D659,158 S * 5/2012 Clymer D14/488
D677,728 S * 3/2013 Self D19/60
D677,729 S * 3/2013 Self D19/60
D696,283 S * 12/2013 Schwengler D14/486
D701,867 S * 4/2014 Thompson D14/485
D780,200 S * 2/2017 Chaudhri D14/486

D782,497 S * 3/2017 Barry D14/485
D813,904 S * 3/2018 Okutsu D14/488
D834,063 S * 11/2018 Stray D14/491
D851,678 S * 6/2019 Clymer D14/492
D873,858 S * 1/2020 Fiol D14/495
D885,434 S * 5/2020 Lee D14/492
D887,443 S * 6/2020 Amini D14/491

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2013/171585 11/2013
WO WO 2016/103033 6/2016

OTHER PUBLICATIONS

Packaging for Pico Single Use Negative Pressure Wound Therapy System (#66801363), [date unknown], in 2 pages.

(Continued)

Primary Examiner — Mary Ann Calabrese

Assistant Examiner — Catherine Ho

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57) **CLAIM**

The ornamental design for a label, as shown and described.

DESCRIPTION



FIG. 1 is a front view of the first embodiment of a label, showing my new design.

FIG. 2 is a front view of the second embodiment of a label, showing my new design; and,

FIG. 3 is a front view of the third embodiment of a label, showing my new design.

The dot-dash perimeter indicates the boundaries of the claim and forms no part thereof. The broken lines in the drawings form no part of the claimed design. The stippling seen in FIGS. 1-3 depicts surface indicia, which forms part of the claimed design.

1 Claim, 3 Drawing Sheets

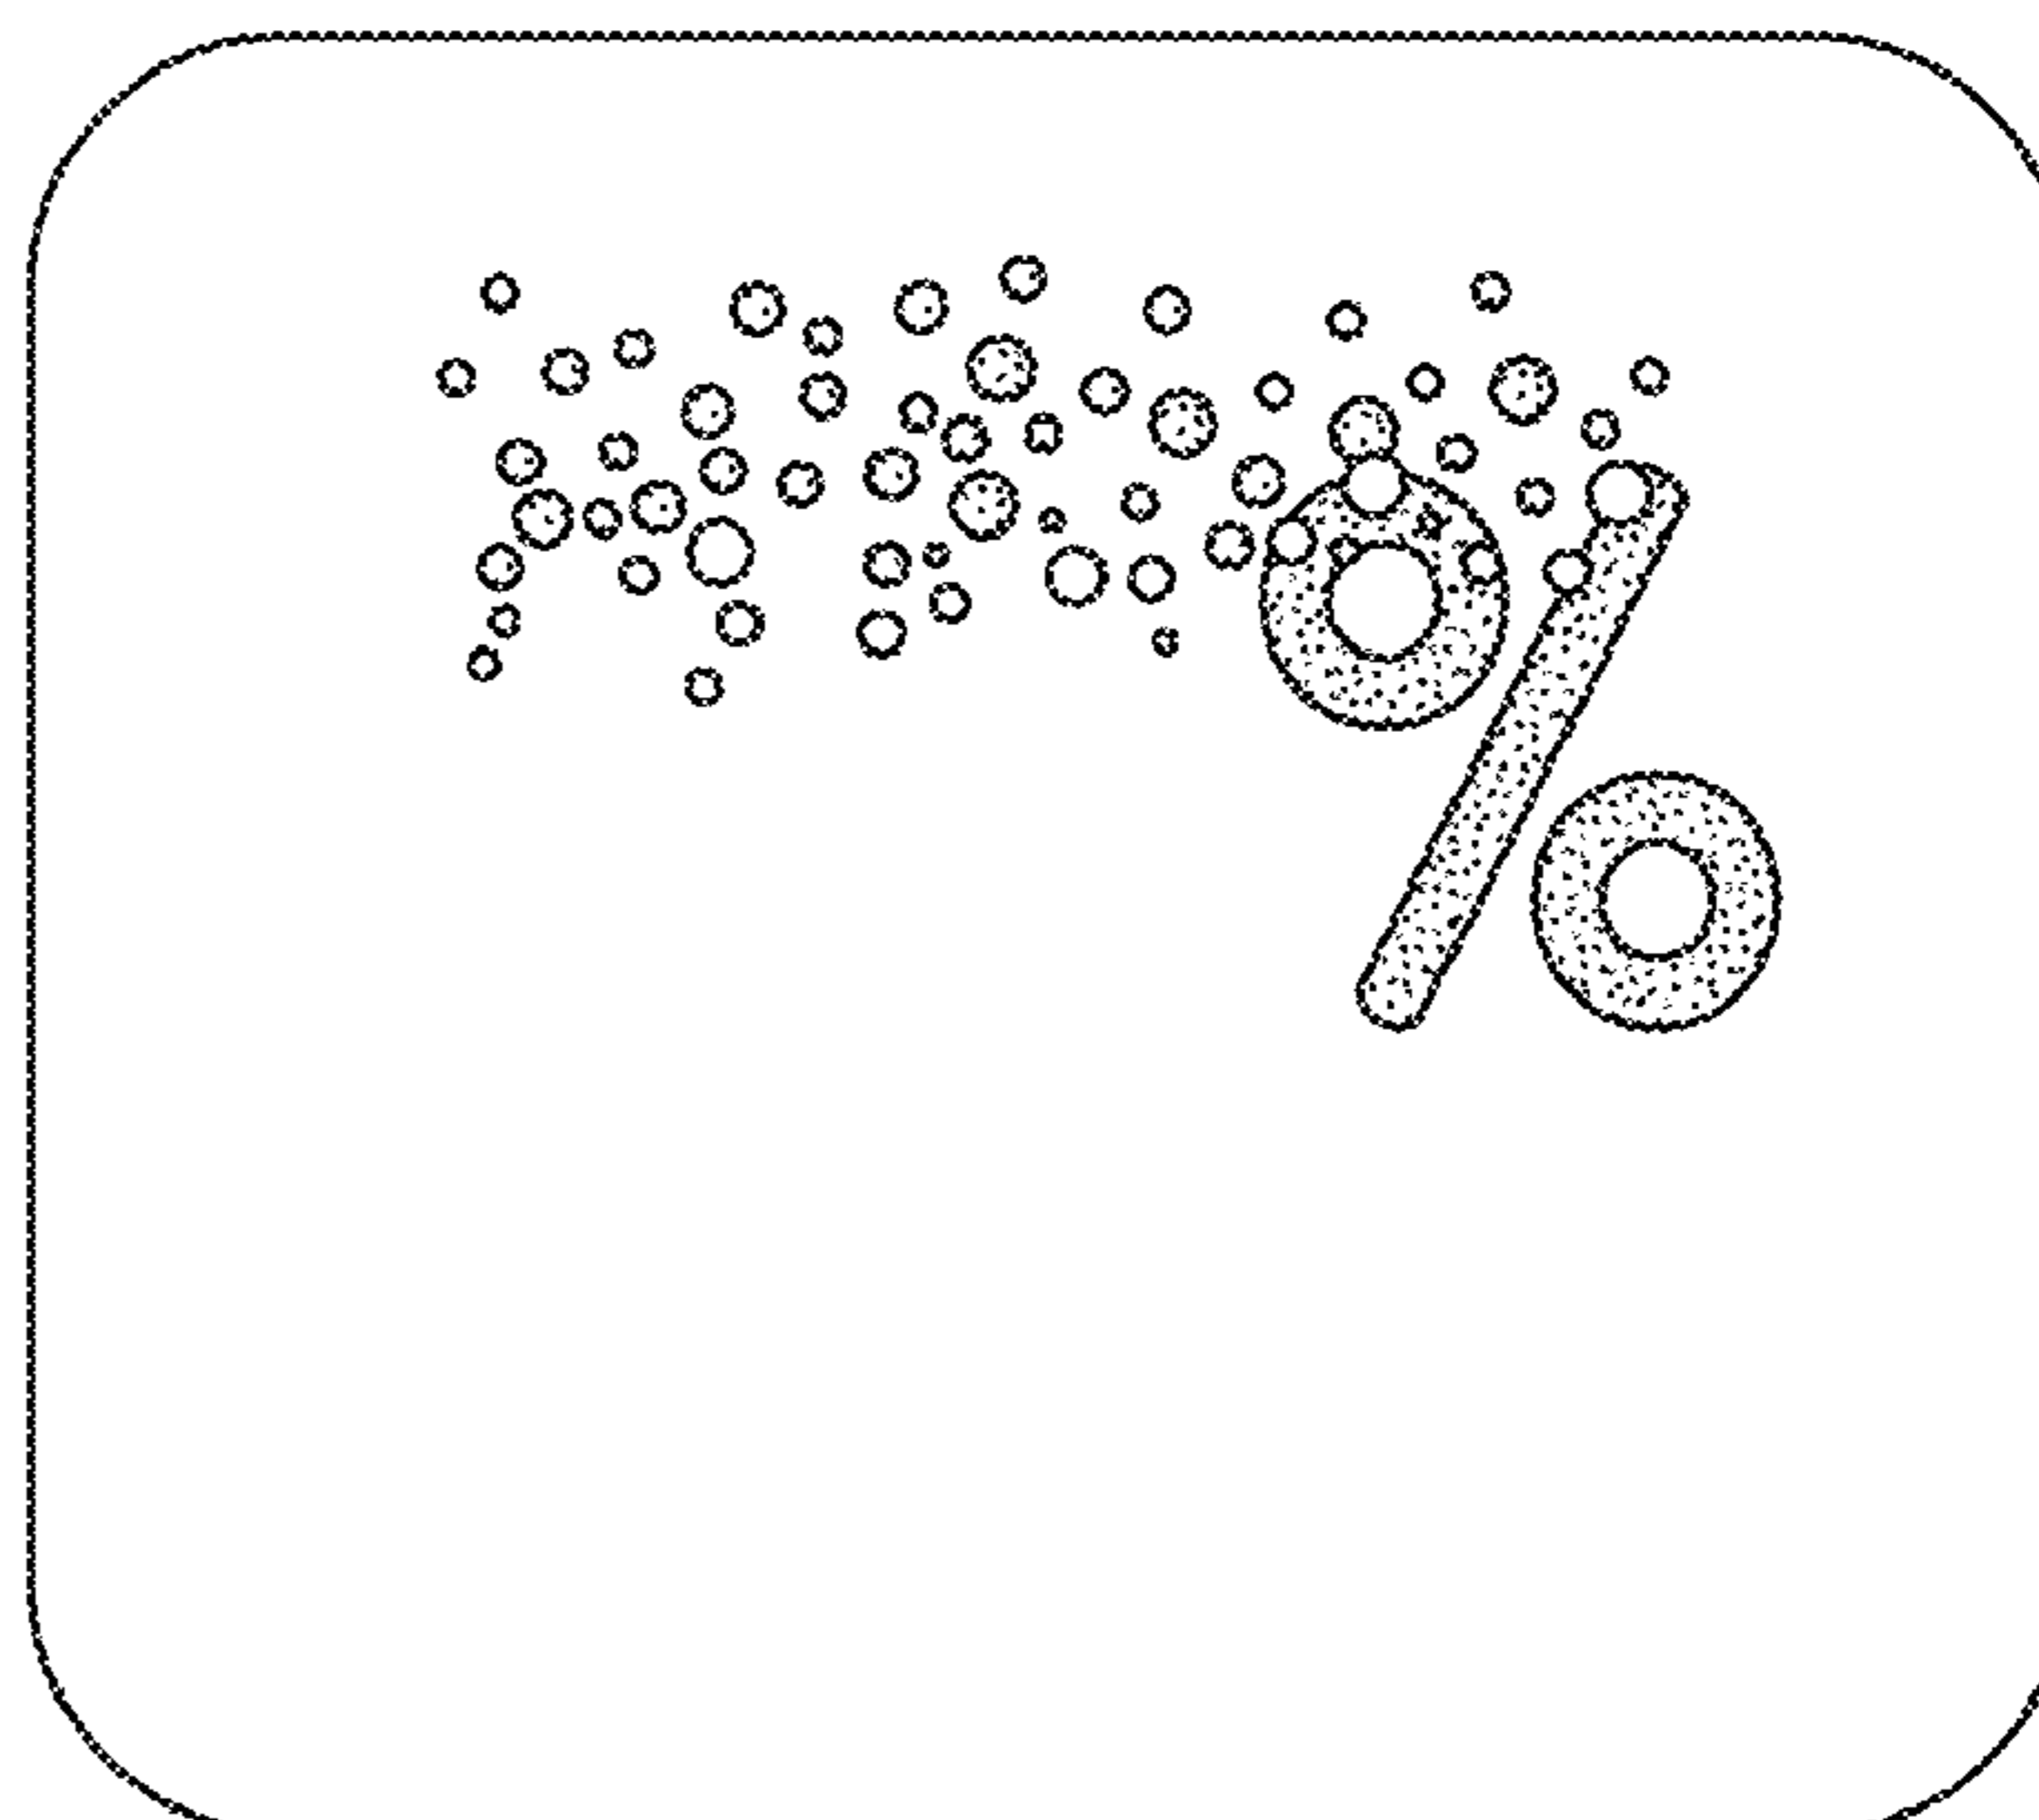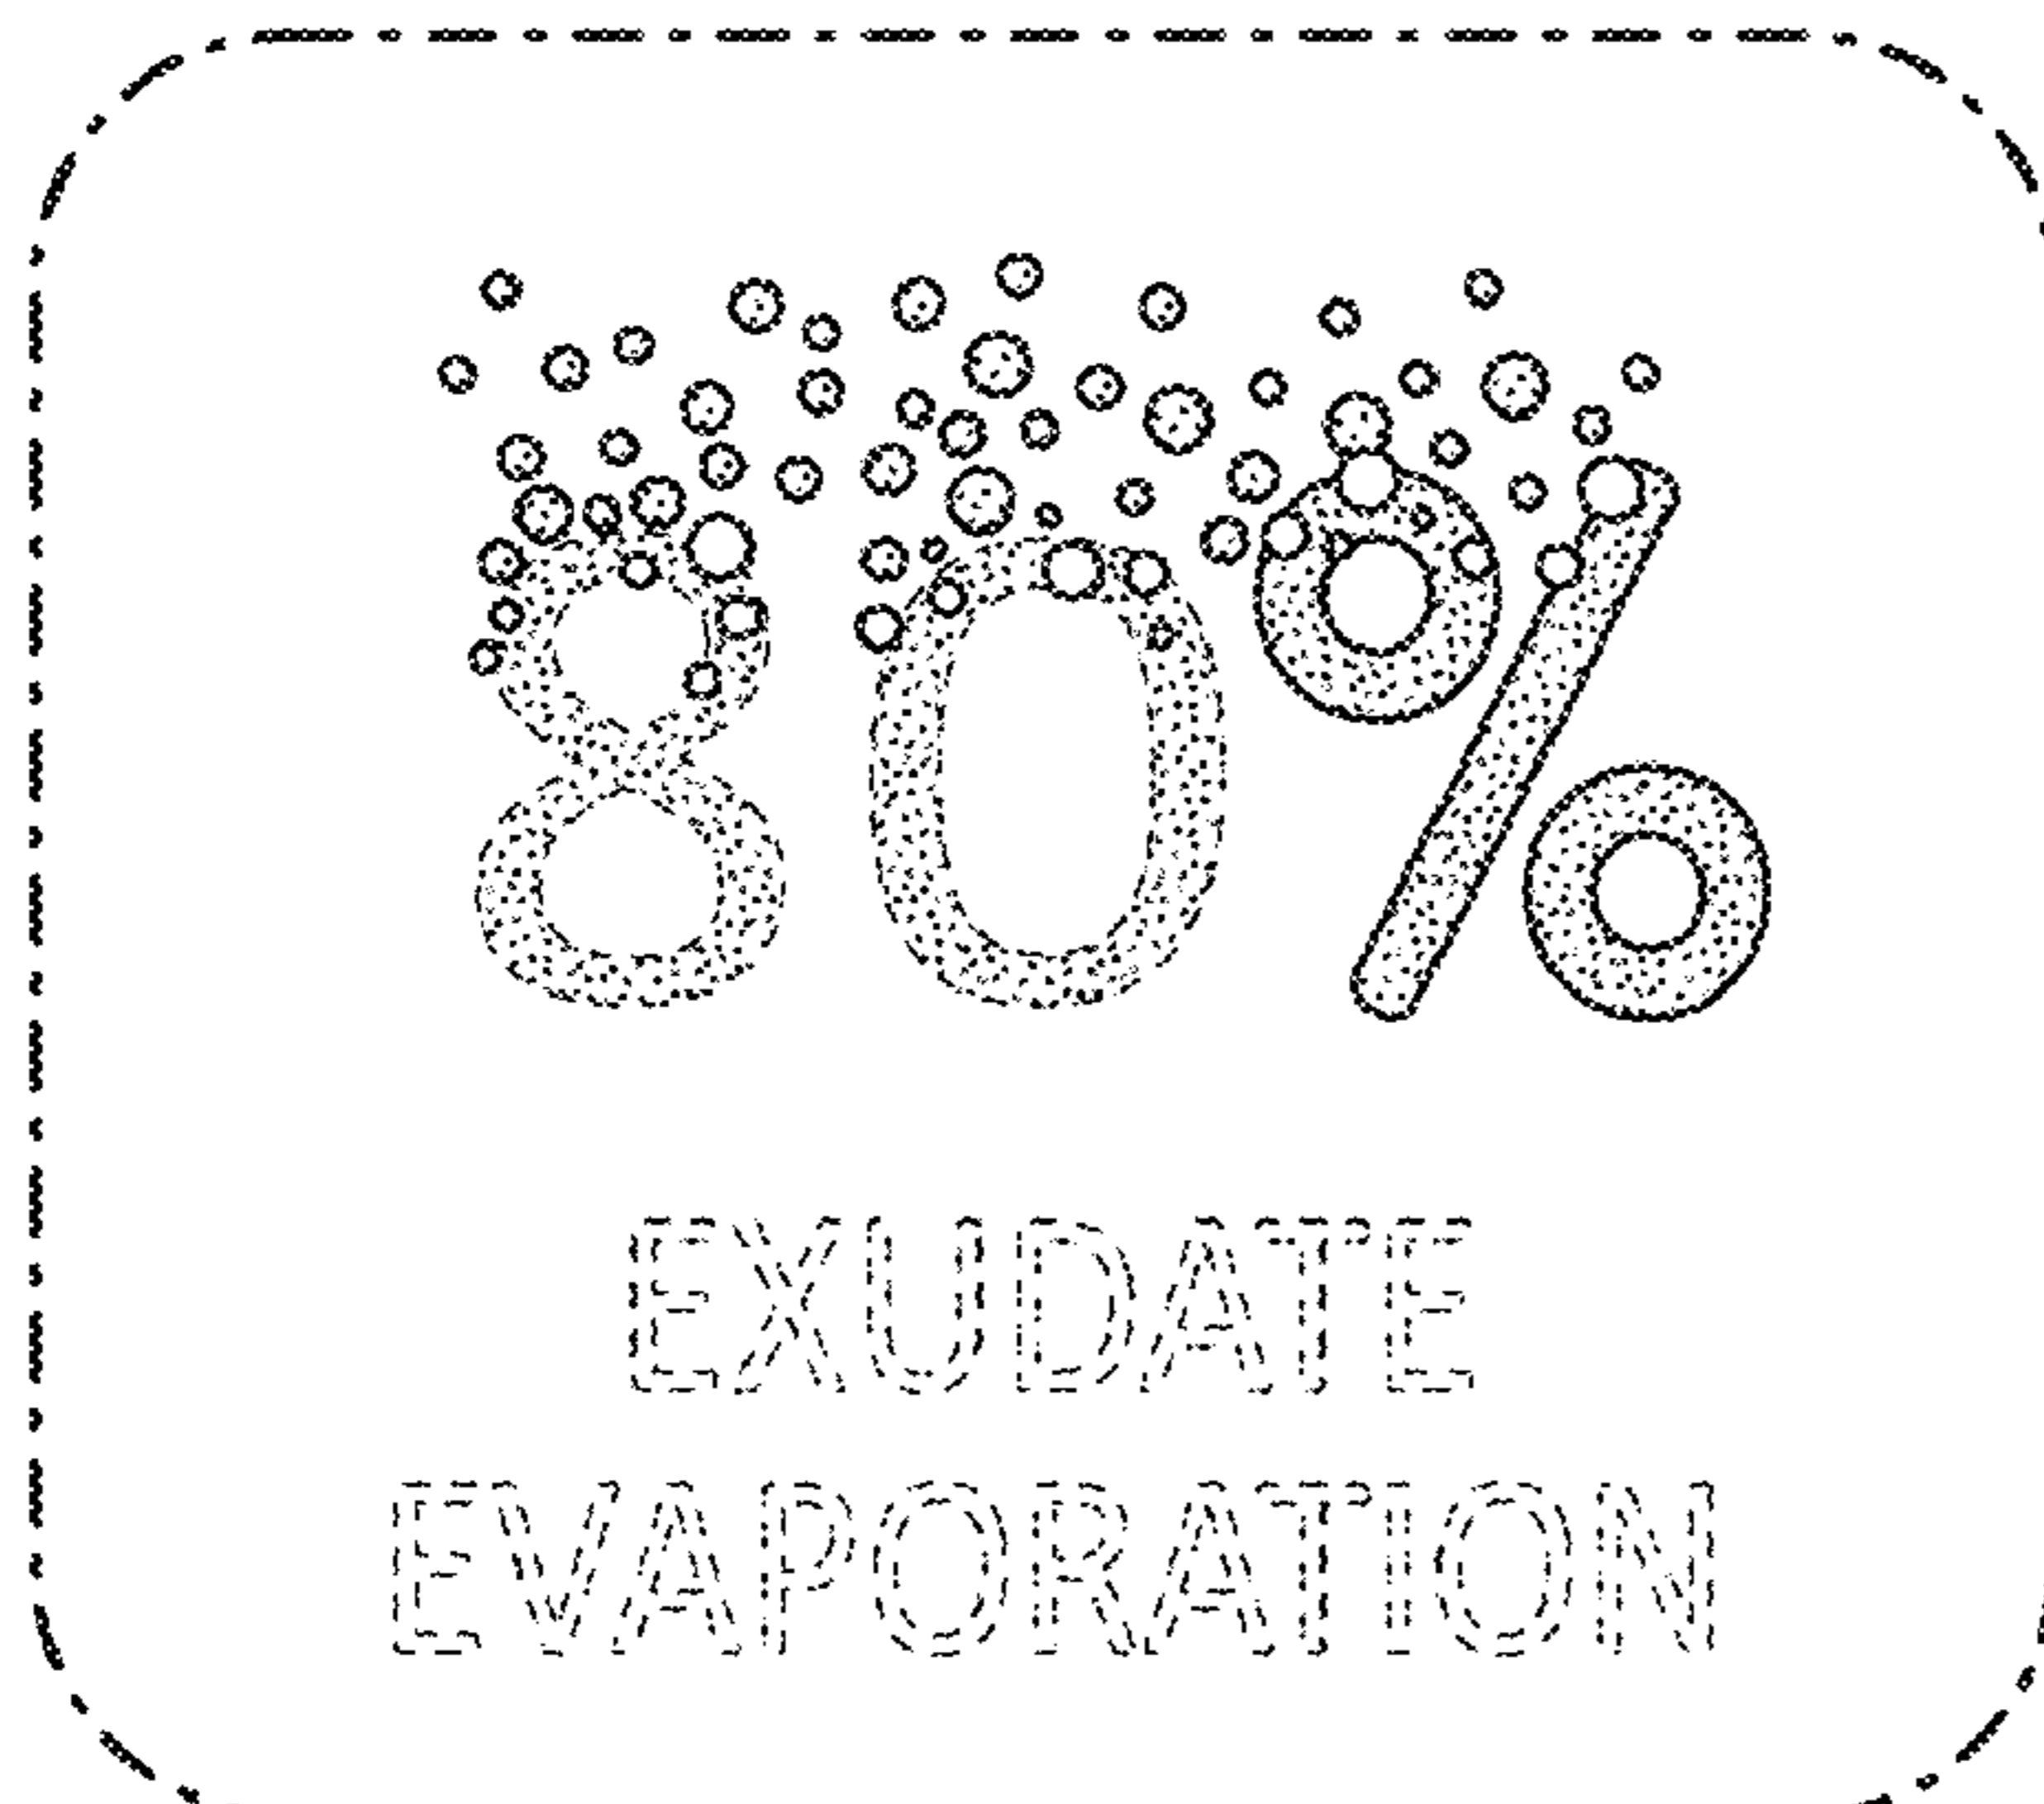

(56)

References Cited

U.S. PATENT DOCUMENTS

D888,762 S * 6/2020 Butcher D14/491
D888,826 S * 6/2020 Luca D20/22
2017/0119487 A1 5/2017 Binder et al.

OTHER PUBLICATIONS

Packaging Details for Pico Single Use Negative Pressure Wound Therapy System (#66801363/Barcode No. 5000223480806), [date unknown], in 1 page.

Smith & Nephew, "PICO Single Use Negative Pressure Wound Therapy System", spiral booklet, Mar. 2011, in 7 pages.

* cited by examiner

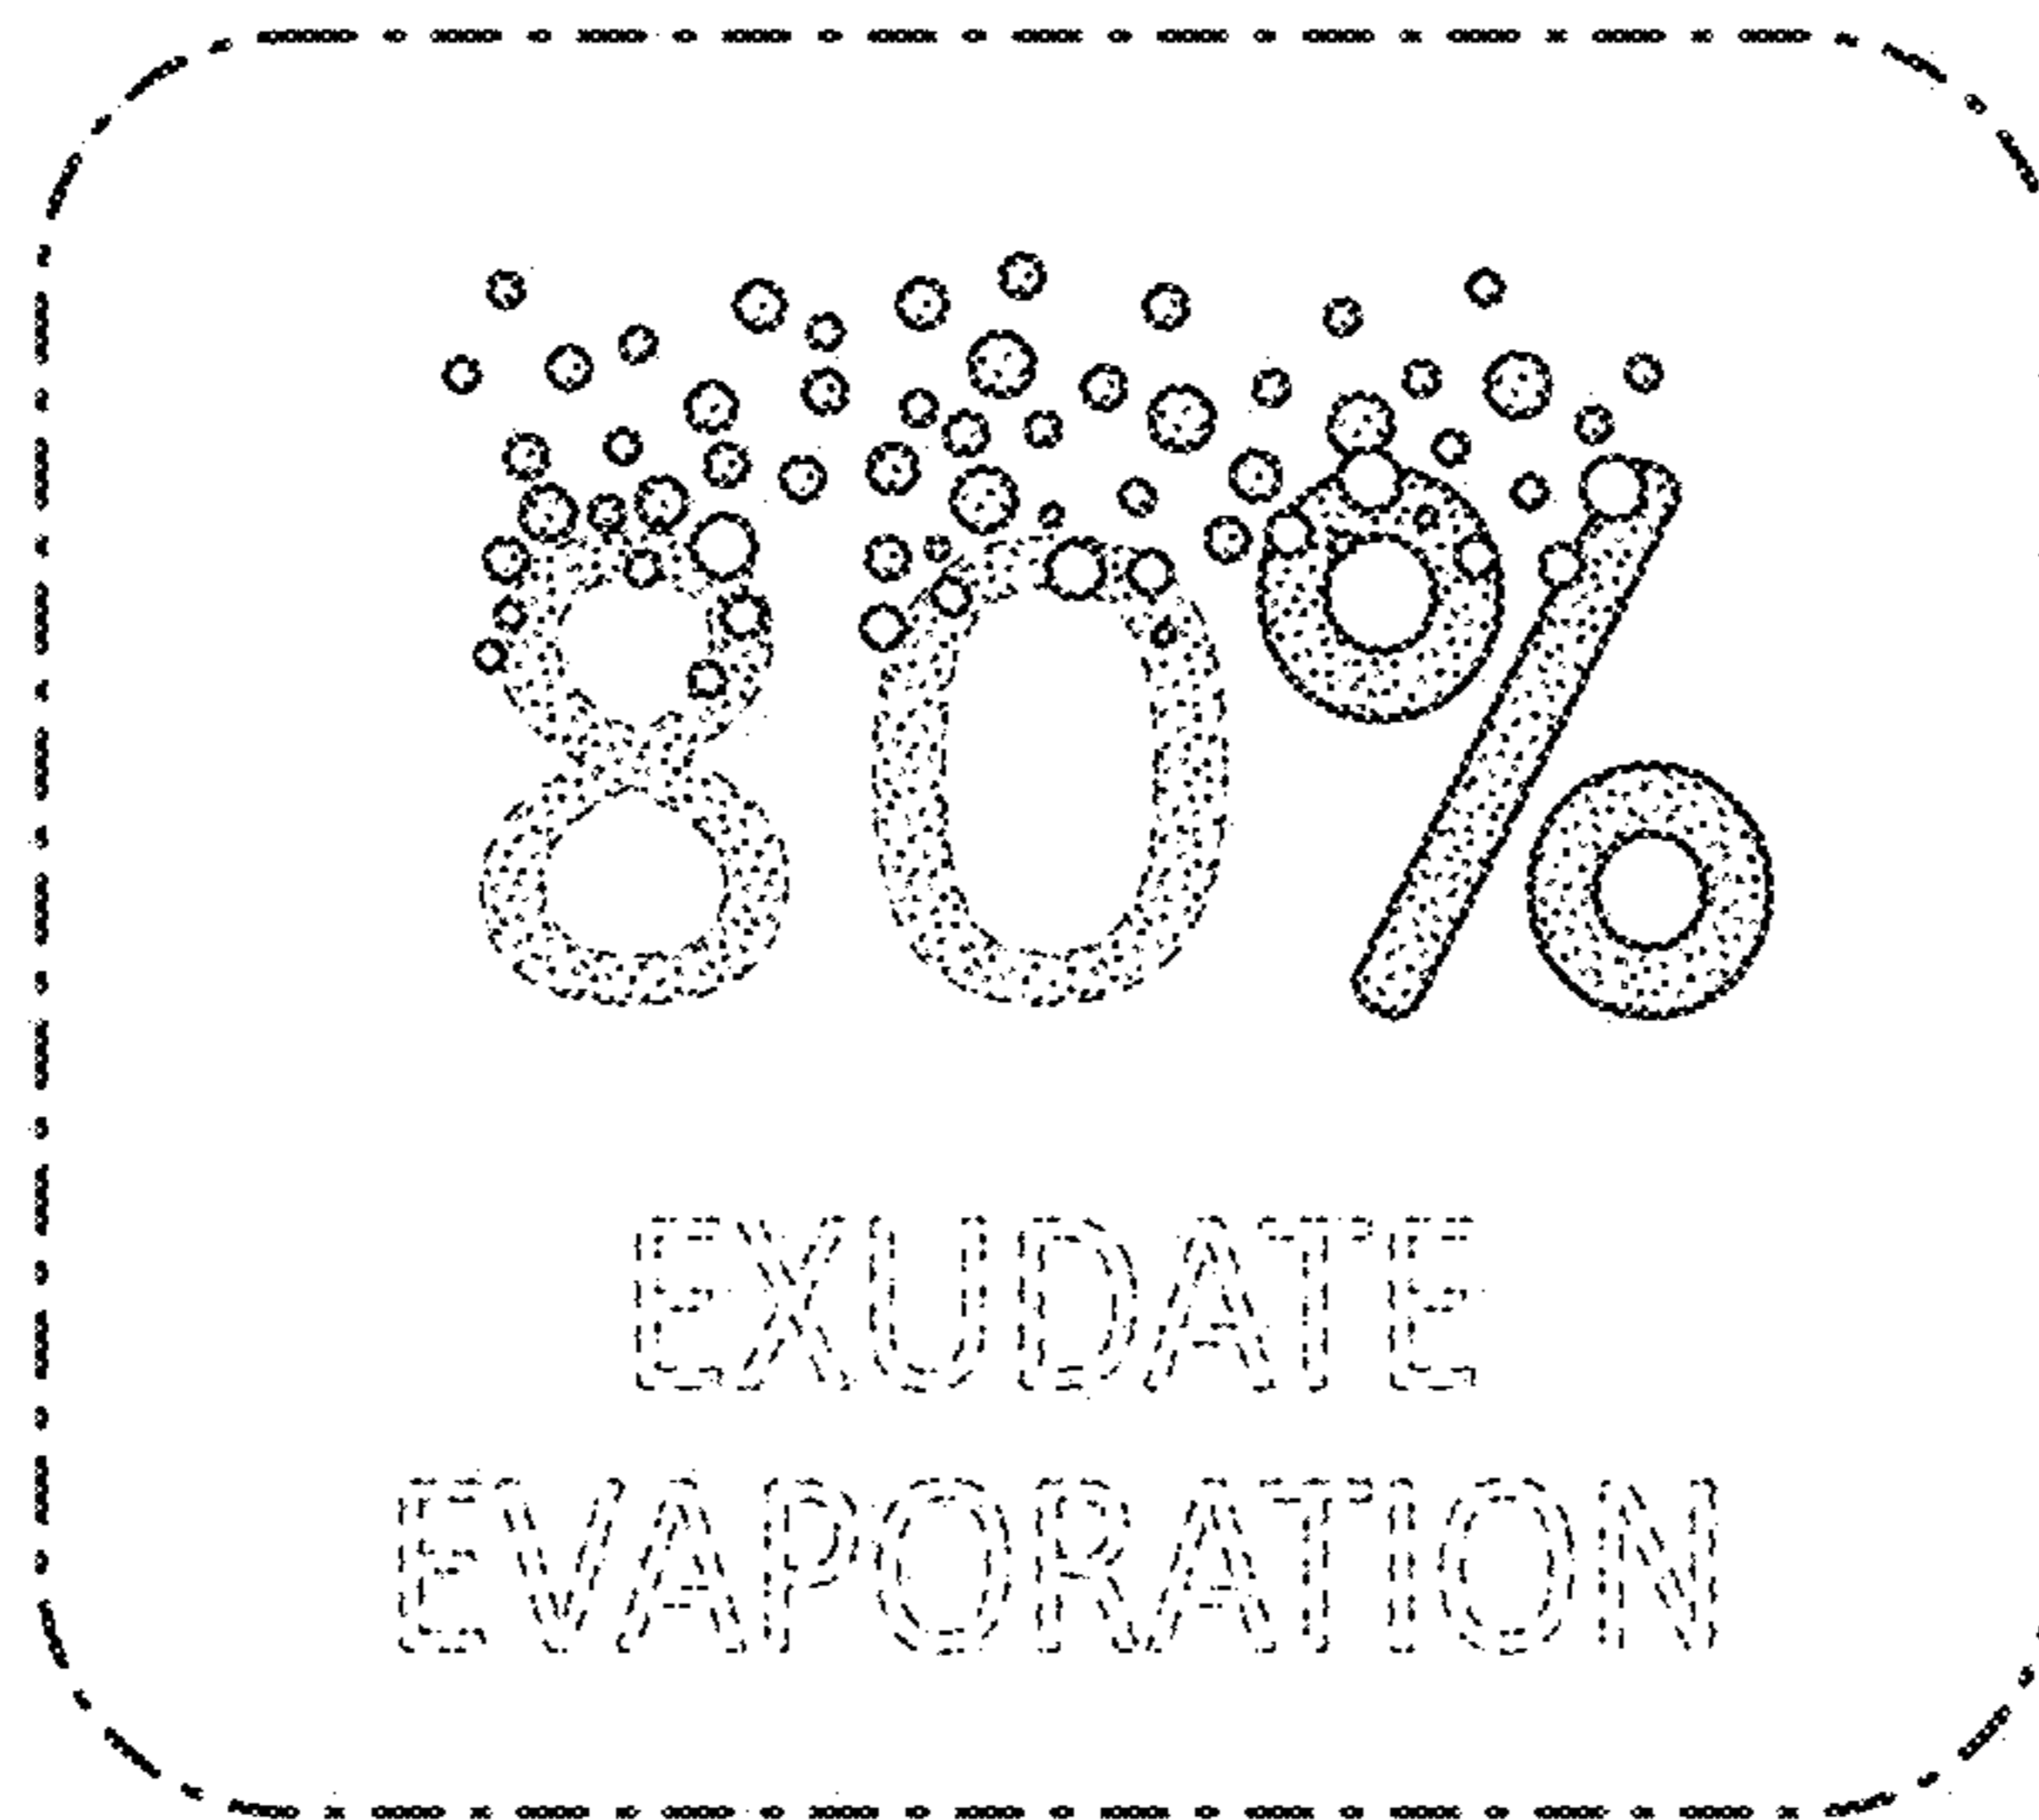


FIG. 1

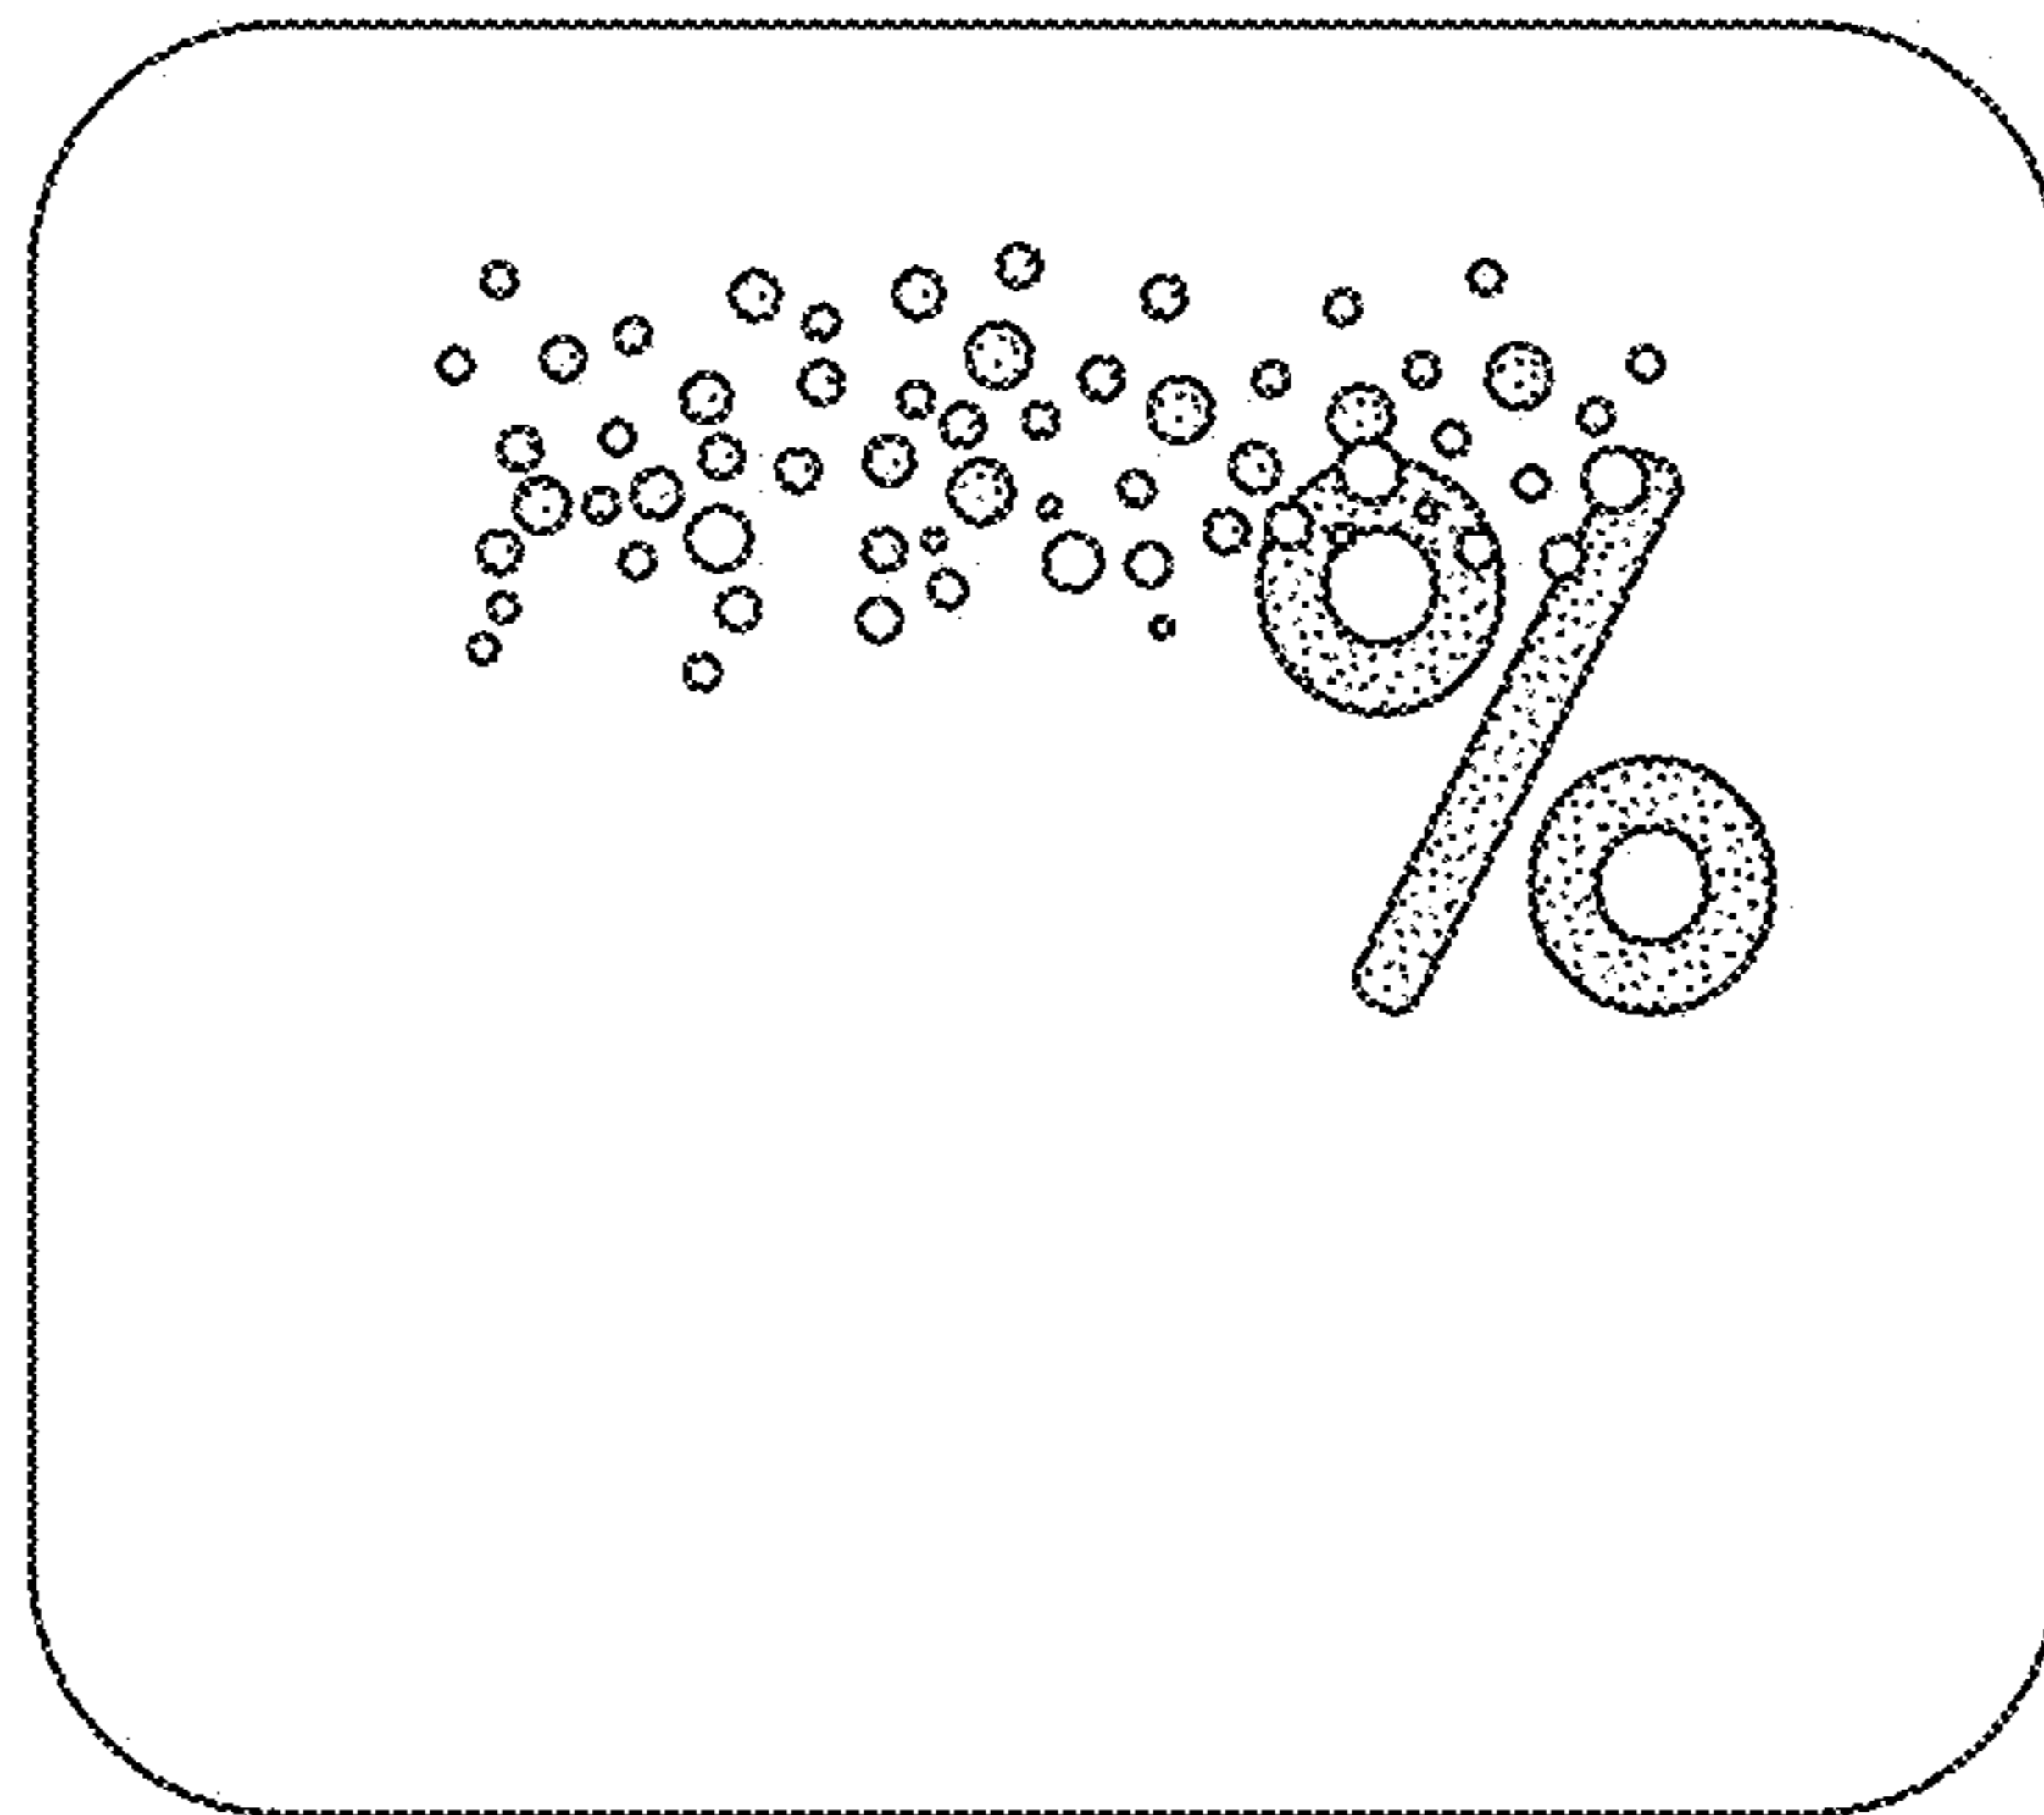


FIG. 2

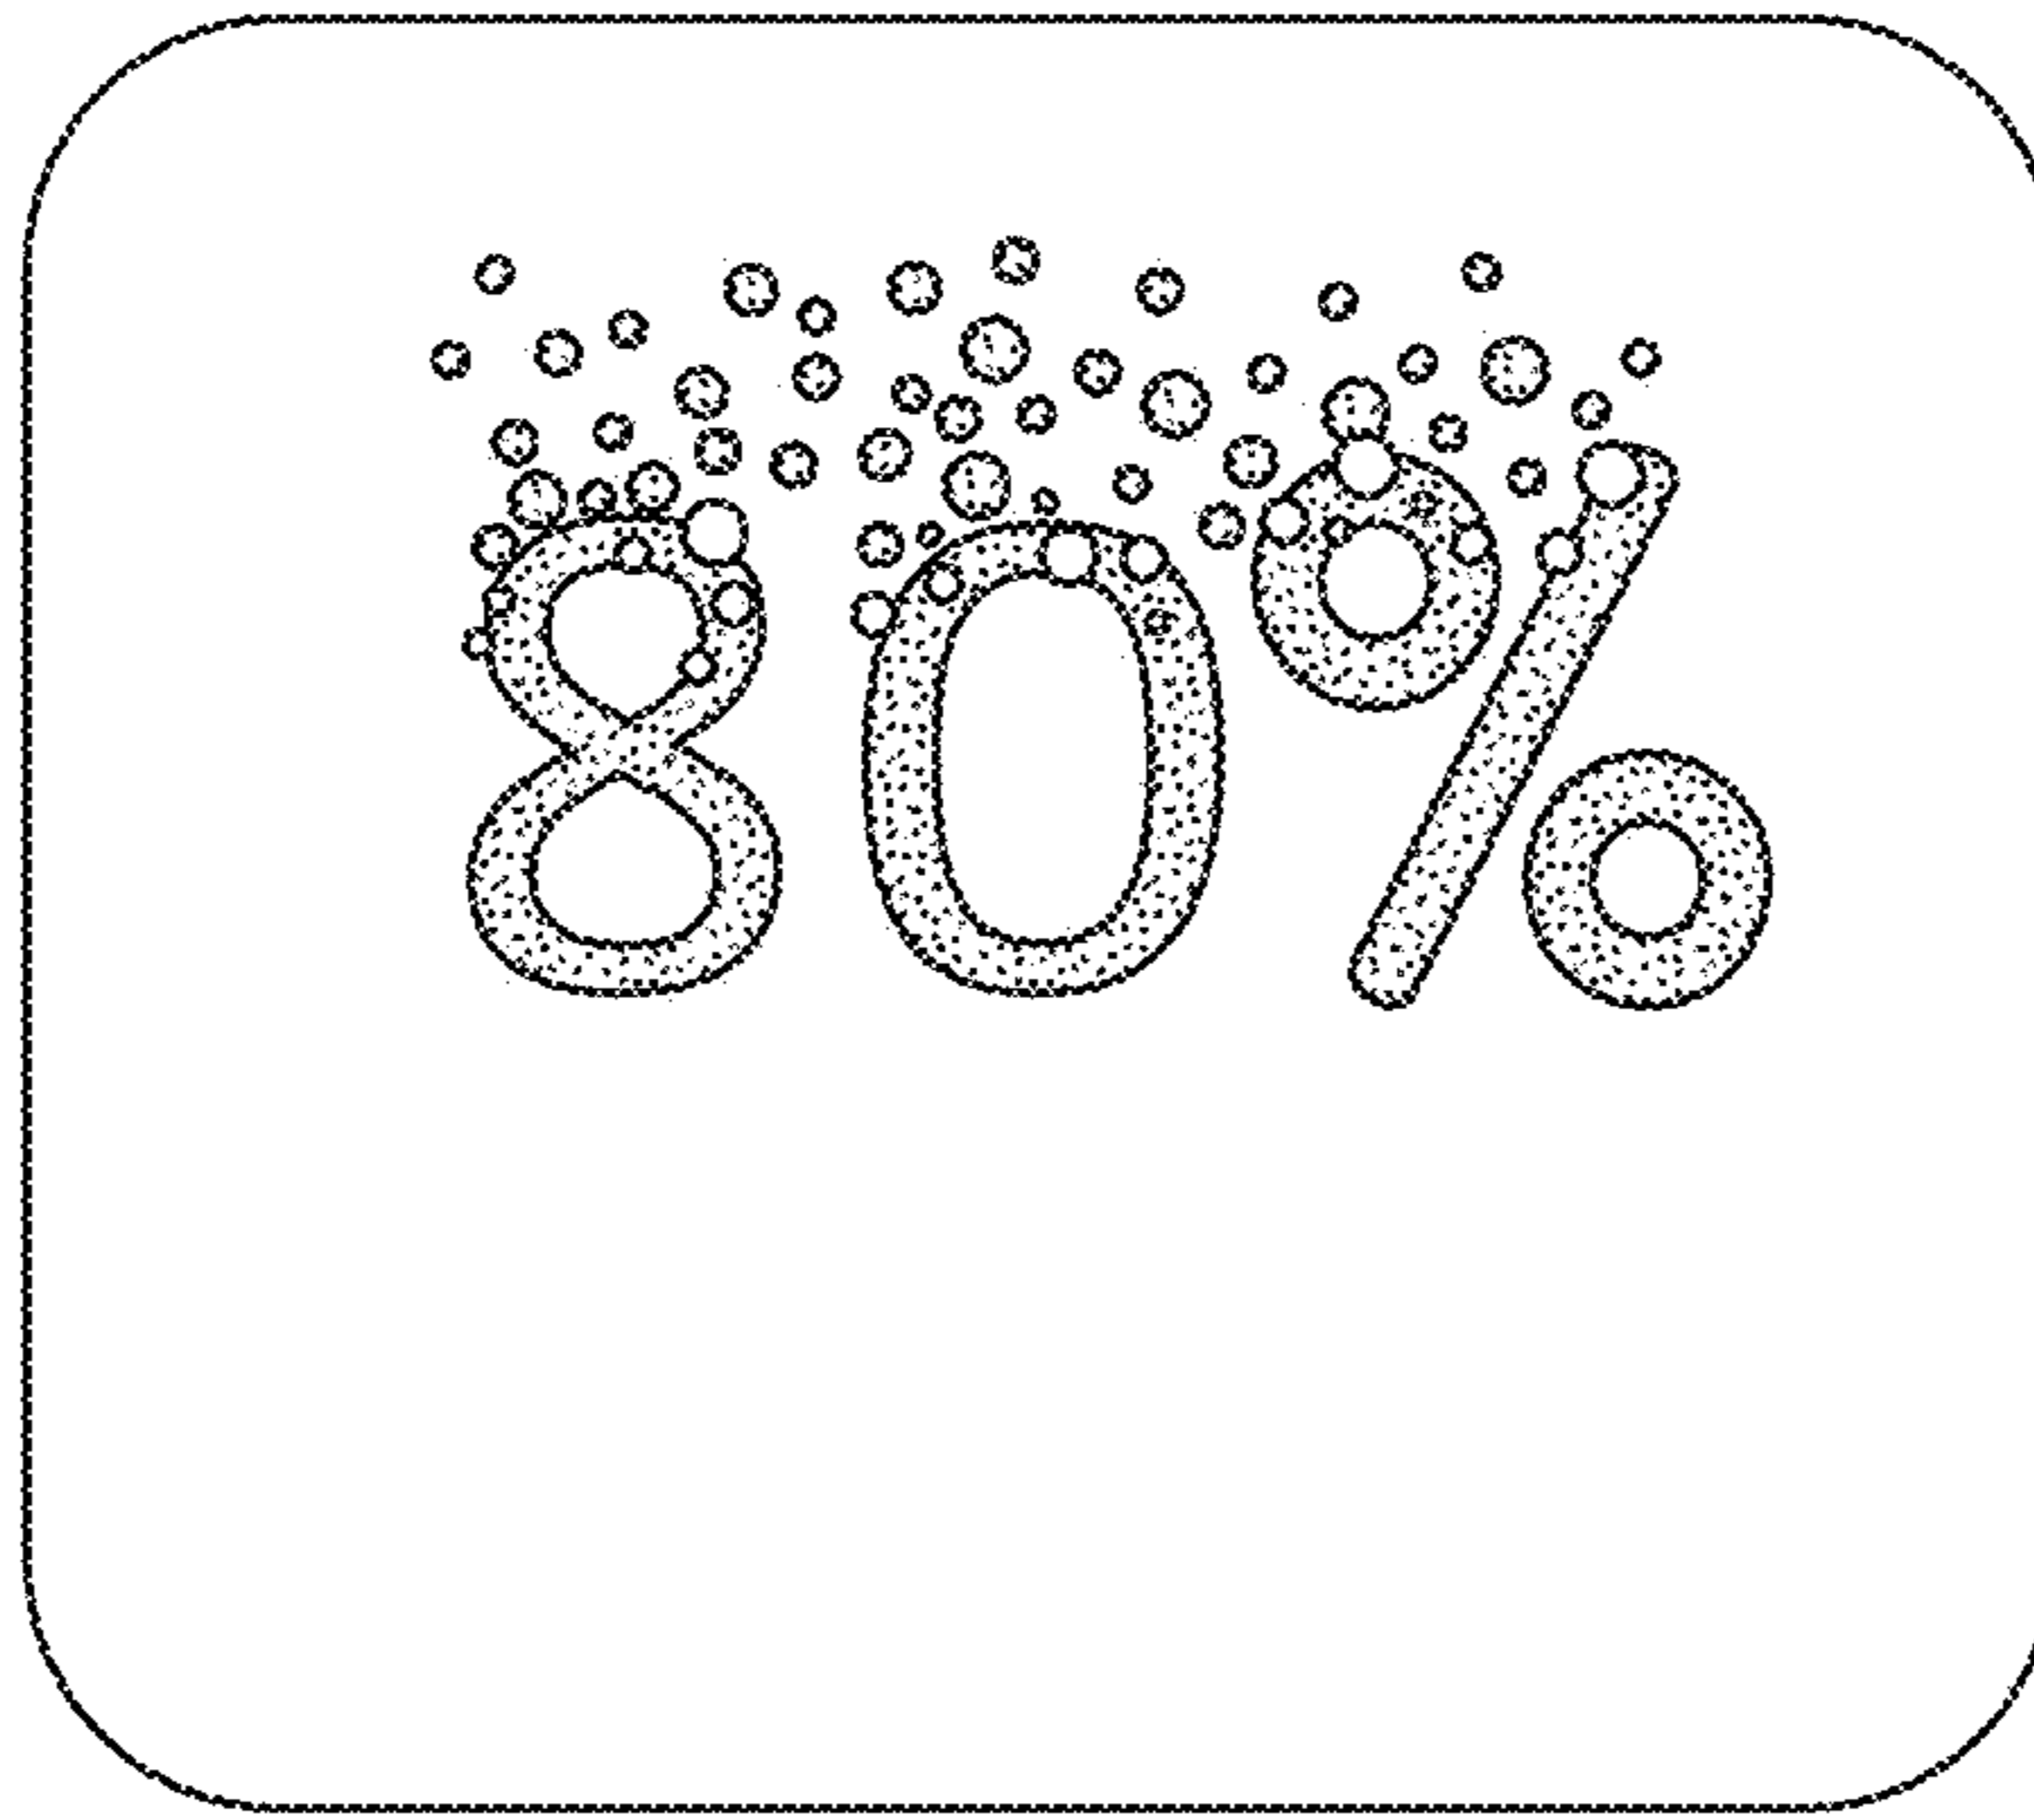


FIG. 3