



US00D938522S

(12) **United States Design Patent**  
**Flatt et al.**

(10) **Patent No.:** **US D938,522 S**

(45) **Date of Patent:** **\*\* Dec. 14, 2021**

(54) **LABEL**

(71) Applicants: **Alexander Flatt**, Norwich (GB);  
**Samuel John Mortimer**, Hull (GB);  
**Mark Parling**, Hull (GB); **Richard Thorpe**, Hull (GB)

(72) Inventors: **Alexander Flatt**, Norwich (GB);  
**Samuel John Mortimer**, Hull (GB);  
**Mark Parling**, Hull (GB); **Richard Thorpe**, Hull (GB)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/661,666**

(22) Filed: **Aug. 29, 2018**

(51) **LOC (13) Cl.** ..... **19-08**

(52) **U.S. Cl.**  
USPC ..... **D20/27**

(58) **Field of Classification Search**  
USPC ..... D9/550, 563; D10/46, 47, 52, 104.1,  
D10/104.2; D14/490, 491; D19/1, 2, 3,  
D19/4, 5, 6, 7, 8, 9, 10, 11, 12; D20/10,  
D20/11, 18, 22, 23, 24, 25, 26, 27, 28,  
D20/29, 40, 43, 44, 49  
CPC ..... G09F 1/00; G09F 1/04; G09F 3/00; G09F  
3/005; G09F 3/0288; G09F 3/0289; G09F  
3/02; G09F 3/04; G09F 3/06; G09F 3/08;  
G09F 3/10; G06K 19/0776

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D425,934 S \* 5/2000 Kunkler ..... D19/11  
D445,445 S \* 7/2001 Kane ..... D17/20  
D659,158 S \* 5/2012 Clymer ..... D14/488  
D677,728 S \* 3/2013 Self ..... D19/60  
D677,729 S \* 3/2013 Self ..... D19/60  
D696,283 S \* 12/2013 Schwengler ..... D14/486  
D701,867 S \* 4/2014 Thompson ..... D14/485  
D780,200 S \* 2/2017 Chaudhri ..... D14/486

D782,497 S \* 3/2017 Barry ..... D14/485  
D813,904 S \* 3/2018 Okutsu ..... D14/488  
D834,063 S \* 11/2018 Stray ..... D14/491  
D851,678 S \* 6/2019 Clymer ..... D14/492  
D873,858 S \* 1/2020 Fiol ..... D14/495  
D885,434 S \* 5/2020 Lee ..... D14/492  
D887,443 S \* 6/2020 Amini ..... D14/491

(Continued)

**FOREIGN PATENT DOCUMENTS**

WO WO 2013/171585 11/2013  
WO WO 2016/103033 6/2016

**OTHER PUBLICATIONS**

Packaging for Pico Single Use Negative Pressure Wound Therapy System (#66801363), [date unknown], in 2 pages.

(Continued)

*Primary Examiner* — Mary Ann Calabrese

*Assistant Examiner* — Catherine Ho

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57) **CLAIM**

The ornamental design for a label, as shown and described.

**DESCRIPTION**



FIG. 1 is a front view of the first embodiment of a label, showing my new design.

FIG. 2 is a front view of the second embodiment of a label, showing my new design; and,

FIG. 3 is a front view of the third embodiment of a label, showing my new design.

The dot-dash perimeter indicates the boundaries of the claim and forms no part thereof. The broken lines in the drawings form no part of the claimed design. The stippling seen in FIGS. 1-3 depicts surface indicia, which forms part of the claimed design.

**1 Claim, 3 Drawing Sheets**

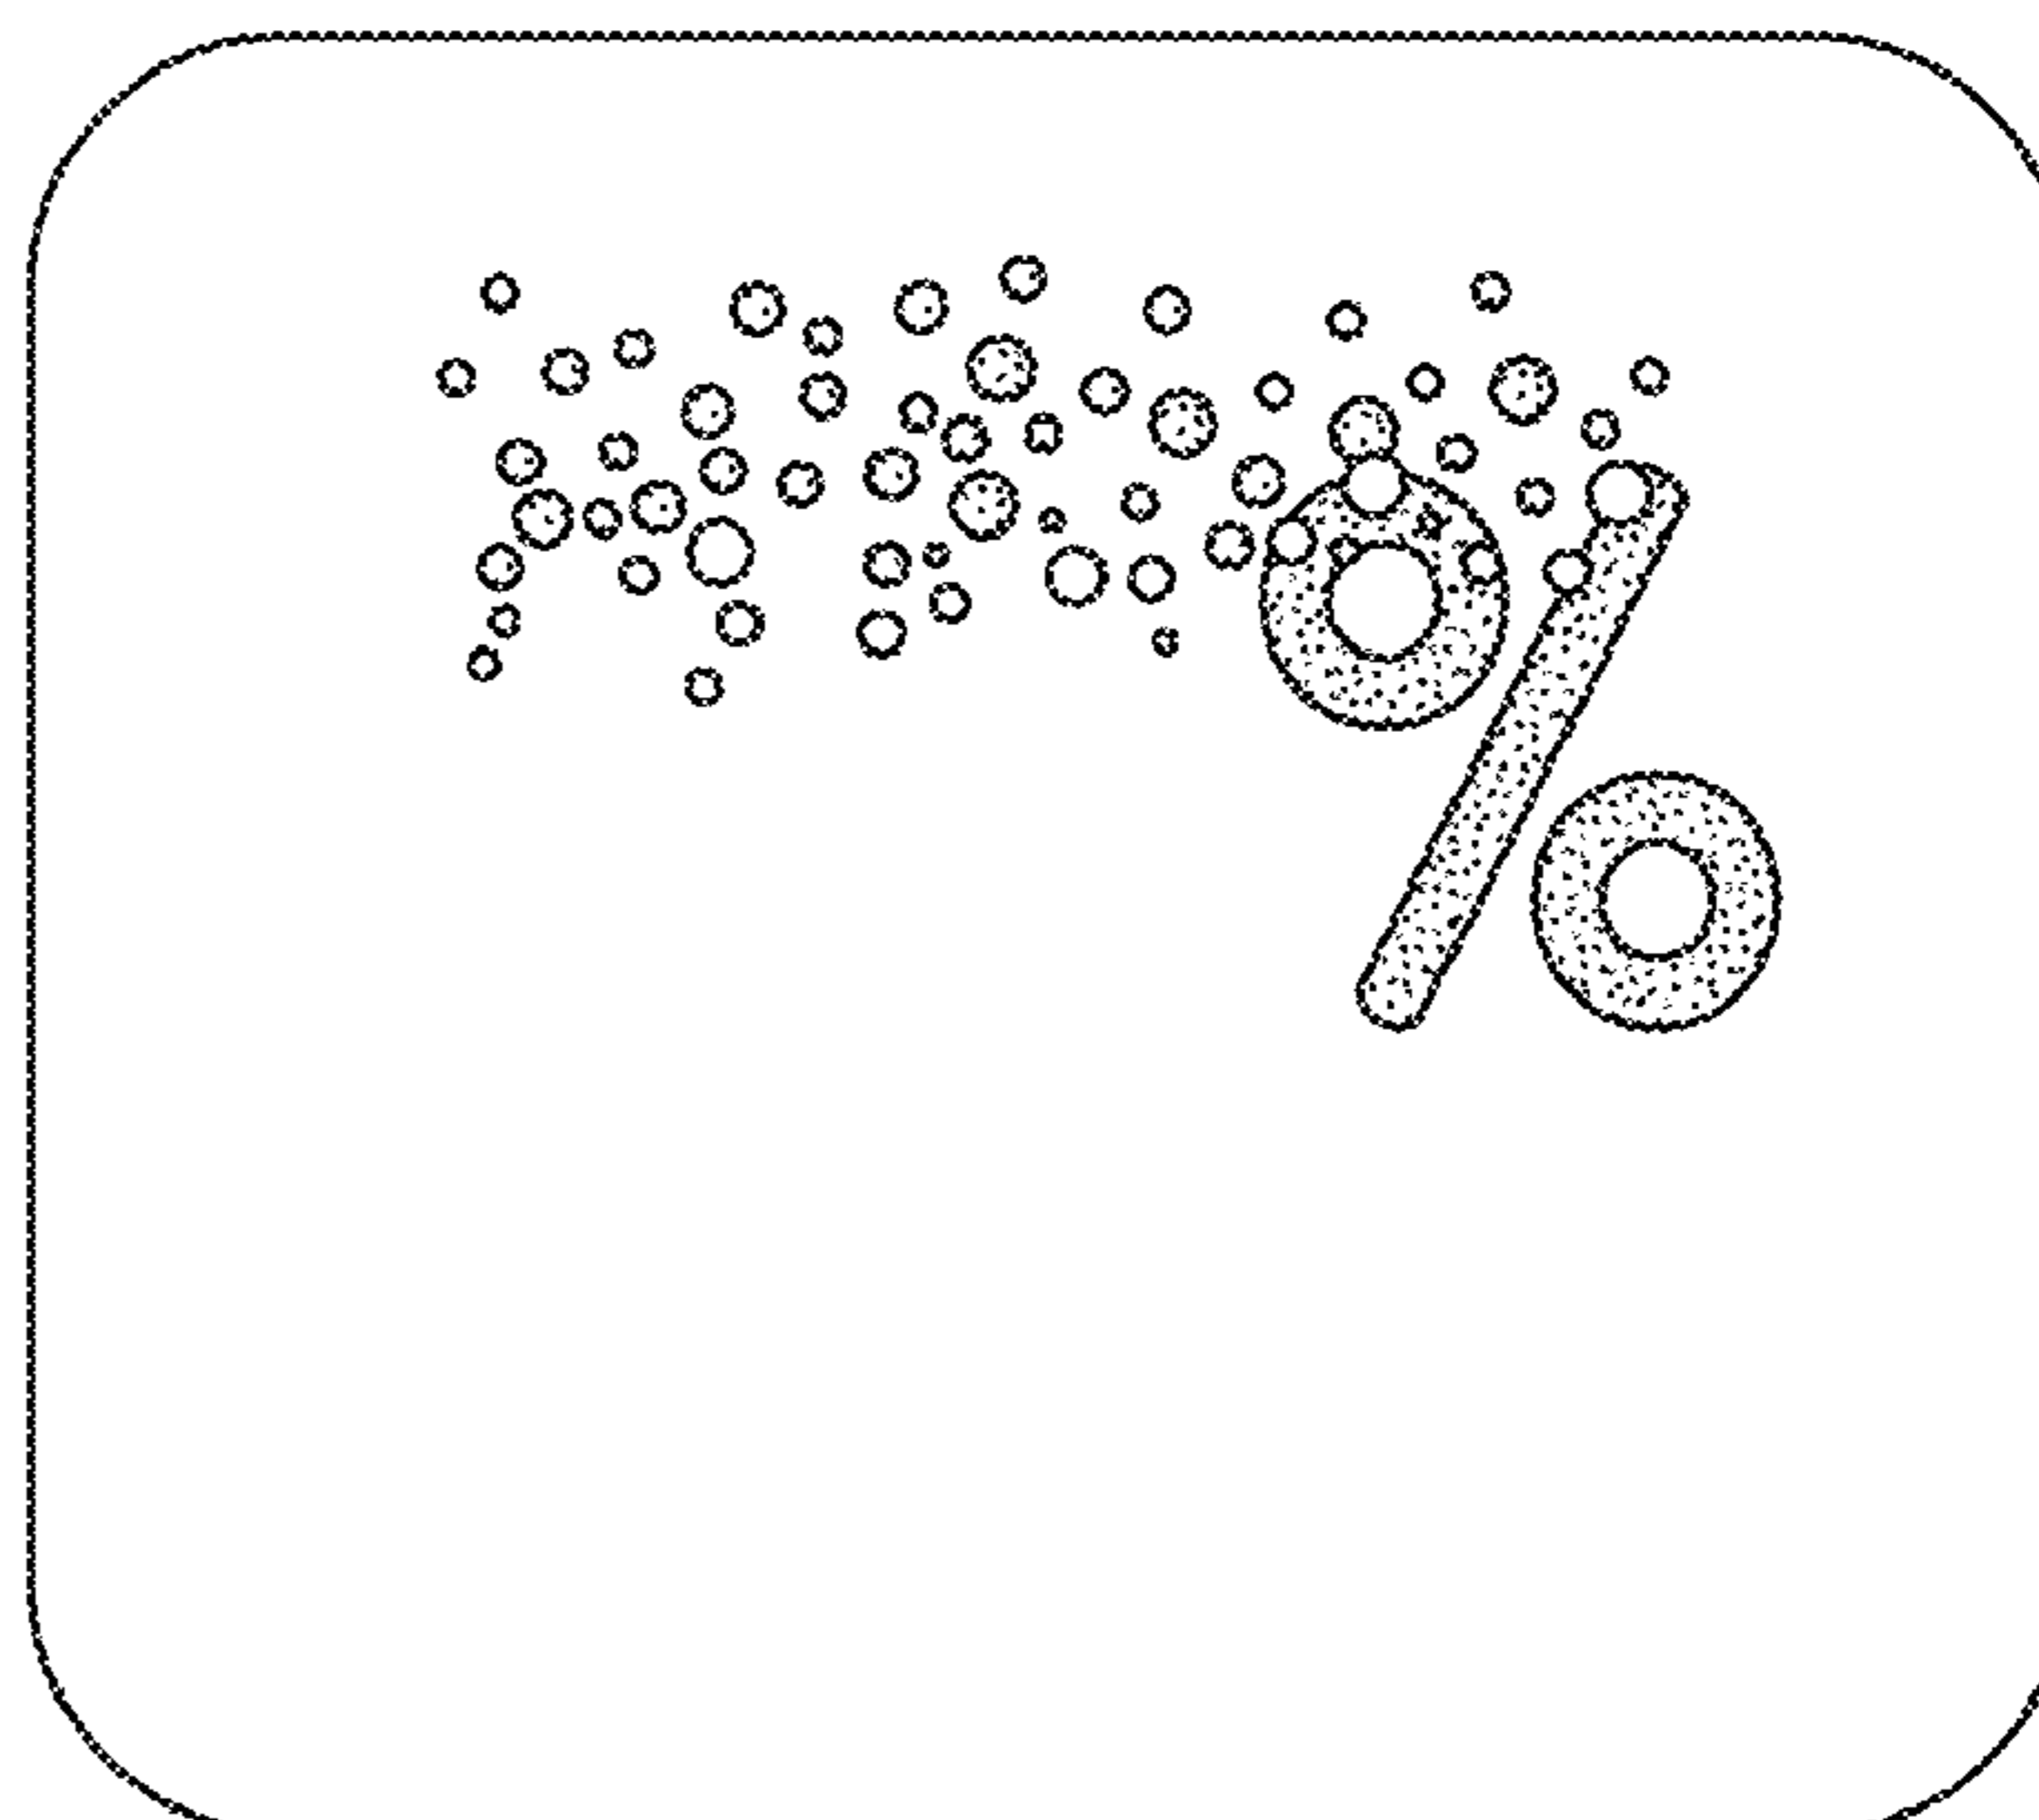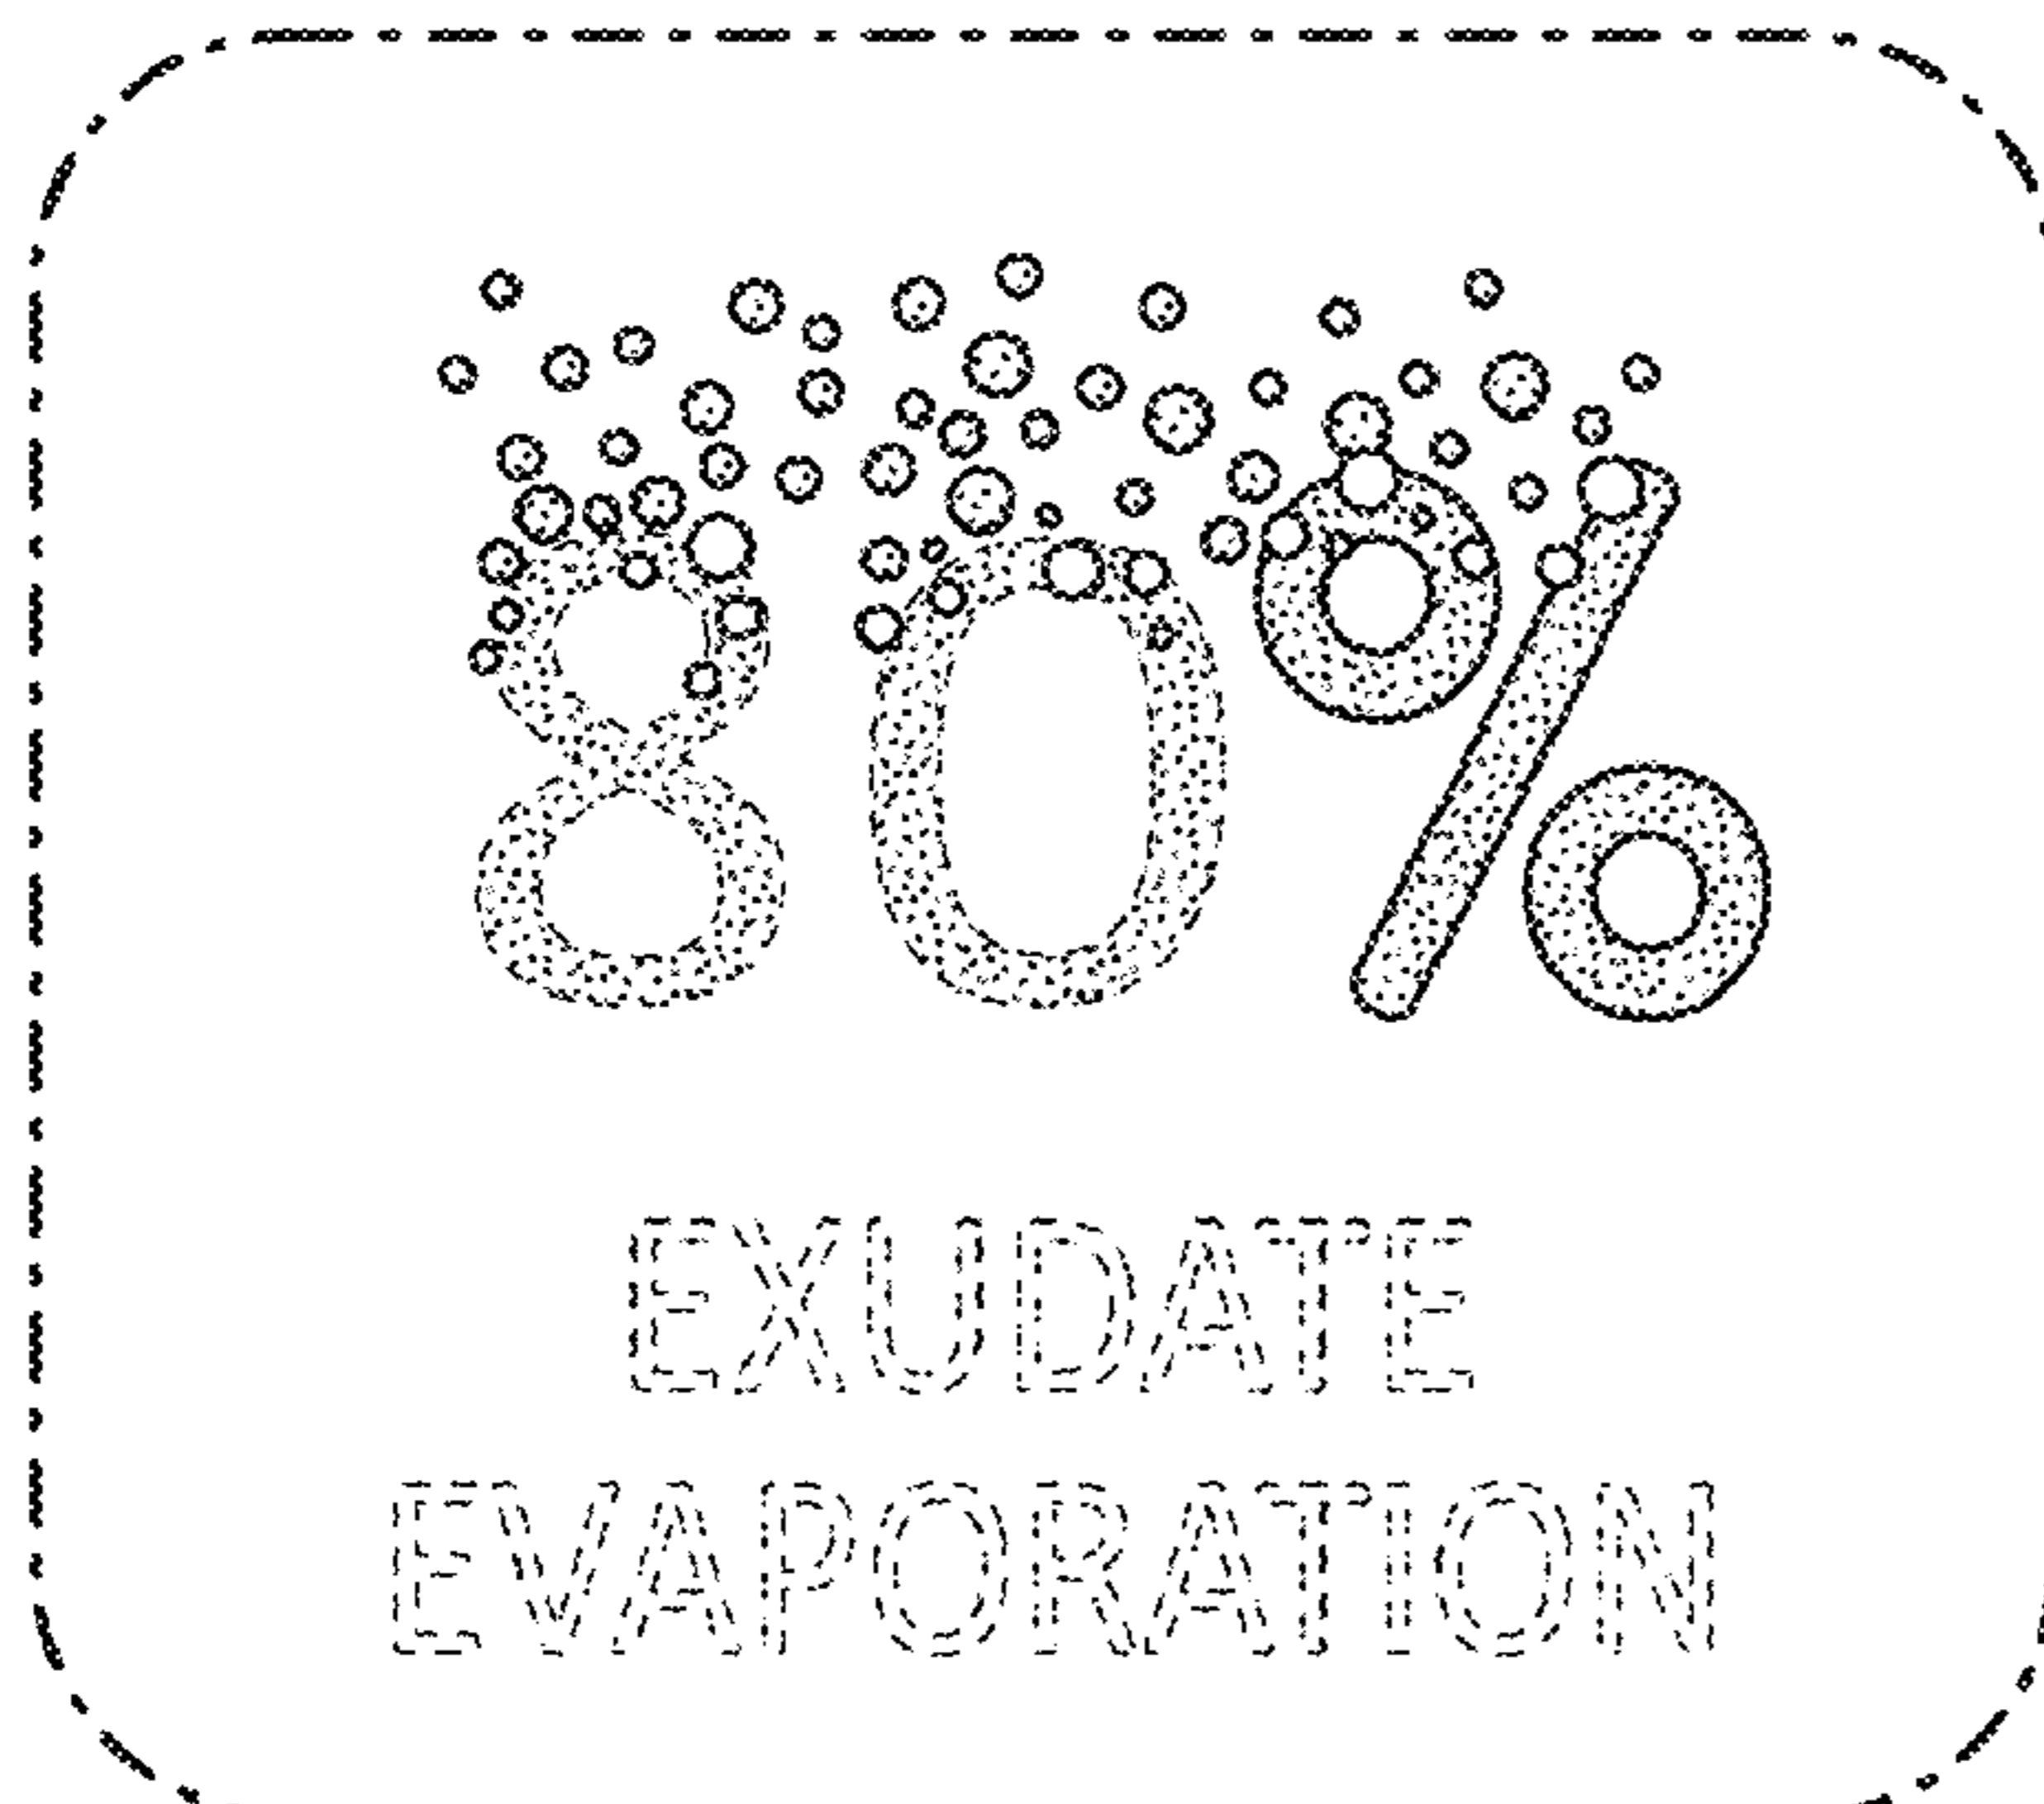

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D888,762 S \* 6/2020 Butcher ..... D14/491  
D888,826 S \* 6/2020 Luca ..... D20/22  
2017/0119487 A1 5/2017 Binder et al.

OTHER PUBLICATIONS

Packaging Details for Pico Single Use Negative Pressure Wound Therapy System (#66801363/Barcode No. 5000223480806), [date unknown], in 1 page.

Smith & Nephew, "PICO Single Use Negative Pressure Wound Therapy System", spiral booklet, Mar. 2011, in 7 pages.

\* cited by examiner

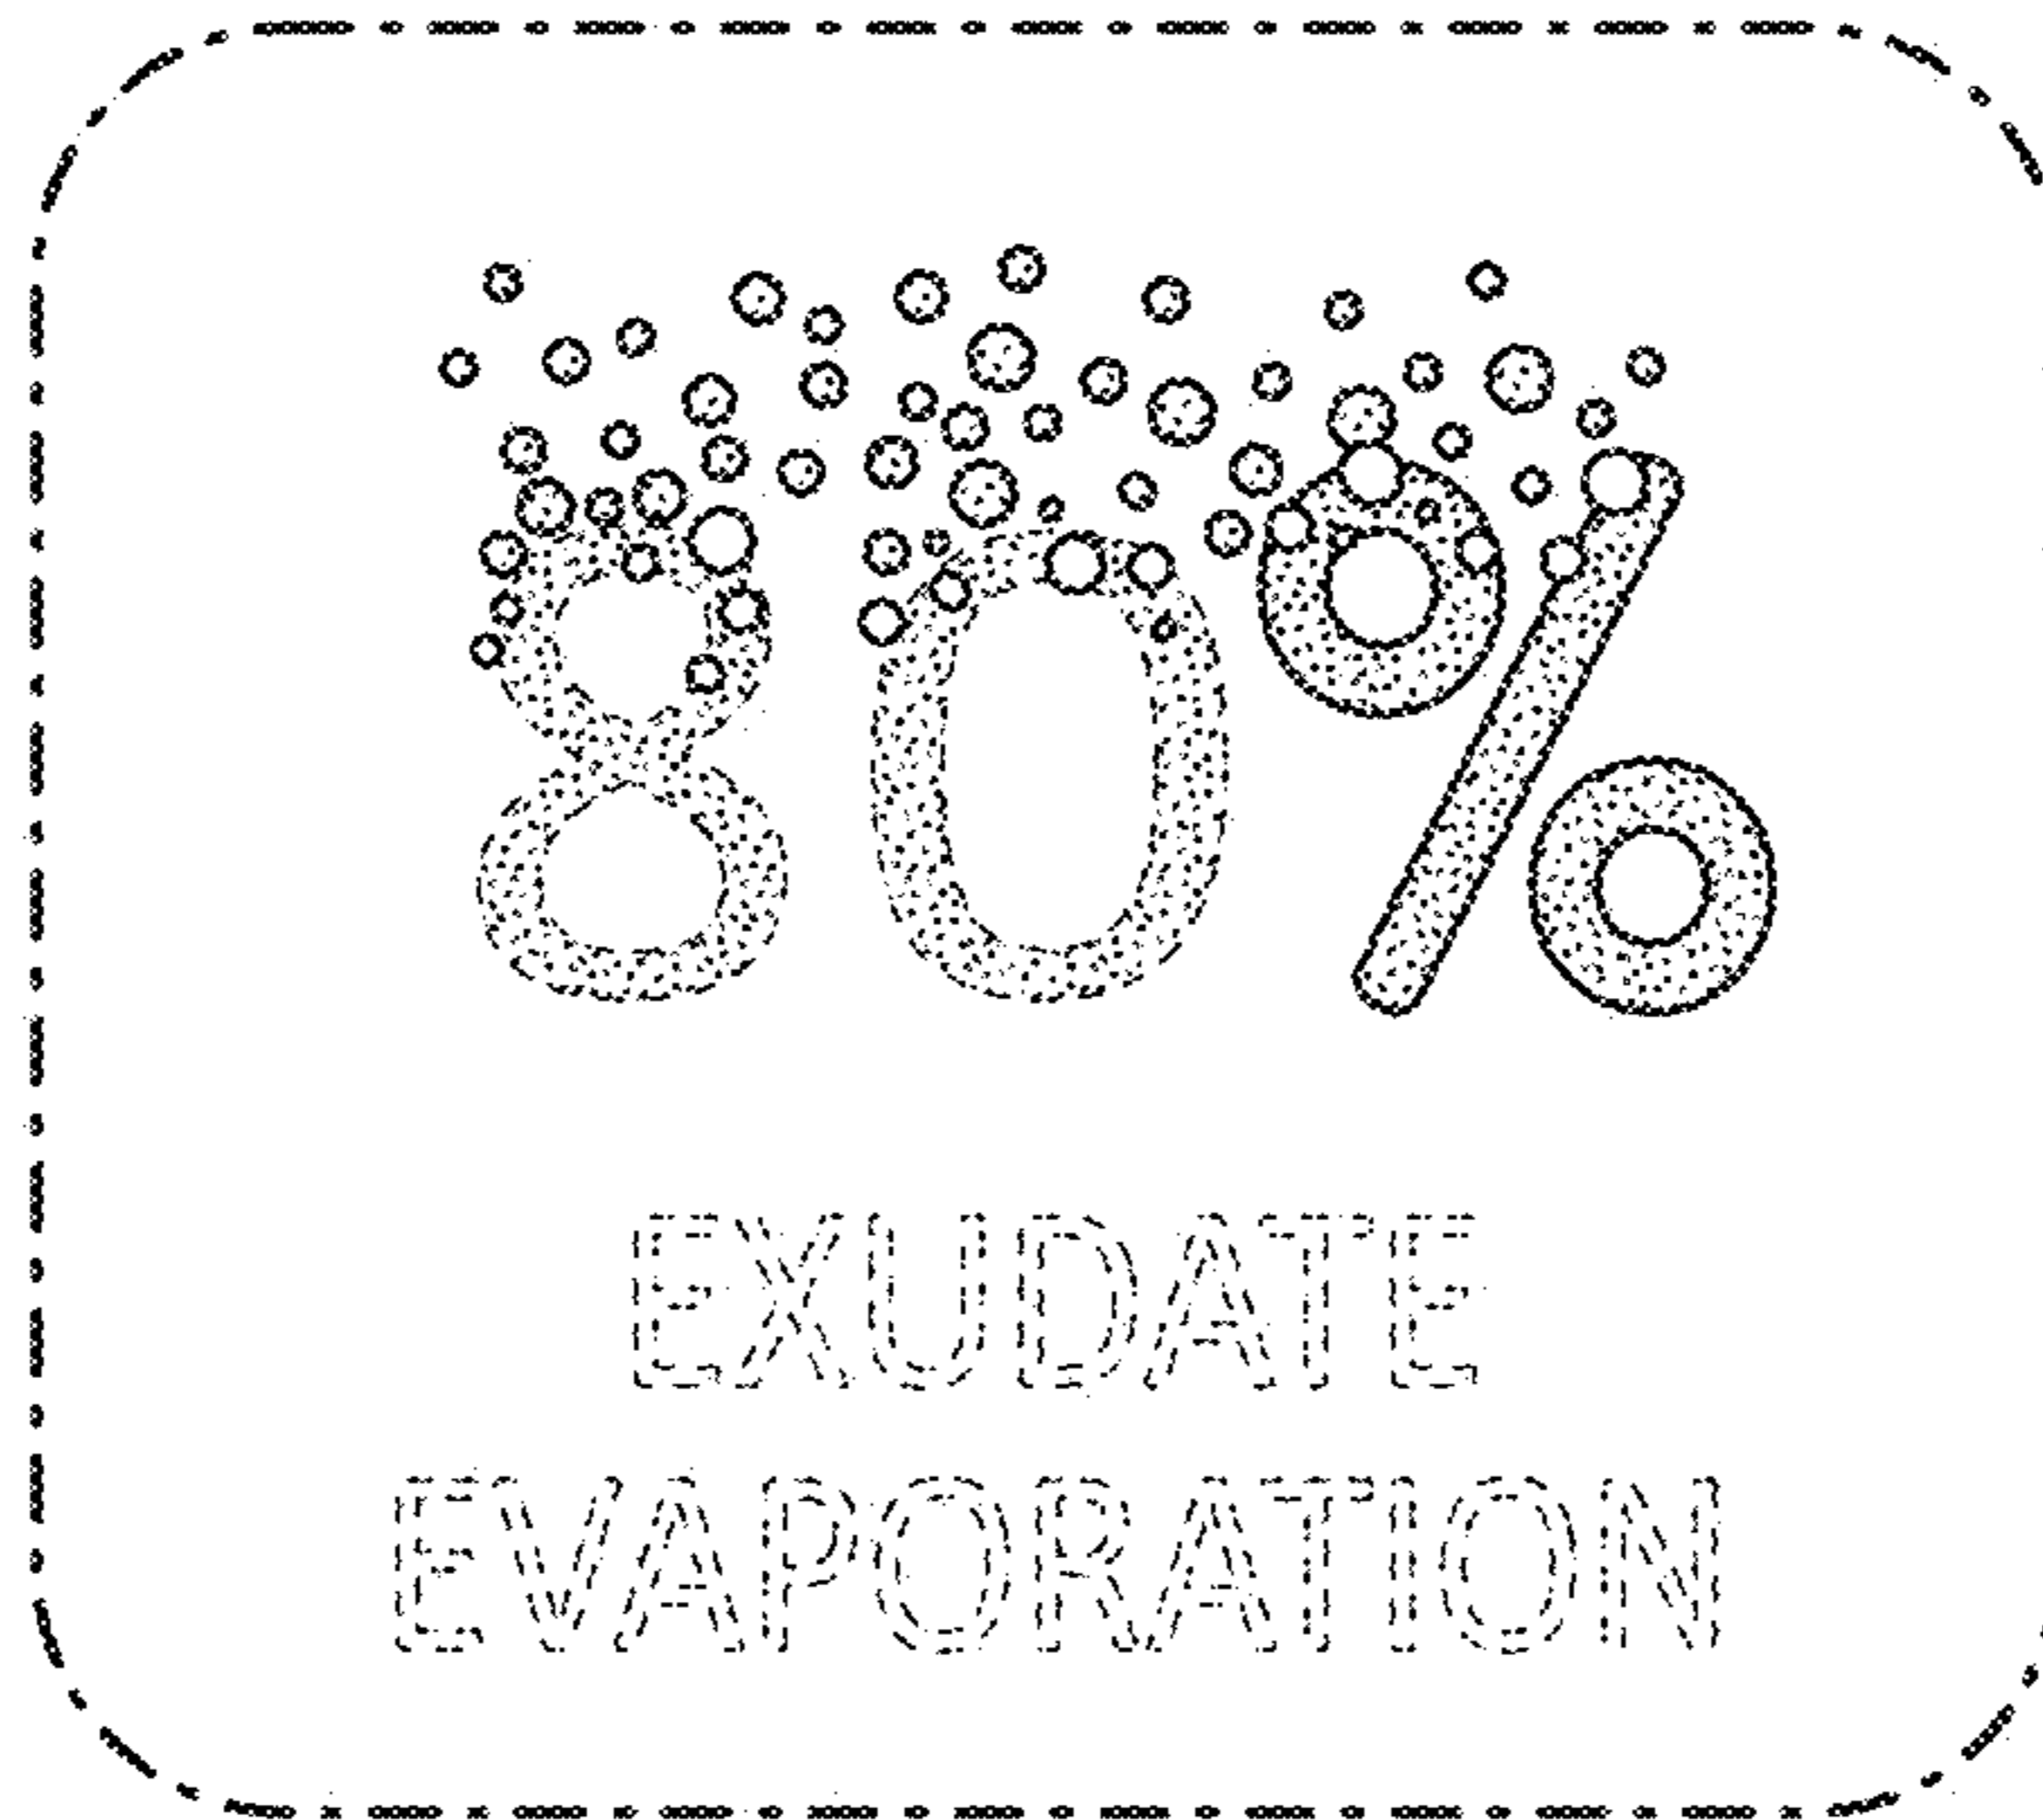


FIG. 1

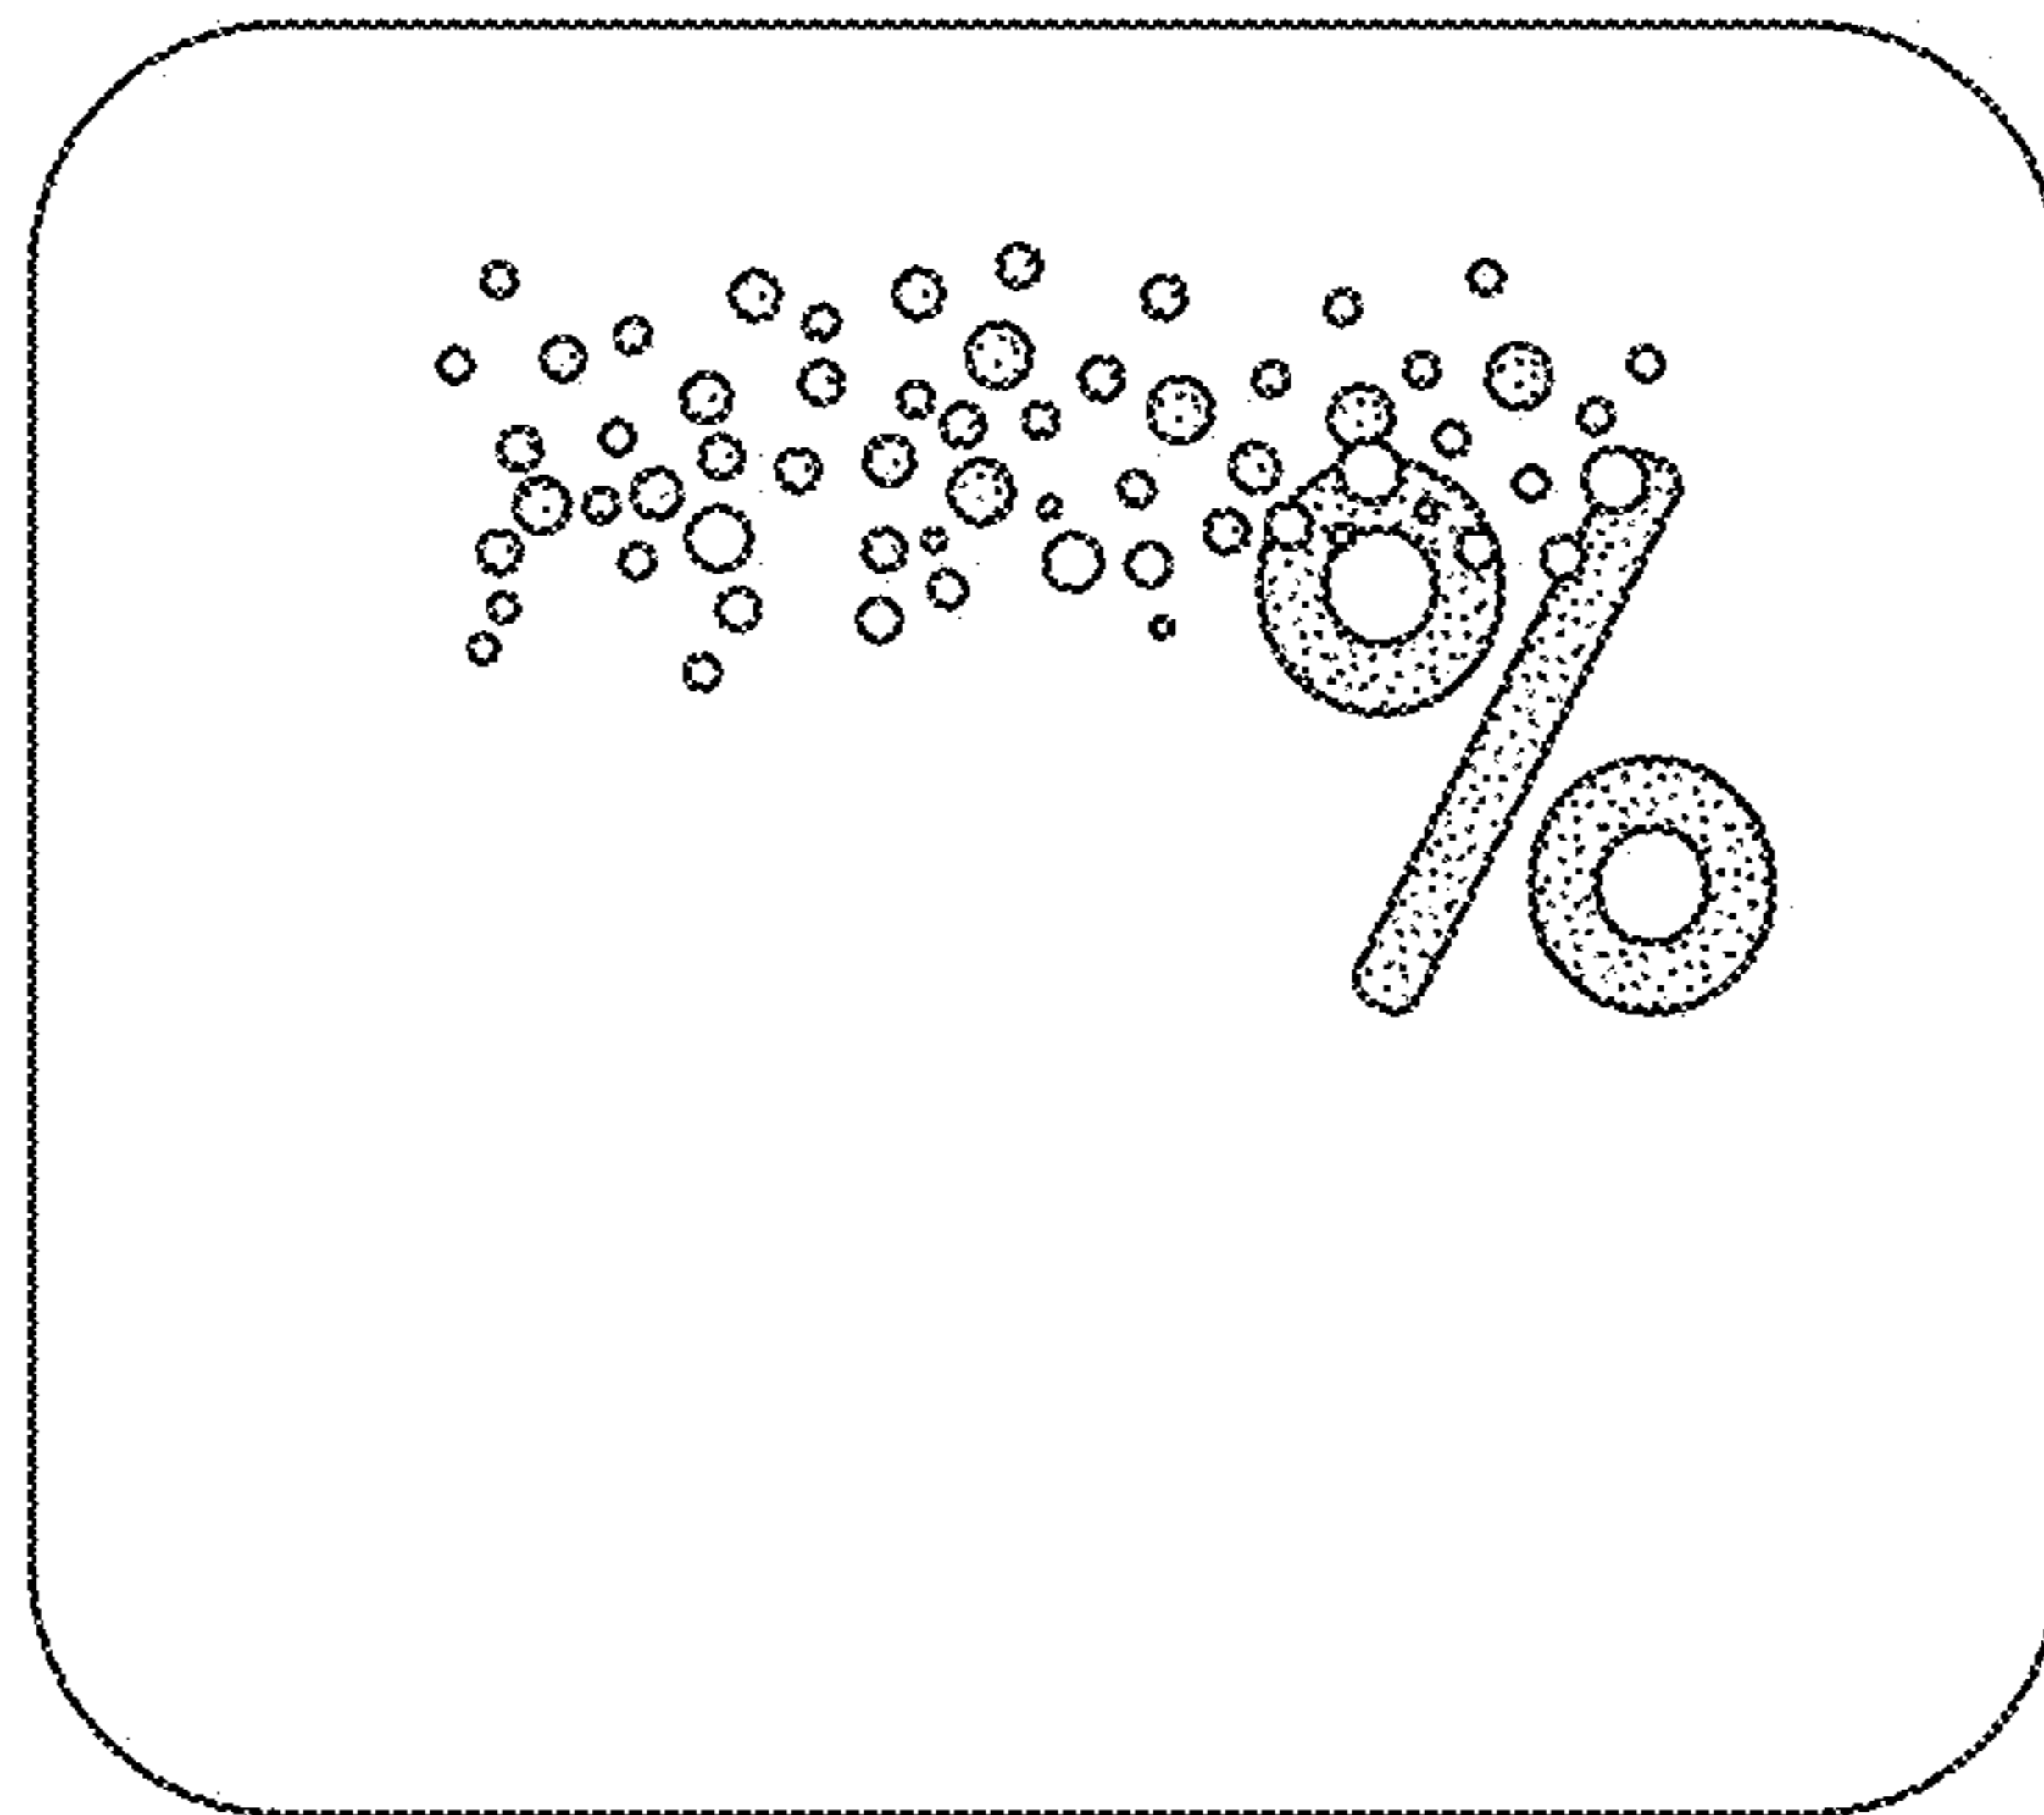


FIG. 2

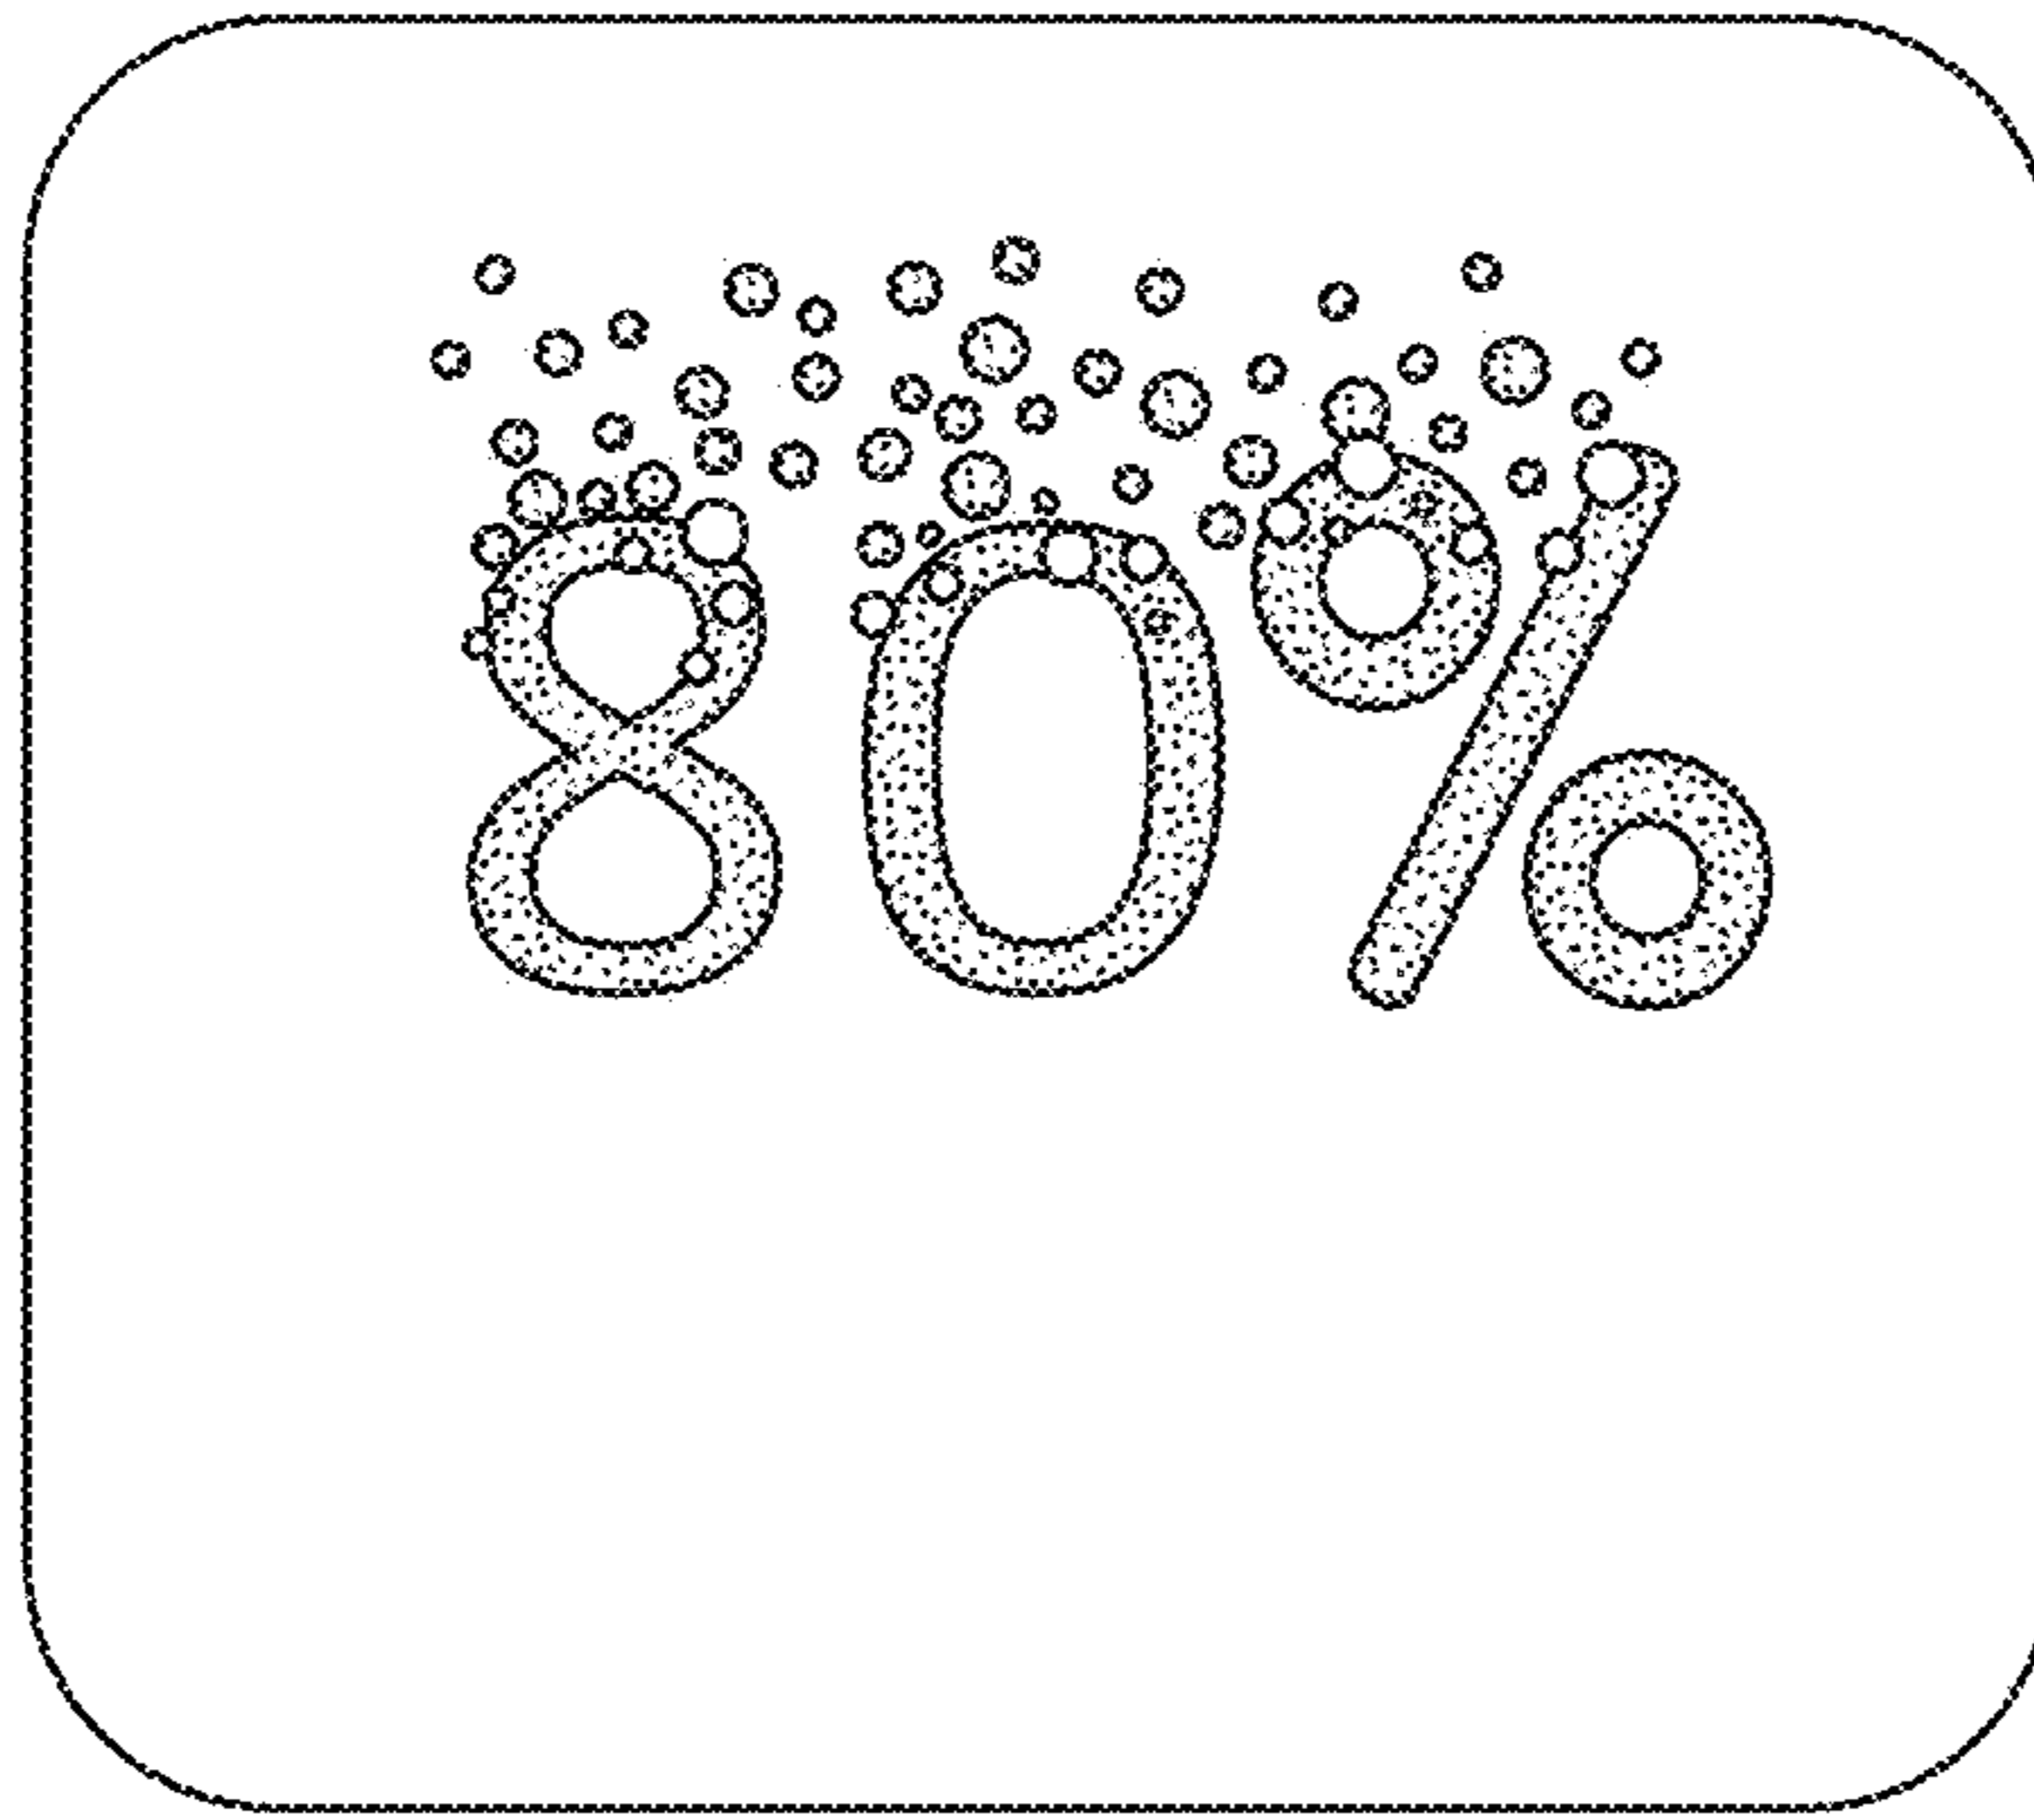


FIG. 3